

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County ALAMANCE Instrument Location ALAMANCE Co JAIL

Instrument Serial No. 008853 109 S. Maple St Graham, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 19 day of December, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Simon Stokes Brasos
Signature of Certifying Official

146221
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

ALAMANCE COUNTY JAIL 000

Serial Number: 008853
Test Date: 12/19/2025

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Barnes, Simon S

Permit Number: 0014-6221

Effective:

02/01/2025-02/01/2027

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG534301

Exp Date: 12/09/2027

Test	g/210L	Time
DIAG	Pass	11:20am
AIR BLK	.00	11:21am
ACCY CHK	.08	11:22am
AIR BLK	.00	11:23am
SUB TEST	.00	11:23am
AIR BLK	.00	11:24am
SUB TEST	.00	11:26am
AIR BLK	.00	11:27am

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

This form is used when performing Preventive Maintenance procedures

Forensic Tests for Alcohol Branch

Department of Health and Human Services

Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

ALAMANCE COUNTY JAIL 000

Serial Number: 008853 Test Record Number: 5223
Test Date: 12/19/2025 Test Time: 11:27am EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	11:27am
FLO	Pass	11:27am
FC	Pass	11:28am

Temperature Tests

Test	Status	Time
FC1	Pass	11:28am
SRC	Pass	11:28am
DET	Pass	11:28am
BAR	Pass	11:28am
BT	Pass	11:28am

Blank Tests

Test	Status	Time
AIR	Pass	11:28am


Printer Tests

Test	Status	Time
PRNT	Pass	11:28am

CRC Tests

Test	Status	Time
COMP	Pass	11:28am
CAL	Pass	11:28am

Preventive Maintenance
Status: Pass



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County Alamance Instrument Location BAT Mobile Unit 13

Instrument Serial No. 008869

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 20th day of December, 2005 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



John Lanier
Signature of Certifying Official

1604930
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

ALAMANCE COUNTY BAT MOBILE UNIT 13 000

Serial Number: 008869
Test Date: 12/20/2025

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Lanier Jr., John P

Permit Number: 4582-9118

Effective:

04/01/2025-04/01/2027

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG417803


Exp Date: 06/26/2026

Test	g/210L	Time
DIAG	Pass	10:24pm
AIR BLK	.00	10:25pm
ACCY CHK	.08	10:26pm
AIR BLK	.00	10:27pm
SUB TEST	.00	10:27pm
AIR BLK	.00	10:28pm
SUB TEST	.00	10:30pm
AIR BLK	.00	10:31pm

Reported AC: .00 g/210L

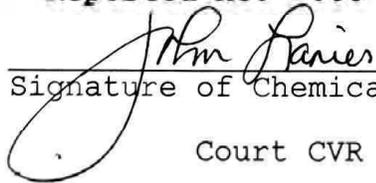
Signature of Chemical Analyst

Court CVR

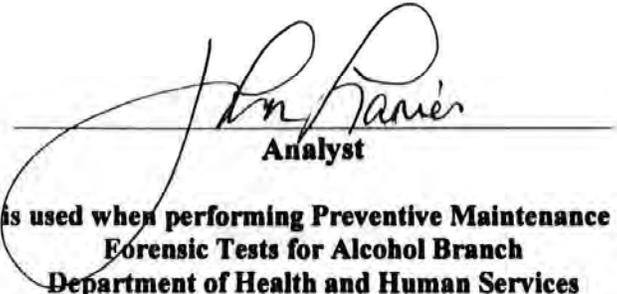
Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

ALAMANCE COUNTY BAT MOBILE UNIT 13 000

Serial Number: 008869 Test Record Number: 2143
Test Date: 12/20/2025 Test Time: 10:31pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	10:32pm
FLO	Pass	10:32pm
FC	Pass	10:32pm

Temperature Tests

Test	Status	Time
FC1	Pass	10:32pm
SRC	Pass	10:32pm
DET	Pass	10:32pm
BAR	Pass	10:32pm
BT	Pass	10:32pm

Blank Tests

Test	Status	Time
AIR	Pass	10:33pm


Printer Tests

Test	Status	Time
PRNT	Pass	10:33pm

CRC Tests

Test	Status	Time
COMP	Pass	10:33pm
CAL	Pass	10:33pm

Preventive Maintenance
Status: Pass

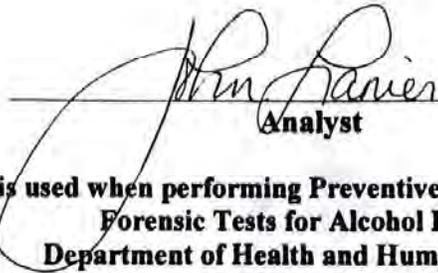

Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County Alamance Instrument Location BAT Mobile Unit 13

Instrument Serial No. 008898

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 20th day of December, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



John Franier
Signature of Certifying Official

1604930
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

ALAMANCE COUNTY BAT MOBILE UNIT 13 000

Serial Number: 008898
Test Date: 12/20/2025

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: Lanier Jr., John P
Permit Number: 4582-9118
Effective:
04/01/2025-04/01/2027

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG506302
Exp Date: 03/04/2027

Test	g/210L	Time
DIAG	Pass	10:23pm
AIR BLK	.00	10:24pm
ACCY CHK	.07	10:25pm
AIR BLK	.00	10:26pm
SUB TEST	.00	10:27pm
AIR BLK	.00	10:28pm
SUB TEST	.00	10:29pm
AIR BLK	.00	10:30pm

Reported AC: .00 g/210L

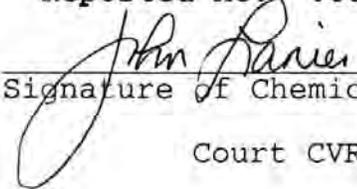

Signature of Chemical Analyst
Court CVR



Analyst

Intox EC/IR-II: Preventive Maintenance

ALAMANCE COUNTY BAT MOBILE UNIT 13 000

Serial Number: 008898 Test Record Number: 2089
Test Date: 12/20/2025 Test Time: 10:32pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	10:32pm
FLO	Pass	10:32pm
FC	Pass	10:32pm

Temperature Tests

Test	Status	Time
FC1	Pass	10:32pm
SRC	Pass	10:32pm
DET	Pass	10:32pm
BAR	Pass	10:32pm
BT	Pass	10:32pm

Blank Tests

Test	Status	Time
AIR	Pass	10:33pm

Printer Tests

Test	Status	Time
PRNT	Pass	10:33pm

CRC Tests

Test	Status	Time
COMP	Pass	10:33pm
CAL	Pass	10:33pm

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County Alamance Instrument Location Alamance Co Jail
Instrument Serial No. 008913 109 S. Maple St Graham, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 19 day of December, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Sam Stokes Bruce
Signature of Certifying Official

146221
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

ALAMANCE COUNTY ALAMANCE CO. JAIL 000

Serial Number: 008913
Test Date: 12/19/2025

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: Barnes, Simon S
Permit Number: 0014-6221
Effective:
02/01/2025-02/01/2027

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG534301
Exp Date: 12/09/2027

Test	g/210L	Time
DIAG	Pass	11:21am
AIR BLK	.00	11:22am
ACCY CHK	.08	11:22am
AIR BLK	.00	11:24am
SUB TEST	.00	11:24am
AIR BLK	.00	11:25am
SUB TEST	.00	11:27am
AIR BLK	.00	11:27am

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

Intox EC/IR-II: Preventive Maintenance

ALAMANCE COUNTY ALAMANCE CO. JAIL 000

Serial Number: 008913 Test Record Number: 5949
Test Date: 12/19/2025 Test Time: 11:28am EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	11:28am
FLO	Pass	11:28am
FC	Pass	11:28am

Temperature Tests

Test	Status	Time
FC1	Pass	11:28am
SRC	Pass	11:28am
DET	Pass	11:28am
BAR	Pass	11:28am
BT	Pass	11:28am

Blank Tests

Test	Status	Time
AIR	Pass	11:29am

Printer Tests

Test	Status	Time
PRNT	Pass	11:29am

CRC Tests

Test	Status	Time
COMP	Pass	11:29am
CAL	Pass	11:29am

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Alamance Instrument Location BAT Mobile Unit 13

Instrument Serial No. 008939

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 20th day of December, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



John Parier
Signature of Certifying Official

1604930
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

ALAMANCE COUNTY BAT MOBILE UNIT 13 000

Serial Number: 008939
Test Date: 12/20/2025

Citation Number: M0000000-0
Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Lanier Jr., John P

Permit Number: 4582-9118

Effective:

04/01/2025-04/01/2027

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG506302

Exp Date: 03/04/2027


Test	g/210L	Time
DIAG	Pass	9:24pm
AIR BLK	.00	9:25pm
ACCY CHK	.08	9:26pm
AIR BLK	.00	9:27pm
SUB TEST	.00	9:28pm
AIR BLK	.00	9:29pm
SUB TEST	.00	9:30pm
AIR BLK	.00	9:31pm

Reported AC: .00 g/210L

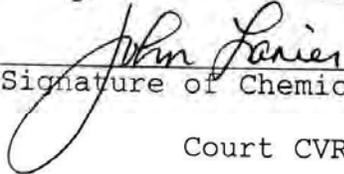

Signature of Chemical Analyst

Court CVR

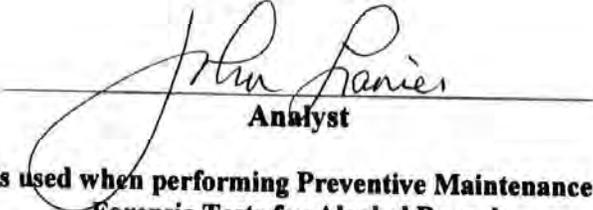

Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

ALAMANCE COUNTY BAT MOBILE UNIT 13 000

Serial Number: 008939 Test Record Number: 1959
Test Date: 12/20/2025 Test Time: 9:32pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	9:33pm
FLO	Pass	9:33pm
FC	Pass	9:33pm

Temperature Tests

Test	Status	Time
FC1	Pass	9:33pm
SRC	Pass	9:33pm
DET	Pass	9:33pm
BAR	Pass	9:33pm
BT	Pass	9:33pm

Blank Tests

Test	Status	Time
AIR	Pass	9:34pm


Printer Tests

Test	Status	Time
PRNT	Pass	9:34pm

CRC Tests

Test	Status	Time
COMP	Pass	9:34pm
CAL	Pass	9:34pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County Alamance

Instrument Location BAT Mobile Unit 11

Instrument Serial No. 008970

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 12th day of December, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



John Lanier
Signature of Certifying Official

1604930
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

ALAMANCE COUNTY BAT MOBILE UNIT 11 000

Serial Number: 008970

Test Date: 12/12/2025

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Lanier Jr., John P

Permit Number: 4582-9118

Effective:

04/01/2025-04/01/2027

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG417802


Exp Date: 06/26/2026

Test	g/210L	Time
DIAG	Pass	9:41pm
AIR BLK	.00	9:41pm
ACCY CHK	.07	9:42pm
AIR BLK	.00	9:43pm
SUB TEST	.00	9:44pm
AIR BLK	.00	9:45pm
SUB TEST	.00	9:46pm
AIR BLK	.00	9:47pm

Reported AC: .00 g/210L

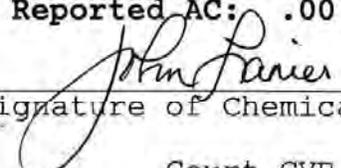
Signature of Chemical Analyst

Court CVR

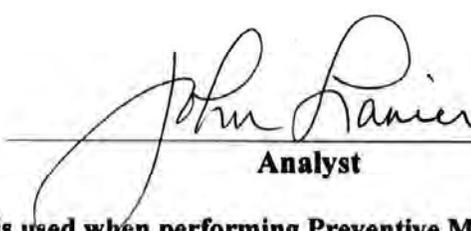
Analyst

Intox EC/IR-II: Preventive Maintenance

ALAMANCE COUNTY BAT MOBILE UNIT 11 000

Serial Number: 008970 Test Record Number: 1344
Test Date: 12/12/2025 Test Time: 9:47pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	9:48pm
FLO	Pass	9:48pm
FC	Pass	9:48pm

Temperature Tests

Test	Status	Time
FC1	Pass	9:48pm
SRC	Pass	9:48pm
DET	Pass	9:48pm
BAR	Pass	9:48pm
BT	Pass	9:48pm

Blank Tests

Test	Status	Time
AIR	Pass	9:48pm


Printer Tests

Test	Status	Time
PRNT	Pass	9:48pm

CRC Tests

Test	Status	Time
COMP	Pass	9:49pm
CAL	Pass	9:49pm

Preventive Maintenance
Status: Pass

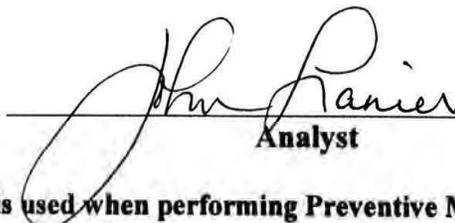

Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County Alamance Instrument Location BAT Mobile Unit 11

Instrument Serial No. 008973

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 12th day of December, 2005 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



John Parier
Signature of Certifying Official

1604930
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

ALAMANCE COUNTY BAT MOBILE UNIT 11 000

Serial Number: 008973
Test Date: 12/12/2025

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Lanier Jr., John P

Permit Number: 4582-9118

Effective:

04/01/2025-04/01/2027

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG431003

Exp Date: 11/05/2026


Test	g/210L	Time
DIAG	Pass	9:33pm
AIR BLK	.00	9:34pm
ACCY CHK	.07	9:35pm
AIR BLK	.00	9:36pm
SUB TEST	.00	9:37pm
AIR BLK	.00	9:38pm
SUB TEST	.00	9:41pm
AIR BLK	.00	9:41pm

Reported AC: .00 g/210L

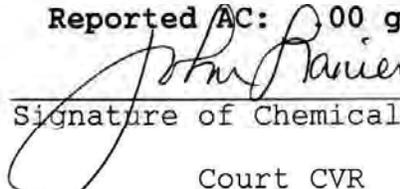

Signature of Chemical Analyst

Court CVR

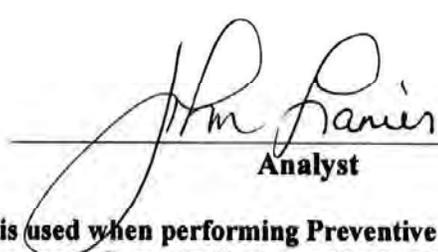

Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

ALAMANCE COUNTY BAT MOBILE UNIT 11 000

Serial Number: 008973 Test Record Number: 1392
Test Date: 12/12/2025 Test Time: 9:43pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	9:43pm
FLO	Pass	9:43pm
FC	Pass	9:43pm

Temperature Tests

Test	Status	Time
FC1	Pass	9:43pm
SRC	Pass	9:43pm
DET	Pass	9:43pm
BAR	Pass	9:43pm
BT	Pass	9:43pm

Blank Tests

Test	Status	Time
AIR	Pass	9:44pm

Printer Tests

Test	Status	Time
PRNT	Pass	9:44pm

CRC Tests

Test	Status	Time
COMP	Pass	9:44pm
CAL	Pass	9:44pm

Preventive Maintenance
Status: Pass



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Alleghany Instrument Location Alleghany Co Jail
Instrument Serial No. 008890 Sparta, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 19th day of December, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

509387
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

ALLEGHANY COUNTY ALLEGHANY CO JAIL 020

Serial Number: 008890
Test Date: 12/19/2025

Citation Number: M0000000-0
Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Long, Thomas A

Permit Number: 0050-9387

Effective:

09/01/2025-09/01/2027

Officer's Name: NONE, NONE

Type of Agency: FTA


Agency: DHHS

Test Type: Breath Test

Lot Number: AG534301
Exp Date: 12/09/2027

Test	g/210L	Time
DIAG	Pass	11:53am
AIR BLK	.00	11:54am
ACCY CHK	.07	11:54am
AIR BLK	.00	11:55am
SUB TEST	.00	11:58am
AIR BLK	.00	11:59am
SUB TEST	.00	12:01pm
AIR BLK	.00	12:01pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

ALLEGHANY COUNTY ALLEGHANY CO JAIL 020

Serial Number: 008890 Test Record Number: 1079
Test Date: 12/19/2025 Test Time: 12:03pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	12:04pm
FLO	Pass	12:04pm
FC	Pass	12:04pm

Temperature Tests

Test	Status	Time
FC1	Pass	12:04pm
SRC	Pass	12:04pm
DET	Pass	12:04pm
BAR	Pass	12:04pm
BT	Pass	12:04pm

Blank Tests

Test	Status	Time
AIR	Pass	12:05pm

Printer Tests

Test	Status	Time
PRNT	Pass	12:05pm

CRC Tests

Test	Status	Time
COMP	Pass	12:05pm
CAL	Pass	12:05pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County ANSON Instrument Location ANSON COUNTY

Instrument Serial No. 008597 SHERIFF'S OFFICE

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 23 day of DECEMBER, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Handwritten signature of the certifying official.

Signature of Certifying Official

239771

Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

ANSON COUNTY SHERIFF'S OFFICE 030

Serial Number: 008597
Test Date: 12/23/2025

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE

Analyst's Name: Galloway, Charles L
Permit Number: 0023-9771
Effective:
02/01/2025-02/01/2027

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG501307
Exp Date: 01/13/2027

Test	g/210L	Time
DIAG	Pass	12:49pm
AIR BLK	.00	12:50pm
ACCY CHK	.07	12:50pm
AIR BLK	.00	12:51pm
SUB TEST	.00	12:52pm
AIR BLK	.00	12:53pm
SUB TEST	.00	12:54pm
AIR BLK	.00	12:55pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

Intox EC/IR-II: Preventive Maintenance

ANSON COUNTY SHERIFF'S OFFICE 030

Serial Number: 008597 Test Record Number: 2040
Test Date: 12/23/2025 Test Time: 12:57pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	12:57pm
FLO	Pass	12:57pm
FC	Pass	12:57pm

Temperature Tests

Test	Status	Time
FC1	Pass	12:58pm
SRC	Pass	12:58pm
DET	Pass	12:58pm
BAR	Pass	12:58pm
BT	Pass	12:58pm

Blank Tests

Test	Status	Time
AIR	Pass	12:58pm

Printer Tests

Test	Status	Time
PRNT	Pass	12:58pm

CRC Tests

Test	Status	Time
COMP	Pass	12:58pm
CAL	Pass	12:58pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County ANSON Instrument Location ANSON COUNTY
Instrument Serial No. 008739 SHERIFF'S OFFICE

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 23 day of DECEMBER, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



A large, stylized handwritten signature in black ink.

Signature of Certifying Official

239771

Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

ANSON COUNTY SHERIFF'S OFFICE 030

Serial Number: 008739
Test Date: 12/23/2025

Citation Number: M0000000-0
Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Galloway, Charles L

Permit Number: 0023-9771

Effective:

02/01/2025-02/01/2027

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG501307

Exp Date: 01/13/2027

Test	g/210L	Time
DIAG	Pass	12:48pm
AIR BLK	.00	12:48pm
ACCY CHK	.07	12:49pm
AIR BLK	.00	12:50pm
SUB TEST	.00	12:51pm
AIR BLK	.00	12:52pm
SUB TEST	.00	12:53pm
AIR BLK	.00	12:54pm

Reported AC: .00 g/210L

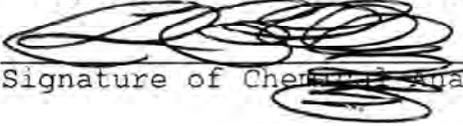
Signature of Chemical Analyst

Court CVR


Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

ANSON COUNTY SHERIFF'S OFFICE 030

Serial Number: 008739 Test Record Number: 1167
Test Date: 12/23/2025 Test Time: 12:55pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	12:55pm
FLO	Pass	12:55pm
FC	Pass	12:55pm

Temperature Tests

Test	Status	Time
FC1	Pass	12:55pm
SRC	Pass	12:55pm
DET	Pass	12:55pm
BAR	Pass	12:55pm
BT	Pass	12:55pm

Blank Tests

Test	Status	Time
AIR	Pass	12:56pm


Printer Tests

Test	Status	Time
PRNT	Pass	12:56pm

CRC Tests

Test	Status	Time
COMP	Pass	12:56pm
CAL	Pass	12:56pm

Preventive Maintenance
Status: Pass

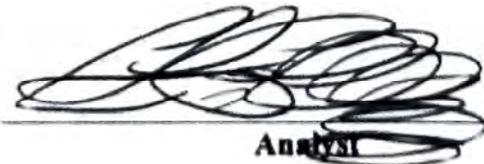

Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County Avery Instrument Location Avery County Jail

Instrument Serial No. 008664 Newland, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 22nd day of December, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

509387
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

AVERY COUNTY AVERY COUNTY JAIL 050

Serial Number: 008664

Test Date: 12/22/2025

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Long, Thomas A

Permit Number: 0050-9387

Effective:

09/01/2025-09/01/2027

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG534301

Exp Date: 12/09/2027

Test	g/210L	Time
DIAG	Pass	12:36pm
AIR BLK	.00	12:37pm
ACCY CHK	.08	12:38pm
AIR BLK	.00	12:39pm
SUB TEST	.00	12:39pm
AIR BLK	.00	12:40pm
SUB TEST	.00	12:42pm
AIR BLK	.00	12:43pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

This form is used when performing Preventive Maintenance procedures

Forensic Tests for Alcohol Branch

Department of Health and Human Services

Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

AVERY COUNTY AVERY COUNTY JAIL 050

Serial Number: 008664 Test Record Number: 1353
Test Date: 12/22/2025 Test Time: 12:45pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	12:46pm
FLO	Pass	12:46pm
FC	Pass	12:46pm

Temperature Tests

Test	Status	Time
FC1	Pass	12:46pm
SRC	Pass	12:46pm
DET	Pass	12:46pm
BAR	Pass	12:46pm
BT	Pass	12:46pm

Blank Tests

Test	Status	Time
AIR	Pass	12:46pm

Printer Tests

Test	Status	Time
PRNT	Pass	12:46pm

CRC Tests

Test	Status	Time
COMP	Pass	12:47pm
CAL	Pass	12:47pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County Avery Instrument Location Beech Mountain PD

Instrument Serial No. 008724 Beech Mountain, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 22nd day of December, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]

Signature of Certifying Official

509387

Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

AVERY COUNTY BEECH MOUNTAIN PD 050

Serial Number: 008724
Test Date: 12/22/2025

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Long, Thomas A

Permit Number: 0050-9387

Effective:

09/01/2025-09/01/2027

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG534301

Exp Date: 12/09/2027


Test	g/210L	Time
DIAG	Pass	10:23am
AIR BLK	.00	10:23am
ACCY CHK	.07	10:24am
AIR BLK	.00	10:25am
SUB TEST	.00	10:26am
AIR BLK	.00	10:27am
SUB TEST	.00	10:28am
AIR BLK	.00	10:29am

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

AVERY COUNTY BEECH MOUNTAIN PD 050

Serial Number: 008724 Test Record Number: 860
Test Date: 12/22/2025 Test Time: 10:33am EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	10:33am
FLO	Pass	10:33am
FC	Pass	10:33am

Temperature Tests

Test	Status	Time
FC1	Pass	10:33am
SRC	Pass	10:33am
DET	Pass	10:33am
BAR	Pass	10:33am
BT	Pass	10:33am

Blank Tests

Test	Status	Time
AIR	Pass	10:34am


Printer Tests

Test	Status	Time
PRNT	Pass	10:34am

CRC Tests

Test	Status	Time
COMP	Pass	10:34am
CAL	Pass	10:34am

Preventive Maintenance
Status: Pass

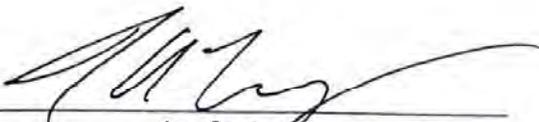

Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Bertie Instrument Location Bertie Co. S.O.
Instrument Serial No. 008897 222 County Farm Rd.
Windsor, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 4th day of December, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

206272
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

BERTIE COUNTY BERTIE CO SO 070

Serial Number: 008897

Test Date: 12/04/2025

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Chappell, Mark A

Permit Number: 0020-6272

Effective:

02/01/2025-02/01/2027

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG516203

Exp Date: 06/11/2027

Test	g/210L	Time
DIAG	Pass	10:41am
AIR BLK	.00	10:41am
ACCY CHK	.08	10:42am
AIR BLK	.00	10:43am
SUB TEST	.00	10:44am
AIR BLK	.00	10:45am
SUB TEST	.00	10:46am
AIR BLK	.00	10:47am

Reported AC: .00 g/210L

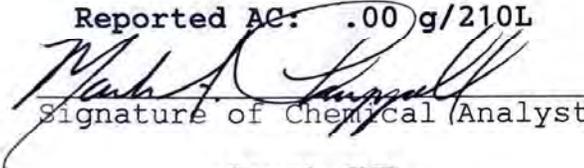
Signature of Chemical Analyst

Court CVR


Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

BERTIE COUNTY BERTIE CO SO 070

Serial Number: 008897 Test Record Number: 1709
Test Date: 12/04/2025 Test Time: 10:48am EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	10:49am
FLO	Pass	10:49am
FC	Pass	10:49am

Temperature Tests

Test	Status	Time
FC1	Pass	10:49am
SRC	Pass	10:49am
DET	Pass	10:49am
BAR	Pass	10:49am
BT	Pass	10:49am

Blank Tests

Test	Status	Time
AIR	Pass	10:49am


Printer Tests

Test	Status	Time
PRNT	Pass	10:49am

CRC Tests

Test	Status	Time
COMP	Pass	10:50am
CAL	Pass	10:50am

Preventive Maintenance
Status: Pass

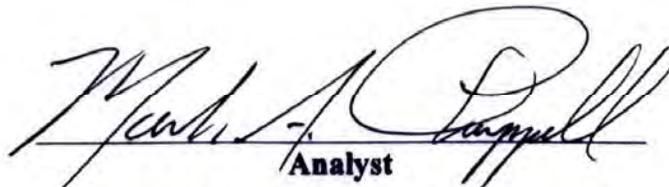
Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County BLADEN Instrument Location BLADEN COUNTY
Instrument Serial No. 008818 DETENTION CENTER

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 15 day of DECEMBER, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Alan R. Benson

Signature of Certifying Official

146279

Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

BLADEN COUNTY DETENTION CENTER 080

Serial Number: 008818
Test Date: 12/15/2025

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: BARNES, ALVIN R

Permit Number: 0014-6279

Effective:

02/01/2025-02/01/2027

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG417803


Exp Date: 06/26/2026

Test	g/210L	Time
DIAG	Pass	3:07pm
AIR BLK	.00	3:08pm
ACCY CHK	.08	3:08pm
AIR BLK	.00	3:09pm
SUB TEST	.00	3:10pm
AIR BLK	.00	3:11pm
SUB TEST	.00	3:13pm
AIR BLK	.00	3:14pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

BLADEN COUNTY DETENTION CENTER 080

Serial Number: 008818 Test Record Number: 2302
Test Date: 12/15/2025 Test Time: 3:14pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	3:15pm
FLO	Pass	3:15pm
FC	Pass	3:15pm

Temperature Tests

Test	Status	Time
FC1	Pass	3:15pm
SRC	Pass	3:15pm
DET	Pass	3:15pm
BAR	Pass	3:15pm
BT	Pass	3:15pm

Blank Tests

Test	Status	Time
AIR	Pass	3:15pm


Printer Tests

Test	Status	Time
PRNT	Pass	3:15pm

CRC Tests

Test	Status	Time
COMP	Pass	3:16pm
CAL	Pass	3:16pm

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County BRUNSWICK Instrument Location BRUNSWICK COUNTY

Instrument Serial No. 008585 DETENTION CENTER

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 19 day of DECEMBER, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Alan R. Burns

Signature of Certifying Official

146279

Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

BRUNSWICK COUNTY DETENTION CENTER 090

Serial Number: 008585

Test Date: 12/19/2025

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: BARNES, ALVIN R

Permit Number: 0014-6279

Effective:

02/01/2025-02/01/2027

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG501307

Exp Date: 01/13/2027

Test	g/210L	Time
DIAG	Pass	11:25am
AIR BLK	.00	11:25am
ACCY CHK	.08	11:26am
AIR BLK	.00	11:28am
SUB TEST	.00	11:29am
AIR BLK	.00	11:29am
SUB TEST	.00	11:31am
AIR BLK	.00	11:32am

Reported AC: .00 g/210L

Alvin R. Barnes

Signature of Chemical Analyst

Court CVR

Alvin R. Barnes

Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

BRUNSWICK COUNTY DETENTION CENTER 090

Serial Number: 008585 Test Record Number: 6170
Test Date: 12/19/2025 Test Time: 11:32am EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	11:33am
FLO	Pass	11:33am
FC	Pass	11:33am

Temperature Tests

Test	Status	Time
FC1	Pass	11:33am
SRC	Pass	11:33am
DET	Pass	11:33am
BAR	Pass	11:33am
BT	Pass	11:33am

Blank Tests

Test	Status	Time
AIR	Pass	11:34am


Printer Tests

Test	Status	Time
PRNT	Pass	11:34am

CRC Tests

Test	Status	Time
COMP	Pass	11:34am
CAL	Pass	11:34am

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County BRUNSWICK Instrument Location BRUNSWICK COUNTY
Instrument Serial No. 008602 DETENTION CENTER

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 19 day of DECEMBER, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Alan R. Burns

Signature of Certifying Official

146229

Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

BRUNSWICK COUNTY DETENTION CENTER 090

Serial Number: 008602

Test Date: 12/19/2025

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: BARNES, ALVIN R

Permit Number: 0014-6279

Effective:

02/01/2025-02/01/2027

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG501307

Exp Date: 01/13/2027


Test	g/210L	Time
DIAG	Pass	11:27am
AIR BLK	.00	11:27am
ACCY CHK	.07	11:28am
AIR BLK	.00	11:30am
SUB TEST	.00	11:31am
AIR BLK	.00	11:31am
SUB TEST	.00	11:33am
AIR BLK	.00	11:34am

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR


Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

BRUNSWICK COUNTY DETENTION CENTER 090

Serial Number: 008602 Test Record Number: 6144
Test Date: 12/19/2025 Test Time: 11:35am EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	11:35am
FLO	Pass	11:35am
FC	Pass	11:35am

Temperature Tests

Test	Status	Time
FC1	Pass	11:35am
SRC	Pass	11:35am
DET	Pass	11:35am
BAR	Pass	11:35am
BT	Pass	11:35am

Blank Tests

Test	Status	Time
AIR	Pass	11:36am


Printer Tests

Test	Status	Time
PRNT	Pass	11:36am

CRC Tests

Test	Status	Time
COMP	Pass	11:36am
CAL	Pass	11:36am

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County BRUNSWICK Instrument Location OAK ISLAND

Instrument Serial No. 008648 POLICE DEPT

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 19 day of DECEMBER, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Alan R. Bann
Signature of Certifying Official

146279
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

BRUNSWICK COUNTY OAK ISLAND PD 090

Serial Number: 008648
Test Date: 12/19/2025

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: BARNES, ALVIN R

Permit Number: 0014-6279

Effective:

02/01/2025-02/01/2027

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG417802

Exp Date: 06/26/2026


Test	g/210L	Time
DIAG	Pass	2:49pm
AIR BLK	.00	2:50pm
ACCY CHK	.07	2:51pm
AIR BLK	.00	2:52pm
SUB TEST	.00	2:52pm
AIR BLK	.00	2:53pm
SUB TEST	.00	2:55pm
AIR BLK	.00	2:56pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

BRUNSWICK COUNTY OAK ISLAND PD 090

Serial Number: 008648 Test Record Number: 2021
Test Date: 12/19/2025 Test Time: 2:56pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	2:56pm
FLO	Pass	2:56pm
FC	Pass	2:56pm

Temperature Tests

Test	Status	Time
FC1	Pass	2:56pm
SRC	Pass	2:56pm
DET	Pass	2:56pm
BAR	Pass	2:56pm
BT	Pass	2:56pm

Blank Tests

Test	Status	Time
AIR	Pass	2:57pm


Printer Tests

Test	Status	Time
PRNT	Pass	2:57pm

CRC Tests

Test	Status	Time
COMP	Pass	2:57pm
CAL	Pass	2:57pm

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County BRUNSWICK Instrument Location SUNSET BEACH

Instrument Serial No. 008874 POLICE DEPT

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 19 day of DECEMBER, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Alan R. Bruno

Signature of Certifying Official

146279

Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

BRUNSWICK COUNTY SUNSET BEACH PD 090

Serial Number: 008874
Test Date: 12/19/2025

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: BARNES, ALVIN R

Permit Number: 0014-6279

Effective:

02/01/2025-02/01/2027

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG417802

Exp Date: 06/26/2026


Test	g/210L	Time
DIAG	Pass	4:21pm
AIR BLK	.00	4:22pm
ACCY CHK	.07	4:22pm
AIR BLK	.00	4:24pm
SUB TEST	.00	4:24pm
AIR BLK	.00	4:25pm
SUB TEST	.00	4:27pm
AIR BLK	.00	4:28pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

BRUNSWICK COUNTY SUNSET BEACH PD 090

Serial Number: 008874 Test Record Number: 1103
Test Date: 12/19/2025 Test Time: 4:28pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	4:28pm
FLO	Pass	4:28pm
FC	Pass	4:28pm

Temperature Tests

Test	Status	Time
FC1	Pass	4:28pm
SRC	Pass	4:28pm
DET	Pass	4:28pm
BAR	Pass	4:28pm
BT	Pass	4:28pm

Blank Tests

Test	Status	Time
AIR	Pass	4:29pm


Printer Tests

Test	Status	Time
PRNT	Pass	4:29pm

CRC Tests

Test	Status	Time
COMP	Pass	4:29pm
CAL	Pass	4:29pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County Buncombe Instrument Location Black Mountain PD
Instrument Serial No. 008697 Black Mountain, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 22 day of December, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.




Signature of Certifying Official

244987
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

BUNCOMBE COUNTY BLACK MOUNTAIN PD 100

Serial Number: 008697

Test Date: 12/22/2025

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Loftis, Benjamin C

Permit Number: 0024-4987

Effective:

03/01/2025-03/01/2027

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG506303


Exp Date: 03/04/2027

Test	g/210L	Time
DIAG	Pass	1:39pm
AIR BLK	.00	1:40pm
ACCY CHK	.07	1:40pm
AIR BLK	.00	1:42pm
SUB TEST	.00	1:42pm
AIR BLK	.00	1:43pm
SUB TEST	.00	1:44pm
AIR BLK	.00	1:45pm

Reported AC: .00 g/210L

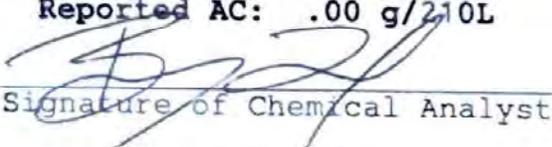
Signature of Chemical Analyst

Court CVR

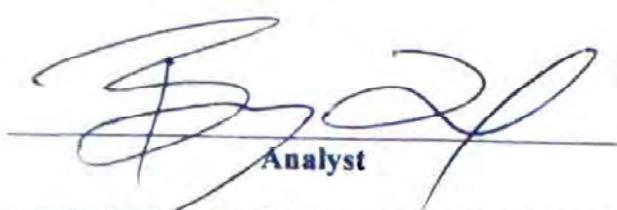
Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

BUNCOMBE COUNTY BLACK MOUNTAIN PD 100

Serial Number: 008697 Test Record Number: 7153
Test Date: 12/22/2025 Test Time: 1:46pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	1:46pm
FLO	Pass	1:46pm
FC	Pass	1:46pm

Temperature Tests

Test	Status	Time
FC1	Pass	1:46pm
SRC	Pass	1:46pm
DET	Pass	1:46pm
BAR	Pass	1:46pm
BT	Pass	1:46pm

Blank Tests

Test	Status	Time
AIR	Pass	1:47pm


Printer Tests

Test	Status	Time
PRNT	Pass	1:47pm

CRC Tests

Test	Status	Time
COMP	Pass	1:47pm
CAL	Pass	1:47pm

Preventive Maintenance
Status: Pass

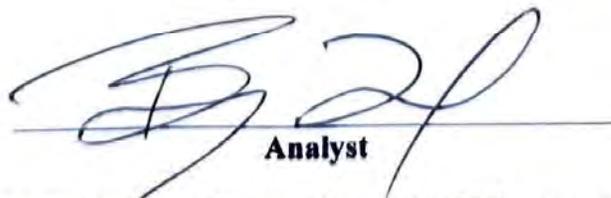
Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)


County Buncombe Instrument Location Buncombe County Detention
Instrument Serial No. 009748 Asheville, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 22 day of December, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.

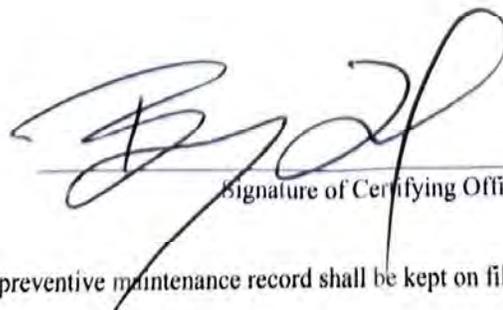


Signature of Certifying Official

244987
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

BUNCOMBE COUNTY BUNCOMBE COUNTY
DETENTION 1:00

Serial Number: 008748
Test Date: 12/22/2025

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: Loftis, Benjamin C
Permit Number: 0024-4987
Effective:
03/01/2025-03/01/2027

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG534301
Exp Date: 12/09/2027

Test	g/210L	Time
DIAG	Pass	12:47pm
AIR BLK	.00	12:48pm
ACCY CHK	.08	12:49pm
AIR BLK	.00	12:50pm
SUB TEST	.00	12:51pm
AIR BLK	.00	12:52pm
SUB TEST	.00	12:53pm
AIR BLK	.00	12:54pm

Reported AC: .00 g/210L

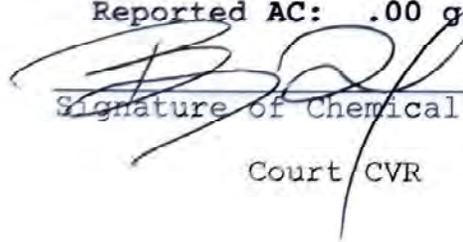

Signature of Chemical Analyst
Court CVR



Analyst

Intox EC/IR-II: Preventive Maintenance

BUNCOMBE COUNTY BUNCOMBE COUNTY DETENTION 100

Serial Number: 008748 Test Record Number: 3419
Test Date: 12/22/2025 Test Time: 12:54pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR:	Pass	12:55pm
FLO	Pass	12:55pm
FC	Pass	12:55pm

Temperature Tests

Test	Status	Time
FC1	Pass	12:55pm
SRC	Pass	12:55pm
DET	Pass	12:55pm
BAR	Pass	12:55pm
BT	Pass	12:55pm

Blank Tests

Test	Status	Time
AIR	Pass	12:56pm

Printer Tests

Test	Status	Time
PRNT	Pass	12:56pm

CRC Tests

Test	Status	Time
COMP	Pass	12:56pm
CAL	Pass	12:56pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Buncombe Instrument Location Buncombe County Detention
Instrument Serial No. 009798 Asheville, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 22 day of December, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

244987
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

BUNCOMBE COUNTY BUNCOMBE COUNTY
DETENTION 100

Serial Number: 008798
Test Date: 12/22/2025

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: Loftis, Benjamin C
Permit Number: 0024-4987
Effective:
03/01/2025-03/01/2027

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test


Lot Number: AG506303
Exp Date: 03/04/2027

Test	g/210L	Time
DIAG	Pass	12:49pm
AIR BLK	.00	12:50pm
ACCY CHK	.07	12:50pm
AIR BLK	.00	12:51pm
SUB TEST	.00	12:52pm
AIR BLK	.00	12:53pm
SUB TEST	.00	12:54pm
AIR BLK	.00	12:55pm

Reported AC: .00 g/210L

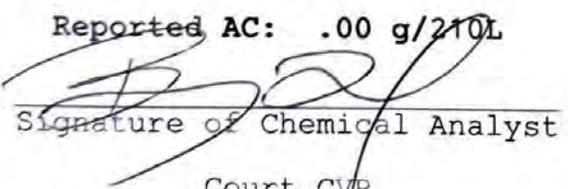
Signature of Chemical Analyst

Court CVR

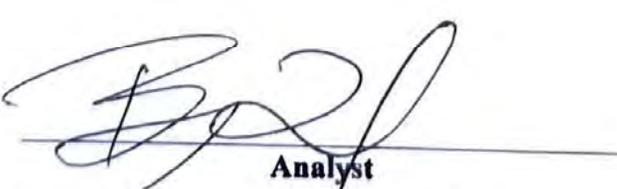
Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

BUNCOMBE COUNTY BUNCOMBE COUNTY DETENTION 100

Serial Number: 008798 Test Record Number: 7499
Test Date: 12/22/2025 Test Time: 12:55pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	12:56pm
FLO	Pass	12:56pm
FC	Pass	12:56pm

Temperature Tests

Test	Status	Time
FC1	Pass	12:56pm
SRC	Pass	12:56pm
DET	Pass	12:56pm
BAR	Pass	12:56pm
BT	Pass	12:56pm

Blank Tests

Test	Status	Time
AIR	Pass	12:57pm


Printer Tests

Test	Status	Time
PRNT	Pass	12:57pm

CRC Tests

Test	Status	Time
COMP	Pass	12:57pm
CAL	Pass	12:57pm

Preventive Maintenance
Status: Pass

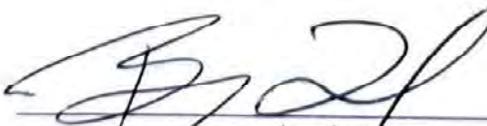

Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County Buncombe Instrument Location BAT Mobile Unit 11

Instrument Serial No. 008970

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 31st day of December, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

62446
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

BUNCOMBE COUNTY BAT MOBILE UNIT 11 100

Serial Number: 008970
Test Date: 12/31/2025

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Gillstrap, Jeffrey L

Permit Number: 0006-2446

Effective:

04/01/2025-04/01/2027

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG417802

Exp Date: 06/26/2026


Test	g/210L	Time
DIAG	Pass	10:59pm
AIR BLK	.00	10:59pm
ACCY CHK	.07	11:00pm
AIR BLK	.00	11:01pm
SUB TEST	.00	11:02pm
AIR BLK	.00	11:03pm
SUB TEST	.00	11:04pm
AIR BLK	.00	11:05pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR

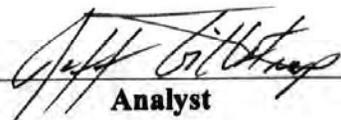

Analyst

Intox EC/IR-II: Preventive Maintenance

BUNCOMBE COUNTY BAT MOBILE UNIT 11 100

Serial Number: 008970 Test Record Number: 1359
Test Date: 12/31/2025 Test Time: 11:06pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	11:07pm
FLO	Pass	11:07pm
FC	Pass	11:07pm

Temperature Tests

Test	Status	Time
FC1	Pass	11:07pm
SRC	Pass	11:07pm
DET	Pass	11:07pm
BAR	Pass	11:07pm
BT	Pass	11:07pm

Blank Tests

Test	Status	Time
AIR	Pass	11:07pm


Printer Tests

Test	Status	Time
PRNT	Pass	11:08pm

CRC Tests

Test	Status	Time
COMP	Pass	11:08pm
CAL	Pass	11:08pm

Preventive Maintenance
Status: Pass

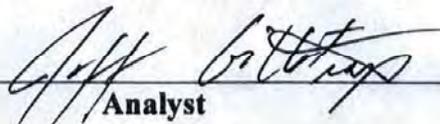

Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Buncombe Instrument Location Pat Mobile Unit 11

Instrument Serial No. 008970

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 31st day of December, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Jeff B. [Signature]
Signature of Certifying Official

62446
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

BUNCOMBE COUNTY BAT MOBILE UNIT 11 100

Serial Number: 008970
Test Date: 12/31/2025

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Gillstrap, Jeffrey L

Permit Number: 0006-2446

Effective:

04/01/2025-04/01/2027

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG417802

Exp Date: 06/26/2026

Test	g/210L	Time
DIAG	Pass	8:31pm
AIR BLK	.00	8:32pm
ACCY CHK	.07	8:33pm
AIR BLK	.00	8:34pm
SUB TEST	.00	8:34pm
AIR BLK	.00	8:35pm
SUB TEST	.00	8:37pm
AIR BLK	.00	8:38pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

BUNCOMBE COUNTY BAT MOBILE UNIT 11 100

Serial Number: 008970 Test Record Number: 1357
Test Date: 12/31/2025 Test Time: 8:39pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	8:39pm
FLO	Pass	8:39pm
FC	Pass	8:40pm

Temperature Tests

Test	Status	Time
FC1	Pass	8:40pm
SRC	Pass	8:40pm
DET	Pass	8:40pm
BAR	Pass	8:40pm
BT	Pass	8:40pm

Blank Tests

Test	Status	Time
AIR	Pass	8:40pm


Printer Tests

Test	Status	Time
PRNT	Pass	8:40pm

CRC Tests

Test	Status	Time
COMP	Pass	8:40pm
CAL	Pass	8:40pm

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County Buncombe Instrument Location BAT Mobile Unit 11

Instrument Serial No. 008973

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 31st day of December, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Jeff Gilstrap
Signature of Certifying Official

62446
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

BUNCOMBE COUNTY BAT MOBILE UNIT 11 100

Serial Number: 008973

Test Date: 12/31/2025

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Gillstrap, Jeffrey L

Permit Number: 0006-2446

Effective:

04/01/2025-04/01/2027

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG431003


Exp Date: 11/05/2026

Test	g/210L	Time
DIAG	Pass	11:04pm
AIR BLK	.00	11:05pm
ACCY CHK	.07	11:06pm
AIR BLK	.00	11:07pm
SUB TEST	.00	11:07pm
AIR BLK	.00	11:08pm
SUB TEST	.00	11:10pm
AIR BLK	.00	11:10pm

Reported AC: .00 g/210L

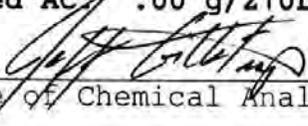
Signature of Chemical Analyst

Court CVR

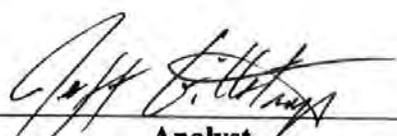
Analyst

Intox EC/IR-II: Preventive Maintenance

BUNCOMBE COUNTY BAT MOBILE UNIT 11 100

Serial Number: 008973 Test Record Number: 1410
Test Date: 12/31/2025 Test Time: 11:11pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	11:11pm
FLO	Pass	11:11pm
FC	Pass	11:11pm

Temperature Tests

Test	Status	Time
FC1	Pass	11:11pm
SRC	Pass	11:11pm
DET	Pass	11:11pm
BAR	Pass	11:11pm
BT	Pass	11:11pm

Blank Tests

Test	Status	Time
AIR	Pass	11:12pm


Printer Tests

Test	Status	Time
PRNT	Pass	11:12pm

CRC Tests

Test	Status	Time
COMP	Pass	11:12pm
CAL	Pass	11:12pm

Preventive Maintenance
Status: Pass

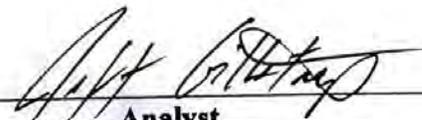

Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County Buncombe Instrument Location Bot Mobile Unit 11

Instrument Serial No. 008973

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 31st day of December, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

62446
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

BUNCOMBE COUNTY BAT MOBILE UNIT 11 100

Serial Number: 008973
Test Date: 12/31/2025

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Gillstrap, Jeffrey L

Permit Number: 0006-2446

Effective:

04/01/2025-04/01/2027

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG431003

Exp Date: 11/05/2026

Test	g/210L	Time
DIAG	Pass	8:27pm
AIR BLK	.00	8:28pm
ACCY CHK	.07	8:28pm
AIR BLK	.00	8:29pm
SUB TEST	.00	8:30pm
AIR BLK	.00	8:31pm
SUB TEST	.00	8:32pm
AIR BLK	.00	8:33pm

Reported AC: .00 g/210L

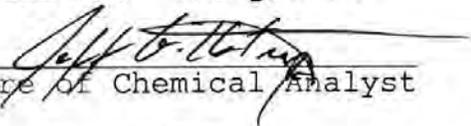
Signature of Chemical Analyst

Court CVR


Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

BUNCOMBE COUNTY BAT MOBILE UNIT 11 100

Serial Number: 008973 Test Record Number: 1408
Test Date: 12/31/2025 Test Time: 8:34pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	8:34pm
FLO	Pass	8:34pm
FC	Pass	8:34pm

Temperature Tests

Test	Status	Time
FC1	Pass	8:35pm
SRC	Pass	8:35pm
DET	Pass	8:35pm
BAR	Pass	8:35pm
BT	Pass	8:35pm

Blank Tests

Test	Status	Time
AIR	Pass	8:35pm


Printer Tests

Test	Status	Time
PRNT	Pass	8:35pm

CRC Tests

Test	Status	Time
COMP	Pass	8:35pm
CAL	Pass	8:35pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County Cabarrus Instrument Location Kannapolis PD
Instrument Serial No. 008589 Kannapolis, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 29th day of December, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

849845
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

KANNAPOLIS PD CABARRUS COUNTY 120

Serial Number: 008589
Test Date: 12/29/2025

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: Helms, Bryce A
Permit Number: 0084-9845
Effective:
02/01/2025-02/01/2027

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test


Lot Number: AG516203
Exp Date: 06/11/2027

Test	g/210L	Time
DIAG	Pass	10:59am
AIR BLK	.00	11:00am
ACCY CHK	.07	11:01am
AIR BLK	.00	11:02am
SUB TEST	.00	11:02am
AIR BLK	.00	11:03am
SUB TEST	.00	11:05am
AIR BLK	.00	11:05am

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR

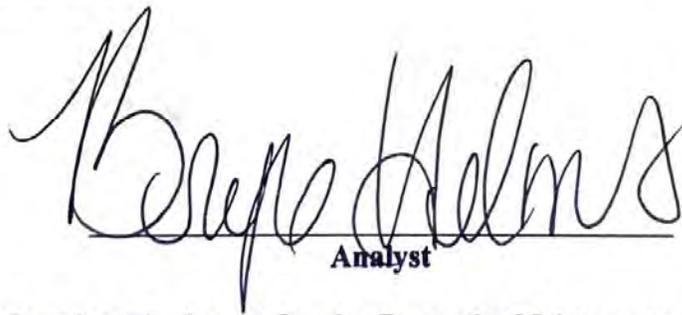
Analyst

Intox EC/IR-II: Preventive Maintenance

KANNAPOLIS PD CABARRUS COUNTY 120

Serial Number: 008589 Test Record Number: 4257
Test Date: 12/29/2025 Test Time: 11:06am EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	11:06am
FLO	Pass	11:06am
FC	Pass	11:06am

Temperature Tests

Test	Status	Time
FC1	Pass	11:06am
SRC	Pass	11:06am
DET	Pass	11:06am
BAR	Pass	11:06am
BT	Pass	11:06am

Blank Tests

Test	Status	Time
AIR	Pass	11:07am


Printer Tests

Test	Status	Time
PRNT	Pass	11:07am

CRC Tests

Test	Status	Time
COMP	Pass	11:07am
CAL	Pass	11:07am

Preventive Maintenance
Status: Pass

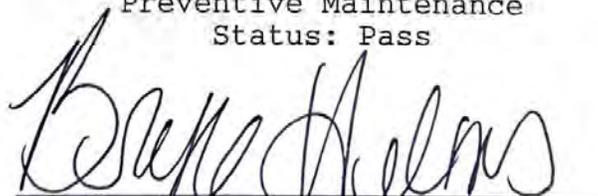
Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County Cabarrus Instrument Location Kannapolis PD
Instrument Serial No. 008589 Kannapolis, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 1st day of December, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

849845
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

KANNAPOLIS PD CABARRUS COUNTY 120

Serial Number: 008589
Test Date: 12/01/2025

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Helms, Bryce A

Permit Number: 0084-9845

Effective:

02/01/2025-02/01/2027

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG417802

Exp Date: 06/26/2026

Test	g/210L	Time
DIAG	Pass	12:50pm
AIR BLK	.00	12:51pm
ACCY CHK	.07	12:52pm
AIR BLK	.00	12:53pm
SUB TEST	.00	12:53pm
AIR BLK	.00	12:54pm
SUB TEST	.00	12:56pm
AIR BLK	.00	12:57pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

Intox EC/IR-II: Preventive Maintenance

KANNAPOLIS PD CABARRUS COUNTY 120

Serial Number: 008589 Test Record Number: 4235
Test Date: 12/01/2025 Test Time: 12:57pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	12:58pm
FLO	Pass	12:58pm
FC	Pass	12:58pm

Temperature Tests

Test	Status	Time
FC1	Pass	12:58pm
SRC	Pass	12:58pm
DET	Pass	12:58pm
BAR	Pass	12:58pm
BT	Pass	12:58pm

Blank Tests

Test	Status	Time
AIR	Pass	12:58pm


Printer Tests

Test	Status	Time
PRNT	Pass	12:58pm

CRC Tests

Test	Status	Time
COMP	Pass	12:59pm
CAL	Pass	12:59pm

Preventive Maintenance
Status: Pass

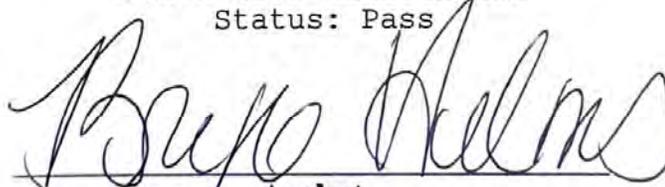

Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Cabarrus Instrument Location Cabarrus County &
Instrument Serial No. 008590 Concord, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 1st day of December, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Handwritten Signature]
Signature of Certifying Official

849845
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

CABARRUS COUNTY CABARRUS COUNTY SO 120

Serial Number: 008590
Test Date: 12/01/2025

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: Helms, Bryce A
Permit Number: 0084-9845
Effective:
02/01/2025-02/01/2027

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG516203
Exp Date: 06/11/2027

Test	g/210L	Time
DIAG	Pass	11:32am
AIR BLK	.00	11:33am
ACCY CHK	.08	11:34am
AIR BLK	.00	11:35am
SUB TEST	.00	11:36am
AIR BLK	.00	11:37am
SUB TEST	.00	11:39am
AIR BLK	.00	11:40am

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

CABARRUS COUNTY CABARRUS COUNTY SO 120

Serial Number: 008590 Test Record Number: 5795
Test Date: 12/01/2025 Test Time: 11:41am EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	11:41am
FLO	Pass	11:41am
FC	Pass	11:41am

Temperature Tests

Test	Status	Time
FC1	Pass	11:41am
SRC	Pass	11:41am
DET	Pass	11:41am
BAR	Pass	11:41am
BT	Pass	11:41am

Blank Tests

Test	Status	Time
AIR	Pass	11:42am


Printer Tests

Test	Status	Time
PRNT	Pass	11:42am

CRC Tests

Test	Status	Time
COMP	Pass	11:42am
CAL	Pass	11:42am

Preventive Maintenance
Status: Pass

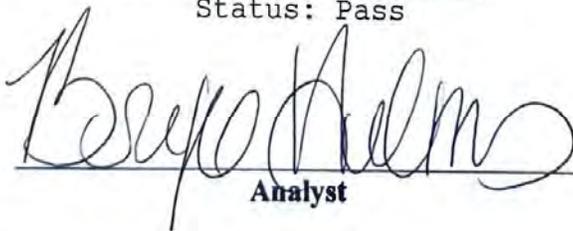
Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Cabarrus Instrument Location BAT Mobile Unit 8

Instrument Serial No. 008615

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 18 day of December, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

2219283
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

CABARRUS COUNTY BAT MOBILE UNIT 8 120

Serial Number: 008615
Test Date: 12/18/2025

Citation Number: M0000000-0
Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Glasscock, Jerry D.

Permit Number: 7180-9235

Effective:

02/01/2025-02/01/2027

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG405102

Exp Date: 02/20/2026

Test	g/210L	Time
DIAG	Pass	8:31am
AIR BLK	.00	8:32am
ACCY CHK	.07	8:32am
AIR BLK	.00	8:33am
SUB TEST	.00	8:34am
AIR BLK	.00	8:35am
SUB TEST	.00	8:36am
AIR BLK	.00	8:37am

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

CABARRUS COUNTY BAT MOBILE UNIT 8 120

Serial Number: 008615 Test Record Number: 6209
Test Date: 12/18/2025 Test Time: 8:38am EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	8:38am
FLO	Pass	8:38am
FC	Pass	8:38am

Temperature Tests

Test	Status	Time
FC1	Pass	8:38am
SRC	Pass	8:38am
DET	Pass	8:38am
BAR	Pass	8:38am
BT	Pass	8:38am

Blank Tests

Test	Status	Time
AIR	Pass	8:39am

Printer Tests

Test	Status	Time
PRNT	Pass	8:39am

CRC Tests

Test	Status	Time
COMP	Pass	8:39am
CAL	Pass	8:39am

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Cabarrus Instrument Location BAT Mobile Unit 8

Instrument Serial No. 008615

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 30 day of December, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

2219283
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

CABARRUS COUNTY BAT MOBILE UNIT 8 120

Serial Number: 008615
Test Date: 12/30/2025

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Glasscock, Jerry D

Permit Number: 7180-9235

Effective:

02/01/2025-02/01/2027

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG405102

Exp Date: 02/20/2026

Test	g/210L	Time
DIAG	Pass	7:55pm
AIR BLK	.00	7:56pm
ACCY CHK	.07	7:56pm
AIR BLK	.00	7:57pm
SUB TEST	.00	7:58pm
AIR BLK	.00	7:59pm
SUB TEST	.00	8:00pm
AIR BLK	.00	8:01pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

CABARRUS COUNTY BAT MOBILE UNIT 8 120

Serial Number: 008615 Test Record Number: 6214
Test Date: 12/30/2025 Test Time: 8:01pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	8:02pm
FLO	Pass	8:02pm
FC	Pass	8:02pm

Temperature Tests

Test	Status	Time
FC1	Pass	8:02pm
SRC	Pass	8:02pm
DET	Pass	8:02pm
BAR	Pass	8:02pm
BT	Pass	8:02pm

Blank Tests

Test	Status	Time
AIR	Pass	8:03pm

Printer Tests

Test	Status	Time
PRNT	Pass	8:03pm

CRC Tests

Test	Status	Time
COMP	Pass	8:03pm
CAL	Pass	8:03pm

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Cabarrus Instrument Location Cabarrus County 80
Instrument Serial No. 008625 Concord, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 1st day of December, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Boyo Helms
Signature of Certifying Official

849845
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

CABARRUS COUNTY CABARRUS COUNTY SO 120

Serial Number: 008625
Test Date: 12/01/2025

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Helms, Bryce A

Permit Number: 0084-9845

Effective:

02/01/2025-02/01/2027

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG506302

Exp Date: 03/04/2027

Test	g/210L	Time
DIAG	Pass	11:35am
AIR BLK	.00	11:36am
ACCY CHK	.07	11:36am
AIR BLK	.00	11:38am
SUB TEST	.00	11:39am
AIR BLK	.00	11:39am
SUB TEST	.00	11:42am
AIR BLK	.00	11:42am

Reported AC: .00 g/210L

Bryce Helms
Signature of Chemical Analyst

Court CVR

Bryce Helms
Analyst

Intox EC/IR-II: Preventive Maintenance

CABARRUS COUNTY CABARRUS COUNTY SO 120

Serial Number: 008625 Test Record Number: 7292
Test Date: 12/01/2025 Test Time: 11:46am EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	11:47am
FLO	Pass	11:47am
FC	Pass	11:47am

Temperature Tests

Test	Status	Time
FC1	Pass	11:47am
SRC	Pass	11:47am
DET	Pass	11:47am
BAR	Pass	11:47am
BT	Pass	11:47am

Blank Tests

Test	Status	Time
AIR	Pass	11:48am


Printer Tests

Test	Status	Time
PRNT	Pass	11:48am

CRC Tests

Test	Status	Time
COMP	Pass	11:48am
CAL	Pass	11:48am

Preventive Maintenance
Status: Pass

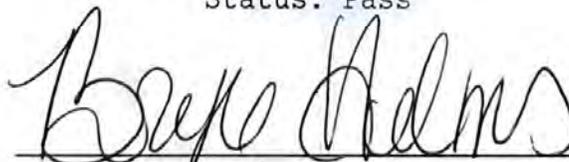

Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Cabarrus Instrument Location BAT Mobile Unit 8

Instrument Serial No. 008736

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 18 day of December, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

2219283
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

CABARRUS COUNTY BAT MOBILE UNIT 8 120

Serial Number: 008736
Test Date: 12/18/2025

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: Glasscock, Jerry D
Permit Number: 7180-9235
Effective:
02/01/2025-02/01/2027

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG405102
Exp Date: 02/20/2026

Test	g/210L	Time
DIAG	Pass	8:29am
AIR BLK	.00	8:30am
ACCY CHK	.07	8:31am
AIR BLK	.00	8:32am
SUB TEST	.00	8:32am
AIR BLK	.00	8:33am
SUB TEST	.00	8:35am
AIR BLK	.00	8:36am

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

Intox EC/IR-II: Preventive Maintenance

CABARRUS COUNTY BAT MOBILE UNIT 8 120

Serial Number: 008736 Test Record Number: 1566
Test Date: 12/18/2025 Test Time: 8:37am EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	8:37am
FLO	Pass	8:37am
FC	Pass	8:37am

Temperature Tests

Test	Status	Time
FC1	Pass	8:37am
SRC	Pass	8:37am
DET	Pass	8:37am
BAR	Pass	8:37am
BT	Pass	8:37am

Blank Tests

Test	Status	Time
AIR	Pass	8:38am


Printer Tests

Test	Status	Time
PRNT	Pass	8:38am

CRC Tests

Test	Status	Time
COMP	Pass	8:38am
CAL	Pass	8:38am

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Cabarrus Instrument Location BAT Mobile Unit 8
Instrument Serial No. 008736

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 30 day of December, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

2219283
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

CABARRUS COUNTY BAT MOBILE UNIT 8 120

Serial Number: 008736
Test Date: 12/30/2025

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Glasscock, Jerry D

Permit Number: 7180-9235

Effective:

02/01/2025-02/01/2027

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG405102

Exp Date: 02/20/2026

Test	g/210L	Time
DIAG	Pass	7:54pm
AIR BLK	.00	7:55pm
ACCY CHK	.07	7:56pm
AIR BLK	.00	7:57pm
SUB TEST	.00	7:57pm
AIR BLK	.00	7:58pm
SUB TEST	.00	7:59pm
AIR BLK	.00	8:00pm

Reported AC: .00 g/210L

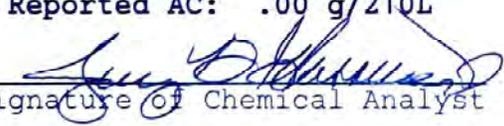
Signature of Chemical Analyst

Court CVR


Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

CABARRUS COUNTY BAT MOBILE UNIT 8 120

Serial Number: 008736 Test Record Number: 1572
Test Date: 12/30/2025 Test Time: 8:01pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	8:01pm
FLO	Pass	8:01pm
FC	Pass	8:01pm

Temperature Tests

Test	Status	Time
FC1	Pass	8:01pm
SRC	Pass	8:01pm
DET	Pass	8:01pm
BAR	Pass	8:01pm
BT	Pass	8:01pm

Blank Tests

Test	Status	Time
AIR	Pass	8:02pm

Printer Tests

Test	Status	Time
PRNT	Pass	8:02pm

CRC Tests

Test	Status	Time
COMP	Pass	8:02pm
CAL	Pass	8:02pm

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Cabarrus Instrument Location BAT Mobile Unit 8

Instrument Serial No. 008775

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 18 day of December, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

2219283
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

CABARRUS COUNTY BAT MOBILE UNIT 8 120

Serial Number: 008775
Test Date: 12/18/2025

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Glasscock, Jerry D

Permit Number: 7180-9235

Effective:

02/01/2025-02/01/2027

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG506303

Exp Date: 03/04/2027

Test	g/210L	Time
DIAG	Pass	8:27am
AIR BLK	.00	8:28am
ACCY CHK	.08	8:29am
AIR BLK	.00	8:30am
SUB TEST	.00	8:31am
AIR BLK	.00	8:32am
SUB TEST	.00	8:33am
AIR BLK	.00	8:34am

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

CABARRUS COUNTY BAT MOBILE UNIT 8 120

Serial Number: 008775 Test Record Number: 2418
Test Date: 12/18/2025 Test Time: 8:35am EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	8:35am
FLO	Pass	8:35am
FC	Pass	8:35am

Temperature Tests

Test	Status	Time
FC1	Pass	8:35am
SRC	Pass	8:35am
DET	Pass	8:35am
BAR	Pass	8:35am
BT	Pass	8:35am

Blank Tests

Test	Status	Time
AIR	Pass	8:36am

Printer Tests

Test	Status	Time
PRNT	Pass	8:36am

CRC Tests

Test	Status	Time
COMP	Pass	8:36am
CAL	Pass	8:36am

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Cabarrus Instrument Location BAT Mobile Unit 8
Instrument Serial No. 008775

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 30 day of December, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

2219283
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

CABARRUS COUNTY BAT MOBILE UNIT 8 120

Serial Number: 008775
Test Date: 12/30/2025

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE

Analyst's Name: Glasscock, Jerry D
Permit Number: 7180-9235
Effective:
02/01/2025-02/01/2027

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG506303
Exp Date: 03/04/2027

Test	g/210L	Time
DIAG	Pass	7:53pm
AIR BLK	.00	7:54pm
ACCY CHK	.08	7:55pm
AIR BLK	.00	7:56pm
SUB TEST	.00	7:57pm
AIR BLK	.00	7:58pm
SUB TEST	.00	7:59pm
AIR BLK	.00	8:00pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

Intox EC/IR-II: Preventive Maintenance

CABARRUS COUNTY BAT MOBILE UNIT 8 120

Serial Number: 008775 Test Record Number: 2423
Test Date: 12/30/2025 Test Time: 8:01pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	8:01pm
FLO	Pass	8:01pm
FC	Pass	8:01pm

Temperature Tests

Test	Status	Time
FC1	Pass	8:01pm
SRC	Pass	8:01pm
DET	Pass	8:01pm
BAR	Pass	8:01pm
BT	Pass	8:01pm

Blank Tests

Test	Status	Time
AIR	Pass	8:02pm

Printer Tests

Test	Status	Time
PRNT	Pass	8:02pm

CRC Tests

Test	Status	Time
COMP	Pass	8:02pm
CAL	Pass	8:02pm

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Cabarrus Instrument Location BAT Mobile Unit 8
Instrument Serial No. 008816

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 30 day of December, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

2219283
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

CABARRUS COUNTY BAT MOBILE UNIT 8 120

Serial Number: 008816
Test Date: 12/30/2025

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Glasscock, Jerry D

Permit Number: 7180-9235

Effective:

02/01/2025-02/01/2027

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG431002

Exp Date: 11/05/2026

Test	g/210L	Time
DIAG	Pass	7:53pm
AIR BLK	.00	7:54pm
ACCY CHK	.08	7:55pm
AIR BLK	.00	7:56pm
SUB TEST	.00	7:57pm
AIR BLK	.00	7:58pm
SUB TEST	.00	8:00pm
AIR BLK	.00	8:00pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

CABARRUS COUNTY BAT MOBILE UNIT 8 120

Serial Number: 008816 Test Record Number: 8006
Test Date: 12/30/2025 Test Time: 8:01pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	8:01pm
FLO	Pass	8:01pm
FC	Pass	8:01pm

Temperature Tests

Test	Status	Time
FC1	Pass	8:01pm
SRC	Pass	8:01pm
DET	Pass	8:01pm
BAR	Pass	8:01pm
BT	Pass	8:01pm

Blank Tests

Test	Status	Time
AIR	Pass	8:02pm

Printer Tests

Test	Status	Time
PRNT	Pass	8:02pm

CRC Tests

Test	Status	Time
COMP	Pass	8:02pm
CAL	Pass	8:02pm

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Cabarrus Instrument Location BAT Mobile Unit 8
Instrument Serial No. 008816 —

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 18 day of December, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

2219283
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

CABARRUS COUNTY BAT MOBILE UNIT 8 120

Serial Number: 008816
Test Date: 12/18/2025

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Glasscock, Jerry D

Permit Number: 7180-9235

Effective:

02/01/2025-02/01/2027

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG431002

Exp Date: 11/05/2026

Test	g/210L	Time
DIAG	Pass	8:26am
AIR BLK	.00	8:27am
ACCY CHK	.07	8:28am
AIR BLK	.00	8:29am
SUB TEST	.00	8:30am
AIR BLK	.00	8:31am
SUB TEST	.00	8:32am
AIR BLK	.00	8:33am

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

Intox EC/IR-II: Preventive Maintenance

CABARRUS COUNTY BAT MOBILE UNIT 8 120

Serial Number: 008816 Test Record Number: 8002
Test Date: 12/18/2025 Test Time: 8:34am EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	8:34am
FLO	Pass	8:34am
FC	Pass	8:34am

Temperature Tests

Test	Status	Time
FC1	Pass	8:34am
SRC	Pass	8:34am
DET	Pass	8:34am
BAR	Pass	8:34am
BT	Pass	8:34am

Blank Tests

Test	Status	Time
AIR	Pass	8:35am


Printer Tests

Test	Status	Time
PRNT	Pass	8:35am

CRC Tests

Test	Status	Time
COMP	Pass	8:35am
CAL	Pass	8:35am

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Cabarrus Instrument Location BAT Mobile Unit 8

Instrument Serial No. 008929 _____

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 18 day of December, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Judy O. Hampton
Signature of Certifying Official

2219283
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

CABARRUS COUNTY BAT MOBILE UNIT 8 120

Serial Number: 008929

Test Date: 12/18/2025

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Glasscock, Jerry D

Permit Number: 7180-9235

Effective:

02/01/2025-02/01/2027

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG506303

Exp Date: 03/04/2027

Test	g/210L	Time
DIAG	Pass	8:25am
AIR BLK	.00	8:26am
ACCY CHK	.08	8:27am
AIR BLK	.00	8:28am
SUB TEST	.00	8:28am
AIR BLK	.00	8:30am
SUB TEST	.00	8:31am
AIR BLK	.00	8:32am

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

This form is used when performing Preventive Maintenance procedures

Forensic Tests for Alcohol Branch

Department of Health and Human Services

Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

CABARRUS COUNTY BAT MOBILE UNIT 8 120

Serial Number: 008929 Test Record Number: 1703
Test Date: 12/18/2025 Test Time: 8:33am EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	8:33am
FLO	Pass	8:33am
FC	Pass	8:33am

Temperature Tests

Test	Status	Time
FC1	Pass	8:33am
SRC	Pass	8:33am
DET	Pass	8:33am
BAR	Pass	8:33am
BT	Pass	8:33am

Blank Tests

Test	Status	Time
AIR	Pass	8:34am


Printer Tests

Test	Status	Time
PRNT	Pass	8:34am

CRC Tests

Test	Status	Time
COMP	Pass	8:34am
CAL	Pass	8:34am

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Cabarrus Instrument Location BAT Mobile Unit 8

Instrument Serial No. 808929 _____

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 30 day of December, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

2219283
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

CABARRUS COUNTY BAT MOBILE UNIT 8 120

Serial Number: 008929

Test Date: 12/30/2025

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Glasscock, Jerry D

Permit Number: 7180-9235

Effective:

02/01/2025-02/01/2027

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG506303

Exp Date: 03/04/2027

Test	g/210L	Time
DIAG	Pass	7:52pm
AIR BLK	.00	7:53pm
ACCY CHK	.08	7:54pm
AIR BLK	.00	7:55pm
SUB TEST	.00	7:55pm
AIR BLK	.00	7:56pm
SUB TEST	.00	7:58pm
AIR BLK	.00	7:59pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

CABARRUS COUNTY BAT MOBILE UNIT 8 120

Serial Number: 008929 Test Record Number: 1707
Test Date: 12/30/2025 Test Time: 8:00pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	8:00pm
FLO	Pass	8:00pm
FC	Pass	8:01pm

Temperature Tests

Test	Status	Time
FC1	Pass	8:01pm
SRC	Pass	8:01pm
DET	Pass	8:01pm
BAR	Pass	8:01pm
BT	Pass	8:01pm

Blank Tests

Test	Status	Time
AIR	Pass	8:01pm

Printer Tests

Test	Status	Time
PRNT	Pass	8:02pm

CRC Tests

Test	Status	Time
COMP	Pass	8:02pm
CAL	Pass	8:02pm

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County Caldwell Instrument Location Caldwell Co. Jail

Instrument Serial No. 008719 LE-1012 NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 01 day of DECEMBER, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

274970
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

CALDWELL COUNTY CALDWELL COUNTY JAIL
130

Serial Number: 008719
Test Date: 12/01/2025

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Fleming, Tina S

Permit Number: 0027-4970

Effective:

02/01/2025-02/01/2027

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG431001


Exp Date: 11/05/2026

Test	g/210L	Time
DIAG	Pass	1:28pm
AIR BLK	.00	1:28pm
ACCY CHK	.08	1:29pm
AIR BLK	.00	1:30pm
SUB TEST	.00	1:31pm
AIR BLK	.00	1:32pm
SUB TEST	.00	1:33pm
AIR BLK	.00	1:34pm

Reported AC: .00 g/210L



Signature of Chemical Analyst
Court CVR



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

CALDWELL COUNTY CALDWELL COUNTY JAIL 130

Serial Number: 008719 Test Record Number: 3611
Test Date: 12/01/2025 Test Time: 1:35pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	1:35pm
FLO	Pass	1:35pm
FC	Pass	1:35pm

Temperature Tests

Test	Status	Time
FC1	Pass	1:35pm
SRC	Pass	1:35pm
DET	Pass	1:35pm
BAR	Pass	1:35pm
BT	Pass	1:35pm

Blank Tests

Test	Status	Time
AIR	Pass	1:36pm


Printer Tests

Test	Status	Time
PRNT	Pass	1:36pm

CRC Tests

Test	Status	Time
COMP	Pass	1:36pm
CAL	Pass	1:36pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Camden Instrument Location Camden Co. S.O.
Instrument Serial No. 008940 117 N. Carolina Hwy. 343
Camden, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 15th day of December, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

206272
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

CAMDEN COUNTY CAMDEN CO SO 140

Serial Number: 008940
Test Date: 12/15/2025

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE

Analyst's Name: Chappell, Mark A
Permit Number: 0020-6272
Effective:
02/01/2025-02/01/2027

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test


Lot Number: AG516203
Exp Date: 06/11/2027

Test	g/210L	Time
DIAG	Pass	9:32am
AIR BLK	.00	9:33am
ACCY CHK	.08	9:34am
AIR BLK	.00	9:35am
SUB TEST	.00	9:36am
AIR BLK	.00	9:37am
SUB TEST	.00	9:38am
AIR BLK	.00	9:39am

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR

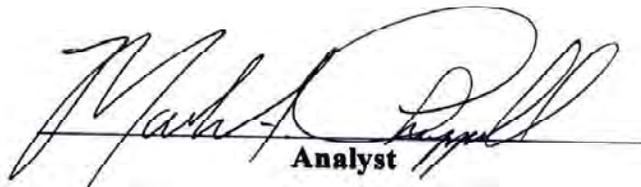
Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

CAMDEN COUNTY CAMDEN CO SO 140

Serial Number: 008940 Test Record Number: 1373
Test Date: 12/15/2025 Test Time: 9:40am EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	9:40am
FLO	Pass	9:40am
FC	Pass	9:40am

Temperature Tests

Test	Status	Time
FC1	Pass	9:40am
SRC	Pass	9:40am
DET	Pass	9:40am
BAR	Pass	9:40am
BT	Pass	9:40am

Blank Tests

Test	Status	Time
AIR	Pass	9:41am


Printer Tests

Test	Status	Time
PRNT	Pass	9:41am

CRC Tests

Test	Status	Time
COMP	Pass	9:41am
CAL	Pass	9:41am

Preventive Maintenance
Status: Pass

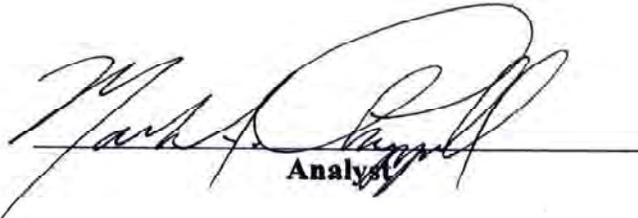
Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County CATAWBA Instrument Location CATAWBA COUNTY 90
Instrument Serial No. 008687 NEWTON, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 01 day of NOVEMBER, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

274970
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

CATAWBA COUNTY CATAWBA COUNTY SO 170

Serial Number: 008687
Test Date: 12/01/2025

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Fleming, Tina S

Permit Number: 0027-4970

Effective:

02/01/2025-02/01/2027

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG516203

Exp Date: 06/11/2027


Test	g/210L	Time
DIAG	Pass	10:30am
AIR BLK	.00	10:31am
ACCY CHK	.08	10:31am
AIR BLK	.00	10:32am
SUB TEST	.00	10:34am
AIR BLK	.00	10:35am
SUB TEST	.00	10:37am
AIR BLK	.00	10:38am

Reported AC: .00 g/210L

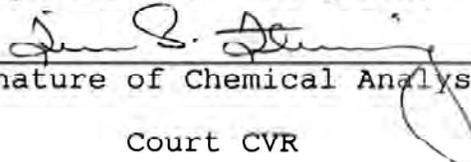

Signature of Chemical Analyst

Court CVR

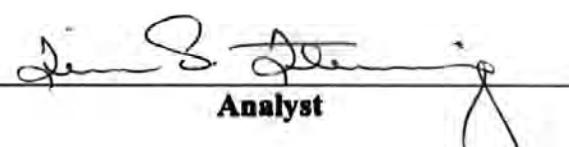

Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

CATAWBA COUNTY CATAWBA COUNTY SO 170

Serial Number: 008687 Test Record Number: 4297
Test Date: 12/01/2025 Test Time: 10:40am EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	10:40am
FLO	Pass	10:40am
FC	Pass	10:40am

Temperature Tests

Test	Status	Time
FC1	Pass	10:40am
SRC	Pass	10:40am
DET	Pass	10:40am
BAR	Pass	10:40am
BT	Pass	10:40am

Blank Tests

Test	Status	Time
AIR	Pass	10:41am


Printer Tests

Test	Status	Time
PRNT	Pass	10:41am

CRC Tests

Test	Status	Time
COMP	Pass	10:41am
CAL	Pass	10:41am

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County CATAWBA Instrument Location CATAWBA COUNTY SC
Instrument Serial No. 008821 Newton, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 01 day of DECEMBER, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

274970
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

CATAWBA COUNTY CATAWBA COUNTY SO 170

Serial Number: 008821
Test Date: 12/01/2025

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Fleming, Tina S

Permit Number: 0027-4970

Effective:

02/01/2025-02/01/2027

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG516203

Exp Date: 06/11/2027


Test	g/210L	Time
DIAG	Pass	11:08am
AIR BLK	.00	11:08am
ACCY CHK	.07	11:09am
AIR BLK	.00	11:10am
SUB TEST	.00	11:11am
AIR BLK	.00	11:12am
SUB TEST	.00	11:13am
AIR BLK	.00	11:14am

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

CATAWBA COUNTY CATAWBA COUNTY SO 170

Serial Number: 008821 Test Record Number: 2672
Test Date: 12/01/2025 Test Time: 11:15am EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	11:15am
FLO	Pass	11:15am
FC	Pass	11:15am

Temperature Tests

Test	Status	Time
FC1	Pass	11:15am
SRC	Pass	11:15am
DET	Pass	11:15am
BAR	Pass	11:15am
BT	Pass	11:15am

Blank Tests

Test	Status	Time
AIR	Pass	11:16am


Printer Tests

Test	Status	Time
PRNT	Pass	11:16am

CRC Tests

Test	Status	Time
COMP	Pass	11:16am
CAL	Pass	11:16am

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County Cherokee Instrument Location BAT Mobile Unit 11

Instrument Serial No. 008970

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 20th day of December, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

62446
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

CHEROKEE COUNTY BAT MOBILE UNIT 11 190

Serial Number: 008970

Test Date: 12/20/2025

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Gillstrap, Jeffrey L

Permit Number: 0006-2446

Effective:

04/01/2025-04/01/2027

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG417802

Exp Date: 06/26/2026

Test	g/210L	Time
DIAG	Pass	8:50pm
AIR BLK	.00	8:51pm
ACCY CHK	.07	8:52pm
AIR BLK	.00	8:53pm
SUB TEST	.00	8:53pm
AIR BLK	.00	8:54pm
SUB TEST	.00	8:56pm
AIR BLK	.00	8:57pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

Intox EC/IR-II: Preventive Maintenance

CHEROKEE COUNTY BAT MOBILE UNIT 11 190

Serial Number: 008970 Test Record Number: 1354
Test Date: 12/20/2025 Test Time: 8:57pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	8:58pm
FLO	Pass	8:58pm
FC	Pass	8:58pm

Temperature Tests

Test	Status	Time
FC1	Pass	8:58pm
SRC	Pass	8:58pm
DET	Pass	8:58pm
BAR	Pass	8:58pm
BT	Pass	8:58pm

Blank Tests

Test	Status	Time
AIR	Pass	8:58pm


Printer Tests

Test	Status	Time
PRNT	Pass	8:58pm

CRC Tests

Test	Status	Time
COMP	Pass	8:59pm
CAL	Pass	8:59pm

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County Cherokee Instrument Location BAT Mobile Unit 11

Instrument Serial No. 008973

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 20~~14~~ day of December, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Jeff Goldstein
Signature of Certifying Official

62446
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

CHEROKEE COUNTY BAT MOBILE UNIT 11 190

Serial Number: 008973
Test Date: 12/20/2025

Citation Number: M0000000-0
Subject's Name: NONE, NONE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: Gillstrap, Jeffrey L.
Permit Number: 0006-2446
Effective:
04/01/2025-04/01/2027

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG431003
Exp Date: 11/05/2026

Test	g/210L	Time
DIAG	Pass	9:00pm
AIR BLK	.00	9:01pm
ACCY CHK	.07	9:02pm
AIR BLK	.00	9:03pm
SUB TEST	.00	9:04pm
AIR BLK	.00	9:04pm
SUB TEST	.00	9:06pm
AIR BLK	.00	9:07pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

Intox EC/IR-II: Preventive Maintenance

CHEROKEE COUNTY BAT MOBILE UNIT 11 190

Serial Number: 008973 Test Record Number: 1406
Test Date: 12/20/2025 Test Time: 9:09pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	9:10pm
FLO	Pass	9:10pm
FC	Pass	9:10pm

Temperature Tests

Test	Status	Time
FC1	Pass	9:10pm
SRC	Pass	9:10pm
DET	Pass	9:10pm
BAR	Pass	9:10pm
BT	Pass	9:10pm

Blank Tests

Test	Status	Time
AIR	Pass	9:11pm

Printer Tests

Test	Status	Time
PRNT	Pass	9:11pm

CRC Tests

Test	Status	Time
COMP	Pass	9:11pm
CAL	Pass	9:11pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County COLUMBUS Instrument Location COLUMBUS COUNTY
Instrument Serial No. 008875 DETENTION CENTER

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 15 day of DECEMBER, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Alan Rg Burns

Signature of Certifying Official

146279

Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

COLUMBUS COUNTY DETENTION CENTER 230

Serial Number: 008875
Test Date: 12/15/2025

Citation Number: M0000000-0
Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: BARNES, ALVIN R

Permit Number: 0014-6279

Effective:

02/01/2025-02/01/2027

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG516204

Exp Date: 06/11/2027


Test	g/210L	Time
DIAG	Pass	1:07pm
AIR BLK	.00	1:07pm
ACCY CHK	.08	1:08pm
AIR BLK	.00	1:09pm
SUB TEST	.00	1:10pm
AIR BLK	.00	1:11pm
SUB TEST	.00	1:13pm
AIR BLK	.00	1:13pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

Intox EC/IR-II: Preventive Maintenance

COLUMBUS COUNTY DETENTION CENTER 230

Serial Number: '008875 Test Record Number: 3373
Test Date: 12/15/2025 Test Time: 1:14pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	1:14pm
FLO	Pass	1:14pm
FC	Pass	1:15pm

Temperature Tests

Test	Status	Time
FC1	Pass	1:15pm
SRC	Pass	1:15pm
DET	Pass	1:15pm
BAR	Pass	1:15pm
BT	Pass	1:15pm

Blank Tests

Test	Status	Time
AIR	Pass	1:15pm

Printer Tests

Test	Status	Time
PRNT	Pass	1:15pm

CRC Tests

Test	Status	Time
COMP	Pass	1:16pm
CAL	Pass	1:16pm

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County COLUMBUS Instrument Location COLUMBUS COUNTY
Instrument Serial No. 008886 DETENTION CENTER

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 15 day of DECEMBER, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Alan Ray Barnes
Signature of Certifying Official

146279
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

COLUMBUS COUNTY DETENTION CENTER 230

Serial Number: 008886
Test Date: 12/15/2025

Citation Number: M0000000-0
Subject's Name:

PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: BARNES, ALVIN R
Permit Number: 0014-6279
Effective:
02/01/2025-02/01/2027

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG501307
Exp Date: 01/13/2027


Test	g/210L	Time
DIAG	Pass	1:38pm
AIR BLK	.00	1:39pm
ACCY CHK	.08	1:40pm
AIR BLK	.00	1:41pm
SUB TEST	.00	1:42pm
AIR BLK	.00	1:43pm
SUB TEST	.00	1:44pm
AIR BLK	.00	1:45pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

COLUMBUS COUNTY DETENTION CENTER 230

Serial Number: 008886 Test Record Number: 1935
Test Date: 12/15/2025 Test Time: 1:46pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	1:46pm
FLO	Pass	1:46pm
FC	Pass	1:46pm

Temperature Tests

Test	Status	Time
FC1	Pass	1:46pm
SRC	Pass	1:46pm
DET	Pass	1:46pm
BAR	Pass	1:46pm
BT	Pass	1:46pm

Blank Tests

Test	Status	Time
AIR	Pass	1:47pm


Printer Tests

Test	Status	Time
PRNT	Pass	1:47pm

CRC Tests

Test	Status	Time
COMP	Pass	1:47pm
CAL	Pass	1:47pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Cumberland Instrument Location Hope Mills
Instrument Serial No. 008614 Police Department

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 2 day of December, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

365156
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

CUMBERLAND COUNTY HOPE MILLS PD 250

Serial Number: 008614
Test Date: 12/02/2025

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: Garner, Joel K
Permit Number: 0036-5156
Effective:
02/01/2025-02/01/2027

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG417802
Exp Date: 06/26/2026

Test	g/210L	Time
DIAG	Pass	9:02am
AIR BLK	.00	9:03am
ACCY CHK	.07	9:04am
AIR BLK	.00	9:05am
SUB TEST	.00	9:05am
AIR BLK	.00	9:06am
SUB TEST	.00	9:08am
AIR BLK	.00	9:09am

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

CUMBERLAND COUNTY HOPE MILLS PD 250

Serial Number: 008614 Test Record Number: 5225
Test Date: 12/02/2025 Test Time: 9:19am EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	9:20am
FLO	Pass	9:20am
FC	Pass	9:20am

Temperature Tests

Test	Status	Time
FC1	Pass	9:20am
SRC	Pass	9:20am
DET	Pass	9:20am
BAR	Pass	9:20am
BT	Pass	9:20am

Blank Tests

Test	Status	Time
AIR	Pass	9:21am

Printer Tests

Test	Status	Time
PRNT	Pass	9:21am

CRC Tests

Test	Status	Time
COMP	Pass	9:21am
CAL	Pass	9:21am

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Currituck Instrument Location Currituck Co. S.O.
Instrument Serial No. 008947 407A Maple Rd. Maple, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 1st day of December, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

206272
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

CURRITUCK COUNTY CURRITUCK SO-MAPLE
260

Serial Number: 008947
Test Date: 12/01/2025

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: Chappell, Mark A
Permit Number: 0020-6272
Effective:
02/01/2025-02/01/2027

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test


Lot Number: AG516203
Exp Date: 06/11/2027

Test	g/210L	Time
DIAG	Pass	2:25pm
AIR BLK	.00	2:26pm
ACCY CHK	.07	2:26pm
AIR BLK	.00	2:27pm
SUB TEST	.00	2:28pm
AIR BLK	.00	2:29pm
SUB TEST	.00	2:31pm
AIR BLK	.00	2:32pm

Reported AC: .00 g/210L

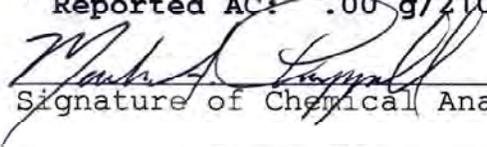
Signature of Chemical Analyst

Court CVR

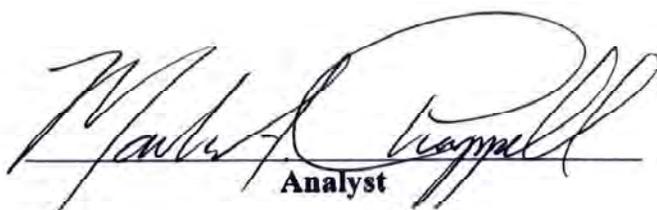
Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

CURRITUCK COUNTY CURRITUCK SO-MAPLE 260

Serial Number: 008947 Test Record Number: 3717
Test Date: 12/01/2025 Test Time: 2:33pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	2:33pm
FLO	Pass	2:33pm
FC	Pass	2:34pm

Temperature Tests

Test	Status	Time
FC1	Pass	2:34pm
SRC	Pass	2:34pm
DET	Pass	2:34pm
BAR	Pass	2:34pm
BT	Pass	2:34pm

Blank Tests

Test	Status	Time
AIR	Pass	2:34pm

Printer Tests

Test	Status	Time
PRNT	Pass	2:34pm

CRC Tests

Test	Status	Time
COMP	Pass	2:34pm
CAL	Pass	2:34pm

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County Dare Instrument Location Kill Devil Hills P.D.
Instrument Serial No. 008844 102 Town Hall Dr.,
Kill Devil Hills, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 19th day of December, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

206272
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

DARE COUNTY KILL DEVIL HILLS PD 270

Serial Number: 008844
Test Date: 12/19/2025

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Chappell, Mark A

Permit Number: 0020-6272

Effective:

02/01/2025-02/01/2027

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG516203


Exp Date: 06/11/2027

Test	g/210L	Time
DIAG	Pass	12:31pm
AIR BLK	.00	12:31pm
ACCY CHK	.08	12:32pm
AIR BLK	.00	12:33pm
SUB TEST	.00	12:34pm
AIR BLK	.00	12:35pm
SUB TEST	.00	12:36pm
AIR BLK	.00	12:37pm

Reported AC: .00 g/210L

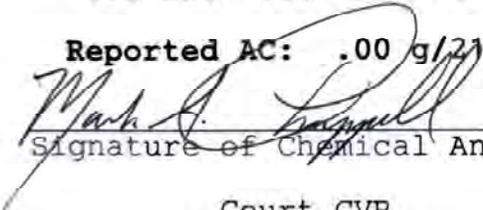
Signature of Chemical Analyst

Court CVR

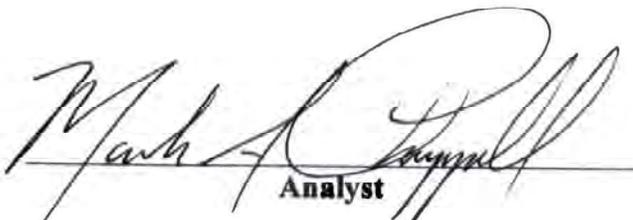
Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

DARE COUNTY KILL DEVIL HILLS PD 270

Serial Number: 008844 Test Record Number: 3359
Test Date: 12/19/2025 Test Time: 12:38pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	12:38pm
FLO	Pass	12:38pm
FC	Pass	12:38pm

Temperature Tests

Test	Status	Time
FC1	Pass	12:39pm
SRC	Pass	12:39pm
DET	Pass	12:39pm
BAR	Pass	12:39pm
BT	Pass	12:39pm

Blank Tests

Test	Status	Time
AIR	Pass	12:39pm


Printer Tests

Test	Status	Time
PRNT	Pass	12:39pm

CRC Tests

Test	Status	Time
COMP	Pass	12:39pm
CAL	Pass	12:39pm

Preventive Maintenance
Status: Pass

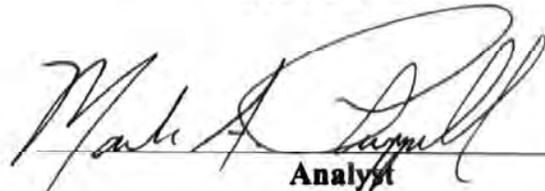

Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Davidson Instrument Location BAT Mobile Unit 8
Instrument Serial No. 008615

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 12 day of December, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Jay D. [Signature]
Signature of Certifying Official

2219283
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

DAVIDSON COUNTY BAT MOBILE UNIT 8 280

Serial Number: 008615

Test Date: 12/12/2025

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Glasscock, Jerry D

Permit Number: 7180-9235

Effective:

02/01/2025-02/01/2027

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG405102

Exp Date: 02/20/2026

Test	g/210L	Time
DIAG	Pass	9:46pm
AIR BLK	.00	9:47pm
ACCY CHK	.07	9:47pm
AIR BLK	.00	9:48pm
SUB TEST	.00	9:49pm
AIR BLK	.00	9:50pm
SUB TEST	.00	9:52pm
AIR BLK	.00	9:52pm

Reported AC: .00 g/210L

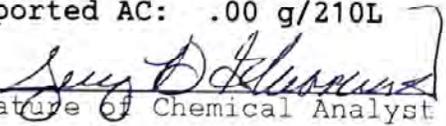
Signature of Chemical Analyst

Court CVR


Analyst

This form is used when performing Preventive Maintenance procedures

Forensic Tests for Alcohol Branch

Department of Health and Human Services

Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

DAVIDSON COUNTY BAT MOBILE UNIT 8 280

Serial Number: 008615 Test Record Number: 6202
Test Date: 12/12/2025 Test Time: 9:53pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	9:53pm
FLO	Pass	9:53pm
FC	Pass	9:53pm

Temperature Tests

Test	Status	Time
FC1	Pass	9:54pm
SRC	Pass	9:54pm
DET	Pass	9:54pm
BAR	Pass	9:54pm
BT	Pass	9:54pm

Blank Tests

Test	Status	Time
AIR	Pass	9:54pm

Printer Tests

Test	Status	Time
PRNT	Pass	9:54pm

CRC Tests

Test	Status	Time
COMP	Pass	9:54pm
CAL	Pass	9:54pm

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County Davidson Instrument Location BAT Mobile Unit 8
Instrument Serial No. 008615

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 31 day of December, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

2219283
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

DAVIDSON COUNTY BAT MOBILE UNIT 8 280

Serial Number: 008615
Test Date: 12/31/2025

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Glasscock, Jerry D

Permit Number: 7180-9235

Effective:

02/01/2025-02/01/2027

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG405102

Exp Date: 02/20/2026

Test	g/210L	Time
DIAG	Pass	8:35pm
AIR BLK	.00	8:36pm
ACCY CHK	.07	8:37pm
AIR BLK	.00	8:38pm
SUB TEST	.00	8:38pm
AIR BLK	.00	8:39pm
SUB TEST	.00	8:41pm
AIR BLK	.00	8:42pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

DAVIDSON COUNTY BAT MOBILE UNIT 8 280

Serial Number: 008615 Test Record Number: 6216
Test Date: 12/31/2025 Test Time: 8:43pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	8:44pm
FLO	Pass	8:44pm
FC	Pass	8:44pm

Temperature Tests

Test	Status	Time
FC1	Pass	8:44pm
SRC	Pass	8:44pm
DET	Pass	8:44pm
BAR	Pass	8:44pm
BT	Pass	8:44pm

Blank Tests

Test	Status	Time
AIR	Pass	8:44pm

Printer Tests

Test	Status	Time
PRNT	Pass	8:45pm

CRC Tests

Test	Status	Time
COMP	Pass	8:45pm
CAL	Pass	8:45pm

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County Davidson Instrument Location BAT Mobile Unit 8
Instrument Serial No. 008736 -

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 12 day of December, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

2219283
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

DAVIDSON COUNTY BAT MOBILE UNIT 8 280

Serial Number: 008736
Test Date: 12/12/2025

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE

Analyst's Name: Glasscock, Jerry D
Permit Number: 7180-9235
Effective:
02/01/2025-02/01/2027

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG405102
Exp Date: 02/20/2026

Test	g/210L	Time
DIAG	Pass	9:44pm
AIR BLK	.00	9:45pm
ACCY CHK	.07	9:46pm
AIR BLK	.00	9:47pm
SUB TEST	.00	9:48pm
AIR BLK	.00	9:49pm
SUB TEST	.00	9:50pm
AIR BLK	.00	9:51pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

Intox EC/IR-II: Preventive Maintenance

DAVIDSON COUNTY BAT MOBILE UNIT 8 280

Serial Number: 008736 Test Record Number: 1562
Test Date: 12/12/2025 Test Time: 9:52pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	9:52pm
FLO	Pass	9:52pm
FC	Pass	9:52pm

Temperature Tests

Test	Status	Time
FC1	Pass	9:52pm
SRC	Pass	9:52pm
DET	Pass	9:52pm
BAR	Pass	9:52pm
BT	Pass	9:52pm

Blank Tests

Test	Status	Time
AIR	Pass	9:53pm

Printer Tests

Test	Status	Time
PRNT	Pass	9:53pm

CRC Tests

Test	Status	Time
COMP	Pass	9:53pm
CAL	Pass	9:53pm

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Davidson Instrument Location BAT Mobile Unit 8

Instrument Serial No. 008736 _____

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 31 day of December, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

2219283
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

DAVIDSON COUNTY BAT MOBILE UNIT 8 280

Serial Number: 008736

Test Date: 12/31/2025

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Glasscock, Jerry D

Permit Number: 7180-9235

Effective:

02/01/2025-02/01/2027

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG405102

Exp Date: 02/20/2026

Test	g/210L	Time
DIAG	Pass	8:33pm
AIR BLK	.00	8:34pm
ACCY CHK	.07	8:35pm
AIR BLK	.00	8:35pm
SUB TEST	.00	8:36pm
AIR BLK	.00	8:37pm
SUB TEST	.00	8:39pm
AIR BLK	.00	8:39pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

Intox EC/IR-II: Preventive Maintenance

DAVIDSON COUNTY BAT MOBILE UNIT 8 280

Serial Number: 008736 Test Record Number: 1574
Test Date: 12/31/2025 Test Time: 8:40pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	8:40pm
FLO	Pass	8:40pm
FC	Pass	8:41pm

Temperature Tests

Test	Status	Time
FC1	Pass	8:41pm
SRC	Pass	8:41pm
DET	Pass	8:41pm
BAR	Pass	8:41pm
BT	Pass	8:41pm

Blank Tests

Test	Status	Time
AIR	Pass	8:41pm

Printer Tests

Test	Status	Time
PRNT	Pass	8:41pm

CRC Tests

Test	Status	Time
COMP	Pass	8:41pm
CAL	Pass	8:42pm

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Davidson Instrument Location BAT Mobile Unit 8
Instrument Serial No. 008775

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 12 day of December, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

2219283
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

DAVIDSON COUNTY BAT MOBILE UNIT 8 280

Serial Number: 008775

Test Date: 12/12/2025

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Glasscock, Jerry D

Permit Number: 7180-9235

Effective:

02/01/2025-02/01/2027

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG506303

Exp Date: 03/04/2027

Test	g/210L	Time
DIAG	Pass	9:44pm
AIR BLK	.00	9:45pm
ACCY CHK	.08	9:45pm
AIR BLK	.00	9:47pm
SUB TEST	.00	9:48pm
AIR BLK	.00	9:49pm
SUB TEST	.00	9:50pm
AIR BLK	.00	9:51pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

DAVIDSON COUNTY BAT MOBILE UNIT 8 280

Serial Number: 008775 Test Record Number: 2413
Test Date: 12/12/2025 Test Time: 9:52pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	9:52pm
FLO	Pass	9:52pm
FC	Pass	9:52pm

Temperature Tests

Test	Status	Time
FC1	Pass	9:52pm
SRC	Pass	9:52pm
DET	Pass	9:52pm
BAR	Pass	9:52pm
BT	Pass	9:52pm

Blank Tests

Test	Status	Time
AIR	Pass	9:53pm


Printer Tests

Test	Status	Time
PRNT	Pass	9:53pm

CRC Tests

Test	Status	Time
COMP	Pass	9:53pm
CAL	Pass	9:53pm

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Davidson Instrument Location BAT Mobile Unit 8

Instrument Serial No. 008775 _____

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 31 day of December, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

2219283
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

DAVIDSON COUNTY BAT MOBILE UNIT 8 280

Serial Number: 008775
Test Date: 12/31/2025

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: Glasscock, Jerry D
Permit Number: 7180-9235
Effective:
02/01/2025-02/01/2027

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG506303
Exp Date: 03/04/2027

Test	g/210L	Time
DIAG	Pass	8:28pm
AIR BLK	.00	8:29pm
ACCY CHK	.08	8:30pm
AIR BLK	.00	8:31pm
SUB TEST	.00	8:32pm
AIR BLK	.00	8:33pm
SUB TEST	.00	8:34pm
AIR BLK	.00	8:35pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

Intox EC/IR-II: Preventive Maintenance

DAVIDSON COUNTY BAT MOBILE UNIT 8 280

Serial Number: 008775 Test Record Number: 2428
Test Date: 12/31/2025 Test Time: 8:40pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	8:40pm
FLO	Pass	8:40pm
FC	Pass	8:40pm

Temperature Tests

Test	Status	Time
FC1	Pass	8:40pm
SRC	Pass	8:40pm
DET	Pass	8:40pm
BAR	Pass	8:40pm
BT	Pass	8:40pm

Blank Tests

Test	Status	Time
AIR	Pass	8:41pm

Printer Tests

Test	Status	Time
PRNT	Pass	8:41pm

CRC Tests

Test	Status	Time
COMP	Pass	8:41pm
CAL	Pass	8:41pm

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Davidson Instrument Location BAT Mobile Unit B
Instrument Serial No. 008816

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 12 day of December, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

2219283
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

DAVIDSON COUNTY BAT MOBILE UNIT 8 280

Serial Number: 008816

Test Date: 12/12/2025

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Glasscock, Jerry D

Permit Number: 7180-9235

Effective:

02/01/2025-02/01/2027

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG431002

Exp Date: 11/05/2026

Test	g/210L	Time
DIAG	Pass	9:44pm
AIR BLK	.00	9:45pm
ACCY CHK	.07	9:45pm
AIR BLK	.00	9:46pm
SUB TEST	.00	9:47pm
AIR BLK	.00	9:48pm
SUB TEST	.00	9:50pm
AIR BLK	.00	9:51pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

DAVIDSON COUNTY BAT MOBILE UNIT 8 280

Serial Number: 008816 Test Record Number: 7997
Test Date: 12/12/2025 Test Time: 9:51pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	9:52pm
FLO	Pass	9:52pm
FC	Pass	9:52pm

Temperature Tests

Test	Status	Time
FC1	Pass	9:52pm
SRC	Pass	9:52pm
DET	Pass	9:52pm
BAR	Pass	9:52pm
BT	Pass	9:52pm

Blank Tests

Test	Status	Time
AIR	Pass	9:52pm

Printer Tests

Test	Status	Time
PRNT	Pass	9:52pm

CRC Tests

Test	Status	Time
COMP	Pass	9:53pm
CAL	Pass	9:53pm

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Davidson Instrument Location BAT Mobile Unit 8

Instrument Serial No. 008816

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 31 day of December, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

2219283
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

DAVIDSON COUNTY BAT MOBILE UNIT 8 280

Serial Number: 008816

Test Date: 12/31/2025

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Glasscock, Jerry D

Permit Number: 7180-9235

Effective:

02/01/2025-02/01/2027

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG431002

Exp Date: 11/05/2026

Test	g/210L	Time
DIAG	Pass	8:28pm
AIR BLK	.00	8:29pm
ACCY CHK	.07	8:29pm
AIR BLK	.00	8:30pm
SUB TEST	.00	8:32pm
AIR BLK	.00	8:33pm
SUB TEST	.00	8:35pm
AIR BLK	.00	8:35pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

This form is used when performing Preventive Maintenance procedures

Forensic Tests for Alcohol Branch

Department of Health and Human Services

Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

DAVIDSON COUNTY BAT MOBILE UNIT 8 280

Serial Number: 008816 Test Record Number: 8010
Test Date: 12/31/2025 Test Time: 8:36pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	8:37pm
FLO	Pass	8:37pm
FC	Pass	8:37pm

Temperature Tests

Test	Status	Time
FC1	Pass	8:37pm
SRC	Pass	8:37pm
DET	Pass	8:37pm
BAR	Pass	8:37pm
BT	Pass	8:37pm

Blank Tests

Test	Status	Time
AIR	Pass	8:37pm

Printer Tests

Test	Status	Time
PRNT	Pass	8:37pm

CRC Tests

Test	Status	Time
COMP	Pass	8:38pm
CAL	Pass	8:38pm

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County DAVIDSON Instrument Location DAVIDSON COUNTY JAIL

Instrument Serial No. 008845 Lexington, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 1st day of December, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.




Signature of Certifying Official

509387
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

DAVIDSON COUNTY DAVIDSON COUNTY JAIL
280

Serial Number: 008845
Test Date: 12/01/2025

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Long, Thomas A

Permit Number: 0050-9387

Effective:

09/01/2025-09/01/2027

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG503001

Exp Date: 01/30/2027

Test	g/210L	Time
DIAG	Pass	12:43pm
AIR BLK	.00	12:44pm
ACCY CHK	.07	12:44pm
AIR BLK	.00	12:45pm
SUB TEST	.00	12:46pm
AIR BLK	.00	12:47pm
SUB TEST	.00	12:48pm
AIR BLK	.00	12:49pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

DAVIDSON COUNTY DAVIDSON COUNTY JAIL 280

Serial Number: 008845 Test Record Number: 4617
Test Date: 12/01/2025 Test Time: 12:52pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	12:53pm
FLO	Pass	12:53pm
FC	Pass	12:53pm

Temperature Tests

Test	Status	Time
FC1	Pass	12:53pm
SRC	Pass	12:53pm
DET	Pass	12:53pm
BAR	Pass	12:53pm
BT	Pass	12:53pm

Blank Tests

Test	Status	Time
AIR	Pass	12:54pm

Printer Tests

Test	Status	Time
PRNT	Pass	12:54pm

CRC Tests

Test	Status	Time
COMP	Pass	12:54pm
CAL	Pass	12:54pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County DAVIDSON Instrument Location Thomasville Police
Instrument Serial No. 008872 Department

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 15th day of December, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

509387
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

DAVIDSON COUNTY THOMASVILLE PD 280

Serial Number: 008872
Test Date: 12/01/2025

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: Long, Thomas A
Permit Number: 0050-9387
Effective:
09/01/2025-09/01/2027

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG503001
Exp Date: 01/30/2027

Test	g/210L	Time
DIAG	Pass	5:38pm
AIR BLK	.00	5:39pm
ACCY CHK	.08	5:40pm
AIR BLK	.00	5:41pm
SUB TEST	.00	5:42pm
AIR BLK	.00	5:43pm
SUB TEST	.00	5:44pm
AIR BLK	.00	5:45pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

DAVIDSON COUNTY THOMASVILLE PD 280

Serial Number: 008872 Test Record Number: 1969
Test Date: 12/01/2025 Test Time: 5:46pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	5:46pm
FLO	Pass	5:46pm
FC	Pass	5:46pm

Temperature Tests

Test	Status	Time
FC1	Pass	5:46pm
SRC	Pass	5:46pm
DET	Pass	5:46pm
BAR	Pass	5:46pm
BT	Pass	5:46pm

Blank Tests

Test	Status	Time
AIR	Pass	5:47pm


Printer Tests

Test	Status	Time
PRNT	Pass	5:47pm

CRC Tests

Test	Status	Time
COMP	Pass	5:47pm
CAL	Pass	5:47pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County DAVIDSON Instrument Location Lexington

Instrument Serial No. 008883 Police Department

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 1st day of December, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

509387
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

DAVIDSON COUNTY LEXINGTON PD 280

Serial Number: 008883

Test Date: 12/01/2025

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Long, Thomas A

Permit Number: 0050-9387

Effective:

09/01/2025-09/01/2027

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG501307

Exp Date: 01/13/2027


Test	g/210L	Time
DIAG	Pass	11:38am
AIR BLK	.00	11:39am
ACCY CHK	.08	11:40am
AIR BLK	.00	11:41am
SUB TEST	.00	11:43am
AIR BLK	.00	11:44am
SUB TEST	.00	11:45am
AIR BLK	.00	11:46am

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR

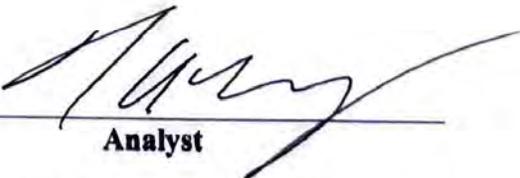

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

DAVIDSON COUNTY LEXINGTON PD 280

Serial Number: 008883 Test Record Number: 3104
Test Date: 12/01/2025 Test Time: 11:48am EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	11:48am
FLO	Pass	11:48am
FC	Pass	11:48am

Temperature Tests

Test	Status	Time
FC1	Pass	11:48am
SRC	Pass	11:48am
DET	Pass	11:48am
BAR	Pass	11:48am
BT	Pass	11:48am

Blank Tests

Test	Status	Time
AIR	Pass	11:49am


Printer Tests

Test	Status	Time
PRNT	Pass	11:49am

CRC Tests

Test	Status	Time
COMP	Pass	11:49am
CAL	Pass	11:49am

Preventive Maintenance
Status: Pass

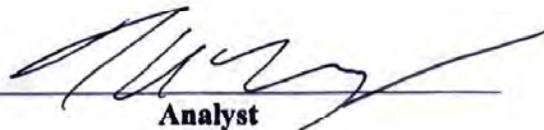

Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Davidson Instrument Location BAT Mobile Unit 8
Instrument Serial No. 008929

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 12 day of December, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

2219283
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

DAVIDSON COUNTY BAT MOBILE UNIT 8 280

Serial Number: 008929
Test Date: 12/12/2025

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Glasscock, Jerry D

Permit Number: 7180-9235

Effective:

02/01/2025-02/01/2027

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG506303


Exp Date: 03/04/2027

Test	g/210L	Time
DIAG	Pass	9:42pm
AIR BLK	.00	9:43pm
ACCY CHK	.08	9:44pm
AIR BLK	.00	9:45pm
SUB TEST	.00	9:46pm
AIR BLK	.00	9:47pm
SUB TEST	.00	9:49pm
AIR BLK	.00	9:50pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

Intox EC/IR-II: Preventive Maintenance

DAVIDSON COUNTY BAT MOBILE UNIT 8 280

Serial Number: 008929 Test Record Number: 1699
Test Date: 12/12/2025 Test Time: 9:51pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	9:51pm
FLO	Pass	9:51pm
FC	Pass	9:52pm

Temperature Tests

Test	Status	Time
FC1	Pass	9:52pm
SRC	Pass	9:52pm
DET	Pass	9:52pm
BAR	Pass	9:52pm
BT	Pass	9:52pm

Blank Tests

Test	Status	Time
AIR	Pass	9:52pm


Printer Tests

Test	Status	Time
PRNT	Pass	9:52pm

CRC Tests

Test	Status	Time
COMP	Pass	9:53pm
CAL	Pass	9:53pm

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County Davidson Instrument Location BAT Mobile Unit 8
Instrument Serial No. 008929 —

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 31 day of December, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

2219283
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

DAVIDSON COUNTY BAT MOBILE UNIT 8 280

Serial Number: 008929
Test Date: 12/31/2025

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Glasscock, Jerry D

Permit Number: 7180-9235

Effective:

02/01/2025-02/01/2027

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG506303

Exp Date: 03/04/2027

Test	g/210L	Time
DIAG	Pass	8:26pm
AIR BLK	.00	8:27pm
ACCY CHK	.08	8:28pm
AIR BLK	.00	8:29pm
SUB TEST	.00	8:30pm
AIR BLK	.00	8:31pm
SUB TEST	.00	8:32pm
AIR BLK	.00	8:33pm

Reported AC: .00 g/210L

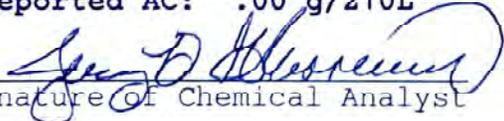
Signature of Chemical Analyst

Court CVR


Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

DAVIDSON COUNTY BAT MOBILE UNIT 8 280

Serial Number: 008929 Test Record Number: 1709
Test Date: 12/31/2025 Test Time: 8:35pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	8:36pm
FLO	Pass	8:36pm
FC	Pass	8:36pm

Temperature Tests

Test	Status	Time
FC1	Pass	8:36pm
SRC	Pass	8:36pm
DET	Pass	8:36pm
BAR	Pass	8:36pm
BT	Pass	8:36pm

Blank Tests

Test	Status	Time
AIR	Pass	8:37pm

Printer Tests

Test	Status	Time
PRNT	Pass	8:37pm

CRC Tests

Test	Status	Time
COMP	Pass	8:37pm
CAL	Pass	8:37pm

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County DUPLIN Instrument Location WALLACE

Instrument Serial No. 008858 POLICE DEPT

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 23 day of DECEMBER, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Alan R. Basso

Signature of Certifying Official

146279

Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

DUPLIN COUNTY WALLACE PD 300

Serial Number: 008858
Test Date: 12/23/2025

Citation Number: M0000000-0
Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: BARNES, ALVIN R

Permit Number: 0014-6279

Effective:

02/01/2025-02/01/2027

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG534301

Exp Date: 12/09/2027


Test	g/210L	Time
DIAG	Pass	9:45am
AIR BLK	.00	9:45am
ACCY CHK	.07	9:46am
AIR BLK	.00	9:47am
SUB TEST	.00	9:48am
AIR BLK	.00	9:49am
SUB TEST	.00	9:50am
AIR BLK	.00	9:51am

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

DUPLIN COUNTY WALLACE PD 300

Serial Number: 008858 Test Record Number: 1387
Test Date: 12/23/2025 Test Time: 9:53am EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	9:54am
FLO	Pass	9:54am
FC	Pass	9:54am

Temperature Tests

Test	Status	Time
FC1	Pass	9:54am
SRC	Pass	9:54am
DET	Pass	9:54am
BAR	Pass	9:54am
BT	Pass	9:54am

Blank Tests

Test	Status	Time
AIR	Pass	9:55am


Printer Tests

Test	Status	Time
PRNT	Pass	9:55am

CRC Tests

Test	Status	Time
COMP	Pass	9:55am
CAL	Pass	9:55am

Preventive Maintenance
Status: Pass



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County DUPLIN Instrument Location DUPLIN COUNTY
Instrument Serial No. 008864 DETENTION CENTER

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 22 day of DECEMBER, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Alan R. Bane

Signature of Certifying Official

146279

Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

DUPLIN COUNTY DETENTION CENTER 300

Serial Number: 008864
Test Date: 12/22/2025

Citation Number: M0000000-0
Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: BARNES, ALVIN R

Permit Number: 0014-6279

Effective:

02/01/2025-02/01/2027

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG534301

Exp Date: 12/09/2027


Test	g/210L	Time
DIAG	Pass	4:35pm
AIR BLK	.00	4:36pm
ACCY CHK	.07	4:37pm
AIR BLK	.00	4:38pm
SUB TEST	.00	4:39pm
AIR BLK	.00	4:40pm
SUB TEST	.00	4:41pm
AIR BLK	.00	4:42pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR


Analyst

Intox EC/IR-II: Preventive Maintenance

DUPLIN COUNTY DETENTION CENTER 300

Serial Number: 008864 Test Record Number: 5323
Test Date: 12/22/2025 Test Time: 4:43pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	4:43pm
FLO	Pass	4:43pm
FC	Pass	4:43pm

Temperature Tests

Test	Status	Time
FC1	Pass	4:43pm
SRC	Pass	4:43pm
DET	Pass	4:43pm
BAR	Pass	4:43pm
BT	Pass	4:43pm

Blank Tests

Test	Status	Time
AIR	Pass	4:44pm


Printer Tests

Test	Status	Time
PRNT	Pass	4:44pm

CRC Tests

Test	Status	Time
COMP	Pass	4:44pm
CAL	Pass	4:44pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County DURHAM Instrument Location DURHAM Co JAIL
Instrument Serial No. 008859 219 S. Mangum ST
Durham, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 19 day of December, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Simon Stokes Bowers
Signature of Certifying Official

146221
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

DURHAM COUNTY DURHAM COUNTY JAIL 310

Serial Number: 008859
Test Date: 12/19/2025

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Barnes, Simon S

Permit Number: 0014-6221

Effective:

02/01/2025-02/01/2027

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG534301

Exp Date: 12/09/2027

Test	g/210L	Time
DIAG	Pass	7:47am
AIR BLK	.00	7:48am
ACCY CHK	.08	7:49am
AIR BLK	.00	7:50am
SUB TEST	.00	7:50am
AIR BLK	.00	7:51am
SUB TEST	.00	7:53am
AIR BLK	.00	7:54am

Reported AC: .00 g/210L

Simon Stokes Barnes

Signature of Chemical Analyst

Court CVR

Simon Stokes Barnes

Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

DURHAM COUNTY DURHAM COUNTY JAIL 310

Serial Number: 008859 Test Record Number: 3420
Test Date: 12/19/2025 Test Time: 7:55am EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	7:55am
FLO	Pass	7:55am
FC	Pass	7:56am

Temperature Tests

Test	Status	Time
FC1	Pass	7:56am
SRC	Pass	7:56am
DET	Pass	7:56am
BAR	Pass	7:56am
BT	Pass	7:56am

Blank Tests

Test	Status	Time
AIR	Pass	7:56am

Printer Tests

Test	Status	Time
PRNT	Pass	7:56am

CRC Tests

Test	Status	Time
COMP	Pass	7:56am
CAL	Pass	7:56am

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Durham Instrument Location DURHAM CO JAIL
Instrument Serial No. 008878 219 S. Mangum ST
Durham, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 19 day of December, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Simon Stokes Barnes
Signature of Certifying Official

146221
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

DURHAM COUNTY DURHAM COUNTY JAIL 310

Serial Number: 008878
Test Date: 12/19/2025

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Barnes, Simon S

Permit Number: 0014-6221

Effective:

02/01/2025-02/01/2027

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG534301

Exp Date: 12/09/2027

Test	g/210L	Time
DIAG	Pass	7:43am
AIR BLK	.00	7:43am
ACCY CHK	.08	7:44am
AIR BLK	.00	7:45am
SUB TEST	.00	7:46am
AIR BLK	.00	7:47am
SUB TEST	.00	7:49am
AIR BLK	.00	7:50am

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

DURHAM COUNTY DURHAM COUNTY JAIL 310

Serial Number: 008878 Test Record Number: 7129
Test Date: 12/19/2025 Test Time: 7:51am EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	7:52am
FLO	Pass	7:52am
FC	Pass	7:52am

Temperature Tests

Test	Status	Time
FC1	Pass	7:52am
SRC	Pass	7:52am
DET	Pass	7:52am
BAR	Pass	7:52am
BT	Pass	7:52am

Blank Tests

Test	Status	Time
AIR	Pass	7:53am

Printer Tests

Test	Status	Time
PRNT	Pass	7:53am

CRC Tests

Test	Status	Time
COMP	Pass	7:53am
CAL	Pass	7:53am

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County Durham Instrument Location Durham Co Jail
Instrument Serial No. 008891 219 S. Mangum St
Durham, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 19 day of December, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Sam Stokes Barnes
Signature of Certifying Official

146221
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

DURHAM COUNTY DURHAM COUNTY JAIL 310

Serial Number: 008891
Test Date: 12/19/2025

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: Barnes, Simon S
Permit Number: 0014-6221
Effective:
02/01/2025-02/01/2027

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG534301
Exp Date: 12/09/2026

Test	g/210L	Time
DIAG	Pass	7:41am
AIR BLK	.00	7:42am
ACCY CHK	.07	7:42am
AIR BLK	.00	7:43am
SUB TEST	.00	7:44am
AIR BLK	.00	7:45am
SUB TEST	.00	7:46am
AIR BLK	.00	7:47am

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

DURHAM COUNTY DURHAM COUNTY JAIL 310

Serial Number: 008891 Test Record Number: 4896
Test Date: 12/19/2025 Test Time: 7:49am EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	7:49am
FLO	Pass	7:49am
FC	Pass	7:49am

Temperature Tests

Test	Status	Time
FC1	Pass	7:50am
SRC	Pass	7:50am
DET	Pass	7:50am
BAR	Pass	7:50am
BT	Pass	7:50am

Blank Tests

Test	Status	Time
AIR	Pass	7:50am

Printer Tests

Test	Status	Time
PRNT	Pass	7:50am

CRC Tests

Test	Status	Time
COMP	Pass	7:50am
CAL	Pass	7:50am

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Forsyth Instrument Location BAT Mobile Unit II

Instrument Serial No. 008973

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 16th day of December, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



John Davies
Signature of Certifying Official

1604930
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

FORSYTH COUNTY BAT MOBILE UNIT 11 330

Serial Number: 008973
Test Date: 12/16/2025

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Lanier Jr., John P

Permit Number: 4582-9118

Effective:

04/01/2025-04/01/2027

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG431003

Exp Date: 11/05/2026


Test	g/210L	Time
DIAG	Pass	1:39pm
AIR BLK	.00	1:40pm
ACCY CHK	.07	1:40pm
AIR BLK	.00	1:41pm
SUB TEST	.00	1:42pm
AIR BLK	.00	1:43pm
SUB TEST	.00	1:44pm
AIR BLK	.00	1:45pm

Reported AC: .00 g/210L

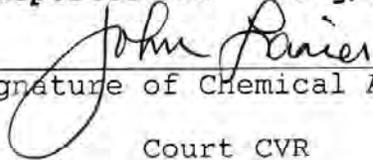

Signature of Chemical Analyst

Court CVR

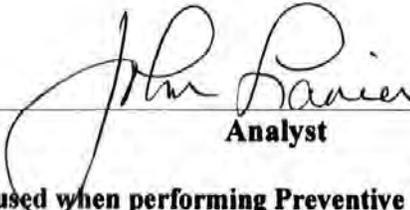

Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

FORSYTH COUNTY BAT MOBILE UNIT 11 330

Serial Number: 008973 Test Record Number: 1394
Test Date: 12/16/2025 Test Time: 1:46pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	1:46pm
FLO	Pass	1:46pm
FC	Pass	1:46pm

Temperature Tests

Test	Status	Time
FC1	Pass	1:46pm
SRC	Pass	1:46pm
DET	Pass	1:46pm
BAR	Pass	1:46pm
BT	Pass	1:46pm

Blank Tests

Test	Status	Time
AIR	Pass	1:47pm


Printer Tests

Test	Status	Time
PRNT	Pass	1:47pm

CRC Tests

Test	Status	Time
COMP	Pass	1:47pm
CAL	Pass	1:47pm

Preventive Maintenance
Status: Pass

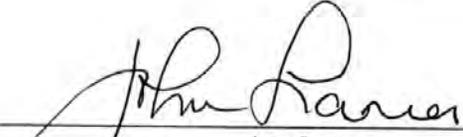

Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County FORSYTH Instrument Location FORSYTH CO. DETENTION

Instrument Serial No. 008583 WINSTON-SALEM

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 30th day of DECEMBER, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.




Signature of Certifying Official

353799
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

FORSYTH COUNTY FORSYTH CO DETENTION
330

Serial Number: 008583
Test Date: 12/30/2025

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Oligmueller, Leo A

Permit Number: 0035-3799

Effective:

02/01/2025-02/01/2027

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG534301


Exp Date: 12/09/2027

Test	g/210L	Time
DIAG	Pass	1:00pm
AIR BLK	.00	1:01pm
ACCY CHK	.08	1:01pm
AIR BLK	.00	1:02pm
SUB TEST	.00	1:03pm
AIR BLK	.00	1:04pm
SUB TEST	.00	1:06pm
AIR BLK	.00	1:07pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR

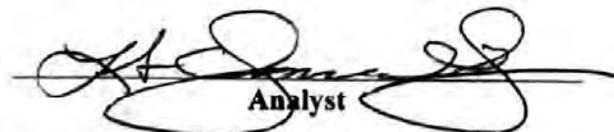
Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

FORSYTH COUNTY FORSYTH CO DETENTION 330

Serial Number: 008583 Test Record Number: 10066
Test Date: 12/30/2025 Test Time: 1:07pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	1:08pm
FLO	Pass	1:08pm
FC	Pass	1:08pm

Temperature Tests

Test	Status	Time
FC1	Pass	1:08pm
SRC	Pass	1:08pm
DET	Pass	1:08pm
BAR	Pass	1:08pm
BT	Pass	1:08pm

Blank Tests

Test	Status	Time
AIR	Pass	1:09pm


Printer Tests

Test	Status	Time
PRNT	Pass	1:09pm

CRC Tests

Test	Status	Time
COMP	Pass	1:09pm
CAL	Pass	1:09pm

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**


County FORSYTH Instrument Location KERNERSVILLE
Instrument Serial No. 008650 POLICE DEPARTMENT

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 30TH day of DECEMBER, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.

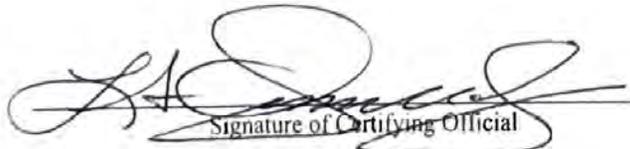


Signature of Certifying Official

353799
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

FORSYTH COUNTY KERNERSVILLE PD 330

Serial Number: 008650

Test Date: 12/30/2025

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Oligmueller, Leo A

Permit Number: 0035-3799

Effective:

02/01/2025-02/01/2027

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG534301

Exp Date: 12/09/2027

Test	g/210L	Time
DIAG	Pass	10:13am
AIR BLK	.00	10:14am
ACCY CHK	.07	10:15am
AIR BLK	.00	10:16am
SUB TEST	.00	10:16am
AIR BLK	.00	10:17am
SUB TEST	.00	10:19am
AIR BLK	.00	10:20am

Reported AC: .00 g/210L

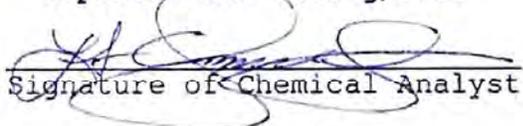
Signature of Chemical Analyst

Court CVR


Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

FORSYTH COUNTY KERNERSVILLE PD 330

Serial Number: 008650 Test Record Number: 2474
Test Date: 12/30/2025 Test Time: 10:20am EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	10:20am
FLO	Pass	10:20am
FC	Pass	10:21am

Temperature Tests

Test	Status	Time
FC1	Pass	10:21am
SRC	Pass	10:21am
DET	Pass	10:21am
BAR	Pass	10:21am
BT	Pass	10:21am

Blank Tests

Test	Status	Time
AIR	Pass	10:21am


Printer Tests

Test	Status	Time
PRNT	Pass	10:21am

CRC Tests

Test	Status	Time
COMP	Pass	10:21am
CAL	Pass	10:21am

Preventive Maintenance
Status: Pass

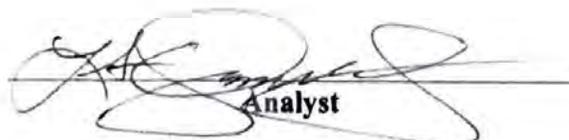
Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County FORSYTH Instrument Location FORSYTH CO. DETENTION

Instrument Serial No. 008660 WINSTON-SALEM

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 30th day of DECEMBER, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.




Signature of Certifying Official

353799
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

FORSYTH COUNTY FORSYTH CO DETENTION
330

Serial Number: 008660
Test Date: 12/30/2025

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Oligmueller, Leo A

Permit Number: 0035-3799

Effective:

02/01/2025-02/01/2027

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG534301

Exp Date: 12/09/2027

Test	g/210L	Time
DIAG	Pass	1:55pm
AIR BLK	.00	1:55pm
ACCY CHK	.07	1:56pm
AIR BLK	.00	1:57pm
SUB TEST	.00	1:58pm
AIR BLK	.00	1:59pm
SUB TEST	.00	2:02pm
AIR BLK	.00	2:03pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

FORSYTH COUNTY FORSYTH CO DETENTION 330

Serial Number: 008660 Test Record Number: 4713
Test Date: 12/30/2025 Test Time: 2:03pm EST

System Check: Passed

Baseline Tests

Test	Status	Time
IR	Pass	2:04pm
FLO	Pass	2:04pm
FC	Pass	2:04pm

Temperature Tests

Test	Status	Time
FC1	Pass	2:04pm
SRC	Pass	2:04pm
DET	Pass	2:04pm
BAR	Pass	2:04pm
BT	Pass	2:04pm

Blank Tests

Test	Status	Time
AIR	Pass	2:05pm

Printer Tests

Test	Status	Time
PRNT	Pass	2:05pm

CRC Tests

Test	Status	Time
COMP	Pass	2:05pm
CAL	Pass	2:05pm

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County FORSYTH Instrument Location FORSYTH CO. DETENTION
Instrument Serial No. 00 8925 WINSTON-SALEM.

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 30th day of DECEMBER, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.




Signature of Certifying Official

353799
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

FORSYTH COUNTY FORSYTH CO DETENTION

330

Serial Number: 008925

Test Date: 12/30/2025

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Oligmueller, Leo A

Permit Number: 0035-3799

Effective:

02/01/2025-02/01/2027

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG534301

Exp Date: 12/09/2027

Test	g/210L	Time
DIAG	Pass	1:07pm
AIR BLK	.00	1:08pm
ACCY CHK	.08	1:08pm
AIR BLK	.00	1:09pm
SUB TEST	.00	1:10pm
AIR BLK	.00	1:11pm
SUB TEST	.00	1:13pm
AIR BLK	.00	1:14pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

FORSYTH COUNTY FORSYTH CO DETENTION 330

Serial Number: 008925 Test Record Number: 5719
Test Date: 12/30/2025 Test Time: 1:15pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	1:16pm
FLO	Pass	1:16pm
FC	Pass	1:16pm

Temperature Tests

Test	Status	Time
FC1	Pass	1:16pm
SRC	Pass	1:16pm
DET	Pass	1:16pm
BAR	Pass	1:16pm
BT	Pass	1:16pm

Blank Tests

Test	Status	Time
AIR	Pass	1:16pm


Printer Tests

Test	Status	Time
PRNT	Pass	1:16pm

CRC Tests

Test	Status	Time
COMP	Pass	1:17pm
CAL	Pass	1:17pm

Preventive Maintenance
Status: Pass

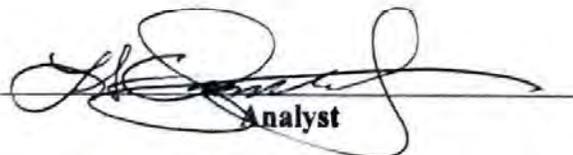
Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County Forsyth Instrument Location BAT Mobile Unit 11
Instrument Serial No. 008970

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 16th day of December, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



John Senior
Signature of Certifying Official

1604930
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

FORSYTH COUNTY BAT MOBILE UNIT 11 330

Serial Number: 008970
Test Date: 12/16/2025

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Lanier Jr., John P

Permit Number: 4582-9118

Effective:

04/01/2025-04/01/2027

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG417802

Exp Date: 06/26/2026


Test	g/210L	Time
DIAG	Pass	1:37pm
AIR BLK	.00	1:38pm
ACCY CHK	.07	1:39pm
AIR BLK	.00	1:40pm
SUB TEST	.00	1:41pm
AIR BLK	.00	1:41pm
SUB TEST	.00	1:43pm
AIR BLK	.00	1:44pm

Reported AC: .00 g/210L

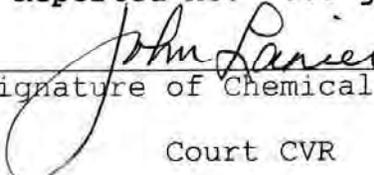

Signature of Chemical Analyst

Court CVR

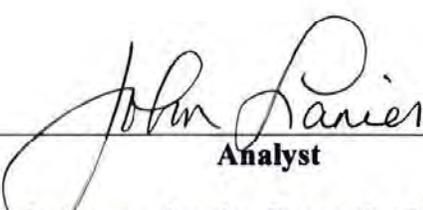

Analyst

Intox EC/IR-II: Preventive Maintenance

FORSYTH COUNTY BAT MOBILE UNIT 11 330

Serial Number: 008970 Test Record Number: 1346
Test Date: 12/16/2025 Test Time: 1:44pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	1:44pm
FLO	Pass	1:44pm
FC	Pass	1:44pm

Temperature Tests

Test	Status	Time
FC1	Pass	1:45pm
SRC	Pass	1:45pm
DET	Pass	1:45pm
BAR	Pass	1:45pm
BT	Pass	1:45pm

Blank Tests

Test	Status	Time
AIR	Pass	1:45pm


Printer Tests

Test	Status	Time
PRNT	Pass	1:45pm

CRC Tests

Test	Status	Time
COMP	Pass	1:45pm
CAL	Pass	1:45pm

Preventive Maintenance
Status: Pass

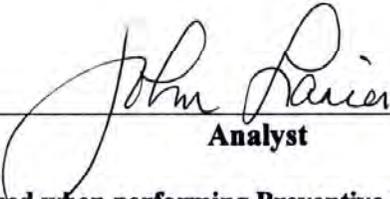

Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County FRANKLIN Instrument Location FRANKLIN Co. LEC
Instrument Serial No. 008933 285 T. KEMP Rd.
LOUISBURG, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 23 day of DECEMBER, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

179707
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

FRANKLIN COUNTY FRANKLIN CO. LEC 340

Serial Number: 008933
Test Date: 12/23/2025

Citation Number: M0000000-0
Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Bryant, Earl A

Permit Number: 0017-9707

Effective:

02/01/2025-02/01/2027

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG534301

Exp Date: 12/09/2027


Test	g/210L	Time
DIAG	Pass	10:29am
AIR BLK	.00	10:30am
ACCY CHK	.08	10:31am
AIR BLK	.00	10:32am
SUB TEST	.00	10:33am
AIR BLK	.00	10:34am
SUB TEST	.00	10:35am
AIR BLK	.00	10:36am

Reported AC: .00 g/210L

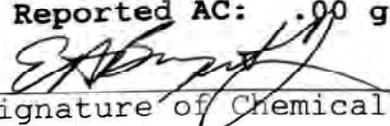

Signature of Chemical Analyst

Court CVR

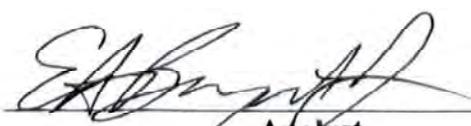

Analyst

Intox EC/IR-II: Preventive Maintenance

FRANKLIN COUNTY FRANKLIN CO. LEC 340

Serial Number: 008933 Test Record Number: 1943
Test Date: 12/23/2025 Test Time: 10:37am EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	10:38am
FLO	Pass	10:38am
FC	Pass	10:38am

Temperature Tests

Test	Status	Time
FC1	Pass	10:38am
SRC	Pass	10:38am
DET	Pass	10:38am
BAR	Pass	10:38am
BT	Pass	10:38am

Blank Tests

Test	Status	Time
AIR	Pass	10:38am

Printer Tests

Test	Status	Time
PRNT	Pass	10:38am

CRC Tests

Test	Status	Time
COMP	Pass	10:39am
CAL	Pass	10:39am

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Franklin Instrument Location Franklin Co. LEC
Instrument Serial No. 008942 285 T. Kemp Rd.
LOUISBURG, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 23 day of DECEMBER, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

179707
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

FRANKLIN COUNTY FRANKLIN CO. LEC 340

Serial Number: 008942
Test Date: 12/23/2025

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE

Analyst's Name: Bryant, Earl A
Permit Number: 0017-9707
Effective:
02/01/2025-02/01/2027

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG534301
Exp Date: 12/09/2027

Test	g/210L	Time
DIAG	Pass	10:30am
AIR BLK	.00	10:31am
ACCY CHK	.07	10:31am
AIR BLK	.00	10:33am
SUB TEST	.00	10:33am
AIR BLK	.00	10:34am
SUB TEST	.00	10:36am
AIR BLK	.00	10:36am

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

Intox EC/IR-II: Preventive Maintenance

FRANKLIN COUNTY FRANKLIN CO. LEC 340

Serial Number: 008942 Test Record Number: 3537
Test Date: 12/23/2025 Test Time: 10:38am EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	10:38am
FLO	Pass	10:38am
FC	Pass	10:38am

Temperature Tests

Test	Status	Time
FC1	Pass	10:38am
SRC	Pass	10:38am
DET	Pass	10:38am
BAR	Pass	10:38am
BT	Pass	10:38am

Blank Tests

Test	Status	Time
AIR	Pass	10:39am


Printer Tests

Test	Status	Time
PRNT	Pass	10:39am

CRC Tests

Test	Status	Time
COMP	Pass	10:39am
CAL	Pass	10:39am

Preventive Maintenance
Status: Pass

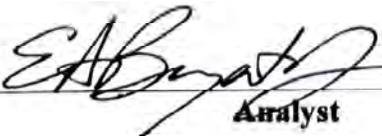
Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Gastonia Instrument Location Gaston County Jail
Instrument Serial No. 008684 Gastonia, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 29th day of December, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

849845
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

GASTON COUNTY GASTON COUNTY SO 350

Serial Number: 008684
Test Date: 12/29/2025

Citation Number: M0000000-0
Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Helms, Bryce A

Permit Number: 0084-9845

Effective:

02/01/2025-02/01/2027

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG516203

Exp Date: 06/11/2027


Test	g/210L	Time
DIAG	Pass	1:01pm
AIR BLK	.00	1:01pm
ACCY CHK	.07	1:02pm
AIR BLK	.00	1:03pm
SUB TEST	.00	1:05pm
AIR BLK	.00	1:05pm
SUB TEST	.00	1:07pm
AIR BLK	.00	1:08pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR

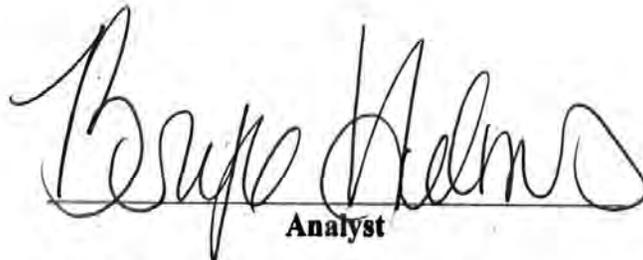

Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

GASTON COUNTY GASTON COUNTY SO 350

Serial Number: 008684 Test Record Number: 6896
Test Date: 12/29/2025 Test Time: 1:08pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	1:09pm
FLO	Pass	1:09pm
FC	Pass	1:09pm

Temperature Tests

Test	Status	Time
FC1	Pass	1:09pm
SRC	Pass	1:09pm
DET	Pass	1:09pm
BAR	Pass	1:09pm
BT	Pass	1:09pm

Blank Tests

Test	Status	Time
AIR	Pass	1:10pm


Printer Tests

Test	Status	Time
PRNT	Pass	1:10pm

CRC Tests

Test	Status	Time
COMP	Pass	1:10pm
CAL	Pass	1:10pm

Preventive Maintenance
Status: Pass

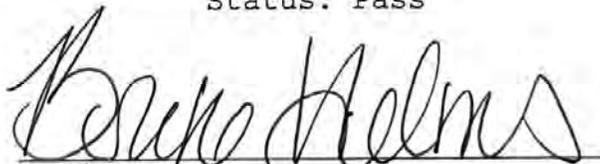
Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Gaston Instrument Location Gaston County Jail
Instrument Serial No. 008684 Gastonia, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 9th day of December, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Bryce Hulms
Signature of Certifying Official

8491845
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

GASTON COUNTY GASTON COUNTY SO 350

Serial Number: 008684
Test Date: 12/09/2025

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Helms, Bryce A

Permit Number: 0084-9845

Effective:

02/01/2025-02/01/2027

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG506303


Exp Date: 03/04/2027

Test	g/210L	Time
DIAG	Pass	11:36am
AIR BLK	.00	11:36am
ACCY CHK	.07	11:37am
AIR BLK	.00	11:38am
SUB TEST	.00	11:39am
AIR BLK	.00	11:40am
SUB TEST	.00	11:41am
AIR BLK	.00	11:42am

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR

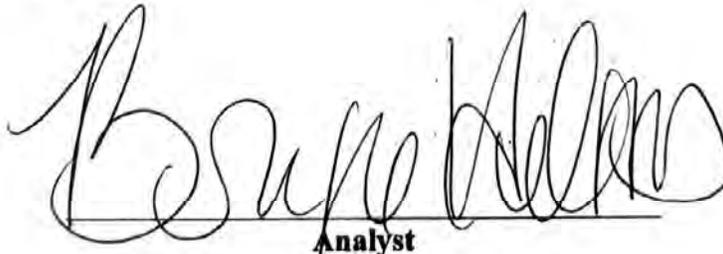
Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

GASTON COUNTY GASTON COUNTY SO 350

Serial Number: 008684 Test Record Number: 6844
Test Date: 12/09/2025 Test Time: 11:43am EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	11:43am
FLO	Pass	11:43am
FC	Pass	11:43am

Temperature Tests

Test	Status	Time
FC1	Pass	11:43am
SRC	Pass	11:43am
DET	Pass	11:43am
BAR	Pass	11:43am
BT	Pass	11:43am

Blank Tests

Test	Status	Time
AIR	Pass	11:44am

Printer Tests


Test	Status	Time
PRNT	Pass	11:44am

CRC Tests

Test	Status	Time
COMP	Pass	11:44am
CAL	Pass	11:44am

Preventive Maintenance

Status: *Pass*

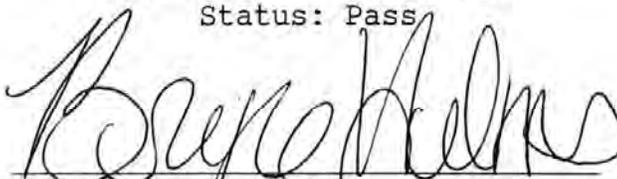

Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Gaston Instrument Location Gaston County Jail
Instrument Serial No. 008702 Gastonia, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 29th day of December, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Boyo Helms
Signature of Certifying Official

849845
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

GASTON COUNTY GASTON COUNTY SO 350

Serial Number: 008702
Test Date: 12/29/2025

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: Helms, Bryce A
Permit Number: 0084-9845
Effective:
02/01/2025-02/01/2027

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG506302
Exp Date: 03/04/2027


Test	g/210L	Time
DIAG	Pass	1:15pm
AIR BLK	.00	1:15pm
ACCY CHK	.08	1:16pm
AIR BLK	.00	1:17pm
SUB TEST	.00	1:17pm
AIR BLK	.00	1:18pm
SUB TEST	.00	1:20pm
AIR BLK	.00	1:21pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR

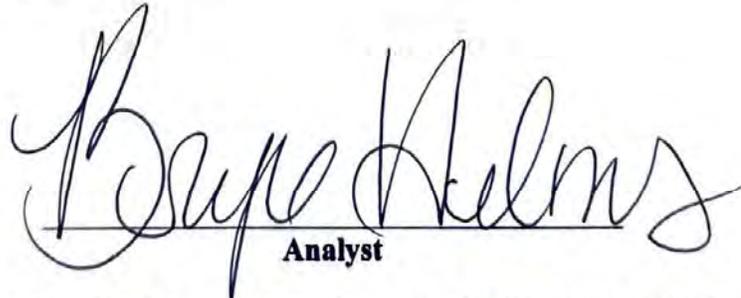

Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

GASTON COUNTY GASTON COUNTY SO 350

Serial Number: 008702 Test Record Number: 2368
Test Date: 12/29/2025 Test Time: 1:21pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	1:21pm
FLO	Pass	1:21pm
FC	Pass	1:22pm

Temperature Tests

Test	Status	Time
FC1	Pass	1:22pm
SRC	Pass	1:22pm
DET	Pass	1:22pm
BAR	Pass	1:22pm
BT	Pass	1:22pm

Blank Tests

Test	Status	Time
AIR	Pass	1:22pm


Printer Tests

Test	Status	Time
PRNT	Pass	1:22pm

CRC Tests

Test	Status	Time
COMP	Pass	1:23pm
CAL	Pass	1:23pm

Preventive Maintenance
Status: Pass

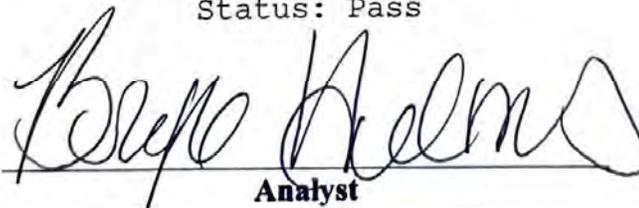
Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Graham Instrument Location Graham Co. S.O.
Instrument Serial No. 008915 Robbinsville, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 10 day of December, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

843310
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

GRAHAM COUNTY GRAHAM COUNTY SD 370

Serial Number: 008915
Test Date: 12/10/2025

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: Cutler, Daniel R
Permit Number: 0084-3310
Effective:
02/01/2025-02/01/2027

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG431002
Exp Date: 11/05/2026

Test	g/210L	Time
DIAG	Pass	11:11am
AIR BLK	.00	11:12am
ACCY CHK	.08	11:13am
AIR BLK	.00	11:14am
SUB TEST	.00	11:14am
AIR BLK	.00	11:15am
SUB TEST	.00	11:17am
AIR BLK	.00	11:18am

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

Intox EC/IR-II: Preventive Maintenance

GRAHAM COUNTY GRAHAM COUNTY SD 370

Serial Number: 008915 Test Record Number: 1016
Test Date: 12/10/2025 Test Time: 11:19am EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	11:19am
FLO	Pass	11:19am
FC	Pass	11:19am

Temperature Tests

Test	Status	Time
FC1	Pass	11:19am
SRC	Pass	11:19am
DET	Pass	11:19am
BAR	Pass	11:19am
BT	Pass	11:19am

Blank Tests

Test	Status	Time
AIR	Pass	11:20am

Printer Tests

Test	Status	Time
PRNT	Pass	11:20am

CRC Tests

Test	Status	Time
COMP	Pass	11:20am
CAL	Pass	11:20am

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County GRANVILLE Instrument Location GRANVILLE CO. LEC
Instrument Serial No. 008635 525 NEW COMMERCE DRIVE
OXFORD, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 29 day of DECEMBER, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

179707
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

GRANVILLE COUNTY GRANVILLE COUNTY LEC
380

Serial Number: 008635
Test Date: 12/29/2025

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Bryant, Earl A

Permit Number: 0017-9707

Effective:

02/01/2025-02/01/2027

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG534301

Exp Date: 12/09/2027


Test	g/210L	Time
DIAG	Pass	1:00pm
AIR BLK	.00	1:01pm
ACCY CHK	.08	1:02pm
AIR BLK	.00	1:03pm
SUB TEST	.00	1:04pm
AIR BLK	.00	1:04pm
SUB TEST	.00	1:06pm
AIR BLK	.00	1:07pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

GRANVILLE COUNTY GRANVILLE COUNTY LEC 380

Serial Number: 008635 Test Record Number: 2261
Test Date: 12/29/2025 Test Time: 1:09pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	1:10pm
FLO	Pass	1:10pm
FC	Pass	1:10pm

Temperature Tests

Test	Status	Time
FC1	Pass	1:10pm
SRC	Pass	1:10pm
DET	Pass	1:10pm
BAR	Pass	1:10pm
BT	Pass	1:10pm

Blank Tests

Test	Status	Time
AIR	Pass	1:11pm

Printer Tests

Test	Status	Time
PRNT	Pass	1:11pm

CRC Tests

Test	Status	Time
COMP	Pass	1:11pm
CAL	Pass	1:11pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County GRANVILLE Instrument Location GRANVILLE Co. LEC
Instrument Serial No. 008923 525 NEW COMMERCE DRIVE
OXFORD, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 29 day of DECEMBER, 20 25 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



EAB
Signature of Certifying Official

179707
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

GRANVILLE COUNTY GRANVILLE COUNTY LEC
380

Serial Number: 008923
Test Date: 12/29/2025

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: Bryant, Earl A
Permit Number: 0017-9707
Effective:
02/01/2025-02/01/2027

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG534301
Exp Date: 12/09/2027


Test	g/210L	Time
DIAG	Pass	1:08pm
AIR BLK	.00	1:09pm
ACCY CHK	.08	1:10pm
AIR BLK	.00	1:11pm
SUB TEST	.00	1:12pm
AIR BLK	.00	1:12pm
SUB TEST	.00	1:14pm
AIR BLK	.00	1:15pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

Intox EC/IR-II: Preventive Maintenance

GRANVILLE COUNTY GRANVILLE COUNTY LEC 380

Serial Number: 008923 Test Record Number: 3584
Test Date: 12/29/2025 Test Time: 1:16pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	1:16pm
FLO	Pass	1:16pm
FC	Pass	1:16pm

Temperature Tests

Test	Status	Time
FC1	Pass	1:16pm
SRC	Pass	1:16pm
DET	Pass	1:16pm
BAR	Pass	1:16pm
BT	Pass	1:16pm

Blank Tests

Test	Status	Time
AIR	Pass	1:17pm

Printer Tests

Test	Status	Time
PRNT	Pass	1:17pm

CRC Tests

Test	Status	Time
COMP	Pass	1:17pm
CAL	Pass	1:17pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Greene Instrument Location Greene Co. S.O.
Instrument Serial No. 008670 301 N. Greene St., Snow Hill, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 19th day of December, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

377722
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

GREENE COUNTY GREENE CO SO 390

Serial Number: 008670
Test Date: 12/19/2025

Citation Number: M0000000-0
Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Gray, Kelly D

Permit Number: 0037-7722

Effective:

02/01/2025-02/01/2027

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG431003

Exp Date: 11/05/2026


Test	g/210L	Time
DIAG	Pass	12:40pm
AIR BLK	.00	12:40pm
ACCY CHK	.08	12:41pm
AIR BLK	.00	12:42pm
SUB TEST	.00	12:42pm
AIR BLK	.00	12:43pm
SUB TEST	.00	12:45pm
AIR BLK	.00	12:46pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

GREENE COUNTY GREENE CO SO 390

Serial Number: 008670 Test Record Number: 2650
Test Date: 12/19/2025 Test Time: 12:46pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	12:47pm
FLO	Pass	12:47pm
FC	Pass	12:47pm

Temperature Tests

Test	Status	Time
FC1	Pass	12:47pm
SRC	Pass	12:47pm
DET	Pass	12:47pm
BAR	Pass	12:47pm
BT	Pass	12:47pm

Blank Tests

Test	Status	Time
AIR	Pass	12:47pm


Printer Tests

Test	Status	Time
PRNT	Pass	12:48pm

CRC Tests

Test	Status	Time
COMP	Pass	12:48pm
CAL	Pass	12:48pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Guilford Instrument Location BAT Mobile Unit 11

Instrument Serial No. 008973

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 18th day of December, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



John Lanier
Signature of Certifying Official

1604930
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

GUILFORD COUNTY BAT MOBILE UNIT 11 400

Serial Number: 008973
Test Date: 12/18/2025

Citation Number: M0000000-0
Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Lanier Jr., John P

Permit Number: 4582-9118

Effective:

04/01/2025-04/01/2027

Officer's Name: NONE, NONE

Type of Agency: FTA


Agency: DHHS

Test Type: Breath Test

Lot Number: AG431003
Exp Date: 11/05/2026


Test	g/210L	Time
DIAG	Pass	10:15pm
AIR BLK	.00	10:16pm
ACCY CHK	.07	10:17pm
AIR BLK	.00	10:18pm
SUB TEST	.00	10:19pm
AIR BLK	.00	10:20pm
SUB TEST	.00	10:21pm
AIR BLK	.00	10:22pm

Reported AC: .00 g/210L

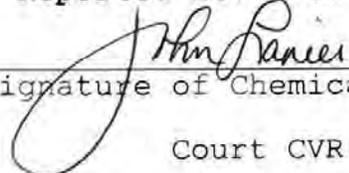

Signature of Chemical Analyst

Court CVR

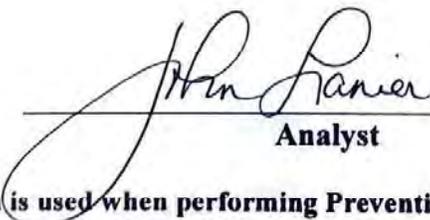

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

GUILFORD COUNTY BAT MOBILE UNIT 11 400

Serial Number: 008973 Test Record Number: 1399
Test Date: 12/18/2025 Test Time: 10:25pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	10:25pm
FLO	Pass	10:25pm
FC	Pass	10:25pm

Temperature Tests

Test	Status	Time
FC1	Pass	10:25pm
SRC	Pass	10:25pm
DET	Pass	10:25pm
BAR	Pass	10:25pm
BT	Pass	10:25pm

Blank Tests

Test	Status	Time
AIR	Pass	10:26pm


Printer Tests

Test	Status	Time
PRNT	Pass	10:26pm

CRC Tests

Test	Status	Time
COMP	Pass	10:26pm
CAL	Pass	10:26pm

Preventive Maintenance
Status: Pass

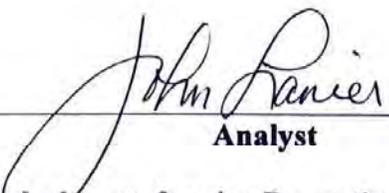

Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Guilford Instrument Location UNC-G Police

Instrument Serial No. 008604 Department

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 29th day of December, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

509387
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

GUILFORD COUNTY UNC-G POLICE DEPT 400

Serial Number: 008604
Test Date: 12/29/2025

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: Long, Thomas A
Permit Number: 0050-9387
Effective:
09/01/2025-09/01/2027

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG534301
Exp Date: 12/09/2027

Test	g/210L	Time
DIAG	Pass	12:57pm
AIR BLK	.00	12:57pm
ACCY CHK	.08	12:58pm
AIR BLK	.00	12:59pm
SUB TEST	.00	1:00pm
AIR BLK	.00	1:02pm
SUB TEST	.00	1:03pm
AIR BLK	.00	1:04pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

GUILFORD COUNTY UNC-G POLICE DEPT 400

Serial Number: 008604 Test Record Number: 2387
Test Date: 12/29/2025 Test Time: 1:05pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	1:05pm
FLO	Pass	1:05pm
FC	Pass	1:05pm

Temperature Tests

Test	Status	Time
FC1	Pass	1:05pm
SRC	Pass	1:05pm
DET	Pass	1:05pm
BAR	Pass	1:05pm
BT	Pass	1:05pm

Blank Tests

Test	Status	Time
AIR	Pass	1:06pm


Printer Tests

Test	Status	Time
PRNT	Pass	1:06pm

CRC Tests

Test	Status	Time
COMP	Pass	1:06pm
CAL	Pass	1:06pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Guilford Instrument Location High Point Jail

Instrument Serial No. 008655

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 29th day of December, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

509387
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

GUILFORD COUNTY HIGH POINT JAIL 400

Serial Number: 008655
Test Date: 12/29/2025

Citation Number: M0000000-0
Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Long, Thomas A

Permit Number: 0050-9387

Effective:

09/01/2025-09/01/2027

Officer's Name: NONE, NONE

Type of Agency: FTA


Agency: DHHS

Test Type: Breath Test

Lot Number: AG534301
Exp Date: 12/09/2027


Test	g/210L	Time
DIAG	Pass	11:31am
AIR BLK	.00	11:31am
ACCY CHK	.08	11:32am
AIR BLK	.00	11:33am
SUB TEST	.00	11:34am
AIR BLK	.00	11:35am
SUB TEST	.00	11:37am
AIR BLK	.00	11:37am

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR

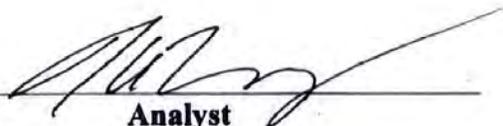

Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

GUILFORD COUNTY HIGH POINT JAIL 400

Serial Number: 008655 Test Record Number: 4122
Test Date: 12/29/2025 Test Time: 11:39am EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	11:39am
FLO	Pass	11:39am
FC	Pass	11:39am

Temperature Tests

Test	Status	Time
FC1	Pass	11:39am
SRC	Pass	11:39am
DET	Pass	11:39am
BAR	Pass	11:39am
BT	Pass	11:39am

Blank Tests

Test	Status	Time
AIR	Pass	11:40am


Printer Tests

Test	Status	Time
PRNT	Pass	11:40am

CRC Tests

Test	Status	Time
COMP	Pass	11:40am
CAL	Pass	11:40am

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Guilford Instrument Location High Point
Instrument Serial No. 008828 Police Department

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 29th day of December, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

509387
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

GUILFORD COUNTY HIGH POINT PD 401

Serial Number: 008828
Test Date: 12/29/2025

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Long, Thomas A

Permit Number: 0050-9387

Effective:

09/01/2025-09/01/2027

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG534301

Exp Date: 12/09/2027

Test	g/210L	Time
DIAG	Pass	10:31am
AIR BLK	.00	10:31am
ACCY CHK	.08	10:32am
AIR BLK	.00	10:33am
SUB TEST	.00	10:34am
AIR BLK	.00	10:35am
SUB TEST	.00	10:37am
AIR BLK	.00	10:37am

Reported AC: .00 g/210L

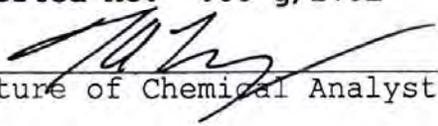

Signature of Chemical Analyst

Court CVR



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

GUILFORD COUNTY HIGH POINT PD 401

Serial Number: 008828 Test Record Number: 4806
Test Date: 12/29/2025 Test Time: 10:40am EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	10:40am
FLO	Pass	10:40am
FC	Pass	10:40am

Temperature Tests

Test	Status	Time
FC1	Pass	10:40am
SRC	Pass	10:40am
DET	Pass	10:40am
BAR	Pass	10:40am
BT	Pass	10:40am

Blank Tests

Test	Status	Time
AIR	Pass	10:41am

Printer Tests

Test	Status	Time
PRNT	Pass	10:41am

CRC Tests

Test	Status	Time
COMP	Pass	10:41am
CAL	Pass	10:41am

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Guilford Instrument Location BAT Mobile Unit 11

Instrument Serial No. 008970

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 18th day of December, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



John Lanier
Signature of Certifying Official

1604930
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

GUILFORD COUNTY BAT MOBILE UNIT 11 400

Serial Number: 008970
Test Date: 12/18/2025

Citation Number: M0000000-0
Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Lanier Jr., John P

Permit Number: 4582-9118

Effective:

04/01/2025-04/01/2027

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG417802

Exp Date: 06/26/2026


Test	g/210L	Time
DIAG	Pass	10:06pm
AIR BLK	.00	10:07pm
ACCY CHK	.07	10:08pm
AIR BLK	.00	10:09pm
SUB TEST	.00	10:09pm
AIR BLK	.00	10:10pm
SUB TEST	.00	10:12pm
AIR BLK	.00	10:13pm

Reported AC: .00 g/210L

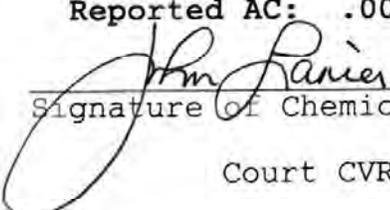

Signature of Chemical Analyst

Court CVR

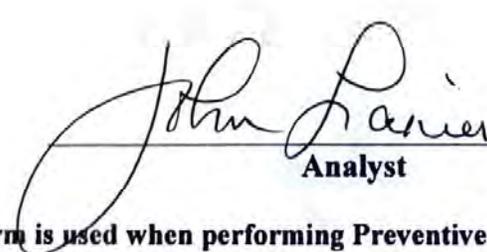

Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

GUILFORD COUNTY BAT MOBILE UNIT 11 400

Serial Number: 008970 Test Record Number: 1351
Test Date: 12/18/2025 Test Time: 10:13pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	10:14pm
FLO	Pass	10:14pm
FC	Pass	10:14pm

Temperature Tests

Test	Status	Time
FC1	Pass	10:14pm
SRC	Pass	10:14pm
DET	Pass	10:14pm
BAR	Pass	10:14pm
BT	Pass	10:14pm

Blank Tests

Test	Status	Time
AIR	Pass	10:14pm


Printer Tests

Test	Status	Time
PRNT	Pass	10:14pm

CRC Tests

Test	Status	Time
COMP	Pass	10:15pm
CAL	Pass	10:15pm

Preventive Maintenance
Status: Pass

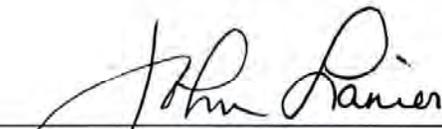

Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Halifax Instrument Location Roanoke Rapids PD
Instrument Serial No. 008656 1040 Roanoke AVENUE
Roanoke RAPIDS, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 19 day of DECEMBER, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



E. A. [Signature]
Signature of Certifying Official

179707
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

HALIFAX CO. ROANOKE RAPIDS PD 410

Serial Number: 008656

Test Date: 12/19/2025

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Bryant, Earl A

Permit Number: 0017-9707

Effective:

02/01/2025-02/01/2027

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG534301

Exp Date: 12/09/2027

Test	g/210L	Time
DIAG	Pass	7:54am
AIR BLK	.00	7:55am
ACCY CHK	.07	7:56am
AIR BLK	.00	7:57am
SUB TEST	.00	7:58am
AIR BLK	.00	7:59am
SUB TEST	.00	8:00am
AIR BLK	.00	8:01am

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

HALIFAX CO. ROANOKE RAPIDS PD 410

Serial Number: 008656 Test Record Number: 1182
Test Date: 12/19/2025 Test Time: 8:02am EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	8:03am
FLO	Pass	8:03am
FC	Pass	8:03am

Temperature Tests

Test	Status	Time
FC1	Pass	8:03am
SRC	Pass	8:03am
DET	Pass	8:03am
BAR	Pass	8:03am
BT	Pass	8:03am

Blank Tests

Test	Status	Time
AIR	Pass	8:04am

Printer Tests

Test	Status	Time
PRNT	Pass	8:04am

CRC Tests

Test	Status	Time
COMP	Pass	8:04am
CAL	Pass	8:04am

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County HALIFAX Instrument Location HALIFAX CO. S.O.
Instrument Serial No. Q08695 355 FERRELL LANE
HALIFAX, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 19 day of DECEMBER, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

179707
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

HALIFAX CO. HALIFAX CO SO 410

Serial Number: 008695
Test Date: 12/19/2025

Citation Number: M0000000-0
Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Bryant, Earl A

Permit Number: 0017-9707

Effective:

02/01/2025-02/01/2027

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG534301

Exp Date: 12/09/2027

Test	g/210L	Time
DIAG	Pass	9:33am
AIR BLK	.00	9:34am
ACCY CHK	.07	9:34am
AIR BLK	.00	9:36am
SUB TEST	.00	9:36am
AIR BLK	.00	9:37am
SUB TEST	.00	9:39am
AIR BLK	.00	9:39am

Reported AC: .00 g/210L

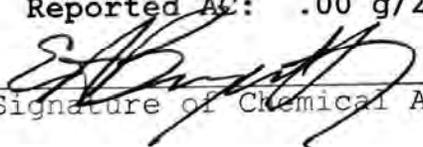
Signature of Chemical Analyst

Court CVR


Analyst

Intox EC/IR-II: Preventive Maintenance

HALIFAX CO. HALIFAX CO SO 410

Serial Number: 008695 Test Record Number: 4039
Test Date: 12/19/2025 Test Time: 9:40am EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	9:41am
FLO	Pass	9:41am
FC	Pass	9:41am

Temperature Tests

Test	Status	Time
FC1	Pass	9:41am
SRC	Pass	9:41am
DET	Pass	9:41am
BAR	Pass	9:41am
BT	Pass	9:41am

Blank Tests

Test	Status	Time
AIR	Pass	9:41am


Printer Tests

Test	Status	Time
PRNT	Pass	9:41am

CRC Tests

Test	Status	Time
COMP	Pass	9:42am
CAL	Pass	9:42am

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Harnett Instrument Location Dunn Police
Instrument Serial No. 008644 Department

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 22 day of December, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

365156
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

HARNETT COUNTY DUNN PD 420

Serial Number: 008644

Test Date: 12/22/2025

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Garner, Joel K

Permit Number: 0036-5156

Effective:

02/01/2025-02/01/2027

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG516204

Exp Date: 06/11/2027

Test	g/210L	Time
DIAG	Pass	11:26am
AIR BLK	.00	11:26am
ACCY CHK	.08	11:27am
AIR BLK	.00	11:28am
SUB TEST	.00	11:29am
AIR BLK	.00	11:30am
SUB TEST	.00	11:31am
AIR BLK	.00	11:32am

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

Intox EC/IR-II: Preventive Maintenance

HARNETT COUNTY DUNN PD 420

Serial Number: 008644 Test Record Number: 1974
Test Date: 12/22/2025 Test Time: 11:33am EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	11:33am
FLO	Pass	11:33am
FC	Pass	11:33am

Temperature Tests

Test	Status	Time
FC1	Pass	11:33am
SRC	Pass	11:33am
DET	Pass	11:33am
BAR	Pass	11:33am
BT	Pass	11:33am

Blank Tests

Test	Status	Time
AIR	Pass	11:34am

Printer Tests

Test	Status	Time
PRNT	Pass	11:34am

CRC Tests

Test	Status	Time
COMP	Pass	11:34am
CAL	Pass	11:34am

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County Harnett Instrument Location Harnett County
Instrument Serial No. 008729 Detention Center

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 22 day of December, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

365156
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

HARNETT COUNTY DETENTION CENTER 420

Serial Number: 008729

Test Date: 12/22/2025

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Garner, Joel K

Permit Number: 0036-5156

Effective:

02/01/2025-02/01/2027

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG534301

Exp Date: 12/09/2027

Test	g/210L	Time
DIAG	Pass	8:08am
AIR BLK	.00	8:09am
ACCY CHK	.08	8:09am
AIR BLK	.00	8:11am
SUB TEST	.00	8:11am
AIR BLK	.00	8:12am
SUB TEST	.00	8:14am
AIR BLK	.00	8:15am

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

Intox EC/IR-II: Preventive Maintenance

HARNETT COUNTY DETENTION CENTER 420

Serial Number: 008729 Test Record Number: 3592
Test Date: 12/22/2025 Test Time: 8:19am EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	8:19am
FLO	Pass	8:19am
FC	Pass	8:19am

Temperature Tests

Test	Status	Time
FC1	Pass	8:20am
SRC	Pass	8:20am
DET	Pass	8:20am
BAR	Pass	8:20am
BT	Pass	8:20am

Blank Tests

Test	Status	Time
AIR	Pass	8:20am

Printer Tests

Test	Status	Time
PRNT	Pass	8:20am

CRC Tests

Test	Status	Time
COMP	Pass	8:20am
CAL	Pass	8:20am

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County Harnett Instrument Location Harnett County
Instrument Serial No. 008730 Detention Center

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 22 day of December, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

365156
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

HARNETT COUNTY DETENTION CENTER 420

Serial Number: 008730
Test Date: 12/22/2025

Citation Number: M0000000-0
Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911
Subject's Sex: Male

Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: Garner, Joel K
Permit Number: 0036-5156
Effective:
02/01/2025-02/01/2027

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG534301
Exp Date: 12/09/2027


Test	g/210L	Time
DIAG	Pass	8:18am
AIR BLK	.00	8:18am
ACCY CHK	.08	8:19am
AIR BLK	.00	8:21am
SUB TEST	.00	8:21am
AIR BLK	.00	8:22am
SUB TEST	.00	8:24am
AIR BLK	.00	8:25am

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

HARNETT COUNTY DETENTION CENTER 420

Serial Number: 008730 Test Record Number: 4897
Test Date: 12/22/2025 Test Time: 8:25am EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	8:26am
FLO	Pass	8:26am
FC	Pass	8:26am

Temperature Tests

Test	Status	Time
FC1	Pass	8:26am
SRC	Pass	8:26am
DET	Pass	8:26am
BAR	Pass	8:26am
BT	Pass	8:26am

Blank Tests

Test	Status	Time
AIR	Pass	8:26am

Printer Tests

Test	Status	Time
PRNT	Pass	8:26am

CRC Tests

Test	Status	Time
COMP	Pass	8:27am
CAL	Pass	8:27am

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Hyde Instrument Location Hyde Co S.O. - Ocracoke
Instrument Serial No. 008797 NC12, Ocracoke, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 17th day of December, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Mark A. [Signature]
Signature of Certifying Official

206272
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

HYDE COUNTY HYDE CO SO OCRACOKE 470

Serial Number: 008797
Test Date: 12/17/2025

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Chappell, Mark A

Permit Number: 0020-6272

Effective:

02/01/2025-02/01/2027

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG516203


Exp Date: 06/11/2027

Test	g/210L	Time
DIAG	Pass	10:18am
AIR BLK	.00	10:19am
ACCY CHK	.07	10:19am
AIR BLK	.00	10:21am
SUB TEST	.00	10:21am
AIR BLK	.00	10:22am
SUB TEST	.00	10:24am
AIR BLK	.00	10:25am

Reported AC: .00 g/210L

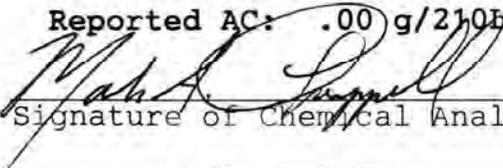
Signature of Chemical Analyst

Court CVR

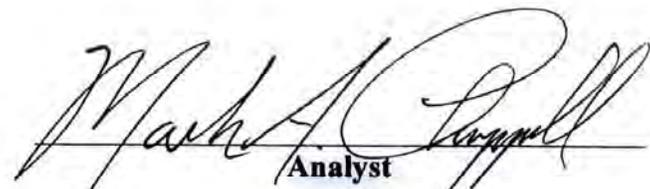
Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

HYDE COUNTY HYDE CO SO OCRACOKE 470

Serial Number: 008797 Test Record Number: 763
Test Date: 12/17/2025 Test Time: 10:26am EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	10:27am
FLO	Pass	10:27am
FC	Pass	10:27am

Temperature Tests

Test	Status	Time
FC1	Pass	10:27am
SRC	Pass	10:27am
DET	Pass	10:27am
BAR	Pass	10:27am
BT	Pass	10:27am

Blank Tests

Test	Status	Time
AIR	Pass	10:28am

Printer Tests

Test	Status	Time
PRNT	Pass	10:28am

CRC Tests

Test	Status	Time
COMP	Pass	10:28am
CAL	Pass	10:28am

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Iredell Instrument Location BAT Mobile Unit 8
Instrument Serial No. 008615

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 20 day of December, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

2219283
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

IREDELL COUNTY BAT MOBILE UNIT 8 480

Serial Number: 008615
Test Date: 12/20/2025

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Glasscock, Jerry D

Permit Number: 7180-9235

Effective:

02/01/2025-02/01/2027

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG405102


Exp Date: 02/20/2026

Test	g/210L	Time
DIAG	Pass	9:38pm
AIR BLK	.00	9:39pm
ACCY CHK	.07	9:40pm
AIR BLK	.00	9:41pm
SUB TEST	.00	9:42pm
AIR BLK	.00	9:43pm
SUB TEST	.00	9:44pm
AIR BLK	.00	9:45pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR

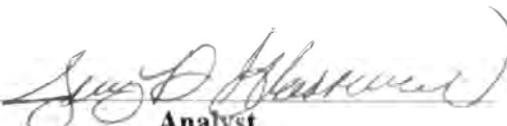
Analyst

Intox EC/IR-II: Preventive Maintenance

IREDELL COUNTY BAT MOBILE UNIT 8 480

Serial Number: 008615 Test Record Number: 6211
Test Date: 12/20/2025 Test Time: 9:45pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	9:46pm
FLO	Pass	9:46pm
FC	Pass	9:46pm

Temperature Tests

Test	Status	Time
FC1	Pass	9:46pm
SRC	Pass	9:46pm
DET	Pass	9:46pm
BAR	Pass	9:46pm
BT	Pass	9:46pm

Blank Tests

Test	Status	Time
AIR	Pass	9:47pm

Printer Tests

Test	Status	Time
PRNT	Pass	9:47pm

CRC Tests

Test	Status	Time
COMP	Pass	9:47pm
CAL	Pass	9:47pm

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County IREDELL Instrument Location STATESVILLE PD
Instrument Serial No. 008619 STATESVILLE NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 17 day of DECEMBER, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

274970
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

IREDELL COUNTY STATESVILLE PD 480

Serial Number: 008619

Test Date: 12/17/2025

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Fleming, Tina S

Permit Number: 0027-4970

Effective:

02/01/2025-02/01/2027

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG506302

Exp Date: 03/04/2027


Test	g/210L	Time
DIAG	Pass	10:07am
AIR BLK	.00	10:08am
ACCY CHK	.07	10:09am
AIR BLK	.00	10:10am
SUB TEST	.00	10:10am
AIR BLK	.00	10:11am
SUB TEST	.00	10:13am
AIR BLK	.00	10:14am

Reported AC: .00 g/210L

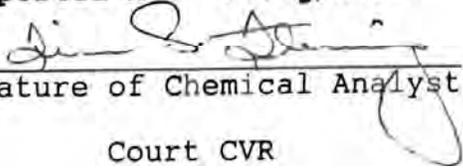

Signature of Chemical Analyst

Court CVR

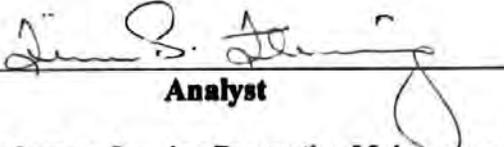

Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

IREDELL COUNTY STATESVILLE PD 480

Serial Number: 008619 Test Record Number: 2362
Test Date: 12/17/2025 Test Time: 10:14am EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	10:15am
FLO	Pass	10:15am
FC	Pass	10:15am

Temperature Tests

Test	Status	Time
FC1	Pass	10:15am
SRC	Pass	10:15am
DET	Pass	10:15am
BAR	Pass	10:15am
BT	Pass	10:15am

Blank Tests

Test	Status	Time
AIR	Pass	10:16am


Printer Tests

Test	Status	Time
PRNT	Pass	10:16am

CRC Tests

Test	Status	Time
COMP	Pass	10:16am
CAL	Pass	10:16am

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Iredell Instrument Location BAT Mobile Unit 8
Instrument Serial No. 008736

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 20 day of December, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

2219283
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

IREDELL COUNTY BAT MOBILE UNIT 8 480

Serial Number: 008736
Test Date: 12/20/2025

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE

Analyst's Name: Glasscock, Jerry D
Permit Number: 7180-9235
Effective:
02/01/2025-02/01/2027

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG405102
Exp Date: 02/20/2026

Test	g/210L	Time
DIAG	Pass	9:33pm
AIR BLK	.00	9:34pm
ACCY CHK	.07	9:35pm
AIR BLK	.00	9:36pm
SUB TEST	.00	9:37pm
AIR BLK	.00	9:38pm
SUB TEST	.00	9:40pm
AIR BLK	.00	9:41pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

Intox EC/IR-II: Preventive Maintenance

IREDELL COUNTY BAT MOBILE UNIT 8 480

Serial Number: 008736 Test Record Number: 1568
Test Date: 12/20/2025 Test Time: 9:41pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	9:42pm
FLO	Pass	9:42pm
FC	Pass	9:42pm

Temperature Tests

Test	Status	Time
FC1	Pass	9:42pm
SRC	Pass	9:42pm
DET	Pass	9:42pm
BAR	Pass	9:42pm
BT	Pass	9:42pm

Blank Tests

Test	Status	Time
AIR	Pass	9:43pm

Printer Tests

Test	Status	Time
PRNT	Pass	9:43pm

CRC Tests

Test	Status	Time
COMP	Pass	9:43pm
CAL	Pass	9:43pm

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Iredell Instrument Location BAT Mobile Unit 8

Instrument Serial No. 008775

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 20 day of December, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

2219283

Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

IREDELL COUNTY BAT MOBILE UNIT 8 480

Serial Number: 008775

Test Date: 12/20/2025

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Glasscock, Jerry D

Permit Number: 7180-9235

Effective:

02/01/2025-02/01/2027

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG506303

Exp Date: 03/04/2027

Test	g/210L	Time
DIAG	Pass	9:32pm
AIR BLK	.00	9:33pm
ACCY CHK	.08	9:34pm
AIR BLK	.00	9:35pm
SUB TEST	.00	9:35pm
AIR BLK	.00	9:36pm
SUB TEST	.00	9:38pm
AIR BLK	.00	9:39pm

Reported AC: .00 g/210L

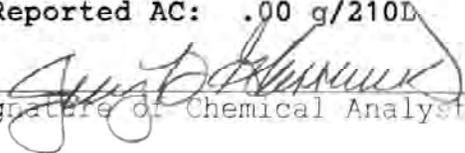
Signature of Chemical Analyst

Court CVR


Analyst

Intox EC/IR-II: Preventive Maintenance

IREDELL COUNTY BAT MOBILE UNIT 8 480

Serial Number: 008775 Test Record Number: 2421
Test Date: 12/20/2025 Test Time: 9:39pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	9:39pm
FLO	Pass	9:39pm
FC	Pass	9:39pm

Temperature Tests

Test	Status	Time
FC1	Pass	9:40pm
SRC	Pass	9:40pm
DET	Pass	9:40pm
BAR	Pass	9:40pm
BT	Pass	9:40pm

Blank Tests

Test	Status	Time
AIR	Pass	9:40pm

Printer Tests

Test	Status	Time
PRNT	Pass	9:40pm

CRC Tests

Test	Status	Time
COMP	Pass	9:40pm
CAL	Pass	9:40pm

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County IRENELL Instrument Location IRENELL CO. S.C.

Instrument Serial No. 008809 STATENVILLE NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 18 day of DECEMBER, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Jim S. Fleming
Signature of Certifying Official

214970
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

IREDELL COUNTY IREDELL COUNTY SO 480

Serial Number: 008809
Test Date: 12/18/2025

Citation Number: M0000000-0
Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Fleming, Tina S

Permit Number: 0027-4970

Effective:

02/01/2025-02/01/2027

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG506302
Exp Date: 03/04/2027

Test	g/210L	Time
DIAG	Pass	9:50am
AIR BLK	.00	9:51am
ACCY CHK	.07	9:52am
AIR BLK	.00	9:53am
SUB TEST	.00	9:53am
AIR BLK	.00	9:54am
SUB TEST	.00	9:56am
AIR BLK	.00	9:57am

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

IREDELL COUNTY IREDELL COUNTY SO 480

Serial Number: 008809 Test Record Number: 6549
Test Date: 12/18/2025 Test Time: 9:58am EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	9:58am
FLO	Pass	9:58am
FC	Pass	9:58am

Temperature Tests

Test	Status	Time
FC1	Pass	9:58am
SRC	Pass	9:58am
DET	Pass	9:58am
BAR	Pass	9:58am
BT	Pass	9:58am

Blank Tests

Test	Status	Time
AIR	Pass	9:59am

Printer Tests

Test	Status	Time
PRNT	Pass	9:59am

CRC Tests

Test	Status	Time
COMP	Pass	9:59am
CAL	Pass	9:59am

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Iredell Instrument Location BAT Mobile Unit 8
Instrument Serial No. 008816

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 20 day of December, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

2219783
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

IREDELL COUNTY BAT MOBILE UNIT 8 480

Serial Number: 008816
Test Date: 12/20/2025

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Glasscock, Jerry D

Permit Number: 7180-9235

Effective:

02/01/2025-02/01/2027

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG431002

Exp Date: 11/05/2026

Test	g/210L	Time
DIAG	Pass	9:31pm
AIR BLK	.00	9:32pm
ACCY CHK	.07	9:33pm
AIR BLK	.00	9:34pm
SUB TEST	.00	9:34pm
AIR BLK	.00	9:35pm
SUB TEST	.00	9:37pm
AIR BLK	.00	9:38pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

Intox EC/IR-II: Preventive Maintenance

IREDELL COUNTY BAT MOBILE UNIT 8 480

Serial Number: 008816 Test Record Number: 8004
Test Date: 12/20/2025 Test Time: 9:39pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	9:40pm
FLO	Pass	9:40pm
FC	Pass	9:40pm

Temperature Tests

Test	Status	Time
FC1	Pass	9:40pm
SRC	Pass	9:40pm
DET	Pass	9:40pm
BAR	Pass	9:40pm
BT	Pass	9:40pm

Blank Tests

Test	Status	Time
AIR	Pass	9:41pm

Printer Tests

Test	Status	Time
PRNT	Pass	9:41pm

CRC Tests

Test	Status	Time
COMP	Pass	9:41pm
CAL	Pass	9:41pm

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Iredell Instrument Location BAT Mobile Unit B
Instrument Serial No. 008929

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 20 day of December, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

2219283
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

IREDELL COUNTY BAT MOBILE UNIT 8 480

Serial Number: 008929

Test Date: 12/20/2025

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Glasscock, Jerry D

Permit Number: 7180-9235

Effective:

02/01/2025-02/01/2027

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG506303

Exp Date: 03/04/2027

Test	g/210L	Time
DIAG	Pass	9:30pm
AIR BLK	.00	9:31pm
ACCY CHK	.08	9:32pm
AIR BLK	.00	9:33pm
SUB TEST	.00	9:34pm
AIR BLK	.00	9:35pm
SUB TEST	.00	9:36pm
AIR BLK	.00	9:37pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

Intox EC/IR-II: Preventive Maintenance

IREDELL COUNTY BAT MOBILE UNIT 8 480

Serial Number: 008929 Test Record Number: 1705
Test Date: 12/20/2025 Test Time: 9:38pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	9:38pm
FLO	Pass	9:38pm
FC	Pass	9:39pm

Temperature Tests

Test	Status	Time
FC1	Pass	9:39pm
SRC	Pass	9:39pm
DET	Pass	9:39pm
BAR	Pass	9:39pm
BT	Pass	9:39pm

Blank Tests

Test	Status	Time
AIR	Pass	9:39pm

Printer Tests

Test	Status	Time
PRNT	Pass	9:39pm

CRC Tests

Test	Status	Time
COMP	Pass	9:40pm
CAL	Pass	9:40pm

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County JONES Instrument Location JONES COUNTY
Instrument Serial No. 008705 DETENTION CENTER

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 12th day of DECEMBER, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

2824950
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

JONES COUNTY DETENTION CENTER 510

Serial Number: 008705
Test Date: 12/12/2025

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: GILLESPIE, PENTTI W

Permit Number: 9523-2149

Effective:

02/01/2025-02/01/2027

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG501307


Exp Date: 01/13/2027

Test	g/210L	Time
DIAG	Pass	1:42pm
AIR BLK	.00	1:42pm
ACCY CHK	.07	1:43pm
AIR BLK	.00	1:44pm
SUB TEST	.00	1:45pm
AIR BLK	.00	1:46pm
SUB TEST	.00	1:47pm
AIR BLK	.00	1:48pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR

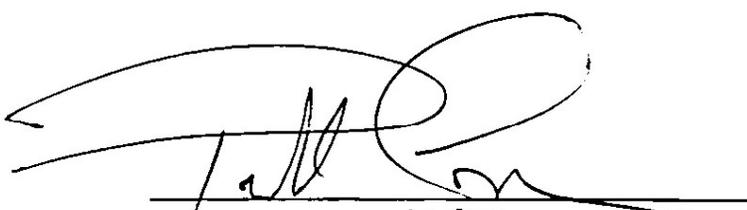
Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

JONES COUNTY DETENTION CENTER 510

Serial Number: 008705 Test Record Number: 1944
Test Date: 12/12/2025 Test Time: 1:49pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	1:50pm
FLO	Pass	1:50pm
FC	Pass	1:50pm

Temperature Tests

Test	Status	Time
FC1	Pass	1:50pm
SRC	Pass	1:50pm
DET	Pass	1:50pm
BAR	Pass	1:50pm
BT	Pass	1:50pm

Blank Tests

Test	Status	Time
AIR	Pass	1:51pm

Printer Tests

Test	Status	Time
PRNT	Pass	1:51pm

CRC Tests

Test	Status	Time
COMP	Pass	1:51pm
CAL	Pass	1:51pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County Lenoir Instrument Location BAT Mobile Unit 7

Instrument Serial No. 008002

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 20th day of December, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.





Signature of Certifying Official

2266313

Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

LENOIR COUNTY BAT MOBILE UNIT 7 530

Serial Number: 008002
Test Date: 12/20/2025

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Sharpe Jr., Robert J

Permit Number: 1820-8591

Effective:

02/01/2025-02/01/2027

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG506303

Exp Date: 03/04/2027

Test	g/210L	Time
DIAG	Pass	9:45pm
AIR BLK	.00	9:46pm
ACCY CHK	.08	9:47pm
AIR BLK	.00	9:47pm
SUB TEST	.00	9:48pm
AIR BLK	.00	9:49pm
SUB TEST	.00	9:50pm
AIR BLK	.00	9:51pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

LENOIR COUNTY BAT MOBILE UNIT 7 530

Serial Number: 008002 Test Record Number: 857
Test Date: 12/20/2025 Test Time: 9:52pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	9:53pm
FLO	Pass	9:53pm
FC	Pass	9:53pm

Temperature Tests

Test	Status	Time
FC1	Pass	9:53pm
SRC	Pass	9:53pm
DET	Pass	9:53pm
BAR	Pass	9:53pm
BT	Pass	9:53pm

Blank Tests

Test	Status	Time
AIR	Pass	9:53pm

Printer Tests

Test	Status	Time
PRNT	Pass	9:53pm

CRC Tests

Test	Status	Time
COMP	Pass	9:54pm
CAL	Pass	9:54pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County Lenoir Instrument Location Kinston P.D.

Instrument Serial No. 008624 205 E King St., Kinston, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 19th day of December, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

377722
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

LENOIR COUNTY KINSTON PD 530

Serial Number: 008624
Test Date: 12/19/2025

Citation Number: M0000000-0
Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Gray, Kelly D

Permit Number: 0037-7722

Effective:

02/01/2025-02/01/2027

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG431003

Exp Date: 11/05/2026


Test	g/210L	Time
DIAG	Pass	9:48am
AIR BLK	.00	9:49am
ACCY CHK	.07	9:49am
AIR BLK	.00	9:50am
SUB TEST	.00	9:51am
AIR BLK	.00	9:52am
SUB TEST	.00	9:54am
AIR BLK	.00	9:55am

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

LENOIR COUNTY KINSTON PD 530

Serial Number: 008624 Test Record Number: 2472
Test Date: 12/19/2025 Test Time: 9:56am EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	9:56am
FLO	Pass	9:56am
FC	Pass	9:56am

Temperature Tests

Test	Status	Time
FC1	Pass	9:56am
SRC	Pass	9:56am
DET	Pass	9:56am
BAR	Pass	9:56am
BT	Pass	9:56am

Blank Tests

Test	Status	Time
AIR	Pass	9:57am


Printer Tests

Test	Status	Time
PRNT	Pass	9:57am

CRC Tests

Test	Status	Time
COMP	Pass	9:57am
CAL	Pass	9:57am

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Lenoir Instrument Location Lenoir Co. S.O.
Instrument Serial No. 608639 130 Queen St., Kinston, NC.

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 19th day of December, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

377722
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

LENOIR COUNTY LENOIR CO SO 530

Serial Number: 008639
Test Date: 12/19/2025

Citation Number: M0000000-0
Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Gray, Kelly D

Permit Number: 0037-7722

Effective:

02/01/2025-02/01/2027

Officer's Name: NONE, NONE

Type of Agency: FTA


Agency: DHHS

Test Type: Breath Test

Lot Number: AG516203
Exp Date: 06/11/2027

Test	g/210L	Time
DIAG	Pass	10:26am
AIR BLK	.00	10:26am
ACCY CHK	.07	10:27am
AIR BLK	.00	10:28am
SUB TEST	.00	10:29am
AIR BLK	.00	10:29am
SUB TEST	.00	10:31am
AIR BLK	.00	10:32am

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

Intox EC/IR-II: Preventive Maintenance

LENOIR COUNTY LENOIR CO SO 530

Serial Number: 008639 Test Record Number: 4365
Test Date: 12/19/2025 Test Time: 10:33am EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	10:33am
FLO	Pass	10:33am
FC	Pass	10:34am

Temperature Tests

Test	Status	Time
FC1	Pass	10:34am
SRC	Pass	10:34am
DET	Pass	10:34am
BAR	Pass	10:34am
BT	Pass	10:34am

Blank Tests

Test	Status	Time
AIR	Pass	10:34am

Printer Tests

Test	Status	Time
PRNT	Pass	10:34am

CRC Tests

Test	Status	Time
COMP	Pass	10:34am
CAL	Pass	10:34am

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Lenoir Instrument Location BAT Mobile Unit 7

Instrument Serial No. 00 8968

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 20th day of December, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

2266313
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

LENOIR COUNTY BAT MOBILE UNIT 7 530

Serial Number: 008968
Test Date: 12/20/2025

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Sharpe Jr., Robert J

Permit Number: 1820-8591

Effective:

02/01/2025-02/01/2027

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG506303

Exp Date: 03/04/2027

Test	g/210L	Time
DIAG	Pass	9:46pm
AIR BLK	.00	9:47pm
ACCY CHK	.08	9:47pm
AIR BLK	.00	9:48pm
SUB TEST	.00	9:49pm
AIR BLK	.00	9:50pm
SUB TEST	.00	9:51pm
AIR BLK	.00	9:52pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

LENOIR COUNTY BAT MOBILE UNIT 7 530

Serial Number: 008968 Test Record Number: 426
Test Date: 12/20/2025 Test Time: 9:53pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	9:53pm
FLO	Pass	9:53pm
FC	Pass	9:54pm

Temperature Tests

Test	Status	Time
FC1	Pass	9:54pm
SRC	Pass	9:54pm
DET	Pass	9:54pm
BAR	Pass	9:54pm
BT	Pass	9:54pm

Blank Tests

Test	Status	Time
AIR	Pass	9:54pm

Printer Tests

Test	Status	Time
PRNT	Pass	9:54pm

CRC Tests

Test	Status	Time
COMP	Pass	9:54pm
CAL	Pass	9:54pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County Lenoir Instrument Location BAT Mobile Unit 7

Instrument Serial No. 008971

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 20th day of December, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]

Signature of Certifying Official

2266313

Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

LENOIR COUNTY BAT MOBILE UNIT 7 530

Serial Number: 008971

Test Date: 12/20/2025

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Sharpe Jr., Robert J

Permit Number: 1820-8591

Effective:

02/01/2025-02/01/2027

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG506302

Exp Date: 03/04/2027

Test	g/210L	Time
DIAG	Pass	9:44pm
AIR BLK	.00	9:45pm
ACCY CHK	.08	9:46pm
AIR BLK	.00	9:47pm
SUB TEST	.00	9:47pm
AIR BLK	.00	9:48pm
SUB TEST	.00	9:50pm
AIR BLK	.00	9:51pm

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR

Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

LENOIR COUNTY BAT MOBILE UNIT 7 530

Serial Number: 008971 Test Record Number: 376
Test Date: 12/20/2025 Test Time: 9:51pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	9:52pm
FLO	Pass	9:52pm
FC	Pass	9:52pm

Temperature Tests

Test	Status	Time
FC1	Pass	9:52pm
SRC	Pass	9:52pm
DET	Pass	9:52pm
BAR	Pass	9:52pm
BT	Pass	9:52pm

Blank Tests

Test	Status	Time
AIR	Pass	9:52pm

Printer Tests

Test	Status	Time
PRNT	Pass	9:52pm

CRC Tests

Test	Status	Time
COMP	Pass	9:53pm
CAL	Pass	9:53pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Lenoir Instrument Location BAT Mobile Unit 7

Instrument Serial No. 008972

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 20th day of December, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

2266313
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

LENOIR COUNTY BAT MOBILE UNIT 7 530

Serial Number: 008972
Test Date: 12/20/2025

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Sharpe Jr., Robert J

Permit Number: 1820-8591

Effective:

02/01/2025-02/01/2027

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG506303

Exp Date: 03/04/2027


Test	g/210L	Time
DIAG	Pass	9:43pm
AIR BLK	.00	9:44pm
ACCY CHK	.08	9:45pm
AIR BLK	.00	9:46pm
SUB TEST	.00	9:47pm
AIR BLK	.00	9:48pm
SUB TEST	.00	9:49pm
AIR BLK	.00	9:50pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR

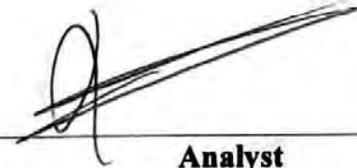

Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

LENOIR COUNTY BAT MOBILE UNIT 7 530

Serial Number: 008972 Test Record Number: 437
Test Date: 12/20/2025 Test Time: 9:51pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	9:51pm
FLO	Pass	9:51pm
FC	Pass	9:52pm

Temperature Tests

Test	Status	Time
FC1	Pass	9:52pm
SRC	Pass	9:52pm
DET	Pass	9:52pm
BAR	Pass	9:52pm
BT	Pass	9:52pm

Blank Tests

Test	Status	Time
AIR	Pass	9:52pm

Printer Tests

Test	Status	Time
PRNT	Pass	9:52pm

CRC Tests

Test	Status	Time
COMP	Pass	9:53pm
CAL	Pass	9:53pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County McDowell Instrument Location McDowell County Jail

Instrument Serial No. 008888 Marion, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 29 day of December, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

244987
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

MCDOWELL COUNTY MCDOWELL COUNTY JAIL
580

Serial Number: 008888
Test Date: 12/29/2025

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Loftis, Benjamin C

Permit Number: 0024-4987

Effective:

03/01/2025-03/01/2027

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG431001

Exp Date: 11/05/2026


Test	g/210L	Time
DIAG	Pass	12:39pm
AIR BLK	.00	12:40pm
ACCY CHK	.07	12:40pm
AIR BLK	.00	12:42pm
SUB TEST	.00	12:42pm
AIR BLK	.00	12:43pm
SUB TEST	.00	12:44pm
AIR BLK	.00	12:45pm

Reported AC: .00 g/210L

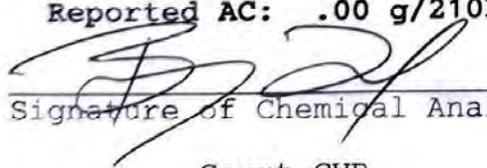

Signature of Chemical Analyst

Court CVR

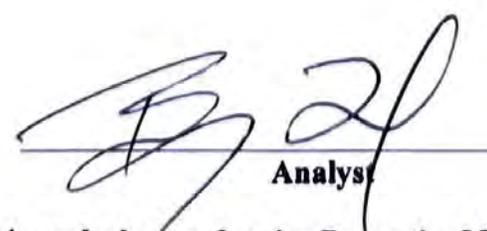

Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

MCDOWELL COUNTY MCDOWELL COUNTY JAIL 580

Serial Number: 008888 Test Record Number: 1930
Test Date: 12/29/2025 Test Time: 12:45pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	12:46pm
FLO	Pass	12:46pm
FC	Pass	12:46pm

Temperature Tests

Test	Status	Time
FC1	Pass	12:46pm
SRC	Pass	12:46pm
DET	Pass	12:46pm
BAR	Pass	12:46pm
BT	Pass	12:46pm

Blank Tests

Test	Status	Time
AIR	Pass	12:47pm

Printer Tests

Test	Status	Time
PRNT	Pass	12:47pm

CRC Tests

Test	Status	Time
COMP	Pass	12:47pm
CAL	Pass	12:47pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County McDowell Instrument Location McDowell County Jail

Instrument Serial No. 008897 Marion, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 29 day of December, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

244987
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

MCDOWELL COUNTY MCDOWELL COUNTY JAIL
580

Serial Number: 008892
Test Date: 12/29/2025

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: Loftis, Benjamin C
Permit Number: 0024-4987
Effective:
03/01/2025-03/01/2027

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test


Lot Number: AG506303
Exp Date: 03/04/2027

Test	g/210L	Time
DIAG	Pass	12:39pm
AIR BLK	.00	12:39pm
ACCY CHK	.07	12:40pm
AIR BLK	.00	12:41pm
SUB TEST	.00	12:42pm
AIR BLK	.00	12:43pm
SUB TEST	.00	12:44pm
AIR BLK	.00	12:45pm

Reported AC: .00 g/210L

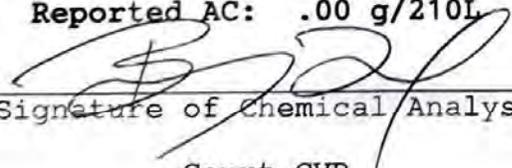

Signature of Chemical Analyst
Court CVR

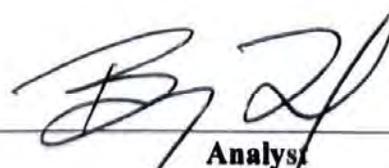

Analyst

Intox EC/IR-II: Preventive Maintenance

MCDOWELL COUNTY MCDOWELL COUNTY JAIL 580

Serial Number: 008892 Test Record Number: 1447
Test Date: 12/29/2025 Test Time: 12:45pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	12:46pm
FLO	Pass	12:46pm
FC	Pass	12:46pm

Temperature Tests

Test	Status	Time
FC1	Pass	12:46pm
SRC	Pass	12:46pm
DET	Pass	12:46pm
BAR	Pass	12:46pm
BT	Pass	12:46pm

Blank Tests

Test	Status	Time
AIR	Pass	12:46pm

Printer Tests

Test	Status	Time
PRNT	Pass	12:47pm

CRC Tests

Test	Status	Time
COMP	Pass	12:47pm
CAL	Pass	12:47pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County Mecklenburg Instrument Location CMPD LEC
Instrument Serial No. 008594 Charlotte, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 18th day of December, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Boye Helms
Signature of Certifying Official

849845
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

MECKLENBURG COUNTY CMPD LEC 590

Serial Number: 008594
Test Date: 12/18/2025

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Helms, Bryce A

Permit Number: 0084-9845

Effective:

02/01/2025-02/01/2027

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG516203


Exp Date: 06/11/2027

Test	g/210L	Time
DIAG	Pass	11:04am
AIR BLK	.00	11:04am
ACCY CHK	.08	11:05am
AIR BLK	.00	11:06am
SUB TEST	.00	11:07am
AIR BLK	.00	11:08am
SUB TEST	.00	11:11am
AIR BLK	.00	11:12am

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR

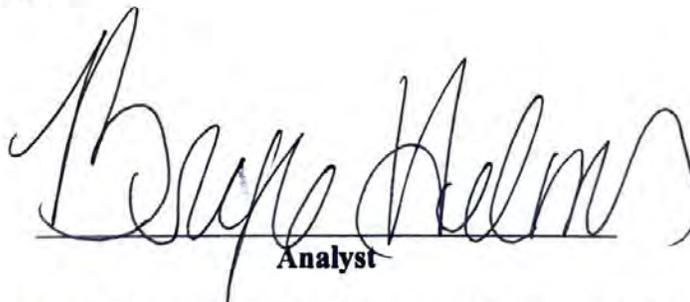
Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

MECKLENBURG COUNTY CMPD LEC 590

Serial Number: 008594 Test Record Number: 6546
Test Date: 12/18/2025 Test Time: 11:14am EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	11:14am
FLO	Pass	11:14am
FC	Pass	11:14am

Temperature Tests

Test	Status	Time
FC1	Pass	11:14am
SRC	Pass	11:14am
DET	Pass	11:14am
BAR	Pass	11:14am
BT	Pass	11:14am

Blank Tests

Test	Status	Time
AIR	Pass	11:15am

Printer Tests


Test	Status	Time
PRNT	Pass	11:15am

CRC Tests

Test	Status	Time
COMP	Pass	11:15am
CAL	Pass	11:15am

Preventive Maintenance

Status: Pass

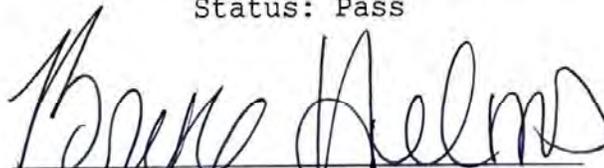
Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Mecklenburg Instrument Location BAT Mobile Unit 8

Instrument Serial No. 0086015

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 11 day of December, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

2219783
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

MECKLENBURG COUNTY BAT MOBILE UNIT 8
590

Serial Number: 008615
Test Date: 12/11/2025

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE

Analyst's Name: Glasscock, Jerry D
Permit Number: 7180-9235
Effective:
02/01/2025-02/01/2027

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG405102
Exp Date: 02/20/2026

Test	g/210L	Time
DIAG	Pass	9:07pm
AIR BLK	.00	9:08pm
ACCY CHK	.07	9:08pm
AIR BLK	.00	9:09pm
SUB TEST	.00	9:10pm
AIR BLK	.00	9:11pm
SUB TEST	.00	9:12pm
AIR BLK	.00	9:13pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

MECKLENBURG COUNTY BAT MOBILE UNIT 8 590

Serial Number: 008615 Test Record Number: 6200
Test Date: 12/11/2025 Test Time: 9:16pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	9:17pm
FLO	Pass	9:17pm
FC	Pass	9:17pm

Temperature Tests

Test	Status	Time
FC1	Pass	9:17pm
SRC	Pass	9:17pm
DET	Pass	9:17pm
BAR	Pass	9:17pm
BT	Pass	9:17pm

Blank Tests

Test	Status	Time
AIR	Pass	9:18pm

Printer Tests

Test	Status	Time
PRNT	Pass	9:18pm

CRC Tests

Test	Status	Time
COMP	Pass	9:18pm
CAL	Pass	9:18pm

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Mecklenburg Instrument Location BAT Mobile Unit 8

Instrument Serial No. 008615 _____

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 11 day of December, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

2219283
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

MECKLENBURG COUNTY BAT MOBILE UNIT 8
590

Serial Number: 008615
Test Date: 12/11/2025

Citation Number: M0000000-0
Subject's Name:

PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: Glasscock, Jerry D
Permit Number: 7180-9235
Effective:
02/01/2025-02/01/2027

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG405102
Exp Date: 02/20/2026

Test	g/210L	Time
DIAG	Pass	8:57am
AIR BLK	.00	8:58am
ACCY CHK	.07	8:58am
AIR BLK	.00	8:59am
SUB TEST	.00	9:00am
AIR BLK	.00	9:01am
SUB TEST	.00	9:02am
AIR BLK	.00	9:03am

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

Intox EC/IR-II: Preventive Maintenance

MECKLENBURG COUNTY BAT MOBILE UNIT 8 590

Serial Number: 008615 Test Record Number: 6198

Test Date: 12/11/2025 Test Time: 9:07am EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	9:07am
FLO	Pass	9:07am
FC	Pass	9:07am

Temperature Tests

Test	Status	Time
FC1	Pass	9:07am
SRC	Pass	9:07am
DET	Pass	9:07am
BAR	Pass	9:07am
BT	Pass	9:07am

Blank Tests

Test	Status	Time
AIR	Pass	9:08am

Printer Tests

Test	Status	Time
PRNT	Pass	9:08am

CRC Tests

Test	Status	Time
COMP	Pass	9:08am
CAL	Pass	9:08am

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Mecklenburg Instrument Location Mecklenburg County 80
Instrument Serial No. 0086605 Charlotte, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 18th day of December, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Barry Helms
Signature of Certifying Official

849845
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

MECKLENBURG COUNTY SHERIFFS OFFICE 590

Serial Number: 008665
Test Date: 12/18/2025

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: Helms, Bryce A
Permit Number: 0084-9845
Effective:
02/01/2025-02/01/2027

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG506302
Exp Date: 03/04/2027


Test	g/210L	Time
DIAG	Pass	10:19am
AIR BLK	.00	10:19am
ACCY CHK	.07	10:20am
AIR BLK	.00	10:21am
SUB TEST	.00	10:22am
AIR BLK	.00	10:23am
SUB TEST	.00	10:24am
AIR BLK	.00	10:25am

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR

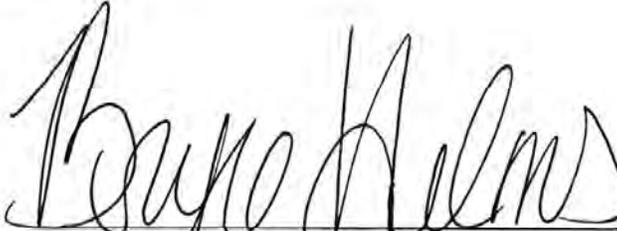

Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

MECKLENBURG COUNTY SHERIFFS OFFICE 590

Serial Number: 008665 Test Record Number: 5919
Test Date: 12/18/2025 Test Time: 10:25am EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	10:26am
FLO	Pass	10:26am
FC	Pass	10:26am

Temperature Tests

Test	Status	Time
FC1	Pass	10:26am
SRC	Pass	10:26am
DET	Pass	10:26am
BAR	Pass	10:26am
BT	Pass	10:26am

Blank Tests

Test	Status	Time
AIR	Pass	10:27am


Printer Tests

Test	Status	Time
PRNT	Pass	10:27am

CRC Tests

Test	Status	Time
COMP	Pass	10:27am
CAL	Pass	10:27am

Preventive Maintenance
Status: Pass

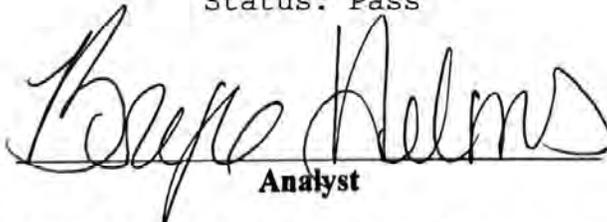
Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Mecklenburg Instrument Location CMPD LEC
Instrument Serial No. 008694 Charlotte, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 18th day of December, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature] 849845
Signature of Certifying Official Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

MECKLENBURG COUNTY CMPD LEC 590

Serial Number: 008691
Test Date: 12/18/2025

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Helms, Bryce A

Permit Number: 0084-9845

Effective:

02/01/2025-02/01/2027

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG506303

Exp Date: 03/04/2027


Test	g/210L	Time
DIAG	Pass	11:05am
AIR BLK	.00	11:06am
ACCY CHK	.07	11:07am
AIR BLK	.00	11:08am
SUB TEST	.00	11:09am
AIR BLK	.00	11:10am
SUB TEST	.00	11:12am
AIR BLK	.00	11:12am

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR

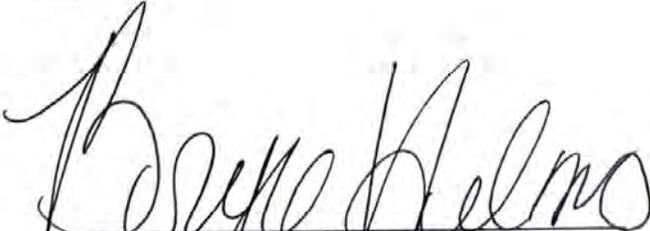

Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

MECKLENBURG COUNTY CMPD LEC 590

Serial Number: 008691 Test Record Number: 10033
Test Date: 12/18/2025 Test Time: 11:13am EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	11:13am
FLO	Pass	11:13am
FC	Pass	11:14am

Temperature Tests

Test	Status	Time
FC1	Pass	11:14am
SRC	Pass	11:14am
DET	Pass	11:14am
BAR	Pass	11:14am
BT	Pass	11:14am

Blank Tests

Test	Status	Time
AIR	Pass	11:14am


Printer Tests

Test	Status	Time
PRNT	Pass	11:14am

CRC Tests

Test	Status	Time
COMP	Pass	11:15am
CAL	Pass	11:15am

Preventive Maintenance
Status: Pass

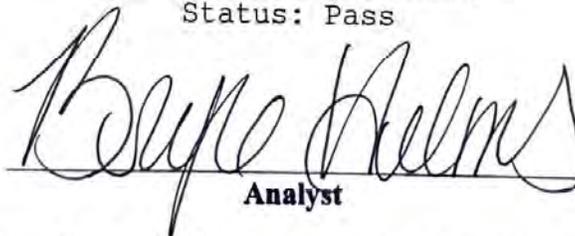
Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County Mecklenburg Instrument Location Pineville PD
Instrument Serial No. 008703 Pineville, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 22nd day of December, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Handwritten Signature]
Signature of Certifying Official

849845
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

MECKLENBURG COUNTY PINEVILLE PD 590

Serial Number: 008703
Test Date: 12/22/2025

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Helms, Bryce A

Permit Number: 0084-9845

Effective:

02/01/2025-02/01/2027

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG405102


Exp Date: 02/20/2026

Test	g/210L	Time
DIAG	Pass	1:05pm
AIR BLK	.00	1:06pm
ACCY CHK	.08	1:07pm
AIR BLK	.00	1:07pm
SUB TEST	.00	1:08pm
AIR BLK	.00	1:09pm
SUB TEST	.00	1:10pm
AIR BLK	.00	1:12pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR

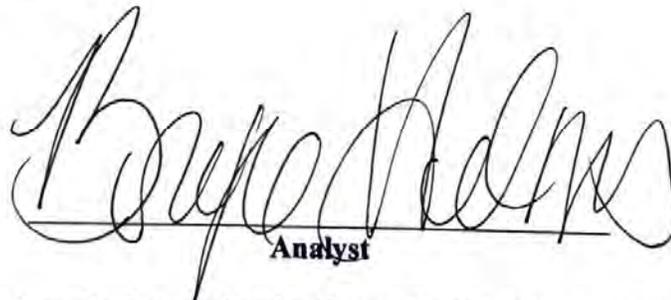
Analyst

Intox EC/IR-II: Preventive Maintenance

MECKLENBURG COUNTY PINEVILLE PD 590

Serial Number: 008703 Test Record Number: 6364
Test Date: 12/22/2025 Test Time: 1:12pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	1:12pm
FLO	Pass	1:12pm
FC	Pass	1:13pm

Temperature Tests

Test	Status	Time
FC1	Pass	1:13pm
SRC	Pass	1:13pm
DET	Pass	1:13pm
BAR	Pass	1:13pm
BT	Pass	1:13pm

Blank Tests

Test	Status	Time
AIR	Pass	1:13pm


Printer Tests

Test	Status	Time
PRNT	Pass	1:13pm

CRC Tests

Test	Status	Time
COMP	Pass	1:14pm
CAL	Pass	1:14pm

Preventive Maintenance
Status: Pass

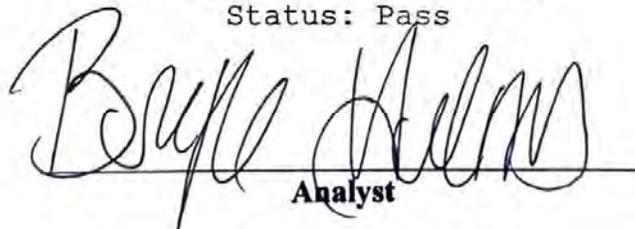
Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Mecklenburg Instrument Location BAT Mobile Unit 8
Instrument Serial No. 008736 _____

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 11 day of December, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

2219283
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

MECKLENBURG COUNTY BAT MOBILE UNIT 8
590

Serial Number: 008736
Test Date: 12/11/2025

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE

Analyst's Name: Glasscock, Jerry D
Permit Number: 7180-9235
Effective:
02/01/2025-02/01/2027

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG405102
Exp Date: 02/20/2026

Test	g/210L	Time
DIAG	Pass	9:06pm
AIR BLK	.00	9:07pm
ACCY CHK	.07	9:07pm
AIR BLK	.00	9:08pm
SUB TEST	.00	9:09pm
AIR BLK	.00	9:10pm
SUB TEST	.00	9:11pm
AIR BLK	.00	9:12pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

Intox EC/IR-II: Preventive Maintenance

MECKLENBURG COUNTY BAT MOBILE UNIT 8 590

Serial Number: 008736 Test Record Number: 1560
Test Date: 12/11/2025 Test Time: 9:13pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	9:13pm
FLO	Pass	9:13pm
FC	Pass	9:13pm

Temperature Tests

Test	Status	Time
FC1	Pass	9:13pm
SRC	Pass	9:13pm
DET	Pass	9:13pm
BAR	Pass	9:13pm
BT	Pass	9:13pm

Blank Tests

Test	Status	Time
AIR	Pass	9:14pm

Printer Tests

Test	Status	Time
PRNT	Pass	9:14pm

CRC Tests

Test	Status	Time
COMP	Pass	9:14pm
CAL	Pass	9:14pm

Preventive Maintenance
Status: *Pass*


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Mecklenburg Instrument Location BAT Mobile Unit 8
Instrument Serial No. 008736

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date; or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 11 day of December, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

2219283
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

MECKLENBURG COUNTY BAT MOBILE UNIT 8
590

Serial Number: 008736
Test Date: 12/11/2025

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Glasscock, Jerry D

Permit Number: 7180-9235

Effective:

02/01/2025-02/01/2027

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG405102

Exp Date: 02/20/2026

Test	g/210L	Time
DIAG	Pass	8:55am
AIR BLK	.00	8:56am
ACCY CHK	.07	8:57am
AIR BLK	.00	8:58am
SUB TEST	.00	8:58am
AIR BLK	.00	8:59am
SUB TEST	.00	9:01am
AIR BLK	.00	9:02am

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

MECKLENBURG COUNTY BAT MOBILE UNIT 8 590

Serial Number: 008736 Test Record Number: 1558
Test Date: 12/11/2025 Test Time: 9:03am EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	9:04am
FLO	Pass	9:04am
FC	Pass	9:04am

Temperature Tests

Test	Status	Time
FC1	Pass	9:04am
SRC	Pass	9:04am
DET	Pass	9:04am
BAR	Pass	9:04am
BT	Pass	9:04am

Blank Tests

Test	Status	Time
AIR	Pass	9:04am

Printer Tests

Test	Status	Time
PRNT	Pass	9:05am

CRC Tests

Test	Status	Time
COMP	Pass	9:05am
CAL	Pass	9:05am

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County MECKLENBURG Instrument Location HUNTERVILLE PD

Instrument Serial No. 008747 HUNTERVILLE NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 12 day of DECEMBER, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

274970
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

MECKLENBURG COUNTY HUNTERSVILLE PD 590

Serial Number: 008747
Test Date: 12/12/2025

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Fleming, Tina S

Permit Number: 0027-4970

Effective:

02/01/2025-02/01/2027

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG516204

Exp Date: 06/11/2027


Test	g/210L	Time
DIAG	Pass	8:53am
AIR BLK	.00	8:53am
ACCY CHK	.07	8:54am
AIR BLK	.00	8:55am
SUB TEST	.00	8:56am
AIR BLK	.00	8:57am
SUB TEST	.00	8:58am
AIR BLK	.00	8:59am

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

MECKLENBURG COUNTY HUNTERSVILLE PD 590

Serial Number: 008747 Test Record Number: 3460
Test Date: 12/12/2025 Test Time: 9:00am EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	9:00am
FLO	Pass	9:00am
FC	Pass	9:00am

Temperature Tests

Test	Status	Time
FC1	Pass	9:00am
SRC	Pass	9:00am
DET	Pass	9:00am
BAR	Pass	9:00am
BT	Pass	9:00am

Blank Tests

Test	Status	Time
AIR	Pass	9:01am


Printer Tests

Test	Status	Time
PRNT	Pass	9:01am

CRC Tests

Test	Status	Time
COMP	Pass	9:01am
CAL	Pass	9:01am

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Mecklenburg Instrument Location BAT Mobile Unit 8
Instrument Serial No. 008775 _____

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 11 day of December, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

2219283
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

MECKLENBURG COUNTY BAT MOBILE UNIT 8
590

Serial Number: 008775
Test Date: 12/11/2025

Citation Number: M0000000-0
Subject's Name:

PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE

Analyst's Name: Glasscock, Jerry D
Permit Number: 7180-9235
Effective:
02/01/2025-02/01/2027

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG506303
Exp Date: 03/04/2027

Test	g/210L	Time
DIAG	Pass	9:05pm
AIR BLK	.00	9:06pm
ACCY CHK	.08	9:06pm
AIR BLK	.00	9:07pm
SUB TEST	.00	9:08pm
AIR BLK	.00	9:09pm
SUB TEST	.00	9:10pm
AIR BLK	.00	9:11pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

Intox EC/IR-II: Preventive Maintenance

MECKLENBURG COUNTY BAT MOBILE UNIT 8 590

Serial Number: 008775 Test Record Number: 2411
Test Date: 12/11/2025 Test Time: 9:12pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	9:12pm
FLO	Pass	9:12pm
FC	Pass	9:12pm

Temperature Tests

Test	Status	Time
FC1	Pass	9:12pm
SRC	Pass	9:12pm
DET	Pass	9:12pm
BAR	Pass	9:12pm
BT	Pass	9:12pm

Blank Tests

Test	Status	Time
AIR	Pass	9:13pm

Printer Tests

Test	Status	Time
PRNT	Pass	9:13pm

CRC Tests

Test	Status	Time
COMP	Pass	9:13pm
CAL	Pass	9:13pm

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Mecklenburg Instrument Location BAT Mobile Unit 8
Instrument Serial No. 008775

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 11 day of December, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

2219283
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

MECKLENBURG COUNTY BAT MOBILE UNIT 8
590

Serial Number: 008775
Test Date: 12/11/2025

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE

Analyst's Name: Glasscock, Jerry D
Permit Number: 7180-9235
Effective:
02/01/2025-02/01/2027

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG506303
Exp Date: 03/04/2027

Test	g/210L	Time
DIAG	Pass	8:55am
AIR BLK	.00	8:56am
ACCY CHK	.08	8:56am
AIR BLK	.00	8:57am
SUB TEST	.00	8:58am
AIR BLK	.00	8:59am
SUB TEST	.00	9:00am
AIR BLK	.00	9:01am

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

MECKLENBURG COUNTY BAT MOBILE UNIT 8 590

Serial Number: 008775 Test Record Number: 2409
Test Date: 12/11/2025 Test Time: 9:03am EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	9:04am
FLO	Pass	9:04am
FC	Pass	9:04am

Temperature Tests

Test	Status	Time
FC1	Pass	9:04am
SRC	Pass	9:04am
DET	Pass	9:04am
BAR	Pass	9:04am
BT	Pass	9:04am

Blank Tests

Test	Status	Time
AIR	Pass	9:05am

Printer Tests

Test	Status	Time
PRNT	Pass	9:05am

CRC Tests

Test	Status	Time
COMP	Pass	9:05am
CAL	Pass	9:05am

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County Mecklenburg Instrument Location BAT Mobile Unit 8

Instrument Serial No. 008816

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 11 day of December, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.




Signature of Certifying Official

2219283
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

MECKLENBURG COUNTY BAT MOBILE UNIT 8
590

Serial Number: 008816
Test Date: 12/11/2025

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Glasscock, Jerry D

Permit Number: 7180-9235

Effective:

02/01/2025-02/01/2027

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG431002

Exp Date: 11/05/2026

Test	g/210L	Time
DIAG	Pass	8:59pm
AIR BLK	.00	9:00pm
ACCY CHK	.08	9:01pm
AIR BLK	.00	9:02pm
SUB TEST	.00	9:03pm
AIR BLK	.00	9:04pm
SUB TEST	.00	9:05pm
AIR BLK	.00	9:06pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

Intox EC/IR-II: Preventive Maintenance

MECKLENBURG COUNTY BAT MOBILE UNIT 8 590

Serial Number: 008816 Test Record Number: 7993
Test Date: 12/11/2025 Test Time: 9:07pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	9:07pm
FLO	Pass	9:07pm
FC	Pass	9:08pm

Temperature Tests

Test	Status	Time
FC1	Pass	9:08pm
SRC	Pass	9:08pm
DET	Pass	9:08pm
BAR	Pass	9:08pm
BT	Pass	9:08pm

Blank Tests

Test	Status	Time
AIR	Pass	9:08pm

Printer Tests

Test	Status	Time
PRNT	Pass	9:08pm

CRC Tests

Test	Status	Time
COMP	Pass	9:09pm
CAL	Pass	9:09pm

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Mecklenburg Instrument Location BAT Mobile Unit 8

Instrument Serial No. 008816

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 11 day of December, 2025 the foregoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

2219283
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

MECKLENBURG COUNTY BAT MOBILE UNIT 8
590

Serial Number: 008816
Test Date: 12/11/2025

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Glasscock, Jerry D

Permit Number: 7180-9235

Effective:

02/01/2025-02/01/2027

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG431002

Exp Date: 11/05/2026

Test	g/210L	Time
DIAG	Pass	8:54am
AIR BLK	.00	8:55am
ACCY CHK	.08	8:56am
AIR BLK	.00	8:57am
SUB TEST	.00	8:58am
AIR BLK	.00	8:59am
SUB TEST	.00	9:00am
AIR BLK	.00	9:01am

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

MECKLENBURG COUNTY BAT MOBILE UNIT 8 590

Serial Number: 008816 Test Record Number: 7991
Test Date: 12/11/2025 Test Time: 9:03am EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	9:04am
FLO	Pass	9:04am
FC	Pass	9:04am

Temperature Tests

Test	Status	Time
FC1	Pass	9:04am
SRC	Pass	9:04am
DET	Pass	9:04am
BAR	Pass	9:04am
BT	Pass	9:04am

Blank Tests

Test	Status	Time
AIR	Pass	9:04am

Printer Tests

Test	Status	Time
PRNT	Pass	9:04am

CRC Tests

Test	Status	Time
COMP	Pass	9:05am
CAL	Pass	9:05am

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Mecklenburg Instrument Location BAT Mobile Unit 8
Instrument Serial No. 008929

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 11 day of December, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

2219283
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

MECKLENBURG COUNTY BAT MOBILE UNIT 8
590

Serial Number: 008929
Test Date: 12/11/2025

Citation Number: M0000000-0
Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Glasscock, Jerry D

Permit Number: 7180-9235

Effective:

02/01/2025-02/01/2027

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG506303

Exp Date: 03/04/2027

Test	g/210L	Time
DIAG	Pass	8:58pm
AIR BLK	.00	8:59pm
ACCY CHK	.08	9:00pm
AIR BLK	.00	9:01pm
SUB TEST	.00	9:02pm
AIR BLK	.00	9:04pm
SUB TEST	.00	9:05pm
AIR BLK	.00	9:06pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

Intox EC/IR-II: Preventive Maintenance

MECKLENBURG COUNTY BAT MOBILE UNIT 8 590

Serial Number: 008929 Test Record Number: 1697
Test Date: 12/11/2025 Test Time: 9:07pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	9:07pm
FLO	Pass	9:07pm
FC	Pass	9:07pm

Temperature Tests

Test	Status	Time
FC1	Pass	9:08pm
SRC	Pass	9:08pm
DET	Pass	9:08pm
BAR	Pass	9:08pm
BT	Pass	9:08pm

Blank Tests

Test	Status	Time
AIR	Pass	9:08pm

Printer Tests

Test	Status	Time
PRNT	Pass	9:08pm

CRC Tests

Test	Status	Time
COMP	Pass	9:09pm
CAL	Pass	9:09pm

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Mecklenburg Instrument Location BAT Mobile Unit 8
Instrument Serial No. 008929

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 11 day of December, 2025 the foregoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

2219283
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

MECKLENBURG COUNTY BAT MOBILE UNIT 8
590

Serial Number: 008929
Test Date: 12/11/2025

Citation Number: M0000000-0
Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Glasscock, Jerry D

Permit Number: 7180-9235

Effective:

02/01/2025-02/01/2027

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG506303


Exp Date: 03/04/2027

Test	g/210L	Time
DIAG	Pass	8:53am
AIR BLK	.00	8:54am
ACCY CHK	.08	8:55am
AIR BLK	.00	8:56am
SUB TEST	.00	8:57am
AIR BLK	.00	8:58am
SUB TEST	.00	9:00am
AIR BLK	.00	9:01am

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR

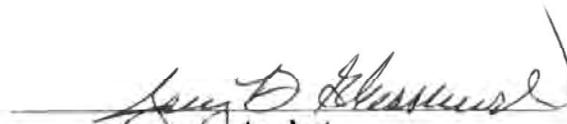
Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

MECKLENBURG COUNTY BAT MOBILE UNIT 8 590

Serial Number: 008929 Test Record Number: 1695
Test Date: 12/11/2025 Test Time: 9:03am EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	9:03am
FLO	Pass	9:03am
FC	Pass	9:03am

Temperature Tests

Test	Status	Time
FC1	Pass	9:03am
SRC	Pass	9:03am
DET	Pass	9:03am
BAR	Pass	9:03am
BT	Pass	9:03am

Blank Tests

Test	Status	Time
AIR	Pass	9:04am

Printer Tests

Test	Status	Time
PRNT	Pass	9:04am

CRC Tests

Test	Status	Time
COMP	Pass	9:04am
CAL	Pass	9:04am

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Moore Instrument Location BAT MOBILE UNIT 12

Instrument Serial No. 008601

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 20th day of December, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

083034
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

MORE COUNTY BAT MOBILE UNIT 12 620

Serial Number: 008601
Test Date: 12/20/2025

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name:
Crutchfield, Jr, Marshall B
Permit Number: 0008-3034
Effective:
07/01/2025-07/01/2027

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG501307
Exp Date: 01/13/2027

Test	g/210L	Time
DIAG	Pass	10:46pm
AIR BLK	.00	10:47pm
ACCY CHK	.08	10:48pm
AIR BLK	.00	10:49pm
SUB TEST	.00	10:50pm
AIR BLK	.00	10:50pm
SUB TEST	.00	10:52pm
AIR BLK	.00	10:53pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

Intox EC/IR-II: Preventive Maintenance

MORE COUNTY BAT MOBILE UNIT 12 620

Serial Number: 008601 Test Record Number: 1863
Test Date: 12/20/2025 Test Time: 10:53pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	10:54pm
FLO	Pass	10:54pm
FC	Pass	10:54pm

Temperature Tests

Test	Status	Time
FC1	Pass	10:54pm
SRC	Pass	10:54pm
DET	Pass	10:54pm
BAR	Pass	10:54pm
BT	Pass	10:54pm

Blank Tests

Test	Status	Time
AIR	Pass	10:55pm


Printer Tests

Test	Status	Time
PRNT	Pass	10:55pm

CRC Tests

Test	Status	Time
COMP	Pass	10:55pm
CAL	Pass	10:55pm

Preventive Maintenance
Status: *Pass*



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Moore Instrument Location BAT MOBILE UNIT 12

Instrument Serial No. 008698

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 20th day of December, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Signature of Certifying Official

083034
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

MOORE COUNTY BAT MOBILE UNIT 12 620

Serial Number: 008698
Test Date: 12/20/2025

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name:

Crutchfield, Jr, Marshall B

Permit Number: 0008-3034

Effective:

07/01/2025-07/01/2027

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG400303

Exp Date: 01/03/2026

Test	g/210L	Time
DIAG	Pass	11:11pm
AIR BLK	.00	11:12pm
ACCY CHK	.07	11:13pm
AIR BLK	.00	11:14pm
SUB TEST	.00	11:15pm
AIR BLK	.00	11:15pm
SUB TEST	.00	11:17pm
AIR BLK	.00	11:18pm

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR

Analyst

Intox EC/IR-II: Preventive Maintenance

MOORE COUNTY BAT MOBILE UNIT 12 620

Serial Number: 008698 Test Record Number: 2694
Test Date: 12/20/2025 Test Time: 11:20pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	11:20pm
FLO	Pass	11:20pm
FC	Pass	11:20pm

Temperature Tests

Test	Status	Time
FC1	Pass	11:20pm
SRC	Pass	11:20pm
DET	Pass	11:20pm
BAR	Pass	11:20pm
BT	Pass	11:20pm

Blank Tests

Test	Status	Time
AIR	Pass	11:21pm

Printer Tests

Test	Status	Time
PRNT	Pass	11:21pm

CRC Tests

Test	Status	Time
COMP	Pass	11:21pm
CAL	Pass	11:21pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County Moore Instrument Location BAT MOBILE UNIT 12

Instrument Serial No. 008788

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 20th day of December, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

083034
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

MOORE COUNTY BAT MOBILE UNIT 12 620

Serial Number: 008788
Test Date: 12/20/2025

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name:

Crutchfield, Jr, Marshall B

Permit Number: 0008-3034

Effective:

07/01/2025-07/01/2027

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG417802

Exp Date: 06/26/2026

Test	g/210L	Time
DIAG	Pass	11:04pm
AIR BLK	.00	11:06pm
ACCY CHK	.08	11:06pm
AIR BLK	.00	11:07pm
SUB TEST	.00	11:08pm
AIR BLK	.00	11:09pm
SUB TEST	.00	11:10pm
AIR BLK	.00	11:11pm

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR

Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

MOORE COUNTY BAT MOBILE UNIT 12 620

Serial Number: 008788 Test Record Number: 2494
Test Date: 12/20/2025 Test Time: 11:13pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	11:14pm
FLO	Pass	11:14pm
FC	Pass	11:14pm

Temperature Tests

Test	Status	Time
FC1	Pass	11:14pm
SRC	Pass	11:14pm
DET	Pass	11:14pm
BAR	Pass	11:14pm
BT	Pass	11:14pm

Blank Tests

Test	Status	Time
AIR	Pass	11:14pm

Printer Tests

Test	Status	Time
PRNT	Pass	11:14pm

CRC Tests

Test	Status	Time
COMP	Pass	11:15pm
CAL	Pass	11:15pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County NASH Instrument Location BAX MOBILE UNIT 12

Instrument Serial No. 008601

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 17th day of December, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.





Signature of Certifying Official

083034

Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

NASH COUNTY BAT MOBILE UNIT 12 630

Serial Number: 008601
Test Date: 12/17/2025

Citation Number: M0000000-0
Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name:

Crutchfield, Jr, Marshall B

Permit Number: 0008-3034

Effective:

07/01/2025-07/01/2027

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG501307

Exp Date: 01/13/2027

Test	g/210L	Time
DIAG	Pass	2:22pm
AIR BLK	.00	2:23pm
ACCY CHK	.08	2:23pm
AIR BLK	.00	2:24pm
SUB TEST	.00	2:25pm
AIR BLK	.00	2:26pm
SUB TEST	.00	2:27pm
AIR BLK	.00	2:28pm

Reported AC: *[Signature]* .00 g/210L

Signature of Chemical Analyst

Court CVR

[Signature]
Analyst

This form is used when performing Preventive Maintenance procedures

Forensic Tests for Alcohol Branch

Department of Health and Human Services

Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

NASH COUNTY BAT MOBILE UNIT 12 630

Serial Number: 008601 Test Record Number: 1861
Test Date: 12/17/2025 Test Time: 2:29pm EST

System Check: Passed

Baseline Tests

Test	Status	Time
IR	Pass	2:30pm
FLO	Pass	2:30pm
FC	Pass	2:30pm

Temperature Tests

Test	Status	Time
FC1	Pass	2:30pm
SRC	Pass	2:30pm
DET	Pass	2:30pm
BAR	Pass	2:30pm
BT	Pass	2:30pm

Blank Tests

Test	Status	Time
AIR	Pass	2:31pm

Printer Tests

Test	Status	Time
PRNT	Pass	2:31pm

CRC Tests

Test	Status	Time
COMP	Pass	2:31pm
CAL	Pass	2:31pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County NASH Instrument Location NASH COUNTY DETENTION CENTER
Instrument Serial No. 008630 222 S. WASHINGTON ST
NASHVILLE, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 19 day of DECEMBER, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

179707
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

NASH COUNTY NASH DETENTION CTR 630

Serial Number: 008630
Test Date: 12/19/2025

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Bryant, Earl A

Permit Number: 0017-9707

Effective:

02/01/2025-02/01/2027

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG534301

Exp Date: 12/09/2027


Test	g/210L	Time
DIAG	Pass	12:36pm
AIR BLK	.00	12:37pm
ACCY CHK	.08	12:37pm
AIR BLK	.00	12:38pm
SUB TEST	.00	12:39pm
AIR BLK	.00	12:40pm
SUB TEST	.00	12:41pm
AIR BLK	.00	12:42pm

Reported AC: .00 g/210L

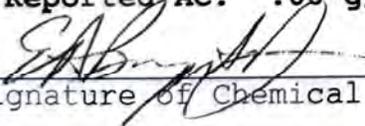

Signature of Chemical Analyst

Court CVR

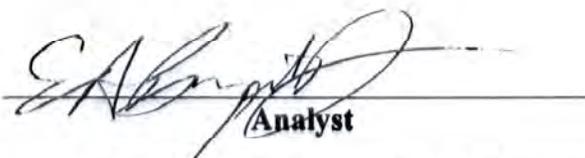

Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

NASH COUNTY NASH DETENTION CTR 630

Serial Number: 008630 Test Record Number: 6817
Test Date: 12/19/2025 Test Time: 12:43pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	12:43pm
FLO	Pass	12:43pm
FC	Pass	12:43pm

Temperature Tests

Test	Status	Time
FC1	Pass	12:43pm
SRC	Pass	12:43pm
DET	Pass	12:43pm
BAR	Pass	12:43pm
BT	Pass	12:43pm

Blank Tests

Test	Status	Time
AIR	Pass	12:44pm

Printer Tests

Test	Status	Time
PRNT	Pass	12:44pm

CRC Tests

Test	Status	Time
COMP	Pass	12:44pm
CAL	Pass	12:44pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County NASH Instrument Location BAT MOBILE UNIT 12
Instrument Serial No. 008698

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 17th day of December, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

083034
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

NASH COUNTY BAT MOBILE UNIT 12 630

Serial Number: 008698

Test Date: 12/17/2025

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name:

Crutchfield, Jr, Marshall B

Permit Number: 0008-3034

Effective:

07/01/2025-07/01/2027

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG400303

Exp Date: 01/03/2026

Test	g/210L	Time
DIAG	Pass	2:16pm
AIR BLK	.00	2:17pm
ACCY CHK	.07	2:18pm
AIR BLK	.00	2:19pm
SUB TEST	.00	2:19pm
AIR BLK	.00	2:20pm
SUB TEST	.00	2:22pm
AIR BLK	.00	2:23pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

This form is used when performing Preventive Maintenance procedures

Forensic Tests for Alcohol Branch

Department of Health and Human Services

Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

NASH COUNTY BAT MOBILE UNIT 12 630

Serial Number: 008698 Test Record Number: 2692
Test Date: 12/17/2025 Test Time: 2:26pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	2:26pm
FLO	Pass	2:26pm
FC	Pass	2:26pm

Temperature Tests

Test	Status	Time
FC1	Pass	2:26pm
SRC	Pass	2:26pm
DET	Pass	2:26pm
BAR	Pass	2:26pm
BT	Pass	2:26pm

Blank Tests

Test	Status	Time
AIR	Pass	2:27pm


Printer Tests

Test	Status	Time
PRNT	Pass	2:27pm

CRC Tests

Test	Status	Time
COMP	Pass	2:27pm
CAL	Pass	2:27pm

Preventive Maintenance
Status: Pass



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County NASH Instrument Location Rocky Mount PD
Instrument Serial No. 008740 330 S. CHURCH ST
Rocky Mount, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 19 day of DECEMBER, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

179707
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

NASH COUNTY ROCKY MOUNT PD 630

Serial Number: 008740
Test Date: 12/19/2025

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: Bryant, Earl A
Permit Number: 0017-9707
Effective:
02/01/2025-02/01/2027

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG534301
Exp Date: 12/09/2027


Test	g/210L	Time
DIAG	Pass	11:24am
AIR BLK	.00	11:24am
ACCY CHK	.07	11:25am
AIR BLK	.00	11:26am
SUB TEST	.00	11:27am
AIR BLK	.00	11:27am
SUB TEST	.00	11:29am
AIR BLK	.00	11:30am

Reported AC: .00 g/210L

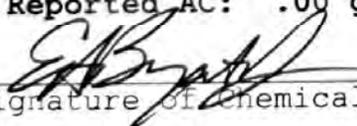

Signature of Chemical Analyst

Court CVR

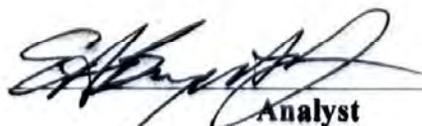

Analyst

Intox EC/IR-II: Preventive Maintenance

NASH COUNTY ROCKY MOUNT PD 630

Serial Number: 008740 Test Record Number: 1141
Test Date: 12/19/2025 Test Time: 11:31am EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	11:32am
FLO	Pass	11:32am
FC	Pass	11:32am

Temperature Tests

Test	Status	Time
FC1	Pass	11:32am
SRC	Pass	11:32am
DET	Pass	11:32am
BAR	Pass	11:32am
BT	Pass	11:32am

Blank Tests

Test	Status	Time
AIR	Pass	11:32am


Printer Tests

Test	Status	Time
PRNT	Pass	11:33am

CRC Tests

Test	Status	Time
COMP	Pass	11:33am
CAL	Pass	11:33am

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County NASH Instrument Location Rocky Mount PD
Instrument Serial No. 008741 330 S. CHURCH ST
Rocky Mount, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 19 day of DECEMBER, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



E. A. Boyd
Signature of Certifying Official

179707
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

NASH COUNTY ROCKY MOUNT PD 630

Serial Number: 008741
Test Date: 12/19/2025

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Bryant, Earl A

Permit Number: 0017-9707

Effective:

02/01/2025-02/01/2027

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG534301

Exp Date: 12/09/2027

Test	g/210L	Time
DIAG	Pass	11:25am
AIR BLK	.00	11:26am
ACCY CHK	.07	11:26am
AIR BLK	.00	11:28am
SUB TEST	.00	11:28am
AIR BLK	.00	11:29am
SUB TEST	.00	11:31am
AIR BLK	.00	11:31am

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

Intox EC/IR-II: Preventive Maintenance

NASH COUNTY ROCKY MOUNT PD 630

Serial Number: 008741 Test Record Number: 3303
Test Date: 12/19/2025 Test Time: 11:32am EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	11:33am
FLO	Pass	11:33am
FC	Pass	11:33am

Temperature Tests

Test	Status	Time
FC1	Pass	11:33am
SRC	Pass	11:33am
DET	Pass	11:33am
BAR	Pass	11:33am
BT	Pass	11:33am

Blank Tests

Test	Status	Time
AIR	Pass	11:33am

Printer Tests

Test	Status	Time
PRNT	Pass	11:33am

CRC Tests

Test	Status	Time
COMP	Pass	11:34am
CAL	Pass	11:34am

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County NASH Instrument Location BAT MOBILE UNIT 12

Instrument Serial No. 008788

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 12th day of December, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

083034
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

NASH COUNTY BAT MOBILE UNIT 12 630

Serial Number: 008788
Test Date: 12/17/2025


Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE

Analyst's Name:
Crutchfield, Jr, Marshall B
Permit Number: 0008-3034
Effective:
07/01/2025-07/01/2027

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG417802
Exp Date: 06/26/2026

Test	g/210L	Time
DIAG	Pass	2:35pm
AIR BLK	.00	2:36pm
ACCY CHK	.07	2:37pm
AIR BLK	.00	2:38pm
SUB TEST	.00	2:38pm
AIR BLK	.00	2:39pm
SUB TEST	.00	2:41pm
AIR BLK	.00	2:42pm

Reported AC:  .00 g/210L

Signature of Chemical Analyst

Court CVR


Analyst

Intox EC/IR-II: Preventive Maintenance

NASH COUNTY BAT MOBILE UNIT 12 630

Serial Number: 008788 Test Record Number: 2492
Test Date: 12/17/2025 Test Time: 2:43pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	2:43pm
FLO	Pass	2:43pm
FC	Pass	2:43pm

Temperature Tests

Test	Status	Time
FC1	Pass	2:44pm
SRC	Pass	2:44pm
DET	Pass	2:44pm
BAR	Pass	2:44pm
BT	Pass	2:44pm

Blank Tests

Test	Status	Time
AIR	Pass	2:44pm


Printer Tests

Test	Status	Time
PRNT	Pass	2:44pm

CRC Tests

Test	Status	Time
COMP	Pass	2:44pm
CAL	Pass	2:44pm

Preventive Maintenance
Status: Pass



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County NEW HANOVER Instrument Location NEW HANOVER COUNTY

Instrument Serial No. 008617 DETENTION CENTER

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 23 day of DECEMBER, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



John Ray Barnes
Signature of Certifying Official

146279
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

NEW HANOVER COUNTY DETENTION CENTER
640

Serial Number: 008617
Test Date: 12/23/2025

Citation Number: M0000000-0
Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: BARNES, ALVIN R

Permit Number: 0014-6279

Effective:

02/01/2025-02/01/2027

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG534301

Exp Date: 12/09/2027


Test	g/210L	Time
DIAG	Pass	1:43pm
AIR BLK	.00	1:44pm
ACCY CHK	.07	1:45pm
AIR BLK	.00	1:46pm
SUB TEST	.00	1:47pm
AIR BLK	.00	1:48pm
SUB TEST	.00	1:50pm
AIR BLK	.00	1:51pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

NEW HANOVER COUNTY DETENTION CENTER 640

Serial Number: 008617 Test Record Number: 5329
Test Date: 12/23/2025 Test Time: 1:51pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	1:51pm
FLO	Pass	1:51pm
FC	Pass	1:52pm

Temperature Tests

Test	Status	Time
FC1	Pass	1:52pm
SRC	Pass	1:52pm
DET	Pass	1:52pm
BAR	Pass	1:52pm
BT	Pass	1:52pm

Blank Tests

Test	Status	Time
AIR	Pass	1:52pm


Printer Tests

Test	Status	Time
PRNT	Pass	1:52pm

CRC Tests

Test	Status	Time
COMP	Pass	1:52pm
CAL	Pass	1:52pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County NEW HANOVER Instrument Location NEW HANOVER COUNTY
Instrument Serial No. 008626 DETENTION CENTER

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 23 day of DECEMBER, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Celan Ray Barnes

Signature of Certifying Official

146279

Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

NEW HANOVER COUNTY DETENTION CENTER
640

Serial Number: 008626
Test Date: 12/23/2025

Citation Number: M0000000-0
Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: BARNES, ALVIN R

Permit Number: 0014-6279

Effective:

02/01/2025-02/01/2027

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG534301

Exp Date: 12/09/2027


Test	g/210L	Time
DIAG	Pass	1:32pm
AIR BLK	.00	1:33pm
ACCY CHK	.07	1:33pm
AIR BLK	.00	1:35pm
SUB TEST	.00	1:35pm
AIR BLK	.00	1:36pm
SUB TEST	.00	1:38pm
AIR BLK	.00	1:39pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

NEW HANOVER COUNTY DETENTION CENTER 640

Serial Number: 008626 Test Record Number: 9142
Test Date: 12/23/2025 Test Time: 1:39pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	1:40pm
FLO	Pass	1:40pm
FC	Pass	1:40pm

Temperature Tests

Test	Status	Time
FC1	Pass	1:40pm
SRC	Pass	1:40pm
DET	Pass	1:40pm
BAR	Pass	1:40pm
BT	Pass	1:40pm

Blank Tests

Test	Status	Time
AIR	Pass	1:41pm


Printer Tests

Test	Status	Time
PRNT	Pass	1:41pm

CRC Tests

Test	Status	Time
COMP	Pass	1:41pm
CAL	Pass	1:41pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County New Hanover Instrument Location Wilmington
Instrument Serial No. 008628 Police Department

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 5th day of December, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

845023
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

NEW HANOVER COUNTY WILMINGTON PD 640

Serial Number: 008628
Test Date: 12/05/2025

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Ryan, Robert F

Permit Number: 0084-5023

Effective:

02/01/2025-02/01/2027

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG501307

Exp Date: 01/13/2027

Test	g/210L	Time
DIAG	Pass	4:30pm
AIR BLK	.00	4:31pm
ACCY CHK	.07	4:31pm
AIR BLK	.00	4:32pm
SUB TEST	.00	4:33pm
AIR BLK	.00	4:34pm
SUB TEST	.00	4:35pm
AIR BLK	.00	4:36pm

Reported AC: .00 g/210L

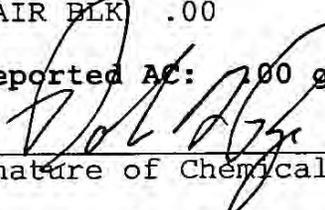

Signature of Chemical Analyst

Court CVR



Analyst

This form is used when performing Preventive Maintenance procedures

Forensic Tests for Alcohol Branch

Department of Health and Human Services

Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

NEW HANOVER COUNTY WILMINGTON PD 640

Serial Number: 008628 Test Record Number: 7367
Test Date: 12/05/2025 Test Time: 4:36pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	4:37pm
FLO	Pass	4:37pm
FC	Pass	4:37pm

Temperature Tests

Test	Status	Time
FC1	Pass	4:37pm
SRC	Pass	4:37pm
DET	Pass	4:37pm
BAR	Pass	4:37pm
BT	Pass	4:37pm

Blank Tests

Test	Status	Time
AIR	Pass	4:38pm

Printer Tests

Test	Status	Time
PRNT	Pass	4:38pm

CRC Tests

Test	Status	Time
COMP	Pass	4:38pm
CAL	Pass	4:38pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County NEW HANOVER Instrument Location CAROLINA BEACH
Instrument Serial No. 008661 POLICE DEPT

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 23 day of DECEMBER, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Alan Ry Bens

Signature of Certifying Official

146279

Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

NEW HANOVER COUNTY CAROLINA BEACH PD
640

Serial Number: 008661
Test Date: 12/23/2025

Citation Number: M0000000-0
Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: BARNES, ALVIN R

Permit Number: 0014-6279

Effective:

02/01/2025-02/01/2027

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG534301

Exp Date: 12/09/2027


Test	g/210L	Time
DIAG	Pass	3:44pm
AIR BLK	.00	3:45pm
ACCY CHK	.08	3:45pm
AIR BLK	.00	3:47pm
SUB TEST	.00	3:47pm
AIR BLK	.00	3:48pm
SUB TEST	.00	3:50pm
AIR BLK	.00	3:50pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR


Analyst

Intox EC/IR-II: Preventive Maintenance

NEW HANOVER COUNTY CAROLINA BEACH PD 640

Serial Number: 008661 Test Record Number: 3494
Test Date: 12/23/2025 Test Time: 3:50pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	3:51pm
FLO	Pass	3:51pm
FC	Pass	3:51pm

Temperature Tests

Test	Status	Time
FC1	Pass	3:51pm
SRC	Pass	3:51pm
DET	Pass	3:51pm
BAR	Pass	3:51pm
BT	Pass	3:51pm

Blank Tests

Test	Status	Time
AIR	Pass	3:52pm


Printer Tests

Test	Status	Time
PRNT	Pass	3:52pm

CRC Tests

Test	Status	Time
COMP	Pass	3:52pm
CAL	Pass	3:52pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County NEW HANOVER Instrument Location WRIGHTSVILLE BEACH
Instrument Serial No. 008667 POLICE DEPT

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 23 day of DECEMBER, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Alan R. Burns

Signature of Certifying Official

146279

Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

NEW HANOVER COUNTY WRIGHTSVILLE BCH PD
640

Serial Number: 008667
Test Date: 12/23/2025

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: BARNES, ALVIN R
Permit Number: 0014-6279
Effective:
02/01/2025-02/01/2027

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG534301
Exp Date: 12/09/2027


Test	g/210L	Time
DIAG	Pass	5:07pm
AIR BLK	.00	5:08pm
ACCY CHK	.08	5:08pm
AIR BLK	.00	5:10pm
SUB TEST	.00	5:10pm
AIR BLK	.00	5:11pm
SUB TEST	.00	5:13pm
AIR BLK	.00	5:13pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

NEW HANOVER COUNTY WRIGHTSVILLE BCH PD 640

Serial Number: 008667 Test Record Number: 3055
Test Date: 12/23/2025 Test Time: 5:14pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	5:14pm
FLO	Pass	5:14pm
FC	Pass	5:14pm

Temperature Tests

Test	Status	Time
FC1	Pass	5:14pm
SRC	Pass	5:14pm
DET	Pass	5:14pm
BAR	Pass	5:14pm
BT	Pass	5:14pm

Blank Tests

Test	Status	Time
AIR	Pass	5:15pm


Printer Tests

Test	Status	Time
PRNT	Pass	5:15pm

CRC Tests

Test	Status	Time
COMP	Pass	5:15pm
CAL	Pass	5:15pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County New Hanover Instrument Location BAT Mobile Unit 13
Instrument Serial No. 008869

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 31 day of December, 20 25 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Tim B. White
Signature of Certifying Official

307699
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

NEW HANOVER COUNTY BAT MOBILE UNIT 13
640

Serial Number: 008869
Test Date: 12/31/2025

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Whitehurst, Timothy B

Permit Number: 0030-7699

Effective:

04/01/2025-04/01/2027

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG417803

Exp Date: 06/26/2026


Test	g/210L	Time
DIAG	Pass	9:59pm
AIR BLK	.00	10:00pm
ACCY CHK	.08	10:01pm
AIR BLK	.00	10:02pm
SUB TEST	.00	10:02pm
AIR BLK	.00	10:03pm
SUB TEST	.00	10:05pm
AIR BLK	.00	10:05pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

Intox EC/IR-II: Preventive Maintenance

NEW HANOVER COUNTY BAT MOBILE UNIT 13 640

Serial Number: 008869 Test Record Number: 2145
Test Date: 12/31/2025 Test Time: 10:06pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	10:06pm
FLO	Pass	10:06pm
FC	Pass	10:06pm

Temperature Tests

Test	Status	Time
FC1	Pass	10:07pm
SRC	Pass	10:07pm
DET	Pass	10:07pm
BAR	Pass	10:07pm
BT	Pass	10:07pm

Blank Tests

Test	Status	Time
AIR	Pass	10:07pm


Printer Tests

Test	Status	Time
PRNT	Pass	10:07pm

CRC Tests

Test	Status	Time
COMP	Pass	10:07pm
CAL	Pass	10:07pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County New Hanover Instrument Location BAT Mobile Unit 13
Instrument Serial No. 008898

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 31 day of December, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Timothy B. White
Signature of Certifying Official

307699
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

NEW HANOVER COUNTY BAT MOBILE UNIT 13
640

Serial Number: 008898
Test Date: 12/31/2025

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Whitehurst, Timothy B

Permit Number: 0030-7699

Effective:

04/01/2025-04/01/2027

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG506302

Exp Date: 03/04/2027

Test	g/210L	Time
DIAG	Pass	10:42pm
AIR BLK	.00	10:43pm
ACCY CHK	.07	10:44pm
AIR BLK	.00	10:45pm
SUB TEST	.00	10:45pm
AIR BLK	.00	10:46pm
SUB TEST	.00	10:48pm
AIR BLK	.00	10:49pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

NEW HANOVER COUNTY BAT MOBILE UNIT 13 640

Serial Number: 008898 Test Record Number: 2093
Test Date: 12/31/2025 Test Time: 10:49pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	10:49pm
FLO	Pass	10:49pm
FC	Pass	10:49pm

Temperature Tests

Test	Status	Time
FC1	Pass	10:50pm
SRC	Pass	10:50pm
DET	Pass	10:50pm
BAR	Pass	10:50pm
BT	Pass	10:50pm

Blank Tests

Test	Status	Time
AIR	Pass	10:50pm


Printer Tests

Test	Status	Time
PRNT	Pass	10:50pm

CRC Tests

Test	Status	Time
COMP	Pass	10:50pm
CAL	Pass	10:50pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County New Hanover Instrument Location BAT Mobile Unit 13
Instrument Serial No. 008939

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 31 day of December, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Tim B. White
Signature of Certifying Official

307699
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

NEW HANOVER COUNTY BAT MOBILE UNIT 13
640

Serial Number: 008939
Test Date: 12/31/2025

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Whitehurst, Timothy B

Permit Number: 0030-7699

Effective:

04/01/2025-04/01/2027

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG506302

Exp Date: 03/04/2027

Test	g/210L	Time
DIAG	Pass	9:53pm
AIR BLK	.00	9:54pm
ACCY CHK	.07	9:55pm
AIR BLK	.00	9:55pm
SUB TEST	.00	9:56pm
AIR BLK	.00	9:57pm
SUB TEST	.00	9:58pm
AIR BLK	.00	9:59pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

Intox EC/IR-II: Preventive Maintenance

NEW HANOVER COUNTY BAT MOBILE UNIT 13 640

Serial Number: 008939 Test Record Number: 1962
Test Date: 12/31/2025 Test Time: 10:00pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	10:01pm
FLO	Pass	10:01pm
FC	Pass	10:01pm

Temperature Tests

Test	Status	Time
FC1	Pass	10:01pm
SRC	Pass	10:01pm
DET	Pass	10:01pm
BAR	Pass	10:01pm
BT	Pass	10:01pm

Blank Tests

Test	Status	Time
AIR	Pass	10:02pm


Printer Tests

Test	Status	Time
PRNT	Pass	10:02pm

CRC Tests

Test	Status	Time
COMP	Pass	10:02pm
CAL	Pass	10:02pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County Onslow Instrument Location BAT Mobile Unit 7

Instrument Serial No. 008002

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 16th day of December, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



A handwritten signature in black ink, consisting of a large, stylized initial 'A' followed by several horizontal strokes.

Signature of Certifying Official

2266313
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

ONslow COUNTY BAT MOBILE UNIT 7 660

Serial Number: 008002
Test Date: 12/18/2025

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Sharpe Jr., Robert J

Permit Number: 1820-8591

Effective:

02/01/2025-02/01/2027

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG506303

Exp Date: 03/04/2027


Test	g/210L	Time
DIAG	Pass	1:28pm
AIR BLK	.00	1:29pm
ACCY CHK	.08	1:30pm
AIR BLK	.00	1:31pm
SUB TEST	.00	1:31pm
AIR BLK	.00	1:32pm
SUB TEST	.00	1:34pm
AIR BLK	.00	1:35pm

Reported AC: 00 g/210L



Signature of Chemical Analyst

Court CVR

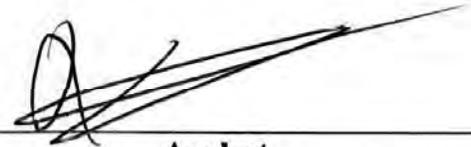

Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

ONslow COUNTY BAT MOBILE UNIT 7 660

Serial Number: 008002 Test Record Number: 852
Test Date: 12/18/2025 Test Time: 1:36pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	1:36pm
FLO	Pass	1:36pm
FC	Pass	1:36pm

Temperature Tests

Test	Status	Time
FC1	Pass	1:37pm
SRC	Pass	1:37pm
DET	Pass	1:37pm
BAR	Pass	1:37pm
BT	Pass	1:37pm

Blank Tests

Test	Status	Time
AIR	Pass	1:37pm

Printer Tests

Test	Status	Time
PRNT	Pass	1:37pm

CRC Tests

Test	Status	Time
COMP	Pass	1:37pm
CAL	Pass	1:37pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County ONSLow Instrument Location BAT MOBILE UNIT 12

Instrument Serial No. 008601

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 31st day of December, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

083034
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

ONslow COUNTY BAT MOBILE UNIT 12 660

Serial Number: 008601
Test Date: 12/31/2025

Citation Number: M0000000-0
Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name:

Crutchfield, Jr, Marshall B

Permit Number: 0008-3034

Effective:

07/01/2025-07/01/2027

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG501307

Exp Date: 01/13/2027

Test	g/210L	Time
DIAG	Pass	10:42pm
AIR BLK	.00	10:43pm
ACCY CHK	.08	10:44pm
AIR BLK	.00	10:45pm
SUB TEST	.00	10:45pm
AIR BLK	.00	10:46pm
SUB TEST	.00	10:48pm
AIR BLK	.00	10:49pm

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR

Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

ONslow COUNTY BAT MOBILE UNIT 12 660

Serial Number: 008601 Test Record Number: 1865
Test Date: 12/31/2025 Test Time: 10:52pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	10:52pm
FLO	Pass	10:52pm
FC	Pass	10:52pm

Temperature Tests

Test	Status	Time
FC1	Pass	10:52pm
SRC	Pass	10:52pm
DET	Pass	10:52pm
BAR	Pass	10:52pm
BT	Pass	10:52pm

Blank Tests

Test	Status	Time
AIR	Pass	10:53pm

Printer Tests

Test	Status	Time
PRNT	Pass	10:53pm

CRC Tests

Test	Status	Time
COMP	Pass	10:53pm
CAL	Pass	10:53pm

Preventive Maintenance
Status: Pass



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County DANLOW Instrument Location IBAT MOBILE UNIT 12

Instrument Serial No. 008698

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 31st day of December, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

083034
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

JANESBORO COUNTY BAT MOBILE UNIT 12 660

Serial Number: 008698
Test Date: 12/29/2025

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name:

Critchfield, Jr, Marshall B

Permit Number: 0008-3034

Effective:

07/01/2025-07/01/2027

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG400303

Exp Date: 01/03/2026

Test	g/210L	Time
DIAG	Pass	10:42pm
AIR BLK	.00	10:43pm
ACTY CHK	.07	10:44pm
AIF BLK	.00	10:45pm
SUB TEST	.00	10:45pm
AIF BLK	.00	10:46pm
SUB TEST	.00	10:48pm
AIR BLK	.00	10:49pm

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR


Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

ONslow COUNTY BAT MOBILE UNIT 12 660

Serial Number: 008698 Test Record Number: 2696
Test Date: 12/29/2025 Test Time: 10:50pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	10:51pm
FLO	Pass	10:51pm
FC	Pass	10:51pm

Temperature Tests

Test	Status	Time
FC1	Pass	10:51pm
SRC	Pass	10:51pm
DET	Pass	10:51pm
BAR	Pass	10:51pm
BT	Pass	10:51pm

Blank Tests

Test	Status	Time
AIR	Pass	10:52pm

Printer Tests

Test	Status	Time
PRNT	Pass	10:52pm

CRC Tests

Test	Status	Time
COMP	Pass	10:52pm
CAL	Pass	10:52pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Onglow Instrument Location BAT MOBILE UNIT 12
Instrument Serial No. 008788

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 31st day of December, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Handwritten Signature]

Signature of Certifying Official

083034

Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

ONslow COUNTY BAT MOBILE UNIT 12 660

Serial Number: 008788
Test Date: 12/31/2025

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name:

Crutchfield, Jr, Marshall B

Permit Number: 0008-3034

Effective:

07/01/2025-07/01/2027

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG417802

Exp Date: 06/26/2026

Test	g/210L	Time
DIAG	Pass	10:53pm
AIR BLK	.00	10:54pm
ACCY CHK	.08	10:55pm
AIR BLK	.00	10:56pm
SUB TEST	.00	10:56pm
AIR BLK	.00	10:57pm
SUB TEST	.00	10:59pm
AIR BLK	.00	11:00pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

ONslow COUNTY BAT MOBILE UNIT 12 660

Serial Number: 008788 Test Record Number: 2496
Test Date: 12/31/2025 Test Time: 11:01pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	11:02pm
FLO	Pass	11:02pm
FC	Pass	11:02pm

Temperature Tests

Test	Status	Time
FC1	Pass	11:02pm
SRC	Pass	11:02pm
DET	Pass	11:02pm
BAR	Pass	11:02pm
BT	Pass	11:02pm

Blank Tests

Test	Status	Time
AIR	Pass	11:02pm

Printer Tests

Test	Status	Time
PRNT	Pass	11:03pm

CRC Tests

Test	Status	Time
COMP	Pass	11:03pm
CAL	Pass	11:03pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County ONSLow Instrument Location ONSLow COUNTY
Instrument Serial No. 008931 DETENTION CENTER

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 11th day of DECEMBER, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

2824950

Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

ONslow COUNTY DETENTION CENTER 660

Serial Number: 008931
Test Date: 12/11/2025

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: GILLESPIE, PENTTI W

Permit Number: 9523-2149

Effective:

02/01/2025-02/01/2027

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG501307


Exp Date: 01/13/2027

Test	g/210L	Time
DIAG	Pass	12:11pm
AIR BLK	.00	12:11pm
ACCY CHK	.07	12:12pm
AIR BLK	.00	12:13pm
SUB TEST	.00	12:14pm
AIR BLK	.00	12:14pm
SUB TEST	.00	12:16pm
AIR BLK	.00	12:17pm

Reported AC: 00 g/210L

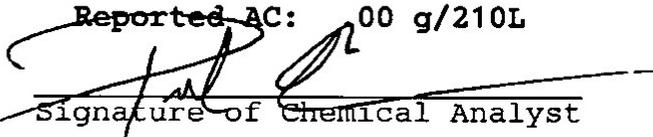
Signature of Chemical Analyst

Court CVR

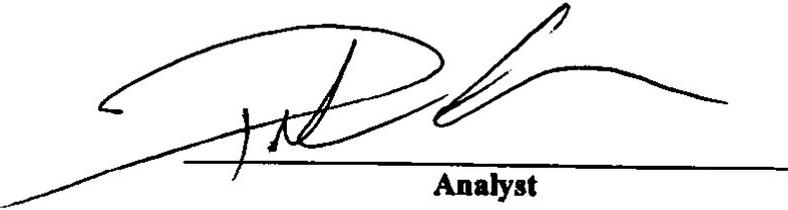
Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

ONSLOW COUNTY DETENTION CENTER 660

Serial Number: 008931 Test Record Number: 5516
Test Date: 12/11/2025 Test Time: 12:17pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	12:17pm
FLO	Pass	12:17pm
FC	Pass	12:17pm

Temperature Tests

Test	Status	Time
FC1	Pass	12:17pm
SRC	Pass	12:17pm
DET	Pass	12:17pm
BAR	Pass	12:17pm
BT	Pass	12:17pm

Blank Tests

Test	Status	Time
AIR	Pass	12:18pm

Printer Tests

Test	Status	Time
PRNT	Pass	12:18pm

CRC Tests

Test	Status	Time
COMP	Pass	12:18pm
CAL	Pass	12:18pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Onslow Instrument Location BAT Mobile Unit 7

Instrument Serial No. 0089168

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 18th day of December, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

2266313
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

ONslow COUNTY BAT MOBILE UNIT 7 660

Serial Number: 008968
Test Date: 12/18/2025

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE

Analyst's Name: Sharpe Jr., Robert J
Permit Number: 1820-8591
Effective:
02/01/2025-02/01/2027

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG506303
Exp Date: 03/04/2027

Test	g/210L	Time
DIAG	Pass	1:28pm
AIR BLK	.00	1:29pm
ACCY CHK	.08	1:30pm
AIR BLK	.00	1:31pm
SUB TEST	.00	1:31pm
AIR BLK	.00	1:32pm
SUB TEST	.00	1:34pm
AIR BLK	.00	1:35pm

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

ONSLOW COUNTY BAT MOBILE UNIT 7 660

Serial Number: 008968 Test Record Number: 422
Test Date: 12/18/2025 Test Time: 1:37pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	1:38pm
FLO	Pass	1:38pm
FC	Pass	1:38pm

Temperature Tests

Test	Status	Time
FC1	Pass	1:38pm
SRC	Pass	1:38pm
DET	Pass	1:38pm
BAR	Pass	1:38pm
BT	Pass	1:38pm

Blank Tests

Test	Status	Time
AIR	Pass	1:39pm

Printer Tests

Test	Status	Time
PRNT	Pass	1:39pm

CRC Tests

Test	Status	Time
COMP	Pass	1:39pm
CAL	Pass	1:39pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Onslow Instrument Location BAT Mobile Unit 7

Instrument Serial No. 008971

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 18th day of December, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

2266313
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

ONSLOW COUNTY BAT MOBILE UNIT 7 660

Serial Number: 008971

Test Date: 12/18/2025

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Sharpe Jr., Robert J

Permit Number: 1820-8591

Effective:

02/01/2025-02/01/2027

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG506302

Exp Date: 03/04/2027

Test	g/210L	Time
DIAG	Pass	1:28pm
AIR BLK	.00	1:29pm
ACCY CHK	.08	1:29pm
AIR BLK	.00	1:30pm
SUB TEST	.00	1:31pm
AIR BLK	.00	1:31pm
SUB TEST	.00	1:34pm
AIR BLK	.00	1:35pm

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR

Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

ONslow COUNTY BAT MOBILE UNIT 7 660

Serial Number: 008971 Test Record Number: 372
Test Date: 12/18/2025 Test Time: 1:37pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	1:37pm
FLO	Pass	1:37pm
FC	Pass	1:37pm

Temperature Tests

Test	Status	Time
FC1	Pass	1:38pm
SRC	Pass	1:38pm
DET	Pass	1:38pm
BAR	Pass	1:38pm
BT	Pass	1:38pm

Blank Tests

Test	Status	Time
AIR	Pass	1:38pm

Printer Tests

Test	Status	Time
PRNT	Pass	1:38pm

CRC Tests

Test	Status	Time
COMP	Pass	1:38pm
CAL	Pass	1:38pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Onslow Instrument Location BAT Mobile Unit 7
Instrument Serial No. 008972

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 18th day of December, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

2266313
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

ONSLOW COUNTY BAT MOBILE UNIT 7 660

Serial Number: 008972
Test Date: 12/18/2025

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Sharpe Jr., Robert J

Permit Number: 1820-8591

Effective:

02/01/2025-02/01/2027

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG506303

Exp Date: 03/04/2027

Test	g/210L	Time
DIAG	Pass	1:27pm
AIR BLK	.00	1:28pm
ACCY CHK	.08	1:28pm
AIR BLK	.00	1:29pm
SUB TEST	.00	1:30pm
AIR BLK	.00	1:31pm
SUB TEST	.00	1:33pm
AIR BLK	.00	1:34pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

ONSLOW COUNTY BAT MOBILE UNIT 7 660

Serial Number: 008972 Test Record Number: 432
Test Date: 12/18/2025 Test Time: 1:35pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	1:35pm
FLO	Pass	1:35pm
FC	Pass	1:35pm

Temperature Tests

Test	Status	Time
FC1	Pass	1:35pm
SRC	Pass	1:35pm
DET	Pass	1:35pm
BAR	Pass	1:35pm
BT	Pass	1:35pm

Blank Tests

Test	Status	Time
AIR	Pass	1:36pm

Printer Tests

Test	Status	Time
PRNT	Pass	1:36pm

CRC Tests

Test	Status	Time
COMP	Pass	1:36pm
CAL	Pass	1:36pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County Pasquotank Instrument Location Elizabeth City P.D.
Instrument Serial No. 008941 305 E. Main St.
Elizabeth City, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 18th day of December, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

206272
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

PASQUOTANK COUNTY ELIZABETH CITY PD
690

Serial Number: 008941
Test Date: 12/18/2025

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: Chappell, Mark A
Permit Number: 0020-6272
Effective:
02/01/2025-02/01/2027

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test


Lot Number: AG516203
Exp Date: 06/11/2027

Test	g/210L	Time
DIAG	Pass	10:08am
AIR BLK	.00	10:09am
ACCY CHK	.08	10:10am
AIR BLK	.00	10:11am
SUB TEST	.00	10:12am
AIR BLK	.00	10:13am
SUB TEST	.00	10:15am
AIR BLK	.00	10:16am

Reported AC: .00 g/210L

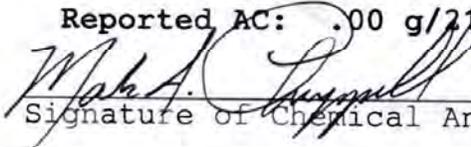
Signature of Chemical Analyst

Court CVR

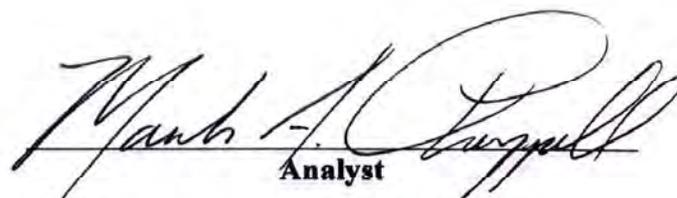
Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

PASQUOTANK COUNTY ELIZABETH CITY PD 690

Serial Number: 008941 Test Record Number: 1770
Test Date: 12/18/2025 Test Time: 10:18am EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	10:18am
FLO	Pass	10:18am
FC	Pass	10:18am

Temperature Tests

Test	Status	Time
FC1	Pass	10:18am
SRC	Pass	10:18am
DET	Pass	10:18am
BAR	Pass	10:18am
BT	Pass	10:18am

Blank Tests

Test	Status	Time
AIR	Pass	10:19am

Printer Tests

Test	Status	Time
PRNT	Pass	10:19am

CRC Tests

Test	Status	Time
COMP	Pass	10:19am
CAL	Pass	10:19am

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Pender Instrument Location BAT Mobile Unit 7

Instrument Serial No 008002

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 19th day of December, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

2266313
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

PENDER COUNTY BAT MOBILE UNIT 7 700

Serial Number: 008002
Test Date: 12/19/2025

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Sharpe Jr., Robert J

Permit Number: 1820-8591

Effective:

02/01/2025-02/01/2027

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG506303

Exp Date: 03/04/2027

Test	g/210L	Time
DIAG	Pass	6:02pm
AIR BLK	.00	6:03pm
ACCY CHK	.08	6:03pm
AIR BLK	.00	6:04pm
SUB TEST	.00	6:05pm
AIR BLK	.00	6:06pm
SUB TEST	.00	6:07pm
AIR BLK	.00	6:08pm

Reported AC: ~~.00 g/210L~~

Signature of Chemical Analyst

Court CVR



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

PENDER COUNTY BAT MOBILE UNIT 7 700

Serial Number: 008002 Test Record Number: 854
Test Date: 12/19/2025 Test Time: 6:09pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	6:09pm
FLO	Pass	6:09pm
FC	Pass	6:10pm

Temperature Tests

Test	Status	Time
FC1	Pass	6:10pm
SRC	Pass	6:10pm
DET	Pass	6:10pm
BAR	Pass	6:10pm
BT	Pass	6:10pm

Blank Tests

Test	Status	Time
AIR	Pass	6:10pm

Printer Tests

Test	Status	Time
PRNT	Pass	6:10pm

CRC Tests

Test	Status	Time
COMP	Pass	6:11pm
CAL	Pass	6:11pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County PENDER Instrument Location PENDER COUNTY
Instrument Serial No. 008935 DETENTION CENTER

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 23 day of DECEMBER, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Alan R. Burns
Signature of Certifying Official

146279
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

PENDER COUNTY DETENTION CENTER 700

Serial Number: 008935
Test Date: 12/23/2025

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: BARNES, ALVIN R
Permit Number: 0014-6279
Effective:
02/01/2025-02/01/2027

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG534301
Exp Date: 12/09/2027


Test	g/210L	Time
DIAG	Pass	11:05am
AIR BLK	.00	11:06am
ACCY CHK	.08	11:06am
AIR BLK	.00	11:08am
SUB TEST	.00	11:08am
AIR BLK	.00	11:09am
SUB TEST	.00	11:11am
AIR BLK	.00	11:12am

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

Intox EC/IR-II: Preventive Maintenance

PENDER COUNTY DETENTION CENTER 700

Serial Number: 008935 Test Record Number: 3822
Test Date: 12/23/2025 Test Time: 11:12am EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	11:13am
FLO	Pass	11:13am
FC	Pass	11:13am

Temperature Tests

Test	Status	Time
FC1	Pass	11:13am
SRC	Pass	11:13am
DET	Pass	11:13am
BAR	Pass	11:13am
BT	Pass	11:13am

Blank Tests

Test	Status	Time
AIR	Pass	11:14am


Printer Tests

Test	Status	Time
PRNT	Pass	11:14am

CRC Tests

Test	Status	Time
COMP	Pass	11:14am
CAL	Pass	11:14am

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County PENDER Instrument Location PENDER COUNTY
Instrument Serial No. 008948 GOVERNMENT ANNEX

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 29th day of DECEMBER, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Handwritten Signature]

Signature of Certifying Official

2824950

Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

PENDER COUNTY GOVERNMENT ANNEX 700

Serial Number: 008948

Test Date: 12/29/2025

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: GILLESPIE, PENTTI W

Permit Number: 9523-2149

Effective:

02/01/2025-02/01/2027

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG534301

Exp Date: 12/09/2027


Test	g/210L	Time
DIAG	Pass	11:36am
AIR BLK	.00	11:37am
ACCY CHK	.07	11:37am
AIR BLK	.00	11:38am
SUB TEST	.00	11:39am
AIR BLK	.00	11:40am
SUB TEST	.00	11:41am
AIR BLK	.00	11:42am

Reported AC: .00 g/210L

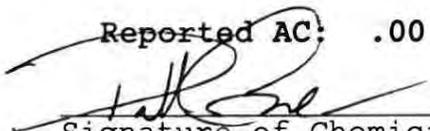

Signature of Chemical Analyst

Court CVR

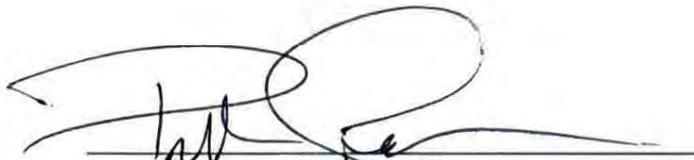

Analyst

Intox EC/IR-II: Preventive Maintenance

PENDER COUNTY GOVERNMENT ANNEX 700

Serial Number: 008948 Test Record Number: 1635
Test Date: 12/29/2025 Test Time: 11:42am EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	11:43am
FLO	Pass	11:43am
FC	Pass	11:43am

Temperature Tests

Test	Status	Time
FC1	Pass	11:43am
SRC	Pass	11:43am
DET	Pass	11:43am
BAR	Pass	11:43am
BT	Pass	11:43am

Blank Tests

Test	Status	Time
AIR	Pass	11:44am


Printer Tests

Test	Status	Time
PRNT	Pass	11:44am

CRC Tests

Test	Status	Time
COMP	Pass	11:44am
CAL	Pass	11:44am

Preventive Maintenance
Status: Pass

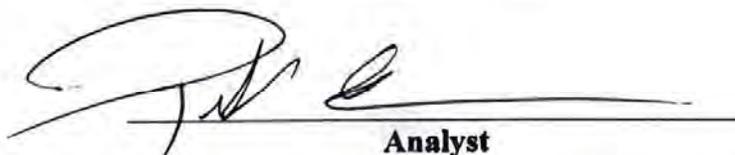
Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County Pender Instrument Location BAT Mobile Unit 7

Instrument Serial No. 008971

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 19th day of December, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

2266313
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

PENDER COUNTY BAT MOBILE UNIT 7 700

Serial Number: 008971
Test Date: 12/19/2025

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: Sharpe Jr., Robert J
Permit Number: 1820-8591
Effective:
02/01/2025-02/01/2027

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG506302
Exp Date: 03/04/2027


Test	g/210L	Time
DIAG	Pass	6:01pm
AIR BLK	.00	6:02pm
ACCY CHK	.08	6:03pm
AIR BLK	.00	6:04pm
SUB TEST	.00	6:04pm
AIR BLK	.00	6:05pm
SUB TEST	.00	6:07pm
AIR BLK	.00	6:08pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR

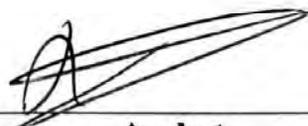

Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

PENDER COUNTY BAT MOBILE UNIT 7 700

Serial Number: 008971 Test Record Number: 374
Test Date: 12/19/2025 Test Time: 6:09pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	6:09pm
FLO	Pass	6:09pm
FC	Pass	6:09pm

Temperature Tests

Test	Status	Time
FC1	Pass	6:10pm
SRC	Pass	6:10pm
DET	Pass	6:10pm
BAR	Pass	6:10pm
BT	Pass	6:10pm

Blank Tests

Test	Status	Time
AIR	Pass	6:10pm


Printer Tests

Test	Status	Time
PRNT	Pass	6:10pm

CRC Tests

Test	Status	Time
COMP	Pass	6:10pm
CAL	Pass	6:10pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Pender Instrument Location BAT Mobile Unit 7

Instrument Serial No. 008972

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 19th day of December, 20 25 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

2266313
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

PENDER COUNTY BAT MOBILE UNIT 7 700

Serial Number: 008972
Test Date: 12/19/2025

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Sharpe Jr., Robert J

Permit Number: 1820-8591

Effective:

02/01/2025-02/01/2027

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG506303

Exp Date: 03/04/2027

Test	g/210L	Time
DIAG	Pass	6:00pm
AIR BLK	.00	6:01pm
ACCY CHK	.08	6:02pm
AIR BLK	.00	6:03pm
SUB TEST	.00	6:04pm
AIR BLK	.00	6:05pm
SUB TEST	.00	6:06pm
AIR BLK	.00	6:07pm

Reported AC: ~~.00~~ g/210L



Signature of Chemical Analyst

Court CVR



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

PENDER COUNTY BAT MOBILE UNIT 7 700

Serial Number: 008972 Test Record Number: 434
Test Date: 12/19/2025 Test Time: 6:08pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	6:08pm
FLO	Pass	6:08pm
FC	Pass	6:09pm

Temperature Tests

Test	Status	Time
FC1	Pass	6:09pm
SRC	Pass	6:09pm
DET	Pass	6:09pm
BAR	Pass	6:09pm
BT	Pass	6:09pm

Blank Tests

Test	Status	Time
AIR	Pass	6:09pm


Printer Tests

Test	Status	Time
PRNT	Pass	6:09pm

CRC Tests

Test	Status	Time
COMP	Pass	6:10pm
CAL	Pass	6:10pm

Preventive Maintenance
Status: Pass

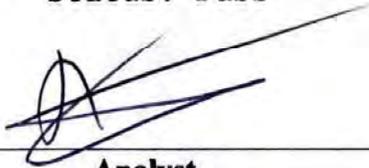

Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County Person Instrument Location Roxboro PD
Instrument Serial No. 008880 109 N. Lamar St
Roxboro, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 17 day of December, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Sum Stokes Brewer
Signature of Certifying Official

146221
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

PERSON COUNTY ROXBORO POLICE DEPT 720

Serial Number: 008880

Test Date: 12/17/2025

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Barnes, Simon S

Permit Number: 0014-6221

Effective:

02/01/2025-02/01/2027

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG516203

Exp Date: 06/11/2027

Test	g/210L	Time
DIAG	Pass	2:33pm
AIR BLK	.00	2:33pm
ACCY CHK	.08	2:34pm
AIR BLK	.00	2:35pm
SUB TEST	.00	2:36pm
AIR BLK	.00	2:37pm
SUB TEST	.00	2:38pm
AIR BLK	.00	2:39pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

PERSON COUNTY ROXBORO POLICE DEPT 720

Serial Number: 008880 Test Record Number: 2556
Test Date: 12/17/2025 Test Time: 2:40pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	2:40pm
FLO	Pass	2:40pm
FC	Pass	2:40pm

Temperature Tests

Test	Status	Time
FC1	Pass	2:40pm
SRC	Pass	2:40pm
DET	Pass	2:40pm
BAR	Pass	2:40pm
BT	Pass	2:40pm

Blank Tests

Test	Status	Time
AIR	Pass	2:41pm

Printer Tests

Test	Status	Time
PRNT	Pass	2:41pm

CRC Tests

Test	Status	Time
COMP	Pass	2:41pm
CAL	Pass	2:41pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Pitt Instrument Location Agden P.D.
Instrument Serial No. 008666 4144 West Ave., Agden, N.C.

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 22nd day of December, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Key P...
Signature of Certifying Official

377722
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

PITT COUNTY AYDEN PD 730

Serial Number: 008666
Test Date: 12/22/2025

Citation Number: M0000000-0
Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Gray, Kelly D

Permit Number: 0037-7722

Effective:

02/01/2025-02/01/2027

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG431003

Exp Date: 11/05/2026

Test	g/210L	Time
DIAG	Pass	9:15am
AIR BLK	.00	9:16am
ACCY CHK	.07	9:17am
AIR BLK	.00	9:18am
SUB TEST	.00	9:18am
AIR BLK	.00	9:19am
SUB TEST	.00	9:21am
AIR BLK	.00	9:22am

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

Intox EC/IR-II: Preventive Maintenance

PITT COUNTY AYDEN PD 730

Serial Number: 008666 Test Record Number: 1653
Test Date: 12/22/2025 Test Time: 9:23am EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	9:23am
FLO	Pass	9:23am
FC	Pass	9:23am

Temperature Tests

Test	Status	Time
FC1	Pass	9:23am
SRC	Pass	9:23am
DET	Pass	9:23am
BAR	Pass	9:23am
BT	Pass	9:23am

Blank Tests

Test	Status	Time
AIR	Pass	9:24am


Printer Tests

Test	Status	Time
PRNT	Pass	9:24am

CRC Tests

Test	Status	Time
COMP	Pass	9:24am
CAL	Pass	9:24am

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Pitt Instrument Location Pitt Co Detention Center
Instrument Serial No. 008668 124 New Hope Rd., Greenville, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 22nd day of December, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

377722
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

PITT COUNTY PITT CO DETENTION 730

Serial Number: 008668
Test Date: 12/22/2025

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Gray, Kelly D

Permit Number: 0037-7722

Effective:

02/01/2025-02/01/2027

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG506303

Exp Date: 03/04/2027

Test	g/210L	Time
DIAG	Pass	10:44am
AIR BLK	.00	10:44am
ACCY CHK	.07	10:45am
AIR BLK	.00	10:46am
SUB TEST	.00	10:47am
AIR BLK	.00	10:48am
SUB TEST	.00	10:49am
AIR BLK	.00	10:50am

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

PITT COUNTY PITT CO DETENTION 730

Serial Number: 008668 Test Record Number: 4876
Test Date: 12/22/2025 Test Time: 10:51am EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	10:52am
FLO	Pass	10:52am
FC	Pass	10:52am

Temperature Tests

Test	Status	Time
FC1	Pass	10:52am
SRC	Pass	10:52am
DET	Pass	10:52am
BAR	Pass	10:52am
BT	Pass	10:52am

Blank Tests

Test	Status	Time
AIR	Pass	10:52am

Printer Tests

Test	Status	Time
PRNT	Pass	10:52am

CRC Tests

Test	Status	Time
COMP	Pass	10:53am
CAL	Pass	10:53am

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County RICHMOND Instrument Location RICHMOND COUNTY
Instrument Serial No. 008701 MAGISTRATE'S OFFICE

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 23 day of DECEMBER, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.




Signature of Certifying Official

239771
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

RICHMOND COUNTY MAGISTRATE'S OFFICE
760

Serial Number: 008701
Test Date: 12/23/2025

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: Galloway, Charles L
Permit Number: 0023-9771
Effective:
02/01/2025-02/01/2027

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test


Lot Number: AG431002
Exp Date: 11/05/2026

Test	g/210L	Time
DIAG	Pass	10:08am
AIR BLK	.00	10:09am
ACCY CHK	.08	10:10am
AIR BLK	.00	10:11am
SUB TEST	.00	10:11am
AIR BLK	.00	10:12am
SUB TEST	.00	10:14am
AIR BLK	.00	10:15am

Reported AC: .00 g/210L

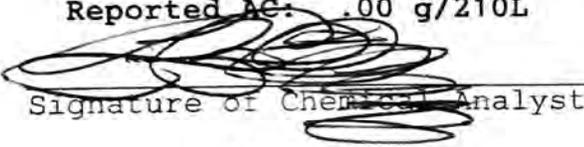
Signature of Chemical Analyst

Court CVR

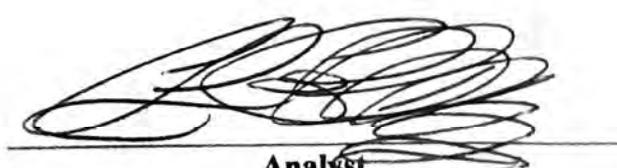
Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

RICHMOND COUNTY MAGISTRATE'S OFFICE 760

Serial Number: 008701 Test Record Number: 1592
Test Date: 12/23/2025 Test Time: 10:16am EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	10:17am
FLO	Pass	10:17am
FC	Pass	10:17am

Temperature Tests

Test	Status	Time
FC1	Pass	10:17am
SRC	Pass	10:17am
DET	Pass	10:17am
BAR	Pass	10:17am
BT	Pass	10:17am

Blank Tests

Test	Status	Time
AIR	Pass	10:17am


Printer Tests

Test	Status	Time
PRNT	Pass	10:17am

CRC Tests

Test	Status	Time
COMP	Pass	10:18am
CAL	Pass	10:18am

Preventive Maintenance
Status: Pass

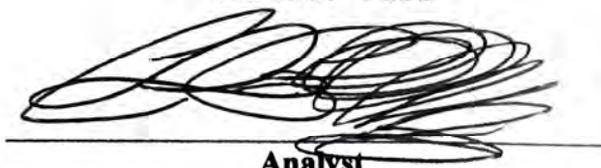

Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County RICHMOND Instrument Location RICHMOND COUNTY
Instrument Serial No. 008840 MAGISTRATE'S OFFICE

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 23 day of DECEMBER, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.




Signature of Certifying Official

239771
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

RICHMOND COUNTY MAGISTRATE'S OFFICE
760

Serial Number: 008840
Test Date: 12/23/2025

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Galloway, Charles L

Permit Number: 0023-9771

Effective:

02/01/2025-02/01/2027

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG431002


Exp Date: 11/05/2026

Test	g/210L	Time
DIAG	Pass	10:06am
AIR BLK	.00	10:07am
ACCY CHK	.08	10:08am
AIR BLK	.00	10:09am
SUB TEST	.00	10:10am
AIR BLK	.00	10:11am
SUB TEST	.00	10:13am
AIR BLK	.00	10:14am

Reported AC: .00 g/210L

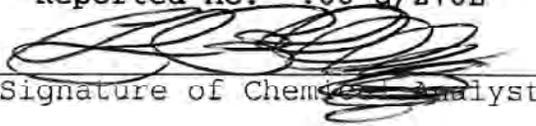
Signature of Chemical Analyst

Court CVR

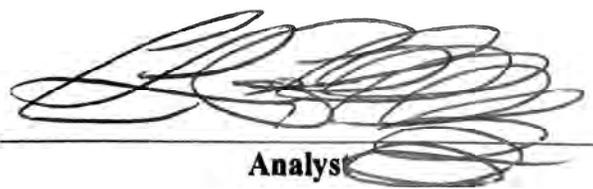
Analyst

This form is used when performing Preventive Maintenance procedures

Forensic Tests for Alcohol Branch

Department of Health and Human Services

Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

RICHMOND COUNTY MAGISTRATE'S OFFICE 760

Serial Number: 008840 Test Record Number: 3374
Test Date: 12/23/2025 Test Time: 10:14am EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	10:15am
FLO	Pass	10:15am
FC	Pass	10:15am

Temperature Tests

Test	Status	Time
FC1	Pass	10:15am
SRC	Pass	10:15am
DET	Pass	10:15am
BAR	Pass	10:15am
BT	Pass	10:15am

Blank Tests

Test	Status	Time
AIR	Pass	10:15am

Printer Tests

Test	Status	Time
PRNT	Pass	10:16am

CRC Tests

Test	Status	Time
COMP	Pass	10:16am
CAL	Pass	10:16am

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Robeson Instrument Location BAT Mobile Unit 7

Instrument Serial No. 008002

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 10th day of December, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Handwritten Signature]

Signature of Certifying Official

2266313

Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

ROBESON COUNTY BAT MOBILE UNIT 7 770

Serial Number: 008002
Test Date: 12/10/2025

Citation Number: M0000000-0
Subject's Name:

PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE

Analyst's Name: Sharpe Jr., Robert J
Permit Number: 1820-8591
Effective:
02/01/2025-02/01/2027

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG506303
Exp Date: 03/04/2027

Test	g/210L	Time
DIAG	Pass	3:19pm
AIR BLK	.00	3:20pm
ACCY CHK	.08	3:21pm
AIR BLK	.00	3:22pm
SUB TEST	.00	3:22pm
AIR BLK	.00	3:23pm
SUB TEST	.00	3:25pm
AIR BLK	.00	3:26pm

Reported AC: ~~00~~ g/210L

Signature of Chemical Analyst

Court CVR



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

ROBESON COUNTY BAT MOBILE UNIT 7 770

Serial Number: 008002 Test Record Number: 850
Test Date: 12/10/2025 Test Time: 3:26pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	3:27pm
FLO	Pass	3:27pm
FC	Pass	3:27pm

Temperature Tests

Test	Status	Time
FC1	Pass	3:27pm
SRC	Pass	3:27pm
DET	Pass	3:27pm
BAR	Pass	3:27pm
BT	Pass	3:27pm

Blank Tests

Test	Status	Time
AIR	Pass	3:28pm


Printer Tests

Test	Status	Time
PRNT	Pass	3:28pm

CRC Tests

Test	Status	Time
COMP	Pass	3:28pm
CAL	Pass	3:28pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Robeson Instrument Location BAT Mobile Unit 7
Instrument Serial No. 0096002

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 30th day of December, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.





Signature of Certifying Official

2266313

Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

ROBESON COUNTY BAT MOBILE UNIT 7 770

Serial Number: 008002
Test Date: 12/30/2025

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: Sharpe Jr., Robert J
Permit Number: 1820-8591
Effective:
02/01/2025-02/01/2027

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG506303
Exp Date: 03/04/2027

Test	g/210L	Time
DIAG	Pass	10:47pm
AIR BLK	.00	10:48pm
ACCY CHK	.08	10:48pm
AIR BLK	.00	10:49pm
SUB TEST	.00	10:50pm
AIR BLK	.00	10:51pm
SUB TEST	.00	10:52pm
AIR BLK	.00	10:53pm

Reported AC: 00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

ROBESON COUNTY BAT MOBILE UNIT 7 770

Serial Number: 008002 Test Record Number: 859
Test Date: 12/30/2025 Test Time: 10:54pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	10:54pm
FLO	Pass	10:54pm
FC	Pass	10:54pm

Temperature Tests

Test	Status	Time
FC1	Pass	10:54pm
SRC	Pass	10:54pm
DET	Pass	10:54pm
BAR	Pass	10:54pm
BT	Pass	10:54pm

Blank Tests

Test	Status	Time
AIR	Pass	10:55pm

Printer Tests

Test	Status	Time
PRNT	Pass	10:55pm

CRC Tests

Test	Status	Time
COMP	Pass	10:55pm
CAL	Pass	10:55pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Robeson Instrument Location BAT Mobile Unit 7

Instrument Serial No. 008968

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 10th day of December, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

2266313
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

ROBESON COUNTY BAT MOBILE UNIT 7 770

Serial Number: 008968
Test Date: 12/10/2025

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Sharpe Jr., Robert J

Permit Number: 1820-8591

Effective:

02/01/2025-02/01/2027

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG506303

Exp Date: 03/04/2027

Test	g/210L	Time
DIAG	Pass	3:08pm
AIR BLK	.00	3:09pm
ACCY CHK	.08	3:10pm
AIR BLK	.00	3:11pm
SUB TEST	.00	3:11pm
AIR BLK	.00	3:12pm
SUB TEST	.00	3:14pm
AIR BLK	.00	3:15pm

Reported AC: ~~.00~~ g/210L

Signature of Chemical Analyst

Court CVR



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

ROBESON COUNTY BAT MOBILE UNIT 7 770

Serial Number: 008968 Test Record Number: 420
Test Date: 12/10/2025 Test Time: 3:18pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	3:19pm
FLO	Pass	3:19pm
FC	Pass	3:19pm

Temperature Tests

Test	Status	Time
FC1	Pass	3:19pm
SRC	Pass	3:19pm
DET	Pass	3:19pm
BAR	Pass	3:19pm
BT	Pass	3:19pm

Blank Tests

Test	Status	Time
AIR	Pass	3:20pm


Printer Tests

Test	Status	Time
PRNT	Pass	3:20pm

CRC Tests

Test	Status	Time
COMP	Pass	3:20pm
CAL	Pass	3:20pm

Preventive Maintenance
Status: Pass

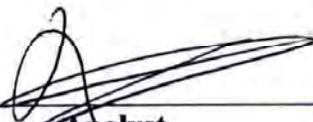

Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County Robeson Instrument Location BAT Mobile Unit 7

Instrument Serial No. 008968

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 30th day of December, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.





Signature of Certifying Official

2266313

Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

ROBESON COUNTY BAT MOBILE UNIT 7 770

Serial Number: 008968
Test Date: 12/30/2025

Citation Number: M0000000-0
Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Sharpe Jr., Robert J

Permit Number: 1820-8591

Effective:

02/01/2025-02/01/2027

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG506303

Exp Date: 03/04/2027

Test	g/210L	Time
DIAG	Pass	6:26pm
AIR BLK	.00	6:27pm
ACCY CHK	.08	6:28pm
AIR BLK	.00	6:28pm
SUB TEST	.00	6:29pm
AIR BLK	.00	6:30pm
SUB TEST	.00	6:31pm
AIR BLK	.00	6:32pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

ROBESON COUNTY BAT MOBILE UNIT 7 770

Serial Number: 008968 Test Record Number: 428
Test Date: 12/30/2025 Test Time: 6:33pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	6:34pm
FLO	Pass	6:34pm
FC	Pass	6:34pm

Temperature Tests

Test	Status	Time
FC1	Pass	6:34pm
SRC	Pass	6:34pm
DET	Pass	6:34pm
BAR	Pass	6:34pm
BT	Pass	6:34pm

Blank Tests

Test	Status	Time
AIR	Pass	6:34pm

Printer Tests

Test	Status	Time
PRNT	Pass	6:34pm

CRC Tests

Test	Status	Time
COMP	Pass	6:35pm
CAL	Pass	6:35pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Robeson Instrument Location BAT Mobile Unit 7

Instrument Serial No. 00 8968

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 31st day of December, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.





Signature of Certifying Official

2266313

Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

ROBESON COUNTY BAT MOBILE UNIT 7 770

Serial Number: 008968

Test Date: 12/31/2025

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Sharpe Jr., Robert J

Permit Number: 1820-8591

Effective:

02/01/2025-02/01/2027

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG506303

Exp Date: 03/04/2027

Test	g/210L	Time
DIAG	Pass	6:34pm
AIR BLK	.00	6:35pm
ACCY CHK	.08	6:36pm
AIR BLK	.00	6:37pm
SUB TEST	.00	6:38pm
AIR BLK	.00	6:39pm
SUB TEST	.00	6:40pm
AIR BLK	.00	6:41pm

Reported AC: ~~09~~ g/210L

Signature of Chemical Analyst

Court CVR


Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

ROBESON COUNTY BAT MOBILE UNIT 7 770

Serial Number: 008968 Test Record Number: 430
Test Date: 12/31/2025 Test Time: 6:43pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	6:43pm
FLO	Pass	6:43pm
FC	Pass	6:43pm

Temperature Tests

Test	Status	Time
FC1	Pass	6:43pm
SRC	Pass	6:43pm
DET	Pass	6:43pm
BAR	Pass	6:43pm
BT	Pass	6:43pm

Blank Tests

Test	Status	Time
AIR	Pass	6:44pm


Printer Tests

Test	Status	Time
PRNT	Pass	6:44pm

CRC Tests

Test	Status	Time
COMP	Pass	6:44pm
CAL	Pass	6:44pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Robeson Instrument Location BAT Mobile Unit 7

Instrument Serial No. 008971

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 10th day of December, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]

Signature of Certifying Official

2266313

Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

ROBESON COUNTY BAT MOBILE UNIT 7 770

Serial Number: 008971

Test Date: 12/10/2025

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Sharpe Jr., Robert J

Permit Number: 1820-8591

Effective:

02/01/2025-02/01/2027

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG506302

Exp Date: 03/04/2027

Test	g/210L	Time
DIAG	Pass	3:09pm
AIR BLK	.00	3:10pm
ACCY CHK	.08	3:11pm
AIR BLK	.00	3:12pm
SUB TEST	.00	3:12pm
AIR BLK	.00	3:13pm
SUB TEST	.00	3:15pm
AIR BLK	.00	3:16pm

Reported AC: ~~.00~~ g/210L

Signature of Chemical Analyst

Court CVR


Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

ROBESON COUNTY BAT MOBILE UNIT 7 770

Serial Number: 008971 Test Record Number: 370
Test Date: 12/10/2025 Test Time: 3:20pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	3:20pm
FLO	Pass	3:20pm
FC	Pass	3:21pm

Temperature Tests

Test	Status	Time
FC1	Pass	3:21pm
SRC	Pass	3:21pm
DET	Pass	3:21pm
BAR	Pass	3:21pm
BT	Pass	3:21pm

Blank Tests

Test	Status	Time
AIR	Pass	3:21pm

Printer Tests

Test	Status	Time
PRNT	Pass	3:21pm

CRC Tests

Test	Status	Time
COMP	Pass	3:21pm
CAL	Pass	3:21pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County Robeson Instrument Location BAT Mobile Unit 7

Instrument Serial No. 008971

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 30th day of December, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

2266313
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

ROBESON COUNTY BAT MOBILE UNIT 7 770

Serial Number: 008971
Test Date: 12/30/2025

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE

Analyst's Name: Sharpe Jr., Robert J
Permit Number: 1820-8591
Effective:
02/01/2025-02/01/2027

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG506302
Exp Date: 03/04/2027

Test	g/210L	Time
DIAG	Pass	6:25pm
AIR BLK	.00	6:26pm
ACCY CHK	.08	6:27pm
AIR BLK	.00	6:28pm
SUB TEST	.00	6:28pm
AIR BLK	.00	6:29pm
SUB TEST	.00	6:31pm
AIR BLK	.00	6:32pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

ROBESON COUNTY BAT MOBILE UNIT 7 770

Serial Number: 008971 Test Record Number: 378
Test Date: 12/30/2025 Test Time: 6:33pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	6:33pm
FLO	Pass	6:33pm
FC	Pass	6:33pm

Temperature Tests

Test	Status	Time
FC1	Pass	6:33pm
SRC	Pass	6:33pm
DET	Pass	6:33pm
BAR	Pass	6:33pm
BT	Pass	6:33pm

Blank Tests

Test	Status	Time
AIR	Pass	6:34pm

Printer Tests

Test	Status	Time
PRNT	Pass	6:34pm

CRC Tests

Test	Status	Time
COMP	Pass	6:34pm
CAL	Pass	6:34pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Robeson Instrument Location BAT Mobile Unit 7

Instrument Serial No. 008971

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 31st day of December, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]

Signature of Certifying Official

2266313

Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

ROBESON COUNTY BAT MOBILE UNIT 7 770

Serial Number: 008971
Test Date: 12/31/2025

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Sharpe Jr., Robert J

Permit Number: 1820-8591

Effective:

02/01/2025-02/01/2027

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG506302

Exp Date: 03/04/2027

Test	g/210L	Time
DIAG	Pass	6:33pm
AIR BLK	.00	6:34pm
ACCY CHK	.08	6:35pm
AIR BLK	.00	6:36pm
SUB TEST	.00	6:37pm
AIR BLK	.00	6:38pm
SUB TEST	.00	6:39pm
AIR BLK	.00	6:40pm

Reported AC: ~~.00 g/210L~~

Signature of Chemical Analyst

Court CVR



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

ROBESON COUNTY BAT MOBILE UNIT 7 770

Serial Number: 008971 Test Record Number: 380
Test Date: 12/31/2025 Test Time: 6:41pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	6:41pm
FLO	Pass	6:41pm
FC	Pass	6:41pm

Temperature Tests

Test	Status	Time
FC1	Pass	6:42pm
SRC	Pass	6:42pm
DET	Pass	6:42pm
BAR	Pass	6:42pm
BT	Pass	6:42pm

Blank Tests

Test	Status	Time
AIR	Pass	6:42pm

Printer Tests

Test	Status	Time
PRNT	Pass	6:42pm

CRC Tests

Test	Status	Time
COMP	Pass	6:42pm
CAL	Pass	6:42pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Robeson Instrument Location BAT Mobile Unit 7

Instrument Serial No. 008972

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 10th day of December, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.





Signature of Certifying Official

2266313

Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

ROBESON COUNTY BAT MOBILE UNIT 7 770

Serial Number: 008972
Test Date: 12/10/2025

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Sharpe Jr., Robert J

Permit Number: 1820-8591

Effective:

02/01/2025-02/01/2027

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG506303

Exp Date: 03/04/2027

Test	g/210L	Time
DIAG	Pass	3:11pm
AIR BLK	.00	3:12pm
ACCY CHK	.08	3:13pm
AIR BLK	.00	3:14pm
SUB TEST	.00	3:14pm
AIR BLK	.00	3:15pm
SUB TEST	.00	3:17pm
AIR BLK	.00	3:18pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

ROBESON COUNTY BAT MOBILE UNIT 7 770

Serial Number: 008972 Test Record Number: 430
Test Date: 12/10/2025 Test Time: 3:21pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	3:22pm
FLO	Pass	3:22pm
FC	Pass	3:22pm

Temperature Tests

Test	Status	Time
FC1	Pass	3:22pm
SRC	Pass	3:22pm
DET	Pass	3:22pm
BAR	Pass	3:22pm
BT	Pass	3:22pm

Blank Tests

Test	Status	Time
AIR	Pass	3:23pm


Printer Tests

Test	Status	Time
PRNT	Pass	3:23pm

CRC Tests

Test	Status	Time
COMP	Pass	3:23pm
CAL	Pass	3:23pm

Preventive Maintenance
Status: Pass

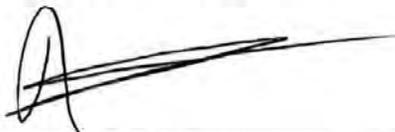

Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County Robeson Instrument Location BAT Mobile Unit 7
Instrument Serial No. 008972

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 30th day of December, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

2266313
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

ROBESON COUNTY BAT MOBILE UNIT 7 770

Serial Number: 008972
Test Date: 12/30/2025

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Sharpe Jr., Robert J

Permit Number: 1820-8591

Effective:

02/01/2025-02/01/2027

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG506303


Exp Date: 03/04/2027

Test	g/210L	Time
DIAG	Pass	6:25pm
AIR BLK	.00	6:26pm
ACCY CHK	.08	6:27pm
AIR BLK	.00	6:28pm
SUB TEST	.00	6:28pm
AIR BLK	.00	6:29pm
SUB TEST	.00	6:31pm
AIR BLK	.00	6:32pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR

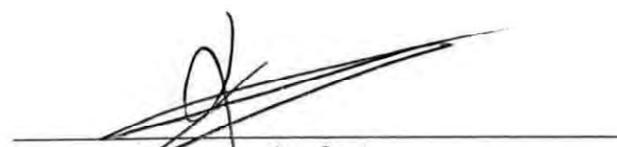
Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

ROBESON COUNTY BAT MOBILE UNIT 7 770

Serial Number: 008972 Test Record Number: 440
Test Date: 12/30/2025 Test Time: 6:32pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	6:33pm
FLO	Pass	6:33pm
FC	Pass	6:33pm

Temperature Tests

Test	Status	Time
FC1	Pass	6:33pm
SRC	Pass	6:33pm
DET	Pass	6:33pm
BAR	Pass	6:33pm
BT	Pass	6:33pm

Blank Tests

Test	Status	Time
AIR	Pass	6:34pm

Printer Tests

Test	Status	Time
PRNT	Pass	6:34pm

CRC Tests

Test	Status	Time
COMP	Pass	6:34pm
CAL	Pass	6:34pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County Robeson Instrument Location BAT Mobile Unit 7

Instrument Serial No. 00 8972

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 31st day of December, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]

Signature of Certifying Official

2266313

Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

ROBESON COUNTY BAT MOBILE UNIT 7 770

Serial Number: 008972
Test Date: 12/31/2025

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Sharpe Jr., Robert J

Permit Number: 1820-8591

Effective:

02/01/2025-02/01/2027

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG506303

Exp Date: 03/04/2027

Test	g/210L	Time
DIAG	Pass	6:33pm
AIR BLK	.00	6:34pm
ACCY CHK	.08	6:35pm
AIR BLK	.00	6:36pm
SUB TEST	.00	6:37pm
AIR BLK	.00	6:38pm
SUB TEST	.00	6:39pm
AIR BLK	.00	6:40pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

ROBESON COUNTY BAT MOBILE UNIT 7 770

Serial Number: 008972 Test Record Number: 442
Test Date: 12/31/2025 Test Time: 6:41pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	6:41pm
FLO	Pass	6:41pm
FC	Pass	6:41pm

Temperature Tests

Test	Status	Time
FC1	Pass	6:41pm
SRC	Pass	6:41pm
DET	Pass	6:41pm
BAR	Pass	6:41pm
BT	Pass	6:41pm

Blank Tests

Test	Status	Time
AIR	Pass	6:42pm

Printer Tests

Test	Status	Time
PRNT	Pass	6:42pm

CRC Tests

Test	Status	Time
COMP	Pass	6:42pm
CAL	Pass	6:42pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Rowan Instrument Location BAT Mobile Unit 8

Instrument Serial No. 008615

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 13 day of December, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

2219283
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

ROWAN COUNTY BAT MOBILE UNIT 8 790

Serial Number: 008615
Test Date: 12/13/2025

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Glasscock, Jerry D

Permit Number: 7180-9235

Effective:

02/01/2025-02/01/2027

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG405102

Exp Date: 02/20/2026

Test	g/210L	Time
DIAG	Pass	8:16pm
AIR BLK	.00	8:17pm
ACCY CHK	.07	8:17pm
AIR BLK	.00	8:18pm
SUB TEST	.00	8:19pm
AIR BLK	.00	8:20pm
SUB TEST	.00	8:21pm
AIR BLK	.00	8:22pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

Intox EC/IR-II: Preventive Maintenance

ROWAN COUNTY BAT MOBILE UNIT 8 790

Serial Number: 008615 Test Record Number: 6204
Test Date: 12/13/2025 Test Time: 8:22pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	8:23pm
FLO	Pass	8:23pm
FC	Pass	8:23pm

Temperature Tests

Test	Status	Time
FC1	Pass	8:23pm
SRC	Pass	8:23pm
DET	Pass	8:23pm
BAR	Pass	8:23pm
BT	Pass	8:23pm

Blank Tests

Test	Status	Time
AIR	Pass	8:24pm

Printer Tests

Test	Status	Time
PRNT	Pass	8:24pm

CRC Tests

Test	Status	Time
COMP	Pass	8:24pm
CAL	Pass	8:24pm

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Rowan Instrument Location BAT Mobile Unit 8

Instrument Serial No. 008736

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 13 day of December, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

2219283
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

ROWAN COUNTY BAT MOBILE UNIT 8 790

Serial Number: 008736

Test Date: 12/13/2025

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENACE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Glasscock, Jerry D

Permit Number: 7180-9235

Effective:

02/01/2025-02/01/2027

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG405102

Exp Date: 02/20/2026

Test	g/210L	Time
DIAG	Pass	8:15pm
AIR BLK	.00	8:16pm
ACCY CHK	.07	8:16pm
AIR BLK	.00	8:17pm
SUB TEST	.00	8:18pm
AIR BLK	.00	8:19pm
SUB TEST	.00	8:20pm
AIR BLK	.00	8:21pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

Intox EC/IR-II: Preventive Maintenance

ROWAN COUNTY BAT MOBILE UNIT 8 790

Serial Number: 008736 Test Record Number: 1564
Test Date: 12/13/2025 Test Time: 8:22pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	8:22pm
FLO	Pass	8:22pm
FC	Pass	8:22pm

Temperature Tests

Test	Status	Time
FC1	Pass	8:22pm
SRC	Pass	8:22pm
DET	Pass	8:22pm
BAR	Pass	8:22pm
BT	Pass	8:22pm

Blank Tests

Test	Status	Time
AIR	Pass	8:23pm


Printer Tests

Test	Status	Time
PRNT	Pass	8:23pm

CRC Tests

Test	Status	Time
COMP	Pass	8:23pm
CAL	Pass	8:23pm

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Rowan Instrument Location BAT Mobile Unit 8
Instrument Serial No. 008775 _____

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass", and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 13 day of December, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

2219283
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

ROWAN COUNTY BAT MOBILE UNIT 8-790

Serial Number: 008775

Test Date: 12/13/2025

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Glasscock, Jerry D

Permit Number: 7180-9235

Effective:

02/01/2025-02/01/2027

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG506303

Exp Date: 03/04/2027

Test	g/210L	Time
DIAG	Pass	8:14pm
AIR BLK	.00	8:15pm
ACCY CHK	.08	8:16pm
AIR BLK	.00	8:17pm
SUB TEST	.00	8:17pm
AIR BLK	.00	8:18pm
SUB TEST	.00	8:19pm
AIR BLK	.00	8:20pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

ROWAN COUNTY BAT MOBILE UNIT 8 790

Serial Number: 008775 Test Record Number: 2416
Test Date: 12/13/2025 Test Time: 8:22pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	8:22pm
FLO	Pass	8:22pm
FC	Pass	8:22pm

Temperature Tests

Test	Status	Time
FC1	Pass	8:22pm
SRC	Pass	8:22pm
DET	Pass	8:22pm
BAR	Pass	8:22pm
BT	Pass	8:22pm

Blank Tests

Test	Status	Time
AIR	Pass	8:23pm

Printer Tests

Test	Status	Time
PRNT	Pass	8:23pm

CRC Tests

Test	Status	Time
COMP	Pass	8:23pm
CAL	Pass	8:23pm

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Rowan Instrument Location BAT Mobile Unit 8

Instrument Serial No. 008816

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 13 day of December, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Jay D. Harrison
Signature of Certifying Official

2219283
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

ROWAN COUNTY BAT MOBILE UNIT 8 790

Serial Number: 008816
Test Date: 12/13/2025

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Glasscock, Jerry D

Permit Number: 7180-9235

Effective:

02/01/2025-02/01/2027

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG431002

Exp Date: 11/05/2026

Test	g/210L	Time
DIAG	Pass	8:13pm
AIR BLK	.00	8:14pm
ACCY CHK	.07	8:14pm
AIR BLK	.00	8:16pm
SUB TEST	.00	8:16pm
AIR BLK	.00	8:17pm
SUB TEST	.00	8:19pm
AIR BLK	.00	8:20pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

ROWAN COUNTY BAT MOBILE UNIT 8 790

Serial Number: 008816 Test Record Number: 7999
Test Date: 12/13/2025 Test Time: 8:22pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	8:22pm
FLO	Pass	8:22pm
FC	Pass	8:23pm

Temperature Tests

Test	Status	Time
FC1	Pass	8:23pm
SRC	Pass	8:23pm
DET	Pass	8:23pm
BAR	Pass	8:23pm
BT	Pass	8:23pm

Blank Tests

Test	Status	Time
AIR	Pass	8:23pm

Printer Tests

Test	Status	Time
PRNT	Pass	8:23pm

CRC Tests

Test	Status	Time
COMP	Pass	8:23pm
CAL	Pass	8:23pm

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County ROWAN Instrument Location SALISBURY


Instrument Serial No. 008835 POLICE DEPARTMENT

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 1st day of DECEMBER, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.

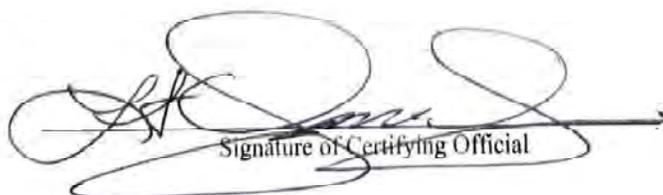


Signature of Certifying Official

353799
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

ROWAN COUNTY SALISBURY PD 790

Serial Number: 008835

Test Date: 12/01/2025

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Oligmueller, Leo A

Permit Number: 0035-3799

Effective:

02/01/2025-02/01/2027

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG506301

Exp Date: 03/04/2027

Test	g/210L	Time
DIAG	Pass	11:55am
AIR BLK	.00	11:56am
ACCY CHK	.08	11:56am
AIR BLK	.00	11:58am
SUB TEST	.00	11:58am
AIR BLK	.00	11:59am
SUB TEST	.00	12:01pm
AIR BLK	.00	12:01pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

ROWAN COUNTY SALISBURY PD 790

Serial Number: 008835 Test Record Number: 3539
Test Date: 12/01/2025 Test Time: 12:07pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	12:07pm
FLO	Pass	12:07pm
FC	Pass	12:07pm

Temperature Tests

Test	Status	Time
FCI	Pass	12:07pm
SRC	Pass	12:07pm
DET	Pass	12:07pm
BAR	Pass	12:07pm
BT	Pass	12:07pm

Blank Tests

Test	Status	Time
AIR	Pass	12:08pm

Printer Tests

Test	Status	Time
PRNT	Pass	12:08pm

CRC Tests

Test	Status	Time
COMP	Pass	12:08pm
CAL	Pass	12:08pm

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)


County ROWAN Instrument Location CHINA GROVE
Instrument Serial No. 008862 POLICE DEPARTMENT

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 1ST day of DECEMBER, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.

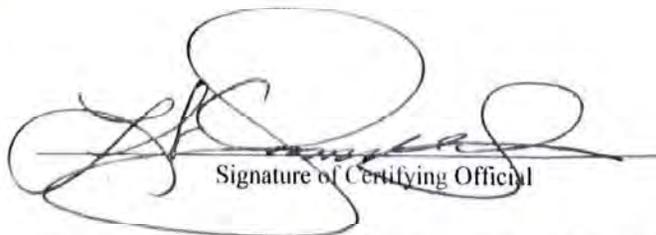


Signature of Certifying Official

353799
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

ROWAN COUNTY CHINA GROVE PD 790

Serial Number: 008862

Test Date: 12/01/2025

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Oligmueller, Leo A

Permit Number: 0035-3799

Effective:

02/01/2025-02/01/2027

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG506303


Exp Date: 03/04/2027

Test	g/210L	Time
DIAG	Pass	1:56pm
AIR BLK	.00	1:57pm
ACCY CHK	.07	1:57pm
AIR BLK	.00	1:58pm
SUB TEST	.00	1:59pm
AIR BLK	.00	2:00pm
SUB TEST	.00	2:02pm
AIR BLK	.00	2:03pm

Reported AC: .00 g/210L

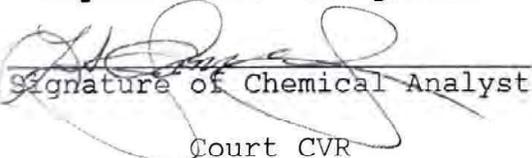
Signature of Chemical Analyst

Court CVR

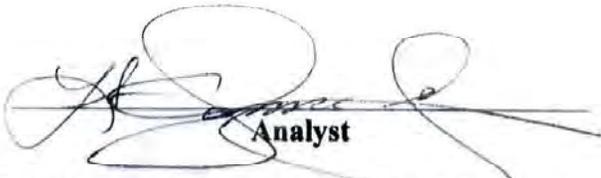
Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

ROWAN COUNTY CHINA GROVE PD 790

Serial Number: 008862 Test Record Number: 1289
Test Date: 12/01/2025 Test Time: 2:03pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	2:04pm
FLO	Pass	2:04pm
FC	Pass	2:04pm

Temperature Tests

Test	Status	Time
FC1	Pass	2:04pm
SRC	Pass	2:04pm
DET	Pass	2:04pm
BAR	Pass	2:04pm
BT	Pass	2:04pm

Blank Tests

Test	Status	Time
AIR	Pass	2:05pm

Printer Tests

Test	Status	Time
PRNT	Pass	2:05pm

CRC Tests

Test	Status	Time
COMP	Pass	2:05pm
CAL	Pass	2:05pm

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)


County ROWAN Instrument Location SALISBURY
Instrument Serial No. 008868 POLICE DEPARTMENT

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 1ST day of DECEMBER, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.

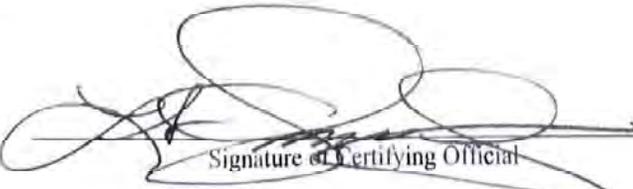


Signature of Certifying Official

353799
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

ROWAN COUNTY SALISBURY PD 790

Serial Number: 008868

Test Date: 12/01/2025

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Oligmueller, Leo A

Permit Number: 0035-3799

Effective:

02/01/2025-02/01/2027

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG506301

Exp Date: 03/04/2027

Test	g/210L	Time
DIAG	Pass	11:51am
AIR BLK	.00	11:52am
ACCY CHK	.07	11:53am
AIR BLK	.00	11:54am
SUB TEST	.00	11:55am
AIR BLK	.00	11:56am
SUB TEST	.00	11:58am
AIR BLK	.00	11:59am

Reported AC: .00 g/210L

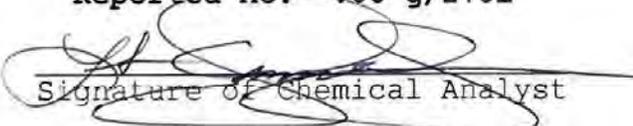
Signature of Chemical Analyst

Court CVR


Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

ROWAN COUNTY SALISBURY PD 790

Serial Number: 008868 Test Record Number: 4005
Test Date: 12/01/2025 Test Time: 12:00pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	12:01pm
FLO	Pass	12:01pm
FC	Pass	12:01pm

Temperature Tests

Test	Status	Time
FC1	Pass	12:01pm
SRC	Pass	12:01pm
DET	Pass	12:01pm
BAR	Pass	12:01pm
BT	Pass	12:01pm

Blank Tests

Test	Status	Time
AIR	Pass	12:02pm


Printer Tests

Test	Status	Time
PRNT	Pass	12:02pm

CRC Tests

Test	Status	Time
COMP	Pass	12:02pm
CAL	Pass	12:02pm

Preventive Maintenance
Status: Pass

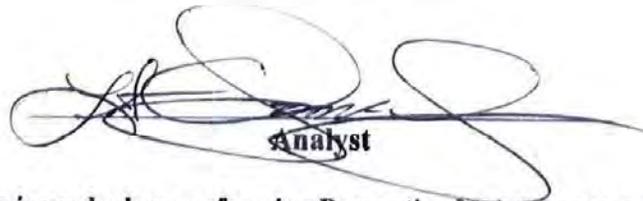
Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Rowan Instrument Location BAT Mobile Unit 8

Instrument Serial No. 008929 _____

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 13 day of December, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

2219283
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

ROWAN COUNTY BAT MOBILE UNIT 8 790

Serial Number: 008929

Test Date: 12/13/2025

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Glasscock, Jerry D

Permit Number: 7180-9235

Effective:

02/01/2025-02/01/2027

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG506303

Exp Date: 03/04/2027

Test	g/210L	Time
DIAG	Pass	8:11pm
AIR BLK	.00	8:13pm
ACCY CHK	.08	8:13pm
AIR BLK	.00	8:14pm
SUB TEST	.00	8:15pm
AIR BLK	.00	8:17pm
SUB TEST	.00	8:18pm
AIR BLK	.00	8:20pm

Reported AC: .00 g/210L

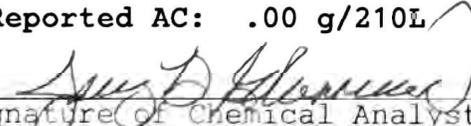
Signature of Chemical Analyst

Court CVR


Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

ROWAN COUNTY BAT MOBILE UNIT 8 790

Serial Number: 008929 Test Record Number: 1701
Test Date: 12/13/2025 Test Time: 8:21pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	8:22pm
FLO	Pass	8:22pm
FC	Pass	8:22pm

Temperature Tests

Test	Status	Time
FC1	Pass	8:22pm
SRC	Pass	8:22pm
DET	Pass	8:22pm
BAR	Pass	8:22pm
BT	Pass	8:22pm

Blank Tests

Test	Status	Time
AIR	Pass	8:23pm

Printer Tests

Test	Status	Time
PRNT	Pass	8:23pm

CRC Tests

Test	Status	Time
COMP	Pass	8:23pm
CAL	Pass	8:23pm

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Rutherford Instrument Location Forest City PD

Instrument Serial No. 008889 Forest City, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 29 day of December, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

244987
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

RUTHERFORD COUNTY FOREST CITY PD 800

Serial Number: 008889
Test Date: 12/29/2025

Citation Number: M0000000-0
Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Loftis, Benjamin C

Permit Number: 0024-4987

Effective:

03/01/2025-03/01/2027

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG431001

Exp Date: 11/05/2026

Test	g/210L	Time
DIAG	Pass	10:56am
AIR BLK	.00	10:56am
ACCY CHK	.07	10:57am
AIR BLK	.00	10:58am
SUB TEST	.00	10:59am
AIR BLK	.00	11:00am
SUB TEST	.00	11:01am
AIR BLK	.00	11:02am

Reported AC: .00 g/210L

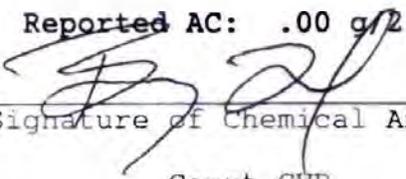

Signature of Chemical Analyst

Court CVR



Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

RUTHERFORD COUNTY FOREST CITY PD 800

Serial Number: 008889 Test Record Number: 1287
Test Date: 12/29/2025 Test Time: 11:02am EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	11:02am
FLO	Pass	11:02am
FC	Pass	11:03am

Temperature Tests

Test	Status	Time
FC1	Pass	11:03am
SRC	Pass	11:03am
DET	Pass	11:03am
BAR	Pass	11:03am
BT	Pass	11:03am

Blank Tests

Test	Status	Time
AIR	Pass	11:04am


Printer Tests

Test	Status	Time
PRNT	Pass	11:04am

CRC Tests

Test	Status	Time
COMP	Pass	11:04am
CAL	Pass	11:04am

Preventive Maintenance
Status: Pass

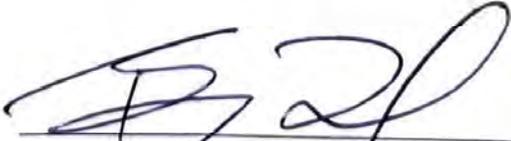

Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Rutherford Instrument Location Rutherford County Jail

Instrument Serial No. 008914 Rutherfordton, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 29 day of December, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

244987
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

RUTHERFORD COUNTY RUTHERFORD COUNTY SO
800

Serial Number: 008914
Test Date: 12/29/2025

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: Loftis, Benjamin C
Permit Number: 0024-4987
Effective:
03/01/2025-03/01/2027

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test


Lot Number: AG534301
Exp Date: 12/09/2027

Test	g/210L	Time
DIAG	Pass	11:39am
AIR BLK	.00	11:39am
ACCY CHK	.08	11:40am
AIR BLK	.00	11:41am
SUB TEST	.00	11:42am
AIR BLK	.00	11:43am
SUB TEST	.00	11:44am
AIR BLK	.00	11:45am

Reported AC: .00 g/210L

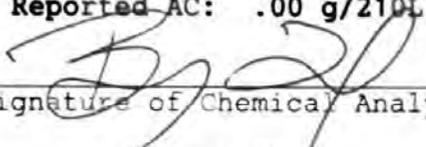
Signature of Chemical Analyst

Court CVR

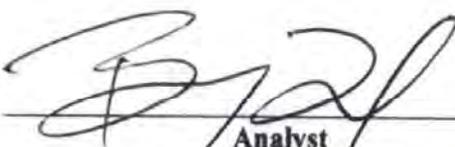
Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

RUTHERFORD COUNTY RUTHERFORD COUNTY SO 800

Serial Number: 008914 Test Record Number: 3029
Test Date: 12/29/2025 Test Time: 11:45am EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	11:45am
FLO	Pass	11:45am
FC	Pass	11:46am

Temperature Tests

Test	Status	Time
FC1	Pass	11:46am
SRC	Pass	11:46am
DET	Pass	11:46am
BAR	Pass	11:46am
BT	Pass	11:46am

Blank Tests

Test	Status	Time
AIR	Pass	11:46am


Printer Tests

Test	Status	Time
PRNT	Pass	11:46am

CRC Tests

Test	Status	Time
COMP	Pass	11:47am
CAL	Pass	11:47am

Preventive Maintenance
Status: Pass

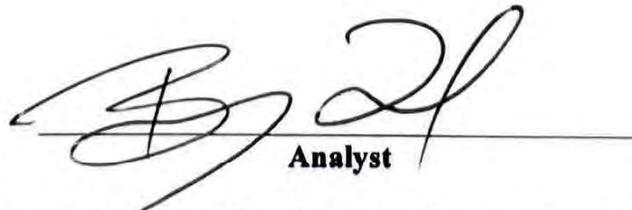

Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Stanly Instrument Location Locust PD
Instrument Serial No. 008706 Locust, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 2nd day of December, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Bruce Helms
Signature of Certifying Official

849845
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

STANLY COUNTY LOCUST PD 830

Serial Number: 008706

Test Date: 12/02/2025

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Helms, Bryce A

Permit Number: 0084-9845

Effective:

02/01/2025-02/01/2027

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG501303

Exp Date: 01/13/2027


Test	g/210L	Time
DIAG	Pass	10:16am
AIR BLK	.00	10:17am
ACCY CHK	.07	10:17am
AIR BLK	.00	10:19am
SUB TEST	.00	10:19am
AIR BLK	.00	10:20am
SUB TEST	.00	10:22am
AIR BLK	.00	10:23am

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR

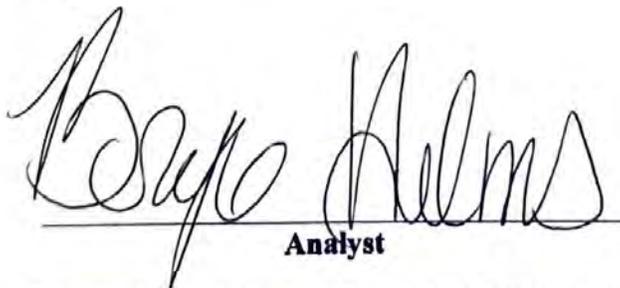

Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

STANLY COUNTY LOCUST PD 830

Serial Number: 008706 Test Record Number: 3875
Test Date: 12/02/2025 Test Time: 10:23am EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	10:23am
FLO	Pass	10:23am
FC	Pass	10:23am

Temperature Tests

Test	Status	Time
FC1	Pass	10:24am
SRC	Pass	10:24am
DET	Pass	10:24am
BAR	Pass	10:24am
BT	Pass	10:24am

Blank Tests

Test	Status	Time
AIR	Pass	10:24am


Printer Tests

Test	Status	Time
PRNT	Pass	10:24am

CRC Tests

Test	Status	Time
COMP	Pass	10:24am
CAL	Pass	10:24am

Preventive Maintenance
Status: Pass

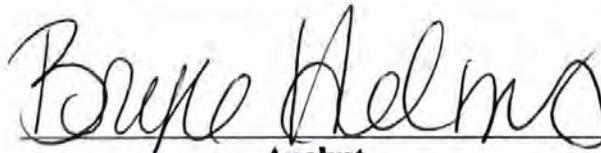
Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County Stanly Instrument Location Stanly County &
Albemarle, NC
Instrument Serial No. 008824

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 30th day of December, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Conny Helms
Signature of Certifying Official

849845
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

STANLY COUNTY STANLY COUNTY SO 830

Serial Number: 008824
Test Date: 12/30/2025

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Helms, Bryce A

Permit Number: 0084-9845

Effective:

02/01/2025-02/01/2027

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG516203

Exp Date: 06/11/2027


Test	g/210L	Time
DIAG	Pass	9:33am
AIR BLK	.00	9:33am
ACCY CHK	.07	9:34am
AIR BLK	.00	9:35am
SUB TEST	.00	9:36am
AIR BLK	.00	9:37am
SUB TEST	.00	9:39am
AIR BLK	.00	9:39am

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR

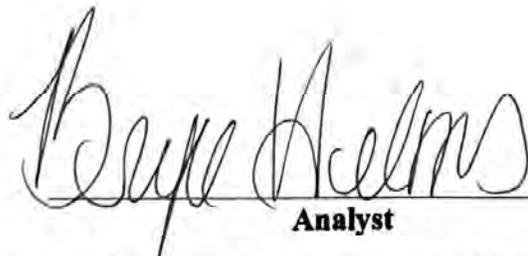

Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

STANLY COUNTY STANLY COUNTY SO 830

Serial Number: 008824 Test Record Number: 2291
Test Date: 12/30/2025 Test Time: 9:40am EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	9:41am
FLO	Pass	9:41am
FC	Pass	9:41am

Temperature Tests

Test	Status	Time
FC1	Pass	9:41am
SRC	Pass	9:41am
DET	Pass	9:41am
BAR	Pass	9:41am
BT	Pass	9:41am

Blank Tests

Test	Status	Time
AIR	Pass	9:42am


Printer Tests

Test	Status	Time
PRNT	Pass	9:42am

CRC Tests

Test	Status	Time
COMP	Pass	9:42am
CAL	Pass	9:42am

Preventive Maintenance
Status: Pass

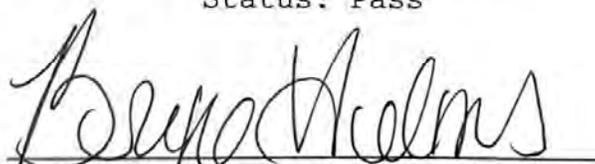
Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County Stanly Instrument Location Stanly County 80
Instrument Serial No. 008842 Albemarle, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 30th day of December, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

849845
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

STANLY COUNTY STANLY COUNTY SO 830

Serial Number: 008842
Test Date: 12/30/2025

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: Helms, Bryce A
Permit Number: 0084-9845
Effective:
02/01/2025-02/01/2027

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG534301
Exp Date: 12/09/2027


Test	g/210L	Time
DIAG	Pass	9:34am
AIR BLK	.00	9:35am
ACCY CHK	.08	9:36am
AIR BLK	.00	9:37am
SUB TEST	.00	9:38am
AIR BLK	.00	9:39am
SUB TEST	.00	9:40am
AIR BLK	.00	9:41am

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR

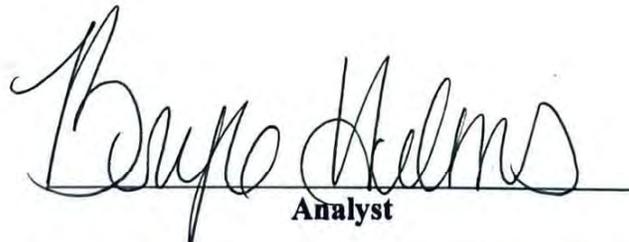

Analyst

Intox EC/IR-II: Preventive Maintenance

STANLY COUNTY STANLY COUNTY SO 830

Serial Number: 008842 Test Record Number: 3289
Test Date: 12/30/2025 Test Time: 9:42am EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	9:42am
FLO	Pass	9:42am
FC	Pass	9:42am

Temperature Tests

Test	Status	Time
FC1	Pass	9:42am
SRC	Pass	9:42am
DET	Pass	9:42am
BAR	Pass	9:42am
BT	Pass	9:42am

Blank Tests

Test	Status	Time
AIR	Pass	9:43am


Printer Tests

Test	Status	Time
PRNT	Pass	9:43am

CRC Tests

Test	Status	Time
COMP	Pass	9:43am
CAL	Pass	9:43am

Preventive Maintenance
Status: Pass

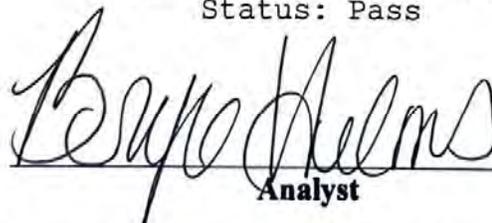

Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County Union Instrument Location Waxhaw PD
Instrument Serial No. 008598 Waxhaw, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 30th day of December, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Bayle Helms
Signature of Certifying Official

849845
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

UNION COUNTY WAXHAW PD 890

Serial Number: 008598

Test Date: 12/30/2025

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Helms, Bryce A

Permit Number: 0084-9845

Effective:

02/01/2025-02/01/2027

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG501303

Exp Date: 01/13/2027


Test	g/210L	Time
DIAG	Pass	11:15am
AIR BLK	.00	11:15am
ACCY CHK	.07	11:16am
AIR BLK	.00	11:17am
SUB TEST	.00	11:18am
AIR BLK	.00	11:19am
SUB TEST	.00	11:20am
AIR BLK	.00	11:21am

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR

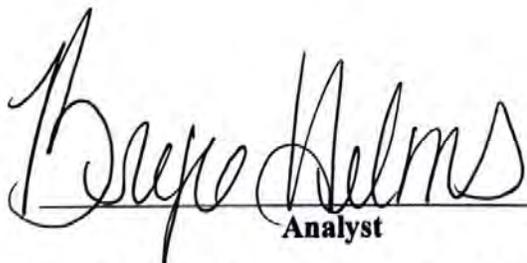

Analyst

Intox EC/IR-II: Preventive Maintenance

UNION COUNTY WAXHAW PD 890

Serial Number: 008598 Test Record Number: 1164
Test Date: 12/30/2025 Test Time: 11:21am EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	11:22am
FLO	Pass	11:22am
FC	Pass	11:22am

Temperature Tests

Test	Status	Time
FC1	Pass	11:22am
SRC	Pass	11:22am
DET	Pass	11:22am
BAR	Pass	11:22am
BT	Pass	11:22am

Blank Tests

Test	Status	Time
AIR	Pass	11:23am


Printer Tests

Test	Status	Time
PRNT	Pass	11:23am

CRC Tests

Test	Status	Time
COMP	Pass	11:23am
CAL	Pass	11:23am

Preventive Maintenance
Status: *Pass*

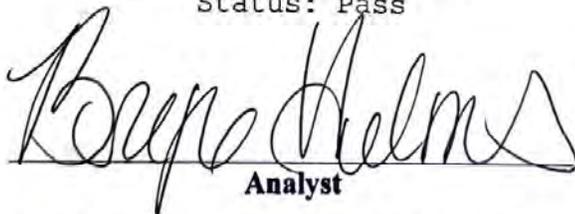
Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County VANCE Instrument Location VANCE CO. S.O

Instrument Serial No. 008870 156 Church ST
HENDERSON, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 29 day of DECEMBER, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



E. Bryant
Signature of Certifying Official

179707
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

VANCE COUNTY SHERIFF'S DEPARTMENT 900

Serial Number: 008870
Test Date: 12/29/2025

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Bryant, Earl A

Permit Number: 0017-9707

Effective:

02/01/2025-02/01/2027

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG534301

Exp Date: 12/09/2027


Test	g/210L	Time
DIAG	Pass	10:37am
AIR BLK	.00	10:38am
ACCY CHK	.07	10:39am
AIR BLK	.00	10:40am
SUB TEST	.00	10:41am
AIR BLK	.00	10:42am
SUB TEST	.00	10:43am
AIR BLK	.00	10:44am

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

VANCE COUNTY SHERIFF'S DEPARTMENT 900

Serial Number: 008870 Test Record Number: 4186
Test Date: 12/29/2025 Test Time: 10:45am EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	10:45am
FLO	Pass	10:45am
FC	Pass	10:45am

Temperature Tests

Test	Status	Time
FC1	Pass	10:46am
SRC	Pass	10:46am
DET	Pass	10:46am
BAR	Pass	10:46am
BT	Pass	10:46am

Blank Tests

Test	Status	Time
AIR	Pass	10:46am


Printer Tests

Test	Status	Time
PRNT	Pass	10:46am

CRC Tests

Test	Status	Time
COMP	Pass	10:46am
CAL	Pass	10:46am

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County VANCE Instrument Location VANCE Co. S.O.

Instrument Serial No. 008937 156 Church ST
HENDERSON, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 29 day of DECEMBER, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



E. Bryant
Signature of Certifying Official

179707
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

VANCE COUNTY SHERIFF'S DEPARTMENT 900

Serial Number: 008937
Test Date: 12/29/2025

Citation Number: M0000000-0
Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Bryant, Earl A

Permit Number: 0017-9707

Effective:

02/01/2025-02/01/2027

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG534301

Exp Date: 12/09/2027


Test	g/210L	Time
DIAG	Pass	10:36am
AIR BLK	.00	10:37am
ACCY CHK	.08	10:38am
AIR BLK	.00	10:39am
SUB TEST	.00	10:40am
AIR BLK	.00	10:41am
SUB TEST	.00	10:42am
AIR BLK	.00	10:43am

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

VANCE COUNTY SHERIFF'S DEPARTMENT 900

Serial Number: 008937 Test Record Number: 3613
Test Date: 12/29/2025 Test Time: 10:44am EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	10:44am
FLO	Pass	10:44am
FC	Pass	10:45am

Temperature Tests

Test	Status	Time
FC1	Pass	10:45am
SRC	Pass	10:45am
DET	Pass	10:45am
BAR	Pass	10:45am
BT	Pass	10:45am

Blank Tests

Test	Status	Time
AIR	Pass	10:45am

Printer Tests

Test	Status	Time
PRNT	Pass	10:45am

CRC Tests

Test	Status	Time
COMP	Pass	10:45am
CAL	Pass	10:45am

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Wake Instrument Location Wake Co Detention Ctr
Instrument Serial No. 008577 3301 HAMMOND RD
Raleigh, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 9 day of December, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Simon Stokes Brasco
Signature of Certifying Official

146221
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

WAKE COUNTY DETENTION CENTER 910

Serial Number: 008577
Test Date: 12/09/2025

Citation Number: M0000000-0
Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Barnes, Simon S

Permit Number: 0014-6221

Effective:

02/01/2025-02/01/2027

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG516203

Exp Date: 06/11/2027

Test	g/210L	Time
DIAG	Pass	4:23pm
AIR BLK	.00	4:24pm
ACCY CHK	.08	4:24pm
AIR BLK	.00	4:26pm
SUB TEST	.00	4:27pm
AIR BLK	.00	4:28pm
SUB TEST	.00	4:29pm
AIR BLK	.00	4:30pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

Intox EC/IR-II: Preventive Maintenance

WAKE COUNTY DETENTION CENTER 910

Serial Number: 008577 Test Record Number: 9310
Test Date: 12/09/2025 Test Time: 4:31pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	4:31pm
FLO	Pass	4:31pm
FC	Pass	4:31pm

Temperature Tests

Test	Status	Time
FC1	Pass	4:31pm
SRC	Pass	4:31pm
DET	Pass	4:31pm
BAR	Pass	4:31pm
BT	Pass	4:31pm

Blank Tests

Test	Status	Time
AIR	Pass	4:32pm

Printer Tests

Test	Status	Time
PRNT	Pass	4:32pm

CRC Tests

Test	Status	Time
COMP	Pass	4:32pm
CAL	Pass	4:32pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County WAKE Instrument Location BAT MOBILE UNIT 10

Instrument Serial No. 008584

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 5 day of November, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

193759
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

WAKE COUNTY BAT MOBILE UNIT 10 910

Serial Number: 008584
Test Date: 12/05/2025

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: Carroll, Barry J
Permit Number: 0019-3759
Effective:
09/01/2025-09/01/2027

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG400303
Exp Date: 01/03/2026

Test	g/210L	Time
DIAG	Pass	10:02pm
AIR BLK	.00	10:03pm
ACCY CHK	.08	10:03pm
AIR BLK	.00	10:04pm
SUB TEST	.00	10:05pm
AIR BLK	.00	10:06pm
SUB TEST	.00	10:07pm
AIR BLK	.00	10:08pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

Intox EC/IR-II: Preventive Maintenance

WAKE COUNTY BAT MOBILE UNIT 10 910

Serial Number: 008584 Test Record Number: 2847
Test Date: 12/05/2025 Test Time: 10:11pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	10:12pm
FLO	Pass	10:12pm
FC	Pass	10:12pm

Temperature Tests

Test	Status	Time
FC1	Pass	10:12pm
SRC	Pass	10:12pm
DET	Pass	10:12pm
BAR	Pass	10:12pm
BT	Pass	10:12pm

Blank Tests

Test	Status	Time
AIR	Pass	10:12pm


Printer Tests

Test	Status	Time
PRNT	Pass	10:13pm

CRC Tests

Test	Status	Time
COMP	Pass	10:13pm
CAL	Pass	10:13pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Wake Instrument Location BAT Mobile Unit 10


Instrument Serial No. 008584

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 20 day of December, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.





Signature of Certifying Official

195759
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

WAKE COUNTY BAT MOBILE UNIT 10 910

Serial Number: 008584
Test Date: 12/20/2025

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE

Analyst's Name: Carroll, Barry J
Permit Number: 0019-3759
Effective:
09/01/2025-09/01/2027

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG400303
Exp Date: 01/03/2026


Test	g/210L	Time
DIAG	Pass	9:29pm
AIR BLK	.00	9:30pm
ACCY CHK	.08	9:31pm
AIR BLK	.00	9:32pm
SUB TEST	.00	9:33pm
AIR BLK	.00	9:33pm
SUB TEST	.00	9:35pm
AIR BLK	.00	9:36pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

Intox EC/IR-II: Preventive Maintenance

WAKE COUNTY BAT MOBILE UNIT 10 910

Serial Number: 008584 Test Record Number: 2853
Test Date: 12/20/2025 Test Time: 9:37pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	9:38pm
FLO	Pass	9:38pm
FC	Pass	9:38pm

Temperature Tests

Test	Status	Time
FC1	Pass	9:38pm
SRC	Pass	9:38pm
DET	Pass	9:38pm
BAR	Pass	9:38pm
BT	Pass	9:38pm

Blank Tests

Test	Status	Time
AIR	Pass	9:39pm

Printer Tests

Test	Status	Time
PRNT	Pass	9:39pm

CRC Tests

Test	Status	Time
COMP	Pass	9:39pm
CAL	Pass	9:39pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County Wake Instrument Location CARY PD
Instrument Serial No. 009557 120 Wilkinson ST Cary, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 15 day of December, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Sam Stokes Braces
Signature of Certifying Official

146221
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

WAKE COUNTY CARY PD 910

Serial Number: 008587
Test Date: 12/15/2025

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Barnes, Simon S

Permit Number: 0014-6221

Effective:

02/01/2025-02/01/2027

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG506303


Exp Date: 03/04/2027

Test	g/210L	Time
DIAG	Pass	8:01am
AIR BLK	.00	8:02am
ACCY CHK	.07	8:03am
AIR BLK	.00	8:04am
SUB TEST	.00	8:05am
AIR BLK	.00	8:06am
SUB TEST	.00	8:07am
AIR BLK	.00	8:08am

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

WAKE COUNTY CARY PD 910

Serial Number: 008587 Test Record Number: 5575
Test Date: 12/15/2025 Test Time: 8:09am EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	8:09am
FLO	Pass	8:09am
FC	Pass	8:09am

Temperature Tests

Test	Status	Time
FC1	Pass	8:09am
SRC	Pass	8:09am
DET	Pass	8:09am
BAR	Pass	8:09am
BT	Pass	8:09am

Blank Tests

Test	Status	Time
AIR	Pass	8:10am


Printer Tests

Test	Status	Time
PRNT	Pass	8:10am

CRC Tests

Test	Status	Time
COMP	Pass	8:10am
CAL	Pass	8:10am

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Wake

Instrument Location Raleigh PD Southwest Dist

Instrument Serial No. 008612

601 Hutton St Raleigh, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 15 day of December, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Simon Stokes Barnes
Signature of Certifying Official

146221
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

WAKE COUNTY SOUTH WEST DISTRICT 910

Serial Number: 008612

Test Date: 12/15/2025

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Barnes, Simon S

Permit Number: 0014-6221

Effective:

02/01/2025-02/01/2027

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG516203

Exp Date: 06/11/2027

Test	g/210L	Time
DIAG	Pass	1:56pm
AIR BLK	.00	1:56pm
ACCY CHK	.07	1:57pm
AIR BLK	.00	1:58pm
SUB TEST	.00	1:59pm
AIR BLK	.00	1:59pm
SUB TEST	.00	2:01pm
AIR BLK	.00	2:02pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

WAKE COUNTY SOUTH WEST DISTRICT 910

Serial Number: 008612 Test Record Number: 5451
Test Date: 12/15/2025 Test Time: 2:04pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	2:04pm
FLO	Pass	2:04pm
FC	Pass	2:04pm

Temperature Tests

Test	Status	Time
FC1	Pass	2:04pm
SRC	Pass	2:04pm
DET	Pass	2:04pm
BAR	Pass	2:04pm
BT	Pass	2:04pm

Blank Tests

Test	Status	Time
AIR	Pass	2:05pm

Printer Tests

Test	Status	Time
PRNT	Pass	2:05pm

CRC Tests

Test	Status	Time
COMP	Pass	2:05pm
CAL	Pass	2:05pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County Wake Instrument Location Apex PD Substation 4
Instrument Serial No. 008621 1615 E. Williams St
Apex, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 15 day of December, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Sam Stokes Barnes
Signature of Certifying Official

146221
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

WAKE COUNTY APEX PD

Serial Number: 008621

Test Date: 12/15/2025

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Barnes, Simon S

Permit Number: 0014-6221

Effective:

02/01/2025-02/01/2027

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG431003

Exp Date: 11/05/2026

Test	g/210L	Time
DIAG	Pass	9:18am
AIR BLK	.00	9:18am
ACCY CHK	.07	9:19am
AIR BLK	.00	9:20am
SUB TEST	.00	9:20am
AIR BLK	.00	9:21am
SUB TEST	.00	9:23am
AIR BLK	.00	9:24am

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

WAKE COUNTY APEX PD

Serial Number: 008621 Test Record Number: 3766
Test Date: 12/15/2025 Test Time: 9:24am EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	9:25am
FLO	Pass	9:25am
FC	Pass	9:25am

Temperature Tests

Test	Status	Time
FC1	Pass	9:25am
SRC	Pass	9:25am
DET	Pass	9:25am
BAR	Pass	9:25am
BT	Pass	9:25am

Blank Tests

Test	Status	Time
AIR	Pass	9:25am

Printer Tests

Test	Status	Time
PRNT	Pass	9:25am

CRC Tests

Test	Status	Time
COMP	Pass	9:26am
CAL	Pass	9:26am

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Wake Instrument Location BAT Mobile Unit 10

Instrument Serial No. 008637

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 5 day of November, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

193759
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

WAKE COUNTY BAT MOBILE UNIT 10 910

Serial Number: 008637
Test Date: 12/05/2025

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: Carroll, Barry J
Permit Number: 0019-3759
Effective:
09/01/2025-09/01/2027

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG400303
Exp Date: 01/03/2026

Test	g/210L	Time
DIAG	Pass	10:14pm
AIR BLK	.00	10:15pm
ACCY CHK	.07	10:15pm
AIR BLK	.00	10:16pm
SUB TEST	.00	10:17pm
AIR BLK	.00	10:18pm
SUB TEST	.00	10:19pm
AIR BLK	.00	10:20pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

WAKE COUNTY BAT MOBILE UNIT 10 910

Serial Number: 008637 Test Record Number: 3568
Test Date: 12/05/2025 Test Time: 10:21pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	10:21pm
FLO	Pass	10:21pm
FC	Pass	10:21pm

Temperature Tests

Test	Status	Time
FC1	Pass	10:21pm
SRC	Pass	10:21pm
DET	Pass	10:21pm
BAR	Pass	10:21pm
BT	Pass	10:21pm

Blank Tests

Test	Status	Time
AIR	Pass	10:22pm

Printer Tests

Test	Status	Time
PRNT	Pass	10:22pm

CRC Tests

Test	Status	Time
COMP	Pass	10:22pm
CAL	Pass	10:22pm

Preventive Maintenance
Status: Pass



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County Wake Instrument Location BAT Mobile Unit 10

Instrument Serial No. 008637

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 20 day of December, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.




Signature of Certifying Official

193759
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

WAKE COUNTY BAT MOBILE UNIT 10 910

Serial Number: 008637
Test Date: 12/20/2025

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE

Analyst's Name: Carroll, Barry J
Permit Number: 0019-3759
Effective:
09/01/2025-09/01/2027

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG400303
Exp Date: 01/03/2026

Test	g/210L	Time
DIAG	Pass	9:44pm
AIR BLK	.00	9:45pm
ACCY CHK	.07	9:46pm
AIR BLK	.00	9:47pm
SUB TEST	.00	9:47pm
AIR BLK	.00	9:48pm
SUB TEST	.00	9:50pm
AIR BLK	.00	9:50pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

Intox EC/IR-II: Preventive Maintenance

WAKE COUNTY BAT MOBILE UNIT 10 910

Serial Number: 008637 Test Record Number: 3571
Test Date: 12/20/2025 Test Time: 9:53pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	9:53pm
FLO	Pass	9:53pm
FC	Pass	9:53pm

Temperature Tests

Test	Status	Time
FC1	Pass	9:53pm
SRC	Pass	9:53pm
DET	Pass	9:53pm
BAR	Pass	9:53pm
BT	Pass	9:53pm

Blank Tests

Test	Status	Time
AIR	Pass	9:54pm

Printer Tests

Test	Status	Time
PRNT	Pass	9:54pm

CRC Tests

Test	Status	Time
COMP	Pass	9:54pm
CAL	Pass	9:54pm

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County Wake Instrument Location BAT mobile unit 10

Instrument Serial No. 008686

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 5 day of November, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

193759
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

WAKE COUNTY BAT MOBILE UNIT 10 910

Serial Number: 008686
Test Date: 12/05/2025

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE

Analyst's Name: Carroll, Barry J
Permit Number: 0019-3759
Effective:
09/01/2025-09/01/2027

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG506302
Exp Date: 03/04/2027

Test	g/210L	Time
DIAG	Pass	10:11pm
AIR BLK	.00	10:12pm
ACCY CHK	.08	10:12pm
AIR BLK	.00	10:13pm
SUB TEST	.00	10:14pm
AIR BLK	.00	10:15pm
SUB TEST	.00	10:16pm
AIR BLK	.00	10:17pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

Intox EC/IR-II: Preventive Maintenance

WAKE COUNTY BAT MOBILE UNIT 10 910

Serial Number: 008686 Test Record Number: 7196
Test Date: 12/05/2025 Test Time: 10:20pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	10:21pm
FLO	Pass	10:21pm
FC	Pass	10:21pm

Temperature Tests

Test	Status	Time
FC1	Pass	10:21pm
SRC	Pass	10:21pm
DET	Pass	10:21pm
BAR	Pass	10:21pm
BT	Pass	10:21pm

Blank Tests

Test	Status	Time
AIR	Pass	10:22pm

Printer Tests

Test	Status	Time
PRNT	Pass	10:22pm

CRC Tests

Test	Status	Time
COMP	Pass	10:22pm
CAL	Pass	10:22pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County Wake Instrument Location BAT Mobile Unit 10
Instrument Serial No. 008686

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 20 day of December, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

193759
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

WAKE COUNTY BAT MOBILE UNIT 10 910

Serial Number: 008686

Test Date: 12/20/2025

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Carroll, Barry J

Permit Number: 0019-3759

Effective:

09/01/2025-09/01/2027

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG506302

Exp Date: 03/04/2027

Test	g/210L	Time
DIAG	Pass	9:46pm
AIR BLK	.00	9:47pm
ACCY CHK	.08	9:47pm
AIR BLK	.00	9:48pm
SUB TEST	.00	9:49pm
AIR BLK	.00	9:50pm
SUB TEST	.00	9:52pm
AIR BLK	.00	9:53pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

Intox EC/IR-II: Preventive Maintenance

WAKE COUNTY BAT MOBILE UNIT 10 910

Serial Number: 008686 Test Record Number: 7198
Test Date: 12/20/2025 Test Time: 9:53pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	9:53pm
FLO	Pass	9:53pm
FC	Pass	9:53pm

Temperature Tests

Test	Status	Time
FC1	Pass	9:53pm
SRC	Pass	9:53pm
DET	Pass	9:53pm
BAR	Pass	9:53pm
BT	Pass	9:53pm

Blank Tests

Test	Status	Time
AIR	Pass	9:54pm

Printer Tests

Test	Status	Time
PRNT	Pass	9:54pm

CRC Tests

Test	Status	Time
COMP	Pass	9:54pm
CAL	Pass	9:54pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County Wake Instrument Location Holly Springs PD
Instrument Serial No. 008757 750 Holly Springs Rd
Holly Springs, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 15 day of December, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Simon Stokes Baucus
Signature of Certifying Official

146221
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

WAKE COUNTY HOLLY SPRINGS PD 910

Serial Number: 008757
Test Date: 12/15/2025

Citation Number: M0000000-0
Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Barnes, Simon S

Permit Number: 0014-6221

Effective:

02/01/2025-02/01/2027

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG516203

Exp Date: 06/11/2027

Test	g/210L	Time
DIAG	Pass	10:06am
AIR BLK	.00	10:07am
ACCY CHK	.08	10:08am
AIR BLK	.00	10:09am
SUB TEST	.00	10:10am
AIR BLK	.00	10:10am
SUB TEST	.00	10:12am
AIR BLK	.00	10:13am

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

Intox EC/IR-II: Preventive Maintenance

WAKE COUNTY HOLLY SPRINGS PD 910

Serial Number: 008757 Test Record Number: 2992
Test Date: 12/15/2025 Test Time: 10:13am EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	10:13am
FLO	Pass	10:13am
FC	Pass	10:13am

Temperature Tests

Test	Status	Time
FC1	Pass	10:14am
SRC	Pass	10:14am
DET	Pass	10:14am
BAR	Pass	10:14am
BT	Pass	10:14am

Blank Tests

Test	Status	Time
AIR	Pass	10:14am


Printer Tests

Test	Status	Time
PRNT	Pass	10:14am

CRC Tests

Test	Status	Time
COMP	Pass	10:14am
CAL	Pass	10:14am

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Wake Instrument Location Wake Co Detention Ctr
Instrument Serial No. 008760 3301 Hammond Rd
Raleigh, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 9 day of December, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Sam Stokes Brasas
Signature of Certifying Official

146221
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

WAKE COUNTY DETENTION CENTER 910

Serial Number: 008760

Test Date: 12/09/2025

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Barnes, Simon S

Permit Number: 0014-6221

Effective:

02/01/2025-02/01/2027

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG516203

Exp Date: 06/11/2027

Test	g/210L	Time
DIAG	Pass	4:26pm
AIR BLK	.00	4:27pm
ACCY CHK	.08	4:27pm
AIR BLK	.00	4:29pm
SUB TEST	.00	4:29pm
AIR BLK	.00	4:30pm
SUB TEST	.00	4:31pm
AIR BLK	.00	4:32pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

Intox EC/IR-II: Preventive Maintenance

WAKE COUNTY DETENTION CENTER 910

Serial Number: 008760 Test Record Number: 7435
Test Date: 12/09/2025 Test Time: 4:34pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	4:34pm
FLO	Pass	4:34pm
FC	Pass	4:34pm

Temperature Tests

Test	Status	Time
FC1	Pass	4:34pm
SRC	Pass	4:34pm
DET	Pass	4:34pm
BAR	Pass	4:34pm
BT	Pass	4:34pm

Blank Tests

Test	Status	Time
AIR	Pass	4:35pm

Printer Tests

Test	Status	Time
PRNT	Pass	4:35pm

CRC Tests

Test	Status	Time
COMP	Pass	4:35pm
CAL	Pass	4:35pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County Wake Instrument Location BAT Mobile Unit 10

Instrument Serial No. 008776

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 5 day of November, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

193759
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

WAKE COUNTY RALEIGH, NC 910

Serial Number: 008776
Test Date: 12/05/2025

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE

Analyst's Name: Carroll, Barry J
Permit Number: 0019-3759
Effective:
09/01/2025-09/01/2027

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG417803
Exp Date: 06/26/2026

Test	g/210L	Time
DIAG	Pass	9:56pm
AIR BLK	.00	9:57pm
ACCY CHK	.08	9:57pm
AIR BLK	.00	9:58pm
SUB TEST	.00	9:59pm
AIR BLK	.00	10:00pm
SUB TEST	.00	10:01pm
AIR BLK	.00	10:02pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

Intox EC/IR-II: Preventive Maintenance

WAKE COUNTY RALEIGH, NC 910

Serial Number: 008776 Test Record Number: 4150
Test Date: 12/05/2025 Test Time: 10:04pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	10:04pm
FLO	Pass	10:04pm
FC	Pass	10:04pm

Temperature Tests

Test	Status	Time
FC1	Pass	10:04pm
SRC	Pass	10:04pm
DET	Pass	10:04pm
BAR	Pass	10:04pm
BT	Pass	10:04pm

Blank Tests

Test	Status	Time
AIR	Pass	10:05pm

Printer Tests

Test	Status	Time
PRNT	Pass	10:05pm

CRC Tests

Test	Status	Time
COMP	Pass	10:05pm
CAL	Pass	10:05pm

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Wake Instrument Location BAT Mobile Unit 10

Instrument Serial No. 009776

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 20 day of December, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

193759
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

WAKE COUNTY BAT MOBILE UNIT 10 910

Serial Number: 008776
Test Date: 12/20/2025

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: Carroll, Barry J
Permit Number: 0019-3759
Effective:
09/01/2025-09/01/2027

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG417803
Exp Date: 06/26/2026


Test	g/210L	Time
DIAG	Pass	9:38pm
AIR BLK	.00	9:39pm
ACCY CHK	.08	9:39pm
AIR BLK	.00	9:40pm
SUB TEST	.00	9:41pm
AIR BLK	.00	9:42pm
SUB TEST	.00	9:44pm
AIR BLK	.00	9:45pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

WAKE COUNTY BAT MOBILE UNIT 10 910

Serial Number: 008776 Test Record Number: 4154
Test Date: 12/20/2025 Test Time: 9:47pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	9:47pm
FLO	Pass	9:47pm
FC	Pass	9:47pm

Temperature Tests

Test	Status	Time
FC1	Pass	9:48pm
SRC	Pass	9:48pm
DET	Pass	9:48pm
BAR	Pass	9:48pm
BT	Pass	9:48pm

Blank Tests

Test	Status	Time
AIR	Pass	9:48pm

Printer Tests

Test	Status	Time
PRNT	Pass	9:48pm

CRC Tests

Test	Status	Time
COMP	Pass	9:48pm
CAL	Pass	9:48pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Wake Instrument Location Wake Co Detention CTR
Instrument Serial No. 008778 3301 Hammond Rd
Raleigh, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 9 day of December, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Erin Stokes Barnes
Signature of Certifying Official

146221
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

WAKE COUNTY DETENTION CENTER 910

Serial Number: 008778
Test Date: 12/09/2025

Citation Number: M0000000-0
Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Barnes, Simon S

Permit Number: 0014-6221

Effective:

02/01/2025-02/01/2027

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG516203

Exp Date: 06/11/2027

Test	g/210L	Time
DIAG	Pass	4:24pm
AIR BLK	.00	4:24pm
ACCY CHK	.07	4:25pm
AIR BLK	.00	4:26pm
SUB TEST	.00	4:29pm
AIR BLK	.00	4:30pm
SUB TEST	.00	4:31pm
AIR BLK	.00	4:32pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

WAKE COUNTY DETENTION CENTER 910

Serial Number: 008778 Test Record Number: 8965
Test Date: 12/09/2025 Test Time: 4:32pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	4:33pm
FLO	Pass	4:33pm
FC	Pass	4:33pm

Temperature Tests

Test	Status	Time
FC1	Pass	4:33pm
SRC	Pass	4:33pm
DET	Pass	4:33pm
BAR	Pass	4:33pm
BT	Pass	4:33pm

Blank Tests

Test	Status	Time
AIR	Pass	4:33pm

Printer Tests

Test	Status	Time
PRNT	Pass	4:34pm

CRC Tests

Test	Status	Time
COMP	Pass	4:34pm
CAL	Pass	4:34pm

Preventive Maintenance
Status: Pass



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County WAKE Instrument Location BAT Mobile Unit 10

Instrument Serial No. 008779

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 5 day of November, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

193759
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

WAKE COUNTY BAT MOBILE UNIT 10 910

Serial Number: 008779
Test Date: 12/05/2025

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: Carroll, Barry J
Permit Number: 0019-3759
Effective:
09/01/2025-09/01/2027

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG431002
Exp Date: 11/05/2026

Test	g/210L	Time
DIAG	Pass	9:59pm
AIR BLK	.00	10:00pm
ACCY CHK	.08	10:00pm
AIR BLK	.00	10:01pm
SUB TEST	.00	10:02pm
AIR BLK	.00	10:03pm
SUB TEST	.00	10:04pm
AIR BLK	.00	10:05pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

Intox EC/IR-II: Preventive Maintenance

WAKE COUNTY BAT MOBILE UNIT 10 910

Serial Number: 008779 Test Record Number: 4095
Test Date: 12/05/2025 Test Time: 10:07pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	10:07pm
FLO	Pass	10:07pm
FC	Pass	10:07pm

Temperature Tests

Test	Status	Time
FC1	Pass	10:07pm
SRC	Pass	10:07pm
DET	Pass	10:07pm
BAR	Pass	10:07pm
BT	Pass	10:07pm

Blank Tests

Test	Status	Time
AIR	Pass	10:08pm

Printer Tests

Test	Status	Time
PRNT	Pass	10:08pm

CRC Tests

Test	Status	Time
COMP	Pass	10:08pm
CAL	Pass	10:08pm

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County WAKE Instrument Location BAT Mobile Unit 10

Instrument Serial No. 008779

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 20 day of December, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

193759
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

WAKE COUNTY BAT MOBILE UNIT 10 910

Serial Number: 008779
Test Date: 12/20/2025

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE

Analyst's Name: *Carroll, Barry J*
Permit Number: 0019-3759
Effective:
09/01/2025-09/01/2027

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: *Breath Test*

Lot Number: AG431002
Exp Date: 11/05/2026

Test	g/210L	Time
DIAG	Pass	9:33pm
AIR BLK	.00	9:34pm
ACCY CHK	.08	9:35pm
AIR BLK	.00	9:36pm
SUB TEST	.00	9:37pm
AIR BLK	.00	9:38pm
SUB TEST	.00	9:39pm
AIR BLK	.00	9:40pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

Intox EC/IR-II: Preventive Maintenance

WAKE COUNTY BAT MOBILE UNIT 10 910

Serial Number: 008779 Test Record Number: 4100
Test Date: 12/20/2025 Test Time: 9:41pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	9:41pm
FLO	Pass	9:41pm
FC	Pass	9:42pm

Temperature Tests

Test	Status	Time
FC1	Pass	9:42pm
SRC	Pass	9:42pm
DET	Pass	9:42pm
BAR	Pass	9:42pm
BT	Pass	9:42pm

Blank Tests

Test	Status	Time
AIR	Pass	9:42pm

Printer Tests

Test	Status	Time
PRNT	Pass	9:42pm

CRC Tests

Test	Status	Time
COMP	Pass	9:43pm
CAL	Pass	9:43pm

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Wake Instrument Location BAR Mobile Unit 13

Instrument Serial No. 008869

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 5th day of December, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Tim B. White
Signature of Certifying Official

307699
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

WAKE COUNTY BAT MOBILE UNIT 13 910

Serial Number: 008869
Test Date: 12/05/2025

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Whitehurst, Timothy B

Permit Number: 0030-7699

Effective:

04/01/2025-04/01/2027

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG417803


Exp Date: 06/26/2026

Test	g/210L	Time
DIAG	Pass	11:06pm
AIR BLK	.00	11:08pm
ACCY CHK	.08	11:08pm
AIR BLK	.00	11:09pm
SUB TEST	.00	11:10pm
AIR BLK	.00	11:10pm
SUB TEST	.00	11:12pm
AIR BLK	.00	11:13pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

Intox EC/IR-II: Preventive Maintenance

WAKE COUNTY BAT MOBILE UNIT 13 910

Serial Number: 008869 Test Record Number: 2141
Test Date: 12/05/2025 Test Time: 11:13pm EST

System Check: Passed

Baseline Tests

Test	Status	Time
IR	Pass	11:14pm
FLO	Pass	11:14pm
FC	Pass	11:14pm

Temperature Tests

Test	Status	Time
FC1	Pass	11:14pm
SRC	Pass	11:14pm
DET	Pass	11:14pm
BAR	Pass	11:14pm
BT	Pass	11:14pm

Blank Tests

Test	Status	Time
AIR	Pass	11:14pm


Printer Tests

Test	Status	Time
PRNT	Pass	11:15pm

CRC Tests

Test	Status	Time
COMP	Pass	11:15pm
CAL	Pass	11:15pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Wake Instrument Location BAT Mobile Unit 13

Instrument Serial No. 008898

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 5th day of December, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Tim B. [Signature]
Signature of Certifying Official

307699
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

WAKE COUNTY BAT MOBILE UNIT 13 910

Serial Number: 008898
Test Date: 12/05/2025

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Whitehurst, Timothy B

Permit Number: 0030-7699

Effective:

04/01/2025-04/01/2027

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG506302


Exp Date: 03/04/2027

Test	g/210L	Time
DIAG	Pass	10:50pm
AIR BLK	.00	10:51pm
ACCY CHK	.07	10:52pm
AIR BLK	.00	10:53pm
SUB TEST	.00	10:54pm
AIR BLK	.00	10:55pm
SUB TEST	.00	10:56pm
AIR BLK	.00	10:57pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

WAKE COUNTY BAT MOBILE UNIT 13 910

Serial Number: 008898 Test Record Number: 2087
Test Date: 12/05/2025 Test Time: 10:59pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	11:00pm
FLO	Pass	11:00pm
FC	Pass	11:00pm

Temperature Tests

Test	Status	Time
FC1	Pass	11:00pm
SRC	Pass	11:00pm
DET	Pass	11:00pm
BAR	Pass	11:00pm
BT	Pass	11:00pm

Blank Tests

Test	Status	Time
AIR	Pass	11:01pm

Printer Tests

Test	Status	Time
PRNT	Pass	11:01pm

CRC Tests

Test	Status	Time
COMP	Pass	11:01pm
CAL	Pass	11:01pm

Preventive Maintenance
Status: Pass



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County Wake Instrument Location Raleigh PD Downtown Dist
Instrument Serial No. 008907 218 W. CABARRUS ST
Raleigh, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 15 day of December, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Erin Stokes Barnes

Signature of Certifying Official

146221

Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

WAKE COUNTY RALEIGH PD DOWNTOWN 910

Serial Number: 008907
Test Date: 12/15/2025

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Barnes, Simon S

Permit Number: 0014-6221

Effective:

02/01/2025-02/01/2027

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG516203

Exp Date: 06/11/2027

Test	g/210L	Time
DIAG	Pass	12:51pm
AIR BLK	.00	12:52pm
ACCY CHK	.08	12:52pm
AIR BLK	.00	12:53pm
SUB TEST	.00	12:54pm
AIR BLK	.00	12:55pm
SUB TEST	.00	12:57pm
AIR BLK	.00	12:58pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

This form is used when performing Preventive Maintenance procedures

Forensic Tests for Alcohol Branch

Department of Health and Human Services

Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

WAKE COUNTY RALEIGH PD DOWNTOWN 910

Serial Number: 008907 Test Record Number: 1700
Test Date: 12/15/2025 Test Time: 12:58pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	12:58pm
FLO	Pass	12:58pm
FC	Pass	12:58pm

Temperature Tests

Test	Status	Time
FC1	Pass	12:59pm
SRC	Pass	12:59pm
DET	Pass	12:59pm
BAR	Pass	12:59pm
BT	Pass	12:59pm

Blank Tests

Test	Status	Time
AIR	Pass	12:59pm

Printer Tests

Test	Status	Time
PRNT	Pass	12:59pm

CRC Tests

Test	Status	Time
COMP	Pass	12:59pm
CAL	Pass	12:59pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Wake Instrument Location BAT Mobile Unit 13

Instrument Serial No. 008939

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 5th day of December, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Timothy B. [Signature]
Signature of Certifying Official

307699
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

WAKE COUNTY BAT MOBILE UNIT 13 910

Serial Number: 008939
Test Date: 12/05/2025

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Whitehurst, Timothy B

Permit Number: 0030-7699

Effective:

04/01/2025-04/01/2027

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG506302

Exp Date: 03/04/2027

Test	g/210L	Time
DIAG	Pass	10:34pm
AIR BLK	.00	10:35pm
ACCY CHK	.07	10:36pm
AIR BLK	.00	10:37pm
SUB TEST	.00	10:38pm
AIR BLK	.00	10:38pm
SUB TEST	.00	10:40pm
AIR BLK	.00	10:41pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

WAKE COUNTY BAT MOBILE UNIT 13 910

Serial Number: 008939 Test Record Number: 1957
Test Date: 12/05/2025 Test Time: 10:41pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	10:42pm
FLO	Pass	10:42pm
FC	Pass	10:42pm

Temperature Tests

Test	Status	Time
FC1	Pass	10:42pm
SRC	Pass	10:42pm
DET	Pass	10:42pm
BAR	Pass	10:42pm
BT	Pass	10:42pm

Blank Tests

Test	Status	Time
AIR	Pass	10:43pm

Printer Tests

Test	Status	Time
PRNT	Pass	10:43pm

CRC Tests

Test	Status	Time
COMP	Pass	10:43pm
CAL	Pass	10:43pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County WARREN Instrument Location WARREN Co. LEC
Instrument Serial No. 008793 128 RAFTERS LANE
WARRENTON, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 22 day of DECEMBER, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

179707
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

WARREN COUNTY WARREN COUNTY JAIL 920

Serial Number: 008793
Test Date: 12/22/2025

Citation Number: M0000000-0
Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Bryant, Earl A

Permit Number: 0017-9707

Effective:

02/01/2025-02/01/2027

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG534301

Exp Date: 12/09/2027


Test	g/210L	Time
DIAG	Pass	4:48pm
AIR BLK	.00	4:48pm
ACCY CHK	.07	4:49pm
AIR BLK	.00	4:50pm
SUB TEST	.00	4:50pm
AIR BLK	.00	4:51pm
SUB TEST	.00	4:53pm
AIR BLK	.00	4:54pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

WARREN COUNTY WARREN COUNTY JAIL 920

Serial Number: 008793 Test Record Number: 2315
Test Date: 12/22/2025 Test Time: 4:55pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	4:55pm
FLO	Pass	4:55pm
FC	Pass	4:55pm

Temperature Tests

Test	Status	Time
FC1	Pass	4:55pm
SRC	Pass	4:55pm
DET	Pass	4:55pm
BAR	Pass	4:55pm
BT	Pass	4:55pm

Blank Tests

Test	Status	Time
AIR	Pass	4:56pm

Printer Tests

Test	Status	Time
PRNT	Pass	4:56pm

CRC Tests

Test	Status	Time
COMP	Pass	4:56pm
CAL	Pass	4:56pm

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County WAYNE Instrument Location BAT MOBILE UNIT 12

Instrument Serial No. 008601

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 10th day of DECEMBER, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

083034
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

WAYNE COUNTY BAT MOBILE UNIT 12 950

Serial Number: 008601
Test Date: 12/12/2025

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name:
Crutchfield, Jr, Marshall B
Permit Number: 0008-3034
Effective:
07/01/2025-07/01/2027

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG501307
Exp Date: 01/13/2027

Test	g/210L	Time
DIAG	Pass	9:03pm
AIR BLK	.00	9:04pm
ACCY CHK	.08	9:05pm
AIR BLK	.00	9:06pm
SUB TEST	.00	9:06pm
AIR BLK	.00	9:07pm
SUB TEST	.00	9:09pm
AIR BLK	.00	9:10pm

Reported AC: .00 g/210L



Signature of Chemical Analyst
Court CVR



Analyst

Intox EC/IR-II: Preventive Maintenance

WAYNE COUNTY BAT MOBILE UNIT 12 950

Serial Number: 008601 Test Record Number: 1858
Test Date: 12/12/2025 Test Time: 9:11pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	9:12pm
FLO	Pass	9:12pm
FC	Pass	9:12pm

Temperature Tests

Test	Status	Time
FC1	Pass	9:12pm
SRC	Pass	9:12pm
DET	Pass	9:12pm
BAR	Pass	9:12pm
BT	Pass	9:12pm

Blank Tests

Test	Status	Time
AIR	Pass	9:13pm

Printer Tests

Test	Status	Time
PRNT	Pass	9:13pm

CRC Tests

Test	Status	Time
COMP	Pass	9:13pm
CAL	Pass	9:13pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Wayne Instrument Location Wayne Co. Detention Center
Instrument Serial No. 008649 200 Stronach Ave., Goldsboro, NC.

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 17th day of December, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Ky...
Signature of Certifying Official

377722
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

WAYNE COUNTY DETENTION CENTER 950

Serial Number: 008649

Test Date: 12/17/2025

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Gray, Kelly D

Permit Number: 0037-7722

Effective:

02/01/2025-02/01/2027

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG516203

Exp Date: 06/11/2027

Test	g/210L	Time
DIAG	Pass	11:13am
AIR BLK	.00	11:14am
ACCY CHK	.08	11:15am
AIR BLK	.00	11:16am
SUB TEST	.00	11:17am
AIR BLK	.00	11:18am
SUB TEST	.00	11:19am
AIR BLK	.00	11:20am

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

WAYNE COUNTY DETENTION CENTER 950

Serial Number: 008649 Test Record Number: 6347
Test Date: 12/17/2025 Test Time: 11:21am EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	11:21am
FLO	Pass	11:21am
FC	Pass	11:21am

Temperature Tests

Test	Status	Time
FC1	Pass	11:22am
SRC	Pass	11:22am
DET	Pass	11:22am
BAR	Pass	11:22am
BT	Pass	11:22am

Blank Tests

Test	Status	Time
AIR	Pass	11:22am


Printer Tests

Test	Status	Time
PRNT	Pass	11:22am

CRC Tests

Test	Status	Time
COMP	Pass	11:22am
CAL	Pass	11:22am

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County WAYNE Instrument Location BAT MOBILE UNIT 12

Instrument Serial No. 008698

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 12th day of December, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Handwritten Signature]

Signature of Certifying Official

083034

Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

WAYNE COUNTY BAT MOBILE UNIT 12 950

Serial Number: 008698
Test Date: 12/12/2025

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name:
Crutchfield, Jr, Marshall B
Permit Number: 0008-3034
Effective:
07/01/2025-07/01/2027

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG400303
Exp Date: 01/03/2026


Test	g/210L	Time
DIAG	Pass	9:22pm
AIR BLK	.00	9:23pm
ACCY CHK	.07	9:24pm
AIR BLK	.00	9:25pm
SUB TEST	.00	9:25pm
AIR BLK	.00	9:26pm
SUB TEST	.00	9:28pm
AIR BLK	.00	9:29pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

WAYNE COUNTY BAT MOBILE UNIT 12 950

Serial Number: 008698 Test Record Number: 2690
Test Date: 12/12/2025 Test Time: 9:30pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	9:30pm
FLO	Pass	9:30pm
FC	Pass	9:30pm

Temperature Tests

Test	Status	Time
FC1	Pass	9:30pm
SRC	Pass	9:30pm
DET	Pass	9:30pm
BAR	Pass	9:30pm
BT	Pass	9:30pm

Blank Tests

Test	Status	Time
AIR	Pass	9:31pm


Printer Tests

Test	Status	Time
PRNT	Pass	9:31pm

CRC Tests

Test	Status	Time
COMP	Pass	9:31pm
CAL	Pass	9:31pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County WAYNE Instrument Location BAT MOBILE UNIT 12

Instrument Serial No. 008788

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 12th day of December, 20 25 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.




Signature of Certifying Official

083034
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

WAYNE COUNTY BAT MOBILE UNIT 12 950

Serial Number: 008788
Test Date: 12/12/2025

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name:
Crutchfield, Jr, Marshall B
Permit Number: 0008-3034
Effective:
07/01/2025-07/01/2027

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AC417802
Exp Date: 06/26/2026

Test	g/210L	Time
DIAG	Pass	9:37pm
AIR BLK	.00	9:38pm
ACCY CHK	.08	9:38pm
AIR BLK	.00	9:39pm
SUB TEST	.00	9:40pm
AIR BLK	.00	9:41pm
SUB TEST	.00	9:42pm
AIR BLK	.00	9:43pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

WAYNE COUNTY BAT MOBILE UNIT 12 950

Serial Number: 008788 Test Record Number: 2489
Test Date: 12/12/2025 Test Time: 9:50pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	9:51pm
FLO	Pass	9:51pm
FC	Pass	9:51pm

Temperature Tests

Test	Status	Time
FC1	Pass	9:51pm
SRC	Pass	9:51pm
DET	Pass	9:51pm
BAR	Pass	9:51pm
BT	Pass	9:51pm

Blank Tests

Test	Status	Time
AIR	Pass	9:52pm

Printer Tests

Test	Status	Time
PRNT	Pass	9:52pm

CRC Tests

Test	Status	Time
COMP	Pass	9:52pm
CAL	Pass	9:52pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Wayne Instrument Location Wayne Co. Detention Center
Instrument Serial No. 008847 200 Stranach Ave., Goldsboro, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 17th day of December, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Key P. [Signature]
Signature of Certifying Official

377722
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

WAYNE COUNTY DETENTION CENTER 950

Serial Number: 008847
Test Date: 12/17/2025

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Gray, Kelly D

Permit Number: 0037-7722

Effective:

02/01/2025-02/01/2027

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG516203

Exp Date: 06/11/2027

Test	g/210L	Time
DIAG	Pass	12:16pm
AIR BLK	.00	12:16pm
ACCY CHK	.07	12:17pm
AIR BLK	.00	12:18pm
SUB TEST	.00	12:18pm
AIR BLK	.00	12:19pm
SUB TEST	.00	12:21pm
AIR BLK	.00	12:22pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

Intox EC/IR-II: Preventive Maintenance

WAYNE COUNTY DETENTION CENTER 950

Serial Number: 008847 Test Record Number: 941
Test Date: 12/17/2025 Test Time: 12:23pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	12:23pm
FLO	Pass	12:23pm
FC	Pass	12:23pm

Temperature Tests

Test	Status	Time
FC1	Pass	12:23pm
SRC	Pass	12:23pm
DET	Pass	12:23pm
BAR	Pass	12:23pm
BT	Pass	12:23pm

Blank Tests

Test	Status	Time
AIR	Pass	12:24pm

Printer Tests

Test	Status	Time
PRNT	Pass	12:24pm

CRC Tests

Test	Status	Time
COMP	Pass	12:24pm
CAL	Pass	12:24pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Wayne Instrument Location Wayne Co. Detention Center
Instrument Serial No. 008879 200 Stronach Ave, Goldsboro, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 17th day of December, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

377722
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

WAYNE COUNTY DETENTION CENTER 950

Serial Number: 008879
Test Date: 12/17/2025

Citation Number: M0000000-0
Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Gray, Kelly D

Permit Number: 0037-7722

Effective:

02/01/2025-02/01/2027

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG516204

Exp Date: 06/11/2027


Test	g/210L	Time
DIAG	Pass	11:47am
AIR BLK	.00	11:48am
ACCY CHK	.08	11:49am
AIR BLK	.00	11:50am
SUB TEST	.00	11:51am
AIR BLK	.00	11:52am
SUB TEST	.00	11:53am
AIR BLK	.00	11:54am

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

WAYNE COUNTY DETENTION CENTER 950

Serial Number: 008879 Test Record Number: 2908
Test Date: 12/17/2025 Test Time: 11:56am EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	11:57am
FLO	Pass	11:57am
FC	Pass	11:57am

Temperature Tests

Test	Status	Time
FC1	Pass	11:57am
SRC	Pass	11:57am
DET	Pass	11:57am
BAR	Pass	11:57am
BT	Pass	11:57am

Blank Tests

Test	Status	Time
AIR	Pass	11:58am

Printer Tests

Test	Status	Time
PRNT	Pass	11:58am

CRC Tests

Test	Status	Time
COMP	Pass	11:58am
CAL	Pass	11:58am

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County WILKES Instrument Location WILKES COUNTY DETENTION

Instrument Serial No. 008843 WILKESBORO, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 19TH day of DECEMBER, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.




Signature of Certifying Official

353799
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

WILKES COUNTY WILKES CO DETENTION 960

Serial Number: 008843

Test Date: 12/19/2025

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Oligmueller, Leo A

Permit Number: 0035-3799

Effective:

02/01/2025-02/01/2027

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG534301

Exp Date: 12/09/2027

Test	g/210L	Time
DIAG	Pass	12:19pm
AIR BLK	.00	12:20pm
ACCY CHK	.08	12:21pm
AIR BLK	.00	12:22pm
SUB TEST	.00	12:22pm
AIR BLK	.00	12:23pm
SUB TEST	.00	12:25pm
AIR BLK	.00	12:26pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

Intox EC/IR-II: Preventive Maintenance

WILKES COUNTY WILKES CO DETENTION 960

Serial Number: 008843 Test Record Number: 3040
Test Date: 12/19/2025 Test Time: 12:26pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	12:27pm
FLO	Pass	12:27pm
FC	Pass	12:27pm

Temperature Tests

Test	Status	Time
FC1	Pass	12:27pm
SRC	Pass	12:27pm
DET	Pass	12:27pm
BAR	Pass	12:27pm
BT	Pass	12:27pm

Blank Tests

Test	Status	Time
AIR	Pass	12:28pm

Printer Tests

Test	Status	Time
PRNT	Pass	12:28pm

CRC Tests

Test	Status	Time
COMP	Pass	12:28pm
CAL	Pass	12:28pm

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County WILKES Instrument Location WILKES COUNTY DETENTION

Instrument Serial No. 008865 WILKESBORO, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus 2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 19TH day of DECEMBER, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.




Signature of Certifying Official

353799
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

WILKES COUNTY WILKES CO DETENTION 960

Serial Number: 008865
Test Date: 12/19/2025

Citation Number: M0000000-0
Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Oligmueller, Leo A

Permit Number: 0035-3799

Effective:

02/01/2025-02/01/2027

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG534301

Exp Date: 12/09/2027

Test	g/210L	Time
DIAG	Pass	12:26pm
AIR BLK	.00	12:26pm
ACCY CHK	.08	12:27pm
AIR BLK	.00	12:28pm
SUB TEST	.00	12:29pm
AIR BLK	.00	12:30pm
SUB TEST	.00	12:32pm
AIR BLK	.00	12:33pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

WILKES COUNTY WILKES CO DETENTION 960

Serial Number: 008865 Test Record Number: 1181
Test Date: 12/19/2025 Test Time: 12:33pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	12:33pm
FLO	Pass	12:33pm
FC	Pass	12:34pm

Temperature Tests

Test	Status	Time
FC1	Pass	12:34pm
SRC	Pass	12:34pm
DET	Pass	12:34pm
BAR	Pass	12:34pm
BT	Pass	12:34pm

Blank Tests

Test	Status	Time
AIR	Pass	12:34pm

Printer Tests

Test	Status	Time
PRNT	Pass	12:34pm

CRC Tests

Test	Status	Time
COMP	Pass	12:35pm
CAL	Pass	12:35pm

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County YADKIN Instrument Location YADKIN COUNTY JAIL
Instrument Serial No. 008854 YADKINVILLE, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 19TH day of DECEMBER, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

353799
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

YADKIN COUNTY YADKIN CO JAIL 980

Serial Number: 008854
Test Date: 12/19/2025

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Oligmueller, Leo A

Permit Number: 0035-3799

Effective:

02/01/2025-02/01/2027

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG534301

Exp Date: 12/09/2027

Test	g/210L	Time
DIAG	Pass	10:40am
AIR BLK	.00	10:41am
ACCY CHK	.08	10:42am
AIR BLK	.00	10:43am
SUB TEST	.00	10:44am
AIR BLK	.00	10:44am
SUB TEST	.00	10:47am
AIR BLK	.00	10:48am

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

Intox EC/IR-II: Preventive Maintenance

YADKIN COUNTY YADKIN CO JAIL 980

Serial Number: 008854 Test Record Number: 1091
Test Date: 12/19/2025 Test Time: 10:49am EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	10:49am
FLO	Pass	10:49am
FC	Pass	10:49am

Temperature Tests

Test	Status	Time
FC1	Pass	10:49am
SRC	Pass	10:49am
DET	Pass	10:49am
BAR	Pass	10:49am
BT	Pass	10:49am

Blank Tests

Test	Status	Time
AIR	Pass	10:50am

Printer Tests

Test	Status	Time
PRNT	Pass	10:50am

CRC Tests

Test	Status	Time
COMP	Pass	10:50am
CAL	Pass	10:50am

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County YADKIN Instrument Location YADKIN COUNTY JAIL
Instrument Serial No. 00 8944 YADKINVILLE, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 19th day of DECEMBER, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.




Signature of Certifying Official

353799
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

YADKIN COUNTY YADKIN CO JAIL 980

Serial Number: 008944
Test Date: 12/19/2025

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Oligmueller, Leo A

Permit Number: 0035-3799

Effective:

02/01/2025-02/01/2027

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG534301

Exp Date: 12/09/2027

Test	g/210L	Time
DIAG	Pass	10:44am
AIR BLK	.00	10:45am
ACCY CHK	.08	10:45am
AIR BLK	.00	10:47am
SUB TEST	.00	10:48am
AIR BLK	.00	10:48am
SUB TEST	.00	10:50am
AIR BLK	.00	10:51am

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

YADKIN COUNTY YADKIN CO JAIL 980

Serial Number: 008944 Test Record Number: 2050
Test Date: 12/19/2025 Test Time: 10:53am EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	10:53am
FLO	Pass	10:53am
FC	Pass	10:54am

Temperature Tests

Test	Status	Time
FC1	Pass	10:54am
SRC	Pass	10:54am
DET	Pass	10:54am
BAR	Pass	10:54am
BT	Pass	10:54am

Blank Tests

Test	Status	Time
AIR	Pass	10:54am

Printer Tests

Test	Status	Time
PRNT	Pass	10:54am

CRC Tests

Test	Status	Time
COMP	Pass	10:55am
CAL	Pass	10:55am

Preventive Maintenance
Status: Pass


Analyst