

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Alamance Instrument Location BAT Mobile Unit 13

Instrument Serial No. 008869

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 28th day of August, 2024 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Timothy B. White
Signature of Certifying Official

307699
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

ALAMANCE COUNTY BAT MOBILE UNIT 13 000

Serial Number: 008869

Test Date: 08/28/2026

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Whitehurst, Timothy B

Permit Number: 0030-7699

Effective:

03/01/2026-03/01/2028

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG506303


Exp Date: 03/04/2027

Test	g/210L	Time
DIAG	Pass	10:21pm
AIR BLK	.00	10:22pm
ACCY CHK	.08	10:23pm
AIR BLK	.00	10:24pm
SUB TEST	.00	10:25pm
AIR BLK	.00	10:25pm
SUB TEST	.00	10:27pm
AIR BLK	.00	10:28pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

Intox EC/IR-II: Preventive Maintenance

ALAMANCE COUNTY BAT MOBILE UNIT 13 000

Serial Number: 008869 Test Record Number: 2282
Test Date: 08/28/2026 Test Time: 10:28pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	10:29pm
FLO	Pass	10:29pm
FC	Pass	10:29pm

Temperature Tests

Test	Status	Time
FC1	Pass	10:29pm
SRC	Pass	10:29pm
DET	Pass	10:29pm
BAR	Pass	10:29pm
BT	Pass	10:29pm

Blank Tests

Test	Status	Time
AIR	Pass	10:29pm

Printer Tests

Test	Status	Time
PRNT	Pass	10:29pm

CRC Tests

Test	Status	Time
COMP	Pass	10:30pm
CAL	Pass	10:30pm

Preventive Maintenance
Status: *Pass*


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Alamance Instrument Location BAT Mobile Unit 13
Instrument Serial No. 008898

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 28th day of August, 20 26 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Tony B. White
Signature of Certifying Official

307699
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

ALAMANCE COUNTY BAT MOBILE UNIT 13 000

Serial Number: 008898

Test Date: 08/28/2026

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Whitehurst, Timothy B

Permit Number: 0030-7699

Effective:

03/01/2026-03/01/2028

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG506302

Exp Date: 03/04/2027

Test	g/210L	Time
DIAG	Pass	9:59pm
AIR BLK	.00	10:00pm
ACCY CHK	.07	10:00pm
AIR BLK	.00	10:01pm
SUB TEST	.00	10:02pm
AIR BLK	.00	10:03pm
SUB TEST	.00	10:04pm
AIR BLK	.00	10:05pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

Intox EC/IR-II: Preventive Maintenance

ALAMANCE COUNTY BAT MOBILE UNIT 13 000

Serial Number: 008898 Test Record Number: 2215
Test Date: 08/28/2026 Test Time: 10:12pm EDT

System Check: Passed

Baseline Tests

Test	Status	Time
IR	Pass	10:13pm
FLO	Pass	10:13pm
FC	Pass	10:13pm

Temperature Tests

Test	Status	Time
FC1	Pass	10:13pm
SRC	Pass	10:13pm
DET	Pass	10:13pm
BAR	Pass	10:13pm
BT	Pass	10:13pm

Blank Tests

Test	Status	Time
AIR	Pass	10:14pm


Printer Tests

Test	Status	Time
PRNT	Pass	10:14pm

CRC Tests

Test	Status	Time
COMP	Pass	10:14pm
CAL	Pass	10:14pm

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Alamance Instrument Location BAT Mobile Unit 13

Instrument Serial No. 008939

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 28th day of August, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Timothy B. [Signature]
Signature of Certifying Official

307699
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

ALAMANCE COUNTY BAT MOBILE UNIT 13 000

Serial Number: 008939

Test Date: 08/28/2026

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Whitehurst, Timothy B

Permit Number: 0030-7699

Effective:

03/01/2026-03/01/2028

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG506302

Exp Date: 03/04/2027

Test	g/210L	Time
DIAG	Pass	9:41pm
AIR BLK	.00	9:42pm
ACCY CHK	.07	9:43pm
AIR BLK	.00	9:44pm
SUB TEST	.00	9:44pm
AIR BLK	.00	9:45pm
SUB TEST	.00	9:47pm
AIR BLK	.00	9:48pm

Reported AC: .00 g/210L

Timothy B Whitehurst
Signature of Chemical Analyst

Court CVR

Timothy B Whitehurst
Analyst

Intox EC/IR-II: Preventive Maintenance

ALAMANCE COUNTY BAT MOBILE UNIT 13 000

Serial Number: 008939 Test Record Number: 2068
Test Date: 08/28/2026 Test Time: 9:48pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	9:48pm
FLO	Pass	9:48pm
FC	Pass	9:49pm

Temperature Tests

Test	Status	Time
FC1	Pass	9:49pm
SRC	Pass	9:49pm
DET	Pass	9:49pm
BAR	Pass	9:49pm
BT	Pass	9:49pm

Blank Tests

Test	Status	Time
AIR	Pass	9:49pm

Printer Tests

Test	Status	Time
PRNT	Pass	9:49pm

CRC Tests

Test	Status	Time
COMP	Pass	9:50pm
CAL	Pass	9:50pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Beaufort Instrument Location Beaufort Co. Courthouse
Instrument Serial No. 008586 Washington, N.C.

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 6th day of August, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Ky P. J.
Signature of Certifying Official

377722
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

BEAUFORT COUNTY COURTHOUSE 060

Serial Number: 008586

Test Date: 08/06/2026

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Gray, Kelly D

Permit Number: 0037-7722

Effective:

02/01/2026-02/01/2028

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG516203

Exp Date: 06/11/2027

Test	g/210L	Time
DIAG	Pass	12:42pm
AIR BLK	.00	12:43pm
ACCY CHK	.07	12:44pm
AIR BLK	.00	12:45pm
SUB TEST	.00	12:45pm
AIR BLK	.00	12:46pm
SUB TEST	.00	12:48pm
AIR BLK	.00	12:49pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

BEAUFORT COUNTY COURTHOUSE 060

Serial Number: 008586 Test Record Number: 2581
Test Date: 08/06/2026 Test Time: 12:50pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	12:50pm
FLO	Pass	12:50pm
FC	Pass	12:51pm

Temperature Tests

Test	Status	Time
FC1	Pass	12:51pm
SRC	Pass	12:51pm
DET	Pass	12:51pm
BAR	Pass	12:51pm
BT	Pass	12:51pm

Blank Tests

Test	Status	Time
AIR	Pass	12:51pm


Printer Tests

Test	Status	Time
PRNT	Pass	12:51pm

CRC Tests

Test	Status	Time
COMP	Pass	12:52pm
CAL	Pass	12:52pm

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County BEAUFORT Instrument Location BAT Mobile Unit 12
Instrument Serial No. 008601

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 8th day of August, 20 26 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

83034
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

BEAUFORT COUNTY BAT MOBILE UNIT 12 060

Serial Number: 008601

Test Date: 08/08/2026

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name:

Crutchfield Jr., Marshall B

Permit Number: 0008-3034

Effective:

03/01/2026-03/01/2028

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG501307

Exp Date: 01/13/2027

Test	g/210L	Time
DIAG	Pass	1:10pm
AIR BLK	.00	1:11pm
ACCY CHK	.07	1:11pm
AIR BLK	.00	1:12pm
SUB TEST	.00	1:13pm
AIR BLK	.00	1:14pm
SUB TEST	.00	1:15pm
AIR BLK	.00	1:16pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

BEAUFORT COUNTY BAT MOBILE UNIT 12 060

Serial Number: 008601 Test Record Number: 1984
Test Date: 08/08/2026 Test Time: 1:17pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	1:17pm
FLO	Pass	1:17pm
FC	Pass	1:17pm

Temperature Tests

Test	Status	Time
FC1	Pass	1:17pm
SRC	Pass	1:17pm
DET	Pass	1:17pm
BAR	Pass	1:17pm
BT	Pass	1:17pm

Blank Tests

Test	Status	Time
AIR	Pass	1:18pm

Printer Tests

Test	Status	Time
PRNT	Pass	1:18pm

CRC Tests

Test	Status	Time
COMP	Pass	1:18pm
CAL	Pass	1:18pm

Preventive Maintenance
Status: *Pass*



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County BEAUFORT Instrument Location BAT Mobile Unit 12

Instrument Serial No. 008698

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 8th day of August, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

83034
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

BEAUFORT COUNTY BAT MOBILE UNIT 12 060

Serial Number: 008698
Test Date: 08/08/2026

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name:

Crutchfield Jr., Marshall B

Permit Number: 0008-3034

Effective:

03/01/2026-03/01/2028

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG431002

Exp Date: 11/05/2026

Test	g/210L	Time
DIAG	Pass	1:17pm
AIR BLK	.00	1:18pm
ACCY CHK	.08	1:19pm
AIR BLK	.00	1:20pm
SUB TEST	.00	1:21pm
AIR BLK	.00	1:21pm
SUB TEST	.00	1:23pm
AIR BLK	.00	1:24pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

BEAUFORT COUNTY BAT MOBILE UNIT 12 060

Serial Number: 008698 Test Record Number: 2836
Test Date: 08/08/2026 Test Time: 1:25pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	1:25pm
FLO	Pass	1:25pm
FC	Pass	1:25pm

Temperature Tests

Test	Status	Time
FC1	Pass	1:25pm
SRC	Pass	1:25pm
DET	Pass	1:25pm
BAR	Pass	1:25pm
BT	Pass	1:25pm

Blank Tests

Test	Status	Time
AIR	Pass	1:26pm

Printer Tests

Test	Status	Time
PRNT	Pass	1:26pm

CRC Tests

Test	Status	Time
COMP	Pass	1:26pm
CAL	Pass	1:26pm

Preventive Maintenance
Status: *Pass*



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County BEAUFORT Instrument Location BAT Mobile Unit 12
Instrument Serial No. 008788

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 8th day of August, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



A handwritten signature in black ink, appearing to be "JFO", written over a horizontal line.

Signature of Certifying Official

83034

Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

BEAUFORT COUNTY BAT MOBILE UNIT 12 060

Serial Number: 008788

Test Date: 08/08/2026

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name:

Crutchfield Jr., Marshall B

Permit Number: 0008-3034

Effective:

03/01/2026-03/01/2028

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG534301

Exp Date: 12/09/2027

Test	g/210L	Time
DIAG	Pass	1:23pm
AIR BLK	.00	1:24pm
ACCY CHK	.07	1:25pm
AIR BLK	.00	1:26pm
SUB TEST	.00	1:26pm
AIR BLK	.00	1:27pm
SUB TEST	.00	1:29pm
AIR BLK	.00	1:30pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

BEAUFORT COUNTY BAT MOBILE UNIT 12 060

Serial Number: 008788 Test Record Number: 2608
Test Date: 08/08/2026 Test Time: 1:31pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	1:32pm
FLO	Pass	1:32pm
FC	Pass	1:32pm

Temperature Tests

Test	Status	Time
FC1	Pass	1:32pm
SRC	Pass	1:32pm
DET	Pass	1:32pm
BAR	Pass	1:32pm
BT	Pass	1:32pm

Blank Tests

Test	Status	Time
AIR	Pass	1:32pm

Printer Tests

Test	Status	Time
PRNT	Pass	1:32pm

CRC Tests

Test	Status	Time
COMP	Pass	1:33pm
CAL	Pass	1:33pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Beaufort Instrument Location Beaufort Co. Courthouse
Instrument Serial No. 008909 Washington, NC.

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 6th day of August, 2020 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

377722

Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

BEAUFORT COUNTY COURTHOUSE 060

Serial Number: 008909

Test Date: 08/06/2026

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Gray, Kelly D

Permit Number: 0037-7722

Effective:

02/01/2026-02/01/2028

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG506303

Exp Date: 03/04/2027

Test	g/210L	Time
DIAG	Pass	12:36pm
AIR BLK	.00	12:37pm
ACCY CHK	.08	12:38pm
AIR BLK	.00	12:39pm
SUB TEST	.00	12:40pm
AIR BLK	.00	12:41pm
SUB TEST	.00	12:42pm
AIR BLK	.00	12:43pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

BEAUFORT COUNTY COURTHOUSE 060

Serial Number: 008909 Test Record Number: 4418
Test Date: 08/06/2026 Test Time: 12:45pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	12:45pm
FLO	Pass	12:45pm
FC	Pass	12:45pm

Temperature Tests

Test	Status	Time
FC1	Pass	12:45pm
SRC	Pass	12:45pm
DET	Pass	12:45pm
BAR	Pass	12:45pm
BT	Pass	12:45pm

Blank Tests

Test	Status	Time
AIR	Pass	12:46pm


Printer Tests

Test	Status	Time
PRNT	Pass	12:46pm

CRC Tests

Test	Status	Time
COMP	Pass	12:46pm
CAL	Pass	12:46pm

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Beaufort Instrument Location Belhaven P.D.
Instrument Serial No. 008928 Belhaven, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 6th day of August, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

377722
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

BEAUFORT COUNTY BELHAVEN PD 060

Serial Number: 008928
Test Date: 08/06/2026

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE

Analyst's Name: Gray, Kelly D
Permit Number: 0037-7722
Effective:
02/01/2026-02/01/2028

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG501303
Exp Date: 01/13/2027

Test	g/210L	Time
DIAG	Pass	9:35am
AIR BLK	.00	9:36am
ACCY CHK	.07	9:36am
AIR BLK	.00	9:37am
SUB TEST	.00	9:38am
AIR BLK	.00	9:39am
SUB TEST	.00	9:40am
AIR BLK	.00	9:41am

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

Intox EC/IR-II: Preventive Maintenance

BEAUFORT COUNTY BELHAVEN PD 060

Serial Number: 008928 Test Record Number: 627
Test Date: 08/06/2026 Test Time: 9:42am EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	9:42am
FLO	Pass	9:42am
FC	Pass	9:43am

Temperature Tests

Test	Status	Time
FC1	Pass	9:43am
SRC	Pass	9:43am
DET	Pass	9:43am
BAR	Pass	9:43am
BT	Pass	9:43am

Blank Tests

Test	Status	Time
AIR	Pass	9:43am

Printer Tests

Test	Status	Time
PRNT	Pass	9:43am

CRC Tests

Test	Status	Time
COMP	Pass	9:44am
CAL	Pass	9:44am

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Brunswick Instrument Location BAT Mobile Unit 13

Instrument Serial No. 008849

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 27th day of August, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Timothy D. White
Signature of Certifying Official

307499
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

BRUNSWICK COUNTY BAT MOBILE UNIT 13
090

Serial Number: 008869
Test Date: 08/27/2026

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Whitehurst, Timothy B

Permit Number: 0030-7699

Effective:

03/01/2026-03/01/2028

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG506303


Exp Date: 03/04/2027

Test	g/210L	Time
DIAG	Pass	8:54pm
AIR BLK	.00	8:55pm
ACCY CHK	.08	8:55pm
AIR BLK	.00	8:56pm
SUB TEST	.00	8:57pm
AIR BLK	.00	8:58pm
SUB TEST	.00	8:59pm
AIR BLK	.00	9:00pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

BRUNSWICK COUNTY BAT MOBILE UNIT 13 090

Serial Number: 008869 Test Record Number: 2279
Test Date: 08/27/2026 Test Time: 9:01pm EDT

System Check: Passed

Baseline Tests

Test	Status	Time
IR	Pass	9:02pm
FLO	Pass	9:02pm
FC	Pass	9:02pm

Temperature Tests

Test	Status	Time
FC1	Pass	9:02pm
SRC	Pass	9:02pm
DET	Pass	9:02pm
BAR	Pass	9:02pm
BT	Pass	9:02pm

Blank Tests

Test	Status	Time
AIR	Pass	9:02pm


Printer Tests

Test	Status	Time
PRNT	Pass	9:03pm

CRC Tests

Test	Status	Time
COMP	Pass	9:03pm
CAL	Pass	9:03pm

**Preventive Maintenance
Status: Pass**



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Brunswick Instrument Location BAT Mobile Unit 13
Instrument Serial No. 008898

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 27th day of August, 2024 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Tony B. Little
Signature of Certifying Official

307699
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

BRUNSWICK COUNTY BAT MOBILE UNIT 13
090

Serial Number: 008898
Test Date: 08/27/2026

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE

Analyst's Name: Whitehurst, Timothy B
Permit Number: 0030-7699
Effective:
03/01/2026-03/01/2028

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG506302
Exp Date: 03/04/2027

Test	g/210L	Time
DIAG	Pass	8:39pm
AIR BLK	.00	8:40pm
ACCY CHK	.07	8:41pm
AIR BLK	.00	8:42pm
SUB TEST	.00	8:43pm
AIR BLK	.00	8:44pm
SUB TEST	.00	8:45pm
AIR BLK	.00	8:46pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

Intox EC/IR-II: Preventive Maintenance

BRUNSWICK COUNTY BAT MOBILE UNIT 13 090

Serial Number: 008898 Test Record Number: 2212
Test Date: 08/27/2026 Test Time: 8:46pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	8:47pm
FLO	Pass	8:47pm
FC	Pass	8:47pm

Temperature Tests

Test	Status	Time
FC1	Pass	8:47pm
SRC	Pass	8:47pm
DET	Pass	8:47pm
BAR	Pass	8:47pm
BT	Pass	8:47pm

Blank Tests

Test	Status	Time
AIR	Pass	8:48pm

Printer Tests

Test	Status	Time
PRNT	Pass	8:48pm

CRC Tests

Test	Status	Time
COMP	Pass	8:48pm
CAL	Pass	8:48pm

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Brunswick Instrument Location BAT Mobile Unit 13

Instrument Serial No. 008939

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 27th day of August, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



T. B. White
Signature of Certifying Official

307499
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

BRUNSWICK COUNTY BAT MOBILE UNIT 13
090

Serial Number: 008939
Test Date: 08/27/2026

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE

Analyst's Name: Whitehurst, Timothy B
Permit Number: 0030-7699
Effective:
03/01/2026-03/01/2028

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG506302
Exp Date: 03/04/2027

Test	g/210L	Time
DIAG	Pass	8:22pm
AIR BLK	.00	8:23pm
ACCY CHK	.07	8:24pm
AIR BLK	.00	8:25pm
SUB TEST	.00	8:25pm
AIR BLK	.00	8:26pm
SUB TEST	.00	8:28pm
AIR BLK	.00	8:29pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

Intox EC/IR-II: Preventive Maintenance

BRUNSWICK COUNTY BAT MOBILE UNIT 13 090

Serial Number: 008939 Test Record Number: 2064
Test Date: 08/27/2026 Test Time: 8:30pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	8:30pm
FLO	Pass	8:30pm
FC	Pass	8:30pm

Temperature Tests

Test	Status	Time
FC1	Pass	8:30pm
SRC	Pass	8:30pm
DET	Pass	8:30pm
BAR	Pass	8:30pm
BT	Pass	8:30pm

Blank Tests

Test	Status	Time
AIR	Pass	8:31pm

Printer Tests

Test	Status	Time
PRNT	Pass	8:31pm

CRC Tests

Test	Status	Time
COMP	Pass	8:31pm
CAL	Pass	8:31pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Buncombe Instrument Location BAT Mobile Unit 13

Instrument Serial No. 008869

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 2nd day of August, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Jeff [Signature]
Signature of Certifying Official

062446
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

BUNCOMBE COUNTY BAT MOBILE UNIT 13 100

Serial Number: 008869

Test Date: 08/02/2026

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Gillstrap, Jeffrey L

Permit Number: 0006-2446

Effective:

03/01/2026-03/01/2028

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG506303

Exp Date: 03/04/2027

Test	g/210L	Time
DIAG	Pass	8:07pm
AIR BLK	.00	8:08pm
ACCY CHK	.08	8:09pm
AIR BLK	.00	8:10pm
SUB TEST	.00	8:10pm
AIR BLK	.00	8:11pm
SUB TEST	.00	8:13pm
AIR BLK	.00	8:14pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

BUNCOMBE COUNTY BAT MOBILE UNIT 13 100

Serial Number: 008869 Test Record Number: 2262
Test Date: 08/02/2026 Test Time: 8:16pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	8:17pm
FLO	Pass	8:17pm
FC	Pass	8:17pm

Temperature Tests

Test	Status	Time
FC1	Pass	8:17pm
SRC	Pass	8:17pm
DET	Pass	8:17pm
BAR	Pass	8:17pm
BT	Pass	8:17pm

Blank Tests

Test	Status	Time
AIR	Pass	8:17pm

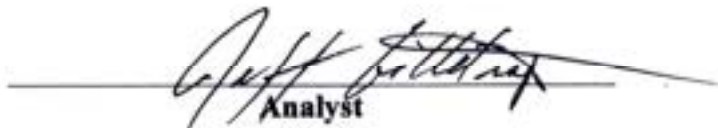
Printer Tests

Test	Status	Time
PRNT	Pass	8:17pm

CRC Tests

Test	Status	Time
COMP	Pass	8:18pm
CAL	Pass	8:18pm

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Buncombe Instrument Location BAT Mobile Unit 13

Instrument Serial No. 008869

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 3rd day of August, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Jeff Bittner
Signature of Certifying Official

062446
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

BUNCOMBE COUNTY BAT MOBILE UNIT 13 100

Serial Number: 008869

Test Date: 08/03/2026

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Gillstrap, Jeffrey L

Permit Number: 0006-2446

Effective:

03/01/2026-03/01/2028

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG506303

Exp Date: 03/04/2027

Test	g/210L	Time
DIAG	Pass	12:03am
AIR BLK	.00	12:04am
ACCY CHK	.08	12:04am
AIR BLK	.00	12:05am
SUB TEST	.00	12:06am
AIR BLK	.00	12:07am
SUB TEST	.00	12:08am
AIR BLK	.00	12:09am

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR

Analyst

Intox EC/IR-II: Preventive Maintenance

BUNCOMBE COUNTY BAT MOBILE UNIT 13 100

Serial Number: 008869 Test Record Number: 2264
Test Date: 08/03/2026 Test Time: 12:10am EDT

System Check: Passed

Baseline Tests

Test	Status	Time
IR	Pass	12:10am
FLO	Pass	12:10am
FC	Pass	12:10am

Temperature Tests

Test	Status	Time
FC1	Pass	12:10am
SRC	Pass	12:10am
DET	Pass	12:10am
BAR	Pass	12:10am
BT	Pass	12:10am

Blank Tests

Test	Status	Time
AIR	Pass	12:11am

Printer Tests

Test	Status	Time
PRNT	Pass	12:11am

CRC Tests

Test	Status	Time
COMP	Pass	12:11am
CAL	Pass	12:11am

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Buncombe Instrument Location BAT Mobile Unit 13
Instrument Serial No. 008869

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 7th day of August, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

062446
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

BUNCOMBE COUNTY BAT MOBILE UNIT 13 100

Serial Number: 008869

Test Date: 08/07/2026

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Gillstrap, Jeffrey L

Permit Number: 0006-2446

Effective:

03/01/2026-03/01/2028

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG506303

Exp Date: 03/04/2027

Test	g/210L	Time
DIAG	Pass	10:53pm
AIR BLK	.00	10:54pm
ACCY CHK	.08	10:55pm
AIR BLK	.00	10:56pm
SUB TEST	.00	10:56pm
AIR BLK	.00	10:57pm
SUB TEST	.00	10:59pm
AIR BLK	.00	11:00pm

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR

Analyst

This form is used when performing Preventive Maintenance procedures

Forensic Tests for Alcohol Branch

Department of Health and Human Services

Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

BUNCOMBE COUNTY BAT MOBILE UNIT 13 100

Serial Number: 008869 Test Record Number: 2269
Test Date: 08/07/2026 Test Time: 11:00pm EDT

System Check: Passed

Baseline Tests

Test	Status	Time
IR	Pass	11:01pm
FLO	Pass	11:01pm
FC	Pass	11:01pm

Temperature Tests

Test	Status	Time
FC1	Pass	11:01pm
SRC	Pass	11:01pm
DET	Pass	11:01pm
BAR	Pass	11:01pm
BT	Pass	11:01pm

Blank Tests

Test	Status	Time
AIR	Pass	11:01pm

Printer Tests

Test	Status	Time
PRNT	Pass	11:02pm

CRC Tests

Test	Status	Time
COMP	Pass	11:02pm
CAL	Pass	11:02pm

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Buncombe Instrument Location BAT Mobile Unit 13

Instrument Serial No. 008869

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 7th day of August, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

062446
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

BUNCOMBE COUNTY BAT MOBILE UNIT 13 100

Serial Number: 008869

Test Date: 08/07/2026

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Gillstrap, Jeffrey L

Permit Number: 0006-2446

Effective:

03/01/2026-03/01/2028

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

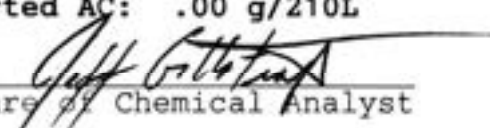
Test Type: Breath Test

Lot Number: AG506303

Exp Date: 03/04/2027

Test	g/210L	Time
DIAG	Pass	8:55pm
AIR BLK	.00	8:56pm
ACCY CHK	.08	8:56pm
AIR BLK	.00	8:57pm
SUB TEST	.00	8:58pm
AIR BLK	.00	8:59pm
SUB TEST	.00	9:02pm
AIR BLK	.00	9:03pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

BUNCOMBE COUNTY BAT MOBILE UNIT 13 100

Serial Number: 008869 Test Record Number: 2267
Test Date: 08/07/2026 Test Time: 9:05pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	9:05pm
FLO	Pass	9:05pm
FC	Pass	9:06pm

Temperature Tests

Test	Status	Time
FC1	Pass	9:06pm
SRC	Pass	9:06pm
DET	Pass	9:06pm
BAR	Pass	9:06pm
BT	Pass	9:06pm

Blank Tests

Test	Status	Time
AIR	Pass	9:06pm

Printer Tests

Test	Status	Time
PRNT	Pass	9:06pm

CRC Tests

Test	Status	Time
COMP	Pass	9:07pm
CAL	Pass	9:07pm

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Buncombe Instrument Location BAT Mobile Unit 13
Instrument Serial No. 008869

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 8th day of August, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

062446
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

BUNCOMBE COUNTY BAT MOBILE UNIT 13 100

Serial Number: 008869

Test Date: 08/08/2026

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Gillstrap, Jeffrey L

Permit Number: 0006-2446

Effective:

03/01/2026-03/01/2028

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

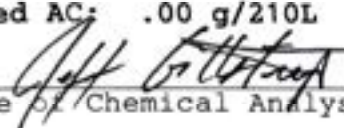
Test Type: Breath Test

Lot Number: AG506303


Exp Date: 03/04/2027

Test	g/210L	Time
DIAG	Pass	11:51pm
AIR BLK	.00	11:52pm
ACCY CHK	.08	11:52pm
AIR BLK	.00	11:53pm
SUB TEST	.00	11:54pm
AIR BLK	.00	11:55pm
SUB TEST	.00	11:56pm
AIR BLK	.00	11:57pm

Reported AC: .00 g/210L

Signature  of Chemical Analyst

Court CVR


Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

BUNCOMBE COUNTY BAT MOBILE UNIT 13 100

Serial Number: 008869 Test Record Number: 2274
Test Date: 08/08/2026 Test Time: 11:58pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	11:58pm
FLO	Pass	11:58pm
FC	Pass	11:58pm

Temperature Tests

Test	Status	Time
FC1	Pass	11:58pm
SRC	Pass	11:58pm
DET	Pass	11:58pm
BAR	Pass	11:58pm
BT	Pass	11:58pm

Blank Tests

Test	Status	Time
AIR	Pass	11:59pm

Printer Tests

Test	Status	Time
PRNT	Pass	11:59pm

CRC Tests

Test	Status	Time
COMP	Pass	11:59pm
CAL	Pass	11:59pm

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Buncombe Instrument Location BAT Mobile Unit 13
Instrument Serial No. 008869

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 8th day of August, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

062446
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

BUNCOMBE COUNTY BAT MOBILE UNIT 13 100

Serial Number: 008869

Test Date: 08/08/2026

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Gillstrap, Jeffrey L

Permit Number: 0006-2446

Effective:

03/01/2026-03/01/2028

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

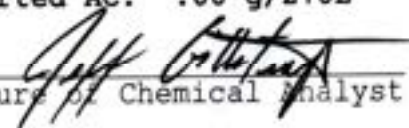
Test Type: Breath Test

Lot Number: AG506303

Exp Date: 03/04/2027

Test	g/210L	Time
DIAG	Pass	6:20pm
AIR BLK	.00	6:21pm
ACCY CHK	.08	6:22pm
AIR BLK	.00	6:23pm
SUB TEST	.00	6:23pm
AIR BLK	.00	6:24pm
SUB TEST	.00	6:26pm
AIR BLK	.00	6:26pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

BUNCOMBE COUNTY BAT MOBILE UNIT 13 100

Serial Number: 008869 Test Record Number: 2272
Test Date: 08/08/2026 Test Time: 6:28pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	6:28pm
FLO	Pass	6:28pm
FC	Pass	6:28pm

Temperature Tests

Test	Status	Time
FC1	Pass	6:28pm
SRC	Pass	6:28pm
DET	Pass	6:28pm
BAR	Pass	6:28pm
BT	Pass	6:28pm

Blank Tests

Test	Status	Time
AIR	Pass	6:29pm

Printer Tests

Test	Status	Time
PRNT	Pass	6:29pm

CRC Tests

Test	Status	Time
COMP	Pass	6:29pm
CAL	Pass	6:29pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Buncombe Instrument Location BAT Mobile Unit 13
Instrument Serial No. 008898

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 2nd day of August, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

062446
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

BUNCOMBE COUNTY BAT MOBILE UNIT 13 100

Serial Number: 008898

Test Date: 08/02/2026

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Gillstrap, Jeffrey L

Permit Number: 0006-2446

Effective:

03/01/2026-03/01/2028

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

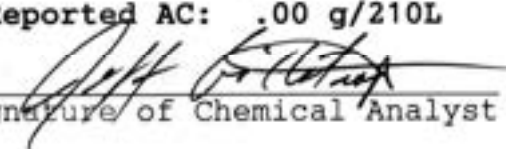
Test Type: Breath Test

Lot Number: AG506302

Exp Date: 03/04/2027

Test	g/210L	Time
DIAG	Pass	8:09pm
AIR BLK	.00	8:10pm
ACCY CHK	.07	8:11pm
AIR BLK	.00	8:12pm
SUB TEST	.00	8:12pm
AIR BLK	.00	8:13pm
SUB TEST	.00	8:15pm
AIR BLK	.00	8:16pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

BUNCOMBE COUNTY BAT MOBILE UNIT 13 100

Serial Number: 008898 Test Record Number: 2195
Test Date: 08/02/2026 Test Time: 8:17pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	8:17pm
FLO	Pass	8:17pm
FC	Pass	8:17pm

Temperature Tests

Test	Status	Time
FC1	Pass	8:17pm
SRC	Pass	8:17pm
DET	Pass	8:17pm
BAR	Pass	8:17pm
BT	Pass	8:17pm

Blank Tests

Test	Status	Time
AIR	Pass	8:18pm

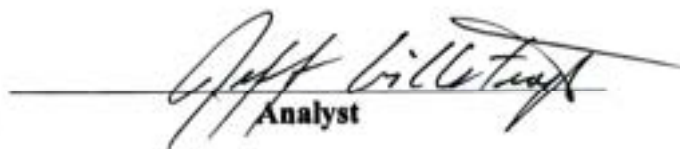
Printer Tests

Test	Status	Time
PRNT	Pass	8:18pm

CRC Tests

Test	Status	Time
COMP	Pass	8:18pm
CAL	Pass	8:18pm

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Buncombe Instrument Location BAT Mobile Unit 13
Instrument Serial No. 008898

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 3rd day of August, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

062446
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

BUNCOMBE COUNTY BAT MOBILE UNIT 13 100

Serial Number: 008898

Test Date: 08/03/2026

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Gillstrap, Jeffrey L

Permit Number: 0006-2446

Effective:

03/01/2026-03/01/2028

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG506302

Exp Date: 03/04/2027

Test	g/210L	Time
DIAG	Pass	12:06am
AIR BLK	.00	12:07am
ACCY CHK	.07	12:07am
AIR BLK	.00	12:08am
SUB TEST	.00	12:09am
AIR BLK	.00	12:10am
SUB TEST	.00	12:11am
AIR BLK	.00	12:12am

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR

Analyst

Intox EC/IR-II: Preventive Maintenance

BUNCOMBE COUNTY BAT MOBILE UNIT 13 100

Serial Number: 008898 Test Record Number: 2197
Test Date: 08/03/2026 Test Time: 12:12am EDT

System Check: Passed

Baseline Tests

Test	Status	Time
IR	Pass	12:13am
FLO	Pass	12:13am
FC	Pass	12:13am

Temperature Tests

Test	Status	Time
FC1	Pass	12:13am
SRC	Pass	12:13am
DET	Pass	12:13am
BAR	Pass	12:13am
BT	Pass	12:13am

Blank Tests

Test	Status	Time
AIR	Pass	12:14am

Printer Tests

Test	Status	Time
PRNT	Pass	12:14am

CRC Tests

Test	Status	Time
COMP	Pass	12:14am
CAL	Pass	12:14am

**Preventive Maintenance
Status: Pass**


Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Buncombe Instrument Location BAT Mobile Unit 13
Instrument Serial No. 008898

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 7th day of August, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

062446
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

BUNCOMBE COUNTY BAT MOBILE UNIT 13 100

Serial Number: 008898

Test Date: 08/07/2026

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Gillstrap, Jeffrey L

Permit Number: 0006-2446

Effective:

03/01/2026-03/01/2028

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG506302

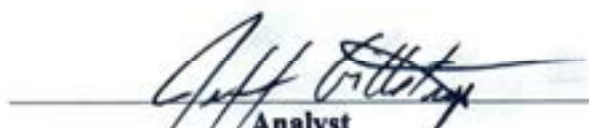
Exp Date: 03/04/2027

Test	g/210L	Time
DIAG	Pass	10:57pm
AIR BLK	.00	10:58pm
ACCY CHK	.07	10:59pm
AIR BLK	.00	11:00pm
SUB TEST	.00	11:01pm
AIR BLK	.00	11:02pm
SUB TEST	.00	11:03pm
AIR BLK	.00	11:04pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

Intox EC/IR-II: Preventive Maintenance

BUNCOMBE COUNTY BAT MOBILE UNIT 13 100

Serial Number: 008898 Test Record Number: 2201
Test Date: 08/07/2026 Test Time: 11:04pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	11:05pm
FLO	Pass	11:05pm
FC	Pass	11:05pm

Temperature Tests

Test	Status	Time
FC1	Pass	11:05pm
SRC	Pass	11:05pm
DET	Pass	11:05pm
BAR	Pass	11:05pm
BT	Pass	11:05pm

Blank Tests

Test	Status	Time
AIR	Pass	11:06pm

Printer Tests

Test	Status	Time
PRNT	Pass	11:06pm

CRC Tests

Test	Status	Time
COMP	Pass	11:06pm
CAL	Pass	11:06pm

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Buncombe Instrument Location BAT Mobile Unit 13
Instrument Serial No. 008898

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 7th day of August, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

062446
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

BUNCOMBE COUNTY BAT MOBILE UNIT 13 100

Serial Number: 008898

Test Date: 08/07/2026

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Gillstrap, Jeffrey L

Permit Number: 0006-2446

Effective:

03/01/2026-03/01/2028

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG506302

Exp Date: 03/04/2027

Test	g/210L	Time
DIAG	Pass	8:58pm
AIR BLK	.00	8:59pm
ACCY CHK	.07	8:59pm
AIR BLK	.00	9:00pm
SUB TEST	.00	9:01pm
AIR BLK	.00	9:02pm
SUB TEST	.00	9:03pm
AIR BLK	.00	9:04pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

BUNCOMBE COUNTY BAT MOBILE UNIT 13 100

Serial Number: 008898 Test Record Number: 2199
Test Date: 08/07/2026 Test Time: 9:05pm EDT

System Check: Passed

Baseline Tests

Test	Status	Time
IR	Pass	9:06pm
FLO	Pass	9:06pm
FC	Pass	9:06pm

Temperature Tests

Test	Status	Time
FC1	Pass	9:06pm
SRC	Pass	9:06pm
DET	Pass	9:06pm
BAR	Pass	9:06pm
BT	Pass	9:06pm

Blank Tests

Test	Status	Time
AIR	Pass	9:07pm

Printer Tests

Test	Status	Time
PRNT	Pass	9:07pm

CRC Tests

Test	Status	Time
COMP	Pass	9:07pm
CAL	Pass	9:07pm

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Buncombe Instrument Location BAT Mobile Unit 13
Instrument Serial No. 008898

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 8th day of August, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Jeff Bittner
Signature of Certifying Official

082446
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

BUNCOMBE COUNTY BAT MOBILE UNIT 13 100

Serial Number: 008898
Test Date: 08/08/2026

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Gillstrap, Jeffrey L

Permit Number: 0006-2446

Effective:

03/01/2026-03/01/2028

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

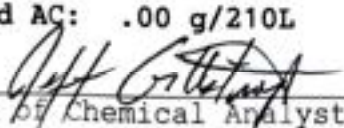
Test Type: Breath Test

Lot Number: AG506302

Exp Date: 03/04/2027

Test	g/210L	Time
DIAG	Pass	11:52pm
AIR BLK	.00	11:53pm
ACCY CHK	.07	11:54pm
AIR BLK	.00	11:55pm
SUB TEST	.00	11:55pm
AIR BLK	.00	11:56pm
SUB TEST	.00	11:58pm
AIR BLK	.00	11:58pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

BUNCOMBE COUNTY BAT MOBILE UNIT 13 100

Serial Number: 008898 Test Record Number: 2205
Test Date: 08/08/2026 Test Time: 11:59pm EDT

System Check: Passed

Baseline Tests

Test	Status	Time
IR	Pass	11:59pm
FLO	Pass	11:59pm
FC	Pass	11:59pm

Temperature Tests

Test	Status	Time
FC1	Pass	12:00am
SRC	Pass	12:00am
DET	Pass	12:00am
BAR	Pass	12:00am
BT	Pass	12:00am

Blank Tests

Test	Status	Time
AIR	Pass	12:00am

Printer Tests

Test	Status	Time
PRNT	Pass	12:00am

CRC Tests

Test	Status	Time
COMP	Pass	12:00am
CAL	Pass	12:00am

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Bamberg Instrument Location BAT Mobile Unit 13
Instrument Serial No. 008898

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 8th day of August, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official
062446
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

BUNCOMBE COUNTY BAT MOBILE UNIT 13 100

Serial Number: 008898

Test Date: 08/08/2026

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Gillstrap, Jeffrey L

Permit Number: 0006-2446

Effective:

03/01/2026-03/01/2028

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG506302

Exp Date: 03/04/2027

Test	g/210L	Time
DIAG	Pass	6:16pm
AIR BLK	.00	6:17pm
ACCY CHK	.07	6:17pm
AIR BLK	.00	6:18pm
SUB TEST	.00	6:19pm
AIR BLK	.00	6:20pm
SUB TEST	.00	6:21pm
AIR BLK	.00	6:22pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

BUNCOMBE COUNTY BAT MOBILE UNIT 13 100

Serial Number: 008898 Test Record Number: 2203
Test Date: 08/08/2026 Test Time: 6:23pm EDT

System Check: Passed

Baseline Tests

Test	Status	Time
IR	Pass	6:23pm
FLO	Pass	6:23pm
FC	Pass	6:23pm

Temperature Tests

Test	Status	Time
FC1	Pass	6:23pm
SRC	Pass	6:23pm
DET	Pass	6:23pm
BAR	Pass	6:23pm
BT	Pass	6:23pm

Blank Tests

Test	Status	Time
AIR	Pass	6:24pm

Printer Tests

Test	Status	Time
PRNT	Pass	6:24pm

CRC Tests

Test	Status	Time
COMP	Pass	6:24pm
CAL	Pass	6:24pm

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Buncombe Instrument Location BAT Mobile Unit 13
Instrument Serial No. 008939

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 2nd day of August, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

062446
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

BUNCOMBE COUNTY BAT MOBILE UNIT 13 100

Serial Number: 008939

Test Date: 08/02/2026

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Gillstrap, Jeffrey L

Permit Number: 0006-2446

Effective:

03/01/2026-03/01/2028

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

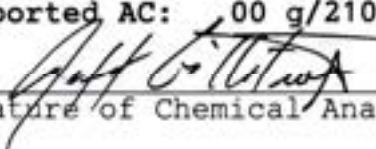
Test Type: Breath Test

Lot Number: AG506302

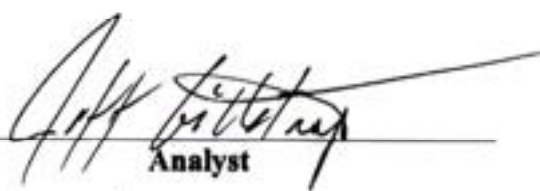
Exp Date: 03/04/2027

Test	g/210L	Time
DIAG	Pass	8:12pm
AIR BLK	.00	8:13pm
ACCY CHK	.07	8:13pm
AIR BLK	.00	8:14pm
SUB TEST	.00	8:15pm
AIR BLK	.00	8:15pm
SUB TEST	.00	8:17pm
AIR BLK	.00	8:18pm

Reported AC: 00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

This form is used when performing Preventive Maintenance procedures

Forensic Tests for Alcohol Branch

Department of Health and Human Services

Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

BUNCOMBE COUNTY BAT MOBILE UNIT 13 100

Serial Number: 008939 Test Record Number: 2050
Test Date: 08/02/2026 Test Time: 8:19pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	8:19pm
FLO	Pass	8:19pm
FC	Pass	8:19pm

Temperature Tests

Test	Status	Time
FC1	Pass	8:19pm
SRC	Pass	8:19pm
DET	Pass	8:19pm
BAR	Pass	8:19pm
BT	Pass	8:19pm

Blank Tests

Test	Status	Time
AIR	Pass	8:20pm

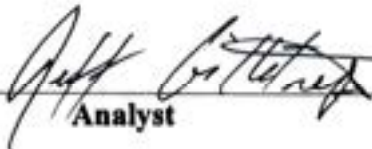
Printer Tests

Test	Status	Time
PRNT	Pass	8:20pm

CRC Tests

Test	Status	Time
COMP	Pass	8:20pm
CAL	Pass	8:20pm

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Buncombe Instrument Location BAT Mobile Unit 13
Instrument Serial No. 008939

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 3rd day of August, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Jeff Gittling
Signature of Certifying Official

062446
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

BUNCOMBE COUNTY BAT MOBILE UNIT 13 100

Serial Number: 008939
Test Date: 08/03/2026

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Gillstrap, Jeffrey L

Permit Number: 0006-2446

Effective:

03/01/2026-03/01/2028

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

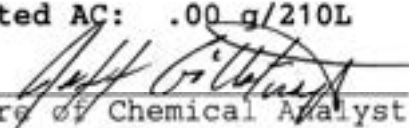
Test Type: Breath Test

Lot Number: AG506302

Exp Date: 03/04/2027

Test	g/210L	Time
DIAG	Pass	12:08am
AIR BLK	.00	12:09am
ACCY CHK	.07	12:09am
AIR BLK	.00	12:10am
SUB TEST	.00	12:11am
AIR BLK	.00	12:12am
SUB TEST	.00	12:13am
AIR BLK	.00	12:14am

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

BUNCOMBE COUNTY BAT MOBILE UNIT 13 100

Serial Number: 008939 Test Record Number: 2052
Test Date: 08/03/2026 Test Time: 12:16am EDT

System Check: Passed

Baseline Tests

Test	Status	Time
IR	Pass	12:16am
FLO	Pass	12:16am
FC	Pass	12:16am

Temperature Tests

Test	Status	Time
FC1	Pass	12:16am
SRC	Pass	12:16am
DET	Pass	12:16am
BAR	Pass	12:16am
BT	Pass	12:16am

Blank Tests

Test	Status	Time
AIR	Pass	12:17am

Printer Tests

Test	Status	Time
PRNT	Pass	12:17am

CRC Tests

Test	Status	Time
COMP	Pass	12:17am
CAL	Pass	12:17am

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Buncombe Instrument Location BAT Mobile Unit 13
Instrument Serial No 008939

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 7th day of August, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Jeff G. [Signature]
Signature of Certifying Official

062446
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

BUNCOMBE COUNTY BAT MOBILE UNIT 13 100

Serial Number: 008939

Test Date: 08/07/2026

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Gillstrap, Jeffrey L

Permit Number: 0006-2446

Effective:

03/01/2026-03/01/2028

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG506302

Exp Date: 03/04/2027

Test	g/210L	Time
DIAG	Pass	10:59pm
AIR BLK	.00	11:00pm
ACCY CHK	.07	11:01pm
AIR BLK	.00	11:02pm
SUB TEST	.00	11:02pm
AIR BLK	.00	11:03pm
SUB TEST	.00	11:06pm
AIR BLK	.00	11:06pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

BUNCOMBE COUNTY BAT MOBILE UNIT 13 100

Serial Number: 008939 Test Record Number: 2056
Test Date: 08/07/2026 Test Time: 11:07pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	11:07pm
FLO	Pass	11:07pm
FC	Pass	11:07pm

Temperature Tests

Test	Status	Time
FC1	Pass	11:08pm
SRC	Pass	11:08pm
DET	Pass	11:08pm
BAR	Pass	11:08pm
BT	Pass	11:08pm

Blank Tests

Test	Status	Time
AIR	Pass	11:08pm

Printer Tests

Test	Status	Time
PRNT	Pass	11:08pm

CRC Tests

Test	Status	Time
COMP	Pass	11:08pm
CAL	Pass	11:08pm

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Buncombe Instrument Location BAT Mobile Unit 13

Instrument Serial No. 008939

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 7th day of August, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

062446
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

BUNCOMBE COUNTY BAT MOBILE UNIT 13 100

Serial Number: 008939

Test Date: 08/07/2026

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Gillstrap, Jeffrey L

Permit Number: 0006-2446

Effective:

03/01/2026-03/01/2028

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

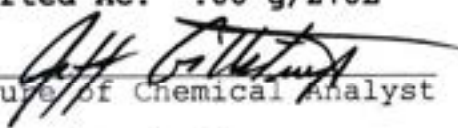
Test Type: Breath Test

Lot Number: AG506302


Exp Date: 03/04/2027

Test	g/210L	Time
DIAG	Pass	9:01pm
AIR BLK	.00	9:02pm
ACCY CHK	.07	9:03pm
AIR BLK	.00	9:04pm
SUB TEST	.00	9:04pm
AIR BLK	.00	9:05pm
SUB TEST	.00	9:07pm
AIR BLK	.00	9:08pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

Intox EC/IR-II: Preventive Maintenance

BUNCOMBE COUNTY BAT MOBILE UNIT 13 100

Serial Number: 008939 Test Record Number: 2054
Test Date: 08/07/2026 Test Time: 9:10pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	9:10pm
FLO	Pass	9:10pm
FC	Pass	9:10pm

Temperature Tests

Test	Status	Time
FC1	Pass	9:10pm
SRC	Pass	9:10pm
DET	Pass	9:10pm
BAR	Pass	9:10pm
BT	Pass	9:10pm

Blank Tests

Test	Status	Time
AIR	Pass	9:11pm

Printer Tests

Test	Status	Time
PRNT	Pass	9:11pm

CRC Tests

Test	Status	Time
COMP	Pass	9:11pm
CAL	Pass	9:11pm

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Buncombe Instrument Location BAT Mobile Unit 13
Instrument Serial No. 008939

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 8th day of August, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

062446
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

BUNCOMBE COUNTY BAT MOBILE UNIT 13 100

Serial Number: 008939

Test Date: 08/08/2026

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Gillstrap, Jeffrey L

Permit Number: 0006-2446

Effective:

03/01/2026-03/01/2028

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

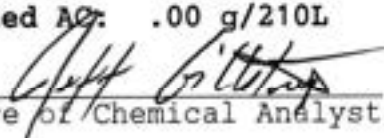
Test Type: Breath Test

Lot Number: AG506302

Exp Date: 03/04/2027

Test	g/210L	Time
DIAG	Pass	11:53pm
AIR BLK	.00	11:54pm
ACCY CHK	.07	11:55pm
AIR BLK	.00	11:56pm
SUB TEST	.00	11:56pm
AIR BLK	.00	11:57pm
SUB TEST	.00	11:59pm
AIR BLK	.00	12:00am

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

BUNCOMBE COUNTY BAT MOBILE UNIT 13 100

Serial Number: 008939 Test Record Number: 2060
Test Date: 08/09/2026 Test Time: 12:03am EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	12:03am
FLO	Pass	12:03am
FC	Pass	12:03am

Temperature Tests

Test	Status	Time
FC1	Pass	12:03am
SRC	Pass	12:03am
DET	Pass	12:03am
BAR	Pass	12:03am
BT	Pass	12:03am

Blank Tests

Test	Status	Time
AIR	Pass	12:04am

Printer Tests

Test	Status	Time
PRNT	Pass	12:04am

CRC Tests

Test	Status	Time
COMP	Pass	12:04am
CAL	Pass	12:04am

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Bancroft Instrument Location BAT Mobile Unit 13
Instrument Serial No. 008939

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 8th day of August, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Officer

062446
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

BUNCOMBE COUNTY BAT MOBILE UNIT 13 100

Serial Number: 008939

Test Date: 08/08/2026

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Gillstrap, Jeffrey L

Permit Number: 0006-2446

Effective:

03/01/2026-03/01/2028

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

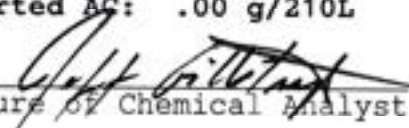
Test Type: Breath Test

Lot Number: AG506302

Exp Date: 03/04/2027

Test	g/210L	Time
DIAG	Pass	6:18pm
AIR BLK	.00	6:19pm
ACCY CHK	.07	6:19pm
AIR BLK	.00	6:20pm
SUB TEST	.00	6:21pm
AIR BLK	.00	6:22pm
SUB TEST	.00	6:23pm
AIR BLK	.00	6:24pm

Reported AG: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

BUNCOMBE COUNTY BAT MOBILE UNIT 13 100

Serial Number: 008939 Test Record Number: 2058
Test Date: 08/08/2026 Test Time: 6:25pm EDT

System Check: Passed

Baseline Tests

Test	Status	Time
IR	Pass	6:25pm
FLO	Pass	6:25pm
FC	Pass	6:25pm

Temperature Tests

Test	Status	Time
FC1	Pass	6:25pm
SRC	Pass	6:25pm
DET	Pass	6:25pm
BAR	Pass	6:25pm
BT	Pass	6:25pm

Blank Tests

Test	Status	Time
AIR	Pass	6:26pm

Printer Tests

Test	Status	Time
PRNT	Pass	6:26pm

CRC Tests

Test	Status	Time
COMP	Pass	6:26pm
CAL	Pass	6:26pm

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Burke Instrument Location Burke County Jail
Instrument Serial No. 008831 Morganton, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 19 day of August, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.





Signature of Certifying Official

244987

Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

BURKE COUNTY BURKE COUNTY JAIL 110

Serial Number: 008831

Test Date: 08/19/2026

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Loftis, Benjamin C

Permit Number: 0024-4987

Effective:

02/01/2026-02/01/2028

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

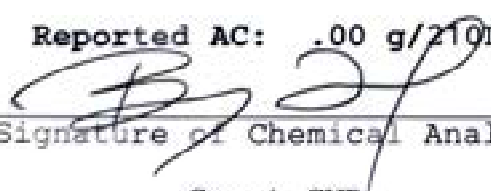
Test Type: Breath Test

Lot Number: AG602101

Exp Date: 01/21/2028

Test	g/210L	Time
DIAG	Pass	9:17am
AIR BLK	.00	9:18am
ACCY CHK	.08	9:19am
AIR BLK	.00	9:20am
SUB TEST	.00	9:20am
AIR BLK	.00	9:21am
SUB TEST	.00	9:23am
AIR BLK	.00	9:24am

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

BURKE COUNTY BURKE COUNTY JAIL 110

Serial Number: 008831

Test Record Number: 3296

Test Date: 08/19/2026

Test Time: 9:24am EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	9:24am
FLO	Pass	9:24am
FC	Pass	9:24am

Temperature Tests

Test	Status	Time
FC1	Pass	9:24am
SRC	Pass	9:24am
DET	Pass	9:24am
BAR	Pass	9:24am
BT	Pass	9:24am

Blank Tests

Test	Status	Time
AIR	Pass	9:25am

Printer Tests

Test	Status	Time
PRNT	Pass	9:25am

CRC Tests

Test	Status	Time
COMP	Pass	9:25am
CAL	Pass	9:25am

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

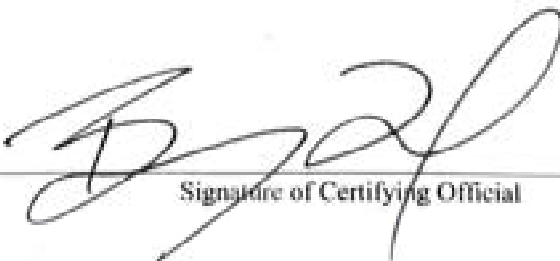
County Burke Instrument Location Burke County Jail
Instrument Serial No. 008904 Morganton, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 19 day of August, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.




Signature of Certifying Official

244787
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

BURKE COUNTY BURKE COUNTY JAIL 110

Serial Number: 008904

Test Date: 08/19/2026

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Loftis, Benjamin C

Permit Number: 0024-4987

Effective:

02/01/2026-02/01/2028

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

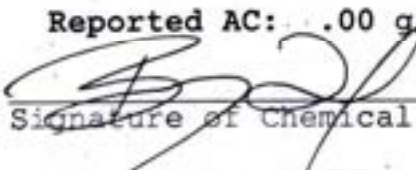
Test Type: Breath Test

Lot Number: AG602101

Exp Date: 01/21/2028

Test	g/210L	Time
DIAG	Pass	9:18am
AIR BLK	.00	9:19am
ACCY CHK	.08	9:20am
AIR BLK	.00	9:21am
SUB TEST	.00	9:21am
AIR BLK	.00	9:22am
SUB TEST	.00	9:24am
AIR BLK	.00	9:24am

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

BURKE COUNTY BURKE COUNTY JAIL 110

Serial Number: 008904 Test Record Number: 3762
Test Date: 08/19/2026 Test Time: 9:25am EDT

System Check: Passed

Baseline Tests

Test	Status	Time
IR	Pass	9:25am
FLO	Pass	9:25am
FC	Pass	9:25am

Temperature Tests

Test	Status	Time
FC1	Pass	9:25am
SRC	Pass	9:25am
DET	Pass	9:25am
BAR	Pass	9:25am
BT	Pass	9:25am

Blank Tests

Test	Status	Time
AIR	Pass	9:26am

Printer Tests

Test	Status	Time
PRNT	Pass	9:26am

CRC Tests

Test	Status	Time
COMP	Pass	9:26am
CAL	Pass	9:26am

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Cabarrus Instrument Location Cabarrus County 80
Instrument Serial No. 008590 Concord, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 19th day of August, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Bryon Helms
Signature of Certifying Official

849845
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

CABARRUS COUNTY CABARRUS COUNTY SO 120

Serial Number: 008590

Test Date: 08/19/2026

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Helms, Bryce A

Permit Number: 0084-9845

Effective:

02/01/2026-02/01/2028

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG602202

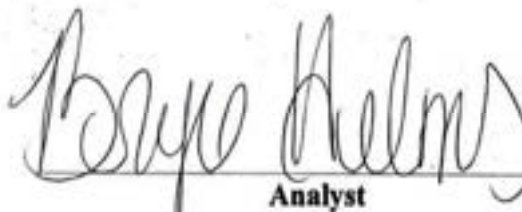
Exp Date: 01/22/2028

Test	g/210L	Time
DIAG	Pass	2:39pm
AIR BLK	.00	2:39pm
ACCY CHK	.08	2:40pm
AIR BLK	.00	2:41pm
SUB TEST	.00	2:42pm
AIR BLK	.00	2:43pm
SUB TEST	.00	2:44pm
AIR BLK	.00	2:46pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

CABARRUS COUNTY CABARRUS COUNTY SO 120

Serial Number: 008590 Test Record Number: 6152
Test Date: 08/19/2026 Test Time: 2:46pm EDT

System Check: Passed

Baseline Tests

Test	Status	Time
IR	Pass	2:46pm
FLO	Pass	2:46pm
FC	Pass	2:47pm

Temperature Tests

Test	Status	Time
FC1	Pass	2:47pm
SRC	Pass	2:47pm
DET	Pass	2:47pm
BAR	Pass	2:47pm
BT	Pass	2:47pm

Blank Tests

Test	Status	Time
AIR	Pass	2:47pm

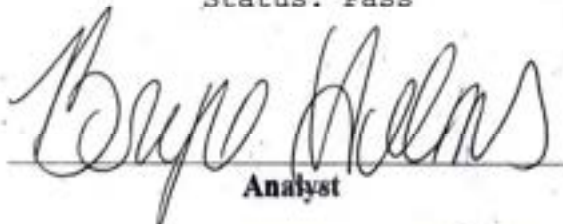
Printer Tests

Test	Status	Time
PRNT	Pass	2:47pm

CRC Tests

Test	Status	Time
COMP	Pass	2:48pm
CAL	Pass	2:48pm

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Cabarrus Instrument Location BAT Mobile Unit 8
Instrument Serial No. 008615 —

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 17 day of August, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

2219283
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

CABARRUS COUNTY BAT MOBILE UNIT 8 120

Serial Number: 008615

Test Date: 08/17/2026

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Glasscock, Jerry D

Permit Number: 7180-9235

Effective:

02/01/2026-02/01/2028

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG506303


Exp Date: 03/04/2027

Test	g/210L	Time
DIAG	Pass	7:08am
AIR BLK	.00	7:09am
ACCY CHK	.07	7:09am
AIR BLK	.00	7:10am
SUB TEST	.00	7:11am
AIR BLK	.00	7:12am
SUB TEST	.00	7:13am
AIR BLK	.00	7:14am

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

This form is used when performing Preventive Maintenance procedures

Forensic Tests for Alcohol Branch

Department of Health and Human Services

Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

CABARRUS COUNTY BAT MOBILE UNIT 8 120

Serial Number: 008615 Test Record Number: 6385
Test Date: 08/17/2026 Test Time: 7:14am EDT

System Check: Passed

Baseline Tests

Test	Status	Time
IR	Pass	7:15am
FLO	Pass	7:15am
FC	Pass	7:15am

Temperature Tests

Test	Status	Time
FC1	Pass	7:15am
SRC	Pass	7:15am
DET	Pass	7:15am
BAR	Pass	7:15am
BT	Pass	7:15am

Blank Tests

Test	Status	Time
AIR	Pass	7:15am

Printer Tests

Test	Status	Time
PRNT	Pass	7:16am

CRC Tests

Test	Status	Time
COMP	Pass	7:16am
CAL	Pass	7:16am

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Cabarrus Instrument Location BAT Mobile Unit 8
Instrument Serial No. 008615

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 24 day of August, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

2219283
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

CABARRUS COUNTY BAT MOBILE UNIT 8 120

Serial Number: 008615

Test Date: 08/24/2026

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Glasscock, Jerry D

Permit Number: 7180-9235

Effective:

02/01/2026-02/01/2028

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG506303


Exp Date: 03/04/2027

Test	g/210L	Time
DIAG	Pass	2:40pm
AIR BLK	.00	2:41pm
ACCY CHK	.07	2:42pm
AIR BLK	.00	2:43pm
SUB TEST	.00	2:44pm
AIR BLK	.00	2:44pm
SUB TEST	.00	2:46pm
AIR BLK	.00	2:47pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

CABARRUS COUNTY BAT MOBILE UNIT 8 120

Serial Number: 008615 Test Record Number: 6398
Test Date: 08/24/2026 Test Time: 2:47pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	2:48pm
FLO	Pass	2:48pm
FC	Pass	2:48pm

Temperature Tests

Test	Status	Time
FC1	Pass	2:48pm
SRC	Pass	2:48pm
DET	Pass	2:48pm
BAR	Pass	2:48pm
BT	Pass	2:48pm

Blank Tests

Test	Status	Time
AIR	Pass	2:48pm

Printer Tests

Test	Status	Time
PRNT	Pass	2:49pm

CRC Tests

Test	Status	Time
COMP	Pass	2:49pm
CAL	Pass	2:49pm

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Cabarrus Instrument Location BAT Mobile Unit 8
Instrument Serial No. 008736

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 17 day of August, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

2219283
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

CABARRUS COUNTY BAT MOBILE UNIT 8 120

Serial Number: 008736

Test Date: 08/17/2026

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Glasscock, Jerry D

Permit Number: 7180-9235

Effective:

02/01/2026-02/01/2028

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG506303

Exp Date: 03/04/2027

Test	g/210L	Time
DIAG	Pass	7:06am
AIR BLK	.00	7:08am
ACCY CHK	.07	7:08am
AIR BLK	.00	7:09am
SUB TEST	.00	7:10am
AIR BLK	.00	7:11am
SUB TEST	.00	7:13am
AIR BLK	.00	7:14am

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

CABARRUS COUNTY BAT MOBILE UNIT 8 120

Serial Number: 008736 Test Record Number: 1735
Test Date: 08/17/2026 Test Time: 7:14am EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	7:14am
FLO	Pass	7:14am
FC	Pass	7:15am

Temperature Tests

Test	Status	Time
FC1	Pass	7:15am
SRC	Pass	7:15am
DET	Pass	7:15am
BAR	Pass	7:15am
BT	Pass	7:15am

Blank Tests

Test	Status	Time
AIR	Pass	7:15am

Printer Tests

Test	Status	Time
PRNT	Pass	7:15am

CRC Tests

Test	Status	Time
COMP	Pass	7:15am
CAL	Pass	7:15am

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Cabarrus Instrument Location BAT Mobile Unit 8

Instrument Serial No. 008736

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 24 day of August, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

2219283
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

CABARRUS COUNTY BAT MOBILE UNIT 8 120

Serial Number: 008736

Test Date: 08/24/2026

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Glasscock, Jerry D

Permit Number: 7180-9235

Effective:

02/01/2026-02/01/2028

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG506303


Exp Date: 03/04/2027

Test	g/210L	Time
DIAG	Pass	2:41pm
AIR BLK	.00	2:42pm
ACCY CHK	.07	2:43pm
AIR BLK	.00	2:44pm
SUB TEST	.00	2:44pm
AIR BLK	.00	2:45pm
SUB TEST	.00	2:47pm
AIR BLK	.00	2:48pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

CABARRUS COUNTY BAT MOBILE UNIT 8 120

Serial Number: 008736 Test Record Number: 1746
Test Date: 08/24/2026 Test Time: 2:48pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	2:48pm
FLO	Pass	2:48pm
FC	Pass	2:48pm

Temperature Tests

Test	Status	Time
FC1	Pass	2:49pm
SRC	Pass	2:49pm
DET	Pass	2:49pm
BAR	Pass	2:49pm
BT	Pass	2:49pm

Blank Tests

Test	Status	Time
AIR	Pass	2:49pm

Printer Tests

Test	Status	Time
PRNT	Pass	2:49pm

CRC Tests

Test	Status	Time
COMP	Pass	2:49pm
CAL	Pass	2:49pm

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Cabarrus Instrument Location BAT Mobile Unit 8
Instrument Serial No. 008775 —

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 17 day of August, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

2219283
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

CABARRUS COUNTY BAT MOBILE UNIT 8 120

Serial Number: 008775

Test Date: 08/17/2026

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Glasscock, Jerry D

Permit Number: 7180-9235

Effective:

02/01/2026-02/01/2028

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG506303

Exp Date: 03/04/2027

Test	g/210L	Time
DIAG	Pass	7:05am
AIR BLK	.00	7:06am
ACCY CHK	.08	7:07am
AIR BLK	.00	7:08am
SUB TEST	.00	7:09am
AIR BLK	.00	7:10am
SUB TEST	.00	7:11am
AIR BLK	.00	7:12am

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

CABARRUS COUNTY BAT MOBILE UNIT 8 120

Serial Number: 008775 Test Record Number: 2601
Test Date: 08/17/2026 Test Time: 7:12am EDT

System Check: Passed

Baseline Tests

Test	Status	Time
IR	Pass	7:13am
FLO	Pass	7:13am
FC	Pass	7:13am

Temperature Tests

Test	Status	Time
FC1	Pass	7:13am
SRC	Pass	7:13am
DET	Pass	7:13am
BAR	Pass	7:13am
BT	Pass	7:13am

Blank Tests

Test	Status	Time
AIR	Pass	7:14am

Printer Tests

Test	Status	Time
PRNT	Pass	7:14am

CRC Tests

Test	Status	Time
COMP	Pass	7:14am
CAL	Pass	7:14am

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Cabarrus Instrument Location BAT Mobile Unit 8
Instrument Serial No. 008775 —

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 24 day of August, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

2219283
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

CABARRUS COUNTY BAT MOBILE UNIT 8 120

Serial Number: 008775

Test Date: 08/24/2026

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Glasscock, Jerry D

Permit Number: 7180-9235

Effective:

02/01/2026-02/01/2028

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

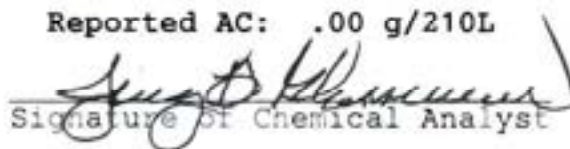
Test Type: Breath Test

Lot Number: AG506303

Exp Date: 03/04/2027

Test	g/210L	Time
DIAG	Pass	2:42pm
AIR BLK	.00	2:43pm
ACCY CHK	.08	2:44pm
AIR BLK	.00	2:45pm
SUB TEST	.00	2:45pm
AIR BLK	.00	2:46pm
SUB TEST	.00	2:47pm
AIR BLK	.00	2:48pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

CABARRUS COUNTY BAT MOBILE UNIT 8 120

Serial Number: 008775 Test Record Number: 2614
Test Date: 08/24/2026 Test Time: 2:49pm EDT

System Check: Passed

Baseline Tests

Test	Status	Time
IR	Pass	2:49pm
FLO	Pass	2:49pm
FC	Pass	2:49pm

Temperature Tests

Test	Status	Time
FC1	Pass	2:49pm
SRC	Pass	2:49pm
DET	Pass	2:49pm
BAR	Pass	2:49pm
BT	Pass	2:49pm

Blank Tests

Test	Status	Time
AIR	Pass	2:50pm

Printer Tests

Test	Status	Time
PRNT	Pass	2:50pm

CRC Tests

Test	Status	Time
COMP	Pass	2:50pm
CAL	Pass	2:50pm

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Cabarrus Instrument Location BAT Mobile Unit 8
Instrument Serial No. 008816 -

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 17 day of August, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

2219283
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

CABARRUS COUNTY BAT MOBILE UNIT 8 120

Serial Number: 008816

Test Date: 08/17/2026

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Glasscock, Jerry D

Permit Number: 7180-9235

Effective:

02/01/2026-02/01/2028

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG431002

Exp Date: 11/05/2026

Test	g/210L	Time
DIAG	Pass	7:05am
AIR BLK	.00	7:06am
ACCY CHK	.07	7:07am
AIR BLK	.00	7:08am
SUB TEST	.00	7:08am
AIR BLK	.00	7:09am
SUB TEST	.00	7:11am
AIR BLK	.00	7:12am

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

Intox EC/IR-II: Preventive Maintenance

CABARRUS COUNTY BAT MOBILE UNIT 8 120

Serial Number: 008816 Test Record Number: 8169
Test Date: 08/17/2026 Test Time: 7:12am EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	7:13am
FLO	Pass	7:13am
FC	Pass	7:13am

Temperature Tests

Test	Status	Time
FC1	Pass	7:13am
SRC	Pass	7:13am
DET	Pass	7:13am
BAR	Pass	7:13am
BT	Pass	7:13am

Blank Tests

Test	Status	Time
AIR	Pass	7:14am

Printer Tests

Test	Status	Time
PRNT	Pass	7:14am

CRC Tests

Test	Status	Time
COMP	Pass	7:14am
CAL	Pass	7:14am

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Cabarrus Instrument Location BAT Mobile Unit 8
Instrument Serial No. 008816

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 24 day of August, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

2219283
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

CABARRUS COUNTY BAT MOBILE UNIT 8 120

Serial Number: 008816
Test Date: 08/24/2026

Citation Number: M00000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Glasscock, Jerry D

Permit Number: 7180-9235

Effective:

02/01/2026-02/01/2028

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG431002

Exp Date: 11/05/2026

Test	g/210L	Time
DIAG	Pass	2:43pm
AIR BLK	.00	2:44pm
ACCY CHK	.07	2:45pm
AIR BLK	.00	2:46pm
SUB TEST	.00	2:46pm
AIR BLK	.00	2:47pm
SUB TEST	.00	2:49pm
AIR BLK	.00	2:50pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

CABARRUS COUNTY BAT MOBILE UNIT 8 120

Serial Number: 008816 Test Record Number: 8181
Test Date: 08/24/2026 Test Time: 2:51pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	2:51pm
FLO	Pass	2:51pm
FC	Pass	2:51pm

Temperature Tests

Test	Status	Time
FC1	Pass	2:51pm
SRC	Pass	2:51pm
DET	Pass	2:51pm
BAR	Pass	2:51pm
BT	Pass	2:51pm

Blank Tests

Test	Status	Time
AIR	Pass	2:52pm


Printer Tests

Test	Status	Time
PRNT	Pass	2:52pm

CRC Tests

Test	Status	Time
COMP	Pass	2:52pm
CAL	Pass	2:52pm

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Cabarrus Instrument Location BAT Mobile Unit 8
Instrument Serial No. 008929 —

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 17 day of August, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

2219283
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

CABARRUS COUNTY BAT MOBILE UNIT 8 120

Serial Number: 008929

Test Date: 08/17/2026

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Glasscock, Jerry D

Permit Number: 7180-9235

Effective:

02/01/2026-02/01/2028

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

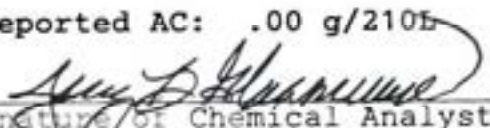
Test Type: Breath Test

Lot Number: AG506303


Exp Date: 03/04/2027

Test	g/210L	Time
DIAG	Pass	7:04am
AIR BLK	.00	7:05am
ACCY CHK	.07	7:06am
AIR BLK	.00	7:07am
SUB TEST	.00	7:08am
AIR BLK	.00	7:09am
SUB TEST	.00	7:11am
AIR BLK	.00	7:12am

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

CABARRUS COUNTY BAT MOBILE UNIT 8 120

Serial Number: 008929 Test Record Number: 1882
Test Date: 08/17/2026 Test Time: 7:12am EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	7:13am
FLO	Pass	7:13am
FC	Pass	7:13am

Temperature Tests

Test	Status	Time
FC1	Pass	7:13am
SRC	Pass	7:13am
DET	Pass	7:13am
BAR	Pass	7:13am
BT	Pass	7:13am

Blank Tests

Test	Status	Time
AIR	Pass	7:14am

Printer Tests

Test	Status	Time
PRNT	Pass	7:14am

CRC Tests

Test	Status	Time
COMP	Pass	7:14am
CAL	Pass	7:14am

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Cabarrus Instrument Location BAT Mobile Unit 8
Instrument Serial No. 008929 —

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 24 day of August, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

2219283
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

CABARRUS COUNTY BAT MOBILE UNIT 8 120

Serial Number: 008929

Test Date: 08/24/2026

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Glasscock, Jerry D

Permit Number: 7180-9235

Effective:

02/01/2026-02/01/2028

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

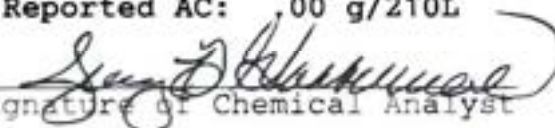
Test Type: Breath Test

Lot Number: AG506303

Exp Date: 03/04/2027

Test	g/210L	Time
DIAG	Pass	2:44pm
AIR BLK	.00	2:45pm
ACCY CHK	.08	2:46pm
AIR BLK	.00	2:47pm
SUB TEST	.00	2:48pm
AIR BLK	.00	2:49pm
SUB TEST	.00	2:50pm
AIR BLK	.00	2:51pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

CABARRUS COUNTY BAT MOBILE UNIT 8 120

Serial Number: 008929 Test Record Number: 1894
Test Date: 08/24/2026 Test Time: 2:51pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	2:52pm
FLO	Pass	2:52pm
FC	Pass	2:52pm

Temperature Tests

Test	Status	Time
FC1	Pass	2:52pm
SRC	Pass	2:52pm
DET	Pass	2:52pm
BAR	Pass	2:52pm
BT	Pass	2:52pm

Blank Tests

Test	Status	Time
AIR	Pass	2:53pm


Printer Tests

Test	Status	Time
PRNT	Pass	2:53pm

CRC Tests

Test	Status	Time
COMP	Pass	2:53pm
CAL	Pass	2:53pm

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County CALOWAY Instrument Location CALOWAY CO. JAIL

Instrument Serial No. 608719 151012 NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 17 day of August, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

274970
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

CALDWELL COUNTY CALDWELL COUNTY JAIL

130

Serial Number: 008719

Test Date: 08/17/2026

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Fleming, Tina S

Permit Number: 0027-4970

Effective:

02/01/2025-02/01/2027

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG602102

Exp Date: 01/21/2028


Test	g/210L	Time
DIAG	Pass	2:50pm
AIR BLK	.00	2:51pm
ACCY CHK	.08	2:52pm
AIR BLK	.00	2:53pm
SUB TEST	.00	2:53pm
AIR BLK	.00	2:54pm
SUB TEST	.00	2:56pm
AIR BLK	.00	2:57pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

CALDWELL COUNTY CALDWELL COUNTY JAIL 130

Serial Number: 008719 Test Record Number: 3722
Test Date: 08/17/2026 Test Time: 2:59pm EDT

System Check: Passed

Baseline Tests

Test	Status	Time
IR	Pass	2:59pm
FLO	Pass	2:59pm
FC	Pass	2:59pm

Temperature Tests

Test	Status	Time
FC1	Pass	2:59pm
SRC	Pass	2:59pm
DET	Pass	2:59pm
BAR	Pass	2:59pm
BT	Pass	2:59pm

Blank Tests

Test	Status	Time
AIR	Pass	3:00pm


Printer Tests

Test	Status	Time
PRNT	Pass	3:00pm

CRC Tests

Test	Status	Time
COMP	Pass	3:00pm
CAL	Pass	3:00pm

Preventive Maintenance
Status: Pass



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Caldwell Instrument Location Caldwell Co. Jail
Instrument Serial No. 008203 LE1012 NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 17 day of August, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

271970
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

CALDWELL COUNTY CALDWELL COUNTY JAIL
130

Serial Number: 008803
Test Date: 08/17/2026

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Fleming, Tina S

Permit Number: 0027-4970

Effective:

02/01/2025-02/01/2027

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG506302

Exp Date: 03/04/2027

Test	g/210L	Time
DIAG	Pass	2:44pm
AIR BLK	.00	2:45pm
ACCY CHK	.08	2:46pm
AIR BLK	.00	2:47pm
SUB TEST	.00	2:48pm
AIR BLK	.00	2:48pm
SUB TEST	.00	2:50pm
AIR BLK	.00	2:51pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

CALDWELL COUNTY CALDWELL COUNTY JAIL 130

Serial Number: 008803 Test Record Number: 929
Test Date: 08/17/2026 Test Time: 2:52pm EDT

System Check: Passed

Baseline Tests

Test	Status	Time
IR	Pass	2:52pm
FLO	Pass	2:52pm
FC	Pass	2:52pm

Temperature Tests

Test	Status	Time
FC1	Pass	2:52pm
SRC	Pass	2:52pm
DET	Pass	2:52pm
BAR	Pass	2:52pm
BT	Pass	2:52pm

Blank Tests

Test	Status	Time
AIR	Pass	2:53pm

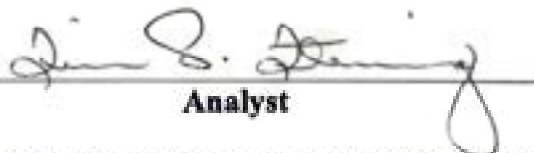
Printer Tests

Test	Status	Time
PRNT	Pass	2:53pm

CRC Tests

Test	Status	Time
COMP	Pass	2:53pm
CAL	Pass	2:53pm

Preventive Maintenance
Status: Pass


Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Carteret Instrument Location BAT Mobile Unit 10

Instrument Serial No. 008584

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 1 day of August, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]

Signature of Certifying Official

193759

Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

CARTERET COUNTY BAT MOBILE UNIT 10 150

Serial Number: 008584

Test Date: 08/01/2026

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Carroll, Barry Jean D

Permit Number: 0019-3759

Effective:

04/01/2026-04/01/2028

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG534301

Exp Date: 12/09/2027

Test	g/210L	Time
DIAG	Pass	2:43pm
AIR BLK	.00	2:44pm
ACCY CHK	.08	2:44pm
AIR BLK	.00	2:45pm
SUB TEST	.00	2:46pm
AIR BLK	.00	2:47pm
SUB TEST	.00	2:48pm
AIR BLK	.00	2:49pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

CARTERET COUNTY BAT MOBILE UNIT 10 150

Serial Number: 008584 Test Record Number: 2937
Test Date: 08/01/2026 Test Time: 2:49pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	2:50pm
FLO	Pass	2:50pm
FC	Pass	2:50pm

Temperature Tests

Test	Status	Time
FC1	Pass	2:50pm
SRC	Pass	2:50pm
DET	Pass	2:50pm
BAR	Pass	2:50pm
BT	Pass	2:50pm

Blank Tests

Test	Status	Time
AIR	Pass	2:50pm

Printer Tests

Test	Status	Time
PRNT	Pass	2:50pm

CRC Tests

Test	Status	Time
COMP	Pass	2:51pm
CAL	Pass	2:51pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Carteret Instrument Location BAT Mobile Unit 10

Instrument Serial No. 008686

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 1 day of August, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]

Signature of Certifying Official

193759

Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

CARTERET COUNTY BAT MOBILE UNIT 10 150

Serial Number: 008686

Test Date: 08/01/2026

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Carroll, Barry Jean D

Permit Number: 0019-3759

Effective:

04/01/2026-04/01/2028

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG506302

Exp Date: 03/04/2027

Test	g/210L	Time
DIAG	Pass	2:49pm
AIR BLK	.00	2:50pm
ACCY CHK	.08	2:51pm
AIR BLK	.00	2:51pm
SUB TEST	.00	2:52pm
AIR BLK	.00	2:53pm
SUB TEST	.00	2:54pm
AIR BLK	.00	2:55pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

CARTERET COUNTY BAT MOBILE UNIT 10 150

Serial Number: 008686 Test Record Number: 7285
Test Date: 08/01/2026 Test Time: 2:56pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	2:56pm
FLO	Pass	2:56pm
FC	Pass	2:56pm

Temperature Tests

Test	Status	Time
FC1	Pass	2:56pm
SRC	Pass	2:56pm
DET	Pass	2:56pm
BAR	Pass	2:56pm
BT	Pass	2:56pm

Blank Tests

Test	Status	Time
AIR	Pass	2:57pm

Printer Tests

Test	Status	Time
PRNT	Pass	2:57pm

CRC Tests

Test	Status	Time
COMP	Pass	2:57pm
CAL	Pass	2:57pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Carteret Instrument Location BAT Mobile unit 10

Instrument Serial No. 008776

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 1 day of August, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]

Signature of Certifying Official

193759

Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

CARTERET COUNTY BAT MOBILE UNIT 10 150

Serial Number: 008776

Test Date: 08/01/2026

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Carroll, Barry Jean D

Permit Number: 0019-3759

Effective:

04/01/2026-04/01/2028

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG534301

Exp Date: 12/09/2027

Test	g/210L	Time
DIAG	Pass	2:46pm
AIR BLK	.00	2:47pm
ACCY CHK	.08	2:48pm
AIR BLK	.00	2:49pm
SUB TEST	.00	2:50pm
AIR BLK	.00	2:51pm
SUB TEST	.00	2:52pm
AIR BLK	.00	2:53pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

Intox EC/IR-II: Preventive Maintenance

CARTERET COUNTY BAT MOBILE UNIT 10 150

Serial Number: 008776 Test Record Number: 4262
Test Date: 08/01/2026 Test Time: 2:54pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	2:54pm
FLO	Pass	2:54pm
FC	Pass	2:54pm

Temperature Tests

Test	Status	Time
FC1	Pass	2:54pm
SRC	Pass	2:54pm
DET	Pass	2:54pm
BAR	Pass	2:54pm
BT	Pass	2:54pm

Blank Tests

Test	Status	Time
AIR	Pass	2:55pm

Printer Tests

Test	Status	Time
PRNT	Pass	2:55pm

CRC Tests

Test	Status	Time
COMP	Pass	2:55pm
CAL	Pass	2:55pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Carteret

Instrument Location BAT Mobile Unit 10

Instrument Serial No. 009779

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 1 day of August, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



B. D. [Signature]

Signature of Certifying Official

193759

Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

CARTERET COUNTY BAT MOBILE UNIT 10 150

Serial Number: 008779

Test Date: 08/01/2026

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Carroll, Barry Jean D

Permit Number: 0019-3759

Effective:

04/01/2026-04/01/2028

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG431002

Exp Date: 11/05/2026

Test	g/210L	Time
DIAG	Pass	2:45pm
AIR BLK	.00	2:46pm
ACCY CHK	.08	2:47pm
AIR BLK	.00	2:48pm
SUB TEST	.00	2:48pm
AIR BLK	.00	2:49pm
SUB TEST	.00	2:51pm
AIR BLK	.00	2:52pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

CARTERET COUNTY BAT MOBILE UNIT 10 150

Serial Number: 008779 Test Record Number: 4180
Test Date: 08/01/2026 Test Time: 2:52pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	2:52pm
FLO	Pass	2:52pm
FC	Pass	2:53pm

Temperature Tests

Test	Status	Time
FC1	Pass	2:53pm
SRC	Pass	2:53pm
DET	Pass	2:53pm
BAR	Pass	2:53pm
BT	Pass	2:53pm

Blank Tests

Test	Status	Time
AIR	Pass	2:53pm

Printer Tests

Test	Status	Time
PRNT	Pass	2:53pm

CRC Tests

Test	Status	Time
COMP	Pass	2:53pm
CAL	Pass	2:53pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County CATAWBA Instrument Location CATAWBA COUNTY S.O.

Instrument Serial No. 008687 Neutral NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 17 day of August, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

214970
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

CATAWBA COUNTY CATAWBA COUNTY SO 170

Serial Number: 008687

Test Date: 08/17/2026

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Fleming, Tina S

Permit Number: 0027-4970

Effective:

02/01/2025-02/01/2027

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

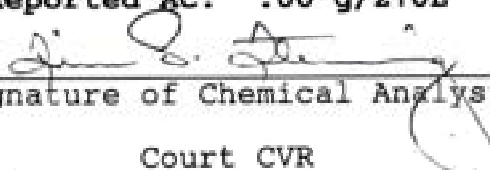
Test Type: Breath Test

Lot Number: AG516203

Exp Date: 06/11/2027

Test	g/210L	Time
DIAG	Pass	9:30am
AIR BLK	.00	9:30am
ACCY CHK	.08	9:31am
AIR BLK	.00	9:32am
SUB TEST	.00	9:33am
AIR BLK	.00	9:34am
SUB TEST	.00	9:36am
AIR BLK	.00	9:36am

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

CATAWBA COUNTY CATAWBA COUNTY SO 170

Serial Number: 008687 Test Record Number: 4425
Test Date: 08/17/2026 Test Time: 9:37am EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	9:37am
FLO	Pass	9:37am
FC	Pass	9:38am

Temperature Tests

Test	Status	Time
FC1	Pass	9:38am
SRC	Pass	9:38am
DET	Pass	9:38am
BAR	Pass	9:38am
BT	Pass	9:38am

Blank Tests

Test	Status	Time
AIR	Pass	9:38am

Printer Tests

Test	Status	Time
PRNT	Pass	9:38am

CRC Tests

Test	Status	Time
COMP	Pass	9:38am
CAL	Pass	9:38am

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County CATAWBA Instrument Location HICKORY PD

Instrument Serial No. 008891 HICKORY NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 17 day of August, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

274970
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

CATAWBA COUNTY HICKORY PD 170

Serial Number: 008841
Test Date: 08/17/2026

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Fleming, Tina S

Permit Number: 0027-4970

Effective:

02/01/2025-02/01/2027

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG534301

Exp Date: 12/09/2027

Test	g/210L	Time
DIAG	Pass	10:41am
AIR BLK	.00	10:41am
ACCY CHK	.08	10:42am
AIR BLK	.00	10:43am
SUB TEST	.00	10:44am
AIR BLK	.00	10:45am
SUB TEST	.00	10:47am
AIR BLK	.00	10:47am

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

CATAWBA COUNTY HICKORY PD 170

Serial Number: 008841 Test Record Number: 2657
Test Date: 08/17/2026 Test Time: 10:50am EDT

System Check: Passed

Baseline Tests

Test	Status	Time
IR	Pass	10:50am
FLO	Pass	10:50am
FC	Pass	10:50am

Temperature Tests

Test	Status	Time
FC1	Pass	10:50am
SRC	Pass	10:50am
DET	Pass	10:50am
BAR	Pass	10:50am
BT	Pass	10:50am

Blank Tests

Test	Status	Time
AIR	Pass	10:51am

Printer Tests

Test	Status	Time
PRNT	Pass	10:51am

CRC Tests

Test	Status	Time
COMP	Pass	10:51am
CAL	Pass	10:51am

Preventive Maintenance
Status: Pass



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Chatham Instrument Location Chatham County Detention
Instrument Serial No. 008728 Pittsboro, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 19 day of August, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.





Signature of Certifying Official

365156
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

CHATHAM COUNTY DETENTION CENTER 180

Serial Number: 008728

Test Date: 08/19/2026

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Garner, Joel K

Permit Number: 0036-5156

Effective:

02/01/2026-02/01/2028

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG516204

Exp Date: 06/11/2027

Test	g/210L	Time
DIAG	Pass	6:31am
AIR BLK	.00	6:31am
ACCY CHK	.08	6:32am
AIR BLK	.00	6:33am
SUB TEST	.00	6:34am
AIR BLK	.00	6:34am
SUB TEST	.00	6:36am
AIR BLK	.00	6:37am

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

Intox EC/IR-II: Preventive Maintenance

CHATHAM COUNTY DETENTION CENTER 180

Serial Number: 008728 Test Record Number: 636
Test Date: 08/19/2026 Test Time: 6:39am EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	6:39am
FLO	Pass	6:39am
FC	Pass	6:39am

Temperature Tests

Test	Status	Time
FC1	Pass	6:39am
SRC	Pass	6:39am
DET	Pass	6:39am
BAR	Pass	6:39am
BT	Pass	6:39am

Blank Tests

Test	Status	Time
AIR	Pass	6:40am

Printer Tests

Test	Status	Time
PRNT	Pass	6:40am

CRC Tests

Test	Status	Time
COMP	Pass	6:40am
CAL	Pass	6:40am

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH


PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Chatham Instrument Location Siler City Police Dept.
Instrument Serial No. 008811 Siler City, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 19 day of August, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Signature of Certifying Official

365156

Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

CHATHAM COUNTY SILER CITY PD 180

Serial Number: 008811

Test Date: 08/19/2026

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Garner, Joel K

Permit Number: 0036-5156

Effective:

02/01/2026-02/01/2028

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG516204

Exp Date: 06/11/2027

Test	g/210L	Time
DIAG	Pass	8:34am
AIR BLK	.00	8:35am
ACCY CHK	.08	8:35am
AIR BLK	.00	8:36am
SUB TEST	.00	8:37am
AIR BLK	.00	8:38am
SUB TEST	.00	8:39am
AIR BLK	.00	8:40am

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

Intox EC/IR-II: Preventive Maintenance

CHATHAM COUNTY SILER CITY PD 180

Serial Number: 008811 Test Record Number: 1963
Test Date: 08/19/2026 Test Time: 8:41am EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	8:41am
FLO	Pass	8:41am
FC	Pass	8:42am

Temperature Tests

Test	Status	Time
FC1	Pass	8:42am
SRC	Pass	8:42am
DET	Pass	8:42am
BAR	Pass	8:42am
BT	Pass	8:42am

Blank Tests

Test	Status	Time
AIR	Pass	8:42am

Printer Tests

Test	Status	Time
PRNT	Pass	8:42am

CRC Tests

Test	Status	Time
COMP	Pass	8:43am
CAL	Pass	8:43am

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Cherokee Instrument Location Cherokee Co. Jail
Instrument Serial No. 008622 Murphy, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 4th day of August, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Paul R. Cuth

Signature of Certifying Official

843310

Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

CHEROKEE COUNTY CHEROKEE COUNTY JAIL
190

Serial Number: 008622
Test Date: 08/04/2026

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE

Analyst's Name: Cutler, Daniel R
Permit Number: 0084-3310
Effective:
02/01/2026-02/01/2028

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG505001
Exp Date: 02/19/2027

Test	g/210L	Time
DIAG	Pass	11:50am
AIR BLK	.00	11:51am
ACCY CHK	.07	11:52am
AIR BLK	.00	11:53am
SUB TEST	.00	11:53am
AIR BLK	.00	11:54am
SUB TEST	.00	11:56am
AIR BLK	.00	11:57am

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

Intox EC/IR-II: Preventive Maintenance

CHEROKEE COUNTY CHEROKEE COUNTY JAIL 190

Serial Number: 008622 Test Record Number: 1374
Test Date: 08/04/2026 Test Time: 11:57am EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	11:58am
FLO	Pass	11:58am
FC	Pass	11:58am

Temperature Tests

Test	Status	Time
FC1	Pass	11:58am
SRC	Pass	11:58am
DET	Pass	11:58am
BAR	Pass	11:58am
BT	Pass	11:58am

Blank Tests

Test	Status	Time
AIR	Pass	11:58am


Printer Tests

Test	Status	Time
PRNT	Pass	11:58am

CRC Tests

Test	Status	Time
COMP	Pass	11:59am
CAL	Pass	11:59am

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Cherokee Instrument Location Cherokee Co. Jail
Instrument Serial No. 008711 Murphy, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 4th day of August, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



David R. Cuth
Signature of Certifying Official

843310
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

CHEROKEE COUNTY CHEROKEE COUNTY JAIL
190

Serial Number: 008711
Test Date: 08/04/2026

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE

Analyst's Name: Cutler, Daniel R
Permit Number: 0084-3310
Effective:
02/01/2026-02/01/2028

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG503001
Exp Date: 01/30/2027

Test	g/210L	Time
DIAG	Pass	11:39am
AIR BLK	.00	11:40am
ACCY CHK	.07	11:40am
AIR BLK	.00	11:41am
SUB TEST	.00	11:42am
AIR BLK	.00	11:43am
SUB TEST	.00	11:44am
AIR BLK	.00	11:45am

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

CHEROKEE COUNTY CHEROKEE COUNTY JAIL 190

Serial Number: 008711 Test Record Number: 1617
Test Date: 08/04/2026 Test Time: 11:46am EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	11:46am
FLO	Pass	11:46am
FC	Pass	11:46am

Temperature Tests

Test	Status	Time
FC1	Pass	11:46am
SRC	Pass	11:46am
DET	Pass	11:46am
BAR	Pass	11:46am
BT	Pass	11:46am

Blank Tests

Test	Status	Time
AIR	Pass	11:47am

Printer Tests

Test	Status	Time
PRNT	Pass	11:47am

CRC Tests

Test	Status	Time
COMP	Pass	11:47am
CAL	Pass	11:47am

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Cleveland Instrument Location Cleveland County SO - Annex
Instrument Serial No. 008887 Shelby, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 19 day of August, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

244987
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

CLEVELAND COUNTY CLEVELAND SO-ANNEX
220

Serial Number: 008887

Test Date: 08/19/2026

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Loftis, Benjamin C

Permit Number: 0024-4

Effective:

02/01/2026-02/01/2028

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

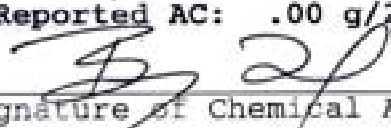
Test Type: Breath Test

Lot Number: AG516203

Exp Date: 06/11/2027

Test	g/210L	Time
DIAG	Pass	11:58am
AIR BLK	.00	11:58am
ACCY CHK	.07	11:59am
AIR BLK	.00	12:00pm
SUB TEST	.00	12:01pm
AIR BLK	.00	12:02pm
SUB TEST	.00	12:03pm
AIR BLK	.00	12:04pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

This form is used when performing Preventive Maintenance procedures

Forensic Tests for Alcohol Branch

Department of Health and Human Services

Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

CLEVELAND COUNTY CLEVELAND SO-ANNEX 220

Serial Number: 008887 Test Record Number: 4606
Test Date: 08/19/2026 Test Time: 12:05pm EDT

System Check: Passed

Baseline Tests

Test	Status	Time
IR	Pass	12:05pm
FLO	Pass	12:05pm
FC	Pass	12:05pm

Temperature Tests

Test	Status	Time
FC1	Pass	12:06pm
SRC	Pass	12:06pm
DET	Pass	12:06pm
BAR	Pass	12:06pm
BT	Pass	12:06pm

Blank Tests

Test	Status	Time
AIR	Pass	12:06pm

Printer Tests

Test	Status	Time
PRNT	Pass	12:06pm

CRC Tests

Test	Status	Time
COMP	Pass	12:06pm
CAL	Pass	12:06pm

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Cleveland Instrument Location Cleveland County SO-Annex
Instrument Serial No. 008893 Shelby, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 19 day of August, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

244987
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

CLEVELAND COUNTY CLEVELAND SO-ANNEX
220

Serial Number: 008893

Test Date: 08/19/2026

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Loftis, Benjamin C

Permit Number: 0024-4987

Effective:

02/01/2026-02/01/2028

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

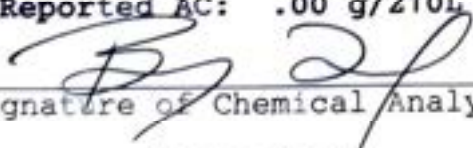
Test Type: Breath Test

Lot Number: AG516203

Exp Date: 06/11/2027

Test	g/210L	Time
DIAG	Pass	12:11pm
AIR BLK	.00	12:11pm
ACCY CHK	.08	12:12pm
AIR BLK	.00	12:13pm
SUB TEST	.00	12:13pm
AIR BLK	.00	12:14pm
SUB TEST	.00	12:15pm
AIR BLK	.00	12:16pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

CLEVELAND COUNTY CLEVELAND SO-ANNEX 220

Serial Number: 008893 Test Record Number: 2142
Test Date: 08/19/2026 Test Time: 12:16pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	12:17pm
FLO	Pass	12:17pm
FC	Pass	12:17pm

Temperature Tests

Test	Status	Time
FC1	Pass	12:17pm
SRC	Pass	12:17pm
DET	Pass	12:17pm
BAR	Pass	12:17pm
BT	Pass	12:17pm

Blank Tests

Test	Status	Time
AIR	Pass	12:18pm

Printer Tests

Test	Status	Time
PRNT	Pass	12:18pm

CRC Tests

Test	Status	Time
COMP	Pass	12:18pm
CAL	Pass	12:18pm

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Cleveland Instrument Location Kings Mountain PD
Instrument Serial No 008900 Kings Mountain, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 19 day of August, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

244987
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

CLEVELAND COUNTY KINGS MOUNTAIN PD 220

Serial Number: 008900
Test Date: 08/19/2026

Citation Number: M00000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Loftis, Benjamin C

Permit Number: 0024-4

Effective:

02/01/2026-02/01/2028

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

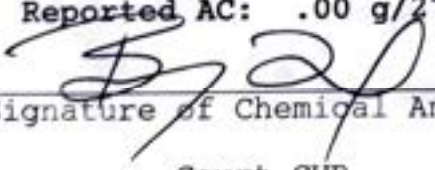
Test Type: Breath Test

Lot Number: AG506303

Exp Date: 03/04/2027

Test	g/210L	Time
DIAG	Pass	10:42am
AIR BLK	.00	10:43am
ACCY CHK	.07	10:43am
AIR BLK	.00	10:45am
SUB TEST	.00	10:45am
AIR BLK	.00	10:46am
SUB TEST	.00	10:47am
AIR BLK	.00	10:48am

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

CLEVELAND COUNTY KINGS MOUNTAIN PD 220

Serial Number: 008900 Test Record Number: 1168
Test Date: 08/19/2026 Test Time: 10:49am EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	10:49am
FLO	Pass	10:49am
FC	Pass	10:49am

Temperature Tests

Test	Status	Time
FC1	Pass	10:49am
SRC	Pass	10:49am
DET	Pass	10:49am
BAR	Pass	10:49am
BT	Pass	10:49am

Blank Tests

Test	Status	Time
AIR	Pass	10:50am

Printer Tests

Test	Status	Time
PRNT	Pass	10:50am

CRC Tests

Test	Status	Time
COMP	Pass	10:50am
CAL	Pass	10:50am

Preventive Maintenance

Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County CLAVEN Instrument Location BAT Mobile Unit 9

Instrument Serial No. 008575

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 26th day of August, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

83034
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

CRAVEN COUNTY BAT MOBILE UNIT 9 240

Serial Number: 008575

Test Date: 08/26/2026

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name:

Crutchfield Jr., Marshall B

Permit Number: 0008-3034

Effective:

03/01/2026-03/01/2028

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG516204

Exp Date: 06/11/2027

Test	g/210L	Time
DIAG	Pass	8:08pm
AIR BLK	.00	8:09pm
ACCY CHK	.07	8:09pm
AIR BLK	.00	8:10pm
SUB TEST	.00	8:10pm
AIR BLK	.00	8:11pm
SUB TEST	.00	8:13pm
AIR BLK	.00	8:14pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

CRAVEN COUNTY BAT MOBILE UNIT 9 240

Serial Number: 008575 Test Record Number: 1646
Test Date: 08/26/2026 Test Time: 8:14pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	8:15pm
FLO	Pass	8:15pm
FC	Pass	8:15pm

Temperature Tests

Test	Status	Time
FC1	Pass	8:15pm
SRC	Pass	8:15pm
DET	Pass	8:15pm
BAR	Pass	8:15pm
BT	Pass	8:15pm

Blank Tests

Test	Status	Time
AIR	Pass	8:16pm

Printer Tests

Test	Status	Time
PRNT	Pass	8:16pm

CRC Tests

Test	Status	Time
COMP	Pass	8:16pm
CAL	Pass	8:16pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County CRAVEN Instrument Location BAT Mobile Unit 9
Instrument Serial No. 008616

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 26th day of August, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

83034
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

CRAVEN COUNTY BAT MOBILE UNIT 9 240

Serial Number: 008616

Test Date: 08/26/2026

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name:

Crutchfield Jr., Marshall B

Permit Number: 0008-3034

Effective:

03/01/2026-03/01/2028

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG506303

Exp Date: 03/04/2027


Test	g/210L	Time
DIAG	Pass	8:18pm
AIR BLK	.00	8:19pm
ACCY CHK	.08	8:19pm
AIR BLK	.00	8:20pm
SUB TEST	.00	8:21pm
AIR BLK	.00	8:22pm
SUB TEST	.00	8:23pm
AIR BLK	.00	8:24pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

CRAVEN COUNTY BAT MOBILE UNIT 9 240

Serial Number: 008616 Test Record Number: 3073
Test Date: 08/26/2026 Test Time: 8:25pm EDT

System Check: Passed

Baseline Tests

Test	Status	Time
IR	Pass	8:25pm
FLO	Pass	8:25pm
FC	Pass	8:25pm

Temperature Tests

Test	Status	Time
FC1	Pass	8:25pm
SRC	Pass	8:25pm
DET	Pass	8:25pm
BAR	Pass	8:25pm
BT	Pass	8:25pm

Blank Tests

Test	Status	Time
AIR	Pass	8:26pm

Printer Tests

Test	Status	Time
PRNT	Pass	8:26pm

CRC Tests

Test	Status	Time
COMP	Pass	8:26pm
CAL	Pass	8:26pm

**Preventive Maintenance
Status: Pass**



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County CRAVEN Instrument Location BAT Mobile Unit 9

Instrument Serial No. 008647

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 26th day of August, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

83034
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

CRAVEN COUNTY BAT MOBILE UNIT 9 240

Serial Number: 008647

Test Date: 08/26/2026

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name:

Crutchfield Jr., Marshall B

Permit Number: 0008-3034

Effective:

03/01/2026-03/01/2028

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG516203

Exp Date: 06/11/2027


Test	g/210L	Time
DIAG	Pass	8:21pm
AIR BLK	.00	8:22pm
ACCY CHK	.07	8:22pm
AIR BLK	.00	8:23pm
SUB TEST	.00	8:24pm
AIR BLK	.00	8:25pm
SUB TEST	.00	8:26pm
AIR BLK	.00	8:27pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

CRAVEN COUNTY BAT MOBILE UNIT 9 240

Serial Number: 008647 Test Record Number: 3034
Test Date: 08/26/2026 Test Time: 8:28pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	8:28pm
FLO	Pass	8:28pm
FC	Pass	8:28pm

Temperature Tests

Test	Status	Time
FC1	Pass	8:28pm
SRC	Pass	8:28pm
DET	Pass	8:28pm
BAR	Pass	8:28pm
BT	Pass	8:28pm

Blank Tests

Test	Status	Time
AIR	Pass	8:29pm

Printer Tests

Test	Status	Time
PRNT	Pass	8:29pm

CRC Tests

Test	Status	Time
COMP	Pass	8:29pm
CAL	Pass	8:29pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County CRAVEN Instrument Location BAT Mobile Unit 9

Instrument Serial No. 008704

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 26th day of August, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Signature of Certifying Official

Certificate Number

83034

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

CRAVEN COUNTY BAT MOBILE UNIT 9 240

Serial Number: 008704

Test Date: 08/26/2026

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name:

Crutchfield Jr., Marshall B

Permit Number: 0008-3034

Effective:

03/01/2026-03/01/2028

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG506303

Exp Date: 03/04/2027

Test	g/210L	Time
DIAG	Pass	8:36pm
AIR BLK	.00	8:36pm
ACCY CHK	.07	8:37pm
AIR BLK	.00	8:38pm
SUB TEST	.00	8:39pm
AIR BLK	.00	8:39pm
SUB TEST	.00	8:41pm
AIR BLK	.00	8:42pm

Reported AC1 .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

CRAVEN COUNTY BAT MOBILE UNIT 9 240

Serial Number: 008704 Test Record Number: 1083
Test Date: 08/26/2026 Test Time: 8:43pm EDT

System Check: Passed

Baseline Tests

Test	Status	Time
IR	Pass	8:43pm
FLO	Pass	8:43pm
FC	Pass	8:43pm

Temperature Tests

Test	Status	Time
FC1	Pass	8:43pm
SRC	Pass	8:43pm
DET	Pass	8:43pm
BAR	Pass	8:43pm
BT	Pass	8:43pm

Blank Tests

Test	Status	Time
AIR	Pass	8:44pm


Printer Tests

Test	Status	Time
PRNT	Pass	8:44pm

CRC Tests

Test	Status	Time
COMP	Pass	8:44pm
CAL	Pass	8:44pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County CRAVEN Instrument Location BAT Mobile Unit 9

Instrument Serial No. 008826

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 26th day of August, 20 26 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.





Signature of Certifying Official

83034

Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

CRAVEN COUNTY BAT MOBILE UNIT 9 240

Serial Number: 008826

Test Date: 08/26/2026

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name:

Crutchfield Jr., Marshall B

Permit Number: 0008-3034

Effective:

03/01/2026-03/01/2028

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG516204

Exp Date: 06/11/2027

Test	g/210L	Time
DIAG	Pass	7:55pm
AIR BLK	.00	7:56pm
ACCY CHK	.07	7:57pm
AIR BLK	.00	7:58pm
SUB TEST	.00	7:58pm
AIR BLK	.00	7:59pm
SUB TEST	.00	8:01pm
AIR BLK	.00	8:02pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

This form is used when performing Preventive Maintenance procedures

Forensic Tests for Alcohol Branch

Department of Health and Human Services

Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

CRAVEN COUNTY BAT MOBILE UNIT 9 240

Serial Number: 008826 Test Record Number: 8723
Test Date: 08/26/2026 Test Time: 8:02pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	8:03pm
FLO	Pass	8:03pm
FC	Pass	8:03pm

Temperature Tests

Test	Status	Time
FC1	Pass	8:03pm
SRC	Pass	8:03pm
DET	Pass	8:03pm
BAR	Pass	8:03pm
BT	Pass	8:03pm

Blank Tests

Test	Status	Time
AIR	Pass	8:03pm

Printer Tests

Test	Status	Time
PRNT	Pass	8:04pm

CRC Tests

Test	Status	Time
COMP	Pass	8:04pm
CAL	Pass	8:04pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Cumberland Instrument Location FT. Bragg L.E.C.
Instrument Serial No. 013868 FT. Bragg, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 10 day of August, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



A handwritten signature in black ink, appearing to be "H. K. ...", written over a horizontal line.

Signature of Certifying Official

365156

Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

CUMBERLAND COUNTY FORT BRAGG LEC 250

Serial Number: 013868
Test Date: 08/10/2026

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Garner, Joel K

Permit Number: 0036-5156

Effective:

02/01/2026-02/01/2028

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG534301

Exp Date: 12/09/2027

Test	g/210L	Time
DIAG	Pass	8:44am
AIR BLK	.00	8:44am
ACCY CHK	.08	8:45am
AIR BLK	.00	8:46am
SUB TEST	.00	8:46am
AIR BLK	.00	8:47am
SUB TEST	.00	8:49am
AIR BLK	.00	8:50am

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

CUMBERLAND COUNTY FORT BRAGG LEC 250

Serial Number: 013868 Test Record Number: 1283
Test Date: 08/10/2026 Test Time: 8:53am EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	8:53am
FLO	Pass	8:53am
FC	Pass	8:54am

Temperature Tests

Test	Status	Time
FC1	Pass	8:54am
SRC	Pass	8:54am
DET	Pass	8:54am
BAR	Pass	8:54am
BT	Pass	8:54am

Blank Tests

Test	Status	Time
AIR	Pass	8:54am

Printer Tests

Test	Status	Time
PRNT	Pass	8:54am

CRC Tests

Test	Status	Time
COMP	Pass	8:55am
CAL	Pass	8:55am

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Cumberland Instrument Location FT. Bragg L.E.C.
Instrument Serial No. 013870 FT. Bragg, N.C.

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 10 day of August, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

365156
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

CUMBERLAND COUNTY FORT BRAGG LEC 250

Serial Number: 013870

Test Date: 08/10/2026

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Garner, Joel K

Permit Number: 0036-5156

Effective:

02/01/2026-02/01/2028

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG534301

Exp Date: 12/09/2027

Test	g/210L	Time
DIAG	Pass	8:43am
AIR BLK	.00	8:43am
ACCY CHK	.08	8:44am
AIR BLK	.00	8:45am
SUB TEST	.00	8:46am
AIR BLK	.00	8:46am
SUB TEST	.00	8:48am
AIR BLK	.00	8:49am

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

CUMBERLAND COUNTY FORT BRAGG LEC 250

Serial Number: 013870 Test Record Number: 1349
Test Date: 08/10/2026 Test Time: 8:53am EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	8:53am
FLO	Pass	8:53am
FC	Pass	8:53am

Temperature Tests

Test	Status	Time
FC1	Pass	8:53am
SRC	Pass	8:53am
DET	Pass	8:53am
BAR	Pass	8:53am
BT	Pass	8:53am

Blank Tests

Test	Status	Time
AIR	Pass	8:54am

Printer Tests

Test	Status	Time
PRNT	Pass	8:54am

CRC Tests

Test	Status	Time
COMP	Pass	8:54am
CAL	Pass	8:54am

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Currituck Instrument Location Currituck Co. S.O. - Corolla
Instrument Serial No. 008949 Corolla, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 4th day of August, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

206272
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

CURRITUCK COUNTY SO-COROLLA 260

Serial Number: 008949

Test Date: 08/04/2026

Citation Number: M00000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Chappell, Mark A

Permit Number: 0020-6272

Effective:

02/01/2026-02/01/2028

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

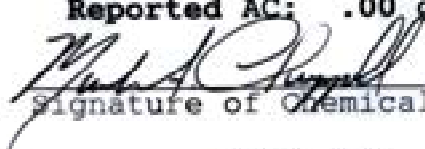
Test Type: Breath Test

Lot Number: AG501303

Exp Date: 01/13/2027

Test	g/210L	Time
DIAG	Pass	2:31pm
AIR BLK	.00	2:31pm
ACCY CHK	.08	2:32pm
AIR BLK	.00	2:33pm
SUB TEST	.00	2:34pm
AIR BLK	.00	2:35pm
SUB TEST	.00	2:36pm
AIR BLK	.00	2:37pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

CURRITUCK COUNTY SO-COROLLA 260

Serial Number: 008949 Test Record Number: 889
Test Date: 08/04/2026 Test Time: 2:38pm EDT

System Check: Passed

Baseline Tests

Test	Status	Time
IR	Pass	2:38pm
FLO	Pass	2:38pm
FC	Pass	2:38pm

Temperature Tests

Test	Status	Time
FC1	Pass	2:38pm
SRC	Pass	2:38pm
DET	Pass	2:38pm
BAR	Pass	2:38pm
BT	Pass	2:38pm

Blank Tests

Test	Status	Time
AIR	Pass	2:39pm

Printer Tests

Test	Status	Time
PRNT	Pass	2:39pm

CRC Tests

Test	Status	Time
COMP	Pass	2:39pm
CAL	Pass	2:39pm

Preventive Maintenance
Status: Pass


Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Dare Instrument Location Dare Co. S.O.
Instrument Serial No. 008807 Buxton, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 25th day of August, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Mark A. Russell
Signature of Certifying Official

206272
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

DARE COUNTY DARE CO SO BUXTON 270

Serial Number: 008807

Test Date: 08/25/2026

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Chappell, Mark A

Permit Number: 0020-6272

Effective:

02/01/2026-02/01/2028

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

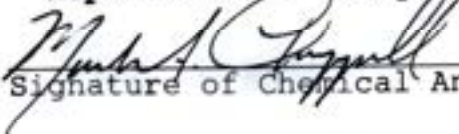
Test Type: Breath Test

Lot Number: AG501303

Exp Date: 01/13/2027

Test	g/210L	Time
DIAG	Pass	1:30pm
AIR BLK	.00	1:30pm
ACCY CHK	.07	1:31pm
AIR BLK	.00	1:32pm
SUB TEST	.00	1:33pm
AIR BLK	.00	1:34pm
SUB TEST	.00	1:35pm
AIR BLK	.00	1:36pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

DARE COUNTY DARE CO SO BUXTON 270

Serial Number: 008807 Test Record Number: 1607
Test Date: 08/25/2026 Test Time: 1:37pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	1:37pm
FLO	Pass	1:37pm
FC	Pass	1:37pm

Temperature Tests

Test	Status	Time
FC1	Pass	1:38pm
SRC	Pass	1:38pm
DET	Pass	1:38pm
BAR	Pass	1:38pm
BT	Pass	1:38pm

Blank Tests

Test	Status	Time
AIR	Pass	1:38pm

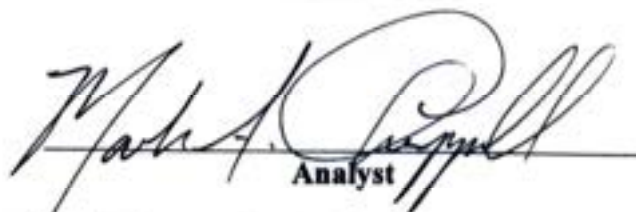
Printer Tests

Test	Status	Time
PRNT	Pass	1:38pm

CRC Tests

Test	Status	Time
COMP	Pass	1:38pm
CAL	Pass	1:38pm

Preventive Maintenance
Status: Pass


Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Davidson Instrument Location BAT Mobile Unit 8
Instrument Serial No. 008615 —

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 31 day of August, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

2219283
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

DAVIDSON COUNTY BAT MOBILE UNIT 8 280

Serial Number: 008615
Test Date: 08/31/2026

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE

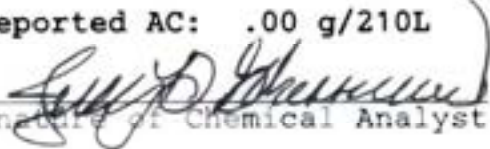
Analyst's Name: Glasscock, Jerry D
Permit Number: 7180-9235
Effective:
02/01/2026-02/01/2028

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

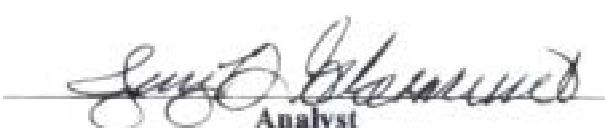
Lot Number: AG506303
Exp Date: 03/04/2027

Test	g/210L	Time
DIAG	Pass	9:01pm
AIR BLK	.00	9:02pm
ACCY CHK	.07	9:02pm
AIR BLK	.00	9:03pm
SUB TEST	.00	9:04pm
AIR BLK	.00	9:05pm
SUB TEST	.00	9:06pm
AIR BLK	.00	9:07pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

Intox EC/IR-II: Preventive Maintenance

DAVIDSON COUNTY BAT MOBILE UNIT 8 280

Serial Number: 008615 Test Record Number: 6404
Test Date: 08/31/2026 Test Time: 9:08pm EDT

System Check: Passed

Baseline Tests

Test	Status	Time
IR	Pass	9:08pm
FLO	Pass	9:08pm
FC	Pass	9:08pm

Temperature Tests

Test	Status	Time
FC1	Pass	9:08pm
SRC	Pass	9:08pm
DET	Pass	9:08pm
BAR	Pass	9:08pm
BT	Pass	9:08pm

Blank Tests

Test	Status	Time
AIR	Pass	9:09pm

Printer Tests

Test	Status	Time
PRNT	Pass	9:09pm

CRC Tests

Test	Status	Time
COMP	Pass	9:09pm
CAL	Pass	9:09pm

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Davidson Instrument Location BAT Mobile Unit 8
Instrument Serial No. 008736 —

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 31 day of August, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

2219283
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

DAVIDSON COUNTY BAT MOBILE UNIT 8 280

Serial Number: 008736

Test Date: 08/31/2026

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Glasscock, Jerry D

Permit Number: 7180-9235

Effective:

02/01/2026-02/01/2028

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

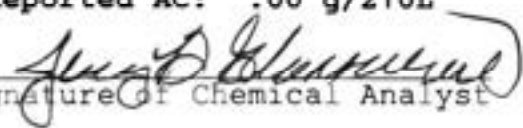
Test Type: Breath Test

Lot Number: AG506303

Exp Date: 03/04/2027

Test	g/210L	Time
DIAG	Pass	9:00pm
AIR BLK	.00	9:01pm
ACCY CHK	.07	9:02pm
AIR BLK	.00	9:03pm
SUB TEST	.00	9:03pm
AIR BLK	.00	9:04pm
SUB TEST	.00	9:06pm
AIR BLK	.00	9:06pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

This form is used when performing Preventive Maintenance procedures

Forensic Tests for Alcohol Branch

Department of Health and Human Services

Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

DAVIDSON COUNTY BAT MOBILE UNIT 8 280

Serial Number: 008736 Test Record Number: 1754
Test Date: 08/31/2026 Test Time: 9:07pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	9:07pm
FLO	Pass	9:07pm
FC	Pass	9:07pm

Temperature Tests

Test	Status	Time
FC1	Pass	9:07pm
SRC	Pass	9:07pm
DET	Pass	9:07pm
BAR	Pass	9:07pm
BT	Pass	9:07pm

Blank Tests

Test	Status	Time
AIR	Pass	9:08pm

Printer Tests

Test	Status	Time
PRNT	Pass	9:08pm

CRC Tests

Test	Status	Time
COMP	Pass	9:08pm
CAL	Pass	9:08pm

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Davidson Instrument Location BAT Mobile Unit 8
Instrument Serial No. 008775 —

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 31 day of August, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

2219283
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

DAVIDSON COUNTY BAT MOBILE UNIT 8 280

Serial Number: 008775

Test Date: 08/31/2026

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Glasscock, Jerry D

Permit Number: 7180-9235

Effective:

02/01/2026-02/01/2028

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG506303


Exp Date: 03/04/2027

Test	g/210L	Time
DIAG	Pass	9:00pm
AIR BLK	.00	9:01pm
ACCY CHK	.08	9:01pm
AIR BLK	.00	9:02pm
SUB TEST	.00	9:03pm
AIR BLK	.00	9:03pm
SUB TEST	.00	9:05pm
AIR BLK	.00	9:06pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

DAVIDSON COUNTY BAT MOBILE UNIT 8 280

Serial Number: 008775 Test Record Number: 2620
Test Date: 08/31/2026 Test Time: 9:09pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	9:09pm
FLO	Pass	9:09pm
FC	Pass	9:09pm

Temperature Tests

Test	Status	Time
FC1	Pass	9:09pm
SRC	Pass	9:09pm
DET	Pass	9:09pm
BAR	Pass	9:09pm
BT	Pass	9:09pm

Blank Tests

Test	Status	Time
AIR	Pass	9:10pm

Printer Tests

Test	Status	Time
PRNT	Pass	9:10pm

CRC Tests

Test	Status	Time
COMP	Pass	9:10pm
CAL	Pass	9:10pm

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Davidson Instrument Location BAT Mobile Unit 8
Instrument Serial No. 008816 —

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 31 day of August, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

2219283
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

DAVIDSON COUNTY BAT MOBILE UNIT 8 280

Serial Number: 008816

Test Date: 08/31/2026

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Glasscock, Jerry D

Permit Number: 7180-9235

Effective:

02/01/2026-02/01/2028

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG431002

Exp Date: 11/05/2026

Test	g/210L	Time
DIAG	Pass	8:59pm
AIR BLK	.00	9:00pm
ACCY CHK	.07	9:01pm
AIR BLK	.00	9:02pm
SUB TEST	.00	9:02pm
AIR BLK	.00	9:03pm
SUB TEST	.00	9:05pm
AIR BLK	.00	9:06pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

DAVIDSON COUNTY BAT MOBILE UNIT 8 280

Serial Number: 008816 Test Record Number: 8187
Test Date: 08/31/2026 Test Time: 9:06pm EDT

System Check: Passed

Baseline Tests

Test	Status	Time
IR	Pass	9:07pm
FLO	Pass	9:07pm
FC	Pass	9:07pm

Temperature Tests

Test	Status	Time
FC1	Pass	9:07pm
SRC	Pass	9:07pm
DET	Pass	9:07pm
BAR	Pass	9:07pm
BT	Pass	9:07pm

Blank Tests

Test	Status	Time
AIR	Pass	9:07pm

Printer Tests

Test	Status	Time
PRNT	Pass	9:07pm

CRC Tests

Test	Status	Time
COMP	Pass	9:08pm
CAL	Pass	9:08pm

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Davidson Instrument Location BAT Mobile Unit 8
Instrument Serial No. 008929 —

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 31 day of August, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

2219283
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

DAVIDSON COUNTY BAT MOBILE UNIT 8 280

Serial Number: 008929
Test Date: 08/31/2026

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Glasscock, Jerry D

Permit Number: 7180-9235

Effective:

02/01/2026-02/01/2028

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG506303

Exp Date: 03/04/2027

Test	g/210L	Time
DIAG	Pass	8:58pm
AIR BLK	.00	8:59pm
ACCY CHK	.07	9:00pm
AIR BLK	.00	9:01pm
SUB TEST	.00	9:02pm
AIR BLK	.00	9:03pm
SUB TEST	.00	9:04pm
AIR BLK	.00	9:05pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

DAVIDSON COUNTY BAT MOBILE UNIT 8 280

Serial Number: 008929 Test Record Number: 1900
Test Date: 08/31/2026 Test Time: 9:06pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	9:06pm
FLO	Pass	9:06pm
FC	Pass	9:06pm

Temperature Tests

Test	Status	Time
FC1	Pass	9:06pm
SRC	Pass	9:06pm
DET	Pass	9:06pm
BAR	Pass	9:06pm
BT	Pass	9:06pm

Blank Tests

Test	Status	Time
AIR	Pass	9:07pm


Printer Tests

Test	Status	Time
PRNT	Pass	9:07pm

CRC Tests

Test	Status	Time
COMP	Pass	9:07pm
CAL	Pass	9:07pm

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Edgecombe Instrument Location Edgecombe Co. Magistrate's Office
Instrument Serial No. 008588 Tarboro, N.C.

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 26th day of August, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

377722
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

EDGECOMBE COUNTY EDGECOMBE CO MAGISTR
320

Serial Number: 008588

Test Date: 08/26/2026

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Gray, Kelly D

Permit Number: 0037-7722

Effective:

02/01/2026-02/01/2028

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG602102

Exp Date: 01/21/2028

Test	g/210L	Time
DIAG	Pass	11:11am
AIR BLK	.00	11:12am
ACCY CHK	.08	11:12am
AIR BLK	.00	11:13am
SUB TEST	.00	11:14am
AIR BLK	.00	11:15am
SUB TEST	.00	11:17am
AIR BLK	.00	11:18am

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

EDGECOMBE COUNTY EDGECOMBE CO MAGISTR 320

Serial Number: 008588 Test Record Number: 1398
Test Date: 08/26/2026 Test Time: 11:19am EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	11:19am
FLO	Pass	11:19am
FC	Pass	11:19am

Temperature Tests

Test	Status	Time
FC1	Pass	11:19am
SRC	Pass	11:19am
DET	Pass	11:19am
BAR	Pass	11:19am
BT	Pass	11:19am

Blank Tests

Test	Status	Time
AIR	Pass	11:20am


Printer Tests

Test	Status	Time
PRNT	Pass	11:20am

CRC Tests

Test	Status	Time
COMP	Pass	11:20am
CAL	Pass	11:20am

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County FORSYTH Instrument Location FORSYTH COUNTY DETENTION
Instrument Serial No. 008583 WINSTON-SALEM, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 3RD day of AUGUST, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.




Signature of Certifying Official

353799
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

FORSYTH COUNTY DETENTION CENTER 330

Serial Number: 008583
Test Date: 08/03/2026

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Oligmueller, Leo A

Permit Number: 0035-3799

Effective:

02/01/2026-02/01/2028

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

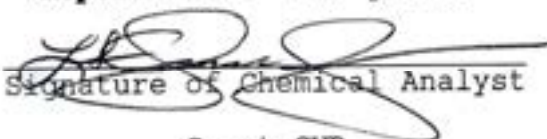
Test Type: Breath Test

Lot Number: AG602102

Exp Date: 01/21/2028

Test	g/210L	Time
DIAG	Pass	10:58am
AIR BLK	.00	10:58am
ACCY CHK	.08	10:59am
AIR BLK	.00	11:00am
SUB TEST	.00	11:01am
AIR BLK	.00	11:02am
SUB TEST	.00	11:04am
AIR BLK	.00	11:05am

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

FORSYTH COUNTY DETENTION CENTER 330

Serial Number: 008583 Test Record Number: 10201
Test Date: 08/03/2026 Test Time: 11:09am EDT

System Check: Passed

Baseline Tests

Test	Status	Time
IR	Pass	11:09am
FLO	Pass	11:09am
FC	Pass	11:09am

Temperature Tests

Test	Status	Time
FC1	Pass	11:09am
SRC	Pass	11:09am
DET	Pass	11:09am
BAR	Pass	11:09am
BT	Pass	11:09am

Blank Tests

Test	Status	Time
AIR	Pass	11:10am

Printer Tests

Test	Status	Time
PRNT	Pass	11:10am

CRC Tests

Test	Status	Time
COMP	Pass	11:10am
CAL	Pass	11:10am

**Preventive Maintenance
Status: Pass**


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County FORSYTH Instrument Location KERNERSVILLE POLICE DEPT
Instrument Serial No. 008650 KERNERSVILLE, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 3rd day of AUGUST, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



A stylized, handwritten signature in black ink, written over a horizontal line.
Signature of Certifying Official

353799
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

FORSYTH COUNTY KERNERSVILLE PD 330

Serial Number: 008650

Test Date: 08/03/2026

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Oligmueller, Leo A

Permit Number: 0035-3799

Effective:

02/01/2026-02/01/2028

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG602102

Exp Date: 01/21/2028

Test	g/210L	Time
DIAG	Pass	2:42pm
AIR BLK	.00	2:43pm
ACCY CHK	.07	2:44pm
AIR BLK	.00	2:45pm
SUB TEST	.00	2:45pm
AIR BLK	.00	2:46pm
SUB TEST	.00	2:48pm
AIR BLK	.00	2:49pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

FORSYTH COUNTY KERNERSVILLE PD 330

Serial Number: 008650 Test Record Number: 2556
Test Date: 08/03/2026 Test Time: 2:49pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	2:49pm
FLO	Pass	2:49pm
FC	Pass	2:49pm

Temperature Tests

Test	Status	Time
FC1	Pass	2:50pm
SRC	Pass	2:50pm
DET	Pass	2:50pm
BAR	Pass	2:50pm
BT	Pass	2:50pm

Blank Tests

Test	Status	Time
AIR	Pass	2:50pm

Printer Tests

Test	Status	Time
PRNT	Pass	2:50pm

CRC Tests

Test	Status	Time
COMP	Pass	2:50pm
CAL	Pass	2:50pm

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County FORSYTH Instrument Location FORSYTH COUNTY DETENTION
Instrument Serial No. 008659 WINSTON-SALEM, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 3RD day of AUGUST, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.




Signature of Certifying Official

353799
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

FORSYTH COUNTY DETENTION CENTER 330

Serial Number: 008659

Test Date: 08/03/2026

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Oligmueller, Leo A

Permit Number: 0035-3799

Effective:

02/01/2026-02/01/2028

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG602102

Exp Date: 01/21/2028

Test	g/210L	Time
DIAG	Pass	10:59am
AIR BLK	.00	10:59am
ACCY CHK	.07	11:00am
AIR BLK	.00	11:01am
SUB TEST	.00	11:02am
AIR BLK	.00	11:03am
SUB TEST	.00	11:05am
AIR BLK	.00	11:06am

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

FORSYTH COUNTY DETENTION CENTER 330

Serial Number: 008659 Test Record Number: 7029
Test Date: 08/03/2026 Test Time: 11:10am EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	11:10am
FLO	Pass	11:10am
FC	Pass	11:10am

Temperature Tests

Test	Status	Time
FC1	Pass	11:10am
SRC	Pass	11:10am
DET	Pass	11:10am
BAR	Pass	11:10am
BT	Pass	11:10am

Blank Tests

Test	Status	Time
AIR	Pass	11:11am

Printer Tests

Test	Status	Time
PRNT	Pass	11:11am

CRC Tests

Test	Status	Time
COMP	Pass	11:11am
CAL	Pass	11:11am

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County FORSYTH Instrument Location FORSYTH COUNTY DETENTION

Instrument Serial No. 008925 WINSTON-SALEM, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 3RD day of AUGUST, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



A handwritten signature in black ink, appearing to be "J. E. Smith", written over a horizontal line.
Signature of Certifying Official

353799
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

FORSYTH COUNTY DETENTION CENTER 330

Serial Number: 008925

Test Date: 08/03/2026

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Oligmueller, Leo A

Permit Number: 0035-3799

Effective:

02/01/2026-02/01/2028

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG602102

Exp Date: 01/21/2028

Test	g/210L	Time
DIAG	Pass	11:07am
AIR BLK	.00	11:08am
ACCY CHK	.08	11:08am
AIR BLK	.00	11:09am
SUB TEST	.00	11:10am
AIR BLK	.00	11:11am
SUB TEST	.00	11:12am
AIR BLK	.00	11:13am

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

FORSYTH COUNTY DETENTION CENTER 330

Serial Number: 008925 Test Record Number: 5986
Test Date: 08/03/2026 Test Time: 11:16am EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	11:16am
FLO	Pass	11:16am
FC	Pass	11:17am

Temperature Tests

Test	Status	Time
FC1	Pass	11:17am
SRC	Pass	11:17am
DET	Pass	11:17am
BAR	Pass	11:17am
BT	Pass	11:17am

Blank Tests

Test	Status	Time
AIR	Pass	11:17am

Printer Tests

Test	Status	Time
PRNT	Pass	11:17am

CRC Tests

Test	Status	Time
COMP	Pass	11:17am
CAL	Pass	11:17am

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Gates Instrument Location Gates Co. S.O.
Instrument Serial No. 008884 Gatesville, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 24th day of August, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

206272
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

GATES COUNTY GATES CO SO 360

Serial Number: 008884
Test Date: 08/24/2026

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE

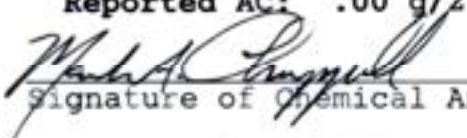
Analyst's Name: Chappell, Mark A
Permit Number: 0020-6272
Effective:
02/01/2026-02/01/2028

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

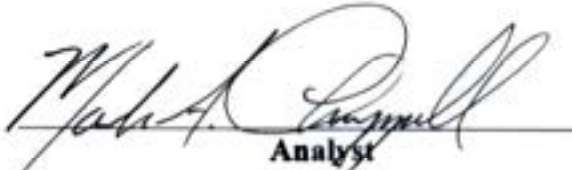
Lot Number: AG501303
Exp Date: 01/13/2027

Test	g/210L	Time
DIAG	Pass	4:03pm
AIR BLK	.00	4:04pm
ACCY CHK	.07	4:05pm
AIR BLK	.00	4:06pm
SUB TEST	.00	4:06pm
AIR BLK	.00	4:07pm
SUB TEST	.00	4:09pm
AIR BLK	.00	4:10pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

GATES COUNTY GATES CO SO 360

Serial Number: 008884 Test Record Number: 1318
Test Date: 08/24/2026 Test Time: 4:12pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	4:12pm
FLO	Pass	4:12pm
FC	Pass	4:12pm

Temperature Tests

Test	Status	Time
FC1	Pass	4:12pm
SRC	Pass	4:12pm
DET	Pass	4:12pm
BAR	Pass	4:12pm
BT	Pass	4:12pm

Blank Tests

Test	Status	Time
AIR	Pass	4:13pm

Printer Tests

Test	Status	Time
PRNT	Pass	4:13pm

CRC Tests

Test	Status	Time
COMP	Pass	4:13pm
CAL	Pass	4:13pm

Preventive Maintenance
Status: Pass


Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Guilford Instrument Location BAT Mobile Unit 13

Instrument Serial No. 008869

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 14th day of August, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



John Panier
Signature of Certifying Official

1604930
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

GUILFORD COUNTY BAT MOBILE UNIT 13 400

Serial Number: 008869

Test Date: 08/14/2026

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Lanier Jr., John P

Permit Number: 4582-9118

Effective:

02/01/2026-02/01/2028

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

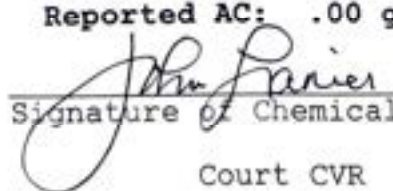
Test Type: Breath Test

Lot Number: AG506303

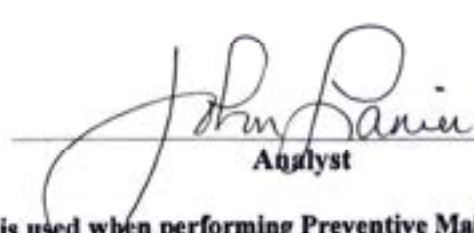
Exp Date: 03/04/2027

Test	g/210L	Time
DIAG	Pass	8:46pm
AIR BLK	.00	8:47pm
ACCY CHK	.08	8:48pm
AIR BLK	.00	8:49pm
SUB TEST	.00	8:49pm
AIR BLK	.00	8:50pm
SUB TEST	.00	8:51pm
AIR BLK	.00	8:52pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

GUILFORD COUNTY BAT MOBILE UNIT 13 400

Serial Number: 008869 Test Record Number: 2277
Test Date: 08/14/2026 Test Time: 8:53pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	8:53pm
FLO	Pass	8:53pm
FC	Pass	8:53pm

Temperature Tests

Test	Status	Time
FC1	Pass	8:53pm
SRC	Pass	8:53pm
DET	Pass	8:53pm
BAR	Pass	8:53pm
BT	Pass	8:53pm

Blank Tests

Test	Status	Time
AIR	Pass	8:54pm

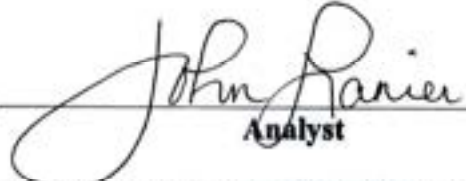
Printer Tests

Test	Status	Time
PRNT	Pass	8:54pm

CRC Tests

Test	Status	Time
COMP	Pass	8:54pm
CAL	Pass	8:54pm

Preventive Maintenance
Status: Pass


Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Guilford Instrument Location BAT Mobile Unit 13

Instrument Serial No. 008898

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 14th day of August, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



John Lanier
Signature of Certifying Official

1604930
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

GUILFORD COUNTY BAT MOBILE UNIT 13 400

Serial Number: 008898
Test Date: 08/14/2026

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Lanier Jr., John P

Permit Number: 4582-9118

Effective:

02/01/2026-02/01/2028

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

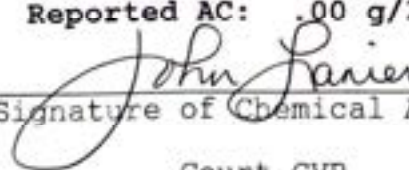
Test Type: Breath Test

Lot Number: AG506302

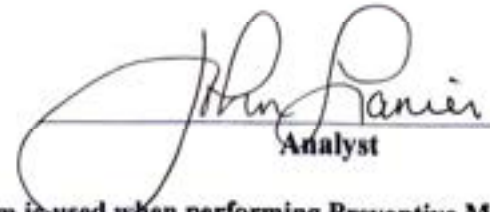
Exp Date: 03/04/2027

Test	g/210L	Time
DIAG	Pass	8:40pm
AIR BLK	.00	8:41pm
ACCY CHK	.07	8:41pm
AIR BLK	.00	8:42pm
SUB TEST	.00	8:44pm
AIR BLK	.00	8:45pm
SUB TEST	.00	8:46pm
AIR BLK	.00	8:47pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

GUILFORD COUNTY BAT MOBILE UNIT 13 400

Serial Number: 008898 Test Record Number: 2210
Test Date: 08/14/2026 Test Time: 8:48pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	8:48pm
FLO	Pass	8:48pm
FC	Pass	8:48pm

Temperature Tests

Test	Status	Time
FC1	Pass	8:48pm
SRC	Pass	8:48pm
DET	Pass	8:48pm
BAR	Pass	8:48pm
BT	Pass	8:48pm

Blank Tests

Test	Status	Time
AIR	Pass	8:49pm

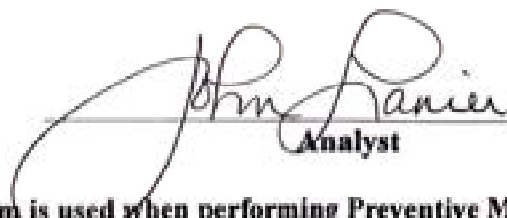
Printer Tests

Test	Status	Time
PRNT	Pass	8:49pm

CRC Tests

Test	Status	Time
COMP	Pass	8:49pm
CAL	Pass	8:49pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Guilford Instrument Location BAT Mobile Unit 13

Instrument Serial No. 008939

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 14th day of August, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



John Paria
Signature of Certifying Official

1604930
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

GUILFORD COUNTY BAT MOBILE UNIT 13 400

Serial Number: 008939

Test Date: 08/14/2026

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Lanier Jr., John P

Permit Number: 4582-9118

Effective:

02/01/2026-02/01/2028

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

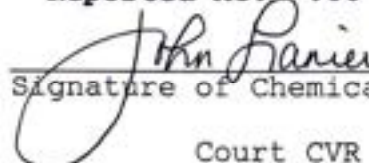
Test Type: Breath Test

Lot Number: AG506302

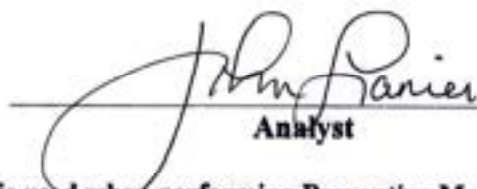
Exp Date: 03/04/2027

Test	g/210L	Time
DIAG	Pass	8:21pm
AIR BLK	.00	8:23pm
ACCY CHK	.07	8:23pm
AIR BLK	.00	8:24pm
SUB TEST	.00	8:26pm
AIR BLK	.00	8:27pm
SUB TEST	.00	8:28pm
AIR BLK	.00	8:29pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

GUILFORD COUNTY BAT MOBILE UNIT 13 400

Serial Number: 008939 Test Record Number: 2062
Test Date: 08/14/2026 Test Time: 8:30pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	8:30pm
FLO	Pass	8:30pm
FC	Pass	8:30pm

Temperature Tests

Test	Status	Time
FC1	Pass	8:30pm
SRC	Pass	8:30pm
DET	Pass	8:30pm
BAR	Pass	8:30pm
BT	Pass	8:30pm

Blank Tests

Test	Status	Time
AIR	Pass	8:31pm

Printer Tests

Test	Status	Time
PRNT	Pass	8:31pm

CRC Tests

Test	Status	Time
COMP	Pass	8:31pm
CAL	Pass	8:31pm

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Guilford Instrument Location BAT Mobile Unit II

Instrument Serial No. 008970

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 27th day of August, 2020 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

1604930
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

GUILFORD COUNTY BAT MOBILE UNIT 11 400

Serial Number: 008970

Test Date: 08/27/2026

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Lanier Jr., John P

Permit Number: 4582-9118

Effective:

02/01/2026-02/01/2028

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

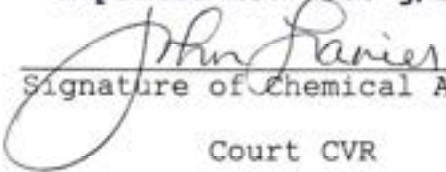
Test Type: Breath Test

Lot Number: AG602101

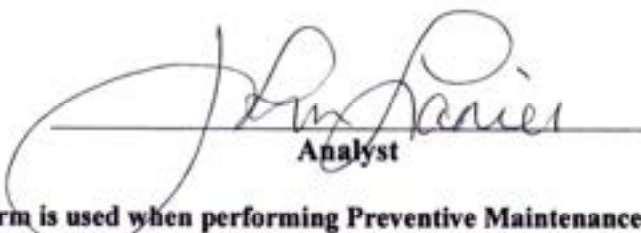
Exp Date: 01/21/2028

Test	g/210L	Time
DIAG	Pass	8:59pm
AIR BLK	.00	9:00pm
ACCY CHK	.07	9:00pm
AIR BLK	.00	9:01pm
SUB TEST	.00	9:02pm
AIR BLK	.00	9:03pm
SUB TEST	.00	9:04pm
AIR BLK	.00	9:05pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

GUILFORD COUNTY BAT MOBILE UNIT 11 400

Serial Number: 008970 Test Record Number: 1519
Test Date: 08/27/2026 Test Time: 9:06pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	9:06pm
FLO	Pass	9:06pm
FC	Pass	9:06pm

Temperature Tests

Test	Status	Time
FC1	Pass	9:06pm
SRC	Pass	9:06pm
DET	Pass	9:06pm
BAR	Pass	9:06pm
BT	Pass	9:06pm

Blank Tests

Test	Status	Time
AIR	Pass	9:07pm

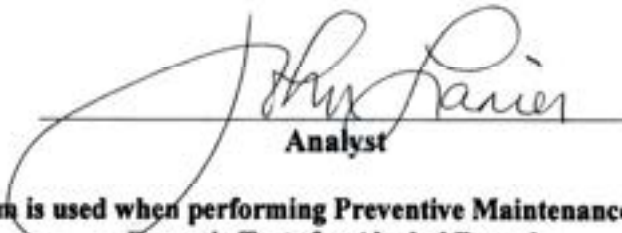
Printer Tests

Test	Status	Time
PRNT	Pass	9:07pm

CRC Tests

Test	Status	Time
COMP	Pass	9:07pm
CAL	Pass	9:07pm

Preventive Maintenance
Status: *Pass*


Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County GUILFORD Instrument Location GREENSBORO JAIL

Instrument Serial No. 008660 GREENSBORO, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 10TH day of AUGUST, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.




Signature of Certifying Official

353799
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

GUILFORD COUNTY GREENSBORO JAIL 400

Serial Number: 008660

Test Date: 08/10/2026

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Oligmueller, Leo A

Permit Number: 0035-3799

Effective:

02/01/2026-02/01/2028

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

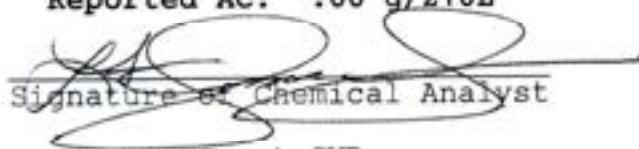
Test Type: Breath Test

Lot Number: AG602102

Exp Date: 01/21/2028

Test	g/210L	Time
DIAG	Pass	10:36am
AIR BLK	.00	10:37am
ACCY CHK	.07	10:37am
AIR BLK	.00	10:38am
SUB TEST	.00	10:39am
AIR BLK	.00	10:40am
SUB TEST	.00	10:41am
AIR BLK	.00	10:43am

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

GUILFORD COUNTY GREENSBORO JAIL 400

Serial Number: 008660 Test Record Number: 4820
Test Date: 08/10/2026 Test Time: 10:44am EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	10:44am
FLO	Pass	10:44am
FC	Pass	10:45am

Temperature Tests

Test	Status	Time
FC1	Pass	10:45am
SRC	Pass	10:45am
DET	Pass	10:45am
BAR	Pass	10:45am
BT	Pass	10:45am

Blank Tests

Test	Status	Time
AIR	Pass	10:45am

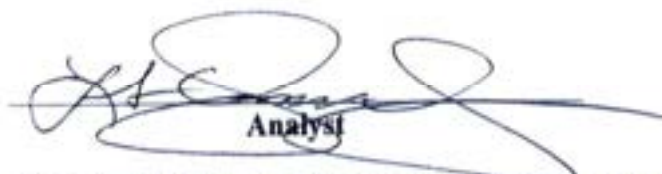
Printer Tests

Test	Status	Time
PRNT	Pass	10:45am

CRC Tests

Test	Status	Time
COMP	Pass	10:46am
CAL	Pass	10:46am

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Guilford Instrument Location Gibsonville Police Dept.
Instrument Serial No. 008812 Gibsonville, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 29th day of July, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.




Signature of Certifying Official

509387
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

GUILFORD COUNTY GIBSONVILLE PD 400

Serial Number: 008812
Test Date: 07/29/2026

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE

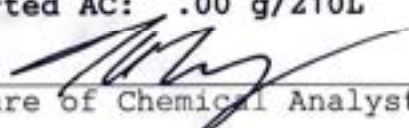
Analyst's Name: Long, Thomas A
Permit Number: 0050-9387
Effective:
02/01/2026-02/01/2028

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG602102
Exp Date: 01/21/2028

Test	g/210L	Time
DIAG	Pass	7:57am
AIR BLK	.00	7:57am
ACCY CHK	.08	7:58am
AIR BLK	.00	7:59am
SUB TEST	.00	7:59am
AIR BLK	.00	8:00am
SUB TEST	.00	8:02am
AIR BLK	.00	8:03am

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

GUILFORD COUNTY GIBSONVILLE PD 400

Serial Number: 008812 Test Record Number: 3918
Test Date: 07/29/2026 Test Time: 8:04am EDT

System Check: Passed

Baseline Tests

Test	Status	Time
IR	Pass	8:04am
FLO	Pass	8:04am
FC	Pass	8:04am

Temperature Tests

Test	Status	Time
FC1	Pass	8:04am
SRC	Pass	8:04am
DET	Pass	8:04am
BAR	Pass	8:04am
BT	Pass	8:04am

Blank Tests

Test	Status	Time
AIR	Pass	8:05am

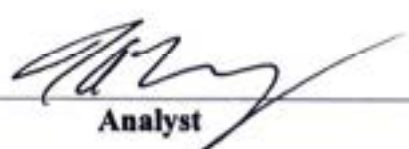
Printer Tests

Test	Status	Time
PRNT	Pass	8:05am

CRC Tests

Test	Status	Time
COMP	Pass	8:05am
CAL	Pass	8:05am

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Guilford Instrument Location BAT Mobile Unit II

Instrument Serial No. 008973

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 27th day of August, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

1604930
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

GUILFORD COUNTY BAT MOBILE UNIT 11 400

Serial Number: 008973

Test Date: 08/27/2026

Citation Number: M00000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Lanier Jr., John P

Permit Number: 4582-9118

Effective:

02/01/2026-02/01/2028

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

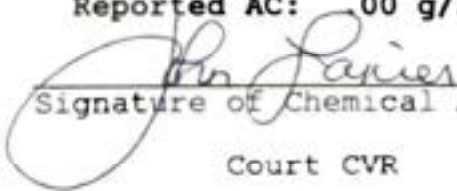
Test Type: Breath Test

Lot Number: AG431003

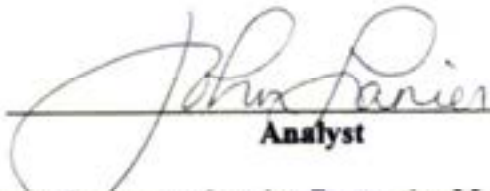
Exp Date: 11/05/2026

Test	g/210L	Time
DIAG	Pass	8:49pm
AIR BLK	.00	8:49pm
ACCY CHK	.07	8:50pm
AIR BLK	.00	8:51pm
SUB TEST	.00	8:52pm
AIR BLK	.00	8:53pm
SUB TEST	.00	8:54pm
AIR BLK	.00	8:55pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

GUILFORD COUNTY BAT MOBILE UNIT 11 400

Serial Number: 008973 Test Record Number: 1557
Test Date: 08/27/2026 Test Time: 8:56pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	8:57pm
FLO	Pass	8:57pm
FC	Pass	8:57pm

Temperature Tests

Test	Status	Time
FC1	Pass	8:57pm
SRC	Pass	8:57pm
DET	Pass	8:57pm
BAR	Pass	8:57pm
BT	Pass	8:57pm

Blank Tests

Test	Status	Time
AIR	Pass	8:57pm

Printer Tests

Test	Status	Time
PRNT	Pass	8:57pm

CRC Tests

Test	Status	Time
COMP	Pass	8:58pm
CAL	Pass	8:58pm

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County HALIFAX Instrument Location BAT Mobile Unit 12

Instrument Serial No. 008601

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 1st day of August, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.





Signature of Certifying Official

83034

Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

HALIFAX COUNTY BAT MOBILE UNIT 12 410

Serial Number: 008601

Test Date: 08/01/2026

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name:

Crutchfield Jr., Marshall B

Permit Number: 0008-3034

Effective:

03/01/2026-03/01/2028

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG501307

Exp Date: 01/13/2027


Test	g/210L	Time
DIAG	Pass	5:37pm
AIR BLK	.00	5:38pm
ACCY CHK	.07	5:38pm
AIR BLK	.00	5:39pm
SUB TEST	.00	5:40pm
AIR BLK	.00	5:41pm
SUB TEST	.00	5:42pm
AIR BLK	.00	5:43pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

HALIFAX COUNTY BAT MOBILE UNIT 12 410

Serial Number: 008601 Test Record Number: 1978
Test Date: 08/01/2026 Test Time: 5:44pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	5:45pm
FLO	Pass	5:45pm
FC	Pass	5:45pm

Temperature Tests

Test	Status	Time
FC1	Pass	5:45pm
SRC	Pass	5:45pm
DET	Pass	5:45pm
BAR	Pass	5:45pm
BT	Pass	5:45pm

Blank Tests

Test	Status	Time
AIR	Pass	5:45pm

Printer Tests

Test	Status	Time
PRNT	Pass	5:45pm

CRC Tests

Test	Status	Time
COMP	Pass	5:46pm
CAL	Pass	5:46pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County HALIFAX Instrument Location Bar Mobile Unit 12
Instrument Serial No. 008698

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 1st day of August, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.




Signature of Certifying Official

83034
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

HALIFAX COUNTY BAT MOBILE UNIT 12 410

Serial Number: 008698

Test Date: 08/01/2026

Citation Number: M00000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name:

Crutchfield Jr., Marshall B

Permit Number: 0008-3034

Effective:

03/01/2026-03/01/2028

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG431002

Exp Date: 11/05/2026

Test	g/210L	Time
DIAG	Pass	5:40pm
AIR BLK	.00	5:42pm
ACCY CHK	.08	5:42pm
AIR BLK	.00	5:43pm
SUB TEST	.00	5:44pm
AIR BLK	.00	5:44pm
SUB TEST	.00	5:46pm
AIR BLK	.00	5:47pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

Intox EC/IR-II: Preventive Maintenance

HALIFAX COUNTY BAT MOBILE UNIT 12 410

Serial Number: 008698 Test Record Number: 2808
Test Date: 08/01/2026 Test Time: 5:49pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	5:49pm
FLO	Pass	5:49pm
FC	Pass	5:49pm

Temperature Tests

Test	Status	Time
FC1	Pass	5:50pm
SRC	Pass	5:50pm
DET	Pass	5:50pm
BAR	Pass	5:50pm
BT	Pass	5:50pm

Blank Tests

Test	Status	Time
AIR	Pass	5:50pm

Printer Tests

Test	Status	Time
PRNT	Pass	5:50pm

CRC Tests

Test	Status	Time
COMP	Pass	5:50pm
CAL	Pass	5:50pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County HALIFAX Instrument Location BAT Mobile Unit 12
Instrument Serial No. 008788

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 1st day of August, 2006 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Signature of Certifying Official

Certificate Number

83034

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

HALIFAX COUNTY BAT MOBILE UNIT 12 410

Serial Number: 008788

Test Date: 08/01/2026

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name:

Crutchfield Jr., Marshall B

Permit Number: 0008-3034

Effective:

03/01/2026-03/01/2028

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG534301

Exp Date: 12/09/2027

Test	g/210L	Time
DIAG	Pass	5:49pm
AIR BLK	.00	5:50pm
ACCY CHK	.08	5:50pm
AIR BLK	.00	5:51pm
SUB TEST	.00	5:53pm
AIR BLK	.00	5:54pm
SUB TEST	.00	5:55pm
AIR BLK	.00	5:56pm

Reported AC: 0.00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

HALIFAX COUNTY BAT MOBILE UNIT 12 410

Serial Number: 008788 Test Record Number: 2592
Test Date: 08/01/2026 Test Time: 5:58pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	5:58pm
FLO	Pass	5:58pm
FC	Pass	5:58pm

Temperature Tests

Test	Status	Time
FC1	Pass	5:58pm
SRC	Pass	5:58pm
DET	Pass	5:58pm
BAR	Pass	5:58pm
BT	Pass	5:58pm

Blank Tests

Test	Status	Time
AIR	Pass	5:59pm

Printer Tests

Test	Status	Time
PRNT	Pass	5:59pm

CRC Tests

Test	Status	Time
COMP	Pass	5:59pm
CAL	Pass	5:59pm

Preventive Maintenance
Status: Pass



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Harnett Instrument Location Harnett County Detention
Instrument Serial No. 008729 Lillington, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 6 day of August, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

365156
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

HARNETT COUNTY DETENTION CENTER 420

Serial Number: 008729

Test Date: 08/06/2026

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Garner, Joel K

Permit Number: 0036-5156

Effective:

02/01/2026-02/01/2028

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

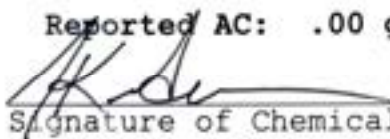
Test Type: Breath Test

Lot Number: AG534301

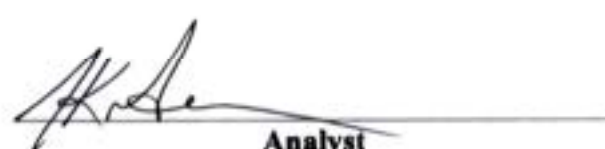
Exp Date: 12/09/2027

Test	g/210L	Time
DIAG	Pass	2:18pm
AIR BLK	.00	2:19pm
ACCY CHK	.08	2:20pm
AIR BLK	.00	2:21pm
SUB TEST	.00	2:22pm
AIR BLK	.00	2:23pm
SUB TEST	.00	2:25pm
AIR BLK	.00	2:26pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

HARNETT COUNTY DETENTION CENTER 420

Serial Number: 008729 Test Record Number: 3734
Test Date: 08/06/2026 Test Time: 2:26pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	2:27pm
FLO	Pass	2:27pm
FC	Pass	2:27pm

Temperature Tests

Test	Status	Time
FC1	Pass	2:27pm
SRC	Pass	2:27pm
DET	Pass	2:27pm
BAR	Pass	2:27pm
BT	Pass	2:27pm

Blank Tests

Test	Status	Time
AIR	Pass	2:27pm

Printer Tests

Test	Status	Time
PRNT	Pass	2:27pm

CRC Tests

Test	Status	Time
COMP	Pass	2:28pm
CAL	Pass	2:28pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Harnett Instrument Location Harnett County Detention
Instrument Serial No. 008730 Lillington, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 6 day of August, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

365156
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

HARNETT COUNTY DETENTION CENTER 420

Serial Number: 008730

Test Date: 08/06/2026

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Garner, Joel K

Permit Number: 0036-5156

Effective:

02/01/2026-02/01/2028

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG534301

Exp Date: 12/09/2027

Test	g/210L	Time
DIAG	Pass	2:21pm
AIR BLK	.00	2:22pm
ACCY CHK	.07	2:23pm
AIR BLK	.00	2:23pm
SUB TEST	.00	2:24pm
AIR BLK	.00	2:25pm
SUB TEST	.00	2:26pm
AIR BLK	.00	2:27pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

HARNETT COUNTY DETENTION CENTER 420

Serial Number: 008730 Test Record Number: 5137
Test Date: 08/06/2026 Test Time: 2:30pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	2:30pm
FLO	Pass	2:30pm
FC	Pass	2:30pm

Temperature Tests

Test	Status	Time
FC1	Pass	2:30pm
SRC	Pass	2:30pm
DET	Pass	2:30pm
BAR	Pass	2:30pm
BT	Pass	2:30pm

Blank Tests

Test	Status	Time
AIR	Pass	2:31pm

Printer Tests

Test	Status	Time
PRNT	Pass	2:31pm

CRC Tests

Test	Status	Time
COMP	Pass	2:31pm
CAL	Pass	2:31pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Hertford Instrument Location Ahoskie P.D.
Instrument Serial No. 008848 Ahoskie, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 24th day of August, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

206272
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

HERTFORD COUNTY AHOSKIE PD 450

Serial Number: 008848

Test Date: 08/24/2026

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Chappell, Mark A

Permit Number: 0020-6272

Effective:

02/01/2026-02/01/2028

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

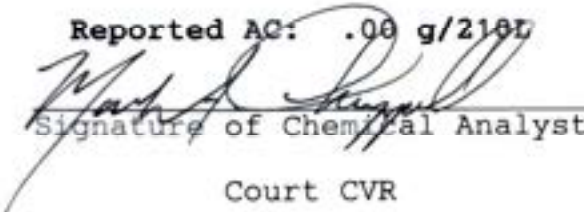
Test Type: Breath Test

Lot Number: AG501303

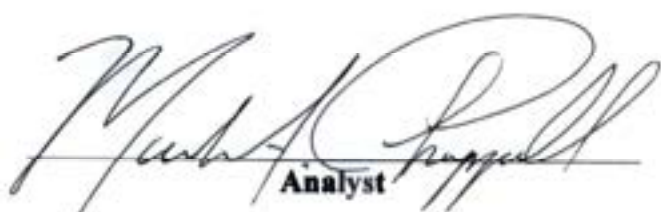
Exp Date: 01/13/2027

Test	g/210L	Time
DIAG	Pass	1:35pm
AIR BLK	.00	1:36pm
ACCY CHK	.08	1:37pm
AIR BLK	.00	1:38pm
SUB TEST	.00	1:38pm
AIR BLK	.00	1:39pm
SUB TEST	.00	1:41pm
AIR BLK	.00	1:42pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

HERTFORD COUNTY AHOSKIE PD 450

Serial Number: 008848 Test Record Number: 2052
Test Date: 08/24/2026 Test Time: 1:42pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	1:43pm
FLO	Pass	1:43pm
FC	Pass	1:43pm

Temperature Tests

Test	Status	Time
FC1	Pass	1:43pm
SRC	Pass	1:43pm
DET	Pass	1:43pm
BAR	Pass	1:43pm
BT	Pass	1:43pm

Blank Tests

Test	Status	Time
AIR	Pass	1:44pm

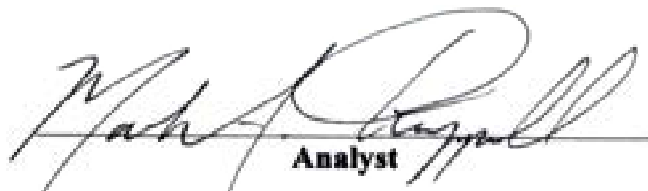
Printer Tests

Test	Status	Time
PRNT	Pass	1:44pm

CRC Tests

Test	Status	Time
COMP	Pass	1:44pm
CAL	Pass	1:44pm

Preventive Maintenance
Status: *Pass*


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Hertford Instrument Location Murfreesboro P.D.
Instrument Serial No. 008906 Murfreesboro, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 24th day of August, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

206272
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

HERTFORD COUNTY MURFREESBORO PD 450

Serial Number: 008906

Test Date: 08/24/2026

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Chappell, Mark A

Permit Number: 0020-6272

Effective:

02/01/2026-02/01/2028

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

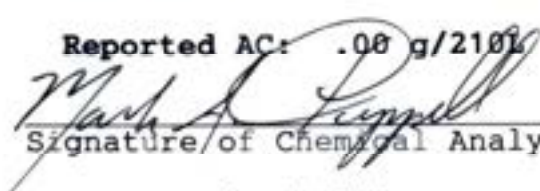
Test Type: Breath Test

Lot Number: AG501303

Exp Date: 01/13/2027

Test	g/210L	Time
DIAG	Pass	2:35pm
AIR BLK	.00	2:36pm
ACCY CHK	.08	2:36pm
AIR BLK	.00	2:38pm
SUB TEST	.00	2:38pm
AIR BLK	.00	2:39pm
SUB TEST	.00	2:41pm
AIR BLK	.00	2:42pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

HERTFORD COUNTY MURFREESBORO PD 450

Serial Number: 008906 Test Record Number: 1032
Test Date: 08/24/2026 Test Time: 2:42pm EDT

System Check: Passed

Baseline Tests

Test	Status	Time
IR	Pass	2:43pm
FLO	Pass	2:43pm
FC	Pass	2:43pm

Temperature Tests

Test	Status	Time
FC1	Pass	2:43pm
SRC	Pass	2:43pm
DET	Pass	2:43pm
BAR	Pass	2:43pm
BT	Pass	2:43pm

Blank Tests

Test	Status	Time
AIR	Pass	2:44pm

Printer Tests

Test	Status	Time
PRNT	Pass	2:44pm

CRC Tests

Test	Status	Time
COMP	Pass	2:44pm
CAL	Pass	2:44pm

Preventive Maintenance
Status: Pass


Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Hoke Instrument Location Hoke County Detention
Instrument Serial No. 008852 Raeford, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 17 day of August, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

365156
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

HOKE COUNTY DETENTION CENTER 460

Serial Number: 008852

Test Date: 08/17/2026

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Garner, Joel K

Permit Number: 0036-5156

Effective:

02/01/2026-02/01/2028

Officer's Name: NONE, NONE

Type of Agency: PTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG534301

Exp Date: 12/09/2027

Test	g/210L	Time
DIAG	Pass	8:20am
AIR BLK	.00	8:21am
ACCY CHK	.08	8:21am
AIR BLK	.00	8:22am
SUB TEST	.00	8:23am
AIR BLK	.00	8:24am
SUB TEST	.00	8:26am
AIR BLK	.00	8:27am

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

This form is used when performing Preventive Maintenance procedures

Forensic Tests for Alcohol Branch

Department of Health and Human Services

Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

HOKE COUNTY DETENTION CENTER 460

Serial Number: 008852 Test Record Number: 1880
Test Date: 08/17/2026 Test Time: 8:28am EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	8:28am
FLO	Pass	8:28am
FC	Pass	8:28am

Temperature Tests

Test	Status	Time
FC1	Pass	8:28am
SRC	Pass	8:28am
DET	Pass	8:28am
BAR	Pass	8:28am
BT	Pass	8:28am

Blank Tests

Test	Status	Time
AIR	Pass	8:29am

Printer Tests

Test	Status	Time
PRNT	Pass	8:29am

CRC Tests

Test	Status	Time
COMP	Pass	8:29am
CAL	Pass	8:29am

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Hoke Instrument Location Hoke County Detention
Instrument Serial No. 008855 Raeford, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 17 day of August, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Signature of Certifying Official

365156

Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

HOKE COUNTY DETENTION CENTER 460

Serial Number: 008855

Test Date: 08/17/2026

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Garner, Joel K

Permit Number: 0036-5156

Effective:

02/01/2026-02/01/2028

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG534301

Exp Date: 12/09/2027

Test	g/210L	Time
DIAG	Pass	8:21am
AIR BLK	.00	8:21am
ACCY CHK	.08	8:22am
AIR BLK	.00	8:23am
SUB TEST	.00	8:24am
AIR BLK	.00	8:24am
SUB TEST	.00	8:26am
AIR BLK	.00	8:27am

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

HOKE COUNTY DETENTION CENTER 460

Serial Number: 008855 Test Record Number: 2069
Test Date: 08/17/2026 Test Time: 8:28am EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	8:29am
FLO	Pass	8:29am
FC	Pass	8:29am

Temperature Tests

Test	Status	Time
FC1	Pass	8:29am
SRC	Pass	8:29am
DET	Pass	8:29am
BAR	Pass	8:29am
BT	Pass	8:29am

Blank Tests

Test	Status	Time
AIR	Pass	8:29am

Printer Tests

Test	Status	Time
PRNT	Pass	8:29am

CRC Tests

Test	Status	Time
COMP	Pass	8:30am
CAL	Pass	8:30am

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Hyde Instrument Location Hyde Co. S. O.
Instrument Serial No. 008797 Acraoke, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 25th day of August, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

206272
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

HYDE COUNTY HYDE CO SO OCRACOKE 470

Serial Number: 008797

Test Date: 08/25/2026

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Chappell, Mark A

Permit Number: 0020-6272

Effective:

02/01/2026-02/01/2028

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG516203

Exp Date: 06/11/2027

Test	g/210L	Time
DIAG	Pass	10:01am
AIR BLK	.00	10:02am
ACCY CHK	.07	10:03am
AIR BLK	.00	10:04am
SUB TEST	.00	10:05am
AIR BLK	.00	10:06am
SUB TEST	.00	10:07am
AIR BLK	.00	10:08am

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

HYDE COUNTY HYDE CO SO OCRACOKE 470

Serial Number: 008797 Test Record Number: 784
Test Date: 08/25/2026 Test Time: 10:09am EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	10:09am
FLO	Pass	10:09am
FC	Pass	10:09am

Temperature Tests

Test	Status	Time
FC1	Pass	10:09am
SRC	Pass	10:09am
DET	Pass	10:09am
BAR	Pass	10:09am
BT	Pass	10:09am

Blank Tests

Test	Status	Time
AIR	Pass	10:10am

Printer Tests

Test	Status	Time
PRNT	Pass	10:10am

CRC Tests

Test	Status	Time
COMP	Pass	10:10am
CAL	Pass	10:10am

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Hyde Instrument Location Hyde Co. S.O.
Instrument Serial No. 008801 Swain Quarter, N.C.

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 6th day of August, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

377722
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

HYDE COUNTY HYDE CO SO SWAN QUAR 470

Serial Number: 008801

Test Date: 08/06/2026

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Gray, Kelly D

Permit Number: 0037-7722

Effective:

02/01/2026-02/01/2028

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG506301

Exp Date: 03/04/2027

Test	g/210L	Time
DIAG	Pass	10:56am
AIR BLK	.00	10:56am
ACCY CHK	.07	10:57am
AIR BLK	.00	10:58am
SUB TEST	.00	10:58am
AIR BLK	.00	10:59am
SUB TEST	.00	11:01am
AIR BLK	.00	11:02am

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

HYDE COUNTY HYDE CO SO SWAN QUAR 470

Serial Number: 008801 Test Record Number: 820
Test Date: 08/06/2026 Test Time: 11:03am EDT

System Check: Passed

Baseline Tests

Test	Status	Time
IR	Pass	11:04am
FLO	Pass	11:04am
FC	Pass	11:04am

Temperature Tests

Test	Status	Time
FC1	Pass	11:04am
SRC	Pass	11:04am
DET	Pass	11:04am
BAR	Pass	11:04am
BT	Pass	11:04am

Blank Tests

Test	Status	Time
AIR	Pass	11:04am

Printer Tests

Test	Status	Time
PRNT	Pass	11:05am

CRC Tests

Test	Status	Time
COMP	Pass	11:05am
CAL	Pass	11:05am

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Iredell Instrument Location BAT Mobile Unit 8
Instrument Serial No. 008615 —

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 8 day of August, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

2219283
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

IREDELL COUNTY BAT MOBILE UNIT 8 480

Serial Number: 008615

Test Date: 08/08/2026

Citation Number: M00000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Glasscock, Jerry D

Permit Number: 7180-9235

Effective:

02/01/2026-02/01/2028

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

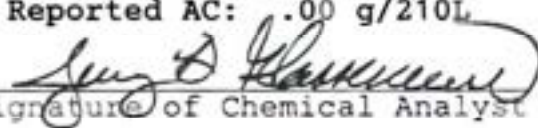
Test Type: Breath Test

Lot Number: AG506303

Exp Date: 03/04/2027

Test	g/210L	Time
DIAG	Pass	11:07pm
AIR BLK	.00	11:08pm
ACCY CHK	.07	11:08pm
AIR BLK	.00	11:09pm
SUB TEST	.00	11:10pm
AIR BLK	.00	11:11pm
SUB TEST	.00	11:12pm
AIR BLK	.00	11:13pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

IREDELL COUNTY BAT MOBILE UNIT 8 480

Serial Number: 008615 Test Record Number: 6383
Test Date: 08/08/2026 Test Time: 11:13pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	11:14pm
FLO	Pass	11:14pm
FC	Pass	11:14pm

Temperature Tests

Test	Status	Time
FC1	Pass	11:14pm
SRC	Pass	11:14pm
DET	Pass	11:14pm
BAR	Pass	11:14pm
BT	Pass	11:14pm

Blank Tests

Test	Status	Time
AIR	Pass	11:14pm

Printer Tests

Test	Status	Time
PRNT	Pass	11:14pm

CRC Tests

Test	Status	Time
COMP	Pass	11:15pm
CAL	Pass	11:15pm

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Iredell Instrument Location BAT Mobile Unit 8

Instrument Serial No. 008615 ✓

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 18 day of August, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

2219283
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

IREDELL COUNTY BAT MOBILE UNIT 8 480

Serial Number: 008615
Test Date: 08/18/2026

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Glasscock, Jerry D

Permit Number: 7180-9235

Effective:

02/01/2026-02/01/2028

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG506303

Exp Date: 03/04/2027

Test	g/210L	Time
DIAG	Pass	10:13pm
AIR BLK	.00	10:14pm
ACCY CHK	.07	10:14pm
AIR BLK	.00	10:15pm
SUB TEST	.00	10:17pm
AIR BLK	.00	10:18pm
SUB TEST	.00	10:20pm
AIR BLK	.00	10:21pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

IREDELL COUNTY BAT MOBILE UNIT 8 480

Serial Number: 008615 Test Record Number: 6387
Test Date: 08/18/2026 Test Time: 10:21pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	10:21pm
FLO	Pass	10:21pm
FC	Pass	10:21pm

Temperature Tests

Test	Status	Time
FC1	Pass	10:21pm
SRC	Pass	10:21pm
DET	Pass	10:21pm
BAR	Pass	10:21pm
BT	Pass	10:21pm

Blank Tests

Test	Status	Time
AIR	Pass	10:22pm

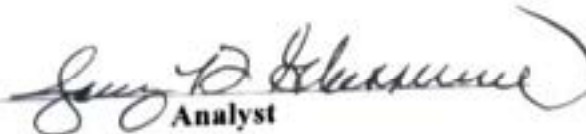
Printer Tests

Test	Status	Time
PRNT	Pass	10:22pm

CRC Tests

Test	Status	Time
COMP	Pass	10:22pm
CAL	Pass	10:22pm

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County IRENELL Instrument Location STATENVILLE PD

Instrument Serial No. 0086191 STATENVILLE NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 05 day of AUGUST, 2020 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

214970
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

IREDELL COUNTY STATESVILLE PD 480

Serial Number: 008619

Test Date: 08/05/2026

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Fleming, Tina S

Permit Number: 0027-4970

Effective:

02/01/2025-02/01/2027

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG534301

Exp Date: 12/09/2027

Test	g/210L	Time
DIAG	Pass	4:48pm
AIR BLK	.00	4:49pm
ACCY CHK	.07	4:49pm
AIR BLK	.00	4:50pm
SUB TEST	.00	4:51pm
AIR BLK	.00	4:52pm
SUB TEST	.00	4:54pm
AIR BLK	.00	4:54pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

IREDELL COUNTY STATESVILLE PD 480

Serial Number: 008619 Test Record Number: 2451
Test Date: 08/05/2026 Test Time: 4:56pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	4:56pm
FLO	Pass	4:56pm
FC	Pass	4:56pm

Temperature Tests

Test	Status	Time
FC1	Pass	4:56pm
SRC	Pass	4:56pm
DET	Pass	4:56pm
BAR	Pass	4:56pm
BT	Pass	4:56pm

Blank Tests

Test	Status	Time
AIR	Pass	4:57pm


Printer Tests

Test	Status	Time
PRNT	Pass	4:57pm

CRC Tests

Test	Status	Time
COMP	Pass	4:57pm
CAL	Pass	4:57pm

Preventive Maintenance
Status: Pass



Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County IRENEN Instrument Location MOOREVILLE PD

Instrument Serial No. 008605 MOOREVILLE NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 24 day of AUGUST, 2020 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

274970
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

IREDELL COUNTY MOORESVILLE PD 480

Serial Number: 008685

Test Date: 08/21/2026

Citation Number: M00000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Fleming, Tina S

Permit Number: 0027-4970

Effective:

02/01/2025-02/01/2027

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

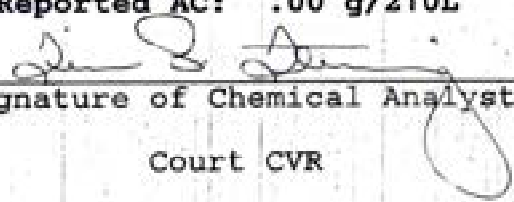
Test Type: Breath Test

Lot Number: AG602202

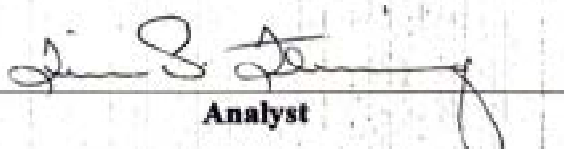
Exp Date: 01/22/2028

Test	g/210L	Time
DIAG	Pass	1:38pm
AIR BLK	.00	1:39pm
ACCY CHK	.08	1:40pm
AIR BLK	.00	1:41pm
SUB TEST	.00	1:42pm
AIR BLK	.00	1:43pm
SUB TEST	.00	1:44pm
AIR BLK	.00	1:45pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

IREDELL COUNTY MOORESVILLE PD 480

Serial Number: 008685 Test Record Number: 5305
Test Date: 08/21/2026 Test Time: 1:47pm EDT

System Check: Passed

Baseline Tests

Test	Status	Time
IR	Pass	1:47pm
FLO	Pass	1:47pm
FC	Pass	1:47pm

Temperature Tests

Test	Status	Time
FC1	Pass	1:47pm
SRC	Pass	1:47pm
DET	Pass	1:47pm
BAR	Pass	1:47pm
BT	Pass	1:47pm

Blank Tests

Test	Status	Time
AIR	Pass	1:48pm

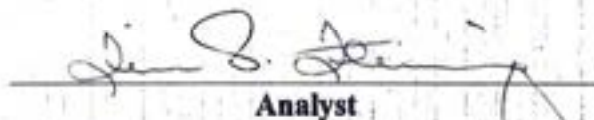
Printer Tests

Test	Status	Time
PRNT	Pass	1:48pm

CRC Tests

Test	Status	Time
COMP	Pass	1:48pm
CAL	Pass	1:48pm

**Preventive Maintenance
Status: Pass**


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Iredell Instrument Location BAT Mobile Unit 8
Instrument Serial No. 008736 —

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 8 day of August, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

2219283
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

IREDELL COUNTY BAT MOBILE UNIT 8 480

Serial Number: 008736

Test Date: 08/08/2026

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Glasscock, Jerry D

Permit Number: 7180-9235

Effective:

02/01/2026-02/01/2028

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG506303

Exp Date: 03/04/2027

Test	g/210L	Time
DIAG	Pass	11:06pm
AIR BLK	.00	11:07pm
ACCY CHK	.07	11:08pm
AIR BLK	.00	11:09pm
SUB TEST	.00	11:09pm
AIR BLK	.00	11:10pm
SUB TEST	.00	11:11pm
AIR BLK	.00	11:12pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

IREDELL COUNTY BAT MOBILE UNIT 8 480

Serial Number: 008736 Test Record Number: 1733
Test Date: 08/08/2026 Test Time: 11:13pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	11:13pm
FLO	Pass	11:13pm
FC	Pass	11:13pm

Temperature Tests

Test	Status	Time
FC1	Pass	11:13pm
SRC	Pass	11:13pm
DET	Pass	11:13pm
BAR	Pass	11:13pm
BT	Pass	11:13pm

Blank Tests

Test	Status	Time
AIR	Pass	11:14pm

Printer Tests

Test	Status	Time
PRNT	Pass	11:14pm

CRC Tests

Test	Status	Time
COMP	Pass	11:14pm
CAL	Pass	11:14pm

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Iredell Instrument Location BAT Mobile Unit 8
Instrument Serial No. 008736 —

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 18 day of August, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

2219283
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

IREDELL COUNTY BAT MOBILE UNIT 8 480

Serial Number: 008736
Test Date: 08/18/2026

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Glasscock, Jerry D

Permit Number: 7180-9235

Effective:

02/01/2026-02/01/2028

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

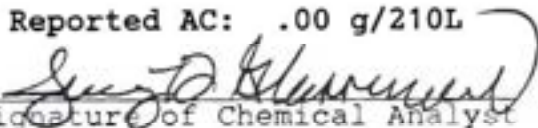
Test Type: Breath Test

Lot Number: AG506303

Exp Date: 03/04/2027

Test	g/210L	Time
DIAG	Pass	10:12pm
AIR BLK	.00	10:13pm
ACCY CHK	.07	10:14pm
AIR BLK	.00	10:15pm
SUB TEST	.00	10:15pm
AIR BLK	.00	10:16pm
SUB TEST	.00	10:17pm
AIR BLK	.00	10:18pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

IREDELLL COUNTY BAT MOBILE UNIT 8 480

Serial Number: 008736 Test Record Number: 1737
Test Date: 08/18/2026 Test Time: 10:19pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	10:19pm
FLO	Pass	10:19pm
FC	Pass	10:19pm

Temperature Tests

Test	Status	Time
FC1	Pass	10:19pm
SRC	Pass	10:19pm
DET	Pass	10:19pm
BAR	Pass	10:19pm
BT	Pass	10:19pm

Blank Tests

Test	Status	Time
AIR	Pass	10:20pm

Printer Tests

Test	Status	Time
PRNT	Pass	10:20pm

CRC Tests

Test	Status	Time
COMP	Pass	10:20pm
CAL	Pass	10:20pm

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Iredell Instrument Location BAT Mobile Unit 8
Instrument Serial No. 008775 —

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 8 day of August, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

2219283
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

IREDELL COUNTY BAT MOBILE UNIT 8 480

Serial Number: 008775
Test Date: 08/08/2026

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE

Analyst's Name: Glasscock, Jerry D
Permit Number: 7180-9235
Effective:
02/01/2026-02/01/2028

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG506303
Exp Date: 03/04/2027

Test	g/210L	Time
DIAG	Pass	11:34pm
AIR BLK	.00	11:35pm
ACCY CHK	.08	11:35pm
AIR BLK	.00	11:36pm
SUB TEST	.00	11:36pm
AIR BLK	.00	11:37pm
SUB TEST	.00	11:39pm
AIR BLK	.00	11:40pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

IREDELL COUNTY BAT MOBILE UNIT 8 480

Serial Number: 008775 Test Record Number: 2598
Test Date: 08/08/2026 Test Time: 11:42pm EDT

System Check: Passed

Baseline Tests

Test	Status	Time
IR	Pass	11:42pm
FLO	Pass	11:42pm
FC	Pass	11:42pm

Temperature Tests

Test	Status	Time
FC1	Pass	11:42pm
SRC	Pass	11:42pm
DET	Pass	11:42pm
BAR	Pass	11:42pm
BT	Pass	11:42pm

Blank Tests

Test	Status	Time
AIR	Pass	11:43pm


Printer Tests

Test	Status	Time
PRNT	Pass	11:43pm

CRC Tests

Test	Status	Time
COMP	Pass	11:43pm
CAL	Pass	11:43pm

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Iredell Instrument Location BAT Mobile Unit 8
Instrument Serial No. 008775

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 18 day of August, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

2219283
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

IREDELL COUNTY BAT MOBILE UNIT 8 480

Serial Number: 008775

Test Date: 08/18/2026

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Glasscock, Jerry D

Permit Number: 7180-9235

Effective:

02/01/2026-02/01/2028

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG506303

Exp Date: 03/04/2027

Test	g/210L	Time
DIAG	Pass	10:11pm
AIR BLK	.00	10:12pm
ACCY CHK	.08	10:13pm
AIR BLK	.00	10:14pm
SUB TEST	.00	10:14pm
AIR BLK	.00	10:15pm
SUB TEST	.00	10:17pm
AIR BLK	.00	10:18pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

IREDELL COUNTY BAT MOBILE UNIT 8 480

Serial Number: 008775 Test Record Number: 2603
Test Date: 08/18/2026 Test Time: 10:18pm EDT

System Check: Passed

Baseline Tests

Test	Status	Time
IR	Pass	10:18pm
FLO	Pass	10:18pm
FC	Pass	10:19pm

Temperature Tests

Test	Status	Time
FC1	Pass	10:19pm
SRC	Pass	10:19pm
DET	Pass	10:19pm
BAR	Pass	10:19pm
BT	Pass	10:19pm

Blank Tests

Test	Status	Time
AIR	Pass	10:19pm

Printer Tests

Test	Status	Time
PRNT	Pass	10:19pm

CRC Tests

Test	Status	Time
COMP	Pass	10:19pm
CAL	Pass	10:19pm

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH


PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County JOHN Instrument Location JOHN CO. 80.
Instrument Serial No. 608809 STATESVILLE NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 05 day of August, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

274970
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

IREDELL COUNTY IREDELL COUNTY SO 480

Serial Number: 008809

Test Date: 08/05/2026

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Fleming, Tina S

Permit Number: 0027-4970

Effective:

02/01/2025-02/01/2027

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

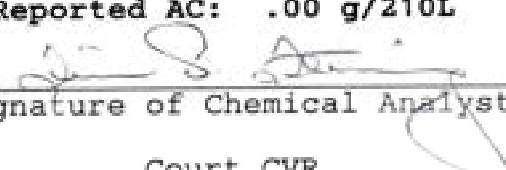
Test Type: Breath Test

Lot Number: AG534301

Exp Date: 12/09/2027

Test	g/210L	Time
DIAG	Pass	3:33pm
AIR BLK	.00	3:34pm
ACCY CHK	.08	3:34pm
AIR BLK	.00	3:35pm
SUB TEST	.00	3:36pm
AIR BLK	.00	3:37pm
SUB TEST	.00	3:38pm
AIR BLK	.00	3:39pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

IREDELL COUNTY IREDELL COUNTY SO 480

Serial Number: 008809 Test Record Number: 6826
Test Date: 08/05/2026 Test Time: 3:43pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	3:44pm
FLO	Pass	3:44pm
FC	Pass	3:44pm

Temperature Tests

Test	Status	Time
FC1	Pass	3:44pm
SRC	Pass	3:44pm
DET	Pass	3:44pm
BAR	Pass	3:44pm
BT	Pass	3:44pm

Blank Tests

Test	Status	Time
AIR	Pass	3:44pm

Printer Tests

Test	Status	Time
PRNT	Pass	3:45pm

CRC Tests

Test	Status	Time
COMP	Pass	3:45pm
CAL	Pass	3:45pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Iredell Instrument Location BAT Mobile Unit 8
Instrument Serial No. 008816 —

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 8 day of August, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature] 2219283
Signature of Certifying Official Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

IREDELL COUNTY BAT MOBILE UNIT 8 480

Serial Number: 008816
Test Date: 08/08/2026

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Glasscock, Jerry D

Permit Number: 7180-9235

Effective:

02/01/2026-02/01/2028

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG431002

Exp Date: 11/05/2026

Test	g/210L	Time
DIAG	Pass	11:33pm
AIR BLK	.00	11:34pm
ACCY CHK	.07	11:35pm
AIR BLK	.00	11:36pm
SUB TEST	.00	11:36pm
AIR BLK	.00	11:37pm
SUB TEST	.00	11:39pm
AIR BLK	.00	11:39pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

Intox EC/IR-II: Preventive Maintenance

IREDELL COUNTY BAT MOBILE UNIT 8 480

Serial Number: 008816 Test Record Number: 8167
Test Date: 08/08/2026 Test Time: 11:41pm EDT

System Check: Passed

Baseline Tests

Test	Status	Time
IR	Pass	11:42pm
FLO	Pass	11:42pm
FC	Pass	11:42pm

Temperature Tests

Test	Status	Time
FC1	Pass	11:42pm
SRC	Pass	11:42pm
DET	Pass	11:42pm
BAR	Pass	11:42pm
BT	Pass	11:42pm

Blank Tests

Test	Status	Time
AIR	Pass	11:42pm

Printer Tests

Test	Status	Time
PRNT	Pass	11:42pm

CRC Tests

Test	Status	Time
COMP	Pass	11:43pm
CAL	Pass	11:43pm

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Iredell

Instrument Location BAT Mobile Unit 8

Instrument Serial No. 008816

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 18 day of August, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

2219283
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

IREDELL COUNTY BAT MOBILE UNIT 8 480

Serial Number: 008816

Test Date: 08/18/2026

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Glasscock, Jerry D

Permit Number: 7180-9235

Effective:

02/01/2026-02/01/2028

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG431002

Exp Date: 11/05/2026

Test	g/210L	Time
DIAG	Pass	10:11pm
AIR BLK	.00	10:12pm
ACCY CHK	.07	10:13pm
AIR BLK	.00	10:14pm
SUB TEST	.00	10:14pm
AIR BLK	.00	10:15pm
SUB TEST	.00	10:17pm
AIR BLK	.00	10:18pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

This form is used when performing Preventive Maintenance procedures

Forensic Tests for Alcohol Branch

Department of Health and Human Services

Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

IREDELL COUNTY BAT MOBILE UNIT 8 480

Serial Number: 008816 Test Record Number: 8173
Test Date: 08/18/2026 Test Time: 10:18pm EDT

System Check: Passed

Baseline Tests

Test	Status	Time
IR	Pass	10:18pm
FLO	Pass	10:18pm
FC	Pass	10:18pm

Temperature Tests

Test	Status	Time
FC1	Pass	10:19pm
SRC	Pass	10:19pm
DET	Pass	10:19pm
BAR	Pass	10:19pm
BT	Pass	10:19pm

Blank Tests

Test	Status	Time
AIR	Pass	10:19pm

Printer Tests

Test	Status	Time
PRNT	Pass	10:19pm

CRC Tests

Test	Status	Time
COMP	Pass	10:19pm
CAL	Pass	10:19pm

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Iredell Instrument Location BAT Mobile Unit 8
Instrument Serial No. 008929 —

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 8 day of August, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

2219283
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

IREDELL COUNTY BAT MOBILE UNIT 8 480

Serial Number: 008929

Test Date: 08/08/2026

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Glasscock, Jerry D

Permit Number: 7180-9235

Effective:

02/01/2026-02/01/2028

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG506303

Exp Date: 03/04/2027

Test	g/210L	Time
DIAG	Pass	11:32pm
AIR BLK	.00	11:33pm
ACCY CHK	.08	11:34pm
AIR BLK	.00	11:35pm
SUB TEST	.00	11:36pm
AIR BLK	.00	11:37pm
SUB TEST	.00	11:38pm
AIR BLK	.00	11:39pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

This form is used when performing Preventive Maintenance procedures

Forensic Tests for Alcohol Branch

Department of Health and Human Services

Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

IREDELL COUNTY BAT MOBILE UNIT 8 480

Serial Number: 008929 Test Record Number: 1879
Test Date: 08/08/2026 Test Time: 11:42pm EDT

System Check: Passed

Baseline Tests

Test	Status	Time
IR	Pass	11:42pm
FLO	Pass	11:42pm
FC	Pass	11:43pm

Temperature Tests

Test	Status	Time
FC1	Pass	11:43pm
SRC	Pass	11:43pm
DET	Pass	11:43pm
BAR	Pass	11:43pm
BT	Pass	11:43pm

Blank Tests

Test	Status	Time
AIR	Pass	11:43pm

Printer Tests

Test	Status	Time
PRNT	Pass	11:44pm

CRC Tests

Test	Status	Time
COMP	Pass	11:44pm
CAL	Pass	11:44pm

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Iredell Instrument Location BAT Mobile Unit 8
Instrument Serial No. 008929

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 18 day of August, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature] 2219283
Signature of Certifying Official Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

IREDELL COUNTY BAT MOBILE UNIT 8 480

Serial Number: 008929

Test Date: 08/18/2026

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Glasscock, Jerry D

Permit Number: 7180-9235

Effective:

02/01/2026-02/01/2028

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

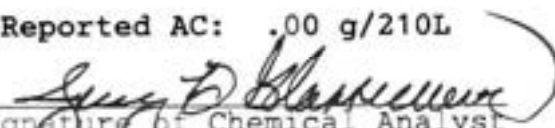
Test Type: Breath Test

Lot Number: AG506303

Exp Date: 03/04/2027

Test	g/210L	Time
DIAG	Pass	10:10pm
AIR BLK	.00	10:11pm
ACCY CHK	.08	10:12pm
AIR BLK	.00	10:13pm
SUB TEST	.00	10:14pm
AIR BLK	.00	10:15pm
SUB TEST	.00	10:16pm
AIR BLK	.00	10:17pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

IREDELL COUNTY BAT MOBILE UNIT 8 480

Serial Number: 008929 Test Record Number: 1884
Test Date: 08/18/2026 Test Time: 10:18pm EDT

System Check: Passed

Baseline Tests

Test	Status	Time
IR	Pass	10:18pm
FLO	Pass	10:18pm
FC	Pass	10:18pm

Temperature Tests

Test	Status	Time
FC1	Pass	10:18pm
SRC	Pass	10:18pm
DET	Pass	10:18pm
BAR	Pass	10:18pm
BT	Pass	10:18pm

Blank Tests

Test	Status	Time
AIR	Pass	10:19pm

Printer Tests

Test	Status	Time
PRNT	Pass	10:19pm

CRC Tests

Test	Status	Time
COMP	Pass	10:19pm
CAL	Pass	10:19pm

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Johnston Instrument Location Selma Police Dept.
Instrument Serial No. 008595 Selma, N.C.

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 18 day of August, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

365156
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

JOHNSTON COUNTY SELMA PD 500

Serial Number: 008595
Test Date: 08/18/2026

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Garner, Joel K

Permit Number: 0036-5156

Effective:

02/01/2026-02/01/2028

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG602203

Exp Date: 01/22/2028

Test	g/210L	Time
DIAG	Pass	9:33am
AIR BLK	.00	9:33am
ACCY CHK	.07	9:34am
AIR BLK	.00	9:35am
SUB TEST	.00	9:36am
AIR BLK	.00	9:36am
SUB TEST	.00	9:38am
AIR BLK	.00	9:39am

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

JOHNSTON COUNTY SELMA PD 500

Serial Number: 008595 Test Record Number: 1960
Test Date: 08/18/2026 Test Time: 9:40am EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	9:40am
FLO	Pass	9:40am
FC	Pass	9:40am

Temperature Tests

Test	Status	Time
FC1	Pass	9:40am
SRC	Pass	9:40am
DET	Pass	9:40am
BAR	Pass	9:40am
BT	Pass	9:40am

Blank Tests

Test	Status	Time
AIR	Pass	9:41am

Printer Tests

Test	Status	Time
PRNT	Pass	9:41am

CRC Tests

Test	Status	Time
COMP	Pass	9:41am
CAL	Pass	9:41am

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Johnston Instrument Location Clayton Police Dept.
Instrument Serial No. 008658 Clayton, N.C.

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 18 day of August, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]

Signature of Certifying Official

365156
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

JOHNSTON COUNTY CLAYTON PD 500

Serial Number: 008658

Test Date: 08/18/2026

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Garner, Joel K

Permit Number: 0036-5156

Effective:

02/01/2026-02/01/2028

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG534301

Exp Date: 12/09/2027

Test	g/210L	Time
DIAG	Pass	11:52am
AIR BLK	.00	11:53am
ACCY CHK	.08	11:53am
AIR BLK	.00	11:55am
SUB TEST	.00	11:55am
AIR BLK	.00	11:56am
SUB TEST	.00	11:58am
AIR BLK	.00	11:59am

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

JOHNSTON COUNTY CLAYTON PD 500

Serial Number: 008658 Test Record Number: 2538
Test Date: 08/18/2026 Test Time: 11:59am EDT

System Check: Passed

Baseline Tests

Test	Status	Time
IR	Pass	11:59am
FLO	Pass	11:59am
FC	Pass	11:59am

Temperature Tests

Test	Status	Time
FC1	Pass	12:00pm
SRC	Pass	12:00pm
DET	Pass	12:00pm
BAR	Pass	12:00pm
BT	Pass	12:00pm

Blank Tests

Test	Status	Time
AIR	Pass	12:00pm

Printer Tests

Test	Status	Time
PRNT	Pass	12:00pm

CRC Tests

Test	Status	Time
COMP	Pass	12:00pm
CAL	Pass	12:00pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Johnston Instrument Location Benson Police Dept.
Instrument Serial No. 008885 Benson, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 17 day of August, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



A handwritten signature in black ink, appearing to be "K. A. ...", written over a horizontal line.

Signature of Certifying Official

365156

Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

JOHNSTON COUNTY BENSON PD 500

Serial Number: 008885

Test Date: 08/17/2026

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Garner, Joel K

Permit Number: 0036-5156

Effective:

02/01/2026-02/01/2028

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG534301

Exp Date: 12/09/2027

Test	g/210L	Time
DIAG	Pass	12:31pm
AIR BLK	.00	12:32pm
ACCY CHK	.08	12:33pm
AIR BLK	.00	12:33pm
SUB TEST	.00	12:34pm
AIR BLK	.00	12:35pm
SUB TEST	.00	12:36pm
AIR BLK	.00	12:37pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

JOHNSTON COUNTY BENSON PD 500

Serial Number: 008885 Test Record Number: 962
Test Date: 08/17/2026 Test Time: 12:38pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	12:38pm
FLO	Pass	12:38pm
FC	Pass	12:39pm

Temperature Tests

Test	Status	Time
FC1	Pass	12:39pm
SRC	Pass	12:39pm
DET	Pass	12:39pm
BAR	Pass	12:39pm
BT	Pass	12:39pm

Blank Tests

Test	Status	Time
AIR	Pass	12:39pm

Printer Tests

Test	Status	Time
PRNT	Pass	12:39pm

CRC Tests

Test	Status	Time
COMP	Pass	12:40pm
CAL	Pass	12:40pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH


PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Lee Instrument Location Lee Detention Center
Instrument Serial No. 008645 Sanford, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 4 day of August, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

365156
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

LEE COUNTY DETENTION CENTER 520

Serial Number: 008645
Test Date: 08/04/2026

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: Garner, Joel K
Permit Number: 0036-5156
Effective:
02/01/2026-02/01/2028

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG602203
Exp Date: 01/22/2028

Test	g/210L	Time
DIAG	Pass	10:34am
AIR BLK	.00	10:34am
ACCY CHK	.08	10:35am
AIR BLK	.00	10:36am
SUB TEST	.00	10:36am
AIR BLK	.00	10:37am
SUB TEST	.00	10:39am
AIR BLK	.00	10:40am

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

Intox EC/IR-II: Preventive Maintenance

LEE COUNTY DETENTION CENTER 520

Serial Number: 008645 Test Record Number: 2899
Test Date: 08/04/2026 Test Time: 10:40am EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	10:41am
FLO	Pass	10:41am
FC	Pass	10:41am

Temperature Tests

Test	Status	Time
FC1	Pass	10:41am
SRC	Pass	10:41am
DET	Pass	10:41am
BAR	Pass	10:41am
BT	Pass	10:41am

Blank Tests

Test	Status	Time
AIR	Pass	10:41am

Printer Tests

Test	Status	Time
PRNT	Pass	10:41am

CRC Tests

Test	Status	Time
COMP	Pass	10:42am
CAL	Pass	10:42am

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Lee Instrument Location Sanford Police Dept.
Instrument Serial No. 008867 Sanford, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 4 day of August, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

365156
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

LEE COUNTY SANFORD POLICE DEPT 520

Serial Number: 008867

Test Date: 08/04/2026

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Garner, Joel K

Permit Number: 0036-5156

Effective:

02/01/2026-02/01/2028

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG534301

Exp Date: 12/09/2027

Test	g/210L	Time
DIAG	Pass	11:20am
AIR BLK	.00	11:20am
ACCY CHK	.08	11:21am
AIR BLK	.00	11:22am
SUB TEST	.00	11:23am
AIR BLK	.00	11:24am
SUB TEST	.00	11:25am
AIR BLK	.00	11:26am

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

LEE COUNTY SANFORD POLICE DEPT 520

Serial Number: 008867 Test Record Number: 1621
Test Date: 08/04/2026 Test Time: 11:26am EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	11:27am
FLO	Pass	11:27am
FC	Pass	11:27am

Temperature Tests

Test	Status	Time
FC1	Pass	11:27am
SRC	Pass	11:27am
DET	Pass	11:27am
BAR	Pass	11:27am
BT	Pass	11:27am

Blank Tests

Test	Status	Time
AIR	Pass	11:28am

Printer Tests

Test	Status	Time
PRNT	Pass	11:28am

CRC Tests

Test	Status	Time
COMP	Pass	11:28am
CAL	Pass	11:28am

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Mecklenburg Instrument Location BAT Mobile Unit 8
Instrument Serial No. 008615

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 21 day of August, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

2219283
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

MECKLENBURG COUNTY BAT MOBILE UNIT 8
590

Serial Number: 008615
Test Date: 08/21/2026

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE

Analyst's Name: Glasscock, Jerry D
Permit Number: 7180-9235
Effective:
02/01/2026-02/01/2028

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test


Lot Number: AG506303
Exp Date: 03/04/2027

Test	g/210L	Time
DIAG	Pass	8:47pm
AIR BLK	.00	8:48pm
ACCY CHK	.07	8:49pm
AIR BLK	.00	8:50pm
SUB TEST	.00	8:51pm
AIR BLK	.00	8:51pm
SUB TEST	.00	8:53pm
AIR BLK	.00	8:54pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

MECKLENBURG COUNTY BAT MOBILE UNIT 8 590

Serial Number: 008615 Test Record Number: 6389
Test Date: 08/21/2026 Test Time: 8:54pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	8:55pm
FLO	Pass	8:55pm
FC	Pass	8:55pm

Temperature Tests

Test	Status	Time
FC1	Pass	8:55pm
SRC	Pass	8:55pm
DET	Pass	8:55pm
BAR	Pass	8:55pm
BT	Pass	8:55pm

Blank Tests

Test	Status	Time
AIR	Pass	8:55pm

Printer Tests

Test	Status	Time
PRNT	Pass	8:55pm

CRC Tests

Test	Status	Time
COMP	Pass	8:56pm
CAL	Pass	8:56pm

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Mecklenburg Instrument Location BAT Mobile Unit 8
Instrument Serial No. 008615

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 22 day of August, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

2219283
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

MECKLENBURG COUNTY BAT MOBILE UNIT 8
590

Serial Number: 008615
Test Date: 08/22/2026

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Glasscock, Jerry D

Permit Number: 7180-9235

Effective:

02/01/2026-02/01/2028

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG506303

Exp Date: 03/04/2027

Test	g/210L	Time
DIAG	Pass	9:47pm
AIR BLK	.00	9:48pm
ACCY CHK	.07	9:49pm
AIR BLK	.00	9:50pm
SUB TEST	.00	9:50pm
AIR BLK	.00	9:51pm
SUB TEST	.00	9:53pm
AIR BLK	.00	9:54pm

Reported AC: 00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

Intox EC/IR-II: Preventive Maintenance

MECKLENBURG COUNTY BAT MOBILE UNIT 8 590

Serial Number: 008615 Test Record Number: 6393
Test Date: 08/22/2026 Test Time: 9:55pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	9:56pm
FLO	Pass	9:56pm
FC	Pass	9:56pm

Temperature Tests

Test	Status	Time
FC1	Pass	9:56pm
SRC	Pass	9:56pm
DET	Pass	9:56pm
BAR	Pass	9:56pm
BT	Pass	9:56pm

Blank Tests

Test	Status	Time
AIR	Pass	9:57pm

Printer Tests

Test	Status	Time
PRNT	Pass	9:57pm

CRC Tests

Test	Status	Time
COMP	Pass	9:57pm
CAL	Pass	9:57pm

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Mecklenburg Instrument Location BAT Mobile Unit 8
Instrument Serial No. 008615

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 27 day of August, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

2219283
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

MECKLENBURG COUNTY BAT MOBILE UNIT 8
590

Serial Number: 008615
Test Date: 08/27/2026

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Glasscock, Jerry D

Permit Number: 7180-9235

Effective:

02/01/2026-02/01/2028

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG506303

Exp Date: 03/04/2027

Test	g/210L	Time
DIAG	Pass	9:20pm
AIR BLK	.00	9:21pm
ACCY CHK	.07	9:22pm
AIR BLK	.00	9:23pm
SUB TEST	.00	9:24pm
AIR BLK	.00	9:25pm
SUB TEST	.00	9:26pm
AIR BLK	.00	9:27pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

MECKLENBURG COUNTY BAT MOBILE UNIT 8 590

Serial Number: 008615 Test Record Number: 6400
Test Date: 08/27/2026 Test Time: 9:28pm EDT

System Check: Passed

Baseline Tests

Test	Status	Time
IR	Pass	9:28pm
FLO	Pass	9:28pm
FC	Pass	9:28pm

Temperature Tests

Test	Status	Time
FC1	Pass	9:29pm
SRC	Pass	9:29pm
DET	Pass	9:29pm
BAR	Pass	9:29pm
BT	Pass	9:29pm

Blank Tests

Test	Status	Time
AIR	Pass	9:29pm

Printer Tests

Test	Status	Time
PRNT	Pass	9:29pm

CRC Tests

Test	Status	Time
COMP	Pass	9:29pm
CAL	Pass	9:29pm

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Mecklenburg Instrument Location BAT Mobile Unit 8
Instrument Serial No. 008615 —

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 29 day of August, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

2219283
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

MECKLENBURG COUNTY BAT MOBILE UNIT 8
590

Serial Number: 008615
Test Date: 08/29/2026

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Glasscock, Jerry D

Permit Number: 7180-9235

Effective:

02/01/2026-02/01/2028

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG506303

Exp Date: 03/04/2027

Test	g/210L	Time
DIAG	Pass	9:13pm
AIR BLK	.00	9:14pm
ACCY CHK	.07	9:15pm
AIR BLK	.00	9:16pm
SUB TEST	.00	9:16pm
AIR BLK	.00	9:17pm
SUB TEST	.00	9:19pm
AIR BLK	.00	9:20pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

Intox EC/IR-II: Preventive Maintenance

MECKLENBURG COUNTY BAT MOBILE UNIT 8 590

Serial Number: 008615 Test Record Number: 6402
Test Date: 08/29/2026 Test Time: 9:20pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	9:20pm
FLO	Pass	9:20pm
FC	Pass	9:20pm

Temperature Tests

Test	Status	Time
FC1	Pass	9:20pm
SRC	Pass	9:20pm
DET	Pass	9:20pm
BAR	Pass	9:20pm
BT	Pass	9:20pm

Blank Tests

Test	Status	Time
AIR	Pass	9:21pm

Printer Tests

Test	Status	Time
PRNT	Pass	9:21pm

CRC Tests

Test	Status	Time
COMP	Pass	9:21pm
CAL	Pass	9:21pm

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Mecklenburg Instrument Location Mecklenburg Co SC
Instrument Serial No 008665 Charlotte, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 18th day of August, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Bryno Helms
Signature of Certifying Official

849845
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

MECKLENBURG COUNTY SHERIFFS OFFICE 590

Serial Number: 008665
Test Date: 08/18/2026

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: Helms, Bryce A
Permit Number: 0084-9845
Effective:
02/01/2026-02/01/2028

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG602202
Exp Date: 01/22/2028

Test	g/210L	Time
DIAG	Pass	11:19am
AIR BLK	.00	11:20am
ACCY CHK	.08	11:20am
AIR BLK	.00	11:22am
SUB TEST	.00	11:22am
AIR BLK	.00	11:23am
SUB TEST	.00	11:25am
AIR BLK	.00	11:26am

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

MECKLENBURG COUNTY SHERIFFS OFFICE 590

Serial Number: 008665 Test Record Number: 6104
Test Date: 08/18/2026 Test Time: 11:26am EDT

System Check: Passed

Baseline Tests

Test	Status	Time
IR	Pass	11:26am
FLO	Pass	11:26am
FC	Pass	11:26am

Temperature Tests

Test	Status	Time
FC1	Pass	11:26am
SRC	Pass	11:26am
DET	Pass	11:26am
BAR	Pass	11:26am
BT	Pass	11:26am

Blank Tests

Test	Status	Time
AIR	Pass	11:27am

Printer Tests

Test	Status	Time
PRNT	Pass	11:27am

CRC Tests

Test	Status	Time
COMP	Pass	11:27am
CAL	Pass	11:27am

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County MEKLENBURG Instrument Location CORNELIUS PD

Instrument Serial No. 008692 CORNELIUS NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 21 day of AUGUST, 2020 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

274970
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

MECKLENBURG COUNTY CORNELIUS PD 590

Serial Number: 008692

Test Date: 08/21/2026

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Fleming, Tina S

Permit Number: 0027-4970

Effective:

02/01/2025-02/01/2027

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

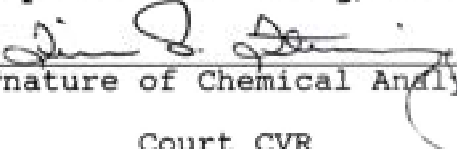
Test Type: Breath Test

Lot Number: AG431001

Exp Date: 11/05/2026

Test	g/210L	Time
DIAG	Pass	11:42am
AIR BLK	.00	11:42am
ACCY CHK	.08	11:43am
AIR BLK	.00	11:44am
SUB TEST	.00	11:45am
AIR BLK	.00	11:45am
SUB TEST	.00	11:47am
AIR BLK	.00	11:48am

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

MECKLENBURG COUNTY CORNELIUS PD 590

Serial Number: 008692 Test Record Number: 3995
Test Date: 08/21/2026 Test Time: 11:49am EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	11:50am
FLO	Pass	11:50am
FC	Pass	11:50am

Temperature Tests

Test	Status	Time
FC1	Pass	11:50am
SRC	Pass	11:50am
DET	Pass	11:50am
BAR	Pass	11:50am
BT	Pass	11:50am

Blank Tests

Test	Status	Time
AIR	Pass	11:51am


Printer Tests

Test	Status	Time
PRNT	Pass	11:51am

CRC Tests

Test	Status	Time
COMP	Pass	11:51am
CAL	Pass	11:51am

Preventive Maintenance
Status: Pass



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County Mecklenburg Instrument Location Matthews PD
Instrument Serial No. 008699 Matthews, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 18th day of August, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Boye Helms
Signature of Certifying Official

849845
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

MECKLENBURG COUNTY MATTHEWS PD 590

Serial Number: 008699

Test Date: 08/18/2026

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Helms, Bryce A

Permit Number: 0084-9845

Effective:

02/01/2026-02/01/2028

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG506303

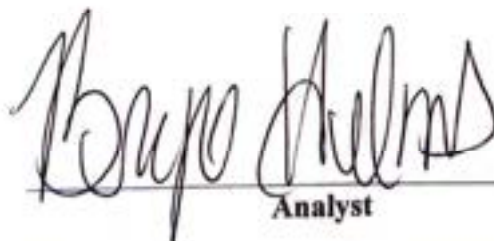
Exp Date: 03/04/2027

Test	g/210L	Time
DIAG	Pass	12:48pm
AIR BLK	.00	12:49pm
ACCY CHK	.08	12:50pm
AIR BLK	.00	12:51pm
SUB TEST	.00	12:52pm
AIR BLK	.00	12:53pm
SUB TEST	.00	12:54pm
AIR BLK	.00	12:55pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

Intox EC/IR-II: Preventive Maintenance

MECKLENBURG COUNTY MATTHEWS PD 590

Serial Number: 008699 Test Record Number: 3605
Test Date: 08/18/2026 Test Time: 12:55pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	12:56pm
FLO	Pass	12:56pm
FC	Pass	12:56pm

Temperature Tests

Test	Status	Time
FC1	Pass	12:56pm
SRC	Pass	12:56pm
DET	Pass	12:56pm
BAR	Pass	12:56pm
BT	Pass	12:56pm

Blank Tests

Test	Status	Time
AIR	Pass	12:57pm

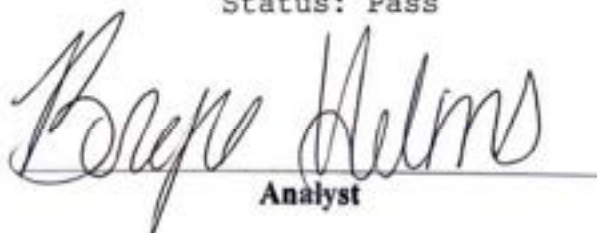
Printer Tests

Test	Status	Time
PRNT	Pass	12:57pm

CRC Tests

Test	Status	Time
COMP	Pass	12:57pm
CAL	Pass	12:57pm

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Mecklenburg Instrument Location Pineville PD
Instrument Serial No. 008703 Pineville, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 25th day of August, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Barry Helms
Signature of Certifying Official

849845
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

MECKLENBURG COUNTY PINEVILLE PD 590

Serial Number: 008703

Test Date: 08/25/2026

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Helms, Bryce A

Permit Number: 0084-9845

Effective:

02/01/2026-02/01/2028

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG534301

Exp Date: 12/09/2027

Test	g/210L	Time
DIAG	Pass	10:18am
AIR BLK	.00	10:19am
ACCY CHK	.08	10:19am
AIR BLK	.00	10:20am
SUB TEST	.00	10:21am
AIR BLK	.00	10:22am
SUB TEST	.00	10:23am
AIR BLK	.00	10:24am

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

Intox EC/IR-II: Preventive Maintenance

MECKLENBURG COUNTY PINEVILLE PD 590

Serial Number: 008703 Test Record Number: 6401
Test Date: 08/25/2026 Test Time: 10:24am EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	10:25am
FLO	Pass	10:25am
FC	Pass	10:25am

Temperature Tests

Test	Status	Time
FC1	Pass	10:25am
SRC	Pass	10:25am
DET	Pass	10:25am
BAR	Pass	10:25am
BT	Pass	10:25am

Blank Tests

Test	Status	Time
AIR	Pass	10:25am

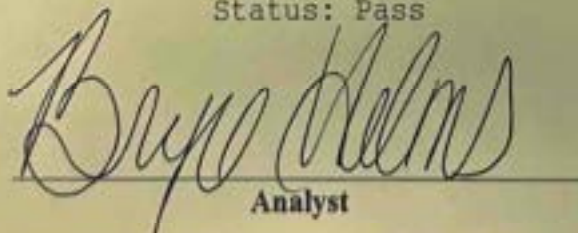
Printer Tests

Test	Status	Time
PRNT	Pass	10:26am

CRC Tests

Test	Status	Time
COMP	Pass	10:26am
CAL	Pass	10:26am

Preventive Maintenance
Status: *Pass*


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Mecklenburg Instrument Location BAT Mobile Unit 8
Instrument Serial No. 008736

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 21 day of August, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

2219283
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

MECKLENBURG COUNTY BAT MOBILE UNIT 8
590

Serial Number: 008736
Test Date: 08/21/2026

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Glasscock, Jerry D

Permit Number: 7180-9235

Effective:

02/01/2026-02/01/2028

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG506303


Exp Date: 03/04/2027

Test	g/210L	Time
DIAG	Pass	8:46pm
AIR BLK	.00	8:47pm
ACCY CHK	.07	8:48pm
AIR BLK	.00	8:49pm
SUB TEST	.00	8:50pm
AIR BLK	.00	8:51pm
SUB TEST	.00	8:52pm
AIR BLK	.00	8:53pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

MECKLENBURG COUNTY BAT MOBILE UNIT 8 590

Serial Number: 008736 Test Record Number: 1739
Test Date: 08/21/2026 Test Time: 8:53pm EDT

System Check: Passed

Baseline Tests

Test	Status	Time
IR	Pass	8:54pm
FLO	Pass	8:54pm
FC	Pass	8:54pm

Temperature Tests

Test	Status	Time
FC1	Pass	8:54pm
SRC	Pass	8:54pm
DET	Pass	8:54pm
BAR	Pass	8:54pm
BT	Pass	8:54pm

Blank Tests

Test	Status	Time
AIR	Pass	8:54pm

Printer Tests

Test	Status	Time
PRNT	Pass	8:55pm

CRC Tests

Test	Status	Time
COMP	Pass	8:55pm
CAL	Pass	8:55pm

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Mecklenburg Instrument Location BAT Mobile Unit 8
Instrument Serial No. 008736

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 22 day of August, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

2219283
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

MECKLENBURG COUNTY BAT MOBILE UNIT 8
590

Serial Number: 008736
Test Date: 08/22/2026

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: Glasscock, Jerry D
Permit Number: 7180-9235
Effective:
02/01/2026-02/01/2028

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG506303
Exp Date: 03/04/2027

Test	g/210L	Time
DIAG	Pass	9:47pm
AIR BLK	.00	9:48pm
ACCY CHK	.07	9:48pm
AIR BLK	.00	9:49pm
SUB TEST	.00	9:50pm
AIR BLK	.00	9:51pm
SUB TEST	.00	9:52pm
AIR BLK	.00	9:53pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

MECKLENBURG COUNTY BAT MOBILE UNIT 8 590

Serial Number: 008736 Test Record Number: 1744
Test Date: 08/22/2026 Test Time: 9:55pm EDT

System Check: Passed

Baseline Tests

Test	Status	Time
IR	Pass	9:55pm
FLO	Pass	9:55pm
FC	Pass	9:55pm

Temperature Tests

Test	Status	Time
FC1	Pass	9:56pm
SRC	Pass	9:56pm
DET	Pass	9:56pm
BAR	Pass	9:56pm
BT	Pass	9:56pm

Blank Tests

Test	Status	Time
AIR	Pass	9:56pm

Printer Tests

Test	Status	Time
PRNT	Pass	9:56pm

CRC Tests

Test	Status	Time
COMP	Pass	9:56pm
CAL	Pass	9:56pm

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Mecklenburg Instrument Location BAT Mobile Unit 8
Instrument Serial No. 008736

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 27 day of August, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

2219283
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

MECKLENBURG COUNTY BAT MOBILE UNIT 8
590

Serial Number: 008736

Test Date: 08/27/2026

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Glasscock, Jerry D

Permit Number: 7180-9235

Effective:

02/01/2026-02/01/2028

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG506303

Exp Date: 03/04/2027

Test	g/210L	Time
DIAG	Pass	9:21pm
AIR BLK	.00	9:22pm
ACCY CHK	.07	9:23pm
AIR BLK	.00	9:24pm
SUB TEST	.00	9:24pm
AIR BLK	.00	9:25pm
SUB TEST	.00	9:27pm
AIR BLK	.00	9:28pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

Intox EC/IR-II: Preventive Maintenance

MECKLENBURG COUNTY BAT MOBILE UNIT 8 590

Serial Number: 008736 Test Record Number: 1749
Test Date: 08/27/2026 Test Time: 9:28pm EDT

System Check: Passed

Baseline Tests

Test	Status	Time
IR	Pass	9:28pm
FLO	Pass	9:28pm
FC	Pass	9:28pm

Temperature Tests

Test	Status	Time
FC1	Pass	9:28pm
SRC	Pass	9:28pm
DET	Pass	9:28pm
BAR	Pass	9:28pm
BT	Pass	9:28pm

Blank Tests

Test	Status	Time
AIR	Pass	9:29pm

Printer Tests

Test	Status	Time
PRNT	Pass	9:29pm

CRC Tests

Test	Status	Time
COMP	Pass	9:29pm
CAL	Pass	9:29pm

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Mecklenburg Instrument Location BAT Mobile Unit 8
Instrument Serial No. 008736

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 29 day of August, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

2219283
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

MECKLENBURG COUNTY BAT MOBILE UNIT 8
590

Serial Number: 008736
Test Date: 08/29/2026

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Glasscock, Jerry D

Permit Number: 7180-9235

Effective:

02/01/2026-02/01/2028

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG506303

Exp Date: 03/04/2027

Test	g/210L	Time
DIAG	Pass	9:13pm
AIR BLK	.00	9:14pm
ACCY CHK	.07	9:15pm
AIR BLK	.00	9:16pm
SUB TEST	.00	9:17pm
AIR BLK	.00	9:18pm
SUB TEST	.00	9:20pm
AIR BLK	.00	9:20pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

MECKLENBURG COUNTY BAT MOBILE UNIT 8 590

Serial Number: 008736 Test Record Number: 1751
Test Date: 08/29/2026 Test Time: 9:21pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	9:21pm
FLO	Pass	9:21pm
FC	Pass	9:21pm

Temperature Tests

Test	Status	Time
FC1	Pass	9:21pm
SRC	Pass	9:21pm
DET	Pass	9:21pm
BAR	Pass	9:21pm
BT	Pass	9:21pm

Blank Tests

Test	Status	Time
AIR	Pass	9:22pm

Printer Tests

Test	Status	Time
PRNT	Pass	9:22pm

CRC Tests

Test	Status	Time
COMP	Pass	9:22pm
CAL	Pass	9:22pm

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Mecklenburg Instrument Location BAT Mobile Unit 8
Instrument Serial No. 008775

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 21 day of August, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

2219283
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

MECKLENBURG COUNTY BAT MOBILE UNIT 8
590

Serial Number: 008775
Test Date: 08/21/2026

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Glasscock, Jerry D

Permit Number: 7180-9235

Effective:

02/01/2026-02/01/2028

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG506303

Exp Date: 03/04/2027

Test	g/210L	Time
DIAG	Pass	8:48pm
AIR BLK	.00	8:49pm
ACCY CHK	.08	8:50pm
AIR BLK	.00	8:51pm
SUB TEST	.00	8:51pm
AIR BLK	.00	8:52pm
SUB TEST	.00	8:54pm
AIR BLK	.00	8:54pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

MECKLENBURG COUNTY BAT MOBILE UNIT 8 590

Serial Number: 008775 Test Record Number: 2606
Test Date: 08/21/2026 Test Time: 8:55pm EDT

System Check: Passed

Baseline Tests

Test	Status	Time
IR	Pass	8:55pm
FLO	Pass	8:55pm
FC	Pass	8:55pm

Temperature Tests

Test	Status	Time
FC1	Pass	8:56pm
SRC	Pass	8:56pm
DET	Pass	8:56pm
BAR	Pass	8:56pm
BT	Pass	8:56pm

Blank Tests

Test	Status	Time
AIR	Pass	8:56pm

Printer Tests

Test	Status	Time
PRNT	Pass	8:56pm

CRC Tests

Test	Status	Time
COMP	Pass	8:56pm
CAL	Pass	8:56pm

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Mecklenburg Instrument Location BAT Mobile Unit 8
Instrument Serial No. 008775

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 22 day of August, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

2219283
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

MECKLENBURG COUNTY BAT MOBILE UNIT 8
590

Serial Number: 008775
Test Date: 08/22/2026

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE

Analyst's Name: Glasscock, Jerry D
Permit Number: 7180-9235
Effective:
02/01/2026-02/01/2028

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG506303
Exp Date: 03/04/2027

Test	g/210L	Time
DIAG	Pass	10:04pm
AIR BLK	.00	10:05pm
ACCY CHK	.08	10:06pm
AIR BLK	.00	10:07pm
SUB TEST	.00	10:08pm
AIR BLK	.00	10:08pm
SUB TEST	.00	10:10pm
AIR BLK	.00	10:11pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

MECKLENBURG COUNTY BAT MOBILE UNIT 8 590

Serial Number: 008775 Test Record Number: 2612
Test Date: 08/22/2026 Test Time: 10:11pm EDT

System Check: Passed

Baseline Tests

Test	Status	Time
IR	Pass	10:12pm
FLO	Pass	10:12pm
FC	Pass	10:12pm

Temperature Tests

Test	Status	Time
FC1	Pass	10:12pm
SRC	Pass	10:12pm
DET	Pass	10:12pm
BAR	Pass	10:12pm
BT	Pass	10:12pm

Blank Tests

Test	Status	Time
AIR	Pass	10:12pm

Printer Tests

Test	Status	Time
PRNT	Pass	10:12pm

CRC Tests

Test	Status	Time
COMP	Pass	10:13pm
CAL	Pass	10:13pm

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Mecklenburg Instrument Location BAT Mobile Unit 8
Instrument Serial No. 008775

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 27 day of August, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

2219283
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

MECKLENBURG COUNTY BAT MOBILE UNIT 8
590

Serial Number: 008775

Test Date: 08/27/2026

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Glasscock, Jerry D

Permit Number: 7180-9235

Effective:

02/01/2026-02/01/2028

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG506303

Exp Date: 03/04/2027

Test	g/210L	Time
DIAG	Pass	9:22pm
AIR BLK	.00	9:23pm
ACCY CHK	.08	9:24pm
AIR BLK	.00	9:25pm
SUB TEST	.00	9:25pm
AIR BLK	.00	9:26pm
SUB TEST	.00	9:28pm
AIR BLK	.00	9:29pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

Intox EC/IR-II: Preventive Maintenance

MECKLENBURG COUNTY BAT MOBILE UNIT 8 590

Serial Number: 008775 Test Record Number: 2616
Test Date: 08/27/2026 Test Time: 9:29pm EDT

System Check: Passed

Baseline Tests

Test	Status	Time
IR	Pass	9:29pm
FLO	Pass	9:29pm
FC	Pass	9:29pm

Temperature Tests

Test	Status	Time
FC1	Pass	9:29pm
SRC	Pass	9:29pm
DET	Pass	9:29pm
BAR	Pass	9:29pm
BT	Pass	9:29pm

Blank Tests

Test	Status	Time
AIR	Pass	9:30pm

Printer Tests

Test	Status	Time
PRNT	Pass	9:30pm

CRC Tests

Test	Status	Time
COMP	Pass	9:30pm
CAL	Pass	9:30pm

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Mecklenburg Instrument Location BAT Mobile Unit 8
Instrument Serial No. 008775 —

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 29 day of August, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

2219283
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

MECKLENBURG COUNTY BAT MOBILE UNIT 8
590

Serial Number: 008775
Test Date: 08/29/2026

Citation Number: M00000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Glasscock, Jerry D

Permit Number: 7180-9235

Effective:

02/01/2026-02/01/2028

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG506303

Exp Date: 03/04/2027

Test	g/210L	Time
DIAG	Pass	9:14pm
AIR BLK	.00	9:15pm
ACCY CHK	.08	9:16pm
AIR BLK	.00	9:17pm
SUB TEST	.00	9:17pm
AIR BLK	.00	9:18pm
SUB TEST	.00	9:20pm
AIR BLK	.00	9:21pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

MECKLENBURG COUNTY BAT MOBILE UNIT 8 590

Serial Number: 008775 Test Record Number: 2618
Test Date: 08/29/2026 Test Time: 9:21pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	9:21pm
FLO	Pass	9:21pm
FC	Pass	9:21pm

Temperature Tests

Test	Status	Time
FC1	Pass	9:21pm
SRC	Pass	9:21pm
DET	Pass	9:21pm
BAR	Pass	9:21pm
BT	Pass	9:21pm

Blank Tests

Test	Status	Time
AIR	Pass	9:22pm


Printer Tests

Test	Status	Time
PRNT	Pass	9:22pm

CRC Tests

Test	Status	Time
COMP	Pass	9:22pm
CAL	Pass	9:22pm

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Mecklenburg Instrument Location BAT Mobile Unit 8
Instrument Serial No. 008816

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 21 day of August, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

2219283
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

MECKLENBURG COUNTY BAT MOBILE UNIT 8
590

Serial Number: 008816
Test Date: 08/21/2026

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Glasscock, Jerry D

Permit Number: 7180-9235

Effective:

02/01/2026-02/01/2028

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG431002


Exp Date: 11/05/2026

Test	g/210L	Time
DIAG	Pass	8:45pm
AIR BLK	.00	8:46pm
ACCY CHK	.07	8:47pm
AIR BLK	.00	8:48pm
SUB TEST	.00	8:49pm
AIR BLK	.00	8:50pm
SUB TEST	.00	8:51pm
AIR BLK	.00	8:52pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

MECKLENBURG COUNTY BAT MOBILE UNIT 8 590

Serial Number: 008816 Test Record Number: 8175
Test Date: 08/21/2026 Test Time: 8:53pm EDT

System Check: Passed

Baseline Tests

Test	Status	Time
IR	Pass	8:53pm
FLO	Pass	8:53pm
FC	Pass	8:53pm

Temperature Tests

Test	Status	Time
FC1	Pass	8:53pm
SRC	Pass	8:53pm
DET	Pass	8:53pm
BAR	Pass	8:53pm
BT	Pass	8:53pm

Blank Tests

Test	Status	Time
AIR	Pass	8:54pm

Printer Tests

Test	Status	Time
PRNT	Pass	8:54pm

CRC Tests

Test	Status	Time
COMP	Pass	8:54pm
CAL	Pass	8:54pm

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Mecklenburg Instrument Location BAT Mobile Unit 8
Instrument Serial No. 008816 —

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 22 day of August, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

2219283
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

MECKLENBURG COUNTY BAT MOBILE UNIT 8
590

Serial Number: 008816

Test Date: 08/22/2026

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Glasscock, Jerry D

Permit Number: 7180-9235

Effective:

02/01/2026-02/01/2028

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG431002

Exp Date: 11/05/2026

Test	g/210L	Time
DIAG	Pass	9:45pm
AIR BLK	.00	9:46pm
ACCY CHK	.07	9:46pm
AIR BLK	.00	9:47pm
SUB TEST	.00	9:48pm
AIR BLK	.00	9:49pm
SUB TEST	.00	9:51pm
AIR BLK	.00	9:51pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

MECKLENBURG COUNTY BAT MOBILE UNIT 8 590

Serial Number: 008816 Test Record Number: 8179
Test Date: 08/22/2026 Test Time: 9:52pm EDT

System Check: Passed

Baseline Tests

Test	Status	Time
IR	Pass	9:52pm
FLO	Pass	9:52pm
FC	Pass	9:52pm

Temperature Tests

Test	Status	Time
FC1	Pass	9:52pm
SRC	Pass	9:52pm
DET	Pass	9:52pm
BAR	Pass	9:52pm
BT	Pass	9:52pm

Blank Tests

Test	Status	Time
AIR	Pass	9:53pm

Printer Tests

Test	Status	Time
PRNT	Pass	9:53pm

CRC Tests

Test	Status	Time
COMP	Pass	9:53pm
CAL	Pass	9:53pm

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Mecklenburg Instrument Location BAT Mobile Unit 8
Instrument Serial No. 008816

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 27 day of August, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

2219283
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years

Intox EC/IR-II: Subject Test

MECKLENBURG COUNTY BAT MOBILE UNIT 8
590

Serial Number: 008816
Test Date: 08/27/2026

Citation Number: M0000000-0
Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Glasscock, Jerry D

Permit Number: 7180-9235

Effective:

02/01/2026-02/01/2028

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG431002

Exp Date: 11/05/2026

Test	g/210L	Time
DIAG	Pass	9:32pm
AIR BLK	.00	9:33pm
ACCY CHK	.07	9:34pm
AIR BLK	.00	9:35pm
SUB TEST	.00	9:35pm
AIR BLK	.00	9:36pm
SUB TEST	.00	9:38pm
AIR BLK	.00	9:39pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

MECKLENBURG COUNTY BAT MOBILE UNIT 8 590

Serial Number: 008816 Test Record Number: 8183
Test Date: 08/27/2026 Test Time: 9:48pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	9:49pm
FLO	Pass	9:49pm
FC	Pass	9:49pm

Temperature Tests

Test	Status	Time
FC1	Pass	9:49pm
SRC	Pass	9:49pm
DET	Pass	9:49pm
BAR	Pass	9:49pm
BT	Pass	9:49pm

Blank Tests

Test	Status	Time
AIR	Pass	9:49pm

Printer Tests

Test	Status	Time
PRNT	Pass	9:49pm

CRC Tests

Test	Status	Time
COMP	Pass	9:50pm
CAL	Pass	9:50pm

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Mecklenburg Instrument Location BAT Mobile Unit 8
Instrument Serial No. 008816

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 29 day of August, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

2219283
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

MECKLENBURG COUNTY BAT MOBILE UNIT 8
590

Serial Number: 008816
Test Date: 08/29/2026

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Glasscock, Jerry D

Permit Number: 7180-9235

Effective:

02/01/2026-02/01/2028

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG431002

Exp Date: 11/05/2026

Test	g/210L	Time
DIAG	Pass	9:15pm
AIR BLK	.00	9:16pm
ACCY CHK	.07	9:17pm
AIR BLK	.00	9:18pm
SUB TEST	.00	9:18pm
AIR BLK	.00	9:19pm
SUB TEST	.00	9:21pm
AIR BLK	.00	9:21pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

Intox EC/IR-II: Preventive Maintenance

MECKLENBURG COUNTY BAT MOBILE UNIT 8 590

Serial Number: 008816 Test Record Number: 8185
Test Date: 08/29/2026 Test Time: 9:22pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	9:22pm
FLO	Pass	9:22pm
FC	Pass	9:22pm

Temperature Tests

Test	Status	Time
FC1	Pass	9:22pm
SRC	Pass	9:22pm
DET	Pass	9:22pm
BAR	Pass	9:22pm
BT	Pass	9:22pm

Blank Tests

Test	Status	Time
AIR	Pass	9:23pm

Printer Tests

Test	Status	Time
PRNT	Pass	9:23pm

CRC Tests

Test	Status	Time
COMP	Pass	9:23pm
CAL	Pass	9:23pm

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Mecklenburg Instrument Location BAT Mobile Unit 8
Instrument Serial No. 008929 —

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 21 day of August, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

2219283
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

MECKLENBURG COUNTY BAT MOBILE UNIT 8
590

Serial Number: 008929
Test Date: 08/21/2026

Citation Number: M0000000-0
Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Glasscock, Jerry D

Permit Number: 7180-9235

Effective:

02/01/2026-02/01/2028

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG506303

Exp Date: 03/04/2027

Test	g/210L	Time
DIAG	Pass	8:45pm
AIR BLK	.00	8:46pm
ACCY CHK	.08	8:46pm
AIR BLK	.00	8:48pm
SUB TEST	.00	8:48pm
AIR BLK	.00	8:50pm
SUB TEST	.00	8:51pm
AIR BLK	.00	8:52pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

MECKLENBURG COUNTY BAT MOBILE UNIT 8 590

Serial Number: 008929 Test Record Number: 1888

Test Date: 08/21/2026 Test Time: 8:52pm EDT

System Check: Passed

Baseline Tests

Test	Status	Time
IR	Pass	8:53pm
FLO	Pass	8:53pm
FC	Pass	8:53pm

Temperature Tests

Test	Status	Time
FC1	Pass	8:53pm
SRC	Pass	8:53pm
DET	Pass	8:53pm
BAR	Pass	8:53pm
BT	Pass	8:53pm

Blank Tests

Test	Status	Time
AIR	Pass	8:54pm


Printer Tests

Test	Status	Time
PRNT	Pass	8:54pm

CRC Tests

Test	Status	Time
COMP	Pass	8:54pm
CAL	Pass	8:54pm

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Mecklenburg Instrument Location BAT Mobile Unit 8
Instrument Serial No. 008929

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 22 day of August, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

2219283
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

MECKLENBURG COUNTY BAT MOBILE UNIT 8
590

Serial Number: 008929
Test Date: 08/22/2026

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE

Analyst's Name: Glasscock, Jerry D
Permit Number: 7180-9235
Effective:
02/01/2026-02/01/2028

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG506303
Exp Date: 03/04/2027

Test	g/210L	Time
DIAG	Pass	9:44pm
AIR BLK	.00	9:45pm
ACCY CHK	.08	9:46pm
AIR BLK	.00	9:47pm
SUB TEST	.00	9:48pm
AIR BLK	.00	9:49pm
SUB TEST	.00	9:50pm
AIR BLK	.00	9:51pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

MECKLENBURG COUNTY BAT MOBILE UNIT 8 590

Serial Number: 008929 Test Record Number: 1892
Test Date: 08/22/2026 Test Time: 9:51pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	9:52pm
FLO	Pass	9:52pm
FC	Pass	9:52pm

Temperature Tests

Test	Status	Time
FC1	Pass	9:52pm
SRC	Pass	9:52pm
DET	Pass	9:52pm
BAR	Pass	9:52pm
BT	Pass	9:52pm

Blank Tests

Test	Status	Time
AIR	Pass	9:53pm

Printer Tests

Test	Status	Time
PRNT	Pass	9:53pm

CRC Tests

Test	Status	Time
COMP	Pass	9:53pm
CAL	Pass	9:53pm

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County Mecklenburg Instrument Location BAT Mobile Unit 8
Instrument Serial No 008929 —

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 27 day of August, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

2219283
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

MECKLENBURG COUNTY BAT MOBILE UNIT 8
590

Serial Number: 008929
Test Date: 08/27/2026

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Glasscock, Jerry D

Permit Number: 7180-9235

Effective:

02/01/2026-02/01/2028

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG506303

Exp Date: 03/04/2027

Test	g/210L	Time
DIAG	Pass	9:24pm
AIR BLK	.00	9:25pm
ACCY CHK	.08	9:26pm
AIR BLK	.00	9:27pm
SUB TEST	.00	9:28pm
AIR BLK	.00	9:29pm
SUB TEST	.00	9:30pm
AIR BLK	.00	9:31pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

Intox EC/IR-II: Preventive Maintenance

MECKLENBURG COUNTY BAT MOBILE UNIT 8 590

Serial Number: 008929 Test Record Number: 1896
Test Date: 08/27/2026 Test Time: 9:31pm EDT

System Check: Passed

Baseline Tests

Test	Status	Time
IR	Pass	9:32pm
FLO	Pass	9:32pm
FC	Pass	9:32pm

Temperature Tests

Test	Status	Time
FC1	Pass	9:32pm
SRC	Pass	9:32pm
DET	Pass	9:32pm
BAR	Pass	9:32pm
BT	Pass	9:32pm

Blank Tests

Test	Status	Time
AIR	Pass	9:33pm

Printer Tests

Test	Status	Time
PRNT	Pass	9:33pm

CRC Tests

Test	Status	Time
COMP	Pass	9:33pm
CAL	Pass	9:33pm

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Mecklenburg Instrument Location BAT Mobile Unit 8
Instrument Serial No. 008929 —

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 29 day of August, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

2219283
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

MECKLENBURG COUNTY BAT MOBILE UNIT 8
590

Serial Number: 008929
Test Date: 08/29/2026

Citation Number: M00000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: Glasscock, Jerry D
Permit Number: 7180-9235
Effective:
02/01/2026-02/01/2028

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test


Lot Number: AG506303
Exp Date: 03/04/2027

Test	g/210L	Time
DIAG	Pass	9:15pm
AIR BLK	.00	9:17pm
ACCY CHK	.08	9:17pm
AIR BLK	.00	9:19pm
SUB TEST	.00	9:19pm
AIR BLK	.00	9:20pm
SUB TEST	.00	9:22pm
AIR BLK	.00	9:23pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

MECKLENBURG COUNTY BAT MOBILE UNIT 8 590

Serial Number: 008929 Test Record Number: 1898
Test Date: 08/29/2026 Test Time: 9:24pm EDT

System Check: Passed

Baseline Tests

Test	Status	Time
IR	Pass	9:24pm
FLO	Pass	9:24pm
FC	Pass	9:24pm

Temperature Tests

Test	Status	Time
FC1	Pass	9:24pm
SRC	Pass	9:24pm
DET	Pass	9:24pm
BAR	Pass	9:24pm
BT	Pass	9:24pm

Blank Tests

Test	Status	Time
AIR	Pass	9:25pm

Printer Tests

Test	Status	Time
PRNT	Pass	9:25pm

CRC Tests

Test	Status	Time
COMP	Pass	9:25pm
CAL	Pass	9:25pm

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County MONTGOMERY Instrument Location BAT Mobile unit 10

Instrument Serial No. 008584

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 29 day of August, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

193759
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

MONTGOMERY COUNTY BAT MOBILE UNIT 10
610

Serial Number: 008584

Test Date: 08/29/2026

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Carroll, Barry Jean D

Permit Number: 0019-3759

Effective:

04/01/2026-04/01/2028

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG534301

Exp Date: 12/09/2027

Test	g/210L	Time
DIAG	Pass	5:50pm
AIR BLK	.00	5:51pm
ACCY CHK	.08	5:51pm
AIR BLK	.00	5:52pm
SUB TEST	.00	5:53pm
AIR BLK	.00	5:54pm
SUB TEST	.00	5:55pm
AIR BLK	.00	5:56pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

This form is used when performing Preventive Maintenance procedures

Forensic Tests for Alcohol Branch

Department of Health and Human Services

Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

MONTGOMERY COUNTY BAT MOBILE UNIT 10 610

Serial Number: 008584 Test Record Number: 2950
Test Date: 08/29/2026 Test Time: 5:58pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	5:58pm
FLO	Pass	5:58pm
FC	Pass	5:58pm

Temperature Tests

Test	Status	Time
FC1	Pass	5:58pm
SRC	Pass	5:58pm
DET	Pass	5:58pm
BAR	Pass	5:58pm
BT	Pass	5:58pm

Blank Tests

Test	Status	Time
AIR	Pass	5:59pm

Printer Tests

Test	Status	Time
PRNT	Pass	5:59pm

CRC Tests

Test	Status	Time
COMP	Pass	5:59pm
CAL	Pass	5:59pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Montgomery Instrument Location BAT Mobile Unit 10

Instrument Serial No. 008037

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 29 day of AUGUST, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



A handwritten signature in black ink, appearing to read "B. E. E.", written over a horizontal line.

Signature of Certifying Official

193759

Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

MONTGOMERY COUNTY BAT MOBILE UNIT 10
610

Serial Number: 008637
Test Date: 08/29/2026

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Carroll, Barry Jean D

Permit Number: 0019-3759

Effective:

04/01/2026-04/01/2028

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG602101

Exp Date: 01/21/2028

Test	g/210L	Time
DIAG	Pass	6:00pm
AIR BLK	.00	6:01pm
ACCY CHK	.07	6:01pm
AIR BLK	.00	6:02pm
SUB TEST	.00	6:03pm
AIR BLK	.00	6:04pm
SUB TEST	.00	6:06pm
AIR BLK	.00	6:07pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

MONTGOMERY COUNTY BAT MOBILE UNIT 10 610

Serial Number: 008637 Test Record Number: 3649
Test Date: 08/29/2026 Test Time: 6:07pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	6:07pm
FLO	Pass	6:07pm
FC	Pass	6:07pm

Temperature Tests

Test	Status	Time
FC1	Pass	6:07pm
SRC	Pass	6:07pm
DET	Pass	6:07pm
BAR	Pass	6:07pm
BT	Pass	6:07pm

Blank Tests

Test	Status	Time
AIR	Pass	6:08pm

Printer Tests

Test	Status	Time
PRNT	Pass	6:08pm

CRC Tests

Test	Status	Time
COMP	Pass	6:08pm
CAL	Pass	6:08pm

Preventive Maintenance
Status: Pass



Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Montgomery Instrument Location BAT Mobile unit 10

Instrument Serial No. 006686

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 29 day of August, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Signature of Certifying Official

193759

Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

MONTGOMERY COUNTY BAT MOBILE UNIT 10
610

Serial Number: 008686
Test Date: 08/29/2026

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Carroll, Barry Jean D

Permit Number: 0019-3759

Effective:

04/01/2026-04/01/2028

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG506302

Exp Date: 03/04/2027

Test	g/210L	Time
DIAG	Pass	6:02pm
AIR BLK	.00	6:03pm
ACCY CHK	.08	6:03pm
AIR BLK	.00	6:04pm
SUB TEST	.00	6:05pm
AIR BLK	.00	6:06pm
SUB TEST	.00	6:07pm
AIR BLK	.00	6:08pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

MONTGOMERY COUNTY BAT MOBILE UNIT 10 610

Serial Number: 008686 Test Record Number: 7293
Test Date: 08/29/2026 Test Time: 6:09pm EDT

System Check: Passed

Baseline Tests

Test	Status	Time
IR	Pass	6:09pm
FLO	Pass	6:09pm
FC	Pass	6:09pm

Temperature Tests

Test	Status	Time
FC1	Pass	6:10pm
SRC	Pass	6:10pm
DET	Pass	6:10pm
BAR	Pass	6:10pm
BT	Pass	6:10pm

Blank Tests

Test	Status	Time
AIR	Pass	6:10pm

Printer Tests

Test	Status	Time
PRNT	Pass	6:10pm

CRC Tests

Test	Status	Time
COMP	Pass	6:10pm
CAL	Pass	6:10pm

**Preventive Maintenance
Status: Pass**



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Montgomery Instrument Location BAT Mobile unit 10

Instrument Serial No. 008776

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 29 day of August, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



A handwritten signature in black ink, appearing to be "B. J. [unclear]".

Signature of Certifying Official

193759

Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

MONTGOMERY COUNTY BAT MOBILE UNIT 10
610

Serial Number: 008776

Test Date: 08/29/2026

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Carroll, Barry Jean D

Permit Number: 0019-3759

Effective:

04/01/2026-04/01/2028

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG534301

Exp Date: 12/09/2027

Test	g/210L	Time
DIAG	Pass	5:54pm
AIR BLK	.00	5:55pm
ACCY CHK	.08	5:56pm
AIR BLK	.00	5:57pm
SUB TEST	.00	5:57pm
AIR BLK	.00	5:58pm
SUB TEST	.00	6:00pm
AIR BLK	.00	6:01pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

MONTGOMERY COUNTY BAT MOBILE UNIT 10 610

Serial Number: 008776 Test Record Number: 4273
Test Date: 08/29/2026 Test Time: 6:01pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	6:02pm
FLO	Pass	6:02pm
FC	Pass	6:02pm

Temperature Tests

Test	Status	Time
FC1	Pass	6:02pm
SRC	Pass	6:02pm
DET	Pass	6:02pm
BAR	Pass	6:02pm
BT	Pass	6:02pm

Blank Tests

Test	Status	Time
AIR	Pass	6:03pm

Printer Tests

Test	Status	Time
PRNT	Pass	6:03pm

CRC Tests

Test	Status	Time
COMP	Pass	6:03pm
CAL	Pass	6:03pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County MONTGOMERY Instrument Location BAT Mobile Unit 10

Instrument Serial No. 008779

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 29 day of August, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]

Signature of Certifying Official

193759

Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

MONTGOMERY COUNTY BAT MOBILE UNIT 10
610

Serial Number: 008779

Test Date: 08/29/2026

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Carroll, Barry Jean D

Permit Number: 0019-3759

Effective:

04/01/2026-04/01/2028

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG431002

Exp Date: 11/05/2026

Test	g/210L	Time
DIAG	Pass	5:52pm
AIR BLK	.00	5:53pm
ACCY CHK	.08	5:54pm
AIR BLK	.00	5:55pm
SUB TEST	.00	5:55pm
AIR BLK	.00	5:56pm
SUB TEST	.00	5:58pm
AIR BLK	.00	5:59pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

Intox EC/IR-II: Preventive Maintenance

MONTGOMERY COUNTY BAT MOBILE UNIT 10 610

Serial Number: 008779 Test Record Number: 4190
Test Date: 08/29/2026 Test Time: 6:00pm EDT

System Check: Passed

Baseline Tests

Test	Status	Time
IR	Pass	6:00pm
FLO	Pass	6:00pm
FC	Pass	6:00pm

Temperature Tests

Test	Status	Time
FC1	Pass	6:00pm
SRC	Pass	6:00pm
DET	Pass	6:00pm
BAR	Pass	6:00pm
BT	Pass	6:00pm

Blank Tests

Test	Status	Time
AIR	Pass	6:01pm

Printer Tests

Test	Status	Time
PRNT	Pass	6:01pm

CRC Tests

Test	Status	Time
COMP	Pass	6:01pm
CAL	Pass	6:01pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County NASH

Instrument Location Rocky Mount PD

Instrument Serial No. 008651

Rocky Mount, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 27 day of AUGUST, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



A handwritten signature in black ink, appearing to read "E. B. Smith", written over a horizontal line.

Signature of Certifying Official

179707

Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

NASH COUNTY ROCKY MOUNT PD 630

Serial Number: 008651

Test Date: 08/27/2026

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Bryant, Earl A

Permit Number: 0017-9707

Effective:

02/01/2026-02/01/2028

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG602202

Exp Date: 01/22/2028

Test	g/210L	Time
DIAG	Pass	4:27pm
AIR BLK	.00	4:28pm
ACCY CHK	.08	4:28pm
AIR BLK	.00	4:29pm
SUB TEST	.00	4:30pm
AIR BLK	.00	4:31pm
SUB TEST	.00	4:32pm
AIR BLK	.00	4:33pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

This form is used when performing Preventive Maintenance procedures

Forensic Tests for Alcohol Branch

Department of Health and Human Services

Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

NASH COUNTY ROCKY MOUNT PD 630

Serial Number: 008651 Test Record Number: 1887
Test Date: 08/27/2026 Test Time: 4:35pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	4:35pm
FLO	Pass	4:35pm
FC	Pass	4:35pm

Temperature Tests

Test	Status	Time
FC1	Pass	4:35pm
SRC	Pass	4:35pm
DET	Pass	4:35pm
BAR	Pass	4:35pm
BT	Pass	4:35pm

Blank Tests

Test	Status	Time
AIR	Pass	4:36pm

Printer Tests

Test	Status	Time
PRNT	Pass	4:36pm

CRC Tests

Test	Status	Time
COMP	Pass	4:36pm
CAL	Pass	4:36pm

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County NASH Instrument Location Rocky Mount PD
Instrument Serial No. 008741 Rocky Mount, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 27 day of AUGUST, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

179707
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

NASH COUNTY ROCKY MOUNT PD 630

Serial Number: 008741

Test Date: 08/27/2026

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Bryant, Earl A

Permit Number: 0017-9707

Effective:

02/01/2026-02/01/2028

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG602202

Exp Date: 01/22/2028

Test	g/210L	Time
DIAG	Pass	3:39pm
AIR BLK	.00	3:40pm
ACCY CHK	.07	3:40pm
AIR BLK	.00	3:42pm
SUB TEST	.00	3:42pm
AIR BLK	.00	3:43pm
SUB TEST	.00	3:44pm
AIR BLK	.00	3:45pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

Intox EC/IR-II: Preventive Maintenance

NASH COUNTY ROCKY MOUNT PD 630

Serial Number: 008741 Test Record Number: 3380
Test Date: 08/27/2026 Test Time: 3:47pm EDT

System Check: Passed

Baseline Tests

Test	Status	Time
IR	Pass	3:47pm
FLO	Pass	3:47pm
FC	Pass	3:47pm

Temperature Tests

Test	Status	Time
FC1	Pass	3:47pm
SRC	Pass	3:47pm
DET	Pass	3:47pm
BAR	Pass	3:47pm
BT	Pass	3:47pm

Blank Tests

Test	Status	Time
AIR	Pass	3:48pm

Printer Tests

Test	Status	Time
PRNT	Pass	3:48pm

CRC Tests

Test	Status	Time
COMP	Pass	3:48pm
CAL	Pass	3:48pm

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Pasquotank Instrument Location Pasquotank Co. Public Safety Bldg.
Elizabeth City, NC
Instrument Serial No. 008950

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 27th day of August, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

206272
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

PASQUOTANK COUNTY PUBLIC SAFETY BLDG
690

Serial Number: 008950
Test Date: 08/27/2026

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE

Analyst's Name: Chappell, Mark A
Permit Number: 0020-6272
Effective:
02/01/2026-02/01/2028

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

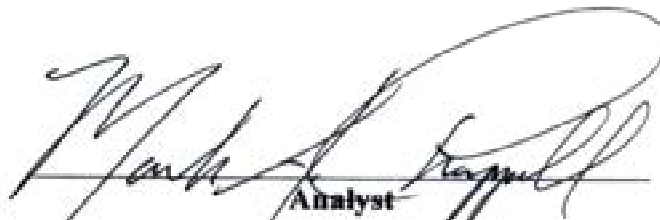
Lot Number: AG501303
Exp Date: 01/13/2027

Test	g/210L	Time
DIAG	Pass	11:11am
AIR BLK	.00	11:12am
ACCY CHK	.07	11:13am
AIR BLK	.00	11:14am
SUB TEST	.00	11:16am
AIR BLK	.00	11:17am
SUB TEST	.00	11:18am
AIR BLK	.00	11:19am

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

PASQUOTANK COUNTY PUBLIC SAFETY BLDG 690

Serial Number: 008950 Test Record Number: 2296
Test Date: 08/27/2026 Test Time: 11:21am EDT

System Check: Passed

Baseline Tests

Test	Status	Time
IR	Pass	11:21am
FLO	Pass	11:21am
FC	Pass	11:21am

Temperature Tests

Test	Status	Time
FC1	Pass	11:21am
SRC	Pass	11:21am
DET	Pass	11:21am
BAR	Pass	11:21am
BT	Pass	11:21am

Blank Tests

Test	Status	Time
AIR	Pass	11:22am

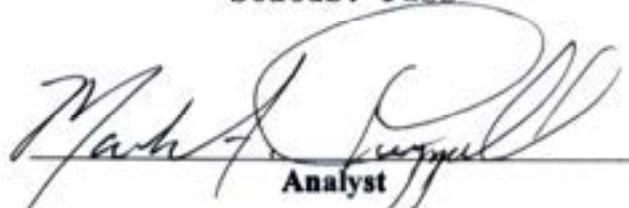
Printer Tests

Test	Status	Time
PRNT	Pass	11:22am

CRC Tests

Test	Status	Time
COMP	Pass	11:22am
CAL	Pass	11:22am

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County PENDER Instrument Location PENDER COUNTY GOVERNMENT AGENCY
Instrument Serial No. 008948 Hampstead NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 7th day of August, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.





Signature of Certifying Official

282-4950

Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

PENDER COUNTY GOVERNMENT ANNEX 700

Serial Number: 008948
Test Date: 08/07/2026

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: GILLESPIE, PENTTI W

Permit Number: 9523-2149

Effective:

02/01/2026-02/01/2028

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

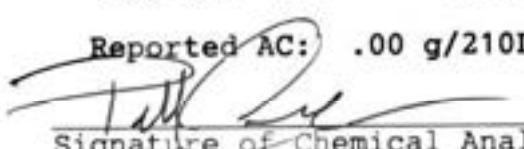
Test Type: Breath Test

Lot Number: AG534301

Exp Date: 12/09/2027

Test	g/210L	Time
DIAG	Pass	9:52am
AIR BLK	.00	9:52am
ACCY CHK	.07	9:53am
AIR BLK	.00	9:54am
SUB TEST	.00	9:55am
AIR BLK	.00	9:55am
SUB TEST	.00	9:57am
AIR BLK	.00	9:58am

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

PENDER COUNTY GOVERNMENT ANNEX 700

Serial Number: 008948 Test Record Number: 1694

Test Date: 08/07/2026 Test Time: 9:58am EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	9:59am
FLO	Pass	9:59am
FC	Pass	9:59am

Temperature Tests

Test	Status	Time
FC1	Pass	9:59am
SRC	Pass	9:59am
DET	Pass	9:59am
BAR	Pass	9:59am
BT	Pass	9:59am

Blank Tests

Test	Status	Time
AIR	Pass	9:59am

Printer Tests

Test	Status	Time
PRNT	Pass	10:00am

CRC Tests

Test	Status	Time
COMP	Pass	10:00am
CAL	Pass	10:00am

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Lobson Instrument Location BAT Mobile Unit 9
Instrument Serial No. 008575

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 20th day of August, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.




Signature of Certifying Official

2266313
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

ROBESON COUNTY BAT MOBILE UNIT 9 770

Serial Number: 008575

Test Date: 08/20/2026

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Sharpe Jr., Robert J

Permit Number: 1820-8591

Effective:

02/01/2026-02/01/2028

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG516204

Exp Date: 06/11/2027

Test	g/210L	Time
DIAG	Pass	6:41pm
AIR BLK	.00	6:42pm
ACCY CHK	.07	6:43pm
AIR BLK	.00	6:44pm
SUB TEST	.00	6:45pm
AIR BLK	.00	6:45pm
SUB TEST	.00	6:47pm
AIR BLK	.00	6:48pm

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR


Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

ROBESON COUNTY BAT MOBILE UNIT 9 770

Serial Number: 008575 Test Record Number: 1644
Test Date: 08/20/2026 Test Time: 6:50pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	6:50pm
FLO	Pass	6:50pm
FC	Pass	6:50pm

Temperature Tests

Test	Status	Time
FC1	Pass	6:50pm
SRC	Pass	6:50pm
DET	Pass	6:50pm
BAR	Pass	6:50pm
BT	Pass	6:50pm

Blank Tests

Test	Status	Time
AIR	Pass	6:51pm

Printer Tests

Test	Status	Time
PRNT	Pass	6:51pm

CRC Tests

Test	Status	Time
COMP	Pass	6:51pm
CAL	Pass	6:51pm

Preventive Maintenance
Status: *Pass*



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Robeson Instrument Location BAT Mobile Unit 9
Instrument Serial No. 008616

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 20th day of August, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

2266313
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

ROBESON COUNTY BAT MOBILE UNIT 9 770

Serial Number: 008616
Test Date: 08/20/2026

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Sharpe Jr., Robert J

Permit Number: 1820-8591

Effective:

02/01/2026-02/01/2028

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG506303

Exp Date: 03/04/2027

Test	g/210L	Time
DIAG	Pass	6:40pm
AIR BLK	.00	6:42pm
ACCY CHK	.07	6:42pm
AIR BLK	.00	6:43pm
SUB TEST	.00	6:44pm
AIR BLK	.00	6:45pm
SUB TEST	.00	6:47pm
AIR BLK	.00	6:48pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

ROBESON COUNTY BAT MOBILE UNIT 9 770

Serial Number: 008616 Test Record Number: 3071
Test Date: 08/20/2026 Test Time: 6:49pm EDT

System Check: Passed

Baseline Tests

Test	Status	Time
IR	Pass	6:49pm
FLO	Pass	6:49pm
FC	Pass	6:50pm

Temperature Tests

Test	Status	Time
FC1	Pass	6:50pm
SRC	Pass	6:50pm
DET	Pass	6:50pm
BAR	Pass	6:50pm
BT	Pass	6:50pm

Blank Tests

Test	Status	Time
AIR	Pass	6:50pm

Printer Tests

Test	Status	Time
PRNT	Pass	6:50pm

CRC Tests

Test	Status	Time
COMP	Pass	6:51pm
CAL	Pass	6:51pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Robeson Instrument Location BAT Mobile Unit 9
Instrument Serial No. 008647

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 20th day of August, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.




Signature of Certifying Official

2266313
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

ROBESON COUNTY BAT MOBILE UNIT 9 770

Serial Number: 008647

Test Date: 08/20/2026

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Sharpe Jr., Robert J

Permit Number: 1820-8591

Effective:

02/01/2026-02/01/2028

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG516203

Exp Date: 06/11/2027

Test	g/210L	Time
DIAG	Pass	6:44pm
AIR BLK	.00	6:45pm
ACCY CHK	.07	6:46pm
AIR BLK	.00	6:47pm
SUB TEST	.00	6:47pm
AIR BLK	.00	6:48pm
SUB TEST	.00	6:50pm
AIR BLK	.00	6:51pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

ROBESON COUNTY BAT MOBILE UNIT 9 770

Serial Number: 008647 Test Record Number: 3032
Test Date: 08/20/2026 Test Time: 6:51pm EDT

System Check: Passed

Baseline Tests

Test	Status	Time
IR	Pass	6:52pm
FLO	Pass	6:52pm
FC	Pass	6:52pm

Temperature Tests

Test	Status	Time
FC1	Pass	6:52pm
SRC	Pass	6:52pm
DET	Pass	6:52pm
BAR	Pass	6:52pm
BT	Pass	6:52pm

Blank Tests

Test	Status	Time
AIR	Pass	6:52pm

Printer Tests

Test	Status	Time
PRNT	Pass	6:53pm

CRC Tests

Test	Status	Time
COMP	Pass	6:53pm
CAL	Pass	6:53pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Robeson Instrument Location BAT Mobile Unit 9

Instrument Serial No. 008704

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 20th day of August, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

2266313
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

ROBESON COUNTY BAT MOBILE UNIT 9 770

Serial Number: 008704

Test Date: 08/20/2026

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Sharpe Jr., Robert J

Permit Number: 1820-8591

Effective:

02/01/2026-02/01/2028

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG506303

Exp Date: 03/04/2027

Test	g/210L	Time
DIAG	Pass	6:43pm
AIR BLK	.00	6:44pm
ACCY CHK	.07	6:45pm
AIR BLK	.00	6:46pm
SUB TEST	.00	6:46pm
AIR BLK	.00	6:47pm
SUB TEST	.00	6:49pm
AIR BLK	.00	6:50pm

Reported AC: 00 g/210L

Signature of Chemical Analyst

Court CVR



Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

ROBESON COUNTY BAT MOBILE UNIT 9 770

Serial Number: 008704 Test Record Number: 1080
Test Date: 08/20/2026 Test Time: 6:50pm EDT

System Check: Passed

Baseline Tests

Test	Status	Time
IR	Pass	6:50pm
FLO	Pass	6:50pm
FC	Pass	6:51pm

Temperature Tests

Test	Status	Time
FC1	Pass	6:51pm
SRC	Pass	6:51pm
DET	Pass	6:51pm
BAR	Pass	6:51pm
BT	Pass	6:51pm

Blank Tests

Test	Status	Time
AIR	Pass	6:51pm

Printer Tests

Test	Status	Time
PRNT	Pass	6:51pm

CRC Tests

Test	Status	Time
COMP	Pass	6:52pm
CAL	Pass	6:52pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Robeson Instrument Location BAT Mobile Unit 9
Instrument Serial No. 008826

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 20th day of August, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

2266313
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

ROBESON COUNTY BAT MOBILE UNIT 9 770

Serial Number: 008826
Test Date: 08/20/2026

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Sharpe Jr., Robert J

Permit Number: 1820-8591

Effective:

02/01/2026-02/01/2028

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG516204

Exp Date: 06/11/2027

Test	g/210L	Time
DIAG	Pass	6:55pm
AIR BLK	.00	6:56pm
ACCY CHK	.07	6:56pm
AIR BLK	.00	6:57pm
SUB TEST	.00	6:58pm
AIR BLK	.00	6:59pm
SUB TEST	.00	7:00pm
AIR BLK	.00	7:01pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

ROBESON COUNTY BAT MOBILE UNIT 9 770

Serial Number: 008826 Test Record Number: 8721
Test Date: 08/20/2026 Test Time: 7:03pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	7:04pm
FLO	Pass	7:04pm
FC	Pass	7:04pm

Temperature Tests

Test	Status	Time
FC1	Pass	7:04pm
SRC	Pass	7:04pm
DET	Pass	7:04pm
BAR	Pass	7:04pm
BT	Pass	7:04pm

Blank Tests

Test	Status	Time
AIR	Pass	7:04pm

Printer Tests

Test	Status	Time
PRNT	Pass	7:04pm

CRC Tests

Test	Status	Time
COMP	Pass	7:05pm
CAL	Pass	7:05pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Rockingham Instrument Location Eden Police Department
Instrument Serial No. 008592 Eden, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 25th day of August, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

509387
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

ROCKINGHAM COUNTY EDEN PD 780

Serial Number: 008592

Test Date: 08/25/2026

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Long, Thomas A

Permit Number: 0050-9387

Effective:

02/01/2026-02/01/2028

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG534301

Exp Date: 12/09/2027

Test	g/210L	Time
DIAG	Pass	9:23am
AIR BLK	.00	9:24am
ACCY CHK	.07	9:24am
AIR BLK	.00	9:26am
SUB TEST	.00	9:27am
AIR BLK	.00	9:28am
SUB TEST	.00	9:29am
AIR BLK	.00	9:30am

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

ROCKINGHAM COUNTY EDEN PD 780

Serial Number: 008592 Test Record Number: 5254
Test Date: 08/25/2026 Test Time: 9:31am EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	9:31am
FLO	Pass	9:31am
FC	Pass	9:31am

Temperature Tests

Test	Status	Time
FC1	Pass	9:31am
SRC	Pass	9:31am
DET	Pass	9:31am
BAR	Pass	9:31am
BT	Pass	9:31am

Blank Tests

Test	Status	Time
AIR	Pass	9:32am

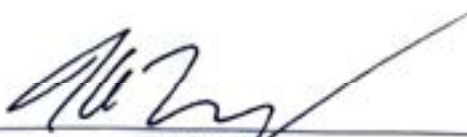
Printer Tests

Test	Status	Time
PRNT	Pass	9:32am

CRC Tests

Test	Status	Time
COMP	Pass	9:32am
CAL	Pass	9:32am

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County SAMPSON Instrument Location SAMPSON COUNTY
Instrument Serial No. 008825 DETENTION CENTER
CLINTON, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 31 day of AUGUST, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Alan R. Burns
Signature of Certifying Official

146279
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

SAMPSON COUNTY DETENTION CENTER 810

Serial Number: 008825

Test Date: 08/31/2026

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: BARNES, ALVIN R

Permit Number: 0014-6279

Effective:

02/01/2026-02/01/2028

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG534301

Exp Date: 12/09/2027

Test . g/210L Time

DIAG Pass 10:33am

AIR BLK .00 10:34am

ACCY CHK .08 10:34am

AIR BLK .00 10:36am


SUB TEST .00 10:36am

AIR BLK .00 10:37am


SUB TEST .00 10:39am

AIR BLK .00 10:40am

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

SAMPSON COUNTY DETENTION CENTER 810

Serial Number: 008825 Test Record Number: 4448
Test Date: 08/31/2026 Test Time: 10:44am EDT

System Check: Passed

Baseline Tests

Test	Status	Time
IR	Pass	10:44am
FLO	Pass	10:44am
FC	Pass	10:44am

Temperature Tests

Test	Status	Time
FC1	Pass	10:45am
SRC	Pass	10:45am
DET	Pass	10:45am
BAR	Pass	10:45am
BT	Pass	10:45am

Blank Tests

Test	Status	Time
AIR	Pass	10:45am


Printer Tests

Test	Status	Time
PRNT	Pass	10:45am

CRC Tests

Test	Status	Time
COMP	Pass	10:45am
CAL	Pass	10:45am

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County SAMPSON Instrument Location SAMPSON COUNTY
Instrument Serial No. 008877 DETENTION CENTER
CLINTON, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 31 day of AUGUST, 20 26 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Alan R. B...

Signature of Certifying Official

146279

Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

SAMPSON COUNTY DETENTION CENTER 810

Serial Number: 008877

Test Date: 08/31/2026

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: BARNES, ALVIN R

Permit Number: 0014-6279

Effective:

02/01/2026-02/01/2028

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG534301


Exp Date: 12/09/2027

Test	g/210L	Time
DIAG	Pass	10:34am
AIR BLK	.00	10:35am
ACCY CHK	.08	10:35am
AIR BLK	.00	10:37am
SUB TEST	.00	10:37am
AIR BLK	.00	10:38am
SUB TEST	.00	10:40am
AIR BLK	.00	10:41am

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

This form is used when performing Preventive Maintenance procedures

Forensic Tests for Alcohol Branch

Department of Health and Human Services

Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

SAMPSON COUNTY DETENTION CENTER 810

Serial Number: 008877 Test Record Number: 4367
Test Date: 08/31/2026 Test Time: 10:44am EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	10:45am
FLO	Pass	10:45am
FC	Pass	10:45am

Temperature Tests

Test	Status	Time
FC1	Pass	10:45am
SRC	Pass	10:45am
DET	Pass	10:45am
BAR	Pass	10:45am
BT	Pass	10:45am

Blank Tests

Test	Status	Time
AIR	Pass	10:45am


Printer Tests

Test	Status	Time
PRNT	Pass	10:45am

CRC Tests

Test	Status	Time
COMP	Pass	10:46am
CAL	Pass	10:46am

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Scotland Instrument Location Laurinburg Police Dept.
Instrument Serial No. 008834 Laurinburg, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 17 day of August, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.





Signature of Certifying Official

365156
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

SCOTLAND COUNTY LAURINBURG PD 820

Serial Number: 008834
Test Date: 08/17/2026

Citation Number: M0000000-0
Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Garner, Joel K

Permit Number: 0036-5156

Effective:

02/01/2026-02/01/2028

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG534301
Exp Date: 12/09/2027

Test	g/210L	Time
DIAG	Pass	9:27am
AIR BLK	.00	9:28am
ACCY CHK	.07	9:29am
AIR BLK	.00	9:30am
SUB TEST	.00	9:30am
AIR BLK	.00	9:31am
SUB TEST	.00	9:33am
AIR BLK	.00	9:33am

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

Intox EC/IR-II: Preventive Maintenance

SCOTLAND COUNTY LAURINBURG PD 820

Serial Number: 008834 Test Record Number: 1408
Test Date: 08/17/2026 Test Time: 9:34am EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	9:34am
FLO	Pass	9:34am
FC	Pass	9:34am

Temperature Tests

Test	Status	Time
FC1	Pass	9:34am
SRC	Pass	9:34am
DET	Pass	9:34am
BAR	Pass	9:34am
BT	Pass	9:34am

Blank Tests

Test	Status	Time
AIR	Pass	9:35am

Printer Tests

Test	Status	Time
PRNT	Pass	9:35am

CRC Tests

Test	Status	Time
COMP	Pass	9:35am
CAL	Pass	9:35am

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Scotland Instrument Location Scotland County S. O.
Instrument Serial No. 008861 Laurinburg, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 17 day of August, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



A handwritten signature in black ink, appearing to be "K. A. L.", written over a horizontal line.

Signature of Certifying Official

365156
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

SCOTLAND COUNTY SHERIFFS OFFICE 820

Serial Number: 008861

Test Date: 08/17/2026

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Garner, Joel K

Permit Number: 0036-5156

Effective:

02/01/2026-02/01/2028

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG602203

Exp Date: 01/22/2028

Test	g/210L	Time
DIAG	Pass	10:35am
AIR BLK	.00	10:36am
ACCY CHK	.08	10:37am
AIR BLK	.00	10:38am
SUB TEST	.00	10:38am
AIR BLK	.00	10:39am
SUB TEST	.00	10:41am
AIR BLK	.00	10:42am

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

SCOTLAND COUNTY SHERIFFS OFFICE 820

Serial Number: 008861 Test Record Number: 2269
Test Date: 08/17/2026 Test Time: 10:42am EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	10:42am
FLO	Pass	10:42am
FC	Pass	10:43am

Temperature Tests

Test	Status	Time
FC1	Pass	10:43am
SRC	Pass	10:43am
DET	Pass	10:43am
BAR	Pass	10:43am
BT	Pass	10:43am

Blank Tests

Test	Status	Time
AIR	Pass	10:43am

Printer Tests

Test	Status	Time
PRNT	Pass	10:43am

CRC Tests

Test	Status	Time
COMP	Pass	10:43am
CAL	Pass	10:43am

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Stanly Instrument Location BAT Mobile Unit 8
Instrument Serial No. 008615 —

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 22 day of August, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature] 2219283
Signature of Certifying Official Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

STANLY COUNTY BAT MOBILE UNIT 8 830

Serial Number: 008615

Test Date: 08/22/2026

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Glasscock, Jerry D

Permit Number: 7180-9235

Effective:

02/01/2026-02/01/2028

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG506303

Exp Date: 03/04/2027

Test	g/210L	Time
DIAG	Pass	3:25pm
AIR BLK	.00	3:26pm
ACCY CHK	.07	3:26pm
AIR BLK	.00	3:27pm
SUB TEST	.00	3:28pm
AIR BLK	.00	3:29pm
SUB TEST	.00	3:30pm
AIR BLK	.00	3:31pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

Intox EC/IR-II: Preventive Maintenance

STANLY COUNTY BAT MOBILE UNIT 8 830

Serial Number: 008615 Test Record Number: 6391
Test Date: 08/22/2026 Test Time: 3:32pm EDT

System Check: Passed

Baseline Tests

Test	Status	Time
IR	Pass	3:32pm
FLO	Pass	3:32pm
FC	Pass	3:32pm

Temperature Tests

Test	Status	Time
FC1	Pass	3:32pm
SRC	Pass	3:32pm
DET	Pass	3:32pm
BAR	Pass	3:32pm
BT	Pass	3:32pm

Blank Tests

Test	Status	Time
AIR	Pass	3:33pm

Printer Tests

Test	Status	Time
PRNT	Pass	3:33pm

CRC Tests

Test	Status	Time
COMP	Pass	3:33pm
CAL	Pass	3:33pm

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Stanly Instrument Location BAT Mobile Unit 8
Instrument Serial No. 008736 —

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 22 day of August, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

2219283
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

STANLY COUNTY BAT MOBILE UNIT 8 830

Serial Number: 008736
Test Date: 08/22/2026

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Glasscock, Jerry D

Permit Number: 7180-9235

Effective:

02/01/2026-02/01/2028

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

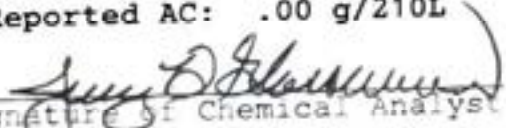
Test Type: Breath Test

Lot Number: AG506303

Exp Date: 03/04/2027

Test	g/210L	Time
DIAG	Pass	3:24pm
AIR BLK	.00	3:25pm
ACCY CHK	.07	3:26pm
AIR BLK	.00	3:27pm
SUB TEST	.00	3:27pm
AIR BLK	.00	3:28pm
SUB TEST	.00	3:29pm
AIR BLK	.00	3:30pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

STANLY COUNTY BAT MOBILE UNIT 8 830

Serial Number: 008736 Test Record Number: 1741
Test Date: 08/22/2026 Test Time: 3:31pm EDT

System Check: Passed

Baseline Tests

Test	Status	Time
IR	Pass	3:31pm
FLO	Pass	3:31pm
FC	Pass	3:31pm

Temperature Tests

Test	Status	Time
FC1	Pass	3:31pm
SRC	Pass	3:31pm
DET	Pass	3:31pm
BAR	Pass	3:31pm
BT	Pass	3:31pm

Blank Tests

Test	Status	Time
AIR	Pass	3:32pm

Printer Tests

Test	Status	Time
PRNT	Pass	3:32pm

CRC Tests

Test	Status	Time
COMP	Pass	3:32pm
CAL	Pass	3:32pm

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Stanly Instrument Location BAT Mobile Unit 8
Instrument Serial No. 008775 —

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 22 day of August, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

2219283
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

STANLY COUNTY BAT MOBILE UNIT 8 830

Serial Number: 008775
Test Date: 08/22/2026

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Glasscock, Jerry D

Permit Number: 7180-9235

Effective:

02/01/2026-02/01/2028

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG506303

Exp Date: 03/04/2027

Test	g/210L	Time
DIAG	Pass	3:23pm
AIR BLK	.00	3:24pm
ACCY CHK	.08	3:25pm
AIR BLK	.00	3:26pm
SUB TEST	.00	3:26pm
AIR BLK	.00	3:27pm
SUB TEST	.00	3:29pm
AIR BLK	.00	3:30pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

STANLY COUNTY BAT MOBILE UNIT 8 830

Serial Number: 008775 Test Record Number: 2608
Test Date: 08/22/2026 Test Time: 3:31pm EDT

System Check: Passed

Baseline Tests

Test	Status	Time
IR	Pass	3:31pm
FLO	Pass	3:31pm
FC	Pass	3:31pm

Temperature Tests

Test	Status	Time
FC1	Pass	3:31pm
SRC	Pass	3:31pm
DET	Pass	3:31pm
BAR	Pass	3:31pm
BT	Pass	3:31pm

Blank Tests

Test	Status	Time
AIR	Pass	3:32pm

Printer Tests

Test	Status	Time
PRNT	Pass	3:32pm

CRC Tests

Test	Status	Time
COMP	Pass	3:32pm
CAL	Pass	3:32pm

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Stanly Instrument Location BAT Mobile Unit 8
Instrument Serial No. 008816

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 22 day of August, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

2219283
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

STANLY COUNTY BAT MOBILE UNIT 8 830

Serial Number: 008816

Test Date: 08/22/2026

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Glasscock, Jerry D

Permit Number: 7180-9235

Effective:

02/01/2026-02/01/2028

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG431002

Exp Date: 11/05/2026

Test	g/210L	Time
DIAG	Pass	3:23pm
AIR BLK	.00	3:24pm
ACCY CHK	.07	3:24pm
AIR BLK	.00	3:26pm
SUB TEST	.00	3:27pm
AIR BLK	.00	3:27pm
SUB TEST	.00	3:29pm
AIR BLK	.00	3:30pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

STANLY COUNTY BAT MOBILE UNIT 8 830

Serial Number: 008816 Test Record Number: 8177
Test Date: 08/22/2026 Test Time: 3:31pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	3:31pm
FLO	Pass	3:31pm
FC	Pass	3:31pm

Temperature Tests

Test	Status	Time
FC1	Pass	3:31pm
SRC	Pass	3:31pm
DET	Pass	3:31pm
BAR	Pass	3:31pm
BT	Pass	3:31pm

Blank Tests

Test	Status	Time
AIR	Pass	3:32pm

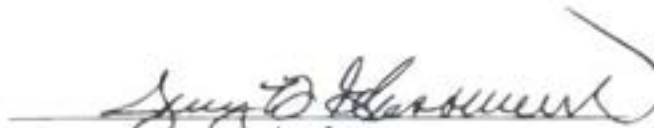
Printer Tests

Test	Status	Time
PRNT	Pass	3:32pm

CRC Tests

Test	Status	Time
COMP	Pass	3:32pm
CAL	Pass	3:32pm

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Stanly Instrument Location Stanly County 80
Instrument Serial No. 008842 Albemarle, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 17th day of August, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

849845
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

STANLY COUNTY STANLY COUNTY SO 830

Serial Number: 008842

Test Date: 08/17/2026

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Helms, Bryce A

Permit Number: 0084-9845

Effective:

02/01/2026-02/01/2028

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG535002

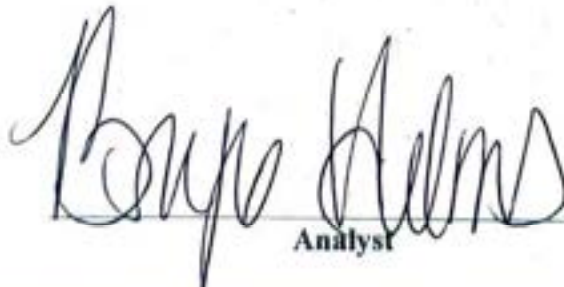
Exp Date: 12/16/2027

Test	g/210L	Time
DIAG	Pass	1:22pm
AIR BLK	.00	1:23pm
ACCY CHK	.08	1:24pm
AIR BLK	.00	1:25pm
SUB TEST	.00	1:25pm
AIR BLK	.00	1:26pm
SUB TEST	.00	1:28pm
AIR BLK	.00	1:29pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

Intox EC/IR-II: Preventive Maintenance

STANLY COUNTY STANLY COUNTY SO 830

Serial Number: 008842 Test Record Number: 3431
Test Date: 08/17/2026 Test Time: 1:29pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	1:29pm
FLO	Pass	1:29pm
FC	Pass	1:29pm

Temperature Tests

Test	Status	Time
FC1	Pass	1:29pm
SRC	Pass	1:29pm
DET	Pass	1:29pm
BAR	Pass	1:29pm
BT	Pass	1:29pm

Blank Tests

Test	Status	Time
AIR	Pass	1:30pm

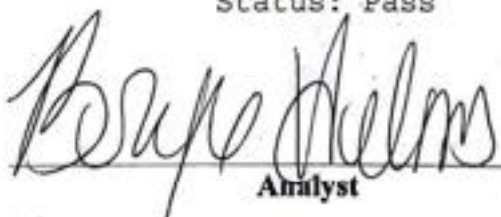
Printer Tests

Test	Status	Time
PRNT	Pass	1:30pm

CRC Tests

Test	Status	Time
COMP	Pass	1:30pm
CAL	Pass	1:30pm

Preventive Maintenance
Status: *Pass*


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Stanly Instrument Location BAT Mobile Unit 8
Instrument Serial No. 008929

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 22 day of August, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

2219283
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

STANLY COUNTY BAT MOBILE UNIT 8 830

Serial Number: 008929

Test Date: 08/22/2026

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Glasscock, Jerry D

Permit Number: 7180-9235

Effective:

02/01/2026-02/01/2028

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG506303

Exp Date: 03/04/2027

Test	g/210L	Time
DIAG	Pass	3:22pm
AIR BLK	.00	3:23pm
ACCY CHK	.08	3:24pm
AIR BLK	.00	3:25pm
SUB TEST	.00	3:26pm
AIR BLK	.00	3:27pm
SUB TEST	.00	3:29pm
AIR BLK	.00	3:30pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

Intox EC/IR-II: Preventive Maintenance

STANLY COUNTY BAT MOBILE UNIT 8 830

Serial Number: 008929 Test Record Number: 1890
Test Date: 08/22/2026 Test Time: 3:30pm EDT

System Check: Passed

Baseline Tests

Test	Status	Time
IR	Pass	3:31pm
FLO	Pass	3:31pm
FC	Pass	3:31pm

Temperature Tests

Test	Status	Time
FC1	Pass	3:31pm
SRC	Pass	3:31pm
DET	Pass	3:31pm
BAR	Pass	3:31pm
BT	Pass	3:31pm

Blank Tests

Test	Status	Time
AIR	Pass	3:32pm

Printer Tests

Test	Status	Time
PRNT	Pass	3:32pm

CRC Tests

Test	Status	Time
COMP	Pass	3:32pm
CAL	Pass	3:32pm

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County STOKES Instrument Location STOKES COUNTY JAIL

Instrument Serial No. 008596 DANBURY, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 4TH day of AUGUST, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.




Signature of Certifying Official

353799
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

STOKES COUNTY JAIL 840

Serial Number: 008596

Test Date: 08/04/2026

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Oligmueller, Leo A

Permit Number: 0035-3799

Effective:

02/01/2026-02/01/2028

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

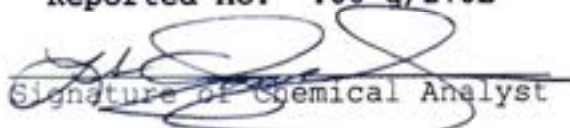
Test Type: Breath Test

Lot Number: AG534301

Exp Date: 12/09/2027

Test	g/210L	Time
DIAG	Pass	9:25am
AIR BLK	.00	9:25am
ACCY CHK	.07	9:26am
AIR BLK	.00	9:27am
SUB TEST	.00	9:28am
AIR BLK	.00	9:28am
SUB TEST	.00	9:30am
AIR BLK	.00	9:31am

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

STOKES COUNTY JAIL 840

Serial Number: 008596 Test Record Number: 1706
Test Date: 08/04/2026 Test Time: 9:32am EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	9:32am
FLO	Pass	9:32am
FC	Pass	9:32am

Temperature Tests

Test	Status	Time
FC1	Pass	9:32am
SRC	Pass	9:32am
DET	Pass	9:32am
BAR	Pass	9:32am
BT	Pass	9:32am

Blank Tests

Test	Status	Time
AIR	Pass	9:33am

Printer Tests

Test	Status	Time
PRNT	Pass	9:33am

CRC Tests

Test	Status	Time
COMP	Pass	9:33am
CAL	Pass	9:33am

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County STOKES Instrument Location KING POLICE DEPARTMENT
Instrument Serial No. 008718 KING, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 4TH day of AUGUST, 2026, the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



A stylized, handwritten signature in black ink, written over a horizontal line. The signature is cursive and appears to be the name of the certifying official.
Signature of Certifying Official

353799
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

STOKES COUNTY KING PD 840

Serial Number: 008718

Test Date: 08/04/2026

Citation Number: M00000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Oligmueller, Leo A

Permit Number: 0035-3799

Effective:

02/01/2026-02/01/2028

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

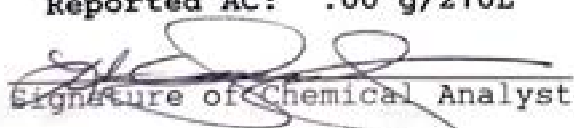
Test Type: Breath Test

Lot Number: AG506301

Exp Date: 03/04/2027

Test	g/210L	Time
DIAG	Pass	11:24am
AIR BLK	.00	11:25am
ACCY CHK	.07	11:25am
AIR BLK	.00	11:26am
SUB TEST	.00	11:27am
AIR BLK	.00	11:28am
SUB TEST	.00	11:31am
AIR BLK	.00	11:32am

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

STOKES COUNTY KING PD 840

Serial Number: 008718 Test Record Number: 2571
Test Date: 08/04/2026 Test Time: 11:35am EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	11:35am
FLO	Pass	11:35am
FC	Pass	11:35am

Temperature Tests

Test	Status	Time
FC1	Pass	11:35am
SRC	Pass	11:35am
DET	Pass	11:35am
BAR	Pass	11:35am
BT	Pass	11:35am

Blank Tests

Test	Status	Time
AIR	Pass	11:36am

Printer Tests

Test	Status	Time
PRNT	Pass	11:36am

CRC Tests

Test	Status	Time
COMP	Pass	11:36am
CAL	Pass	11:36am

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Stokes Instrument Location BAT Mobile Unit 11
Instrument Serial No. 008970

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 28th day of August, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



John Panier
Signature of Certifying Official

1604930
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

STOKES COUNTY BAT MOBILE UNIT 11 840

Serial Number: 008970

Test Date: 08/28/2026

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Lanier Jr., John P

Permit Number: 4582-9118

Effective:

02/01/2026-02/01/2028

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

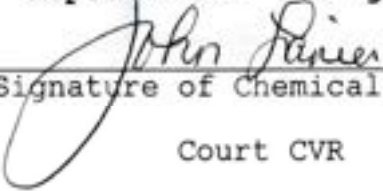
Test Type: Breath Test

Lot Number: AG602101

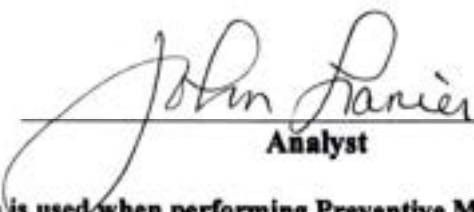
Exp Date: 01/21/2028

Test	g/210L	Time
DIAG	Pass	8:57pm
AIR BLK	.00	8:58pm
ACCY CHK	.07	8:59pm
AIR BLK	.00	9:00pm
SUB TEST	.00	9:01pm
AIR BLK	.00	9:02pm
SUB TEST	.00	9:03pm
AIR BLK	.00	9:04pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

STOKES COUNTY BAT MOBILE UNIT 11 840

Serial Number: 008970 Test Record Number: 1525
Test Date: 08/28/2026 Test Time: 9:08pm EDT

System Check: Passed

Baseline Tests

Test	Status	Time
IR	Pass	9:08pm
FLO	Pass	9:08pm
FC	Pass	9:08pm

Temperature Tests

Test	Status	Time
FC1	Pass	9:08pm
SRC	Pass	9:08pm
DET	Pass	9:08pm
BAR	Pass	9:08pm
BT	Pass	9:08pm

Blank Tests

Test	Status	Time
AIR	Pass	9:09pm

Printer Tests

Test	Status	Time
PRNT	Pass	9:09pm

CRC Tests

Test	Status	Time
COMP	Pass	9:09pm
CAL	Pass	9:09pm

Preventive Maintenance
Status: Pass


Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Stokes Instrument Location BAT Mobile Unit 11

Instrument Serial No. 008973

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 28th day of August, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

1604930
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

STOKES COUNTY BAT MOBILE UNIT 11 840

Serial Number: 008973
Test Date: 08/28/2026

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Lanier Jr., John P

Permit Number: 4582-9118

Effective:

02/01/2026-02/01/2028

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

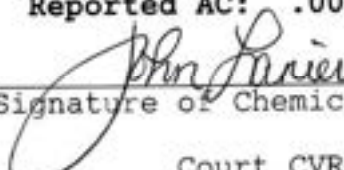
Test Type: Breath Test

Lot Number: AG431003

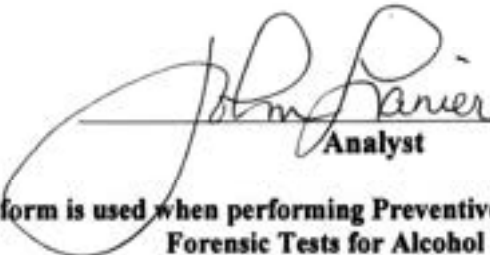
Exp Date: 11/05/2026

Test	g/210L	Time
DIAG	Pass	8:54pm
AIR BLK	.00	8:55pm
ACCY CHK	.07	8:55pm
AIR BLK	.00	8:56pm
SUB TEST	.00	8:57pm
AIR BLK	.00	8:58pm
SUB TEST	.00	9:00pm
AIR BLK	.00	9:01pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

STOKES COUNTY BAT MOBILE UNIT 11 840

Serial Number: 008973 Test Record Number: 1560
Test Date: 08/28/2026 Test Time: 9:01pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	9:02pm
FLO	Pass	9:02pm
FC	Pass	9:02pm

Temperature Tests

Test	Status	Time
FC1	Pass	9:02pm
SRC	Pass	9:02pm
DET	Pass	9:02pm
BAR	Pass	9:02pm
BT	Pass	9:02pm

Blank Tests

Test	Status	Time
AIR	Pass	9:02pm

Printer Tests

Test	Status	Time
PRNT	Pass	9:03pm

CRC Tests

Test	Status	Time
COMP	Pass	9:03pm
CAL	Pass	9:03pm

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County SURRY Instrument Location PILOT MOUNTAIN PO
Instrument Serial No. 008938 PILOT MOUNTAIN, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 4TH day of AUGUST, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.




Signature of Certifying Official

353799
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

SURRY COUNTY PILOT MOUNTAIN PD 850

Serial Number: 008938

Test Date: 08/04/2026

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Oligmueller, Leo A

Permit Number: 0035-3799

Effective:

02/01/2026-02/01/2028

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

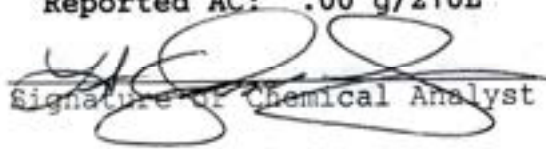
Test Type: Breath Test

Lot Number: AG506301

Exp Date: 03/04/2027

Test	g/210L	Time
DIAG	Pass	10:29am
AIR BLK	.00	10:29am
ACCY CHK	.08	10:30am
AIR BLK	.00	10:31am
SUB TEST	.00	10:32am
AIR BLK	.00	10:33am
SUB TEST	.00	10:34am
AIR BLK	.00	10:35am

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

SURRY COUNTY PILOT MOUNTAIN PD 850

Serial Number: 008938 Test Record Number: 932
Test Date: 08/04/2026 Test Time: 10:37am EDT

System Check: Passed

Baseline Tests

Test	Status	Time
IR	Pass	10:37am
FLO	Pass	10:37am
FC	Pass	10:37am

Temperature Tests

Test	Status	Time
FC1	Pass	10:38am
SRC	Pass	10:38am
DET	Pass	10:38am
BAR	Pass	10:38am
BT	Pass	10:38am

Blank Tests

Test	Status	Time
AIR	Pass	10:38am

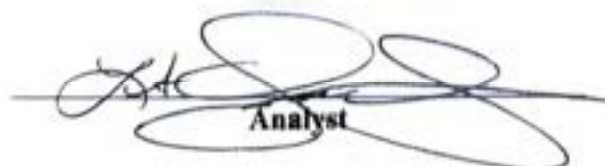
Printer Tests

Test	Status	Time
PRNT	Pass	10:38am

CRC Tests

Test	Status	Time
COMP	Pass	10:38am
CAL	Pass	10:38am

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Swain Instrument Location Swain County Jail
Instrument Serial No. 008723 Bryson City, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 27 day of August, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

244987
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

SWAIN COUNTY JAIL 860

Serial Number: 008723

Test Date: 08/27/2026

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Loftis, Benjamin C

Permit Number: 0024-4987

Effective:

02/01/2026-02/01/2028

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

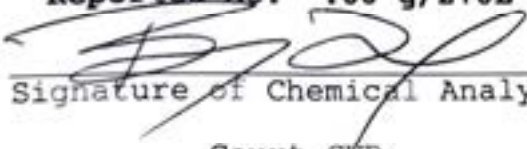
Test Type: Breath Test

Lot Number: AG505001

Exp Date: 02/19/2027

Test	g/210L	Time
DIAG	Pass	1:47pm
AIR BLK	.00	1:47pm
ACCY CHK	.08	1:48pm
AIR BLK	.00	1:49pm
SUB TEST	.00	1:50pm
AIR BLK	.00	1:51pm
SUB TEST	.00	1:52pm
AIR BLK	.00	1:53pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

SWAIN COUNTY JAIL 860

Serial Number: 008723 Test Record Number: 970
Test Date: 08/27/2026 Test Time: 1:55pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	1:55pm
FLO	Pass	1:55pm
FC	Pass	1:55pm

Temperature Tests

Test	Status	Time
FC1	Pass	1:55pm
SRC	Pass	1:55pm
DET	Pass	1:55pm
BAR	Pass	1:55pm
BT	Pass	1:55pm

Blank Tests

Test	Status	Time
AIR	Pass	1:56pm

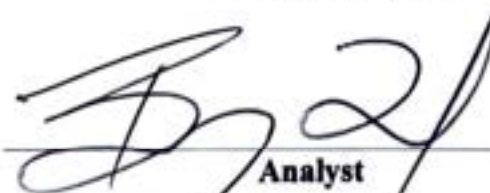
Printer Tests

Test	Status	Time
PRNT	Pass	1:56pm

CRC Tests

Test	Status	Time
COMP	Pass	1:56pm
CAL	Pass	1:56pm

Preventive Maintenance
Status: Pass


Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Swain Instrument Location Swain County Jail
Instrument Serial No. 008727 Bryson City, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 27 day of August, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

244987
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

SWAIN COUNTY JAIL 860

Serial Number: 008727

Test Date: 08/27/2026

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Loftis, Benjamin C

Permit Number: 0024-4987

Effective:

02/01/2026-02/01/2028

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

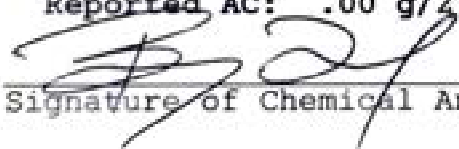
Test Type: Breath Test

Lot Number: AG503001

Exp Date: 01/30/2027

Test	g/210L	Time
DIAG	Pass	1:46pm
AIR BLK	.00	1:47pm
ACCY CHK	.07	1:48pm
AIR BLK	.00	1:49pm
SUB TEST	.00	1:49pm
AIR BLK	.00	1:50pm
SUB TEST	.00	1:52pm
AIR BLK	.00	1:53pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

This form is used when performing Preventive Maintenance procedures

Forensic Tests for Alcohol Branch

Department of Health and Human Services

Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

SWAIN COUNTY JAIL 860

Serial Number: 008727 Test Record Number: 1759
Test Date: 08/27/2026 Test Time: 1:54pm EDT

System Check: Passed

Baseline Tests

Test	Status	Time
IR	Pass	1:55pm
FLO	Pass	1:55pm
FC	Pass	1:55pm

Temperature Tests

Test	Status	Time
FC1	Pass	1:55pm
SRC	Pass	1:55pm
DET	Pass	1:55pm
BAR	Pass	1:55pm
BT	Pass	1:55pm

Blank Tests

Test	Status	Time
AIR	Pass	1:56pm

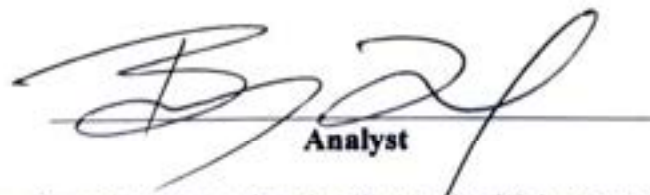
Printer Tests

Test	Status	Time
PRNT	Pass	1:56pm

CRC Tests

Test	Status	Time
COMP	Pass	1:56pm
CAL	Pass	1:56pm

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Swain Instrument Location Cherokee Tribal Detention
Instrument Serial No. 008782 Cherokee, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 27 day of August, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

244987
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

SWAIN COUNTY CHEROKEE DETENTION 860

Serial Number: 008782
Test Date: 08/27/2026

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Loftis, Benjamin C

Permit Number: 0024-4987

Effective:

02/01/2026-02/01/2028

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

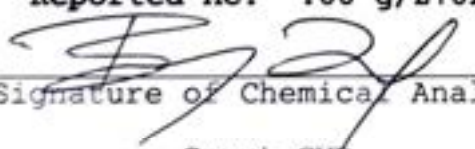
Test Type: Breath Test

Lot Number: AG505001

Exp Date: 02/19/2027

Test	g/210L	Time
DIAG	Pass	2:39pm
AIR BLK	.00	2:40pm
ACCY CHK	.07	2:40pm
AIR BLK	.00	2:42pm
SUB TEST	.00	2:42pm
AIR BLK	.00	2:43pm
SUB TEST	.00	2:44pm
AIR BLK	.00	2:45pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

This form is used when performing Preventive Maintenance procedures

Forensic Tests for Alcohol Branch

Department of Health and Human Services

Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

SWAIN COUNTY CHEROKEE DETENTION 860

Serial Number: 008782 Test Record Number: 1680
Test Date: 08/27/2026 Test Time: 2:45pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	2:46pm
FLO	Pass	2:46pm
FC	Pass	2:46pm

Temperature Tests

Test	Status	Time
FC1	Pass	2:46pm
SRC	Pass	2:46pm
DET	Pass	2:46pm
BAR	Pass	2:46pm
BT	Pass	2:46pm

Blank Tests

Test	Status	Time
AIR	Pass	2:47pm

Printer Tests

Test	Status	Time
PRNT	Pass	2:47pm

CRC Tests

Test	Status	Time
COMP	Pass	2:47pm
CAL	Pass	2:47pm

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Tyrrell Instrument Location Tyrrell Co. S.O.
Instrument Serial No. 008902 Columbia, N.C.

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 5th day of August, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

377722
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

TYRRELL COUNTY SHERIFF'S OFFICE 880

Serial Number: 008902
Test Date: 08/05/2026

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Gray, Kelly D

Permit Number: 0037-7722

Effective:

02/01/2026-02/01/2028

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG516204

Exp Date: 06/11/2027

Test	g/210L	Time
DIAG	Pass	11:06am
AIR BLK	.00	11:06am
ACCY CHK	.07	11:07am
AIR BLK	.00	11:08am
SUB TEST	.00	11:09am
AIR BLK	.00	11:10am
SUB TEST	.00	11:12am
AIR BLK	.00	11:12am

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

Intox EC/IR-II: Preventive Maintenance

TYRRELL COUNTY SHERIFF'S OFFICE 880

Serial Number: 008902 Test Record Number: 1303
Test Date: 08/05/2026 Test Time: 11:13am EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	11:13am
FLO	Pass	11:13am
FC	Pass	11:13am

Temperature Tests

Test	Status	Time
FC1	Pass	11:14am
SRC	Pass	11:14am
DET	Pass	11:14am
BAR	Pass	11:14am
BT	Pass	11:14am

Blank Tests

Test	Status	Time
AIR	Pass	11:14am


Printer Tests

Test	Status	Time
PRNT	Pass	11:14am

CRC Tests

Test	Status	Time
COMP	Pass	11:14am
CAL	Pass	11:14am

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Union Instrument Location Union County & Monroe, NC
Instrument Serial No. 0088606

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 21st day of August, 2024 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

849845
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

UNION COUNTY UNION COUNTY SO 890

Serial Number: 008866
Test Date: 08/21/2026

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Helms, Bryce A

Permit Number: 0084-9845

Effective:

02/01/2026-02/01/2028

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG602101

Exp Date: 01/21/2028

Test	g/210L	Time
DIAG	Pass	12:05pm
AIR BLK	.00	12:05pm
ACCY CHK	.07	12:06pm
AIR BLK	.00	12:07pm
SUB TEST	.00	12:07pm
AIR BLK	.00	12:08pm
SUB TEST	.00	12:10pm
AIR BLK	.00	12:11pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

Intox EC/IR-II: Preventive Maintenance

UNION COUNTY UNION COUNTY SO 890

Serial Number: 008866 Test Record Number: 5085
Test Date: 08/21/2026 Test Time: 12:11pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	12:12pm
FLO	Pass	12:12pm
FC	Pass	12:12pm

Temperature Tests

Test	Status	Time
FC1	Pass	12:12pm
SRC	Pass	12:12pm
DET	Pass	12:12pm
BAR	Pass	12:12pm
BT	Pass	12:12pm

Blank Tests

Test	Status	Time
AIR	Pass	12:12pm

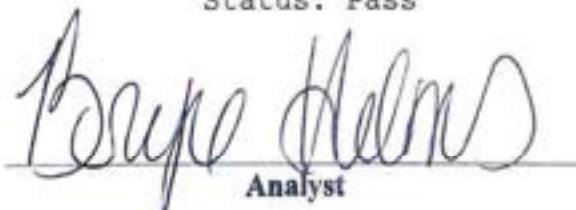
Printer Tests

Test	Status	Time
PRNT	Pass	12:13pm

CRC Tests

Test	Status	Time
COMP	Pass	12:13pm
CAL	Pass	12:13pm

Preventive Maintenance
Status: *Pass*


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Union Instrument Location Union County &
Monroe, NC
Instrument Serial No. 008876

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 21st day of August, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

849845
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

UNION COUNTY UNION COUNTY SO 890

Serial Number: 008876
Test Date: 08/21/2026

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Helms, Bryce A

Permit Number: 0084-9845

Effective:

02/01/2026-02/01/2028

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG602202

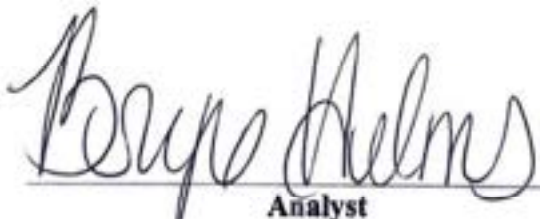
Exp Date: 01/22/2028

Test	g/210L	Time
DIAG	Pass	11:57am
AIR BLK	.00	11:58am
ACCY CHK	.08	11:58am
AIR BLK	.00	12:00pm
SUB TEST	.00	12:01pm
AIR BLK	.00	12:02pm
SUB TEST	.00	12:03pm
AIR BLK	.00	12:04pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

Intox EC/IR-II: Preventive Maintenance

UNION COUNTY UNION COUNTY SO 890

Serial Number: 008876 Test Record Number: 7868
Test Date: 08/21/2026 Test Time: 12:05pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	12:06pm
FLO	Pass	12:06pm
FC	Pass	12:06pm

Temperature Tests

Test	Status	Time
FC1	Pass	12:06pm
SRC	Pass	12:06pm
DET	Pass	12:06pm
BAR	Pass	12:06pm
BT	Pass	12:06pm

Blank Tests

Test	Status	Time
AIR	Pass	12:07pm

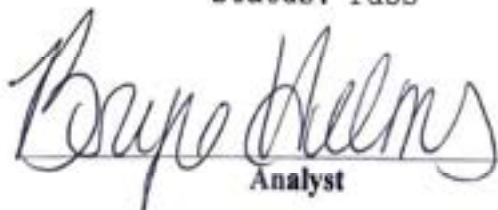
Printer Tests

Test	Status	Time
PRNT	Pass	12:07pm

CRC Tests

Test	Status	Time
COMP	Pass	12:07pm
CAL	Pass	12:07pm

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County WAKE Instrument Location Wake County Detention Center

Instrument Serial No. 008577 Raleigh, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 4 day of August, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]

Signature of Certifying Official

169451

Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

WAKE COUNTY DETENTION CENTER 910

Serial Number: 008577

Test Date: 08/04/2026

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Brame, Bryant T

Permit Number: 0016-9451

Effective:

04/01/2026-04/01/2028

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG534301

Exp Date: 12/09/2027

Test	g/210L	Time
DIAG	Pass	11:38am
AIR BLK	.00	11:39am
ACCY CHK	.08	11:40am
AIR BLK	.00	11:41am
SUB TEST	.00	11:42am
AIR BLK	.00	11:43am
SUB TEST	.00	11:44am
AIR BLK	.00	11:45am

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

WAKE COUNTY DETENTION CENTER 910

Serial Number: 008577 Test Record Number: 9681
Test Date: 08/04/2026 Test Time: 11:46am EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	11:46am
FLO	Pass	11:46am
FC	Pass	11:46am

Temperature Tests

Test	Status	Time
FC1	Pass	11:46am
SRC	Pass	11:46am
DET	Pass	11:46am
BAR	Pass	11:46am
BT	Pass	11:46am

Blank Tests

Test	Status	Time
AIR	Pass	11:47am

Printer Tests

Test	Status	Time
PRNT	Pass	11:47am

CRC Tests

Test	Status	Time
COMP	Pass	11:47am
CAL	Pass	11:47am

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Wake Instrument Location BAT Mobile Unit 10

Instrument Serial No. 006584

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 8 day of August, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]

Signature of Certifying Official

193459

Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

WAKE COUNTY BAT MOBILE UNIT 10 910

Serial Number: 008584

Test Date: 08/08/2026

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Carroll, Barry Jean D

Permit Number: 0019-3759

Effective:

04/01/2026-04/01/2028

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG534301

Exp Date: 12/09/2027

Test	g/210L	Time
DIAG	Pass	9:24pm
AIR BLK	.00	9:25pm
ACCY CHK	.08	9:25pm
AIR BLK	.00	9:26pm
SUB TEST	.00	9:27pm
AIR BLK	.00	9:28pm
SUB TEST	.00	9:29pm
AIR BLK	.00	9:30pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

WAKE COUNTY BAT MOBILE UNIT 10 910

Serial Number: 008584 Test Record Number: 2940
Test Date: 08/08/2026 Test Time: 9:31pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	9:31pm
FLO	Pass	9:31pm
FC	Pass	9:31pm

Temperature Tests

Test	Status	Time
FC1	Pass	9:32pm
SRC	Pass	9:32pm
DET	Pass	9:32pm
BAR	Pass	9:32pm
BT	Pass	9:32pm

Blank Tests

Test	Status	Time
AIR	Pass	9:32pm

Printer Tests

Test	Status	Time
PRNT	Pass	9:32pm

CRC Tests

Test	Status	Time
COMP	Pass	9:32pm
CAL	Pass	9:32pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Wake Instrument Location BAT Mobile Unit 10

Instrument Serial No. 008584

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 21 day of August, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



A handwritten signature in black ink, appearing to be "J. B. [unclear]".

Signature of Certifying Official

193759

Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

WAKE COUNTY BAT MOBILE UNIT 10 910

Serial Number: 008584

Test Date: 08/21/2026

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Carroll, Barry Jean D

Permit Number: 0019-3759

Effective:

04/01/2026-04/01/2028

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG534301

Exp Date: 12/09/2027

Test	g/210L	Time
DIAG	Pass	8:22pm
AIR BLK	.00	8:23pm
ACCY CHK	.08	8:24pm
AIR BLK	.00	8:24pm
SUB TEST	.00	8:25pm
AIR BLK	.00	8:26pm
SUB TEST	.00	8:27pm
AIR BLK	.00	8:28pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

Intox EC/IR-II: Preventive Maintenance

WAKE COUNTY BAT MOBILE UNIT 10 910

Serial Number: 008584 Test Record Number: 2946
Test Date: 08/21/2026 Test Time: 8:30pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	8:30pm
FLO	Pass	8:30pm
FC	Pass	8:30pm

Temperature Tests

Test	Status	Time
FC1	Pass	8:30pm
SRC	Pass	8:30pm
DET	Pass	8:30pm
BAR	Pass	8:30pm
BT	Pass	8:30pm

Blank Tests

Test	Status	Time
AIR	Pass	8:31pm

Printer Tests

Test	Status	Time
PRNT	Pass	8:31pm

CRC Tests

Test	Status	Time
COMP	Pass	8:31pm
CAL	Pass	8:31pm

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Wake Instrument Location BAT Mobile unit 10

Instrument Serial No. 008584

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 28 day of August, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]

Signature of Certifying Official

193759

Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

WAKE COUNTY BAT MOBILE UNIT 10 910

Serial Number: 008584

Test Date: 08/28/2026

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Carroll, Barry Jean D

Permit Number: 0019-3759

Effective:

04/01/2026-04/01/2028

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG534301

Exp Date: 12/09/2027

Test	g/210L	Time
DIAG	Pass	8:34pm
AIR BLK	.00	8:35pm
ACCY CHK	.08	8:35pm
AIR BLK	.00	8:36pm
SUB TEST	.00	8:37pm
AIR BLK	.00	8:38pm
SUB TEST	.00	8:39pm
AIR BLK	.00	8:40pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

WAKE COUNTY BAT MOBILE UNIT 10 910

Serial Number: 008584 Test Record Number: 2948
Test Date: 08/28/2026 Test Time: 8:41pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	8:41pm
FLO	Pass	8:41pm
FC	Pass	8:41pm

Temperature Tests

Test	Status	Time
FC1	Pass	8:41pm
SRC	Pass	8:41pm
DET	Pass	8:41pm
BAR	Pass	8:41pm
BT	Pass	8:41pm

Blank Tests

Test	Status	Time
AIR	Pass	8:42pm

Printer Tests

Test	Status	Time
PRNT	Pass	8:42pm

CRC Tests

Test	Status	Time
COMP	Pass	8:42pm
CAL	Pass	8:42pm

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County NACE Instrument Location BAT Mobile Unit 10

Instrument Serial No. 008637

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 21 day of August, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.





Signature of Certifying Official

193759

Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

WAKE COUNTY BAT MOBILE UNIT 10 910

Serial Number: 008637

Test Date: 08/21/2026

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Carroll, Barry Jean D

Permit Number: 0019-3759

Effective:

04/01/2026-04/01/2028

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG602101

Exp Date: 01/21/2028

Test	g/210L	Time
DIAG	Pass	8:37pm
AIR BLK	.00	8:38pm
ACCY CHK	.07	8:38pm
AIR BLK	.00	8:39pm
SUB TEST	.00	8:40pm
AIR BLK	.00	8:41pm
SUB TEST	.00	8:42pm
AIR BLK	.00	8:43pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

WAKE COUNTY BAT MOBILE UNIT 10 910

Serial Number: 008637 Test Record Number: 3643
Test Date: 08/21/2026 Test Time: 8:45pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	8:45pm
FLO	Pass	8:45pm
FC	Pass	8:45pm

Temperature Tests

Test	Status	Time
FC1	Pass	8:46pm
SRC	Pass	8:46pm
DET	Pass	8:46pm
BAR	Pass	8:46pm
BT	Pass	8:46pm

Blank Tests

Test	Status	Time
AIR	Pass	8:46pm

Printer Tests

Test	Status	Time
PRNT	Pass	8:46pm

CRC Tests

Test	Status	Time
COMP	Pass	8:46pm
CAL	Pass	8:46pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Wake

Instrument Location BPT Mobile Unit 10

Instrument Serial No. 008637

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 28 day of August, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]

Signature of Certifying Official

193759

Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

WAKE COUNTY BAT MOBILE UNIT 10 910

Serial Number: 008637

Test Date: 08/28/2026

Citation Number: M00000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Carroll, Barry Jean D

Permit Number: 0019-3759

Effective:

04/01/2026-04/01/2028

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG602101

Exp Date: 01/21/2028

Test	g/210L	Time
DIAG	Pass	9:01pm
AIR BLK	.00	9:02pm
ACCY CHK	.07	9:03pm
AIR BLK	.00	9:04pm
SUB TEST	.00	9:05pm
AIR BLK	.00	9:06pm
SUB TEST	.00	9:07pm
AIR BLK	.00	9:08pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

Intox EC/IR-II: Preventive Maintenance

WAKE COUNTY BAT MOBILE UNIT 10 910

Serial Number: 008637 Test Record Number: 3645

Test Date: 08/28/2026 Test Time: 9:08pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	9:09pm
FLO	Pass	9:09pm
FC	Pass	9:09pm

Temperature Tests

Test	Status	Time
FC1	Pass	9:09pm
SRC	Pass	9:09pm
DET	Pass	9:09pm
BAR	Pass	9:09pm
BT	Pass	9:09pm

Blank Tests

Test	Status	Time
AIR	Pass	9:09pm

Printer Tests

Test	Status	Time
PRNT	Pass	9:10pm

CRC Tests

Test	Status	Time
COMP	Pass	9:10pm
CAL	Pass	9:10pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Wake

Instrument Location BAT Mobile unit 10

Instrument Serial No. 008686

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 8 day of August, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]

Signature of Certifying Official

193759

Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

WAKE COUNTY BAT MOBILE UNIT 10 910

Serial Number: 008686

Test Date: 08/08/2026

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Carroll, Barry Jean D

Permit Number: 0019-3759

Effective:

04/01/2026-04/01/2028

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG506302

Exp Date: 03/04/2027

Test	g/210L	Time
DIAG	Pass	9:22pm
AIR BLK	.00	9:23pm
ACCY CHK	.08	9:23pm
AIR BLK	.00	9:24pm
SUB TEST	.00	9:24pm
AIR BLK	.00	9:25pm
SUB TEST	.00	9:27pm
AIR BLK	.00	9:28pm

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR

Analyst

Intox EC/IR-II: Preventive Maintenance

WAKE COUNTY BAT MOBILE UNIT 10 910

Serial Number: 008686 Test Record Number: 7287
Test Date: 08/08/2026 Test Time: 9:28pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	9:29pm
FLO	Pass	9:29pm
FC	Pass	9:29pm

Temperature Tests

Test	Status	Time
FC1	Pass	9:29pm
SRC	Pass	9:29pm
DET	Pass	9:29pm
BAR	Pass	9:29pm
BT	Pass	9:29pm

Blank Tests

Test	Status	Time
AIR	Pass	9:29pm

Printer Tests

Test	Status	Time
PRNT	Pass	9:29pm

CRC Tests

Test	Status	Time
COMP	Pass	9:30pm
CAL	Pass	9:30pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Wake Instrument Location BAT Mobile unit 10

Instrument Serial No. 008686

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 21 day of August, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



A handwritten signature in black ink, appearing to be "B. J. [unclear]".

Signature of Certifying Official

193759

Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

WAKE COUNTY BAT MOBILE UNIT 10 910

Serial Number: 008686

Test Date: 08/21/2026

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Carroll, Barry Jean D

Permit Number: 0019-3759

Effective:

04/01/2026-04/01/2028

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG506302

Exp Date: 03/04/2027

Test	g/210L	Time
DIAG	Pass	8:41pm
AIR BLK	.00	8:42pm
ACCY CHK	.08	8:43pm
AIR BLK	.00	8:44pm
SUB TEST	.00	8:44pm
AIR BLK	.00	8:45pm
SUB TEST	.00	8:47pm
AIR BLK	.00	8:48pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

WAKE COUNTY BAT MOBILE UNIT 10 910

Serial Number: 008686 Test Record Number: 7289
Test Date: 08/21/2026 Test Time: 8:49pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	8:49pm
FLO	Pass	8:49pm
FC	Pass	8:50pm

Temperature Tests

Test	Status	Time
FC1	Pass	8:50pm
SRC	Pass	8:50pm
DET	Pass	8:50pm
BAR	Pass	8:50pm
BT	Pass	8:50pm

Blank Tests

Test	Status	Time
AIR	Pass	8:50pm

Printer Tests

Test	Status	Time
PRNT	Pass	8:50pm

CRC Tests

Test	Status	Time
COMP	Pass	8:51pm
CAL	Pass	8:51pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Wake

Instrument Location BAT Mobile Unit 10

Instrument Serial No. 008686

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 28 day of August, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

143759
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

WAKE COUNTY BAT MOBILE UNIT 10 910

Serial Number: 008686.

Test Date: 08/28/2026

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Carroll, Barry Jean D

Permit Number: 0019-3759

Effective:

04/01/2026-04/01/2028

Officer's Name: NONE, NONE

Type of Agency: PTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG506302

Exp Date: 03/04/2027

Test	g/210L	Time
DIAG	Pass	8:41pm
AIR BLK	.00	8:42pm
ACCY CHK	.08	8:43pm
AIR BLK	.00	8:44pm
SUB TEST	.00	8:45pm
AIR BLK	.00	8:45pm
SUB TEST	.00	8:48pm
AIR BLK	.00	8:48pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

WAKE COUNTY BAT MOBILE UNIT 10 910

Serial Number: 008686 Test Record Number: 7291
Test Date: 08/28/2026 Test Time: 8:54pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	8:55pm
FLO	Pass	8:55pm
FC	Pass	8:55pm

Temperature Tests

Test	Status	Time
FC1	Pass	8:55pm
SRC	Pass	8:55pm
DET	Pass	8:55pm
BAR	Pass	8:55pm
BT	Pass	8:55pm

Blank Tests

Test	Status	Time
AIR	Pass	8:56pm

Printer Tests

Test	Status	Time
PRNT	Pass	8:56pm

CRC Tests

Test	Status	Time
COMP	Pass	8:56pm
CAL	Pass	8:56pm

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Wake

Instrument Location BAT mobile unit 10

Instrument Serial No. C 08 776

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 8 day of August, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

193759
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

WAKE COUNTY BAT MOBILE UNIT 10 910

Serial Number: 008776

Test Date: 08/08/2026

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Carroll, Barry Jean D

Permit Number: 0019-3759

Effective:

04/01/2026-04/01/2028

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG534301

Exp Date: 12/09/2027

Test	g/210L	Time
DIAG	Pass	9:19pm
AIR BLK	.00	9:20pm
ACCY CHK	.08	9:21pm
AIR BLK	.00	9:22pm
SUB TEST	.00	9:22pm
AIR BLK	.00	9:23pm
SUB TEST	.00	9:25pm
AIR BLK	.00	9:25pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

Intox EC/IR-II: Preventive Maintenance

WAKE COUNTY BAT MOBILE UNIT 10 910

Serial Number: 008776 Test Record Number: 4265
Test Date: 08/08/2026 Test Time: 9:26pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	9:26pm
FLO	Pass	9:26pm
FC	Pass	9:26pm

Temperature Tests

Test	Status	Time
FC1	Pass	9:26pm
SRC	Pass	9:26pm
DET	Pass	9:26pm
BAR	Pass	9:26pm
BT	Pass	9:26pm

Blank Tests

Test	Status	Time
AIR	Pass	9:27pm

Printer Tests

Test	Status	Time
PRNT	Pass	9:27pm

CRC Tests

Test	Status	Time
COMP	Pass	9:27pm
CAL	Pass	9:27pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Wake Instrument Location BAT Mobile unit 10

Instrument Serial No. 008776

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 21 day of August, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Signature of Certifying Official

193759

Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

WAKE COUNTY BAT MOBILE UNIT 10 910

Serial Number: 008776

Test Date: 08/21/2026

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Carroll, Barry Jean D

Permit Number: 0019-3759

Effective:

04/01/2026-04/01/2028

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG534301

Exp Date: 12/09/2027

Test	g/210L	Time
DIAG	Pass	8:29pm
AIR BLK	.00	8:30pm
ACCY CHK	.08	8:31pm
AIR BLK	.00	8:31pm
SUB TEST	.00	8:32pm
AIR BLK	.00	8:33pm
SUB TEST	.00	8:34pm
AIR BLK	.00	8:35pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

Intox EC/IR-II: Preventive Maintenance

WAKE COUNTY BAT MOBILE UNIT 10 910

Serial Number: 008776 Test Record Number: 4268
Test Date: 08/21/2026 Test Time: 8:36pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	8:36pm
FLO	Pass	8:36pm
FC	Pass	8:36pm

Temperature Tests

Test	Status	Time
FC1	Pass	8:36pm
SRC	Pass	8:36pm
DET	Pass	8:36pm
BAR	Pass	8:36pm
BT	Pass	8:36pm

Blank Tests

Test	Status	Time
AIR	Pass	8:37pm

Printer Tests

Test	Status	Time
PRNT	Pass	8:37pm

CRC Tests

Test	Status	Time
COMP	Pass	8:37pm
CAL	Pass	8:37pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Wake Instrument Location BAT Mobile Unit 10

Instrument Serial No. 008776

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 28 day of August, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

193759
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

WAKE COUNTY BAT MOBILE UNIT 10 910

Serial Number: 008776

Test Date: 08/28/2026

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Carroll, Barry Jean D

Permit Number: 0019-3759

Effective:

04/01/2026-04/01/2028

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG534301

Exp Date: 12/09/2027

Test	g/210L	Time
DIAG	Pass	8:38pm
AIR BLK	.00	8:39pm
ACCY CHK	.08	8:40pm
AIR BLK	.00	8:41pm
SUB TEST	.00	8:41pm
AIR BLK	.00	8:42pm
SUB TEST	.00	8:44pm
AIR BLK	.00	8:45pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

Intox EC/IR-II: Preventive Maintenance

WAKE COUNTY BAT MOBILE UNIT 10 910

Serial Number: 008776 Test Record Number: 4271
Test Date: 08/28/2026 Test Time: 8:47pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	8:48pm
FLO	Pass	8:48pm
FC	Pass	8:48pm

Temperature Tests

Test	Status	Time
FC1	Pass	8:48pm
SRC	Pass	8:48pm
DET	Pass	8:48pm
BAR	Pass	8:48pm
BT	Pass	8:48pm

Blank Tests

Test	Status	Time
AIR	Pass	8:49pm

Printer Tests

Test	Status	Time
PRNT	Pass	8:49pm

CRC Tests

Test	Status	Time
COMP	Pass	8:49pm
CAL	Pass	8:49pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County WAKE Instrument Location Wake County Detention Center
Instrument Serial No. 008778 Raleigh, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 4 day of August, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

169451

Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

WAKE COUNTY DETENTION CENTER 910

Serial Number: 008778

Test Date: 08/04/2026

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Brame, Bryant T

Permit Number: 0016-9451

Effective:

04/01/2026-04/01/2028

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG534301


Exp Date: 12/09/2027

Test	g/210L	Time
DIAG	Pass	11:41am
AIR BLK	.00	11:42am
ACCY CHK	.07	11:43am
AIR BLK	.00	11:44am
SUB TEST	.00	11:44am
AIR BLK	.00	11:45am
SUB TEST	.00	11:47am
AIR BLK	.00	11:48am

Reported AC: 00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

WAKE COUNTY DETENTION CENTER 910

Serial Number: 008778 Test Record Number: 9260
Test Date: 08/04/2026 Test Time: 11:49am EDT

System Check: Passed

Baseline Tests

Test	Status	Time
IR	Pass	11:49am
FLO	Pass	11:49am
FC	Pass	11:49am

Temperature Tests

Test	Status	Time
FC1	Pass	11:49am
SRC	Pass	11:49am
DET	Pass	11:49am
BAR	Pass	11:49am
BT	Pass	11:49am

Blank Tests

Test	Status	Time
AIR	Pass	11:50am

Printer Tests

Test	Status	Time
PRNT	Pass	11:50am

CRC Tests

Test	Status	Time
COMP	Pass	11:50am
CAL	Pass	11:50am

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Wake Instrument Location BAT Mobile unit 10

Instrument Serial No. 006779

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 8 day of August, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

193759
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

WAKE COUNTY BAT MOBILE UNIT 10 910

Serial Number: 008779

Test Date: 08/08/2026

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Carroll, Barry Jean D

Permit Number: 0019-3759

Effective:

04/01/2026-04/01/2028

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG431002

Exp Date: 11/05/2026

Test	g/210L	Time
DIAG	Pass	9:18pm
AIR BLK	.00	9:19pm
ACCY CHK	.08	9:20pm
AIR BLK	.00	9:21pm
SUB TEST	.00	9:22pm
AIR BLK	.00	9:23pm
SUB TEST	.00	9:24pm
AIR BLK	.00	9:25pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

WAKE COUNTY BAT MOBILE UNIT 10 910

Serial Number: 008779 Test Record Number: 4182
Test Date: 08/08/2026 Test Time: 9:26pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	9:26pm
FLO	Pass	9:26pm
FC	Pass	9:26pm

Temperature Tests

Test	Status	Time
FC1	Pass	9:26pm
SRC	Pass	9:26pm
DET	Pass	9:26pm
BAR	Pass	9:26pm
BT	Pass	9:26pm

Blank Tests

Test	Status	Time
AIR	Pass	9:27pm

Printer Tests

Test	Status	Time
PRNT	Pass	9:27pm

CRC Tests

Test	Status	Time
COMP	Pass	9:27pm
CAL	Pass	9:27pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Wake Instrument Location BAT Mobile Unit 10

Instrument Serial No. 008779

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 21 day of August, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



A handwritten signature in black ink, appearing to be "B. J. [unclear]".

Signature of Certifying Official

193759

Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

WAKE COUNTY BAT MOBILE UNIT 10 910

Serial Number: 008779

Test Date: 08/21/2026

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Carroll, Barry Jean D

Permit Number: 0019-3759

Effective:

04/01/2026-04/01/2028

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG431002

Exp Date: 11/05/2026

Test	g/210L	Time
DIAG	Pass	8:31pm
AIR BLK	.00	8:31pm
ACCY CHK	.08	8:32pm
AIR BLK	.00	8:33pm
SUB TEST	.00	8:34pm
AIR BLK	.00	8:35pm
SUB TEST	.00	8:36pm
AIR BLK	.00	8:37pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

WAKE COUNTY BAT MOBILE UNIT 10 910

Serial Number: 008779 Test Record Number: 4186
Test Date: 08/21/2026 Test Time: 8:37pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	8:38pm
FLO	Pass	8:38pm
FC	Pass	8:38pm

Temperature Tests

Test	Status	Time
FC1	Pass	8:38pm
SRC	Pass	8:38pm
DET	Pass	8:38pm
BAR	Pass	8:38pm
BT	Pass	8:38pm

Blank Tests

Test	Status	Time
AIR	Pass	8:38pm

Printer Tests

Test	Status	Time
PRNT	Pass	8:38pm

CRC Tests

Test	Status	Time
COMP	Pass	8:39pm
CAL	Pass	8:39pm

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Wake Instrument Location BAT Mobile Unit 10

Instrument Serial No. 008779

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 28 day of August, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.





Signature of Certifying Official

193759
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

WAKE COUNTY BAT MOBILE UNIT 10 910

Serial Number: 008779

Test Date: 08/28/2026

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Carroll, Barry Jean D

Permit Number: 0019-3759

Effective:

04/01/2026-04/01/2028

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG431002

Exp Date: 11/05/2026

Test	g/210L	Time
DIAG	Pass	8:36pm
AIR BLK	.00	8:37pm
ACCY CHK	.08	8:38pm
AIR BLK	.00	8:39pm
SUB TEST	.00	8:40pm
AIR BLK	.00	8:40pm
SUB TEST	.00	8:42pm
AIR BLK	.00	8:43pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

Intox EC/IR-II: Preventive Maintenance

WAKE COUNTY BAT MOBILE UNIT 10 910

Serial Number: 008779 Test Record Number: 4188
Test Date: 08/28/2026 Test Time: 8:45pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	8:45pm
FLO	Pass	8:45pm
FC	Pass	8:46pm

Temperature Tests

Test	Status	Time
FC1	Pass	8:46pm
SRC	Pass	8:46pm
DET	Pass	8:46pm
BAR	Pass	8:46pm
BT	Pass	8:46pm

Blank Tests

Test	Status	Time
AIR	Pass	8:46pm

Printer Tests

Test	Status	Time
PRNT	Pass	8:46pm

CRC Tests

Test	Status	Time
COMP	Pass	8:46pm
CAL	Pass	8:46pm

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Wake Instrument Location Wake County Detention Center
Instrument Serial No. 008724 Raleigh, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 4 day of August, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Deputy J. L. L.
Signature of Certifying Official

169451
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

WAKE COUNTY DETENTION CENTER 910

Serial Number: 008924
Test Date: 08/04/2026

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Brame, Bryant T

Permit Number: 0016-9451

Effective:

04/01/2026-04/01/2028

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG534301

Exp Date: 12/09/2027

Test	g/210L	Time
DIAG	Pass	12:41pm
AIR BLK	.00	12:42pm
ACCY CHK	.07	12:42pm
AIR BLK	.00	12:43pm
SUB TEST	.00	12:44pm
AIR BLK	.00	12:45pm
SUB TEST	.00	12:47pm
AIR BLK	.00	12:48pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

WAKE COUNTY DETENTION CENTER 910

Serial Number: 008924 Test Record Number: 2125
Test Date: 08/04/2026 Test Time: 12:48pm EDT

System Check: Passed

Baseline Tests

Test	Status	Time
IR	Pass	12:49pm
FLO	Pass	12:49pm
FC	Pass	12:49pm

Temperature Tests

Test	Status	Time
FC1	Pass	12:49pm
SRC	Pass	12:49pm
DET	Pass	12:49pm
BAR	Pass	12:49pm
BT	Pass	12:49pm

Blank Tests

Test	Status	Time
AIR	Pass	12:50pm

Printer Tests

Test	Status	Time
PRNT	Pass	12:50pm

CRC Tests

Test	Status	Time
COMP	Pass	12:50pm
CAL	Pass	12:50pm

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Washington Instrument Location Washington Co. S.O.
Instrument Serial No. 008829 Plymouth, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 5th day of August, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Ky Perry
Signature of Certifying Official

377722
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

WASHINGTON COUNTY SHERIFF'S OFFICE 930

Serial Number: 008829

Test Date: 08/05/2026

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Gray, Kelly D

Permit Number: 0037-7722

Effective:

02/01/2026-02/01/2028

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG506301

Exp Date: 03/04/2027

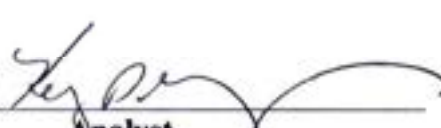
Test	g/210L	Time
DIAG	Pass	12:41pm
AIR BLK	.00	12:42pm
ACCY CHK	.08	12:42pm
AIR BLK	.00	12:44pm
SUB TEST	.00	12:44pm
AIR BLK	.00	12:45pm
SUB TEST	.00	12:47pm
AIR BLK	.00	12:48pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

WASHINGTON COUNTY SHERIFF'S OFFICE 930

Serial Number: 008829 Test Record Number: 1353
Test Date: 08/05/2026 Test Time: 12:49pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	12:49pm
FLO	Pass	12:49pm
FC	Pass	12:49pm

Temperature Tests

Test	Status	Time
FC1	Pass	12:50pm
SRC	Pass	12:50pm
DET	Pass	12:50pm
BAR	Pass	12:50pm
BT	Pass	12:50pm

Blank Tests

Test	Status	Time
AIR	Pass	12:50pm

Printer Tests

Test	Status	Time
PRNT	Pass	12:50pm

CRC Tests

Test	Status	Time
COMP	Pass	12:50pm
CAL	Pass	12:50pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County WATAUGA Instrument Location BOONE POLICE DEPARTMENT
Instrument Serial No. 008716 BOONE, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 31ST day of AUGUST, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.




Signature of Certifying Official

353799

Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

WATAUGA COUNTY BOONE PD 940

Serial Number: 008716

Test Date: 08/31/2026

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Oligmueller, Leo A

Permit Number: 0035-3799

Effective:

02/01/2026-02/01/2028

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG534301

Exp Date: 12/09/2027

Test	g/210L	Time
DIAG	Pass	9:29am
AIR BLK	.00	9:29am
ACCY CHK	.07	9:30am
AIR BLK	.00	9:31am
SUB TEST	.00	9:32am
AIR BLK	.00	9:33am
SUB TEST	.00	9:35am
AIR BLK	.00	9:36am

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

WATAUGA COUNTY BOONE PD 940

Serial Number: 008716 Test Record Number: 3619
Test Date: 08/31/2026 Test Time: 9:36am EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	9:36am
FLO	Pass	9:36am
FC	Pass	9:37am

Temperature Tests

Test	Status	Time
FC1	Pass	9:37am
SRC	Pass	9:37am
DET	Pass	9:37am
BAR	Pass	9:37am
BT	Pass	9:37am

Blank Tests

Test	Status	Time
AIR	Pass	9:37am

Printer Tests

Test	Status	Time
PRNT	Pass	9:37am

CRC Tests

Test	Status	Time
COMP	Pass	9:37am
CAL	Pass	9:37am

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Wayne Instrument Location Wayne Co. Detention Center
Instrument Serial No. 008671 Goldsboro, N.C.

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 7th day of August, 2020 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

377722
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

WAYNE COUNTY DETENTION CENTER 950

Serial Number: 008671

Test Date: 08/07/2026

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Gray, Kelly D

Permit Number: 0037-7722

Effective:

02/01/2026-02/01/2028

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG516203

Exp Date: 06/11/2027


Test	g/210L	Time
DIAG	Pass	11:54am
AIR BLK	.00	11:55am
ACCY CHK	.08	11:56am
AIR BLK	.00	11:57am
SUB TEST	.00	11:57am
AIR BLK	.00	11:58am
SUB TEST	.00	12:00pm
AIR BLK	.00	12:01pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

WAYNE COUNTY DETENTION CENTER 950

Serial Number: 008671 Test Record Number: 5568
Test Date: 08/07/2026 Test Time: 12:02pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	12:02pm
FLO	Pass	12:02pm
FC	Pass	12:02pm

Temperature Tests

Test	Status	Time
FC1	Pass	12:02pm
SRC	Pass	12:02pm
DET	Pass	12:02pm
BAR	Pass	12:02pm
BT	Pass	12:02pm

Blank Tests

Test	Status	Time
AIR	Pass	12:03pm

Printer Tests

Test	Status	Time
PRNT	Pass	12:03pm

CRC Tests

Test	Status	Time
COMP	Pass	12:03pm
CAL	Pass	12:03pm

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Wayne Instrument Location Seymour Johnson AFB
Instrument Serial No. 008786 Goldsboro, N.C.

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 7th day of August, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

377722
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

WAYNE COUNTY SEYMOUR JOHNSON AFB 950

Serial Number: 008786

Test Date: 08/07/2026

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Gray, Kelly D

Permit Number: 0037-7722

Effective:

02/01/2026-02/01/2028

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG501303

Exp Date: 01/13/2027

Test	g/210L	Time
DIAG	Pass	10:26am
AIR BLK	.00	10:26am
ACCY CHK	.08	10:27am
AIR BLK	.00	10:28am
SUB TEST	.00	10:29am
AIR BLK	.00	10:30am
SUB TEST	.00	10:32am
AIR BLK	.00	10:32am

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

WAYNE COUNTY SEYMOUR JOHNSON AFB 950

Serial Number: 008786 Test Record Number: 543
Test Date: 08/07/2026 Test Time: 10:39am EDT

System Check: Passed

Baseline Tests

Test	Status	Time
IR	Pass	10:40am
FLO	Pass	10:40am
FC	Pass	10:40am

Temperature Tests

Test	Status	Time
FC1	Pass	10:40am
SRC	Pass	10:40am
DET	Pass	10:40am
BAR	Pass	10:40am
BT	Pass	10:40am

Blank Tests

Test	Status	Time
AIR	Pass	10:40am

Printer Tests

Test	Status	Time
PRNT	Pass	10:40am

CRC Tests

Test	Status	Time
COMP	Pass	10:41am
CAL	Pass	10:41am

Preventive Maintenance
Status: Pass


Analyst