

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County Alamance Instrument Location BAT Mobile Unit 13

Instrument Serial No. 008869

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 27th day of February, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



John Lanier
Signature of Certifying Official

1404930
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

ALAMANCE COUNTY BAT MOBILE UNIT 13 000

Serial Number: 008869
Test Date: 02/27/2026

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: Lanier Jr., John P
Permit Number: 4582-9118
Effective:
02/01/2026-02/01/2028

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG417803
Exp Date: 06/26/2026


Test	g/210L	Time
DIAG	Pass	8:47pm
AIR BLK	.00	8:48pm
ACCY CHK	.08	8:49pm
AIR BLK	.00	8:50pm
SUB TEST	.00	8:50pm
AIR BLK	.00	8:51pm
SUB TEST	.00	8:53pm
AIR BLK	.00	8:54pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR

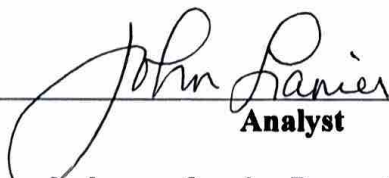

Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

ALAMANCE COUNTY BAT MOBILE UNIT 13 000

Serial Number: 008869 Test Record Number: 2149
Test Date: 02/27/2026 Test Time: 8:54pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	8:55pm
FLO	Pass	8:55pm
FC	Pass	8:55pm

Temperature Tests

Test	Status	Time
FC1	Pass	8:55pm
SRC	Pass	8:55pm
DET	Pass	8:55pm
BAR	Pass	8:55pm
BT	Pass	8:55pm

Blank Tests

Test	Status	Time
AIR	Pass	8:55pm


Printer Tests

Test	Status	Time
PRNT	Pass	8:56pm

CRC Tests

Test	Status	Time
COMP	Pass	8:56pm
CAL	Pass	8:56pm

Preventive Maintenance
Status: Pass

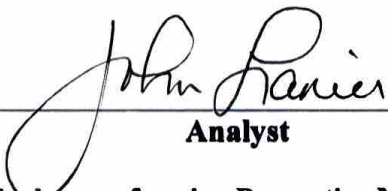

Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County Alamance

Instrument Location BAT Mobile Unit 13

Instrument Serial No. 008939

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 27th day of February, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



John Ranier
Signature of Certifying Official

1604930
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

ALAMANCE COUNTY BAT MOBILE UNIT 13 000

Serial Number: 008939
Test Date: 02/27/2026

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: Lanier Jr., John P
Permit Number: 4582-9118
Effective:
02/01/2026-02/01/2028

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG506302
Exp Date: 03/04/2027


Test	g/210L	Time
DIAG	Pass	8:48pm
AIR BLK	.00	8:49pm
ACCY CHK	.08	8:50pm
AIR BLK	.00	8:51pm
SUB TEST	.00	8:51pm
AIR BLK	.00	8:52pm
SUB TEST	.00	8:53pm
AIR BLK	.00	8:54pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

ALAMANCE COUNTY BAT MOBILE UNIT 13 000

Serial Number: 008939 Test Record Number: 1966
Test Date: 02/27/2026 Test Time: 8:55pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	8:55pm
FLO	Pass	8:55pm
FC	Pass	8:56pm

Temperature Tests

Test	Status	Time
FC1	Pass	8:56pm
SRC	Pass	8:56pm
DET	Pass	8:56pm
BAR	Pass	8:56pm
BT	Pass	8:56pm

Blank Tests

Test	Status	Time
AIR	Pass	8:56pm

Printer Tests

Test	Status	Time
PRNT	Pass	8:56pm

CRC Tests

Test	Status	Time
COMP	Pass	8:57pm
CAL	Pass	8:57pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County ALEXANDER Instrument Location ALEXANDER CO. S.C.

Instrument Serial No. 008813 TAYLORSVILLE NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 19 day of FEBRUARY, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

274970
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

ALEXANDER COUNTY ALEXANDER COUNTY SO
010

Serial Number: 008813
Test Date: 02/19/2026

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE

Analyst's Name: Fleming, Tina S
Permit Number: 0027-4970
Effective:
02/01/2025-02/01/2027

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG431001
Exp Date: 11/05/2026

Test	g/210L	Time
DIAG	Pass	8:59am
AIR BLK	.00	9:00am
ACCY CHK	.08	9:01am
AIR BLK	.00	9:02am
SUB TEST	.00	9:03am
AIR BLK	.00	9:03am
SUB TEST	.00	9:05am
AIR BLK	.00	9:06am

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

ALEXANDER COUNTY ALEXANDER COUNTY SO 010

Serial Number: 008813 Test Record Number: 2527
Test Date: 02/19/2026 Test Time: 9:10am EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	9:10am
FLO	Pass	9:10am
FC	Pass	9:10am

Temperature Tests

Test	Status	Time
FC1	Pass	9:10am
SRC	Pass	9:10am
DET	Pass	9:10am
BAR	Pass	9:10am
BT	Pass	9:10am

Blank Tests

Test	Status	Time
AIR	Pass	9:11am


Printer Tests

Test	Status	Time
PRNT	Pass	9:11am

CRC Tests

Test	Status	Time
COMP	Pass	9:11am
CAL	Pass	9:11am

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County Ashe Instrument Location Ashe County
Instrument Serial No. 008849 Jail

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 4th day of February, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

509387
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

ASHE COUNTY ASHE COUNTY JAIL 040

Serial Number: 008849
Test Date: 02/04/2026

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: Long, Thomas A
Permit Number: 0050-9387
Effective:
09/01/2025-09/01/2027

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG417803
Exp Date: 06/26/2026

Test	g/210L	Time
DIAG	Pass	9:00am
AIR BLK	.00	9:00am
ACCY CHK	.07	9:01am
AIR BLK	.00	9:02am
SUB TEST	.00	9:04am
AIR BLK	.00	9:05am
SUB TEST	.00	9:06am
AIR BLK	.00	9:07am

Reported AC: .00 g/210L

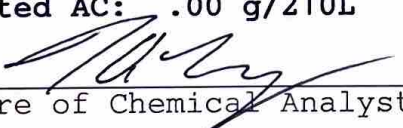

Signature of Chemical Analyst

Court CVR



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

ASHE COUNTY ASHE COUNTY JAIL 040

Serial Number: 008849 Test Record Number: 1871
Test Date: 02/04/2026 Test Time: 9:08am EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	9:08am
FLO	Pass	9:08am
FC	Pass	9:08am

Temperature Tests

Test	Status	Time
FC1	Pass	9:08am
SRC	Pass	9:08am
DET	Pass	9:08am
BAR	Pass	9:08am
BT	Pass	9:08am

Blank Tests

Test	Status	Time
AIR	Pass	9:09am

Printer Tests

Test	Status	Time
PRNT	Pass	9:09am

CRC Tests

Test	Status	Time
COMP	Pass	9:09am
CAL	Pass	9:09am

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County Beaufort Instrument Location Beaufort Co. Courthouse
Instrument Serial No. 008586 112 W. 2nd St., Washington, N.C.

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 9th day of February, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Key P. M.
Signature of Certifying Official

377722
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

BEAUFORT COUNTY COURTHOUSE 060

Serial Number: 008586
Test Date: 02/09/2026

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: Gray, Kelly D
Permit Number: 0037-7722
Effective:
02/01/2026-02/01/2028

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG516203
Exp Date: 06/11/2027

Test	g/210L	Time
DIAG	Pass	2:12pm
AIR BLK	.00	2:13pm
ACCY CHK	.07	2:13pm
AIR BLK	.00	2:15pm
SUB TEST	.00	2:16pm
AIR BLK	.00	2:17pm
SUB TEST	.00	2:18pm
AIR BLK	.00	2:19pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

Intox EC/IR-II: Preventive Maintenance

BEAUFORT COUNTY COURTHOUSE 060

Serial Number: 008586 Test Record Number: 2452
Test Date: 02/09/2026 Test Time: 2:22pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	2:23pm
FLO	Pass	2:23pm
FC	Pass	2:23pm

Temperature Tests

Test	Status	Time
FC1	Pass	2:23pm
SRC	Pass	2:23pm
DET	Pass	2:23pm
BAR	Pass	2:23pm
BT	Pass	2:23pm

Blank Tests

Test	Status	Time
AIR	Pass	2:23pm

Printer Tests

Test	Status	Time
PRNT	Pass	2:23pm

CRC Tests

Test	Status	Time
COMP	Pass	2:24pm
CAL	Pass	2:24pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Beaufort Instrument Location Beaufort Co. Courthouse
Instrument Serial No. 008909 112 W. 2nd St., Washington, NC.

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 9th day of February, 2020 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Kery D. G.
Signature of Certifying Official

377722
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

BEAUFORT COUNTY COURTHOUSE 060

Serial Number: 008909
Test Date: 02/09/2026

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: Gray, Kelly D
Permit Number: 0037-7722
Effective:
02/01/2026-02/01/2028

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG506303
Exp Date: 03/04/2027


Test	g/210L	Time
DIAG	Pass	1:44pm
AIR BLK	.00	1:45pm
ACCY CHK	.08	1:46pm
AIR BLK	.00	1:47pm
SUB TEST	.00	1:48pm
AIR BLK	.00	1:49pm
SUB TEST	.00	1:50pm
AIR BLK	.00	1:51pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR

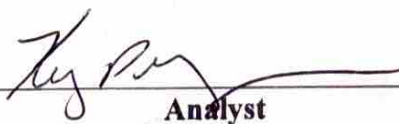

Analyst

Intox EC/IR-II: Preventive Maintenance

BEAUFORT COUNTY COURTHOUSE 060

Serial Number: 008909 Test Record Number: 4373
Test Date: 02/09/2026 Test Time: 1:55pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	1:56pm
FLO	Pass	1:56pm
FC	Pass	1:56pm

Temperature Tests

Test	Status	Time
FC1	Pass	1:56pm
SRC	Pass	1:56pm
DET	Pass	1:56pm
BAR	Pass	1:56pm
BT	Pass	1:56pm

Blank Tests

Test	Status	Time
AIR	Pass	1:57pm

Printer Tests

Test	Status	Time
PRNT	Pass	1:57pm

CRC Tests

Test	Status	Time
COMP	Pass	1:57pm
CAL	Pass	1:57pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Beaufort Instrument Location Belhaven P.D.
Instrument Serial No. 008928 144 W. Main St., Belhaven, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 9th day of February, 2020 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

377722
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

BEAUFORT COUNTY BELHAVEN PD 060

Serial Number: 008928
Test Date: 02/09/2026

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Gray, Kelly D

Permit Number: 0037-7722

Effective:

02/01/2026-02/01/2028

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG501303

Exp Date: 01/13/2027

Test	g/210L	Time
DIAG	Pass	12:12pm
AIR BLK	.00	12:12pm
ACCY CHK	.07	12:13pm
AIR BLK	.00	12:14pm
SUB TEST	.00	12:15pm
AIR BLK	.00	12:16pm
SUB TEST	.00	12:17pm
AIR BLK	.00	12:18pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

Intox EC/IR-II: Preventive Maintenance

BEAUFORT COUNTY BELHAVEN PD 060

Serial Number: 008928 Test Record Number: 611
Test Date: 02/09/2026 Test Time: 12:19pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	12:20pm
FLO	Pass	12:20pm
FC	Pass	12:20pm

Temperature Tests

Test	Status	Time
FC1	Pass	12:20pm
SRC	Pass	12:20pm
DET	Pass	12:20pm
BAR	Pass	12:20pm
BT	Pass	12:20pm

Blank Tests

Test	Status	Time
AIR	Pass	12:20pm

Printer Tests

Test	Status	Time
PRNT	Pass	12:21pm

CRC Tests

Test	Status	Time
COMP	Pass	12:21pm
CAL	Pass	12:21pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**


County Buncombe Instrument Location Buncombe County Detention
Instrument Serial No. 003808 Asheville, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 8 day of February, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.

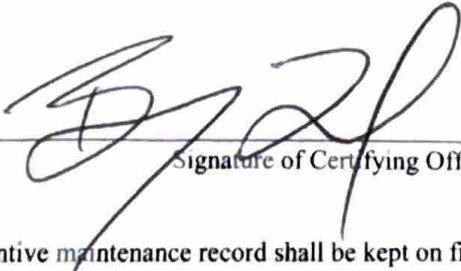


Signature of Certifying Official

244987
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

BUNCOMBE COUNTY BUNCOMBE COUNTY
DETENTION 100

Serial Number: 008808
Test Date: 02/08/2026

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE

Analyst's Name: Loftis, Benjamin C
Permit Number: 0024-4987
Effective:
02/01/2026-02/01/2028

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG534301
Exp Date: 12/09/2027

Test	g/210L	Time
DIAG	Pass	8:49pm
AIR BLK	.00	8:50pm
ACCY CHK	.08	8:51pm
AIR BLK	.00	8:52pm
SUB TEST	.00	8:52pm
AIR BLK	.00	8:53pm
SUB TEST	.00	8:55pm
AIR BLK	.00	8:56pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

BUNCOMBE COUNTY BUNCOMBE COUNTY DETENTION 100

Serial Number: 008808 Test Record Number: 1566
Test Date: 02/08/2026 Test Time: 8:56pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	8:56pm
FLO	Pass	8:56pm
FC	Pass	8:56pm

Temperature Tests

Test	Status	Time
FC1	Pass	8:56pm
SRC	Pass	8:56pm
DET	Pass	8:56pm
BAR	Pass	8:56pm
BT	Pass	8:56pm

Blank Tests

Test	Status	Time
AIR	Pass	8:57pm

Printer Tests

Test	Status	Time
PRNT	Pass	8:57pm

CRC Tests

Test	Status	Time
COMP	Pass	8:57pm
CAL	Pass	8:57pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County Buncombe Instrument Location Buncombe County Detention
Asheville, NC
Instrument Serial No. 008916

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 8 day of February, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

244987
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

BUNCOMBE COUNTY BUNCOMBE COUNTY
DETENTION 100

Serial Number: 008916
Test Date: 02/08/2026

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: Loftis, Benjamin C
Permit Number: 0024-4987
Effective:
02/01/2026-02/01/2028

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG506303
Exp Date: 03/04/2027

Test	g/210L	Time
DIAG	Pass	8:42pm
AIR BLK	.00	8:42pm
ACCY CHK	.07	8:43pm
AIR BLK	.00	8:44pm
SUB TEST	.00	8:44pm
AIR BLK	.00	8:45pm
SUB TEST	.00	8:47pm
AIR BLK	.00	8:48pm

Reported AC: .00 g/210L

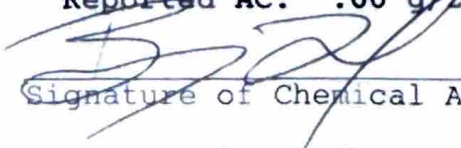

Signature of Chemical Analyst

Court CVR



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

BUNCOMBE COUNTY BUNCOMBE COUNTY DETENTION 100

Serial Number: 008916 Test Record Number: 1999
Test Date: 02/08/2026 Test Time: 8:48pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	8:48pm
FLO	Pass	8:48pm
FC	Pass	8:48pm

Temperature Tests

Test	Status	Time
FC1	Pass	8:49pm
SRC	Pass	8:49pm
DET	Pass	8:49pm
BAR	Pass	8:49pm
BT	Pass	8:49pm

Blank Tests

Test	Status	Time
AIR	Pass	8:49pm

Printer Tests

Test	Status	Time
PRNT	Pass	8:49pm

CRC Tests

Test	Status	Time
COMP	Pass	8:50pm
CAL	Pass	8:50pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Burcombe Instrument Location BAT Mobile Unit 11

Instrument Serial No. 008970

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 24th day of February, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Jeff Bithorn
Signature of Certifying Official

062446
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

BUNCOMBE COUNTY BAT MOBILE UNIT 11 100

Serial Number: 008970
Test Date: 02/24/2026

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE

Analyst's Name: Gillstrap, Jeffrey L
Permit Number: 0006-2446
Effective:
04/01/2025-04/01/2027

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG417802
Exp Date: 06/26/2026


Test	g/210L	Time
DIAG	Pass	9:31pm
AIR BLK	.00	9:32pm
ACCY CHK	.08	9:32pm
AIR BLK	.00	9:33pm
SUB TEST	.00	9:34pm
AIR BLK	.00	9:35pm
SUB TEST	.00	9:36pm
AIR BLK	.00	9:37pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR

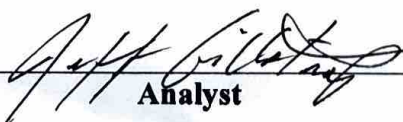

Analyst

P
Intox EC/IR-II: Preventive Maintenance

BUNCOMBE COUNTY BAT MOBILE UNIT 11 100

Serial Number: 008970 Test Record Number: 1374
Test Date: 02/24/2026 Test Time: 9:38pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	9:38pm
FLO	Pass	9:38pm
FC	Pass	9:38pm

Temperature Tests

Test	Status	Time
FC1	Pass	9:39pm
SRC	Pass	9:39pm
DET	Pass	9:39pm
BAR	Pass	9:39pm
BT	Pass	9:39pm

Blank Tests

Test	Status	Time
AIR	Pass	9:39pm


Printer Tests

Test	Status	Time
PRNT	Pass	9:39pm

CRC Tests

Test	Status	Time
COMP	Pass	9:39pm
CAL	Pass	9:39pm

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County Buncombe Instrument Location BAT Mobile Unit 11

Instrument Serial No. 008970

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 25th day of February, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Jeff B. [Signature]
Signature of Certifying Official

062446
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

BUNCOMBE COUNTY BAT MOBILE UNIT 11 100

Serial Number: 008970
Test Date: 02/25/2026

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: Gillstrap, Jeffrey L
Permit Number: 0006-2446
Effective:
04/01/2025-04/01/2027

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG417802
Exp Date: 06/26/2026

Test	g/210L	Time
DIAG	Pass	12:03am
AIR BLK	.00	12:04am
ACCY CHK	.07	12:04am
AIR BLK	.00	12:05am
SUB TEST	.00	12:06am
AIR BLK	.00	12:07am
SUB TEST	.00	12:08am
AIR BLK	.00	12:09am

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

Intox EC/IR-II: Preventive Maintenance

BUNCOMBE COUNTY BAT MOBILE UNIT 11 100

Serial Number: 008970 Test Record Number: 1376
Test Date: 02/25/2026 Test Time: 12:10am EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	12:11am
FLO	Pass	12:11am
FC	Pass	12:11am

Temperature Tests

Test	Status	Time
FC1	Pass	12:11am
SRC	Pass	12:11am
DET	Pass	12:11am
BAR	Pass	12:11am
BT	Pass	12:11am

Blank Tests

Test	Status	Time
AIR	Pass	12:11am

Printer Tests

Test	Status	Time
PRNT	Pass	12:12am

CRC Tests

Test	Status	Time
COMP	Pass	12:12am
CAL	Pass	12:12am

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County Buncombe Instrument Location BAT Mobile Unit 11

Instrument Serial No. 008970

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 26th day of February, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Jeff Bittner
Signature of Certifying Official

062446
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

BUNCOMBE COUNTY BAT MOBILE UNIT 11 100

Serial Number: 008970
Test Date: 02/26/2026

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: Gillstrap, Jeffrey L
Permit Number: 0006-2446
Effective:
04/01/2025-04/01/2027

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG417802
Exp Date: 06/26/2026


Test	g/210L	Time
DIAG	Pass	12:09am
AIR BLK	.00	12:10am
ACCY CHK	.07	12:11am
AIR BLK	.00	12:12am
SUB TEST	.00	12:12am
AIR BLK	.00	12:13am
SUB TEST	.00	12:15am
AIR BLK	.00	12:16am

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR

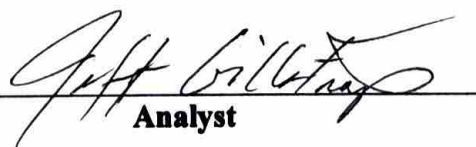

Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

BUNCOMBE COUNTY BAT MOBILE UNIT 11 100

Serial Number: 008970 Test Record Number: 1381
Test Date: 02/26/2026 Test Time: 12:17am EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	12:18am
FLO	Pass	12:18am
FC	Pass	12:18am

Temperature Tests

Test	Status	Time
FC1	Pass	12:18am
SRC	Pass	12:18am
DET	Pass	12:18am
BAR	Pass	12:18am
BT	Pass	12:18am

Blank Tests

Test	Status	Time
AIR	Pass	12:18am

Printer Tests

Test	Status	Time
PRNT	Pass	12:18am

CRC Tests

Test	Status	Time
COMP	Pass	12:19am
CAL	Pass	12:19am

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Buncombe Instrument Location BHT Mobile Unit 11

Instrument Serial No. 008970

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 27th day of February, 20 26 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

062446
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

BUNCOMBE COUNTY BAT MOBILE UNIT 11 100

Serial Number: 008970
Test Date: 02/27/2026

Citation Number: M0000000-0
Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Gillstrap, Jeffrey L

Permit Number: 0006-2446

Effective:

04/01/2025-04/01/2027

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG417802

Exp Date: 06/26/2026


Test	g/210L	Time
DIAG	Pass	9:19pm
AIR BLK	.00	9:20pm
ACCY CHK	.08	9:21pm
AIR BLK	.00	9:22pm
SUB TEST	.00	9:23pm
AIR BLK	.00	9:24pm
SUB TEST	.00	9:25pm
AIR BLK	.00	9:26pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR

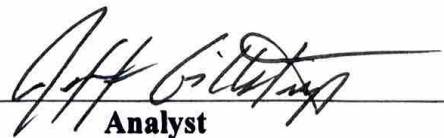

Analyst

Intox EC/IR-II: Preventive Maintenance

BUNCOMBE COUNTY BAT MOBILE UNIT 11 100

Serial Number: 008970 Test Record Number: 1385
Test Date: 02/27/2026 Test Time: 9:27pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	9:27pm
FLO	Pass	9:27pm
FC	Pass	9:27pm

Temperature Tests

Test	Status	Time
FC1	Pass	9:27pm
SRC	Pass	9:27pm
DET	Pass	9:27pm
BAR	Pass	9:27pm
BT	Pass	9:27pm

Blank Tests

Test	Status	Time
AIR	Pass	9:28pm


Printer Tests

Test	Status	Time
PRNT	Pass	9:28pm

CRC Tests

Test	Status	Time
COMP	Pass	9:28pm
CAL	Pass	9:28pm

Preventive Maintenance
Status: Pass

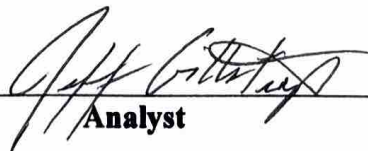

Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Buncombe Instrument Location BAT Mobile Unit 11

Instrument Serial No. 008970

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 28th day of February, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

062446
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

BUNCOMBE COUNTY BAT MOBILE UNIT 11 100

Serial Number: 008970
Test Date: 02/28/2026

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Gillstrap, Jeffrey L

Permit Number: 0006-2446

Effective:

04/01/2025-04/01/2027

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG417802

Exp Date: 06/26/2026

Test	g/210L	Time
DIAG	Pass	12:42am
AIR BLK	.00	12:43am
ACCY CHK	.07	12:43am
AIR BLK	.00	12:44am
SUB TEST	.00	12:45am
AIR BLK	.00	12:46am
SUB TEST	.00	12:47am
AIR BLK	.00	12:48am

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

BUNCOMBE COUNTY BAT MOBILE UNIT 11 100

Serial Number: 008970 Test Record Number: 1387
Test Date: 02/28/2026 Test Time: 12:49am EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	12:49am
FLO	Pass	12:49am
FC	Pass	12:49am

Temperature Tests

Test	Status	Time
FC1	Pass	12:49am
SRC	Pass	12:49am
DET	Pass	12:49am
BAR	Pass	12:49am
BT	Pass	12:49am

Blank Tests

Test	Status	Time
AIR	Pass	12:50am

Printer Tests

Test	Status	Time
PRNT	Pass	12:50am

CRC Tests

Test	Status	Time
COMP	Pass	12:50am
CAL	Pass	12:50am

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Buncombe Instrument Location BAT Mobile Unit II
Instrument Serial No. 008973

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 24th day of February, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Jeff Bittner
Signature of Certifying Official

062446
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

BUNCOMBE COUNTY BAT MOBILE UNIT 11 100

Serial Number: 008973
Test Date: 02/24/2026

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Gillstrap, Jeffrey L

Permit Number: 0006-2446

Effective:

04/01/2025-04/01/2027

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG431003

Exp Date: 11/05/2026

Test	g/210L	Time
DIAG	Pass	9:39pm
AIR BLK	.00	9:40pm
ACCY CHK	.07	9:41pm
AIR BLK	.00	9:42pm
SUB TEST	.00	9:42pm
AIR BLK	.00	9:43pm
SUB TEST	.00	9:46pm
AIR BLK	.00	9:47pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

BUNCOMBE COUNTY BAT MOBILE UNIT 11 100

Serial Number: 008973 Test Record Number: 1425
Test Date: 02/24/2026 Test Time: 9:48pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	9:48pm
FLO	Pass	9:48pm
FC	Pass	9:48pm

Temperature Tests

Test	Status	Time
FC1	Pass	9:48pm
SRC	Pass	9:48pm
DET	Pass	9:48pm
BAR	Pass	9:48pm
BT	Pass	9:48pm

Blank Tests

Test	Status	Time
AIR	Pass	9:49pm

Printer Tests

Test	Status	Time
PRNT	Pass	9:49pm

CRC Tests

Test	Status	Time
COMP	Pass	9:49pm
CAL	Pass	9:49pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County Buncombe Instrument Location BAT Mobile Unit 11
Instrument Serial No. 008973

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 25th day of February, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Jeff P. Helms
Signature of Certifying Official

062446
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

BUNCOMBE COUNTY BAT MOBILE UNIT 11 100

Serial Number: 008973
Test Date: 02/25/2026

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: NC
Driver's License Number: XX

Analyst's Name: Gillstrap, Jeffrey L
Permit Number: 0006-2446
Effective:
04/01/2025-04/01/2027

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG431003
Exp Date: 11/05/2026

Test	g/210L	Time
DIAG	Pass	12:10am
AIR BLK	.00	12:11am
ACCY CHK	.07	12:11am
AIR BLK	.00	12:12am
SUB TEST	.00	12:13am
AIR BLK	.00	12:14am
SUB TEST	.00	12:15am
AIR BLK	.00	12:16am

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

BUNCOMBE COUNTY BAT MOBILE UNIT 11 100

Serial Number: 008973 Test Record Number: 1427
Test Date: 02/25/2026 Test Time: 12:18am EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	12:19am
FLO	Pass	12:19am
FC	Pass	12:19am

Temperature Tests

Test	Status	Time
FC1	Pass	12:19am
SRC	Pass	12:19am
DET	Pass	12:19am
BAR	Pass	12:19am
BT	Pass	12:19am

Blank Tests

Test	Status	Time
AIR	Pass	12:20am

Printer Tests

Test	Status	Time
PRNT	Pass	12:20am

CRC Tests

Test	Status	Time
COMP	Pass	12:20am
CAL	Pass	12:20am

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Buncombe Instrument Location BAT Mobile Unit 11

Instrument Serial No. 008973

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 26th day of February, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Jeff Dittus
Signature of Certifying Official

062446
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

BUNCOMBE COUNTY BAT MOBILE UNIT 11 100

Serial Number: 008973
Test Date: 02/26/2026

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Gillstrap, Jeffrey L

Permit Number: 0006-2446

Effective:

04/01/2025-04/01/2027

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG431003

Exp Date: 11/05/2026

Test	g/210L	Time
DIAG	Pass	12:17am
AIR BLK	.00	12:17am
ACCY CHK	.07	12:18am
AIR BLK	.00	12:19am
SUB TEST	.00	12:19am
AIR BLK	.00	12:20am
SUB TEST	.00	12:22am
AIR BLK	.00	12:23am

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

BUNCOMBE COUNTY BAT MOBILE UNIT 11 100

Serial Number: 008973 Test Record Number: 1432
Test Date: 02/26/2026 Test Time: 12:24am EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	12:24am
FLO	Pass	12:24am
FC	Pass	12:24am

Temperature Tests

Test	Status	Time
FC1	Pass	12:24am
SRC	Pass	12:24am
DET	Pass	12:24am
BAR	Pass	12:24am
BT	Pass	12:24am

Blank Tests

Test	Status	Time
AIR	Pass	12:25am

Printer Tests

Test	Status	Time
PRNT	Pass	12:25am

CRC Tests

Test	Status	Time
COMP	Pass	12:25am
CAL	Pass	12:25am

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County Buncombe Instrument Location BAT Mobile Unit 11

Instrument Serial No. 008973

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 27th day of February, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

062446
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

BUNCOMBE COUNTY BAT MOBILE UNIT 11 100

Serial Number: 008973
Test Date: 02/27/2026

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE

Analyst's Name: Gillstrap, Jeffrey L
Permit Number: 0006-2446
Effective:
04/01/2025-04/01/2027

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG431003
Exp Date: 11/05/2026

Test	g/210L	Time
DIAG	Pass	9:20pm
AIR BLK	.00	9:21pm
ACCY CHK	.07	9:22pm
AIR BLK	.00	9:23pm
SUB TEST	.00	9:24pm
AIR BLK	.00	9:24pm
SUB TEST	.00	9:26pm
AIR BLK	.00	9:27pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

BUNCOMBE COUNTY BAT MOBILE UNIT 11 100

Serial Number: 008973 Test Record Number: 1436
Test Date: 02/27/2026 Test Time: 9:29pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	9:29pm
FLO	Pass	9:29pm
FC	Pass	9:29pm

Temperature Tests

Test	Status	Time
FC1	Pass	9:29pm
SRC	Pass	9:29pm
DET	Pass	9:29pm
BAR	Pass	9:29pm
BT	Pass	9:29pm

Blank Tests

Test	Status	Time
AIR	Pass	9:30pm

Printer Tests

Test	Status	Time
PRNT	Pass	9:30pm

CRC Tests

Test	Status	Time
COMP	Pass	9:30pm
CAL	Pass	9:30pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County Buncombe Instrument Location BAT Mobile Unit 11

Instrument Serial No. 008973

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 28th day of February, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Jeff Gillette
Signature of Certifying Official

062446
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

BUNCOMBE COUNTY BAT MOBILE UNIT 11 100

Serial Number: 008973
Test Date: 02/28/2026

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE

Analyst's Name: *Gillstrap, Jeffrey L*
Permit Number: 0006-2446
Effective:
04/01/2025-04/01/2027

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: *Breath Test*

Lot Number: AG431003
Exp Date: 11/05/2026

Test	g/210L	Time
DIAG	Pass	12:44am
AIR BLK	.00	12:45am
ACCY CHK	.07	12:45am
AIR BLK	.00	12:46am
SUB TEST	.00	12:47am
AIR BLK	.00	12:48am
SUB TEST	.00	12:50am
AIR BLK	.00	12:50am

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

BUNCOMBE COUNTY BAT MOBILE UNIT 11 100

Serial Number: 008973 Test Record Number: 1439
Test Date: 02/28/2026 Test Time: 12:52am EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	12:53am
FLO	Pass	12:53am
FC	Pass	12:53am

Temperature Tests

Test	Status	Time
FC1	Pass	12:53am
SRC	Pass	12:53am
DET	Pass	12:53am
BAR	Pass	12:53am
BT	Pass	12:53am

Blank Tests

Test	Status	Time
AIR	Pass	12:53am

Printer Tests

Test	Status	Time
PRNT	Pass	12:53am

CRC Tests

Test	Status	Time
COMP	Pass	12:54am
CAL	Pass	12:54am

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County Cabarrus Instrument Location BAT Mobile Unit 8

Instrument Serial No. 008615

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 8 day of February, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Jerry D. Johnson
Signature of Certifying Official

2219283
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

CABARRUS COUNTY BAT MOBILE UNIT 8 120

Serial Number: 008615

Test Date: 02/08/2026

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Glasscock, Jerry D

Permit Number: 7180-9235

Effective:

02/01/2026-02/01/2028

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG405102

Exp Date: 02/20/2026

Test	g/210L	Time
DIAG	Pass	8:10pm
AIR BLK	.00	8:11pm
ACCY CHK	.07	8:11pm
AIR BLK	.00	8:12pm
SUB TEST	.00	8:13pm
AIR BLK	.00	8:14pm
SUB TEST	.00	8:15pm
AIR BLK	.00	8:16pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

CABARRUS COUNTY BAT MOBILE UNIT 8 120

Serial Number: 008615 Test Record Number: 6239
Test Date: 02/08/2026 Test Time: 8:17pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	8:17pm
FLO	Pass	8:17pm
FC	Pass	8:17pm

Temperature Tests

Test	Status	Time
FC1	Pass	8:17pm
SRC	Pass	8:17pm
DET	Pass	8:17pm
BAR	Pass	8:17pm
BT	Pass	8:17pm

Blank Tests

Test	Status	Time
AIR	Pass	8:18pm

Printer Tests

Test	Status	Time
PRNT	Pass	8:18pm

CRC Tests

Test	Status	Time
COMP	Pass	8:18pm
CAL	Pass	8:18pm

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County Cabarrus Instrument Location BAT Mobile Unit 8

Instrument Serial No. 008615

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 11 day of February, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

2219283
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

CABARRUS COUNTY BAT MOBILE UNIT 8 120

Serial Number: 008615
Test Date: 02/11/2026

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: Glasscock, Jerry D
Permit Number: 7180-9235
Effective:
02/01/2026-02/01/2028

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG405102
Exp Date: 02/20/2026

Test	g/210L	Time
DIAG	Pass	7:01am
AIR BLK	.00	7:02am
ACCY CHK	.07	7:03am
AIR BLK	.00	7:04am
SUB TEST	.00	7:04am
AIR BLK	.00	7:05am
SUB TEST	.00	7:07am
AIR BLK	.00	7:08am

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

Intox EC/IR-II: Preventive Maintenance

CABARRUS COUNTY BAT MOBILE UNIT 8 120

Serial Number: 008615 Test Record Number: 6241
Test Date: 02/11/2026 Test Time: 7:09am EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	7:09am
FLO	Pass	7:09am
FC	Pass	7:09am

Temperature Tests

Test	Status	Time
FC1	Pass	7:09am
SRC	Pass	7:09am
DET	Pass	7:09am
BAR	Pass	7:09am
BT	Pass	7:09am

Blank Tests

Test	Status	Time
AIR	Pass	7:10am

Printer Tests

Test	Status	Time
PRNT	Pass	7:10am

CRC Tests

Test	Status	Time
COMP	Pass	7:10am
CAL	Pass	7:10am

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County Cabarrus Instrument Location BAT Mobile Unit 8
Instrument Serial No. 008615 -

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 26 day of February, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

2219283
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

CABARRUS COUNTY BAT MOBILE UNIT 8 120

Serial Number: 008615
Test Date: 02/26/2026

Citation Number: M0000000-0
Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Glasscock, Jerry D

Permit Number: 7180-9235

Effective:

02/01/2026-02/01/2028

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG506303

Exp Date: 03/04/2027

Test	g/210L	Time
DIAG	Pass	1:47pm
AIR BLK	.00	1:48pm
ACCY CHK	.07	1:49pm
AIR BLK	.00	1:50pm
SUB TEST	.00	1:50pm
AIR BLK	.00	1:51pm
SUB TEST	.00	1:53pm
AIR BLK	.00	1:54pm

Reported AC: .00 g/210L

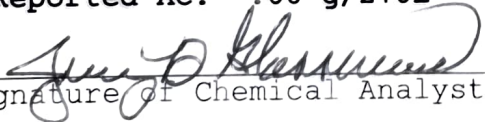
Signature of Chemical Analyst

Court CVR


Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

CABARRUS COUNTY BAT MOBILE UNIT 8 120

Serial Number: 008615 Test Record Number: 6257
Test Date: 02/26/2026 Test Time: 1:54pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	1:54pm
FLO	Pass	1:54pm
FC	Pass	1:54pm

Temperature Tests

Test	Status	Time
FC1	Pass	1:55pm
SRC	Pass	1:55pm
DET	Pass	1:55pm
BAR	Pass	1:55pm
BT	Pass	1:55pm

Blank Tests

Test	Status	Time
AIR	Pass	1:55pm

Printer Tests

Test	Status	Time
PRNT	Pass	1:55pm

CRC Tests

Test	Status	Time
COMP	Pass	1:55pm
CAL	Pass	1:55pm

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Cabarrus Instrument Location BAT Mobile Unit 8

Instrument Serial No. 008736 —

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 8 day of February, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Jay D. Blum
Signature of Certifying Official

2219283
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

CABARRUS COUNTY BAT MOBILE UNIT 8 120

Serial Number: 008736

Test Date: 02/08/2026

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Glasscock, Jerry D

Permit Number: 7180-9235

Effective:

02/01/2026-02/01/2028

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG405102

Exp Date: 02/20/2026

Test	g/210L	Time
DIAG	Pass	8:09pm
AIR BLK	.00	8:10pm
ACCY CHK	.07	8:11pm
AIR BLK	.00	8:11pm
SUB TEST	.00	8:12pm
AIR BLK	.00	8:13pm
SUB TEST	.00	8:14pm
AIR BLK	.00	8:15pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

CABARRUS COUNTY BAT MOBILE UNIT 8 120

Serial Number: 008736 Test Record Number: 1595
Test Date: 02/08/2026 Test Time: 8:16pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	8:17pm
FLO	Pass	8:17pm
FC	Pass	8:17pm

Temperature Tests

Test	Status	Time
FC1	Pass	8:17pm
SRC	Pass	8:17pm
DET	Pass	8:17pm
BAR	Pass	8:17pm
BT	Pass	8:17pm

Blank Tests

Test	Status	Time
AIR	Pass	8:17pm

Printer Tests

Test	Status	Time
PRNT	Pass	8:17pm

CRC Tests

Test	Status	Time
COMP	Pass	8:18pm
CAL	Pass	8:18pm

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Cabarrus Instrument Location BAT Mobile Unit 8
Instrument Serial No. 008736

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 11 day of February, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

2219283
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

CABARRUS COUNTY BAT MOBILE UNIT 8 120

Serial Number: 008736
Test Date: 02/11/2026

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Glasscock, Jerry D

Permit Number: 7180-9235

Effective:

02/01/2026-02/01/2028

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG405102

Exp Date: 02/20/2026

Test	g/210L	Time
DIAG	Pass	7:00am
AIR BLK	.00	7:01am
ACCY CHK	.07	7:02am
AIR BLK	.00	7:03am
SUB TEST	.00	7:03am
AIR BLK	.00	7:04am
SUB TEST	.00	7:05am
AIR BLK	.00	7:06am

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

CABARRUS COUNTY BAT MOBILE UNIT 8 120

Serial Number: 008736 Test Record Number: 1597
Test Date: 02/11/2026 Test Time: 7:09am EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	7:09am
FLO	Pass	7:09am
FC	Pass	7:09am

Temperature Tests

Test	Status	Time
FC1	Pass	7:09am
SRC	Pass	7:09am
DET	Pass	7:09am
BAR	Pass	7:09am
BT	Pass	7:09am

Blank Tests

Test	Status	Time
AIR	Pass	7:10am

Printer Tests

Test	Status	Time
PRNT	Pass	7:10am

CRC Tests

Test	Status	Time
COMP	Pass	7:10am
CAL	Pass	7:10am

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Cabarrus Instrument Location BAT Mobile Unit 8
Instrument Serial No. 008736

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 11 day of February, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

2219283
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

CABARRUS COUNTY BAT MOBILE UNIT 8 120

Serial Number: 008736
Test Date: 02/11/2026

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Glasscock, Jerry D

Permit Number: 7180-9235

Effective:

02/01/2026-02/01/2028

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG405102

Exp Date: 02/20/2026

Test	g/210L	Time
DIAG	Pass	7:00am
AIR BLK	.00	7:01am
ACCY CHK	.07	7:02am
AIR BLK	.00	7:03am
SUB TEST	.00	7:03am
AIR BLK	.00	7:04am
SUB TEST	.00	7:05am
AIR BLK	.00	7:06am

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

Intox EC/IR-II: Preventive Maintenance

CABARRUS COUNTY BAT MOBILE UNIT 8 120

Serial Number: 008736 Test Record Number: 1597
Test Date: 02/11/2026 Test Time: 7:09am EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	7:09am
FLO	Pass	7:09am
FC	Pass	7:09am

Temperature Tests

Test	Status	Time
FC1	Pass	7:09am
SRC	Pass	7:09am
DET	Pass	7:09am
BAR	Pass	7:09am
BT	Pass	7:09am

Blank Tests

Test	Status	Time
AIR	Pass	7:10am

Printer Tests

Test	Status	Time
PRNT	Pass	7:10am

CRC Tests

Test	Status	Time
COMP	Pass	7:10am
CAL	Pass	7:10am

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)


County Cabarrus Instrument Location BAT Mobile Unit 3

Instrument Serial No. 008736 —

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 26 day of February, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

2219283
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

CABARRUS COUNTY BAT MOBILE UNIT 8 120

Serial Number: 008736
Test Date: 02/26/2026

Citation Number: M0000000-0
Subject's Name:

PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: Glasscock, Jerry D
Permit Number: 7180-9235
Effective:
02/01/2026-02/01/2028

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG506303
Exp Date: 03/04/2027

Test	g/210L	Time
DIAG	Pass	1:48pm
AIR BLK	.00	1:49pm
ACCY CHK	.07	1:49pm
AIR BLK	.00	1:51pm
SUB TEST	.00	1:51pm
AIR BLK	.00	1:52pm
SUB TEST	.00	1:53pm
AIR BLK	.00	1:54pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

CABARRUS COUNTY BAT MOBILE UNIT 8 120

Serial Number: 008736 Test Record Number: 1613
Test Date: 02/26/2026 Test Time: 1:56pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	1:56pm
FLO	Pass	1:56pm
FC	Pass	1:56pm

Temperature Tests

Test	Status	Time
FC1	Pass	1:56pm
SRC	Pass	1:56pm
DET	Pass	1:56pm
BAR	Pass	1:56pm
BT	Pass	1:56pm

Blank Tests

Test	Status	Time
AIR	Pass	1:57pm

Printer Tests

Test	Status	Time
PRNT	Pass	1:57pm

CRC Tests

Test	Status	Time
COMP	Pass	1:57pm
CAL	Pass	1:57pm

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Cabarrus Instrument Location BAT Mobile Unit 8

Instrument Serial No. 008775 -

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 11 day of February, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

2219283
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

CABARRUS COUNTY BAT MOBILE UNIT 8 120

Serial Number: 008775

Test Date: 02/11/2026

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Glasscock, Jerry D

Permit Number: 7180-9235

Effective:

02/01/2026-02/01/2028

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG506303

Exp Date: 03/04/2027

Test	g/210L	Time
DIAG	Pass	6:59am
AIR BLK	.00	7:00am
ACCY CHK	.08	7:01am
AIR BLK	.00	7:02am
SUB TEST	.00	7:03am
AIR BLK	.00	7:03am
SUB TEST	.00	7:05am
AIR BLK	.00	7:06am

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

CABARRUS COUNTY BAT MOBILE UNIT 8 120

Serial Number: 008775 Test Record Number: 2449
Test Date: 02/11/2026 Test Time: 7:08am EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	7:08am
FLO	Pass	7:08am
FC	Pass	7:08am

Temperature Tests

Test	Status	Time
FC1	Pass	7:08am
SRC	Pass	7:08am
DET	Pass	7:08am
BAR	Pass	7:08am
BT	Pass	7:08am

Blank Tests

Test	Status	Time
AIR	Pass	7:09am

Printer Tests

Test	Status	Time
PRNT	Pass	7:09am

CRC Tests

Test	Status	Time
COMP	Pass	7:09am
CAL	Pass	7:09am

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Cabarrus Instrument Location BAT Mobile Unit 8

Instrument Serial No. 008775 -

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 11 day of February, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

2219283
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

CABARRUS COUNTY BAT MOBILE UNIT 8 120

Serial Number: 008775

Test Date: 02/11/2026

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Glasscock, Jerry D

Permit Number: 7180-9235

Effective:

02/01/2026-02/01/2028

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG506303

Exp Date: 03/04/2027

Test	g/210L	Time
DIAG	Pass	6:59am
AIR BLK	.00	7:00am
ACCY CHK	.08	7:01am
AIR BLK	.00	7:02am
SUB TEST	.00	7:03am
AIR BLK	.00	7:03am
SUB TEST	.00	7:05am
AIR BLK	.00	7:06am

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

Intox EC/IR-II: Preventive Maintenance

CABARRUS COUNTY BAT MOBILE UNIT 8 120

Serial Number: 008775 Test Record Number: 2449
Test Date: 02/11/2026 Test Time: 7:08am EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	7:08am
FLO	Pass	7:08am
FC	Pass	7:08am

Temperature Tests

Test	Status	Time
FC1	Pass	7:08am
SRC	Pass	7:08am
DET	Pass	7:08am
BAR	Pass	7:08am
BT	Pass	7:08am

Blank Tests

Test	Status	Time
AIR	Pass	7:09am

Printer Tests

Test	Status	Time
PRNT	Pass	7:09am

CRC Tests

Test	Status	Time
COMP	Pass	7:09am
CAL	Pass	7:09am

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)


County Cabarrus Instrument Location BAT Mobile Unit 8

Instrument Serial No. 008775 —

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 26 day of February, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

2219283
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

CABARRUS COUNTY BAT MOBILE UNIT 8 120

Serial Number: 008775
Test Date: 02/26/2026

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: Glasscock, Jerry D
Permit Number: 7180-9235
Effective:
02/01/2026-02/01/2028

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG506303
Exp Date: 03/04/2027

Test	g/210L	Time
DIAG	Pass	1:49pm
AIR BLK	.00	1:50pm
ACCY CHK	.08	1:51pm
AIR BLK	.00	1:52pm
SUB TEST	.00	1:52pm
AIR BLK	.00	1:53pm
SUB TEST	.00	1:55pm
AIR BLK	.00	1:56pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

Intox EC/IR-II: Preventive Maintenance

CABARRUS COUNTY BAT MOBILE UNIT 8 120

Serial Number: 008775 Test Record Number: 2462
Test Date: 02/26/2026 Test Time: 1:56pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	1:57pm
FLO	Pass	1:57pm
FC	Pass	1:57pm

Temperature Tests

Test	Status	Time
FC1	Pass	1:57pm
SRC	Pass	1:57pm
DET	Pass	1:57pm
BAR	Pass	1:57pm
BT	Pass	1:57pm

Blank Tests

Test	Status	Time
AIR	Pass	1:58pm

Printer Tests

Test	Status	Time
PRNT	Pass	1:58pm

CRC Tests

Test	Status	Time
COMP	Pass	1:58pm
CAL	Pass	1:58pm

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH


**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County Cabarrus Instrument Location BAT Mobile Unit 8
Instrument Serial No. 008316 _____

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 8 day of February, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official
2219283
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

CABARRUS COUNTY BAT MOBILE UNIT 8 120

Serial Number: 008816

Test Date: 02/08/2026

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Glasscock, Jerry D

Permit Number: 7180-9235

Effective:

02/01/2026-02/01/2028

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG431002

Exp Date: 11/05/2026

Test	g/210L	Time
DIAG	Pass	8:08pm
AIR BLK	.00	8:09pm
ACCY CHK	.07	8:10pm
AIR BLK	.00	8:11pm
SUB TEST	.00	8:12pm
AIR BLK	.00	8:13pm
SUB TEST	.00	8:14pm
AIR BLK	.00	8:15pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

CABARRUS COUNTY BAT MOBILE UNIT 8 120

Serial Number: 008816 Test Record Number: 8031
Test Date: 02/08/2026 Test Time: 8:16pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	8:16pm
FLO	Pass	8:16pm
FC	Pass	8:16pm

Temperature Tests

Test	Status	Time
FC1	Pass	8:17pm
SRC	Pass	8:17pm
DET	Pass	8:17pm
BAR	Pass	8:17pm
BT	Pass	8:17pm

Blank Tests

Test	Status	Time
AIR	Pass	8:17pm

Printer Tests

Test	Status	Time
PRNT	Pass	8:17pm

CRC Tests

Test	Status	Time
COMP	Pass	8:17pm
CAL	Pass	8:17pm

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Cabarrus Instrument Location BAT Mobile Unit 8
Instrument Serial No. 008816 _____

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 11 day of February, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

2219283
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

CABARRUS COUNTY BAT MOBILE UNIT 8 120

Serial Number: 008816
Test Date: 02/11/2026

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Glasscock, Jerry D

Permit Number: 7180-9235

Effective:

02/01/2026-02/01/2028

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG431002

Exp Date: 11/05/2026

Test	g/210L	Time
DIAG	Pass	6:58am
AIR BLK	.00	6:59am
ACCY CHK	.08	7:00am
AIR BLK	.00	7:01am
SUB TEST	.00	7:02am
AIR BLK	.00	7:03am
SUB TEST	.00	7:04am
AIR BLK	.00	7:05am

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

CABARRUS COUNTY BAT MOBILE UNIT 8 120

Serial Number: 008816 Test Record Number: 8033
Test Date: 02/11/2026 Test Time: 7:06am EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	7:07am
FLO	Pass	7:07am
FC	Pass	7:07am

Temperature Tests

Test	Status	Time
FC1	Pass	7:07am
SRC	Pass	7:07am
DET	Pass	7:07am
BAR	Pass	7:07am
BT	Pass	7:07am

Blank Tests

Test	Status	Time
AIR	Pass	7:07am

Printer Tests

Test	Status	Time
PRNT	Pass	7:08am

CRC Tests

Test	Status	Time
COMP	Pass	7:08am
CAL	Pass	7:08am

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Cabarrus Instrument Location BAT Mobile Unit 8

Instrument Serial No. 008929 —

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 8 day of February, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

2219283
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

CABARRUS COUNTY BAT MOBILE UNIT 8 120

Serial Number: 008929

Test Date: 02/08/2026

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Glasscock, Jerry D

Permit Number: 7180-9235

Effective:

02/01/2026-02/01/2028

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG506303

Exp Date: 03/04/2027

Test	g/210L	Time
DIAG	Pass	8:08pm
AIR BLK	.00	8:09pm
ACCY CHK	.08	8:10pm
AIR BLK	.00	8:11pm
SUB TEST	.00	8:11pm
AIR BLK	.00	8:13pm
SUB TEST	.00	8:14pm
AIR BLK	.00	8:15pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

CABARRUS COUNTY BAT MOBILE UNIT 8 120

Serial Number: 008929 Test Record Number: 1733
Test Date: 02/08/2026 Test Time: 8:16pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	8:17pm
FLO	Pass	8:17pm
FC	Pass	8:17pm

Temperature Tests

Test	Status	Time
FC1	Pass	8:17pm
SRC	Pass	8:17pm
DET	Pass	8:17pm
BAR	Pass	8:17pm
BT	Pass	8:17pm

Blank Tests

Test	Status	Time
AIR	Pass	8:18pm

Printer Tests

Test	Status	Time
PRNT	Pass	8:18pm

CRC Tests

Test	Status	Time
COMP	Pass	8:18pm
CAL	Pass	8:18pm

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County Cabarrus Instrument Location BAT Mobile Unit 8
Instrument Serial No. 608929 —

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 11 day of February, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

2219283
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

CABARRUS COUNTY BAT MOBILE UNIT 8 120

Serial Number: 008929

Test Date: 02/11/2026

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Glasscock, Jerry D

Permit Number: 7180-9235

Effective:

02/01/2026-02/01/2028

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG506303

Exp Date: 03/04/2027

Test	g/210L	Time
DIAG	Pass	6:59am
AIR BLK	.00	7:00am
ACCY CHK	.08	7:01am
AIR BLK	.00	7:02am
SUB TEST	.00	7:02am
AIR BLK	.00	7:04am
SUB TEST	.00	7:05am
AIR BLK	.00	7:06am

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

CABARRUS COUNTY BAT MOBILE UNIT 8 120

Serial Number: 008929 Test Record Number: 1735
Test Date: 02/11/2026 Test Time: 7:07am EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	7:08am
FLO	Pass	7:08am
FC	Pass	7:08am

Temperature Tests

Test	Status	Time
FC1	Pass	7:08am
SRC	Pass	7:08am
DET	Pass	7:08am
BAR	Pass	7:08am
BT	Pass	7:08am

Blank Tests

Test	Status	Time
AIR	Pass	7:09am

Printer Tests

Test	Status	Time
PRNT	Pass	7:09am

CRC Tests

Test	Status	Time
COMP	Pass	7:09am
CAL	Pass	7:09am

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Cabarrus Instrument Location BAT Mobile Unit 8

Instrument Serial No. 008929

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 26 day of February, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

2219283
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

CABARRUS COUNTY BAT MOBILE UNIT 8 120

Serial Number: 008929
Test Date: 02/26/2026

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Glasscock, Jerry D

Permit Number: 7180-9235

Effective:

02/01/2026-02/01/2028

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG506303

Exp Date: 03/04/2027

Test	g/210L	Time
DIAG	Pass	1:46pm
AIR BLK	.00	1:47pm
ACCY CHK	.08	1:48pm
AIR BLK	.00	1:49pm
SUB TEST	.00	1:50pm
AIR BLK	.00	1:51pm
SUB TEST	.00	1:53pm
AIR BLK	.00	1:54pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

CABARRUS COUNTY BAT MOBILE UNIT 8 120

Serial Number: 008929 Test Record Number: 1748
Test Date: 02/26/2026 Test Time: 1:55pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	1:55pm
FLO	Pass	1:55pm
FC	Pass	1:56pm

Temperature Tests

Test	Status	Time
FC1	Pass	1:56pm
SRC	Pass	1:56pm
DET	Pass	1:56pm
BAR	Pass	1:56pm
BT	Pass	1:56pm

Blank Tests

Test	Status	Time
AIR	Pass	1:56pm

Printer Tests

Test	Status	Time
PRNT	Pass	1:56pm

CRC Tests

Test	Status	Time
COMP	Pass	1:57pm
CAL	Pass	1:57pm

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County CALDWELL Instrument Location CALDWELL CO. JAIL

Instrument Serial No. 008719 LENOIR NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 04 day of FEBRUARY, 2020 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

274970
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

CALDWELL COUNTY CALDWELL COUNTY JAIL
130

Serial Number: 008719
Test Date: 02/04/2026

Citation Number: M0000000-0
Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Fleming, Tina S

Permit Number: 0027-4970

Effective:

02/01/2025-02/01/2027

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG431001

Exp Date: 11/05/2026


Test	g/210L	Time
DIAG	Pass	11:01am
AIR BLK	.00	11:02am
ACCY CHK	.08	11:02am
AIR BLK	.00	11:04am
SUB TEST	.00	11:04am
AIR BLK	.00	11:05am
SUB TEST	.00	11:07am
AIR BLK	.00	11:07am

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

CALDWELL COUNTY CALDWELL COUNTY JAIL 130

Serial Number: 008719 Test Record Number: 3637
Test Date: 02/04/2026 Test Time: 11:09am EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	11:09am
FLO	Pass	11:09am
FC	Pass	11:10am

Temperature Tests

Test	Status	Time
FC1	Pass	11:10am
SRC	Pass	11:10am
DET	Pass	11:10am
BAR	Pass	11:10am
BT	Pass	11:10am

Blank Tests

Test	Status	Time
AIR	Pass	11:10am


Printer Tests

Test	Status	Time
PRNT	Pass	11:10am

CRC Tests

Test	Status	Time
COMP	Pass	11:10am
CAL	Pass	11:10am

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County CALDWELL Instrument Location CALDWELL CO. JAIL

Instrument Serial No. 008803 LENOIR NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 04 day of FEBRUARY, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Jim S. Steung
Signature of Certifying Official

274970
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

CALDWELL COUNTY CALDWELL COUNTY JAIL
130

Serial Number: 008803
Test Date: 02/04/2026

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: Fleming, Tina S
Permit Number: 0027-4970
Effective:
02/01/2025-02/01/2027

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG506302
Exp Date: 03/04/2027


Test	g/210L	Time
DIAG	Pass	11:02am
AIR BLK	.00	11:03am
ACCY CHK	.07	11:04am
AIR BLK	.00	11:05am
SUB TEST	.00	11:06am
AIR BLK	.00	11:07am
SUB TEST	.00	11:08am
AIR BLK	.00	11:09am

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

CALDWELL COUNTY CALDWELL COUNTY JAIL 130

Serial Number: 008803 Test Record Number: 911
Test Date: 02/04/2026 Test Time: 11:10am EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	11:10am
FLO	Pass	11:10am
FC	Pass	11:10am

Temperature Tests

Test	Status	Time
FC1	Pass	11:10am
SRC	Pass	11:10am
DET	Pass	11:10am
BAR	Pass	11:10am
BT	Pass	11:10am

Blank Tests

Test	Status	Time
AIR	Pass	11:11am

Printer Tests

Test	Status	Time
PRNT	Pass	11:11am

CRC Tests

Test	Status	Time
COMP	Pass	11:11am
CAL	Pass	11:11am

Preventive Maintenance
Status: Pass



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Caldwell Instrument Location BAT Mobile Unit II

Instrument Serial No. 008970

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 19th day of February, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

062446
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

CALDWELL COUNTY BAT MOBILE UNIT 11 130

Serial Number: 008970
Test Date: 02/19/2026

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE

Analyst's Name: Gillstrap, Jeffrey L
Permit Number: 0006-2446
Effective:
04/01/2025-04/01/2027

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG417802
Exp Date: 06/26/2026

Test	g/210L	Time
DIAG	Pass	9:14pm
AIR BLK	.00	9:15pm
ACCY CHK	.07	9:16pm
AIR BLK	.00	9:17pm
SUB TEST	.00	9:17pm
AIR BLK	.00	9:18pm
SUB TEST	.00	9:20pm
AIR BLK	.00	9:21pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

Intox EC/IR-II: Preventive Maintenance

CALDWELL COUNTY BAT MOBILE UNIT 11 130

Serial Number: 008970 Test Record Number: 1372
Test Date: 02/19/2026 Test Time: 9:21pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	9:22pm
FLO	Pass	9:22pm
FC	Pass	9:22pm

Temperature Tests

Test	Status	Time
FC1	Pass	9:22pm
SRC	Pass	9:22pm
DET	Pass	9:22pm
BAR	Pass	9:22pm
BT	Pass	9:22pm

Blank Tests

Test	Status	Time
AIR	Pass	9:23pm

Printer Tests

Test	Status	Time
PRNT	Pass	9:23pm

CRC Tests

Test	Status	Time
COMP	Pass	9:23pm
CAL	Pass	9:23pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County Caldwell Instrument Location BAT Mobile Unit 11

Instrument Serial No. 008970

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 26th day of February, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Jeff Bittling
Signature of Certifying Official

062446
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

CALDWELL COUNTY BAT MOBILE UNIT 11 130

Serial Number: 008970
Test Date: 02/26/2026

Citation Number: M0000000-0
Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Gillstrap, Jeffrey L

Permit Number: 0006-2446

Effective:

04/01/2025-04/01/2027

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG417802

Exp Date: 06/26/2026

Test	g/210L	Time
DIAG	Pass	9:05pm
AIR BLK	.00	9:06pm
ACCY CHK	.07	9:07pm
AIR BLK	.00	9:08pm
SUB TEST	.00	9:09pm
AIR BLK	.00	9:09pm
SUB TEST	.00	9:11pm
AIR BLK	.00	9:12pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

CALDWELL COUNTY BAT MOBILE UNIT 11 130

Serial Number: 008970 Test Record Number: 1383
Test Date: 02/26/2026 Test Time: 9:13pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	9:13pm
FLO	Pass	9:13pm
FC	Pass	9:13pm

Temperature Tests

Test	Status	Time
FC1	Pass	9:13pm
SRC	Pass	9:13pm
DET	Pass	9:13pm
BAR	Pass	9:13pm
BT	Pass	9:13pm

Blank Tests

Test	Status	Time
AIR	Pass	9:14pm

Printer Tests

Test	Status	Time
PRNT	Pass	9:14pm

CRC Tests

Test	Status	Time
COMP	Pass	9:14pm
CAL	Pass	9:14pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Caldwell Instrument Location BAT Mobile Unit 11

Instrument Serial No. 008973

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 19th day of February, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

062446
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

CALDWELL COUNTY BAT MOBILE UNIT 11 130

Serial Number: 008973
Test Date: 02/19/2026

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Gillstrap, Jeffrey L

Permit Number: 0006-2446

Effective:

04/01/2025-04/01/2027

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG431003

Exp Date: 11/05/2026

Test	g/210L	Time
DIAG	Pass	9:20pm
AIR BLK	.00	9:21pm
ACCY CHK	.07	9:21pm
AIR BLK	.00	9:22pm
SUB TEST	.00	9:23pm
AIR BLK	.00	9:24pm
SUB TEST	.00	9:25pm
AIR BLK	.00	9:26pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

Intox EC/IR-II: Preventive Maintenance

CALDWELL COUNTY BAT MOBILE UNIT 11 130

Serial Number: 008973 Test Record Number: 1423
Test Date: 02/19/2026 Test Time: 9:27pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	9:27pm
FLO	Pass	9:27pm
FC	Pass	9:27pm

Temperature Tests

Test	Status	Time
FC1	Pass	9:27pm
SRC	Pass	9:27pm
DET	Pass	9:27pm
BAR	Pass	9:27pm
BT	Pass	9:27pm

Blank Tests

Test	Status	Time
AIR	Pass	9:28pm

Printer Tests

Test	Status	Time
PRNT	Pass	9:28pm

CRC Tests

Test	Status	Time
COMP	Pass	9:28pm
CAL	Pass	9:28pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County Caldwell Instrument Location BAT Mobile Unit 11

Instrument Serial No. 008973

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 26th day of February, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

062446
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

CALDWELL COUNTY BAT MOBILE UNIT 11 130

Serial Number: 008973
Test Date: 02/26/2026

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE

Analyst's Name: Gillstrap, Jeffrey L
Permit Number: 0006-2446
Effective:
04/01/2025-04/01/2027

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG431003
Exp Date: 11/05/2026


Test	g/210L	Time
DIAG	Pass	9:09pm
AIR BLK	.00	9:10pm
ACCY CHK	.07	9:10pm
AIR BLK	.00	9:11pm
SUB TEST	.00	9:12pm
AIR BLK	.00	9:13pm
SUB TEST	.00	9:14pm
AIR BLK	.00	9:15pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

CALDWELL COUNTY BAT MOBILE UNIT 11 130

Serial Number: 008973 Test Record Number: 1434
Test Date: 02/26/2026 Test Time: 9:16pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	9:17pm
FLO	Pass	9:17pm
FC	Pass	9:17pm

Temperature Tests

Test	Status	Time
FC1	Pass	9:17pm
SRC	Pass	9:17pm
DET	Pass	9:17pm
BAR	Pass	9:17pm
BT	Pass	9:17pm

Blank Tests

Test	Status	Time
AIR	Pass	9:18pm

Printer Tests

Test	Status	Time
PRNT	Pass	9:18pm

CRC Tests

Test	Status	Time
COMP	Pass	9:18pm
CAL	Pass	9:18pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County CARTERET Instrument Location CARTERET COUNTY
Instrument Serial No. 008605 DETENTION CENTER

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 9th day of FEBRUARY, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

2824950
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

CARTERET COUNTY DETENTION CENTER 150

Serial Number: 008605
Test Date: 02/09/2026

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE

Analyst's Name: GILLESPIE, PENTTI W
Permit Number: 9523-2149
Effective:
02/01/2026-02/01/2028

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG516203
Exp Date: 06/11/2027

Test	g/210L	Time
DIAG	Pass	3:07pm
AIR BLK	.00	3:07pm
ACCY CHK	.07	3:08pm
AIR BLK	.00	3:10pm
SUB TEST	.00	3:10pm
AIR BLK	.00	3:11pm
SUB TEST	.00	3:12pm
AIR BLK	.00	3:13pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

CARTERET COUNTY DETENTION CENTER 150

Serial Number: 008605 Test Record Number: 4683
Test Date: 02/09/2026 Test Time: 3:14pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	3:14pm
FLO	Pass	3:14pm
FC	Pass	3:14pm

Temperature Tests

Test	Status	Time
FC1	Pass	3:14pm
SRC	Pass	3:14pm
DET	Pass	3:14pm
BAR	Pass	3:14pm
BT	Pass	3:14pm

Blank Tests

Test	Status	Time
AIR	Pass	3:15pm

Printer Tests

Test	Status	Time
PRNT	Pass	3:15pm

CRC Tests

Test	Status	Time
COMP	Pass	3:15pm
CAL	Pass	3:15pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County CARTERET Instrument Location EMERALD ISLE
Instrument Serial No. 008620 POLICE DEPT

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 9th day of FEBRUARY, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.





Signature of Certifying Official

2824950

Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

CARTERET COUNTY EMERALD ISLE PD 150

Serial Number: 008620
Test Date: 02/09/2026

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: GILLESPIE, PENTTI W

Permit Number: 9523-2149

Effective:

02/01/2026-02/01/2028

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG534301

Exp Date: 12/09/2027

Test	g/210L	Time
DIAG	Pass	11:03am
AIR BLK	.00	11:04am
ACCY CHK	.08	11:04am
AIR BLK	.00	11:06am
SUB TEST	.00	11:06am
AIR BLK	.00	11:07am
SUB TEST	.00	11:09am
AIR BLK	.00	11:10am

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

CARTERET COUNTY EMERALD ISLE PD 150

Serial Number: 008620 Test Record Number: 2648
Test Date: 02/09/2026 Test Time: 11:10am EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	11:10am
FLO	Pass	11:10am
FC	Pass	11:10am

Temperature Tests

Test	Status	Time
FC1	Pass	11:11am
SRC	Pass	11:11am
DET	Pass	11:11am
BAR	Pass	11:11am
BT	Pass	11:11am

Blank Tests

Test	Status	Time
AIR	Pass	11:11am

Printer Tests

Test	Status	Time
PRNT	Pass	11:11am

CRC Tests

Test	Status	Time
COMP	Pass	11:11am
CAL	Pass	11:11am

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County CARTERET Instrument Location MOREHEAD CITY
Instrument Serial No. 008731 POLICE DEPT

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 9th day of FEBRUARY, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

2824950

Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

CARTERET COUNTY MOREHEAD CITY PD 150

Serial Number: 008731
Test Date: 02/09/2026

Citation Number: M0000000-0
Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: GILLESPIE, PENTTI W

Permit Number: 9523-2149

Effective:

02/01/2026-02/01/2028

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG534301

Exp Date: 12/09/2027

Test	g/210L	Time
DIAG	Pass	2:13pm
AIR BLK	.00	2:14pm
ACCY CHK	.08	2:15pm
AIR BLK	.00	2:16pm
SUB TEST	.00	2:16pm
AIR BLK	.00	2:17pm
SUB TEST	.00	2:19pm
AIR BLK	.00	2:19pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

CARTERET COUNTY MOREHEAD CITY PD 150

Serial Number: 008731 Test Record Number: 2900
Test Date: 02/09/2026 Test Time: 2:20pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	2:20pm
FLO	Pass	2:20pm
FC	Pass	2:20pm

Temperature Tests

Test	Status	Time
FC1	Pass	2:20pm
SRC	Pass	2:20pm
DET	Pass	2:20pm
BAR	Pass	2:20pm
BT	Pass	2:20pm

Blank Tests

Test	Status	Time
AIR	Pass	2:21pm

Printer Tests

Test	Status	Time
PRNT	Pass	2:21pm

CRC Tests

Test	Status	Time
COMP	Pass	2:21pm
CAL	Pass	2:21pm

Preventive Maintenance
Status: *Pass*



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County CARTERET Instrument Location ATLANTIC BEACH

Instrument Serial No. 008785 POLICE DEPT

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 12th day of FEBRUARY, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Handwritten Signature]
Signature of Certifying Official

2824950
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

CARTERET COUNTY ATLANTIC BEACH PD 150

Serial Number: 008785
Test Date: 02/12/2026

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: GILLESPIE, PENTTI W
Permit Number: 9523-2149
Effective:
02/01/2026-02/01/2028

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG506303
Exp Date: 03/04/2027

Test	g/210L	Time
DIAG	Pass	4:02pm
AIR BLK	.00	4:03pm
ACCY CHK	.08	4:03pm
AIR BLK	.00	4:05pm
SUB TEST	.00	4:05pm
AIR BLK	.00	4:06pm
SUB TEST	.00	4:08pm
AIR BLK	.00	4:09pm

Reported AC: .00 g/210L

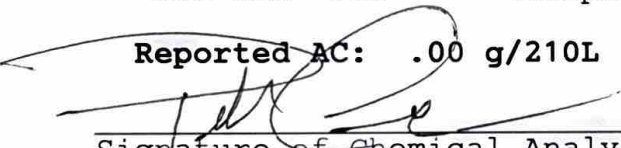

Signature of Chemical Analyst

Court CVR



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

CARTERET COUNTY ATLANTIC BEACH PD 150

Serial Number: 008785 Test Record Number: 1667
Test Date: 02/12/2026 Test Time: 4:09pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	4:09pm
FLO	Pass	4:09pm
FC	Pass	4:09pm

Temperature Tests

Test	Status	Time
FC1	Pass	4:09pm
SRC	Pass	4:09pm
DET	Pass	4:09pm
BAR	Pass	4:09pm
BT	Pass	4:09pm

Blank Tests

Test	Status	Time
AIR	Pass	4:10pm


Printer Tests

Test	Status	Time
PRNT	Pass	4:10pm

CRC Tests

Test	Status	Time
COMP	Pass	4:10pm
CAL	Pass	4:10pm

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County CARTERET Instrument Location CARTERET COUNTY


Instrument Serial No. 008882 DETENTION CENTER

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 9th day of FEBRUARY, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.

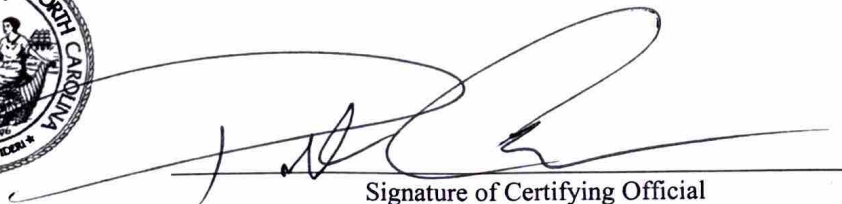


Signature of Certifying Official

2824950

Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

CARTERET COUNTY DETENTION CENTER 150

Serial Number: 008882
Test Date: 02/09/2026

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE

Analyst's Name: GILLESPIE, PENTTI W
Permit Number: 9523-2149
Effective:
02/01/2026-02/01/2028

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG516203
Exp Date: 06/11/2027

Test	g/210L	Time
DIAG	Pass	3:05pm
AIR BLK	.00	3:06pm
ACCY CHK	.08	3:06pm
AIR BLK	.00	3:07pm
SUB TEST	.00	3:08pm
AIR BLK	.00	3:09pm
SUB TEST	.00	3:10pm
AIR BLK	.00	3:11pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

CARTERET COUNTY DETENTION CENTER 150

Serial Number: 008882 Test Record Number: 2747
Test Date: 02/09/2026 Test Time: 3:11pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	3:12pm
FLO	Pass	3:12pm
FC	Pass	3:12pm

Temperature Tests

Test	Status	Time
FC1	Pass	3:12pm
SRC	Pass	3:12pm
DET	Pass	3:12pm
BAR	Pass	3:12pm
BT	Pass	3:12pm

Blank Tests

Test	Status	Time
AIR	Pass	3:13pm


Printer Tests

Test	Status	Time
PRNT	Pass	3:13pm

CRC Tests

Test	Status	Time
COMP	Pass	3:13pm
CAL	Pass	3:13pm

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County CATAWBA Instrument Location HICKORY RD

Instrument Serial No. 008221 HICKORY NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 01 day of FEBRUARY, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

2749710
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

CATAWBA COUNTY HICKORY PD 170

Serial Number: 008841
Test Date: 02/04/2026

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Fleming, Tina S

Permit Number: 0027-4970

Effective:

02/01/2025-02/01/2027

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG534301

Exp Date: 12/09/2027

Test	g/210L	Time
DIAG	Pass	1:42pm
AIR BLK	.00	1:43pm
ACCY CHK	.08	1:44pm
AIR BLK	.00	1:45pm
SUB TEST	.00	1:46pm
AIR BLK	.00	1:47pm
SUB TEST	.00	1:48pm
AIR BLK	.00	1:49pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

CATAWBA COUNTY HICKORY PD 170

Serial Number: 008841 Test Record Number: 2594
Test Date: 02/04/2026 Test Time: 1:52pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	1:52pm
FLO	Pass	1:52pm
FC	Pass	1:52pm

Temperature Tests

Test	Status	Time
FC1	Pass	1:52pm
SRC	Pass	1:52pm
DET	Pass	1:52pm
BAR	Pass	1:52pm
BT	Pass	1:52pm

Blank Tests

Test	Status	Time
AIR	Pass	1:53pm


Printer Tests

Test	Status	Time
PRNT	Pass	1:53pm

CRC Tests

Test	Status	Time
COMP	Pass	1:53pm
CAL	Pass	1:53pm

Preventive Maintenance
Status: Pass

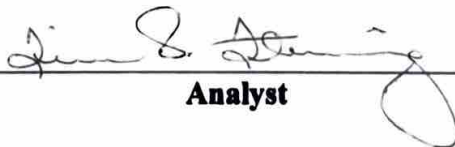

Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)


County Columbus Instrument Location BAT Mobile Unit 9
Instrument Serial No. 00 8575

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 27th day of February, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.

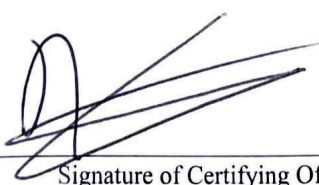


Signature of Certifying Official

2266313
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

COLUMBUS COUNTY BAT MOBILE UNIT 9 230

Serial Number: 008575
Test Date: 02/27/2026

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE

Analyst's Name: Sharpe Jr., Robert J
Permit Number: 1820-8591
Effective:
02/01/2026-02/01/2028

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG516204
Exp Date: 06/11/2027

Test	g/210L	Time
DIAG	Pass	7:24pm
AIR BLK	.00	7:25pm
ACCY CHK	.08	7:25pm
AIR BLK	.00	7:26pm
SUB TEST	.00	7:27pm
AIR BLK	.00	7:28pm
SUB TEST	.00	7:30pm
AIR BLK	.00	7:31pm

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

COLUMBUS COUNTY BAT MOBILE UNIT 9 230

Serial Number: 008575 Test Record Number: 1533
Test Date: 02/27/2026 Test Time: 7:32pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	7:32pm
FLO	Pass	7:32pm
FC	Pass	7:33pm

Temperature Tests

Test	Status	Time
FC1	Pass	7:33pm
SRC	Pass	7:33pm
DET	Pass	7:33pm
BAR	Pass	7:33pm
BT	Pass	7:33pm

Blank Tests

Test	Status	Time
AIR	Pass	7:33pm

Printer Tests

Test	Status	Time
PRNT	Pass	7:33pm

CRC Tests

Test	Status	Time
COMP	Pass	7:33pm
CAL	Pass	7:33pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**


County Columbus Instrument Location BAT Mobile Unit 9

Instrument Serial No. 008616

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 27th day of February, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

2266313
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

COLUMBUS COUNTY BAT MOBILE UNIT 9 230

Serial Number: 008616
Test Date: 02/27/2026

Citation Number: M0000000-0
Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Sharpe Jr., Robert J

Permit Number: 1820-8591

Effective:

02/01/2026-02/01/2028

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG506303

Exp Date: 03/04/2027

Test	g/210L	Time
DIAG	Pass	7:26pm
AIR BLK	.00	7:27pm
ACCY CHK	.08	7:28pm
AIR BLK	.00	7:29pm
SUB TEST	.00	7:30pm
AIR BLK	.00	7:31pm
SUB TEST	.00	7:32pm
AIR BLK	.00	7:33pm

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR

Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

COLUMBUS COUNTY BAT MOBILE UNIT 9 230

Serial Number: 008616 Test Record Number: 2930
Test Date: 02/27/2026 Test Time: 7:35pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	7:35pm
FLO	Pass	7:35pm
FC	Pass	7:35pm

Temperature Tests

Test	Status	Time
FC1	Pass	7:35pm
SRC	Pass	7:35pm
DET	Pass	7:35pm
BAR	Pass	7:35pm
BT	Pass	7:35pm

Blank Tests

Test	Status	Time
AIR	Pass	7:36pm

Printer Tests

Test	Status	Time
PRNT	Pass	7:36pm

CRC Tests

Test	Status	Time
COMP	Pass	7:36pm
CAL	Pass	7:36pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County Columbus Instrument Location BAT Mobile Unit 9

Instrument Serial No. 008647

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 27th day of February, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Handwritten Signature]

Signature of Certifying Official

2266313

Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

COLUMBUS COUNTY BAT MOBILE UNIT 9 230

Serial Number: 008647
Test Date: 02/27/2026

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Sharpe Jr., Robert J

Permit Number: 1820-8591

Effective:

02/01/2026-02/01/2028

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG516203

Exp Date: 06/11/2027

Test	g/210L	Time
DIAG	Pass	7:26pm
AIR BLK	.00	7:27pm
ACCY CHK	.08	7:28pm
AIR BLK	.00	7:29pm
SUB TEST	.00	7:30pm
AIR BLK	.00	7:30pm
SUB TEST	.00	7:32pm
AIR BLK	.00	7:33pm

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR

Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

COLUMBUS COUNTY BAT MOBILE UNIT 9 230

Serial Number: 008647 Test Record Number: 2921
Test Date: 02/27/2026 Test Time: 7:36pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	7:36pm
FLO	Pass	7:36pm
FC	Pass	7:36pm

Temperature Tests

Test	Status	Time
FC1	Pass	7:36pm
SRC	Pass	7:36pm
DET	Pass	7:36pm
BAR	Pass	7:36pm
BT	Pass	7:36pm

Blank Tests

Test	Status	Time
AIR	Pass	7:37pm

Printer Tests

Test	Status	Time
PRNT	Pass	7:37pm

CRC Tests

Test	Status	Time
COMP	Pass	7:37pm
CAL	Pass	7:37pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH


**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County Columbus Instrument Location BAT Mobile Unit 9
Instrument Serial No. 008704

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 27th day of February, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

2266313
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

COLUMBUS COUNTY BAT MOBILE UNIT 9 230

Serial Number: 008704
Test Date: 02/27/2026

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Sharpe Jr., Robert J

Permit Number: 1820-8591

Effective:

02/01/2026-02/01/2028

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG506303

Exp Date: 03/04/2027

Test	g/210L	Time
DIAG	Pass	7:26pm
AIR BLK	.00	7:27pm
ACCY CHK	.07	7:27pm
AIR BLK	.00	7:28pm
SUB TEST	.00	7:29pm
AIR BLK	.00	7:30pm
SUB TEST	.00	7:32pm
AIR BLK	.00	7:33pm

Reported AC: .00 g/210L

Signature  Chemical Analyst

Court CVR


Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

COLUMBUS COUNTY BAT MOBILE UNIT 9 230

Serial Number: 008704 Test Record Number: 970
Test Date: 02/27/2026 Test Time: 7:35pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	7:36pm
FLO	Pass	7:36pm
FC	Pass	7:36pm

Temperature Tests

Test	Status	Time
FC1	Pass	7:36pm
SRC	Pass	7:36pm
DET	Pass	7:36pm
BAR	Pass	7:36pm
BT	Pass	7:36pm

Blank Tests

Test	Status	Time
AIR	Pass	7:37pm

Printer Tests

Test	Status	Time
PRNT	Pass	7:37pm

CRC Tests

Test	Status	Time
COMP	Pass	7:37pm
CAL	Pass	7:37pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)


County Columbus Instrument Location BAT Mobile Unit 9

Instrument Serial No. 008826

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 27th day of February, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]

Signature of Certifying Official

2266313

Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

COLUMBUS COUNTY BAT MOBILE UNIT 9 230

Serial Number: 008826

Test Date: 02/27/2026

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Sharpe Jr., Robert J

Permit Number: 1820-8591

Effective:

02/01/2026-02/01/2028

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG516204

Exp Date: 06/11/2027

Test	g/210L	Time
DIAG	Pass	7:23pm
AIR BLK	.00	7:24pm
ACCY CHK	.07	7:25pm
AIR BLK	.00	7:25pm
SUB TEST	.00	7:26pm
AIR BLK	.00	7:27pm
SUB TEST	.00	7:29pm
AIR BLK	.00	7:30pm

Reported AS: .00 g/210L

Signature of Chemical Analyst

Court CVR


Analyst

Intox EC/IR-II: Preventive Maintenance

COLUMBUS COUNTY BAT MOBILE UNIT 9 230

Serial Number: 008826 Test Record Number: 8603
Test Date: 02/27/2026 Test Time: 7:31pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	7:32pm
FLO	Pass	7:32pm
FC	Pass	7:32pm

Temperature Tests

Test	Status	Time
FC1	Pass	7:32pm
SRC	Pass	7:32pm
DET	Pass	7:32pm
BAR	Pass	7:32pm
BT	Pass	7:32pm

Blank Tests

Test	Status	Time
AIR	Pass	7:32pm

Printer Tests

Test	Status	Time
PRNT	Pass	7:32pm

CRC Tests

Test	Status	Time
COMP	Pass	7:33pm
CAL	Pass	7:33pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**


County Craven Instrument Location BAT Mobile Unit 12

Instrument Serial No. 008601

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 20th day of February, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

2266313
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

CRAVEN COUNTY BAT MOBILE UNIT 12 240

Serial Number: 008601
Test Date: 02/20/2026

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Sharpe Jr., Robert J

Permit Number: 1820-8591

Effective:

02/01/2026-02/01/2028

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG501307

Exp Date: 01/13/2027

Test	g/210L	Time
DIAG	Pass	8:26pm
AIR BLK	.00	8:27pm
ACCY CHK	.08	8:27pm
AIR BLK	.00	8:28pm
SUB TEST	.00	8:29pm
AIR BLK	.00	8:30pm
SUB TEST	.00	8:31pm
AIR BLK	.00	8:32pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

CRAVEN COUNTY BAT MOBILE UNIT 12 240

Serial Number: 008601 Test Record Number: 1879
Test Date: 02/20/2026 Test Time: 8:33pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	8:33pm
FLO	Pass	8:33pm
FC	Pass	8:33pm

Temperature Tests

Test	Status	Time
FC1	Pass	8:33pm
SRC	Pass	8:33pm
DET	Pass	8:33pm
BAR	Pass	8:33pm
BT	Pass	8:33pm

Blank Tests

Test	Status	Time
AIR	Pass	8:34pm

Printer Tests

Test	Status	Time
PRNT	Pass	8:34pm

CRC Tests

Test	Status	Time
COMP	Pass	8:34pm
CAL	Pass	8:34pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**


County Craven Instrument Location BAT Mobile Unit 12

Instrument Serial No. 00 8788

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 20th day of February, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

2266313
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

CRAVEN COUNTY BAT MOBILE UNIT 12 240

Serial Number: 008788

Test Date: 02/20/2026

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Sharpe Jr., Robert J

Permit Number: 1820-8591

Effective:

02/01/2026-02/01/2028

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG417802

Exp Date: 06/26/2026

Test	g/210L	Time
DIAG	Pass	8:23pm
AIR BLK	.00	8:24pm
ACCY CHK	.08	8:25pm
AIR BLK	.00	8:26pm
SUB TEST	.00	8:26pm
AIR BLK	.00	8:27pm
SUB TEST	.00	8:28pm
AIR BLK	.00	8:29pm

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR

Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

CRAVEN COUNTY BAT MOBILE UNIT 12 240

Serial Number: 008788 Test Record Number: 2504
Test Date: 02/20/2026 Test Time: 8:31pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	8:31pm
FLO	Pass	8:31pm
FC	Pass	8:31pm

Temperature Tests

Test	Status	Time
FC1	Pass	8:31pm
SRC	Pass	8:31pm
DET	Pass	8:31pm
BAR	Pass	8:31pm
BT	Pass	8:31pm

Blank Tests

Test	Status	Time
AIR	Pass	8:32pm

Printer Tests

Test	Status	Time
PRNT	Pass	8:32pm

CRC Tests

Test	Status	Time
COMP	Pass	8:32pm
CAL	Pass	8:32pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)


County CRAVEN Instrument Location HAVELOCK

Instrument Serial No. 008800 POLICE DEPT

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 3rd day of FEBRUARY, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.

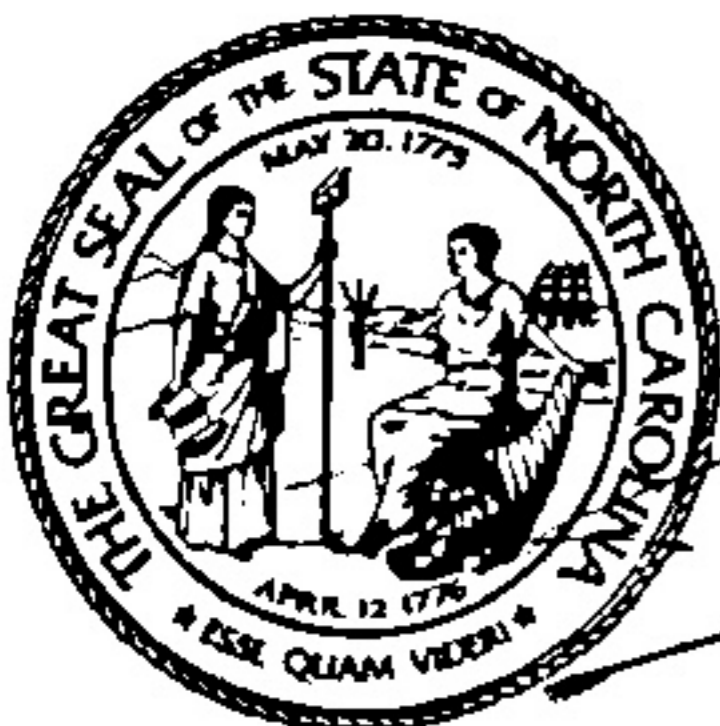

[Handwritten Signature]

Signature of Certifying Official

2824950

Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

CRAVEN COUNTY HAVELOCK PD 240

Serial Number: 008800
Test Date: 02/03/2026

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: GILLESPIE, PENTTI W

Permit Number: 9523-2149

Effective:

02/01/2026-02/01/2028

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG534301

Exp Date: 12/09/2027

Test	g/210L	Time
DIAG	Pass	9:33am
AIR BLK	.00	9:34am
ACCY CHK	.07	9:35am
AIR BLK	.00	9:36am
SUB TEST	.00	9:37am
AIR BLK	.00	9:38am
SUB TEST	.00	9:40am
AIR BLK	.00	9:41am

Reported AC: .00 g/210L

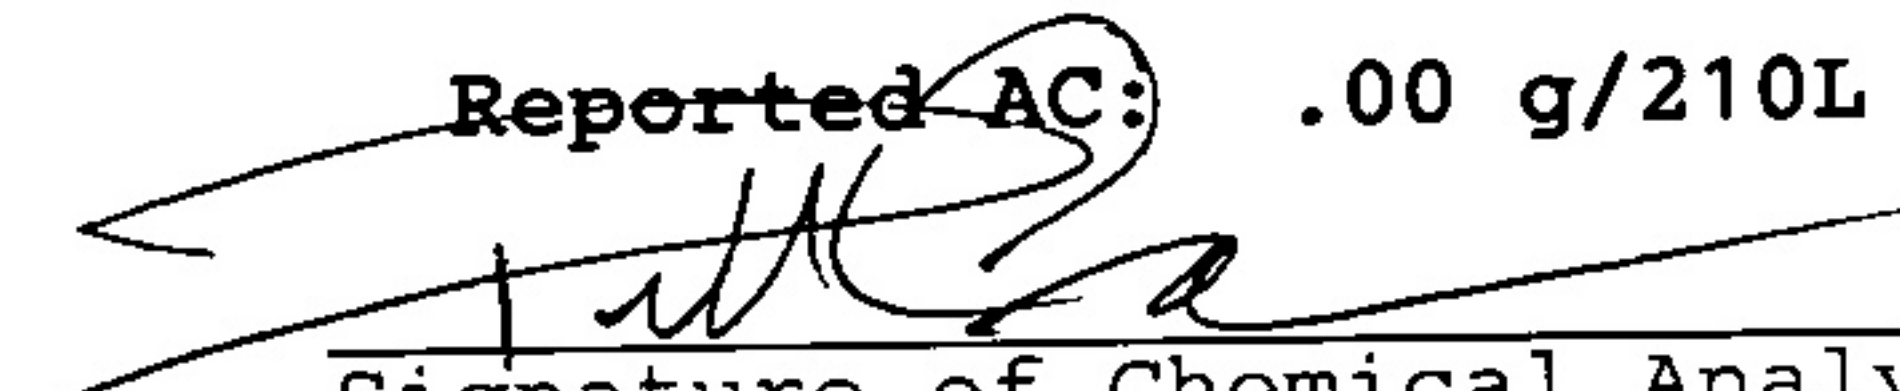
Signature of Chemical Analyst

Court CVR


Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

CRAVEN COUNTY HAVELOCK PD 240

Serial Number: 008800 Test Record Number: 1774
Test Date: 02/03/2026 Test Time: 9:41am EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	9:41am
FLO	Pass	9:41am
FC	Pass	9:41am

Temperature Tests

Test	Status	Time
FC1	Pass	9:41am
SRC	Pass	9:41am
DET	Pass	9:41am
BAR	Pass	9:41am
BT	Pass	9:41am

Blank Tests

Test	Status	Time
AIR	Pass	9:42am


Printer Tests

Test	Status	Time
PRNT	Pass	9:42am

CRC Tests

Test	Status	Time
COMP	Pass	9:42am
CAL	Pass	9:42am

Preventive Maintenance
Status: Pass



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County CRAVEN Instrument Location NEW BERN


Instrument Serial No. 008817 POLICE DEPT

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 3rd day of FEBRUARY, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.




Signature of Certifying Official

2824950
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

CRAVEN COUNTY NEW BERN PD 240

Serial Number: 008817
Test Date: 02/03/2026

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: GILLESPIE, PENTTI W
Permit Number: 9523-2149
Effective:
02/01/2026-02/01/2028

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG534301
Exp Date: 12/09/2027

Test	g/210L	Time
DIAG	Pass	3:05pm
AIR BLK	.00	3:05pm
ACCY CHK	.07	3:06pm
AIR BLK	.00	3:07pm
SUB TEST	.00	3:08pm
AIR BLK	.00	3:09pm
SUB TEST	.00	3:10pm
AIR BLK	.00	3:11pm

Reported AC; .00 g/210L

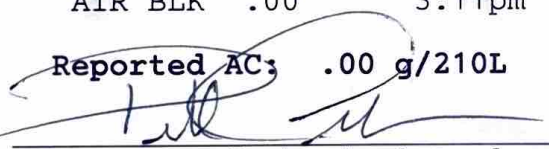

Signature of Chemical Analyst

Court CVR



Analyst

Intox EC/IR-II: Preventive Maintenance

CRAVEN COUNTY NEW BERN PD 240

Serial Number: 008817 Test Record Number: 2233
Test Date: 02/03/2026 Test Time: 3:12pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	3:12pm
FLO	Pass	3:12pm
FC	Pass	3:12pm

Temperature Tests

Test	Status	Time
FC1	Pass	3:12pm
SRC	Pass	3:12pm
DET	Pass	3:12pm
BAR	Pass	3:12pm
BT	Pass	3:12pm

Blank Tests

Test	Status	Time
AIR	Pass	3:13pm


Printer Tests

Test	Status	Time
PRNT	Pass	3:13pm

CRC Tests

Test	Status	Time
COMP	Pass	3:13pm
CAL	Pass	3:13pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County CRAVEN Instrument Location MCAS Pmo
Instrument Serial No. 010819 CHERRY POINT

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 3rd day of FEBRUARY, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



A large, stylized handwritten signature in black ink, written over a horizontal line.

Signature of Certifying Official

2824950

Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

CRAVEN COUNTY MCAS CHERRY POINT 240

Serial Number: 010819
Test Date: 02/03/2026

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: GILLESPIE, PENTTI W

Permit Number: 9523-2149

Effective:

02/01/2026-02/01/2028

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG534301

Exp Date: 12/09/2027

Test	g/210L	Time
DIAG	Pass	10:28am
AIR BLK	.00	10:29am
ACCY CHK	.07	10:29am
AIR BLK	.00	10:31am
SUB TEST	.00	10:32am
AIR BLK	.00	10:33am
SUB TEST	.00	10:34am
AIR BLK	.00	10:35am

~~Reported AC:~~ .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

CRAVEN COUNTY MCAS CHERRY POINT 240

Serial Number: 010819 Test Record Number: 978
Test Date: 02/03/2026 Test Time: 10:36am EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	10:36am
FLO	Pass	10:36am
FC	Pass	10:36am

Temperature Tests

Test	Status	Time
FC1	Pass	10:36am
SRC	Pass	10:36am
DET	Pass	10:36am
BAR	Pass	10:36am
BT	Pass	10:36am

Blank Tests

Test	Status	Time
AIR	Pass	10:37am


Printer Tests

Test	Status	Time
PRNT	Pass	10:37am

CRC Tests

Test	Status	Time
COMP	Pass	10:37am
CAL	Pass	10:37am

Preventive Maintenance
Status: *Pass*

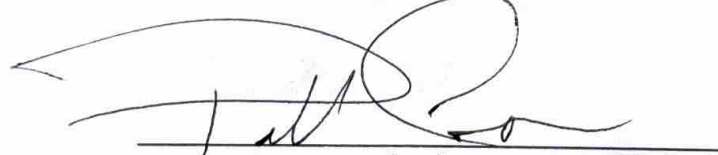

Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County Cumberland Instrument Location Cumberland County
Instrument Serial No. 008632 Detention Center

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 25 day of February, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

365156
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

CUMBERLAND COUNTY DETENTION CENTER 250

Serial Number: 008632
Test Date: 02/25/2026

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: Garner, Joel K
Permit Number: 0036-5156
Effective:
02/01/2026-02/01/2028

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG534301
Exp Date: 12/09/2027

Test	g/210L	Time
DIAG	Pass	9:48am
AIR BLK	.00	9:49am
ACCY CHK	.07	9:50am
AIR BLK	.00	9:51am
SUB TEST	.00	9:52am
AIR BLK	.00	9:53am
SUB TEST	.00	9:54am
AIR BLK	.00	9:55am

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

CUMBERLAND COUNTY DETENTION CENTER 250

Serial Number: 008632 Test Record Number: 5048
Test Date: 02/25/2026 Test Time: 10:01am EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	10:01am
FLO	Pass	10:01am
FC	Pass	10:01am

Temperature Tests

Test	Status	Time
FC1	Pass	10:01am
SRC	Pass	10:01am
DET	Pass	10:01am
BAR	Pass	10:01am
BT	Pass	10:01am

Blank Tests

Test	Status	Time
AIR	Pass	10:02am

Printer Tests

Test	Status	Time
PRNT	Pass	10:02am

CRC Tests

Test	Status	Time
COMP	Pass	10:02am
CAL	Pass	10:02am

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Cumberland Instrument Location Cumberland County
Instrument Serial No. 008672 Detention Center

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 25 day of February, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

365156
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

CUMBERLAND COUNTY DETENTION CENTER 250

Serial Number: 008672
Test Date: 02/25/2026

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: Garner, Joel K
Permit Number: 0036-5156
Effective:
02/01/2026-02/01/2028

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG534301
Exp Date: 12/09/2027

Test	g/210L	Time
DIAG	Pass	9:49am
AIR BLK	.00	9:50am
ACCY CHK	.07	9:51am
AIR BLK	.00	9:52am
SUB TEST	.00	9:53am
AIR BLK	.00	9:53am
SUB TEST	.00	9:55am
AIR BLK	.00	9:56am

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

Intox EC/IR-II: Preventive Maintenance

CUMBERLAND COUNTY DETENTION CENTER 250

Serial Number: 008672 Test Record Number: 8966
Test Date: 02/25/2026 Test Time: 10:10am EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	10:10am
FLO	Pass	10:10am
FC	Pass	10:11am

Temperature Tests

Test	Status	Time
FC1	Pass	10:11am
SRC	Pass	10:11am
DET	Pass	10:11am
BAR	Pass	10:11am
BT	Pass	10:11am

Blank Tests

Test	Status	Time
AIR	Pass	10:11am


Printer Tests

Test	Status	Time
PRNT	Pass	10:11am

CRC Tests

Test	Status	Time
COMP	Pass	10:11am
CAL	Pass	10:11am

Preventive Maintenance
Status: Pass

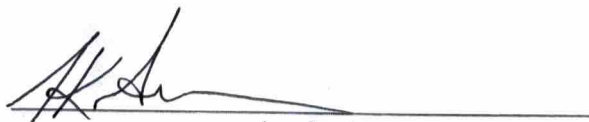

Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County Currituck Instrument Location Currituck Co. S.O. - Corolla
Instrument Serial No. 008949 1123 Ocean Trl., Corolla, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 5th day of February, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Mark A. Russell
Signature of Certifying Official

206272
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

CURRITUCK COUNTY SO-COROLLA 260

Serial Number: 008949
Test Date: 02/05/2026

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: Chappell, Mark A
Permit Number: 0020-6272
Effective:
02/01/2026-02/01/2028

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG501303
Exp Date: 01/13/2027

Test	g/210L	Time
DIAG	Pass	12:02pm
AIR BLK	.00	12:02pm
ACCY CHK	.08	12:03pm
AIR BLK	.00	12:05pm
SUB TEST	.00	12:05pm
AIR BLK	.00	12:06pm
SUB TEST	.00	12:08pm
AIR BLK	.00	12:09pm

Reported AC: .00 g/210L

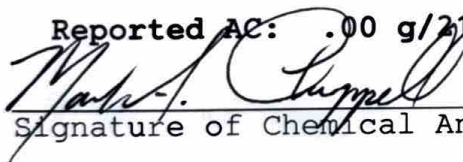

Signature of Chemical Analyst

Court CVR



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

CURRITUCK COUNTY SO-COROLLA 260

Serial Number: 008949 Test Record Number: 863
Test Date: 02/05/2026 Test Time: 12:12pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	12:13pm
FLO	Pass	12:13pm
FC	Pass	12:13pm

Temperature Tests

Test	Status	Time
FC1	Pass	12:13pm
SRC	Pass	12:13pm
DET	Pass	12:13pm
BAR	Pass	12:13pm
BT	Pass	12:13pm

Blank Tests

Test	Status	Time
AIR	Pass	12:13pm

Printer Tests

Test	Status	Time
PRNT	Pass	12:14pm

CRC Tests

Test	Status	Time
COMP	Pass	12:14pm
CAL	Pass	12:14pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County Dare Instrument Location Dare Co. S.O. - Buxton
Instrument Serial No. 008807 50347 Hwy. NC 12, Buxton,
NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 12th day of February, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Mark A. Pugh
Signature of Certifying Official

206272
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

DARE COUNTY DARE CO SO BUXTON 270

Serial Number: 008807
Test Date: 02/12/2026

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE

Analyst's Name: Chappell, Mark A
Permit Number: 0020-6272
Effective:
02/01/2026-02/01/2028

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG501303
Exp Date: 01/13/2027

Test	g/210L	Time
DIAG	Pass	11:23am
AIR BLK	.00	11:24am
ACCY CHK	.07	11:25am
AIR BLK	.00	11:26am
SUB TEST	.00	11:26am
AIR BLK	.00	11:27am
SUB TEST	.00	11:29am
AIR BLK	.00	11:30am

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

DARE COUNTY DARE CO SO BUXTON 270

Serial Number: 008807 Test Record Number: 1574
Test Date: 02/12/2026 Test Time: 11:31am EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	11:32am
FLO	Pass	11:32am
FC	Pass	11:32am

Temperature Tests

Test	Status	Time
FC1	Pass	11:32am
SRC	Pass	11:32am
DET	Pass	11:32am
BAR	Pass	11:32am
BT	Pass	11:32am

Blank Tests

Test	Status	Time
AIR	Pass	11:33am

Printer Tests

Test	Status	Time
PRNT	Pass	11:33am

CRC Tests

Test	Status	Time
COMP	Pass	11:33am
CAL	Pass	11:33am

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Davidson Instrument Location BAT Mobile Unit 8
Instrument Serial No. 008615

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 13 day of February, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

2219283
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

DAVIDSON COUNTY BAT MOBILE UNIT 8 280

Serial Number: 008615
Test Date: 02/13/2026

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Glasscock, Jerry D

Permit Number: 7180-9235

Effective:

02/01/2026-02/01/2028

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG405102

Exp Date: 02/20/2026

Test	g/210L	Time
DIAG	Pass	6:05am
AIR BLK	.00	6:06am
ACCY CHK	.07	6:06am
AIR BLK	.00	6:07am
SUB TEST	.00	6:08am
AIR BLK	.00	6:09am
SUB TEST	.00	6:10am
AIR BLK	.00	6:11am

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

Intox EC/IR-II: Preventive Maintenance

DAVIDSON COUNTY BAT MOBILE UNIT 8 280

Serial Number: 008615 Test Record Number: 6245
Test Date: 02/13/2026 Test Time: 6:12am EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	6:12am
FLO	Pass	6:12am
FC	Pass	6:12am

Temperature Tests

Test	Status	Time
FC1	Pass	6:12am
SRC	Pass	6:12am
DET	Pass	6:12am
BAR	Pass	6:12am
BT	Pass	6:12am

Blank Tests

Test	Status	Time
AIR	Pass	6:13am

Printer Tests

Test	Status	Time
PRNT	Pass	6:13am

CRC Tests

Test	Status	Time
COMP	Pass	6:13am
CAL	Pass	6:13am

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Davidson Instrument Location BAT Mobile Unit 8

Instrument Serial No. 008615

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 20 day of February, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

2219283
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

DAVIDSON COUNTY BAT MOBILE UNIT 8 280

Serial Number: 008615
Test Date: 02/20/2026

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: *Glasscock, Jerry D*
Permit Number: 7180-9235
Effective:
02/01/2026-02/01/2028

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: *Breath Test*

Lot Number: AG506303
Exp Date: 03/04/2027

Test	g/210L	Time
DIAG	Pass	9:13pm
AIR BLK	.00	9:14pm
ACCY CHK	.07	9:14pm
AIR BLK	.00	9:15pm
SUB TEST	.00	9:16pm
AIR BLK	.00	9:17pm
SUB TEST	.00	9:18pm
AIR BLK	.00	9:19pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

DAVIDSON COUNTY BAT MOBILE UNIT 8 280

Serial Number: 008615 Test Record Number: 6255
Test Date: 02/20/2026 Test Time: 9:19pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	9:20pm
FLO	Pass	9:20pm
FC	Pass	9:20pm

Temperature Tests

Test	Status	Time
FC1	Pass	9:20pm
SRC	Pass	9:20pm
DET	Pass	9:20pm
BAR	Pass	9:20pm
BT	Pass	9:20pm

Blank Tests

Test	Status	Time
AIR	Pass	9:21pm

Printer Tests

Test	Status	Time
PRNT	Pass	9:21pm

CRC Tests

Test	Status	Time
COMP	Pass	9:21pm
CAL	Pass	9:21pm

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**


County Davidson Instrument Location BAT Mobile Unit 8

Instrument Serial No. 008736 —

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 13 day of February, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

2219283
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

DAVIDSON COUNTY BAT MOBILE UNIT 8 280

Serial Number: 008736
Test Date: 02/13/2026

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Glasscock, Jerry D

Permit Number: 7180-9235

Effective:

02/01/2026-02/01/2028

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG405102

Exp Date: 02/20/2026

Test	g/210L	Time
DIAG	Pass	6:05am
AIR BLK	.00	6:06am
ACCY CHK	.07	6:07am
AIR BLK	.00	6:08am
SUB TEST	.00	6:08am
AIR BLK	.00	6:09am
SUB TEST	.00	6:11am
AIR BLK	.00	6:11am

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

Intox EC/IR-II: Preventive Maintenance

DAVIDSON COUNTY BAT MOBILE UNIT 8 280

Serial Number: 008736 Test Record Number: 1601
Test Date: 02/13/2026 Test Time: 6:12am EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	6:12am
FLO	Pass	6:12am
FC	Pass	6:12am

Temperature Tests

Test	Status	Time
FC1	Pass	6:12am
SRC	Pass	6:12am
DET	Pass	6:12am
BAR	Pass	6:12am
BT	Pass	6:12am

Blank Tests

Test	Status	Time
AIR	Pass	6:13am

Printer Tests

Test	Status	Time
PRNT	Pass	6:13am

CRC Tests

Test	Status	Time
COMP	Pass	6:13am
CAL	Pass	6:13am

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Davidson Instrument Location BAT Mobile Unit 8

Instrument Serial No. 008736 —

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 20 day of February, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

2219283
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

DAVIDSON COUNTY BAT MOBILE UNIT 8 280

Serial Number: 008736
Test Date: 02/20/2026

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: Glasscock, Jerry D
Permit Number: 7180-9235
Effective:
02/01/2026-02/01/2028

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG506303
Exp Date: 03/04/2027

Test	g/210L	Time
DIAG	Pass	9:12pm
AIR BLK	.00	9:13pm
ACCY CHK	.07	9:13pm
AIR BLK	.00	9:14pm
SUB TEST	.00	9:15pm
AIR BLK	.00	9:16pm
SUB TEST	.00	9:17pm
AIR BLK	.00	9:18pm

Reported AC: .00 g/210L

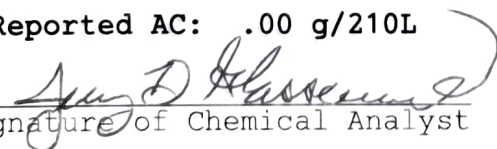
Signature of Chemical Analyst

Court CVR


Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

DAVIDSON COUNTY BAT MOBILE UNIT 8 280

Serial Number: 008736 Test Record Number: 1611
Test Date: 02/20/2026 Test Time: 9:20pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	9:20pm
FLO	Pass	9:20pm
FC	Pass	9:20pm

Temperature Tests

Test	Status	Time
FC1	Pass	9:20pm
SRC	Pass	9:20pm
DET	Pass	9:20pm
BAR	Pass	9:20pm
BT	Pass	9:20pm

Blank Tests

Test	Status	Time
AIR	Pass	9:21pm

Printer Tests

Test	Status	Time
PRNT	Pass	9:21pm

CRC Tests

Test	Status	Time
COMP	Pass	9:21pm
CAL	Pass	9:21pm

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County Davidson Instrument Location BAT Mobile Unit 8

Instrument Serial No. 008775 -

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 13 day of February, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

2219283
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

DAVIDSON COUNTY BAT MOBILE UNIT 8 280

Serial Number: 008775

Test Date: 02/13/2026

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Glasscock, Jerry D

Permit Number: 7180-9235

Effective:

02/01/2026-02/01/2028

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG506303

Exp Date: 03/04/2027

Test	g/210L	Time
DIAG	Pass	6:06am
AIR BLK	.00	6:07am
ACCY CHK	.08	6:08am
AIR BLK	.00	6:08am
SUB TEST	.00	6:09am
AIR BLK	.00	6:10am
SUB TEST	.00	6:12am
AIR BLK	.00	6:12am

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

This form is used when performing Preventive Maintenance procedures

Forensic Tests for Alcohol Branch

Department of Health and Human Services

Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

DAVIDSON COUNTY BAT MOBILE UNIT 8 280

Serial Number: 008775 Test Record Number: 2453
Test Date: 02/13/2026 Test Time: 6:13am EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	6:13am
FLO	Pass	6:13am
FC	Pass	6:13am

Temperature Tests

Test	Status	Time
FC1	Pass	6:13am
SRC	Pass	6:13am
DET	Pass	6:13am
BAR	Pass	6:13am
BT	Pass	6:13am

Blank Tests

Test	Status	Time
AIR	Pass	6:14am

Printer Tests

Test	Status	Time
PRNT	Pass	6:14am

CRC Tests

Test	Status	Time
COMP	Pass	6:14am
CAL	Pass	6:14am

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)


County Davidson Instrument Location BAT Mobile Unit 8

Instrument Serial No. 008775 —

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 20 day of February, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

2219283
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

DAVIDSON COUNTY BAT MOBILE UNIT 8 280

Serial Number: 008775
Test Date: 02/20/2026

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: Glasscock, Jerry D
Permit Number: 7180-9235
Effective:
02/01/2026-02/01/2028

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG506303
Exp Date: 03/04/2027

Test	g/210L	Time
DIAG	Pass	9:11pm
AIR BLK	.00	9:12pm
ACCY CHK	.08	9:12pm
AIR BLK	.00	9:13pm
SUB TEST	.00	9:14pm
AIR BLK	.00	9:15pm
SUB TEST	.00	9:16pm
AIR BLK	.00	9:17pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

Intox EC/IR-II: Preventive Maintenance

DAVIDSON COUNTY BAT MOBILE UNIT 8 280

Serial Number: 008775 Test Record Number: 2459
Test Date: 02/20/2026 Test Time: 9:17pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	9:18pm
FLO	Pass	9:18pm
FC	Pass	9:18pm

Temperature Tests

Test	Status	Time
FC1	Pass	9:18pm
SRC	Pass	9:18pm
DET	Pass	9:18pm
BAR	Pass	9:18pm
BT	Pass	9:18pm

Blank Tests

Test	Status	Time
AIR	Pass	9:18pm

Printer Tests

Test	Status	Time
PRNT	Pass	9:19pm

CRC Tests

Test	Status	Time
COMP	Pass	9:19pm
CAL	Pass	9:19pm

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)


County Davidson Instrument Location BAT Mobile Unit 8

Instrument Serial No. 008816 —

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 13 day of February, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

2219283
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

DAVIDSON COUNTY BAT MOBILE UNIT 8 280

Serial Number: 008816

Test Date: 02/13/2026

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Glasscock, Jerry D

Permit Number: 7180-9235

Effective:

02/01/2026-02/01/2028

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG431002

Exp Date: 11/05/2026

Test	g/210L	Time
DIAG	Pass	6:07am
AIR BLK	.00	6:08am
ACCY CHK	.07	6:08am
AIR BLK	.00	6:09am
SUB TEST	.00	6:10am
AIR BLK	.00	6:11am
SUB TEST	.00	6:12am
AIR BLK	.00	6:13am

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

DAVIDSON COUNTY BAT MOBILE UNIT 8 280

Serial Number: 008816 Test Record Number: 8037
Test Date: 02/13/2026 Test Time: 6:14am EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	6:14am
FLO	Pass	6:14am
FC	Pass	6:14am

Temperature Tests

Test	Status	Time
FC1	Pass	6:15am
SRC	Pass	6:15am
DET	Pass	6:15am
BAR	Pass	6:15am
BT	Pass	6:15am

Blank Tests

Test	Status	Time
AIR	Pass	6:15am

Printer Tests

Test	Status	Time
PRNT	Pass	6:15am

CRC Tests

Test	Status	Time
COMP	Pass	6:15am
CAL	Pass	6:15am

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)


County Davidson Instrument Location BAT Mobile Unit 8

Instrument Serial No. 008816 —

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 20 day of February, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

2219283
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

DAVIDSON COUNTY BAT MOBILE UNIT 8 280

Serial Number: 008816
Test Date: 02/20/2026

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: Glasscock, Jerry D
Permit Number: 7180-9235
Effective:
02/01/2026-02/01/2028

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG431002
Exp Date: 11/05/2026

Test	g/210L	Time
DIAG	Pass	9:09pm
AIR BLK	.00	9:10pm
ACCY CHK	.07	9:11pm
AIR BLK	.00	9:12pm
SUB TEST	.00	9:13pm
AIR BLK	.00	9:14pm
SUB TEST	.00	9:16pm
AIR BLK	.00	9:17pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

Intox EC/IR-II: Preventive Maintenance

DAVIDSON COUNTY BAT MOBILE UNIT 8 280

Serial Number: 008816 Test Record Number: 8043
Test Date: 02/20/2026 Test Time: 9:17pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	9:17pm
FLO	Pass	9:17pm
FC	Pass	9:17pm

Temperature Tests

Test	Status	Time
FC1	Pass	9:17pm
SRC	Pass	9:17pm
DET	Pass	9:17pm
BAR	Pass	9:17pm
BT	Pass	9:17pm

Blank Tests

Test	Status	Time
AIR	Pass	9:18pm

Printer Tests

Test	Status	Time
PRNT	Pass	9:18pm

CRC Tests

Test	Status	Time
COMP	Pass	9:18pm
CAL	Pass	9:18pm

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**


County Davidson Instrument Location BAT Mobile Unit 8

Instrument Serial No. 008929 —

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 13 day of February, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Jay A. [Signature]
Signature of Certifying Official

2219283
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

DAVIDSON COUNTY BAT MOBILE UNIT 8 280

Serial Number: 008929
Test Date: 02/13/2026

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: *Glasscock, Jerry D*
Permit Number: 7180-9235
Effective:
02/01/2026-02/01/2028

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: *Breath Test*

Lot Number: AG506303
Exp Date: 03/04/2027

Test	g/210L	Time
DIAG	Pass	6:07am
AIR BLK	.00	6:09am
ACCY CHK	.08	6:09am
AIR BLK	.00	6:11am
SUB TEST	.00	6:11am
AIR BLK	.00	6:12am
SUB TEST	.00	6:13am
AIR BLK	.00	6:15am

Reported AC: .00 g/210L

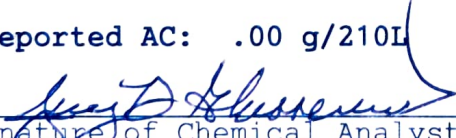
Signature of Chemical Analyst

Court CVR


Analyst

Intox EC/IR-II: Preventive Maintenance

DAVIDSON COUNTY BAT MOBILE UNIT 8 280

Serial Number: 008929 Test Record Number: 1739
Test Date: 02/13/2026 Test Time: 6:16am EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	6:16am
FLO	Pass	6:16am
FC	Pass	6:16am

Temperature Tests

Test	Status	Time
FC1	Pass	6:16am
SRC	Pass	6:16am
DET	Pass	6:16am
BAR	Pass	6:16am
BT	Pass	6:16am

Blank Tests

Test	Status	Time
AIR	Pass	6:17am

Printer Tests

Test	Status	Time
PRNT	Pass	6:17am

CRC Tests

Test	Status	Time
COMP	Pass	6:17am
CAL	Pass	6:17am

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Davidson Instrument Location BAT Mobile Unit 8

Instrument Serial No. 008929

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 20 day of February, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

2219283
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

DAVIDSON COUNTY BAT MOBILE UNIT 8 280

Serial Number: 008929
Test Date: 02/20/2026

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE

Analyst's Name: Glasscock, Jerry D
Permit Number: 7180-9235
Effective:
02/01/2026-02/01/2028

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG506303
Exp Date: 03/04/2027

Test	g/210L	Time
DIAG	Pass	9:09pm
AIR BLK	.00	9:10pm
ACCY CHK	.07	9:11pm
AIR BLK	.00	9:12pm
SUB TEST	.00	9:13pm
AIR BLK	.00	9:14pm
SUB TEST	.00	9:15pm
AIR BLK	.00	9:16pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

Intox EC/IR-II: Preventive Maintenance

DAVIDSON COUNTY BAT MOBILE UNIT 8 280

Serial Number: 008929 Test Record Number: 1746
Test Date: 02/20/2026 Test Time: 9:17pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	9:17pm
FLO	Pass	9:17pm
FC	Pass	9:18pm

Temperature Tests

Test	Status	Time
FC1	Pass	9:18pm
SRC	Pass	9:18pm
DET	Pass	9:18pm
BAR	Pass	9:18pm
BT	Pass	9:18pm

Blank Tests

Test	Status	Time
AIR	Pass	9:18pm

Printer Tests

Test	Status	Time
PRNT	Pass	9:18pm

CRC Tests

Test	Status	Time
COMP	Pass	9:19pm
CAL	Pass	9:19pm

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Forsyth Instrument Location BAT Mobile Unit 11

Instrument Serial No. 008970

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 11th day of February, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



John Francis
Signature of Certifying Official

1604930
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

FORSYTH COUNTY BAT MOBILE UNIT 11 330

Serial Number: 008970
Test Date: 02/11/2026

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: Lanier Jr., John P
Permit Number: 4582-9118
Effective:
02/01/2026-02/01/2028

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG417802
Exp Date: 06/26/2026


Test	g/210L	Time
DIAG	Pass	7:58pm
AIR BLK	.00	7:59pm
ACCY CHK	.08	8:00pm
AIR BLK	.00	8:01pm
SUB TEST	.00	8:01pm
AIR BLK	.00	8:02pm
SUB TEST	.00	8:04pm
AIR BLK	.00	8:05pm

Reported AC: .00 g/210L

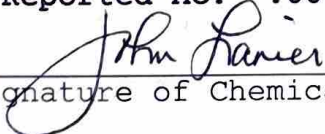

Signature of Chemical Analyst

Court CVR

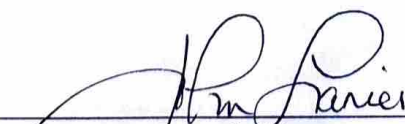

Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

FORSYTH COUNTY BAT MOBILE UNIT 11 330

Serial Number: 008970 Test Record Number: 1368
Test Date: 02/11/2026 Test Time: 8:05pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	8:06pm
FLO	Pass	8:06pm
FC	Pass	8:06pm

Temperature Tests

Test	Status	Time
FC1	Pass	8:06pm
SRC	Pass	8:06pm
DET	Pass	8:06pm
BAR	Pass	8:06pm
BT	Pass	8:06pm

Blank Tests

Test	Status	Time
AIR	Pass	8:07pm


Printer Tests

Test	Status	Time
PRNT	Pass	8:07pm

CRC Tests

Test	Status	Time
COMP	Pass	8:07pm
CAL	Pass	8:07pm

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Gaston Instrument Location Mt. Holly PD
Instrument Serial No. 008733 Mt. Holly, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 16th day of February, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

849845
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

GASTON COUNTY MT. HOLLY PD 350

Serial Number: 008733

Test Date: 02/16/2026

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Helms, Bryce A

Permit Number: 0084-9845

Effective:

02/01/2025-02/01/2027

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG431002

Exp Date: 11/05/2026


Test	g/210L	Time
DIAG	Pass	2:42pm
AIR BLK	.00	2:43pm
ACCY CHK	.07	2:43pm
AIR BLK	.00	2:44pm
SUB TEST	.00	2:45pm
AIR BLK	.00	2:46pm
SUB TEST	.00	2:48pm
AIR BLK	.00	2:48pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR

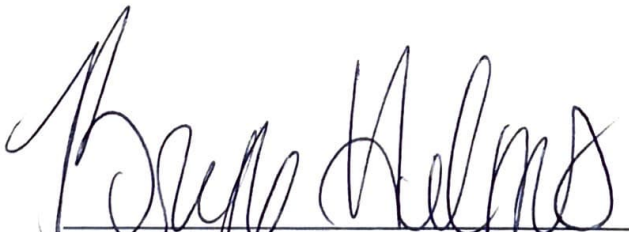

Analyst

Intox EC/IR-II: Preventive Maintenance

GASTON COUNTY MT. HOLLY PD 350

Serial Number: 008733 Test Record Number: 1623
Test Date: 02/16/2026 Test Time: 2:49pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	2:49pm
FLO	Pass	2:49pm
FC	Pass	2:49pm

Temperature Tests

Test	Status	Time
FC1	Pass	2:49pm
SRC	Pass	2:49pm
DET	Pass	2:49pm
BAR	Pass	2:49pm
BT	Pass	2:49pm

Blank Tests

Test	Status	Time
AIR	Pass	2:50pm


Printer Tests

Test	Status	Time
PRNT	Pass	2:50pm

CRC Tests

Test	Status	Time
COMP	Pass	2:50pm
CAL	Pass	2:50pm

Preventive Maintenance
Status: Pass

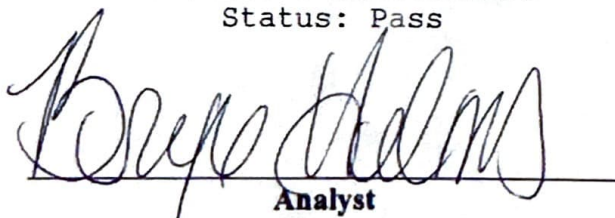

Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County Gates Instrument Location Gates G.S.O.
Instrument Serial No. 008884 202 Court St, Gatesville, N.C.

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 11th day of February, 2020 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature] Signature of Certifying Official 377722 Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

GATES COUNTY GATES CO SO 360

Serial Number: 008884
Test Date: 02/11/2026

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: Gray, Kelly D
Permit Number: 0037-7722
Effective:
02/01/2026-02/01/2028

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG501303
Exp Date: 01/13/2027

Test	g/210L	Time
DIAG	Pass	10:52am
AIR BLK	.00	10:53am
ACCY CHK	.07	10:54am
AIR BLK	.00	10:55am
SUB TEST	.00	10:56am
AIR BLK	.00	10:56am
SUB TEST	.00	10:58am
AIR BLK	.00	10:59am

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

Intox EC/IR-II: Preventive Maintenance

GATES COUNTY GATES CO SO 360

Serial Number: 008884 Test Record Number: 1299
Test Date: 02/11/2026 Test Time: 11:01am EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	11:01am
FLO	Pass	11:01am
FC	Pass	11:01am

Temperature Tests

Test	Status	Time
FC1	Pass	11:02am
SRC	Pass	11:02am
DET	Pass	11:02am
BAR	Pass	11:02am
BT	Pass	11:02am

Blank Tests

Test	Status	Time
AIR	Pass	11:02am

Printer Tests

Test	Status	Time
PRNT	Pass	11:02am

CRC Tests

Test	Status	Time
COMP	Pass	11:02am
CAL	Pass	11:02am

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County Guilford Instrument Location BAT Mobile Unit 11

Instrument Serial No. 008970

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 18th day of February, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



John Ranier
Signature of Certifying Official

1604930
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

GUILFORD COUNTY BAT MOBILE UNIT 11 400

Serial Number: 008970
Test Date: 02/18/2026

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE

Analyst's Name: Lanier Jr., John P
Permit Number: 4582-9118
Effective:
02/01/2026-02/01/2028

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG417802
Exp Date: 06/26/2026

Test	g/210L	Time
DIAG	Pass	7:17am
AIR BLK	.00	7:19am
ACCY CHK	.08	7:19am
AIR BLK	.00	7:20am
SUB TEST	.00	7:21am
AIR BLK	.00	7:21am
SUB TEST	.00	7:23am
AIR BLK	.00	7:24am

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

GUILFORD COUNTY BAT MOBILE UNIT 11 400

Serial Number: 008970 Test Record Number: 1370
Test Date: 02/18/2026 Test Time: 7:24am EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	7:25am
FLO	Pass	7:25am
FC	Pass	7:25am

Temperature Tests

Test	Status	Time
FC1	Pass	7:25am
SRC	Pass	7:25am
DET	Pass	7:25am
BAR	Pass	7:25am
BT	Pass	7:25am

Blank Tests

Test	Status	Time
AIR	Pass	7:26am


Printer Tests

Test	Status	Time
PRNT	Pass	7:26am

CRC Tests

Test	Status	Time
COMP	Pass	7:26am
CAL	Pass	7:26am

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Guilford Instrument Location BAT Mobile Unit 11

Instrument Serial No. 008973

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 18th day of February, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



John Rancier
Signature of Certifying Official

1604930
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

GUILFORD COUNTY BAT MOBILE UNIT 11 400

Serial Number: 008973
Test Date: 02/18/2026

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Lanier Jr., John P

Permit Number: 4582-9118

Effective:

02/01/2026-02/01/2028

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG431003


Exp Date: 11/05/2026

Test	g/210L	Time
DIAG	Pass	7:19am
AIR BLK	.00	7:20am
ACCY CHK	.07	7:20am
AIR BLK	.00	7:21am
SUB TEST	.00	7:22am
AIR BLK	.00	7:23am
SUB TEST	.00	7:24am
AIR BLK	.00	7:25am

Reported AC: .00 g/210L

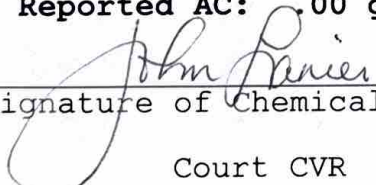

Signature of Chemical Analyst
Court CVR

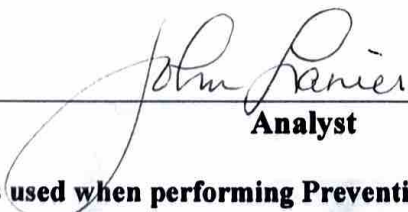

Analyst

Intox EC/IR-II: Preventive Maintenance

GUILFORD COUNTY BAT MOBILE UNIT 11 400

Serial Number: 008973 Test Record Number: 1421
Test Date: 02/18/2026 Test Time: 7:26am EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	7:26am
FLO	Pass	7:26am
FC	Pass	7:26am

Temperature Tests

Test	Status	Time
FC1	Pass	7:26am
SRC	Pass	7:26am
DET	Pass	7:26am
BAR	Pass	7:26am
BT	Pass	7:26am

Blank Tests

Test	Status	Time
AIR	Pass	7:27am

Printer Tests

Test	Status	Time
PRNT	Pass	7:27am

CRC Tests

Test	Status	Time
COMP	Pass	7:27am
CAL	Pass	7:27am

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Haywood Instrument Location Haywood Co. Jail
Instrument Serial No. 008712 Waynesville, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 9th day of February, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



David R. Cuth

Signature of Certifying Official

843310

Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

HAYWOOD COUNTY JAIL 430

Serial Number: 008712
Test Date: 02/09/2026

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE

Analyst's Name: Cutler, Daniel R
Permit Number: 0084-3310
Effective:
02/01/2026-02/01/2028

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG505001
Exp Date: 02/19/2027


Test	g/210L	Time
DIAG	Pass	11:44am
AIR BLK	.00	11:45am
ACCY CHK	.07	11:45am
AIR BLK	.00	11:46am
SUB TEST	.00	11:47am
AIR BLK	.00	11:48am
SUB TEST	.00	11:49am
AIR BLK	.00	11:50am

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR

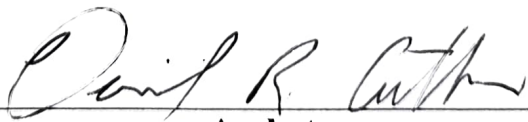

Analyst

Intox EC/IR-II: Preventive Maintenance

HAYWOOD COUNTY JAIL 430

Serial Number: 008712 Test Record Number: 2563
Test Date: 02/09/2026 Test Time: 11:52am EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	11:53am
FLO	Pass	11:53am
FC	Pass	11:53am

Temperature Tests

Test	Status	Time
FC1	Pass	11:53am
SRC	Pass	11:53am
DET	Pass	11:53am
BAR	Pass	11:53am
BT	Pass	11:53am

Blank Tests

Test	Status	Time
AIR	Pass	11:54am

Printer Tests

Test	Status	Time
PRNT	Pass	11:54am

CRC Tests

Test	Status	Time
COMP	Pass	11:54am
CAL	Pass	11:54am

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Haywood Instrument Location Haywood Co. Jail
Instrument Serial No. 008714 Waynesville, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 9th day of February, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



David R. Cutler

Signature of Certifying Official

843310

Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

HAYWOOD COUNTY HAYWOOD COUNTY JAIL 430

Serial Number: 008714
Test Date: 02/09/2026

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE

Analyst's Name: Cutler, Daniel R
Permit Number: 0084-3310
Effective:
02/01/2026-02/01/2028

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test


Lot Number: AG431002
Exp Date: 11/05/2026

Test	g/210L	Time
DIAG	Pass	11:53am
AIR BLK	.00	11:54am
ACCY CHK	.08	11:55am
AIR BLK	.00	11:56am
SUB TEST	.00	11:57am
AIR BLK	.00	11:58am
SUB TEST	.00	12:00pm
AIR BLK	.00	12:01pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

Intox EC/IR-II: Preventive Maintenance

HAYWOOD COUNTY HAYWOOD COUNTY JAIL 430

Serial Number: 008714 Test Record Number: 2572
Test Date: 02/09/2026 Test Time: 12:01pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	12:02pm
FLO	Pass	12:02pm
FC	Pass	12:02pm

Temperature Tests

Test	Status	Time
FC1	Pass	12:02pm
SRC	Pass	12:02pm
DET	Pass	12:02pm
BAR	Pass	12:02pm
BT	Pass	12:02pm

Blank Tests

Test	Status	Time
AIR	Pass	12:03pm

Printer Tests

Test	Status	Time
PRNT	Pass	12:03pm

CRC Tests

Test	Status	Time
COMP	Pass	12:03pm
CAL	Pass	12:03pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Hertford Instrument Location Ahoskie P.D.
Instrument Serial No. 008848 705 W. Main St. Ahoskie,
NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 4th day of February, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Mark A. Russell
Signature of Certifying Official

206272
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

HERTFORD COUNTY AHOSKIE PD 450

Serial Number: 008848
Test Date: 02/04/2026

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE

Analyst's Name: Chappell, Mark A
Permit Number: 0020-6272
Effective:
02/01/2026-02/01/2028

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG501303
Exp Date: 01/13/2027

Test	g/210L	Time
DIAG	Pass	12:15pm
AIR BLK	.00	12:15pm
ACCY CHK	.07	12:16pm
AIR BLK	.00	12:17pm
SUB TEST	.00	12:18pm
AIR BLK	.00	12:19pm
SUB TEST	.00	12:21pm
AIR BLK	.00	12:21pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

HERTFORD COUNTY AHOSKIE PD 450

Serial Number: 008848 Test Record Number: 2021
Test Date: 02/04/2026 Test Time: 12:22pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	12:22pm
FLO	Pass	12:22pm
FC	Pass	12:22pm

Temperature Tests

Test	Status	Time
FC1	Pass	12:22pm
SRC	Pass	12:22pm
DET	Pass	12:22pm
BAR	Pass	12:22pm
BT	Pass	12:22pm

Blank Tests

Test	Status	Time
AIR	Pass	12:23pm


Printer Tests

Test	Status	Time
PRNT	Pass	12:23pm

CRC Tests

Test	Status	Time
COMP	Pass	12:23pm
CAL	Pass	12:23pm

Preventive Maintenance
Status: Pass

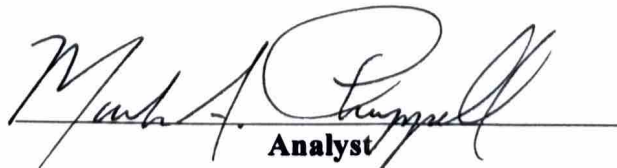
Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County Hertford Instrument Location Murfreesboro P.D.
Instrument Serial No. 008906 115 E. Broad St.
Murfreesboro, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 4th day of February, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

206272
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

HERTFORD COUNTY MURFREESBORO PD 450

Serial Number: 008906
Test Date: 02/04/2026

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: Chappell, Mark A
Permit Number: 0020-6272
Effective:
02/01/2026-02/01/2028

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG501303
Exp Date: 01/13/2027

Test	g/210L	Time
DIAG	Pass	10:58am
AIR BLK	.00	10:59am
ACCY CHK	.08	10:59am
AIR BLK	.00	11:00am
SUB TEST	.00	11:01am
AIR BLK	.00	11:02am
SUB TEST	.00	11:04am
AIR BLK	.00	11:04am

Reported AC: .00 g/210L

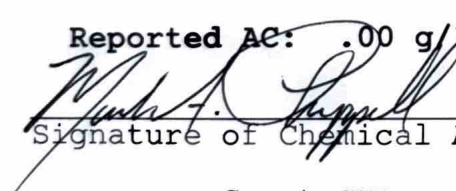

Signature of Chemical Analyst

Court CVR



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

HERTFORD COUNTY MURFREESBORO PD 450

Serial Number: 008906 Test Record Number: 1011
Test Date: 02/04/2026 Test Time: 11:05am EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	11:05am
FLO	Pass	11:05am
FC	Pass	11:05am

Temperature Tests

Test	Status	Time
FC1	Pass	11:06am
SRC	Pass	11:06am
DET	Pass	11:06am
BAR	Pass	11:06am
BT	Pass	11:06am

Blank Tests

Test	Status	Time
AIR	Pass	11:06am


Printer Tests

Test	Status	Time
PRNT	Pass	11:06am

CRC Tests

Test	Status	Time
COMP	Pass	11:06am
CAL	Pass	11:06am

Preventive Maintenance
Status: Pass

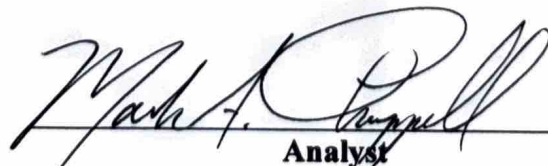

Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County Hyde Instrument Location Hyde Co. S.O.
Instrument Serial No. 008801 1223 Main St., Swan Quarter, N.C.

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 9th day of February, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

377722
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

HYDE COUNTY HYDE CO SO SWAN QUAR 470

Serial Number: 008801
Test Date: 02/09/2026

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: Gray, Kelly D
Permit Number: 0037-7722
Effective:
02/01/2026-02/01/2028

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG506301
Exp Date: 03/04/2027

Test	g/210L	Time
DIAG	Pass	10:59am
AIR BLK	.00	10:59am
ACCY CHK	.07	11:00am
AIR BLK	.00	11:01am
SUB TEST	.00	11:03am
AIR BLK	.00	11:04am
SUB TEST	.00	11:05am
AIR BLK	.00	11:06am

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

Intox EC/IR-II: Preventive Maintenance

HYDE COUNTY HYDE CO SO SWAN QUAR 470

Serial Number: 008801 Test Record Number: 800
Test Date: 02/09/2026 Test Time: 11:07am EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	11:07am
FLO	Pass	11:07am
FC	Pass	11:07am

Temperature Tests

Test	Status	Time
FC1	Pass	11:07am
SRC	Pass	11:07am
DET	Pass	11:07am
BAR	Pass	11:07am
BT	Pass	11:07am

Blank Tests

Test	Status	Time
AIR	Pass	11:08am

Printer Tests

Test	Status	Time
PRNT	Pass	11:08am

CRC Tests

Test	Status	Time
COMP	Pass	11:08am
CAL	Pass	11:08am

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH


PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Iredell Instrument Location BAT Mobile Unit 8
Instrument Serial No. 008615

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 27 day of February, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature] 2219283
Signature of Certifying Official Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

IREDELL COUNTY BAT MOBILE UNIT 8 480

Serial Number: 008615

Test Date: 02/27/2026

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Glasscock, Jerry D

Permit Number: 7180-9235

Effective:

02/01/2026-02/01/2028

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG506303

Exp Date: 03/04/2027

Test	g/210L	Time
DIAG	Pass	9:51pm
AIR BLK	.00	9:52pm
ACCY CHK	.07	9:52pm
AIR BLK	.00	9:53pm
SUB TEST	.00	9:54pm
AIR BLK	.00	9:55pm
SUB TEST	.00	9:57pm
AIR BLK	.00	9:58pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

Intox EC/IR-II: Preventive Maintenance

IREDELL COUNTY BAT MOBILE UNIT 8 480

Serial Number: 008615 Test Record Number: 6261
Test Date: 02/27/2026 Test Time: 9:58pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	9:58pm
FLO	Pass	9:58pm
FC	Pass	9:58pm

Temperature Tests

Test	Status	Time
FC1	Pass	9:58pm
SRC	Pass	9:58pm
DET	Pass	9:58pm
BAR	Pass	9:58pm
BT	Pass	9:58pm

Blank Tests

Test	Status	Time
AIR	Pass	9:59pm

Printer Tests

Test	Status	Time
PRNT	Pass	9:59pm

CRC Tests

Test	Status	Time
COMP	Pass	9:59pm
CAL	Pass	9:59pm

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Iredell Instrument Location BAT Mobile Unit 8
Instrument Serial No. 008615 —

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 28 day of February, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature] 2219283
Signature of Certifying Official Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

IREDELL COUNTY BAT MOBILE UNIT 8 480

Serial Number: 008615
Test Date: 02/28/2026

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE

Analyst's Name: Glasscock, Jerry D
Permit Number: 7180-9235
Effective:
02/01/2026-02/01/2028

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test


Lot Number: AG506303
Exp Date: 03/04/2027

Test	g/210L	Time
DIAG	Pass	11:00pm
AIR BLK	.00	11:01pm
ACCY CHK	.07	11:02pm
AIR BLK	.00	11:03pm
SUB TEST	.00	11:03pm
AIR BLK	.00	11:04pm
SUB TEST	.00	11:06pm
AIR BLK	.00	11:06pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

Intox EC/IR-II: Preventive Maintenance

IREDELL COUNTY BAT MOBILE UNIT 8 480

Serial Number: 008615 Test Record Number: 6263
Test Date: 02/28/2026 Test Time: 11:07pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	11:07pm
FLO	Pass	11:07pm
FC	Pass	11:07pm

Temperature Tests

Test	Status	Time
FC1	Pass	11:07pm
SRC	Pass	11:07pm
DET	Pass	11:07pm
BAR	Pass	11:07pm
BT	Pass	11:07pm

Blank Tests

Test	Status	Time
AIR	Pass	11:08pm

Printer Tests

Test	Status	Time
PRNT	Pass	11:08pm

CRC Tests

Test	Status	Time
COMP	Pass	11:08pm
CAL	Pass	11:08pm

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County IREDELL Instrument Location MOOREVILLE PD

Instrument Serial No. 008685 MOOREVILLE NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 19 day of FEBRUARY, 2020 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

214970
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

IREDELL COUNTY MOORESVILLE PD 480

Serial Number: 008685
Test Date: 02/19/2026

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Fleming, Tina S

Permit Number: 0027-4970

Effective:

02/01/2025-02/01/2027

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG506302

Exp Date: 03/04/2027


Test	g/210L	Time
DIAG	Pass	1:55pm
AIR BLK	.00	1:55pm
ACCY CHK	.08	1:56pm
AIR BLK	.00	1:58pm
SUB TEST	.00	1:59pm
AIR BLK	.00	2:00pm
SUB TEST	.00	2:02pm
AIR BLK	.00	2:03pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

Intox EC/IR-II: Preventive Maintenance

IREDELL COUNTY MOORESVILLE PD 480

Serial Number: 008685 Test Record Number: 5168
Test Date: 02/19/2026 Test Time: 2:03pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	2:04pm
FLO	Pass	2:04pm
FC	Pass	2:04pm

Temperature Tests

Test	Status	Time
FC1	Pass	2:04pm
SRC	Pass	2:04pm
DET	Pass	2:04pm
BAR	Pass	2:04pm
BT	Pass	2:04pm

Blank Tests

Test	Status	Time
AIR	Pass	2:04pm

Printer Tests

Test	Status	Time
PRNT	Pass	2:05pm

CRC Tests

Test	Status	Time
COMP	Pass	2:05pm
CAL	Pass	2:05pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)


County Iredell Instrument Location BAT Mobile Unit 8

Instrument Serial No. 008736

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 27 day of February, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

2219283
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

IREDELL COUNTY BAT MOBILE UNIT 8 480

Serial Number: 008736
Test Date: 02/27/2026

Citation Number: M0000000-0
Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Glasscock, Jerry D

Permit Number: 7180-9235

Effective:

02/01/2026-02/01/2028

Officer's Name: NONE, NONE

Type of Agency: FTA


Agency: DHHS

Test Type: Breath Test

Lot Number: AG506303
Exp Date: 03/04/2027

Test	g/210L	Time
DIAG	Pass	9:38pm
AIR BLK	.00	9:39pm
ACCY CHK	.07	9:40pm
AIR BLK	.00	9:41pm
SUB TEST	.00	9:41pm
AIR BLK	.00	9:42pm
SUB TEST	.00	9:44pm
AIR BLK	.00	9:44pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

Intox EC/IR-II: Preventive Maintenance

IREDELL COUNTY BAT MOBILE UNIT 8 480

Serial Number: 008736 Test Record Number: 1617
Test Date: 02/27/2026 Test Time: 9:45pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	9:45pm
FLO	Pass	9:45pm
FC	Pass	9:45pm

Temperature Tests

Test	Status	Time
FC1	Pass	9:45pm
SRC	Pass	9:45pm
DET	Pass	9:45pm
BAR	Pass	9:45pm
BT	Pass	9:45pm

Blank Tests

Test	Status	Time
AIR	Pass	9:46pm

Printer Tests

Test	Status	Time
PRNT	Pass	9:46pm

CRC Tests

Test	Status	Time
COMP	Pass	9:46pm
CAL	Pass	9:46pm

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**


County Iredell Instrument Location BAT Mobile Unit 8

Instrument Serial No. 008736 —

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 28 day of February, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

2219283
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

IREDELL COUNTY BAT MOBILE UNIT 8 480

Serial Number: 008736
Test Date: 02/28/2026

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Glasscock, Jerry D

Permit Number: 7180-9235

Effective:

02/01/2026-02/01/2028

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG506303

Exp Date: 03/04/2027

Test	g/210L	Time
DIAG	Pass	11:00pm
AIR BLK	.00	11:01pm
ACCY CHK	.07	11:01pm
AIR BLK	.00	11:02pm
SUB TEST	.00	11:03pm
AIR BLK	.00	11:04pm
SUB TEST	.00	11:05pm
AIR BLK	.00	11:06pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

Intox EC/IR-II: Preventive Maintenance

IREDELL COUNTY BAT MOBILE UNIT 8 480

Serial Number: 008736 Test Record Number: 1619
Test Date: 02/28/2026 Test Time: 11:07pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	11:07pm
FLO	Pass	11:07pm
FC	Pass	11:07pm

Temperature Tests

Test	Status	Time
FC1	Pass	11:07pm
SRC	Pass	11:07pm
DET	Pass	11:07pm
BAR	Pass	11:07pm
BT	Pass	11:07pm

Blank Tests

Test	Status	Time
AIR	Pass	11:08pm

Printer Tests

Test	Status	Time
PRNT	Pass	11:08pm

CRC Tests

Test	Status	Time
COMP	Pass	11:08pm
CAL	Pass	11:08pm

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**


County Iredell Instrument Location BAT Mobile Unit 8

Instrument Serial No. 008775

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 27 day of February, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

2219283
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

IREDELL COUNTY BAT MOBILE UNIT 8 480

Serial Number: 008775

Test Date: 02/27/2026

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Glasscock, Jerry D

Permit Number: 7180-9235

Effective:

02/01/2026-02/01/2028

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG506303

Exp Date: 03/04/2027

Test	g/210L	Time
DIAG	Pass	9:46pm
AIR BLK	.00	9:47pm
ACCY CHK	.08	9:47pm
AIR BLK	.00	9:48pm
SUB TEST	.00	9:49pm
AIR BLK	.00	9:50pm
SUB TEST	.00	9:51pm
AIR BLK	.00	9:52pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

Intox EC/IR-II: Preventive Maintenance

IREDELL COUNTY BAT MOBILE UNIT 8 480

Serial Number: 008775 Test Record Number: 2466
Test Date: 02/27/2026 Test Time: 9:54pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	9:55pm
FLO	Pass	9:55pm
FC	Pass	9:55pm

Temperature Tests

Test	Status	Time
FC1	Pass	9:55pm
SRC	Pass	9:55pm
DET	Pass	9:55pm
BAR	Pass	9:55pm
BT	Pass	9:55pm

Blank Tests

Test	Status	Time
AIR	Pass	9:56pm

Printer Tests

Test	Status	Time
PRNT	Pass	9:56pm

CRC Tests

Test	Status	Time
COMP	Pass	9:56pm
CAL	Pass	9:56pm

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Iredell Instrument Location BAT Mobile Unit 8

Instrument Serial No. 008775 . —

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 28 day of February, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

2219283
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

IREDELL COUNTY BAT MOBILE UNIT 8 480

Serial Number: 008775

Test Date: 02/28/2026

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Glasscock, Jerry D

Permit Number: 7180-9235

Effective:

02/01/2026-02/01/2028

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG506303

Exp Date: 03/04/2027

Test	g/210L	Time
DIAG	Pass	10:59pm
AIR BLK	.00	11:00pm
ACCY CHK	.08	11:01pm
AIR BLK	.00	11:02pm
SUB TEST	.00	11:02pm
AIR BLK	.00	11:03pm
SUB TEST	.00	11:04pm
AIR BLK	.00	11:05pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

Intox EC/IR-II: Preventive Maintenance

IREDELL COUNTY BAT MOBILE UNIT 8 480

Serial Number: 008775 Test Record Number: 2469
Test Date: 02/28/2026 Test Time: 11:06pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	11:06pm
FLO	Pass	11:06pm
FC	Pass	11:06pm

Temperature Tests

Test	Status	Time
FC1	Pass	11:07pm
SRC	Pass	11:07pm
DET	Pass	11:07pm
BAR	Pass	11:07pm
BT	Pass	11:07pm

Blank Tests

Test	Status	Time
AIR	Pass	11:07pm

Printer Tests

Test	Status	Time
PRNT	Pass	11:07pm

CRC Tests

Test	Status	Time
COMP	Pass	11:07pm
CAL	Pass	11:07pm

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)


County Iredell Instrument Location BAT Mobile Unit 8

Instrument Serial No. 008816

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 27 day of February, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

2219283
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

IREDELL COUNTY BAT MOBILE UNIT 8 480

Serial Number: 008816
Test Date: 02/27/2026

Citation Number: M0000000-0
Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Glasscock, Jerry D

Permit Number: 7180-9235

Effective:

02/01/2026-02/01/2028

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG431002

Exp Date: 11/05/2026

Test	g/210L	Time
DIAG	Pass	9:37pm
AIR BLK	.00	9:39pm
ACCY CHK	.08	9:39pm
AIR BLK	.00	9:40pm
SUB TEST	.00	9:41pm
AIR BLK	.00	9:42pm
SUB TEST	.00	9:43pm
AIR BLK	.00	9:44pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

Intox EC/IR-II: Preventive Maintenance

IREDELL COUNTY BAT MOBILE UNIT 8 480

Serial Number: 008816 Test Record Number: 8049
Test Date: 02/27/2026 Test Time: 9:47pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	9:47pm
FLO	Pass	9:47pm
FC	Pass	9:47pm

Temperature Tests

Test	Status	Time
FC1	Pass	9:47pm
SRC	Pass	9:47pm
DET	Pass	9:47pm
BAR	Pass	9:47pm
BT	Pass	9:47pm

Blank Tests

Test	Status	Time
AIR	Pass	9:48pm

Printer Tests

Test	Status	Time
PRNT	Pass	9:48pm

CRC Tests

Test	Status	Time
COMP	Pass	9:48pm
CAL	Pass	9:48pm

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Iredell Instrument Location BAT Mobile Unit 8
Instrument Serial No. 008816 —

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 28 day of February, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

2219283
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

IREDELL COUNTY BAT MOBILE UNIT 8 480

Serial Number: 008816
Test Date: 02/28/2026

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: Glasscock, Jerry D
Permit Number: 7180-9235
Effective:
02/01/2026-02/01/2028

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG431002
Exp Date: 11/05/2026

Test	g/210L	Time
DIAG	Pass	10:59pm
AIR BLK	.00	11:00pm
ACCY CHK	.07	11:00pm
AIR BLK	.00	11:01pm
SUB TEST	.00	11:02pm
AIR BLK	.00	11:03pm
SUB TEST	.00	11:05pm
AIR BLK	.00	11:05pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

Intox EC/IR-II: Preventive Maintenance

IREDELL COUNTY BAT MOBILE UNIT 8 480

Serial Number: 008816 Test Record Number: 8051
Test Date: 02/28/2026 Test Time: 11:06pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	11:06pm
FLO	Pass	11:06pm
FC	Pass	11:06pm

Temperature Tests

Test	Status	Time
FC1	Pass	11:07pm
SRC	Pass	11:07pm
DET	Pass	11:07pm
BAR	Pass	11:07pm
BT	Pass	11:07pm

Blank Tests

Test	Status	Time
AIR	Pass	11:07pm

Printer Tests

Test	Status	Time
PRNT	Pass	11:07pm

CRC Tests

Test	Status	Time
COMP	Pass	11:07pm
CAL	Pass	11:07pm

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County IRENELL Instrument Location MOOREVILLE PD

Instrument Serial No. 008823 MOOREVILLE NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 19 day of FEBRUARY, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Jim S. Fleming
Signature of Certifying Official

274970
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

IREDELL COUNTY MOORESVILLE PD 480

Serial Number: 008823
Test Date: 02/19/2026

Citation Number: M0000000-0
Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Fleming, Tina S

Permit Number: 0027-4970

Effective:

02/01/2025-02/01/2027

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG506302

Exp Date: 03/04/2027

Test	g/210L	Time
DIAG	Pass	1:48pm
AIR BLK	.00	1:48pm
ACCY CHK	.08	1:49pm
AIR BLK	.00	1:50pm
SUB TEST	.00	1:51pm
AIR BLK	.00	1:51pm
SUB TEST	.00	1:53pm
AIR BLK	.00	1:54pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

IREDELL COUNTY MOORESVILLE PD 480

Serial Number: 008823 Test Record Number: 2190
Test Date: 02/19/2026 Test Time: 1:57pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	1:57pm
FLO	Pass	1:57pm
FC	Pass	1:57pm

Temperature Tests

Test	Status	Time
FC1	Pass	1:57pm
SRC	Pass	1:57pm
DET	Pass	1:57pm
BAR	Pass	1:57pm
BT	Pass	1:57pm

Blank Tests

Test	Status	Time
AIR	Pass	1:58pm

Printer Tests

Test	Status	Time
PRNT	Pass	1:58pm

CRC Tests

Test	Status	Time
COMP	Pass	1:58pm
CAL	Pass	1:58pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Frederick Instrument Location BAT Mobile Unit 8

Instrument Serial No. 008929 —

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 27 day of February, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

2219283
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

IREDELL COUNTY BAT MOBILE UNIT 8 480

Serial Number: 008929

Test Date: 02/27/2026

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Glasscock, Jerry D

Permit Number: 7180-9235

Effective:

02/01/2026-02/01/2028

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG506303

Exp Date: 03/04/2027

Test	g/210L	Time
DIAG	Pass	9:37pm
AIR BLK	.00	9:38pm
ACCY CHK	.08	9:39pm
AIR BLK	.00	9:40pm
SUB TEST	.00	9:41pm
AIR BLK	.00	9:42pm
SUB TEST	.00	9:43pm
AIR BLK	.00	9:44pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

Intox EC/IR-II: Preventive Maintenance

IREDELL COUNTY BAT MOBILE UNIT 8 480

Serial Number: 008929 Test Record Number: 1752
Test Date: 02/27/2026 Test Time: 9:45pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	9:45pm
FLO	Pass	9:45pm
FC	Pass	9:45pm

Temperature Tests

Test	Status	Time
FC1	Pass	9:45pm
SRC	Pass	9:45pm
DET	Pass	9:45pm
BAR	Pass	9:45pm
BT	Pass	9:45pm

Blank Tests

Test	Status	Time
AIR	Pass	9:46pm

Printer Tests

Test	Status	Time
PRNT	Pass	9:46pm

CRC Tests

Test	Status	Time
COMP	Pass	9:46pm
CAL	Pass	9:46pm

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Iredell Instrument Location BAT Mobile Unit 8
Instrument Serial No. 008929 —

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 28 day of February, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

2219283
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

IREDELL COUNTY BAT MOBILE UNIT 8 480

Serial Number: 008929
Test Date: 02/28/2026

Citation Number: M0000000-0
Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Glasscock, Jerry D

Permit Number: 7180-9235

Effective:

02/01/2026-02/01/2028

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG506303

Exp Date: 03/04/2027

Test	g/210L	Time
DIAG	Pass	10:58pm
AIR BLK	.00	10:59pm
ACCY CHK	.08	11:00pm
AIR BLK	.00	11:01pm
SUB TEST	.00	11:02pm
AIR BLK	.00	11:03pm
SUB TEST	.00	11:04pm
AIR BLK	.00	11:05pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

Intox EC/IR-II: Preventive Maintenance

IREDELL COUNTY BAT MOBILE UNIT 8 480

Serial Number: 008929 Test Record Number: 1754
Test Date: 02/28/2026 Test Time: 11:06pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	11:06pm
FLO	Pass	11:06pm
FC	Pass	11:06pm

Temperature Tests

Test	Status	Time
FC1	Pass	11:06pm
SRC	Pass	11:06pm
DET	Pass	11:06pm
BAR	Pass	11:06pm
BT	Pass	11:06pm

Blank Tests

Test	Status	Time
AIR	Pass	11:07pm

Printer Tests

Test	Status	Time
PRNT	Pass	11:07pm

CRC Tests

Test	Status	Time
COMP	Pass	11:07pm
CAL	Pass	11:07pm

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH


**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County Jackson Instrument Location Jackson Co. Jail
Sylva, NC
Instrument Serial No. 008708

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 4th day of February, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

843310
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

JACKSON COUNTY JAIL 490

Serial Number: 008708

Test Date: 02/04/2026

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Cutler, Daniel R

Permit Number: 0084-3310

Effective:

02/01/2025-02/01/2027

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG431002

Exp Date: 11/05/2026

Test	g/210L	Time
DIAG	Pass	12:03pm
AIR BLK	.00	12:04pm
ACCY CHK	.07	12:05pm
AIR BLK	.00	12:06pm
SUB TEST	.00	12:07pm
AIR BLK	.00	12:07pm
SUB TEST	.00	12:09pm
AIR BLK	.00	12:10pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

Intox EC/IR-II: Preventive Maintenance

JACKSON COUNTY JAIL 490

Serial Number: 008708 Test Record Number: 2156
Test Date: 02/04/2026 Test Time: 12:10pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	12:11pm
FLO	Pass	12:11pm
FC	Pass	12:11pm

Temperature Tests

Test	Status	Time
FC1	Pass	12:11pm
SRC	Pass	12:11pm
DET	Pass	12:11pm
BAR	Pass	12:11pm
BT	Pass	12:11pm

Blank Tests

Test	Status	Time
AIR	Pass	12:11pm


Printer Tests

Test	Status	Time
PRNT	Pass	12:12pm

CRC Tests

Test	Status	Time
COMP	Pass	12:12pm
CAL	Pass	12:12pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Jackson Instrument Location Jackson Co. Jail
Instrument Serial No. 008722 Sylva, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 4th day of February, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Carol R. Luther
Signature of Certifying Official

843310
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

JACKSON COUNTY JACKSON COUNTY JAIL 490

Serial Number: 008722
Test Date: 02/04/2026

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE

Analyst's Name: Cutler, Daniel R
Permit Number: 0084-3310
Effective:
02/01/2025-02/01/2027

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG431002
Exp Date: 11/05/2026


Test	g/210L	Time
DIAG	Pass	12:14pm
AIR BLK	.00	12:15pm
ACCY CHK	.07	12:16pm
AIR BLK	.00	12:17pm
SUB TEST	.00	12:18pm
AIR BLK	.00	12:19pm
SUB TEST	.00	12:20pm
AIR BLK	.00	12:21pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

JACKSON COUNTY JACKSON COUNTY JAIL 490

Serial Number: 008722 Test Record Number: 1704
Test Date: 02/04/2026 Test Time: 12:21pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	12:22pm
FLO	Pass	12:22pm
FC	Pass	12:22pm

Temperature Tests

Test	Status	Time
FC1	Pass	12:22pm
SRC	Pass	12:22pm
DET	Pass	12:22pm
BAR	Pass	12:22pm
BT	Pass	12:22pm

Blank Tests

Test	Status	Time
AIR	Pass	12:22pm


Printer Tests

Test	Status	Time
PRNT	Pass	12:23pm

CRC Tests

Test	Status	Time
COMP	Pass	12:23pm
CAL	Pass	12:23pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Johnston Instrument Location Johnston County
Instrument Serial No. 008728 Detention Center

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 15 day of February, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

365156
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

JOHNSTON COUNTY DETENTION CENTER 500

Serial Number: 008728
Test Date: 02/15/2026

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: Garner, Joel K
Permit Number: 0036-5156
Effective:
02/01/2026-02/01/2028

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG534301
Exp Date: 12/09/2027

Test	g/210L	Time
DIAG	Pass	2:28am
AIR BLK	.00	2:29am
ACCY CHK	.07	2:30am
AIR BLK	.00	2:30am
SUB TEST	.00	2:31am
AIR BLK	.00	2:32am
SUB TEST	.00	2:33am
AIR BLK	.00	2:34am

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

Intox EC/IR-II: Preventive Maintenance

JOHNSTON COUNTY DETENTION CENTER 500

Serial Number: 008728 Test Record Number: 558
Test Date: 02/15/2026 Test Time: 2:35am EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	2:35am
FLO	Pass	2:35am
FC	Pass	2:35am

Temperature Tests

Test	Status	Time
FC1	Pass	2:35am
SRC	Pass	2:35am
DET	Pass	2:35am
BAR	Pass	2:35am
BT	Pass	2:35am

Blank Tests

Test	Status	Time
AIR	Pass	2:36am

Printer Tests

Test	Status	Time
PRNT	Pass	2:36am

CRC Tests

Test	Status	Time
COMP	Pass	2:36am
CAL	Pass	2:36am

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County Macon Instrument Location Macon Co. Jail
Instrument Serial No. 008618 Franklin, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 3rd day of February, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

843310
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

MACON COUNTY MACON COUNTY JAIL 550

Serial Number: 008618
Test Date: 02/03/2026

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: Cutler, Daniel R
Permit Number: 0084-3310
Effective:
02/01/2025-02/01/2027

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG503001
Exp Date: 01/30/2027

Test	g/210L	Time
DIAG	Pass	12:01pm
AIR BLK	.00	12:02pm
ACCY CHK	.07	12:03pm
AIR BLK	.00	12:04pm
SUB TEST	.00	12:05pm
AIR BLK	.00	12:06pm
SUB TEST	.00	12:07pm
AIR BLK	.00	12:08pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

MACON COUNTY MACON COUNTY JAIL 550

Serial Number: 008618 Test Record Number: 2866
Test Date: 02/03/2026 Test Time: 12:09pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	12:09pm
FLO	Pass	12:09pm
FC	Pass	12:09pm

Temperature Tests

Test	Status	Time
FC1	Pass	12:09pm
SRC	Pass	12:09pm
DET	Pass	12:09pm
BAR	Pass	12:09pm
BT	Pass	12:09pm

Blank Tests

Test	Status	Time
AIR	Pass	12:10pm


Printer Tests

Test	Status	Time
PRNT	Pass	12:10pm

CRC Tests

Test	Status	Time
COMP	Pass	12:10pm
CAL	Pass	12:10pm

Preventive Maintenance
Status: Pass

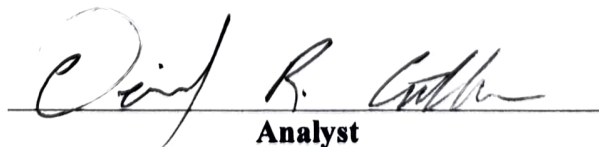
Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Macon Instrument Location Macon Co. Jail
Instrument Serial No. 008789 Franklin, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 3rd day of February, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



David R. Carter
Signature of Certifying Official

843310
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

MACON COUNTY MACON COUNTY JAIL 550

Serial Number: 008789
Test Date: 02/03/2026

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: Cutler, Daniel R
Permit Number: 0084-3310
Effective:
02/01/2025-02/01/2027

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG503001
Exp Date: 01/30/2027

Test	g/210L	Time
DIAG	Pass	12:02pm
AIR BLK	.00	12:03pm
ACCY CHK	.07	12:04pm
AIR BLK	.00	12:05pm
SUB TEST	.00	12:06pm
AIR BLK	.00	12:07pm
SUB TEST	.00	12:08pm
AIR BLK	.00	12:09pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

Intox EC/IR-II: Preventive Maintenance

MACON COUNTY MACON COUNTY JAIL 550

Serial Number: 008789 Test Record Number: 1006
Test Date: 02/03/2026 Test Time: 12:10pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	12:10pm
FLO	Pass	12:10pm
FC	Pass	12:10pm

Temperature Tests

Test	Status	Time
FC1	Pass	12:10pm
SRC	Pass	12:10pm
DET	Pass	12:10pm
BAR	Pass	12:10pm
BT	Pass	12:10pm

Blank Tests

Test	Status	Time
AIR	Pass	12:11pm

Printer Tests

Test	Status	Time
PRNT	Pass	12:11pm

CRC Tests

Test	Status	Time
COMP	Pass	12:11pm
CAL	Pass	12:11pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Macon Instrument Location Macon Co. Magistrate
Instrument Serial No. 008795 Highlands, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 26 day of February, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Orin R. Cutler
Signature of Certifying Official

843310
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

MACON COUNTY MACON CO MAGISTRATE 550

Serial Number: 008795
Test Date: 02/26/2026

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE

Analyst's Name: Cutler, Daniel R
Permit Number: 0084-3310
Effective:
02/01/2026-02/01/2028

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG417803
Exp Date: 06/26/2026

Test	g/210L	Time
DIAG	Pass	12:56pm
AIR BLK	.00	12:56pm
ACCY CHK	.07	12:57pm
AIR BLK	.00	12:58pm
SUB TEST	.00	12:59pm
AIR BLK	.00	1:00pm
SUB TEST	.00	1:02pm
AIR BLK	.00	1:02pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

Intox EC/IR-II: Preventive Maintenance

MACON COUNTY MACON CO MAGISTRATE 550

Serial Number: 008795 Test Record Number: 771
Test Date: 02/26/2026 Test Time: 1:11pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	1:12pm
FLO	Pass	1:12pm
FC	Pass	1:12pm

Temperature Tests

Test	Status	Time
FC1	Pass	1:12pm
SRC	Pass	1:12pm
DET	Pass	1:12pm
BAR	Pass	1:12pm
BT	Pass	1:12pm

Blank Tests

Test	Status	Time
AIR	Pass	1:13pm

Printer Tests

Test	Status	Time
PRNT	Pass	1:13pm

CRC Tests

Test	Status	Time
COMP	Pass	1:13pm
CAL	Pass	1:13pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County Madison Instrument Location Mars Hill PD

Instrument Serial No 009582 Mars Hill, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 25 day of February, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

244987
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

MADISON COUNTY MARS HILL PD 560

Serial Number: 008582
Test Date: 02/25/2026

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Loftis, Benjamin C

Permit Number: 0024-4987

Effective:

02/01/2026-02/01/2028

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG516204

Exp Date: 06/11/2027

Test	g/210L	Time
DIAG	Pass	10:02am
AIR BLK	.00	10:03am
ACCY CHK	.07	10:04am
AIR BLK	.00	10:05am
SUB TEST	.00	10:06am
AIR BLK	.00	10:06am
SUB TEST	.00	10:08am
AIR BLK	.00	10:09am

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

MADISON COUNTY MARS HILL PD 560

Serial Number: 008582 Test Record Number: 1368
Test Date: 02/25/2026 Test Time: 10:09am EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	10:09am
FLO	Pass	10:09am
FC	Pass	10:10am

Temperature Tests

Test	Status	Time
FC1	Pass	10:10am
SRC	Pass	10:10am
DET	Pass	10:10am
BAR	Pass	10:10am
BT	Pass	10:10am

Blank Tests

Test	Status	Time
AIR	Pass	10:10am


Printer Tests

Test	Status	Time
PRNT	Pass	10:10am

CRC Tests

Test	Status	Time
COMP	Pass	10:11am
CAL	Pass	10:11am

Preventive Maintenance
Status: Pass

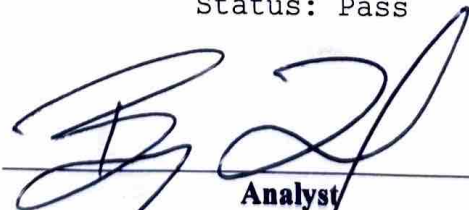

Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Madison Instrument Location Madison County Jail
Instrument Serial No. 008599 Marshall, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 25 day of February, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

244987
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

MADISON COUNTY MADISON COUNTY JAIL 560

Serial Number: 008599

Test Date: 02/25/2026

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Loftis, Benjamin C

Permit Number: 0024-4987

Effective:

02/01/2026-02/01/2028

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG503001

Exp Date: 01/30/2027

Test	g/210L	Time
DIAG	Pass	10:43am
AIR BLK	.00	10:44am
ACCY CHK	.07	10:44am
AIR BLK	.00	10:46am
SUB TEST	.00	10:46am
AIR BLK	.00	10:47am
SUB TEST	.00	10:49am
AIR BLK	.00	10:50am

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

MADISON COUNTY MADISON COUNTY JAIL 560

Serial Number: 008599 Test Record Number: 1596
Test Date: 02/25/2026 Test Time: 10:50am EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	10:50am
FLO	Pass	10:50am
FC	Pass	10:50am

Temperature Tests

Test	Status	Time
FC1	Pass	10:50am
SRC	Pass	10:50am
DET	Pass	10:50am
BAR	Pass	10:50am
BT	Pass	10:50am

Blank Tests

Test	Status	Time
AIR	Pass	10:51am


Printer Tests

Test	Status	Time
PRNT	Pass	10:51am

CRC Tests

Test	Status	Time
COMP	Pass	10:51am
CAL	Pass	10:51am

Preventive Maintenance
Status: Pass

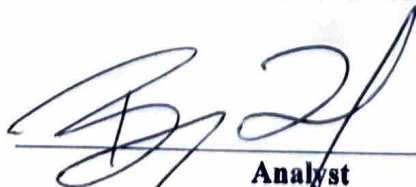

Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Mecklenburg Instrument Location BAT Mobile Unit 8
Instrument Serial No. 008615

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 12 day of February, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

2219283
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

MECKLENBURG COUNTY BAT MOBILE UNIT 8
590

Serial Number: 008615
Test Date: 02/12/2026

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Glasscock, Jerry D

Permit Number: 7180-9235

Effective:

02/01/2026-02/01/2028

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG405102

Exp Date: 02/20/2026

Test	g/210L	Time
DIAG	Pass	9:20am
AIR BLK	.00	9:21am
ACCY CHK	.08	9:22am
AIR BLK	.00	9:23am
SUB TEST	.00	9:24am
AIR BLK	.00	9:25am
SUB TEST	.00	9:26am
AIR BLK	.00	9:27am

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

Intox EC/IR-II: Preventive Maintenance

MECKLENBURG COUNTY BAT MOBILE UNIT 8 590

Serial Number: 008615 Test Record Number: 6243
Test Date: 02/12/2026 Test Time: 9:28am EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	9:29am
FLO	Pass	9:29am
FC	Pass	9:29am

Temperature Tests

Test	Status	Time
FC1	Pass	9:29am
SRC	Pass	9:29am
DET	Pass	9:29am
BAR	Pass	9:29am
BT	Pass	9:29am

Blank Tests

Test	Status	Time
AIR	Pass	9:30am

Printer Tests

Test	Status	Time
PRNT	Pass	9:30am

CRC Tests

Test	Status	Time
COMP	Pass	9:30am
CAL	Pass	9:30am

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Mecklenburg Instrument Location BAT Mobile Unit 8
Instrument Serial No. 008615

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 18 day of February, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

2219283
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

MECKLENBURG COUNTY BAT MOBILE UNIT 8
590

Serial Number: 008615
Test Date: 02/18/2026

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE

Analyst's Name: Glasscock, Jerry D
Permit Number: 7180-9235
Effective:
02/01/2026-02/01/2028

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG405102
Exp Date: 02/20/2026

Test	g/210L	Time
DIAG	Pass	8:24pm
AIR BLK	.00	8:25pm
ACCY CHK	.07	8:25pm
AIR BLK	.00	8:26pm
SUB TEST	.00	8:27pm
AIR BLK	.00	8:28pm
SUB TEST	.00	8:29pm
AIR BLK	.00	8:30pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

MECKLENBURG COUNTY BAT MOBILE UNIT 8 590

Serial Number: 008615 Test Record Number: 6247
Test Date: 02/18/2026 Test Time: 8:30pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	8:31pm
FLO	Pass	8:31pm
FC	Pass	8:31pm

Temperature Tests

Test	Status	Time
FC1	Pass	8:31pm
SRC	Pass	8:31pm
DET	Pass	8:31pm
BAR	Pass	8:31pm
BT	Pass	8:31pm

Blank Tests

Test	Status	Time
AIR	Pass	8:32pm


Printer Tests

Test	Status	Time
PRNT	Pass	8:32pm

CRC Tests

Test	Status	Time
COMP	Pass	8:32pm
CAL	Pass	8:32pm

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Mecklenburg Instrument Location BAT Mobile Unit 8

Instrument Serial No. 008615 _____

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 19 day of February, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

2219283
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

MECKLENBURG COUNTY BAT MOBILE UNIT 8
590

Serial Number: 008615
Test Date: 02/19/2026

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: Glasscock, Jerry D
Permit Number: 7180-9235
Effective:
02/01/2026-02/01/2028

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test


Lot Number: AG506303
Exp Date: 03/04/2027

Test	g/210L	Time
DIAG	Pass	8:29pm
AIR BLK	.00	8:29pm
ACCY CHK	.07	8:30pm
AIR BLK	.00	8:31pm
SUB TEST	.00	8:32pm
AIR BLK	.00	8:33pm
SUB TEST	.00	8:35pm
AIR BLK	.00	8:37pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR

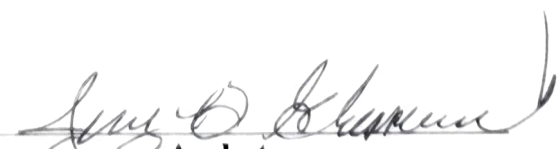
Analyst

Intox EC/IR-II: Preventive Maintenance

MECKLENBURG COUNTY BAT MOBILE UNIT 8 590

Serial Number: 008615 Test Record Number: 6253
Test Date: 02/19/2026 Test Time: 8:39pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	8:39pm
FLO	Pass	8:39pm
FC	Pass	8:39pm

Temperature Tests

Test	Status	Time
FC1	Pass	8:40pm
SRC	Pass	8:40pm
DET	Pass	8:40pm
BAR	Pass	8:40pm
BT	Pass	8:40pm

Blank Tests

Test	Status	Time
AIR	Pass	8:40pm

Printer Tests

Test	Status	Time
PRNT	Pass	8:40pm

CRC Tests

Test	Status	Time
COMP	Pass	8:40pm
CAL	Pass	8:40pm

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Mecklenburg Instrument Location BAT Mobile Unit 8

Instrument Serial No. 008615

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 26 day of February, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

2219283
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

MECKLENBURG COUNTY BAT MOBILE UNIT 8
590

Serial Number: 008615
Test Date: 02/26/2026

Citation Number: M0000000-0
Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Glasscock, Jerry D

Permit Number: 7180-9235

Effective:

02/01/2026-02/01/2028

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG506303

Exp Date: 03/04/2027

Test	g/210L	Time
DIAG	Pass	10:02pm
AIR BLK	.00	10:03pm
ACCY CHK	.07	10:03pm
AIR BLK	.00	10:04pm
SUB TEST	.00	10:05pm
AIR BLK	.00	10:06pm
SUB TEST	.00	10:07pm
AIR BLK	.00	10:08pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

Intox EC/IR-II: Preventive Maintenance

MECKLENBURG COUNTY BAT MOBILE UNIT 8 590

Serial Number: 008615 Test Record Number: 6259
Test Date: 02/26/2026 Test Time: 10:09pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	10:09pm
FLO	Pass	10:09pm
FC	Pass	10:09pm

Temperature Tests

Test	Status	Time
FC1	Pass	10:09pm
SRC	Pass	10:09pm
DET	Pass	10:09pm
BAR	Pass	10:09pm
BT	Pass	10:09pm

Blank Tests

Test	Status	Time
AIR	Pass	10:10pm

Printer Tests

Test	Status	Time
PRNT	Pass	10:10pm

CRC Tests

Test	Status	Time
COMP	Pass	10:10pm
CAL	Pass	10:10pm

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Mecklenburg Instrument Location Matthews PD
Instrument Serial No. 008099 Matthews, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 17th day of February, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Bryce Helms
Signature of Certifying Official

849845
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

MECKLENBURG COUNTY MATTHEWS PD 590

Serial Number: 008699
Test Date: 02/17/2026

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: Helms, Bryce A
Permit Number: 0084-9845
Effective:
02/01/2025-02/01/2027

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG506303
Exp Date: 03/04/2027


Test	g/210L	Time
DIAG	Pass	11:48am
AIR BLK	.00	11:49am
ACCY CHK	.08	11:49am
AIR BLK	.00	11:51am
SUB TEST	.00	11:52am
AIR BLK	.00	11:53am
SUB TEST	.00	11:54am
AIR BLK	.00	11:55am

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR

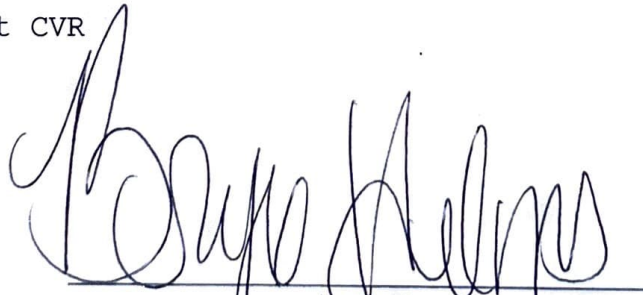

Analyst

Intox EC/IR-II: Preventive Maintenance

MECKLENBURG COUNTY MATTHEWS PD 590

Serial Number: 008699 Test Record Number: 3499
Test Date: 02/17/2026 Test Time: 11:55am EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	11:56am
FLO	Pass	11:56am
FC	Pass	11:56am

Temperature Tests

Test	Status	Time
FC1	Pass	11:56am
SRC	Pass	11:56am
DET	Pass	11:56am
BAR	Pass	11:56am
BT	Pass	11:56am

Blank Tests

Test	Status	Time
AIR	Pass	11:57am


Printer Tests

Test	Status	Time
PRNT	Pass	11:57am

CRC Tests

Test	Status	Time
COMP	Pass	11:57am
CAL	Pass	11:57am

Preventive Maintenance
Status: Pass

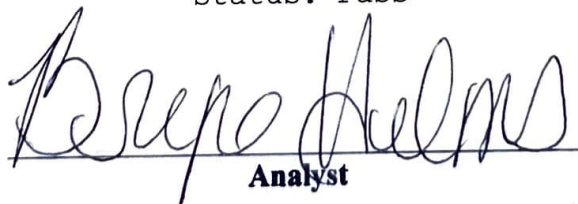
Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Mecklenburg Instrument Location Pineville PD
Instrument Serial No. 008703 Pineville, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 17 day of February, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

849845
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

MECKLENBURG COUNTY PINEVILLE PD 590

Serial Number: 008703
Test Date: 02/17/2026

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE

Analyst's Name: Helms, Bryce A
Permit Number: 0084-9845
Effective:
02/01/2025-02/01/2027

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG534301
Exp Date: 12/09/2027

Test	g/210L	Time
DIAG	Pass	10:50am
AIR BLK	.00	10:50am
ACCY CHK	.08	10:51am
AIR BLK	.00	10:52am
SUB TEST	.00	10:52am
AIR BLK	.00	10:53am
SUB TEST	.00	10:55am
AIR BLK	.00	10:56am

Reported AC: .00 g/210L

Bryce Helms
Signature of Chemical Analyst

Court CVR

Bryce Helms
Analyst

Intox EC/IR-II: Preventive Maintenance

MECKLENBURG COUNTY PINEVILLE PD 590

Serial Number: 008703 Test Record Number: 6369
Test Date: 02/17/2026 Test Time: 10:56am EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	10:56am
FLO	Pass	10:56am
FC	Pass	10:56am

Temperature Tests

Test	Status	Time
FC1	Pass	10:57am
SRC	Pass	10:57am
DET	Pass	10:57am
BAR	Pass	10:57am
BT	Pass	10:57am

Blank Tests

Test	Status	Time
AIR	Pass	10:57am


Printer Tests

Test	Status	Time
PRNT	Pass	10:57am

CRC Tests

Test	Status	Time
COMP	Pass	10:57am
CAL	Pass	10:57am

Preventive Maintenance
Status: Pass

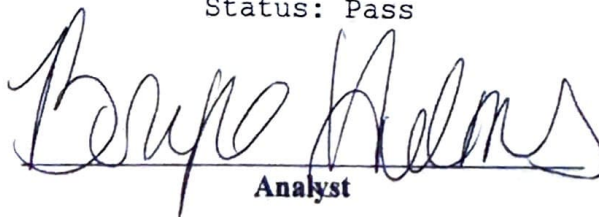
Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Mecklenburg Instrument Location BAT Mobile Unit 8
Instrument Serial No. 008736 —

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 18 day of February, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

2219283
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

MECKLENBURG COUNTY BAT MOBILE UNIT 8
590

Serial Number: 008736
Test Date: 02/18/2026

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Glasscock, Jerry D

Permit Number: 7180-9235

Effective:

02/01/2026-02/01/2028

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG405102

Exp Date: 02/20/2026

Test	g/210L	Time
DIAG	Pass	8:23pm
AIR BLK	.00	8:24pm
ACCY CHK	.07	8:25pm
AIR BLK	.00	8:25pm
SUB TEST	.00	8:26pm
AIR BLK	.00	8:27pm
SUB TEST	.00	8:28pm
AIR BLK	.00	8:29pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

MECKLENBURG COUNTY BAT MOBILE UNIT 8 590

Serial Number: 008736 Test Record Number: 1603

Test Date: 02/18/2026 Test Time: 8:30pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	8:30pm
FLO	Pass	8:30pm
FC	Pass	8:30pm

Temperature Tests

Test	Status	Time
FC1	Pass	8:30pm
SRC	Pass	8:30pm
DET	Pass	8:30pm
BAR	Pass	8:30pm
BT	Pass	8:30pm

Blank Tests

Test	Status	Time
AIR	Pass	8:31pm

Printer Tests

Test	Status	Time
PRNT	Pass	8:31pm

CRC Tests

Test	Status	Time
COMP	Pass	8:31pm
CAL	Pass	8:31pm

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH


PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Mecklenburg Instrument Location BAT Mobile Unit 8
Instrument Serial No. 008736 _____

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 19 day of February, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Signature of Certifying Official 2219283
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

MECKLENBURG COUNTY BAT MOBILE UNIT 8
590

Serial Number: 008736
Test Date: 02/19/2026

Citation Number: M0000000-0
Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Glasscock, Jerry D

Permit Number: 7180-9235

Effective:

02/01/2026-02/01/2028

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG506303

Exp Date: 03/04/2027

Test	g/210L	Time
DIAG	Pass	8:32pm
AIR BLK	.00	8:33pm
ACCY CHK	.07	8:33pm
AIR BLK	.00	8:35pm
SUB TEST	.00	8:35pm
AIR BLK	.00	8:36pm
SUB TEST	.00	8:38pm
AIR BLK	.00	8:38pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

MECKLENBURG COUNTY BAT MOBILE UNIT 8 590

Serial Number: 008736 Test Record Number: 1608
Test Date: 02/19/2026 Test Time: 8:39pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	8:40pm
FLO	Pass	8:40pm
FC	Pass	8:40pm

Temperature Tests

Test	Status	Time
FC1	Pass	8:40pm
SRC	Pass	8:40pm
DET	Pass	8:40pm
BAR	Pass	8:40pm
BT	Pass	8:40pm

Blank Tests

Test	Status	Time
AIR	Pass	8:41pm

Printer Tests

Test	Status	Time
PRNT	Pass	8:41pm

CRC Tests

Test	Status	Time
COMP	Pass	8:41pm
CAL	Pass	8:41pm

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County Mecklenburg Instrument Location BAT Mobile Unit 8

Instrument Serial No. 008736 —

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 26 day of February, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

2219283
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

MECKLENBURG COUNTY BAT MOBILE UNIT 8
590

Serial Number: 008736
Test Date: 02/26/2026

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Glasscock, Jerry D

Permit Number: 7180-9235

Effective:

02/01/2026-02/01/2028

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG506303

Exp Date: 03/04/2027

Test	g/210L	Time
DIAG	Pass	10:01pm
AIR BLK	.00	10:02pm
ACCY CHK	.07	10:03pm
AIR BLK	.00	10:03pm
SUB TEST	.00	10:04pm
AIR BLK	.00	10:05pm
SUB TEST	.00	10:06pm
AIR BLK	.00	10:07pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

MECKLENBURG COUNTY BAT MOBILE UNIT 8 590

Serial Number: 008736 Test Record Number: 1615
Test Date: 02/26/2026 Test Time: 10:11pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	10:11pm
FLO	Pass	10:11pm
FC	Pass	10:11pm

Temperature Tests

Test	Status	Time
FC1	Pass	10:12pm
SRC	Pass	10:12pm
DET	Pass	10:12pm
BAR	Pass	10:12pm
BT	Pass	10:12pm

Blank Tests

Test	Status	Time
AIR	Pass	10:12pm

Printer Tests

Test	Status	Time
PRNT	Pass	10:12pm

CRC Tests

Test	Status	Time
COMP	Pass	10:12pm
CAL	Pass	10:12pm

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County NECKLE BUCH Instrument Location HUNTERSVILLE PD

Instrument Serial No. 008747 HUNTERSVILLE NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 20 day of FEBRUARY, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

274970
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

MECKLENBURG COUNTY HUNTERSVILLE PD 590

Serial Number: 008747
Test Date: 02/20/2026

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Fleming, Tina S

Permit Number: 0027-4970

Effective:

02/01/2025-02/01/2027

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG516204

Exp Date: 06/11/2027

Test	g/210L	Time
DIAG	Pass	11:38am
AIR BLK	.00	11:39am
ACCY CHK	.07	11:39am
AIR BLK	.00	11:40am
SUB TEST	.00	11:41am
AIR BLK	.00	11:42am
SUB TEST	.00	11:43am
AIR BLK	.00	11:44am

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

MECKLENBURG COUNTY HUNTERSVILLE PD 590

Serial Number: 008747 Test Record Number: 3486
Test Date: 02/20/2026 Test Time: 11:45am EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	11:46am
FLO	Pass	11:46am
FC	Pass	11:46am

Temperature Tests

Test	Status	Time
FC1	Pass	11:46am
SRC	Pass	11:46am
DET	Pass	11:46am
BAR	Pass	11:46am
BT	Pass	11:46am

Blank Tests

Test	Status	Time
AIR	Pass	11:46am

Printer Tests

Test	Status	Time
PRNT	Pass	11:46am

CRC Tests

Test	Status	Time
COMP	Pass	11:47am
CAL	Pass	11:47am

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Mecklenburg Instrument Location BAT Mobile Unit 8
Instrument Serial No. 008775 -

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 12 day of February, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

2219283
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

MECKLENBURG COUNTY BAT MOBILE UNIT 8
590

Serial Number: 008775
Test Date: 02/12/2026

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE

Analyst's Name: Glasscock, Jerry D
Permit Number: 7180-9235
Effective:
02/01/2026-02/01/2028

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG506303
Exp Date: 03/04/2027

Test	g/210L	Time
DIAG	Pass	9:17am
AIR BLK	.00	9:18am
ACCY CHK	.08	9:18am
AIR BLK	.00	9:19am
SUB TEST	.00	9:20am
AIR BLK	.00	9:21am
SUB TEST	.00	9:22am
AIR BLK	.00	9:23am

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

MECKLENBURG COUNTY BAT MOBILE UNIT 8 590

Serial Number: 008775 Test Record Number: 2451
Test Date: 02/12/2026 Test Time: 9:24am EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	9:25am
FLO	Pass	9:25am
FC	Pass	9:25am

Temperature Tests

Test	Status	Time
FC1	Pass	9:25am
SRC	Pass	9:25am
DET	Pass	9:25am
BAR	Pass	9:25am
BT	Pass	9:25am

Blank Tests

Test	Status	Time
AIR	Pass	9:26am

Printer Tests

Test	Status	Time
PRNT	Pass	9:26am

CRC Tests

Test	Status	Time
COMP	Pass	9:26am
CAL	Pass	9:26am

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Mecklenburg Instrument Location BAT Mobile Unit 8
Instrument Serial No. 008775 —

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 18 day of February, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Jerry D. Blarocum
Signature of Certifying Official

2219283
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

MECKLENBURG COUNTY BAT MOBILE UNIT 8
590

Serial Number: 008775
Test Date: 02/18/2026

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: Glasscock, Jerry D
Permit Number: 7180-9235
Effective:
02/01/2026-02/01/2028

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG506303
Exp Date: 03/04/2027

Test	g/210L	Time
DIAG	Pass	8:22pm
AIR BLK	.00	8:23pm
ACCY CHK	.08	8:24pm
AIR BLK	.00	8:25pm
SUB TEST	.00	8:26pm
AIR BLK	.00	8:27pm
SUB TEST	.00	8:28pm
AIR BLK	.00	8:29pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

Intox EC/IR-II: Preventive Maintenance

MECKLENBURG COUNTY BAT MOBILE UNIT 8 590

Serial Number: 008775 Test Record Number: 2455
Test Date: 02/18/2026 Test Time: 8:57pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	8:58pm
FLO	Pass	8:58pm
FC	Pass	8:58pm

Temperature Tests

Test	Status	Time
FC1	Pass	8:58pm
SRC	Pass	8:58pm
DET	Pass	8:58pm
BAR	Pass	8:58pm
BT	Pass	8:58pm

Blank Tests

Test	Status	Time
AIR	Pass	8:59pm

Printer Tests

Test	Status	Time
PRNT	Pass	8:59pm

CRC Tests

Test	Status	Time
COMP	Pass	8:59pm
CAL	Pass	8:59pm

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County Mecklenburg Instrument Location BAT Mobile Unit 8
Instrument Serial No. 008775 —

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 19 day of February, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

2219283
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

MECKLENBURG COUNTY BAT MOBILE UNIT 8
590

Serial Number: 008775
Test Date: 02/19/2026

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE

Analyst's Name: Glasscock, Jerry D
Permit Number: 7180-9235
Effective:
02/01/2026-02/01/2028

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG506303
Exp Date: 03/04/2027

Test	g/210L	Time
DIAG	Pass	8:19pm
AIR BLK	.00	8:20pm
ACCY CHK	.08	8:21pm
AIR BLK	.00	8:21pm
SUB TEST	.00	8:22pm
AIR BLK	.00	8:23pm
SUB TEST	.00	8:24pm
AIR BLK	.00	8:25pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

Intox EC/IR-II: Preventive Maintenance

MECKLENBURG COUNTY BAT MOBILE UNIT 8 590

Serial Number: 008775 Test Record Number: 2457
Test Date: 02/19/2026 Test Time: 8:26pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	8:26pm
FLO	Pass	8:26pm
FC	Pass	8:27pm

Temperature Tests

Test	Status	Time
FC1	Pass	8:27pm
SRC	Pass	8:27pm
DET	Pass	8:27pm
BAR	Pass	8:27pm
BT	Pass	8:27pm

Blank Tests

Test	Status	Time
AIR	Pass	8:27pm

Printer Tests

Test	Status	Time
PRNT	Pass	8:27pm

CRC Tests

Test	Status	Time
COMP	Pass	8:27pm
CAL	Pass	8:27pm

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County Mecklenburg Instrument Location BAT Mobile Unit 8

Instrument Serial No. 008775 —

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 26 day of February, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

2219283
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

MECKLENBURG COUNTY BAT MOBILE UNIT 8
590

Serial Number: 008775
Test Date: 02/26/2026

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: Glasscock, Jerry D
Permit Number: 7180-9235
Effective:
02/01/2026-02/01/2028

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG506303
Exp Date: 03/04/2027

Test	g/210L	Time
DIAG	Pass	10:01pm
AIR BLK	.00	10:02pm
ACCY CHK	.08	10:02pm
AIR BLK	.00	10:03pm
SUB TEST	.00	10:04pm
AIR BLK	.00	10:04pm
SUB TEST	.00	10:06pm
AIR BLK	.00	10:07pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

Intox EC/IR-II: Preventive Maintenance

MECKLENBURG COUNTY BAT MOBILE UNIT 8 590

Serial Number: 008775 Test Record Number: 2464
Test Date: 02/26/2026 Test Time: 10:08pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	10:08pm
FLO	Pass	10:08pm
FC	Pass	10:08pm

Temperature Tests

Test	Status	Time
FC1	Pass	10:08pm
SRC	Pass	10:08pm
DET	Pass	10:08pm
BAR	Pass	10:08pm
BT	Pass	10:08pm

Blank Tests

Test	Status	Time
AIR	Pass	10:09pm

Printer Tests

Test	Status	Time
PRNT	Pass	10:09pm

CRC Tests

Test	Status	Time
COMP	Pass	10:09pm
CAL	Pass	10:09pm

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County Mecklenburg Instrument Location BAT Mobile Unit 8

Instrument Serial No. 008816 _____

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 12 day of February, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

2219283
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

MECKLENBURG COUNTY BAT MOBILE UNIT 8
590

Serial Number: 008816
Test Date: 02/12/2026

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: *Glasscock, Jerry D*
Permit Number: 7180-9235
Effective:
02/01/2026-02/01/2028

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: *Breath Test*

Lot Number: AG431002
Exp Date: 11/05/2026

Test	g/210L	Time
DIAG	Pass	9:16am
AIR BLK	.00	9:17am
ACCY CHK	.08	9:17am
AIR BLK	.00	9:18am
SUB TEST	.00	9:19am
AIR BLK	.00	9:20am
SUB TEST	.00	9:22am
AIR BLK	.00	9:22am

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

Intox EC/IR-II: Preventive Maintenance

MECKLENBURG COUNTY BAT MOBILE UNIT 8 590

Serial Number: 008816 Test Record Number: 8035
Test Date: 02/12/2026 Test Time: 9:23am EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	9:24am
FLO	Pass	9:24am
FC	Pass	9:24am

Temperature Tests

Test	Status	Time
FC1	Pass	9:24am
SRC	Pass	9:24am
DET	Pass	9:24am
BAR	Pass	9:24am
BT	Pass	9:24am

Blank Tests

Test	Status	Time
AIR	Pass	9:25am

Printer Tests

Test	Status	Time
PRNT	Pass	9:25am

CRC Tests

Test	Status	Time
COMP	Pass	9:25am
CAL	Pass	9:25am

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Mecklenburg Instrument Location BAT Mobile Unit 8
Instrument Serial No. 008816

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 18 day of February, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

2219283
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

MECKLENBURG COUNTY BAT MOBILE UNIT 8
590

Serial Number: 008816
Test Date: 02/18/2026

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: Glasscock, Jerry D
Permit Number: 7180-9235
Effective:
02/01/2026-02/01/2028

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG431002
Exp Date: 11/05/2026

Test	g/210L	Time
DIAG	Pass	8:22pm
AIR BLK	.00	8:23pm
ACCY CHK	.07	8:23pm
AIR BLK	.00	8:25pm
SUB TEST	.00	8:25pm
AIR BLK	.00	8:26pm
SUB TEST	.00	8:28pm
AIR BLK	.00	8:29pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

Intox EC/IR-II: Preventive Maintenance

MECKLENBURG COUNTY BAT MOBILE UNIT 8 590

Serial Number: 008816 Test Record Number: 8039
Test Date: 02/18/2026 Test Time: 8:29pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	8:30pm
FLO	Pass	8:30pm
FC	Pass	8:30pm

Temperature Tests

Test	Status	Time
FC1	Pass	8:30pm
SRC	Pass	8:30pm
DET	Pass	8:30pm
BAR	Pass	8:30pm
BT	Pass	8:30pm

Blank Tests

Test	Status	Time
AIR	Pass	8:30pm

Printer Tests

Test	Status	Time
PRNT	Pass	8:30pm

CRC Tests

Test	Status	Time
COMP	Pass	8:31pm
CAL	Pass	8:31pm

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH


**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County Mecklenburg Instrument Location BAT Mobile Unit 8
Instrument Serial No. 008816

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 19 day of February, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

2219283
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

MECKLENBURG COUNTY BAT MOBILE UNIT 8
590

Serial Number: 008816
Test Date: 02/19/2026

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: Glasscock, Jerry D
Permit Number: 7180-9235
Effective:
02/01/2026-02/01/2028

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG431002
Exp Date: 11/05/2026

Test	g/210L	Time
DIAG	Pass	8:18pm
AIR BLK	.00	8:19pm
ACCY CHK	.07	8:20pm
AIR BLK	.00	8:21pm
SUB TEST	.00	8:22pm
AIR BLK	.00	8:23pm
SUB TEST	.00	8:24pm
AIR BLK	.00	8:25pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

Intox EC/IR-II: Preventive Maintenance

MECKLENBURG COUNTY BAT MOBILE UNIT 8 590

Serial Number: 008816 Test Record Number: 8041
Test Date: 02/19/2026 Test Time: 8:26pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	8:26pm
FLO	Pass	8:26pm
FC	Pass	8:26pm

Temperature Tests

Test	Status	Time
FC1	Pass	8:26pm
SRC	Pass	8:26pm
DET	Pass	8:26pm
BAR	Pass	8:26pm
BT	Pass	8:26pm

Blank Tests

Test	Status	Time
AIR	Pass	8:27pm

Printer Tests

Test	Status	Time
PRNT	Pass	8:27pm

CRC Tests

Test	Status	Time
COMP	Pass	8:27pm
CAL	Pass	8:27pm

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)


County Mecklenburg Instrument Location BAT Mobile Unit 8

Instrument Serial No. 008816 —

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 26 day of February, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Jay D. Alvarado
Signature of Certifying Official

2219283
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

MECKLENBURG COUNTY BAT MOBILE UNIT 8
590

Serial Number: 008816
Test Date: 02/26/2026

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: Glasscock, Jerry D
Permit Number: 7180-9235
Effective:
02/01/2026-02/01/2028

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG431002
Exp Date: 11/05/2026

Test	g/210L	Time
DIAG	Pass	10:00pm
AIR BLK	.00	10:01pm
ACCY CHK	.07	10:02pm
AIR BLK	.00	10:03pm
SUB TEST	.00	10:04pm
AIR BLK	.00	10:05pm
SUB TEST	.00	10:06pm
AIR BLK	.00	10:07pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

Intox EC/IR-II: Preventive Maintenance

MECKLENBURG COUNTY BAT MOBILE UNIT 8 590

Serial Number: 008816 Test Record Number: 8047
Test Date: 02/26/2026 Test Time: 10:08pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	10:08pm
FLO	Pass	10:08pm
FC	Pass	10:08pm

Temperature Tests

Test	Status	Time
FC1	Pass	10:08pm
SRC	Pass	10:08pm
DET	Pass	10:08pm
BAR	Pass	10:08pm
BT	Pass	10:08pm

Blank Tests

Test	Status	Time
AIR	Pass	10:09pm

Printer Tests

Test	Status	Time
PRNT	Pass	10:09pm

CRC Tests

Test	Status	Time
COMP	Pass	10:09pm
CAL	Pass	10:09pm

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County Mecklenburg Instrument Location BAT Mobile Unit 8
Instrument Serial No. 008929

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 12 day of February, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

2219283
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

MECKLENBURG COUNTY BAT MOBILE UNIT 8
590

Serial Number: 008929
Test Date: 02/12/2026

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: Glasscock, Jerry D
Permit Number: 7180-9235
Effective:
02/01/2026-02/01/2028

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG506303
Exp Date: 03/04/2027

Test	g/210L	Time
DIAG	Pass	9:15am
AIR BLK	.00	9:16am
ACCY CHK	.08	9:17am
AIR BLK	.00	9:18am
SUB TEST	.00	9:19am
AIR BLK	.00	9:20am
SUB TEST	.00	9:22am
AIR BLK	.00	9:23am

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

Intox EC/IR-II: Preventive Maintenance

MECKLENBURG COUNTY BAT MOBILE UNIT 8 590

Serial Number: 008929 Test Record Number: 1737
Test Date: 02/12/2026 Test Time: 9:24am EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	9:24am
FLO	Pass	9:24am
FC	Pass	9:25am

Temperature Tests

Test	Status	Time
FC1	Pass	9:25am
SRC	Pass	9:25am
DET	Pass	9:25am
BAR	Pass	9:25am
BT	Pass	9:25am

Blank Tests

Test	Status	Time
AIR	Pass	9:26am

Printer Tests

Test	Status	Time
PRNT	Pass	9:26am

CRC Tests

Test	Status	Time
COMP	Pass	9:26am
CAL	Pass	9:26am

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Mecklenburg Instrument Location BAT Mobile Unit 8
Instrument Serial No. 008929 _____

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 18 day of February, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

2219283
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

MECKLENBURG COUNTY BAT MOBILE UNIT 8
590

Serial Number: 008929
Test Date: 02/18/2026

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE

Analyst's Name: Glasscock, Jerry D
Permit Number: 7180-9235
Effective:
02/01/2026-02/01/2028

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG506303
Exp Date: 03/04/2027

Test	g/210L	Time
DIAG	Pass	8:21pm
AIR BLK	.00	8:22pm
ACCY CHK	.08	8:23pm
AIR BLK	.00	8:24pm
SUB TEST	.00	8:25pm
AIR BLK	.00	8:26pm
SUB TEST	.00	8:28pm
AIR BLK	.00	8:29pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

Intox EC/IR-II: Preventive Maintenance

MECKLENBURG COUNTY BAT MOBILE UNIT 8 590

Serial Number: 008929 Test Record Number: 1741
Test Date: 02/18/2026 Test Time: 8:29pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	8:30pm
FLO	Pass	8:30pm
FC	Pass	8:30pm

Temperature Tests

Test	Status	Time
FC1	Pass	8:30pm
SRC	Pass	8:30pm
DET	Pass	8:30pm
BAR	Pass	8:30pm
BT	Pass	8:30pm

Blank Tests

Test	Status	Time
AIR	Pass	8:31pm


Printer Tests

Test	Status	Time
PRNT	Pass	8:31pm

CRC Tests

Test	Status	Time
COMP	Pass	8:31pm
CAL	Pass	8:31pm

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Mecklenburg Instrument Location BAT Mobile Unit 8

Instrument Serial No. 008929

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 19 day of February, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

2219283
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

MECKLENBURG COUNTY BAT MOBILE UNIT 8
590

Serial Number: 008929
Test Date: 02/19/2026

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE

Analyst's Name: Glasscock, Jerry D
Permit Number: 7180-9235
Effective:
02/01/2026-02/01/2028

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG506303
Exp Date: 03/04/2027

Test	g/210L	Time
DIAG	Pass	8:18pm
AIR BLK	.00	8:19pm
ACCY CHK	.08	8:20pm
AIR BLK	.00	8:21pm
SUB TEST	.00	8:21pm
AIR BLK	.00	8:22pm
SUB TEST	.00	8:24pm
AIR BLK	.00	8:25pm

Reported AC: 00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

Intox EC/IR-II: Preventive Maintenance

MECKLENBURG COUNTY BAT MOBILE UNIT 8 590

Serial Number: 008929 Test Record Number: 1743
Test Date: 02/19/2026 Test Time: 8:25pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	8:26pm
FLO	Pass	8:26pm
FC	Pass	8:26pm

Temperature Tests

Test	Status	Time
FC1	Pass	8:26pm
SRC	Pass	8:26pm
DET	Pass	8:26pm
BAR	Pass	8:26pm
BT	Pass	8:26pm

Blank Tests

Test	Status	Time
AIR	Pass	8:27pm

Printer Tests

Test	Status	Time
PRNT	Pass	8:27pm

CRC Tests

Test	Status	Time
COMP	Pass	8:27pm
CAL	Pass	8:27pm

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**


County Mecklenburg Instrument Location BAT Mobile Unit 8

Instrument Serial No. 008929

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 26 day of February, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

2219283
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

MECKLENBURG COUNTY BAT MOBILE UNIT 8
590

Serial Number: 008929
Test Date: 02/26/2026

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE

Analyst's Name: Glasscock, Jerry D
Permit Number: 7180-9235
Effective:
02/01/2026-02/01/2028

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG506303
Exp Date: 03/04/2027

Test	g/210L	Time
DIAG	Pass	9:59pm
AIR BLK	.00	10:01pm
ACCY CHK	.08	10:01pm
AIR BLK	.00	10:03pm
SUB TEST	.00	10:03pm
AIR BLK	.00	10:04pm
SUB TEST	.00	10:06pm
AIR BLK	.00	10:07pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

MECKLENBURG COUNTY BAT MOBILE UNIT 8 590

Serial Number: 008929 Test Record Number: 1750
Test Date: 02/26/2026 Test Time: 10:08pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	10:08pm
FLO	Pass	10:08pm
FC	Pass	10:08pm

Temperature Tests

Test	Status	Time
FC1	Pass	10:08pm
SRC	Pass	10:08pm
DET	Pass	10:08pm
BAR	Pass	10:08pm
BT	Pass	10:08pm

Blank Tests

Test	Status	Time
AIR	Pass	10:09pm

Printer Tests

Test	Status	Time
PRNT	Pass	10:09pm

CRC Tests

Test	Status	Time
COMP	Pass	10:09pm
CAL	Pass	10:09pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Mitchell Instrument Location Spruce Pine Police Dept.
Instrument Serial No. 008726 Spruce Pine, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 9 day of February, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Handwritten Signature]
Signature of Certifying Official

244987
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

MITCHELL COUNTY SPRUCE PINE PD 600

Serial Number: 008726
Test Date: 02/09/2026

Citation Number: M0000000-0
Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Loftis, Benjamin C

Permit Number: 0024-4987

Effective:

02/01/2026-02/01/2028

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG503001

Exp Date: 01/30/2027

Test	g/210L	Time
DIAG	Pass	12:41pm
AIR BLK	.00	12:42pm
ACCY CHK	.08	12:42pm
AIR BLK	.00	12:44pm
SUB TEST	.00	12:44pm
AIR BLK	.00	12:45pm
SUB TEST	.00	12:47pm
AIR BLK	.00	12:48pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

MITCHELL COUNTY SPRUCE PINE PD 600

Serial Number: 008726 Test Record Number: 1578
Test Date: 02/09/2026 Test Time: 12:48pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	12:48pm
FLO	Pass	12:48pm
FC	Pass	12:48pm

Temperature Tests

Test	Status	Time
FC1	Pass	12:49pm
SRC	Pass	12:49pm
DET	Pass	12:49pm
BAR	Pass	12:49pm
BT	Pass	12:49pm

Blank Tests

Test	Status	Time
AIR	Pass	12:49pm

Printer Tests

Test	Status	Time
PRNT	Pass	12:49pm

CRC Tests

Test	Status	Time
COMP	Pass	12:49pm
CAL	Pass	12:49pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County ONslow Instrument Location ONslow COUNTY

Instrument Serial No. 008578 SNEADS FERRY SUBSTATION

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 16th day of FEBRUARY, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

2824950
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

ONSLOW COUNTY SNEADS FERRY SUB 660

Serial Number: 008578

Test Date: 02/16/2026

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: GILLESPIE, PENTTI W

Permit Number: 9523-2149

Effective:

02/01/2026-02/01/2028

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG501307

Exp Date: 01/13/2027

Test	g/210L	Time
DIAG	Pass	4:07pm
AIR BLK	.00	4:08pm
ACCY CHK	.07	4:08pm
AIR BLK	.00	4:09pm
SUB TEST	.00	4:10pm
AIR BLK	.00	4:11pm
SUB TEST	.00	4:12pm
AIR BLK	.00	4:13pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

ONslow COUNTY SNEADS FERRY SUB 660

Serial Number: 008578 Test Record Number: 3724
Test Date: 02/16/2026 Test Time: 4:14pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	4:14pm
FLO	Pass	4:14pm
FC	Pass	4:14pm

Temperature Tests

Test	Status	Time
FC1	Pass	4:14pm
SRC	Pass	4:14pm
DET	Pass	4:14pm
BAR	Pass	4:14pm
BT	Pass	4:14pm

Blank Tests

Test	Status	Time
AIR	Pass	4:15pm

Printer Tests

Test	Status	Time
PRNT	Pass	4:15pm

CRC Tests

Test	Status	Time
COMP	Pass	4:15pm
CAL	Pass	4:15pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County ONslow Instrument Location SWANS BORO

Instrument Serial No. 008894 POLICE DEPT

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 16th day of FEBRUARY, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

282 4950
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

ONslow COUNTY SWANSBORO PD 660

Serial Number: 008894
Test Date: 02/16/2026

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: GILLESPIE, PENTTI W
Permit Number: 9523-2149
Effective:
02/01/2026-02/01/2028

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG417803
Exp Date: 06/26/2026


Test	g/210L	Time
DIAG	Pass	1:51pm
AIR BLK	.00	1:51pm
ACCY CHK	.08	1:52pm
AIR BLK	.00	1:53pm
SUB TEST	.00	1:54pm
AIR BLK	.00	1:54pm
SUB TEST	.00	1:56pm
AIR BLK	.00	1:57pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR

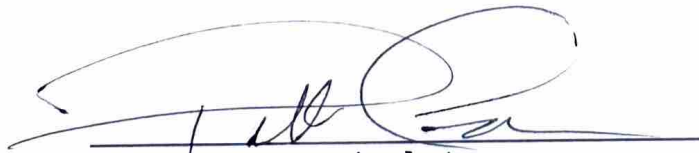

Analyst

Intox EC/IR-II: Preventive Maintenance

ONslow COUNTY SWANSBORO PD 660

Serial Number: 008894 Test Record Number: 1839
Test Date: 02/16/2026 Test Time: 1:58pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	1:58pm
FLO	Pass	1:58pm
FC	Pass	1:58pm

Temperature Tests

Test	Status	Time
FC1	Pass	1:58pm
SRC	Pass	1:58pm
DET	Pass	1:58pm
BAR	Pass	1:58pm
BT	Pass	1:58pm

Blank Tests

Test	Status	Time
AIR	Pass	1:59pm


Printer Tests

Test	Status	Time
PRNT	Pass	1:59pm

CRC Tests

Test	Status	Time
COMP	Pass	1:59pm
CAL	Pass	1:59pm

Preventive Maintenance
Status: Pass

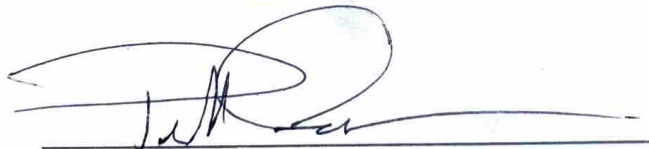

Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County ONSLow Instrument Location MCAS
Instrument Serial No. 008919 NEW RIVER PMO

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 16th day of FEBRUARY, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Handwritten Signature]

Signature of Certifying Official

2824950

Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

ONslow COUNTY MCAS NEW RIVER 660

Serial Number: 008919

Test Date: 02/16/2026

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: GILLESPIE, PENTTI W

Permit Number: 9523-2149

Effective:

02/01/2026-02/01/2028

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG501307

Exp Date: 01/13/2027

Test	g/210L	Time
DIAG	Pass	10:01am
AIR BLK	.00	10:01am
ACCY CHK	.07	10:02am
AIR BLK	.00	10:03am
SUB TEST	.00	10:04am
AIR BLK	.00	10:04am
SUB TEST	.00	10:06am
AIR BLK	.00	10:07am

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

ONSLOW COUNTY MCAS NEW RIVER 660

Serial Number: 008919 Test Record Number: 945
Test Date: 02/16/2026 Test Time: 10:07am EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	10:08am
FLO	Pass	10:08am
FC	Pass	10:08am

Temperature Tests

Test	Status	Time
FC1	Pass	10:08am
SRC	Pass	10:08am
DET	Pass	10:08am
BAR	Pass	10:08am
BT	Pass	10:08am

Blank Tests

Test	Status	Time
AIR	Pass	10:08am

Printer Tests

Test	Status	Time
PRNT	Pass	10:08am

CRC Tests

Test	Status	Time
COMP	Pass	10:09am
CAL	Pass	10:09am

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County ONSLow Instrument Location CAMP LESTUNE
Instrument Serial No. 00 8920 PMO

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 20th day of FEBRUARY, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Handwritten Signature]
Signature of Certifying Official

282-4950
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

ONslow COUNTY CAMP LEJEUNE PMO 660

Serial Number: 008920
Test Date: 02/20/2026

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE

Analyst's Name: GILLESPIE, PENTTI W
Permit Number: 9523-2149
Effective:
02/01/2026-02/01/2028

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG501307
Exp Date: 01/13/2027

Test	g/210L	Time
DIAG	Pass	2:32pm
AIR BLK	.00	2:32pm
ACCY CHK	.07	2:33pm
AIR BLK	.00	2:34pm
SUB TEST	.00	2:35pm
AIR BLK	.00	2:36pm
SUB TEST	.00	2:37pm
AIR BLK	.00	2:38pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

Intox EC/IR-II: Preventive Maintenance

ONslow COUNTY CAMP LEJEUNE PMO 660

Serial Number: 008920 Test Record Number: 2549
Test Date: 02/20/2026 Test Time: 2:38pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	2:39pm
FLO	Pass	2:39pm
FC	Pass	2:39pm

Temperature Tests

Test	Status	Time
FC1	Pass	2:39pm
SRC	Pass	2:39pm
DET	Pass	2:39pm
BAR	Pass	2:39pm
BT	Pass	2:39pm

Blank Tests

Test	Status	Time
AIR	Pass	2:39pm

Printer Tests

Test	Status	Time
PRNT	Pass	2:40pm

CRC Tests

Test	Status	Time
COMP	Pass	2:40pm
CAL	Pass	2:40pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County ONslow Instrument Location JACKSONVILLE
Instrument Serial No. 008930 POLICE DEPT

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 16th day of FEBRUARY, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.





Signature of Certifying Official

2824950

Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

ONslow COUNTY JACKSONVILLE PD 660

Serial Number: 008930
Test Date: 02/16/2026

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: GILLESPIE, PENTTI W
Permit Number: 9523-2149
Effective:
02/01/2026-02/01/2028

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG534301
Exp Date: 12/09/2027

Test	g/210L	Time
DIAG	Pass	11:13am
AIR BLK	.00	11:14am
ACCY CHK	.08	11:14am
AIR BLK	.00	11:16am
SUB TEST	.00	11:16am
AIR BLK	.00	11:17am
SUB TEST	.00	11:19am
AIR BLK	.00	11:19am

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

ONslow COUNTY JACKSONVILLE PD 660

Serial Number: 008930 Test Record Number: 2457
Test Date: 02/16/2026 Test Time: 11:19am EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	11:20am
FLO	Pass	11:20am
FC	Pass	11:20am

Temperature Tests

Test	Status	Time
FC1	Pass	11:20am
SRC	Pass	11:20am
DET	Pass	11:20am
BAR	Pass	11:20am
BT	Pass	11:20am

Blank Tests

Test	Status	Time
AIR	Pass	11:21am

Printer Tests

Test	Status	Time
PRNT	Pass	11:21am

CRC Tests

Test	Status	Time
COMP	Pass	11:21am
CAL	Pass	11:21am

Preventive Maintenance
Status: Pass



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County ONslow Instrument Location ONslow COUNTY
Instrument Serial No. 008931 DETENTION CENTER

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 16th day of FEBRUARY, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]

Signature of Certifying Official

2824950

Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

ONSLOW COUNTY DETENTION CENTER 660

Serial Number: 008931
Test Date: 02/16/2026

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: GILLESPIE, PENTTI W

Permit Number: 9523-2149

Effective:

02/01/2026-02/01/2028

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG501307

Exp Date: 01/13/2027

Test	g/210L	Time
DIAG	Pass	12:16pm
AIR BLK	.00	12:17pm
ACCY CHK	.07	12:17pm
AIR BLK	.00	12:18pm
SUB TEST	.00	12:19pm
AIR BLK	.00	12:20pm
SUB TEST	.00	12:21pm
AIR BLK	.00	12:22pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

ONSLOW COUNTY DETENTION CENTER 660

Serial Number: 008931 Test Record Number: 5628
Test Date: 02/16/2026 Test Time: 12:23pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	12:23pm
FLO	Pass	12:23pm
FC	Pass	12:23pm

Temperature Tests

Test	Status	Time
FC1	Pass	12:23pm
SRC	Pass	12:23pm
DET	Pass	12:23pm
BAR	Pass	12:23pm
BT	Pass	12:23pm

Blank Tests

Test	Status	Time
AIR	Pass	12:24pm

Printer Tests

Test	Status	Time
PRNT	Pass	12:24pm

CRC Tests

Test	Status	Time
COMP	Pass	12:24pm
CAL	Pass	12:24pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County ONSLOW Instrument Location ONSLOW COUNTY
Instrument Serial No. 008932 DETENTION CENTER

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 16th day of FEBRUARY, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

2824950

Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

ONSLOW COUNTY DETENTION CENTER 660

Serial Number: 008932
Test Date: 02/16/2026

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: GILLESPIE, PENTTI W
Permit Number: 9523-2149
Effective:
02/01/2026-02/01/2028

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG534301
Exp Date: 12/09/2027


Test	g/210L	Time
DIAG	Pass	12:13pm
AIR BLK	.00	12:14pm
ACCY CHK	.07	12:15pm
AIR BLK	.00	12:16pm
SUB TEST	.00	12:16pm
AIR BLK	.00	12:17pm
SUB TEST	.00	12:19pm
AIR BLK	.00	12:20pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR

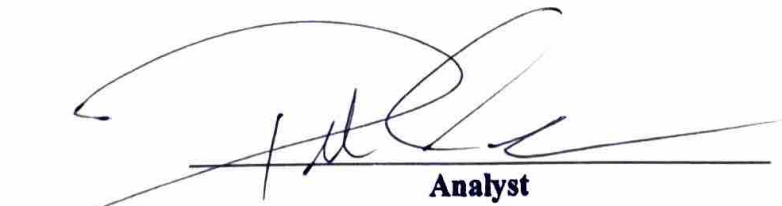

Analyst

Intox EC/IR-II: Preventive Maintenance

ONslow COUNTY DETENTION CENTER 660

Serial Number: 008932 Test Record Number: 7920
Test Date: 02/16/2026 Test Time: 12:20pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	12:20pm
FLO	Pass	12:20pm
FC	Pass	12:20pm

Temperature Tests

Test	Status	Time
FC1	Pass	12:20pm
SRC	Pass	12:20pm
DET	Pass	12:20pm
BAR	Pass	12:20pm
BT	Pass	12:20pm

Blank Tests

Test	Status	Time
AIR	Pass	12:21pm


Printer Tests

Test	Status	Time
PRNT	Pass	12:21pm

CRC Tests

Test	Status	Time
COMP	Pass	12:21pm
CAL	Pass	12:21pm

Preventive Maintenance
Status: Pass

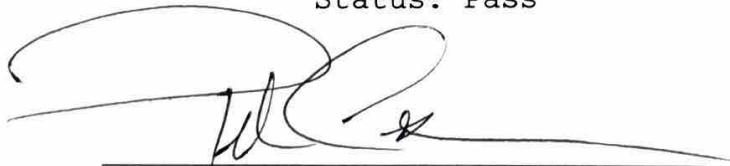

Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County PAMLICO Instrument Location PAMLICO COUNTY

Instrument Serial No. 008640 DETENTION CENTER

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 3rd day of FEBRUARY, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

2824950
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

PAMLICO COUNTY DETENTION CENTER 680

Serial Number: 008640
Test Date: 02/03/2026

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: GILLESPIE, PENTTI W
Permit Number: 9523-2149
Effective:
02/01/2026-02/01/2028

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG534301
Exp Date: 12/09/2027

Test	g/210L	Time
DIAG	Pass	1:45pm
AIR BLK	.00	1:46pm
ACCY CHK	.08	1:47pm
AIR BLK	.00	1:48pm
SUB TEST	.00	1:49pm
AIR BLK	.00	1:49pm
SUB TEST	.00	1:51pm
AIR BLK	.00	1:52pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

PAMLICO COUNTY DETENTION CENTER 680

Serial Number: 008640 Test Record Number: 1743
Test Date: 02/03/2026 Test Time: 1:53pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	1:53pm
FLO	Pass	1:53pm
FC	Pass	1:53pm

Temperature Tests

Test	Status	Time
FC1	Pass	1:53pm
SRC	Pass	1:53pm
DET	Pass	1:53pm
BAR	Pass	1:53pm
BT	Pass	1:53pm

Blank Tests

Test	Status	Time
AIR	Pass	1:54pm

Printer Tests

Test	Status	Time
PRNT	Pass	1:54pm

CRC Tests

Test	Status	Time
COMP	Pass	1:54pm
CAL	Pass	1:54pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)


County Pasquotank Instrument Location Pasquotank Co. Public Safety Bldg.
200 E. Colonial Ave
Elizabeth City, NC

Instrument Serial No. 008950

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 3rd day of February, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

206272
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

PASQUOTANK COUNTY PUBLIC SAFETY BLDG
690

Serial Number: 008950
Test Date: 02/03/2026

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE

Analyst's Name: Chappell, Mark A
Permit Number: 0020-6272
Effective:
02/01/2025-02/01/2027

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG501303
Exp Date: 01/13/2027

Test	g/210L	Time
DIAG	Pass	10:42am
AIR BLK	.00	10:43am
ACCY CHK	.07	10:44am
AIR BLK	.00	10:45am
SUB TEST	.00	10:46am
AIR BLK	.00	10:47am
SUB TEST	.00	10:48am
AIR BLK	.00	10:49am

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

PASQUOTANK COUNTY PUBLIC SAFETY BLDG 690

Serial Number: 008950 Test Record Number: 2258
Test Date: 02/03/2026 Test Time: 10:55am EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	10:55am
FLO	Pass	10:55am
FC	Pass	10:55am

Temperature Tests

Test	Status	Time
FC1	Pass	10:55am
SRC	Pass	10:55am
DET	Pass	10:55am
BAR	Pass	10:55am
BT	Pass	10:55am

Blank Tests

Test	Status	Time
AIR	Pass	10:56am


Printer Tests

Test	Status	Time
PRNT	Pass	10:56am

CRC Tests

Test	Status	Time
COMP	Pass	10:56am
CAL	Pass	10:56am

Preventive Maintenance
Status: Pass

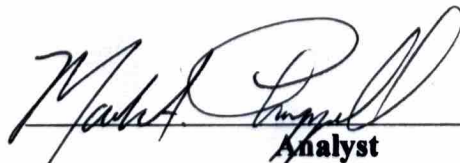

Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County Polk Instrument Location Polk County Jail
Instrument Serial No. 008832 Columbus, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 26 day of February, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

244987
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

POLK COUNTY POLK COUNTY JAIL 740

Serial Number: 008832
Test Date: 02/26/2026

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Loftis, Benjamin C

Permit Number: 0024-4987

Effective:

02/01/2026-02/01/2028

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG431001

Exp Date: 11/05/2026

Test	g/210L	Time
DIAG	Pass	11:10am
AIR BLK	.00	11:11am
ACCY CHK	.07	11:12am
AIR BLK	.00	11:13am
SUB TEST	.00	11:14am
AIR BLK	.00	11:15am
SUB TEST	.00	11:17am
AIR BLK	.00	11:18am

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

POLK COUNTY POLK COUNTY JAIL 740

Serial Number: 008832 Test Record Number: 2031
Test Date: 02/26/2026 Test Time: 11:18am EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	11:18am
FLO	Pass	11:18am
FC	Pass	11:18am

Temperature Tests

Test	Status	Time
FC1	Pass	11:18am
SRC	Pass	11:18am
DET	Pass	11:18am
BAR	Pass	11:18am
BT	Pass	11:18am

Blank Tests

Test	Status	Time
AIR	Pass	11:19am

Printer Tests

Test	Status	Time
PRNT	Pass	11:19am

CRC Tests

Test	Status	Time
COMP	Pass	11:19am
CAL	Pass	11:19am

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County Polk Instrument Location Polk County Jail

Instrument Serial No. 008881 Columbus, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 26 day of February, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.




Signature of Certifying Official

244987
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

POLK COUNTY POLK COUNTY JAIL 740

Serial Number: 008881
Test Date: 02/26/2026

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Loftis, Benjamin C

Permit Number: 0024-4987

Effective:

02/01/2026-02/01/2028

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG506301

Exp Date: 03/04/2027

Test	g/210L	Time
DIAG	Pass	11:11am
AIR BLK	.00	11:12am
ACCY CHK	.08	11:12am
AIR BLK	.00	11:13am
SUB TEST	.00	11:14am
AIR BLK	.00	11:15am
SUB TEST	.00	11:17am
AIR BLK	.00	11:18am

Reported AC? .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

POLK COUNTY POLK COUNTY JAIL 740

Serial Number: 008881 Test Record Number: 1314
Test Date: 02/26/2026 Test Time: 11:18am EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	11:18am
FLO	Pass	11:18am
FC	Pass	11:18am

Temperature Tests

Test	Status	Time
FC1	Pass	11:19am
SRC	Pass	11:19am
DET	Pass	11:19am
BAR	Pass	11:19am
BT	Pass	11:19am

Blank Tests

Test	Status	Time
AIR	Pass	11:19am


Printer Tests

Test	Status	Time
PRNT	Pass	11:19am

CRC Tests

Test	Status	Time
COMP	Pass	11:19am
CAL	Pass	11:19am

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County RANDOLPH Instrument Location LIBERTY POLICE
Instrument Serial No. 008830 DEPARTMENT

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 27 day of FEBRUARY, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Handwritten Signature]
Signature of Certifying Official

239771
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

RANDOLPH COUNTY LIBERTY PD 750

Serial Number: 008830
Test Date: 02/27/2026

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE

Analyst's Name: Galloway, Charles L
Permit Number: 0023-9771
Effective:
02/01/2025-02/01/2027

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG534301
Exp Date: 12/09/2027

Test	g/210L	Time
DIAG	Pass	10:06am
AIR BLK	.00	10:07am
ACCY CHK	.08	10:07am
AIR BLK	.00	10:09am
SUB TEST	.00	10:09am
AIR BLK	.00	10:10am
SUB TEST	.00	10:12am
AIR BLK	.00	10:12am

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

Intox EC/IR-II: Preventive Maintenance

RANDOLPH COUNTY LIBERTY PD 750

Serial Number: 008830 Test Record Number: 968
Test Date: 02/27/2026 Test Time: 10:17am EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	10:17am
FLO	Pass	10:17am
FC	Pass	10:17am

Temperature Tests

Test	Status	Time
FC1	Pass	10:17am
SRC	Pass	10:17am
DET	Pass	10:17am
BAR	Pass	10:17am
BT	Pass	10:17am

Blank Tests

Test	Status	Time
AIR	Pass	10:18am

Printer Tests

Test	Status	Time
PRNT	Pass	10:18am

CRC Tests

Test	Status	Time
COMP	Pass	10:18am
CAL	Pass	10:18am

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Robeson Instrument Location BAT Mobile Unit 7

Instrument Serial No. 00 8090

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 11th day of February, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

2266313
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

ROBESON COUNTY BAT MOBILE UNIT 7 770

Serial Number: 008090

Test Date: 02/11/2026

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Sharpe Jr., Robert J

Permit Number: 1820-8591

Effective:

02/01/2026-02/01/2028

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG506303

Exp Date: 03/04/2027

Test	g/210L	Time
DIAG	Pass	3:13pm
AIR BLK	.00	3:14pm
ACCY CHK	.08	3:15pm
AIR BLK	.00	3:16pm
SUB TEST	.00	3:16pm
AIR BLK	.00	3:17pm
SUB TEST	.00	3:19pm
AIR BLK	.00	3:20pm

Reported AC: 00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

ROBESON COUNTY BAT MOBILE UNIT 7 770

Serial Number: 008090 Test Record Number: 256
Test Date: 02/11/2026 Test Time: 3:21pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	3:21pm
FLO	Pass	3:21pm
FC	Pass	3:22pm

Temperature Tests

Test	Status	Time
FC1	Pass	3:22pm
SRC	Pass	3:22pm
DET	Pass	3:22pm
BAR	Pass	3:22pm
BT	Pass	3:22pm

Blank Tests

Test	Status	Time
AIR	Pass	3:22pm

Printer Tests

Test	Status	Time
PRNT	Pass	3:22pm

CRC Tests

Test	Status	Time
COMP	Pass	3:22pm
CAL	Pass	3:22pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)


County Robeson Instrument Location BAT Mobile Unit 9

Instrument Serial No. 00 8575

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 26th day of February, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

2266313
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

ROBESON COUNTY BAT MOBILE UNIT 9 770

Serial Number: 008575
Test Date: 02/26/2026

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Sharpe Jr., Robert J

Permit Number: 1820-8591

Effective:

02/01/2026-02/01/2028

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG516204

Exp Date: 06/11/2027

Test	g/210L	Time
DIAG	Pass	8:00pm
AIR BLK	.00	8:01pm
ACCY CHK	.08	8:01pm
AIR BLK	.00	8:02pm
SUB TEST	.00	8:04pm
AIR BLK	.00	8:04pm
SUB TEST	.00	8:06pm
AIR BLK	.00	8:07pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

ROBESON COUNTY BAT MOBILE UNIT 9 770

Serial Number: 008575 Test Record Number: 1531
Test Date: 02/26/2026 Test Time: 8:09pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	8:09pm
FLO	Pass	8:09pm
FC	Pass	8:09pm

Temperature Tests

Test	Status	Time
FC1	Pass	8:09pm
SRC	Pass	8:09pm
DET	Pass	8:09pm
BAR	Pass	8:09pm
BT	Pass	8:09pm

Blank Tests

Test	Status	Time
AIR	Pass	8:10pm

Printer Tests

Test	Status	Time
PRNT	Pass	8:10pm

CRC Tests

Test	Status	Time
COMP	Pass	8:10pm
CAL	Pass	8:10pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)


County Robeson Instrument Location BAT Mobile Unit 9

Instrument Serial No. 00 8616

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 26th day of February, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

2266313
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

ROBESON COUNTY BAT MOBILE UNIT 9 770

Serial Number: 008616
Test Date: 02/26/2026

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Sharpe Jr., Robert J

Permit Number: 1820-8591

Effective:

02/01/2026-02/01/2028

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG506303

Exp Date: 03/04/2027

Test	g/210L	Time
DIAG	Pass	8:02pm
AIR BLK	.00	8:03pm
ACCY CHK	.07	8:04pm
AIR BLK	.00	8:05pm
SUB TEST	.00	8:05pm
AIR BLK	.00	8:06pm
SUB TEST	.00	8:08pm
AIR BLK	.00	8:09pm

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR

Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

ROBESON COUNTY BAT MOBILE UNIT 9 770

Serial Number: 008616 Test Record Number: 2928
Test Date: 02/26/2026 Test Time: 8:11pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	8:11pm
FLO	Pass	8:11pm
FC	Pass	8:11pm

Temperature Tests

Test	Status	Time
FC1	Pass	8:11pm
SRC	Pass	8:11pm
DET	Pass	8:11pm
BAR	Pass	8:11pm
BT	Pass	8:11pm

Blank Tests

Test	Status	Time
AIR	Pass	8:12pm

Printer Tests

Test	Status	Time
PRNT	Pass	8:12pm

CRC Tests

Test	Status	Time
COMP	Pass	8:12pm
CAL	Pass	8:12pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)


County Robeson Instrument Location BAT Mobile Unit 9

Instrument Serial No. 00 8647

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 26th day of February, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

2266313
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

ROBESON COUNTY BAT MOBILE UNIT 9 770

Serial Number: 008647
Test Date: 02/26/2026

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Sharpe Jr., Robert J

Permit Number: 1820-8591

Effective:

02/01/2026-02/01/2028

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG516203

Exp Date: 06/11/2027

Test	g/210L	Time
DIAG	Pass	8:14pm
AIR BLK	.00	8:14pm
ACCY CHK	.07	8:15pm
AIR BLK	.00	8:16pm
SUB TEST	.00	8:17pm
AIR BLK	.00	8:18pm
SUB TEST	.00	8:19pm
AIR BLK	.00	8:20pm

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR

Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

ROBESON COUNTY BAT MOBILE UNIT 9 770

Serial Number: 008647 Test Record Number: 2919
Test Date: 02/26/2026 Test Time: 8:21pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	8:21pm
FLO	Pass	8:21pm
FC	Pass	8:22pm

Temperature Tests

Test	Status	Time
FC1	Pass	8:22pm
SRC	Pass	8:22pm
DET	Pass	8:22pm
BAR	Pass	8:22pm
BT	Pass	8:22pm

Blank Tests

Test	Status	Time
AIR	Pass	8:22pm

Printer Tests

Test	Status	Time
PRNT	Pass	8:22pm

CRC Tests

Test	Status	Time
COMP	Pass	8:22pm
CAL	Pass	8:22pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH


PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Robeson Instrument Location BAT Mobile Unit 9
Instrument Serial No. 00 8704

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 26th day of February, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

2266313
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

ROBESON COUNTY BAT MOBILE UNIT 9 770

Serial Number: 008704
Test Date: 02/26/2026

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE

Analyst's Name: Sharpe Jr., Robert J
Permit Number: 1820-8591
Effective:
02/01/2026-02/01/2028

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG506303
Exp Date: 03/04/2027

Test	g/210L	Time
DIAG	Pass	8:02pm
AIR BLK	.00	8:03pm
ACCY CHK	.07	8:04pm
AIR BLK	.00	8:04pm
SUB TEST	.00	8:05pm
AIR BLK	.00	8:06pm
SUB TEST	.00	8:08pm
AIR BLK	.00	8:08pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

ROBESON COUNTY BAT MOBILE UNIT 9 770

Serial Number: 008704 Test Record Number: 968
Test Date: 02/26/2026 Test Time: 8:11pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	8:11pm
FLO	Pass	8:11pm
FC	Pass	8:11pm

Temperature Tests

Test	Status	Time
FC1	Pass	8:11pm
SRC	Pass	8:11pm
DET	Pass	8:11pm
BAR	Pass	8:11pm
BT	Pass	8:11pm

Blank Tests

Test	Status	Time
AIR	Pass	8:12pm

Printer Tests

Test	Status	Time
PRNT	Pass	8:12pm

CRC Tests

Test	Status	Time
COMP	Pass	8:12pm
CAL	Pass	8:12pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)


County Robeson Instrument Location BAT Mobile Unit 9

Instrument Serial No. 008826

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 26th day of February, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

2266313
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

ROBESON COUNTY BAT MOBILE UNIT 9 770

Serial Number: 008826
Test Date: 02/26/2026

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Sharpe Jr., Robert J

Permit Number: 1820-8591

Effective:

02/01/2026-02/01/2028

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG516204

Exp Date: 06/11/2027

Test	g/210L	Time
DIAG	Pass	7:59pm
AIR BLK	.00	8:00pm
ACCY CHK	.07	8:01pm
AIR BLK	.00	8:01pm
SUB TEST	.00	8:03pm
AIR BLK	.00	8:03pm
SUB TEST	.00	8:05pm
AIR BLK	.00	8:06pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

ROBESON COUNTY BAT MOBILE UNIT 9 770

Serial Number: 008826 Test Record Number: 8601
Test Date: 02/26/2026 Test Time: 8:08pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	8:08pm
FLO	Pass	8:08pm
FC	Pass	8:08pm

Temperature Tests

Test	Status	Time
FC1	Pass	8:08pm
SRC	Pass	8:08pm
DET	Pass	8:08pm
BAR	Pass	8:08pm
BT	Pass	8:08pm

Blank Tests

Test	Status	Time
AIR	Pass	8:09pm


Printer Tests

Test	Status	Time
PRNT	Pass	8:09pm

CRC Tests

Test	Status	Time
COMP	Pass	8:09pm
CAL	Pass	8:09pm

Preventive Maintenance
Status: Pass

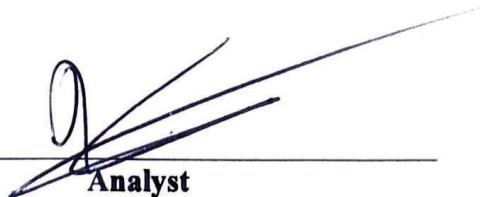

Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County Robeson Instrument Location BAT Mobile Unit 7

Instrument Serial No. 008968

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 11th day of February, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

2266313
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

ROBESON COUNTY BAT MOBILE UNIT 7 770

Serial Number: 008968

Test Date: 02/11/2026

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Sharpe Jr., Robert J

Permit Number: 1820-8591

Effective:

02/01/2026-02/01/2028

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG506303

Exp Date: 03/04/2027

Test	g/210L	Time
DIAG	Pass	3:27pm
AIR BLK	.00	3:28pm
ACCY CHK	.08	3:28pm
AIR BLK	.00	3:29pm
SUB TEST	.00	3:31pm
AIR BLK	.00	3:32pm
SUB TEST	.00	3:33pm
AIR BLK	.00	3:34pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

Intox EC/IR-II: Preventive Maintenance

ROBESON COUNTY BAT MOBILE UNIT 7 770

Serial Number: 008968 Test Record Number: 438
Test Date: 02/11/2026 Test Time: 3:35pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	3:36pm
FLO	Pass	3:36pm
FC	Pass	3:36pm

Temperature Tests

Test	Status	Time
FC1	Pass	3:36pm
SRC	Pass	3:36pm
DET	Pass	3:36pm
BAR	Pass	3:36pm
BT	Pass	3:36pm

Blank Tests

Test	Status	Time
AIR	Pass	3:36pm

Printer Tests

Test	Status	Time
PRNT	Pass	3:36pm

CRC Tests

Test	Status	Time
COMP	Pass	3:37pm
CAL	Pass	3:37pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)


County Robeson Instrument Location BAT Mobile Unit 7

Instrument Serial No. 00 8971

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 11th day of February, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

2266313
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

ROBESON COUNTY BAT MOBILE UNIT 7 770

Serial Number: 008971

Test Date: 02/11/2026

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Sharpe Jr., Robert J

Permit Number: 1820-8591

Effective:

02/01/2026-02/01/2028

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG506302

Exp Date: 03/04/2027

Test	g/210L	Time
DIAG	Pass	3:14pm
AIR BLK	.00	3:15pm
ACCY CHK	.08	3:16pm
AIR BLK	.00	3:17pm
SUB TEST	.00	3:17pm
AIR BLK	.00	3:18pm
SUB TEST	.00	3:20pm
AIR BLK	.00	3:21pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

ROBESON COUNTY BAT MOBILE UNIT 7 770

Serial Number: 008971 Test Record Number: 388
Test Date: 02/11/2026 Test Time: 3:24pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	3:24pm
FLO	Pass	3:24pm
FC	Pass	3:24pm

Temperature Tests

Test	Status	Time
FC1	Pass	3:24pm
SRC	Pass	3:24pm
DET	Pass	3:24pm
BAR	Pass	3:24pm
BT	Pass	3:24pm

Blank Tests

Test	Status	Time
AIR	Pass	3:25pm

Printer Tests

Test	Status	Time
PRNT	Pass	3:25pm

CRC Tests

Test	Status	Time
COMP	Pass	3:25pm
CAL	Pass	3:25pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County Robeson Instrument Location BAT Mobile Unit 7

Instrument Serial No. 00 8972

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 1st day of February, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

2266313
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

ROBESON COUNTY BAT MOBILE UNIT 7 770

Serial Number: 008972
Test Date: 02/11/2026

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE

Analyst's Name: Sharpe Jr., Robert J
Permit Number: 1820-8591
Effective:
02/01/2026-02/01/2028

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG506303
Exp Date: 03/04/2027

Test	g/210L	Time
DIAG	Pass	3:11pm
AIR BLK	.00	3:12pm
ACCY CHK	.08	3:12pm
AIR BLK	.00	3:13pm
SUB TEST	.00	3:14pm
AIR BLK	.00	3:15pm
SUB TEST	.00	3:17pm
AIR BLK	.00	3:18pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

ROBESON COUNTY BAT MOBILE UNIT 7 770

Serial Number: 008972 Test Record Number: 450
Test Date: 02/11/2026 Test Time: 3:19pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	3:19pm
FLO	Pass	3:19pm
FC	Pass	3:19pm

Temperature Tests

Test	Status	Time
FC1	Pass	3:19pm
SRC	Pass	3:19pm
DET	Pass	3:19pm
BAR	Pass	3:19pm
BT	Pass	3:19pm

Blank Tests

Test	Status	Time
AIR	Pass	3:20pm

Printer Tests

Test	Status	Time
PRNT	Pass	3:20pm

CRC Tests

Test	Status	Time
COMP	Pass	3:20pm
CAL	Pass	3:20pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH


**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County Sampson Instrument Location BAT Mobile Unit 9
Instrument Serial No. 008575

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 28th day of February, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

2266313
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

SAMPSON COUNTY BAT MOBILE UNIT 9 810

Serial Number: 008575
Test Date: 02/28/2026

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Sharpe Jr., Robert J

Permit Number: 1820-8591

Effective:

02/01/2026-02/01/2028

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG516204

Exp Date: 06/11/2027

Test	g/210L	Time
DIAG	Pass	8:10pm
AIR BLK	.00	8:11pm
ACCY CHK	.07	8:11pm
AIR BLK	.00	8:12pm
SUB TEST	.00	8:13pm
AIR BLK	.00	8:14pm
SUB TEST	.00	8:15pm
AIR BLK	.00	8:16pm

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

SAMPSON COUNTY BAT MOBILE UNIT 9 810

Serial Number: 008575 Test Record Number: 1535
Test Date: 02/28/2026 Test Time: 8:17pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	8:18pm
FLO	Pass	8:18pm
FC	Pass	8:18pm

Temperature Tests

Test	Status	Time
FC1	Pass	8:18pm
SRC	Pass	8:18pm
DET	Pass	8:18pm
BAR	Pass	8:18pm
BT	Pass	8:18pm

Blank Tests

Test	Status	Time
AIR	Pass	8:18pm

Printer Tests

Test	Status	Time
PRNT	Pass	8:19pm

CRC Tests

Test	Status	Time
COMP	Pass	8:19pm
CAL	Pass	8:19pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH


PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Sampson Instrument Location BAT Mobile Unit 9
Instrument Serial No. 00 8616

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 28th day of February, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

2266313
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

SAMPSON COUNTY BAT MOBILE UNIT 9 810

Serial Number: 008616
Test Date: 02/28/2026

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Sharpe Jr., Robert J

Permit Number: 1820-8591

Effective:

02/01/2026-02/01/2028

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG506303

Exp Date: 03/04/2027

Test	g/210L	Time
DIAG	Pass	8:13pm
AIR BLK	.00	8:14pm
ACCY CHK	.07	8:14pm
AIR BLK	.00	8:15pm
SUB TEST	.00	8:16pm
AIR BLK	.00	8:17pm
SUB TEST	.00	8:19pm
AIR BLK	.00	8:20pm

Reported AC: .00 g/210L

Signature of  Chemical Analyst

Court CVR



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

SAMPSON COUNTY BAT MOBILE UNIT 9 810

Serial Number: 008616 Test Record Number: 2933
Test Date: 02/28/2026 Test Time: 8:21pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	8:21pm
FLO	Pass	8:21pm
FC	Pass	8:21pm

Temperature Tests

Test	Status	Time
FC1	Pass	8:22pm
SRC	Pass	8:22pm
DET	Pass	8:22pm
BAR	Pass	8:22pm
BT	Pass	8:22pm

Blank Tests

Test	Status	Time
AIR	Pass	8:22pm


Printer Tests

Test	Status	Time
PRNT	Pass	8:22pm

CRC Tests

Test	Status	Time
COMP	Pass	8:22pm
CAL	Pass	8:22pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)


County Sampson Instrument Location BAT Mobile Unit 9

Instrument Serial No. 008647

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 28th day of February, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

2266313
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

SAMPSON COUNTY BAT MOBILE UNIT 9 810

Serial Number: 008647
Test Date: 02/28/2026

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Sharpe Jr., Robert J

Permit Number: 1820-8591

Effective:

02/01/2026-02/01/2028

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG516203

Exp Date: 06/11/2027

Test	g/210L	Time
DIAG	Pass	8:13pm
AIR BLK	.00	8:14pm
ACCY CHK	.08	8:15pm
AIR BLK	.00	8:16pm
SUB TEST	.00	8:16pm
AIR BLK	.00	8:17pm
SUB TEST	.00	8:19pm
AIR BLK	.00	8:20pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

SAMPSON COUNTY BAT MOBILE UNIT 9 810

Serial Number: 008647 Test Record Number: 2923
Test Date: 02/28/2026 Test Time: 8:21pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	8:21pm
FLO	Pass	8:21pm
FC	Pass	8:22pm

Temperature Tests

Test	Status	Time
FC1	Pass	8:22pm
SRC	Pass	8:22pm
DET	Pass	8:22pm
BAR	Pass	8:22pm
BT	Pass	8:22pm

Blank Tests

Test	Status	Time
AIR	Pass	8:22pm

Printer Tests

Test	Status	Time
PRNT	Pass	8:22pm

CRC Tests

Test	Status	Time
COMP	Pass	8:22pm
CAL	Pass	8:22pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County Sampson Instrument Location BAT Mobile Unit 9

Instrument Serial No. 00 8704

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 28th day of February, 20 26 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.





Signature of Certifying Official

2266 313
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

SAMPSON COUNTY BAT MOBILE UNIT 9 810

Serial Number: 008704
Test Date: 02/28/2026

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Sharpe Jr., Robert J

Permit Number: 1820-8591

Effective:

02/01/2026-02/01/2028

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG506303

Exp Date: 03/04/2027

Test	g/210L	Time
DIAG	Pass	8:13pm
AIR BLK	.00	8:14pm
ACCY CHK	.07	8:14pm
AIR BLK	.00	8:15pm
SUB TEST	.00	8:16pm
AIR BLK	.00	8:17pm
SUB TEST	.00	8:19pm
AIR BLK	.00	8:20pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

SAMPSON COUNTY BAT MOBILE UNIT 9 810

Serial Number: 008704 Test Record Number: 972
Test Date: 02/28/2026 Test Time: 8:21pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	8:21pm
FLO	Pass	8:21pm
FC	Pass	8:21pm

Temperature Tests

Test	Status	Time
FC1	Pass	8:21pm
SRC	Pass	8:21pm
DET	Pass	8:21pm
BAR	Pass	8:21pm
BT	Pass	8:21pm

Blank Tests

Test	Status	Time
AIR	Pass	8:22pm

Printer Tests

Test	Status	Time
PRNT	Pass	8:22pm

CRC Tests

Test	Status	Time
COMP	Pass	8:22pm
CAL	Pass	8:22pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**


County Sampson Instrument Location BAT Mobile Unit 9

Instrument Serial No. 008826

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 28th day of February, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

2266313
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

SAMPSON COUNTY BAT MOBILE UNIT 9 810

Serial Number: 008826
Test Date: 02/28/2026

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE

Analyst's Name: Sharpe Jr., Robert J
Permit Number: 1820-8591
Effective:
02/01/2026-02/01/2028

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG516204
Exp Date: 06/11/2027

Test	g/210L	Time
DIAG	Pass	8:09pm
AIR BLK	.00	8:10pm
ACCY CHK	.07	8:11pm
AIR BLK	.00	8:11pm
SUB TEST	.00	8:12pm
AIR BLK	.00	8:13pm
SUB TEST	.00	8:15pm
AIR BLK	.00	8:15pm

Reported AC: ~~.00~~ g/210L

Signature of Chemical Analyst

Court CVR



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

SAMPSON COUNTY BAT MOBILE UNIT 9 810

Serial Number: 008826 Test Record Number: 8606
Test Date: 02/28/2026 Test Time: 8:16pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	8:16pm
FLO	Pass	8:16pm
FC	Pass	8:16pm

Temperature Tests

Test	Status	Time
FC1	Pass	8:17pm
SRC	Pass	8:17pm
DET	Pass	8:17pm
BAR	Pass	8:17pm
BT	Pass	8:17pm

Blank Tests

Test	Status	Time
AIR	Pass	8:17pm


Printer Tests

Test	Status	Time
PRNT	Pass	8:17pm

CRC Tests

Test	Status	Time
COMP	Pass	8:17pm
CAL	Pass	8:17pm

Preventive Maintenance
Status: Pass

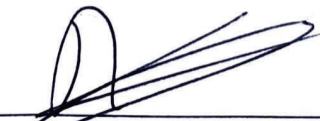

Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County Surry Instrument Location Elkin Police
Instrument Serial No. 008926 Department

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 9th day of February, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Timothy Harbo
Signature of Certifying Official

633175
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

SURRY COUNTY ELKIN PD 850

Serial Number: 008926
Test Date: 02/09/2026

Citation Number: M0000000-0
Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Hanks, Timothy S

Permit Number: 0063-3175

Effective:

02/01/2025-02/01/2027

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG417803

Exp Date: 06/26/2026

Test	g/210L	Time
DIAG	Pass	1:59pm
AIR BLK	.00	2:00pm
ACCY CHK	.08	2:01pm
AIR BLK	.00	2:02pm
SUB TEST	.00	2:03pm
AIR BLK	.00	2:04pm
SUB TEST	.00	2:05pm
AIR BLK	.00	2:06pm

Reported AC: .00 g/210L

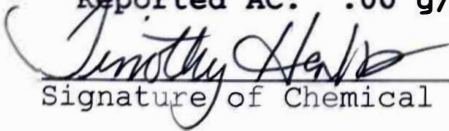
Signature of Chemical Analyst

Court CVR


Analyst

Intox EC/IR-II: Preventive Maintenance

SURRY COUNTY ELKIN PD 850

Serial Number: 008926 Test Record Number: 1247
Test Date: 02/09/2026 Test Time: 2:07pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	2:07pm
FLO	Pass	2:07pm
FC	Pass	2:07pm

Temperature Tests

Test	Status	Time
FC1	Pass	2:07pm
SRC	Pass	2:07pm
DET	Pass	2:07pm
BAR	Pass	2:07pm
BT	Pass	2:07pm

Blank Tests

Test	Status	Time
AIR	Pass	2:08pm

Printer Tests

Test	Status	Time
PRNT	Pass	2:08pm

CRC Tests

Test	Status	Time
COMP	Pass	2:08pm
CAL	Pass	2:08pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County Surry Instrument Location Surry County Jail
Dobson, NC
Instrument Serial No. 008934

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 9th day of February, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Timothy Hambro
Signature of Certifying Official

633175
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

SURRY COUNTY SURRY CO JAIL 850

Serial Number: 008934
Test Date: 02/09/2026

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: Hanks, Timothy S
Permit Number: 0063-3175
Effective:
02/01/2025-02/01/2027

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG534301
Exp Date: 12/09/2027


Test	g/210L	Time
DIAG	Pass	4:37pm
AIR BLK	.00	4:38pm
ACCY CHK	.07	4:38pm
AIR BLK	.00	4:40pm
SUB TEST	.00	4:40pm
AIR BLK	.00	4:41pm
SUB TEST	.00	4:43pm
AIR BLK	.00	4:44pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR

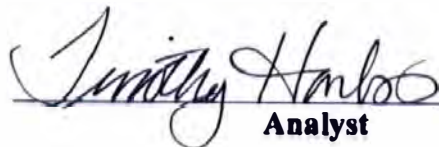

Analyst

Intox EC/IR-II: Preventive Maintenance

SURRY COUNTY SURRY CO JAIL 850

Serial Number: 008934 Test Record Number: 2825
Test Date: 02/09/2026 Test Time: 4:45pm EST

System Check: Passed

Baseline Tests

Test	Status	Time
IR	Pass	4:45pm
FLO	Pass	4:45pm
FC	Pass	4:45pm

Temperature Tests

Test	Status	Time
FC1	Pass	4:45pm
SRC	Pass	4:45pm
DET	Pass	4:45pm
BAR	Pass	4:45pm
BT	Pass	4:45pm

Blank Tests

Test	Status	Time
AIR	Pass	4:46pm


Printer Tests

Test	Status	Time
PRNT	Pass	4:46pm

CRC Tests

Test	Status	Time
COMP	Pass	4:46pm
CAL	Pass	4:46pm

Preventive Maintenance
Status: Pass

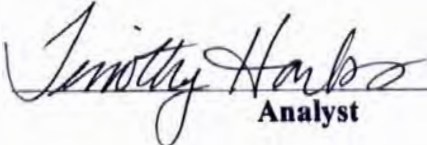
Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County Surry Instrument Location Mount Airy Police
Instrument Serial No. 008943 Department

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 9th day of February, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Timothy Harbo
Signature of Certifying Official

633175
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

SURRY COUNTY MOUNT AIRY PD 850

Serial Number: 008943

Test Date: 02/09/2026

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Hanks, Timothy S

Permit Number: 0063-3175

Effective:

02/01/2025-02/01/2027

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG516203

Exp Date: 06/11/2027

Test	g/210L	Time
DIAG	Pass	3:34pm
AIR BLK	.00	3:35pm
ACCY CHK	.07	3:36pm
AIR BLK	.00	3:37pm
SUB TEST	.00	3:37pm
AIR BLK	.00	3:38pm
SUB TEST	.00	3:40pm
AIR BLK	.00	3:40pm

Reported AC: .00 g/210L



 Signature of Chemical Analyst

Court CVR



 Analyst

Intox EC/IR-II: Preventive Maintenance

SURRY COUNTY MOUNT AIRY PD 850

Serial Number: 008943 Test Record Number: 2815
Test Date: 02/09/2026 Test Time: 3:41pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	3:42pm
FLO	Pass	3:42pm
FC	Pass	3:42pm

Temperature Tests

Test	Status	Time
FC1	Pass	3:42pm
SRC	Pass	3:42pm
DET	Pass	3:42pm
BAR	Pass	3:42pm
BT	Pass	3:42pm

Blank Tests

Test	Status	Time
AIR	Pass	3:42pm

Printer Tests

Test	Status	Time
PRNT	Pass	3:42pm

CRC Tests

Test	Status	Time
COMP	Pass	3:43pm
CAL	Pass	3:43pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Swain Instrument Location Cherokee Tribal Det.
Instrument Serial No. 008782 Cherokee, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 5th day of February, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Cliff R. Cuth
Signature of Certifying Official

843310
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

SWAIN COUNTY CHEROKEE DETENTION 860

Serial Number: 008782
Test Date: 02/06/2026

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE

Analyst's Name: Cutler, Daniel R
Permit Number: 0084-3310
Effective:
02/01/2026-02/01/2028

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG505001
Exp Date: 02/19/2027

Test	g/210L	Time
DIAG	Pass	11:06am
AIR BLK	.00	11:07am
ACCY CHK	.07	11:08am
AIR BLK	.00	11:09am
SUB TEST	.00	11:10am
AIR BLK	.00	11:11am
SUB TEST	.00	11:12am
AIR BLK	.00	11:13am

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

Intox EC/IR-II: Preventive Maintenance

SWAIN COUNTY CHEROKEE DETENTION 860

Serial Number: 008782 Test Record Number: 1643
Test Date: 02/06/2026 Test Time: 11:14am EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	11:14am
FLO	Pass	11:14am
FC	Pass	11:14am

Temperature Tests

Test	Status	Time
FC1	Pass	11:14am
SRC	Pass	11:14am
DET	Pass	11:14am
BAR	Pass	11:14am
BT	Pass	11:14am

Blank Tests

Test	Status	Time
AIR	Pass	11:15am

Printer Tests

Test	Status	Time
PRNT	Pass	11:15am

CRC Tests

Test	Status	Time
COMP	Pass	11:15am
CAL	Pass	11:15am

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Tyrrell Instrument Location Tyrrell Co. S.O.
Instrument Serial No. 008902 412 Main St., Columbia, N.C.

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 11th day of February, 2024 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

377722
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

TYRRELL COUNTY SHERIFF'S OFFICE 880

Serial Number: 008902
Test Date: 02/11/2026

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: Gray, Kelly D
Permit Number: 0037-7722
Effective:
02/01/2026-02/01/2028

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG516204
Exp Date: 06/11/2027

Test	g/210L	Time
DIAG	Pass	2:20pm
AIR BLK	.00	2:20pm
ACCY CHK	.07	2:21pm
AIR BLK	.00	2:22pm
SUB TEST	.00	2:23pm
AIR BLK	.00	2:24pm
SUB TEST	.00	2:26pm
AIR BLK	.00	2:26pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

Intox EC/IR-II: Preventive Maintenance

TYRRELL COUNTY SHERIFF'S OFFICE 880

Serial Number: 008902 Test Record Number: 1279
Test Date: 02/11/2026 Test Time: 2:27pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	2:28pm
FLO	Pass	2:28pm
FC	Pass	2:28pm

Temperature Tests

Test	Status	Time
FC1	Pass	2:28pm
SRC	Pass	2:28pm
DET	Pass	2:28pm
BAR	Pass	2:28pm
BT	Pass	2:28pm

Blank Tests

Test	Status	Time
AIR	Pass	2:28pm

Printer Tests

Test	Status	Time
PRNT	Pass	2:29pm

CRC Tests

Test	Status	Time
COMP	Pass	2:29pm
CAL	Pass	2:29pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Union Instrument Location Stallings PD
Instrument Serial No. 0082094 Stallings, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 10th day of February, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Handwritten Signature]
Signature of Certifying Official

849845
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

UNION COUNTY STALLINGS PD 890

Serial Number: 008694

Test Date: 02/10/2026

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Helms, Bryce A

Permit Number: 0084-9845

Effective:

02/01/2025-02/01/2027

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG534301

Exp Date: 12/09/2027


Test	g/210L	Time
DIAG	Pass	3:11pm
AIR BLK	.00	3:12pm
ACCY CHK	.08	3:12pm
AIR BLK	.00	3:13pm
SUB TEST	.00	3:14pm
AIR BLK	.00	3:15pm
SUB TEST	.00	3:16pm
AIR BLK	.00	3:17pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR

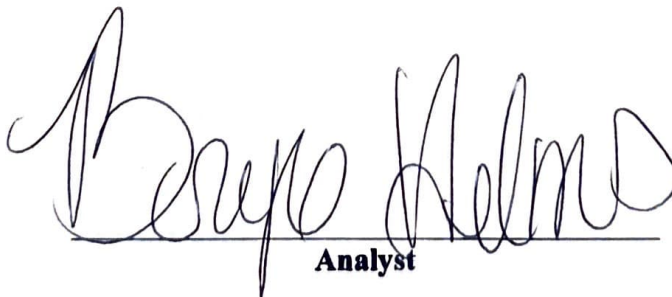

Analyst

Intox EC/IR-II: Preventive Maintenance

UNION COUNTY STALLINGS PD 890

Serial Number: 008694 Test Record Number: 1987
Test Date: 02/10/2026 Test Time: 3:18pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	3:18pm
FLO	Pass	3:18pm
FC	Pass	3:18pm

Temperature Tests

Test	Status	Time
FC1	Pass	3:19pm
SRC	Pass	3:19pm
DET	Pass	3:19pm
BAR	Pass	3:19pm
BT	Pass	3:19pm

Blank Tests

Test	Status	Time
AIR	Pass	3:19pm


Printer Tests

Test	Status	Time
PRNT	Pass	3:19pm

CRC Tests

Test	Status	Time
COMP	Pass	3:20pm
CAL	Pass	3:20pm

Preventive Maintenance
Status: Pass

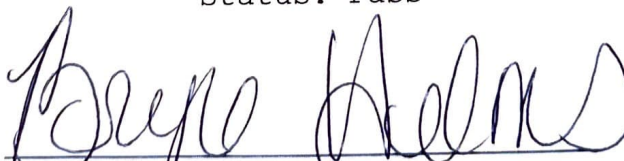

Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Union Instrument Location Stallings PD
Instrument Serial No. 008927 Stallings, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 17th day of February, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

849845
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

UNION COUNTY STALLINGS PD 890

Serial Number: 008927
Test Date: 02/17/2026

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: Helms, Bryce A
Permit Number: 0084-9845
Effective:
02/01/2025-02/01/2027

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG534301
Exp Date: 12/09/2027


Test	g/210L	Time
DIAG	Pass	12:46pm
AIR BLK	.00	12:47pm
ACCY CHK	.07	12:47pm
AIR BLK	.00	12:49pm
SUB TEST	.00	12:49pm
AIR BLK	.00	12:50pm
SUB TEST	.00	12:52pm
AIR BLK	.00	12:53pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR

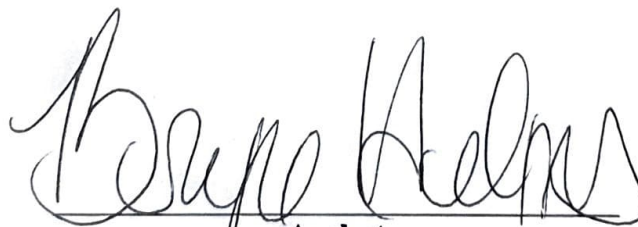

Analyst

Intox EC/IR-II: Preventive Maintenance

UNION COUNTY STALLINGS PD 890

Serial Number: 008927 Test Record Number: 1320
Test Date: 02/17/2026 Test Time: 12:53pm EST

System Check: Passed

Baseline Tests

Test	Status	Time
IR	Pass	12:54pm
FLO	Pass	12:54pm
FC	Pass	12:54pm

Temperature Tests

Test	Status	Time
FC1	Pass	12:54pm
SRC	Pass	12:54pm
DET	Pass	12:54pm
BAR	Pass	12:54pm
BT	Pass	12:54pm

Blank Tests

Test	Status	Time
AIR	Pass	12:55pm


Printer Tests

Test	Status	Time
PRNT	Pass	12:55pm

CRC Tests

Test	Status	Time
COMP	Pass	12:55pm
CAL	Pass	12:55pm

Preventive Maintenance
Status: Pass

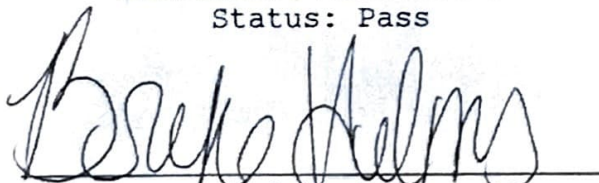

Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH


**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County Washington Instrument Location Washington Co SO.
Instrument Serial No. 008829 120 Adams St, Plymouth, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 11th day of February, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Key Pur
Signature of Certifying Official

377722
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

WASHINGTON COUNTY SHERIFF'S OFFICE 930

Serial Number: 008829
Test Date: 02/11/2026

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE

Analyst's Name: Gray, Kelly D
Permit Number: 0037-7722
Effective:
02/01/2026-02/01/2028

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG506301
Exp Date: 03/04/2027

Test	g/210L	Time
DIAG	Pass	1:01pm
AIR BLK	.00	1:01pm
ACCY CHK	.08	1:02pm
AIR BLK	.00	1:04pm
SUB TEST	.00	1:05pm
AIR BLK	.00	1:06pm
SUB TEST	.00	1:07pm
AIR BLK	.00	1:08pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

Intox EC/IR-II: Preventive Maintenance

WASHINGTON COUNTY SHERIFF'S OFFICE 930

Serial Number: 008829 Test Record Number: 1331
Test Date: 02/11/2026 Test Time: 1:09pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	1:10pm
FLO	Pass	1:10pm
FC	Pass	1:10pm

Temperature Tests

Test	Status	Time
FC1	Pass	1:10pm
SRC	Pass	1:10pm
DET	Pass	1:10pm
BAR	Pass	1:10pm
BT	Pass	1:10pm

Blank Tests

Test	Status	Time
AIR	Pass	1:10pm

Printer Tests

Test	Status	Time
PRNT	Pass	1:10pm

CRC Tests

Test	Status	Time
COMP	Pass	1:11pm
CAL	Pass	1:11pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County Watauga Instrument Location BAT Mobile Unit 13

Instrument Serial No. 008869

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 28th day of February, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



John Lanier
Signature of Certifying Official

1604930
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

WATAUGA COUNTY BAT MOBILE UNIT 13 940

Serial Number: 008869
Test Date: 02/28/2026

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Lanier Jr., John P

Permit Number: 4582-9118

Effective:

02/01/2026-02/01/2028

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG417803

Exp Date: 06/26/2026


Test	g/210L	Time
DIAG	Pass	8:32pm
AIR BLK	.00	8:33pm
ACCY CHK	.08	8:34pm
AIR BLK	.00	8:35pm
SUB TEST	.00	8:36pm
AIR BLK	.00	8:36pm
SUB TEST	.00	8:38pm
AIR BLK	.00	8:39pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

Intox EC/IR-II: Preventive Maintenance

WATAUGA COUNTY BAT MOBILE UNIT 13 940

Serial Number: 008869 Test Record Number: 2152
Test Date: 02/28/2026 Test Time: 8:40pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	8:40pm
FLO	Pass	8:40pm
FC	Pass	8:41pm

Temperature Tests

Test	Status	Time
FC1	Pass	8:41pm
SRC	Pass	8:41pm
DET	Pass	8:41pm
BAR	Pass	8:41pm
BT	Pass	8:41pm

Blank Tests

Test	Status	Time
AIR	Pass	8:41pm

Printer Tests

Test	Status	Time
PRNT	Pass	8:41pm

CRC Tests

Test	Status	Time
COMP	Pass	8:42pm
CAL	Pass	8:42pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County Watayga Instrument Location BAT Mobile Unit 13

Instrument Serial No. 008898

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 28th day of February, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



John Parier
Signature of Certifying Official

1604930
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

WATAUGA COUNTY BAT MOBILE UNIT 13 940

Serial Number: 008898
Test Date: 02/28/2026

Citation Number: M0000000-0
Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Lanier Jr., John P

Permit Number: 4582-9118

Effective:

02/01/2026-02/01/2028

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG506302

Exp Date: 03/04/2027

Test	g/210L	Time
DIAG	Pass	8:36pm
AIR BLK	.00	8:37pm
ACCY CHK	.07	8:38pm
AIR BLK	.00	8:38pm
SUB TEST	.00	8:39pm
AIR BLK	.00	8:40pm
SUB TEST	.00	8:41pm
AIR BLK	.00	8:42pm

Reported AC: .00 g/210L

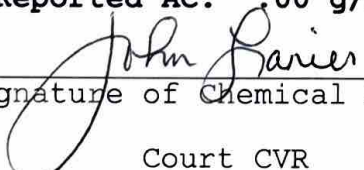

Signature of Chemical Analyst

Court CVR



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

WATAUGA COUNTY BAT MOBILE UNIT 13 940

Serial Number: 008898 Test Record Number: 2097
Test Date: 02/28/2026 Test Time: 8:43pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	8:43pm
FLO	Pass	8:43pm
FC	Pass	8:44pm

Temperature Tests

Test	Status	Time
FC1	Pass	8:44pm
SRC	Pass	8:44pm
DET	Pass	8:44pm
BAR	Pass	8:44pm
BT	Pass	8:44pm

Blank Tests

Test	Status	Time
AIR	Pass	8:44pm


Printer Tests

Test	Status	Time
PRNT	Pass	8:44pm

CRC Tests

Test	Status	Time
COMP	Pass	8:45pm
CAL	Pass	8:45pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Watauga Instrument Location BAT Mobile Unit 13
Instrument Serial No. 008939

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 28th day of February, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



John Ranier
Signature of Certifying Official

1604930
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

WATAUGA COUNTY BAT MOBILE UNIT 13 940

Serial Number: 008939
Test Date: 02/28/2026

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Lanier Jr., John P

Permit Number: 4582-9118

Effective:

02/01/2026-02/01/2028

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG506302

Exp Date: 03/04/2027

Test	g/210L	Time
DIAG	Pass	8:38pm
AIR BLK	.00	8:39pm
ACCY CHK	.07	8:40pm
AIR BLK	.00	8:41pm
SUB TEST	.00	8:42pm
AIR BLK	.00	8:43pm
SUB TEST	.00	8:44pm
AIR BLK	.00	8:45pm

Reported AC: .00 g/210L

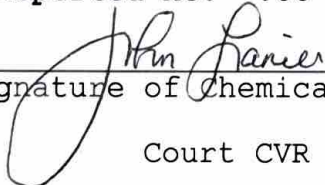

Signature of Chemical Analyst

Court CVR



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

WATAUGA COUNTY BAT MOBILE UNIT 13 940

Serial Number: 008939 Test Record Number: 1970
Test Date: 02/28/2026 Test Time: 8:45pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	8:46pm
FLO	Pass	8:46pm
FC	Pass	8:46pm

Temperature Tests

Test	Status	Time
FC1	Pass	8:46pm
SRC	Pass	8:46pm
DET	Pass	8:46pm
BAR	Pass	8:46pm
BT	Pass	8:46pm

Blank Tests

Test	Status	Time
AIR	Pass	8:47pm

Printer Tests

Test	Status	Time
PRNT	Pass	8:47pm

CRC Tests

Test	Status	Time
COMP	Pass	8:47pm
CAL	Pass	8:47pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County Wayne Instrument Location Seymour Johnson AFB
Instrument Serial No. 008786 1010 Vermont Garrison St.
Goldsboro, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 10th day of February, 2020 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

377722
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

WAYNE COUNTY SEYMOUR JOHNSON AFB 950

Serial Number: 008786
Test Date: 02/10/2026

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Gray, Kelly D

Permit Number: 0037-7722

Effective:

02/01/2026-02/01/2028

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG501303

Exp Date: 01/13/2027

Test	g/210L	Time
DIAG	Pass	10:34am
AIR BLK	.00	10:34am
ACCY CHK	.08	10:35am
AIR BLK	.00	10:36am
SUB TEST	.00	10:37am
AIR BLK	.00	10:38am
SUB TEST	.00	10:39am
AIR BLK	.00	10:40am

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

Intox EC/IR-II: Preventive Maintenance

WAYNE COUNTY SEYMOUR JOHNSON AFB 950

Serial Number: 008786 Test Record Number: 527
Test Date: 02/10/2026 Test Time: 10:41am EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	10:42am
FLO	Pass	10:42am
FC	Pass	10:42am

Temperature Tests

Test	Status	Time
FC1	Pass	10:42am
SRC	Pass	10:42am
DET	Pass	10:42am
BAR	Pass	10:42am
BT	Pass	10:42am

Blank Tests

Test	Status	Time
AIR	Pass	10:43am

Printer Tests

Test	Status	Time
PRNT	Pass	10:43am

CRC Tests

Test	Status	Time
COMP	Pass	10:43am
CAL	Pass	10:43am

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County Yancey Instrument Location Yancey County Jail
Instrument Serial No. 008653 Burnsville, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 9 day of February, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

244987
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

YANCEY COUNTY YANCEY COUNTY JAIL 990

Serial Number: 008653
Test Date: 02/09/2026

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE

Analyst's Name: Loftis, Benjamin C
Permit Number: 0024-4987
Effective:
02/01/2026-02/01/2028

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG503001
Exp Date: 01/30/2027

Test	g/210L	Time
DIAG	Pass	10:59am
AIR BLK	.00	11:00am
ACCY CHK	.08	11:01am
AIR BLK	.00	11:02am
SUB TEST	.00	11:02am
AIR BLK	.00	11:03am
SUB TEST	.00	11:05am
AIR BLK	.00	11:06am

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

YANCEY COUNTY YANCEY COUNTY JAIL 990

Serial Number: 008653 Test Record Number: 1904
Test Date: 02/09/2026 Test Time: 11:06am EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	11:06am
FLO	Pass	11:06am
FC	Pass	11:07am

Temperature Tests

Test	Status	Time
FC1	Pass	11:07am
SRC	Pass	11:07am
DET	Pass	11:07am
BAR	Pass	11:07am
BT	Pass	11:07am

Blank Tests

Test	Status	Time
AIR	Pass	11:08am


Printer Tests

Test	Status	Time
PRNT	Pass	11:08am

CRC Tests

Test	Status	Time
COMP	Pass	11:08am
CAL	Pass	11:08am

Preventive Maintenance
Status: Pass



Analyst