

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County ALAMANCE Instrument Location ALAMANCE Co JAIL

Instrument Serial No. 008853 109 S. Maple St Graham, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 6 day of February, 2024 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Simon Stokes Brasas
Signature of Certifying Official

662
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

ALAMANCE COUNTY JAIL 000

Serial Number: 008853

Test Date: 02/06/2024

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Barnes, Simon S

Permit Number: 0014-6221

Effective:

10/01/2023-10/01/2025

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG308703

Exp Date: 03/28/2025


Test	g/210L	Time
DIAG	Pass	10:44am
AIR BLK	.00	10:45am
ACCY CHK	.08	10:45am
AIR BLK	.00	10:47am
SUB TEST	.00	10:47am
AIR BLK	.00	10:48am
SUB TEST	.00	10:50am
AIR BLK	.00	10:51am

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

ALAMANCE COUNTY JAIL 000

Serial Number: 008853 Test Record Number: 4484
Test Date: 02/06/2024 Test Time: 10:52am EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	10:52am
FLO	Pass	10:52am
FC	Pass	10:52am

Temperature Tests

Test	Status	Time
FC1	Pass	10:52am
SRC	Pass	10:52am
DET	Pass	10:52am
BAR	Pass	10:52am
BT	Pass	10:52am

Blank Tests

Test	Status	Time
AIR	Pass	10:53am

Printer Tests

Test	Status	Time
PRNT	Pass	10:53am

CRC Tests

Test	Status	Time
COMP	Pass	10:53am
CAL	Pass	10:53am

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Alamance Instrument Location Alamance Co Jail

Instrument Serial No. 008913 109 S. Maple St Graham, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 6 day of February, 2024 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Sam Akes Bowers
Signature of Certifying Official

662
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

ALAMANCE COUNTY ALAMANCE CO. JAIL 000

Serial Number: 008913

Test Date: 02/06/2024

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Barnes, Simon S

Permit Number: 0014-6221

Effective:

10/01/2023-10/01/2025

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG308703

Exp Date: 03/28/2025

Test	g/210L	Time
DIAG	Pass	10:45am
AIR BLK	.00	10:46am
ACCY CHK	.07	10:46am
AIR BLK	.00	10:48am
SUB TEST	.00	10:48am
AIR BLK	.00	10:49am
SUB TEST	.00	10:50am
AIR BLK	.00	10:51am

Reported AC: .00 g/210L

Simon Stokes Barnes
Signature of Chemical Analyst

Court CVR

Simon Stokes Barnes
Analyst

Intox EC/IR-II: Preventive Maintenance

ALAMANCE COUNTY ALAMANCE CO. JAIL 000

Serial Number: 008913

Test Record Number: 5293

Test Date: 02/06/2024

Test Time: 10:52am EST

System Check: Passed

Baseline Tests

Test	Status	Time
IR	Pass	10:53am
FLO	Pass	10:53am
FC	Pass	10:53am

Temperature Tests

Test	Status	Time
FC1	Pass	10:53am
SRC	Pass	10:53am
DET	Pass	10:53am
BAR	Pass	10:53am
BT	Pass	10:53am

Blank Tests

Test	Status	Time
AIR	Pass	10:53am

Printer Tests

Test	Status	Time
PRNT	Pass	10:53am

CRC Tests

Test	Status	Time
COMP	Pass	10:54am
CAL	Pass	10:54am

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County ALEXANDER Instrument Location ALEXANDER CO. S.C.
Instrument Serial No. 008813 TAYLORSVILLE NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 20 day of FEBRUARY, 2024 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

646
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

ALEXANDER COUNTY ALEXANDER COUNTY SO
010

Serial Number: 008813

Test Date: 02/20/2024

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Fleming, Tina S

Permit Number: 0027-4970

Effective:

07/01/2022-07/01/2024

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG302703

Exp Date: 01/27/2025


Test	g/210L	Time
DIAG	Pass	10:10am
AIR BLK	.00	10:11am
ACCY CHK	.08	10:11am
AIR BLK	.00	10:13am
SUB TEST	.00	10:14am
AIR BLK	.00	10:15am
SUB TEST	.00	10:16am
AIR BLK	.00	10:17am

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

ALEXANDER COUNTY ALEXANDER COUNTY SO 010

Serial Number: 008813 Test Record Number: 2336
Test Date: 02/20/2024 Test Time: 10:18am EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	10:18am
FLO	Pass	10:18am
FC	Pass	10:18am

Temperature Tests

Test	Status	Time
FC1	Pass	10:18am
SRC	Pass	10:18am
DET	Pass	10:18am
BAR	Pass	10:18am
BT	Pass	10:18am

Blank Tests

Test	Status	Time
AIR	Pass	10:19am


Printer Tests

Test	Status	Time
PRNT	Pass	10:19am

CRC Tests

Test	Status	Time
COMP	Pass	10:19am
CAL	Pass	10:19am

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County ANSON Instrument Location ANSON COUNTY
Instrument Serial No. 008597 SHERIFF'S OFFICE

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 22 day of FEBRUARY, 2024 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

667
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

ANSON COUNTY SHERIFF'S OFFICE 030

Serial Number: 008597

Test Date: 02/22/2024

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Galloway, Charles L

Permit Number: 0023-9771

Effective:

10/01/2023-10/01/2025

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

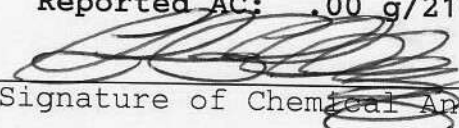
Test Type: Breath Test

Lot Number: AG308003

Exp Date: 03/21/2025

Test	g/210L	Time
DIAG	Pass	1:39pm
AIR BLK	.00	1:40pm
ACCY CHK	.07	1:40pm
AIR BLK	.00	1:41pm
SUB TEST	.00	1:42pm
AIR BLK	.00	1:43pm
SUB TEST	.00	1:45pm
AIR BLK	.00	1:46pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

ANSON COUNTY SHERIFF'S OFFICE 030

Serial Number: 008597 Test Record Number: 1909
Test Date: 02/22/2024 Test Time: 1:46pm EST

System Check: Passed

Baseline Tests

Test	Status	Time
IR	Pass	1:47pm
FLO	Pass	1:47pm
FC	Pass	1:47pm

Temperature Tests

Test	Status	Time
FC1	Pass	1:47pm
SRC	Pass	1:47pm
DET	Pass	1:47pm
BAR	Pass	1:47pm
BT	Pass	1:47pm

Blank Tests

Test	Status	Time
AIR	Pass	1:48pm

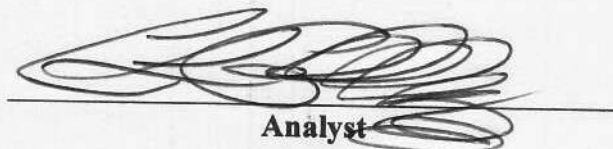
Printer Tests

Test	Status	Time
PRNT	Pass	1:48pm

CRC Tests

Test	Status	Time
COMP	Pass	1:48pm
CAL	Pass	1:48pm

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County ANSON Instrument Location ANSON COUNTY
Instrument Serial No. 008739 SHERIFF'S OFFICE

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 22 day of FEBRUARY, 2024 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

667
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

ANSON COUNTY SHERIFF'S OFFICE 030

Serial Number: 008739

Test Date: 02/22/2024

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Galloway, Charles L

Permit Number: 0023-9771

Effective:

10/01/2023-10/01/2025

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG308003

Exp Date: 03/21/2025

Test	g/210L	Time
DIAG	Pass	1:40pm
AIR BLK	.00	1:41pm
ACCY CHK	.08	1:41pm
AIR BLK	.00	1:42pm
SUB TEST	.00	1:43pm
AIR BLK	.00	1:44pm
SUB TEST	.00	1:45pm
AIR BLK	.00	1:46pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

ANSON COUNTY SHERIFF'S OFFICE 030

Serial Number: 008739 Test Record Number: 970
Test Date: 02/22/2024 Test Time: 1:48pm EST

System Check: Passed

Baseline Tests

Test	Status	Time
IR	Pass	1:48pm
FLO	Pass	1:48pm
FC	Pass	1:48pm

Temperature Tests

Test	Status	Time
FC1	Pass	1:48pm
SRC	Pass	1:48pm
DET	Pass	1:48pm
BAR	Pass	1:48pm
BT	Pass	1:48pm

Blank Tests

Test	Status	Time
AIR	Pass	1:49pm

Printer Tests

Test	Status	Time
PRNT	Pass	1:49pm

CRC Tests

Test	Status	Time
COMP	Pass	1:49pm
CAL	Pass	1:49pm

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County BRUNSWICK Instrument Location BRUNSWICK COUNTY
Instrument Serial No. 008585 DETENTION CENTER

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 15 day of FEBRUARY, 2024 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Alan Rg Bane

Signature of Certifying Official

648

Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

BRUNSWICK COUNTY DETENTION CENTER 090

Serial Number: 008585
Test Date: 02/15/2024

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: BARNES, ALVIN R
Permit Number: 0014-6279
Effective:
10/01/2023-10/01/2025

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG400301
Exp Date: 01/03/2026


Test	g/210L	Time
DIAG	Pass	2:06pm
AIR BLK	.00	2:07pm
ACCY CHK	.08	2:08pm
AIR BLK	.00	2:10pm
SUB TEST	.00	2:10pm
AIR BLK	.00	2:11pm
SUB TEST	.00	2:13pm
AIR BLK	.00	2:14pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

BRUNSWICK COUNTY DETENTION CENTER 090

Serial Number: 008585 Test Record Number: 5714
Test Date: 02/15/2024 Test Time: 2:14pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	2:14pm
FLO	Pass	2:14pm
FC	Pass	2:15pm

Temperature Tests

Test	Status	Time
FC1	Pass	2:15pm
SRC	Pass	2:15pm
DET	Pass	2:15pm
BAR	Pass	2:15pm
BT	Pass	2:15pm

Blank Tests

Test	Status	Time
AIR	Pass	2:15pm


Printer Tests

Test	Status	Time
PRNT	Pass	2:15pm

CRC Tests

Test	Status	Time
COMP	Pass	2:16pm
CAL	Pass	2:16pm

Preventive Maintenance
Status: Pass



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County BRUNSWICK Instrument Location BRUNSWICK COUNTY
Instrument Serial No. 008602 DETENTION CENTER

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 15 day of FEBRUARY, 20 24 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Alan R. Barnes

Signature of Certifying Official

648

Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

BRUNSWICK COUNTY DETENTION CENTER 090

Serial Number: 008602

Test Date: 02/15/2024

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: BARNES, ALVIN R

Permit Number: 0014-6279

Effective:

10/01/2023-10/01/2025

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG400301

Exp Date: 01/03/2026

Test	g/210L	Time
DIAG	Pass	2:14pm
AIR BLK	.00	2:15pm
ACCY CHK	.07	2:16pm
AIR BLK	.00	2:17pm
SUB TEST	.00	2:17pm
AIR BLK	.00	2:18pm
SUB TEST	.00	2:20pm
AIR BLK	.00	2:21pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

BRUNSWICK COUNTY DETENTION CENTER 090

Serial Number: 008602 Test Record Number: 5463
Test Date: 02/15/2024 Test Time: 2:21pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	2:21pm
FLO	Pass	2:21pm
FC	Pass	2:21pm

Temperature Tests

Test	Status	Time
FC1	Pass	2:21pm
SRC	Pass	2:21pm
DET	Pass	2:21pm
BAR	Pass	2:21pm
BT	Pass	2:21pm

Blank Tests

Test	Status	Time
AIR	Pass	2:22pm


Printer Tests

Test	Status	Time
PRNT	Pass	2:22pm

CRC Tests

Test	Status	Time
COMP	Pass	2:22pm
CAL	Pass	2:22pm

Preventive Maintenance
Status: Pass



Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County BRUNSWICK Instrument Location OAK ISLAND
Instrument Serial No. 008648 POLICE DEPT

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 15 day of FEBRUARY, 2024 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Alan R. Bero

Signature of Certifying Official

648

Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

BRUNSWICK COUNTY OAK ISLAND PD 090

Serial Number: 008648

Test Date: 02/15/2024

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: BARNES, ALVIN R

Permit Number: 0014-6279

Effective:

10/01/2023-10/01/2025

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG308101


Exp Date: 03/22/2025

Test	g/210L	Time
DIAG	Pass	12:27pm
AIR BLK	.00	12:28pm
ACCY CHK	.07	12:29pm
AIR BLK	.00	12:30pm
SUB TEST	.00	12:30pm
AIR BLK	.00	12:31pm
SUB TEST	.00	12:33pm
AIR BLK	.00	12:34pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

BRUNSWICK COUNTY OAK ISLAND PD 090

Serial Number: 008648 Test Record Number: 1917
Test Date: 02/15/2024 Test Time: 12:36pm EST

System Check: Passed

Baseline Tests

Test	Status	Time
IR	Pass	12:36pm
FLO	Pass	12:36pm
FC	Pass	12:36pm

Temperature Tests

Test	Status	Time
FC1	Pass	12:36pm
SRC	Pass	12:36pm
DET	Pass	12:36pm
BAR	Pass	12:36pm
BT	Pass	12:36pm

Blank Tests

Test	Status	Time
AIR	Pass	12:37pm

Printer Tests

Test	Status	Time
PRNT	Pass	12:37pm

CRC Tests

Test	Status	Time
COMP	Pass	12:37pm
CAL	Pass	12:37pm

**Preventive Maintenance
Status: Pass**



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County BRUNSWICK Instrument Location LELAND
Instrument Serial No. 008787 POLICE DEPT

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 15 day of FEBRUARY, 2024 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



John R. Bane

Signature of Certifying Official

648

Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

BRUNSWICK COUNTY LELAND PD 090

Serial Number: 008787
Test Date: 02/15/2024

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: BARNES, ALVIN R

Permit Number: 0014-6279

Effective:

10/01/2023-10/01/2025

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG400301


Exp Date: 01/03/2026

Test	g/210L	Time
DIAG	Pass	10:04am
AIR BLK	.00	10:05am
ACCY CHK	.07	10:05am
AIR BLK	.00	10:06am
SUB TEST	.00	10:09am
AIR BLK	.00	10:10am
SUB TEST	.00	10:11am
AIR BLK	.00	10:12am

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

BRUNSWICK COUNTY LELAND PD 090

Serial Number: 008787 Test Record Number: 1201
Test Date: 02/15/2024 Test Time: 10:13am EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	10:14am
FLO	Pass	10:14am
FC	Pass	10:14am

Temperature Tests

Test	Status	Time
FC1	Pass	10:14am
SRC	Pass	10:14am
DET	Pass	10:14am
BAR	Pass	10:14am
BT	Pass	10:14am

Blank Tests

Test	Status	Time
AIR	Pass	10:14am


Printer Tests

Test	Status	Time
PRNT	Pass	10:14am

CRC Tests

Test	Status	Time
COMP	Pass	10:15am
CAL	Pass	10:15am

Preventive Maintenance
Status: Pass



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Cabarrus Instrument Location Cabarrus County SO
Instrument Serial No. 008792 Concord, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 22nd day of February, 2024 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

6074
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

CABARRUS COUNTY CABARRUS COUNTY SO 120

Serial Number: 008792

Test Date: 02/22/2024

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Helms, Bryce A

Permit Number: 0084-9845

Effective:

10/01/2023-10/01/2025

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG400303


Exp Date: 01/03/2026

Test	g/210L	Time
DIAG	Pass	12:10pm
AIR BLK	.00	12:11pm
ACCY CHK	.08	12:12pm
AIR BLK	.00	12:13pm
SUB TEST	.00	12:15pm
AIR BLK	.00	12:16pm
SUB TEST	.00	12:17pm
AIR BLK	.00	12:18pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

Intox EC/IR-II: Preventive Maintenance

CABARRUS COUNTY CABARRUS COUNTY SO 120

Serial Number: 008792 Test Record Number: 4246
Test Date: 02/22/2024 Test Time: 12:21pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	12:21pm
FLO	Pass	12:21pm
FC	Pass	12:21pm

Temperature Tests

Test	Status	Time
FC1	Pass	12:21pm
SRC	Pass	12:21pm
DET	Pass	12:21pm
BAR	Pass	12:21pm
BT	Pass	12:21pm

Blank Tests

Test	Status	Time
AIR	Pass	12:22pm

Printer Tests

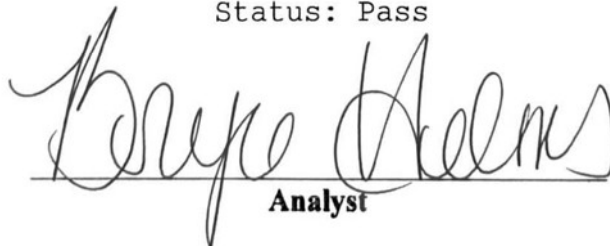
Test	Status	Time
PRNT	Pass	12:22pm

CRC Tests

Test	Status	Time
COMP	Pass	12:22pm
CAL	Pass	12:22pm

Preventive Maintenance

Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County CABARRUS Instrument Location BAT MOBILE REGION 3
Instrument Serial No. 008869 CONCORD PD

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 23 day of FEBRUARY, 2024 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



M.C. Fley
Signature of Certifying Official

676
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

CABARRUS COUNTY BAT MOBILE REGION 3
120

Serial Number: 008869
Test Date: 02/23/2024

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: Unknown

Analyst's Name: Fleming, Marshall C

Permit Number: 0027-5012

Effective:

10/01/2023-10/01/2025

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG302704

Exp Date: 01/27/2025

Test	g/210L	Time
DIAG	Pass	8:37pm
AIR BLK	.00	8:38pm
ACCY CHK	.07	8:39pm
AIR BLK	.00	8:40pm
SUB TEST	.00	8:40pm
AIR BLK	.00	8:41pm
SUB TEST	.00	8:43pm
AIR BLK	.00	8:44pm

Reported AC: .00 g/210L

MC. Fley
Signature of Chemical Analyst

Court CVR

MC. Fley
Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

CABARRUS COUNTY BAT MOBILE REGION 3 120

Serial Number: 008869 Test Record Number: 1775
Test Date: 02/23/2024 Test Time: 8:49pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	8:49pm
FLO	Pass	8:49pm
FC	Pass	8:49pm

Temperature Tests

Test	Status	Time
FC1	Pass	8:49pm
SRC	Pass	8:49pm
DET	Pass	8:49pm
BAR	Pass	8:49pm
BT	Pass	8:49pm

Blank Tests

Test	Status	Time
AIR	Pass	8:50pm

Printer Tests

Test	Status	Time
PRNT	Pass	8:50pm

CRC Tests

Test	Status	Time
COMP	Pass	8:50pm
CAL	Pass	8:50pm

Preventive Maintenance
Status: Pass

M. C. Hg

Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County CABARRUS Instrument Location BAT MOBILE REGION 3
Instrument Serial No. 008898 KANNAPOLIS PD

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 21 day of FEBRUARY, 2024 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



M.C. Flay
Signature of Certifying Official

676
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

CABARRUS COUNTY BAT MOBILE REGION 3
120

Serial Number: 008898
Test Date: 02/21/2024

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Fleming, Marshall C

Permit Number: 0027-5012

Effective:

10/01/2023-10/01/2025

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG225701

Exp Date: 09/14/2024

Test	g/210L	Time
DIAG	Pass	9:06pm
AIR BLK	.00	9:07pm
ACCY CHK	.07	9:08pm
AIR BLK	.00	9:09pm
SUB TEST	.00	9:10pm
AIR BLK	.00	9:11pm
SUB TEST	.00	9:13pm
AIR BLK	.00	9:14pm

Reported AC: .00 g/210L

M.C. Fleming
Signature of Chemical Analyst

Court CVR

M.C. Fleming
Analyst

Intox EC/IR-II: Preventive Maintenance

CABARRUS COUNTY BAT MOBILE REGION 3 120

Serial Number: 008898 Test Record Number: 1786
Test Date: 02/21/2024 Test Time: 9:17pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	9:17pm
FLO	Pass	9:17pm
FC	Pass	9:17pm

Temperature Tests

Test	Status	Time
FC1	Pass	9:17pm
SRC	Pass	9:17pm
DET	Pass	9:17pm
BAR	Pass	9:17pm
BT	Pass	9:17pm

Blank Tests

Test	Status	Time
AIR	Pass	9:18pm

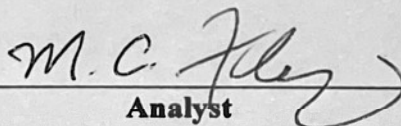
Printer Tests

Test	Status	Time
PRNT	Pass	9:18pm

CRC Tests

Test	Status	Time
COMP	Pass	9:18pm
CAL	Pass	9:18pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County CABARRUS Instrument Location BAT MOBILE REGION 3
Instrument Serial No. 008898 CONCORD PD

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 23 day of FEBRUARY, 2024 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



M.C. Fleenor
Signature of Certifying Official

676
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

CABARRUS COUNTY BAT MOBILE REGION 3
120

Serial Number: 008898
Test Date: 02/23/2024

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Fleming, Marshall C

Permit Number: 0027-5012

Effective:

10/01/2023-10/01/2025

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG225701

Exp Date: 09/14/2024

Test	g/210L	Time
DIAG	Pass	8:24pm
AIR BLK	.00	8:26pm
ACCY CHK	.07	8:26pm
AIR BLK	.00	8:27pm
SUB TEST	.00	8:29pm
AIR BLK	.00	8:30pm
SUB TEST	.00	8:32pm
AIR BLK	.00	8:33pm

Reported AC: .00 g/210L

M.C. Fleg
Signature of Chemical Analyst

Court CVR

M.C. Fleg
Analyst

Intox EC/IR-II: Preventive Maintenance

CABARRUS COUNTY BAT MOBILE REGION 3 120

Serial Number: 008898 Test Record Number: 1793
Test Date: 02/23/2024 Test Time: 8:33pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	8:34pm
FLO	Pass	8:34pm
FC	Pass	8:34pm

Temperature Tests

Test	Status	Time
FC1	Pass	8:34pm
SRC	Pass	8:34pm
DET	Pass	8:34pm
BAR	Pass	8:34pm
BT	Pass	8:34pm

Blank Tests

Test	Status	Time
AIR	Pass	8:35pm

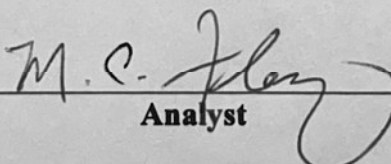
Printer Tests

Test	Status	Time
PRNT	Pass	8:35pm

CRC Tests

Test	Status	Time
COMP	Pass	8:35pm
CAL	Pass	8:35pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County CASWELL Instrument Location CASWELL CO. JAIL

Instrument Serial No. 008719 LENOIR, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 08 day of FEBRUARY, 2024 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

6446
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

CALDWELL COUNTY CALDWELL COUNTY JAIL
130

Serial Number: 008719
Test Date: 02/08/2024

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Fleming, Tina S

Permit Number: 0027-4970

Effective:

07/01/2022-07/01/2024

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG308702

Exp Date: 03/28/2025


Test	g/210L	Time
DIAG	Pass	11:24am
AIR BLK	.00	11:25am
ACCY CHK	.08	11:25am
AIR BLK	.00	11:27am
SUB TEST	.00	11:28am
AIR BLK	.00	11:29am
SUB TEST	.00	11:30am
AIR BLK	.00	11:31am

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

CALDWELL COUNTY CALDWELL COUNTY JAIL 130

Serial Number: 008719 Test Record Number: 3268
Test Date: 02/08/2024 Test Time: 11:39am EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	11:40am
FLO	Pass	11:40am
FC	Pass	11:40am

Temperature Tests

Test	Status	Time
FC1	Pass	11:40am
SRC	Pass	11:40am
DET	Pass	11:40am
BAR	Pass	11:40am
BT	Pass	11:40am

Blank Tests

Test	Status	Time
AIR	Pass	11:41am


Printer Tests

Test	Status	Time
PRNT	Pass	11:41am

CRC Tests

Test	Status	Time
COMP	Pass	11:41am
CAL	Pass	11:41am

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County CALDWELL Instrument Location CALDWELL CO. JAIL
Instrument Serial No. 008803 LE1012 NK

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 08 day of FEBRUARY, 2024 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Jim S. Steining
Signature of Certifying Official

646
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

CALDWELL COUNTY CALDWELL COUNTY JAIL
130

Serial Number: 008803
Test Date: 02/08/2024

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Fleming, Tina S

Permit Number: 0027-4970

Effective:

07/01/2022-07/01/2024

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG308702

Exp Date: 03/28/2025

Test	g/210L	Time
DIAG	Pass	11:25am
AIR BLK	.00	11:26am
ACCY CHK	.07	11:26am
AIR BLK	.00	11:28am
SUB TEST	.00	11:28am
AIR BLK	.00	11:29am
SUB TEST	.00	11:31am
AIR BLK	.00	11:31am

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

CALDWELL COUNTY CALDWELL COUNTY JAIL 130

Serial Number: 008803 Test Record Number: 818
Test Date: 02/08/2024 Test Time: 11:39am EST

System Check: Passed

Baseline Tests

Test	Status	Time
IR	Pass	11:40am
FLO	Pass	11:40am
FC	Pass	11:40am

Temperature Tests

Test	Status	Time
FC1	Pass	11:40am
SRC	Pass	11:40am
DET	Pass	11:40am
BAR	Pass	11:40am
BT	Pass	11:40am

Blank Tests

Test	Status	Time
AIR	Pass	11:40am

Printer Tests

Test	Status	Time
PRNT	Pass	11:40am

CRC Tests

Test	Status	Time
COMP	Pass	11:41am
CAL	Pass	11:41am

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County CARTERET Instrument Location MOREHEAD CITY
Instrument Serial No. 008731 POLICE DEPT

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 12 day of FEBRUARY, 2024 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Alan R. B...
Signature of Certifying Official

648
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

CARTERET COUNTY MOREHEAD CITY PD 150

Serial Number: 008731

Test Date: 02/12/2024

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: BARNES, ALVIN R

Permit Number: 0014-6279

Effective:

10/01/2023-10/01/2025

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG308101

Exp Date: 03/22/2025

Test g/210L Time

DIAG Pass 6:16pm

AIR BLK .00 6:17pm

ACCY CHK .08 6:17pm

AIR BLK .00 6:19pm


SUB TEST .00 6:19pm

AIR BLK .00 6:20pm


SUB TEST .00 6:22pm

AIR BLK .00 6:23pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

CARTERET COUNTY MOREHEAD CITY PD 150

Serial Number: 008731 Test Record Number: 2594
Test Date: 02/12/2024 Test Time: 6:23pm EST

System Check: Passed

Baseline Tests

Test	Status	Time
IR	Pass	6:23pm
FLO	Pass	6:23pm
FC	Pass	6:23pm

Temperature Tests

Test	Status	Time
FC1	Pass	6:24pm
SRC	Pass	6:24pm
DET	Pass	6:24pm
BAR	Pass	6:24pm
BT	Pass	6:24pm

Blank Tests

Test	Status	Time
AIR	Pass	6:24pm

Printer Tests

Test	Status	Time
PRNT	Pass	6:24pm

CRC Tests

Test	Status	Time
COMP	Pass	6:24pm
CAL	Pass	6:24pm

Preventive Maintenance
Status: Pass


Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Caswell Instrument Location Caswell Co Detention Ctr
Instrument Serial No. 008593 211 County Park Rd
Yanceyville, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 6 day of February, 2024 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Sam Ades Barnes
Signature of Certifying Official

662
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

CASWELL COUNTY DETENTION CENTER 160

Serial Number: 008593

Test Date: 02/06/2024

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Barnes, Simon S

Permit Number: 0014-6221

Effective:

10/01/2023-10/01/2025

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG308703

Exp Date: 03/28/2025

Test	g/210L	Time
DIAG	Pass	8:42am
AIR BLK	.00	8:43am
ACCY CHK	.07	8:44am
AIR BLK	.00	8:45am
SUB TEST	.00	8:46am
AIR BLK	.00	8:46am
SUB TEST	.00	8:48am
AIR BLK	.00	8:49am

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

This form is used when performing Preventive Maintenance procedures

Forensic Tests for Alcohol Branch

Department of Health and Human Services

Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

CASWELL COUNTY DETENTION CENTER 160

Serial Number: 008593 Test Record Number: 2173
Test Date: 02/06/2024 Test Time: 8:49am EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	8:50am
FLO	Pass	8:50am
FC	Pass	8:50am

Temperature Tests

Test	Status	Time
FC1	Pass	8:50am
SRC	Pass	8:50am
DET	Pass	8:50am
BAR	Pass	8:50am
BT	Pass	8:50am

Blank Tests

Test	Status	Time
AIR	Pass	8:50am

Printer Tests

Test	Status	Time
PRNT	Pass	8:50am

CRC Tests

Test	Status	Time
COMP	Pass	8:51am
CAL	Pass	8:51am

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Caswell Instrument Location Caswell Co. Detention Ctr
Instrument Serial No. 008873 211 County Park Rd
Yanceypville, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 20 day of February, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Simon Adams Bruns

Signature of Certifying Official

642

Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

CASWELL COUNTY DETENTION CENTER 160

Serial Number: 008873

Test Date: 02/20/2024

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Barnes, Simon S

Permit Number: 0014-6221

Effective:

10/01/2023-10/01/2025

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG400301

Exp Date: 01/03/2026

Test	g/210L	Time
DIAG	Pass	6:43am
AIR BLK	.00	6:44am
ACCY CHK	.07	6:44am
AIR BLK	.00	6:45am
SUB TEST	.00	6:46am
AIR BLK	.00	6:47am
SUB TEST	.00	6:48am
AIR BLK	.00	6:49am

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

CASWELL COUNTY DETENTION CENTER 160

Serial Number: 008873 Test Record Number: 2195
Test Date: 02/20/2024 Test Time: 6:49am EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	6:50am
FLO	Pass	6:50am
FC	Pass	6:50am

Temperature Tests

Test	Status	Time
FC1	Pass	6:50am
SRC	Pass	6:50am
DET	Pass	6:50am
BAR	Pass	6:50am
BT	Pass	6:50am

Blank Tests

Test	Status	Time
AIR	Pass	6:51am


Printer Tests

Test	Status	Time
PRNT	Pass	6:51am

CRC Tests

Test	Status	Time
COMP	Pass	6:51am
CAL	Pass	6:51am

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Catawba Instrument Location Catawba County 80
Instrument Serial No. 008687 Newton, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 27th day of February, 2024 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Brejo Helms
Signature of Certifying Official

6074
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

CATAWBA COUNTY CATAWBA COUNTY SO 170

Serial Number: 008687

Test Date: 02/27/2024

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Helms, Bryce A

Permit Number: 0084-9845

Effective:

10/01/2023-10/01/2025

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG302703

Exp Date: 01/27/2025

Test	g/210L	Time
DIAG	Pass	12:55pm
AIR BLK	.00	12:56pm
ACCY CHK	.07	12:57pm
AIR BLK	.00	12:58pm
SUB TEST	.00	12:59pm
AIR BLK	.00	12:59pm
SUB TEST	.00	1:01pm
AIR BLK	.00	1:02pm

Reported AC: .00 g/210L

Bryce Helms
Signature of Chemical Analyst

Court CVR

Bryce Helms
Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch,
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

CATAWBA COUNTY CATAWBA COUNTY SO 170

Serial Number: 008687 Test Record Number: 3835
Test Date: 02/27/2024 Test Time: 1:02pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	1:03pm
FLO	Pass	1:03pm
FC	Pass	1:03pm

Temperature Tests

Test	Status	Time
FC1	Pass	1:03pm
SRC	Pass	1:03pm
DET	Pass	1:03pm
BAR	Pass	1:03pm
BT	Pass	1:03pm

Blank Tests

Test	Status	Time
AIR	Pass	1:03pm

Printer Tests

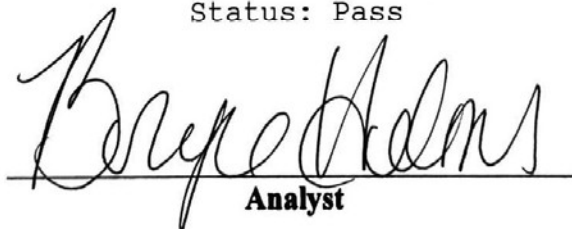
Test	Status	Time
PRNT	Pass	1:03pm

CRC Tests

Test	Status	Time
COMP	Pass	1:04pm
CAL	Pass	1:04pm

Preventive Maintenance

Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Columbus Instrument Location BAT Mobile Unit 5
Instrument Serial No. 00 8575 Columbus County SO

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 8th day of February, 2024 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Signature of Certifying Official

684

Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

COLUMBUS COUNTY BAT MOBILE UNIT 5 230

Serial Number: 008575

Test Date: 02/08/2024

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Sharpe Jr., Robert J

Permit Number: 1820-8591

Effective:

10/01/2023-10/01/2025

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG308101

Exp Date: 03/22/2025

Test	g/210L	Time
DIAG	Pass	8:35pm
AIR BLK	.00	8:36pm
ACCY CHK	.08	8:37pm
AIR BLK	.00	8:38pm
SUB TEST	.00	8:38pm
AIR BLK	.00	8:39pm
SUB TEST	.00	8:41pm
AIR BLK	.00	8:42pm

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR

Analyst

This form is used when performing Preventive Maintenance procedures

Forensic Tests for Alcohol Branch

Department of Health and Human Services

Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

COLUMBUS COUNTY BAT MOBILE UNIT 5 230

Serial Number: 008575 Test Record Number: 1427
Test Date: 02/08/2024 Test Time: 8:53pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	8:53pm
FLO	Pass	8:54pm
FC	Pass	8:54pm

Temperature Tests

Test	Status	Time
FC1	Pass	8:54pm
SRC	Pass	8:54pm
DET	Pass	8:54pm
BAR	Pass	8:54pm
BT	Pass	8:54pm

Blank Tests

Test	Status	Time
AIR	Pass	8:54pm

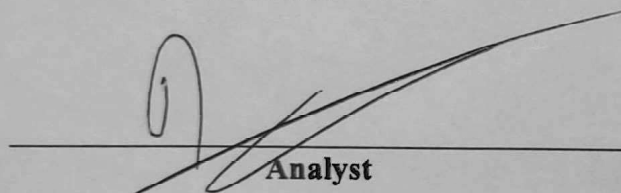
Printer Tests

Test	Status	Time
PRNT	Pass	8:54pm

CRC Tests

Test	Status	Time
COMP	Pass	8:55pm
CAL	Pass	8:55pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Columbus Instrument Location BAT Mobile Unit 5
Instrument Serial No. 008616 Columbus County So

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 8th day of February, 2024 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

684
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

COLUMBUS COUNTY BAT MOBILE UNIT 5 230

Serial Number: 008616

Test Date: 02/08/2024

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Sharpe Jr., Robert J

Permit Number: 1820-8591

Effective:

10/01/2023-10/01/2025

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG308101

Exp Date: 03/22/2025

Test	g/210L	Time
DIAG	Pass	8:17pm
AIR BLK	.00	8:18pm
ACCY CHK	.08	8:19pm
AIR BLK	.00	8:20pm
SUB TEST	.00	8:20pm
AIR BLK	.00	8:21pm
SUB TEST	.00	8:23pm
AIR BLK	.00	8:24pm

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR

Analyst

Intox EC/IR-II: Preventive Maintenance

COLUMBUS COUNTY BAT MOBILE UNIT 5 230

Serial Number: 008616 Test Record Number: 2820
Test Date: 02/08/2024 Test Time: 8:25pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	8:25pm
FLO	Pass	8:25pm
FC	Pass	8:25pm

Temperature Tests

Test	Status	Time
FC1	Pass	8:25pm
SRC	Pass	8:25pm
DET	Pass	8:25pm
BAR	Pass	8:25pm
BT	Pass	8:25pm

Blank Tests

Test	Status	Time
AIR	Pass	8:26pm

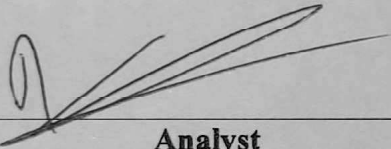
Printer Tests

Test	Status	Time
PRNT	Pass	8:26pm

CRC Tests

Test	Status	Time
COMP	Pass	8:26pm
CAL	Pass	8:26pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Columbus Instrument Location BAT Mobile Unit 5
Instrument Serial No. 008707 Columbus County SO

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 6th day of February, 2024 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

684
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

COLUMBUS COUNTY BAT MOBILE UNIT 5 230

Serial Number: 008707

Test Date: 02/08/2024

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Sharpe Jr., Robert J

Permit Number: 1820-8591

Effective:

10/01/2023-10/01/2025

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG308704

Exp Date: 03/28/2025

Test	g/210L	Time
DIAG	Pass	8:16pm
AIR BLK	.00	8:17pm
ACCY CHK	.08	8:17pm
AIR BLK	.00	8:19pm
SUB TEST	.00	8:19pm
AIR BLK	.00	8:20pm
SUB TEST	.00	8:22pm
AIR BLK	.00	8:23pm

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

COLUMBUS COUNTY BAT MOBILE UNIT 5 230

Serial Number: 008707 Test Record Number: 2816
Test Date: 02/08/2024 Test Time: 8:24pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	8:24pm
FLO	Pass	8:24pm
FC	Pass	8:24pm

Temperature Tests

Test	Status	Time
FC1	Pass	8:24pm
SRC	Pass	8:24pm
DET	Pass	8:24pm
BAR	Pass	8:24pm
BT	Pass	8:24pm

Blank Tests

Test	Status	Time
AIR	Pass	8:25pm

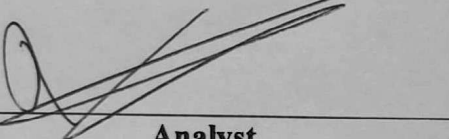
Printer Tests

Test	Status	Time
PRNT	Pass	8:25pm

CRC Tests

Test	Status	Time
COMP	Pass	8:25pm
CAL	Pass	8:25pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County COLUMBUS Instrument Location COLUMBUS COUNTY
Instrument Serial No. 008901 DETENTION CENTER

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 20 day of FEBRUARY, 2024 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Alan Rg Bann

Signature of Certifying Official

648

Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

COLUMBUS COUNTY DETENTION CENTER 230

Serial Number: 008901
Test Date: 02/20/2024

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: BARNES, ALVIN R

Permit Number: 0014-6279

Effective:

10/01/2023-10/01/2025

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG400301
Exp Date: 01/03/2026

Test	g/210L	Time
DIAG	Pass	3:32pm
AIR BLK	.00	3:33pm
ACCY CHK	.08	3:33pm
AIR BLK	.00	3:35pm
SUB TEST	.00	3:35pm
AIR BLK	.00	3:36pm
SUB TEST	.00	3:38pm
AIR BLK	.00	3:39pm

Reported AC: .00 g/210L

Alvin R. Barnes
Signature of Chemical Analyst

Court CVR

Alvin R. Barnes
Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

COLUMBUS COUNTY DETENTION CENTER 230

Serial Number: 008901 Test Record Number: 1690
Test Date: 02/20/2024 Test Time: 3:40pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	3:41pm
FLO	Pass	3:41pm
FC	Pass	3:41pm

Temperature Tests

Test	Status	Time
FC1	Pass	3:41pm
SRC	Pass	3:41pm
DET	Pass	3:41pm
BAR	Pass	3:41pm
BT	Pass	3:41pm

Blank Tests

Test	Status	Time
AIR	Pass	3:41pm


Printer Tests

Test	Status	Time
PRNT	Pass	3:41pm

CRC Tests

Test	Status	Time
COMP	Pass	3:42pm
CAL	Pass	3:42pm

Preventive Maintenance
Status: Pass



Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County COLUMBUS Instrument Location COLUMBUS COUNTY
Instrument Serial No. 008917 DETENTION CENTER

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 19 day of FEBRUARY, 2024 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Alvin R. B...
Signature of Certifying Official

648
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

COLUMBUS COUNTY DETENTION CENTER 230

Serial Number: 008917
Test Date: 02/19/2024

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE

Analyst's Name: BARNES, ALVIN R
Permit Number: 0014-6279
Effective:
10/01/2023-10/01/2025

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG400301
Exp Date: 01/03/2026

Test	g/210L	Time
DIAG	Pass	10:46am
AIR BLK	.00	10:47am
ACCY CHK	.07	10:47am
AIR BLK	.00	10:49am
SUB TEST	.00	10:49am
AIR BLK	.00	10:50am
SUB TEST	.00	10:52am
AIR BLK	.00	10:53am

Reported AC: .00 g/210L

Alvin R. Barnes
Signature of Chemical Analyst

Court CVR

Alvin R. Barnes
Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

COLUMBUS COUNTY DETENTION CENTER 230

Serial Number: 008917 Test Record Number: 1212
Test Date: 02/19/2024 Test Time: 10:54am EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	10:55am
FLO	Pass	10:55am
FC	Pass	10:55am

Temperature Tests

Test	Status	Time
FC1	Pass	10:55am
SRC	Pass	10:55am
DET	Pass	10:55am
BAR	Pass	10:55am
BT	Pass	10:55am

Blank Tests

Test	Status	Time
AIR	Pass	10:55am


Printer Tests

Test	Status	Time
PRNT	Pass	10:55am

CRC Tests

Test	Status	Time
COMP	Pass	10:56am
CAL	Pass	10:56am

Preventive Maintenance
Status: Pass


Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County CRAVEN Instrument Location BAT mobile unit 7

Instrument Serial No. 008600 CRAVEN SD

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 16 day of February, 2024 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]

Signature of Certifying Official

665

Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

CRAVEN COUNTY BAT MOBILE UNIT 7 240

Serial Number: 008600

Test Date: 02/16/2024

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Anderson, Mark G

Permit Number: 0013-1517

Effective:

10/01/2023-10/01/2025

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

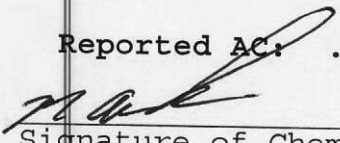
Test Type: Breath Test

Lot Number: AG38004

Exp Date: 03/21/2025

Test	g/210L	Time
DIAG	Pass	9:17pm
AIR BLK	.00	9:18pm
ACCY CHK	.08	9:19pm
AIR BLK	.00	9:20pm
SUB TEST	.00	9:21pm
AIR BLK	.00	9:21pm
SUB TEST	.00	9:23pm
AIR BLK	.00	9:24pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

CRAVEN COUNTY BAT MOBILE UNIT 7 240

Serial Number: 008600 Test Record Number: 2679

Test Date: 02/16/2024 Test Time: 9:26pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	9:26pm
FLO	Pass	9:26pm
FC	Pass	9:26pm

Temperature Tests

Test	Status	Time
FC1	Pass	9:26pm
SRC	Pass	9:26pm
DET	Pass	9:26pm
BAR	Pass	9:26pm
BT	Pass	9:26pm

Blank Tests

Test	Status	Time
AIR	Pass	9:27pm

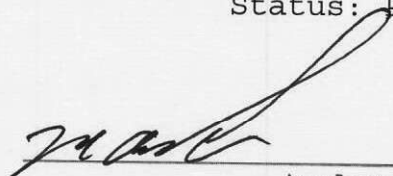
Printer Tests

Test	Status	Time
PRNT	Pass	9:27pm

CRC Tests

Test	Status	Time
COMP	Pass	9:27pm
CAL	Pass	9:27pm

Preventive Maintenance
Status: *Pass*



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Graen Instrument Location BAT mobile unit 7
Instrument Serial No. 008628 Graen 30

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 16 day of February, 2024 the forgoing preventive maintenance procedures were performed on the instrument indicated above in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]

Signature of Certifying Official

665

Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

CRAVEN COUNTY BAT MOBILE UNIT 7 240

Serial Number: 008698

Test Date: 02/16/2024

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Anderson, Mark G

Permit Number: 0013-1517

Effective:

10/01/2023-10/01/2025

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

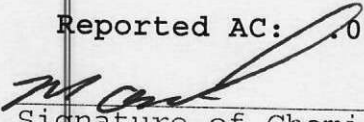
Test Type: Breath Test

Lot Number: AG302703

Exp Date: 01/27/2025

Test	g/210L	Time
DIAG	Pass	8:49pm
AIR BLK	.00	8:50pm
ACCY CHK	.07	8:51pm
AIR BLK	.00	8:52pm
SUB TEST	.00	8:53pm
AIR BLK	.00	8:54pm
SUB TEST	.00	8:55pm
AIR BLK	.00	8:56pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

CRAVEN COUNTY BAT MOBILE UNIT 7 240

Serial Number: 008698 Test Record Number: 2295
Test Date: 02/16/2024 Test Time: 8:58pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	8:58pm
FLO	Pass	8:58pm
FC	Pass	8:58pm

Temperature Tests

Test	Status	Time
FC1	Pass	8:58pm
SRC	Pass	8:58pm
DET	Pass	8:58pm
BAR	Pass	8:58pm
BT	Pass	8:58pm

Blank Tests

Test	Status	Time
AIR	Pass	8:59pm

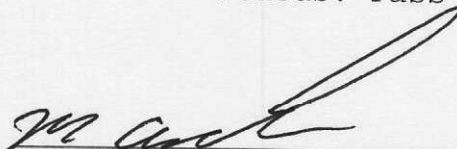
Printer Tests

Test	Status	Time
PRNT	Pass	8:59pm

CRC Tests

Test	Status	Time
COMP	Pass	8:59pm
CAL	Pass	8:59pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Craven Instrument Location BAT mobile unit 7
Instrument Serial No. 008788 Craven SO

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 16 day of February, 2024 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Signature of Certifying Official

665

Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

CRAVEN COUNTY BAT MOBILE UNIT 7 240

Serial Number: 008788
Test Date: 02/16/2024

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Anderson, Mark G

Permit Number: 0013-1517

Effective:

10/01/2023-10/01/2025

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

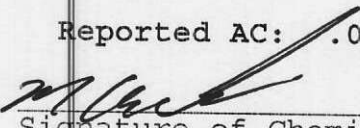
Test Type: Breath Test

Lot Number: AG302703

Exp Date: 01/27/2025

Test	g/210L	Time
DIAG	Pass	9:03pm
AIR BLK	.00	9:04pm
ACCY CHK	.08	9:05pm
AIR BLK	.00	9:05pm
SUB TEST	.00	9:06pm
AIR BLK	.00	9:07pm
SUB TEST	.00	9:09pm
AIR BLK	.00	9:10pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

CRAVEN COUNTY BAT MOBILE UNIT 7 240

Serial Number: 008788 Test Record Number: 2177
Test Date: 02/16/2024 Test Time: 9:11pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	9:12pm
FLO	Pass	9:12pm
FC	Pass	9:12pm

Temperature Tests

Test	Status	Time
FC1	Pass	9:12pm
SRC	Pass	9:12pm
DET	Pass	9:12pm
BAR	Pass	9:12pm
BT	Pass	9:12pm

Blank Tests

Test	Status	Time
AIR	Pass	9:12pm

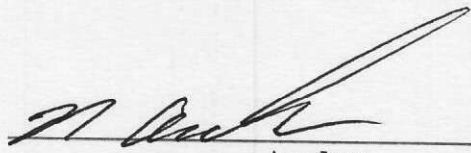
Printer Tests

Test	Status	Time
PRNT	Pass	9:12pm

CRC Tests

Test	Status	Time
COMP	Pass	9:13pm
CAL	Pass	9:13pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Cumberland Instrument Location Hope Mills
Instrument Serial No. 008614 Police Department

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 5 day of February, 2024 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

675
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

HOPE MILLS POLICE DEPARTMENT 250

Serial Number: 008614

Test Date: 02/05/2024

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Garner, Joel K

Permit Number: 0036-5156

Effective:

10/01/2023-10/01/2025

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG400301

Exp Date: 01/03/2026

Test	g/210L	Time
DIAG	Pass	9:30am
AIR BLK	.00	9:30am
ACCY CHK	.07	9:31am
AIR BLK	.00	9:32am
SUB TEST	.00	9:33am
AIR BLK	.00	9:34am
SUB TEST	.00	9:35am
AIR BLK	.00	9:36am

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

HOPE MILLS POLICE DEPARTMENT 250

Serial Number: 008614 Test Record Number: 4984
Test Date: 02/05/2024 Test Time: 9:37am EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	9:38am
FLO	Pass	9:38am
FC	Pass	9:38am

Temperature Tests

Test	Status	Time
FC1	Pass	9:38am
SRC	Pass	9:38am
DET	Pass	9:38am
BAR	Pass	9:38am
BT	Pass	9:38am

Blank Tests

Test	Status	Time
AIR	Pass	9:38am


Printer Tests

Test	Status	Time
PRNT	Pass	9:38am

CRC Tests

Test	Status	Time
COMP	Pass	9:39am
CAL	Pass	9:39am

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Currituck Instrument Location Currituck Co. Sheriff's Office
Instrument Serial No. 008588 407-A Maple Rd., Maple, N.C.

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 19th day of February, 2024 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

643
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

CURRITUCK COUNTY CURRITUCK SO-MAPLE
260

Serial Number: 008588

Test Date: 02/19/2024

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Gray, Kelly D

Permit Number: 0037-7722

Effective:

10/01/2023-10/01/2025

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG302703

Exp Date: 01/27/2025

Test	g/210L	Time
DIAG	Pass	12:48pm
AIR BLK	.00	12:49pm
ACCY CHK	.07	12:50pm
AIR BLK	.00	12:51pm
SUB TEST	.00	12:51pm
AIR BLK	.00	12:52pm
SUB TEST	.00	12:54pm
AIR BLK	.00	12:55pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

CURRITUCK COUNTY CURRITUCK SO-MAPLE 260

Serial Number: 008588 Test Record Number: 1282
Test Date: 02/19/2024 Test Time: 12:56pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	12:57pm
FLO	Pass	12:57pm
FC	Pass	12:57pm

Temperature Tests

Test	Status	Time
FC1	Pass	12:57pm
SRC	Pass	12:57pm
DET	Pass	12:57pm
BAR	Pass	12:57pm
BT	Pass	12:57pm

Blank Tests

Test	Status	Time
AIR	Pass	12:58pm

Printer Tests

Test	Status	Time
PRNT	Pass	12:58pm

CRC Tests

Test	Status	Time
COMP	Pass	12:58pm
CAL	Pass	12:58pm

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County

Dare

Instrument Location

Dare Co. Detention Center

Instrument Serial No.

008783

1044 Driftwood Dr. Manteo,

NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 22nd day of February, 2024 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

680
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

DARE COUNTY DARE CO DETENTION CE 270

Serial Number: 008783

Test Date: 02/22/2024

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Chappell, Mark A

Permit Number: 0020-6272

Effective:

10/01/2023-10/01/2025

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

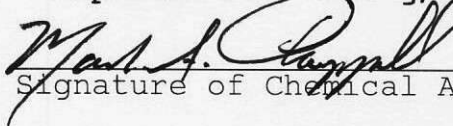
Test Type: Breath Test

Lot Number: AG400303

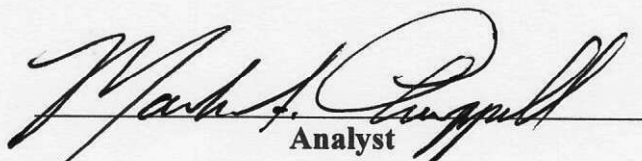
Exp Date: 01/03/2026

Test	g/210L	Time
DIAG	Pass	12:16pm
AIR BLK	.00	12:17pm
ACCY CHK	.07	12:18pm
AIR BLK	.00	12:19pm
SUB TEST	.00	12:20pm
AIR BLK	.00	12:21pm
SUB TEST	.00	12:22pm
AIR BLK	.00	12:23pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

DARE COUNTY DARE CO DETENTION CE 270

Serial Number: 008783 Test Record Number: 1519
Test Date: 02/22/2024 Test Time: 12:24pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	12:24pm
FLO	Pass	12:24pm
FC	Pass	12:24pm

Temperature Tests

Test	Status	Time
FC1	Pass	12:25pm
SRC	Pass	12:25pm
DET	Pass	12:25pm
BAR	Pass	12:25pm
BT	Pass	12:25pm

Blank Tests

Test	Status	Time
AIR	Pass	12:25pm

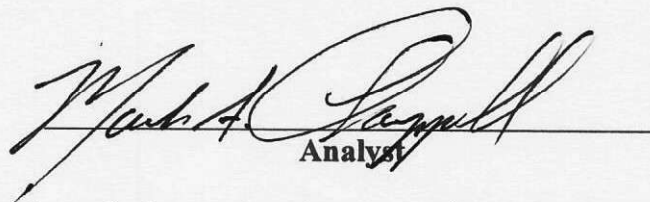
Printer Tests

Test	Status	Time
PRNT	Pass	12:25pm

CRC Tests

Test	Status	Time
COMP	Pass	12:25pm
CAL	Pass	12:25pm

Preventive Maintenance
Status: Pass


Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Dare Instrument Location Dare Co. Detention Center
Instrument Serial No. 008804 1044 Driftwood Dr. Montecore
NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 22nd day of February, 2024 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

680
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

DARE COUNTY DARE CO DETENTION CE 270

Serial Number: 008804

Test Date: 02/22/2024

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Chappell, Mark A

Permit Number: 0020-6272

Effective:

10/01/2023-10/01/2025

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG400303

Exp Date: 01/03/2026

Test	g/210L	Time
DIAG	Pass	12:18pm
AIR BLK	.00	12:19pm
ACCY CHK	.07	12:19pm
AIR BLK	.00	12:20pm
SUB TEST	.00	12:21pm
AIR BLK	.00	12:22pm
SUB TEST	.00	12:23pm
AIR BLK	.00	12:24pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

DARE COUNTY DARE CO DETENTION CE 270

Serial Number: 008804 Test Record Number: 2803
Test Date: 02/22/2024 Test Time: 12:26pm EST

System Check: Passed

Baseline Tests

Test	Status	Time
IR	Pass	12:26pm
FLO	Pass	12:26pm
FC	Pass	12:26pm

Temperature Tests

Test	Status	Time
FC1	Pass	12:26pm
SRC	Pass	12:26pm
DET	Pass	12:26pm
BAR	Pass	12:26pm
BT	Pass	12:26pm

Blank Tests

Test	Status	Time
AIR	Pass	12:27pm

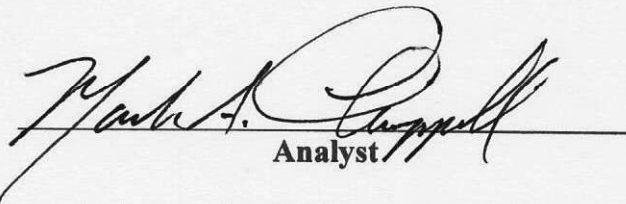
Printer Tests

Test	Status	Time
PRNT	Pass	12:27pm

CRC Tests

Test	Status	Time
COMP	Pass	12:27pm
CAL	Pass	12:27pm

Preventive Maintenance
Status: Pass


Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

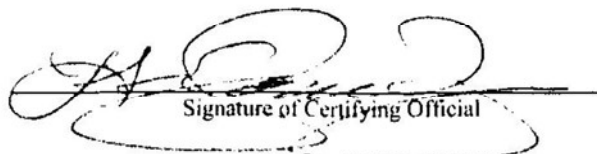
County DAVIDSON Instrument Location LEXINGTON POLICE
Instrument Serial No. 008683 DEPARTMENT

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 19TH day of FEBRUARY, 2024 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.




Signature of Certifying Official

669
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

DAVIDSON COUNTY LEXINGTON PD 280

Serial Number: 008683

Test Date: 02/19/2024

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Oligmueller, Leo A

Permit Number: 0035-3799

Effective:

10/01/2023-10/01/2025

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG308704

Exp Date: 03/28/2025

Test	g/210L	Time
DIAG	Pass	12:45pm
AIR BLK	.00	12:46pm
ACCY CHK	.08	12:47pm
AIR BLK	.00	12:48pm
SUB TEST	.00	12:49pm
AIR BLK	.00	12:50pm
SUB TEST	.00	12:51pm
AIR BLK	.00	12:52pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

DAVIDSON COUNTY LEXINGTON PD 280

Serial Number: 008683 Test Record Number: 1198
Test Date: 02/19/2024 Test Time: 12:54pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	12:54pm
FLO	Pass	12:54pm
FC	Pass	12:54pm

Temperature Tests

Test	Status	Time
FC1	Pass	12:55pm
SRC	Pass	12:55pm
DET	Pass	12:55pm
BAR	Pass	12:55pm
BT	Pass	12:55pm

Blank Tests

Test	Status	Time
AIR	Pass	12:55pm


Printer Tests

Test	Status	Time
PRNT	Pass	12:55pm

CRC Tests

Test	Status	Time
COMP	Pass	12:55pm
CAL	Pass	12:55pm

Preventive Maintenance
Status: Pass


Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Edgercombe Instrument Location Edgercombe Co. Magistrate's
Instrument Serial No. 008603 Office, 3005 Anaconda Rd.,
Tarboro, N.C.

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 20th day of February, 2024 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Key P. Day
Signature of Certifying Official

6043
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

EDGECOMBE COUNTY EDGECOMBE CO MAGISTR
320

Serial Number: 008603
Test Date: 02/20/2024

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: Gray, Kelly D
Permit Number: 0037-7722
Effective:
10/01/2023-10/01/2025

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG302702
Exp Date: 01/27/2025

Test	g/210L	Time
DIAG	Pass	1:35pm
AIR BLK	.00	1:36pm
ACCY CHK	.08	1:37pm
AIR BLK	.00	1:38pm
SUB TEST	.00	1:39pm
AIR BLK	.00	1:40pm
SUB TEST	.00	1:42pm
AIR BLK	.00	1:43pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

EDGECOMBE COUNTY EDGECOMBE CO MAGISTR 320

Serial Number: 008603 Test Record Number: 2383
Test Date: 02/20/2024 Test Time: 1:44pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	1:44pm
FLO	Pass	1:44pm
FC	Pass	1:45pm

Temperature Tests

Test	Status	Time
FC1	Pass	1:45pm
SRC	Pass	1:45pm
DET	Pass	1:45pm
BAR	Pass	1:45pm
BT	Pass	1:45pm

Blank Tests

Test	Status	Time
AIR	Pass	1:45pm


Printer Tests

Test	Status	Time
PRNT	Pass	1:45pm

CRC Tests

Test	Status	Time
COMP	Pass	1:45pm
CAL	Pass	1:45pm

Preventive Maintenance
Status: Pass



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Edgecombe Instrument Location Edgecombe Co. Magistrate's
Office, 3005 Anaconda Rd.
Tarboro, NC

Instrument Serial No. 008847

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 27th day of February, 2024 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

680
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

EDGECOMBE COUNTY EDGECOMBE CO MAGISTR
320

Serial Number: 008847

Test Date: 02/27/2024

Citation Number: M00000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Chappell, Mark A

Permit Number: 0020-6272

Effective:

10/01/2023-10/01/2025

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

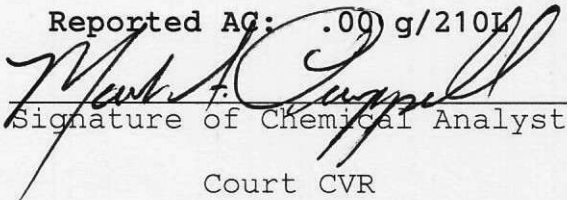
Test Type: Breath Test

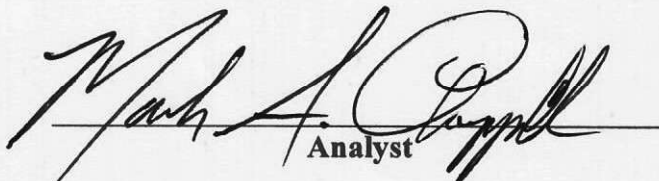
Lot Number: AG308004

Exp Date: 03/21/2025

Test	g/210L	Time
DIAG	Pass	11:04am
AIR BLK	.00	11:05am
ACCY CHK	.07	11:05am
AIR BLK	.00	11:06am
SUB TEST	.00	11:07am
AIR BLK	.00	11:08am
SUB TEST	.00	11:09am
AIR BLK	.00	11:10am

Reported AG: .00 g/210L


Signature of Chemical Analyst
Court CVR


Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

EDGECOMBE COUNTY EDGECOMBE CO MAGISTR 320

Serial Number: 008847 Test Record Number: 876
Test Date: 02/27/2024 Test Time: 11:12am EST

System Check: Passed

Baseline Tests

Test	Status	Time
IR	Pass	11:13am
FLO	Pass	11:13am
FC	Pass	11:13am

Temperature Tests

Test	Status	Time
FC1	Pass	11:13am
SRC	Pass	11:13am
DET	Pass	11:13am
BAR	Pass	11:13am
BT	Pass	11:13am

Blank Tests

Test	Status	Time
AIR	Pass	11:13am

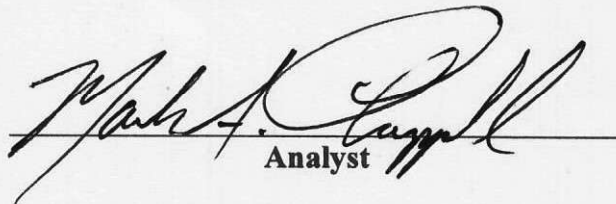
Printer Tests

Test	Status	Time
PRNT	Pass	11:14am

CRC Tests

Test	Status	Time
COMP	Pass	11:14am
CAL	Pass	11:14am

Preventive Maintenance
Status: Pass


Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Edgecombe

Instrument Location Edgecombe Co. Magistrate's

Instrument Serial No. 008918

Office, 3005 Anaconda Rd.,
Tarboro, NC.

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 26th day of February, 2024 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Kelly P. Ayers
Signature of Certifying Official

1643
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

EDGECOMBE COUNTY EDGECOMBE CO MAGISTR
320

Serial Number: 008918

Test Date: 02/26/2024

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Gray, Kelly D

Permit Number: 0037-7722

Effective:

10/01/2023-10/01/2025

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG302702


Exp Date: 01/27/2025

Test	g/210L	Time
DIAG	Pass	12:25pm
AIR BLK	.00	12:26pm
ACCY CHK	.07	12:27pm
AIR BLK	.00	12:28pm
SUB TEST	.00	12:29pm
AIR BLK	.00	12:30pm
SUB TEST	.00	12:31pm
AIR BLK	.00	12:32pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

EDGECOMBE COUNTY EDGECOMBE CO MAGISTR 320

Serial Number: 008918 Test Record Number: 933
Test Date: 02/26/2024 Test Time: 12:34pm EST

System Check: Passed

Baseline Tests

Test	Status	Time
IR	Pass	12:34pm
FLO	Pass	12:34pm
FC	Pass	12:34pm

Temperature Tests

Test	Status	Time
FC1	Pass	12:34pm
SRC	Pass	12:34pm
DET	Pass	12:34pm
BAR	Pass	12:34pm
BT	Pass	12:34pm

Blank Tests

Test	Status	Time
AIR	Pass	12:35pm


Printer Tests

Test	Status	Time
PRNT	Pass	12:35pm

CRC Tests

Test	Status	Time
COMP	Pass	12:35pm
CAL	Pass	12:35pm

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County FORSYTH Instrument Location FORSYTH CO. DETENTION

Instrument Serial No 008583 WINSTON-SALEM, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are.

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus 2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 2ND day of FEBRUARY, 2024 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

669
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

FORSYTH COUNTY FORSYTH CO DETENTION
330

Serial Number: 008583
Test Date: 02/02/2024

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: Oligmueller, Leo A
Permit Number: 0035-3799
Effective:
10/01/2023-10/01/2025

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

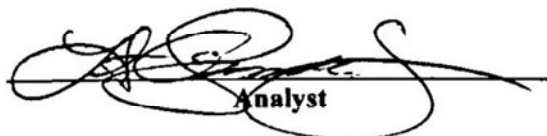
Lot Number: AG400302
Exp Date: 01/03/2026

Test	g/210L	Time
DIAG	Pass	8:49am
AIR BLK	.00	8:50am
ACCY CHK	.08	8:51am
AIR BLK	.00	8:52am
SUB TEST	.00	8:53am
AIR BLK	.00	8:54am
SUB TEST	.00	8:55am
AIR BLK	.00	8:57am

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

FORSYTH COUNTY FORSYTH CO DETENTION 330

Serial Number: 008583 Test Record Number: 9512
Test Date: 02/02/2024 Test Time: 8:58am EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	8:58am
FLO	Pass	8:58am
FC	Pass	8:58am

Temperature Tests

Test	Status	Time
FC1	Pass	8:59am
SRC	Pass	8:59am
DET	Pass	8:59am
BAR	Pass	8:59am
BT	Pass	8:59am

Blank Tests

Test	Status	Time
AIR	Pass	8:59am


Printer Tests

Test	Status	Time
PRNT	Pass	8:59am

CRC Tests

Test	Status	Time
COMP	Pass	8:59am
CAL	Pass	8:59am

Preventive Maintenance
Status: Pass


Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County FORSYTH Instrument Location FORSYTH CO. DETENTION
Instrument Serial No. 008659 WINSTON-SALEM, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 2ND day of FEBRUARY, 2024 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

669
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

FORSYTH COUNTY FORSYTH CO DETENTION
330

Serial Number: 008659
Test Date: 02/02/2024

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE

Analyst's Name: Oligmueller, Leo A
Permit Number: 0035-3799
Effective:
10/01/2023-10/01/2025

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG400302
Exp Date: 01/03/2026

Test	g/210L	Time
DIAG	Pass	9:19am
AIR BLK	.00	9:20am
ACCY CHK	.07	9:20am
AIR BLK	.00	9:21am
SUB TEST	.00	9:22am
AIR BLK	.00	9:23am
SUB TEST	.00	9:25am
AIR BLK	.00	9:25am

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

FORSYTH COUNTY FORSYTH CO DETENTION 330

Serial Number: 008659 Test Record Number: 6263
Test Date: 02/02/2024 Test Time: 9:28am EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	9:28am
FLO	Pass	9:28am
FC	Pass	9:28am

Temperature Tests

Test	Status	Time
FC1	Pass	9:28am
SRC	Pass	9:28am
DET	Pass	9:28am
BAR	Pass	9:28am
BT	Pass	9:28am

Blank Tests

Test	Status	Time
AIR	Pass	9:29am


Printer Tests

Test	Status	Time
PRNT	Pass	9:29am

CRC Tests

Test	Status	Time
COMP	Pass	9:29am
CAL	Pass	9:29am

Preventive Maintenance
Status: Pass


Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County FORSYTH Instrument Location FORSYTH CO. DETENTION
Instrument Serial No. 008660 WINSTON-SALEM, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 6TH day of FEBRUARY, 2024 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

669
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

FORSYTH COUNTY FORSYTH CO DETENTION
330

Serial Number: 008660
Test Date: 02/06/2024

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE

Analyst's Name: Oligmueller, Leo A
Permit Number: 0035-3799
Effective:
10/01/2023-10/01/2025

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test


Lot Number: AG400302
Exp Date: 01/03/2026

Test	g/210L	Time
DIAG	Pass	9:03am
AIR BLK	.00	9:03am
ACCY CHK	.08	9:04am
AIR BLK	.00	9:05am
SUB TEST	.00	9:06am
AIR BLK	.00	9:07am
SUB TEST	.00	9:08am
AIR BLK	.00	9:09am

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

FORSYTH COUNTY FORSYTH CO DETENTION 330

Serial Number: 008660 Test Record Number: 4516
Test Date: 02/06/2024 Test Time: 9:11am EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	9:11am
FLO	Pass	9:11am
FC	Pass	9:11am

Temperature Tests

Test	Status	Time
FC1	Pass	9:12am
SRC	Pass	9:12am
DET	Pass	9:12am
BAR	Pass	9:12am
BT	Pass	9:12am

Blank Tests

Test	Status	Time
AIR	Pass	9:12am

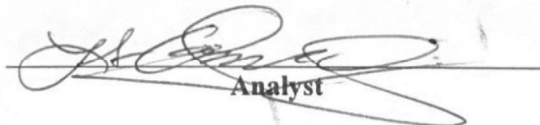
Printer Tests

Test	Status	Time
PRNT	Pass	9:12am

CRC Tests

Test	Status	Time
COMP	Pass	9:12am
CAL	Pass	9:12am

Preventive Maintenance
Status: Pass


Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County FORSYTH Instrument Location KERNERSVILLE POLICE

Instrument Serial No. 008876 DEPARTMENT

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 14TH day of FEBRUARY, 2024 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

1669
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

FORSYTH COUNTY KERNERSVILLE PD 330

Serial Number: 008896

Test Date: 02/14/2024

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Oligmueller, Leo A

Permit Number: 0035-3799

Effective:

10/01/2023-10/01/2025

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG308704


Exp Date: 03/28/2025

Test	g/210L	Time
DIAG	Pass	10:17am
AIR BLK	.00	10:18am
ACCY CHK	.08	10:19am
AIR BLK	.00	10:20am
SUB TEST	.00	10:21am
AIR BLK	.00	10:22am
SUB TEST	.00	10:24am
AIR BLK	.00	10:25am

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

FORSYTH COUNTY KERNERSVILLE PD 330

Serial Number: 008896 Test Record Number: 1687
Test Date: 02/14/2024 Test Time: 10:25am EST

System Check: Passed

Baseline Tests

Test	Status	Time
IR	Pass	10:26am
FLO	Pass	10:26am
FC	Pass	10:26am

Temperature Tests

Test	Status	Time
FC1	Pass	10:26am
SRC	Pass	10:26am
DET	Pass	10:26am
BAR	Pass	10:26am
BT	Pass	10:26am

Blank Tests

Test	Status	Time
AIR	Pass	10:27am


Printer Tests

Test	Status	Time
PRNT	Pass	10:27am

CRC Tests

Test	Status	Time
COMP	Pass	10:27am
CAL	Pass	10:27am

Preventive Maintenance
Status: Pass


Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County FORSYTH Instrument Location FORSYTH CO. DETENTION
Instrument Serial No. 008925 WINSTON-SALEM, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 2ND day of FEBRUARY, 2024 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.




Signature of Certifying Official

669
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

FORSYTH COUNTY FORSYTH CO DETENTION
330

Serial Number: 008925
Test Date: 02/02/2024

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: Oligmueller, Leo A
Permit Number: 0035-3799
Effective:
10/01/2023-10/01/2025

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test


Lot Number: AG400302
Exp Date: 01/03/2026

Test	g/210L	Time
DIAG	Pass	8:37am
AIR BLK	.00	8:38am
ACCY CHK	.08	8:39am
AIR BLK	.00	8:40am
SUB TEST	.00	8:41am
AIR BLK	.00	8:42am
SUB TEST	.00	8:44am
AIR BLK	.00	8:44am

Reported AC: .00 g/210L


~~Signature of Chemical Analyst~~

Court CVR


Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

FORSYTH COUNTY FORSYTH CO DETENTION 330

Serial Number: 008925 Test Record Number: 4834
Test Date: 02/02/2024 Test Time: 8:47am EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	8:47am
FLO	Pass	8:47am
FC	Pass	8:47am

Temperature Tests

Test	Status	Time
FC1	Pass	8:47am
SRC	Pass	8:47am
DET	Pass	8:47am
BAR	Pass	8:47am
BT	Pass	8:47am

Blank Tests

Test	Status	Time
AIR	Pass	8:48am

Printer Tests

Test	Status	Time
PRNT	Pass	8:48am

CRC Tests

Test	Status	Time
COMP	Pass	8:48am
CAL	Pass	8:48am

Preventive Maintenance
Status: Pass


Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Gaston Instrument Location Gaston County Jail
Instrument Serial No. 008643 Gaston, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 19th day of February, 2024 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Bryce Helms
Signature of Certifying Official

674
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

GASTON COUNTY GASTON COUNTY SO 350

Serial Number: 008643

Test Date: 02/19/2024

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Helms, Bryce A

Permit Number: 0084-9845

Effective:

10/01/2023-10/01/2025

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG308702


Exp Date: 03/28/2025

Test	g/210L	Time
DIAG	Pass	11:12am
AIR BLK	.00	11:13am
ACCY CHK	.08	11:14am
AIR BLK	.00	11:15am
SUB TEST	.00	11:16am
AIR BLK	.00	11:17am
SUB TEST	.00	11:18am
AIR BLK	.00	11:19am

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

GASTON COUNTY GASTON COUNTY SO 350

Serial Number: 008643 Test Record Number: 4731
Test Date: 02/19/2024 Test Time: 11:21am EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	11:21am
FLO	Pass	11:21am
FC	Pass	11:21am

Temperature Tests

Test	Status	Time
FC1	Pass	11:21am
SRC	Pass	11:21am
DET	Pass	11:21am
BAR	Pass	11:21am
BT	Pass	11:21am

Blank Tests

Test	Status	Time
AIR	Pass	11:22am

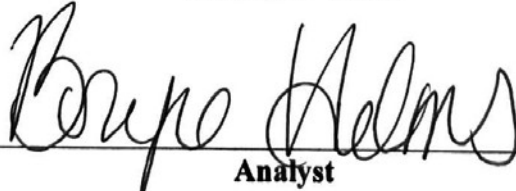
Printer Tests

Test	Status	Time
PRNT	Pass	11:22am

CRC Tests

Test	Status	Time
COMP	Pass	11:22am
CAL	Pass	11:22am

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Gates

Instrument Location

Gates Co. S.O.

Instrument Serial No. 008847

202 Court St. Gatesville,
NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 2nd day of February, 2024 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Mark A. Russell
Signature of Certifying Official

680
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

GATES COUNTY GATES CO SO 360

Serial Number: 008847

Test Date: 02/02/2024

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Chappell, Mark A

Permit Number: 0020-6272

Effective:

10/01/2023-10/01/2025

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG308003

Exp Date: 03/21/2025

Test	g/210L	Time
DIAG	Pass	2:38pm
AIR BLK	.00	2:38pm
ACCY CHK	.07	2:39pm
AIR BLK	.00	2:40pm
SUB TEST	.00	2:41pm
AIR BLK	.00	2:41pm
SUB TEST	.00	2:43pm
AIR BLK	.00	2:44pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

GATES COUNTY GATES CO SO 360

Serial Number: 008847 Test Record Number: 867
Test Date: 02/02/2024 Test Time: 2:45pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	2:45pm
FLO	Pass	2:45pm
FC	Pass	2:45pm

Temperature Tests

Test	Status	Time
FC1	Pass	2:46pm
SRC	Pass	2:46pm
DET	Pass	2:46pm
BAR	Pass	2:46pm
BT	Pass	2:46pm

Blank Tests

Test	Status	Time
AIR	Pass	2:46pm

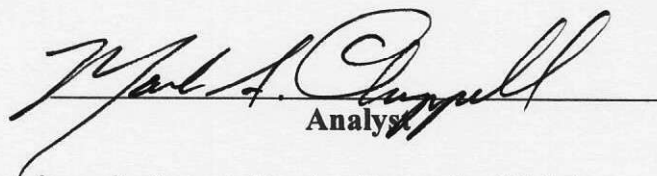
Printer Tests

Test	Status	Time
PRNT	Pass	2:46pm

CRC Tests

Test	Status	Time
COMP	Pass	2:46pm
CAL	Pass	2:46pm

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Gates Instrument Location Gates Co. Sheriff's Office
Instrument Serial No. 008884 202 Court St. Gatesville,
NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 23rd day of February, 2024 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

680
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

GATES COUNTY GATES CO SO 360

Serial Number: 008884
Test Date: 02/23/2024

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Chappell, Mark A

Permit Number: 0020-6272

Effective:

10/01/2023-10/01/2025

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

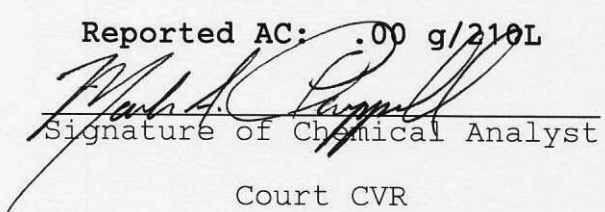
Test Type: Breath Test

Lot Number: AG308003

Exp Date: 03/21/2025

Test	g/210L	Time
DIAG	Pass	2:10pm
AIR BLK	.00	2:10pm
ACCY CHK	.07	2:11pm
AIR BLK	.00	2:12pm
SUB TEST	.00	2:13pm
AIR BLK	.00	2:14pm
SUB TEST	.00	2:16pm
AIR BLK	.00	2:16pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

GATES COUNTY GATES CO SO 360

Serial Number: 008884 Test Record Number: 1171
Test Date: 02/23/2024 Test Time: 2:17pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	2:17pm
FLO	Pass	2:17pm
FC	Pass	2:18pm

Temperature Tests

Test	Status	Time
FC1	Pass	2:18pm
SRC	Pass	2:18pm
DET	Pass	2:18pm
BAR	Pass	2:18pm
BT	Pass	2:18pm

Blank Tests

Test	Status	Time
AIR	Pass	2:18pm


Printer Tests

Test	Status	Time
PRNT	Pass	2:18pm

CRC Tests

Test	Status	Time
COMP	Pass	2:19pm
CAL	Pass	2:19pm

Preventive Maintenance
Status: Pass


Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Greene Instrument Location Greene Co. S.O.

Instrument Serial No. 008670 301 W. Greene St., Snow Hill,
N.C.

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 21st day of February, 2024 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Key D. Day
Signature of Certifying Official

643
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

GREENE COUNTY GREENE CO SO 390

Serial Number: 008670

Test Date: 02/21/2024

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Gray, Kelly D

Permit Number: 0037-7722

Effective:

10/01/2023-10/01/2025

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG302703


Exp Date: 01/27/2025

Test	g/210L	Time
DIAG	Pass	2:04pm
AIR BLK	.00	2:05pm
ACCY CHK	.08	2:05pm
AIR BLK	.00	2:06pm
SUB TEST	.00	2:07pm
AIR BLK	.00	2:08pm
SUB TEST	.00	2:10pm
AIR BLK	.00	2:11pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

Intox EC/IR-II: Preventive Maintenance

GREENE COUNTY GREENE CO SO 390

Serial Number: 008670 Test Record Number: 2412
Test Date: 02/21/2024 Test Time: 2:12pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	2:12pm
FLO	Pass	2:12pm
FC	Pass	2:12pm

Temperature Tests

Test	Status	Time
FC1	Pass	2:12pm
SRC	Pass	2:12pm
DET	Pass	2:12pm
BAR	Pass	2:12pm
BT	Pass	2:12pm

Blank Tests

Test	Status	Time
AIR	Pass	2:13pm


Printer Tests

Test	Status	Time
PRNT	Pass	2:13pm

CRC Tests

Test	Status	Time
COMP	Pass	2:13pm
CAL	Pass	2:13pm

Preventive Maintenance
Status: Pass


Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County GUILFORD Instrument Location HIGH POINT JAIL
Instrument Serial No. 008655 HIGH POINT, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 26TH day of FEBRUARY, 2024 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

6669
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

GUILFORD COUNTY HIGH POINT JAIL 400

Serial Number: 008655
Test Date: 02/26/2024

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Oligmueller, Leo A

Permit Number: 0035-3799

Effective:

10/01/2023-10/01/2025

Officer's Name: NONE,

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG303001

Exp Date: 01/30/2025

Test	g/210L	Time
DIAG	Pass	10:33am
AIR BLK	.00	10:34am
ACCY CHK	.08	10:35am
AIR BLK	.00	10:36am
SUB TEST	.00	10:37am
AIR BLK	.00	10:38am
SUB TEST	.00	10:40am
AIR BLK	.00	10:41am

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

GUILFORD COUNTY HIGH POINT JAIL 400

Serial Number: 008655 Test Record Number: 3987
Test Date: 02/26/2024 Test Time: 10:41am EST

System Check: Passed

Baseline Tests

Test	Status	Time
IR	Pass	10:42am
FLO	Pass	10:42am
FC	Pass	10:42am

Temperature Tests

Test	Status	Time
FC1	Pass	10:42am
SRC	Pass	10:42am
DET	Pass	10:42am
BAR	Pass	10:42am
BT	Pass	10:42am

Blank Tests

Test	Status	Time
AIR	Pass	10:43am

Printer Tests

Test	Status	Time
PRNT	Pass	10:43am

CRC Tests

Test	Status	Time
COMP	Pass	10:43am
CAL	Pass	10:43am

Preventive Maintenance
Status: Pass


Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County GUILFORD Instrument Location GREENSBORO POLICE
Instrument Serial No. 008725 DEPARTMENT

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 7TH day of FEBRUARY, 2024 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.




Signature of Certifying Official

669
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

GUILFORD COUNTY GREENSBORO PD 400

Serial Number: 008725

Test Date: 02/07/2024

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Oligmueller, Leo A

Permit Number: 0035-3799

Effective:

10/01/2023-10/01/2025

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG308101

Exp Date: 03/22/2025

Test	g/210L	Time
DIAG	Pass	2:24pm
AIR BLK	.00	2:25pm
ACCY CHK	.08	2:25pm
AIR BLK	.00	2:27pm
SUB TEST	.00	2:27pm
AIR BLK	.00	2:28pm
SUB TEST	.00	2:30pm
AIR BLK	.00	2:30pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

GUILFORD COUNTY GREENSBORO PD 400

Serial Number: 008725 Test Record Number: 4888
Test Date: 02/07/2024 Test Time: 2:31pm EST

System Check: Passed

Baseline Tests

Test	Status	Time
IR	Pass	2:31pm
FLO	Pass	2:31pm
FC	Pass	2:31pm

Temperature Tests

Test	Status	Time
FC1	Pass	2:32pm
SRC	Pass	2:32pm
DET	Pass	2:32pm
BAR	Pass	2:32pm
BT	Pass	2:32pm

Blank Tests

Test	Status	Time
AIR	Pass	2:32pm

Printer Tests

Test	Status	Time
PRNT	Pass	2:32pm

CRC Tests

Test	Status	Time
COMP	Pass	2:32pm
CAL	Pass	2:32pm

Preventive Maintenance
Status: Pass


Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County GUILFORD Instrument Location GREENSBORO JAIL

Instrument Serial No. 008790

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 15TH day of FEBRUARY, 2024 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



A handwritten signature in black ink, appearing to be "H. [unclear]".
Signature of Certifying Official

669
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

GUILFORD COUNTY GREENSBORO JAIL 400

Serial Number: 008790
Test Date: 02/15/2024

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE

Analyst's Name: Oligmueller, Leo A
Permit Number: 0035-3799
Effective:
10/01/2023-10/01/2025

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG400302
Exp Date: 01/03/2026

Test	g/210L	Time
DIAG	Pass	10:48am
AIR BLK	.00	10:49am
ALCOHOL CHK	.08	10:50am
AIR BLK	.00	10:51am
SUB TEST	.00	10:53am
AIR BLK	.00	10:53am
SUB TEST	.00	10:55am
AIR BLK	.00	10:56am

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

GUILFORD COUNTY GREENSBORO JAIL 400

Serial Number: 008790 Test Record Number: 8063
Test Date: 02/15/2024 Test Time: 10:59am EST

System Check: Passed

Baseline Tests

Test	Status	Time
IR	Pass	10:59am
FLO	Pass	10:59am
FC	Pass	10:59am

Temperature Tests

Test	Status	Time
FC1	Pass	10:59am
SRC	Pass	10:59am
DET	Pass	10:59am
BAR	Pass	10:59am
BT	Pass	10:59am

Blank Tests

Test	Status	Time
AIR	Pass	11:00am

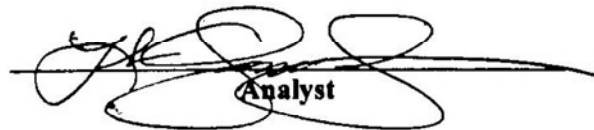
Printer Tests

Test	Status	Time
PRNT	Pass	11:00am

CRC Tests

Test	Status	Time
COMP	Pass	11:00am
CAL	Pass	11:00am

**Preventive Maintenance
Status: Pass**


Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County HALIFAX Instrument Location HALIFAX CO. S.D.
Instrument Serial No. 008695 355 FERRELL LANE
HALIFAX, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 7 day of FEBRUARY, 2024 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

671
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

HALIFAX CO. HALIFAX CO SO 410

Serial Number: 008695

Test Date: 02/07/2024

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Bryant, Earl A

Permit Number: 0017-9707

Effective:

10/01/2023-10/01/2025

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG303102


Exp Date: 01/31/2025

Test	g/210L	Time
DIAG	Pass	3:59pm
AIR BLK	.00	3:59pm
ACCY CHK	.07	4:00pm
AIR BLK	.00	4:01pm
SUB TEST	.00	4:02pm
AIR BLK	.00	4:03pm
SUB TEST	.00	4:04pm
AIR BLK	.00	4:05pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

HALIFAX CO. HALIFAX CO SO 410

Serial Number: 008695

Test Record Number: 3721

Test Date: 02/07/2024

Test Time: 4:06pm EST

System Check: Passed

Baseline Tests

Test	Status	Time
IR	Pass	4:06pm
FLO	Pass	4:06pm
FC	Pass	4:06pm

Temperature Tests

Test	Status	Time
FC1	Pass	4:07pm
SRC	Pass	4:07pm
DET	Pass	4:07pm
BAR	Pass	4:07pm
BT	Pass	4:07pm

Blank Tests

Test	Status	Time
AIR	Pass	4:07pm

Printer Tests

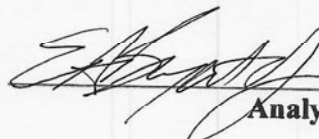
Test	Status	Time
PRNT	Pass	4:07pm

CRC Tests

Test	Status	Time
COMP	Pass	4:07pm
CAL	Pass	4:07pm

Preventive Maintenance

Status: Pass


Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Henderson

Instrument Location Henderson County Detention

Instrument Serial No. 008806

Hendersonville, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 6 day of February, 2024 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

668
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

HENDERSON COUNTY HENDERSON COUNTY
DETENTION 440

Serial Number: 008806

Test Date: 02/06/2024

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Loftis, Benjamin C

Permit Number: 0024-4987

Effective:

10/01/2023-10/01/2025

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

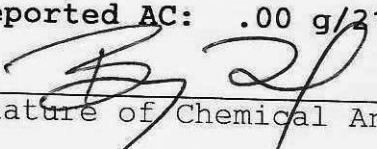
Test Type: Breath Test

Lot Number: AG308704

Exp Date: 03/28/2025

Test	g/210L	Time
DIAG	Pass	12:01pm
AIR BLK	.00	12:02pm
ACCY CHK	.08	12:02pm
AIR BLK	.00	12:04pm
SUB TEST	.00	12:04pm
AIR BLK	.00	12:05pm
SUB TEST	.00	12:07pm
AIR BLK	.00	12:08pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

HENDERSON COUNTY HENDERSON COUNTY DETENTION 440

Serial Number: 008806 Test Record Number: 3511
Test Date: 02/06/2024 Test Time: 12:08pm EST

System Check: Passed

Baseline Tests

Test	Status	Time
IR	Pass	12:08pm
FLO	Pass	12:08pm
FC	Pass	12:08pm

Temperature Tests

Test	Status	Time
FC1	Pass	12:09pm
SRC	Pass	12:09pm
DET	Pass	12:09pm
BAR	Pass	12:09pm
BT	Pass	12:09pm

Blank Tests

Test	Status	Time
AIR	Pass	12:09pm

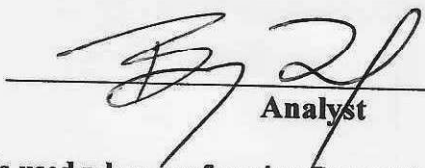
Printer Tests

Test	Status	Time
PRNT	Pass	12:09pm

CRC Tests

Test	Status	Time
COMP	Pass	12:09pm
CAL	Pass	12:09pm

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH


PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Henderson Instrument Location Henderson County Detention
Instrument Serial No. 608822 Hendersonville, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 6 day of February, 2024 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

668
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

HENDERSON COUNTY HENDERSON COUNTY
DETENTION 440

Serial Number: 008822
Test Date: 02/06/2024

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE

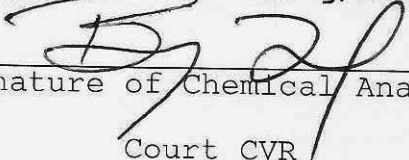
Analyst's Name: Loftis, Benjamin C
Permit Number: 0024-4987
Effective:
10/01/2023-10/01/2025

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG308004
Exp Date: 03/21/2025

Test	g/210L	Time
DIAG	Pass	11:59am
AIR BLK	.00	12:00pm
ACCY CHK	.07	12:01pm
AIR BLK	.00	12:02pm
SUB TEST	.00	12:03pm
AIR BLK	.00	12:03pm
SUB TEST	.00	12:05pm
AIR BLK	.00	12:06pm

Reported AC: .00 g/210L



Signature of Chemical Analyst
Court CVR



Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

HENDERSON COUNTY HENDERSON COUNTY DETENTION 440

Serial Number: 008822 Test Record Number: 3375
Test Date: 02/06/2024 Test Time: 12:07pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	12:07pm
FLO	Pass	12:07pm
FC	Pass	12:07pm

Temperature Tests

Test	Status	Time
FC1	Pass	12:07pm
SRC	Pass	12:07pm
DET	Pass	12:07pm
BAR	Pass	12:07pm
BT	Pass	12:07pm

Blank Tests

Test	Status	Time
AIR	Pass	12:08pm

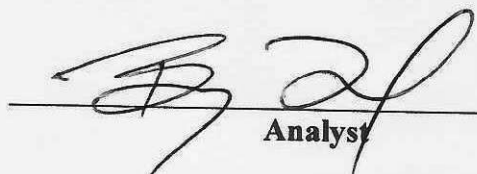
Printer Tests

Test	Status	Time
PRNT	Pass	12:08pm

CRC Tests

Test	Status	Time
COMP	Pass	12:08pm
CAL	Pass	12:08pm

Preventive Maintenance
Status: Pass


Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Hertford Instrument Location Murfreesboro P.D.
Instrument Serial No. 008906 115 E. Broad St Murfreesboro,
NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 2nd day of February, 2024 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Mark A. Russell
Signature of Certifying Official

680
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

HERTFORD COUNTY MURFREESBORO PD 450

Serial Number: 008906

Test Date: 02/02/2024

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Chappell, Mark A

Permit Number: 0020-6272

Effective:

10/01/2023-10/01/2025

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG308003

Exp Date: 03/21/2025

Test	g/210L	Time
DIAG	Pass	11:32am
AIR BLK	.00	11:33am
ACCY CHK	.08	11:34am
AIR BLK	.00	11:35am
SUB TEST	.00	11:36am
AIR BLK	.00	11:37am
SUB TEST	.00	11:38am
AIR BLK	.00	11:39am

Reported AC: .08 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

HERTFORD COUNTY MURFREESBORO PD 450

Serial Number: 008906 Test Record Number: 907
Test Date: 02/02/2024 Test Time: 11:40am EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	11:41am
FLO	Pass	11:41am
FC	Pass	11:41am

Temperature Tests

Test	Status	Time
FC1	Pass	11:41am
SRC	Pass	11:41am
DET	Pass	11:41am
BAR	Pass	11:41am
BT	Pass	11:41am

Blank Tests

Test	Status	Time
AIR	Pass	11:42am

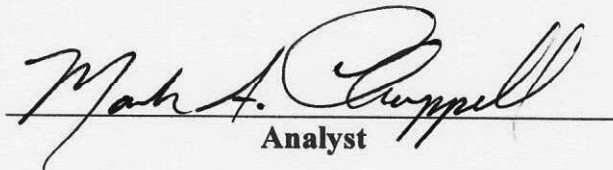
Printer Tests

Test	Status	Time
PRNT	Pass	11:42am

CRC Tests

Test	Status	Time
COMP	Pass	11:42am
CAL	Pass	11:42am

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Hyde Instrument Location Hyde Co. S.O.
Instrument Serial No. 008801 1223 Main St., Swan Quarter, NC.

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 27th day of February, 2024 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Key D. Gray
Signature of Certifying Official

643
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

HYDE COUNTY HYDE CO SO SWAN QUAR 470

Serial Number: 008801
Test Date: 02/27/2024

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: Gray, Kelly D
Permit Number: 0037-7722
Effective:
10/01/2023-10/01/2025

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG302702
Exp Date: 01/27/2025

Test	g/210L	Time
DIAG	Pass	11:26am
AIR BLK	.00	11:26am
ACCY CHK	.08	11:27am
AIR BLK	.00	11:28am
SUB TEST	.00	11:29am
AIR BLK	.00	11:30am
SUB TEST	.00	11:32am
AIR BLK	.00	11:33am

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

HYDE COUNTY HYDE CO SO SWAN QUAR 470

Serial Number: 008801 Test Record Number: 720
Test Date: 02/27/2024 Test Time: 11:35am EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	11:35am
FLO	Pass	11:35am
FC	Pass	11:35am

Temperature Tests

Test	Status	Time
FC1	Pass	11:36am
SRC	Pass	11:36am
DET	Pass	11:36am
BAR	Pass	11:36am
BT	Pass	11:36am

Blank Tests

Test	Status	Time
AIR	Pass	11:37am


Printer Tests

Test	Status	Time
PRNT	Pass	11:37am

CRC Tests

Test	Status	Time
COMP	Pass	11:37am
CAL	Pass	11:37am

Preventive Maintenance
Status: Pass


Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County WENDELL Instrument Location MOORESVILLE PD
Instrument Serial No. 008685 MOORESVILLE NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 19 day of FEBRUARY, 2024 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Jim S. Steining
Signature of Certifying Official

646
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

IREDELL COUNTY MOORESVILLE PD 480

Serial Number: 008685

Test Date: 02/19/2024

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Fleming, Tina S

Permit Number: 0027-4970

Effective:

07/01/2022-07/01/2024

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG400303

Exp Date: 01/03/2026

Test	g/210L	Time
DIAG	Pass	9:15am
AIR BLK	.00	9:16am
ACCY CHK	.08	9:17am
AIR BLK	.00	9:18am
SUB TEST	.00	9:19am
AIR BLK	.00	9:20am
SUB TEST	.00	9:21am
AIR BLK	.00	9:22am

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

IREDELL COUNTY MOORESVILLE PD 480

Serial Number: 008685 Test Record Number: 4571
Test Date: 02/19/2024 Test Time: 9:23am EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	9:24am
FLO	Pass	9:24am
FC	Pass	9:24am

Temperature Tests

Test	Status	Time
FC1	Pass	9:24am
SRC	Pass	9:24am
DET	Pass	9:24am
BAR	Pass	9:24am
BT	Pass	9:24am

Blank Tests

Test	Status	Time
AIR	Pass	9:24am


Printer Tests

Test	Status	Time
PRNT	Pass	9:25am

CRC Tests

Test	Status	Time
COMP	Pass	9:25am
CAL	Pass	9:25am

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Johnston Instrument Location Johnston County
Instrument Serial No. 008846 Detention Center

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 1 day of February, 2024 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

675
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

JOHNSTON COUNTY DETENTION CENTER 500

Serial Number: 008846
Test Date: 02/01/2024

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Garner, Joel K

Permit Number: 0036-5156

Effective:

10/01/2023-10/01/2025

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG308101

Exp Date: 03/22/2025


Test	g/210L	Time
DIAG	Pass	1:53pm
AIR BLK	.00	1:54pm
ACCY CHK	.08	1:55pm
AIR BLK	.00	1:56pm
SUB TEST	.00	1:57pm
AIR BLK	.00	1:58pm
SUB TEST	.00	1:59pm
AIR BLK	.00	2:00pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

JOHNSTON COUNTY DETENTION CENTER 500

Serial Number: 008846 Test Record Number: 6259
Test Date: 02/01/2024 Test Time: 2:01pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	2:01pm
FLO	Pass	2:01pm
FC	Pass	2:01pm

Temperature Tests

Test	Status	Time
FC1	Pass	2:02pm
SRC	Pass	2:02pm
DET	Pass	2:02pm
BAR	Pass	2:02pm
BT	Pass	2:02pm

Blank Tests

Test	Status	Time
AIR	Pass	2:02pm

Printer Tests

Test	Status	Time
PRNT	Pass	2:02pm

CRC Tests

Test	Status	Time
COMP	Pass	2:02pm
CAL	Pass	2:02pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Lenoir Instrument Location Lenoir Co. S.O.

Instrument Serial No. 008851 130 Queen St., Kingston, N.C.

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 21st day of February, 2024 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Ky. P. Boy

Signature of Certifying Official

643

Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

LENOIR COUNTY LENOIR CO SO 530

Serial Number: 008851
Test Date: 02/21/2024

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: Gray, Kelly D
Permit Number: 0037-7722
Effective:
10/01/2023-10/01/2025

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG302702
Exp Date: 01/27/2025


Test	g/210L	Time
DIAG	Pass	12:10pm
AIR BLK	.00	12:10pm
ACCY CHK	.08	12:11pm
AIR BLK	.00	12:12pm
SUB TEST	.00	12:13pm
AIR BLK	.00	12:14pm
SUB TEST	.00	12:16pm
AIR BLK	.00	12:17pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

LENOIR COUNTY LENOIR CO SO 530

Serial Number: 008851 Test Record Number: 942
Test Date: 02/21/2024 Test Time: 12:18pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	12:18pm
FLO	Pass	12:18pm
FC	Pass	12:18pm

Temperature Tests

Test	Status	Time
FC1	Pass	12:18pm
SRC	Pass	12:18pm
DET	Pass	12:18pm
BAR	Pass	12:18pm
BT	Pass	12:18pm

Blank Tests

Test	Status	Time
AIR	Pass	12:19pm


Printer Tests

Test	Status	Time
PRNT	Pass	12:19pm

CRC Tests

Test	Status	Time
COMP	Pass	12:19pm
CAL	Pass	12:19pm

Preventive Maintenance
Status: Pass


Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Lincoln Instrument Location Lincoln Co Jail
Instrument Serial No. 008823 Lincolnton, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 19th day of February, 2024 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

674
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

LINCOLN COUNTY LINCOLN COUNTY SO 540

Serial Number: 008823

Test Date: 02/19/2024

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Helms, Bryce A

Permit Number: 0084-9845

Effective:

10/01/2023-10/01/2025

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG212402

Exp Date: 05/04/2024


Test	g/210L	Time
DIAG	Pass	12:20pm
AIR BLK	.00	12:20pm
ACCY CHK	.08	12:21pm
AIR BLK	.00	12:22pm
SUB TEST	.00	12:22pm
AIR BLK	.00	12:23pm
SUB TEST	.00	12:25pm
AIR BLK	.00	12:26pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

LINCOLN COUNTY LINCOLN COUNTY SO 540

Serial Number: 008823 Test Record Number: 1918
Test Date: 02/19/2024 Test Time: 12:26pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	12:26pm
FLO	Pass	12:26pm
FC	Pass	12:27pm

Temperature Tests

Test	Status	Time
FC1	Pass	12:27pm
SRC	Pass	12:27pm
DET	Pass	12:27pm
BAR	Pass	12:27pm
BT	Pass	12:27pm

Blank Tests

Test	Status	Time
AIR	Pass	12:27pm

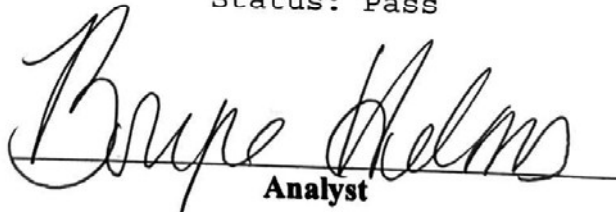
Printer Tests

Test	Status	Time
PRNT	Pass	12:27pm

CRC Tests

Test	Status	Time
COMP	Pass	12:28pm
CAL	Pass	12:28pm

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Lincoln Instrument Location Lincoln Co Jail
Lincolnton, NC
Instrument Serial No. 008827

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 19th day of February, 2024 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Bruce Helms
Signature of Certifying Official

674
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

LINCOLN COUNTY LINCOLN COUNTY SO 540

Serial Number: 008827

Test Date: 02/19/2024

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Helms, Bryce A

Permit Number: 0084-9845

Effective:

10/01/2023-10/01/2025

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG212403

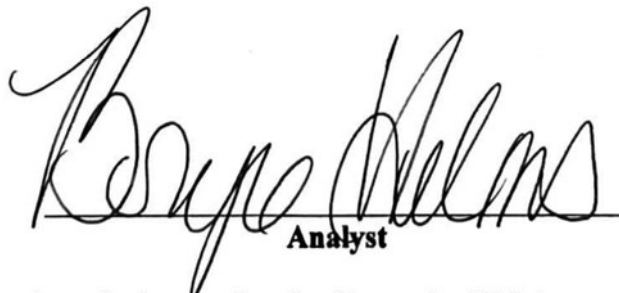
Exp Date: 05/04/2024

Test	g/210L	Time
DIAG	Pass	12:20pm
AIR BLK	.00	12:21pm
ACCY CHK	.08	12:22pm
AIR BLK	.00	12:23pm
SUB TEST	.00	12:23pm
AIR BLK	.00	12:24pm
SUB TEST	.00	12:26pm
AIR BLK	.00	12:27pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

LINCOLN COUNTY LINCOLN COUNTY SO 540

Serial Number: 008827 Test Record Number: 4083
Test Date: 02/19/2024 Test Time: 12:27pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	12:27pm
FLO	Pass	12:27pm
FC	Pass	12:27pm

Temperature Tests

Test	Status	Time
FC1	Pass	12:27pm
SRC	Pass	12:27pm
DET	Pass	12:27pm
BAR	Pass	12:27pm
BT	Pass	12:27pm

Blank Tests

Test	Status	Time
AIR	Pass	12:28pm

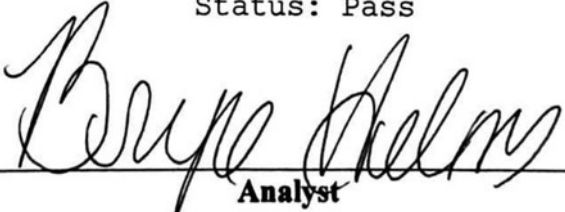
Printer Tests

Test	Status	Time
PRNT	Pass	12:28pm

CRC Tests

Test	Status	Time
COMP	Pass	12:28pm
CAL	Pass	12:28pm

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County McDowell County Instrument Location BAT Mobile unit 2
Instrument Serial No. 008970 Marion PD

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 11th day of February, 2024 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

679
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

MCDOWELL COUNTY BAT MOBILE UNIT 2 580

Serial Number: 008970

Test Date: 02/11/2024

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Greene, Nathaniel T

Permit Number: 0067-5960

Effective:

10/01/2023-10/01/2025

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

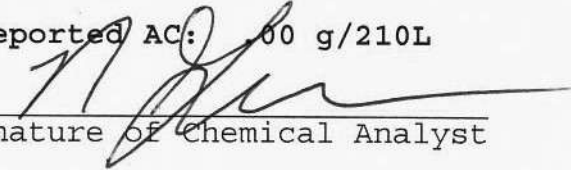
Test Type: Breath Test

Lot Number: AG302703

Exp Date: 01/27/2025

Test	g/210L	Time
DIAG	Pass	5:58pm
AIR BLK	.00	5:59pm
ACCY CHK	.08	5:59pm
AIR BLK	.00	6:00pm
SUB TEST	.00	6:01pm
AIR BLK	.00	6:02pm
SUB TEST	.00	6:04pm
AIR BLK	.00	6:05pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

MCDOWELL COUNTY BAT MOBILE UNIT 2 580

Serial Number: 008970 Test Record Number: 1068
Test Date: 02/11/2024 Test Time: 6:05pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	6:06pm
FLO	Pass	6:06pm
FC	Pass	6:06pm

Temperature Tests

Test	Status	Time
FC1	Pass	6:06pm
SRC	Pass	6:06pm
DET	Pass	6:06pm
BAR	Pass	6:06pm
BT	Pass	6:06pm

Blank Tests

Test	Status	Time
AIR	Pass	6:06pm

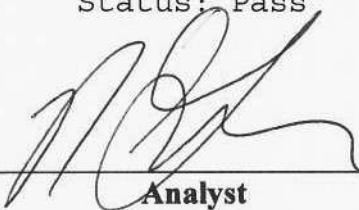
Printer Tests

Test	Status	Time
PRNT	Pass	6:07pm

CRC Tests

Test	Status	Time
COMP	Pass	6:07pm
CAL	Pass	6:07pm

Preventive Maintenance
Status: *Pass*



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County McDowell County Instrument Location BAT Mobile unit 2
Instrument Serial No. 008970 Marion PD

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 17th day of February, 2024 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

679
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

MCDOWELL COUNTY BAT MOBILE UNIT 2 580

Serial Number: 008970

Test Date: 02/11/2024

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Greene, Nathaniel T

Permit Number: 0067-5960

Effective:

10/01/2023-10/01/2025

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

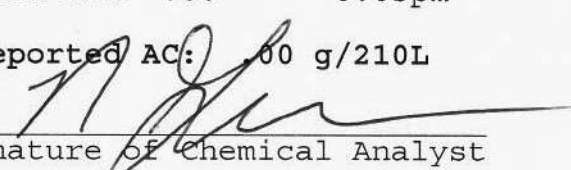
Test Type: Breath Test

Lot Number: AG302703

Exp Date: 01/27/2025

Test	g/210L	Time
DIAG	Pass	5:58pm
AIR BLK	.00	5:59pm
ACCY CHK	.08	5:59pm
AIR BLK	.00	6:00pm
SUB TEST	.00	6:01pm
AIR BLK	.00	6:02pm
SUB TEST	.00	6:04pm
AIR BLK	.00	6:05pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

MCDOWELL COUNTY BAT MOBILE UNIT 2 580

Serial Number: 008970 Test Record Number: 1068
Test Date: 02/11/2024 Test Time: 6:05pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	6:06pm
FLO	Pass	6:06pm
FC	Pass	6:06pm

Temperature Tests

Test	Status	Time
FC1	Pass	6:06pm
SRC	Pass	6:06pm
DET	Pass	6:06pm
BAR	Pass	6:06pm
BT	Pass	6:06pm

Blank Tests

Test	Status	Time
AIR	Pass	6:06pm

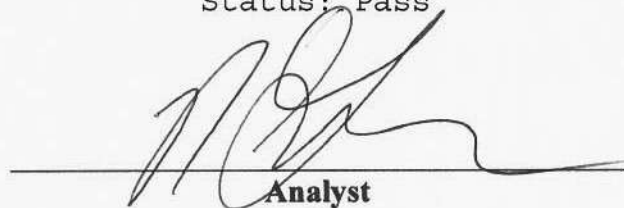
Printer Tests

Test	Status	Time
PRNT	Pass	6:07pm

CRC Tests

Test	Status	Time
COMP	Pass	6:07pm
CAL	Pass	6:07pm

Preventive Maintenance
Status: *Pass*



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County McDowell County Instrument Location BAT Mobile unit 2
Instrument Serial No. 008973 Marion PD

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 11th day of February, 2024 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

679
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

MCDOWELL COUNTY BAT MOBILE UNIT 2 580

Serial Number: 008973

Test Date: 02/11/2024

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Greene, Nathaniel T

Permit Number: 0067-5960

Effective:

10/01/2023-10/01/2025

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

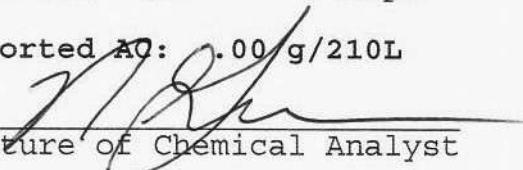
Test Type: Breath Test

Lot Number: AG302703

Exp Date: 01/27/2025

Test	g/210L	Time
DIAG	Pass	5:46pm
AIR BLK	.00	5:47pm
ACCY CHK	.08	5:48pm
AIR BLK	.00	5:48pm
SUB TEST	.00	5:49pm
AIR BLK	.00	5:50pm
SUB TEST	.00	5:52pm
AIR BLK	.00	5:52pm

Reported AQ: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

Intox EC/IR-II: Preventive Maintenance

MCDOWELL COUNTY BAT MOBILE UNIT 2 580

Serial Number: 008973 Test Record Number: 1123
Test Date: 02/11/2024 Test Time: 5:57pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	5:57pm
FLO	Pass	5:57pm
FC	Pass	5:57pm

Temperature Tests

Test	Status	Time
FC1	Pass	5:57pm
SRC	Pass	5:57pm
DET	Pass	5:57pm
BAR	Pass	5:57pm
BT	Pass	5:57pm

Blank Tests

Test	Status	Time
AIR	Pass	5:58pm


Printer Tests

Test	Status	Time
PRNT	Pass	5:58pm

CRC Tests

Test	Status	Time
COMP	Pass	5:58pm
CAL	Pass	5:58pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County McDowell County Instrument Location BAT Mobile unit 2
Instrument Serial No. 008973 Marion PD

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 11th day of February, 2024 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

679
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

MCDOWELL COUNTY BAT MOBILE UNIT 2 580

Serial Number: 008973

Test Date: 02/11/2024

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Greene, Nathaniel T

Permit Number: 0067-5960

Effective:

10/01/2023-10/01/2025

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

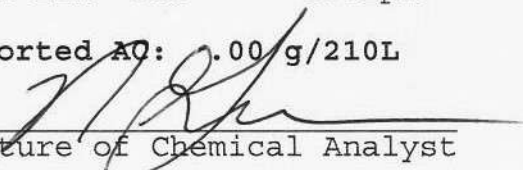
Test Type: Breath Test

Lot Number: AG302703

Exp Date: 01/27/2025

Test	g/210L	Time
DIAG	Pass	5:46pm
AIR BLK	.00	5:47pm
ACCY CHK	.08	5:48pm
AIR BLK	.00	5:48pm
SUB TEST	.00	5:49pm
AIR BLK	.00	5:50pm
SUB TEST	.00	5:52pm
AIR BLK	.00	5:52pm

Reported AO: .00/g/210L


Signature of Chemical Analyst

Court CVR


Analyst

Intox EC/IR-II: Preventive Maintenance

MCDOWELL COUNTY BAT MOBILE UNIT 2 580

Serial Number: 008973 Test Record Number: 1123
Test Date: 02/11/2024 Test Time: 5:57pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	5:57pm
FLO	Pass	5:57pm
FC	Pass	5:57pm

Temperature Tests

Test	Status	Time
FC1	Pass	5:57pm
SRC	Pass	5:57pm
DET	Pass	5:57pm
BAR	Pass	5:57pm
BT	Pass	5:57pm

Blank Tests

Test	Status	Time
AIR	Pass	5:58pm


Printer Tests

Test	Status	Time
PRNT	Pass	5:58pm

CRC Tests

Test	Status	Time
COMP	Pass	5:58pm
CAL	Pass	5:58pm

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Mecklenburg Instrument Location CMPTD LEC
Instrument Serial No. 008594 Charlotte, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 23rd day of February, 2024 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Brepe Helms
Signature of Certifying Official

6074
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

MECKLENBURG COUNTY CMPD LEC 590

Serial Number: 008594

Test Date: 02/23/2024

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Helms, Bryce A

Permit Number: 0084-9845

Effective:

10/01/2023-10/01/2025

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG400303

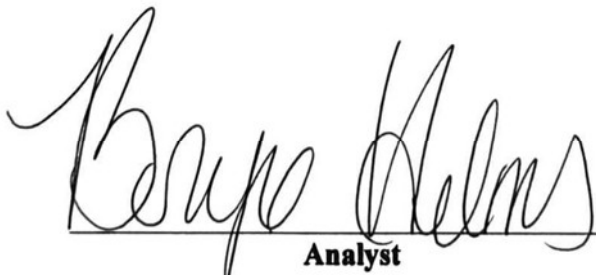
Exp Date: 01/03/2026

Test	g/210L	Time
DIAG	Pass	12:08pm
AIR BLK	.00	12:08pm
ACCY CHK	.07	12:09pm
AIR BLK	.00	12:10pm
SUB TEST	.00	12:11pm
AIR BLK	.00	12:12pm
SUB TEST	.00	12:13pm
AIR BLK	.00	12:14pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

Intox EC/IR-II: Preventive Maintenance

MECKLENBURG COUNTY CMPD LEC 590

Serial Number: 008594 • Test Record Number: 5875
Test Date: 02/23/2024 Test Time: 12:14pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	12:15pm
FLO	Pass	12:15pm
FC	Pass	12:15pm

Temperature Tests

Test	Status	Time
FC1	Pass	12:15pm
SRC	Pass	12:15pm
DET	Pass	12:15pm
BAR	Pass	12:15pm
BT	Pass	12:15pm

Blank Tests

Test	Status	Time
AIR	Pass	12:15pm


Printer Tests

Test	Status	Time
PRNT	Pass	12:15pm

CRC Tests

Test	Status	Time
COMP	Pass	12:16pm
CAL	Pass	12:16pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Mecklenburg Instrument Location Mecklenburg County 80
Instrument Serial No. 008665 Charlotte, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 23rd day of February, 2024 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Bryce Helms
Signature of Certifying Official

674
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

MECKLENBURG COUNTY SHERIFFS OFFICE 590

Serial Number: 008665
Test Date: 02/23/2024

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Helms, Bryce A

Permit Number: 0084-9845

Effective:

10/01/2023-10/01/2025

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG400303

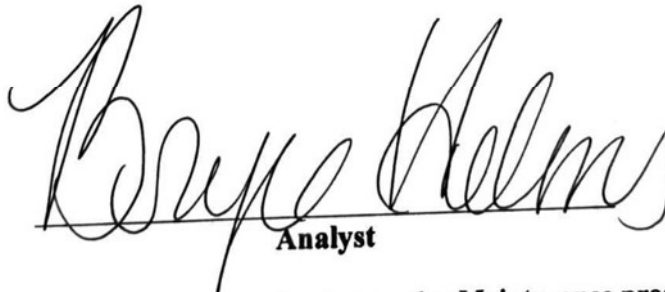
Exp Date: 01/03/2026

Test	g/210L	Time
DIAG	Pass	11:14am
AIR BLK	.00	11:15am
ACCY CHK	.08	11:16am
AIR BLK	.00	11:17am
SUB TEST	.00	11:17am
AIR BLK	.00	11:18am
SUB TEST	.00	11:20am
AIR BLK	.00	11:20am

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

MECKLENBURG COUNTY SHERIFFS OFFICE 590

Serial Number: 008665 Test Record Number: 5555
Test Date: 02/23/2024 Test Time: 11:21am EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	11:21am
FLO	Pass	11:21am
FC	Pass	11:21am

Temperature Tests

Test	Status	Time
FC1	Pass	11:21am
SRC	Pass	11:21am
DET	Pass	11:21am
BAR	Pass	11:21am
BT	Pass	11:21am

Blank Tests

Test	Status	Time
AIR	Pass	11:22am

Printer Tests

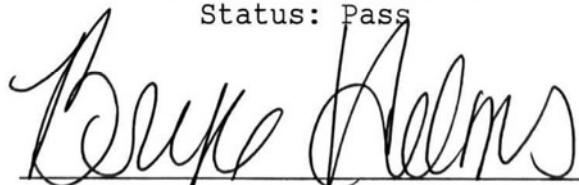
Test	Status	Time
PRNT	Pass	11:22am

CRC Tests

Test	Status	Time
COMP	Pass	11:22am
CAL	Pass	11:22am

Preventive Maintenance

Status: *Pass*


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County MECKLENBURG Instrument Location MECKLENBURG COUNTY 20
Instrument Serial No. 008665 CHARLOTTE NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 02 day of FEBRUARY, 2024 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Jim S. Stearns
Signature of Certifying Official

6440
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

MECKLENBURG COUNTY SHERIFFS OFFICE 590

Serial Number: 008665

Test Date: 02/02/2024

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Fleming, Tina S

Permit Number: 0027-4970

Effective:

07/01/2022-07/01/2024

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG308003

Exp Date: 03/21/2025

Test	g/210L	Time
DIAG	Pass	10:07am
AIR BLK	.00	10:08am
ACCY CHK	.08	10:09am
AIR BLK	.00	10:09am
SUB TEST	.00	10:10am
AIR BLK	.00	10:11am
SUB TEST	.00	10:12am
AIR BLK	.00	10:13am

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

MECKLENBURG COUNTY SHERIFFS OFFICE 590

Serial Number: 008665 Test Record Number: 5551
Test Date: 02/02/2024 Test Time: 10:14am EST

System Check: Passed

Baseline Tests

Test	Status	Time
IR	Pass	10:14am
FLO	Pass	10:14am
FC	Pass	10:15am

Temperature Tests

Test	Status	Time
FC1	Pass	10:15am
SRC	Pass	10:15am
DET	Pass	10:15am
BAR	Pass	10:15am
BT	Pass	10:15am

Blank Tests

Test	Status	Time
AIR	Pass	10:15am


Printer Tests

Test	Status	Time
PRNT	Pass	10:15am

CRC Tests

Test	Status	Time
COMP	Pass	10:16am
CAL	Pass	10:16am

Preventive Maintenance
Status: Pass



Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Mecklenburg Instrument Location Mecklenburg County 80
Instrument Serial No. 008690 Charlotte, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 23rd day of February, 2024 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Breke Helms
Signature of Certifying Official

6074
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

MECKLENBURG COUNTY SHERIFFS OFFICE 590

Serial Number: 008690
Test Date: 02/23/2024

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Helms, Bryce A

Permit Number: 0084-9845

Effective:

10/01/2023-10/01/2025

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG308003

Exp Date: 03/21/2025

Test	g/210L	Time
DIAG	Pass	11:12am
AIR BLK	.00	11:13am
ACCY CHK	.08	11:14am
AIR BLK	.00	11:15am
SUB TEST	.00	11:15am
AIR BLK	.00	11:16am
SUB TEST	.00	11:18am
AIR BLK	.00	11:19am

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR


Analyst

Intox EC/IR-II: Preventive Maintenance

MECKLENBURG COUNTY SHERIFFS OFFICE 590

Serial Number: 008690 Test Record Number: 7303
Test Date: 02/23/2024 Test Time: 11:19am EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	11:20am
FLO	Pass	11:20am
FC	Pass	11:20am

Temperature Tests

Test	Status	Time
FC1	Pass	11:20am
SRC	Pass	11:20am
DET	Pass	11:20am
BAR	Pass	11:20am
BT	Pass	11:20am

Blank Tests

Test	Status	Time
AIR	Pass	11:20am

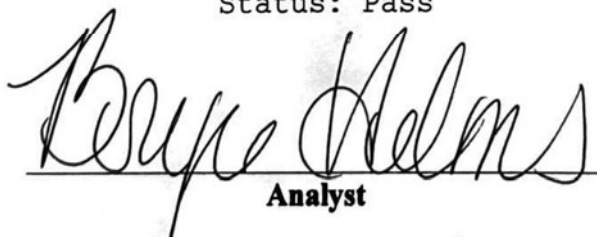
Printer Tests

Test	Status	Time
PRNT	Pass	11:20am

CRC Tests

Test	Status	Time
COMP	Pass	11:20am
CAL	Pass	11:20am

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Mecklenburg Instrument Location CMPD LEC
Instrument Serial No. 008702 Charlotte, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 23rd day of February, 2024 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Bryno Helms
Signature of Certifying Official

6074
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

MECKLENBURG COUNTY CMPD LEC 590

Serial Number: 008702

Test Date: 02/23/2024

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Helms, Bryce A

Permit Number: 0084-9845

Effective:

10/01/2023-10/01/2025

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG308702

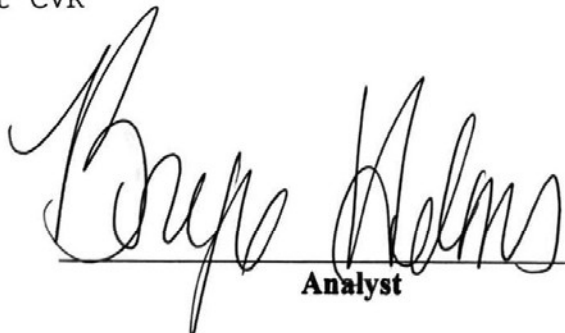
Exp Date: 03/28/2025

Test	g/210L	Time
DIAG	Pass	12:43pm
AIR BLK	.00	12:43pm
ACCY CHK	.07	12:44pm
AIR BLK	.00	12:45pm
SUB TEST	.00	12:46pm
AIR BLK	.00	12:47pm
SUB TEST	.00	12:48pm
AIR BLK	.00	12:49pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

MECKLENBURG COUNTY CMPD LEC 590

Serial Number: 008702 Test Record Number: 1979
Test Date: 02/23/2024 Test Time: 12:49pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	12:50pm
FLO	Pass	12:50pm
FC	Pass	12:50pm

Temperature Tests

Test	Status	Time
FC1	Pass	12:50pm
SRC	Pass	12:50pm
DET	Pass	12:50pm
BAR	Pass	12:50pm
BT	Pass	12:50pm

Blank Tests

Test	Status	Time
AIR	Pass	12:50pm

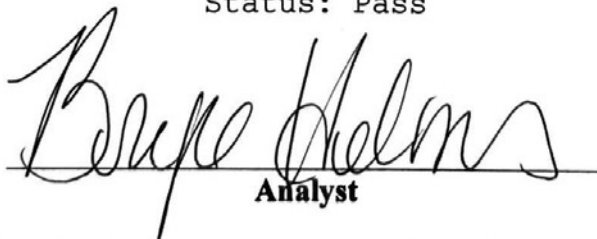
Printer Tests

Test	Status	Time
PRNT	Pass	12:50pm

CRC Tests

Test	Status	Time
COMP	Pass	12:51pm
CAL	Pass	12:51pm

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Mecklenburg Instrument Location Pineville Police Department
Instrument Serial No. 008703 Pineville, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 27th day of February, 2024 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Bruce Helms
Signature of Certifying Official

674
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

MECKLENBURG COUNTY PINEVILLE PD 590

Serial Number: 008703

Test Date: 02/27/2024

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Helms, Bryce A

Permit Number: 0084-9845

Effective:

10/01/2023-10/01/2025

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG212403


Exp Date: 05/04/2024

Test	g/210L	Time
DIAG	Pass	10:32am
AIR BLK	.00	10:32am
ACCY CHK	.08	10:33am
AIR BLK	.00	10:34am
SUB TEST	.00	10:35am
AIR BLK	.00	10:36am
SUB TEST	.00	10:37am
AIR BLK	.00	10:38am

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

Intox EC/IR-II: Preventive Maintenance

MECKLENBURG COUNTY PINEVILLE PD 590

Serial Number: 008703 Test Record Number: 6244
Test Date: 02/27/2024 Test Time: 10:39am EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	10:39am
FLO	Pass	10:39am
FC	Pass	10:39am

Temperature Tests

Test	Status	Time
FC1	Pass	10:39am
SRC	Pass	10:39am
DET	Pass	10:39am
BAR	Pass	10:39am
BT	Pass	10:39am

Blank Tests

Test	Status	Time
AIR	Pass	10:40am

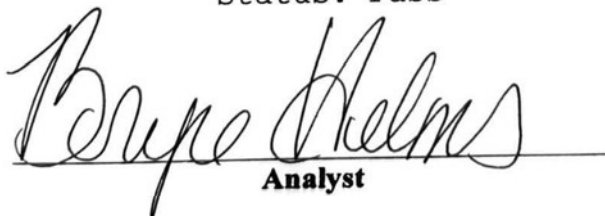
Printer Tests

Test	Status	Time
PRNT	Pass	10:40am

CRC Tests

Test	Status	Time
COMP	Pass	10:40am
CAL	Pass	10:40am

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County MECKLENBURG Instrument Location HUNTERSVILLE PD

Instrument Serial No. 008747 HUNTERSVILLE NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 27 day of FEBRUARY, 2024 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Jim S. Fleming
Signature of Certifying Official

646
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

MECKLENBURG HUNTERSVILLE PD 590

Serial Number: 008747

Test Date: 02/27/2024

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Fleming, Tina S

Permit Number: 0027-4970

Effective:

07/01/2022-07/01/2024

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG212402

Exp Date: 05/04/2024

Test	g/210L	Time
DIAG	Pass	2:10pm
AIR BLK	.00	2:11pm
ACCY CHK	.08	2:12pm
AIR BLK	.00	2:13pm
SUB TEST	.00	2:13pm
AIR BLK	.00	2:14pm
SUB TEST	.00	2:16pm
AIR BLK	.00	2:17pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

MECKLENBURG HUNTERSVILLE PD 590

Serial Number: 008747 Test Record Number: 3237
Test Date: 02/27/2024 Test Time: 2:17pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	2:18pm
FLO	Pass	2:18pm
FC	Pass	2:18pm

Temperature Tests

Test	Status	Time
FC1	Pass	2:18pm
SRC	Pass	2:18pm
DET	Pass	2:18pm
BAR	Pass	2:18pm
BT	Pass	2:18pm

Blank Tests

Test	Status	Time
AIR	Pass	2:19pm


Printer Tests

Test	Status	Time
PRNT	Pass	2:19pm

CRC Tests

Test	Status	Time
COMP	Pass	2:19pm
CAL	Pass	2:19pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County MECKLENBURG Instrument Location BAT MOBILE REGION 3
Instrument Serial No. 008898 MATTHEWS PD

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 08 day of FEBRUARY, 2024 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



M.C. Fleming
Signature of Certifying Official

676
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

MECKLENBURG COUNTY BAT MOBILE REGION 3
590

Serial Number: 008898
Test Date: 02/08/2024

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Fleming, Marshall C

Permit Number: 0027-5012

Effective:

10/01/2023-10/01/2025

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

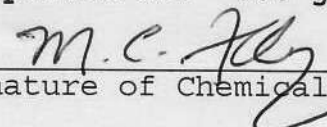
Test Type: Breath Test

Lot Number: AG225701

Exp Date: 09/14/2024

Test	g/210L	Time
DIAG	Pass	10:25pm
AIR BLK	.00	10:26pm
ACCY CHK	.08	10:26pm
AIR BLK	.00	10:27pm
SUB TEST	.00	10:28pm
AIR BLK	.00	10:29pm
SUB TEST	.00	10:30pm
AIR BLK	.00	10:31pm

Reported AC: .00 g/210L



Signature of Chemical Analyst
Court CVR



Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

MECKLENBURG COUNTY BAT MOBILE REGION 3 590

Serial Number: 008898 Test Record Number: 1768
Test Date: 02/08/2024 Test Time: 10:32pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	10:32pm
FLO	Pass	10:32pm
FC	Pass	10:32pm

Temperature Tests

Test	Status	Time
FC1	Pass	10:32pm
SRC	Pass	10:32pm
DET	Pass	10:32pm
BAR	Pass	10:32pm
BT	Pass	10:32pm

Blank Tests

Test	Status	Time
AIR	Pass	10:33pm

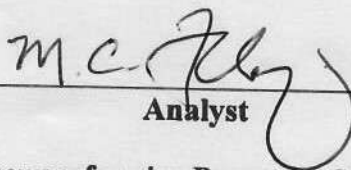
Printer Tests

Test	Status	Time
PRNT	Pass	10:33pm

CRC Tests

Test	Status	Time
COMP	Pass	10:33pm
CAL	Pass	10:33pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County MECKLENBURG Instrument Location BAT MOBILE REGION 3
Instrument Serial No. 008898 CMPD

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 14 day of FEBRUARY, 2024 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



M.C. Fly
Signature of Certifying Official

676
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

MECKLENBURG COUNTY BAT MOBILE REGION 3
590

Serial Number: 008898
Test Date: 02/14/2024

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Fleming, Marshall C

Permit Number: 0027-5012

Effective:

10/01/2023-10/01/2025

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG225701

Exp Date: 09/14/2024

Test	g/210L	Time
DIAG	Pass	9:09pm
AIR BLK	.00	9:10pm
ACCY CHK	.07	9:11pm
AIR BLK	.00	9:12pm
SUB TEST	.00	9:13pm
AIR BLK	.00	9:14pm
SUB TEST	.00	9:17pm
AIR BLK	.00	9:17pm

Reported AC: .00 g/210L

M.C. Fleming
Signature of Chemical Analyst
Court CVR

M.C. Fleming
Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

MECKLENBURG COUNTY BAT MOBILE REGION 3 590

Serial Number: 008898 Test Record Number: 1773
Test Date: 02/14/2024 Test Time: 9:29pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	9:30pm
FLO	Pass	9:30pm
FC	Pass	9:30pm

Temperature Tests

Test	Status	Time
FC1	Pass	9:30pm
SRC	Pass	9:30pm
DET	Pass	9:30pm
BAR	Pass	9:30pm
BT	Pass	9:30pm

Blank Tests

Test	Status	Time
AIR	Pass	9:31pm

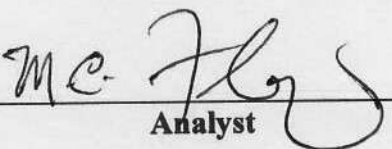
Printer Tests

Test	Status	Time
PRNT	Pass	9:31pm

CRC Tests

Test	Status	Time
COMP	Pass	9:31pm
CAL	Pass	9:31pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County MECKLENBURG Instrument Location BAT MOBILE REGION 3
Instrument Serial No. 008898 CMPO

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 15 day of FEBRUARY, 2024 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



M.C. [Signature]
Signature of Certifying Official

676
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

MECKLENBURG COUNTY BAT MOBILE REGION 3
590

Serial Number: 008898

Test Date: 02/15/2024

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Fleming, Marshall C

Permit Number: 0027-5012

Effective:

10/01/2023-10/01/2025

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG225701

Exp Date: 09/14/2024

Test	g/210L	Time
DIAG	Pass	9:10pm
AIR BLK	.00	9:11pm
ACCY CHK	.07	9:12pm
AIR BLK	.00	9:13pm
SUB TEST	.00	9:15pm
AIR BLK	.00	9:16pm
SUB TEST	.00	9:17pm
AIR BLK	.00	9:18pm

Reported AC: .00 g/210L

M.C. Fleming
Signature of Chemical Analyst

Court CVR

M.C. Fleming
Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

MECKLENBURG COUNTY BAT MOBILE REGION 3 590

Serial Number: 008898 Test Record Number: 1780
Test Date: 02/15/2024 Test Time: 9:20pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	9:20pm
FLO	Pass	9:20pm
FC	Pass	9:21pm

Temperature Tests

Test	Status	Time
FC1	Pass	9:21pm
SRC	Pass	9:21pm
DET	Pass	9:21pm
BAR	Pass	9:21pm
BT	Pass	9:21pm

Blank Tests

Test	Status	Time
AIR	Pass	9:21pm

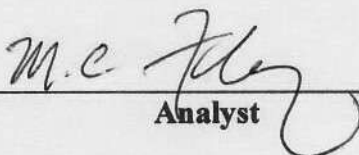
Printer Tests

Test	Status	Time
PRNT	Pass	9:21pm

CRC Tests

Test	Status	Time
COMP	Pass	9:22pm
CAL	Pass	9:22pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County MECKLENBURG Instrument Location BAT MOBILE REGION 3
Instrument Serial No. 008939 MATTHEWS PD

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 08 day of FEBRUARY, 20 24 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



M.C. Feltz
Signature of Certifying Official

676
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

MECKLENBURG COUNTY BAT MOBILE REGION 3
590

Serial Number: 008939
Test Date: 02/08/2024

Citation Number: M0000000-0
Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Fleming, Marshall C

Permit Number: 0027-5012

Effective:

10/01/2023-10/01/2025

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG225701

Exp Date: 09/14/2024

Test	g/210L	Time
DIAG	Pass	10:46pm
AIR BLK	.00	10:47pm
ACCY CHK	.08	10:48pm
AIR BLK	.00	10:49pm
SUB TEST	.00	10:50pm
AIR BLK	.00	10:50pm
SUB TEST	.00	10:52pm
AIR BLK	.00	10:53pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

MECKLENBURG COUNTY BAT MOBILE REGION 3 590

Serial Number: 008939 Test Record Number: 1621
Test Date: 02/08/2024 Test Time: 10:55pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	10:55pm
FLO	Pass	10:55pm
FC	Pass	10:55pm

Temperature Tests

Test	Status	Time
FC1	Pass	10:55pm
SRC	Pass	10:55pm
DET	Pass	10:55pm
BAR	Pass	10:55pm
BT	Pass	10:55pm

Blank Tests

Test	Status	Time
AIR	Pass	10:56pm

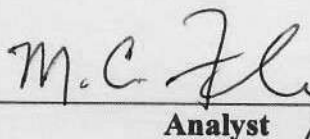
Printer Tests

Test	Status	Time
PRNT	Pass	10:56pm

CRC Tests

Test	Status	Time
COMP	Pass	10:56pm
CAL	Pass	10:56pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County MECKLENBURG Instrument Location BAT MOBILE REGION 3
Instrument Serial No. 008939 CMPO

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 15 day of FEBRUARY, 2024 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



M.C. Henry
Signature of Certifying Official

676
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

MECKLENBURG COUNTY BAT MOBILE REGION 3
590

Serial Number: 008939

Test Date: 02/15/2024

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Fleming, Marshall C

Permit Number: 0027-5012

Effective:

10/01/2023-10/01/2025

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG225701

Exp Date: 09/14/2024

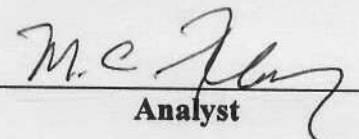
Test	g/210L	Time
DIAG	Pass	9:13pm
AIR BLK	.00	9:14pm
ACCY CHK	.07	9:15pm
AIR BLK	.00	9:16pm
SUB TEST	.00	9:17pm
AIR BLK	.00	9:18pm
SUB TEST	.00	9:20pm
AIR BLK	.00	9:20pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

MECKLENBURG COUNTY BAT MOBILE REGION 3 590

Serial Number: 008939 Test Record Number: 1628
Test Date: 02/15/2024 Test Time: 9:22pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	9:22pm
FLO	Pass	9:22pm
FC	Pass	9:22pm

Temperature Tests

Test	Status	Time
FC1	Pass	9:22pm
SRC	Pass	9:22pm
DET	Pass	9:22pm
BAR	Pass	9:22pm
BT	Pass	9:22pm

Blank Tests

Test	Status	Time
AIR	Pass	9:23pm

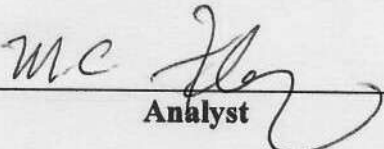
Printer Tests

Test	Status	Time
PRNT	Pass	9:23pm

CRC Tests

Test	Status	Time
COMP	Pass	9:23pm
CAL	Pass	9:23pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Montgomery Instrument Location Montgomery County
Instrument Serial No. 008657 Detention Center

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 26 day of February, 2024 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

675
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

MONTGOMERY COUNTY DETENTION CENTER 610

Serial Number: 008657

Test Date: 02/26/2024

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Garner, Joel K

Permit Number: 0036-5156

Effective:

10/01/2023-10/01/2025

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG303001

Exp Date: 01/30/2025

Test	g/210L	Time
DIAG	Pass	9:07am
AIR BLK	.00	9:07am
ACCY CHK	.08	9:08am
AIR BLK	.00	9:09am
SUB TEST	.00	9:10am
AIR BLK	.00	9:10am
SUB TEST	.00	9:12am
AIR BLK	.00	9:13am

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

MONTGOMERY COUNTY DETENTION CENTER 610

Serial Number: 008657 Test Record Number: 2124
Test Date: 02/26/2024 Test Time: 9:14am EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	9:14am
FLO	Pass	9:14am
FC	Pass	9:14am

Temperature Tests

Test	Status	Time
FC1	Pass	9:15am
SRC	Pass	9:15am
DET	Pass	9:15am
BAR	Pass	9:15am
BT	Pass	9:15am

Blank Tests

Test	Status	Time
AIR	Pass	9:15am


Printer Tests

Test	Status	Time
PRNT	Pass	9:15am

CRC Tests

Test	Status	Time
COMP	Pass	9:15am
CAL	Pass	9:15am

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Montgomery Instrument Location Montgomery County
Instrument Serial No. 008709 Detention Center

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 26 day of February, 2024 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

675

Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

MONTGOMERY COUNTY DETENTION CENTER 610

Serial Number: 008709

Test Date: 02/26/2024

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Garner, Joel K

Permit Number: 0036-5156

Effective:

10/01/2023-10/01/2025

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

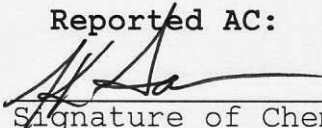
Test Type: Breath Test

Lot Number: AG303001

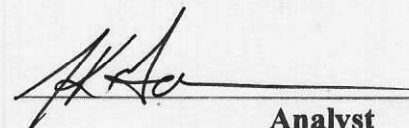
Exp Date: 01/30/2025

Test	g/210L	Time
DIAG	Pass	9:08am
AIR BLK	.00	9:08am
ACCY CHK	.07	9:09am
AIR BLK	.00	9:10am
SUB TEST	.00	9:11am
AIR BLK	.00	9:12am
SUB TEST	.00	9:13am
AIR BLK	.00	9:14am

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

MONTGOMERY COUNTY DETENTION CENTER 610

Serial Number: 008709 Test Record Number: 1471
Test Date: 02/26/2024 Test Time: 9:15am EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	9:15am
FLO	Pass	9:15am
FC	Pass	9:15am

Temperature Tests

Test	Status	Time
FC1	Pass	9:15am
SRC	Pass	9:15am
DET	Pass	9:15am
BAR	Pass	9:15am
BT	Pass	9:15am

Blank Tests

Test	Status	Time
AIR	Pass	9:16am


Printer Tests

Test	Status	Time
PRNT	Pass	9:16am

CRC Tests

Test	Status	Time
COMP	Pass	9:16am
CAL	Pass	9:16am

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County NEW HANOVER Instrument Location NEW HANOVER COUNTY
Instrument Serial No. 008617 DETENTION CENTER

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 22 day of FEBRUARY, 2024 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Alan R. Jones

Signature of Certifying Official

648

Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

NEW HANOVER COUNTY DETENTION CENTER
640

Serial Number: 008617
Test Date: 02/22/2024

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: BARNES, ALVIN R
Permit Number: 0014-6279
Effective:
10/01/2023-10/01/2025

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG308703
Exp Date: 03/28/2025

Test	g/210L	Time
DIAG	Pass	4:02pm
AIR BLK	.00	4:03pm
ACCY CHK	.07	4:04pm
AIR BLK	.00	4:05pm
SUB TEST	.00	4:06pm
AIR BLK	.00	4:07pm
SUB TEST	.00	4:08pm
AIR BLK	.00	4:09pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

NEW HANOVER COUNTY DETENTION CENTER 640

Serial Number: 008617 Test Record Number: 4842
Test Date: 02/22/2024 Test Time: 4:10pm EST

System Check: Passed

Baseline Tests

Test	Status	Time
IR	Pass	4:10pm
FLO	Pass	4:10pm
FC	Pass	4:10pm

Temperature Tests

Test	Status	Time
FC1	Pass	4:10pm
SRC	Pass	4:10pm
DET	Pass	4:10pm
BAR	Pass	4:10pm
BT	Pass	4:10pm

Blank Tests

Test	Status	Time
AIR	Pass	4:11pm

Printer Tests

Test	Status	Time
PRNT	Pass	4:11pm

CRC Tests

Test	Status	Time
COMP	Pass	4:11pm
CAL	Pass	4:11pm

Preventive Maintenance
Status: Pass


Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County NEW HANOVER Instrument Location NEW HANOVER COUNTY

Instrument Serial No. 008626 DETENTION CENTER

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 22 day of FEBRUARY, 2024 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Alan R. B...

Signature of Certifying Official

648

Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

**NEW HANOVER COUNTY DETENTION CENTER
640**

Serial Number: 008626
Test Date: 02/22/2024

Citation Number: M0000000-0
Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: BARNES, ALVIN R

Permit Number: 0014-6279

Effective:

10/01/2023-10/01/2025

Officer's Name: NONE, NONE

Type of Agency: FTA


Agency: DHHS

Test Type: Breath Test

Lot Number: AG308703
Exp Date: 03/28/2025

Test	g/210L	Time
DIAG	Pass	4:00pm
AIR BLK	.00	4:01pm
ACCY CHK	.08	4:02pm
AIR BLK	.00	4:03pm
SUB TEST	.00	4:04pm
AIR BLK	.00	4:05pm
SUB TEST	.00	4:06pm
AIR BLK	.00	4:07pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

NEW HANOVER COUNTY DETENTION CENTER 640

Serial Number: 008626 Test Record Number: 8525
Test Date: 02/22/2024 Test Time: 4:08pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	4:08pm
FLO	Pass	4:08pm
FC	Pass	4:08pm

Temperature Tests

Test	Status	Time
FC1	Pass	4:08pm
SRC	Pass	4:08pm
DET	Pass	4:08pm
BAR	Pass	4:08pm
BT	Pass	4:08pm

Blank Tests

Test	Status	Time
AIR	Pass	4:09pm


Printer Tests

Test	Status	Time
PRNT	Pass	4:09pm

CRC Tests

Test	Status	Time
COMP	Pass	4:09pm
CAL	Pass	4:09pm

Preventive Maintenance
Status: Pass


Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County NEW HAMPSHIRE Instrument Location CAROLINA BEACH
Instrument Serial No. 008661 POLICE DEPT

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 22 day of FEBRUARY, 2024 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Chas Rg Bano
Signature of Certifying Official

648
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

NEW HANOVER COUNTY CAROLINA BEACH PD
640

Serial Number: 008661
Test Date: 02/22/2024

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE

Analyst's Name: BARNES, ALVIN R
Permit Number: 0014-6279
Effective:
10/01/2023-10/01/2025

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG400301
Exp Date: 01/03/2026

Test	g/210L	Time
DIAG	Pass	11:54am
AIR BLK	.00	11:55am
ACCY CHK	.08	11:56am
AIR BLK	.00	11:57am
SUB TEST	.00	11:58am
AIR BLK	.00	11:59am
SUB TEST	.00	12:00pm
AIR BLK	.00	12:01pm

Reported AC: .00 g/210L

Alvin R. Barnes
Signature of Chemical Analyst

Court CVR

Alvin R. Barnes
Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

NEW HANOVER COUNTY CAROLINA BEACH PD 640

Serial Number: 008661 Test Record Number: 3204
Test Date: 02/22/2024 Test Time: 12:01pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	12:02pm
FLO	Pass	12:02pm
FC	Pass	12:02pm

Temperature Tests

Test	Status	Time
FC1	Pass	12:02pm
SRC	Pass	12:02pm
DET	Pass	12:02pm
BAR	Pass	12:02pm
BT	Pass	12:02pm

Blank Tests

Test	Status	Time
AIR	Pass	12:03pm


Printer Tests

Test	Status	Time
PRNT	Pass	12:03pm

CRC Tests

Test	Status	Time
COMP	Pass	12:03pm
CAL	Pass	12:03pm

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County NEW HAMPSHIRE Instrument Location WRIGHTSVILLE BEACH

Instrument Serial No. 008667 POLICE DEPT

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 22 day of FEBRUARY, 20 24 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Alan R. B...
Signature of Certifying Official

648
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

NEW HANOVER COUNTY WRIGHTSVILLE BCH PD
640

Serial Number: 008667
Test Date: 02/22/2024

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: BARNES, ALVIN R
Permit Number: 0014-6279
Effective:
10/01/2023-10/01/2025

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test


Lot Number: AG308703
Exp Date: 03/28/2025

Test	g/210L	Time
DIAG	Pass	2:31pm
AIR BLK	.00	2:32pm
ACCY CHK	.07	2:32pm
AIR BLK	.00	2:33pm
SUB TEST	.00	2:34pm
AIR BLK	.00	2:35pm
SUB TEST	.00	2:36pm
AIR BLK	.00	2:37pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

NEW HANOVER COUNTY WRIGHTSVILLE BCH PD 640

Serial Number: 008667 Test Record Number: 2589
Test Date: 02/22/2024 Test Time: 2:38pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	2:38pm
FLO	Pass	2:38pm
FC	Pass	2:38pm

Temperature Tests

Test	Status	Time
FC1	Pass	2:38pm
SRC	Pass	2:38pm
DET	Pass	2:38pm
BAR	Pass	2:38pm
BT	Pass	2:38pm

Blank Tests

Test	Status	Time
AIR	Pass	2:39pm


Printer Tests

Test	Status	Time
PRNT	Pass	2:39pm

CRC Tests

Test	Status	Time
COMP	Pass	2:39pm
CAL	Pass	2:39pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County NEW HANOVER Instrument Location NEW HANOVER COUNTY
Instrument Serial No. 008946 DETENTION CENTER

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 14 day of FEBRUARY, 2024 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Blm Rg Bams

Signature of Certifying Official

648

Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

NEW HANOVER COUNTY DETENTION CENTER
640

Serial Number: 008946
Test Date: 02/14/2024

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: BARNES, ALVIN R
Permit Number: 0014-6279
Effective:
10/01/2023-10/01/2025

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test


Lot Number: AG308703
Exp Date: 03/28/2025

Test	g/210L	Time
DIAG	Pass	12:34pm
AIR BLK	.00	12:35pm
ACCY CHK	.08	12:35pm
AIR BLK	.00	12:36pm
SUB TEST	.00	12:37pm
AIR BLK	.00	12:38pm
SUB TEST	.00	12:40pm
AIR BLK	.00	12:40pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

NEW HANOVER COUNTY DETENTION CENTER 640

Serial Number: 008946 Test Record Number: 1640
Test Date: 02/14/2024 Test Time: 12:41pm EST

System Check: Passed

Baseline Tests

Test	Status	Time
IR	Pass	12:42pm
FLO	Pass	12:42pm
FC	Pass	12:42pm

Temperature Tests

Test	Status	Time
FC1	Pass	12:42pm
SRC	Pass	12:42pm
DET	Pass	12:42pm
BAR	Pass	12:42pm
BT	Pass	12:42pm

Blank Tests

Test	Status	Time
AIR	Pass	12:42pm


Printer Tests

Test	Status	Time
PRNT	Pass	12:42pm

CRC Tests

Test	Status	Time
COMP	Pass	12:43pm
CAL	Pass	12:43pm

Preventive Maintenance
Status: Pass


Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County ONSLOW Instrument Location ONSLOW COUNTY
Instrument Serial No. 008578 JNEADS FERRY SUBSTATION

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 21 day of FEBRUARY, 2024 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Chris R. Bano

Signature of Certifying Official

648

Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

ONslow COUNTY SNEADS FERRY SUB 660

Serial Number: 008578
Test Date: 02/21/2024

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE

Analyst's Name: BARNES, ALVIN R
Permit Number: 0014-6279
Effective:
10/01/2023-10/01/2025

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG308101
Exp Date: 03/22/2025

Test	g/210L	Time
DIAG	Pass	11:00am
AIR BLK	.00	11:00am
ACCY CHK	.08	11:01am
AIR BLK	.00	11:02am
SUB TEST	.00	11:03am
AIR BLK	.00	11:04am
SUB TEST	.00	11:05am
AIR BLK	.00	11:06am

Reported AC: .00 g/210L

Alvin Rg Barnes
Signature of Chemical Analyst

Court CVR

Alvin Rg Barnes
Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

ONslow COUNTY SNEADS FERRY SUB 660

Serial Number: 008578 Test Record Number: 3528
Test Date: 02/21/2024 Test Time: 11:06am EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	11:07am
FLO	Pass	11:07am
FC	Pass	11:07am

Temperature Tests

Test	Status	Time
FC1	Pass	11:07am
SRC	Pass	11:07am
DET	Pass	11:07am
BAR	Pass	11:07am
BT	Pass	11:07am

Blank Tests

Test	Status	Time
AIR	Pass	11:08am


Printer Tests

Test	Status	Time
PRNT	Pass	11:08am

CRC Tests

Test	Status	Time
COMP	Pass	11:08am
CAL	Pass	11:08am

Preventive Maintenance
Status: Pass


Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County onslow Instrument Location BAT mobile unit 7

Instrument Serial No. 008600 onslow 50

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 24 day of February, 2024 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]

Signature of Certifying Official

665

Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

ONSLOW COUNTY BAT MOBILE UNIT 7 660

Serial Number: 008600

Test Date: 02/24/2024

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Anderson, Mark G

Permit Number: 0013-1517

Effective:

10/01/2023-10/01/2025

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG38004

Exp Date: 03/21/2025

Test	g/210L	Time
DIAG	Pass	10:56pm
AIR BLK	.00	10:57pm
ACCY CHK	.08	10:57pm
AIR BLK	.00	10:58pm
SUB TEST	.00	10:59pm
AIR BLK	.00	11:00pm
SUB TEST	.00	11:01pm
AIR BLK	.00	11:02pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

ONSLOW COUNTY BAT MOBILE UNIT 7 660

Serial Number: 008600 Test Record Number: 2685
Test Date: 02/24/2024 Test Time: 11:07pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	11:08pm
FLO	Pass	11:08pm
FC	Pass	11:08pm

Temperature Tests

Test	Status	Time
FC1	Pass	11:08pm
SRC	Pass	11:08pm
DET	Pass	11:08pm
BAR	Pass	11:08pm
BT	Pass	11:08pm

Blank Tests

Test	Status	Time
AIR	Pass	11:09pm

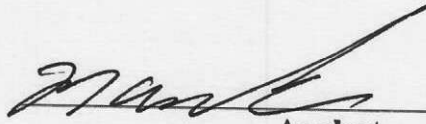
Printer Tests

Test	Status	Time
PRNT	Pass	11:09pm

CRC Tests

Test	Status	Time
COMP	Pass	11:09pm
CAL	Pass	11:09pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County onslow Instrument Location BAT Mobile Unit 7

Instrument Serial No. 008698 onslow 50

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 10 day of February, 2024 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]

Signature of Certifying Official

665

Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

ONSLOW COUNTY BAT MOBILE UNIT 7 660

Serial Number: 008698
Test Date: 02/10/2024

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Anderson, Mark G

Permit Number: 0013-1517

Effective:

10/01/2023-10/01/2025

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG302703

Exp Date: 01/27/2025

Test	g/210L	Time
DIAG	Pass	11:09pm
AIR BLK	.00	11:10pm
ACCY CHK	.07	11:11pm
AIR BLK	.00	11:12pm
SUB TEST	.00	11:12pm
AIR BLK	.00	11:13pm
SUB TEST	.00	11:14pm
AIR BLK	.00	11:15pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

ONslow COUNTY BAT MOBILE UNIT 7 660

Serial Number: 008698 Test Record Number: 2288
Test Date: 02/10/2024 Test Time: 11:18pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	11:19pm
FLO	Pass	11:19pm
FC	Pass	11:19pm

Temperature Tests

Test	Status	Time
FC1	Pass	11:19pm
SRC	Pass	11:19pm
DET	Pass	11:19pm
BAR	Pass	11:19pm
BT	Pass	11:19pm

Blank Tests

Test	Status	Time
AIR	Pass	11:20pm

Printer Tests

Test	Status	Time
PRNT	Pass	11:20pm

CRC Tests

Test	Status	Time
COMP	Pass	11:20pm
CAL	Pass	11:20pm

Preventive Maintenance
Status: *Pass*



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County onslow Instrument Location BAT Mobile Unit 7

Instrument Serial No. 008698 onslow SO

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 24 day of February, 2024 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

665
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

ONSLOW COUNTY BAT MOBILE UNIT 7 660

Serial Number: 008698

Test Date: 02/24/2024

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Anderson, Mark G

Permit Number: 0013-1517

Effective:

10/01/2023-10/01/2025

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG302703

Exp Date: 01/27/2025

Test	g/210L	Time
DIAG	Pass	10:54pm
AIR BLK	.00	10:55pm
ACCY CHK	.07	10:55pm
AIR BLK	.00	10:56pm
SUB TEST	.00	10:57pm
AIR BLK	.00	10:58pm
SUB TEST	.00	10:59pm
AIR BLK	.00	11:00pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

ONSLOW COUNTY BAT MOBILE UNIT 7 660

Serial Number: 008698 Test Record Number: 2298
Test Date: 02/24/2024 Test Time: 11:03pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	11:04pm
FLO	Pass	11:04pm
FC	Pass	11:04pm

Temperature Tests

Test	Status	Time
FC1	Pass	11:04pm
SRC	Pass	11:04pm
DET	Pass	11:04pm
BAR	Pass	11:04pm
BT	Pass	11:04pm

Blank Tests

Test	Status	Time
AIR	Pass	11:05pm

Printer Tests

Test	Status	Time
PRNT	Pass	11:05pm

CRC Tests

Test	Status	Time
COMP	Pass	11:05pm
CAL	Pass	11:05pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County onslow Instrument Location BAT mobile unit 7
Instrument Serial No. 008288 Swansboro PD

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 10 day of February, 2024 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Mark

Signature of Certifying Official

665

Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

ONSLOW COUNTY BAT MOBILE UNIT 7 660

Serial Number: 008788
Test Date: 02/10/2024

Citation Number: M0000000-0
Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Anderson, Mark G

Permit Number: 0013-1517

Effective:
10/01/2023-10/01/2025

Officer's Name: NONE, NONE

Type of Agency: FTA

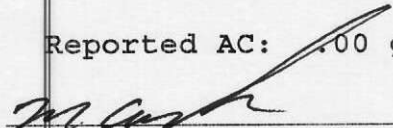
Agency: DHHS

Test Type: Breath Test

Lot Number: AG302703
Exp Date: 01/27/2025

Test	g/210L	Time
DIAG	Pass	9:36pm
AIR BLK	.00	9:36pm
ACCY CHK	.08	9:37pm
AIR BLK	.00	9:38pm
SUB TEST	.00	9:39pm
AIR BLK	.00	9:40pm
SUB TEST	.00	9:42pm
AIR BLK	.00	9:43pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

ONSLOW COUNTY BAT MOBILE UNIT 7 660

Serial Number: 008788 Test Record Number: 2166
Test Date: 02/10/2024 Test Time: 9:46pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	9:46pm
FLO	Pass	9:46pm
FC	Pass	9:46pm

Temperature Tests

Test	Status	Time
FC1	Pass	9:46pm
SRC	Pass	9:46pm
DET	Pass	9:46pm
BAR	Pass	9:46pm
BT	Pass	9:46pm

Blank Tests

Test	Status	Time
AIR	Pass	9:47pm


Printer Tests

Test	Status	Time
PRNT	Pass	9:47pm

CRC Tests

Test	Status	Time
COMP	Pass	9:47pm
CAL	Pass	9:47pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County onslow Instrument Location BAT Mobile Unit 7
Instrument Serial No. 008784 onslow 50

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 24 day of February, 2024 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

665
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

ONSLOW COUNTY BAT MOBILE UNIT 7 660

Serial Number: 008788

Test Date: 02/24/2024

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Anderson, Mark G

Permit Number: 0013-1517

Effective:

10/01/2023-10/01/2025

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

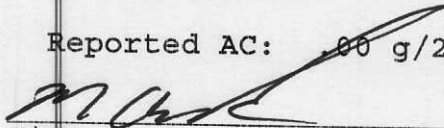
Test Type: Breath Test

Lot Number: AG302703

Exp Date: 01/27/2025

Test	g/210L	Time
DIAG	Pass	10:51pm
AIR BLK	.00	10:52pm
ACCY CHK	.08	10:53pm
AIR BLK	.00	10:54pm
SUB TEST	.00	10:56pm
AIR BLK	.00	10:57pm
SUB TEST	.00	10:59pm
AIR BLK	.00	11:00pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

ONSLOW COUNTY BAT MOBILE UNIT 7 660

Serial Number: 008788 Test Record Number: 2180
Test Date: 02/24/2024 Test Time: 11:01pm EST

System Check: Passed

Baseline Tests

Test	Status	Time
IR	Pass	11:02pm
FLO	Pass	11:02pm
FC	Pass	11:02pm

Temperature Tests

Test	Status	Time
FC1	Pass	11:02pm
SRC	Pass	11:02pm
DET	Pass	11:02pm
BAR	Pass	11:02pm
BT	Pass	11:02pm

Blank Tests

Test	Status	Time
AIR	Pass	11:03pm

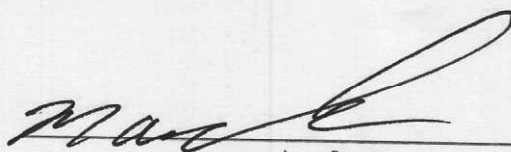
Printer Tests

Test	Status	Time
PRNT	Pass	11:03pm

CRC Tests

Test	Status	Time
COMP	Pass	11:03pm
CAL	Pass	11:03pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County ONslow Instrument Location MCA6
Instrument Serial No. 008919 NEW RIVER PMO

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 21 day of FEBRUARY, 2024 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Alan R. Benson
Signature of Certifying Official

648
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

ONslow COUNTY MCAS NEW RIVER 660

Serial Number: 008919

Test Date: 02/21/2024

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: BARNES, ALVIN R

Permit Number: 0014-6279

Effective:

10/01/2023-10/01/2025

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG308704

Exp Date: 03/28/2025

Test	g/210L	Time
DIAG	Pass	10:08am
AIR BLK	.00	10:08am
ACCY CHK	.07	10:09am
AIR BLK	.00	10:10am
SUB TEST	.00	10:11am
AIR BLK	.00	10:12am
SUB TEST	.00	10:13am
AIR BLK	.00	10:14am

Reported AC: .00 g/210L

Alvin Rg Barnes
Signature of Chemical Analyst

Court CVR

Alvin Rg Barnes
Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

ONSLOW COUNTY MCAS NEW RIVER 660

Serial Number: 008919 Test Record Number: 890
Test Date: 02/21/2024 Test Time: 10:15am EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	10:15am
FLO	Pass	10:15am
FC	Pass	10:15am

Temperature Tests

Test	Status	Time
FC1	Pass	10:15am
SRC	Pass	10:15am
DET	Pass	10:15am
BAR	Pass	10:15am
BT	Pass	10:15am

Blank Tests

Test	Status	Time
AIR	Pass	10:16am


Printer Tests

Test	Status	Time
PRNT	Pass	10:16am

CRC Tests

Test	Status	Time
COMP	Pass	10:16am
CAL	Pass	10:16am

Preventive Maintenance
Status: Pass


Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County ONslow Instrument Location CAMP LEJEUNE
Instrument Serial No. 008920 PMO

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 21 day of FEBRUARY, 2024 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Alan Rg Bane
Signature of Certifying Official

648
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

ONSLOW COUNTY CAMP LEJEUNE PMO 660

Serial Number: 008920

Test Date: 02/21/2024

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: BARNES, ALVIN R

Permit Number: 0014-6279

Effective:

10/01/2023-10/01/2025

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG400301

Exp Date: 01/03/2026

Test	g/210L	Time
DIAG	Pass	1:26pm
AIR BLK	.00	1:27pm
ACCY CHK	.08	1:27pm
AIR BLK	.00	1:29pm
SUB TEST	.00	1:29pm
AIR BLK	.00	1:30pm
SUB TEST	.00	1:31pm
AIR BLK	.00	1:32pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

ONslow COUNTY CAMP LEJEUNE PMO 660

Serial Number: 008920 Test Record Number: 2178
Test Date: 02/21/2024 Test Time: 1:33pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	1:34pm
FLO	Pass	1:34pm
FC	Pass	1:34pm

Temperature Tests

Test	Status	Time
FC1	Pass	1:34pm
SRC	Pass	1:34pm
DET	Pass	1:34pm
BAR	Pass	1:34pm
BT	Pass	1:34pm

Blank Tests

Test	Status	Time
AIR	Pass	1:34pm


Printer Tests

Test	Status	Time
PRNT	Pass	1:34pm

CRC Tests

Test	Status	Time
COMP	Pass	1:35pm
CAL	Pass	1:35pm

Preventive Maintenance
Status: Pass


Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County ONslow Instrument Location JACKSONVILLE

Instrument Serial No. 008930 POLICE DEPT

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 28 day of FEBRUARY, 2024 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Alan R. Bane
Signature of Certifying Official

648
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

ONslow COUNTY JACKSONVILLE PD 660

Serial Number: 008930
Test Date: 02/28/2024

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: BARNES, ALVIN R

Permit Number: 0014-6279

Effective:

10/01/2023-10/01/2025

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG225701

Exp Date: 09/14/2024

Test	g/210L	Time
DIAG	Pass	10:06am
AIR BLK	.00	10:07am
ACCY CHK	.08	10:07am
AIR BLK	.00	10:08am
SUB TEST	.00	10:09am
AIR BLK	.00	10:10am
SUB TEST	.00	10:12am
AIR BLK	.00	10:13am

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

ONSLOW COUNTY JACKSONVILLE PD 660

Serial Number: 008930 Test Record Number: 2275
Test Date: 02/28/2024 Test Time: 10:13am EST

System Check: Passed

Baseline Tests

Test	Status	Time
IR	Pass	10:14am
FLO	Pass	10:14am
FC	Pass	10:14am

Temperature Tests

Test	Status	Time
FC1	Pass	10:14am
SRC	Pass	10:14am
DET	Pass	10:14am
BAR	Pass	10:14am
BT	Pass	10:14am

Blank Tests

Test	Status	Time
AIR	Pass	10:14am


Printer Tests

Test	Status	Time
PRNT	Pass	10:14am

CRC Tests

Test	Status	Time
COMP	Pass	10:15am
CAL	Pass	10:15am

Preventive Maintenance
Status: Pass


Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County ONSLOW Instrument Location ONSLOW COUNTY
Instrument Serial No. 008931 DETENTION CENTER

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 21 day of FEBRUARY, 2024 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Ch Rg Burns

Signature of Certifying Official

648

Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

ONSLOW COUNTY DETENTION CENTER 660

Serial Number: 008931
Test Date: 02/21/2024

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE

Analyst's Name: BARNES, ALVIN R
Permit Number: 0014-6279
Effective:
10/01/2023-10/01/2025

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG400301
Exp Date: 01/03/2026

Test	g/210L	Time
DIAG	Pass	3:17pm
AIR BLK	.00	3:18pm
ACCY CHK	.07	3:19pm
AIR BLK	.00	3:20pm
SUB TEST	.00	3:21pm
AIR BLK	.00	3:22pm
SUB TEST	.00	3:23pm
AIR BLK	.00	3:24pm

Reported AC: .00 g/210L

Alvin R Barnes
Signature of Chemical Analyst

Court CVR

Alvin R Barnes
Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

ONslow COUNTY DETENTION CENTER 660

Serial Number: 008931 Test Record Number: 4660
Test Date: 02/21/2024 Test Time: 3:26pm EST

System Check: Passed

Baseline Tests

Test	Status	Time
IR	Pass	3:26pm
FLO	Pass	3:26pm
FC	Pass	3:26pm

Temperature Tests

Test	Status	Time
FC1	Pass	3:26pm
SRC	Pass	3:26pm
DET	Pass	3:26pm
BAR	Pass	3:26pm
BT	Pass	3:26pm

Blank Tests

Test	Status	Time
AIR	Pass	3:27pm


Printer Tests

Test	Status	Time
PRNT	Pass	3:27pm

CRC Tests

Test	Status	Time
COMP	Pass	3:27pm
CAL	Pass	3:27pm

Preventive Maintenance
Status: Pass


Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County ONSLOW Instrument Location ONSLOW COUNTY

Instrument Serial No. 008932 DETENTION CENTER

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 21 day of FEBRUARY, 2024 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Alan R. Banks
Signature of Certifying Official

648
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

ONSLOW COUNTY DETENTION CENTER 660

Serial Number: 008932

Test Date: 02/21/2024

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: BARNES, ALVIN R

Permit Number: 0014-6279

Effective:

10/01/2023-10/01/2025

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG400301

Exp Date: 01/03/2026

Test	g/210L	Time
DIAG	Pass	3:15pm
AIR BLK	.00	3:16pm
ACCY CHK	.08	3:16pm
AIR BLK	.00	3:17pm
SUB TEST	.00	3:18pm
AIR BLK	.00	3:19pm
SUB TEST	.00	3:21pm
AIR BLK	.00	3:21pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

ONslow COUNTY DETENTION CENTER 660

Serial Number: 008932 Test Record Number: 7264
Test Date: 02/21/2024 Test Time: 3:22pm EST

System Check: Passed

Baseline Tests

Test	Status	Time
IR	Pass	3:22pm
FLO	Pass	3:22pm
FC	Pass	3:22pm

Temperature Tests

Test	Status	Time
FC1	Pass	3:22pm
SRC	Pass	3:22pm
DET	Pass	3:22pm
BAR	Pass	3:22pm
BT	Pass	3:22pm

Blank Tests

Test	Status	Time
AIR	Pass	3:23pm


Printer Tests

Test	Status	Time
PRNT	Pass	3:23pm

CRC Tests

Test	Status	Time
COMP	Pass	3:23pm
CAL	Pass	3:23pm

Preventive Maintenance
Status: Pass


Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County ORANGE Instrument Location ORANGE Co. Detention Ctr
Instrument Serial No. 008839 1200 US Hwy 70 West
Hillsborough, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 13 day of February, 2024 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Sam Stokes Barrios

Signature of Certifying Official

662

Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

ORANGE COUNTY DETENTION CENTER 670

Serial Number: 008839

Test Date: 02/13/2024

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Barnes, Simon S

Permit Number: 0014-6221

Effective:

10/01/2023-10/01/2025

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG303102

Exp Date: 01/31/2025

Test	g/210L	Time
DIAG	Pass	1:20pm
AIR BLK	.00	1:21pm
ACCY CHK	.08	1:22pm
AIR BLK	.00	1:23pm
SUB TEST	.00	1:24pm
AIR BLK	.00	1:24pm
SUB TEST	.00	1:26pm
AIR BLK	.00	1:27pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

Intox EC/IR-II: Preventive Maintenance

ORANGE COUNTY DETENTION CENTER 670

Serial Number: 008839

Test Record Number: 2728

Test Date: 02/13/2024

Test Time: 1:27pm EST

System Check: Passed

Baseline Tests

Test	Status	Time
IR	Pass	1:28pm
FLO	Pass	1:28pm
FC	Pass	1:28pm

Temperature Tests

Test	Status	Time
FC1	Pass	1:28pm
SRC	Pass	1:28pm
DET	Pass	1:28pm
BAR	Pass	1:28pm
BT	Pass	1:28pm

Blank Tests

Test	Status	Time
AIR	Pass	1:28pm


Printer Tests

Test	Status	Time
PRNT	Pass	1:28pm

CRC Tests

Test	Status	Time
COMP	Pass	1:29pm
CAL	Pass	1:29pm

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County ORANGE Instrument Location CARRBORO PD
Instrument Serial No. 008924 100 N. GREENSBORO ST
CARRBORO, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 8 day of February, 2024 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Simon Adams Brown
Signature of Certifying Official

642
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

ORANGE COUNTY CARRBORO PD 670

Serial Number: 008924

Test Date: 02/08/2024

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Barnes, Simon S

Permit Number: 0014-6221

Effective:

10/01/2023-10/01/2025

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG308004


Exp Date: 03/21/2025

Test	g/210L	Time
DIAG	Pass	6:47pm
AIR BLK	.00	6:47pm
ACCY CHK	.08	6:48pm
AIR BLK	.00	6:49pm
SUB TEST	.00	6:50pm
AIR BLK	.00	6:51pm
SUB TEST	.00	6:52pm
AIR BLK	.00	6:53pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

Intox EC/IR-II: Preventive Maintenance

ORANGE COUNTY CARRBORO PD 670

Serial Number: 008924 Test Record Number: 1883
Test Date: 02/08/2024 Test Time: 6:54pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	6:54pm
FLO	Pass	6:54pm
FC	Pass	6:54pm

Temperature Tests

Test	Status	Time
FC1	Pass	6:54pm
SRC	Pass	6:54pm
DET	Pass	6:54pm
BAR	Pass	6:54pm
BT	Pass	6:54pm

Blank Tests

Test	Status	Time
AIR	Pass	6:55pm

Printer Tests

Test	Status	Time
PRNT	Pass	6:55pm

CRC Tests

Test	Status	Time
COMP	Pass	6:55pm
CAL	Pass	6:55pm

Preventive Maintenance
Status: *Pass*


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County ORANGE Instrument Location Caribou PD
Instrument Serial No. 008845 100 N. Greenbriar ST
Caribou, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 12 day of February, 2024 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Simon Stokes Barnes
Signature of Certifying Official

662
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

ORANGE COUNTY CARRBORO PD 670

Serial Number: 008945

Test Date: 02/12/2024

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Barnes, Simon S

Permit Number: 0014-6221

Effective:

10/01/2023-10/01/2025

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG308004

Exp Date: 03/21/2025

Test	g/210L	Time
DIAG	Pass	7:20am
AIR BLK	.00	7:20am
ACCY CHK	.08	7:21am
AIR BLK	.00	7:22am
SUB TEST	.00	7:23am
AIR BLK	.00	7:23am
SUB TEST	.00	7:25am
AIR BLK	.00	7:26am

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

ORANGE COUNTY CARRBORO PD 670

Serial Number: 008945 Test Record Number: 760
Test Date: 02/12/2024 Test Time: 7:29am EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	7:29am
FLO	Pass	7:29am
FC	Pass	7:29am

Temperature Tests

Test	Status	Time
FC1	Pass	7:30am
SRC	Pass	7:30am
DET	Pass	7:30am
BAR	Pass	7:30am
BT	Pass	7:30am

Blank Tests

Test	Status	Time
AIR	Pass	7:30am

Printer Tests

Test	Status	Time
PRNT	Pass	7:30am

CRC Tests

Test	Status	Time
COMP	Pass	7:30am
CAL	Pass	7:30am

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Pasquotank Instrument Location Elizabeth City P.D.
Instrument Serial No. 008941 315 Main St. Elizabeth City,
NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 9th day of February, 2024 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Mat A. [Signature]
Signature of Certifying Official

680
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

PASQUOTANK COUNTY ELIZABETH CITY 690

Serial Number: 008941

Test Date: 02/09/2024

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Chappell, Mark A

Permit Number: 0020-6272

Effective:

10/01/2023-10/01/2025

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG212403

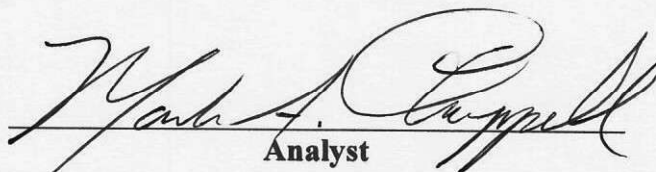
Exp Date: 05/04/2024

Test	g/210L	Time
DIAG	Pass	10:49am
AIR BLK	.00	10:49am
ACCY CHK	.07	10:50am
AIR BLK	.00	10:51am
SUB TEST	.00	10:52am
AIR BLK	.00	10:53am
SUB TEST	.00	10:55am
AIR BLK	.00	10:55am

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

PASQUOTANK COUNTY ELIZABETH CITY 690

Serial Number: 008941 Test Record Number: 1648
Test Date: 02/09/2024 Test Time: 10:57am EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	10:57am
FLO	Pass	10:57am
FC	Pass	10:57am

Temperature Tests

Test	Status	Time
FC1	Pass	10:57am
SRC	Pass	10:57am
DET	Pass	10:57am
BAR	Pass	10:57am
BT	Pass	10:57am

Blank Tests

Test	Status	Time
AIR	Pass	10:58am

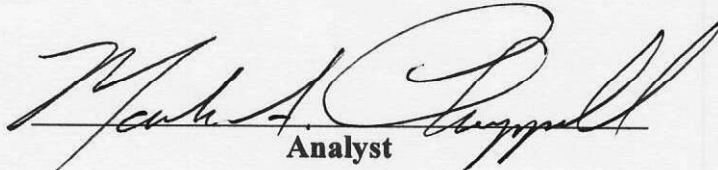
Printer Tests

Test	Status	Time
PRNT	Pass	10:58am

CRC Tests

Test	Status	Time
COMP	Pass	10:58am
CAL	Pass	10:58am

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Pasquotank Instrument Location Pasquotank Co. Public Safety Bldg
200 E Colonial Ave.
Elizabeth City, NC

Instrument Serial No. 008950

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 8th day of February, 2024 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

680

Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

PASQUOTANK COUNTY PUBLIC SAFETY BLDG
690

Serial Number: 008950
Test Date: 02/08/2024

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE

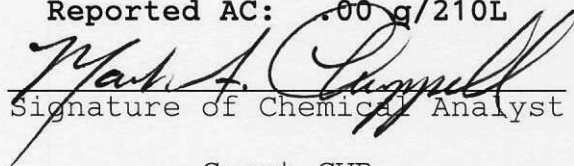
Analyst's Name: Chappell, Mark A
Permit Number: 0020-6272
Effective:
10/01/2023-10/01/2025

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

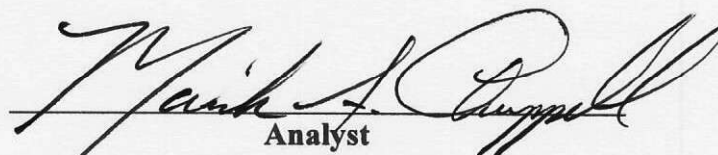
Lot Number: AG308003
Exp Date: 03/21/2025

Test	g/210L	Time
DIAG	Pass	10:20am
AIR BLK	.00	10:21am
ACCY CHK	.07	10:22am
AIR BLK	.00	10:23am
SUB TEST	.00	10:23am
AIR BLK	.00	10:24am
SUB TEST	.00	10:26am
AIR BLK	.00	10:27am

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

PASQUOTANK COUNTY PUBLIC SAFETY BLDG 690

Serial Number: 008950 Test Record Number: 2100
Test Date: 02/08/2024 Test Time: 10:28am EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	10:28am
FLO	Pass	10:28am
FC	Pass	10:28am

Temperature Tests

Test	Status	Time
FC1	Pass	10:28am
SRC	Pass	10:28am
DET	Pass	10:28am
BAR	Pass	10:28am
BT	Pass	10:28am

Blank Tests

Test	Status	Time
AIR	Pass	10:29am

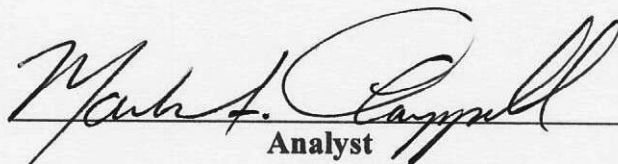
Printer Tests

Test	Status	Time
PRNT	Pass	10:29am

CRC Tests

Test	Status	Time
COMP	Pass	10:29am
CAL	Pass	10:29am

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County PENDER Instrument Location PENDER COUNTY

Instrument Serial No. 008935 DETENTION CENTER

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 20 day of FEBRUARY, 2024 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Alan R. B...
Signature of Certifying Official

648
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

PENDER COUNTY DETENTION CENTER 700

Serial Number: 008935

Test Date: 02/20/2024

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: BARNES, ALVIN R

Permit Number: 0014-6279

Effective:

10/01/2023-10/01/2025

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG400301

Exp Date: 01/03/2026

Test	g/210L	Time
DIAG	Pass	11:08am
AIR BLK	.00	11:09am
ACCY CHK	.07	11:10am
AIR BLK	.00	11:11am
SUB TEST	.00	11:12am
AIR BLK	.00	11:13am
SUB TEST	.00	11:15am
AIR BLK	.00	11:15am

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

PENDER COUNTY DETENTION CENTER 700

Serial Number: 008935 Test Record Number: 3422
Test Date: 02/20/2024 Test Time: 11:16am EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	11:16am
FLO	Pass	11:16am
FC	Pass	11:16am

Temperature Tests

Test	Status	Time
FC1	Pass	11:17am
SRC	Pass	11:17am
DET	Pass	11:17am
BAR	Pass	11:17am
BT	Pass	11:17am

Blank Tests

Test	Status	Time
AIR	Pass	11:17am


Printer Tests

Test	Status	Time
PRNT	Pass	11:17am

CRC Tests

Test	Status	Time
COMP	Pass	11:17am
CAL	Pass	11:17am

Preventive Maintenance
Status: Pass


Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Person Instrument Location Person 6 LEC

Instrument Serial No. 008924 120 Court St Roxboro, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 22 day of February, 2024 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Simon Stokes Barnes
Signature of Certifying Official

662
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

PERSON COUNTY PERSON COUNTY LEC 720

Serial Number: 008924

Test Date: 02/22/2024

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Barnes, Simon S

Permit Number: 0014-6221

Effective:

10/01/2023-10/01/2025

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG400301

Exp Date: 01/03/2026

Test	g/210L	Time
DIAG	Pass	9:23am
AIR BLK	.00	9:24am
ACCY CHK	.08	9:25am
AIR BLK	.00	9:26am
SUB TEST	.00	9:27am
AIR BLK	.00	9:28am
SUB TEST	.00	9:29am
AIR BLK	.00	9:30am

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

This form is used when performing Preventive Maintenance procedures

Forensic Tests for Alcohol Branch

Department of Health and Human Services

Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

PERSON COUNTY PERSON COUNTY LEC 720

Serial Number: 008924 Test Record Number: 1907
Test Date: 02/22/2024 Test Time: 9:30am EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	9:31am
FLO	Pass	9:31am
FC	Pass	9:31am

Temperature Tests

Test	Status	Time
FC1	Pass	9:31am
SRC	Pass	9:31am
DET	Pass	9:31am
BAR	Pass	9:31am
BT	Pass	9:31am

Blank Tests

Test	Status	Time
AIR	Pass	9:32am

Printer Tests

Test	Status	Time
PRNT	Pass	9:32am

CRC Tests

Test	Status	Time
COMP	Pass	9:32am
CAL	Pass	9:32am

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Pitt Instrument Location Pitt Co. Detention Center
Instrument Serial No. 008668 124 New Hope Rd, Greenville
NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 21st day of February, 2024 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Thy D. Ay
Signature of Certifying Official

643
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

PITT COUNTY PITT CO DETENTION 730

Serial Number: 008668
Test Date: 02/21/2024

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Gray, Kelly D

Permit Number: 0037-7722

Effective:

10/01/2023-10/01/2025

Officer's Name: NONE, NONE

Type of Agency: FTA


Agency: DHHS

Test Type: Breath Test


Lot Number: AG400303
Exp Date: 01/03/2026

Test	g/210L	Time
DIAG	Pass	9:44am
AIR BLK	.00	9:45am
ACCY CHK	.08	9:46am
AIR BLK	.00	9:47am
SUB TEST	.00	9:48am
AIR BLK	.00	9:48am
SUB TEST	.00	9:50am
AIR BLK	.00	9:51am

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

PITT COUNTY PITT CO DETENTION 730

Serial Number: 008668 Test Record Number: 4637
Test Date: 02/21/2024 Test Time: 9:53am EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	9:54am
FLO	Pass	9:54am
FC	Pass	9:54am

Temperature Tests

Test	Status	Time
FC1	Pass	9:54am
SRC	Pass	9:54am
DET	Pass	9:54am
BAR	Pass	9:54am
BT	Pass	9:54am

Blank Tests

Test	Status	Time
AIR	Pass	9:54am


Printer Tests

Test	Status	Time
PRNT	Pass	9:55am

CRC Tests

Test	Status	Time
COMP	Pass	9:55am
CAL	Pass	9:55am

Preventive Maintenance
Status: Pass



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County Polk Instrument Location Polk County Jail
Instrument Serial No. 008832 Columbus, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 8 day of February, 2024 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

668
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

POLK COUNTY POLK COUNTY JAIL 740

Serial Number: 008832

Test Date: 02/08/2024

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Loftis, Benjamin C

Permit Number: 0024-4987

Effective:

10/01/2023-10/01/2025

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

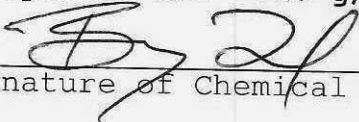
Test Type: Breath Test

Lot Number: AG308704

Exp Date: 03/28/2025

Test	g/210L	Time
DIAG	Pass	10:58am
AIR BLK	.00	10:59am
ACCY CHK	.08	11:00am
AIR BLK	.00	11:01am
SUB TEST	.00	11:01am
AIR BLK	.00	11:02am
SUB TEST	.00	11:04am
AIR BLK	.00	11:05am

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

This form is used when performing Preventive Maintenance procedures

Forensic Tests for Alcohol Branch

Department of Health and Human Services

Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

POLK COUNTY POLK COUNTY JAIL 740

Serial Number: 008832 Test Record Number: 1846
Test Date: 02/08/2024 Test Time: 11:05am EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	11:05am
FLO	Pass	11:05am
FC	Pass	11:05am

Temperature Tests

Test	Status	Time
FC1	Pass	11:06am
SRC	Pass	11:06am
DET	Pass	11:06am
BAR	Pass	11:06am
BT	Pass	11:06am

Blank Tests

Test	Status	Time
AIR	Pass	11:06am

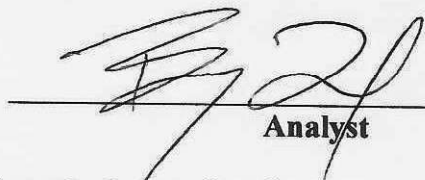
Printer Tests

Test	Status	Time
PRNT	Pass	11:06am

CRC Tests

Test	Status	Time
COMP	Pass	11:06am
CAL	Pass	11:06am

Preventive Maintenance
Status: Pass


Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Polk Instrument Location Polk County Jail
Instrument Serial No. 008881 Columbus, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 8 day of February, 2024 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

6608
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

POLK COUNTY POLK COUNTY JAIL 740

Serial Number: 008881

Test Date: 02/08/2024

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Loftis, Benjamin C

Permit Number: 0024-4987

Effective:

10/01/2023-10/01/2025

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG308704

Exp Date: 03/28/2025

Test	g/210L	Time
DIAG	Pass	10:59am
AIR BLK	.00	11:00am
ACCY CHK	.08	11:01am
AIR BLK	.00	11:02am
SUB TEST	.00	11:02am
AIR BLK	.00	11:03am
SUB TEST	.00	11:05am
AIR BLK	.00	11:06am

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

POLK COUNTY POLK COUNTY JAIL 740

Serial Number: 008881 Test Record Number: 1168
Test Date: 02/08/2024 Test Time: 11:06am EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	11:06am
FLO	Pass	11:06am
FC	Pass	11:06am

Temperature Tests

Test	Status	Time
FC1	Pass	11:06am
SRC	Pass	11:06am
DET	Pass	11:06am
BAR	Pass	11:06am
BT	Pass	11:06am

Blank Tests

Test	Status	Time
AIR	Pass	11:07am

Printer Tests

Test	Status	Time
PRNT	Pass	11:07am

CRC Tests

Test	Status	Time
COMP	Pass	11:07am
CAL	Pass	11:07am

Preventive Maintenance
Status: Pass


Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH


PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County RANDOLPH Instrument Location LIBERTY POLICE
Instrument Serial No. 008830 DEPARTMENT

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 2 day of FEBRUARY, 2024 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

667
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

RANDOLPH COUNTY LIBERTY PD 750

Serial Number: 008830

Test Date: 02/02/2024

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Galloway, Charles L

Permit Number: 0023-9771

Effective:

10/01/2023-10/01/2025

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG308703

Exp Date: 03/28/2025

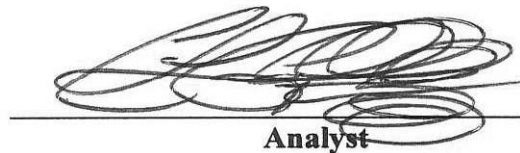
Test	g/210L	Time
DIAG	Pass	10:35am
AIR BLK	.00	10:35am
ACCY CHK	.08	10:36am
AIR BLK	.00	10:37am
SUB TEST	.00	10:38am
AIR BLK	.00	10:39am
SUB TEST	.00	10:41am
AIR BLK	.00	10:42am

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

Intox EC/IR-II: Preventive Maintenance

RANDOLPH COUNTY LIBERTY PD 750

Serial Number: 008830 Test Record Number: 842
Test Date: 02/02/2024 Test Time: 10:43am EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	10:43am
FLO	Pass	10:43am
FC	Pass	10:43am

Temperature Tests

Test	Status	Time
FC1	Pass	10:43am
SRC	Pass	10:43am
DET	Pass	10:43am
BAR	Pass	10:43am
BT	Pass	10:43am

Blank Tests

Test	Status	Time
AIR	Pass	10:44am

Printer Tests

Test	Status	Time
PRNT	Pass	10:44am

CRC Tests

Test	Status	Time
COMP	Pass	10:44am
CAL	Pass	10:44am

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH


PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County RICHMOND Instrument Location RICHMOND COUNTY
Instrument Serial No. 008701 MAGISTRATE'S OFFICE

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 8 day of FEBRUARY, 2024 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Signature of Certifying Official

Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

RICHMOND COUNTY MAGISTRATE'S OFFICE
760

Serial Number: 008701
Test Date: 02/08/2024

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Galloway, Charles L

Permit Number: 0023-9771

Effective:

10/01/2023-10/01/2025

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

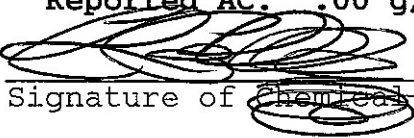
Test Type: Breath Test

Lot Number: AG308003

Exp Date: 03/21/2025

Test	g/210L	Time
DIAG	Pass	12:01pm
AIR BLK	.00	12:02pm
ACCY CHK	.07	12:03pm
AIR BLK	.00	12:04pm
SUB TEST	.00	12:04pm
AIR BLK	.00	12:05pm
SUB TEST	.00	12:06pm
AIR BLK	.00	12:07pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

RICHMOND COUNTY MAGISTRATE'S OFFICE 760

Serial Number: 008701 Test Record Number: 1428
Test Date: 02/08/2024 Test Time: 12:08pm EST

System Check: Passed

Baseline Tests

Test	Status	Time
IR	Pass	12:08pm
FLO	Pass	12:08pm
FC	Pass	12:08pm

Temperature Tests

Test	Status	Time
FC1	Pass	12:09pm
SRC	Pass	12:09pm
DET	Pass	12:09pm
BAR	Pass	12:09pm
BT	Pass	12:09pm

Blank Tests

Test	Status	Time
AIR	Pass	12:09pm

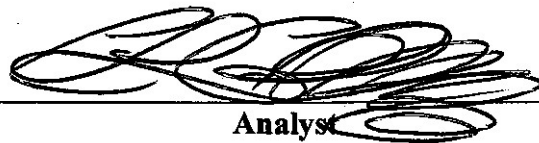
Printer Tests

Test	Status	Time
PRNT	Pass	12:09pm

CRC Tests

Test	Status	Time
COMP	Pass	12:09pm
CAL	Pass	12:09pm

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH


PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

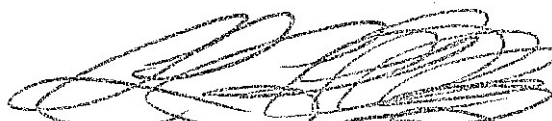
County RICHMOND Instrument Location RICHMOND COUNTY
Instrument Serial No. 008840 MAGISTRATE'S OFFICE

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 8 day of FEBRUARY, 2024 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.




Signature of Certifying Official

667
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

RICHMOND COUNTY MAGISTRATE'S OFFICE
760

Serial Number: 008840

Test Date: 02/08/2024

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Galloway, Charles L

Permit Number: 0023-9771

Effective:

10/01/2023-10/01/2025

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG308003

Exp Date: 03/21/2025

Test	g/210L	Time
DIAG	Pass	11:57am
AIR BLK	.00	11:57am
ACCY CHK	.07	11:58am
AIR BLK	.00	11:59am
SUB TEST	.00	12:01pm
AIR BLK	.00	12:02pm
SUB TEST	.00	12:04pm
AIR BLK	.00	12:05pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

Intox EC/IR-II: Preventive Maintenance

RICHMOND COUNTY MAGISTRATE'S OFFICE 760

Serial Number: 008840 Test Record Number: 3013
Test Date: 02/08/2024 Test Time: 12:07pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	12:07pm
FLO	Pass	12:07pm
FC	Pass	12:07pm

Temperature Tests

Test	Status	Time
FC1	Pass	12:08pm
SRC	Pass	12:08pm
DET	Pass	12:08pm
BAR	Pass	12:08pm
BT	Pass	12:08pm

Blank Tests

Test	Status	Time
AIR	Pass	12:08pm

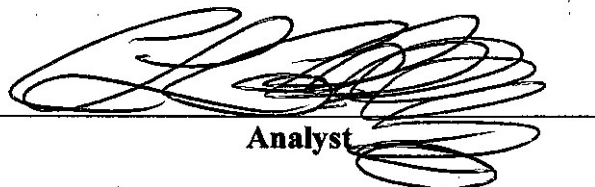
Printer Tests

Test	Status	Time
PRNT	Pass	12:08pm

CRC Tests

Test	Status	Time
COMP	Pass	12:08pm
CAL	Pass	12:08pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Robeson Instrument Location BAT Mobile Unit 5
Instrument Serial No. 00 8575 Robeson County SO

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 21st day of February, 2024 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

684
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

ROBESON COUNTY BAT MOBILE UNIT 5 770

Serial Number: 008575

Test Date: 02/21/2024

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Sharpe Jr., Robert J

Permit Number: 1820-8591

Effective:

10/01/2023-10/01/2025

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG308101

Exp Date: 03/22/2025

Test	g/210L	Time
DIAG	Pass	1:22pm
AIR BLK	.00	1:23pm
ACCY CHK	.08	1:24pm
AIR BLK	.00	1:25pm
SUB TEST	.00	1:26pm
AIR BLK	.00	1:26pm
SUB TEST	.00	1:28pm
AIR BLK	.00	1:29pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

ROBESON COUNTY BAT MOBILE UNIT 5 770

Serial Number: 008575 Test Record Number: 1430
Test Date: 02/21/2024 Test Time: 1:30pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	1:30pm
FLO	Pass	1:30pm
FC	Pass	1:30pm

Temperature Tests

Test	Status	Time
FC1	Pass	1:30pm
SRC	Pass	1:30pm
DET	Pass	1:30pm
BAR	Pass	1:30pm
BT	Pass	1:30pm

Blank Tests

Test	Status	Time
AIR	Pass	1:31pm

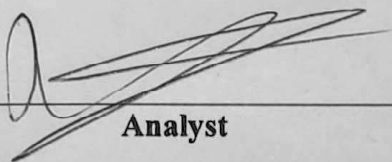
Printer Tests

Test	Status	Time
PRNT	Pass	1:31pm

CRC Tests

Test	Status	Time
COMP	Pass	1:31pm
CAL	Pass	1:31pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Robeson Instrument Location BAT Mobile Unit 5
Instrument Serial No. 00 8575 Lumberton PD

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 22nd day of February, 2024 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

684
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

ROBESON COUNTY BAT MOBILE UNIT 5 770

Serial Number: 008575

Test Date: 02/22/2024

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Sharpe Jr., Robert J

Permit Number: 1820-8591

Effective:

10/01/2023-10/01/2025

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG308101

Exp Date: 03/22/2025

Test	g/210L	Time
DIAG	Pass	9:09pm
AIR BLK	.00	9:10pm
ACCY CHK	.08	9:10pm
AIR BLK	.00	9:11pm
SUB TEST	.00	9:12pm
AIR BLK	.00	9:13pm
SUB TEST	.00	9:14pm
AIR BLK	.00	9:15pm

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

ROBESON COUNTY BAT MOBILE UNIT 5 770

Serial Number: 008575 Test Record Number: 1432
Test Date: 02/22/2024 Test Time: 9:16pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	9:16pm
FLO	Pass	9:16pm
FC	Pass	9:16pm

Temperature Tests

Test	Status	Time
FC1	Pass	9:16pm
SRC	Pass	9:16pm
DET	Pass	9:16pm
BAR	Pass	9:16pm
BT	Pass	9:16pm

Blank Tests

Test	Status	Time
AIR	Pass	9:17pm

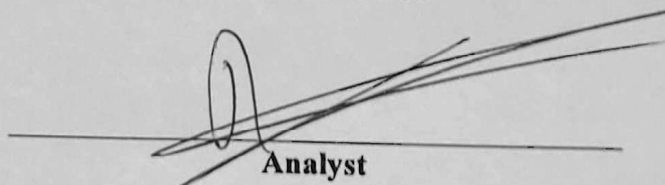
Printer Tests

Test	Status	Time
PRNT	Pass	9:17pm

CRC Tests

Test	Status	Time
COMP	Pass	9:17pm
CAL	Pass	9:17pm

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Robeson Instrument Location BAT Mobile Unit 5
Instrument Serial No. 008616 Robeson County SO

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 9th day of February, 2024 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

684
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

ROBESON COUNTY BAT MOBILE UNIT 5 770

Serial Number: 008616

Test Date: 02/09/2024

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Sharpe Jr., Robert J

Permit Number: 1820-8591

Effective:

10/01/2023-10/01/2025

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

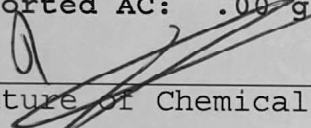
Test Type: Breath Test

Lot Number: AG308101

Exp Date: 03/22/2025

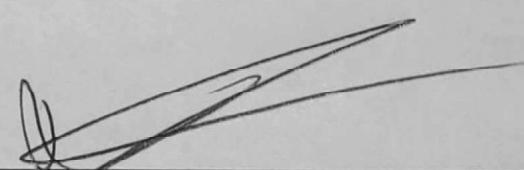
Test	g/210L	Time
DIAG	Pass	8:39pm
AIR BLK	.00	8:40pm
ACCY CHK	.08	8:41pm
AIR BLK	.00	8:42pm
SUB TEST	.00	8:42pm
AIR BLK	.00	8:44pm
SUB TEST	.00	8:45pm
AIR BLK	.00	8:46pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

ROBESON COUNTY BAT MOBILE UNIT 5 770

Serial Number: 008616 Test Record Number: 2822
Test Date: 02/09/2024 Test Time: 8:47pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	8:47pm
FLO	Pass	8:47pm
FC	Pass	8:47pm

Temperature Tests

Test	Status	Time
FC1	Pass	8:47pm
SRC	Pass	8:47pm
DET	Pass	8:47pm
BAR	Pass	8:47pm
BT	Pass	8:47pm

Blank Tests

Test	Status	Time
AIR	Pass	8:48pm

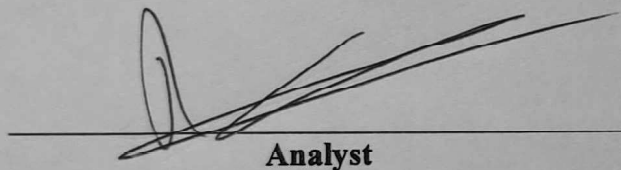
Printer Tests

Test	Status	Time
PRNT	Pass	8:48pm

CRC Tests

Test	Status	Time
COMP	Pass	8:48pm
CAL	Pass	8:48pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Robeson Instrument Location BAT Mobile Unit 5
Instrument Serial No. 00 8616 Lumberton PD

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 15th day of February, 2024 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.




Signature of Certifying Official

684
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

ROBESON COUNTY BAT MOBILE UNIT 5 770

Serial Number: 008616

Test Date: 02/15/2024

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Sharpe Jr., Robert J

Permit Number: 1820-8591

Effective:

10/01/2023-10/01/2025

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG308101

Exp Date: 03/22/2025

Test	g/210L	Time
DIAG	Pass	8:08pm
AIR BLK	.00	8:09pm
ACCY CHK	.08	8:10pm
AIR BLK	.00	8:11pm
SUB TEST	.00	8:11pm
AIR BLK	.00	8:12pm
SUB TEST	.00	8:14pm
AIR BLK	.00	8:15pm

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR

Analyst

This form is used when performing Preventive Maintenance procedures

Forensic Tests for Alcohol Branch

Department of Health and Human Services

Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

ROBESON COUNTY BAT MOBILE UNIT 5 770

Serial Number: 008616 Test Record Number: 2824
Test Date: 02/15/2024 Test Time: 8:16pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	8:16pm
FLO	Pass	8:16pm
FC	Pass	8:16pm

Temperature Tests

Test	Status	Time
FC1	Pass	8:16pm
SRC	Pass	8:16pm
DET	Pass	8:16pm
BAR	Pass	8:16pm
BT	Pass	8:16pm

Blank Tests

Test	Status	Time
AIR	Pass	8:17pm

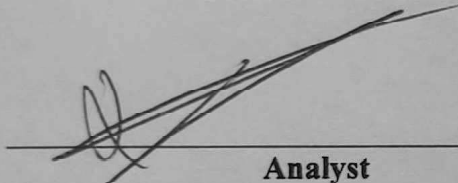
Printer Tests

Test	Status	Time
PRNT	Pass	8:17pm

CRC Tests

Test	Status	Time
COMP	Pass	8:17pm
CAL	Pass	8:17pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Robeson Instrument Location BAT Mobile Unit 5
Instrument Serial No. 008647 St. Pauls PD

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 3rd day of February, 2024 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

684

Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

ROBESON COUNTY BAT MOBILE UNIT 5 770

Serial Number: 008647

Test Date: 02/03/2024

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Sharpe Jr., Robert J

Permit Number: 1820-8591

Effective:

10/01/2023-10/01/2025

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

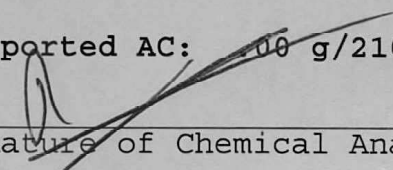
Test Type: Breath Test

Lot Number: AG308101

Exp Date: 03/22/2025

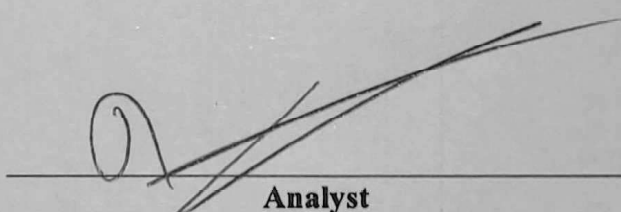
Test	g/210L	Time
DIAG	Pass	7:43pm
AIR BLK	.00	7:44pm
ACCY CHK	.08	7:45pm
AIR BLK	.00	7:45pm
SUB TEST	.00	7:46pm
AIR BLK	.00	7:47pm
SUB TEST	.00	7:49pm
AIR BLK	.00	7:49pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

Intox EC/IR-II: Preventive Maintenance

ROBESON COUNTY BAT MOBILE UNIT 5 770
Serial Number: 008647 Test Record Number: 2817
Test Date: 02/03/2024 Test Time: 7:51pm EST
System Check: Passed

Baseline Tests

Test	Status	Time
IR	Pass	7:51pm
FLO	Pass	7:51pm
FC	Pass	7:51pm

Temperature Tests

Test	Status	Time
FC1	Pass	7:51pm
SRC	Pass	7:51pm
DET	Pass	7:51pm
BAR	Pass	7:51pm
BT	Pass	7:51pm

Blank Tests

Test	Status	Time
AIR	Pass	7:52pm

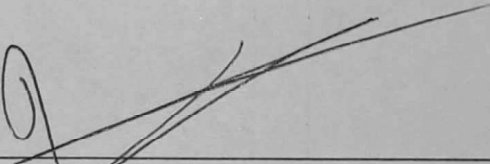
Printer Tests

Test	Status	Time
PRNT	Pass	7:52pm

CRC Tests

Test	Status	Time
COMP	Pass	7:52pm
CAL	Pass	7:52pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Robeson Instrument Location BAT Mobile Unit 5
Instrument Serial No. 008647 Fairmont PD

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 16th day of February, 2024 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

684
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

ROBESON COUNTY BAT MOBILE UNIT 5 770

Serial Number: 008647

Test Date: 02/16/2024

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Sharpe Jr., Robert J

Permit Number: 1820-8591

Effective:

10/01/2023-10/01/2025

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG308101

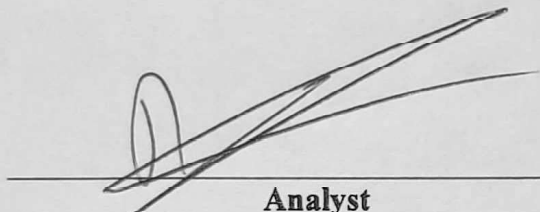
Exp Date: 03/22/2025

Test	g/210L	Time
DIAG	Pass	7:25pm
AIR BLK	.00	7:26pm
ACCY CHK	.08	7:26pm
AIR BLK	.00	7:27pm
SUB TEST	.00	7:28pm
AIR BLK	.00	7:29pm
SUB TEST	.00	7:30pm
AIR BLK	.00	7:31pm

Reported AC: ~~.00 g/210L~~


Signature of Chemical Analyst

Court CVR


Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

ROBESON COUNTY BAT MOBILE UNIT 5 770
Serial Number: 008647 Test Record Number: 2819
Test Date: 02/16/2024 Test Time: 7:33pm EST
System Check: Passed

Baseline Tests

Test	Status	Time
IR	Pass	7:33pm
FLO	Pass	7:33pm
FC	Pass	7:33pm

Temperature Tests

Test	Status	Time
FC1	Pass	7:33pm
SRC	Pass	7:33pm
DET	Pass	7:33pm
BAR	Pass	7:33pm
BT	Pass	7:33pm

Blank Tests

Test	Status	Time
AIR	Pass	7:34pm


Printer Tests

Test	Status	Time
PRNT	Pass	7:34pm

CRC Tests

Test	Status	Time
COMP	Pass	7:34pm
CAL	Pass	7:34pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Robeson Instrument Location BAT Mobile Unit 5
Instrument Serial No. 008647 Lumberton PD

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 29th day of February, 2024 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

684
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

ROBESON COUNTY BAT MOBILE UNIT 5 770

Serial Number: 008647

Test Date: 02/29/2024

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Sharpe Jr., Robert J

Permit Number: 1820-8591

Effective:

10/01/2023-10/01/2025

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG308101

Exp Date: 03/22/2025

Test	g/210L	Time
DIAG	Pass	9:10pm
AIR BLK	.00	9:11pm
ACCY CHK	.08	9:12pm
AIR BLK	.00	9:13pm
SUB TEST	.00	9:13pm
AIR BLK	.00	9:14pm
SUB TEST	.00	9:16pm
AIR BLK	.00	9:17pm

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR

Analyst

Intox EC/IR-II: Preventive Maintenance

ROBESON COUNTY BAT MOBILE UNIT 5 770
Serial Number: 008647 Test Record Number: 2825
Test Date: 02/29/2024 Test Time: 9:17pm EST
System Check: Passed

Baseline Tests

Test	Status	Time
IR	Pass	9:18pm
FLO	Pass	9:18pm
FC	Pass	9:18pm

Temperature Tests

Test	Status	Time
FC1	Pass	9:18pm
SRC	Pass	9:18pm
DET	Pass	9:18pm
BAR	Pass	9:18pm
BT	Pass	9:18pm

Blank Tests

Test	Status	Time
AIR	Pass	9:19pm

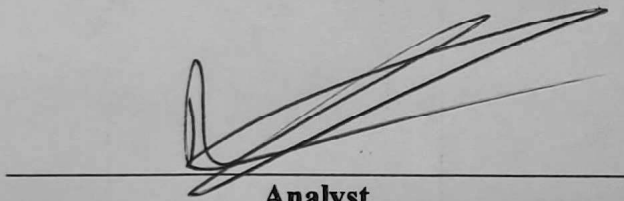
Printer Tests

Test	Status	Time
PRNT	Pass	9:19pm

CRC Tests

Test	Status	Time
COMP	Pass	9:19pm
CAL	Pass	9:19pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Robeson Instrument Location BAT Mobile Unit 5
Instrument Serial No. 008704 Robeson County SO

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 9th day of February, 2024 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

684
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

ROBESON COUNTY BAT MOBILE UNIT 5 770

Serial Number: 008704

Test Date: 02/09/2024

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Sharpe Jr., Robert J

Permit Number: 1820-8591

Effective:

10/01/2023-10/01/2025

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

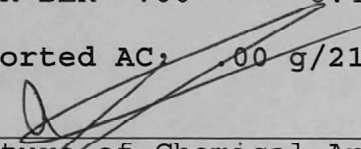
Test Type: Breath Test

Lot Number: AG308101

Exp Date: 03/22/2025

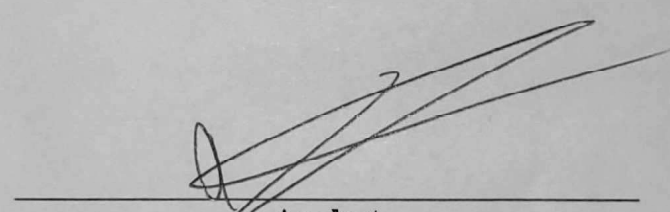
Test	g/210L	Time
DIAG	Pass	8:41pm
AIR BLK	.00	8:42pm
ACCY CHK	.08	8:43pm
AIR BLK	.00	8:44pm
SUB TEST	.00	8:44pm
AIR BLK	.00	8:45pm
SUB TEST	.00	8:47pm
AIR BLK	.00	8:48pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

This form is used when performing Preventive Maintenance procedures

Forensic Tests for Alcohol Branch

Department of Health and Human Services

Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

ROBESON COUNTY BAT MOBILE UNIT 5 770

Serial Number: 008704 Test Record Number: 862
Test Date: 02/09/2024 Test Time: 8:48pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	8:48pm
FLO	Pass	8:48pm
FC	Pass	8:49pm

Temperature Tests

Test	Status	Time
FC1	Pass	8:49pm
SRC	Pass	8:49pm
DET	Pass	8:49pm
BAR	Pass	8:49pm
BT	Pass	8:49pm

Blank Tests

Test	Status	Time
AIR	Pass	8:49pm

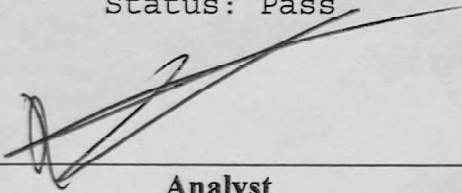
Printer Tests

Test	Status	Time
PRNT	Pass	8:49pm

CRC Tests

Test	Status	Time
COMP	Pass	8:49pm
CAL	Pass	8:49pm

Preventive Maintenance
Status: *Pass*



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Robeson Instrument Location BAT Mobile Units
Instrument Serial No. 008704 Robeson County SO

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 21st day of February, 2024 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.





Signature of Certifying Official

684

Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

ROBESON COUNTY BAT MOBILE UNIT 5 770

Serial Number: 008704

Test Date: 02/21/2024

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Sharpe Jr., Robert J

Permit Number: 1820-8591

Effective:

10/01/2023-10/01/2025

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG308101

Exp Date: 03/22/2025

Test	g/210L	Time
DIAG	Pass	1:24pm
AIR BLK	.00	1:25pm
ACCY CHK	.08	1:25pm
AIR BLK	.00	1:26pm
SUB TEST	.00	1:27pm
AIR BLK	.00	1:28pm
SUB TEST	.00	1:29pm
AIR BLK	.00	1:31pm

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR

Analyst

Intox EC/IR-II: Preventive Maintenance

ROBESON COUNTY BAT MOBILE UNIT 5 770

Serial Number: 008704 Test Record Number: 864
Test Date: 02/21/2024 Test Time: 1:32pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	1:32pm
FLO	Pass	1:32pm
FC	Pass	1:32pm

Temperature Tests

Test	Status	Time
FC1	Pass	1:32pm
SRC	Pass	1:32pm
DET	Pass	1:32pm
BAR	Pass	1:32pm
BT	Pass	1:32pm

Blank Tests

Test	Status	Time
AIR	Pass	1:33pm

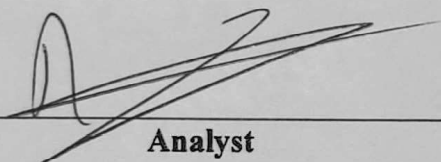
Printer Tests

Test	Status	Time
PRNT	Pass	1:33pm

CRC Tests

Test	Status	Time
COMP	Pass	1:33pm
CAL	Pass	1:33pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Robeson Instrument Location BAT Mobile Unit 5
Instrument Serial No. 008704 Lumberton PD

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 22nd day of February, 2024 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

684
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

ROBESON COUNTY BAT MOBILE UNIT 5 770

Serial Number: 008704

Test Date: 02/22/2024

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Sharpe Jr., Robert J

Permit Number: 1820-8591

Effective:

10/01/2023-10/01/2025

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG308101

Exp Date: 03/22/2025

Test	g/210L	Time
DIAG	Pass	9:06pm
AIR BLK	.00	9:07pm
ACCY CHK	.08	9:08pm
AIR BLK	.00	9:09pm
SUB TEST	.00	9:10pm
AIR BLK	.00	9:11pm
SUB TEST	.00	9:12pm
AIR BLK	.00	9:13pm

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

ROBESON COUNTY BAT MOBILE UNIT 5 770

Serial Number: 008704 Test Record Number: 866
Test Date: 02/22/2024 Test Time: 9:14pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	9:15pm
FLO	Pass	9:15pm
FC	Pass	9:15pm

Temperature Tests

Test	Status	Time
FC1	Pass	9:15pm
SRC	Pass	9:15pm
DET	Pass	9:15pm
BAR	Pass	9:15pm
BT	Pass	9:15pm

Blank Tests

Test	Status	Time
AIR	Pass	9:16pm

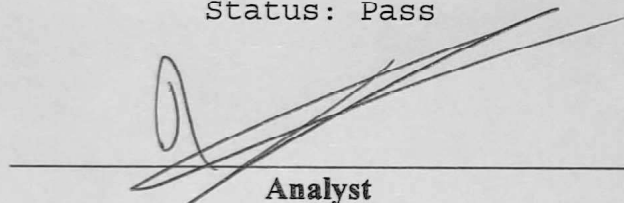
Printer Tests

Test	Status	Time
PRNT	Pass	9:16pm

CRC Tests

Test	Status	Time
COMP	Pass	9:16pm
CAL	Pass	9:16pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

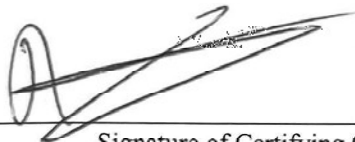
County Robeson Instrument Location BAT Mobile Unit 5
Instrument Serial No. 008707 Lumberton PD

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 15th day of February, 2024 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.





Signature of Certifying Official

Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

ROBESON COUNTY BAT MOBILE UNIT 5 770

Serial Number: 008707

Test Date: 02/15/2024

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Sharpe Jr., Robert J

Permit Number: 1820-8591

Effective:

10/01/2023-10/01/2025

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG308704

Exp Date: 03/28/2025

Test	g/210L	Time
DIAG	Pass	8:10pm
AIR BLK	.00	8:11pm
ACCY CHK	.07	8:11pm
AIR BLK	.00	8:12pm
SUB TEST	.00	8:13pm
AIR BLK	.00	8:14pm
SUB TEST	.00	8:15pm
AIR BLK	.00	8:16pm

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR

Analyst

This form is used when performing Preventive Maintenance procedures

Forensic Tests for Alcohol Branch

Department of Health and Human Services

Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

ROBESON COUNTY BAT MOBILE UNIT 5 770

Serial Number: 008707 Test Record Number: 2820

Test Date: 02/15/2024 Test Time: 8:17pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	8:17pm
FLO	Pass	8:17pm
FC	Pass	8:17pm

Temperature Tests

Test	Status	Time
FC1	Pass	8:18pm
SRC	Pass	8:18pm
DET	Pass	8:18pm
BAR	Pass	8:18pm
BT	Pass	8:18pm

Blank Tests

Test	Status	Time
AIR	Pass	8:18pm

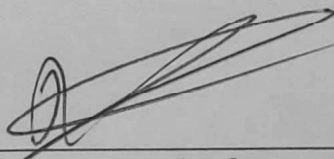
Printer Tests

Test	Status	Time
PRNT	Pass	8:18pm

CRC Tests

Test	Status	Time
COMP	Pass	8:18pm
CAL	Pass	8:18pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Robeson Instrument Location BAT Mobile Unit 5
Instrument Serial No. 008826 St. Pauls PD

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 3rd day of February, 2024 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

684
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

ROBESON COUNTY BAT MOBILE UNIT 5 770

Serial Number: 008826

Test Date: 02/03/2024

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Sharpe Jr., Robert J

Permit Number: 1820-8591

Effective:

10/01/2023-10/01/2025

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG308703

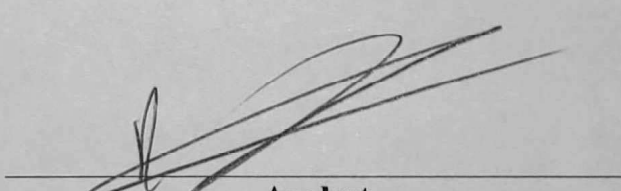
Exp Date: 03/28/2025

Test	g/210L	Time
DIAG	Pass	7:45pm
AIR BLK	.00	7:46pm
ACCY CHK	.07	7:47pm
AIR BLK	.00	7:47pm
SUB TEST	.00	7:48pm
AIR BLK	.00	7:49pm
SUB TEST	.00	7:50pm
AIR BLK	.00	7:51pm

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR


Analyst

Intox EC/IR-II: Preventive Maintenance

ROBESON COUNTY BAT MOBILE UNIT 5 770

Serial Number: 008826 Test Record Number: 8498
Test Date: 02/03/2024 Test Time: 7:52pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	7:52pm
FLO	Pass	7:52pm
FC	Pass	7:52pm

Temperature Tests

Test	Status	Time
FC1	Pass	7:52pm
SRC	Pass	7:52pm
DET	Pass	7:52pm
BAR	Pass	7:52pm
BT	Pass	7:52pm

Blank Tests

Test	Status	Time
AIR	Pass	7:53pm

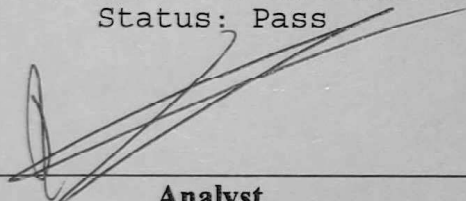
Printer Tests

Test	Status	Time
PRNT	Pass	7:53pm

CRC Tests

Test	Status	Time
COMP	Pass	7:53pm
CAL	Pass	7:53pm

Preventive Maintenance
Status: *Pass*



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Robeson Instrument Location BAT Mobile Unit 5
Instrument Serial No. 008826 Fairmont PD

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 16th day of February, 2024 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

684

Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

ROBESON COUNTY BAT MOBILE UNIT 5 770

Serial Number: 008826

Test Date: 02/16/2024

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Sharpe Jr., Robert J

Permit Number: 1820-8591

Effective:

10/01/2023-10/01/2025

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG308703

Exp Date: 03/28/2025

Test	g/210L	Time
DIAG	Pass	7:29pm
AIR BLK	.00	7:30pm
ACCY CHK	.07	7:31pm
AIR BLK	.00	7:32pm
SUB TEST	.00	7:32pm
AIR BLK	.00	7:33pm
SUB TEST	.00	7:35pm
AIR BLK	.00	7:36pm

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR

Analyst

Intox EC/IR-II: Preventive Maintenance

ROBESON COUNTY BAT MOBILE UNIT 5 770

Serial Number: 008826 Test Record Number: 8501
Test Date: 02/16/2024 Test Time: 7:36pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	7:37pm
FLO	Pass	7:37pm
FC	Pass	7:37pm

Temperature Tests

Test	Status	Time
FC1	Pass	7:37pm
SRC	Pass	7:37pm
DET	Pass	7:37pm
BAR	Pass	7:37pm
BT	Pass	7:37pm

Blank Tests

Test	Status	Time
AIR	Pass	7:38pm

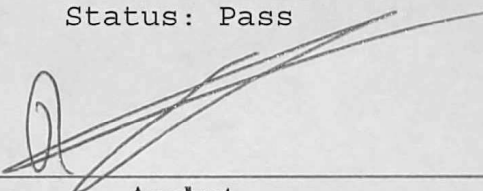
Printer Tests

Test	Status	Time
PRNT	Pass	7:38pm

CRC Tests

Test	Status	Time
COMP	Pass	7:38pm
CAL	Pass	7:38pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Robeson Instrument Location BAT Mobile Unit 5
Instrument Serial No. 00 8826 Lumberton PD

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 29th day of February, 2024 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

684
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

ROBESON COUNTY BAT MOBILE UNIT 5 770

Serial Number: 008826

Test Date: 02/29/2024

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Sharpe Jr., Robert J

Permit Number: 1820-8591

Effective:

10/01/2023-10/01/2025

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG308703

Exp Date: 03/28/2025

Test	g/210L	Time
DIAG	Pass	9:08pm
AIR BLK	.00	9:09pm
ACCY CHK	.07	9:10pm
AIR BLK	.00	9:10pm
SUB TEST	.00	9:11pm
AIR BLK	.00	9:12pm
SUB TEST	.00	9:14pm
AIR BLK	.00	9:14pm

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR

Analyst

Intox EC/IR-II: Preventive Maintenance

ROBESON COUNTY BAT MOBILE UNIT 5 770

Serial Number: 008826 Test Record Number: 8505
Test Date: 02/29/2024 Test Time: 9:15pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	9:15pm
FLO	Pass	9:15pm
FC	Pass	9:15pm

Temperature Tests

Test	Status	Time
FC1	Pass	9:15pm
SRC	Pass	9:15pm
DET	Pass	9:15pm
BAR	Pass	9:15pm
BT	Pass	9:15pm

Blank Tests

Test	Status	Time
AIR	Pass	9:16pm

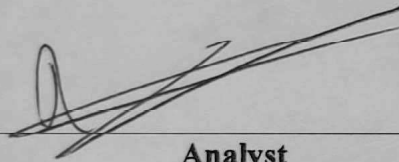
Printer Tests

Test	Status	Time
PRNT	Pass	9:16pm

CRC Tests

Test	Status	Time
COMP	Pass	9:16pm
CAL	Pass	9:16pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County ROCKINGHAM Instrument Location EDEN POLICE

Instrument Serial No. 008636 DEPARTMENT

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 5TH day of FEBRUARY, 2024 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

669
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

ROCKINGHAM COUNTY EDEN PD 780

Serial Number: 008636
Test Date: 02/05/2024

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: Oligmueller, Leo A
Permit Number: 0035-3799
Effective:
10/01/2023-10/01/2025

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG303001
Exp Date: 01/30/2025

Test	g/210L	Time
DIAG	Pass	11:35am
AIR BLK	.00	11:36am
ACCY CHK	.08	11:37am
AIR BLK	.00	11:38am
SUB TEST	.00	11:39am
AIR BLK	.00	11:40am
SUB TEST	.00	11:41am
AIR BLK	.00	11:42am

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

ROCKINGHAM COUNTY EDEN PD 780

Serial Number: 008636 Test Record Number: 2616
Test Date: 02/05/2024 Test Time: 11:43am EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	11:44am
FLO	Pass	11:44am
FC	Pass	11:44am

Temperature Tests

Test	Status	Time
FC1	Pass	11:44am
SRC	Pass	11:44am
DET	Pass	11:44am
BAR	Pass	11:44am
BT	Pass	11:44am

Blank Tests

Test	Status	Time
AIR	Pass	11:45am

Printer Tests

Test	Status	Time
PRNT	Pass	11:45am

CRC Tests

Test	Status	Time
COMP	Pass	11:45am
CAL	Pass	11:45am

Preventive Maintenance
Status: Pass


Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

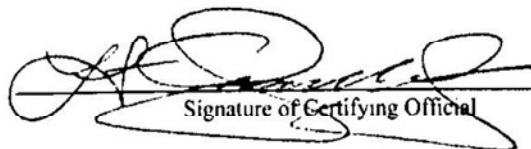
County ROCKINGHAM Instrument Location REIDSVILLE POLICE
Instrument Serial No 008784 DEPARTMENT

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus 2 degree centigrade,
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 5TH day of FEBRUARY, 2024 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.




Signature of Certifying Official

669
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

ROCKINGHAM COUNTY REIDSVILLE PD 780

Serial Number: 008784

Test Date: 02/05/2024

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Oligmueller, Leo A

Permit Number: 0035-3799

Effective:

10/01/2023-10/01/2025

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG303001

Exp Date: 01/30/2025

Test	g/210L	Time
DIAG	Pass	10:07am
AIR BLK	.00	10:08am
ACCY CHK	.08	10:08am
AIR BLK	.00	10:09am
SUB TEST	.00	10:10am
AIR BLK	.00	10:11am
SUB TEST	.00	10:12am
AIR BLK	.00	10:13am

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

This form is used when performing Preventive Maintenance procedures

Forensic Tests for Alcohol Branch

Department of Health and Human Services

Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

ROCKINGHAM COUNTY REIDSVILLE PD 780

Serial Number: 008784 Test Record Number: 1488
Test Date: 02/05/2024 Test Time: 10:14am EST

System Check: Passed

Baseline Tests

Test	Status	Time
IR	Pass	10:14am
FLO	Pass	10:14am
FC	Pass	10:14am

Temperature Tests

Test	Status	Time
FC1	Pass	10:14am
SRC	Pass	10:14am
DET	Pass	10:14am
BAR	Pass	10:14am
BT	Pass	10:14am

Blank Tests

Test	Status	Time
AIR	Pass	10:15am


Printer Tests

Test	Status	Time
PRNT	Pass	10:15am

CRC Tests:

Test	Status	Time
COMP	Pass	10:15am
CAL	Pass	10:15am

Preventive Maintenance
Status: Pass


Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH


PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Rutherford Instrument Location Forest City Police Dept.
Instrument Serial No. 008889 Forest City, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 8 day of February, 2024 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

1668
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

RUTHERFORD COUNTY FOREST CITY PD 800

Serial Number: 008889

Test Date: 02/08/2024

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Loftis, Benjamin C

Permit Number: 0024-4987

Effective:

10/01/2023-10/01/2025

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG308704

Exp Date: 03/28/2025

Test	g/210L	Time
DIAG	Pass	9:54am
AIR BLK	.00	9:55am
ACCY CHK	.07	9:56am
AIR BLK	.00	9:57am
SUB TEST	.00	9:57am
AIR BLK	.00	9:59am
SUB TEST	.00	10:00am
AIR BLK	.00	10:01am

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

RUTHERFORD COUNTY FOREST CITY PD 800

Serial Number: 008889 Test Record Number: 1125
Test Date: 02/08/2024 Test Time: 10:01am EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	10:02am
FLO	Pass	10:02am
FC	Pass	10:02am

Temperature Tests

Test	Status	Time
FC1	Pass	10:02am
SRC	Pass	10:02am
DET	Pass	10:02am
BAR	Pass	10:02am
BT	Pass	10:02am

Blank Tests

Test	Status	Time
AIR	Pass	10:02am


Printer Tests

Test	Status	Time
PRNT	Pass	10:02am

CRC Tests

Test	Status	Time
COMP	Pass	10:03am
CAL	Pass	10:03am

Preventive Maintenance
Status: Pass


Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Rutherford Instrument Location Rutherford County Jail

Instrument Serial No. 008914 Rutherfordton, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 8 day of February, 2024 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

6068
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

RUTHERFORD COUNTY RUTHERFORD COUNTY SO
800

Serial Number: 008914

Test Date: 02/08/2024

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Loftis, Benjamin C

Permit Number: 0024-4987

Effective:

10/01/2023-10/01/2025

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

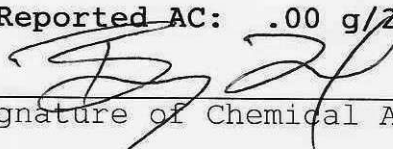
Test Type: Breath Test

Lot Number: AG308704

Exp Date: 03/28/2025

Test	g/210L	Time
DIAG	Pass	11:51am
AIR BLK	.00	11:52am
ACCY CHK	.08	11:53am
AIR BLK	.00	11:54am
SUB TEST	.00	11:55am
AIR BLK	.00	11:56am
SUB TEST	.00	11:57am
AIR BLK	.00	11:58am

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

RUTHERFORD COUNTY RUTHERFORD COUNTY SO 800

Serial Number: 008914 Test Record Number: 2720
Test Date: 02/08/2024 Test Time: 11:59am EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	12:00pm
FLO	Pass	12:00pm
FC	Pass	12:00pm

Temperature Tests

Test	Status	Time
FC1	Pass	12:00pm
SRC	Pass	12:00pm
DET	Pass	12:00pm
BAR	Pass	12:00pm
BT	Pass	12:00pm

Blank Tests

Test	Status	Time
AIR	Pass	12:00pm

Printer Tests

Test	Status	Time
PRNT	Pass	12:01pm

CRC Tests

Test	Status	Time
COMP	Pass	12:01pm
CAL	Pass	12:01pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County SAMPSON Instrument Location SAMPSON COUNTY

Instrument Serial No. 005825 DETENTION CENTER

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 20 day of FEBRUARY, 2024 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Alan R. Benson

Signature of Certifying Official

648

Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

SAMPSON COUNTY DETENTION CENTER 810

Serial Number: 008825
Test Date: 02/20/2024

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE

Analyst's Name: BARNES, ALVIN R
Permit Number: 0014-6279
Effective:
10/01/2023-10/01/2025

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG400301
Exp Date: 01/03/2026

Test	g/210L	Time
DIAG	Pass	8:55am
AIR BLK	.00	8:56am
ACCY CHK	.08	8:56am
AIR BLK	.00	8:58am
SUB TEST	.00	8:58am
AIR BLK	.00	8:59am
SUB TEST	.00	9:01am
AIR BLK	.00	9:02am

Reported AC: .00 g/210L

Alvin R. Barnes
Signature of Chemical Analyst

Court CVR

Alvin R. Barnes
Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

SAMPSON COUNTY DETENTION CENTER 810

Serial Number: 008825 Test Record Number: 3660
Test Date: 02/20/2024 Test Time: 9:03am EST

System Check: Passed

Baseline Tests

Test	Status	Time
IR	Pass	9:03am
FLO	Pass	9:03am
FC	Pass	9:03am

Temperature Tests

Test	Status	Time
FC1	Pass	9:04am
SRC	Pass	9:04am
DET	Pass	9:04am
BAR	Pass	9:04am
BT	Pass	9:04am

Blank Tests

Test	Status	Time
AIR	Pass	9:04am


Printer Tests

Test	Status	Time
PRNT	Pass	9:04am

CRC Tests

Test	Status	Time
COMP	Pass	9:04am
CAL	Pass	9:04am

Preventive Maintenance
Status: Pass



Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County JAMPSON Instrument Location JAMPSON COUNTY
Instrument Serial No. 008877 DETENTION CENTER

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 20 day of FEBRUARY, 2024 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Alan R. Benson

Signature of Certifying Official

648

Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

SAMPSON COUNTY DETENTION CENTER 810

Serial Number: 008877

Test Date: 02/20/2024

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: BARNES, ALVIN R

Permit Number: 0014-6279

Effective:

10/01/2023-10/01/2025

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG400301

Exp Date: 01/03/2026

Test	g/210L	Time
DIAG	Pass	8:47am
AIR BLK	.00	8:48am
ACCY CHK	.08	8:48am
AIR BLK	.00	8:50am
SUB TEST	.00	8:50am
AIR BLK	.00	8:51am
SUB TEST	.00	8:53am
AIR BLK	.00	8:54am

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR


Analyst

This form is used when performing Preventive Maintenance procedures

Forensic Tests for Alcohol Branch

Department of Health and Human Services

Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

SAMPSON COUNTY DETENTION CENTER 810

Serial Number: 008877 Test Record Number: 4149
Test Date: 02/20/2024 Test Time: 8:55am EST

System Check: Passed

Baseline Tests

Test	Status	Time
IR	Pass	8:55am
FLO	Pass	8:55am
FC	Pass	8:56am

Temperature Tests

Test	Status	Time
FC1	Pass	8:56am
SRC	Pass	8:56am
DET	Pass	8:56am
BAR	Pass	8:56am
BT	Pass	8:56am

Blank Tests

Test	Status	Time
AIR	Pass	8:56am

Printer Tests

Test	Status	Time
PRNT	Pass	8:56am

CRC Tests

Test	Status	Time
COMP	Pass	8:57am
CAL	Pass	8:57am

Preventive Maintenance
Status: Pass


Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County STANLEY Instrument Location STANLEY COUNTY SO
Instrument Serial No. 008824 ALBEMARLE NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 05 day of FEBRUARY, 2024 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

6460
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

STANLY COUNTY STANLY COUNTY SO 830

Serial Number: 008824
Test Date: 02/05/2024

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Fleming, Tina S

Permit Number: 0027-4970

Effective:

07/01/2022-07/01/2024

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG212403

Exp Date: 05/04/2024

Test	g/210L	Time
DIAG	Pass	1:03pm
AIR BLK	.00	1:04pm
ACCY CHK	.07	1:05pm
AIR BLK	.00	1:06pm
SUB TEST	.00	1:07pm
AIR BLK	.00	1:07pm
SUB TEST	.00	1:09pm
AIR BLK	.00	1:10pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

STANLY COUNTY STANLY COUNTY SO 830

Serial Number: 008824 Test Record Number: 2100
Test Date: 02/05/2024 Test Time: 1:11pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	1:11pm
FLO	Pass	1:11pm
FC	Pass	1:11pm

Temperature Tests

Test	Status	Time
FC1	Pass	1:11pm
SRC	Pass	1:11pm
DET	Pass	1:11pm
BAR	Pass	1:11pm
BT	Pass	1:11pm

Blank Tests

Test	Status	Time
AIR	Pass	1:12pm


Printer Tests

Test	Status	Time
PRNT	Pass	1:12pm

CRC Tests

Test	Status	Time
COMP	Pass	1:12pm
CAL	Pass	1:12pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Stanly Instrument Location Stanly County SO

Instrument Serial No. 608842 ALLENABLE NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 05 day of FEBRUARY, 2024 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Jim S. Fleming
Signature of Certifying Official

646
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

STANLY COUNTY SHERIFFS OFFICE 830

Serial Number: 008842

Test Date: 02/05/2024

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Fleming, Tina S

Permit Number: 0027-4970

Effective:

07/01/2022-07/01/2024

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG400303

Exp Date: 01/03/2026


Test	g/210L	Time
DIAG	Pass	12:39pm
AIR BLK	.00	12:39pm
ACCY CHK	.08	12:40pm
AIR BLK	.00	12:41pm
SUB TEST	.00	12:42pm
AIR BLK	.00	12:43pm
SUB TEST	.00	12:45pm
AIR BLK	.00	12:46pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

STANLY COUNTY SHERIFFS OFFICE 830

Serial Number: 008842 Test Record Number: 2936
Test Date: 02/05/2024 Test Time: 12:46pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	12:47pm
FLO	Pass	12:47pm
FC	Pass	12:47pm

Temperature Tests

Test	Status	Time
FC1	Pass	12:47pm
SRC	Pass	12:47pm
DET	Pass	12:47pm
BAR	Pass	12:47pm
BT	Pass	12:47pm

Blank Tests

Test	Status	Time
AIR	Pass	12:48pm


Printer Tests

Test	Status	Time
PRNT	Pass	12:48pm

CRC Tests

Test	Status	Time
COMP	Pass	12:48pm
CAL	Pass	12:48pm

Preventive Maintenance
Status: Pass



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

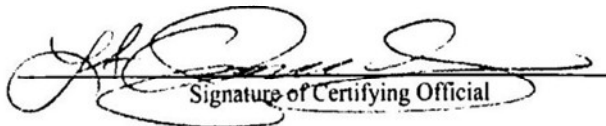
County STOKES Instrument Location STOKES COUNTY JAIL
Instrument Serial No. 008596 DANBURY, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 5TH day of FEBRUARY, 2024 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.




Signature of Certifying Official

669
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

STOKES COUNTY STOKES COUNTY JAIL 840

Serial Number: 008596

Test Date: 02/05/2024

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Oligmueller, Leo A

Permit Number: 0035-3799

Effective:

10/01/2023-10/01/2025

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

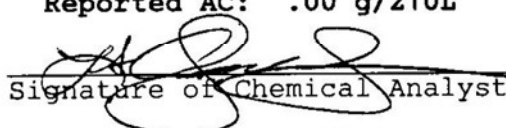
Test Type: Breath Test

Lot Number: AG303001

Exp Date: 01/30/2025

Test	g/210L	Time
DIAG	Pass	1:55pm
AIR BLK	.00	1:56pm
ACCY CHK	.07	1:56pm
AIR BLK	.00	1:57pm
SUB TEST	.00	1:58pm
AIR BLK	.00	1:59pm
SUB TEST	.00	2:00pm
AIR BLK	.00	2:01pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

STOKES COUNTY STOKES COUNTY JAIL 840

Serial Number: 008596 Test Record Number: 1435
Test Date: 02/05/2024 Test Time: 2:02pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	2:02pm
FLO	Pass	2:02pm
FC	Pass	2:03pm

Temperature Tests

Test	Status	Time
FC1	Pass	2:03pm
SRC	Pass	2:03pm
DET	Pass	2:03pm
BAR	Pass	2:03pm
BT	Pass	2:03pm

Blank Tests

Test	Status	Time
AIR	Pass	2:03pm

Printer Tests

Test	Status	Time
PRNT	Pass	2:03pm

CRC Tests

Test	Status	Time
COMP	Pass	2:03pm
CAL	Pass	2:03pm

Preventive Maintenance
Status: Pass


Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County STOKES Instrument Location KING POLICE
Instrument Serial No. 008718 DEPARTMENT

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 5TH day of FEBRUARY, 2024 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

669
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

STOKES COUNTY KING PD 840

Serial Number: 008718

Test Date: 02/05/2024

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Oligmueller, Leo A

Permit Number: 0035-3799

Effective:

10/01/2023-10/01/2025

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG308704

Exp Date: 03/28/2025

Test	g/210L	Time
DIAG	Pass	3:52pm
AIR BLK	.00	3:53pm
ACCY CHK	.08	3:54pm
AIR BLK	.00	3:55pm
SUB TEST	.00	3:56pm
AIR BLK	.00	3:57pm
SUB TEST	.00	3:58pm
AIR BLK	.00	3:59pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

STOKES COUNTY KING PD 840

Serial Number: 008718 Test Record Number: 2362
Test Date: 02/05/2024 Test Time: 4:00pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	4:00pm
FLO	Pass	4:00pm
FC	Pass	4:00pm

Temperature Tests

Test	Status	Time
FC1	Pass	4:00pm
SRC	Pass	4:00pm
DET	Pass	4:00pm
BAR	Pass	4:00pm
BT	Pass	4:00pm

Blank Tests

Test	Status	Time
AIR	Pass	4:01pm

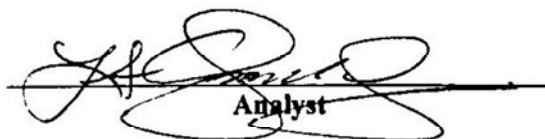
Printer Tests

Test	Status	Time
PRNT	Pass	4:01pm

CRC Tests

Test	Status	Time
COMP	Pass	4:01pm
CAL	Pass	4:01pm

Preventive Maintenance
Status: Pass


Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County SURRY Instrument Location PILOT MOUNTAIN
Instrument Serial No. 008938 POLICE DEPARTMENT

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 5TH day of FEBRUARY, 2024 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



A handwritten signature in black ink, appearing to be "J. H. [unclear]".
Signature of Certifying Official

669
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

SURRY COUNTY PILOT MOUNTAIN PD 850

Serial Number: 008938

Test Date: 02/05/2024

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Oligmueller, Leo A

Permit Number: 0035-3799

Effective:

10/01/2023-10/01/2025

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test


Lot Number: AG308101

Exp Date: 03/22/2025

Test	g/210L	Time
DIAG	Pass	3:09pm
AIR BLK	.00	3:10pm
ACCY CHK	.08	3:11pm
AIR BLK	.00	3:13pm
SUB TEST	.00	3:13pm
AIR BLK	.00	3:14pm
SUB TEST	.00	3:16pm
AIR BLK	.00	3:17pm

Reported AC: .00 g/210L


Signature of Chemical Analyst
Court CVR


Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

SURRY COUNTY PILOT MOUNTAIN PD 850

Serial Number: 008938 Test Record Number: 844
Test Date: 02/05/2024 Test Time: 3:17pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	3:18pm
FLO	Pass	3:18pm
FC	Pass	3:18pm

Temperature Tests

Test	Status	Time
FC1	Pass	3:18pm
SRC	Pass	3:18pm
DET	Pass	3:18pm
BAR	Pass	3:18pm
BT	Pass	3:18pm

Blank Tests

Test	Status	Time
AIR	Pass	3:18pm

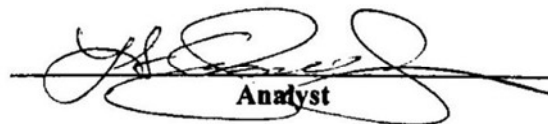
Printer Tests

Test	Status	Time
PRNT	Pass	3:18pm

CRC Tests

Test	Status	Time
COMP	Pass	3:19pm
CAL	Pass	3:19pm

Preventive Maintenance
Status: Pass


Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County Swain

Instrument Location

Swain Co Jail

Instrument Serial No. 008723

Bryson City, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 21 day of February, 2024 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Phil R. Cotton

Signature of Certifying Official

635

Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

SWAIN COUNTY JAIL 860

Serial Number: 008723

Test Date: 02/21/2024

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Cutler, Daniel R

Permit Number: 0084-3310

Effective:

10/01/2023-10/01/2025

Officer's Name: NONE,

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG303102

Exp Date: 01/31/2025


Test	g/210L	Time
DIAG	Pass	1:49pm
AIR BLK	.00	1:50pm
ACCY CHK	.08	1:51pm
AIR BLK	.00	1:52pm
SUB TEST	.00	1:53pm
AIR BLK	.00	1:54pm
SUB TEST	.00	1:55pm
AIR BLK	.00	1:56pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

Intox EC/IR-II: Preventive Maintenance

SWAIN COUNTY JAIL 860

Serial Number: 008723 Test Record Number: 887
Test Date: 02/21/2024 Test Time: 2:00pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	2:01pm
FLO	Pass	2:01pm
FC	Pass	2:01pm

Temperature Tests

Test	Status	Time
FC1	Pass	2:01pm
SRC	Pass	2:01pm
DET	Pass	2:01pm
BAR	Pass	2:01pm
BT	Pass	2:01pm

Blank Tests

Test	Status	Time
AIR	Pass	2:01pm


Printer Tests

Test	Status	Time
PRNT	Pass	2:02pm

CRC Tests

Test	Status	Time
COMP	Pass	2:02pm
CAL	Pass	2:02pm

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County Swain Instrument Location Swain County Jail
Instrument Serial No. 008727 Bryson City, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 21 day of February, 2024 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



David R. Guther
Signature of Certifying Official

635
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

SWAIN COUNTY JAIL 860

Serial Number: 008727

Test Date: 02/21/2024

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Cutler, Daniel R

Permit Number: 0084-3310

Effective:

10/01/2023-10/01/2025

Officer's Name: NONE,

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG308704

Exp Date: 03/28/2025


Test	g/210L	Time
DIAG	Pass	1:47pm
AIR BLK	.00	1:48pm
ACCY CHK	.07	1:49pm
AIR BLK	.00	1:50pm
SUB TEST	.00	1:50pm
AIR BLK	.00	1:51pm
SUB TEST	.00	1:53pm
AIR BLK	.00	1:54pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

This form is used when performing Preventive Maintenance procedures

Forensic Tests for Alcohol Branch

Department of Health and Human Services

Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

SWAIN COUNTY JAIL 860

Serial Number: 008727 Test Record Number: 1635
Test Date: 02/21/2024 Test Time: 1:54pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	1:55pm
FLO	Pass	1:55pm
FC	Pass	1:55pm

Temperature Tests

Test	Status	Time
FC1	Pass	1:55pm
SRC	Pass	1:55pm
DET	Pass	1:55pm
BAR	Pass	1:55pm
BT	Pass	1:55pm

Blank Tests

Test	Status	Time
AIR	Pass	1:56pm

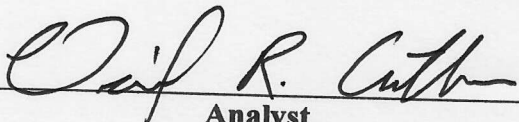
Printer Tests

Test	Status	Time
PRNT	Pass	1:56pm

CRC Tests

Test	Status	Time
COMP	Pass	1:56pm
CAL	Pass	1:56pm

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Swain Instrument Location Cherokee Tribal Detention
Instrument Serial No. 008782 Cherokee, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 20 day of February, 2024 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Chief R. Cuth
Signature of Certifying Official

635
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

SWAIN COUNTY CHEROKEE DETENTION 860

Serial Number: 008782

Test Date: 02/20/2024

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Cutler, Daniel R

Permit Number: 0084-3310

Effective:

10/01/2023-10/01/2025

Officer's Name: NONE,

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG302702

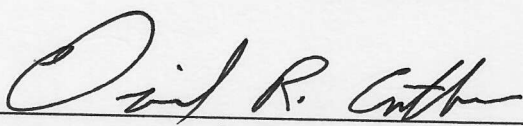
Exp Date: 01/27/2025

Test	g/210L	Time
DIAG	Pass	2:05pm
AIR BLK	.00	2:06pm
ACCY CHK	.07	2:06pm
AIR BLK	.00	2:08pm
SUB TEST	.00	2:08pm
AIR BLK	.00	2:09pm
SUB TEST	.00	2:11pm
AIR BLK	.00	2:12pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

SWAIN COUNTY CHEROKEE DETENTION 860

Serial Number: 008782 Test Record Number: 1523
Test Date: 02/20/2024 Test Time: 2:13pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	2:13pm
FLO	Pass	2:13pm
FC	Pass	2:13pm

Temperature Tests

Test	Status	Time
FC1	Pass	2:13pm
SRC	Pass	2:13pm
DET	Pass	2:13pm
BAR	Pass	2:13pm
BT	Pass	2:13pm

Blank Tests

Test	Status	Time
AIR	Pass	2:14pm


Printer Tests

Test	Status	Time
PRNT	Pass	2:14pm

CRC Tests

Test	Status	Time
COMP	Pass	2:14pm
CAL	Pass	2:14pm

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH


PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Transylvania Instrument Location Transylvania County Jail
Instrument Serial No. 008609 Brevard, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 10 day of February, 2024 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

668
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

TRANSYLVANIA COUNTY TRANSYLVANIA CO
JAIL 870

Serial Number: 008609

Test Date: 02/06/2024

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Loftis, Benjamin C

Permit Number: 0024-4987

Effective:

10/01/2023-10/01/2025

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

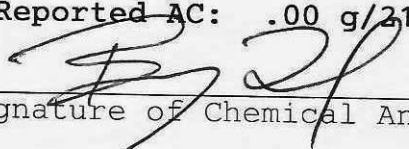
Test Type: Breath Test

Lot Number: AG308004

Exp Date: 03/21/2025

Test	g/210L	Time
DIAG	Pass	10:37am
AIR BLK	.00	10:37am
ACCY CHK	.07	10:38am
AIR BLK	.00	10:39am
SUB TEST	.00	10:40am
AIR BLK	.00	10:40am
SUB TEST	.00	10:42am
AIR BLK	.00	10:43am

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

TRANSYLVANIA COUNTY TRANSYLVANIA CO JAIL 870

Serial Number: 008609 Test Record Number: 1190
Test Date: 02/06/2024 Test Time: 10:43am EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	10:43am
FLO	Pass	10:43am
FC	Pass	10:43am

Temperature Tests

Test	Status	Time
FC1	Pass	10:44am
SRC	Pass	10:44am
DET	Pass	10:44am
BAR	Pass	10:44am
BT	Pass	10:44am

Blank Tests

Test	Status	Time
AIR	Pass	10:44am

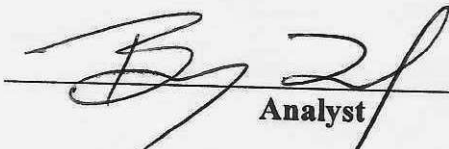
Printer Tests

Test	Status	Time
PRNT	Pass	10:44am

CRC Tests

Test	Status	Time
COMP	Pass	10:44am
CAL	Pass	10:44am

Preventive Maintenance
Status: *Pass*



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Transylvania Instrument Location Transylvania County Jail
Instrument Serial No. 008820 Brevard, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 10 day of February, 2024 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

668
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

TRANSYLVANIA COUNTY TRANSYLVANIA CO
JAIL 870

Serial Number: 008820
Test Date: 02/06/2024

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Loftis, Benjamin C

Permit Number: 0024-4987

Effective:

10/01/2023-10/01/2025

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

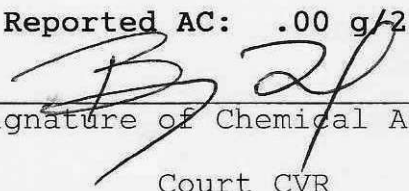
Test Type: Breath Test

Lot Number: AG308004

Exp Date: 03/21/2025

Test	g/210L	Time
DIAG	Pass	10:37am
AIR BLK	.00	10:38am
ACCY CHK	.07	10:38am
AIR BLK	.00	10:39am
SUB TEST	.00	10:40am
AIR BLK	.00	10:41am
SUB TEST	.00	10:42am
AIR BLK	.00	10:43am

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

TRANSYLVANIA COUNTY TRANSYLVANIA CO JAIL 870

Serial Number: 008820 Test Record Number: 1664
Test Date: 02/06/2024 Test Time: 10:44am EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	10:44am
FLO	Pass	10:44am
FC	Pass	10:44am

Temperature Tests

Test	Status	Time
FC1	Pass	10:44am
SRC	Pass	10:44am
DET	Pass	10:44am
BAR	Pass	10:44am
BT	Pass	10:44am

Blank Tests

Test	Status	Time
AIR	Pass	10:45am

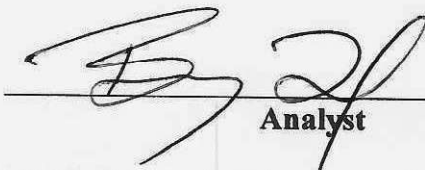
Printer Tests

Test	Status	Time
PRNT	Pass	10:45am

CRC Tests

Test	Status	Time
COMP	Pass	10:45am
CAL	Pass	10:45am

Preventive Maintenance
Status: Pass



Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Transylvania County Instrument Location BAT Mobile unit 2
Instrument Serial No. 008970 Transylvania County SO

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 16th day of February, 2024 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

679
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

TRANSYLVANIA COUNTY BAT MOBILE UNIT 2
870

Serial Number: 008970
Test Date: 02/16/2024

Citation Number: M00000000-0
Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Greene, Nathaniel T

Permit Number: 0067-5960

Effective:

10/01/2023-10/01/2025

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

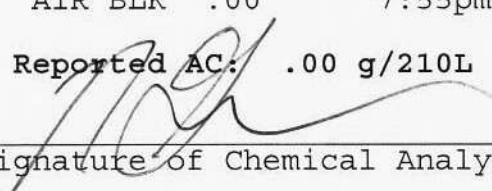
Test Type: Breath Test

Lot Number: AG302703

Exp Date: 01/27/2025

Test	g/210L	Time
DIAG	Pass	7:48pm
AIR BLK	.00	7:49pm
ACCY CHK	.08	7:50pm
AIR BLK	.00	7:51pm
SUB TEST	.00	7:51pm
AIR BLK	.00	7:52pm
SUB TEST	.00	7:54pm
AIR BLK	.00	7:55pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

TRANSYLVANIA COUNTY BAT MOBILE UNIT 2 870

Serial Number: 008970 Test Record Number: 1070
Test Date: 02/16/2024 Test Time: 7:58pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	7:59pm
FLO	Pass	7:59pm
FC	Pass	7:59pm

Temperature Tests

Test	Status	Time
FC1	Pass	7:59pm
SRC	Pass	7:59pm
DET	Pass	7:59pm
BAR	Pass	7:59pm
BT	Pass	7:59pm

Blank Tests

Test	Status	Time
AIR	Pass	8:00pm


Printer Tests

Test	Status	Time
PRNT	Pass	8:00pm

CRC Tests

Test	Status	Time
COMP	Pass	8:00pm
CAL	Pass	8:00pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Tyrrell Instrument Location Tyrrell Co. S.O.
Instrument Serial No. 008902 412 Main St., Columbia, N.C.

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 2nd day of February, 2024 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Key D. Day

Signature of Certifying Official

643

Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

TYRRELL COUNTY SHERIFF'S OFFICE 880

Serial Number: 008902

Test Date: 02/02/2024

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Gray, Kelly D

Permit Number: 0037-7722

Effective:

10/01/2023-10/01/2025

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG212403

Exp Date: 05/04/2024


Test	g/210L	Time
DIAG	Pass	10:32am
AIR BLK	.00	10:32am
ACCY CHK	.07	10:33am
AIR BLK	.00	10:34am
SUB TEST	.00	10:35am
AIR BLK	.00	10:36am
SUB TEST	.00	10:38am
AIR BLK	.00	10:39am

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

TYRRELL COUNTY SHERIFF'S OFFICE 880

Serial Number: 008902 Test Record Number: 1160
Test Date: 02/02/2024 Test Time: 10:41am EST

System Check: Passed

Baseline Tests

Test	Status	Time
IR	Pass	10:41am
FLO	Pass	10:41am
FC	Pass	10:42am

Temperature Tests

Test	Status	Time
FC1	Pass	10:42am
SRC	Pass	10:42am
DET	Pass	10:42am
BAR	Pass	10:42am
BT	Pass	10:42am

Blank Tests

Test	Status	Time
AIR	Pass	10:42am


Printer Tests

Test	Status	Time
PRNT	Pass	10:42am

CRC Tests

Test	Status	Time
COMP	Pass	10:43am
CAL	Pass	10:43am

Preventive Maintenance
Status: Pass


Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Union Instrument Location Stallings PD
Instrument Serial No. 008694 Stallings, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 23rd day of February, 2024 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Bruce Helms
Signature of Certifying Official

674

Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

UNION COUNTY STALLINGS PD 890

Serial Number: 008694

Test Date: 02/23/2024

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Helms, Bryce A

Permit Number: 0084-9845

Effective:

10/01/2023-10/01/2025

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG212403

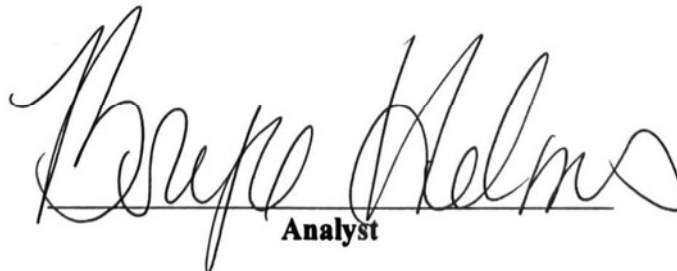
Exp Date: 05/04/2024

Test	g/210L	Time
DIAG	Pass	10:14am
AIR BLK	.00	10:15am
ACCY CHK	.07	10:16am
AIR BLK	.00	10:17am
SUB TEST	.00	10:18am
AIR BLK	.00	10:18am
SUB TEST	.00	10:20am
AIR BLK	.00	10:21am

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

UNION COUNTY STALLINGS PD 890

Serial Number: 008694 Test Record Number: 1797
Test Date: 02/23/2024 Test Time: 10:21am EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	10:22am
FLO	Pass	10:22am
FC	Pass	10:22am

Temperature Tests

Test	Status	Time
FC1	Pass	10:22am
SRC	Pass	10:22am
DET	Pass	10:22am
BAR	Pass	10:22am
BT	Pass	10:22am

Blank Tests

Test	Status	Time
AIR	Pass	10:23am

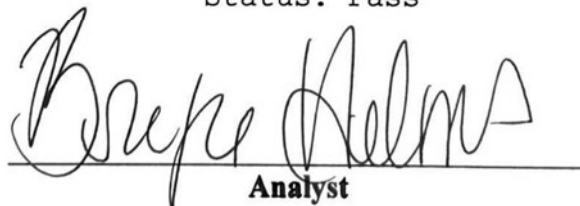
Printer Tests

Test	Status	Time
PRNT	Pass	10:23am

CRC Tests

Test	Status	Time
COMP	Pass	10:23am
CAL	Pass	10:23am

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Wake Instrument Location CARY PD

Instrument Serial No. 008587 120 Wilkerson Ave Cary, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 19 day of February, 2024 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Sam Stokes Barnes
Signature of Certifying Official

662
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

WAKE COUNTY CARY PD 910

Serial Number: 008587

Test Date: 02/19/2024

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Barnes, Simon S

Permit Number: 0014-6221

Effective:

10/01/2023-10/01/2025

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG308704


Exp Date: 03/28/2025

Test	g/210L	Time
DIAG	Pass	9:58am
AIR BLK	.00	9:59am
ACCY CHK	.07	9:59am
AIR BLK	.00	10:00am
SUB TEST	.00	10:01am
AIR BLK	.00	10:02am
SUB TEST	.00	10:03am
AIR BLK	.00	10:04am

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

WAKE COUNTY CARY PD 910

Serial Number: 008587 Test Record Number: 5207
Test Date: 02/19/2024 Test Time: 10:04am EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	10:05am
FLO	Pass	10:05am
FC	Pass	10:05am

Temperature Tests

Test	Status	Time
FC1	Pass	10:05am
SRC	Pass	10:05am
DET	Pass	10:05am
BAR	Pass	10:05am
BT	Pass	10:05am

Blank Tests

Test	Status	Time
AIR	Pass	10:06am

Printer Tests

Test	Status	Time
PRNT	Pass	10:06am

CRC Tests

Test	Status	Time
COMP	Pass	10:06am
CAL	Pass	10:06am

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County Wake Instrument Location Alex PD Substation 4
Instrument Serial No. 008621 1615 E. Williams St Apex, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 20 day of February, 2024 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Simon Stokes Barnes
Signature of Certifying Official

662
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

WAKE COUNTY APEX PD

Serial Number: 008621

Test Date: 02/20/2024

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Barnes, Simon S

Permit Number: 0014-6221

Effective:

10/01/2023-10/01/2025

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG303102

Exp Date: 01/31/2025

Test	g/210L	Time
DIAG	Pass	10:46am
AIR BLK	.00	10:46am
ACCY CHK	.08	10:47am
AIR BLK	.00	10:48am
SUB TEST	.00	10:49am
AIR BLK	.00	10:49am
SUB TEST	.00	10:51am
AIR BLK	.00	10:52am

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

Intox EC/IR-II: Preventive Maintenance

WAKE COUNTY APEX PD

Serial Number: 008621 Test Record Number: 3571
Test Date: 02/20/2024 Test Time: 10:55am EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	10:55am
FLO	Pass	10:55am
FC	Pass	10:55am

Temperature Tests

Test	Status	Time
FC1	Pass	10:55am
SRC	Pass	10:55am
DET	Pass	10:55am
BAR	Pass	10:55am
BT	Pass	10:55am

Blank Tests

Test	Status	Time
AIR	Pass	10:56am


Printer Tests

Test	Status	Time
PRNT	Pass	10:56am

CRC Tests

Test	Status	Time
COMP	Pass	10:56am
CAL	Pass	10:56am

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County WAKE Instrument Location RALEIGH PD NORTHEAST DIST
Instrument Serial No. 008623 5228 GREEN'S DAIRY Rd
RALEIGH, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 13 day of FEBRUARY, 2024 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

671
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

WAKE COUNTY NORTH EAST DISTRICT 910

Serial Number: 008623
Test Date: 02/13/2024

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Bryant, Earl A

Permit Number: 0017-9707

Effective:

10/01/2023-10/01/2025

Officer's Name: NONE, NONE

Type of Agency: FTA

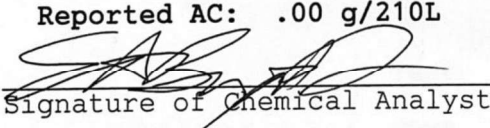
Agency: DHHS

Test Type: Breath Test

Lot Number: AG303102
Exp Date: 01/31/2025

Test	g/210L	Time
DIAG	Pass	10:02am
AIR BLK	.00	10:03am
ACCY CHK	.07	10:04am
AIR BLK	.00	10:05am
SUB TEST	.00	10:05am
AIR BLK	.00	10:06am
SUB TEST	.00	10:08am
AIR BLK	.00	10:09am

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

WAKE COUNTY NORTH EAST DISTRICT 910

Serial Number: 008623 Test Record Number: 4792
Test Date: 02/13/2024 Test Time: 10:09am EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	10:10am
FLO	Pass	10:10am
FC	Pass	10:10am

Temperature Tests

Test	Status	Time
FC1	Pass	10:10am
SRC	Pass	10:10am
DET	Pass	10:10am
BAR	Pass	10:10am
BT	Pass	10:10am

Blank Tests

Test	Status	Time
AIR	Pass	10:11am

Printer Tests

Test	Status	Time
PRNT	Pass	10:11am

CRC Tests

Test	Status	Time
COMP	Pass	10:11am
CAL	Pass	10:11am

Preventive Maintenance
Status: Pass


Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County WAKE Instrument Location KNIGHTDALE PD
Instrument Serial No. 008651 879 STEEPLE SQUARE CT.
KNIGHTDALE, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 26 day of FEBRUARY, 20 24 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

671
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

WAKE COUNTY KNIGHTDALE PD 910

Serial Number: 008651

Test Date: 02/26/2024

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Bryant, Earl A

Permit Number: 0017-9707

Effective:

10/01/2023-10/01/2025

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG308003

Exp Date: 03/21/2025

Test	g/210L	Time
DIAG	Pass	11:50am
AIR BLK	.00	11:51am
ACCY CHK	.08	11:52am
AIR BLK	.00	11:53am
SUB TEST	.00	11:54am
AIR BLK	.00	11:54am
SUB TEST	.00	11:56am
AIR BLK	.00	11:57am

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

WAKE COUNTY KNIGHTDALE PD 910

Serial Number: 008651 Test Record Number: 1679
Test Date: 02/26/2024 Test Time: 11:58am EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	11:58am
FLO	Pass	11:58am
FC	Pass	11:58am

Temperature Tests

Test	Status	Time
FC1	Pass	11:58am
SRC	Pass	11:58am
DET	Pass	11:58am
BAR	Pass	11:58am
BT	Pass	11:58am

Blank Tests

Test	Status	Time
AIR	Pass	11:59am


Printer Tests

Test	Status	Time
PRNT	Pass	11:59am

CRC Tests

Test	Status	Time
COMP	Pass	11:59am
CAL	Pass	11:59am

Preventive Maintenance
Status: Pass



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Wake Instrument Location Wake Co Detention Ctr
Instrument Serial No. 008651 3301 Hammond Rd
Raleigh, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 12 day of February, 2024 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Sam Adams
Signature of Certifying Official

662
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

WAKE COUNTY DETENTION CENTER 910

Serial Number: 008651

Test Date: 02/12/2024

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Barnes, Simon S

Permit Number: 0014-6221

Effective:

10/01/2023-10/01/2025

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG308703

Exp Date: 03/28/2025

Test	g/210L	Time
DIAG	Pass	2:25pm
AIR BLK	.00	2:26pm
ACCY CHK	.08	2:27pm
AIR BLK	.00	2:28pm
SUB TEST	.00	2:28pm
AIR BLK	.00	2:29pm
SUB TEST	.00	2:31pm
AIR BLK	.00	2:32pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

WAKE COUNTY DETENTION CENTER 910

Serial Number: 008651 Test Record Number: 1660
Test Date: 02/12/2024 Test Time: 2:32pm EST

System Check: Passed

Baseline Tests

Test	Status	Time
IR	Pass	2:32pm
FLO	Pass	2:32pm
FC	Pass	2:32pm

Temperature Tests

Test	Status	Time
FC1	Pass	2:33pm
SRC	Pass	2:33pm
DET	Pass	2:33pm
BAR	Pass	2:33pm
BT	Pass	2:33pm

Blank Tests

Test	Status	Time
AIR	Pass	2:33pm

Printer Tests

Test	Status	Time
PRNT	Pass	2:33pm

CRC Tests

Test	Status	Time
COMP	Pass	2:33pm
CAL	Pass	2:33pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County WAKE Instrument Location WAKE FOREST PD

Instrument Serial No. 008700 225 S. Taylor ST
WAKE FOREST, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 9 day of FEBRUARY, 2024 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

671
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

WAKE COUNTY WAKE FOREST PD 910

Serial Number: 008700

Test Date: 02/09/2024

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Bryant, Earl A

Permit Number: 0017-9707

Effective:

10/01/2023-10/01/2025

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG308003


Exp Date: 03/21/2025

Test	g/210L	Time
DIAG	Pass	3:12pm
AIR BLK	.00	3:13pm
ACCY CHK	.07	3:14pm
AIR BLK	.00	3:15pm
SUB TEST	.00	3:15pm
AIR BLK	.00	3:16pm
SUB TEST	.00	3:18pm
AIR BLK	.00	3:19pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

WAKE COUNTY WAKE FOREST PD 910

Serial Number: 008700 Test Record Number: 2327
Test Date: 02/09/2024 Test Time: 3:19pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	3:20pm
FLO	Pass	3:20pm
FC	Pass	3:20pm

Temperature Tests

Test	Status	Time
FC1	Pass	3:20pm
SRC	Pass	3:20pm
DET	Pass	3:20pm
BAR	Pass	3:20pm
BT	Pass	3:20pm

Blank Tests

Test	Status	Time
AIR	Pass	3:20pm

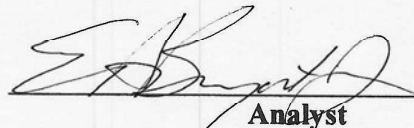
Printer Tests

Test	Status	Time
PRNT	Pass	3:21pm

CRC Tests

Test	Status	Time
COMP	Pass	3:21pm
CAL	Pass	3:21pm

Preventive Maintenance
Status: Pass


Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Wake Instrument Location Wake Co Detention Ctr
Instrument Serial No. 008760 3301 Hammond Rd Raleigh NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 21 day of February, 2024 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Simon Stokes Powers
Signature of Certifying Official

662
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

WAKE COUNTY DETENTION CENTER 910

Serial Number: 008760

Test Date: 02/21/2024

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Barnes, Simon S

Permit Number: 0014-6221

Effective:

10/01/2023-10/01/2025

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG308703

Exp Date: 03/28/2025

Test	g/210L	Time
DIAG	Pass	11:26am
AIR BLK	.00	11:27am
ACCY CHK	.07	11:27am
AIR BLK	.00	11:29am
SUB TEST	.00	11:29am
AIR BLK	.00	11:30am
SUB TEST	.00	11:32am
AIR BLK	.00	11:33am

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

This form is used when performing Preventive Maintenance procedures

Forensic Tests for Alcohol Branch

Department of Health and Human Services

Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

WAKE COUNTY DETENTION CENTER 910

Serial Number: 008760

Test Record Number: 6758

Test Date: 02/21/2024

Test Time: 11:33am EST

System Check: Passed

Baseline Tests

Test	Status	Time
IR	Pass	11:33am
FLO	Pass	11:33am
FC	Pass	11:33am

Temperature Tests

Test	Status	Time
FC1	Pass	11:34am
SRC	Pass	11:34am
DET	Pass	11:34am
BAR	Pass	11:34am
BT	Pass	11:34am

Blank Tests

Test	Status	Time
AIR	Pass	11:34am


Printer Tests

Test	Status	Time
PRNT	Pass	11:34am

CRC Tests

Test	Status	Time
COMP	Pass	11:34am
CAL	Pass	11:34am

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County LAKE Instrument Location KNIGHTDALE PD

Instrument Serial No. 008838 879 STEEPLE SQUARE CT

KNIGHTDALE, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 9 day of FEBRUARY, 20 24 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]

Signature of Certifying Official

671

Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

WAKE COUNTY KNIGHTDALE PD 910

Serial Number: 008838

Test Date: 02/09/2024

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Bryant, Earl A

Permit Number: 0017-9707

Effective:

10/01/2023-10/01/2025

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG308003

Exp Date: 03/21/2025

Test	g/210L	Time
DIAG	Pass	4:20pm
AIR BLK	.00	4:21pm
ACCY CHK	.07	4:21pm
AIR BLK	.00	4:22pm
SUB TEST	.00	4:23pm
AIR BLK	.00	4:24pm
SUB TEST	.00	4:25pm
AIR BLK	.00	4:26pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

WAKE COUNTY KNIGHTDALE PD 910

Serial Number: 008838 Test Record Number: 2649
Test Date: 02/09/2024 Test Time: 4:27pm EST

System Check: Passed

Baseline Tests

Test	Status	Time
IR	Pass	4:27pm
FLO	Pass	4:27pm
FC	Pass	4:27pm

Temperature Tests

Test	Status	Time
FC1	Pass	4:27pm
SRC	Pass	4:27pm
DET	Pass	4:27pm
BAR	Pass	4:27pm
BT	Pass	4:27pm

Blank Tests

Test	Status	Time
AIR	Pass	4:28pm


Printer Tests

Test	Status	Time
PRNT	Pass	4:28pm

CRC Tests

Test	Status	Time
COMP	Pass	4:28pm
CAL	Pass	4:28pm

Preventive Maintenance
Status: Pass



Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Wake Instrument Location Raleigh PD Northeast Dist
Instrument Serial No. 008839 5228 Green's Dairy Rd
Raleigh, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 9 day of February, 2024 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Simon Stokes Bures
Signature of Certifying Official

662
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

WAKE COUNTY NORTHEAST DIST 910

Serial Number: 008839
Test Date: 02/09/2024

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Barnes, Simon S

Permit Number: 0014-6221

Effective:

10/01/2023-10/01/2025

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG303102

Exp Date: 01/31/2025

Test	g/210L	Time
DIAG	Pass	2:32pm
AIR BLK	.00	2:32pm
ACCY CHK	.07	2:33pm
AIR BLK	.00	2:34pm
SUB TEST	.00	2:35pm
AIR BLK	.00	2:36pm
SUB TEST	.00	2:37pm
AIR BLK	.00	2:38pm

Reported AC: .00 g/210L

Simon Stokes Barnes
Signature of Chemical Analyst

Court CVR

Simon Stokes Barnes
Analyst

Intox EC/IR-II: Preventive Maintenance

WAKE COUNTY NORTHEAST DIST 910

Serial Number: 008839 Test Record Number: 2724
Test Date: 02/09/2024 Test Time: 2:38pm EST

System Check: Passed

Baseline Tests

Test	Status	Time
IR	Pass	2:39pm
FLO	Pass	2:39pm
FC	Pass	2:39pm

Temperature Tests

Test	Status	Time
FC1	Pass	2:39pm
SRC	Pass	2:39pm
DET	Pass	2:39pm
BAR	Pass	2:39pm
BT	Pass	2:39pm

Blank Tests

Test	Status	Time
AIR	Pass	2:40pm

Printer Tests

Test	Status	Time
PRNT	Pass	2:40pm

CRC Tests

Test	Status	Time
COMP	Pass	2:40pm
CAL	Pass	2:40pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County Wake Instrument Location Wake County
Instrument Serial No. 008863 Detention Center

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 25 day of February, 2024 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

675
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

WAKE COUNTY DETENTION CENTER 910

Serial Number: 008863

Test Date: 02/25/2024

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Garner, Joel K

Permit Number: 0036-5156

Effective:

10/01/2023-10/01/2025

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG308703

Exp Date: 03/28/2025

Test	g/210L	Time
DIAG	Pass	11:15am
AIR BLK	.00	11:15am
ACCY CHK	.07	11:16am
AIR BLK	.00	11:17am
SUB TEST	.00	11:18am
AIR BLK	.00	11:19am
SUB TEST	.00	11:20am
AIR BLK	.00	11:21am

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

WAKE COUNTY DETENTION CENTER 910

Serial Number: 008863 Test Record Number: 980
Test Date: 02/25/2024 Test Time: 11:21am EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	11:22am
FLO	Pass	11:22am
FC	Pass	11:22am

Temperature Tests

Test	Status	Time
FC1	Pass	11:22am
SRC	Pass	11:22am
DET	Pass	11:22am
BAR	Pass	11:22am
BT	Pass	11:22am

Blank Tests

Test	Status	Time
AIR	Pass	11:23am

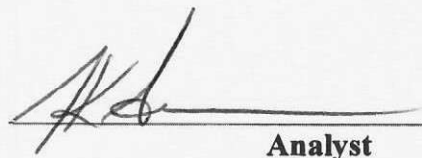
Printer Tests

Test	Status	Time
PRNT	Pass	11:23am

CRC Tests

Test	Status	Time
COMP	Pass	11:23am
CAL	Pass	11:23am

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Wake Instrument Location Wake County Detention Ctr
Instrument Serial No. 008924 3301 Hammond Rd
Raleigh, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 12 day of February, 2024 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Sam Adams Barnes
Signature of Certifying Official

662
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

WAKE COUNTY DETENTION CENTER 910

Serial Number: 008924

Test Date: 02/12/2024

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Barnes, Simon S

Permit Number: 0014-6221

Effective:

10/01/2023-10/01/2025

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG308703

Exp Date: 03/28/2025


Test	g/210L	Time
DIAG	Pass	2:18pm
AIR BLK	.00	2:19pm
ACCY CHK	.08	2:20pm
AIR BLK	.00	2:21pm
SUB TEST	.00	2:21pm
AIR BLK	.00	2:22pm
SUB TEST	.00	2:23pm
AIR BLK	.00	2:24pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

Intox EC/IR-II: Preventive Maintenance

WAKE COUNTY DETENTION CENTER 910

Serial Number: 008924 Test Record Number: 1888
Test Date: 02/12/2024 Test Time: 2:25pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	2:26pm
FLO	Pass	2:26pm
FC	Pass	2:26pm

Temperature Tests

Test	Status	Time
FC1	Pass	2:26pm
SRC	Pass	2:26pm
DET	Pass	2:26pm
BAR	Pass	2:26pm
BT	Pass	2:26pm

Blank Tests

Test	Status	Time
AIR	Pass	2:27pm

Printer Tests

Test	Status	Time
PRNT	Pass	2:27pm

CRC Tests

Test	Status	Time
COMP	Pass	2:27pm
CAL	Pass	2:27pm

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County WARREN Instrument Location WARREN CO. LEC
Instrument Serial No. 008738 128 RAFTERS LANE
WARRENTON, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 8 day of February, 20 24 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

671
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

WARREN COUNTY WARREN COUNTY JAIL 920

Serial Number: 008738

Test Date: 02/08/2024

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Bryant, Earl A

Permit Number: 0017-9707

Effective:

10/01/2023-10/01/2025

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG308702

Exp Date: 03/28/2025

Test	g/210L	Time
DIAG	Pass	4:04pm
AIR BLK	.00	4:05pm
ACCY CHK	.07	4:06pm
AIR BLK	.00	4:07pm
SUB TEST	.00	4:07pm
AIR BLK	.00	4:09pm
SUB TEST	.00	4:10pm
AIR BLK	.00	4:11pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

WARREN COUNTY WARREN COUNTY JAIL 920

Serial Number: 008738 Test Record Number: 1337
Test Date: 02/08/2024 Test Time: 4:12pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	4:12pm
FLO	Pass	4:12pm
FC	Pass	4:12pm

Temperature Tests

Test	Status	Time
FC1	Pass	4:12pm
SRC	Pass	4:12pm
DET	Pass	4:12pm
BAR	Pass	4:12pm
BT	Pass	4:12pm

Blank Tests

Test	Status	Time
AIR	Pass	4:13pm

Printer Tests

Test	Status	Time
PRNT	Pass	4:13pm

CRC Tests

Test	Status	Time
COMP	Pass	4:13pm
CAL	Pass	4:13pm

Preventive Maintenance
Status: Pass



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County WARREN Instrument Location WARREN Co. LEC
Instrument Serial No. 008793 128 RAFTERS LANE
WARRENTON, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 22 day of FEBRUARY, 20 24 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

671
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

WARREN COUNTY WARREN COUNTY JAIL 920

Serial Number: 008793

Test Date: 02/22/2024

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Bryant, Earl A

Permit Number: 0017-9707

Effective:

10/01/2023-10/01/2025

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG308702

Exp Date: 03/28/2025

Test	g/210L	Time
DIAG	Pass	2:07pm
AIR BLK	.00	2:08pm
ACCY CHK	.08	2:09pm
AIR BLK	.00	2:10pm
SUB TEST	.00	2:10pm
AIR BLK	.00	2:11pm
SUB TEST	.00	2:12pm
AIR BLK	.00	2:13pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

This form is used when performing Preventive Maintenance procedures

Forensic Tests for Alcohol Branch

Department of Health and Human Services

Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

WARREN COUNTY WARREN COUNTY JAIL 920

Serial Number: 008793 Test Record Number: 2118
Test Date: 02/22/2024 Test Time: 2:15pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	2:15pm
FLO	Pass	2:15pm
FC	Pass	2:15pm

Temperature Tests

Test	Status	Time
FC1	Pass	2:15pm
SRC	Pass	2:15pm
DET	Pass	2:15pm
BAR	Pass	2:15pm
BT	Pass	2:15pm

Blank Tests

Test	Status	Time
AIR	Pass	2:16pm

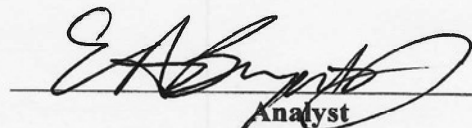
Printer Tests

Test	Status	Time
PRNT	Pass	2:16pm

CRC Tests

Test	Status	Time
COMP	Pass	2:16pm
CAL	Pass	2:16pm

Preventive Maintenance
Status: Pass



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Watauga Instrument Location Boone PD
Instrument Serial No. 008592 Boone, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 2 day of February, 2024 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

649
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

WATAUGA COUNTY BOONE P D 940

Serial Number: 008592

Test Date: 02/02/2024

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Burnette, Anthony J

Permit Number: 0018-4401

Effective:

10/01/2023-10/01/2025

Officer's Name: NONE,

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG308101

Exp Date: 03/22/2025

Test g/210L Time

DIAG Pass 3:22pm

AIR BLK .00 3:23pm

ACCY CHK .08 3:24pm

AIR BLK .00 3:25pm

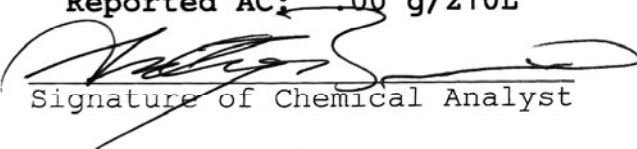
SUB TEST .00 3:25pm

AIR BLK .00 3:26pm

SUB TEST .00 3:27pm

AIR BLK .00 3:28pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

This form is used when performing Preventive Maintenance procedures

Forensic Tests for Alcohol Branch

Department of Health and Human Services

Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

WATAUGA COUNTY BOONE P D 940

Serial Number: 008592 Test Record Number: 5147
Test Date: 02/02/2024 Test Time: 3:29pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	3:30pm
FLO	Pass	3:30pm
FC	Pass	3:30pm

Temperature Tests

Test	Status	Time
FC1	Pass	3:30pm
SRC	Pass	3:30pm
DET	Pass	3:30pm
BAR	Pass	3:30pm
BT	Pass	3:30pm

Blank Tests

Test	Status	Time
AIR	Pass	3:31pm

Printer Tests

Test	Status	Time
PRNT	Pass	3:31pm

CRC Tests

Test	Status	Time
COMP	Pass	3:31pm
CAL	Pass	3:31pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Wayne Instrument Location Seymour Johnson AFB
Instrument Serial No. 008786 1010 Vermont Garrison St.,
Goldsboro, NC.

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 22nd day of February, 2024 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Kerry D. [Signature]
Signature of Certifying Official

643

Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

WAYNE COUNTY SEYMOUR JOHNSON AFB 950

Serial Number: 008786

Test Date: 02/22/2024

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Gray, Kelly D

Permit Number: 0037-7722

Effective:

10/01/2023-10/01/2025

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG308004

Exp Date: 03/21/2025

Test	g/210L	Time
DIAG	Pass	1:20pm
AIR BLK	.00	1:21pm
ACCY CHK	.08	1:21pm
AIR BLK	.00	1:22pm
SUB TEST	.00	1:24pm
AIR BLK	.00	1:24pm
SUB TEST	.00	1:26pm
AIR BLK	.00	1:27pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

WAYNE COUNTY SEYMOUR JOHNSON AFB 950

Serial Number: 008786 Test Record Number: 450
Test Date: 02/22/2024 Test Time: 1:28pm EST

System Check: Passed

Baseline Tests

Test	Status	Time
IR	Pass	1:29pm
FLO	Pass	1:29pm
FC	Pass	1:29pm

Temperature Tests

Test	Status	Time
FC1	Pass	1:29pm
SRC	Pass	1:29pm
DET	Pass	1:29pm
BAR	Pass	1:29pm
BT	Pass	1:29pm

Blank Tests

Test	Status	Time
AIR	Pass	1:30pm


Printer Tests

Test	Status	Time
PRNT	Pass	1:30pm

CRC Tests

Test	Status	Time
COMP	Pass	1:30pm
CAL	Pass	1:30pm

Preventive Maintenance
Status: Pass


Analyst