

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Brunswick Instrument Location BAT Mobile Unit 7
Instrument Serial No. 008002

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 22nd day of January, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

2266313
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

BRUNSWICK COUNTY BAT MOBILE UNIT 7 090

Serial Number: 008002
Test Date: 01/22/2026

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Sharpe Jr., Robert J

Permit Number: 1820-8591

Effective:

02/01/2025-02/01/2027

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG506303

Exp Date: 03/04/2027

Test	g/210L	Time
DIAG	Pass	1:11pm
AIR BLK	.00	1:11pm
ACCY CHK	.08	1:12pm
AIR BLK	.00	1:13pm
SUB TEST	.00	1:14pm
AIR BLK	.00	1:15pm
SUB TEST	.00	1:16pm
AIR BLK	.00	1:17pm

Reported AC: ~~.00 g/210L~~

Signature of Chemical Analyst

Court CVR


Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

BRUNSWICK COUNTY BAT MOBILE UNIT 7 090

Serial Number: 008002 Test Record Number: 869
Test Date: 01/22/2026 Test Time: 1:19pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	1:19pm
FLO	Pass	1:19pm
FC	Pass	1:19pm

Temperature Tests

Test	Status	Time
FC1	Pass	1:20pm
SRC	Pass	1:20pm
DET	Pass	1:20pm
BAR	Pass	1:20pm
BT	Pass	1:20pm

Blank Tests

Test	Status	Time
AIR	Pass	1:20pm


Printer Tests

Test	Status	Time
PRNT	Pass	1:20pm

CRC Tests

Test	Status	Time
COMP	Pass	1:20pm
CAL	Pass	1:20pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Brunswick Instrument Location BAT Mobile Unit 7

Instrument Serial No. 008090

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 22nd day of January, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

2266313
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

BRUNSWICK COUNTY BAT MOBILE UNIT 7 090

Serial Number: 008090

Test Date: 01/22/2026

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Sharpe Jr., Robert J

Permit Number: 1820-8591

Effective:

02/01/2025-02/01/2027

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG506303

Exp Date: 03/04/2027

Test	g/210L	Time
DIAG	Pass	1:25pm
AIR BLK	.00	1:26pm
ACCY CHK	.07	1:27pm
AIR BLK	.00	1:28pm
SUB TEST	.00	1:29pm
AIR BLK	.00	1:30pm
SUB TEST	.00	1:32pm
AIR BLK	.00	1:33pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

Intox EC/IR-II: Preventive Maintenance

BRUNSWICK COUNTY BAT MOBILE UNIT 7 090

Serial Number: 008090 Test Record Number: 254
Test Date: 01/22/2026 Test Time: 1:33pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	1:34pm
FLO	Pass	1:34pm
FC	Pass	1:34pm

Temperature Tests

Test	Status	Time
FC1	Pass	1:34pm
SRC	Pass	1:34pm
DET	Pass	1:34pm
BAR	Pass	1:34pm
BT	Pass	1:34pm

Blank Tests

Test	Status	Time
AIR	Pass	1:34pm

Printer Tests

Test	Status	Time
PRNT	Pass	1:35pm

CRC Tests

Test	Status	Time
COMP	Pass	1:35pm
CAL	Pass	1:35pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Buncombe Instrument Location BAT Mobile Unit 11

Instrument Serial No. 008970

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 15th day of January, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

62446
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

BUNCOMBE COUNTY BAT MOBILE UNIT 11 100

Serial Number: 008970
Test Date: 01/01/2026

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Gillstrap, Jeffrey L

Permit Number: 0006-2446

Effective:

04/01/2025-04/01/2027

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG417802

Exp Date: 06/26/2026

Test	g/210L	Time
DIAG	Pass	1:12am
AIR BLK	.00	1:13am
ACCY CHK	.07	1:14am
AIR BLK	.00	1:15am
SUB TEST	.00	1:15am
AIR BLK	.00	1:16am
SUB TEST	.00	1:18am
AIR BLK	.00	1:18am

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

BUNCOMBE COUNTY BAT MOBILE UNIT 11 100

Serial Number: 008970 Test Record Number: 1361
Test Date: 01/01/2026 Test Time: 1:19am EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	1:20am
FLO	Pass	1:20am
FC	Pass	1:20am

Temperature Tests

Test	Status	Time
FC1	Pass	1:20am
SRC	Pass	1:20am
DET	Pass	1:20am
BAR	Pass	1:20am
BT	Pass	1:20am

Blank Tests

Test	Status	Time
AIR	Pass	1:20am


Printer Tests

Test	Status	Time
PRNT	Pass	1:20am

CRC Tests

Test	Status	Time
COMP	Pass	1:21am
CAL	Pass	1:21am

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County Buncombe Instrument Location BAT Mobile Unit 11

Instrument Serial No. 008973

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 1st day of January, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

62446
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

BUNCOMBE COUNTY BAT MOBILE UNIT 11 100

Serial Number: 008973
Test Date: 01/01/2026

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Gillstrap, Jeffrey L

Permit Number: 0006-2446

Effective:

04/01/2025-04/01/2027

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG431003

Exp Date: 11/05/2026

Test	g/210L	Time
DIAG	Pass	1:16am
AIR BLK	.00	1:17am
ACCY CHK	.07	1:17am
AIR BLK	.00	1:18am
SUB TEST	.00	1:19am
AIR BLK	.00	1:20am
SUB TEST	.00	1:21am
AIR BLK	.00	1:22am

Reported AC: .00 g/210L

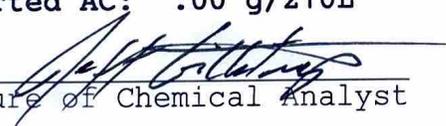

Signature of Chemical Analyst

Court CVR



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

BUNCOMBE COUNTY BAT MOBILE UNIT 11 100

Serial Number: 008973 Test Record Number: 1412
Test Date: 01/01/2026 Test Time: 1:23am EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	1:23am
FLO	Pass	1:23am
FC	Pass	1:23am

Temperature Tests

Test	Status	Time
FC1	Pass	1:24am
SRC	Pass	1:24am
DET	Pass	1:24am
BAR	Pass	1:24am
BT	Pass	1:24am

Blank Tests

Test	Status	Time
AIR	Pass	1:24am

Printer Tests

Test	Status	Time
PRNT	Pass	1:24am

CRC Tests

Test	Status	Time
COMP	Pass	1:24am
CAL	Pass	1:24am

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County Burke Instrument Location Burke County Jail


Instrument Serial No. 008831 Morganton, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 20 day of January, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



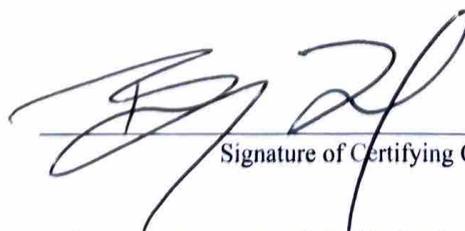

Signature of Certifying Official

244987

Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

BURKE COUNTY BURKE COUNTY JAIL 110

Serial Number: 008831
Test Date: 01/20/2026

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: Loftis, Benjamin C
Permit Number: 0024-4987
Effective:
03/01/2025-03/01/2027

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG417803
Exp Date: 06/26/2026


Test	g/210L	Time
DIAG	Pass	12:21pm
AIR BLK	.00	12:22pm
ACCY CHK	.08	12:23pm
AIR BLK	.00	12:24pm
SUB TEST	.00	12:25pm
AIR BLK	.00	12:26pm
SUB TEST	.00	12:27pm
AIR BLK	.00	12:28pm

~~Reported AC: .00 g/210L~~

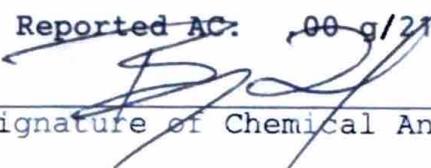

Signature of Chemical Analyst

Court CVR

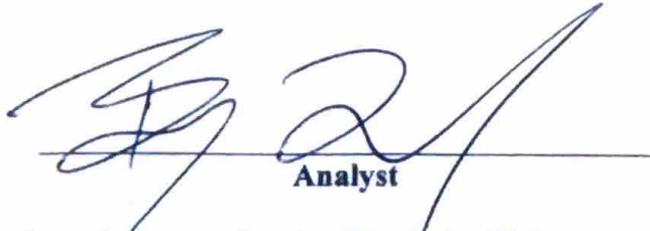

Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

BURKE COUNTY BURKE COUNTY JAIL 110

Serial Number: 008831 Test Record Number: 3140
Test Date: 01/20/2026 Test Time: 12:31pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	12:31pm
FLO	Pass	12:31pm
FC	Pass	12:31pm

Temperature Tests

Test	Status	Time
FC1	Pass	12:32pm
SRC	Pass	12:32pm
DET	Pass	12:32pm
BAR	Pass	12:32pm
BT	Pass	12:32pm

Blank Tests

Test	Status	Time
AIR	Pass	12:32pm

Printer Tests

Test	Status	Time
PRNT	Pass	12:32pm

CRC Tests

Test	Status	Time
COMP	Pass	12:32pm
CAL	Pass	12:32pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County Burke Instrument Location Burke County Jail

Instrument Serial No. 008904 Morganton, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 20 day of January, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

244987
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

BURKE COUNTY BURKE COUNTY JAIL 110

Serial Number: 008904

Test Date: 01/20/2026

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Loftis, Benjamin C

Permit Number: 0024-4987

Effective:

03/01/2025-03/01/2027

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG417803

Exp Date: 06/26/2026

Test	g/210L	Time
DIAG	Pass	12:22pm
AIR BLK	.00	12:23pm
ACCY CHK	.08	12:24pm
AIR BLK	.00	12:25pm
SUB TEST	.00	12:25pm
AIR BLK	.00	12:26pm
SUB TEST	.00	12:28pm
AIR BLK	.00	12:29pm

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR

Analyst

Intox EC/IR-II: Preventive Maintenance

BURKE COUNTY BURKE COUNTY JAIL 110

Serial Number: 008904 Test Record Number: 3652
Test Date: 01/20/2026 Test Time: 12:31pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	12:32pm
FLO	Pass	12:32pm
FC	Pass	12:32pm

Temperature Tests

Test	Status	Time
FC1	Pass	12:32pm
SRC	Pass	12:32pm
DET	Pass	12:32pm
BAR	Pass	12:32pm
BT	Pass	12:32pm

Blank Tests

Test	Status	Time
AIR	Pass	12:33pm


Printer Tests

Test	Status	Time
PRNT	Pass	12:33pm

CRC Tests

Test	Status	Time
COMP	Pass	12:33pm
CAL	Pass	12:33pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Cabarrus Instrument Location BAT Mobile Unit 8

Instrument Serial No. 008615

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 19 day of January, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

2219283
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

CABARRUS COUNTY BAT MOBILE UNIT 8 120

Serial Number: 008615
Test Date: 01/19/2026

Citation Number: M0000000-0
Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Glasscock, Jerry D

Permit Number: 7180-9235

Effective:

02/01/2025-02/01/2027

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG405102

Exp Date: 02/20/2026

Test	g/210L	Time
DIAG	Pass	1:17pm
AIR BLK	.00	1:18pm
ACCY CHK	.07	1:19pm
AIR BLK	.00	1:20pm
SUB TEST	.00	1:20pm
AIR BLK	.00	1:21pm
SUB TEST	.00	1:23pm
AIR BLK	.00	1:24pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

Intox EC/IR-II: Preventive Maintenance

CABARRUS COUNTY BAT MOBILE UNIT 8 120

Serial Number: 008615 Test Record Number: 6227
Test Date: 01/19/2026 Test Time: 1:24pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	1:25pm
FLO	Pass	1:25pm
FC	Pass	1:25pm

Temperature Tests

Test	Status	Time
FC1	Pass	1:25pm
SRC	Pass	1:25pm
DET	Pass	1:25pm
BAR	Pass	1:25pm
BT	Pass	1:25pm

Blank Tests

Test	Status	Time
AIR	Pass	1:25pm

Printer Tests

Test	Status	Time
PRNT	Pass	1:25pm

CRC Tests

Test	Status	Time
COMP	Pass	1:26pm
CAL	Pass	1:26pm

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Cabarrus Instrument Location BAT Mobile Unit 8

Instrument Serial No. 008615

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 27 day of January, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

2219283
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

CABARRUS COUNTY BAT MOBILE UNIT 8 120

Serial Number: 008615

Test Date: 01/27/2026

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Glasscock, Jerry D

Permit Number: 7180-9235

Effective:

02/01/2025-02/01/2027

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG405102

Exp Date: 02/20/2026

Test	g/210L	Time
DIAG	Pass	8:20pm
AIR BLK	.00	8:22pm
ACCY CHK	.07	8:23pm
AIR BLK	.00	8:23pm
SUB TEST	.00	8:25pm
AIR BLK	.00	8:26pm
SUB TEST	.00	8:27pm
AIR BLK	.00	8:28pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

Intox EC/IR-II: Preventive Maintenance

CABARRUS COUNTY BAT MOBILE UNIT 8 120

Serial Number: 008615 Test Record Number: 6233
Test Date: 01/27/2026 Test Time: 8:29pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	8:29pm
FLO	Pass	8:29pm
FC	Pass	8:29pm

Temperature Tests

Test	Status	Time
FC1	Pass	8:29pm
SRC	Pass	8:29pm
DET	Pass	8:29pm
BAR	Pass	8:29pm
BT	Pass	8:29pm

Blank Tests

Test	Status	Time
AIR	Pass	8:30pm

Printer Tests

Test	Status	Time
PRNT	Pass	8:30pm

CRC Tests

Test	Status	Time
COMP	Pass	8:30pm
CAL	Pass	8:30pm

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Cabarrus Instrument Location BAT Mobile Unit 8

Instrument Serial No. 008736 _____

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 19 day of January, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

2219283
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

CABARRUS COUNTY BAT MOBILE UNIT 8 120

Serial Number: 008736

Test Date: 01/19/2026

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Glasscock, Jerry D

Permit Number: 7180-9235

Effective:

02/01/2025-02/01/2027

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG405102

Exp Date: 02/20/2026

Test	g/210L	Time
DIAG	Pass	1:15pm
AIR BLK	.00	1:16pm
ACCY CHK	.07	1:17pm
AIR BLK	.00	1:18pm
SUB TEST	.00	1:19pm
AIR BLK	.00	1:20pm
SUB TEST	.00	1:22pm
AIR BLK	.00	1:22pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

Intox EC/IR-II: Preventive Maintenance

CABARRUS COUNTY BAT MOBILE UNIT 8 120

Serial Number: 008736 Test Record Number: 1585
Test Date: 01/19/2026 Test Time: 1:24pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	1:25pm
FLO	Pass	1:25pm
FC	Pass	1:25pm

Temperature Tests

Test	Status	Time
FC1	Pass	1:25pm
SRC	Pass	1:25pm
DET	Pass	1:25pm
BAR	Pass	1:25pm
BT	Pass	1:25pm

Blank Tests

Test	Status	Time
AIR	Pass	1:26pm

Printer Tests

Test	Status	Time
PRNT	Pass	1:26pm

CRC Tests

Test	Status	Time
COMP	Pass	1:26pm
CAL	Pass	1:26pm

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Cabarrus Instrument Location BAT Mobile Unit 8
Instrument Serial No. 008736 —

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 27 day of January, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

2219283
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

CABARRUS COUNTY BAT MOBILE UNIT 8 120

Serial Number: 008736
Test Date: 01/27/2026

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: Glasscock, Jerry D
Permit Number: 7180-9235
Effective:
02/01/2025-02/01/2027

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG405102
Exp Date: 02/20/2026

Test	g/210L	Time
DIAG	Pass	8:21pm
AIR BLK	.00	8:22pm
ACCY CHK	.07	8:23pm
AIR BLK	.00	8:24pm
SUB TEST	.00	8:25pm
AIR BLK	.00	8:26pm
SUB TEST	.00	8:27pm
AIR BLK	.00	8:28pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

Intox EC/IR-II: Preventive Maintenance

CABARRUS COUNTY BAT MOBILE UNIT 8 120

Serial Number: 008736 Test Record Number: 1589
Test Date: 01/27/2026 Test Time: 8:29pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	8:29pm
FLO	Pass	8:29pm
FC	Pass	8:29pm

Temperature Tests

Test	Status	Time
FC1	Pass	8:29pm
SRC	Pass	8:29pm
DET	Pass	8:29pm
BAR	Pass	8:29pm
BT	Pass	8:29pm

Blank Tests

Test	Status	Time
AIR	Pass	8:30pm

Printer Tests

Test	Status	Time
PRNT	Pass	8:30pm

CRC Tests

Test	Status	Time
COMP	Pass	8:30pm
CAL	Pass	8:30pm

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Cabarrus Instrument Location BAT Mobile Unit 8

Instrument Serial No. 008775

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 19 day of January, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

2219283
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

CABARRUS COUNTY BAT MOBILE UNIT 8 120

Serial Number: 008775
Test Date: 01/19/2026

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE

Analyst's Name: *Glasscock, Jerry D*
Permit Number: 7180-9235
Effective:
02/01/2025-02/01/2027

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: *Breath Test*

Lot Number: AG506303
Exp Date: 03/04/2027

Test	g/210L	Time
DIAG	Pass	1:14pm
AIR BLK	.00	1:15pm
ACCY CHK	.08	1:16pm
AIR BLK	.00	1:17pm
SUB TEST	.00	1:17pm
AIR BLK	.00	1:18pm
SUB TEST	.00	1:20pm
AIR BLK	.00	1:21pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

Intox EC/IR-II: Preventive Maintenance

CABARRUS COUNTY BAT MOBILE UNIT 8 120

Serial Number: 008775 Test Record Number: 2439
Test Date: 01/19/2026 Test Time: 1:21pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	1:22pm
FLO	Pass	1:22pm
FC	Pass	1:22pm

Temperature Tests

Test	Status	Time
FC1	Pass	1:22pm
SRC	Pass	1:22pm
DET	Pass	1:22pm
BAR	Pass	1:22pm
BT	Pass	1:22pm

Blank Tests

Test	Status	Time
AIR	Pass	1:22pm

Printer Tests

Test	Status	Time
PRNT	Pass	1:22pm

CRC Tests

Test	Status	Time
COMP	Pass	1:23pm
CAL	Pass	1:23pm

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Cabarrus Instrument Location BAT Mobile Unit 3
Instrument Serial No. 008775 _____

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 27 day of January, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

2219283
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

CABARRUS COUNTY BAT MOBILE UNIT 8 120

Serial Number: 008775
Test Date: 01/27/2026

Citation Number: M0000000-0
Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Glasscock, Jerry D

Permit Number: 7180-9235

Effective:

02/01/2025-02/01/2027

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG506303

Exp Date: 03/04/2027

Test	g/210L	Time
DIAG	Pass	8:22pm
AIR BLK	.00	8:23pm
ACCY CHK	.08	8:23pm
AIR BLK	.00	8:24pm
SUB TEST	.00	8:25pm
AIR BLK	.00	8:26pm
SUB TEST	.00	8:27pm
AIR BLK	.00	8:28pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

Intox EC/IR-II: Preventive Maintenance

CABARRUS COUNTY BAT MOBILE UNIT 8 120

Serial Number: 008775 Test Record Number: 2443
Test Date: 01/27/2026 Test Time: 8:29pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	8:29pm
FLO	Pass	8:29pm
FC	Pass	8:29pm

Temperature Tests

Test	Status	Time
FC1	Pass	8:30pm
SRC	Pass	8:30pm
DET	Pass	8:30pm
BAR	Pass	8:30pm
BT	Pass	8:30pm

Blank Tests

Test	Status	Time
AIR	Pass	8:30pm

Printer Tests

Test	Status	Time
PRNT	Pass	8:30pm

CRC Tests

Test	Status	Time
COMP	Pass	8:30pm
CAL	Pass	8:30pm

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Cabarrus Instrument Location Cabarrus County SO
Instrument Serial No. 008792 Concord, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 30th day of January, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Handwritten Signature]
Signature of Certifying Official

849845
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

CABARRUS COUNTY CABARRUS COUNTY SO 120

Serial Number: 008792
Test Date: 01/30/2026

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE

Analyst's Name: Helms, Bryce A
Permit Number: 0084-9845
Effective:
02/01/2025-02/01/2027

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG516204
Exp Date: 06/11/2027


Test	g/210L	Time
DIAG	Pass	10:50am
AIR BLK	.00	10:51am
ACCY CHK	.08	10:51am
AIR BLK	.00	10:53am
SUB TEST	.00	10:54am
AIR BLK	.00	10:55am
SUB TEST	.00	10:56am
AIR BLK	.00	10:57am

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR

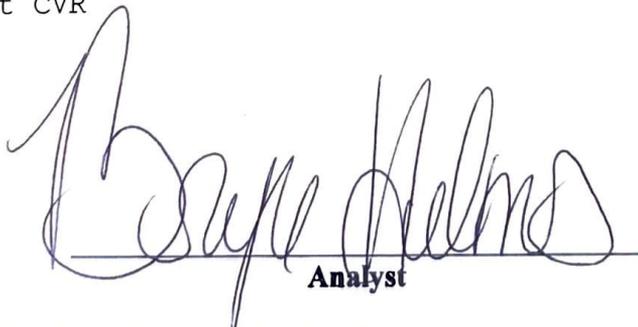

Analyst

Intox EC/IR-II: Preventive Maintenance

CABARRUS COUNTY CABARRUS COUNTY SO 120

Serial Number: 008792 Test Record Number: 4763
Test Date: 01/30/2026 Test Time: 10:58am EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	10:58am
FLO	Pass	10:58am
FC	Pass	10:59am

Temperature Tests

Test	Status	Time
FC1	Pass	10:59am
SRC	Pass	10:59am
DET	Pass	10:59am
BAR	Pass	10:59am
BT	Pass	10:59am

Blank Tests

Test	Status	Time
AIR	Pass	10:59am

Printer Tests

Test	Status	Time
PRNT	Pass	10:59am

CRC Tests

Test	Status	Time
COMP	Pass	11:00am
CAL	Pass	11:00am

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Cabarrus Instrument Location BAT Mobile Unit 8

Instrument Serial No. 008816

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 19 day of January, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

2219283
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

CABARRUS COUNTY BAT MOBILE UNIT 8 120

Serial Number: 008816
Test Date: 01/19/2026

Citation Number: M0000000-0
Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Glasscock, Jerry D

Permit Number: 7180-9235

Effective:

02/01/2025-02/01/2027

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG431002

Exp Date: 11/05/2026

Test	g/210L	Time
DIAG	Pass	1:13pm
AIR BLK	.00	1:14pm
ACCY CHK	.08	1:15pm
AIR BLK	.00	1:16pm
SUB TEST	.00	1:16pm
AIR BLK	.00	1:17pm
SUB TEST	.00	1:19pm
AIR BLK	.00	1:20pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

Intox EC/IR-II: Preventive Maintenance

CABARRUS COUNTY BAT MOBILE UNIT 8 120

Serial Number: 008816 Test Record Number: 8021
Test Date: 01/19/2026 Test Time: 1:21pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	1:21pm
FLO	Pass	1:21pm
FC	Pass	1:21pm

Temperature Tests

Test	Status	Time
FC1	Pass	1:22pm
SRC	Pass	1:22pm
DET	Pass	1:22pm
BAR	Pass	1:22pm
BT	Pass	1:22pm

Blank Tests

Test	Status	Time
AIR	Pass	1:22pm

Printer Tests

Test	Status	Time
PRNT	Pass	1:22pm

CRC Tests

Test	Status	Time
COMP	Pass	1:22pm
CAL	Pass	1:22pm

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Cabarrus Instrument Location BAT Mobile Unit 8

Instrument Serial No. 008816 —

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 27 day of January, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Jerry D. Blumhardt
Signature of Certifying Official

2219283
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

CABARRUS COUNTY BAT MOBILE UNIT 8 120

Serial Number: 008816
Test Date: 01/27/2026

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: Glasscock, Jerry D
Permit Number: 7180-9235
Effective:
02/01/2025-02/01/2027

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG431002
Exp Date: 11/05/2026

Test	g/210L	Time
DIAG	Pass	8:22pm
AIR BLK	.00	8:23pm
ACCY CHK	.08	8:24pm
AIR BLK	.00	8:25pm
SUB TEST	.00	8:26pm
AIR BLK	.00	8:26pm
SUB TEST	.00	8:28pm
AIR BLK	.00	8:29pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

Intox EC/IR-II: Preventive Maintenance

CABARRUS COUNTY BAT MOBILE UNIT 8 120

Serial Number: 008816 Test Record Number: 8025
Test Date: 01/27/2026 Test Time: 8:29pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	8:29pm
FLO	Pass	8:29pm
FC	Pass	8:29pm

Temperature Tests

Test	Status	Time
FC1	Pass	8:30pm
SRC	Pass	8:30pm
DET	Pass	8:30pm
BAR	Pass	8:30pm
BT	Pass	8:30pm

Blank Tests

Test	Status	Time
AIR	Pass	8:30pm

Printer Tests

Test	Status	Time
PRNT	Pass	8:30pm

CRC Tests

Test	Status	Time
COMP	Pass	8:30pm
CAL	Pass	8:30pm

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Cabarrus Instrument Location BAT Mobile Unit 8
Instrument Serial No. 008929 _____

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 19 day of January, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

2219283
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

CABARRUS COUNTY BAT MOBILE UNIT 8 120

Serial Number: 008929

Test Date: 01/19/2026

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Glasscock, Jerry D

Permit Number: 7180-9235

Effective:

02/01/2025-02/01/2027

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG506303


Exp Date: 03/04/2027

Test	g/210L	Time
DIAG	Pass	1:12pm
AIR BLK	.00	1:13pm
ACCY CHK	.08	1:14pm
AIR BLK	.00	1:15pm
SUB TEST	.00	1:16pm
AIR BLK	.00	1:17pm
SUB TEST	.00	1:19pm
AIR BLK	.00	1:21pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR

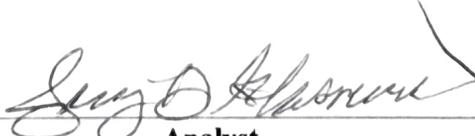
Analyst

Intox EC/IR-II: Preventive Maintenance

CABARRUS COUNTY BAT MOBILE UNIT 8 120

Serial Number: 008929 Test Record Number: 1722
Test Date: 01/19/2026 Test Time: 1:21pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	1:21pm
FLO	Pass	1:21pm
FC	Pass	1:22pm

Temperature Tests

Test	Status	Time
FC1	Pass	1:22pm
SRC	Pass	1:22pm
DET	Pass	1:22pm
BAR	Pass	1:22pm
BT	Pass	1:22pm

Blank Tests

Test	Status	Time
AIR	Pass	1:22pm

Printer Tests

Test	Status	Time
PRNT	Pass	1:22pm

CRC Tests

Test	Status	Time
COMP	Pass	1:23pm
CAL	Pass	1:23pm

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Cabarrus Instrument Location BAT Mobile Unit 8

Instrument Serial No. 008929 —

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 27 day of January, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

2219283
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

CABARRUS COUNTY BAT MOBILE UNIT 8 120

Serial Number: 008929
Test Date: 01/27/2026

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE

Analyst's Name: Glasscock, Jerry D
Permit Number: 7180-9235
Effective:
02/01/2025-02/01/2027

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test


Lot Number: AG506303
Exp Date: 03/04/2027

Test	g/210L	Time
DIAG	Pass	8:23pm
AIR BLK	.00	8:24pm
ACCY CHK	.08	8:25pm
AIR BLK	.00	8:26pm
SUB TEST	.00	8:27pm
AIR BLK	.00	8:28pm
SUB TEST	.00	8:29pm
AIR BLK	.00	8:30pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

Intox EC/IR-II: Preventive Maintenance

CABARRUS COUNTY BAT MOBILE UNIT 8 120

Serial Number: 008929 Test Record Number: 1726

Test Date: 01/27/2026 Test Time: 8:33pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	8:34pm
FLO	Pass	8:34pm
FC	Pass	8:34pm

Temperature Tests

Test	Status	Time
FC1	Pass	8:34pm
SRC	Pass	8:34pm
DET	Pass	8:34pm
BAR	Pass	8:34pm
BT	Pass	8:34pm

Blank Tests

Test	Status	Time
AIR	Pass	8:35pm

Printer Tests

Test	Status	Time
PRNT	Pass	8:35pm

CRC Tests

Test	Status	Time
COMP	Pass	8:35pm
CAL	Pass	8:35pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Caswell Instrument Location Caswell Co Detention Ctr
Instrument Serial No. 008593 211 County Park Dr
Yanceyville, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 9 day of January, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Sam Stokes Barnes
Signature of Certifying Official

146221
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

CASWELL COUNTY DETENTION CENTER 160

Serial Number: 008593
Test Date: 01/09/2026

Citation Number: M0000000-0
Subject's Name: MONTHLY, INSPECTION
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: Barnes, Simon S
Permit Number: 0014-6221
Effective:
02/01/2025-02/01/2027

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG534301
Exp Date: 12/09/2027

Test	g/210L	Time
DIAG	Pass	1:34pm
AIR BLK	.00	1:35pm
ACCY CHK	.07	1:36pm
AIR BLK	.00	1:36pm
SUB TEST	.00	1:37pm
AIR BLK	.00	1:38pm
SUB TEST	.00	1:39pm
AIR BLK	.00	1:40pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

CASWELL COUNTY DETENTION CENTER 160

Serial Number: 008593 Test Record Number: 2441
Test Date: 01/09/2026 Test Time: 1:41pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	1:41pm
FLO	Pass	1:41pm
FC	Pass	1:41pm

Temperature Tests

Test	Status	Time
FC1	Pass	1:41pm
SRC	Pass	1:41pm
DET	Pass	1:41pm
BAR	Pass	1:41pm
BT	Pass	1:41pm

Blank Tests

Test	Status	Time
AIR	Pass	1:42pm

Printer Tests

Test	Status	Time
PRNT	Pass	1:42pm

CRC Tests

Test	Status	Time
COMP	Pass	1:42pm
CAL	Pass	1:42pm

Preventive Maintenance
Status: Pass



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County CHATHAM Instrument Location CHATHAM COUNTY
Instrument Serial No. 008591 DETENTION CENTER

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 8 day of JANUARY, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

239771
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

CHATHAM COUNTY DETENTION CENTER 180

Serial Number: 008591
Test Date: 01/08/2026

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: Galloway, Charles L
Permit Number: 0023-9771
Effective:
02/01/2025-02/01/2027

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG516204
Exp Date: 06/11/2027

Test	g/210L	Time
DIAG	Pass	10:42am
AIR BLK	.00	10:42am
ACCY CHK	.08	10:43am
AIR BLK	.00	10:44am
SUB TEST	.00	10:46am
AIR BLK	.00	10:47am
SUB TEST	.00	10:48am
AIR BLK	.00	10:49am

Reported AC: .00 g/210L

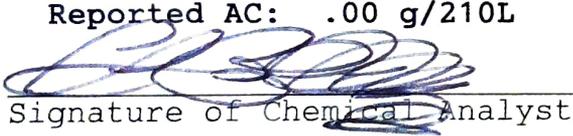
Signature of Chemical Analyst

Court CVR


Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

CHATHAM COUNTY DETENTION CENTER 180

Serial Number: 008591 Test Record Number: 3393
Test Date: 01/08/2026 Test Time: 10:50am EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	10:50am
FLO	Pass	10:50am
FC	Pass	10:50am

Temperature Tests

Test	Status	Time
FC1	Pass	10:51am
SRC	Pass	10:51am
DET	Pass	10:51am
BAR	Pass	10:51am
BT	Pass	10:51am

Blank Tests

Test	Status	Time
AIR	Pass	10:51am

Printer Tests

Test	Status	Time
PRNT	Pass	10:51am

CRC Tests

Test	Status	Time
COMP	Pass	10:52am
CAL	Pass	10:52am

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County CHATHAM Instrument Location SILER CITY
Instrument Serial No. 008811 POLICE DEPARTMENT

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 8 day of JANUARY, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

239771
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

CHATHAM COUNTY SILER CITY PD 180

Serial Number: 008811
Test Date: 01/08/2026

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Galloway, Charles L

Permit Number: 0023-9771

Effective:

02/01/2025-02/01/2027

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG516204


Exp Date: 06/11/2027

Test	g/210L	Time
DIAG	Pass	12:20pm
AIR BLK	.00	12:21pm
ACCY CHK	.08	12:21pm
AIR BLK	.00	12:23pm
SUB TEST	.00	12:23pm
AIR BLK	.00	12:24pm
SUB TEST	.00	12:25pm
AIR BLK	.00	12:26pm

Reported AC: .00 g/210L

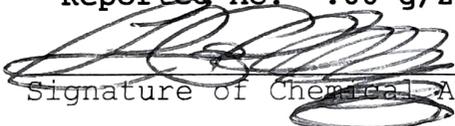
Signature of Chemical Analyst

Court CVR

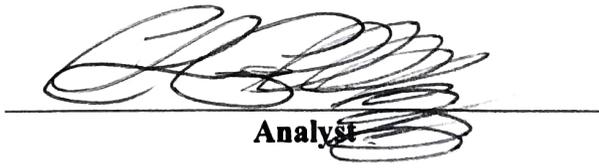
Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

CHATHAM COUNTY SILER CITY PD 180

Serial Number: 008811 Test Record Number: 1883
Test Date: 01/08/2026 Test Time: 12:27pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	12:28pm
FLO	Pass	12:28pm
FC	Pass	12:28pm

Temperature Tests

Test	Status	Time
FC1	Pass	12:28pm
SRC	Pass	12:28pm
DET	Pass	12:28pm
BAR	Pass	12:28pm
BT	Pass	12:28pm

Blank Tests

Test	Status	Time
AIR	Pass	12:29pm

Printer Tests

Test	Status	Time
PRNT	Pass	12:29pm

CRC Tests

Test	Status	Time
COMP	Pass	12:29pm
CAL	Pass	12:29pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Cherokee Instrument Location Cherokee Co. Jail

Instrument Serial No. 008622 Murphy, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 6 day of January, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



David R. Cuth
Signature of Certifying Official

843310
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

CHEROKEE COUNTY CHEROKEE COUNTY JAIL
190

Serial Number: 008622
Test Date: 01/06/2026

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Cutler, Daniel R

Permit Number: 0084-3310

Effective:

02/01/2025-02/01/2027

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG505001

Exp Date: 02/19/2027

Test	g/210L	Time
DIAG	Pass	1:25pm
AIR BLK	.00	1:26pm
ACCY CHK	.07	1:26pm
AIR BLK	.00	1:28pm
SUB TEST	.00	1:28pm
AIR BLK	.00	1:29pm
SUB TEST	.00	1:31pm
AIR BLK	.00	1:31pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

CHEROKEE COUNTY CHEROKEE COUNTY JAIL 190

Serial Number: 008622 Test Record Number: 1340
Test Date: 01/06/2026 Test Time: 1:32pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	1:32pm
FLO	Pass	1:32pm
FC	Pass	1:32pm

Temperature Tests

Test	Status	Time
FC1	Pass	1:33pm
SRC	Pass	1:33pm
DET	Pass	1:33pm
BAR	Pass	1:33pm
BT	Pass	1:33pm

Blank Tests

Test	Status	Time
AIR	Pass	1:33pm

Printer Tests

Test	Status	Time
PRNT	Pass	1:33pm

CRC Tests

Test	Status	Time
COMP	Pass	1:33pm
CAL	Pass	1:33pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Cherokee Instrument Location Cherokee Co. Jail
Instrument Serial No. 008711 Murphy, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 6 day of January, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



David R. Luthin
Signature of Certifying Official

843310
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

CHEROKEE COUNTY CHEROKEE COUNTY JAIL
190

Serial Number: 008711
Test Date: 01/06/2026

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: Cutler, Daniel R
Permit Number: 0084-3310
Effective:
02/01/2025-02/01/2027

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG503001
Exp Date: 01/30/2027

Test	g/210L	Time
DIAG	Pass	1:24pm
AIR BLK	.00	1:25pm
ACCY CHK	.07	1:26pm
AIR BLK	.00	1:27pm
SUB TEST	.00	1:27pm
AIR BLK	.00	1:28pm
SUB TEST	.00	1:30pm
AIR BLK	.00	1:31pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

Intox EC/IR-II: Preventive Maintenance

CHEROKEE COUNTY CHEROKEE COUNTY JAIL 190

Serial Number: 008711 Test Record Number: 1569
Test Date: 01/06/2026 Test Time: 1:32pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	1:32pm
FLO	Pass	1:32pm
FC	Pass	1:32pm

Temperature Tests

Test	Status	Time
FC1	Pass	1:32pm
SRC	Pass	1:32pm
DET	Pass	1:32pm
BAR	Pass	1:32pm
BT	Pass	1:32pm

Blank Tests

Test	Status	Time
AIR	Pass	1:33pm


Printer Tests

Test	Status	Time
PRNT	Pass	1:33pm

CRC Tests

Test	Status	Time
COMP	Pass	1:33pm
CAL	Pass	1:33pm

Preventive Maintenance
Status: Pass

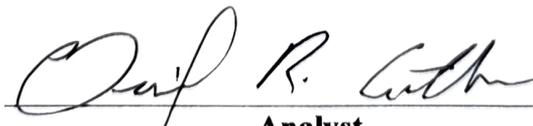

Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Chowan Instrument Location Chowan Co. Public Safety Center
Instrument Serial No. 008895 305 Freemason St. Edenton, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 9th day of January, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Mark A. Trappell
Signature of Certifying Official

206272
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

CHOWAN COUNTY PUBLIC SAFETY CENTER 200

Serial Number: 008895
Test Date: 01/09/2026

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE

Analyst's Name: *Chappell, Mark A*
Permit Number: 0020-6272
Effective:
02/01/2025-02/01/2027

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: *Breath Test*

Lot Number: AG431001
Exp Date: 11/05/2026


Test	g/210L	Time
DIAG	Pass	9:47am
AIR BLK	.00	9:48am
ACCY CHK	.07	9:49am
AIR BLK	.00	9:50am
SUB TEST	.00	9:50am
AIR BLK	.00	9:51am
SUB TEST	.00	9:53am
AIR BLK	.00	9:54am

Reported AC: **.00** g/210L



Signature of Chemical Analyst

Court CVR

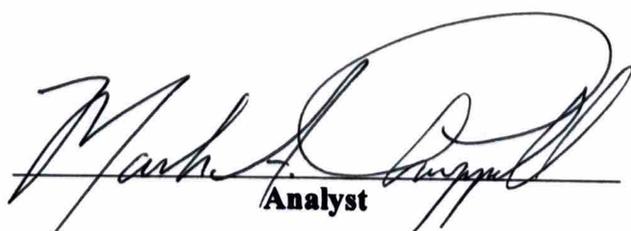

Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

CHOWAN COUNTY PUBLIC SAFETY CENTER 200

Serial Number: 008895 Test Record Number: 1296
Test Date: 01/09/2026 Test Time: 9:55am EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	9:55am
FLO	Pass	9:55am
FC	Pass	9:55am

Temperature Tests

Test	Status	Time
FC1	Pass	9:55am
SRC	Pass	9:55am
DET	Pass	9:55am
BAR	Pass	9:55am
BT	Pass	9:55am

Blank Tests

Test	Status	Time
AIR	Pass	9:56am


Printer Tests

Test	Status	Time
PRNT	Pass	9:56am

CRC Tests

Test	Status	Time
COMP	Pass	9:56am
CAL	Pass	9:56am

Preventive Maintenance
Status: Pass

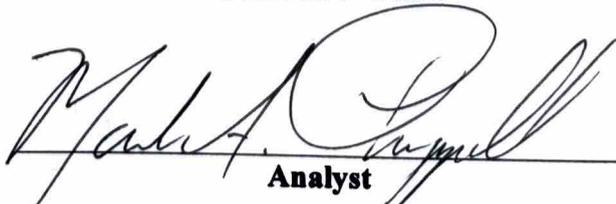
Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County Clay Instrument Location Clay Co. Jail
Instrument Serial No. 008608 Hayesville, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 6 day of January, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Carol R. Cuth

Signature of Certifying Official

843310

Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

CLAY COUNTY CLAY COUNTY JAIL 210

Serial Number: 008608
Test Date: 01/06/2026

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE

Analyst's Name: Cutler, Daniel R
Permit Number: 0084-3310
Effective:
02/01/2025-02/01/2027

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG431002
Exp Date: 11/05/2026

Test	g/210L	Time
DIAG	Pass	2:44pm
AIR BLK	.00	2:45pm
ACCY CHK	.07	2:46pm
AIR BLK	.00	2:47pm
SUB TEST	.00	2:48pm
AIR BLK	.00	2:49pm
SUB TEST	.00	2:50pm
AIR BLK	.00	2:51pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

Intox EC/IR-II: Preventive Maintenance

CLAY COUNTY CLAY COUNTY JAIL 210

Serial Number: 008608 Test Record Number: 1654
Test Date: 01/06/2026 Test Time: 2:52pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	2:52pm
FLO	Pass	2:52pm
FC	Pass	2:52pm

Temperature Tests

Test	Status	Time
FC1	Pass	2:52pm
SRC	Pass	2:52pm
DET	Pass	2:52pm
BAR	Pass	2:52pm
BT	Pass	2:52pm

Blank Tests

Test	Status	Time
AIR	Pass	2:53pm


Printer Tests

Test	Status	Time
PRNT	Pass	2:53pm

CRC Tests

Test	Status	Time
COMP	Pass	2:53pm
CAL	Pass	2:53pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County Clay Instrument Location Clay Co. Jail

Instrument Serial No. 008608 Hayesville, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 6 day of January, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Carol R. Cuth

Signature of Certifying Official

843310

Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

CLAY COUNTY CLAY COUNTY JAIL 210

Serial Number: 008608
Test Date: 01/06/2026

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE

Analyst's Name: Cutler, Daniel R
Permit Number: 0084-3310
Effective:
02/01/2025-02/01/2027

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG431002
Exp Date: 11/05/2026

Test	g/210L	Time
DIAG	Pass	2:44pm
AIR BLK	.00	2:45pm
ACCY CHK	.07	2:46pm
AIR BLK	.00	2:47pm
SUB TEST	.00	2:48pm
AIR BLK	.00	2:49pm
SUB TEST	.00	2:50pm
AIR BLK	.00	2:51pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

Intox EC/IR-II: Preventive Maintenance

CLAY COUNTY CLAY COUNTY JAIL 210

Serial Number: 008608 Test Record Number: 1654
Test Date: 01/06/2026 Test Time: 2:52pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	2:52pm
FLO	Pass	2:52pm
FC	Pass	2:52pm

Temperature Tests

Test	Status	Time
FC1	Pass	2:52pm
SRC	Pass	2:52pm
DET	Pass	2:52pm
BAR	Pass	2:52pm
BT	Pass	2:52pm

Blank Tests

Test	Status	Time
AIR	Pass	2:53pm

Printer Tests

Test	Status	Time
PRNT	Pass	2:53pm

CRC Tests

Test	Status	Time
COMP	Pass	2:53pm
CAL	Pass	2:53pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County Clay Instrument Location Clay Co. Jail
Instrument Serial No. 008608 Hayesville, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 6 day of January, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Carol R. Cuth

Signature of Certifying Official

843310

Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

CLAY COUNTY CLAY COUNTY JAIL 210

Serial Number: 008608
Test Date: 01/06/2026

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE

Analyst's Name: Cutler, Daniel R
Permit Number: 0084-3310
Effective:
02/01/2025-02/01/2027

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG431002
Exp Date: 11/05/2026

Test	g/210L	Time
DIAG	Pass	2:44pm
AIR BLK	.00	2:45pm
ACCY CHK	.07	2:46pm
AIR BLK	.00	2:47pm
SUB TEST	.00	2:48pm
AIR BLK	.00	2:49pm
SUB TEST	.00	2:50pm
AIR BLK	.00	2:51pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

Intox EC/IR-II: Preventive Maintenance

CLAY COUNTY CLAY COUNTY JAIL 210

Serial Number: 008608 Test Record Number: 1654
Test Date: 01/06/2026 Test Time: 2:52pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	2:52pm
FLO	Pass	2:52pm
FC	Pass	2:52pm

Temperature Tests

Test	Status	Time
FC1	Pass	2:52pm
SRC	Pass	2:52pm
DET	Pass	2:52pm
BAR	Pass	2:52pm
BT	Pass	2:52pm

Blank Tests

Test	Status	Time
AIR	Pass	2:53pm


Printer Tests

Test	Status	Time
PRNT	Pass	2:53pm

CRC Tests

Test	Status	Time
COMP	Pass	2:53pm
CAL	Pass	2:53pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Cleveland Instrument Location Cleveland County 50-Annex

Instrument Serial No. 009897 Shelby, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 21 day of January, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

244987
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

CLEVELAND COUNTY CLEVELAND SO-ANNEX
220

Serial Number: 008887
Test Date: 01/21/2026

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: Loftis, Benjamin C
Permit Number: 0024-4
Effective:
03/01/2025-03/01/2027

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test


Lot Number: AG516203
Exp Date: 06/11/2027

Test	g/210L	Time
DIAG	Pass	11:58am
AIR BLK	.00	11:59am
ACCY CHK	.07	12:00pm
AIR BLK	.00	12:01pm
SUB TEST	.00	12:02pm
AIR BLK	.00	12:03pm
SUB TEST	.00	12:04pm
AIR BLK	.00	12:05pm

Reported AC: .00 g/210L

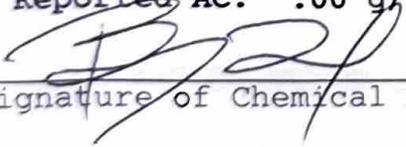

Signature of Chemical Analyst
Court CVR

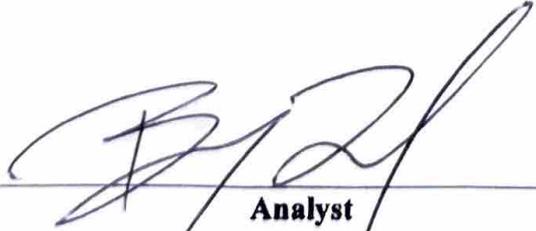

Analyst

Intox EC/IR-II: Preventive Maintenance

CLEVELAND COUNTY CLEVELAND SO-ANNEX 220

Serial Number: 008887 Test Record Number: 4479
Test Date: 01/21/2026 Test Time: 12:05pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	12:06pm
FLO	Pass	12:06pm
FC	Pass	12:06pm

Temperature Tests

Test	Status	Time
FC1	Pass	12:06pm
SRC	Pass	12:06pm
DET	Pass	12:06pm
BAR	Pass	12:06pm
BT	Pass	12:06pm

Blank Tests

Test	Status	Time
AIR	Pass	12:06pm


Printer Tests

Test	Status	Time
PRNT	Pass	12:07pm

CRC Tests

Test	Status	Time
COMP	Pass	12:07pm
CAL	Pass	12:07pm

Preventive Maintenance
Status: Pass

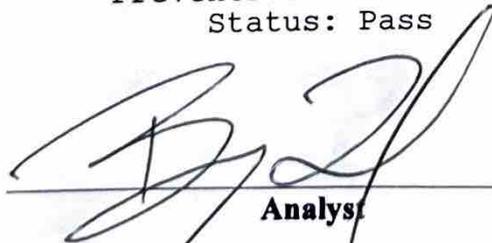

Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County Cleveland Instrument Location Cleveland County SD-Annex
Instrument Serial No. 008893 Shelby, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 21 day of January, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.




Signature of Certifying Official

244987
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

CLEVELAND COUNTY CLEVELAND SO-ANNEX
220

Serial Number: 008893
Test Date: 01/21/2026

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: Loftis, Benjamin C
Permit Number: 0024-4
Effective:
03/01/2025-03/01/2027

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test


Lot Number: AG516203
Exp Date: 06/11/2027

Test	g/210L	Time
DIAG	Pass	11:59am
AIR BLK	.00	12:00pm
ACCY CHK	.08	12:01pm
AIR BLK	.00	12:02pm
SUB TEST	.00	12:03pm
AIR BLK	.00	12:03pm
SUB TEST	.00	12:05pm
AIR BLK	.00	12:06pm

Reported AC: .00 g/210L

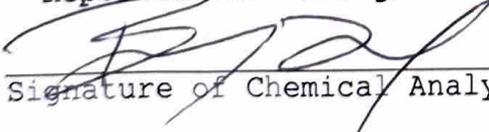

Signature of Chemical Analyst
Court CVR

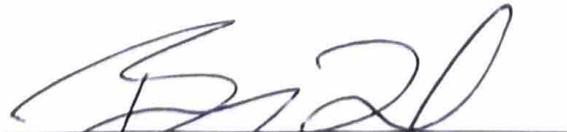

Analyst

Intox EC/IR-II: Preventive Maintenance

CLEVELAND COUNTY CLEVELAND SO-ANNEX 220

Serial Number: 008893 Test Record Number: 2098
Test Date: 01/21/2026 Test Time: 12:09pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	12:10pm
FLO	Pass	12:10pm
FC	Pass	12:10pm

Temperature Tests

Test	Status	Time
FC1	Pass	12:10pm
SRC	Pass	12:10pm
DET	Pass	12:10pm
BAR	Pass	12:10pm
BT	Pass	12:10pm

Blank Tests

Test	Status	Time
AIR	Pass	12:11pm


Printer Tests

Test	Status	Time
PRNT	Pass	12:11pm

CRC Tests

Test	Status	Time
COMP	Pass	12:11pm
CAL	Pass	12:11pm

Preventive Maintenance
Status: Pass

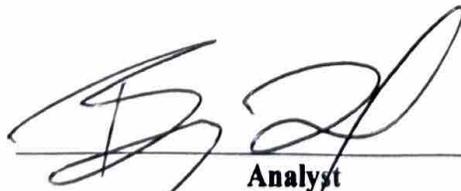

Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County Cleveland Instrument Location Kings Mountain P.D.

Instrument Serial No. 003900 Kings Mountain, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 21 day of January, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

244987
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

CLEVELAND COUNTY KINGS MOUNTAIN PD 220

Serial Number: 008900
Test Date: 01/21/2026

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: Loftis, Benjamin C
Permit Number: 0024-4
Effective:
03/01/2025-03/01/2027

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG506303
Exp Date: 03/04/2027

Test	g/210L	Time
DIAG	Pass	10:57am
AIR BLK	.00	10:57am
ACCY CHK	.07	10:58am
AIR BLK	.00	10:59am
SUB TEST	.00	11:00am
AIR BLK	.00	11:01am
SUB TEST	.00	11:02am
AIR BLK	.00	11:03am

Reported AC: .00 g/210L

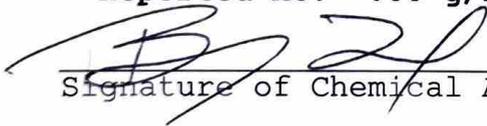

Signature of Chemical Analyst

Court CVR



Analyst

Intox EC/IR-II: Preventive Maintenance

CLEVELAND COUNTY KINGS MOUNTAIN PD 220

Serial Number: 008900 Test Record Number: 1130
Test Date: 01/21/2026 Test Time: 11:03am EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	11:04am
FLO	Pass	11:04am
FC	Pass	11:04am

Temperature Tests

Test	Status	Time
FC1	Pass	11:04am
SRC	Pass	11:04am
DET	Pass	11:04am
BAR	Pass	11:04am
BT	Pass	11:04am

Blank Tests

Test	Status	Time
AIR	Pass	11:04am

Printer Tests

Test	Status	Time
PRNT	Pass	11:05am

CRC Tests

Test	Status	Time
COMP	Pass	11:05am
CAL	Pass	11:05am

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County Craven Instrument Location BAT Mobile Unit 7

Instrument Serial No. 008002

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 30th day of January, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

2266313
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

CRAVEN COUNTY BAT MOBILE UNIT 7 240

Serial Number: 008002
Test Date: 01/30/2026

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE

Analyst's Name: Sharpe Jr., Robert J
Permit Number: 1820-8591
Effective:
02/01/2025-02/01/2027

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG506303
Exp Date: 03/04/2027

Test	g/210L	Time
DIAG	Pass	6:23pm
AIR BLK	.00	6:24pm
ACCY CHK	.08	6:24pm
AIR BLK	.00	6:25pm
SUB TEST	.00	6:26pm
AIR BLK	.00	6:27pm
SUB TEST	.00	6:28pm
AIR BLK	.00	6:29pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

CRAVEN COUNTY BAT MOBILE UNIT 7 240

Serial Number: 008002 Test Record Number: 873
Test Date: 01/30/2026 Test Time: 6:30pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	6:30pm
FLO	Pass	6:30pm
FC	Pass	6:30pm

Temperature Tests

Test	Status	Time
FC1	Pass	6:30pm
SRC	Pass	6:30pm
DET	Pass	6:30pm
BAR	Pass	6:30pm
BT	Pass	6:30pm

Blank Tests

Test	Status	Time
AIR	Pass	6:31pm


Printer Tests

Test	Status	Time
PRNT	Pass	6:31pm

CRC Tests

Test	Status	Time
COMP	Pass	6:31pm
CAL	Pass	6:31pm

Preventive Maintenance
Status: Pass

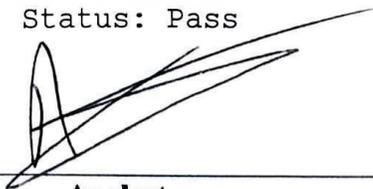

Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County CRAVEN Instrument Location CRAVEN COUNTY
Instrument Serial No. 008901 DETENTION CENTER

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 27th day of JANUARY, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Handwritten Signature]

Signature of Certifying Official

2824950

Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

CRAVEN COUNTY DETENTION CENTER 240

Serial Number: 008901
Test Date: 01/27/2026

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE

Analyst's Name: GILLESPIE, PENTTI W
Permit Number: 9523-2149
Effective:
02/01/2025-02/01/2027

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG534301
Exp Date: 12/09/2027

Test	g/210L	Time
DIAG	Pass	12:54pm
AIR BLK	.00	12:54pm
ACCY CHK	.08	12:55pm
AIR BLK	.00	12:56pm
SUB TEST	.00	12:57pm
AIR BLK	.00	12:58pm
SUB TEST	.00	12:59pm
AIR BLK	.00	1:00pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

Intox EC/IR-II: Preventive Maintenance

CRAVEN COUNTY DETENTION CENTER 240

Serial Number: 008901 Test Record Number: 1811
Test Date: 01/27/2026 Test Time: 1:00pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	1:00pm
FLO	Pass	1:00pm
FC	Pass	1:00pm

Temperature Tests

Test	Status	Time
FC1	Pass	1:01pm
SRC	Pass	1:01pm
DET	Pass	1:01pm
BAR	Pass	1:01pm
BT	Pass	1:01pm

Blank Tests

Test	Status	Time
AIR	Pass	1:01pm


Printer Tests

Test	Status	Time
PRNT	Pass	1:01pm

CRC Tests

Test	Status	Time
COMP	Pass	1:01pm
CAL	Pass	1:01pm

Preventive Maintenance
Status: Pass

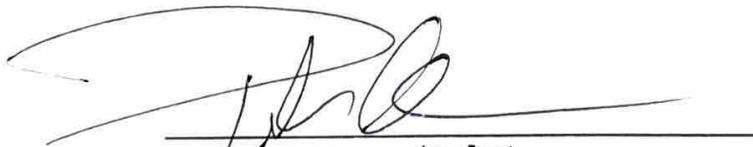

Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Craven Instrument Location BAT Mobile Unit 7

Instrument Serial No. 008968

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 30th day of January, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

2266313
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

CRAVEN COUNTY BAT MOBILE UNIT 7 240

Serial Number: 008968
Test Date: 01/30/2026

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Sharpe Jr., Robert J

Permit Number: 1820-8591

Effective:

02/01/2025-02/01/2027

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG506303

Exp Date: 03/04/2027


Test	g/210L	Time
DIAG	Pass	6:23pm
AIR BLK	.00	6:24pm
ACCY CHK	.08	6:25pm
AIR BLK	.00	6:26pm
SUB TEST	.00	6:26pm
AIR BLK	.00	6:27pm
SUB TEST	.00	6:29pm
AIR BLK	.00	6:30pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR

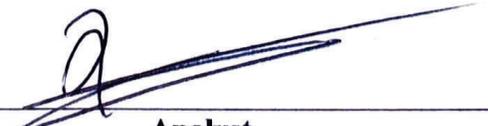

Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

CRAVEN COUNTY BAT MOBILE UNIT 7 240

Serial Number: 008968 Test Record Number: 436
Test Date: 01/30/2026 Test Time: 6:33pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	6:34pm
FLO	Pass	6:34pm
FC	Pass	6:34pm

Temperature Tests

Test	Status	Time
FC1	Pass	6:34pm
SRC	Pass	6:34pm
DET	Pass	6:34pm
BAR	Pass	6:34pm
BT	Pass	6:34pm

Blank Tests

Test	Status	Time
AIR	Pass	6:35pm

Printer Tests

Test	Status	Time
PRNT	Pass	6:35pm

CRC Tests

Test	Status	Time
COMP	Pass	6:35pm
CAL	Pass	6:35pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County Craven Instrument Location BAT Mobile Unit 7
Instrument Serial No. 00 8971

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 30th day of January, 2020 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

2266313
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

CRAVEN COUNTY BAT MOBILE UNIT 7 240

Serial Number: 008971
Test Date: 01/30/2026

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE

Analyst's Name: Sharpe Jr., Robert J
Permit Number: 1820-8591
Effective:
02/01/2025-02/01/2027

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG506302
Exp Date: 03/04/2027

Test	g/210L	Time
DIAG	Pass	6:23pm
AIR BLK	.00	6:24pm
ACCY CHK	.08	6:24pm
AIR BLK	.00	6:25pm
SUB TEST	.00	6:26pm
AIR BLK	.00	6:27pm
SUB TEST	.00	6:28pm
AIR BLK	.00	6:29pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

CRAVEN COUNTY BAT MOBILE UNIT 7 240

Serial Number: 008971 Test Record Number: 386
Test Date: 01/30/2026 Test Time: 6:30pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	6:30pm
FLO	Pass	6:30pm
FC	Pass	6:30pm

Temperature Tests

Test	Status	Time
FC1	Pass	6:30pm
SRC	Pass	6:30pm
DET	Pass	6:30pm
BAR	Pass	6:30pm
BT	Pass	6:30pm

Blank Tests

Test	Status	Time
AIR	Pass	6:31pm

Printer Tests

Test	Status	Time
PRNT	Pass	6:31pm

CRC Tests

Test	Status	Time
COMP	Pass	6:31pm
CAL	Pass	6:31pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County Craven Instrument Location BAT Mobile Unit 7

Instrument Serial No. 008972

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 30th day of January, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

2266313
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

CRAVEN COUNTY BAT MOBILE UNIT 7 240

Serial Number: 008972

Test Date: 01/30/2026

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Sharpe Jr., Robert J

Permit Number: 1820-8591

Effective:

02/01/2025-02/01/2027

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG506303

Exp Date: 03/04/2027

Test	g/210L	Time
DIAG	Pass	6:21pm
AIR BLK	.00	6:22pm
ACCY CHK	.08	6:23pm
AIR BLK	.00	6:24pm
SUB TEST	.00	6:25pm
AIR BLK	.00	6:26pm
SUB TEST	.00	6:27pm
AIR BLK	.00	6:28pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

CRAVEN COUNTY BAT MOBILE UNIT 7 240

Serial Number: 008972 Test Record Number: 448
Test Date: 01/30/2026 Test Time: 6:29pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	6:29pm
FLO	Pass	6:29pm
FC	Pass	6:29pm

Temperature Tests

Test	Status	Time
FC1	Pass	6:29pm
SRC	Pass	6:29pm
DET	Pass	6:29pm
BAR	Pass	6:29pm
BT	Pass	6:29pm

Blank Tests

Test	Status	Time
AIR	Pass	6:30pm

Printer Tests

Test	Status	Time
PRNT	Pass	6:30pm

CRC Tests

Test	Status	Time
COMP	Pass	6:30pm
CAL	Pass	6:30pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County Cumberland Instrument Location FT. Bragg
Instrument Serial No. 013868 L.E.C.

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 2 day of January, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

365156
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

CUMBERLAND COUNTY FORT BRAGG LEC 250

Serial Number: 013868
Test Date: 01/02/2026

Citation Number: M0000000-0
Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Garner, Joel K

Permit Number: 0036-5156

Effective:

02/01/2025-02/01/2027

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG534301

Exp Date: 12/09/2027

Test	g/210L	Time
DIAG	Pass	11:03am
AIR BLK	.00	11:04am
ACCY CHK	.08	11:05am
AIR BLK	.00	11:06am
SUB TEST	.00	11:07am
AIR BLK	.00	11:08am
SUB TEST	.00	11:10am
AIR BLK	.00	11:10am

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

CUMBERLAND COUNTY FORT BRAGG LEC 250

Serial Number: 013868 Test Record Number: 1238
Test Date: 01/02/2026 Test Time: 11:11am EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	11:12am
FLO	Pass	11:12am
FC	Pass	11:12am

Temperature Tests

Test	Status	Time
FC1	Pass	11:12am
SRC	Pass	11:12am
DET	Pass	11:12am
BAR	Pass	11:12am
BT	Pass	11:12am

Blank Tests

Test	Status	Time
AIR	Pass	11:13am

Printer Tests

Test	Status	Time
PRNT	Pass	11:13am

CRC Tests

Test	Status	Time
COMP	Pass	11:13am
CAL	Pass	11:13am

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Cumberland Instrument Location FT. Bragg
Instrument Serial No. 013870 L.E.C.

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 2 day of January, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

365156
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

CUMBERLAND COUNTY FORT BRAGG LEC 250

Serial Number: 013870
Test Date: 01/02/2026

Citation Number: M0000000-0
Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Garner, Joel K

Permit Number: 0036-5156

Effective:

02/01/2025-02/01/2027

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG534301

Exp Date: 12/09/2027

Test	g/210L	Time
DIAG	Pass	11:07am
AIR BLK	.00	11:08am
ACCY CHK	.08	11:08am
AIR BLK	.00	11:10am
SUB TEST	.00	11:11am
AIR BLK	.00	11:12am
SUB TEST	.00	11:13am
AIR BLK	.00	11:14am

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

Intox EC/IR-II: Preventive Maintenance

CUMBERLAND COUNTY FORT BRAGG LEC 250

Serial Number: 013870 Test Record Number: 1135
Test Date: 01/02/2026 Test Time: 11:16am EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	11:17am
FLO	Pass	11:17am
FC	Pass	11:17am

Temperature Tests

Test	Status	Time
FC1	Pass	11:17am
SRC	Pass	11:17am
DET	Pass	11:17am
BAR	Pass	11:17am
BT	Pass	11:17am

Blank Tests

Test	Status	Time
AIR	Pass	11:18am

Printer Tests

Test	Status	Time
PRNT	Pass	11:18am

CRC Tests

Test	Status	Time
COMP	Pass	11:18am
CAL	Pass	11:18am

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Dare Instrument Location Dare Co. Detention Center
Instrument Serial No. 008783 1044 Driftwood Dr. Manteo,
NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 6th day of January, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

206272
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

DARE COUNTY DARE CO DETENTION CE 270

Serial Number: 008783
Test Date: 01/06/2026

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE

Analyst's Name: Chappell, Mark A
Permit Number: 0020-6272
Effective:
02/01/2025-02/01/2027

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG506301
Exp Date: 03/04/2027

Test	g/210L	Time
DIAG	Pass	10:42am
AIR BLK	.00	10:42am
ACCY CHK	.07	10:43am
AIR BLK	.00	10:44am
SUB TEST	.00	10:45am
AIR BLK	.00	10:46am
SUB TEST	.00	10:47am
AIR BLK	.00	10:48am

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

DARE COUNTY DARE CO DETENTION CE 270

Serial Number: 008783 Test Record Number: 1804
Test Date: 01/06/2026 Test Time: 10:48am EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	10:49am
FLO	Pass	10:49am
FC	Pass	10:49am

Temperature Tests

Test	Status	Time
FC1	Pass	10:49am
SRC	Pass	10:49am
DET	Pass	10:49am
BAR	Pass	10:49am
BT	Pass	10:49am

Blank Tests

Test	Status	Time
AIR	Pass	10:50am


Printer Tests

Test	Status	Time
PRNT	Pass	10:50am

CRC Tests

Test	Status	Time
COMP	Pass	10:50am
CAL	Pass	10:50am

Preventive Maintenance
Status: Pass

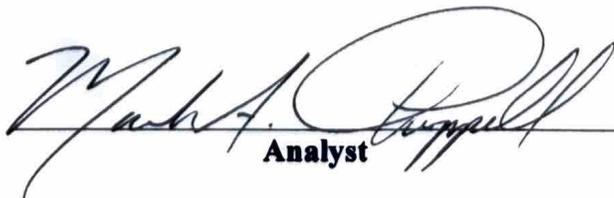
Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County Dare Instrument Location Dare Co. Detention Center
Instrument Serial No. 008804 1044 Driftwood Dr. Manteo,
NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 6th day of January, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Mark A. Huppell
Signature of Certifying Official

206272
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

DARE COUNTY DARE CO DETENTION CE 270

Serial Number: 008804
Test Date: 01/06/2026

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: Chappell, Mark A
Permit Number: 0020-6272
Effective:
02/01/2025-02/01/2027

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG506301
Exp Date: 03/04/2027


Test	g/210L	Time
DIAG	Pass	10:40am
AIR BLK	.00	10:41am
ACCY CHK	.07	10:41am
AIR BLK	.00	10:42am
SUB TEST	.00	10:43am
AIR BLK	.00	10:44am
SUB TEST	.00	10:45am
AIR BLK	.00	10:46am

Reported AC: .00 g/210L

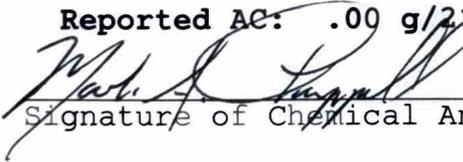

Signature of Chemical Analyst

Court CVR

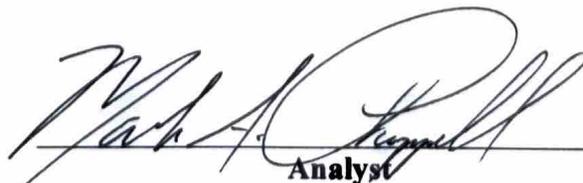

Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

DARE COUNTY DARE CO DETENTION CE 270

Serial Number: 008804 Test Record Number: 2996
Test Date: 01/06/2026 Test Time: 10:48am EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	10:48am
FLO	Pass	10:48am
FC	Pass	10:48am

Temperature Tests

Test	Status	Time
FC1	Pass	10:48am
SRC	Pass	10:48am
DET	Pass	10:48am
BAR	Pass	10:48am
BT	Pass	10:48am

Blank Tests

Test	Status	Time
AIR	Pass	10:49am


Printer Tests

Test	Status	Time
PRNT	Pass	10:49am

CRC Tests

Test	Status	Time
COMP	Pass	10:49am
CAL	Pass	10:49am

Preventive Maintenance
Status: Pass

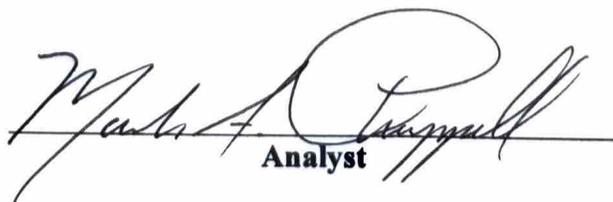
Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County Davidson Instrument Location BAT Mobile Unit 8
Instrument Serial No. 008615

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 15 day of January, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

2219283
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

DAVIDSON COUNTY BAT MOBILE UNIT 8 280

Serial Number: 008615
Test Date: 01/15/2026

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE

Analyst's Name: Glasscock, Jerry D
Permit Number: 7180-9235
Effective:
02/01/2025-02/01/2027

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG405102
Exp Date: 02/20/2026

Test	g/210L	Time
DIAG	Pass	12:51pm
AIR BLK	.00	12:52pm
ACCY CHK	.07	12:53pm
AIR BLK	.00	12:54pm
SUB TEST	.00	12:55pm
AIR BLK	.00	12:56pm
SUB TEST	.00	12:58pm
AIR BLK	.00	12:58pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

Intox EC/IR-II: Preventive Maintenance

DAVIDSON COUNTY BAT MOBILE UNIT 8 280

Serial Number: 008615 Test Record Number: 6225
Test Date: 01/15/2026 Test Time: 12:59pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	12:59pm
FLO	Pass	12:59pm
FC	Pass	12:59pm

Temperature Tests

Test	Status	Time
FC1	Pass	12:59pm
SRC	Pass	12:59pm
DET	Pass	12:59pm
BAR	Pass	12:59pm
BT	Pass	12:59pm

Blank Tests

Test	Status	Time
AIR	Pass	1:00pm

Printer Tests

Test	Status	Time
PRNT	Pass	1:00pm

CRC Tests

Test	Status	Time
COMP	Pass	1:00pm
CAL	Pass	1:00pm

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County Davidson Instrument Location BAT Mobile Unit 8
Instrument Serial No. 008736 _____

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 15 day of January, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

2219283
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

DAVIDSON COUNTY BAT MOBILE UNIT 8 280

Serial Number: 008736
Test Date: 01/15/2026

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: Glasscock, Jerry D
Permit Number: 7180-9235
Effective:
02/01/2025-02/01/2027

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test


Lot Number: AG405102
Exp Date: 02/20/2026

Test	g/210L	Time
DIAG	Pass	12:52pm
AIR BLK	.00	12:53pm
ACCY CHK	.07	12:54pm
AIR BLK	.00	12:55pm
SUB TEST	.00	12:55pm
AIR BLK	.00	12:56pm
SUB TEST	.00	12:57pm
AIR BLK	.00	12:58pm

Reported AC: .00 g/210L

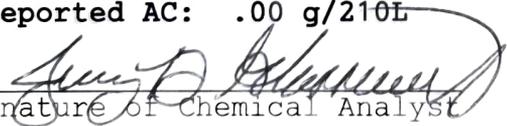
Signature of Chemical Analyst

Court CVR


Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

DAVIDSON COUNTY BAT MOBILE UNIT 8 280

Serial Number: 008736 Test Record Number: 1583
Test Date: 01/15/2026 Test Time: 12:59pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	12:59pm
FLO	Pass	12:59pm
FC	Pass	12:59pm

Temperature Tests

Test	Status	Time
FC1	Pass	12:59pm
SRC	Pass	12:59pm
DET	Pass	12:59pm
BAR	Pass	12:59pm
BT	Pass	12:59pm

Blank Tests

Test	Status	Time
AIR	Pass	1:00pm

Printer Tests

Test	Status	Time
PRNT	Pass	1:00pm

CRC Tests

Test	Status	Time
COMP	Pass	1:00pm
CAL	Pass	1:00pm

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Davidson Instrument Location BAT Mobile Unit 8

Instrument Serial No. 008775 —

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 15 day of January, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

2219283
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

DAVIDSON COUNTY BAT MOBILE UNIT 8 280

Serial Number: 008775
Test Date: 01/15/2026

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE

Analyst's Name: *Glasscock, Jerry D*
Permit Number: 7180-9235
Effective:
02/01/2025-02/01/2027

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: *Breath Test*

Lot Number: AG506303
Exp Date: 03/04/2027

Test	g/210L	Time
DIAG	Pass	12:53pm
AIR BLK	.00	12:54pm
ACCY CHK	.08	12:55pm
AIR BLK	.00	12:56pm
SUB TEST	.00	12:56pm
AIR BLK	.00	12:57pm
SUB TEST	.00	12:58pm
AIR BLK	.00	12:59pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

Intox EC/IR-II: Preventive Maintenance

DAVIDSON COUNTY BAT MOBILE UNIT 8 280

Serial Number: 008775 Test Record Number: 2437
Test Date: 01/15/2026 Test Time: 1:00pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	1:00pm
FLO	Pass	1:00pm
FC	Pass	1:00pm

Temperature Tests

Test	Status	Time
FC1	Pass	1:00pm
SRC	Pass	1:00pm
DET	Pass	1:00pm
BAR	Pass	1:00pm
BT	Pass	1:00pm

Blank Tests

Test	Status	Time
AIR	Pass	1:01pm


Printer Tests

Test	Status	Time
PRNT	Pass	1:01pm

CRC Tests

Test	Status	Time
COMP	Pass	1:01pm
CAL	Pass	1:01pm

Preventive Maintenance
Status: Pass

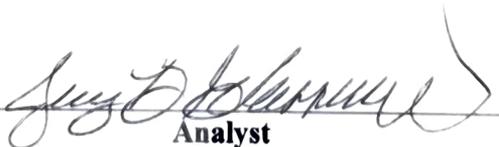
Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Davidson Instrument Location BAT Mobile Unit 8

Instrument Serial No. 008816 _____

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 15 day of January, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

2219283
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

DAVIDSON COUNTY BAT MOBILE UNIT 8 280

Serial Number: 008816
Test Date: 01/15/2026

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE

Analyst's Name: *Glasscock, Jerry D*
Permit Number: 7180-9235
Effective:
02/01/2025-02/01/2027

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: *Breath Test*

Lot Number: AG431002
Exp Date: 11/05/2026

Test	g/210L	Time
DIAG	Pass	12:54pm
AIR BLK	.00	12:55pm
ACCY CHK	.07	12:56pm
AIR BLK	.00	12:57pm
SUB TEST	.00	12:58pm
AIR BLK	.00	12:59pm
SUB TEST	.00	1:00pm
AIR BLK	.00	1:01pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

Intox EC/IR-II: Preventive Maintenance

DAVIDSON COUNTY BAT MOBILE UNIT 8 280

Serial Number: 008816 Test Record Number: 8019
Test Date: 01/15/2026 Test Time: 1:01pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	1:02pm
FLO	Pass	1:02pm
FC	Pass	1:02pm

Temperature Tests

Test	Status	Time
FC1	Pass	1:02pm
SRC	Pass	1:02pm
DET	Pass	1:02pm
BAR	Pass	1:02pm
BT	Pass	1:02pm

Blank Tests

Test	Status	Time
AIR	Pass	1:02pm

Printer Tests

Test	Status	Time
PRNT	Pass	1:03pm

CRC Tests

Test	Status	Time
COMP	Pass	1:03pm
CAL	Pass	1:03pm

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Davidson Instrument Location BAT Mobile Unit 8

Instrument Serial No. 008929 ✓

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 15 day of January, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

2219283
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

DAVIDSON COUNTY BAT MOBILE UNIT 8 280

Serial Number: 008929

Test Date: 01/15/2026

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Glasscock, Jerry D

Permit Number: 7180-9235

Effective:

02/01/2025-02/01/2027

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG506303


Exp Date: 03/04/2027

Test	g/210L	Time
DIAG	Pass	12:54pm
AIR BLK	.00	12:56pm
ACCY CHK	.08	12:56pm
AIR BLK	.00	12:57pm
SUB TEST	.00	12:58pm
AIR BLK	.00	12:59pm
SUB TEST	.00	1:00pm
AIR BLK	.00	1:02pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR

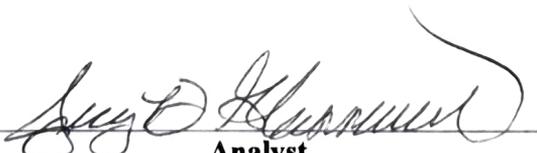
Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

DAVIDSON COUNTY BAT MOBILE UNIT 8 280

Serial Number: 008929 Test Record Number: 1720
Test Date: 01/15/2026 Test Time: 1:02pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	1:03pm
FLO	Pass	1:03pm
FC	Pass	1:03pm

Temperature Tests

Test	Status	Time
FC1	Pass	1:03pm
SRC	Pass	1:03pm
DET	Pass	1:03pm
BAR	Pass	1:03pm
BT	Pass	1:03pm

Blank Tests

Test	Status	Time
AIR	Pass	1:03pm

Printer Tests

Test	Status	Time
PRNT	Pass	1:03pm

CRC Tests

Test	Status	Time
COMP	Pass	1:04pm
CAL	Pass	1:04pm

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County Davie Instrument Location Davie County Jail
Instrument Serial No. 008905 Mocksville, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 13th day of January, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

509387
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

DAVIE COUNTY DAVIE COUNTY JAIL 290

Serial Number: 008905
Test Date: 01/13/2026

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE

Analyst's Name: Long, Thomas A
Permit Number: 0050-9387
Effective:
09/01/2025-09/01/2027

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG431003
Exp Date: 11/05/2026


Test	g/210L	Time
DIAG	Pass	9:35am
AIR BLK	.00	9:36am
ACCY CHK	.07	9:37am
AIR BLK	.00	9:38am
SUB TEST	.00	9:39am
AIR BLK	.00	9:40am
SUB TEST	.00	9:41am
AIR BLK	.00	9:42am

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

Intox EC/IR-II: Preventive Maintenance

DAVIE COUNTY DAVIE COUNTY JAIL 290

Serial Number: 008905 Test Record Number: 3293
Test Date: 01/13/2026 Test Time: 9:43am EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	9:44am
FLO	Pass	9:44am
FC	Pass	9:44am

Temperature Tests

Test	Status	Time
FC1	Pass	9:44am
SRC	Pass	9:44am
DET	Pass	9:44am
BAR	Pass	9:44am
BT	Pass	9:44am

Blank Tests

Test	Status	Time
AIR	Pass	9:45am

Printer Tests

Test	Status	Time
PRNT	Pass	9:45am

CRC Tests

Test	Status	Time
COMP	Pass	9:45am
CAL	Pass	9:45am

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County Edgecombe Instrument Location Edgecombe County Magistrate's
Instrument Serial No. 008603 Office, 3005 Anaconda Rd., Tarboro,
NC.

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 13th day of January, 2020 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Key D. [Signature]
Signature of Certifying Official

377722
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

EDGECOMBE COUNTY EDGECOMBE CO MAGISTR
320

Serial Number: 008603
Test Date: 01/13/2026

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Gray, Kelly D

Permit Number: 0037-7722

Effective:

02/01/2025-02/01/2027

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG506301

Exp Date: 03/04/2027

Test	g/210L	Time
DIAG	Pass	10:27am
AIR BLK	.00	10:28am
ACCY CHK	.07	10:29am
AIR BLK	.00	10:30am
SUB TEST	.00	10:31am
AIR BLK	.00	10:32am
SUB TEST	.00	10:34am
AIR BLK	.00	10:35am

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

EDGECOMBE COUNTY EDGECOMBE CO MAGISTR 320

Serial Number: 008603 Test Record Number: 2778
Test Date: 01/13/2026 Test Time: 10:37am EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	10:38am
FLO	Pass	10:38am
FC	Pass	10:38am

Temperature Tests

Test	Status	Time
FC1	Pass	10:38am
SRC	Pass	10:38am
DET	Pass	10:38am
BAR	Pass	10:38am
BT	Pass	10:38am

Blank Tests

Test	Status	Time
AIR	Pass	10:39am

Printer Tests

Test	Status	Time
PRNT	Pass	10:39am

CRC Tests

Test	Status	Time
COMP	Pass	10:39am
CAL	Pass	10:39am

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Edgecombe Instrument Location Edgecombe County Magistrate's
Instrument Serial No. 008663 Office, 3005 Anacanda Rd., Tarboro,
N.C.

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 13th day of January, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

377722
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

EDGECOMBE COUNTY EDGECOMBE CO MAGISTR
320

Serial Number: 008663
Test Date: 01/13/2026

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Gray, Kelly D

Permit Number: 0037-7722

Effective:

02/01/2025-02/01/2027

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG501303

Exp Date: 01/13/2027


Test	g/210L	Time
DIAG	Pass	10:48am
AIR BLK	.00	10:49am
ACCY CHK	.07	10:50am
AIR BLK	.00	10:51am
SUB TEST	.00	10:51am
AIR BLK	.00	10:52am
SUB TEST	.00	10:54am
AIR BLK	.00	10:55am

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

EDGECOMBE COUNTY EDGECOMBE CO MAGISTR 320

Serial Number: 008663 Test Record Number: 3853
Test Date: 01/13/2026 Test Time: 10:56am EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	10:56am
FLO	Pass	10:56am
FC	Pass	10:56am

Temperature Tests

Test	Status	Time
FC1	Pass	10:56am
SRC	Pass	10:56am
DET	Pass	10:56am
BAR	Pass	10:56am
BT	Pass	10:56am

Blank Tests

Test	Status	Time
AIR	Pass	10:57am


Printer Tests

Test	Status	Time
PRNT	Pass	10:57am

CRC Tests

Test	Status	Time
COMP	Pass	10:57am
CAL	Pass	10:57am

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Forsyth Instrument Location BAT Mobile Unit 10

Instrument Serial No. 008584

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 2 day of January, 2016 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Signature of Certifying Official

193759

Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

FORSYTH COUNTY BAT MOBILE UNIT 10 330

Serial Number: 008584
Test Date: 01/02/2026

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE

Analyst's Name: Carroll, Barry J
Permit Number: 0019-3759
Effective:
09/01/2025-09/01/2027

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG400303
Exp Date: 01/03/2026

Test	g/210L	Time
DIAG	Pass	9:39pm
AIR BLK	.00	9:40pm
ACCY CHK	.08	9:40pm
AIR BLK	.00	9:41pm
SUB TEST	.00	9:42pm
AIR BLK	.00	9:43pm
SUB TEST	.00	9:44pm
AIR BLK	.00	9:45pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

FORSYTH COUNTY BAT MOBILE UNIT 10 330

Serial Number: 008584 Test Record Number: 2856
Test Date: 01/02/2026 Test Time: 9:46pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	9:46pm
FLO	Pass	9:46pm
FC	Pass	9:47pm

Temperature Tests

Test	Status	Time
FC1	Pass	9:47pm
SRC	Pass	9:47pm
DET	Pass	9:47pm
BAR	Pass	9:47pm
BT	Pass	9:47pm

Blank Tests

Test	Status	Time
AIR	Pass	9:47pm

Printer Tests

Test	Status	Time
PRNT	Pass	9:47pm

CRC Tests

Test	Status	Time
COMP	Pass	9:47pm
CAL	Pass	9:47pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County Forsyth Instrument Location BAT Mobile Unit 10

Instrument Serial No. 008637

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 2 day of January, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

193759
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

FORSYTH COUNTY BAT MOBILE UNIT 10 330

Serial Number: 008637
Test Date: 01/02/2026

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: Carroll, Barry J
Permit Number: 0019-3759
Effective:
09/01/2025-09/01/2027

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG400303
Exp Date: 01/03/2026

Test	g/210L	Time
DIAG	Pass	9:30pm
AIR BLK	.00	9:31pm
ACCY CHK	.07	9:32pm
AIR BLK	.00	9:33pm
SUB TEST	.00	9:34pm
AIR BLK	.00	9:34pm
SUB TEST	.00	9:36pm
AIR BLK	.00	9:37pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

FORSYTH COUNTY BAT MOBILE UNIT 10 330

Serial Number: 008637 Test Record Number: 3574
Test Date: 01/02/2026 Test Time: 9:40pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	9:40pm
FLO	Pass	9:40pm
FC	Pass	9:40pm

Temperature Tests

Test	Status	Time
FC1	Pass	9:41pm
SRC	Pass	9:41pm
DET	Pass	9:41pm
BAR	Pass	9:41pm
BT	Pass	9:41pm

Blank Tests

Test	Status	Time
AIR	Pass	9:41pm

Printer Tests

Test	Status	Time
PRNT	Pass	9:41pm

CRC Tests

Test	Status	Time
COMP	Pass	9:41pm
CAL	Pass	9:41pm

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County Forsyth Instrument Location BAT Mobile Unit 10
Instrument Serial No. 008686

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 2 day of January, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

193759
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

FORSYTH COUNTY BAT MOBILE UNIT 10 330

Serial Number: 008686
Test Date: 01/02/2026

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE

Analyst's Name: Carroll, Barry J
Permit Number: 0019-3759
Effective:
09/01/2025-09/01/2027

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG506302
Exp Date: 03/04/2027

Test	g/210L	Time
DIAG	Pass	9:33pm
AIR BLK	.00	9:34pm
ACCY CHK	.08	9:35pm
AIR BLK	.00	9:35pm
SUB TEST	.00	9:36pm
AIR BLK	.00	9:37pm
SUB TEST	.00	9:39pm
AIR BLK	.00	9:40pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

FORSYTH COUNTY BAT MOBILE UNIT 10 330

Serial Number: 008686 Test Record Number: 7202
Test Date: 01/02/2026 Test Time: 9:40pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	9:40pm
FLO	Pass	9:40pm
FC	Pass	9:41pm

Temperature Tests

Test	Status	Time
FC1	Pass	9:41pm
SRC	Pass	9:41pm
DET	Pass	9:41pm
BAR	Pass	9:41pm
BT	Pass	9:41pm

Blank Tests

Test	Status	Time
AIR	Pass	9:41pm

Printer Tests

Test	Status	Time
PRNT	Pass	9:41pm

CRC Tests

Test	Status	Time
COMP	Pass	9:41pm
CAL	Pass	9:41pm

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Forsyth Instrument Location BAT Mobile Unit 10

Instrument Serial No. 008776

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 2 day of January, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

193759
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

FORSYTH COUNTY BAT MOBILE UNIT 10 330

Serial Number: 008776

Test Date: 01/02/2026

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Carroll, Barry J

Permit Number: 0019-3759

Effective:

09/01/2025-09/01/2027

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG417803

Exp Date: 06/26/2026


Test	g/210L	Time
DIAG	Pass	9:28pm
AIR BLK	.00	9:29pm
ACCY CHK	.08	9:30pm
AIR BLK	.00	9:31pm
SUB TEST	.00	9:31pm
AIR BLK	.00	9:32pm
SUB TEST	.00	9:34pm
AIR BLK	.00	9:35pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

FORSYTH COUNTY BAT MOBILE UNIT 10 330

Serial Number: 008776 Test Record Number: 4160
Test Date: 01/02/2026 Test Time: 9:36pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	9:36pm
FLO	Pass	9:36pm
FC	Pass	9:36pm

Temperature Tests

Test	Status	Time
FC1	Pass	9:36pm
SRC	Pass	9:36pm
DET	Pass	9:36pm
BAR	Pass	9:36pm
BT	Pass	9:36pm

Blank Tests

Test	Status	Time
AIR	Pass	9:37pm

Printer Tests

Test	Status	Time
PRNT	Pass	9:37pm

CRC Tests

Test	Status	Time
COMP	Pass	9:37pm
CAL	Pass	9:37pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County Forsyth Instrument Location BAT Mobile Unit 10

Instrument Serial No. 006779

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 2 day of January, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

193759
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

FORSYTH COUNTY BAT MOBILE UNIT 10 330

Serial Number: 008779
Test Date: 01/02/2026

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE

Analyst's Name: Carroll, Barry J
Permit Number: 0019-3759
Effective:
09/01/2025-09/01/2027

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG431002
Exp Date: 11/05/2026

Test	g/210L	Time
DIAG	Pass	9:24pm
AIR BLK	.00	9:25pm
ACCY CHK	.08	9:26pm
AIR BLK	.00	9:26pm
SUB TEST	.00	9:28pm
AIR BLK	.00	9:28pm
SUB TEST	.00	9:31pm
AIR BLK	.00	9:31pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

Intox EC/IR-II: Preventive Maintenance

FORSYTH COUNTY BAT MOBILE UNIT 10 330

Serial Number: 008779 Test Record Number: 4104
Test Date: 01/02/2026 Test Time: 9:34pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	9:34pm
FLO	Pass	9:34pm
FC	Pass	9:34pm

Temperature Tests

Test	Status	Time
FC1	Pass	9:34pm
SRC	Pass	9:34pm
DET	Pass	9:34pm
BAR	Pass	9:34pm
BT	Pass	9:34pm

Blank Tests

Test	Status	Time
AIR	Pass	9:35pm


Printer Tests

Test	Status	Time
PRNT	Pass	9:35pm

CRC Tests

Test	Status	Time
COMP	Pass	9:35pm
CAL	Pass	9:35pm

Preventive Maintenance
Status: Pass

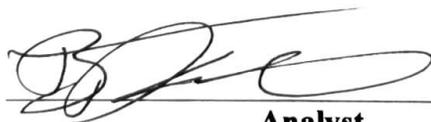

Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Guilford Instrument Location Gibsonville PD

Instrument Serial No. 008912 129 W. Main St Gibsonville, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 30 day of January, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Simon Stokes Bruns
Signature of Certifying Official

146221
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

GUILFORD COUNTY GIBSONVILLE PD 400

Serial Number: 008812
Test Date: 01/30/2026

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE

Analyst's Name: Barnes, Simon S
Permit Number: 0014-6221
Effective:
02/01/2025-02/01/2027

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG501303
Exp Date: 01/13/2027

Test	g/210L	Time
DIAG	Pass	1:29pm
AIR BLK	.00	1:30pm
ACCY CHK	.08	1:30pm
AIR BLK	.00	1:32pm
SUB TEST	.00	1:32pm
AIR BLK	.00	1:33pm
SUB TEST	.00	1:34pm
AIR BLK	.00	1:35pm

Reported AC: .00 g/210L

Simon Stokes Barnes
Signature of Chemical Analyst

Court CVR

Simon Stokes Barnes
Analyst

Intox EC/IR-II: Preventive Maintenance

GUILFORD COUNTY GIBSONVILLE PD 400

Serial Number: 008812 Test Record Number: 3868
Test Date: 01/30/2026 Test Time: 1:36pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	1:36pm
FLO	Pass	1:36pm
FC	Pass	1:36pm

Temperature Tests

Test	Status	Time
FC1	Pass	1:36pm
SRC	Pass	1:36pm
DET	Pass	1:36pm
BAR	Pass	1:36pm
BT	Pass	1:36pm

Blank Tests

Test	Status	Time
AIR	Pass	1:37pm

Printer Tests

Test	Status	Time
PRNT	Pass	1:37pm

CRC Tests

Test	Status	Time
COMP	Pass	1:37pm
CAL	Pass	1:37pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Guilford Instrument Location BAT Mobile Unit 11

Instrument Serial No. 008970

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 14th day of January, 2024 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



John Panier
Signature of Certifying Official

1604930
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

GUILFORD COUNTY BAT MOBILE UNIT 11 400

Serial Number: 008970

Test Date: 01/14/2026

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Lanier Jr., John P

Permit Number: 4582-9118

Effective:

04/01/2025-04/01/2027

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG417802

Exp Date: 06/26/2026


Test	g/210L	Time
DIAG	Pass	8:18am
AIR BLK	.00	8:19am
ACCY CHK	.07	8:20am
AIR BLK	.00	8:21am
SUB TEST	.00	8:22am
AIR BLK	.00	8:23am
SUB TEST	.00	8:24am
AIR BLK	.00	8:25am

Reported AC: .00 g/210L

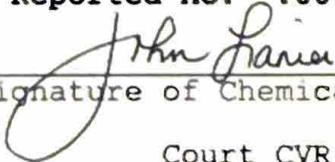

Signature of Chemical Analyst

Court CVR

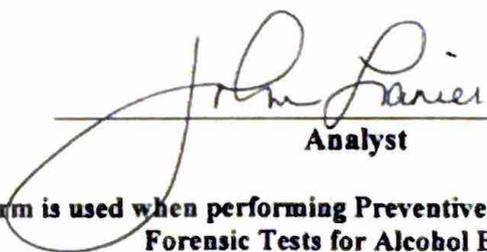

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

GUILFORD COUNTY BAT MOBILE UNIT 11 400

Serial Number: 008970 Test Record Number: 1366
Test Date: 01/14/2026 Test Time: 8:26am EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	8:26am
FLO	Pass	8:26am
FC	Pass	8:26am

Temperature Tests

Test	Status	Time
FC1	Pass	8:26am
SRC	Pass	8:26am
DET	Pass	8:26am
BAR	Pass	8:26am
BT	Pass	8:26am

Blank Tests

Test	Status	Time
AIR	Pass	8:27am


Printer Tests

Test	Status	Time
PRNT	Pass	8:27am

CRC Tests

Test	Status	Time
COMP	Pass	8:27am
CAL	Pass	8:27am

Preventive Maintenance
Status: Pass

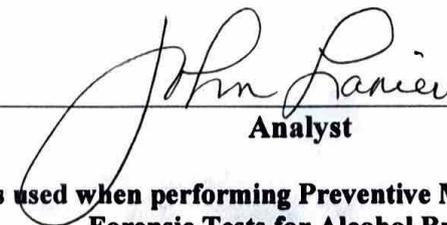

Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Guilford Instrument Location BAT Mobile Unit II

Instrument Serial No. 008973

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 14th day of January, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



John Lanier
Signature of Certifying Official

1604930
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

GUILFORD COUNTY BAT MOBILE UNIT 11 400

Serial Number: 008973

Test Date: 01/14/2026

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Lanier Jr., John P

Permit Number: 4582-9118

Effective:

04/01/2025-04/01/2027

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG431003


Exp Date: 11/05/2026

Test	g/210L	Time
DIAG	Pass	8:21am
AIR BLK	.00	8:22am
ACCY CHK	.07	8:22am
AIR BLK	.00	8:23am
SUB TEST	.00	8:24am
AIR BLK	.00	8:25am
SUB TEST	.00	8:26am
AIR BLK	.00	8:27am

Reported AC: .00 g/210L

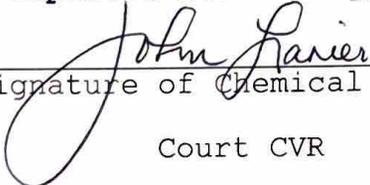

Signature of Chemical Analyst
Court CVR

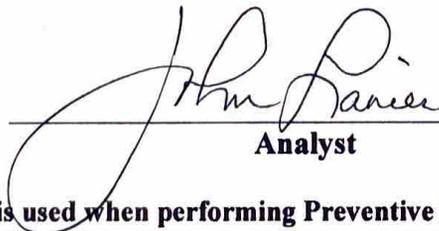

Analyst

Intox EC/IR-II: Preventive Maintenance

GUILFORD COUNTY BAT MOBILE UNIT 11 400

Serial Number: 008973 Test Record Number: 1417
Test Date: 01/14/2026 Test Time: 8:28am EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	8:28am
FLO	Pass	8:28am
FC	Pass	8:28am

Temperature Tests

Test	Status	Time
FC1	Pass	8:28am
SRC	Pass	8:28am
DET	Pass	8:28am
BAR	Pass	8:28am
BT	Pass	8:28am

Blank Tests

Test	Status	Time
AIR	Pass	8:29am

Printer Tests

Test	Status	Time
PRNT	Pass	8:29am

CRC Tests

Test	Status	Time
COMP	Pass	8:29am
CAL	Pass	8:29am

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County Henderson Instrument Location Henderson County Detention
Instrument Serial No 004306 Hendersonville, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 15 day of January, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

244987
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

HENDERSON COUNTY HENDERSON COUNTY
DETENTION 440

Serial Number: 008806
Test Date: 01/15/2026

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: Loftis, Benjamin C
Permit Number: 0024-4987
Effective:
03/01/2025-03/01/2027

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG516203
Exp Date: 06/11/2027

Test	g/210L	Time
DIAG	Pass	5:27pm
AIR BLK	.00	5:28pm
ACCY CHK	.08	5:28pm
AIR BLK	.00	5:29pm
SUB TEST	.00	5:30pm
AIR BLK	.00	5:31pm
SUB TEST	.00	5:32pm
AIR BLK	.00	5:33pm

Reported AC: .00 g/210L

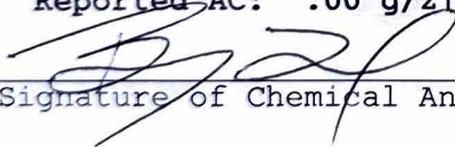

Signature of Chemical Analyst
Court CVR



Analyst

Intox EC/IR-II: Preventive Maintenance

HENDERSON COUNTY HENDERSON COUNTY DETENTION 440

Serial Number: 008806 Test Record Number: 4270
Test Date: 01/15/2026 Test Time: 5:33pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	5:34pm
FLO	Pass	5:34pm
FC	Pass	5:34pm

Temperature Tests

Test	Status	Time
FC1	Pass	5:34pm
SRC	Pass	5:34pm
DET	Pass	5:34pm
BAR	Pass	5:34pm
BT	Pass	5:34pm

Blank Tests

Test	Status	Time
AIR	Pass	5:35pm

Printer Tests

Test	Status	Time
PRNT	Pass	5:35pm

CRC Tests

Test	Status	Time
COMP	Pass	5:35pm
CAL	Pass	5:35pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County Henderson Instrument Location Henderson County Detention

Instrument Serial No. 008822 Hendersonville, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 8 day of January, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.




Signature of Certifying Official

244987
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

HENDERSON COUNTY HENDERSON COUNTY
DETENTION 440

Serial Number: 008822
Test Date: 01/08/2026

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: Loftis, Benjamin C
Permit Number: 0024-4987
Effective:
03/01/2025-03/01/2027

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG516203
Exp Date: 06/11/2027

Test	g/210L	Time
DIAG	Pass	1:15pm
AIR BLK	.00	1:15pm
ACCY CHK	.07	1:16pm
AIR BLK	.00	1:17pm
SUB TEST	.00	1:18pm
AIR BLK	.00	1:19pm
SUB TEST	.00	1:20pm
AIR BLK	.00	1:21pm

Reported AC: .00 g/210L

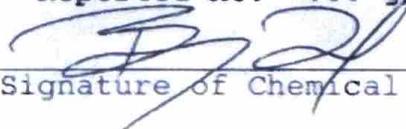

Signature of Chemical Analyst

Court CVR



Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

HENDERSON COUNTY HENDERSON COUNTY DETENTION 440

Serial Number: 008822 Test Record Number: 3560
Test Date: 01/08/2026 Test Time: 1:22pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	1:22pm
FLO	Pass	1:22pm
FC	Pass	1:22pm

Temperature Tests

Test	Status	Time
FC1	Pass	1:22pm
SRC	Pass	1:22pm
DET	Pass	1:22pm
BAR	Pass	1:22pm
BT	Pass	1:22pm

Blank Tests

Test	Status	Time
AIR	Pass	1:23pm


Printer Tests

Test	Status	Time
PRNT	Pass	1:23pm

CRC Tests

Test	Status	Time
COMP	Pass	1:23pm
CAL	Pass	1:23pm

Preventive Maintenance
Status: Pass

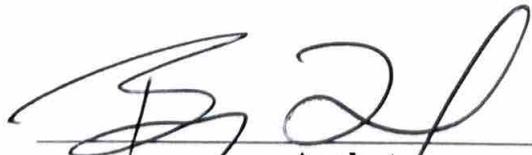

Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County Henderson Instrument Location Henderson County Detention
Instrument Serial No. 008916 Hendersonville, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 8 day of January, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

244987
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

HENDERSON COUNTY HENDERSON COUNTY
DETENTION 440

Serial Number: 008916
Test Date: 01/08/2026

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: Loftis, Benjamin C
Permit Number: 0024-4987
Effective:
03/01/2025-03/01/2027

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG516203
Exp Date: 06/11/2027

Test	g/210L	Time
DIAG	Pass	1:54pm
AIR BLK	.00	1:55pm
ACCY CHK	.07	1:55pm
AIR BLK	.00	1:56pm
SUB TEST	.00	1:57pm
AIR BLK	.00	1:58pm
SUB TEST	.00	1:59pm
AIR BLK	.00	2:00pm

Reported AC: .00 g/210L

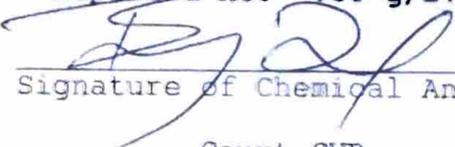

Signature of Chemical Analyst

Court CVR



Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

HENDERSON COUNTY HENDERSON COUNTY DETENTION 440

Serial Number: 008916 Test Record Number: 1989
Test Date: 01/08/2026 Test Time: 2:00pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	2:01pm
FLO	Pass	2:01pm
FC	Pass	2:01pm

Temperature Tests

Test	Status	Time
FC1	Pass	2:01pm
SRC	Pass	2:01pm
DET	Pass	2:01pm
BAR	Pass	2:01pm
BT	Pass	2:01pm

Blank Tests

Test	Status	Time
AIR	Pass	2:01pm

Printer Tests

Test	Status	Time
PRNT	Pass	2:01pm

CRC Tests

Test	Status	Time
COMP	Pass	2:02pm
CAL	Pass	2:02pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Hoke Instrument Location Hoke County
Instrument Serial No. 008852 Detention Center

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 21 day of January, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

365156
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

HOKE COUNTY DETENTION CENTER 460

Serial Number: 008852
Test Date: 01/21/2026

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE

Analyst's Name: Garner, Joel K
Permit Number: 0036-5156
Effective:
02/01/2025-02/01/2027

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG534301
Exp Date: 12/09/2027

Test	g/210L	Time
DIAG	Pass	10:25am
AIR BLK	.00	10:26am
ACCY CHK	.08	10:27am
AIR BLK	.00	10:28am
SUB TEST	.00	10:29am
AIR BLK	.00	10:29am
SUB TEST	.00	10:31am
AIR BLK	.00	10:32am

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

Intox EC/IR-II: Preventive Maintenance

HOKE COUNTY DETENTION CENTER 460

Serial Number: 008852 Test Record Number: 1800
Test Date: 01/21/2026 Test Time: 10:33am EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	10:33am
FLO	Pass	10:33am
FC	Pass	10:33am

Temperature Tests

Test	Status	Time
FC1	Pass	10:33am
SRC	Pass	10:33am
DET	Pass	10:33am
BAR	Pass	10:33am
BT	Pass	10:33am

Blank Tests

Test	Status	Time
AIR	Pass	10:34am

Printer Tests

Test	Status	Time
PRNT	Pass	10:34am

CRC Tests

Test	Status	Time
COMP	Pass	10:34am
CAL	Pass	10:34am

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Hoke Instrument Location Hoke County
Instrument Serial No. 008855 Detention Center

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 21 day of January, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

365156
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

HOKE COUNTY DETENTION CENTER 460

Serial Number: 008855
Test Date: 01/21/2026

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE

Analyst's Name: Garner, Joel K
Permit Number: 0036-5156
Effective:
02/01/2025-02/01/2027

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG534301
Exp Date: 12/09/2027

Test	g/210L	Time
DIAG	Pass	10:26am
AIR BLK	.00	10:26am
ACCY CHK	.08	10:27am
AIR BLK	.00	10:28am
SUB TEST	.00	10:29am
AIR BLK	.00	10:30am
SUB TEST	.00	10:32am
AIR BLK	.00	10:33am

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

Intox EC/IR-II: Preventive Maintenance

HOKE COUNTY DETENTION CENTER 460

Serial Number: 008855 Test Record Number: 2042
Test Date: 01/21/2026 Test Time: 10:33am EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	10:33am
FLO	Pass	10:33am
FC	Pass	10:34am

Temperature Tests

Test	Status	Time
FC1	Pass	10:34am
SRC	Pass	10:34am
DET	Pass	10:34am
BAR	Pass	10:34am
BT	Pass	10:34am

Blank Tests

Test	Status	Time
AIR	Pass	10:34am

Printer Tests

Test	Status	Time
PRNT	Pass	10:34am

CRC Tests

Test	Status	Time
COMP	Pass	10:35am
CAL	Pass	10:35am

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)


County Iredell Instrument Location BAT Mobile Unit 8

Instrument Serial No. 008615 -

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 2 day of January, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

2219283
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

IREDELL COUNTY BAT MOBILE UNIT 8 480

Serial Number: 008615
Test Date: 01/02/2026

Citation Number: M0000000-0
Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Glasscock, Jerry D

Permit Number: 7180-9235

Effective:

02/01/2025-02/01/2027

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG405102

Exp Date: 02/20/2026

Test	g/210L	Time
DIAG	Pass	10:46pm
AIR BLK	.00	10:47pm
ACCY CHK	.07	10:48pm
AIR BLK	.00	10:49pm
SUB TEST	.00	10:50pm
AIR BLK	.00	10:50pm
SUB TEST	.00	10:52pm
AIR BLK	.00	10:53pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

Intox EC/IR-II: Preventive Maintenance

IREDELL COUNTY BAT MOBILE UNIT 8 480

Serial Number: 008615 Test Record Number: 6219
Test Date: 01/02/2026 Test Time: 10:56pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	10:57pm
FLO	Pass	10:57pm
FC	Pass	10:57pm

Temperature Tests

Test	Status	Time
FC1	Pass	10:57pm
SRC	Pass	10:57pm
DET	Pass	10:57pm
BAR	Pass	10:57pm
BT	Pass	10:57pm

Blank Tests

Test	Status	Time
AIR	Pass	10:58pm

Printer Tests

Test	Status	Time
PRNT	Pass	10:58pm

CRC Tests

Test	Status	Time
COMP	Pass	10:58pm
CAL	Pass	10:58pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Iredell Instrument Location BAT Mobile Unit 8
Instrument Serial No. 008615

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 14 day of January, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

2219283
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

IREDELL COUNTY BAT MOBILE UNIT 8 480

Serial Number: 008615
Test Date: 01/14/2026

Citation Number: M0000000-0
Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Glasscock, Jerry D

Permit Number: 7180-9235

Effective:

02/01/2025-02/01/2027

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG405102

Exp Date: 02/20/2026

Test	g/210L	Time
DIAG	Pass	7:41am
AIR BLK	.00	7:42am
ACCY CHK	.07	7:42am
AIR BLK	.00	7:43am
SUB TEST	.00	7:44am
AIR BLK	.00	7:45am
SUB TEST	.00	7:46am
AIR BLK	.00	7:47am

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

Intox EC/IR-II: Preventive Maintenance

IREDELL COUNTY BAT MOBILE UNIT 8 480

Serial Number: 008615 Test Record Number: 6221
Test Date: 01/14/2026 Test Time: 7:48am EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	7:48am
FLO	Pass	7:48am
FC	Pass	7:48am

Temperature Tests

Test	Status	Time
FC1	Pass	7:48am
SRC	Pass	7:48am
DET	Pass	7:48am
BAR	Pass	7:48am
BT	Pass	7:48am

Blank Tests

Test	Status	Time
AIR	Pass	7:49am

Printer Tests

Test	Status	Time
PRNT	Pass	7:49am

CRC Tests

Test	Status	Time
COMP	Pass	7:49am
CAL	Pass	7:49am

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Iredell Instrument Location BAT Mobile Unit 8

Instrument Serial No. 008736 _____

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 2 day of January, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

2219283
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

IREDELL COUNTY BAT MOBILE UNIT 8 480

Serial Number: 008736
Test Date: 01/02/2026

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Glasscock, Jerry D

Permit Number: 7180-9235

Effective:

02/01/2025-02/01/2027

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG405102

Exp Date: 02/20/2026

Test	g/210L	Time
DIAG	Pass	10:47pm
AIR BLK	.00	10:48pm
ACCY CHK	.07	10:49pm
AIR BLK	.00	10:50pm
SUB TEST	.00	10:50pm
AIR BLK	.00	10:51pm
SUB TEST	.00	10:53pm
AIR BLK	.00	10:53pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

Intox EC/IR-II: Preventive Maintenance

IREDELL COUNTY BAT MOBILE UNIT 8 480

Serial Number: 008736 Test Record Number: 1577
Test Date: 01/02/2026 Test Time: 10:55pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	10:55pm
FLO	Pass	10:55pm
FC	Pass	10:55pm

Temperature Tests

Test	Status	Time
FC1	Pass	10:56pm
SRC	Pass	10:56pm
DET	Pass	10:56pm
BAR	Pass	10:56pm
BT	Pass	10:56pm

Blank Tests

Test	Status	Time
AIR	Pass	10:56pm

Printer Tests

Test	Status	Time
PRNT	Pass	10:56pm

CRC Tests

Test	Status	Time
COMP	Pass	10:56pm
CAL	Pass	10:56pm

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Iredell Instrument Location BAT Mobile Unit 8

Instrument Serial No. 008736 -

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 14 day of January, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

2219283
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

IREDELL COUNTY BAT MOBILE UNIT 8 480

Serial Number: 008736
Test Date: 01/14/2026

Citation Number: M0000000-0
Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Glasscock, Jerry D

Permit Number: 7180-9235

Effective:

02/01/2025-02/01/2027

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG405102

Exp Date: 02/20/2026

Test	g/210L	Time
DIAG	Pass	7:39am
AIR BLK	.00	7:40am
ACCY CHK	.07	7:41am
AIR BLK	.00	7:42am
SUB TEST	.00	7:43am
AIR BLK	.00	7:44am
SUB TEST	.00	7:45am
AIR BLK	.00	7:46am

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

IREDELL COUNTY BAT MOBILE UNIT 8 480

Serial Number: 008736 Test Record Number: 1579
Test Date: 01/14/2026 Test Time: 7:47am EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	7:48am
FLO	Pass	7:48am
FC	Pass	7:48am

Temperature Tests

Test	Status	Time
FC1	Pass	7:48am
SRC	Pass	7:48am
DET	Pass	7:48am
BAR	Pass	7:48am
BT	Pass	7:48am

Blank Tests

Test	Status	Time
AIR	Pass	7:48am

Printer Tests

Test	Status	Time
PRNT	Pass	7:49am

CRC Tests

Test	Status	Time
COMP	Pass	7:49am
CAL	Pass	7:49am

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Iredell Instrument Location BAT Mobile Unit 8
Instrument Serial No. 008775

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 2 day of January, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

2219283
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

IREDELL COUNTY BAT MOBILE UNIT 8 480

Serial Number: 008775

Test Date: 01/02/2026

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Glasscock, Jerry D

Permit Number: 7180-9235

Effective:

02/01/2025-02/01/2027

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG506303

Exp Date: 03/04/2027

Test	g/210L	Time
DIAG	Pass	10:45pm
AIR BLK	.00	10:46pm
ACCY CHK	.08	10:46pm
AIR BLK	.00	10:47pm
SUB TEST	.00	10:48pm
AIR BLK	.00	10:49pm
SUB TEST	.00	10:50pm
AIR BLK	.00	10:51pm

Reported AC: .00 g/210L

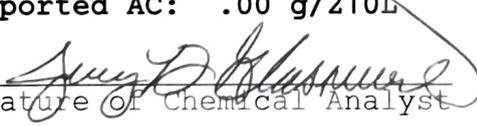
Signature of Chemical Analyst

Court CVR


Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

IREDELL COUNTY BAT MOBILE UNIT 8 480

Serial Number: 008775 Test Record Number: 2431
Test Date: 01/02/2026 Test Time: 10:53pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	10:53pm
FLO	Pass	10:53pm
FC	Pass	10:53pm

Temperature Tests

Test	Status	Time
FC1	Pass	10:53pm
SRC	Pass	10:53pm
DET	Pass	10:53pm
BAR	Pass	10:53pm
BT	Pass	10:53pm

Blank Tests

Test	Status	Time
AIR	Pass	10:54pm


Printer Tests

Test	Status	Time
PRNT	Pass	10:54pm

CRC Tests

Test	Status	Time
COMP	Pass	10:54pm
CAL	Pass	10:54pm

Preventive Maintenance
Status: Pass

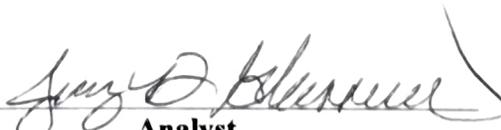

Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Iredell Instrument Location BAT Mobile Unit 8
Instrument Serial No. 008775 —

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 14 day of January, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

2219283
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

IREDELL COUNTY BAT MOBILE UNIT 8 480

Serial Number: 008775
Test Date: 01/14/2026

Citation Number: M0000000-0
Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Glasscock, Jerry D

Permit Number: 7180-9235

Effective:

02/01/2025-02/01/2027

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG506303

Exp Date: 03/04/2027

Test	g/210L	Time
DIAG	Pass	7:39am
AIR BLK	.00	7:40am
ACCY CHK	.08	7:40am
AIR BLK	.00	7:41am
SUB TEST	.00	7:42am
AIR BLK	.00	7:43am
SUB TEST	.00	7:44am
AIR BLK	.00	7:45am

Reported AC: .00 g/210L

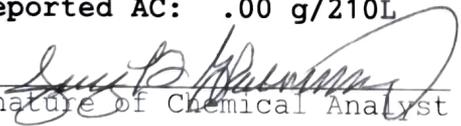
Signature of Chemical Analyst

Court CVR


Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

IREDELL COUNTY BAT MOBILE UNIT 8 480

Serial Number: 008775 Test Record Number: 2433
Test Date: 01/14/2026 Test Time: 7:46am EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	7:46am
FLO	Pass	7:46am
FC	Pass	7:46am

Temperature Tests

Test	Status	Time
FC1	Pass	7:46am
SRC	Pass	7:46am
DET	Pass	7:46am
BAR	Pass	7:46am
BT	Pass	7:46am

Blank Tests

Test	Status	Time
AIR	Pass	7:47am

Printer Tests

Test	Status	Time
PRNT	Pass	7:47am

CRC Tests

Test	Status	Time
COMP	Pass	7:47am
CAL	Pass	7:47am

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Iredell Instrument Location BAT Mobile Unit 8

Instrument Serial No. 008816

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 2 day of January, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

2219283
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

IREDELL COUNTY BAT MOBILE UNIT 8 480

Serial Number: 008816

Test Date: 01/02/2026

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Glasscock, Jerry D

Permit Number: 7180-9235

Effective:

02/01/2025-02/01/2027

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG431002

Exp Date: 11/05/2026

Test	g/210L	Time
DIAG	Pass	10:44pm
AIR BLK	.00	10:45pm
ACCY CHK	.07	10:46pm
AIR BLK	.00	10:47pm
SUB TEST	.00	10:48pm
AIR BLK	.00	10:49pm
SUB TEST	.00	10:51pm
AIR BLK	.00	10:52pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

Intox EC/IR-II: Preventive Maintenance

IREDELL COUNTY BAT MOBILE UNIT 8 480

Serial Number: 008816 Test Record Number: 8012
Test Date: 01/02/2026 Test Time: 10:53pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	10:53pm
FLO	Pass	10:53pm
FC	Pass	10:53pm

Temperature Tests

Test	Status	Time
FC1	Pass	10:53pm
SRC	Pass	10:53pm
DET	Pass	10:53pm
BAR	Pass	10:53pm
BT	Pass	10:53pm

Blank Tests

Test	Status	Time
AIR	Pass	10:54pm


Printer Tests

Test	Status	Time
PRNT	Pass	10:54pm

CRC Tests

Test	Status	Time
COMP	Pass	10:54pm
CAL	Pass	10:54pm

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Iredell Instrument Location BAT Mobile Unit 8

Instrument Serial No. 008816 -

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 14 day of January, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

2219283
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

IREDELL COUNTY BAT MOBILE UNIT 8 480

Serial Number: 008816
Test Date: 01/14/2026

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Glasscock, Jerry D

Permit Number: 7180-9235

Effective:

02/01/2025-02/01/2027

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG431002


Exp Date: 11/05/2026

Test	g/210L	Time
DIAG	Pass	7:38am
AIR BLK	.00	7:39am
ACCY CHK	.08	7:40am
AIR BLK	.00	7:41am
SUB TEST	.00	7:41am
AIR BLK	.00	7:42am
SUB TEST	.00	7:44am
AIR BLK	.00	7:45am

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

IREDELL COUNTY BAT MOBILE UNIT 8 480

Serial Number: 008816 Test Record Number: 8015
Test Date: 01/14/2026 Test Time: 7:46am EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	7:46am
FLO	Pass	7:46am
FC	Pass	7:46am

Temperature Tests

Test	Status	Time
FC1	Pass	7:46am
SRC	Pass	7:46am
DET	Pass	7:46am
BAR	Pass	7:46am
BT	Pass	7:46am

Blank Tests

Test	Status	Time
AIR	Pass	7:47am

Printer Tests

Test	Status	Time
PRNT	Pass	7:47am

CRC Tests

Test	Status	Time
COMP	Pass	7:47am
CAL	Pass	7:47am

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Iredell Instrument Location BAT Mobile Unit 8

Instrument Serial No. 008929 -

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 2 day of January, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature] 2219283
Signature of Certifying Official Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

IREDELL COUNTY BAT MOBILE UNIT 8 480

Serial Number: 008929

Test Date: 01/02/2026

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Glasscock, Jerry D

Permit Number: 7180-9235

Effective:

02/01/2025-02/01/2027

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG506303

Exp Date: 03/04/2027

Test	g/210L	Time
DIAG	Pass	10:43pm
AIR BLK	.00	10:44pm
ACCY CHK	.08	10:45pm
AIR BLK	.00	10:46pm
SUB TEST	.00	10:47pm
AIR BLK	.00	10:48pm
SUB TEST	.00	10:50pm
AIR BLK	.00	10:51pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

IREDELL COUNTY BAT MOBILE UNIT 8 480

Serial Number: 008929 Test Record Number: 1712
Test Date: 01/02/2026 Test Time: 10:52pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	10:52pm
FLO	Pass	10:52pm
FC	Pass	10:52pm

Temperature Tests

Test	Status	Time
FC1	Pass	10:52pm
SRC	Pass	10:52pm
DET	Pass	10:52pm
BAR	Pass	10:52pm
BT	Pass	10:52pm

Blank Tests

Test	Status	Time
AIR	Pass	10:53pm

Printer Tests

Test	Status	Time
PRNT	Pass	10:53pm

CRC Tests

Test	Status	Time
COMP	Pass	10:53pm
CAL	Pass	10:53pm

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Iredell Instrument Location BAT Mobile Unit 8
Instrument Serial No. 008929

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 14 day of January, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

2219283
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

IREDELL COUNTY BAT MOBILE UNIT 8 480

Serial Number: 008929

Test Date: 01/14/2026

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Glasscock, Jerry D

Permit Number: 7180-9235

Effective:

02/01/2025-02/01/2027

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG506303

Exp Date: 03/04/2027

Test	g/210L	Time
DIAG	Pass	7:37am
AIR BLK	.00	7:38am
ACCY CHK	.08	7:38am
AIR BLK	.00	7:39am
SUB TEST	.00	7:40am
AIR BLK	.00	7:41am
SUB TEST	.00	7:43am
AIR BLK	.00	7:44am

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

Intox EC/IR-II: Preventive Maintenance

IREDELL COUNTY BAT MOBILE UNIT 8 480

Serial Number: 008929 Test Record Number: 1716
Test Date: 01/14/2026 Test Time: 7:45am EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	7:45am
FLO	Pass	7:45am
FC	Pass	7:45am

Temperature Tests

Test	Status	Time
FC1	Pass	7:45am
SRC	Pass	7:45am
DET	Pass	7:45am
BAR	Pass	7:45am
BT	Pass	7:45am

Blank Tests

Test	Status	Time
AIR	Pass	7:46am

Printer Tests

Test	Status	Time
PRNT	Pass	7:46am

CRC Tests

Test	Status	Time
COMP	Pass	7:46am
CAL	Pass	7:46am

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Johnston Instrument Location Selma Police

Instrument Serial No. 008595 Department

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 12 day of January, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

365156
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

JOHNSTON COUNTY SELMA PD 500

Serial Number: 008595
Test Date: 01/12/2026

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: Garner, Joel K
Permit Number: 0036-5156
Effective:
02/01/2025-02/01/2027

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG417803
Exp Date: 06/26/2026

Test	g/210L	Time
DIAG	Pass	11:04am
AIR BLK	.00	11:05am
ACCY CHK	.07	11:05am
AIR BLK	.00	11:07am
SUB TEST	.00	11:07am
AIR BLK	.00	11:08am
SUB TEST	.00	11:10am
AIR BLK	.00	11:10am

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

Intox EC/IR-II: Preventive Maintenance

JOHNSTON COUNTY SELMA PD 500

Serial Number: 008595 Test Record Number: 1909
Test Date: 01/12/2026 Test Time: 11:11am EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	11:12am
FLO	Pass	11:12am
FC	Pass	11:12am

Temperature Tests

Test	Status	Time
FC1	Pass	11:12am
SRC	Pass	11:12am
DET	Pass	11:12am
BAR	Pass	11:12am
BT	Pass	11:12am

Blank Tests

Test	Status	Time
AIR	Pass	11:13am

Printer Tests

Test	Status	Time
PRNT	Pass	11:13am

CRC Tests

Test	Status	Time
COMP	Pass	11:13am
CAL	Pass	11:13am

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Johnston Instrument Location Clayton Police
Instrument Serial No. 008658 Department

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 14 day of January, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

365156
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

JOHNSTON COUNTY CLAYTON PD 500

Serial Number: 008658
Test Date: 01/14/2026

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE

Analyst's Name: Garner, Joel K
Permit Number: 0036-5156
Effective:
02/01/2025-02/01/2027

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG534301
Exp Date: 12/09/2027


Test	g/210L	Time
DIAG	Pass	9:40am
AIR BLK	.00	9:41am
ACCY CHK	.08	9:42am
AIR BLK	.00	9:43am
SUB TEST	.00	9:44am
AIR BLK	.00	9:45am
SUB TEST	.00	9:46am
AIR BLK	.00	9:47am

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR

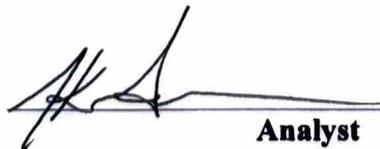

Analyst

Intox EC/IR-II: Preventive Maintenance

JOHNSTON COUNTY CLAYTON PD 500

Serial Number: 008658 Test Record Number: 2437
Test Date: 01/14/2026 Test Time: 9:48am EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	9:48am
FLO	Pass	9:48am
FC	Pass	9:48am

Temperature Tests

Test	Status	Time
FC1	Pass	9:48am
SRC	Pass	9:48am
DET	Pass	9:48am
BAR	Pass	9:48am
BT	Pass	9:48am

Blank Tests

Test	Status	Time
AIR	Pass	9:49am


Printer Tests

Test	Status	Time
PRNT	Pass	9:49am

CRC Tests

Test	Status	Time
COMP	Pass	9:49am
CAL	Pass	9:49am

Preventive Maintenance
Status: Pass

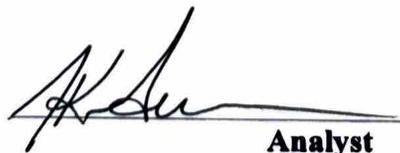

Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County Johnston Instrument Location Johnston County
Instrument Serial No. 008721 Detention Center

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 20 day of January, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

365156
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

JOHNSTON COUNTY DETENTION CENTER 500

Serial Number: 008721
Test Date: 01/20/2026

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: Garner, Joel K
Permit Number: 0036-5156
Effective:
02/01/2025-02/01/2027

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG534301
Exp Date: 12/09/2027


Test	g/210L	Time
DIAG	Pass	4:35pm
AIR BLK	.00	4:36pm
ACCY CHK	.07	4:37pm
AIR BLK	.00	4:38pm
SUB TEST	.00	4:39pm
AIR BLK	.00	4:39pm
SUB TEST	.00	4:41pm
AIR BLK	.00	4:42pm

Reported AC: .00 g/210L

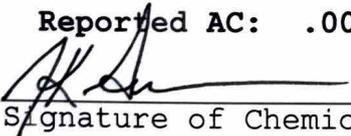

Signature of Chemical Analyst

Court CVR

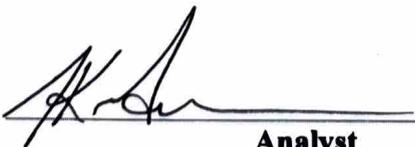

Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

JOHNSTON COUNTY DETENTION CENTER 500

Serial Number: 008721 Test Record Number: 2426
Test Date: 01/20/2026 Test Time: 4:43pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	4:43pm
FLO	Pass	4:43pm
FC	Pass	4:43pm

Temperature Tests

Test	Status	Time
FC1	Pass	4:43pm
SRC	Pass	4:43pm
DET	Pass	4:43pm
BAR	Pass	4:43pm
BT	Pass	4:43pm

Blank Tests

Test	Status	Time
AIR	Pass	4:44pm

Printer Tests

Test	Status	Time
PRNT	Pass	4:44pm

CRC Tests

Test	Status	Time
COMP	Pass	4:44pm
CAL	Pass	4:44pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County Johnston Instrument Location Johnston County
Instrument Serial No. 008863 Detention Center

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 20 day of January, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

365156
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

JOHNSTON COUNTY DETENTION CENTER 500

Serial Number: 008863
Test Date: 01/20/2026

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: Garner, Joel K
Permit Number: 0036-5156
Effective:
02/01/2025-02/01/2027

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG534301
Exp Date: 12/09/2027

Test	g/210L	Time
DIAG	Pass	5:44pm
AIR BLK	.00	5:45pm
ACCY CHK	.07	5:45pm
AIR BLK	.00	5:46pm
SUB TEST	.00	5:47pm
AIR BLK	.00	5:48pm
SUB TEST	.00	5:50pm
AIR BLK	.00	5:51pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

JOHNSTON COUNTY DETENTION CENTER 500

Serial Number: 008863 Test Record Number: 1098
Test Date: 01/20/2026 Test Time: 5:51pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	5:52pm
FLO	Pass	5:52pm
FC	Pass	5:52pm

Temperature Tests

Test	Status	Time
FC1	Pass	5:52pm
SRC	Pass	5:52pm
DET	Pass	5:52pm
BAR	Pass	5:52pm
BT	Pass	5:52pm

Blank Tests

Test	Status	Time
AIR	Pass	5:53pm


Printer Tests

Test	Status	Time
PRNT	Pass	5:53pm

CRC Tests

Test	Status	Time
COMP	Pass	5:53pm
CAL	Pass	5:53pm

Preventive Maintenance
Status: Pass

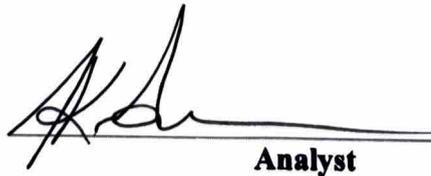

Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Johnston Instrument Location Benson Police
Instrument Serial No. 008885 Department

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 14 day of January, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

365156
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

JOHNSTON COUNTY BENSON PD 500

Serial Number: 008885
Test Date: 01/14/2026

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Garner, Joel K

Permit Number: 0036-5156

Effective:

02/01/2025-02/01/2027

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG534301

Exp Date: 12/09/2027

Test	g/210L	Time
DIAG	Pass	10:54am
AIR BLK	.00	10:54am
ACCY CHK	.08	10:55am
AIR BLK	.00	10:56am
SUB TEST	.00	10:57am
AIR BLK	.00	10:57am
SUB TEST	.00	10:59am
AIR BLK	.00	11:00am

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

JOHNSTON COUNTY BENSON PD 500

Serial Number: 008885 Test Record Number: 925
Test Date: 01/14/2026 Test Time: 11:01am EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	11:01am
FLO	Pass	11:01am
FC	Pass	11:01am

Temperature Tests

Test	Status	Time
FC1	Pass	11:01am
SRC	Pass	11:01am
DET	Pass	11:01am
BAR	Pass	11:01am
BT	Pass	11:01am

Blank Tests

Test	Status	Time
AIR	Pass	11:02am


Printer Tests

Test	Status	Time
PRNT	Pass	11:02am

CRC Tests

Test	Status	Time
COMP	Pass	11:02am
CAL	Pass	11:02am

Preventive Maintenance
Status: Pass

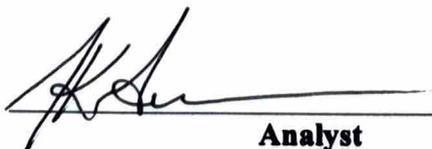

Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County LEE Instrument Location LEE COUNTY
Instrument Serial No. 008645 DETENTION CENTER

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 9 day of JANUARY, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Handwritten Signature]
Signature of Certifying Official

239771
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

LEE COUNTY DETENTION CENTER 520

Serial Number: 008645
Test Date: 01/09/2026

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE

Analyst's Name: Galloway, Charles L
Permit Number: 0023-9771
Effective:
02/01/2025-02/01/2027

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG431002
Exp Date: 11/05/2026

Test	g/210L	Time
DIAG	Pass	3:01pm
AIR BLK	.00	3:02pm
ACCY CHK	.08	3:02pm
AIR BLK	.00	3:03pm
SUB TEST	.00	3:04pm
AIR BLK	.00	3:05pm
SUB TEST	.00	3:06pm
AIR BLK	.00	3:07pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

Intox EC/IR-II: Preventive Maintenance

LEE COUNTY DETENTION CENTER 520

Serial Number: 008645 Test Record Number: 2768
Test Date: 01/09/2026 Test Time: 3:09pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	3:10pm
FLO	Pass	3:10pm
FC	Pass	3:10pm

Temperature Tests

Test	Status	Time
FC1	Pass	3:10pm
SRC	Pass	3:10pm
DET	Pass	3:10pm
BAR	Pass	3:10pm
BT	Pass	3:10pm

Blank Tests

Test	Status	Time
AIR	Pass	3:10pm

Printer Tests

Test	Status	Time
PRNT	Pass	3:10pm

CRC Tests

Test	Status	Time
COMP	Pass	3:11pm
CAL	Pass	3:11pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County LEE Instrument Location SANFORD POLICE
Instrument Serial No. 008867 DEPARTMENT

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 9 day of JANUARY, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.




Signature of Certifying Official

239771
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

LEE COUNTY SANFORD POLICE DEPT 520

Serial Number: 008867
Test Date: 01/09/2026

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: Galloway, Charles L
Permit Number: 0023-9771
Effective:
02/01/2025-02/01/2027

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test


Lot Number: AG534301
Exp Date: 12/09/2027

Test	g/210L	Time
DIAG	Pass	12:40pm
AIR BLK	.00	12:40pm
ACCY CHK	.08	12:41pm
AIR BLK	.00	12:42pm
SUB TEST	.00	12:43pm
AIR BLK	.00	12:43pm
SUB TEST	.00	12:45pm
AIR BLK	.00	12:46pm

Reported AC: .00 g/210L

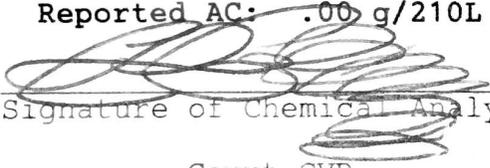
Signature of Chemical Analyst

Court CVR

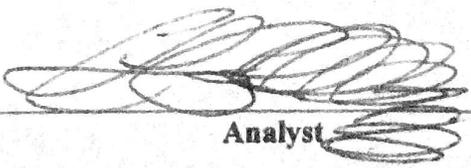
Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

LEE COUNTY SANFORD POLICE DEPT 520

Serial Number: 008867 Test Record Number: 1585
Test Date: 01/09/2026 Test Time: 12:52pm EST

System Check: Passed

Baseline Tests

Test	Status	Time
IR	Pass	12:53pm
FLO	Pass	12:53pm
FC	Pass	12:53pm

Temperature Tests

Test	Status	Time
FC1	Pass	12:53pm
SRC	Pass	12:53pm
DET	Pass	12:53pm
BAR	Pass	12:53pm
BT	Pass	12:53pm

Blank Tests

Test	Status	Time
AIR	Pass	12:54pm


Printer Tests

Test	Status	Time
PRNT	Pass	12:54pm

CRC Tests

Test	Status	Time
COMP	Pass	12:54pm
CAL	Pass	12:54pm

Preventive Maintenance
Status: Pass

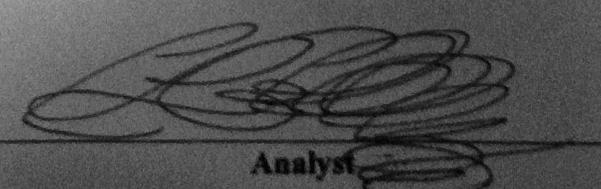
Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County LENOIR Instrument Location BAT MOBILE UNIT 12

Instrument Serial No. 008601

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 3rd day of JANUARY, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Signature of Certifying Official

Certificate Number

083034

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

LENOIR COUNTY BAT MOBILE UNIT 12 530

Serial Number: 008601
Test Date: 01/03/2026

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name:
Crutchfield, Jr, Marshall B
Permit Number: 0008-3034
Effective:
07/01/2025-07/01/2027

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG501307
Exp Date: 01/13/2027

Test	g/210L	Time
DIAG	Pass	10:35pm
AIR BLK	.00	10:36pm
ACCY CHK	.07	10:37pm
AIR BLK	.00	10:38pm
SUB TEST	.00	10:38pm
AIR BLK	.00	10:39pm
SUB TEST	.00	10:41pm
AIR BLK	.00	10:42pm

Reported AC: .00 g/210L



Signature of Chemical Analyst
Court CVR



Analyst

Intox EC/IR-II: Preventive Maintenance

LENOIR COUNTY BAT MOBILE UNIT 12 530

Serial Number: 008601 Test Record Number: 1869
Test Date: 01/03/2026 Test Time: 10:43pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	10:43pm
FLO	Pass	10:43pm
FC	Pass	10:43pm

Temperature Tests

Test	Status	Time
FC1	Pass	10:44pm
SRC	Pass	10:44pm
DET	Pass	10:44pm
BAR	Pass	10:44pm
BT	Pass	10:44pm

Blank Tests

Test	Status	Time
AIR	Pass	10:44pm

Printer Tests

Test	Status	Time
PRNT	Pass	10:44pm

CRC Tests

Test	Status	Time
COMP	Pass	10:44pm
CAL	Pass	10:44pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County LENOIR Instrument Location BAT MOBILE UNIT 12

Instrument Serial No. 008788

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 3rd day of January, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

083034
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

LENOIR COUNTY BAT MOBILE UNIT 12 530

Serial Number: 008788

Test Date: 01/03/2026

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name:

Crutchfield, Jr, Marshall B

Permit Number: 0008-3034

Effective:

07/01/2025-07/01/2027

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG417802

Exp Date: 06/26/2026

Test	g/210L	Time
DIAG	Pass	10:31pm
AIR BLK	.00	10:32pm
ACCY CHK	.08	10:32pm
AIR BLK	.00	10:33pm
SUB TEST	.00	10:34pm
AIR BLK	.00	10:35pm
SUB TEST	.00	10:36pm
AIR BLK	.00	10:37pm

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR

Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

LENOIR COUNTY BAT MOBILE UNIT 12 530

Serial Number: 008788 Test Record Number: 2498
Test Date: 01/03/2026 Test Time: 10:39pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	10:39pm
FLO	Pass	10:39pm
FC	Pass	10:39pm

Temperature Tests

Test	Status	Time
FC1	Pass	10:39pm
SRC	Pass	10:39pm
DET	Pass	10:39pm
BAR	Pass	10:39pm
BT	Pass	10:39pm

Blank Tests

Test	Status	Time
AIR	Pass	10:40pm

Printer Tests

Test	Status	Time
PRNT	Pass	10:40pm

CRC Tests

Test	Status	Time
COMP	Pass	10:40pm
CAL	Pass	10:40pm

Preventive Maintenance
Status: Pass



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Lincoln Instrument Location Lincoln County Jail
Instrument Serial No. 008827 Lincolnton, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 28th day of January, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Boyo Hulms
Signature of Certifying Official

849845
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

LINCOLN COUNTY LINCOLN COUNTY SO 540

Serial Number: 008827
Test Date: 01/28/2026

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: Helms, Bryce A
Permit Number: 0084-9845
Effective:
02/01/2025-02/01/2027

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG506303
Exp Date: 03/04/2027


Test	g/210L	Time
DIAG	Pass	1:52pm
AIR BLK	.00	1:52pm
ACCY CHK	.08	1:53pm
AIR BLK	.00	1:54pm
SUB TEST	.00	1:55pm
AIR BLK	.00	1:56pm
SUB TEST	.00	1:57pm
AIR BLK	.00	1:58pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR

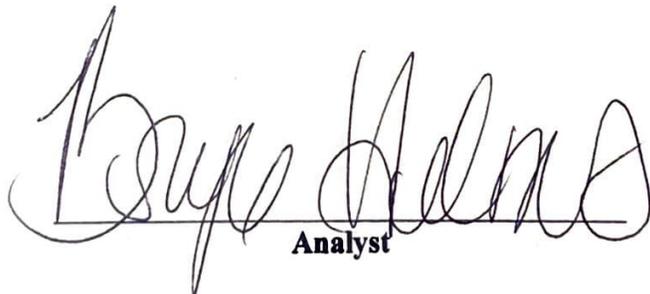

Analyst

Intox EC/IR-II: Preventive Maintenance

LINCOLN COUNTY LINCOLN COUNTY SO 540

Serial Number: 008827 Test Record Number: 4491
Test Date: 01/28/2026 Test Time: 1:59pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	1:59pm
FLO	Pass	1:59pm
FC	Pass	1:59pm

Temperature Tests

Test	Status	Time
FC1	Pass	1:59pm
SRC	Pass	1:59pm
DET	Pass	1:59pm
BAR	Pass	1:59pm
BT	Pass	1:59pm

Blank Tests

Test	Status	Time
AIR	Pass	2:00pm


Printer Tests

Test	Status	Time
PRNT	Pass	2:00pm

CRC Tests

Test	Status	Time
COMP	Pass	2:00pm
CAL	Pass	2:00pm

Preventive Maintenance
Status: Pass

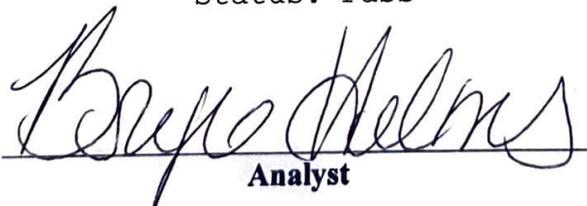
Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County Martin Instrument Location Martin Co. S.O.
Instrument Serial No. 008912 305 E. Main St.
Williamston, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 7th day of January, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Mark J. Russell
Signature of Certifying Official

206727
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

MARTIN COUNTY SHERIFF'S OFFICE 570

Serial Number: 008912

Test Date: 01/07/2026

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Chappell, Mark A

Permit Number: 0020-6272

Effective:

02/01/2025-02/01/2027

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG431001


Exp Date: 11/05/2026

Test	g/210L	Time
DIAG	Pass	10:39am
AIR BLK	.00	10:40am
ACCY CHK	.08	10:40am
AIR BLK	.00	10:42am
SUB TEST	.00	10:43am
AIR BLK	.00	10:44am
SUB TEST	.00	10:45am
AIR BLK	.00	10:46am

Reported AC: .00 g/210L

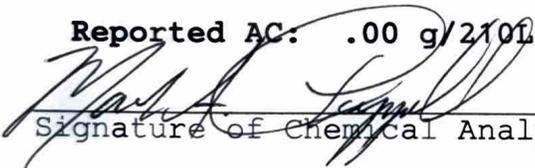
Signature of Chemical Analyst

Court CVR

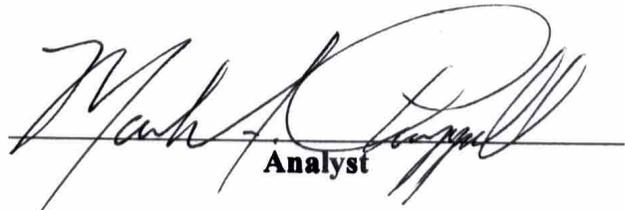
Analyst

Intox EC/IR-II: Preventive Maintenance

MARTIN COUNTY SHERIFF'S OFFICE 570

Serial Number: 008912 Test Record Number: 2387
Test Date: 01/07/2026 Test Time: 10:47am EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	10:47am
FLO	Pass	10:47am
FC	Pass	10:47am

Temperature Tests

Test	Status	Time
FC1	Pass	10:47am
SRC	Pass	10:47am
DET	Pass	10:47am
BAR	Pass	10:47am
BT	Pass	10:47am

Blank Tests

Test	Status	Time
AIR	Pass	10:48am


Printer Tests

Test	Status	Time
PRNT	Pass	10:48am

CRC Tests

Test	Status	Time
COMP	Pass	10:48am
CAL	Pass	10:48am

Preventive Maintenance
Status: Pass

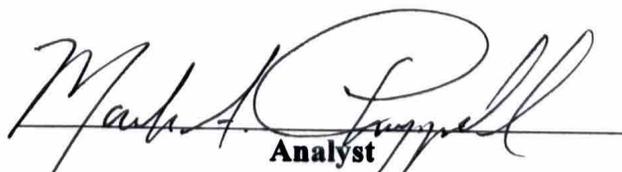
Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Mecklenburg Instrument Location BAT Mobile Unit 8
Instrument Serial No. 008615 —

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 15 day of January, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

2219283
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

MECKLENBURG COUNTY BAT MOBILE UNIT 8
590

Serial Number: 008615
Test Date: 01/15/2026

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Glasscock, Jerry D

Permit Number: 7180-9235

Effective:

02/01/2025-02/01/2027

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG405102

Exp Date: 02/20/2026

Test	g/210L	Time
DIAG	Pass	8:36am
AIR BLK	.00	8:37am
ACCY CHK	.07	8:38am
AIR BLK	.00	8:39am
SUB TEST	.00	8:39am
AIR BLK	.00	8:40am
SUB TEST	.00	8:42am
AIR BLK	.00	8:43am

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

MECKLENBURG COUNTY BAT MOBILE UNIT 8 590

Serial Number: 008615 Test Record Number: 6223
Test Date: 01/15/2026 Test Time: 8:44am EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	8:44am
FLO	Pass	8:44am
FC	Pass	8:44am

Temperature Tests

Test	Status	Time
FC1	Pass	8:44am
SRC	Pass	8:44am
DET	Pass	8:44am
BAR	Pass	8:44am
BT	Pass	8:44am

Blank Tests

Test	Status	Time
AIR	Pass	8:45am

Printer Tests

Test	Status	Time
PRNT	Pass	8:45am

CRC Tests

Test	Status	Time
COMP	Pass	8:45am
CAL	Pass	8:45am

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Mecklenburg Instrument Location BAT Mobile Unit 8
Instrument Serial No. 008615

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 22 day of January, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

2219283
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

MECKLENBURG COUNTY BAT MOBILE UNIT 8
590

Serial Number: 008615
Test Date: 01/22/2026

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: Glasscock, Jerry D
Permit Number: 7180-9235
Effective:
02/01/2025-02/01/2027

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG405102
Exp Date: 02/20/2026

Test	g/210L	Time
DIAG	Pass	9:08pm
AIR BLK	.00	9:09pm
ACCY CHK	.07	9:09pm
AIR BLK	.00	9:10pm
SUB TEST	.00	9:11pm
AIR BLK	.00	9:12pm
SUB TEST	.00	9:14pm
AIR BLK	.00	9:15pm

Reported AC: .00 g/210L

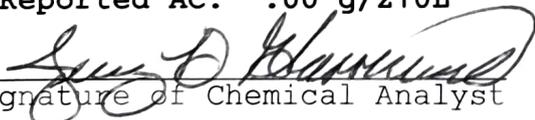
Signature of Chemical Analyst

Court CVR


Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

MECKLENBURG COUNTY BAT MOBILE UNIT 8 590

Serial Number: 008615 Test Record Number: 6229
Test Date: 01/22/2026 Test Time: 9:15pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	9:16pm
FLO	Pass	9:16pm
FC	Pass	9:16pm

Temperature Tests

Test	Status	Time
FC1	Pass	9:16pm
SRC	Pass	9:16pm
DET	Pass	9:16pm
BAR	Pass	9:16pm
BT	Pass	9:16pm

Blank Tests

Test	Status	Time
AIR	Pass	9:17pm

Printer Tests

Test	Status	Time
PRNT	Pass	9:17pm

CRC Tests

Test	Status	Time
COMP	Pass	9:17pm
CAL	Pass	9:17pm

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Mecklenburg Instrument Location BAT Mobile Unit 8

Instrument Serial No. 008615 _____

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 29 day of January, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

2219283
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

MECKLENBURG COUNTY BAT MOBILE UNIT 8
590

Serial Number: 008615
Test Date: 01/29/2026

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE

Analyst's Name: Glasscock, Jerry D
Permit Number: 7180-9235
Effective:
02/01/2025-02/01/2027

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG405102
Exp Date: 02/20/2026

Test	g/210L	Time
DIAG	Pass	9:43pm
AIR BLK	.00	9:44pm
ACCY CHK	.07	9:44pm
AIR BLK	.00	9:45pm
SUB TEST	.00	9:46pm
AIR BLK	.00	9:47pm
SUB TEST	.00	9:48pm
AIR BLK	.00	9:49pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

Intox EC/IR-II: Preventive Maintenance

MECKLENBURG COUNTY BAT MOBILE UNIT 8 590

Serial Number: 008615 Test Record Number: 6235

Test Date: 01/29/2026 Test Time: 9:50pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	9:50pm
FLO	Pass	9:50pm
FC	Pass	9:50pm

Temperature Tests

Test	Status	Time
FC1	Pass	9:50pm
SRC	Pass	9:50pm
DET	Pass	9:50pm
BAR	Pass	9:50pm
BT	Pass	9:50pm

Blank Tests

Test	Status	Time
AIR	Pass	9:51pm

Printer Tests

Test	Status	Time
PRNT	Pass	9:51pm

CRC Tests

Test	Status	Time
COMP	Pass	9:51pm
CAL	Pass	9:51pm

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Mecklenburg Instrument Location Mecklenburg Co 80
Instrument Serial No. 008690 Charlotte, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 22nd day of January, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

849845
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

MECKLENBURG COUNTY SHERIFFS OFFICE 590

Serial Number: 008690
Test Date: 01/22/2026

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: Helms, Bryce A
Permit Number: 0084-9845
Effective:
02/01/2025-02/01/2027

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG506303
Exp Date: 03/04/2027

Test	g/210L	Time
DIAG	Pass	11:29am
AIR BLK	.00	11:30am
ACCY CHK	.08	11:30am
AIR BLK	.00	11:32am
SUB TEST	.00	11:32am
AIR BLK	.00	11:33am
SUB TEST	.00	11:35am
AIR BLK	.00	11:35am

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

Intox EC/IR-II: Preventive Maintenance

MECKLENBURG COUNTY SHERIFFS OFFICE 590

Serial Number: 008690 Test Record Number: 7892
Test Date: 01/22/2026 Test Time: 11:40am EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	11:41am
FLO	Pass	11:41am
FC	Pass	11:41am

Temperature Tests

Test	Status	Time
FC1	Pass	11:41am
SRC	Pass	11:41am
DET	Pass	11:41am
BAR	Pass	11:41am
BT	Pass	11:41am

Blank Tests

Test	Status	Time
AIR	Pass	11:42am


Printer Tests

Test	Status	Time
PRNT	Pass	11:42am

CRC Tests

Test	Status	Time
COMP	Pass	11:42am
CAL	Pass	11:42am

Preventive Maintenance
Status: Pass

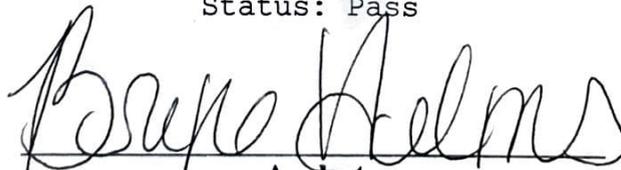
Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County MECKLENBURG Instrument Location CORNELIUS PD

Instrument Serial No. 008692 CORNELIUS NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 28 day of JANUARY, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



James S. Fleming
Signature of Certifying Official

274970
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

MECKLENBURG COUNTY CORNELIUS PD 590

Serial Number: 008692
Test Date: 01/28/2026

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: Fleming, Tina S
Permit Number: 0027-4970
Effective:
02/01/2025-02/01/2027

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG431001
Exp Date: 11/05/2026

Test	g/210L	Time
DIAG	Pass	11:12am
AIR BLK	.00	11:13am
ACCY CHK	.08	11:13am
AIR BLK	.00	11:15am
SUB TEST	.00	11:15am
AIR BLK	.00	11:16am
SUB TEST	.00	11:18am
AIR BLK	.00	11:19am

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

MECKLENBURG COUNTY CORNELIUS PD 590

Serial Number: 008692 Test Record Number: 3920
Test Date: 01/28/2026 Test Time: 11:21am EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	11:21am
FLO	Pass	11:21am
FC	Pass	11:21am

Temperature Tests

Test	Status	Time
FC1	Pass	11:21am
SRC	Pass	11:21am
DET	Pass	11:21am
BAR	Pass	11:21am
BT	Pass	11:21am

Blank Tests

Test	Status	Time
AIR	Pass	11:22am

Printer Tests

Test	Status	Time
PRNT	Pass	11:22am

CRC Tests

Test	Status	Time
COMP	Pass	11:22am
CAL	Pass	11:22am

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County Mecklenburg Instrument Location BAT Mobile Unit 8
Instrument Serial No. 008736 —

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 15 day of January, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

2219283
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

MECKLENBURG COUNTY BAT MOBILE UNIT 8
590

Serial Number: 008736
Test Date: 01/15/2026

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE

Analyst's Name: Glasscock, Jerry D
Permit Number: 7180-9235
Effective:
02/01/2025-02/01/2027

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG405102
Exp Date: 02/20/2026

Test	g/210L	Time
DIAG	Pass	8:36am
AIR BLK	.00	8:37am
ACCY CHK	.07	8:38am
AIR BLK	.00	8:39am
SUB TEST	.00	8:39am
AIR BLK	.00	8:40am
SUB TEST	.00	8:42am
AIR BLK	.00	8:43am

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

MECKLENBURG COUNTY BAT MOBILE UNIT 8 590

Serial Number: 008736 Test Record Number: 1581
Test Date: 01/15/2026 Test Time: 8:44am EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	8:44am
FLO	Pass	8:44am
FC	Pass	8:44am

Temperature Tests

Test	Status	Time
FC1	Pass	8:44am
SRC	Pass	8:44am
DET	Pass	8:44am
BAR	Pass	8:44am
BT	Pass	8:44am

Blank Tests

Test	Status	Time
AIR	Pass	8:45am

Printer Tests

Test	Status	Time
PRNT	Pass	8:45am

CRC Tests

Test	Status	Time
COMP	Pass	8:45am
CAL	Pass	8:45am

Preventive Maintenance
Status: Pass


Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Mecklenburg Instrument Location BAT Mobile Unit 8

Instrument Serial No. 008736

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 22 day of January, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

2219283
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

MECKLENBURG COUNTY BAT MOBILE UNIT 8
590

Serial Number: 008736
Test Date: 01/22/2026

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: Glasscock, Jerry D
Permit Number: 7180-9235
Effective:
02/01/2025-02/01/2027

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG405102
Exp Date: 02/20/2026

Test	g/210L	Time
DIAG	Pass	9:11pm
AIR BLK	.00	9:12pm
ACCY CHK	.07	9:13pm
AIR BLK	.00	9:13pm
SUB TEST	.00	9:14pm
AIR BLK	.00	9:15pm
SUB TEST	.00	9:17pm
AIR BLK	.00	9:17pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

Intox EC/IR-II: Preventive Maintenance

MECKLENBURG COUNTY BAT MOBILE UNIT 8 590

Serial Number: 008736 Test Record Number: 1587
Test Date: 01/22/2026 Test Time: 9:18pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	9:18pm
FLO	Pass	9:18pm
FC	Pass	9:18pm

Temperature Tests

Test	Status	Time
FC1	Pass	9:18pm
SRC	Pass	9:18pm
DET	Pass	9:18pm
BAR	Pass	9:18pm
BT	Pass	9:18pm

Blank Tests

Test	Status	Time
AIR	Pass	9:19pm


Printer Tests

Test	Status	Time
PRNT	Pass	9:19pm

CRC Tests

Test	Status	Time
COMP	Pass	9:19pm
CAL	Pass	9:19pm

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County Mecklenburg Instrument Location BAT Mobile Unit 8
Instrument Serial No. 008736 _____

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 29 day of January, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

2219283
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

MECKLENBURG COUNTY BAT MOBILE UNIT 8
590

Serial Number: 008736
Test Date: 01/29/2026

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE

Analyst's Name: Glasscock, Jerry D
Permit Number: 7180-9235
Effective:
02/01/2025-02/01/2027

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG405102
Exp Date: 02/20/2026

Test	g/210L	Time
DIAG	Pass	9:42pm
AIR BLK	.00	9:43pm
ACCY CHK	.07	9:44pm
AIR BLK	.00	9:45pm
SUB TEST	.00	9:45pm
AIR BLK	.00	9:46pm
SUB TEST	.00	9:48pm
AIR BLK	.00	9:49pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

Intox EC/IR-II: Preventive Maintenance

MECKLENBURG COUNTY BAT MOBILE UNIT 8 590

Serial Number: 008736 Test Record Number: 1591
Test Date: 01/29/2026 Test Time: 9:49pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	9:50pm
FLO	Pass	9:50pm
FC	Pass	9:50pm

Temperature Tests

Test	Status	Time
FC1	Pass	9:50pm
SRC	Pass	9:50pm
DET	Pass	9:50pm
BAR	Pass	9:50pm
BT	Pass	9:50pm

Blank Tests

Test	Status	Time
AIR	Pass	9:51pm

Printer Tests

Test	Status	Time
PRNT	Pass	9:51pm

CRC Tests

Test	Status	Time
COMP	Pass	9:51pm
CAL	Pass	9:51pm

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County Mecklenburg Instrument Location BAT Mobile Unit 8
Instrument Serial No. 008775 ✓

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 15 day of January, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature] 2219283
Signature of Certifying Official Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

MECKLENBURG COUNTY BAT MOBILE UNIT 8
590

Serial Number: 008775
Test Date: 01/15/2026

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE

Analyst's Name: Glasscock, Jerry D
Permit Number: 7180-9235
Effective:
02/01/2025-02/01/2027

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG506303
Exp Date: 03/04/2027

Test	g/210L	Time
DIAG	Pass	8:37am
AIR BLK	.00	8:38am
ACCY CHK	.08	8:39am
AIR BLK	.00	8:40am
SUB TEST	.00	8:40am
AIR BLK	.00	8:41am
SUB TEST	.00	8:43am
AIR BLK	.00	8:44am

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

MECKLENBURG COUNTY BAT MOBILE UNIT 8 590

Serial Number: 008775 Test Record Number: 2435
Test Date: 01/15/2026 Test Time: 8:44am EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	8:45am
FLO	Pass	8:45am
FC	Pass	8:45am

Temperature Tests

Test	Status	Time
FC1	Pass	8:45am
SRC	Pass	8:45am
DET	Pass	8:45am
BAR	Pass	8:45am
BT	Pass	8:45am

Blank Tests

Test	Status	Time
AIR	Pass	8:45am

Printer Tests

Test	Status	Time
PRNT	Pass	8:45am

CRC Tests

Test	Status	Time
COMP	Pass	8:46am
CAL	Pass	8:46am

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Mecklenburg Instrument Location BAT Mobile Unit 8
Instrument Serial No. 008775 -

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 22 day of January, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

2219283
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

MECKLENBURG COUNTY BAT MOBILE UNIT 8
590

Serial Number: 008775
Test Date: 01/22/2026

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE

Analyst's Name: Glasscock, Jerry D
Permit Number: 7180-9235
Effective:
02/01/2025-02/01/2027

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG506303
Exp Date: 03/04/2027

Test	g/210L	Time
DIAG	Pass	9:13pm
AIR BLK	.00	9:14pm
ACCY CHK	.08	9:14pm
AIR BLK	.00	9:15pm
SUB TEST	.00	9:16pm
AIR BLK	.00	9:16pm
SUB TEST	.00	9:18pm
AIR BLK	.00	9:19pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

Intox EC/IR-II: Preventive Maintenance

MECKLENBURG COUNTY BAT MOBILE UNIT 8 590

Serial Number: 008775 Test Record Number: 2441
Test Date: 01/22/2026 Test Time: 9:20pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	9:20pm
FLO	Pass	9:20pm
FC	Pass	9:20pm

Temperature Tests

Test	Status	Time
FC1	Pass	9:20pm
SRC	Pass	9:20pm
DET	Pass	9:20pm
BAR	Pass	9:20pm
BT	Pass	9:20pm

Blank Tests

Test	Status	Time
AIR	Pass	9:21pm

Printer Tests

Test	Status	Time
PRNT	Pass	9:21pm

CRC Tests

Test	Status	Time
COMP	Pass	9:21pm
CAL	Pass	9:21pm

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH


PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Mecklenburg Instrument Location BAT Mobile Unit 8
Instrument Serial No. 008775 _____

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 29 day of January, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Gay D. Klawns
Signature of Certifying Official

2219283
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

MECKLENBURG COUNTY BAT MOBILE UNIT 8
590

Serial Number: 008775
Test Date: 01/29/2026

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE

Analyst's Name: *Glasscock, Jerry D*
Permit Number: 7180-9235
Effective:
02/01/2025-02/01/2027

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG506303
Exp Date: 03/04/2027

Test	g/210L	Time
DIAG	Pass	9:42pm
AIR BLK	.00	9:43pm
ACCY CHK	.08	9:43pm
AIR BLK	.00	9:44pm
SUB TEST	.00	9:45pm
AIR BLK	.00	9:45pm
SUB TEST	.00	9:47pm
AIR BLK	.00	9:48pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

Intox EC/IR-II: Preventive Maintenance

MECKLENBURG COUNTY BAT MOBILE UNIT 8 590

Serial Number: 008775 Test Record Number: 2445
Test Date: 01/29/2026 Test Time: 9:49pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	9:49pm
FLO	Pass	9:49pm
FC	Pass	9:50pm

Temperature Tests

Test	Status	Time
FC1	Pass	9:50pm
SRC	Pass	9:50pm
DET	Pass	9:50pm
BAR	Pass	9:50pm
BT	Pass	9:50pm

Blank Tests

Test	Status	Time
AIR	Pass	9:50pm

Printer Tests

Test	Status	Time
PRNT	Pass	9:50pm

CRC Tests

Test	Status	Time
COMP	Pass	9:51pm
CAL	Pass	9:51pm

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Mecklenburg Instrument Location BAT Mobile Unit 8
Instrument Serial No. 008816

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 15 day of January, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

2219283
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

MECKLENBURG COUNTY BAT MOBILE UNIT 8
590

Serial Number: 008816
Test Date: 01/15/2026

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE

Analyst's Name: Glasscock, Jerry D
Permit Number: 7180-9235
Effective:
02/01/2025-02/01/2027

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG431002
Exp Date: 11/05/2026

Test	g/210L	Time
DIAG	Pass	8:39am
AIR BLK	.00	8:40am
ACCY CHK	.08	8:40am
AIR BLK	.00	8:41am
SUB TEST	.00	8:42am
AIR BLK	.00	8:43am
SUB TEST	.00	8:44am
AIR BLK	.00	8:45am

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

MECKLENBURG COUNTY BAT MOBILE UNIT 8 590

Serial Number: 008816 Test Record Number: 8017
Test Date: 01/15/2026 Test Time: 8:46am EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	8:46am
FLO	Pass	8:46am
FC	Pass	8:46am

Temperature Tests

Test	Status	Time
FC1	Pass	8:46am
SRC	Pass	8:46am
DET	Pass	8:46am
BAR	Pass	8:46am
BT	Pass	8:46am

Blank Tests

Test	Status	Time
AIR	Pass	8:47am

Printer Tests

Test	Status	Time
PRNT	Pass	8:47am

CRC Tests

Test	Status	Time
COMP	Pass	8:47am
CAL	Pass	8:47am

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County Mecklenburg Instrument Location BAT Mobile Unit 8
Instrument Serial No. 008816 _____

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 22 day of January, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

2219283
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

MECKLENBURG COUNTY BAT MOBILE UNIT 8
590

Serial Number: 008816
Test Date: 01/22/2026

Citation Number: M0000000-0
Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911
Subject's Sex: Male

Driver's License State: XX
Driver's License Number: NONE

Analyst's Name: Glasscock, Jerry D
Permit Number: 7180-9235
Effective:
02/01/2025-02/01/2027

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG431002
Exp Date: 11/05/2026

Test	g/210L	Time
DIAG	Pass	9:15pm
AIR BLK	.00	9:16pm
ACCY CHK	.08	9:17pm
AIR BLK	.00	9:18pm
SUB TEST	.00	9:18pm
AIR BLK	.00	9:19pm
SUB TEST	.00	9:21pm
AIR BLK	.00	9:22pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

Intox EC/IR-II: Preventive Maintenance

MECKLENBURG COUNTY BAT MOBILE UNIT 8 590

Serial Number: 008816 Test Record Number: 8023
Test Date: 01/22/2026 Test Time: 9:23pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	9:24pm
FLO	Pass	9:24pm
FC	Pass	9:24pm

Temperature Tests

Test	Status	Time
FC1	Pass	9:24pm
SRC	Pass	9:24pm
DET	Pass	9:24pm
BAR	Pass	9:24pm
BT	Pass	9:24pm

Blank Tests

Test	Status	Time
AIR	Pass	9:25pm

Printer Tests

Test	Status	Time
PRNT	Pass	9:25pm

CRC Tests

Test	Status	Time
COMP	Pass	9:25pm
CAL	Pass	9:25pm

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Mecklenburg Instrument Location BAT Mobile Unit 8
Instrument Serial No. 008816

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 29 day of January, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

2219283
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

MECKLENBURG COUNTY BAT MOBILE UNIT 8
590

Serial Number: 008816
Test Date: 01/29/2026

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE

Analyst's Name: Glasscock, Jerry D
Permit Number: 7180-9235
Effective:
02/01/2025-02/01/2027

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG431002
Exp Date: 11/05/2026

Test	g/210L	Time
DIAG	Pass	9:41pm
AIR BLK	.00	9:42pm
ACCY CHK	.08	9:43pm
AIR BLK	.00	9:44pm
SUB TEST	.00	9:44pm
AIR BLK	.00	9:45pm
SUB TEST	.00	9:47pm
AIR BLK	.00	9:47pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

Intox EC/IR-II: Preventive Maintenance

MECKLENBURG COUNTY BAT MOBILE UNIT 8 590

Serial Number: 008816 Test Record Number: 8027
Test Date: 01/29/2026 Test Time: 9:53pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	9:54pm
FLO	Pass	9:54pm
FC	Pass	9:54pm

Temperature Tests

Test	Status	Time
FC1	Pass	9:54pm
SRC	Pass	9:54pm
DET	Pass	9:54pm
BAR	Pass	9:54pm
BT	Pass	9:54pm

Blank Tests

Test	Status	Time
AIR	Pass	9:55pm

Printer Tests

Test	Status	Time
PRNT	Pass	9:55pm

CRC Tests

Test	Status	Time
COMP	Pass	9:55pm
CAL	Pass	9:55pm

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County Mecklenburg Instrument Location BAT Mobile Unit 8
Instrument Serial No. 008929

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 15 day of January, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

2219283
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

MECKLENBURG COUNTY BAT MOBILE UNIT 8
590

Serial Number: 008929
Test Date: 01/15/2026

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE

Analyst's Name: Glasscock, Jerry D
Permit Number: 7180-9235
Effective:
02/01/2025-02/01/2027

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG506303
Exp Date: 03/04/2027

Test	g/210L	Time
DIAG	Pass	8:39am
AIR BLK	.00	8:40am
ACCY CHK	.08	8:41am
AIR BLK	.00	8:42am
SUB TEST	.00	8:42am
AIR BLK	.00	8:43am
SUB TEST	.00	8:45am
AIR BLK	.00	8:46am

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

MECKLENBURG COUNTY BAT MOBILE UNIT 8 590

Serial Number: 008929 Test Record Number: 1718
Test Date: 01/15/2026 Test Time: 8:47am EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	8:47am
FLO	Pass	8:47am
FC	Pass	8:47am

Temperature Tests

Test	Status	Time
FC1	Pass	8:47am
SRC	Pass	8:47am
DET	Pass	8:47am
BAR	Pass	8:47am
BT	Pass	8:47am

Blank Tests

Test	Status	Time
AIR	Pass	8:48am

Printer Tests

Test	Status	Time
PRNT	Pass	8:48am

CRC Tests

Test	Status	Time
COMP	Pass	8:48am
CAL	Pass	8:48am

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Mecklenburg Instrument Location BAT Mobile Unit 8
Instrument Serial No. 008929

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 22 day of January, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

2219283
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

MECKLENBURG COUNTY BAT MOBILE UNIT 8
590

Serial Number: 008929
Test Date: 01/22/2026

Citation Number: M0000000-0
Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Glasscock, Jerry D

Permit Number: 7180-9235

Effective:

02/01/2025-02/01/2027

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG506303

Exp Date: 03/04/2027

Test	g/210L	Time
DIAG	Pass	9:19pm
AIR BLK	.00	9:20pm
ACCY CHK	.08	9:21pm
AIR BLK	.00	9:22pm
SUB TEST	.00	9:24pm
AIR BLK	.00	9:25pm
SUB TEST	.00	9:26pm
AIR BLK	.00	9:27pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

Intox EC/IR-II: Preventive Maintenance

MECKLENBURG COUNTY BAT MOBILE UNIT 8 590

Serial Number: 008929 Test Record Number: 1724
Test Date: 01/22/2026 Test Time: 9:27pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	9:28pm
FLO	Pass	9:28pm
FC	Pass	9:28pm

Temperature Tests

Test	Status	Time
FC1	Pass	9:28pm
SRC	Pass	9:28pm
DET	Pass	9:28pm
BAR	Pass	9:28pm
BT	Pass	9:28pm

Blank Tests

Test	Status	Time
AIR	Pass	9:29pm

Printer Tests

Test	Status	Time
PRNT	Pass	9:29pm

CRC Tests

Test	Status	Time
COMP	Pass	9:29pm
CAL	Pass	9:29pm

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County Mecklenburg Instrument Location BAT Mobile Unit 8
Instrument Serial No. 008929 -

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 29 day of January, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

2219283
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

MECKLENBURG COUNTY BAT MOBILE UNIT 8
590

Serial Number: 008929
Test Date: 01/29/2026

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE

Analyst's Name: Glasscock, Jerry D
Permit Number: 7180-9235
Effective:
02/01/2025-02/01/2027

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG506303
Exp Date: 03/04/2027

Test	g/210L	Time
DIAG	Pass	9:40pm
AIR BLK	.00	9:42pm
ACCY CHK	.08	9:42pm
AIR BLK	.00	9:43pm
SUB TEST	.00	9:44pm
AIR BLK	.00	9:45pm
SUB TEST	.00	9:46pm
AIR BLK	.00	9:47pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

Intox EC/IR-II: Preventive Maintenance

MECKLENBURG COUNTY BAT MOBILE UNIT 8 590

Serial Number: 008929 Test Record Number: 1728
Test Date: 01/29/2026 Test Time: 9:48pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	9:49pm
FLO	Pass	9:49pm
FC	Pass	9:49pm

Temperature Tests

Test	Status	Time
FC1	Pass	9:49pm
SRC	Pass	9:49pm
DET	Pass	9:49pm
BAR	Pass	9:49pm
BT	Pass	9:49pm

Blank Tests

Test	Status	Time
AIR	Pass	9:50pm

Printer Tests

Test	Status	Time
PRNT	Pass	9:50pm

CRC Tests

Test	Status	Time
COMP	Pass	9:50pm
CAL	Pass	9:50pm

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County NORTHAMPTON Instrument Location NORTHAMPTON C.O.S.O.

Instrument Serial No. 008607 105 WEST JEFFERSON ST.
JACKSON, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 6 day of JANUARY, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



E.A. Bryant
Signature of Certifying Official

179707
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

NORTHAMPTON COUNTY SHERIFFS DEPARTMENT
650

Serial Number: 008607
Test Date: 01/06/2026

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE

Analyst's Name: Bryant, Earl A
Permit Number: 0017-9707
Effective:
02/01/2025-02/01/2027

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG501307
Exp Date: 01/13/2027

Test	g/210L	Time
DIAG	Pass	10:25am
AIR BLK	.00	10:26am
ACCY CHK	.07	10:27am
AIR BLK	.00	10:28am
SUB TEST	.00	10:28am
AIR BLK	.00	10:29am
SUB TEST	.00	10:31am
AIR BLK	.00	10:32am

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

NORTHAMPTON COUNTY SHERIFFS DEPARTMENT 650

Serial Number: 008607 Test Record Number: 1398
Test Date: 01/06/2026 Test Time: 10:34am EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	10:34am
FLO	Pass	10:34am
FC	Pass	10:34am

Temperature Tests

Test	Status	Time
FC1	Pass	10:34am
SRC	Pass	10:34am
DET	Pass	10:34am
BAR	Pass	10:34am
BT	Pass	10:34am

Blank Tests

Test	Status	Time
AIR	Pass	10:35am

Printer Tests

Test	Status	Time
PRNT	Pass	10:35am

CRC Tests

Test	Status	Time
COMP	Pass	10:35am
CAL	Pass	10:35am

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County NORTHAMPTON Instrument Location NORTHAMPTON CO. S.O.

Instrument Serial No. 008688 105 WEST JEFFERSON ST
JACKSON, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 6 day of JANUARY, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

179707
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

NORTHAMPTON COUNTY SHERIFFS DEPARTMENT
650

Serial Number: 008688
Test Date: 01/06/2026

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: Bryant, Earl A
Permit Number: 0017-9707
Effective:
02/01/2025-02/01/2027

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG501307
Exp Date: 01/13/2027

Test	g/210L	Time
DIAG	Pass	10:26am
AIR BLK	.00	10:27am
ACCY CHK	.07	10:28am
AIR BLK	.00	10:29am
SUB TEST	.00	10:30am
AIR BLK	.00	10:31am
SUB TEST	.00	10:33am
AIR BLK	.00	10:33am

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

NORTHAMPTON COUNTY SHERIFFS DEPARTMENT 650

Serial Number: 008688 Test Record Number: 1189
Test Date: 01/06/2026 Test Time: 10:35am EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	10:35am
FLO	Pass	10:35am
FC	Pass	10:35am

Temperature Tests

Test	Status	Time
FC1	Pass	10:35am
SRC	Pass	10:35am
DET	Pass	10:35am
BAR	Pass	10:35am
BT	Pass	10:35am

Blank Tests

Test	Status	Time
AIR	Pass	10:36am

Printer Tests

Test	Status	Time
PRNT	Pass	10:36am

CRC Tests

Test	Status	Time
COMP	Pass	10:36am
CAL	Pass	10:36am

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County Onslow Instrument Location BAT Mobile Unit 7

Instrument Serial No. 008002

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 2nd day of January, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

2266313
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

ONslow COUNTY BAT MOBILE UNIT 7 660

Serial Number: 008002

Test Date: 01/02/2026

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Sharpe Jr., Robert J

Permit Number: 1820-8591

Effective:

02/01/2025-02/01/2027

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG506303

Exp Date: 03/04/2027

Test	g/210L	Time
DIAG	Pass	9:03pm
AIR BLK	.00	9:04pm
ACCY CHK	.08	9:05pm
AIR BLK	.00	9:06pm
SUB TEST	.00	9:07pm
AIR BLK	.00	9:08pm
SUB TEST	.00	9:09pm
AIR BLK	.00	9:10pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

This form is used when performing Preventive Maintenance procedures

Forensic Tests for Alcohol Branch

Department of Health and Human Services

Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

ONSLOW COUNTY BAT MOBILE UNIT 7 660

Serial Number: 008002 Test Record Number: 861
Test Date: 01/02/2026 Test Time: 9:10pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	9:11pm
FLO	Pass	9:11pm
FC	Pass	9:11pm

Temperature Tests

Test	Status	Time
FC1	Pass	9:11pm
SRC	Pass	9:11pm
DET	Pass	9:11pm
BAR	Pass	9:11pm
BT	Pass	9:11pm

Blank Tests

Test	Status	Time
AIR	Pass	9:12pm

Printer Tests

Test	Status	Time
PRNT	Pass	9:12pm

CRC Tests

Test	Status	Time
COMP	Pass	9:12pm
CAL	Pass	9:12pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County Onslow Instrument Location BAT Mobile Unit 7
Instrument Serial No. 008968

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 2nd day of January, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

2266313
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

ONSLOW COUNTY BAT MOBILE UNIT 7 660

Serial Number: 008968
Test Date: 01/02/2026

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Sharpe Jr., Robert J

Permit Number: 1820-8591

Effective:

02/01/2025-02/01/2027

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG506303

Exp Date: 03/04/2027

Test	g/210L	Time
DIAG	Pass	9:06pm
AIR BLK	.00	9:07pm
ACCY CHK	.08	9:08pm
AIR BLK	.00	9:08pm
SUB TEST	.00	9:09pm
AIR BLK	.00	9:10pm
SUB TEST	.00	9:12pm
AIR BLK	.00	9:13pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

ONslow COUNTY BAT MOBILE UNIT 7 660

Serial Number: 008968 Test Record Number: 432
Test Date: 01/02/2026 Test Time: 9:14pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	9:14pm
FLO	Pass	9:14pm
FC	Pass	9:14pm

Temperature Tests

Test	Status	Time
FC1	Pass	9:15pm
SRC	Pass	9:15pm
DET	Pass	9:15pm
BAR	Pass	9:15pm
BT	Pass	9:15pm

Blank Tests

Test	Status	Time
AIR	Pass	9:15pm


Printer Tests

Test	Status	Time
PRNT	Pass	9:15pm

CRC Tests

Test	Status	Time
COMP	Pass	9:15pm
CAL	Pass	9:15pm

Preventive Maintenance
Status: Pass

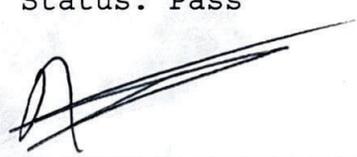

Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County Onslow Instrument Location BAT Mobile Unit 7

Instrument Serial No. 008971

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 2nd day of January, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

2266313
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

ONSLOW COUNTY BAT MOBILE UNIT 7 660

Serial Number: 008971
Test Date: 01/02/2026

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE

Analyst's Name: Sharpe Jr., Robert J
Permit Number: 1820-8591
Effective:
02/01/2025-02/01/2027

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG506302
Exp Date: 03/04/2027

Test	g/210L	Time
DIAG	Pass	9:04pm
AIR BLK	.00	9:05pm
ACCY CHK	.08	9:05pm
AIR BLK	.00	9:06pm
SUB TEST	.00	9:07pm
AIR BLK	.00	9:08pm
SUB TEST	.00	9:09pm
AIR BLK	.00	9:10pm

Reported AC: ~~00~~ g/210L

Signature of Chemical Analyst

Court CVR

Analyst

Intox EC/IR-II: Preventive Maintenance

ONSLOW COUNTY BAT MOBILE UNIT 7 660

Serial Number: 008971 Test Record Number: 382
Test Date: 01/02/2026 Test Time: 9:11pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	9:11pm
FLO	Pass	9:11pm
FC	Pass	9:11pm

Temperature Tests

Test	Status	Time
FC1	Pass	9:11pm
SRC	Pass	9:11pm
DET	Pass	9:11pm
BAR	Pass	9:11pm
BT	Pass	9:11pm

Blank Tests

Test	Status	Time
AIR	Pass	9:12pm

Printer Tests

Test	Status	Time
PRNT	Pass	9:12pm

CRC Tests

Test	Status	Time
COMP	Pass	9:12pm
CAL	Pass	9:12pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Onslow Instrument Location BAT Mobile Unit 7

Instrument Serial No. 008972

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 2nd day of January, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

2266313
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

ONslow COUNTY BAT MOBILE UNIT 7 660

Serial Number: 008972
Test Date: 01/02/2026

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE

Analyst's Name: Sharpe Jr., Robert J
Permit Number: 1820-8591
Effective:
02/01/2025-02/01/2027

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test


Lot Number: AG506303
Exp Date: 03/04/2027

Test	g/210L	Time
DIAG	Pass	9:01pm
AIR BLK	.00	9:02pm
ACCY CHK	.08	9:03pm
AIR BLK	.00	9:04pm
SUB TEST	.00	9:05pm
AIR BLK	.00	9:06pm
SUB TEST	.00	9:08pm
AIR BLK	.00	9:08pm

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR

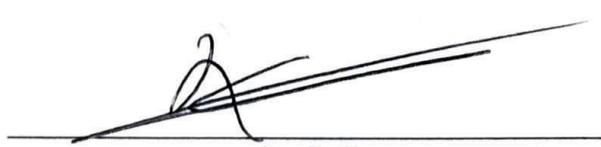
Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

ONSLOW COUNTY BAT MOBILE UNIT 7 660

Serial Number: 008972 Test Record Number: 444
Test Date: 01/02/2026 Test Time: 9:09pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	9:09pm
FLO	Pass	9:09pm
FC	Pass	9:09pm

Temperature Tests

Test	Status	Time
FC1	Pass	9:10pm
SRC	Pass	9:10pm
DET	Pass	9:10pm
BAR	Pass	9:10pm
BT	Pass	9:10pm

Blank Tests

Test	Status	Time
AIR	Pass	9:10pm

Printer Tests

Test	Status	Time
PRNT	Pass	9:10pm

CRC Tests

Test	Status	Time
COMP	Pass	9:10pm
CAL	Pass	9:10pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County Orange Instrument Location Orange Co Detention Ctr
Instrument Serial No. 008799 1200 US Hwy 70 West
Hillsborough, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 13 day of January, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Simon Stokes Bruce
Signature of Certifying Official

146221
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

ORANGE COUNTY DETENTION CENTER 670

Serial Number: 008799
Test Date: 01/13/2026

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE

Analyst's Name: Barnes, Simon S
Permit Number: 0014-6221
Effective:
02/01/2025-02/01/2027

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG534301
Exp Date: 12/09/2027

Test	g/210L	Time
DIAG	Pass	3:23pm
AIR BLK	.00	3:24pm
ACCY CHK	.08	3:25pm
AIR BLK	.00	3:26pm
SUB TEST	.00	3:27pm
AIR BLK	.00	3:28pm
SUB TEST	.00	3:29pm
AIR BLK	.00	3:30pm

Reported AC: .00 g/210L

Simon Ales Barnes
Signature of Chemical Analyst

Court CVR

Simon Ales Barnes
Analyst

Intox EC/IR-II: Preventive Maintenance

ORANGE COUNTY DETENTION CENTER 670

Serial Number: 008799 Test Record Number: 4300
Test Date: 01/13/2026 Test Time: 3:31pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	3:31pm
FLO	Pass	3:31pm
FC	Pass	3:31pm

Temperature Tests

Test	Status	Time
FC1	Pass	3:31pm
SRC	Pass	3:31pm
DET	Pass	3:31pm
BAR	Pass	3:31pm
BT	Pass	3:31pm

Blank Tests

Test	Status	Time
AIR	Pass	3:32pm

Printer Tests

Test	Status	Time
PRNT	Pass	3:32pm

CRC Tests

Test	Status	Time
COMP	Pass	3:32pm
CAL	Pass	3:32pm

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County DRAWES Instrument Location Orange Co Detention Ctr
Instrument Serial No. 008839 1200 US Hwy 70 West
Hillsborough, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 13 day of January, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Simon Stokes Bruns

Signature of Certifying Official

146221

Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

ORANGE COUNTY DETENTION CENTER 670

Serial Number: 008839
Test Date: 01/13/2026

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE

Analyst's Name: Barnes, Simon S
Permit Number: 0014-6221
Effective:
02/01/2025-02/01/2027

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG534301
Exp Date: 12/09/2027

Test	g/210L	Time
DIAG	Pass	3:27pm
AIR BLK	.00	3:27pm
ACCY CHK	.08	3:28pm
AIR BLK	.00	3:29pm
SUB TEST	.00	3:30pm
AIR BLK	.00	3:31pm
SUB TEST	.00	3:33pm
AIR BLK	.00	3:33pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

ORANGE COUNTY DETENTION CENTER 670

Serial Number: 008839 Test Record Number: 3019
Test Date: 01/13/2026 Test Time: 3:35pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	3:35pm
FLO	Pass	3:35pm
FC	Pass	3:35pm

Temperature Tests

Test	Status	Time
FC1	Pass	3:35pm
SRC	Pass	3:35pm
DET	Pass	3:35pm
BAR	Pass	3:35pm
BT	Pass	3:35pm

Blank Tests

Test	Status	Time
AIR	Pass	3:36pm

Printer Tests

Test	Status	Time
PRNT	Pass	3:36pm

CRC Tests

Test	Status	Time
COMP	Pass	3:36pm
CAL	Pass	3:36pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County ORANGE Instrument Location Chapel Hill PD
Instrument Serial No. 008856 7300 M.II House Rd Suite 150
Chapel Hill, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 13 day of January, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Simon Stokes Barcus
Signature of Certifying Official

146221
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

ORANGE COUNTY CHAPEL HILL PD 670

Serial Number: 008856
Test Date: 01/13/2026

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE

Analyst's Name: Barnes, Simon S
Permit Number: 0014-6221
Effective:
02/01/2025-02/01/2027

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG431003
Exp Date: 11/05/2026

Test	g/210L	Time
DIAG	Pass	2:18pm
AIR BLK	.00	2:19pm
ACCY CHK	.08	2:20pm
AIR BLK	.00	2:21pm
SUB TEST	.00	2:21pm
AIR BLK	.00	2:22pm
SUB TEST	.00	2:24pm
AIR BLK	.00	2:25pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

Intox EC/IR-II: Preventive Maintenance

ORANGE COUNTY CHAPEL HILL PD 670

Serial Number: 008856 Test Record Number: 3374
Test Date: 01/13/2026 Test Time: 2:31pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	2:32pm
FLO	Pass	2:32pm
FC	Pass	2:32pm

Temperature Tests

Test	Status	Time
FC1	Pass	2:32pm
SRC	Pass	2:32pm
DET	Pass	2:32pm
BAR	Pass	2:32pm
BT	Pass	2:32pm

Blank Tests

Test	Status	Time
AIR	Pass	2:33pm

Printer Tests

Test	Status	Time
PRNT	Pass	2:33pm

CRC Tests

Test	Status	Time
COMP	Pass	2:33pm
CAL	Pass	2:33pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County ORANGE Instrument Location CARRBORO PD
Instrument Serial No. 008945 100 N Greensboro St
CARRBORO, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 13 day of January, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Sam Stokes Barnes
Signature of Certifying Official

146221
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

ORANGE COUNTY CARRBORO PD 670

Serial Number: 008945
Test Date: 01/13/2026

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE

Analyst's Name: Barnes, Simon S
Permit Number: 0014-6221
Effective:
02/01/2025-02/01/2027

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG505001
Exp Date: 02/19/2027

Test	g/210L	Time
DIAG	Pass	1:10pm
AIR BLK	.00	1:11pm
ACCY CHK	.07	1:11pm
AIR BLK	.00	1:13pm
SUB TEST	.00	1:13pm
AIR BLK	.00	1:14pm
SUB TEST	.00	1:16pm
AIR BLK	.00	1:17pm

Reported AC: .00 g/210L

Simon Stokes Barnes
Signature of Chemical Analyst

Court CVR

Simon Stokes Barnes
Analyst

Intox EC/IR-II: Preventive Maintenance

ORANGE COUNTY CARRBORO PD 670

Serial Number: 008945 Test Record Number: 887
Test Date: 01/13/2026 Test Time: 1:17pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	1:17pm
FLO	Pass	1:17pm
FC	Pass	1:17pm

Temperature Tests

Test	Status	Time
FC1	Pass	1:17pm
SRC	Pass	1:17pm
DET	Pass	1:17pm
BAR	Pass	1:17pm
BT	Pass	1:17pm

Blank Tests

Test	Status	Time
AIR	Pass	1:18pm

Printer Tests

Test	Status	Time
PRNT	Pass	1:18pm

CRC Tests

Test	Status	Time
COMP	Pass	1:18pm
CAL	Pass	1:18pm

Preventive Maintenance
Status: Pass



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County Perquimans Instrument Location Perquimans Co. S.O.
Instrument Serial No. 008921 110 N. Church St. Hertford, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 12th day of January, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

206272
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

PERQUIMANS COUNTY PERQUIMANS CO SO 710

Serial Number: 008921
Test Date: 01/12/2026

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: Chappell, Mark A
Permit Number: 0020-6272
Effective:
02/01/2025-02/01/2027

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test


Lot Number: AG431001
Exp Date: 11/05/2026

Test	g/210L	Time
DIAG	Pass	10:04am
AIR BLK	.00	10:05am
ACCY CHK	.07	10:06am
AIR BLK	.00	10:07am
SUB TEST	.00	10:07am
AIR BLK	.00	10:08am
SUB TEST	.00	10:10am
AIR BLK	.00	10:11am

Reported AC: .00 g/210L

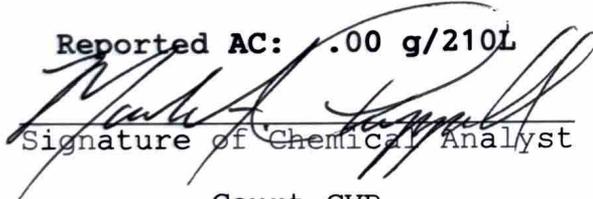
Signature of Chemical Analyst

Court CVR

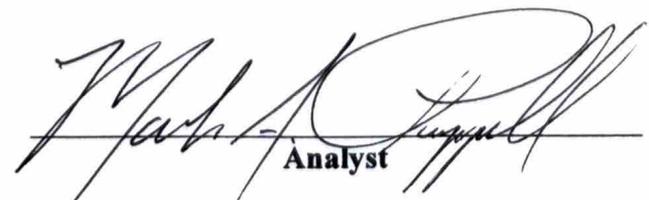
Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

PERQUIMANS COUNTY PERQUIMANS CO SO 710

Serial Number: 008921 Test Record Number: 1420
Test Date: 01/12/2026 Test Time: 10:11am EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	10:11am
FLO	Pass	10:11am
FC	Pass	10:12am

Temperature Tests

Test	Status	Time
FC1	Pass	10:12am
SRC	Pass	10:12am
DET	Pass	10:12am
BAR	Pass	10:12am
BT	Pass	10:12am

Blank Tests

Test	Status	Time
AIR	Pass	10:12am


Printer Tests

Test	Status	Time
PRNT	Pass	10:12am

CRC Tests

Test	Status	Time
COMP	Pass	10:13am
CAL	Pass	10:13am

Preventive Maintenance
Status: Pass

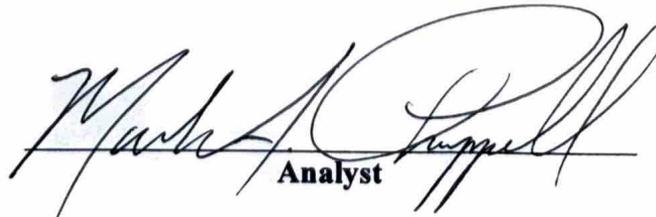
Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County Pitt Instrument Location Pitt Co Detention Center
Instrument Serial No. 008646 124 New Hope Rd, Greenville, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 27th day of January, 20 26 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

377722
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

PITT COUNTY PITT CO DETENTION 730

Serial Number: 008646
Test Date: 01/27/2026

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: Gray, Kelly D
Permit Number: 0037-7722
Effective:
02/01/2025-02/01/2027

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG516203
Exp Date: 06/11/2027


Test	g/210L	Time
DIAG	Pass	10:33am
AIR BLK	.00	10:34am
ACCY CHK	.07	10:34am
AIR BLK	.00	10:36am
SUB TEST	.00	10:36am
AIR BLK	.00	10:38am
SUB TEST	.00	10:39am
AIR BLK	.00	10:40am

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

Intox EC/IR-II: Preventive Maintenance

PITT COUNTY PITT CO DETENTION 730

Serial Number: 008646 Test Record Number: 5393
Test Date: 01/27/2026 Test Time: 10:41am EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	10:41am
FLO	Pass	10:41am
FC	Pass	10:41am

Temperature Tests

Test	Status	Time
FC1	Pass	10:41am
SRC	Pass	10:41am
DET	Pass	10:41am
BAR	Pass	10:41am
BT	Pass	10:41am

Blank Tests

Test	Status	Time
AIR	Pass	10:42am


Printer Tests

Test	Status	Time
PRNT	Pass	10:42am

CRC Tests

Test	Status	Time
COMP	Pass	10:42am
CAL	Pass	10:42am

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County Pitt Instrument Location Pitt Co. Detention Center

Instrument Serial No. 008662 124 New Hope Rd., Greenville, N.C.

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 27th day of January, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Key D...

Signature of Certifying Official

377722

Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

PITT COUNTY PITT CO DETENTION 730

Serial Number: 008662
Test Date: 01/27/2026

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE

Analyst's Name: Gray, Kelly D
Permit Number: 0037-7722
Effective:
02/01/2025-02/01/2027

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG431003
Exp Date: 11/05/2026

Test	g/210L	Time
DIAG	Pass	10:56am
AIR BLK	.00	10:57am
ACCY CHK	.08	10:57am
AIR BLK	.00	10:59am
SUB TEST	.00	11:00am
AIR BLK	.00	11:00am
SUB TEST	.00	11:02am
AIR BLK	.00	11:03am

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

PITT COUNTY PITT CO DETENTION 730

Serial Number: 008662 Test Record Number: 1460
Test Date: 01/27/2026 Test Time: 11:04am EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	11:04am
FLO	Pass	11:04am
FC	Pass	11:04am

Temperature Tests

Test	Status	Time
FC1	Pass	11:04am
SRC	Pass	11:04am
DET	Pass	11:04am
BAR	Pass	11:04am
BT	Pass	11:04am

Blank Tests

Test	Status	Time
AIR	Pass	11:05am


Printer Tests

Test	Status	Time
PRNT	Pass	11:05am

CRC Tests

Test	Status	Time
COMP	Pass	11:05am
CAL	Pass	11:05am

Preventive Maintenance
Status: Pass

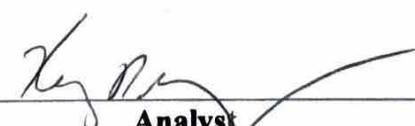

Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County Robeson Instrument Location BAT Mobile Unit 7

Instrument Serial No. 008002

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 29th day of January, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.





Signature of Certifying Official

2266313

Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

ROBESON COUNTY BAT MOBILE UNIT 7 770

Serial Number: 008002
Test Date: 01/29/2026

Citation Number: M0000000-0
Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Sharpe Jr., Robert J

Permit Number: 1820-8591

Effective:

02/01/2025-02/01/2027

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG506303

Exp Date: 03/04/2027

Test	g/210L	Time
DIAG	Pass	8:19pm
AIR BLK	.00	8:20pm
ACCY CHK	.08	8:20pm
AIR BLK	.00	8:21pm
SUB TEST	.00	8:22pm
AIR BLK	.00	8:23pm
SUB TEST	.00	8:24pm
AIR BLK	.00	8:25pm

Reported AG: .00 g/210L

Signature of Chemical Analyst

Court CVR


Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

ROBESON COUNTY BAT MOBILE UNIT 7 770

Serial Number: 008002 Test Record Number: 871
Test Date: 01/29/2026 Test Time: 8:27pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	8:27pm
FLO	Pass	8:27pm
FC	Pass	8:27pm

Temperature Tests

Test	Status	Time
FC1	Pass	8:27pm
SRC	Pass	8:27pm
DET	Pass	8:27pm
BAR	Pass	8:27pm
BT	Pass	8:27pm

Blank Tests

Test	Status	Time
AIR	Pass	8:28pm

Printer Tests

Test	Status	Time
PRNT	Pass	8:28pm

CRC Tests

Test	Status	Time
COMP	Pass	8:28pm
CAL	Pass	8:28pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County Robeson Instrument Location BAT Mobile Unit 7

Instrument Serial No. 00 8968

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 29th day of January, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

2266313
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

ROBESON COUNTY BAT MOBILE UNIT 7 770

Serial Number: 008968
Test Date: 01/29/2026

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: Sharpe Jr., Robert J
Permit Number: 1820-8591
Effective:
02/01/2025-02/01/2027

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG506303
Exp Date: 03/04/2027

Test	g/210L	Time
DIAG	Pass	8:23pm
AIR BLK	.00	8:24pm
ACCY CHK	.08	8:24pm
AIR BLK	.00	8:25pm
SUB TEST	.00	8:26pm
AIR BLK	.00	8:27pm
SUB TEST	.00	8:28pm
AIR BLK	.00	8:29pm

Reported AC: .00 g/210L

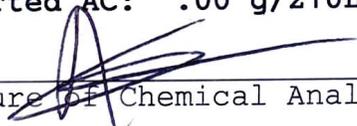

Signature of Chemical Analyst

Court CVR



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

ROBESON COUNTY BAT MOBILE UNIT 7 770

Serial Number: 008968 Test Record Number: 434
Test Date: 01/29/2026 Test Time: 8:30pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	8:31pm
FLO	Pass	8:31pm
FC	Pass	8:31pm

Temperature Tests

Test	Status	Time
FC1	Pass	8:31pm
SRC	Pass	8:31pm
DET	Pass	8:31pm
BAR	Pass	8:31pm
BT	Pass	8:31pm

Blank Tests

Test	Status	Time
AIR	Pass	8:31pm


Printer Tests

Test	Status	Time
PRNT	Pass	8:31pm

CRC Tests

Test	Status	Time
COMP	Pass	8:32pm
CAL	Pass	8:32pm

Preventive Maintenance
Status: Pass

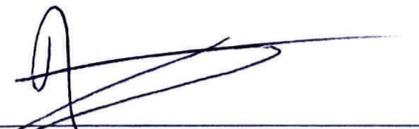

Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County Robeson Instrument Location BAT Mobile Unit 7

Instrument Serial No. 008971

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 29th day of January, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

2266313
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

ROBESON COUNTY BAT MOBILE UNIT 7 770

Serial Number: 008971
Test Date: 01/29/2026

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE

Analyst's Name: Sharpe Jr., Robert J
Permit Number: 1820-8591
Effective:
02/01/2025-02/01/2027

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG506302
Exp Date: 03/04/2027


Test	g/210L	Time
DIAG	Pass	8:18pm
AIR BLK	.00	8:19pm
ACCY CHK	.08	8:20pm
AIR BLK	.00	8:21pm
SUB TEST	.00	8:22pm
AIR BLK	.00	8:22pm
SUB TEST	.00	8:24pm
AIR BLK	.00	8:25pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR

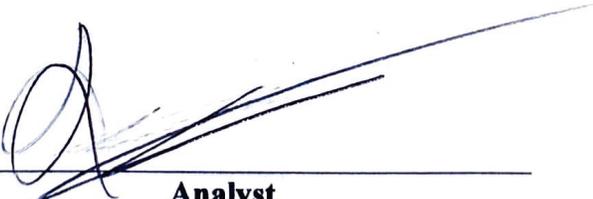

Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

ROBESON COUNTY BAT MOBILE UNIT 7 770

Serial Number: 008971 Test Record Number: 384
Test Date: 01/29/2026 Test Time: 8:37pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	8:37pm
FLO	Pass	8:37pm
FC	Pass	8:37pm

Temperature Tests

Test	Status	Time
FC1	Pass	8:38pm
SRC	Pass	8:38pm
DET	Pass	8:38pm
BAR	Pass	8:38pm
BT	Pass	8:38pm

Blank Tests

Test	Status	Time
AIR	Pass	8:38pm

Printer Tests

Test	Status	Time
PRNT	Pass	8:38pm

CRC Tests

Test	Status	Time
COMP	Pass	8:38pm
CAL	Pass	8:38pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County Robeson Instrument Location BAT Mobile Unit 7

Instrument Serial No. 008972

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 29th day of January, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

2266313
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

ROBESON COUNTY BAT MOBILE UNIT 7 770

Serial Number: 008972
Test Date: 01/29/2026

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Sharpe Jr., Robert J

Permit Number: 1820-8591

Effective:

02/01/2025-02/01/2027

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG506303


Exp Date: 03/04/2027

Test	g/210L	Time
DIAG	Pass	8:17pm
AIR BLK	.00	8:18pm
ACCY CHK	.08	8:19pm
AIR BLK	.00	8:20pm
SUB TEST	.00	8:21pm
AIR BLK	.00	8:22pm
SUB TEST	.00	8:24pm
AIR BLK	.00	8:25pm

Reported AC: ~~0.00~~ .00 g/210L

Signature of Chemical Analyst

Court CVR

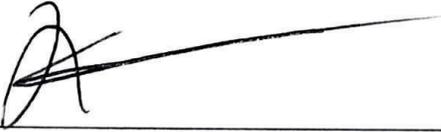

Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

ROBESON COUNTY BAT MOBILE UNIT 7 770

Serial Number: 008972 Test Record Number: 446
Test Date: 01/29/2026 Test Time: 8:26pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	8:26pm
FLO	Pass	8:26pm
FC	Pass	8:26pm

Temperature Tests

Test	Status	Time
FC1	Pass	8:26pm
SRC	Pass	8:26pm
DET	Pass	8:26pm
BAR	Pass	8:26pm
BT	Pass	8:26pm

Blank Tests

Test	Status	Time
AIR	Pass	8:27pm


Printer Tests

Test	Status	Time
PRNT	Pass	8:27pm

CRC Tests

Test	Status	Time
COMP	Pass	8:27pm
CAL	Pass	8:27pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County Rockingham Instrument Location Eden Police
Instrument Serial No. 008636 Department

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 23rd day of January, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

509387
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

ROCKINGHAM COUNTY EDEN PD 780

Serial Number: 008636
Test Date: 01/23/2026

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE

Analyst's Name: Long, Thomas A
Permit Number: 0050-9387
Effective:
09/01/2025-09/01/2027

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG534301
Exp Date: 12/09/2027


Test	g/210L	Time
DIAG	Pass	3:12pm
AIR BLK	.00	3:13pm
ACCY CHK	.08	3:14pm
AIR BLK	.00	3:15pm
SUB TEST	.00	3:16pm
AIR BLK	.00	3:17pm
SUB TEST	.00	3:18pm
AIR BLK	.00	3:19pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

Intox EC/IR-II: Preventive Maintenance

ROCKINGHAM COUNTY EDEN PD 780

Serial Number: 008636 Test Record Number: 2985
Test Date: 01/23/2026 Test Time: 3:20pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	3:20pm
FLO	Pass	3:20pm
FC	Pass	3:20pm

Temperature Tests

Test	Status	Time
FC1	Pass	3:20pm
SRC	Pass	3:20pm
DET	Pass	3:20pm
BAR	Pass	3:20pm
BT	Pass	3:20pm

Blank Tests

Test	Status	Time
AIR	Pass	3:21pm

Printer Tests

Test	Status	Time
PRNT	Pass	3:21pm

CRC Tests

Test	Status	Time
COMP	Pass	3:21pm
CAL	Pass	3:21pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**


County ROCKINGHAM Instrument Location REIDSVILLE POLICE
Instrument Serial No. 008784 DEPARTMENT

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 23RD day of JANUARY, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.

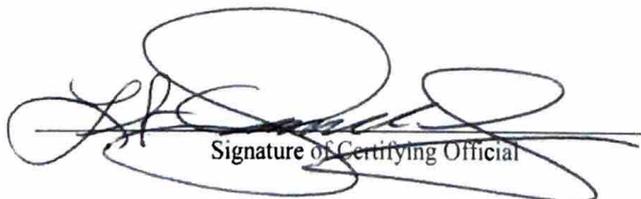


Signature of Certifying Official

353799
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

ROCKINGHAM COUNTY REIDSVILLE PD 780

Serial Number: 008784

Test Date: 01/23/2026

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Oligmueller, Leo A

Permit Number: 0035-3799

Effective:

02/01/2025-02/01/2027

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG506301

Exp Date: 03/04/2027

Test	g/210L	Time
DIAG	Pass	9:52am
AIR BLK	.00	9:53am
ACCY CHK	.08	9:53am
AIR BLK	.00	9:54am
SUB TEST	.00	9:55am
AIR BLK	.00	9:56am
SUB TEST	.00	9:58am
AIR BLK	.00	9:59am

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

ROCKINGHAM COUNTY REIDSVILLE PD 780

Serial Number: 008784 Test Record Number: 1654
Test Date: 01/23/2026 Test Time: 9:59am EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	10:00am
FLO	Pass	10:00am
FC	Pass	10:00am

Temperature Tests

Test	Status	Time
FC1	Pass	10:00am
SRC	Pass	10:00am
DET	Pass	10:00am
BAR	Pass	10:00am
BT	Pass	10:00am

Blank Tests

Test	Status	Time
AIR	Pass	10:01am


Printer Tests

Test	Status	Time
PRNT	Pass	10:01am

CRC Tests

Test	Status	Time
COMP	Pass	10:01am
CAL	Pass	10:01am

Preventive Maintenance
Status: Pass

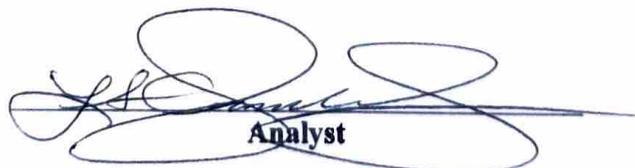

Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Rockingham Instrument Location Rockingham County
Instrument Serial No. 008796 Sail

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 23rd day of January, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

509387
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

ROCKINGHAM COUNTY ROCKINGHAM CO JAIL
780

Serial Number: 008796
Test Date: 01/23/2026

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE

Analyst's Name: Long, Thomas A
Permit Number: 0050-9387
Effective:
09/01/2025-09/01/2027

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG516204
Exp Date: 06/11/2027

Test	g/210L	Time
DIAG	Pass	4:03pm
AIR BLK	.00	4:04pm
ACCY CHK	.08	4:05pm
AIR BLK	.00	4:06pm
SUB TEST	.00	4:07pm
AIR BLK	.00	4:07pm
SUB TEST	.00	4:09pm
AIR BLK	.00	4:10pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

ROCKINGHAM COUNTY ROCKINGHAM CO JAIL 780

Serial Number: 008796 Test Record Number: 4043
Test Date: 01/23/2026 Test Time: 4:10pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	4:11pm
FLO	Pass	4:11pm
FC	Pass	4:11pm

Temperature Tests

Test	Status	Time
FC1	Pass	4:11pm
SRC	Pass	4:11pm
DET	Pass	4:11pm
BAR	Pass	4:11pm
BT	Pass	4:11pm

Blank Tests

Test	Status	Time
AIR	Pass	4:12pm


Printer Tests

Test	Status	Time
PRNT	Pass	4:12pm

CRC Tests

Test	Status	Time
COMP	Pass	4:12pm
CAL	Pass	4:12pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County ROCKINGHAM Instrument Location MADISON POLICE


Instrument Serial No. 008802 DEPARTMENT

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 23RD day of JANUARY, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.

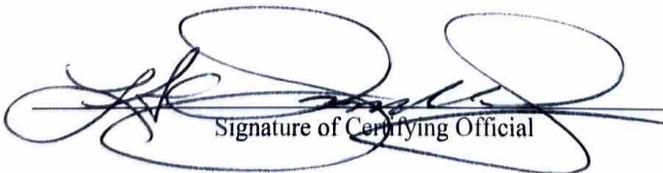


Signature of Certifying Official

353799
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

ROCKINGHAM COUNTY MADISON PD 780

Serial Number: 008802
Test Date: 01/23/2026

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE \

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Oligmueller, Leo A

Permit Number: 0035-3799

Effective:

02/01/2025-02/01/2027

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG431003

Exp Date: 11/05/2026

Test	g/210L	Time
DIAG	Pass	11:50am
AIR BLK	.00	11:51am
ACCY CHK	.08	11:52am
AIR BLK	.00	11:53am
SUB TEST	.00	11:54am
AIR BLK	.00	11:55am
SUB TEST	.00	11:56am
AIR BLK	.00	11:57am

Reported AC: .00 g/210L

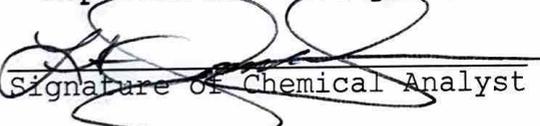
Signature of Chemical Analyst

Court CVR


Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

ROCKINGHAM COUNTY MADISON PD 780

Serial Number: 008802 Test Record Number: 1141
Test Date: 01/23/2026 Test Time: 11:57am EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	11:58am
FLO	Pass	11:58am
FC	Pass	11:58am

Temperature Tests

Test	Status	Time
FC1	Pass	11:58am
SRC	Pass	11:58am
DET	Pass	11:58am
BAR	Pass	11:58am
BT	Pass	11:58am

Blank Tests

Test	Status	Time
AIR	Pass	11:59am


Printer Tests

Test	Status	Time
PRNT	Pass	11:59am

CRC Tests

Test	Status	Time
COMP	Pass	11:59am
CAL	Pass	11:59am

Preventive Maintenance
Status: Pass

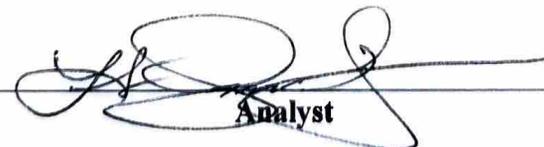
Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County Rutherford Instrument Location BAT Mobile Unit 11

Instrument Serial No. 008970

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 2nd day of January, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

62446
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

RUTHERFORD COUNTY BAT MOBILE UNIT 11
800

Serial Number: 008970
Test Date: 01/02/2026

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE

Analyst's Name: Gillstrap, Jeffrey L
Permit Number: 0006-2446
Effective:
04/01/2025-04/01/2027

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG417802
Exp Date: 06/26/2026


Test	g/210L	Time
DIAG	Pass	11:05pm
AIR BLK	.00	11:06pm
ACCY CHK	.07	11:07pm
AIR BLK	.00	11:08pm
SUB TEST	.00	11:08pm
AIR BLK	.00	11:09pm
SUB TEST	.00	11:11pm
AIR BLK	.00	11:12pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

RUTHERFORD COUNTY BAT MOBILE UNIT 11 800

Serial Number: 008970 Test Record Number: 1364
Test Date: 01/02/2026 Test Time: 11:12pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	11:13pm
FLO	Pass	11:13pm
FC	Pass	11:13pm

Temperature Tests

Test	Status	Time
FC1	Pass	11:13pm
SRC	Pass	11:13pm
DET	Pass	11:13pm
BAR	Pass	11:13pm
BT	Pass	11:13pm

Blank Tests

Test	Status	Time
AIR	Pass	11:13pm

Printer Tests

Test	Status	Time
PRNT	Pass	11:14pm

CRC Tests

Test	Status	Time
COMP	Pass	11:14pm
CAL	Pass	11:14pm

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Rutherford Instrument Location BAT Mobile Unit 11

Instrument Serial No. 008973

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 2nd day of January, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

62446
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

RUTHERFORD COUNTY BAT MOBILE UNIT 11
800

Serial Number: 008973
Test Date: 01/02/2026

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE

Analyst's Name: Gillstrap, Jeffrey L
Permit Number: 0006-2446
Effective:
04/01/2025-04/01/2027

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG431003
Exp Date: 11/05/2026

Test	g/210L	Time
DIAG	Pass	11:07pm
AIR BLK	.00	11:08pm
ACCY CHK	.07	11:09pm
AIR BLK	.00	11:10pm
SUB TEST	.00	11:11pm
AIR BLK	.00	11:11pm
SUB TEST	.00	11:13pm
AIR BLK	.00	11:14pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

Intox EC/IR-II: Preventive Maintenance

RUTHERFORD COUNTY BAT MOBILE UNIT 11 800

Serial Number: 008973 Test Record Number: 1415
Test Date: 01/02/2026 Test Time: 11:16pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	11:16pm
FLO	Pass	11:16pm
FC	Pass	11:16pm

Temperature Tests

Test	Status	Time
FC1	Pass	11:16pm
SRC	Pass	11:16pm
DET	Pass	11:16pm
BAR	Pass	11:16pm
BT	Pass	11:16pm

Blank Tests

Test	Status	Time
AIR	Pass	11:17pm

Printer Tests

Test	Status	Time
PRNT	Pass	11:17pm

CRC Tests

Test	Status	Time
COMP	Pass	11:17pm
CAL	Pass	11:17pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County JAMPSON Instrument Location JAMPSON COUNTY
Instrument Serial No. 008825 DETENTION CENTER

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 16 day of JANUARY, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Alan R. Bero
Signature of Certifying Official

146279
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

SAMPSON COUNTY DETENTION CENTER 810

Serial Number: 008825
Test Date: 01/16/2026

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: BARNES, ALVIN R
Permit Number: 0014-6279
Effective:
02/01/2025-02/01/2027

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG534301
Exp Date: 12/09/2027

Test	g/210L	Time
DIAG	Pass	2:37pm
AIR BLK	.00	2:38pm
ACCY CHK	.08	2:38pm
AIR BLK	.00	2:40pm
SUB TEST	.00	2:41pm
AIR BLK	.00	2:42pm
SUB TEST	.00	2:43pm
AIR BLK	.00	2:44pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

Intox EC/IR-II: Preventive Maintenance

SAMPSON COUNTY DETENTION CENTER 810

Serial Number: 008825 Test Record Number: 4276
Test Date: 01/16/2026 Test Time: 2:46pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	2:47pm
FLO	Pass	2:47pm
FC	Pass	2:47pm

Temperature Tests

Test	Status	Time
FC1	Pass	2:47pm
SRC	Pass	2:47pm
DET	Pass	2:47pm
BAR	Pass	2:47pm
BT	Pass	2:47pm

Blank Tests

Test	Status	Time
AIR	Pass	2:48pm

Printer Tests

Test	Status	Time
PRNT	Pass	2:48pm

CRC Tests

Test	Status	Time
COMP	Pass	2:48pm
CAL	Pass	2:48pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County SAMPSON Instrument Location SAMPSON COUNTY

Instrument Serial No. 008877 DETENTION CENTER

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 16 day of JANUARY, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Alan R. Barnes

Signature of Certifying Official

146279

Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

SAMPSON COUNTY DETENTION CENTER 810

Serial Number: 008877
Test Date: 01/16/2026

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE

Analyst's Name: BARNES, ALVIN R
Permit Number: 0014-6279
Effective:
02/01/2025-02/01/2027

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG534301
Exp Date: 12/09/2027


Test	g/210L	Time
DIAG	Pass	2:38pm
AIR BLK	.00	2:39pm
ACCY CHK	.08	2:40pm
AIR BLK	.00	2:41pm
SUB TEST	.00	2:42pm
AIR BLK	.00	2:42pm
SUB TEST	.00	2:44pm
AIR BLK	.00	2:45pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

Intox EC/IR-II: Preventive Maintenance

SAMPSON COUNTY DETENTION CENTER 810

Serial Number: 008877 Test Record Number: 4331
Test Date: 01/16/2026 Test Time: 2:46pm EST

System Check: Passed

Baseline Tests

Test	Status	Time
IR	Pass	2:46pm
FLO	Pass	2:46pm
FC	Pass	2:46pm

Temperature Tests

Test	Status	Time
FC1	Pass	2:46pm
SRC	Pass	2:46pm
DET	Pass	2:46pm
BAR	Pass	2:46pm
BT	Pass	2:46pm

Blank Tests

Test	Status	Time
AIR	Pass	2:47pm

Printer Tests

Test	Status	Time
PRNT	Pass	2:47pm

CRC Tests

Test	Status	Time
COMP	Pass	2:47pm
CAL	Pass	2:47pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Scotland Instrument Location Scotland County
Instrument Serial No. 008861 Sheriff's Office

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 21 day of January, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

365156
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

SCOTLAND COUNTY SHERIFFS OFFICE 820

Serial Number: 008861
Test Date: 01/21/2026

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: Garner, Joel K
Permit Number: 0036-5156
Effective:
02/01/2025-02/01/2027

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG417803
Exp Date: 06/26/2026

Test	g/210L	Time
DIAG	Pass	9:04am
AIR BLK	.00	9:05am
ACCY CHK	.08	9:06am
AIR BLK	.00	9:07am
SUB TEST	.00	9:08am
AIR BLK	.00	9:09am
SUB TEST	.00	9:11am
AIR BLK	.00	9:12am

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

Intox EC/IR-II: Preventive Maintenance

SCOTLAND COUNTY SHERIFFS OFFICE 820

Serial Number: 008861 Test Record Number: 2193
Test Date: 01/21/2026 Test Time: 9:12am EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	9:13am
FLO	Pass	9:13am
FC	Pass	9:13am

Temperature Tests

Test	Status	Time
FC1	Pass	9:13am
SRC	Pass	9:13am
DET	Pass	9:13am
BAR	Pass	9:13am
BT	Pass	9:13am

Blank Tests

Test	Status	Time
AIR	Pass	9:14am

Printer Tests

Test	Status	Time
PRNT	Pass	9:14am

CRC Tests

Test	Status	Time
COMP	Pass	9:14am
CAL	Pass	9:14am

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**


County STOKES Instrument Location STOKES COUNTY JAIL
Instrument Serial No. 008596 DANBURY, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 9th day of JANUARY, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.

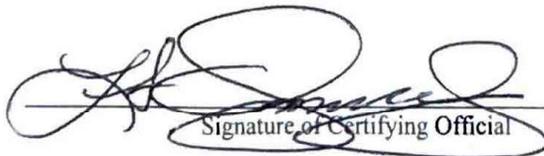


Signature of Certifying Official

353799
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

STOKES COUNTY STOKES COUNTY JAIL 840

Serial Number: 008596
Test Date: 01/09/2026

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Oligmueller, Leo A

Permit Number: 0035-3799

Effective:

02/01/2025-02/01/2027

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG534301

Exp Date: 12/09/2027

Test	g/210L	Time
DIAG	Pass	11:31am
AIR BLK	.00	11:32am
ACCY CHK	.08	11:33am
AIR BLK	.00	11:34am
SUB TEST	.00	11:34am
AIR BLK	.00	11:35am
SUB TEST	.00	11:37am
AIR BLK	.00	11:38am

Reported AC: .00 g/210L

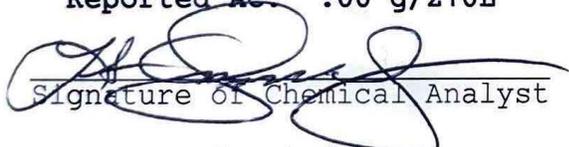
Signature of Chemical Analyst

Court CVR


Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

STOKES COUNTY STOKES COUNTY JAIL 840

Serial Number: 008596 Test Record Number: 1634
Test Date: 01/09/2026 Test Time: 11:39am EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	11:40am
FLO	Pass	11:40am
FC	Pass	11:40am

Temperature Tests

Test	Status	Time
FC1	Pass	11:40am
SRC	Pass	11:40am
DET	Pass	11:40am
BAR	Pass	11:40am
BT	Pass	11:40am

Blank Tests

Test	Status	Time
AIR	Pass	11:41am

Printer Tests

Test	Status	Time
PRNT	Pass	11:41am

CRC Tests

Test	Status	Time
COMP	Pass	11:41am
CAL	Pass	11:41am

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County STOKES Instrument Location KING POLICE

Instrument Serial No. 008718 DEPARTMENT

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 9th day of JANUARY, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

353799
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

STOKES COUNTY KING PD 840

Serial Number: 008718
Test Date: 01/09/2026

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Oligmueller, Leo A

Permit Number: 0035-3799

Effective:

02/01/2025-02/01/2027

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG506301

Exp Date: 03/04/2027

Test	g/210L	Time
DIAG	Pass	1:46pm
AIR BLK	.00	1:47pm
ACCY CHK	.07	1:48pm
AIR BLK	.00	1:49pm
SUB TEST	.00	1:49pm
AIR BLK	.00	1:50pm
SUB TEST	.00	1:51pm
AIR BLK	.00	1:52pm

Reported AC: .00 g/210L

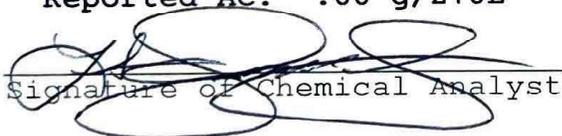
Signature of Chemical Analyst

Court CVR


Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

STOKES COUNTY KING PD 840

Serial Number: 008718 Test Record Number: 2534
Test Date: 01/09/2026 Test Time: 1:53pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	1:53pm
FLO	Pass	1:53pm
FC	Pass	1:53pm

Temperature Tests

Test	Status	Time
FC1	Pass	1:53pm
SRC	Pass	1:53pm
DET	Pass	1:53pm
BAR	Pass	1:53pm
BT	Pass	1:53pm

Blank Tests

Test	Status	Time
AIR	Pass	1:54pm

Printer Tests

Test	Status	Time
PRNT	Pass	1:54pm

CRC Tests

Test	Status	Time
COMP	Pass	1:54pm
CAL	Pass	1:54pm

Preventive Maintenance
Status: Pass


Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County SURRY Instrument Location PILOT MOUNTAIN
Instrument Serial No. 00 8938 POLICE DEPARTMENT

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 9th day of JANUARY, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.




Signature of Certifying Official

353799
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

SURRY COUNTY PILOT MOUNTAIN PD 850

Serial Number: 008938

Test Date: 01/09/2026

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Oligmueller, Leo A

Permit Number: 0035-3799

Effective:

02/01/2025-02/01/2027

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG506301

Exp Date: 03/04/2027

Test	g/210L	Time
DIAG	Pass	12:40pm
AIR BLK	.00	12:41pm
ACCY CHK	.08	12:42pm
AIR BLK	.00	12:43pm
SUB TEST	.00	12:45pm
AIR BLK	.00	12:46pm
SUB TEST	.00	12:48pm
AIR BLK	.00	12:49pm

Reported AC: .00 g/210L

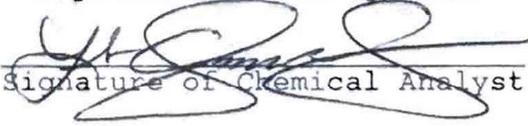
Signature of Chemical Analyst

Court CVR


Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

SURRY COUNTY PILOT MOUNTAIN PD 850

Serial Number: 008938 Test Record Number: 914
Test Date: 01/09/2026 Test Time: 12:51pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	12:51pm
FLO	Pass	12:51pm
FC	Pass	12:51pm

Temperature Tests

Test	Status	Time
FC1	Pass	12:51pm
SRC	Pass	12:51pm
DET	Pass	12:51pm
BAR	Pass	12:51pm
BT	Pass	12:51pm

Blank Tests

Test	Status	Time
AIR	Pass	12:52pm

Printer Tests

Test	Status	Time
PRNT	Pass	12:52pm

CRC Tests

Test	Status	Time
COMP	Pass	12:52pm
CAL	Pass	12:52pm

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County Swain Instrument Location Swain Co. Jail

Instrument Serial No. 008723 Bryson City, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 22 day of January, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Cliff R. Guth
Signature of Certifying Official

843310
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

SWAIN COUNTY JAIL 860

Serial Number: 008723
Test Date: 01/22/2026

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE

Analyst's Name: *Cutler, Daniel R*
Permit Number: 0084-3310
Effective:
02/01/2025-02/01/2027

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: *Breath Test*

Lot Number: AG505001
Exp Date: 02/19/2027

Test	g/210L	Time
DIAG	Pass	12:17pm
AIR BLK	.00	12:17pm
ACCY CHK	.07	12:18pm
AIR BLK	.00	12:20pm
SUB TEST	.00	12:20pm
AIR BLK	.00	12:21pm
SUB TEST	.00	12:23pm
AIR BLK	.00	12:24pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

Intox EC/IR-II: Preventive Maintenance

SWAIN COUNTY JAIL 860

Serial Number: 008723 Test Record Number: 945
Test Date: 01/22/2026 Test Time: 12:26pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	12:26pm
FLO	Pass	12:26pm
FC	Pass	12:26pm

Temperature Tests

Test	Status	Time
FC1	Pass	12:26pm
SRC	Pass	12:26pm
DET	Pass	12:26pm
BAR	Pass	12:26pm
BT	Pass	12:26pm

Blank Tests

Test	Status	Time
AIR	Pass	12:27pm

Printer Tests

Test	Status	Time
PRNT	Pass	12:27pm

CRC Tests

Test	Status	Time
COMP	Pass	12:27pm
CAL	Pass	12:27pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County Swain Instrument Location Swain Co. Jail
Instrument Serial No. 008727 Bryson City, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 22 day of January, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Erin R. Luth
Signature of Certifying Official

843310
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

SWAIN COUNTY JAIL 860

Serial Number: 008727

Test Date: 01/22/2026

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Cutler, Daniel R

Permit Number: 0084-3310

Effective:

02/01/2025-02/01/2027

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG503001

Exp Date: 01/30/2027

Test	g/210L	Time
DIAG	Pass	12:08pm
AIR BLK	.00	12:09pm
ACCY CHK	.07	12:09pm
AIR BLK	.00	12:10pm
SUB TEST	.00	12:11pm
AIR BLK	.00	12:12pm
SUB TEST	.00	12:13pm
AIR BLK	.00	12:14pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

SWAIN COUNTY JAIL 860

Serial Number: 008727 Test Record Number: 1734
Test Date: 01/22/2026 Test Time: 12:16pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	12:16pm
FLO	Pass	12:16pm
FC	Pass	12:16pm

Temperature Tests

Test	Status	Time
FC1	Pass	12:16pm
SRC	Pass	12:16pm
DET	Pass	12:16pm
BAR	Pass	12:16pm
BT	Pass	12:16pm

Blank Tests

Test	Status	Time
AIR	Pass	12:17pm


Printer Tests

Test	Status	Time
PRNT	Pass	12:17pm

CRC Tests

Test	Status	Time
COMP	Pass	12:17pm
CAL	Pass	12:17pm

Preventive Maintenance
Status: Pass

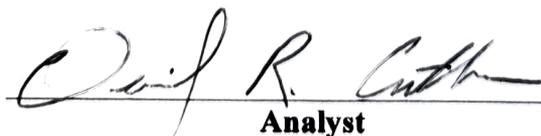

Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County Transylvania Instrument Location Transylvania County Jail

Instrument Serial No. 008609 Brevard, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 08 day of January, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

244987
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

TRANSYLVANIA COUNTY TRANSYLVANIA
COUNTY JAIL 870

Serial Number: 008609
Test Date: 01/08/2026

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: Loftis, Benjamin C
Permit Number: 0024-4987
Effective:
03/01/2025-03/01/2027

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG534301
Exp Date: 12/09/2027

Test	g/210L	Time
DIAG	Pass	11:27am
AIR BLK	.00	11:28am
ACCY CHK	.07	11:29am
AIR BLK	.00	11:30am
SUB TEST	.00	11:30am
AIR BLK	.00	11:31am
SUB TEST	.00	11:33am
AIR BLK	.00	11:34am

Reported AC: .00 g/210L

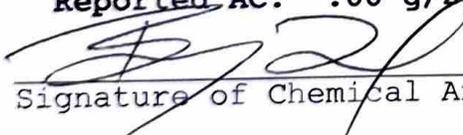

Signature of Chemical Analyst
Court CVR



Analyst

Intox EC/IR-II: Preventive Maintenance

TRANSYLVANIA COUNTY TRANSYLVANIA COUNTY JAIL 870

Serial Number: 008609 Test Record Number: 1382
Test Date: 01/08/2026 Test Time: 11:34am EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	11:34am
FLO	Pass	11:34am
FC	Pass	11:34am

Temperature Tests

Test	Status	Time
FC1	Pass	11:34am
SRC	Pass	11:34am
DET	Pass	11:34am
BAR	Pass	11:34am
BT	Pass	11:34am

Blank Tests

Test	Status	Time
AIR	Pass	11:35am


Printer Tests

Test	Status	Time
PRNT	Pass	11:35am

CRC Tests

Test	Status	Time
COMP	Pass	11:35am
CAL	Pass	11:35am

Preventive Maintenance
Status: Pass

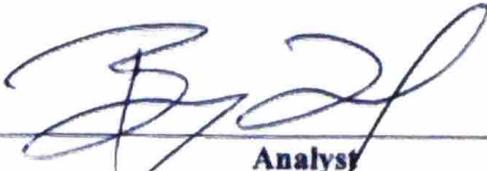

Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County Transylvania Instrument Location Transylvania County Jail
Instrument Serial No. 003820 Brevard, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 03 day of January, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

244987
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

TRANSYLVANIA COUNTY TRANSYLVANIA
COUNTY JAIL 870

Serial Number: 008820
Test Date: 01/08/2026

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Loftis, Benjamin C

Permit Number: 0024-4987

Effective:

03/01/2025-03/01/2027

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG534301


Exp Date: 12/09/2027

Test	g/210L	Time
DIAG	Pass	11:28am
AIR BLK	.00	11:29am
ACCY CHK	.07	11:29am
AIR BLK	.00	11:30am
SUB TEST	.00	11:31am
AIR BLK	.00	11:32am
SUB TEST	.00	11:33am
AIR BLK	.00	11:34am

Reported AC: .00 g/210L

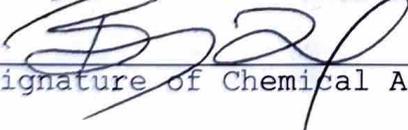

Signature of Chemical Analyst
Court CVR

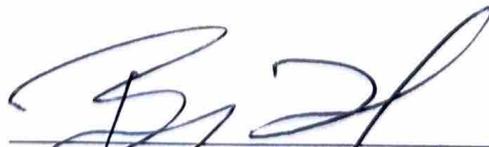

Analyst

Intox EC/IR-II: Preventive Maintenance

TRANSYLVANIA COUNTY TRANSYLVANIA COUNTY JAIL 870

Serial Number: 008820 Test Record Number: 1843
Test Date: 01/08/2026 Test Time: 11:34am EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	11:35am
FLO	Pass	11:35am
FC	Pass	11:35am

Temperature Tests

Test	Status	Time
FC1	Pass	11:35am
SRC	Pass	11:35am
DET	Pass	11:35am
BAR	Pass	11:35am
BT	Pass	11:35am

Blank Tests

Test	Status	Time
AIR	Pass	11:36am

Printer Tests

Test	Status	Time
PRNT	Pass	11:36am

CRC Tests

Test	Status	Time
COMP	Pass	11:36am
CAL	Pass	11:36am

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Union Instrument Location Stallings PD
Instrument Serial No. 008694 Stallings, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 27th day of January, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Handwritten Signature]
Signature of Certifying Official

849845
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

UNION COUNTY STALLINGS PD 890

Serial Number: 008694

Test Date: 01/27/2026

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Helms, Bryce A

Permit Number: 0084-9845

Effective:

02/01/2025-02/01/2027

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG516203

Exp Date: 06/11/2027

Test	g/210L	Time
DIAG	Pass	1:57pm
AIR BLK	.00	1:58pm
ACCY CHK	.08	1:59pm
AIR BLK	.00	2:00pm
SUB TEST	.00	2:00pm
AIR BLK	.00	2:01pm
SUB TEST	.00	2:03pm
AIR BLK	.00	2:04pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

Intox EC/IR-II: Preventive Maintenance

UNION COUNTY STALLINGS PD 890

Serial Number: 008694 Test Record Number: 1982
Test Date: 01/27/2026 Test Time: 2:04pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	2:04pm
FLO	Pass	2:04pm
FC	Pass	2:05pm

Temperature Tests

Test	Status	Time
FC1	Pass	2:05pm
SRC	Pass	2:05pm
DET	Pass	2:05pm
BAR	Pass	2:05pm
BT	Pass	2:05pm

Blank Tests

Test	Status	Time
AIR	Pass	2:05pm

Printer Tests

Test	Status	Time
PRNT	Pass	2:05pm

CRC Tests

Test	Status	Time
COMP	Pass	2:06pm
CAL	Pass	2:06pm

Preventive Maintenance
Status: *Pass*



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County Union Instrument Location Union County NC
Instrument Serial No 0088866 Monroe, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 8th day of January, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Boyo Helms
Signature of Certifying Official

849845
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

UNION COUNTY UNION COUNTY SO 890

Serial Number: 008866
Test Date: 01/08/2026

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE

Analyst's Name: Helms, Bryce A
Permit Number: 0084-9845
Effective:
02/01/2025-02/01/2027

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test


Lot Number: AG506302
Exp Date: 03/04/2027

Test	g/210L	Time
DIAG	Pass	11:15am
AIR BLK	.00	11:15am
ACCY CHK	.07	11:16am
AIR BLK	.00	11:17am
SUB TEST	.00	11:18am
AIR BLK	.00	11:19am
SUB TEST	.00	11:20am
AIR BLK	.00	11:21am

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR

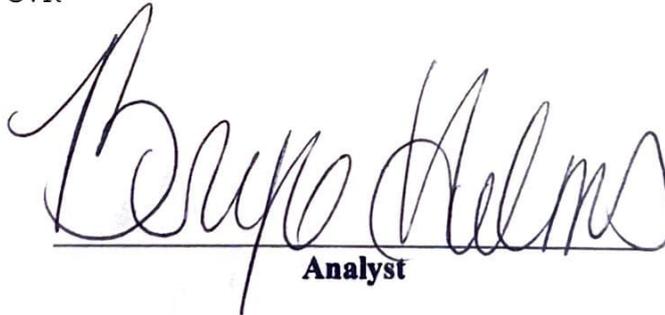
Analyst

Intox EC/IR-II: Preventive Maintenance

UNION COUNTY UNION COUNTY SO 890

Serial Number: 008866 Test Record Number: 4948
Test Date: 01/08/2026 Test Time: 11:21am EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	11:22am
FLO	Pass	11:22am
FC	Pass	11:22am

Temperature Tests

Test	Status	Time
FC1	Pass	11:22am
SRC	Pass	11:22am
DET	Pass	11:22am
BAR	Pass	11:22am
BT	Pass	11:22am

Blank Tests

Test	Status	Time
AIR	Pass	11:23am


Printer Tests

Test	Status	Time
PRNT	Pass	11:23am

CRC Tests

Test	Status	Time
COMP	Pass	11:23am
CAL	Pass	11:23am

Preventive Maintenance
Status: Pass

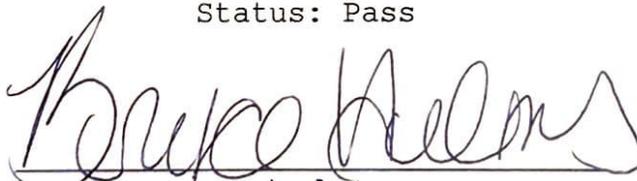
Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Union Instrument Location Union County
Instrument Serial No. 008876 Monroe, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 8th day of January, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Bryon Helms
Signature of Certifying Official

849845
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

UNION COUNTY UNION COUNTY SO 890

Serial Number: 008876
Test Date: 01/08/2026

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: Helms, Bryce A
Permit Number: 0084-9845
Effective:
02/01/2025-02/01/2027

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG506302
Exp Date: 03/04/2027


Test	g/210L	Time
DIAG	Pass	11:13am
AIR BLK	.00	11:14am
ACCY CHK	.07	11:15am
AIR BLK	.00	11:16am
SUB TEST	.00	11:17am
AIR BLK	.00	11:18am
SUB TEST	.00	11:20am
AIR BLK	.00	11:21am

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR

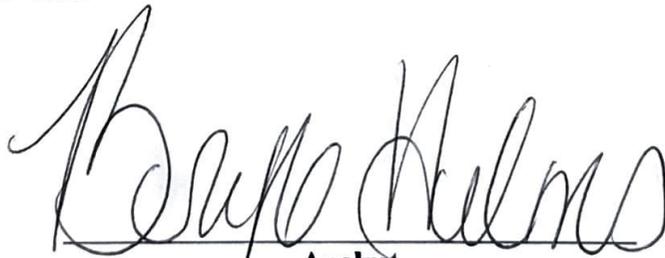

Analyst

Intox EC/IR-II: Preventive Maintenance

UNION COUNTY UNION COUNTY SO 890

Serial Number: 008876 Test Record Number: 7585
Test Date: 01/08/2026 Test Time: 11:21am EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	11:21am
FLO	Pass	11:21am
FC	Pass	11:21am

Temperature Tests

Test	Status	Time
FC1	Pass	11:22am
SRC	Pass	11:22am
DET	Pass	11:22am
BAR	Pass	11:22am
BT	Pass	11:22am

Blank Tests

Test	Status	Time
AIR	Pass	11:22am


Printer Tests

Test	Status	Time
PRNT	Pass	11:22am

CRC Tests

Test	Status	Time
COMP	Pass	11:22am
CAL	Pass	11:22am

Preventive Maintenance
Status: Pass

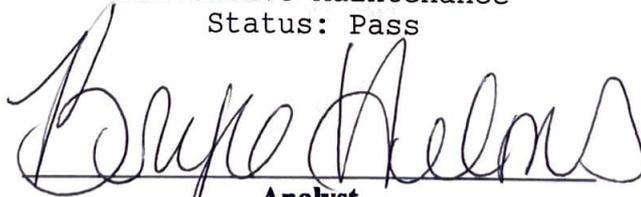
Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County Union Instrument Location Stallings PD
Instrument Serial No. 008927 Stallings, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 6th day of January, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Bryce Helms
Signature of Certifying Official

849845
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

UNION COUNTY STALLINGS PD 890

Serial Number: 008927
Test Date: 01/06/2026

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE

Analyst's Name: Helms, Bryce A
Permit Number: 0084-9845
Effective:
02/01/2025-02/01/2027

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG516203
Exp Date: 06/11/2027

Test	g/210L	Time
DIAG	Pass	12:09pm
AIR BLK	.00	12:10pm
ACCY CHK	.07	12:11pm
AIR BLK	.00	12:12pm
SUB TEST	.00	12:12pm
AIR BLK	.00	12:13pm
SUB TEST	.00	12:15pm
AIR BLK	.00	12:16pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

Intox EC/IR-II: Preventive Maintenance

UNION COUNTY STALLINGS PD 890

Serial Number: 008927 Test Record Number: 1313
Test Date: 01/06/2026 Test Time: 12:18pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	12:18pm
FLO	Pass	12:18pm
FC	Pass	12:18pm

Temperature Tests

Test	Status	Time
FC1	Pass	12:18pm
SRC	Pass	12:18pm
DET	Pass	12:18pm
BAR	Pass	12:18pm
BT	Pass	12:18pm

Blank Tests

Test	Status	Time
AIR	Pass	12:19pm


Printer Tests

Test	Status	Time
PRNT	Pass	12:19pm

CRC Tests

Test	Status	Time
COMP	Pass	12:19pm
CAL	Pass	12:19pm

Preventive Maintenance
Status: Pass

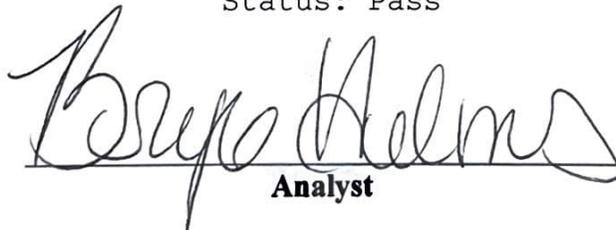
Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Wake Instrument Location BAT Mobile Unit 10

Instrument Serial No. 008584

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 23 day of January, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.




Signature of Certifying Official

193759
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

WAKE COUNTY BAT MOBILE UNIT 10 910

Serial Number: 008584

Test Date: 01/23/2026

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Carroll, Barry J

Permit Number: 0019-3759

Effective:

09/01/2025-09/01/2027

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG534301

Exp Date: 12/09/2027

Test	g/210L	Time
DIAG	Pass	11:07pm
AIR BLK	.00	11:08pm
ACCY CHK	.08	11:09pm
AIR BLK	.00	11:09pm
SUB TEST	.00	11:10pm
AIR BLK	.00	11:11pm
SUB TEST	.00	11:12pm
AIR BLK	.00	11:13pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

Intox EC/IR-II: Preventive Maintenance

WAKE COUNTY BAT MOBILE UNIT 10 910

Serial Number: 008584 Test Record Number: 2859
Test Date: 01/23/2026 Test Time: 11:20pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	11:21pm
FLO	Pass	11:21pm
FC	Pass	11:21pm

Temperature Tests

Test	Status	Time
FC1	Pass	11:21pm
SRC	Pass	11:21pm
DET	Pass	11:21pm
BAR	Pass	11:21pm
BT	Pass	11:21pm

Blank Tests

Test	Status	Time
AIR	Pass	11:21pm

Printer Tests

Test	Status	Time
PRNT	Pass	11:22pm

CRC Tests

Test	Status	Time
COMP	Pass	11:22pm
CAL	Pass	11:22pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County WAKE Instrument Location RALEIGH PD NORTHWEST DIST.
Instrument Serial No. 008623 5228 GREENS DAIRY RD
RALEIGH, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 5 day of JANUARY, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

179707
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

WAKE COUNTY NORTH EAST DISTRICT 910

Serial Number: 008623
Test Date: 01/05/2026

Citation Number: M0000000-0
Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Bryant, Earl A

Permit Number: 0017-9707

Effective:

02/01/2025-02/01/2027

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG505001

Exp Date: 02/19/2027

Test	g/210L	Time
DIAG	Pass	11:26am
AIR BLK	.00	11:27am
ACCY CHK	.07	11:28am
AIR BLK	.00	11:29am
SUB TEST	.00	11:29am
AIR BLK	.00	11:30am
SUB TEST	.00	11:32am
AIR BLK	.00	11:33am

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

Intox EC/IR-II: Preventive Maintenance

WAKE COUNTY NORTH EAST DISTRICT 910

Serial Number: 008623 Test Record Number: 5029
Test Date: 01/05/2026 Test Time: 11:33am EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	11:34am
FLO	Pass	11:34am
FC	Pass	11:34am

Temperature Tests

Test	Status	Time
FC1	Pass	11:34am
SRC	Pass	11:34am
DET	Pass	11:34am
BAR	Pass	11:34am
BT	Pass	11:34am

Blank Tests

Test	Status	Time
AIR	Pass	11:35am

Printer Tests

Test	Status	Time
PRNT	Pass	11:35am

CRC Tests

Test	Status	Time
COMP	Pass	11:35am
CAL	Pass	11:35am

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Wake Instrument Location BAT Mobile Unit 10

Instrument Serial No. 008637

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 23 day of January, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Signature of Certifying Official

193759

Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

WAKE COUNTY BAT MOBILE UNIT 10 910

Serial Number: 008637
Test Date: 01/23/2026

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE

Analyst's Name: Carroll, Barry J
Permit Number: 0019-3759
Effective:
09/01/2025-09/01/2027

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG534301
Exp Date: 12/09/2027

Test	g/210L	Time
DIAG	Pass	11:33pm
AIR BLK	.00	11:34pm
ACCY CHK	.07	11:34pm
AIR BLK	.00	11:35pm
SUB TEST	.00	11:36pm
AIR BLK	.00	11:36pm
SUB TEST	.00	11:38pm
AIR BLK	.00	11:39pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

Intox EC/IR-II: Preventive Maintenance

WAKE COUNTY BAT MOBILE UNIT 10 910

Serial Number: 008637 Test Record Number: 3577
Test Date: 01/23/2026 Test Time: 11:39pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	11:40pm
FLO	Pass	11:40pm
FC	Pass	11:40pm

Temperature Tests

Test	Status	Time
FC1	Pass	11:40pm
SRC	Pass	11:40pm
DET	Pass	11:40pm
BAR	Pass	11:40pm
BT	Pass	11:40pm

Blank Tests

Test	Status	Time
AIR	Pass	11:40pm


Printer Tests

Test	Status	Time
PRNT	Pass	11:41pm

CRC Tests

Test	Status	Time
COMP	Pass	11:41pm
CAL	Pass	11:41pm

Preventive Maintenance
Status: Pass

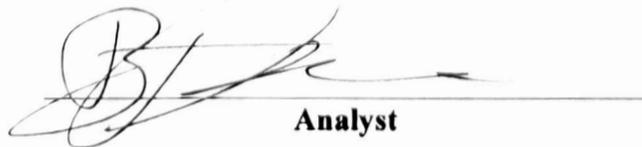

Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Wake Instrument Location BAT Mobile Unit 10


Instrument Serial No. 008686

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 23 day of January, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.





Signature of Certifying Official

193759

Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

WAKE COUNTY BAT MOBILE UNIT 10 910

Serial Number: 008686
Test Date: 01/23/2026

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE

Analyst's Name: Carroll, Barry J
Permit Number: 0019-3759
Effective:
09/01/2025-09/01/2027

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG506302
Exp Date: 03/04/2027

Test	g/210L	Time
DIAG	Pass	9:44pm
AIR BLK	.00	9:45pm
ACCY CHK	.08	9:45pm
AIR BLK	.00	9:46pm
SUB TEST	.00	9:47pm
AIR BLK	.00	9:48pm
SUB TEST	.00	9:50pm
AIR BLK	.00	9:51pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

Intox EC/IR-II: Preventive Maintenance

WAKE COUNTY BAT MOBILE UNIT 10 910

Serial Number: 008686 Test Record Number: 7204
Test Date: 01/23/2026 Test Time: 9:51pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	9:52pm
FLO	Pass	9:52pm
FC	Pass	9:52pm

Temperature Tests

Test	Status	Time
FC1	Pass	9:52pm
SRC	Pass	9:52pm
DET	Pass	9:52pm
BAR	Pass	9:52pm
BT	Pass	9:52pm

Blank Tests

Test	Status	Time
AIR	Pass	9:52pm

Printer Tests

Test	Status	Time
PRNT	Pass	9:52pm

CRC Tests

Test	Status	Time
COMP	Pass	9:53pm
CAL	Pass	9:53pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County WAKE Instrument Location WAKE FOREST P.D.

Instrument Serial No. 008700 225 S. TAYLOR ST
WAKE FOREST, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 9 day of JANUARY, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



E. A. [Signature]
Signature of Certifying Official

179707
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

WAKE COUNTY WAKE FOREST PD 910

Serial Number: 008700
Test Date: 01/09/2026

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Bryant, Earl A

Permit Number: 0017-9707

Effective:

02/01/2025-02/01/2027

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG505001

Exp Date: 02/19/2027

Test	g/210L	Time
DIAG	Pass	3:55pm
AIR BLK	.00	3:56pm
ACCY CHK	.08	3:57pm
AIR BLK	.00	3:58pm
SUB TEST	.00	3:59pm
AIR BLK	.00	3:59pm
SUB TEST	.00	4:01pm
AIR BLK	.00	4:02pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

Intox EC/IR-II: Preventive Maintenance

WAKE COUNTY WAKE FOREST PD 910

Serial Number: 008700 Test Record Number: 2806
Test Date: 01/09/2026 Test Time: 4:02pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	4:03pm
FLO	Pass	4:03pm
FC	Pass	4:03pm

Temperature Tests

Test	Status	Time
FC1	Pass	4:03pm
SRC	Pass	4:03pm
DET	Pass	4:03pm
BAR	Pass	4:03pm
BT	Pass	4:03pm

Blank Tests

Test	Status	Time
AIR	Pass	4:03pm

Printer Tests

Test	Status	Time
PRNT	Pass	4:03pm

CRC Tests

Test	Status	Time
COMP	Pass	4:04pm
CAL	Pass	4:04pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County Wake Instrument Location BAT Mobile Unit 10

Instrument Serial No. 008776

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 23 day of January, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.




Signature of Certifying Official

193759
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

WAKE COUNTY BAT MOBILE UNIT 10 910

Serial Number: 008776
Test Date: 01/23/2026

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: Carroll, Barry J
Permit Number: 0019-3759
Effective:
09/01/2025-09/01/2027

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG417803
Exp Date: 06/26/2026

Test	g/210L	Time
DIAG	Pass	9:34pm
AIR BLK	.00	9:35pm
ACCY CHK	.08	9:35pm
AIR BLK	.00	9:36pm
SUB TEST	.00	9:37pm
AIR BLK	.00	9:38pm
SUB TEST	.00	9:39pm
AIR BLK	.00	9:40pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

Intox EC/IR-II: Preventive Maintenance

WAKE COUNTY BAT MOBILE UNIT 10 910

Serial Number: 008776 Test Record Number: 4162
Test Date: 01/23/2026 Test Time: 9:45pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	9:45pm
FLO	Pass	9:45pm
FC	Pass	9:45pm

Temperature Tests

Test	Status	Time
FC1	Pass	9:45pm
SRC	Pass	9:45pm
DET	Pass	9:45pm
BAR	Pass	9:45pm
BT	Pass	9:45pm

Blank Tests

Test	Status	Time
AIR	Pass	9:46pm


Printer Tests

Test	Status	Time
PRNT	Pass	9:46pm

CRC Tests

Test	Status	Time
COMP	Pass	9:46pm
CAL	Pass	9:46pm

Preventive Maintenance
Status: Pass

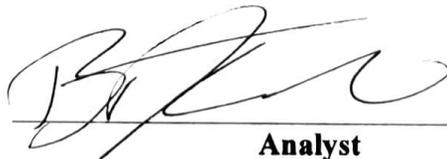

Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Wake Instrument Location BAT Mobile Unit 10

Instrument Serial No. 008779

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 23 day of January, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.





Signature of Certifying Official

193759
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

WAKE COUNTY BAT MOBILE UNIT 10 910

Serial Number: 008779
Test Date: 01/23/2026

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE

Analyst's Name: Carroll, Barry J
Permit Number: 0019-3759
Effective:
09/01/2025-09/01/2027

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG431002
Exp Date: 11/05/2026

Test	g/210L	Time
DIAG	Pass	9:28pm
AIR BLK	.00	9:29pm
ACCY CHK	.08	9:29pm
AIR BLK	.00	9:30pm
SUB TEST	.00	9:30pm
AIR BLK	.00	9:31pm
SUB TEST	.00	9:33pm
AIR BLK	.00	9:34pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

Intox EC/IR-II: Preventive Maintenance

WAKE COUNTY BAT MOBILE UNIT 10 910

Serial Number: 008779 Test Record Number: 4106
Test Date: 01/23/2026 Test Time: 9:35pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	9:35pm
FLO	Pass	9:35pm
FC	Pass	9:35pm

Temperature Tests

Test	Status	Time
FC1	Pass	9:35pm
SRC	Pass	9:35pm
DET	Pass	9:35pm
BAR	Pass	9:35pm
BT	Pass	9:35pm

Blank Tests

Test	Status	Time
AIR	Pass	9:36pm


Printer Tests

Test	Status	Time
PRNT	Pass	9:36pm

CRC Tests

Test	Status	Time
COMP	Pass	9:36pm
CAL	Pass	9:36pm

Preventive Maintenance
Status: Pass

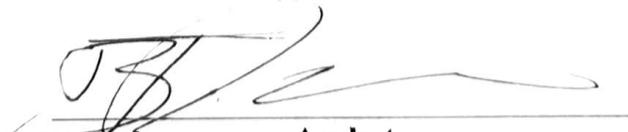

Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Watauga Instrument Location Watauga County Jail
Instrument Serial No. 008715 Boone, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 20th day of January, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

509387
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

WATAUGA COUNTY WATAUGA JAIL 940

Serial Number: 008715
Test Date: 01/20/2026

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: Long, Thomas A
Permit Number: 0050-9387
Effective:
09/01/2025-09/01/2027

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG534301
Exp Date: 12/09/2027

Test	g/210L	Time
DIAG	Pass	10:47am
AIR BLK	.00	10:47am
ACCY CHK	.08	10:48am
AIR BLK	.00	10:49am
SUB TEST	.00	10:50am
AIR BLK	.00	10:51am
SUB TEST	.00	10:52am
AIR BLK	.00	10:53am

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

WATAUGA COUNTY WATAUGA JAIL 940

Serial Number: 008715 Test Record Number: 3123
Test Date: 01/20/2026 Test Time: 10:54am EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	10:54am
FLO	Pass	10:54am
FC	Pass	10:54am

Temperature Tests

Test	Status	Time
FC1	Pass	10:54am
SRC	Pass	10:54am
DET	Pass	10:54am
BAR	Pass	10:54am
BT	Pass	10:54am

Blank Tests

Test	Status	Time
AIR	Pass	10:55am

Printer Tests

Test	Status	Time
PRNT	Pass	10:55am

CRC Tests

Test	Status	Time
COMP	Pass	10:55am
CAL	Pass	10:55am

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County Watauga Instrument Location Boone Police
Instrument Serial No. 008716 Dept

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 20th day of January, 20 26 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

509387
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

WATAUGA COUNTY BOONE PD 940

Serial Number: 008716
Test Date: 01/20/2026

Citation Number: M0000000-0
Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Long, Thomas A

Permit Number: 0050-9387

Effective:

09/01/2025-09/01/2027

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG534301

Exp Date: 12/09/2027


Test	g/210L	Time
DIAG	Pass	9:32am
AIR BLK	.00	9:33am
ACCY CHK	.07	9:33am
AIR BLK	.00	9:34am
SUB TEST	.00	9:35am
AIR BLK	.00	9:36am
SUB TEST	.00	9:38am
AIR BLK	.00	9:39am

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

Intox EC/IR-II: Preventive Maintenance

WATAUGA COUNTY BOONE PD 940

Serial Number: 008716 Test Record Number: 3482
Test Date: 01/20/2026 Test Time: 9:42am EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	9:42am
FLO	Pass	9:42am
FC	Pass	9:42am

Temperature Tests

Test	Status	Time
FC1	Pass	9:42am
SRC	Pass	9:42am
DET	Pass	9:42am
BAR	Pass	9:42am
BT	Pass	9:42am

Blank Tests

Test	Status	Time
AIR	Pass	9:43am


Printer Tests

Test	Status	Time
PRNT	Pass	9:43am

CRC Tests

Test	Status	Time
COMP	Pass	9:43am
CAL	Pass	9:43am

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Wilson Instrument Location Wilson County Detention Center
Instrument Serial No. 008627 100 E. Green St., Wilson, NC.

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 8th day of January, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

377722
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

WILSON COUNTY DETENTION CENTER 970

Serial Number: 008627
Test Date: 01/08/2026

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: Gray, Kelly D
Permit Number: 0037-7722
Effective:
02/01/2025-02/01/2027

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG516203
Exp Date: 06/11/2027


Test	g/210L	Time
DIAG	Pass	1:15pm
AIR BLK	.00	1:16pm
ACCY CHK	.07	1:17pm
AIR BLK	.00	1:18pm
SUB TEST	.00	1:19pm
AIR BLK	.00	1:19pm
SUB TEST	.00	1:21pm
AIR BLK	.00	1:22pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

WILSON COUNTY DETENTION CENTER 970

Serial Number: 008627 Test Record Number: 3659
Test Date: 01/08/2026 Test Time: 1:23pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	1:23pm
FLO	Pass	1:23pm
FC	Pass	1:23pm

Temperature Tests

Test	Status	Time
FC1	Pass	1:23pm
SRC	Pass	1:23pm
DET	Pass	1:23pm
BAR	Pass	1:23pm
BT	Pass	1:23pm

Blank Tests

Test	Status	Time
AIR	Pass	1:24pm


Printer Tests

Test	Status	Time
PRNT	Pass	1:24pm

CRC Tests

Test	Status	Time
COMP	Pass	1:24pm
CAL	Pass	1:24pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Wilson Instrument Location Wilson County Detention Center
Instrument Serial No. 008652 100 E. Green St., Wilson, NC.

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 8th day of January, 2020 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

377722
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

WILSON COUNTY DETENTION CENTER 970

Serial Number: 008652
Test Date: 01/08/2026

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: Gray, Kelly D
Permit Number: 0037-7722
Effective:
02/01/2025-02/01/2027

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG506301
Exp Date: 03/04/2027

Test	g/210L	Time
DIAG	Pass	1:06pm
AIR BLK	.00	1:06pm
ACCY CHK	.08	1:07pm
AIR BLK	.00	1:08pm
SUB TEST	.00	1:09pm
AIR BLK	.00	1:10pm
SUB TEST	.00	1:12pm
AIR BLK	.00	1:12pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

Intox EC/IR-II: Preventive Maintenance

WILSON COUNTY DETENTION CENTER 970

Serial Number: 008652 Test Record Number: 4142
Test Date: 01/08/2026 Test Time: 1:14pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	1:14pm
FLO	Pass	1:14pm
FC	Pass	1:15pm

Temperature Tests

Test	Status	Time
FC1	Pass	1:15pm
SRC	Pass	1:15pm
DET	Pass	1:15pm
BAR	Pass	1:15pm
BT	Pass	1:15pm

Blank Tests

Test	Status	Time
AIR	Pass	1:15pm

Printer Tests

Test	Status	Time
PRNT	Pass	1:15pm

CRC Tests

Test	Status	Time
COMP	Pass	1:16pm
CAL	Pass	1:16pm

Preventive Maintenance
Status: Pass



Analyst