DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Alamance Instrument Location BAT Mobile Unit 7

Instrument Serial No. D08002

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

(1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;

(2) Verify instrument displays time and date;

(3) Initiate breath test sequence;

(4) Enter information as prompted;

(5) Verify instrument accuracy;

(6) When "PLEASE BLOW" appears, collect breath sample;

(7) When "PLEASE BLOW" appears, collect breath sample;

(8) Print test record;

(9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and

(10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 5th day of June, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.

THE GREAT SEAL OF THE STATE OF NORTH CAROLINA

John Lanier
Signature of Certifying Official

1604930
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

DHHS 4080 (04/20)

Intox EC/IR-II: Subject Test

ALAMANCE COUNTY BAT MOBILE UNIT 7 000

Serial Number: *008002*
Test Date: *06/05/2026*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name: *Lanier Jr., John P*
Permit Number: *4582-9118*
Effective:
02/01/2026-02/01/2028

Officer's Name: *NONE, NONE*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG506303
Exp Date: 03/04/2027

Test	g/210L	Time
DIAG	Pass	8:44pm
AIR BLK	.00	8:45pm
ACCY CHK	.07	8:46pm
AIR BLK	.00	8:46pm
SUB TEST	**.00**	**8:47pm**
AIR BLK	.00	8:48pm
SUB TEST	**.00**	**8:49pm**
AIR BLK	.00	8:50pm

Reported AC: .00 g/210L

John Lanier
Signature of Chemical Analyst

Court CVR

John Lanier
Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

ALAMANCE COUNTY BAT MOBILE UNIT 7 000

Serial Number: *008002* Test Record Number: *918*
Test Date: *06/05/2026* Test Time: *8:51pm EDT*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	8:51pm
FLO	Pass	8:51pm
FC	Pass	8:51pm

Temperature Tests

Test	Status	Time
FC1	Pass	8:51pm
SRC	Pass	8:51pm
DET	Pass	8:51pm
BAR	Pass	8:51pm
BT	Pass	8:51pm

Blank Tests

Test	Status	Time
AIR	Pass	8:52pm

Printer Tests

Test	Status	Time
PRNT	Pass	8:52pm

CRC Tests

Test	Status	Time
COMP	Pass	8:52pm
CAL	Pass	8:52pm

Preventive Maintenance
Status: Pass

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD INTOXIMETERS, MODEL INTOX EC/IR II and MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Alamance Instrument Location Alamance Co. Jail

Instrument Serial No. 008853 109 S. Maple St

Graham, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

(1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;

(2) Verify instrument displays time and date;

(3) Initiate breath test sequence;

(4) Enter information as prompted;

(5) Verify instrument accuracy;

(6) When "PLEASE BLOW" appears, collect breath sample;

(7) When "PLEASE BLOW" appears, collect breath sample;

(8) Print test record;

(9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and

(10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 22 day of June, 20 24 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.

Signature of Certifying Official

169451
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

DHHS 4080 (04/20)

Intox EC/IR-II: Subject Test

ALAMANCE COUNTY JAIL 000

Serial Number: *008853*
Test Date: *06/22/2026*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name: *Brame, Bryant T*
Permit Number: *0016-9451*
Effective:
04/01/2026-04/01/2028

Officer's Name: *NONE, NONE*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG602101
Exp Date: 01/28/2028

Test	g/210L	Time
DIAG	Pass	11:32am
AIR BLK	.00	11:33am
ACCY CHK	.07	11:34am
AIR BLK	.00	11:35am
SUB TEST	**.00**	**11:35am**
AIR BLK	.00	11:36am
SUB TEST	**.00**	**11:38am**
AIR BLK	.00	11:39am

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

ALAMANCE COUNTY JAIL 000

Serial Number: *008853* Test Record Number: *5463*
Test Date: *06/22/2026* Test Time: *11:39am EDT*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	11:40am
FLO	Pass	11:40am
FC	Pass	11:40am

Temperature Tests

Test	Status	Time
FC1	Pass	11:40am
SRC	Pass	11:40am
DET	Pass	11:40am
BAR	Pass	11:40am
BT	Pass	11:40am

Blank Tests

Test	Status	Time
AIR	Pass	11:41am

Printer Tests

Test	Status	Time
PRNT	Pass	11:41am

CRC Tests

Test	Status	Time
COMP	Pass	11:41am
CAL	Pass	11:41am

Preventive Maintenance
Status: Pass



Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Alamance Instrument Location Alamance Co. Jail

Instrument Serial No. 008913 109 S. Maple St.

Graham, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

(1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;

(2) Verify instrument displays time and date;

(3) Initiate breath test sequence;

(4) Enter information as prompted;

(5) Verify instrument accuracy;

(6) When "PLEASE BLOW" appears, collect breath sample;

(7) When "PLEASE BLOW" appears, collect breath sample;

(8) Print test record;

(9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and

(10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 22 day of June, 2024 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.

Signature of Certifying Official

169457
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

ALAMANCE COUNTY JAIL 000

Serial Number: *008913*
Test Date: *06/22/2026*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name: *Brame, Bryant T*
Permit Number: *0016-9451*
Effective:
04/01/2026-04/01/2028

Officer's Name: *NONE, NONE*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG602101
Exp Date: 01/28/2028

Test	g/210L	Time
DIAG	Pass	11:25am
AIR BLK	.00	11:25am
ACCY CHK	.07	11:26am
AIR BLK	.00	11:27am
SUB TEST	**.00**	**11:28am**
AIR BLK	.00	11:29am
SUB TEST	**.00**	**11:30am**
AIR BLK	.00	11:31am

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

ALAMANCE COUNTY JAIL 000

Serial Number: *008913* Test Record Number: *6042*
Test Date: *06/22/2026* Test Time: *11:33am EDT*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	11:33am
FLO	Pass	11:33am
FC	Pass	11:33am

Temperature Tests

Test	Status	Time
FC1	Pass	11:33am
SRC	Pass	11:33am
DET	Pass	11:33am
BAR	Pass	11:33am
BT	Pass	11:33am

Blank Tests

Test	Status	Time
AIR	Pass	11:34am

Printer Tests

Test	Status	Time
PRNT	Pass	11:34am

CRC Tests

Test	Status	Time
COMP	Pass	11:34am
CAL	Pass	11:34am

Preventive Maintenance
Status: Pass



Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Alamance Instrument Location BAT Mobile Unit 7

Instrument Serial No. 008968

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

(1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;

(2) Verify instrument displays time and date;

(3) Initiate breath test sequence;

(4) Enter information as prompted;

(5) Verify instrument accuracy;

(6) When "PLEASE BLOW" appears, collect breath sample;

(7) When "PLEASE BLOW" appears, collect breath sample;

(8) Print test record;

(9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and

(10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 5th day of June, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.

John Lanier
Signature of Certifying Official

1604930
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

DHHS 4080 (04/20)

Intox EC/IR-II: Subject Test

ALAMANCE COUNTY BAT MOBILE UNIT 7 000

Serial Number: *008968*
Test Date: *06/05/2026*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name: *Lanier Jr., John P*
Permit Number: *4582-9118*
Effective:
02/01/2026-02/01/2028

Officer's Name: *NONE, NONE*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG506303
Exp Date: 03/04/2027

Test	g/210L	Time
DIAG	Pass	8:38pm
AIR BLK	.00	8:39pm
ACCY CHK	.08	8:40pm
AIR BLK	.00	8:41pm
SUB TEST	**.00**	**8:42pm**
AIR BLK	.00	8:43pm
SUB TEST	**.00**	**8:44pm**
AIR BLK	.00	8:45pm

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

ALAMANCE COUNTY BAT MOBILE UNIT 7 000

Serial Number: *008968* Test Record Number: *473*
Test Date: *06/05/2026* Test Time: *8:45pm EDT*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	8:46pm
FLO	Pass	8:46pm
FC	Pass	8:46pm

Temperature Tests

Test	Status	Time
FC1	Pass	8:46pm
SRC	Pass	8:46pm
DET	Pass	8:46pm
BAR	Pass	8:46pm
BT	Pass	8:46pm

Blank Tests

Test	Status	Time
AIR	Pass	8:47pm

Printer Tests

Test	Status	Time
PRNT	Pass	8:47pm

CRC Tests

Test	Status	Time
COMP	Pass	8:47pm
CAL	Pass	8:47pm

Preventive Maintenance
Status: Pass

John Lanier

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Alamance Instrument Location BAT Mobile Unit II

Instrument Serial No. 008970

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

(1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;

(2) Verify instrument displays time and date;

(3) Initiate breath test sequence;

(4) Enter information as prompted;

(5) Verify instrument accuracy;

(6) When "PLEASE BLOW" appears, collect breath sample;

(7) When "PLEASE BLOW" appears, collect breath sample;

(8) Print test record;

(9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and

(10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 20th day of June, 20 24 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.

Signature of Certifying Official

062446
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

DHHS 4080 (04/20)

Intox EC/IR-II: Subject Test

ALAMANCE COUNTY BAT MOBILE UNIT 11 000

Serial Number: *008970*
Test Date: *06/20/2026*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name: *Gillstrap, Jeffrey L*
Permit Number: *0006-2446*
Effective:
03/01/2026-03/01/2028

Officer's Name: *NONE, NONE*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG602101
Exp Date: 01/21/2028

Test	g/210L	Time
DIAG	Pass	8:44pm
AIR BLK	.00	8:45pm
ACCY CHK	.07	8:45pm
AIR BLK	.00	8:46pm
SUB TEST	**.00**	**8:47pm**
AIR BLK	.00	8:48pm
SUB TEST	**.00**	**8:49pm**
AIR BLK	.00	8:50pm

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

ALAMANCE COUNTY BAT MOBILE UNIT 11 000

Serial Number: *008970* Test Record Number: *1471*
Test Date: *06/20/2026* Test Time: *8:51pm EDT*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	8:52pm
FLO	Pass	8:52pm
FC	Pass	8:52pm

Temperature Tests

Test	Status	Time
FC1	Pass	8:52pm
SRC	Pass	8:52pm
DET	Pass	8:52pm
BAR	Pass	8:52pm
BT	Pass	8:52pm

Blank Tests

Test	Status	Time
AIR	Pass	8:53pm


Printer Tests

Test	Status	Time
PRNT	Pass	8:53pm

CRC Tests

Test	Status	Time
COMP	Pass	8:53pm
CAL	Pass	8:53pm

Preventive Maintenance
Status: Pass

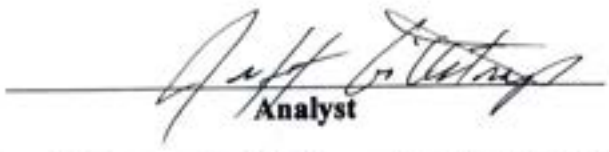

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Alamance Instrument Location BAT Mobile Unit 7

Instrument Serial No. 008971

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

(1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;

(2) Verify instrument displays time and date;

(3) Initiate breath test sequence;

(4) Enter information as prompted;

(5) Verify instrument accuracy;

(6) When "PLEASE BLOW" appears, collect breath sample;

(7) When "PLEASE BLOW" appears, collect breath sample;

(8) Print test record;

(9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and

(10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 5th day of June, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.

John Lanier
Signature of Certifying Official

1604930
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

DHHS 4080 (04/20)

Intox EC/IR-II: Subject Test

ALAMANCE COUNTY BAT MOBILE UNIT 7 000

Serial Number: *008971*
Test Date: *06/05/2026*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name: *Lanier Jr., John P*
Permit Number: *4582-9118*
Effective:
02/01/2026-02/01/2028

Officer's Name: *NONE, NONE*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG506302
Exp Date: 03/04/2027

Test	g/210L	Time
DIAG	Pass	8:52pm
AIR BLK	.00	8:53pm
ACCY CHK	.08	8:54pm
AIR BLK	.00	8:55pm
SUB TEST	**.00**	**8:55pm**
AIR BLK	.00	8:56pm
SUB TEST	**.00**	**8:58pm**
AIR BLK	.00	8:59pm

Reported AC: .00 g/210L

John Lanier

Signature of Chemical Analyst

Court CVR

John Lanier

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

ALAMANCE COUNTY BAT MOBILE UNIT 7 000

Serial Number: *008971* Test Record Number: *420*
Test Date: *06/05/2026* Test Time: *8:59pm EDT*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	9:00pm
FLO	Pass	9:00pm
FC	Pass	9:00pm

Temperature Tests

Test	Status	Time
FC1	Pass	9:00pm
SRC	Pass	9:00pm
DET	Pass	9:00pm
BAR	Pass	9:00pm
BT	Pass	9:00pm

Blank Tests

Test	Status	Time
AIR	Pass	9:01pm

Printer Tests

Test	Status	Time
PRNT	Pass	9:01pm

CRC Tests

Test	Status	Time
COMP	Pass	9:01pm
CAL	Pass	9:01pm

Preventive Maintenance
Status: Pass

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Alamance Instrument Location BAT Mobile Unit 7

Instrument Serial No. DD8972

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

(1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;

(2) Verify instrument displays time and date;

(3) Initiate breath test sequence;

(4) Enter information as prompted;

(5) Verify instrument accuracy;

(6) When "PLEASE BLOW" appears, collect breath sample;

(7) When "PLEASE BLOW" appears, collect breath sample;

(8) Print test record;

(9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and

(10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 5th day of June, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.

John Lanier
Signature of Certifying Official

1604930
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

DHHS 4080 (04/20)

Intox EC/IR-II: Subject Test

ALAMANCE COUNTY BAT MOBILE UNIT 7 000

Serial Number: *008972*
Test Date: *06/05/2026*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name: *Lanier Jr., John P*
Permit Number: *4582-9118*
Effective:
02/01/2026-02/01/2028

Officer's Name: *NONE, NONE*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG506303
Exp Date: 03/04/2027

Test	g/210L	Time
DIAG	Pass	8:40pm
AIR BLK	.00	8:41pm
ACCY CHK	.08	8:41pm
AIR BLK	.00	8:42pm
SUB TEST	**.00**	**8:44pm**
AIR BLK	.00	8:45pm
SUB TEST	**.00**	**8:46pm**
AIR BLK	.00	8:47pm

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

ALAMANCE COUNTY BAT MOBILE UNIT 7 000

Serial Number: *008972* Test Record Number: *488*
Test Date: *06/05/2026* Test Time: *8:48pm EDT*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	8:48pm
FLO	Pass	8:48pm
FC	Pass	8:48pm

Temperature Tests

Test	Status	Time
FC1	Pass	8:48pm
SRC	Pass	8:48pm
DET	Pass	8:48pm
BAR	Pass	8:48pm
BT	Pass	8:48pm

Blank Tests

Test	Status	Time
AIR	Pass	8:49pm

Printer Tests

Test	Status	Time
PRNT	Pass	8:49pm

CRC Tests

Test	Status	Time
COMP	Pass	8:49pm
CAL	Pass	8:49pm

Preventive Maintenance
Status: Pass

John Lanier
Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Alamance Instrument Location BAT Mobile Unit II

Instrument Serial No. 008973

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

(1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;

(2) Verify instrument displays time and date;

(3) Initiate breath test sequence;

(4) Enter information as prompted;

(5) Verify instrument accuracy;

(6) When "PLEASE BLOW" appears, collect breath sample;

(7) When "PLEASE BLOW" appears, collect breath sample;

(8) Print test record;

(9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and

(10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 20th day of June, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.

Signature of Certifying Official

062446
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

DHHS 4080 (04/20)

Intox EC/IR-II: Subject Test

ALAMANCE COUNTY BAT MOBILE UNIT 11 000

Serial Number: *008973*
Test Date: *06/20/2026*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name: *Gillstrap, Jeffrey L*
Permit Number: *0006-2446*
Effective:
03/01/2026-03/01/2028

Officer's Name: *NONE, NONE*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG431003
Exp Date: 11/05/2026

Test	g/210L	Time
DIAG	Pass	8:47pm
AIR BLK	.00	8:48pm
ACCY CHK	.07	8:49pm
AIR BLK	.00	8:50pm
SUB TEST	**.00**	**8:50pm**
AIR BLK	.00	8:51pm
SUB TEST	**.00**	**8:52pm**
AIR BLK	.00	8:53pm

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

ALAMANCE COUNTY BAT MOBILE UNIT 11 000

Serial Number: *008973* Test Record Number: *1510*
Test Date: *06/20/2026* Test Time: *8:54pm EDT*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	8:54pm
FLO	Pass	8:54pm
FC	Pass	8:55pm

Temperature Tests

Test	Status	Time
FC1	Pass	8:55pm
SRC	Pass	8:55pm
DET	Pass	8:55pm
BAR	Pass	8:55pm
BT	Pass	8:55pm

Blank Tests

Test	Status	Time
AIR	Pass	8:55pm

Printer Tests

Test	Status	Time
PRNT	Pass	8:55pm

CRC Tests

Test	Status	Time
COMP	Pass	8:56pm
CAL	Pass	8:56pm

Preventive Maintenance
Status: Pass



Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County ALEXANDER Instrument Location ALEXANDER CO. S.O.

Instrument Serial No. 005883 TAYLORSVILLE NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

(1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;

(2) Verify instrument displays time and date;

(3) Initiate breath test sequence;

(4) Enter information as prompted;

(5) Verify instrument accuracy;

(6) When "PLEASE BLOW" appears, collect breath sample;

(7) When "PLEASE BLOW" appears, collect breath sample;

(8) Print test record;

(9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and

(10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 01 day of JUNE, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.

Signature of Certifying Official

274970
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

DHHS 4080 (04/20)

Intox EC/IR-II: Subject Test

ALEXANDER COUNTY ALEXANDER COUNTY SO 010

Serial Number: *008813*
Test Date: *06/01/2026*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name: *Fleming, Tina S*
Permit Number: *0027-4970*
Effective:
02/01/2025-02/01/2027

Officer's Name: *NONE, NONE*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG431001
Exp Date: 11/05/2026

Test	g/210L	Time
DIAG	Pass	3:36pm
AIR BLK	.00	3:37pm
ACCY CHK	.08	3:38pm
AIR BLK	.00	3:39pm
SUB TEST	**.00**	**3:40pm**
AIR BLK	.00	3:40pm
SUB TEST	**.00**	**3:43pm**
AIR BLK	.00	3:44pm

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

ALEXANDER COUNTY ALEXANDER COUNTY SO 010

Serial Number: *008813* Test Record Number: *2551*
Test Date: *06/01/2026* Test Time: *3:46pm EDT*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	3:47pm
FLO	Pass	3:47pm
FC	Pass	3:47pm

Temperature Tests

Test	Status	Time
FC1	Pass	3:47pm
SRC	Pass	3:47pm
DET	Pass	3:47pm
BAR	Pass	3:47pm
BT	Pass	3:47pm

Blank Tests

Test	Status	Time
AIR	Pass	3:48pm


Printer Tests

Test	Status	Time
PRNT	Pass	3:48pm

CRC Tests

Test	Status	Time
COMP	Pass	3:48pm
CAL	Pass	3:48pm

Preventive Maintenance
Status: Pass

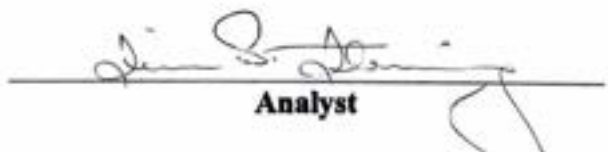

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County BEAUFORT Instrument Location BAT Mobile Unit 12

Instrument Serial No. 008601

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

(1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;

(2) Verify instrument displays time and date;

(3) Initiate breath test sequence;

(4) Enter information as prompted;

(5) Verify instrument accuracy;

(6) When "PLEASE BLOW" appears, collect breath sample;

(7) When "PLEASE BLOW" appears, collect breath sample;

(8) Print test record;

(9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and

(10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 19th day of June, 20 26 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.

Signature of Certifying Official

83034
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

DHHS 4080 (04/20)

Intox EC/IR-II: Subject Test

BEAUFORT COUNTY BAT MOBILE UNIT 12 060

Serial Number: *008601*
Test Date: *06/13/2026*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name:
Crutchfield Jr., Marshall B
Permit Number: *0008-3034*
Effective:
03/01/2026-03/01/2028

Officer's Name: *NONE, NONE*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG501307
Exp Date: 01/13/2027

Test	g/210L	Time
DIAG	Pass	3:39pm
AIR BLK	.00	3:40pm
ACCY CHK	.07	3:41pm
AIR BLK	.00	3:42pm
SUB TEST	**.00**	**3:43pm**
AIR BLK	.00	3:44pm
SUB TEST	**.00**	**3:45pm**
AIR BLK	.00	3:46pm

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

BEAUFORT COUNTY BAT MOBILE UNIT 12 060

Serial Number: *008601* Test Record Number: *1950*
Test Date: *06/13/2026* Test Time: *3:47pm EDT*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	3:47pm
FLO	Pass	3:47pm
FC	Pass	3:48pm

Temperature Tests

Test	Status	Time
FC1	Pass	3:48pm
SRC	Pass	3:48pm
DET	Pass	3:48pm
BAR	Pass	3:48pm
BT	Pass	3:48pm

Blank Tests

Test	Status	Time
AIR	Pass	3:48pm

Printer Tests

Test	Status	Time
PRNT	Pass	3:48pm

CRC Tests

Test	Status	Time
COMP	Pass	3:48pm
CAL	Pass	3:48pm

Preventive Maintenance
Status: Pass



Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County BEAUFORT Instrument Location BAT Mobile Unit 12

Instrument Serial No. 008698

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

(1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;

(2) Verify instrument displays time and date;

(3) Initiate breath test sequence;

(4) Enter information as prompted;

(5) Verify instrument accuracy;

(6) When "PLEASE BLOW" appears, collect breath sample;

(7) When "PLEASE BLOW" appears, collect breath sample;

(8) Print test record;

(9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and

(10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 13th day of June, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.

Signature of Certifying Official

83034
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

BEAUFORT COUNTY BAT MOBILE UNIT 12 060

Serial Number: *008698*
Test Date: *06/13/2026*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name:
Crutchfield Jr., Marshall B
Permit Number: *0008-3034*
Effective:
03/01/2026-03/01/2028

Officer's Name: *NONE, NONE*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG431002
Exp Date: 11/05/2026

Test	g/210L	Time
DIAG	Pass	3:27pm
AIR BLK	.00	3:28pm
ACCY CHK	.07	3:28pm
AIR BLK	.00	3:29pm
SUB TEST	**.00**	**3:30pm**
AIR BLK	.00	3:31pm
SUB TEST	**.00**	**3:32pm**
AIR BLK	.00	3:33pm

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

BEAUFORT COUNTY BAT MOBILE UNIT 12 060

Serial Number: *008698* Test Record Number: *2782*
Test Date: *06/13/2026* Test Time: *3:36pm EDT*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	3:36pm
FLO	Pass	3:36pm
FC	Pass	3:36pm

Temperature Tests

Test	Status	Time
FC1	Pass	3:36pm
SRC	Pass	3:36pm
DET	Pass	3:36pm
BAR	Pass	3:36pm
BT	Pass	3:36pm

Blank Tests

Test	Status	Time
AIR	Pass	3:37pm

Printer Tests

Test	Status	Time
PRNT	Pass	3:37pm

CRC Tests

Test	Status	Time
COMP	Pass	3:37pm
CAL	Pass	3:37pm

Preventive Maintenance
Status: Pass



Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Beaufort Instrument Location BAT Mobile Unit 12

Instrument Serial No. 008788

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

(1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;

(2) Verify instrument displays time and date;

(3) Initiate breath test sequence;

(4) Enter information as prompted;

(5) Verify instrument accuracy;

(6) When "PLEASE BLOW" appears, collect breath sample;

(7) When "PLEASE BLOW" appears, collect breath sample;

(8) Print test record;

(9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and

(10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 13th day of June, 20 26 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.

Signature of Certifying Official

83034
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

BEAUFORT COUNTY BAT MOBILE UNIT 12 060

Serial Number: *008788*
Test Date: *06/13/2026*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name:
Crutchfield Jr., Marshall B
Permit Number: *0008-3034*
Effective:
03/01/2026-03/01/2028

Officer's Name: *NONE, NONE*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG417802
Exp Date: 06/26/2026

Test	g/210L	Time
DIAG	Pass	3:26pm
AIR BLK	.00	3:27pm
ACCY CHK	.07	3:27pm
AIR BLK	.00	3:28pm
SUB TEST	**.00**	**3:29pm**
AIR BLK	.00	3:30pm
SUB TEST	**.00**	**3:31pm**
AIR BLK	.00	3:32pm

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

BEAUFORT COUNTY BAT MOBILE UNIT 12 060

Serial Number: *008788* Test Record Number: *2563*
Test Date: *06/13/2026* Test Time: *3:33pm EDT*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	3:33pm
FLO	Pass	3:33pm
FC	Pass	3:34pm

Temperature Tests

Test	Status	Time
FC1	Pass	3:34pm
SRC	Pass	3:34pm
DET	Pass	3:34pm
BAR	Pass	3:34pm
BT	Pass	3:34pm

Blank Tests

Test	Status	Time
AIR	Pass	3:34pm


Printer Tests

Test	Status	Time
PRNT	Pass	3:34pm

CRC Tests

Test	Status	Time
COMP	Pass	3:34pm
CAL	Pass	3:34pm

Preventive Maintenance
Status: Pass



Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Bertie Instrument Location Bertie Co. S.O.

Instrument Serial No. 008897 222 County Farm Rd. Windsor, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

(1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;

(2) Verify instrument displays time and date;

(3) Initiate breath test sequence;

(4) Enter information as prompted;

(5) Verify instrument accuracy;

(6) When "PLEASE BLOW" appears, collect breath sample;

(7) When "PLEASE BLOW" appears, collect breath sample;

(8) Print test record;

(9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and

(10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 3rd day of June, 20 26 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.

Signature of Certifying Official

206272
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

DHHS 4080 (04/20)

Intox EC/IR-II: Subject Test

BERTIE COUNTY BERTIE CO SO 070

Serial Number: *008897*
Test Date: *06/03/2026*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name: *Chappell, Mark A*
Permit Number: *0020-6272*
Effective:
02/01/2026-02/01/2028

Officer's Name: *NONE, NONE*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG516203
Exp Date: 06/11/2027

Test	g/210L	Time
DIAG	Pass	10:02am
AIR BLK	.00	10:02am
ACCY CHK	.08	10:03am
AIR BLK	.00	10:04am
SUB TEST	**.00**	**10:05am**
AIR BLK	.00	10:06am
SUB TEST	**.00**	**10:07am**
AIR BLK	.00	10:08am

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

BERTIE COUNTY BERTIE CO SO 070

Serial Number: *008897* Test Record Number: *1732*
Test Date: *06/03/2026* Test Time: *10:09am EDT*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	10:09am
FLO	Pass	10:09am
FC	Pass	10:09am

Temperature Tests

Test	Status	Time
FC1	Pass	10:09am
SRC	Pass	10:09am
DET	Pass	10:09am
BAR	Pass	10:09am
BT	Pass	10:09am

Blank Tests

Test	Status	Time
AIR	Pass	10:10am

Printer Tests

Test	Status	Time
PRNT	Pass	10:10am

CRC Tests

Test	Status	Time
COMP	Pass	10:10am
CAL	Pass	10:10am

Preventive Maintenance
Status: Pass

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Brunswick Instrument Location Leland Police Department

Instrument Serial No. 008787

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

(1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;

(2) Verify instrument displays time and date;

(3) Initiate breath test sequence;

(4) Enter information as prompted;

(5) Verify instrument accuracy;

(6) When "PLEASE BLOW" appears, collect breath sample;

(7) When "PLEASE BLOW" appears, collect breath sample;

(8) Print test record;

(9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and

(10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 8th day of June, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.

Signature of Certifying Official

845023
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

DHHS 4080 (04/20)

Intox EC/IR-II: Subject Test

BRUNSWICK COUNTY LELAND PD 090

Serial Number: *008787*
Test Date: *06/08/2026*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name: *Ryan, Robert F*
Permit Number: *0084-5023*
Effective:
02/01/2026-02/01/2028

Officer's Name: *NONE, NONE*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG516204
Exp Date: 06/11/2027

Test	g/210L	Time
DIAG	Pass	12:54pm
AIR BLK	.00	12:55pm
ACCY CHK	.08	12:55pm
AIR BLK	.00	12:57pm
SUB TEST	**.00**	**12:57pm**
AIR BLK	.00	12:58pm
SUB TEST	**.00**	**1:00pm**
AIR BLK	.00	1:00pm

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

BRUNSWICK COUNTY LELAND PD 090

Serial Number: *008787* Test Record Number: *1451*
Test Date: *06/08/2026* Test Time: *1:01pm EDT*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	1:01pm
FLO	Pass	1:01pm
FC	Pass	1:01pm

Temperature Tests

Test	Status	Time
FC1	Pass	1:02pm
SRC	Pass	1:02pm
DET	Pass	1:02pm
BAR	Pass	1:02pm
BT	Pass	1:02pm

Blank Tests

Test	Status	Time
AIR	Pass	1:02pm

Printer Tests

Test	Status	Time
PRNT	Pass	1:02pm

CRC Tests

Test	Status	Time
COMP	Pass	1:02pm
CAL	Pass	1:02pm

Preventive Maintenance
Status: Pass

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Buncombe Instrument Location BAT Mobile Unit II

Instrument Serial No. 008970

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

(1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;

(2) Verify instrument displays time and date;

(3) Initiate breath test sequence;

(4) Enter information as prompted;

(5) Verify instrument accuracy;

(6) When "PLEASE BLOW" appears, collect breath sample;

(7) When "PLEASE BLOW" appears, collect breath sample;

(8) Print test record;

(9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and

(10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 10th day of June, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.

Signature of Certifying Official

062446
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

DHHS 4080 (04/20)

Intox EC/IR-II: Subject Test

BUNCOMBE COUNTY BAT MOBILE UNIT 11 100

Serial Number: *008970*
Test Date: *06/10/2026*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name: *Gillstrap, Jeffrey L*
Permit Number: *0006-2446*
Effective:
03/01/2026-03/01/2028

Officer's Name: *NONE, NONE*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG417802
Exp Date: 06/26/2026

Test	g/210L	Time
DIAG	Pass	8:23pm
AIR BLK	.00	8:24pm
ACCY CHK	.07	8:25pm
AIR BLK	.00	8:26pm
SUB TEST	**.00**	**8:26pm**
AIR BLK	.00	8:27pm
SUB TEST	**.00**	**8:29pm**
AIR BLK	.00	8:30pm

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

BUNCOMBE COUNTY BAT MOBILE UNIT 11 100

Serial Number: *008970* Test Record Number: *1459*
Test Date: *06/10/2026* Test Time: *8:30pm EDT*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	8:30pm
FLO	Pass	8:30pm
FC	Pass	8:31pm

Temperature Tests

Test	Status	Time
FC1	Pass	8:31pm
SRC	Pass	8:31pm
DET	Pass	8:31pm
BAR	Pass	8:31pm
BT	Pass	8:31pm

Blank Tests

Test	Status	Time
AIR	Pass	8:31pm

Printer Tests

Test	Status	Time
PRNT	Pass	8:31pm

CRC Tests

Test	Status	Time
COMP	Pass	8:32pm
CAL	Pass	8:32pm

Preventive Maintenance
Status: Pass



Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Buncombe Instrument Location BAT Mobile Unit II

Instrument Serial No. 008970

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

(1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;

(2) Verify instrument displays time and date;

(3) Initiate breath test sequence;

(4) Enter information as prompted;

(5) Verify instrument accuracy;

(6) When "PLEASE BLOW" appears, collect breath sample;

(7) When "PLEASE BLOW" appears, collect breath sample;

(8) Print test record;

(9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and

(10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 29th day of June, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.

Signature of Certifying Official

06 2446
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

DHHS 4080 (04/20)

Intox EC/IR-II: Subject Test

BUNCOMBE COUNTY BAT MOBILE UNIT 11 100

Serial Number: *008970*
Test Date: *06/29/2026*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name: *Gillstrap, Jeffrey L*
Permit Number: *0006-2446*
Effective:
03/01/2026-03/01/2028

Officer's Name: *NONE, NONE*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG602101
Exp Date: 01/21/2028

Test	g/210L	Time
DIAG	Pass	11:57pm
AIR BLK	.00	11:58pm
ACCY CHK	.07	11:58pm
AIR BLK	.00	11:59pm
SUB TEST	**.00**	**12:00am**
AIR BLK	.00	12:01am
SUB TEST	**.00**	**12:02am**
AIR BLK	.00	12:03am

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

BUNCOMBE COUNTY BAT MOBILE UNIT 11 100

Serial Number: *008970* Test Record Number: *1475*
Test Date: *06/30/2026* Test Time: *12:04am EDT*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	12:05am
FLO	Pass	12:05am
FC	Pass	12:05am

Temperature Tests

Test	Status	Time
FC1	Pass	12:05am
SRC	Pass	12:05am
DET	Pass	12:05am
BAR	Pass	12:05am
BT	Pass	12:05am

Blank Tests

Test	Status	Time
AIR	Pass	12:05am

Printer Tests

Test	Status	Time
PRNT	Pass	12:05am

CRC Tests

Test	Status	Time
COMP	Pass	12:06am
CAL	Pass	12:06am

Preventive Maintenance
Status: Pass



Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD INTOXIMETERS, MODEL INTOX EC/IR II and MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Buncombe Instrument Location BAT Mobile Unit II

Instrument Serial No. 008970

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

(1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;

(2) Verify instrument displays time and date;

(3) Initiate breath test sequence;

(4) Enter information as prompted;

(5) Verify instrument accuracy;

(6) When "PLEASE BLOW" appears, collect breath sample;

(7) When "PLEASE BLOW" appears, collect breath sample;

(8) Print test record;

(9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and

(10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 29th day of June, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.

Signature of Certifying Official

062446
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

DHHS 4080 (04/20)

BUNCOMBE COUNTY BAT MOBILE UNIT 11 100

Serial Number: *008970*
Test Date: *06/29/2026*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name: *Gillstrap, Jeffrey L*
Permit Number: *0006-2446*
Effective:
03/01/2026-03/01/2028

Officer's Name: *NONE, NONE*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG602101
Exp Date: 01/21/2028

Test	g/210L	Time
DIAG	Pass	8:34pm
AIR BLK	.00	8:35pm
ACCY CHK	.07	8:35pm
AIR BLK	.00	8:36pm
SUB TEST	**.00**	**8:37pm**
AIR BLK	.00	8:38pm
SUB TEST	**.00**	**8:39pm**
AIR BLK	.00	8:40pm

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

BUNCOMBE COUNTY BAT MOBILE UNIT 11 100

Serial Number: *008970* Test Record Number: *1473*
Test Date: *06/29/2026* Test Time: *8:45pm EDT*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	8:45pm
FLO	Pass	8:45pm
FC	Pass	8:45pm

Temperature Tests

Test	Status	Time
FC1	Pass	8:45pm
SRC	Pass	8:45pm
DET	Pass	8:45pm
BAR	Pass	8:45pm
BT	Pass	8:45pm

Blank Tests

Test	Status	Time
AIR	Pass	8:46pm

Printer Tests

Test	Status	Time
PRNT	Pass	8:46pm

CRC Tests

Test	Status	Time
COMP	Pass	8:46pm
CAL	Pass	8:46pm

Preventive Maintenance
Status: Pass



Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Buncombe Instrument Location BAT Mobile Unit II

Instrument Serial No. 008970

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

(1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;

(2) Verify instrument displays time and date;

(3) Initiate breath test sequence;

(4) Enter information as prompted;

(5) Verify instrument accuracy;

(6) When "PLEASE BLOW" appears, collect breath sample;

(7) When "PLEASE BLOW" appears, collect breath sample;

(8) Print test record;

(9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and

(10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 30th day of June, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.

Signature of Certifying Official

062446
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

DHHS 4080 (04/20)

BUNCOMBE COUNTY BAT MOBILE UNIT 11 100

Serial Number: 008970
Test Date: 06/30/2026

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE

Analyst's Name: Gillstrap, Jeffrey L
Permit Number: 0006-2446
Effective:
03/01/2026-03/01/2028

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG602101
Exp Date: 01/21/2028

Test	g/210L	Time
DIAG	Pass	8:33pm
AIR BLK	.00	8:34pm
ACCY CHK	.07	8:35pm
AIR BLK	.00	8:36pm
SUB TEST	**.00**	**8:36pm**
AIR BLK	.00	8:37pm
SUB TEST	**.00**	**8:39pm**
AIR BLK	.00	8:39pm

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

BUNCOMBE COUNTY BAT MOBILE UNIT 11 100

Serial Number: *008970* Test Record Number: *1478*
Test Date: *06/30/2026* Test Time: *8:42pm EDT*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	8:42pm
FLO	Pass	8:42pm
FC	Pass	8:42pm

Temperature Tests

Test	Status	Time
FC1	Pass	8:43pm
SRC	Pass	8:43pm
DET	Pass	8:43pm
BAR	Pass	8:43pm
BT	Pass	8:43pm

Blank Tests

Test	Status	Time
AIR	Pass	8:43pm

Printer Tests

Test	Status	Time
PRNT	Pass	8:43pm

CRC Tests

Test	Status	Time
COMP	Pass	8:43pm
CAL	Pass	8:43pm

Preventive Maintenance
Status: Pass

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Buncombe Instrument Location BAT Mobile Unit II

Instrument Serial No. 008973

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

(1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;

(2) Verify instrument displays time and date;

(3) Initiate breath test sequence;

(4) Enter information as prompted;

(5) Verify instrument accuracy;

(6) When "PLEASE BLOW" appears, collect breath sample;

(7) When "PLEASE BLOW" appears, collect breath sample;

(8) Print test record;

(9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and

(10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 10th day of June, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.

Signature of Certifying Official

062446
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

DHHS 4080 (04/20)

Intox EC/IR-II: Subject Test

BUNCOMBE COUNTY BAT MOBILE UNIT 11 100

Serial Number: *008973*
Test Date: *06/10/2026*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name: *Gillstrap, Jeffrey L*
Permit Number: *0006-2446*
Effective:
03/01/2026-03/01/2028

Officer's Name: *NONE, NONE*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG431003
Exp Date: 11/05/2026

Test	g/210L	Time
DIAG	Pass	8:27pm
AIR BLK	.00	8:28pm
ACCY CHK	.07	8:28pm
AIR BLK	.00	8:29pm
SUB TEST	**.00**	**8:30pm**
AIR BLK	.00	8:31pm
SUB TEST	**.00**	**8:32pm**
AIR BLK	.00	8:33pm

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

BUNCOMBE COUNTY BAT MOBILE UNIT 11 100

Serial Number: *008973* Test Record Number: *1498*
Test Date: *06/10/2026* Test Time: *8:34pm EDT*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	8:34pm
FLO	Pass	8:34pm
FC	Pass	8:34pm

Temperature Tests

Test	Status	Time
FC1	Pass	8:34pm
SRC	Pass	8:34pm
DET	Pass	8:34pm
BAR	Pass	8:34pm
BT	Pass	8:34pm

Blank Tests

Test	Status	Time
AIR	Pass	8:35pm

Printer Tests

Test	Status	Time
PRNT	Pass	8:35pm

CRC Tests

Test	Status	Time
COMP	Pass	8:35pm
CAL	Pass	8:35pm

Preventive Maintenance
Status: Pass



Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Buncombe Instrument Location BAT Mobile Unit II

Instrument Serial No. 008973

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

(1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;

(2) Verify instrument displays time and date;

(3) Initiate breath test sequence;

(4) Enter information as prompted;

(5) Verify instrument accuracy;

(6) When "PLEASE BLOW" appears, collect breath sample;

(7) When "PLEASE BLOW" appears, collect breath sample;

(8) Print test record;

(9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and

(10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 29th day of June, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.

Signature of Certifying Official

062446
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

DHHS 4080 (04/20)

Intox EC/IR-II: Subject Test

BUNCOMBE COUNTY BAT MOBILE UNIT 11 100

Serial Number: *008973*
Test Date: *06/29/2026*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name: *Gillstrap, Jeffrey L*
Permit Number: *0006-2446*
Effective:
03/01/2026-03/01/2028

Officer's Name: *NONE, NONE*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG431003
Exp Date: 11/05/2026

Test	g/210L	Time
DIAG	Pass	8:37pm
AIR BLK	.00	8:38pm
ACCY CHK	.07	8:38pm
AIR BLK	.00	8:39pm
SUB TEST	**.00**	**8:40pm**
AIR BLK	.00	8:41pm
SUB TEST	**.00**	**8:42pm**
AIR BLK	.00	8:43pm

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

BUNCOMBE COUNTY BAT MOBILE UNIT 11 100

Serial Number: *008973* Test Record Number: *1512*
Test Date: *06/29/2026* Test Time: *8:45pm EDT*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	8:45pm
FLO	Pass	8:45pm
FC	Pass	8:45pm

Temperature Tests

Test	Status	Time
FC1	Pass	8:45pm
SRC	Pass	8:45pm
DET	Pass	8:45pm
BAR	Pass	8:45pm
BT	Pass	8:45pm

Blank Tests

Test	Status	Time
AIR	Pass	8:46pm


Printer Tests

Test	Status	Time
PRNT	Pass	8:46pm

CRC Tests

Test	Status	Time
COMP	Pass	8:46pm
CAL	Pass	8:46pm

Preventive Maintenance
Status: Pass

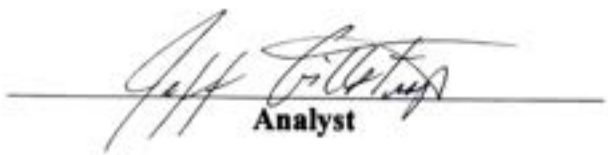

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Buncombe Instrument Location BAT Mobile Unit #11

Instrument Serial No. 008973

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

(1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;

(2) Verify instrument displays time and date;

(3) Initiate breath test sequence;

(4) Enter information as prompted;

(5) Verify instrument accuracy;

(6) When "PLEASE BLOW" appears, collect breath sample;

(7) When "PLEASE BLOW" appears, collect breath sample;

(8) Print test record;

(9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and

(10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 30th day of June, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.

Signature of Certifying Official

062446
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

DHHS 4080 (04/20)

BUNCOMBE COUNTY BAT MOBILE UNIT 11 100

Serial Number: *008973*
Test Date: *06/30/2026*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name: *Gillstrap, Jeffrey L*
Permit Number: *0006-2446*
Effective:
03/01/2026-03/01/2028

Officer's Name: *NONE, NONE*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG431003
Exp Date: 11/05/2026

Test	g/210L	Time
DIAG	Pass	8:30pm
AIR BLK	.00	8:31pm
ACCY CHK	.07	8:32pm
AIR BLK	.00	8:33pm
SUB TEST	**.00**	**8:33pm**
AIR BLK	.00	8:34pm
SUB TEST	**.00**	**8:36pm**
AIR BLK	.00	8:36pm

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

BUNCOMBE COUNTY BAT MOBILE UNIT 11 100

Serial Number: *008973* Test Record Number: *1516*
Test Date: *06/30/2026* Test Time: *8:39pm EDT*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	8:39pm
FLO	Pass	8:39pm
FC	Pass	8:39pm

Temperature Tests

Test	Status	Time
FC1	Pass	8:39pm
SRC	Pass	8:39pm
DET	Pass	8:39pm
BAR	Pass	8:39pm
BT	Pass	8:39pm

Blank Tests

Test	Status	Time
AIR	Pass	8:40pm

Printer Tests

Test	Status	Time
PRNT	Pass	8:40pm

CRC Tests

Test	Status	Time
COMP	Pass	8:40pm
CAL	Pass	8:40pm

Preventive Maintenance
Status: Pass



Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Buncombe Instrument Location BAT Mobile Unit II

Instrument Serial No. 008973

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

(1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;

(2) Verify instrument displays time and date;

(3) Initiate breath test sequence;

(4) Enter information as prompted;

(5) Verify instrument accuracy;

(6) When "PLEASE BLOW" appears, collect breath sample;

(7) When "PLEASE BLOW" appears, collect breath sample;

(8) Print test record;

(9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and

(10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 30th day of June, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.

Signature of Certifying Official

062446
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

DHHS 4080 (04/20)

Intox EC/IR-II: Subject Test

BUNCOMBE COUNTY BAT MOBILE UNIT 11 100

Serial Number: *008973*
Test Date: *06/30/2026*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name: *Gillstrap, Jeffrey L*
Permit Number: *0006-2446*
Effective:
03/01/2026-03/01/2028

Officer's Name: *NONE, NONE*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG431003
Exp Date: 11/05/2026

Test	g/210L	Time
DIAG	Pass	12:00am
AIR BLK	.00	12:01am
ACCY CHK	.07	12:01am
AIR BLK	.00	12:02am
SUB TEST	**.00**	**12:03am**
AIR BLK	.00	12:04am
SUB TEST	**.00**	**12:05am**
AIR BLK	.00	12:06am

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

BUNCOMBE COUNTY BAT MOBILE UNIT 11 100

Serial Number: *008973* Test Record Number: *1514*
Test Date: *06/30/2026* Test Time: *12:07am EDT*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	12:07am
FLO	Pass	12:07am
FC	Pass	12:07am

Temperature Tests

Test	Status	Time
FC1	Pass	12:07am
SRC	Pass	12:07am
DET	Pass	12:07am
BAR	Pass	12:07am
BT	Pass	12:07am

Blank Tests

Test	Status	Time
AIR	Pass	12:08am

Printer Tests

Test	Status	Time
PRNT	Pass	12:08am

CRC Tests

Test	Status	Time
COMP	Pass	12:08am
CAL	Pass	12:08am

Preventive Maintenance
Status: Pass



Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Cabarrus Instrument Location BAT Mobile Unit 8

Instrument Serial No. 008615

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

(1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;

(2) Verify instrument displays time and date;

(3) Initiate breath test sequence;

(4) Enter information as prompted;

(5) Verify instrument accuracy;

(6) When "PLEASE BLOW" appears, collect breath sample;

(7) When "PLEASE BLOW" appears, collect breath sample;

(8) Print test record;

(9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and

(10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 4 day of June, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.

Signature of Certifying Official

2219283
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

DHHS 4080 (04/20)

Intox EC/IR-II: Subject Test

CABARRUS COUNTY BAT MOBILE UNIT 8 120

Serial Number: *008615*
Test Date: *06/04/2026*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name: *Glasscock, Jerry D*
Permit Number: *7180-9235*
Effective:
02/01/2026-02/01/2028

Officer's Name: *NONE, NONE*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG506303
Exp Date: 03/04/2027

Test	g/210L	Time
DIAG	Pass	7:37pm
AIR BLK	.00	7:38pm
ACCY CHK	.07	7:38pm
AIR BLK	.00	7:39pm
SUB TEST	**.00**	**7:40pm**
AIR BLK	.00	7:41pm
SUB TEST	**.00**	**7:42pm**
AIR BLK	.00	7:43pm

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

CABARRUS COUNTY BAT MOBILE UNIT 8 120

Serial Number: *008615* Test Record Number: *6328*
Test Date: *06/04/2026* Test Time: *7:44pm EDT*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	7:44pm
FLO	Pass	7:44pm
FC	Pass	7:44pm

Temperature Tests

Test	Status	Time
FC1	Pass	7:45pm
SRC	Pass	7:45pm
DET	Pass	7:45pm
BAR	Pass	7:45pm
BT	Pass	7:45pm

Blank Tests

Test	Status	Time
AIR	Pass	7:45pm

Printer Tests

Test	Status	Time
PRNT	Pass	7:45pm

CRC Tests

Test	Status	Time
COMP	Pass	7:45pm
CAL	Pass	7:45pm

Preventive Maintenance
Status: Pass

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Cabarrus Instrument Location BAT Mobile Unit 8

Instrument Serial No. 008615

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

(1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;

(2) Verify instrument displays time and date;

(3) Initiate breath test sequence;

(4) Enter information as prompted;

(5) Verify instrument accuracy;

(6) When "PLEASE BLOW" appears, collect breath sample;

(7) When "PLEASE BLOW" appears, collect breath sample;

(8) Print test record;

(9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and

(10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 13 day of June, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.

Signature of Certifying Official

2219283
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

DHHS 4080 (04/20)

Intox EC/IR-II: Subject Test

CABARRUS COUNTY BAT MOBILE UNIT 8 120

Serial Number: *008615*
Test Date: *06/13/2026*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name: *Glasscock, Jerry D*
Permit Number: *7180-9235*
Effective:
02/01/2026-02/01/2028

Officer's Name: *NONE, NONE*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG506303
Exp Date: 03/04/2027

Test	g/210L	Time
DIAG	Pass	6:22pm
AIR BLK	.00	6:23pm
ACCY CHK	.07	6:23pm
AIR BLK	.00	6:24pm
SUB TEST	**.00**	**6:26pm**
AIR BLK	.00	6:26pm
SUB TEST	**.00**	**6:28pm**
AIR BLK	.00	6:29pm

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

CABARRUS COUNTY BAT MOBILE UNIT 8 120

Serial Number: *008615* Test Record Number: *6338*
Test Date: *06/13/2026* Test Time: *6:29pm EDT*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	6:29pm
FLO	Pass	6:29pm
FC	Pass	6:29pm

Temperature Tests

Test	Status	Time
FC1	Pass	6:30pm
SRC	Pass	6:30pm
DET	Pass	6:30pm
BAR	Pass	6:30pm
BT	Pass	6:30pm

Blank Tests

Test	Status	Time
AIR	Pass	6:30pm

Printer Tests

Test	Status	Time
PRNT	Pass	6:30pm

CRC Tests

Test	Status	Time
COMP	Pass	6:30pm
CAL	Pass	6:30pm

Preventive Maintenance
Status: Pass



Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Cabarrus Instrument Location BAT Mobile Unit 8

Instrument Serial No. 008615 —

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

(1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;

(2) Verify instrument displays time and date;

(3) Initiate breath test sequence;

(4) Enter information as prompted;

(5) Verify instrument accuracy;

(6) When "PLEASE BLOW" appears, collect breath sample;

(7) When "PLEASE BLOW" appears, collect breath sample;

(8) Print test record;

(9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and

(10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 25 day of June, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.

Signature of Certifying Official

2219283
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

DHHS 4080 (04/20)

Intox EC/IR-II: Subject Test

CABARRUS COUNTY BAT MOBILE UNIT 8 120

Serial Number: *008615*
Test Date: *06/25/2026*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name: *Glasscock, Jerry D*
Permit Number: *7180-9235*
Effective:
02/01/2026-02/01/2028

Officer's Name: *NONE, NONE*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG506303
Exp Date: 03/04/2027

Test	g/210L	Time
DIAG	Pass	7:39pm
AIR BLK	.00	7:40pm
ACCY CHK	.07	7:41pm
AIR BLK	.00	7:42pm
SUB TEST	**.00**	**7:42pm**
AIR BLK	.00	7:43pm
SUB TEST	**.00**	**7:45pm**
AIR BLK	.00	7:45pm

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

CABARRUS COUNTY BAT MOBILE UNIT 8 120

Serial Number: *008615* Test Record Number: *6351*
Test Date: *06/25/2026* Test Time: *7:46pm EDT*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	7:47pm
FLO	Pass	7:47pm
FC	Pass	7:47pm

Temperature Tests

Test	Status	Time
FC1	Pass	7:47pm
SRC	Pass	7:47pm
DET	Pass	7:47pm
BAR	Pass	7:47pm
BT	Pass	7:47pm

Blank Tests

Test	Status	Time
AIR	Pass	7:47pm

Printer Tests

Test	Status	Time
PRNT	Pass	7:48pm

CRC Tests

Test	Status	Time
COMP	Pass	7:48pm
CAL	Pass	7:48pm

Preventive Maintenance
Status: Pass

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Cabarrus Instrument Location Cabarrus County 80 Concord, NC

Instrument Serial No. 008625

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

(1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;

(2) Verify instrument displays time and date;

(3) Initiate breath test sequence;

(4) Enter information as prompted;

(5) Verify instrument accuracy;

(6) When "PLEASE BLOW" appears, collect breath sample;

(7) When "PLEASE BLOW" appears, collect breath sample;

(8) Print test record;

(9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and

(10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 17th day of June, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.

Signature of Certifying Official

849845
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

DHHS 4080 (04/20)

Intox EC/IR-II: Subject Test

CABARRUS COUNTY CABARRUS COUNTY SO 120

Serial Number: *008625*
Test Date: *06/17/2026*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name: *Helms, Bryce A*
Permit Number: *0084-9845*
Effective:
02/01/2026-02/01/2028

Officer's Name: *NONE, NONE*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG516203
Exp Date: 06/11/2027

Test	g/210L	Time
DIAG	Pass	11:58am
AIR BLK	.00	11:59am
ACCY CHK	.08	11:59am
AIR BLK	.00	12:00pm
SUB TEST	**.00**	**12:01pm**
AIR BLK	.00	12:02pm
SUB TEST	**.00**	**12:04pm**
AIR BLK	.00	12:05pm

Reported AC: .00 g/210L

Bryce Helms
Signature of Chemical Analyst

Court CVR

Bryce Helms
Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

CABARRUS COUNTY CABARRUS COUNTY SO 120

Serial Number: *008625* Test Record Number: *7456*
Test Date: *06/17/2026* Test Time: *12:07pm EDT*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	12:07pm
FLO	Pass	12:07pm
FC	Pass	12:07pm

Temperature Tests

Test	Status	Time
FC1	Pass	12:08pm
SRC	Pass	12:08pm
DET	Pass	12:08pm
BAR	Pass	12:08pm
BT	Pass	12:08pm

Blank Tests

Test	Status	Time
AIR	Pass	12:08pm


Printer Tests

Test	Status	Time
PRNT	Pass	12:08pm

CRC Tests

Test	Status	Time
COMP	Pass	12:08pm
CAL	Pass	12:08pm

Preventive Maintenance
Status: Pass

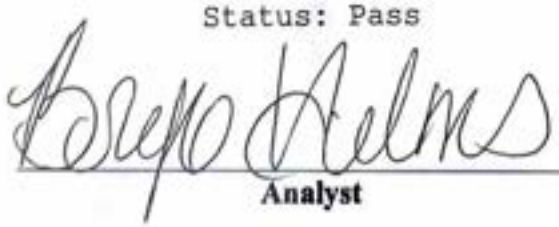

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Cabarrus Instrument Location Kannapolis PD

Instrument Serial No. 008702 Kannapolis, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

(1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;

(2) Verify instrument displays time and date;

(3) Initiate breath test sequence;

(4) Enter information as prompted;

(5) Verify instrument accuracy;

(6) When "PLEASE BLOW" appears, collect breath sample;

(7) When "PLEASE BLOW" appears, collect breath sample;

(8) Print test record;

(9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and

(10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 17th day of June, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.

Signature of Certifying Official

849845
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

DHHS 4080 (04/20)

Intox EC/IR-II: Subject Test

KANNAPOLIS PD CABARRUS COUNTY SO 120

Serial Number: *008702*
Test Date: *06/17/2026*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name: *Helms, Bryce A*
Permit Number: *0084-9845*
Effective:
02/01/2026-02/01/2028

Officer's Name: *NONE, NONE*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG602101
Exp Date: 01/21/2028

Test	g/210L	Time
DIAG	Pass	10:43am
AIR BLK	.00	10:44am
ACCY CHK	.08	10:44am
AIR BLK	.00	10:46am
SUB TEST	**.00**	**10:46am**
AIR BLK	.00	10:47am
SUB TEST	**.00**	**10:49am**
AIR BLK	.00	10:49am

Reported AC: .00 g/210L

Bryce Helms
Signature of Chemical Analyst

Court CVR

Bryce Helms
Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

KANNAPOLIS PD CABARRUS COUNTY SO 120

Serial Number: *008702* Test Record Number: *2437*
Test Date: *06/17/2026* Test Time: *10:50am EDT*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	10:50am
FLO	Pass	10:50am
FC	Pass	10:50am

Temperature Tests

Test	Status	Time
FC1	Pass	10:50am
SRC	Pass	10:50am
DET	Pass	10:50am
BAR	Pass	10:50am
BT	Pass	10:50am

Blank Tests

Test	Status	Time
AIR	Pass	10:51am


Printer Tests

Test	Status	Time
PRNT	Pass	10:51am

CRC Tests

Test	Status	Time
COMP	Pass	10:51am
CAL	Pass	10:51am

Preventive Maintenance
Status: Pass

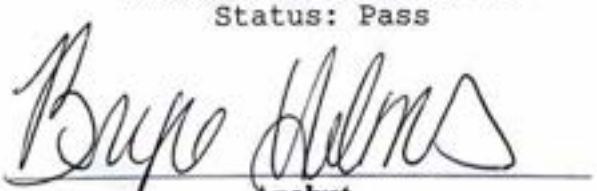

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Cabarrus Instrument Location BAT Mobile Unit 8

Instrument Serial No. 008736 –

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

(1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;

(2) Verify instrument displays time and date;

(3) Initiate breath test sequence;

(4) Enter information as prompted;

(5) Verify instrument accuracy;

(6) When "PLEASE BLOW" appears, collect breath sample;

(7) When "PLEASE BLOW" appears, collect breath sample;

(8) Print test record;

(9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and

(10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 4 day of June, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.

THE GREAT SEAL OF THE STATE OF NORTH CAROLINA

Signature of Certifying Official 2219283 Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

CABARRUS COUNTY BAT MOBILE UNIT 8 120

Serial Number: *008736*
Test Date: *06/04/2026*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name: *Glasscock, Jerry D*
Permit Number: *7180-9235*
Effective:
02/01/2026-02/01/2028

Officer's Name: *NONE, NONE*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG506303
Exp Date: 03/04/2027

Test	g/210L	Time
DIAG	Pass	7:35pm
AIR BLK	.00	7:36pm
ACCY CHK	.07	7:36pm
AIR BLK	.00	7:37pm
SUB TEST	**.00**	**7:38pm**
AIR BLK	.00	7:39pm
SUB TEST	**.00**	**7:40pm**
AIR BLK	.00	7:41pm

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

CABARRUS COUNTY BAT MOBILE UNIT 8 120

Serial Number: *008736* Test Record Number: *1684*
Test Date: *06/04/2026* Test Time: *7:42pm EDT*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	7:43pm
FLO	Pass	7:43pm
FC	Pass	7:43pm

Temperature Tests

Test	Status	Time
FC1	Pass	7:43pm
SRC	Pass	7:43pm
DET	Pass	7:43pm
BAR	Pass	7:43pm
BT	Pass	7:43pm

Blank Tests

Test	Status	Time
AIR	Pass	7:44pm

Printer Tests

Test	Status	Time
PRNT	Pass	7:44pm

CRC Tests

Test	Status	Time
COMP	Pass	7:44pm
CAL	Pass	7:44pm

Preventive Maintenance
Status: Pass



Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Cabarrus Instrument Location BAT Mobile Unit 8

Instrument Serial No. 008736 —

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

(1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;

(2) Verify instrument displays time and date;

(3) Initiate breath test sequence;

(4) Enter information as prompted;

(5) Verify instrument accuracy;

(6) When "PLEASE BLOW" appears, collect breath sample;

(7) When "PLEASE BLOW" appears, collect breath sample;

(8) Print test record;

(9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and

(10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 13 day of June, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.

Signature of Certifying Official

2219283
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

DHHS 4080 (04/20)

Intox EC/IR-II: Subject Test

CABARRUS COUNTY BAT MOBILE UNIT 8 120

Serial Number: *008736*
Test Date: *06/13/2026*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name: *Glasscock, Jerry D*
Permit Number: *7180-9235*
Effective:
02/01/2026-02/01/2028

Officer's Name: *NONE, NONE*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG506303
Exp Date: 03/04/2027

Test	g/210L	Time
DIAG	Pass	6:22pm
AIR BLK	.00	6:23pm
ACCY CHK	.07	6:23pm
AIR BLK	.00	6:24pm
SUB TEST	**.00**	**6:25pm**
AIR BLK	.00	6:26pm
SUB TEST	**.00**	**6:28pm**
AIR BLK	.00	6:29pm

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

CABARRUS COUNTY BAT MOBILE UNIT 8 120

Serial Number: *008736* Test Record Number: *1694*
Test Date: *06/13/2026* Test Time: *6:29pm EDT*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	6:29pm
FLO	Pass	6:29pm
FC	Pass	6:29pm

Temperature Tests

Test	Status	Time
FC1	Pass	6:29pm
SRC	Pass	6:29pm
DET	Pass	6:29pm
BAR	Pass	6:29pm
BT	Pass	6:29pm

Blank Tests

Test	Status	Time
AIR	Pass	6:30pm

Printer Tests

Test	Status	Time
PRNT	Pass	6:30pm

CRC Tests

Test	Status	Time
COMP	Pass	6:30pm
CAL	Pass	6:30pm

Preventive Maintenance
Status: Pass

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Cabarrus Instrument Location BAT Mobile Unit 8

Instrument Serial No. 008736 —

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

(1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;

(2) Verify instrument displays time and date;

(3) Initiate breath test sequence;

(4) Enter information as prompted;

(5) Verify instrument accuracy;

(6) When "PLEASE BLOW" appears, collect breath sample;

(7) When "PLEASE BLOW" appears, collect breath sample;

(8) Print test record;

(9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and

(10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 25 day of June, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.

Signature of Certifying Official

2219283
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

DHHS 4080 (04/20)

Intox EC/IR-II: Subject Test

CABARRUS COUNTY BAT MOBILE UNIT 8 120

Serial Number: *008736*
Test Date: *06/25/2026*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name: *Glasscock, Jerry D*
Permit Number: *7180-9235*
Effective:
02/01/2026-02/01/2028

Officer's Name: *NONE, NONE*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG506303
Exp Date: 03/04/2027

Test	g/210L	Time
DIAG	Pass	7:38pm
AIR BLK	.00	7:39pm
ACCY CHK	.07	7:40pm
AIR BLK	.00	7:41pm
SUB TEST	**.00**	**7:41pm**
AIR BLK	.00	7:42pm
SUB TEST	**.00**	**7:44pm**
AIR BLK	.00	7:44pm

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

CABARRUS COUNTY BAT MOBILE UNIT 8 120

Serial Number: *008736* Test Record Number: *1706*
Test Date: *06/25/2026* Test Time: *7:45pm EDT*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	7:45pm
FLO	Pass	7:45pm
FC	Pass	7:45pm

Temperature Tests

Test	Status	Time
FC1	Pass	7:46pm
SRC	Pass	7:46pm
DET	Pass	7:46pm
BAR	Pass	7:46pm
BT	Pass	7:46pm

Blank Tests

Test	Status	Time
AIR	Pass	7:46pm

Printer Tests

Test	Status	Time
PRNT	Pass	7:46pm

CRC Tests

Test	Status	Time
COMP	Pass	7:46pm
CAL	Pass	7:46pm

Preventive Maintenance
Status: Pass

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Cabarrus Instrument Location BAT Mobile Unit 8

Instrument Serial No. 008775 —

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

(1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;

(2) Verify instrument displays time and date;

(3) Initiate breath test sequence;

(4) Enter information as prompted;

(5) Verify instrument accuracy;

(6) When "PLEASE BLOW" appears, collect breath sample;

(7) When "PLEASE BLOW" appears, collect breath sample;

(8) Print test record;

(9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and

(10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 4 day of June, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.

Signature of Certifying Official

2219283
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

CABARRUS COUNTY BAT MOBILE UNIT 8 120

Serial Number: *008775*
Test Date: *06/04/2026*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name: *Glasscock, Jerry D*
Permit Number: *7180-9235*
Effective:
02/01/2026-02/01/2028

Officer's Name: *NONE, NONE*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG506303
Exp Date: 03/04/2027

Test	g/210L	Time
DIAG	Pass	7:35pm
AIR BLK	.00	7:36pm
ACCY CHK	.08	7:37pm
AIR BLK	.00	7:38pm
SUB TEST	**.00**	**7:38pm**
AIR BLK	.00	7:39pm
SUB TEST	**.00**	**7:41pm**
AIR BLK	.00	7:41pm

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

CABARRUS COUNTY BAT MOBILE UNIT 8 120

Serial Number: *008775* Test Record Number: *2534*
Test Date: *06/04/2026* Test Time: *7:42pm EDT*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	7:43pm
FLO	Pass	7:43pm
FC	Pass	7:43pm

Temperature Tests

Test	Status	Time
FC1	Pass	7:43pm
SRC	Pass	7:43pm
DET	Pass	7:43pm
BAR	Pass	7:43pm
BT	Pass	7:43pm

Blank Tests

Test	Status	Time
AIR	Pass	7:43pm

Printer Tests

Test	Status	Time
PRNT	Pass	7:43pm

CRC Tests

Test	Status	Time
COMP	Pass	7:44pm
CAL	Pass	7:44pm

Preventive Maintenance
Status: Pass

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Cabarrus Instrument Location BAT Mobile Unit 8

Instrument Serial No. 008775 –

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

(1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;

(2) Verify instrument displays time and date;

(3) Initiate breath test sequence;

(4) Enter information as prompted;

(5) Verify instrument accuracy;

(6) When "PLEASE BLOW" appears, collect breath sample;

(7) When "PLEASE BLOW" appears, collect breath sample;

(8) Print test record;

(9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and

(10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 13 day of June, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.

THE GREAT SEAL OF THE STATE OF NORTH CAROLINA

Signature of Certifying Official

2219283
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

CABARRUS COUNTY BAT MOBILE UNIT 8 120

Serial Number: *008775*
Test Date: *06/13/2026*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name: *Glasscock, Jerry D*
Permit Number: *7180-9235*
Effective:
02/01/2026-02/01/2028

Officer's Name: *NONE, NONE*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG506303
Exp Date: 03/04/2027

Test	g/210L	Time
DIAG	Pass	6:22pm
AIR BLK	.00	6:23pm
ACCY CHK	.08	6:24pm
AIR BLK	.00	6:25pm
SUB TEST	**.00**	**6:26pm**
AIR BLK	.00	6:26pm
SUB TEST	**.00**	**6:28pm**
AIR BLK	.00	6:29pm

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

CABARRUS COUNTY BAT MOBILE UNIT 8 120

Serial Number: *008775* Test Record Number: *2545*
Test Date: *06/13/2026* Test Time: *6:29pm EDT*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	6:29pm
FLO	Pass	6:29pm
FC	Pass	6:30pm

Temperature Tests

Test	Status	Time
FC1	Pass	6:30pm
SRC	Pass	6:30pm
DET	Pass	6:30pm
BAR	Pass	6:30pm
BT	Pass	6:30pm

Blank Tests

Test	Status	Time
AIR	Pass	6:30pm

Printer Tests

Test	Status	Time
PRNT	Pass	6:30pm

CRC Tests

Test	Status	Time
COMP	Pass	6:31pm
CAL	Pass	6:31pm

Preventive Maintenance
Status: Pass



Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Cabarrus Instrument Location BAT Mobile Unit 8

Instrument Serial No. 008775 —

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

(1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;

(2) Verify instrument displays time and date;

(3) Initiate breath test sequence;

(4) Enter information as prompted;

(5) Verify instrument accuracy;

(6) When "PLEASE BLOW" appears, collect breath sample;

(7) When "PLEASE BLOW" appears, collect breath sample;

(8) Print test record;

(9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and

(10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 25 day of June, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.

Signature of Certifying Official 2219283 Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

CABARRUS COUNTY BAT MOBILE UNIT 8 120

Serial Number: *008775*
Test Date: *06/25/2026*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name: *Glasscock, Jerry D*
Permit Number: *7180-9235*
Effective:
02/01/2026-02/01/2028

Officer's Name: *NONE, NONE*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG506303
Exp Date: 03/04/2027

Test	g/210L	Time
DIAG	Pass	7:38pm
AIR BLK	.00	7:39pm
ACCY CHK	.08	7:39pm
AIR BLK	.00	7:40pm
SUB TEST	**.00**	**7:41pm**
AIR BLK	.00	7:42pm
SUB TEST	**.00**	**7:44pm**
AIR BLK	.00	7:44pm

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

CABARRUS COUNTY BAT MOBILE UNIT 8 120

Serial Number: *008775* Test Record Number: *2564*
Test Date: *06/25/2026* Test Time: *7:45pm EDT*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	7:45pm
FLO	Pass	7:45pm
FC	Pass	7:45pm

Temperature Tests

Test	Status	Time
FC1	Pass	7:45pm
SRC	Pass	7:45pm
DET	Pass	7:45pm
BAR	Pass	7:45pm
BT	Pass	7:45pm

Blank Tests

Test	Status	Time
AIR	Pass	7:46pm

Printer Tests

Test	Status	Time
PRNT	Pass	7:46pm

CRC Tests

Test	Status	Time
COMP	Pass	7:46pm
CAL	Pass	7:46pm

Preventive Maintenance
Status: Pass



Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Cabarrus Instrument Location BAT Mobile Unit 8

Instrument Serial No. 008816 –

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

(1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;

(2) Verify instrument displays time and date;

(3) Initiate breath test sequence;

(4) Enter information as prompted;

(5) Verify instrument accuracy;

(6) When "PLEASE BLOW" appears, collect breath sample;

(7) When "PLEASE BLOW" appears, collect breath sample;

(8) Print test record;

(9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and

(10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 4 day of June, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.

THE GREAT SEAL OF THE STATE OF NORTH CAROLINA

Signature of Certifying Official

2219283
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

CABARRUS COUNTY BAT MOBILE UNIT 8 120

Serial Number: *008816*
Test Date: *06/04/2026*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name: *Glasscock, Jerry D*
Permit Number: *7180-9235*
Effective:
02/01/2026-02/01/2028

Officer's Name: *NONE, NONE*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG431002
Exp Date: 11/05/2026

Test	g/210L	Time
DIAG	Pass	7:38pm
AIR BLK	.00	7:39pm
ACCY CHK	.07	7:39pm
AIR BLK	.00	7:40pm
SUB TEST	**.00**	**7:41pm**
AIR BLK	.00	7:42pm
SUB TEST	**.00**	**7:43pm**
AIR BLK	.00	7:44pm

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

CABARRUS COUNTY BAT MOBILE UNIT 8 120

Serial Number: *008816* Test Record Number: *8113*
Test Date: *06/04/2026* Test Time: *7:44pm EDT*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	7:45pm
FLO	Pass	7:45pm
FC	Pass	7:45pm

Temperature Tests

Test	Status	Time
FC1	Pass	7:45pm
SRC	Pass	7:45pm
DET	Pass	7:45pm
BAR	Pass	7:45pm
BT	Pass	7:45pm

Blank Tests

Test	Status	Time
AIR	Pass	7:45pm

Printer Tests

Test	Status	Time
PRNT	Pass	7:45pm

CRC Tests

Test	Status	Time
COMP	Pass	7:46pm
CAL	Pass	7:46pm

Preventive Maintenance
Status: Pass

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Cabarrus Instrument Location BAT Mobile Unit 8

Instrument Serial No. 008816 —

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

(1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;

(2) Verify instrument displays time and date;

(3) Initiate breath test sequence;

(4) Enter information as prompted;

(5) Verify instrument accuracy;

(6) When "PLEASE BLOW" appears, collect breath sample;

(7) When "PLEASE BLOW" appears, collect breath sample;

(8) Print test record;

(9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and

(10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 13 day of June, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.

Signature of Certifying Official

2219283
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

DHHS 4080 (04/20)

Intox EC/IR-II: Subject Test

CABARRUS COUNTY BAT MOBILE UNIT 8 120

Serial Number: *008816*
Test Date: *06/13/2026*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name: *Glasscock, Jerry D*
Permit Number: *7180-9235*
Effective:
02/01/2026-02/01/2028

Officer's Name: *NONE, NONE*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG431002
Exp Date: 11/05/2026

Test	g/210L	Time
DIAG	Pass	6:23pm
AIR BLK	.00	6:24pm
ACCY CHK	.07	6:25pm
AIR BLK	.00	6:26pm
SUB TEST	**.00**	**6:26pm**
AIR BLK	.00	6:27pm
SUB TEST	**.00**	**6:29pm**
AIR BLK	.00	6:30pm

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

CABARRUS COUNTY BAT MOBILE UNIT 8 120

Serial Number: *008816* Test Record Number: *8123*
Test Date: *06/13/2026* Test Time: *6:30pm EDT*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	6:30pm
FLO	Pass	6:30pm
FC	Pass	6:30pm

Temperature Tests

Test	Status	Time
FC1	Pass	6:30pm
SRC	Pass	6:30pm
DET	Pass	6:30pm
BAR	Pass	6:30pm
BT	Pass	6:30pm

Blank Tests

Test	Status	Time
AIR	Pass	6:31pm

Printer Tests

Test	Status	Time
PRNT	Pass	6:31pm

CRC Tests

Test	Status	Time
COMP	Pass	6:31pm
CAL	Pass	6:31pm

Preventive Maintenance
Status: Pass

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Cabarrus Instrument Location BAT Mobile Unit 8

Instrument Serial No. 008816 —

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

(1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;

(2) Verify instrument displays time and date;

(3) Initiate breath test sequence;

(4) Enter information as prompted;

(5) Verify instrument accuracy;

(6) When "PLEASE BLOW" appears, collect breath sample;

(7) When "PLEASE BLOW" appears, collect breath sample;

(8) Print test record;

(9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and

(10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 25 day of June, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.

Signature of Certifying Official

2219283
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

CABARRUS COUNTY BAT MOBILE UNIT 8 120

Serial Number: *008816*
Test Date: *06/25/2026*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name: *Glasscock, Jerry D*
Permit Number: *7180-9235*
Effective:
02/01/2026-02/01/2028

Officer's Name: *NONE, NONE*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG431002
Exp Date: 11/05/2026

Test	g/210L	Time
DIAG	Pass	7:37pm
AIR BLK	.00	7:38pm
ACCY CHK	.07	7:39pm
AIR BLK	.00	7:40pm
SUB TEST	**.00**	**7:41pm**
AIR BLK	.00	7:42pm
SUB TEST	**.00**	**7:44pm**
AIR BLK	.00	7:45pm

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

CABARRUS COUNTY BAT MOBILE UNIT 8 120

Serial Number: *008816* Test Record Number: *8136*
Test Date: *06/25/2026* Test Time: *7:45pm EDT*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	7:46pm
FLO	Pass	7:46pm
FC	Pass	7:46pm

Temperature Tests

Test	Status	Time
FC1	Pass	7:46pm
SRC	Pass	7:46pm
DET	Pass	7:46pm
BAR	Pass	7:46pm
BT	Pass	7:46pm

Blank Tests

Test	Status	Time
AIR	Pass	7:46pm

Printer Tests

Test	Status	Time
PRNT	Pass	7:46pm

CRC Tests

Test	Status	Time
COMP	Pass	7:47pm
CAL	Pass	7:47pm

Preventive Maintenance
Status: Pass

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Cabarrus Instrument Location BAT Mobile Unit 8

Instrument Serial No. 008929 —

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

(1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;

(2) Verify instrument displays time and date;

(3) Initiate breath test sequence;

(4) Enter information as prompted;

(5) Verify instrument accuracy;

(6) When "PLEASE BLOW" appears, collect breath sample;

(7) When "PLEASE BLOW" appears, collect breath sample;

(8) Print test record;

(9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and

(10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 4 day of June, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.

Signature of Certifying Official

2219283
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

CABARRUS COUNTY BAT MOBILE UNIT 8 120

Serial Number: *008929*
Test Date: *06/04/2026*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name: *Glasscock, Jerry D*
Permit Number: *7180-9235*
Effective:
02/01/2026-02/01/2028

Officer's Name: *NONE, NONE*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG506303
Exp Date: 03/04/2027

Test	g/210L	Time
DIAG	Pass	7:38pm
AIR BLK	.00	7:39pm
ACCY CHK	.07	7:40pm
AIR BLK	.00	7:41pm
SUB TEST	**.00**	**7:42pm**
AIR BLK	.00	7:43pm
SUB TEST	**.00**	**7:44pm**
AIR BLK	.00	7:45pm

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

CABARRUS COUNTY BAT MOBILE UNIT 8 120

Serial Number: *008929* Test Record Number: *1820*
Test Date: *06/04/2026* Test Time: *7:45pm EDT*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	7:46pm
FLO	Pass	7:46pm
FC	Pass	7:46pm

Temperature Tests

Test	Status	Time
FC1	Pass	7:46pm
SRC	Pass	7:46pm
DET	Pass	7:46pm
BAR	Pass	7:46pm
BT	Pass	7:46pm

Blank Tests

Test	Status	Time
AIR	Pass	7:47pm

Printer Tests

Test	Status	Time
PRNT	Pass	7:47pm

CRC Tests

Test	Status	Time
COMP	Pass	7:47pm
CAL	Pass	7:47pm

Preventive Maintenance
Status: Pass



Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Cabarrus Instrument Location BAT Mobile Unit 8

Instrument Serial No. 008929

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

(1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;

(2) Verify instrument displays time and date;

(3) Initiate breath test sequence;

(4) Enter information as prompted;

(5) Verify instrument accuracy;

(6) When "PLEASE BLOW" appears, collect breath sample;

(7) When "PLEASE BLOW" appears, collect breath sample;

(8) Print test record;

(9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and

(10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 13 day of June, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.

Signature of Certifying Official

2219283
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

DHHS 4080 (04/20)

Intox EC/IR-II: Subject Test

CABARRUS COUNTY BAT MOBILE UNIT 8 120

Serial Number: *008929*
Test Date: *06/13/2026*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name: *Glasscock, Jerry D*
Permit Number: *7180-9235*
Effective:
02/01/2026-02/01/2028

Officer's Name: *NONE, NONE*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG506303
Exp Date: 03/04/2027

Test	g/210L	Time
DIAG	Pass	6:23pm
AIR BLK	.00	6:25pm
ACCY CHK	.07	6:25pm
AIR BLK	.00	6:27pm
SUB TEST	**.00**	**6:27pm**
AIR BLK	.00	6:28pm
SUB TEST	**.00**	**6:30pm**
AIR BLK	.00	6:31pm

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

CABARRUS COUNTY BAT MOBILE UNIT 8 120

Serial Number: *008929* Test Record Number: *1830*
Test Date: *06/13/2026* Test Time: *6:32pm EDT*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	6:33pm
FLO	Pass	6:33pm
FC	Pass	6:33pm

Temperature Tests

Test	Status	Time
FC1	Pass	6:33pm
SRC	Pass	6:33pm
DET	Pass	6:33pm
BAR	Pass	6:33pm
BT	Pass	6:33pm

Blank Tests

Test	Status	Time
AIR	Pass	6:34pm

Printer Tests

Test	Status	Time
PRNT	Pass	6:34pm

CRC Tests

Test	Status	Time
COMP	Pass	6:34pm
CAL	Pass	6:34pm

Preventive Maintenance
Status: Pass



Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Cabarrus Instrument Location BAT Mobile Unit 8

Instrument Serial No. 008929 —

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

(1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;

(2) Verify instrument displays time and date;

(3) Initiate breath test sequence;

(4) Enter information as prompted;

(5) Verify instrument accuracy;

(6) When "PLEASE BLOW" appears, collect breath sample;

(7) When "PLEASE BLOW" appears, collect breath sample;

(8) Print test record;

(9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and

(10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 25 day of June, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.

THE GREAT SEAL OF THE STATE OF NORTH CAROLINA

Signature of Certifying Official

2219283
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

CABARRUS COUNTY BAT MOBILE UNIT 8 120

Serial Number: *008929*
Test Date: *06/25/2026*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name: *Glasscock, Jerry D*
Permit Number: *7180-9235*
Effective:
02/01/2026-02/01/2028

Officer's Name: *NONE, NONE*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG506303
Exp Date: 03/04/2027

Test	g/210L	Time
DIAG	Pass	7:36pm
AIR BLK	.00	7:37pm
ACCY CHK	.08	7:38pm
AIR BLK	.00	7:39pm
SUB TEST	**.00**	**7:40pm**
AIR BLK	.00	7:41pm
SUB TEST	**.00**	**7:43pm**
AIR BLK	.00	7:44pm

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

CABARRUS COUNTY BAT MOBILE UNIT 8 120

Serial Number: *008929* Test Record Number: *1845*
Test Date: *06/25/2026* Test Time: *7:44pm EDT*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	7:45pm
FLO	Pass	7:45pm
FC	Pass	7:45pm

Temperature Tests

Test	Status	Time
FC1	Pass	7:45pm
SRC	Pass	7:45pm
DET	Pass	7:45pm
BAR	Pass	7:45pm
BT	Pass	7:45pm

Blank Tests

Test	Status	Time
AIR	Pass	7:46pm

Printer Tests

Test	Status	Time
PRNT	Pass	7:46pm

CRC Tests

Test	Status	Time
COMP	Pass	7:46pm
CAL	Pass	7:46pm

Preventive Maintenance
Status: Pass



Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Caldwell Instrument Location BAT Mobile Unit II

Instrument Serial No. 008970

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

(1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;

(2) Verify instrument displays time and date;

(3) Initiate breath test sequence;

(4) Enter information as prompted;

(5) Verify instrument accuracy;

(6) When "PLEASE BLOW" appears, collect breath sample;

(7) When "PLEASE BLOW" appears, collect breath sample;

(8) Print test record;

(9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and

(10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 6th day of June, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.

Signature of Certifying Official

062446
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

DHHS 4080 (04/20)

Intox EC/IR-II: Subject Test

CALDWELL COUNTY BAT MOBILE UNIT 11 130

Serial Number: *008970*
Test Date: *06/06/2026*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name: *Gillstrap, Jeffrey L*
Permit Number: *0006-2446*
Effective:
03/01/2026-03/01/2028

Officer's Name: *NONE, NONE*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG417802
Exp Date: 06/26/2026

Test	g/210L	Time
DIAG	Pass	6:24pm
AIR BLK	.00	6:24pm
ACCY CHK	.07	6:25pm
AIR BLK	.00	6:26pm
SUB TEST	**.00**	**6:26pm**
AIR BLK	.00	6:27pm
SUB TEST	**.00**	**6:29pm**
AIR BLK	.00	6:30pm

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

CALDWELL COUNTY BAT MOBILE UNIT 11 130

Serial Number: *008970* Test Record Number: *1454*
Test Date: *06/06/2026* Test Time: *6:31pm EDT*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	6:31pm
FLO	Pass	6:31pm
FC	Pass	6:31pm

Temperature Tests

Test	Status	Time
FC1	Pass	6:31pm
SRC	Pass	6:31pm
DET	Pass	6:31pm
BAR	Pass	6:31pm
BT	Pass	6:31pm

Blank Tests

Test	Status	Time
AIR	Pass	6:32pm


Printer Tests

Test	Status	Time
PRNT	Pass	6:32pm

CRC Tests

Test	Status	Time
COMP	Pass	6:32pm
CAL	Pass	6:32pm

Preventive Maintenance
Status: Pass

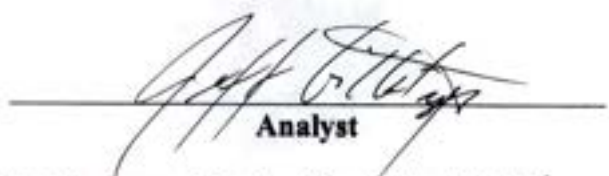

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Caldwell Instrument Location BAT Mobile Unit 11

Instrument Serial No. 008973

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

(1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;

(2) Verify instrument displays time and date;

(3) Initiate breath test sequence;

(4) Enter information as prompted;

(5) Verify instrument accuracy;

(6) When "PLEASE BLOW" appears, collect breath sample;

(7) When "PLEASE BLOW" appears, collect breath sample;

(8) Print test record;

(9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and

(10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 6th day of June, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.

Signature of Certifying Official

06 2446
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

DHHS 4080 (04/20)

Intox EC/IR-II: Subject Test

CALDWELL COUNTY BAT MOBILE UNIT 11 130

Serial Number: *008973*
Test Date: *06/06/2026*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name: *Gillstrap, Jeffrey L*
Permit Number: *0006-2446*
Effective:
03/01/2026-03/01/2028

Officer's Name: *NONE, NONE*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG431003
Exp Date: 11/05/2026

Test	g/210L	Time
DIAG	Pass	6:24pm
AIR BLK	.00	6:25pm
ACCY CHK	.07	6:25pm
AIR BLK	.00	6:27pm
SUB TEST	**.00**	**6:27pm**
AIR BLK	.00	6:28pm
SUB TEST	**.00**	**6:29pm**
AIR BLK	.00	6:30pm

Reported AC: .00 g/210L

Jeff Gillstrap
Signature of Chemical Analyst

Court CVR

Jeff Gillstrap
Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

CALDWELL COUNTY BAT MOBILE UNIT 11 130

Serial Number: *008973* Test Record Number: *1494*
Test Date: *06/06/2026* Test Time: *6:31pm EDT*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	6:31pm
FLO	Pass	6:31pm
FC	Pass	6:31pm

Temperature Tests

Test	Status	Time
FC1	Pass	6:31pm
SRC	Pass	6:31pm
DET	Pass	6:31pm
BAR	Pass	6:31pm
BT	Pass	6:31pm

Blank Tests

Test	Status	Time
AIR	Pass	6:32pm


Printer Tests

Test	Status	Time
PRNT	Pass	6:32pm

CRC Tests

Test	Status	Time
COMP	Pass	6:32pm
CAL	Pass	6:32pm

Preventive Maintenance
Status: Pass

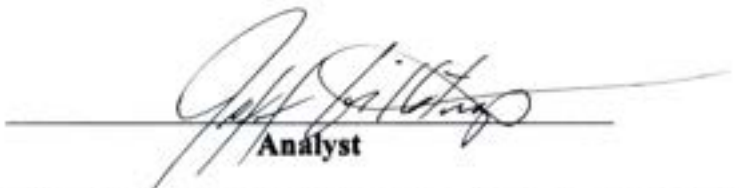

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Camden Instrument Location Camden Co. S.O.

Instrument Serial No. 008940 117 N. Carolina Hwy. 343 Camden, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

(1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;

(2) Verify instrument displays time and date;

(3) Initiate breath test sequence;

(4) Enter information as prompted;

(5) Verify instrument accuracy;

(6) When "PLEASE BLOW" appears, collect breath sample;

(7) When "PLEASE BLOW" appears, collect breath sample;

(8) Print test record;

(9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and

(10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 22nd day of June, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.

Mark A. Campbell
Signature of Certifying Official

206272
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

CAMDEN COUNTY CAMDEN CO SO 140

Serial Number: *008940*
Test Date: *06/22/2026*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name: *Chappell, Mark A*
Permit Number: *0020-6272*
Effective:
02/01/2026-02/01/2028

Officer's Name: *NONE, NONE*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG516203
Exp Date: 06/11/2027

Test	g/210L	Time
DIAG	Pass	11:30am
AIR BLK	.00	11:30am
ACCY CHK	.08	11:31am
AIR BLK	.00	11:32am
SUB TEST	**.00**	**11:33am**
AIR BLK	.00	11:33am
SUB TEST	**.00**	**11:35am**
AIR BLK	.00	11:36am

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

CAMDEN COUNTY CAMDEN CO SO 140

Serial Number: *008940* Test Record Number: *1398*
Test Date: *06/22/2026* Test Time: *11:36am EDT*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	11:37am
FLO	Pass	11:37am
FC	Pass	11:37am

Temperature Tests

Test	Status	Time
FC1	Pass	11:37am
SRC	Pass	11:37am
DET	Pass	11:37am
BAR	Pass	11:37am
BT	Pass	11:37am

Blank Tests

Test	Status	Time
AIR	Pass	11:37am

Printer Tests

Test	Status	Time
PRNT	Pass	11:38am

CRC Tests

Test	Status	Time
COMP	Pass	11:38am
CAL	Pass	11:38am

Preventive Maintenance
Status: Pass

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County CATAWBA Instrument Location CATAWBA COUNTY S.O.

Instrument Serial No. 008821 NEWTON NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

(1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;

(2) Verify instrument displays time and date;

(3) Initiate breath test sequence;

(4) Enter information as prompted;

(5) Verify instrument accuracy;

(6) When "PLEASE BLOW" appears, collect breath sample;

(7) When "PLEASE BLOW" appears, collect breath sample;

(8) Print test record;

(9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and

(10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 02 day of June, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.

Signature of Certifying Official

274970
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

DHHS 4080 (04/20)

Intox EC/IR-II: Subject Test

CATAWBA COUNTY CATAWBA COUNTY SO 170

Serial Number: *008821*
Test Date: *06/02/2026*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name: *Fleming, Tina S*
Permit Number: *0027-4970*
Effective:
02/01/2025-02/01/2027

Officer's Name: *NONE, NONE*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG516203
Exp Date: 06/11/2027

Test	g/210L	Time
DIAG	Pass	12:21pm
AIR BLK	.00	12:21pm
ACCY CHK	.07	12:22pm
AIR BLK	.00	12:23pm
SUB TEST	**.00**	**12:24pm**
AIR BLK	.00	12:25pm
SUB TEST	**.00**	**12:27pm**
AIR BLK	.00	12:28pm

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

CATAWBA COUNTY CATAWBA COUNTY SO 170

Serial Number: *008821* Test Record Number: *2791*
Test Date: *06/02/2026* Test Time: *12:28pm EDT*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	12:28pm
FLO	Pass	12:28pm
FC	Pass	12:29pm

Temperature Tests

Test	Status	Time
FC1	Pass	12:29pm
SRC	Pass	12:29pm
DET	Pass	12:29pm
BAR	Pass	12:29pm
BT	Pass	12:29pm

Blank Tests

Test	Status	Time
AIR	Pass	12:29pm

Printer Tests

Test	Status	Time
PRNT	Pass	12:29pm

CRC Tests

Test	Status	Time
COMP	Pass	12:29pm
CAL	Pass	12:29pm

Preventive Maintenance
Status: Pass

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Clay Instrument Location Clay County Jail

Instrument Serial No. 008608 Hayesville, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

(1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;

(2) Verify instrument displays time and date;

(3) Initiate breath test sequence;

(4) Enter information as prompted;

(5) Verify instrument accuracy;

(6) When "PLEASE BLOW" appears, collect breath sample;

(7) When "PLEASE BLOW" appears, collect breath sample;

(8) Print test record;

(9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and

(10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 8th day of June, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.

THE GREAT SEAL OF THE STATE OF NORTH CAROLINA

David R. Cuthrell
Signature of Certifying Official

843310
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

DHHS 4080 (04/20)

Intox EC/IR-II: Subject Test

CLAY COUNTY CLAY COUNTY JAIL 210

Serial Number: *008608*
Test Date: *06/08/2026*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name: *Cutler, Daniel R*
Permit Number: *0084-3310*
Effective:
02/01/2026-02/01/2028

Officer's Name: *NONE, NONE*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG534301
Exp Date: 12/09/2027

Test	g/210L	Time
DIAG	Pass	1:24pm
AIR BLK	.00	1:25pm
ACCY CHK	.07	1:25pm
AIR BLK	.00	1:26pm
SUB TEST	**.00**	**1:26pm**
AIR BLK	.00	1:27pm
SUB TEST	**.00**	**1:29pm**
AIR BLK	.00	1:30pm

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

CLAY COUNTY CLAY COUNTY JAIL 210

Serial Number: *008608* Test Record Number: *1684*
Test Date: *06/08/2026* Test Time: *1:30pm EDT*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	1:30pm
FLO	Pass	1:30pm
FC	Pass	1:31pm

Temperature Tests

Test	Status	Time
FC1	Pass	1:31pm
SRC	Pass	1:31pm
DET	Pass	1:31pm
BAR	Pass	1:31pm
BT	Pass	1:31pm

Blank Tests

Test	Status	Time
AIR	Pass	1:31pm

Printer Tests

Test	Status	Time
PRNT	Pass	1:31pm

CRC Tests

Test	Status	Time
COMP	Pass	1:32pm
CAL	Pass	1:32pm

Preventive Maintenance
Status: Pass

David R. Cuthbert

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Cumberland Instrument Location Hope Mills

Instrument Serial No. 008614 Police Department

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

(1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;

(2) Verify instrument displays time and date;

(3) Initiate breath test sequence;

(4) Enter information as prompted;

(5) Verify instrument accuracy;

(6) When "PLEASE BLOW" appears, collect breath sample;

(7) When "PLEASE BLOW" appears, collect breath sample;

(8) Print test record;

(9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and

(10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 3 day of June, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.

Signature of Certifying Official

365156
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

DHHS 4080 (04/20)

Intox EC/IR-II: Subject Test

CUMBERLAND COUNTY HOPE MILLS PD 250

Serial Number: *008614*
Test Date: *06/03/2026*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name: *Garner, Joel K*
Permit Number: *0036-5156*
Effective:
02/01/2026-02/01/2028

Officer's Name: *NONE, NONE*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG534301
Exp Date: 12/09/2027

Test	g/210L	Time
DIAG	Pass	12:31pm
AIR BLK	.00	12:32pm
ACCY CHK	.07	12:33pm
AIR BLK	.00	12:34pm
SUB TEST	**.00**	**12:34pm**
AIR BLK	.00	12:35pm
SUB TEST	**.00**	**12:37pm**
AIR BLK	.00	12:38pm

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

CUMBERLAND COUNTY HOPE MILLS PD 250

Serial Number: *008614* Test Record Number: *5281*
Test Date: *06/03/2026* Test Time: *12:38pm EDT*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	12:38pm
FLO	Pass	12:39pm
FC	Pass	12:39pm

Temperature Tests

Test	Status	Time
FC1	Pass	12:39pm
SRC	Pass	12:39pm
DET	Pass	12:39pm
BAR	Pass	12:39pm
BT	Pass	12:39pm

Blank Tests

Test	Status	Time
AIR	Pass	12:39pm

Printer Tests

Test	Status	Time
PRNT	Pass	12:39pm

CRC Tests

Test	Status	Time
COMP	Pass	12:40pm
CAL	Pass	12:40pm

Preventive Maintenance
Status: Pass



Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Cumberland Instrument Location Cumberland County Detention Center

Instrument Serial No. 008632

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

(1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;

(2) Verify instrument displays time and date;

(3) Initiate breath test sequence;

(4) Enter information as prompted;

(5) Verify instrument accuracy;

(6) When "PLEASE BLOW" appears, collect breath sample;

(7) When "PLEASE BLOW" appears, collect breath sample;

(8) Print test record;

(9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and

(10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 3 day of June, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.

Signature of Certifying Official

365156
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

CUMBERLAND COUNTY DETENTION CENTER 250

Serial Number: *008632*
Test Date: *06/03/2026*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name: *Garner, Joel K*
Permit Number: *0036-5156*
Effective:
02/01/2026-02/01/2028

Officer's Name: *NONE, NONE*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG534301
Exp Date: 12/09/2027

Test	g/210L	Time
DIAG	Pass	10:49am
AIR BLK	.00	10:50am
ACCY CHK	.07	10:50am
AIR BLK	.00	10:51am
SUB TEST	**.00**	**10:52am**
AIR BLK	.00	10:53am
SUB TEST	**.00**	**10:54am**
AIR BLK	.00	10:55am

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

CUMBERLAND COUNTY DETENTION CENTER 250

Serial Number: *008632* Test Record Number: *5084*
Test Date: *06/03/2026* Test Time: *10:56am EDT*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	10:56am
FLO	Pass	10:56am
FC	Pass	10:57am

Temperature Tests

Test	Status	Time
FC1	Pass	10:57am
SRC	Pass	10:57am
DET	Pass	10:57am
BAR	Pass	10:57am
BT	Pass	10:57am

Blank Tests

Test	Status	Time
AIR	Pass	10:57am

Printer Tests

Test	Status	Time
PRNT	Pass	10:57am

CRC Tests

Test	Status	Time
COMP	Pass	10:57am
CAL	Pass	10:57am

Preventive Maintenance
Status: Pass



Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Cumberland Instrument Location Cumberland County Detention Center

Instrument Serial No. 008633

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

(1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;

(2) Verify instrument displays time and date;

(3) Initiate breath test sequence;

(4) Enter information as prompted;

(5) Verify instrument accuracy;

(6) When "PLEASE BLOW" appears, collect breath sample;

(7) When "PLEASE BLOW" appears, collect breath sample;

(8) Print test record;

(9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and

(10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 3 day of June, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.

Signature of Certifying Official

365156
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

DHHS 4080 (04/20)

Intox EC/IR-II: Subject Test

CUMBERLAND COUNTY DETENTION CENTER 250

Serial Number: *008633*
Test Date: *06/03/2026*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name: *Garner, Joel K*
Permit Number: *0036-5156*
Effective:
02/01/2026-02/01/2028

Officer's Name: *NONE, NONE*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG534301
Exp Date: 12/09/2027

Test	g/210L	Time
DIAG	Pass	10:50am
AIR BLK	.00	10:51am
ACCY CHK	.07	10:52am
AIR BLK	.00	10:53am
SUB TEST	**.00**	**10:54am**
AIR BLK	.00	10:54am
SUB TEST	**.00**	**10:56am**
AIR BLK	.00	10:57am

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

CUMBERLAND COUNTY DETENTION CENTER 250

Serial Number: *008633* Test Record Number: *7583*
Test Date: *06/03/2026* Test Time: *10:57am EDT*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	10:58am
FLO	Pass	10:58am
FC	Pass	10:58am

Temperature Tests

Test	Status	Time
FC1	Pass	10:58am
SRC	Pass	10:58am
DET	Pass	10:58am
BAR	Pass	10:58am
BT	Pass	10:58am

Blank Tests

Test	Status	Time
AIR	Pass	10:59am

Printer Tests

Test	Status	Time
PRNT	Pass	10:59am

CRC Tests

Test	Status	Time
COMP	Pass	10:59am
CAL	Pass	10:59am

Preventive Maintenance
Status: Pass



Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Cumberland Instrument Location Cumberland County Detention Center

Instrument Serial No. 008672

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

(1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;

(2) Verify instrument displays time and date;

(3) Initiate breath test sequence;

(4) Enter information as prompted;

(5) Verify instrument accuracy;

(6) When "PLEASE BLOW" appears, collect breath sample;

(7) When "PLEASE BLOW" appears, collect breath sample;

(8) Print test record;

(9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and

(10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 3 day of June, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.

Signature of Certifying Official

365156
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

CUMBERLAND COUNTY DETENTION CENTER 250

Serial Number: *008672*
Test Date: *06/03/2026*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name: *Garner, Joel K*
Permit Number: *0036-5156*
Effective:
02/01/2026-02/01/2028

Officer's Name: *NONE, NONE*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG534301
Exp Date: 12/09/2027

Test	g/210L	Time
DIAG	Pass	10:51am
AIR BLK	.00	10:52am
ACCY CHK	.07	10:53am
AIR BLK	.00	10:54am
SUB TEST	**.00**	**10:55am**
AIR BLK	.00	10:55am
SUB TEST	**.00**	**10:57am**
AIR BLK	.00	10:58am

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

CUMBERLAND COUNTY DETENTION CENTER 250

Serial Number: *008672* Test Record Number: *9077*
Test Date: *06/03/2026* Test Time: *11:00am EDT*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	11:00am
FLO	Pass	11:00am
FC	Pass	11:00am

Temperature Tests

Test	Status	Time
FC1	Pass	11:00am
SRC	Pass	11:00am
DET	Pass	11:00am
BAR	Pass	11:00am
BT	Pass	11:00am

Blank Tests

Test	Status	Time
AIR	Pass	11:01am

Printer Tests

Test	Status	Time
PRNT	Pass	11:01am

CRC Tests

Test	Status	Time
COMP	Pass	11:01am
CAL	Pass	11:01am

Preventive Maintenance
Status: Pass



Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Currituck Instrument Location Currituck Co. S.O.

Instrument Serial No. 008947 407A. Maple Rd., Maple, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

(1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;

(2) Verify instrument displays time and date;

(3) Initiate breath test sequence;

(4) Enter information as prompted;

(5) Verify instrument accuracy;

(6) When "PLEASE BLOW" appears, collect breath sample;

(7) When "PLEASE BLOW" appears, collect breath sample;

(8) Print test record;

(9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and

(10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 22nd day of June, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.

Signature of Certifying Official

206272
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

DHHS 4080 (04/20)

Intox EC/IR-II: Subject Test

CURRITUCK COUNTY CURRITUCK SO-MAPLE 260

Serial Number: *008947*
Test Date: *06/22/2026*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name: *Chappell, Mark A*
Permit Number: *0020-6272*
Effective:
02/01/2026-02/01/2028

Officer's Name: *NONE, NONE*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG516203
Exp Date: 06/11/2027

Test	g/210L	Time
DIAG	Pass	9:19am
AIR BLK	.00	9:19am
ACCY CHK	.07	9:20am
AIR BLK	.00	9:21am
SUB TEST	**.00**	**9:22am**
AIR BLK	.00	9:23am
SUB TEST	**.00**	**9:24am**
AIR BLK	.00	9:25am

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

CURRITUCK COUNTY CURRITUCK SO-MAPLE 260

Serial Number: *008947* Test Record Number: *3825*
Test Date: *06/22/2026* Test Time: *9:26am EDT*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	9:26am
FLO	Pass	9:26am
FC	Pass	9:26am

Temperature Tests

Test	Status	Time
FC1	Pass	9:27am
SRC	Pass	9:27am
DET	Pass	9:27am
BAR	Pass	9:27am
BT	Pass	9:27am

Blank Tests

Test	Status	Time
AIR	Pass	9:27am

Printer Tests

Test	Status	Time
PRNT	Pass	9:27am

CRC Tests

Test	Status	Time
COMP	Pass	9:27am
CAL	Pass	9:27am

Preventive Maintenance
Status: Pass



Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County DARE Instrument Location BAT Mobile Unit 12

Instrument Serial No. 008601

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

(1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;

(2) Verify instrument displays time and date;

(3) Initiate breath test sequence;

(4) Enter information as prompted;

(5) Verify instrument accuracy;

(6) When "PLEASE BLOW" appears, collect breath sample;

(7) When "PLEASE BLOW" appears, collect breath sample;

(8) Print test record;

(9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and

(10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 23rd day of June, 20 26 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.

Signature of Certifying Official

83034
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

DHHS 4080 (04/20)

Intox EC/IR-II: Subject Test

DARE COUNTY BAT MOBILE UNIT 12 270

Serial Number: *008601*
Test Date: *06/23/2026*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name:
Crutchfield Jr., Marshall B
Permit Number: *0008-3034*
Effective:
03/01/2026-03/01/2028

Officer's Name: *NONE, NONE*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG501307
Exp Date: 01/13/2027

Test	g/210L	Time
DIAG	Pass	5:45pm
AIR BLK	.00	5:46pm
ACCY CHK	.07	5:46pm
AIR BLK	.00	5:47pm
SUB TEST	**.00**	**5:48pm**
AIR BLK	.00	5:49pm
SUB TEST	**.00**	**5:50pm**
AIR BLK	.00	5:51pm

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

DARE COUNTY BAT MOBILE UNIT 12 270

Serial Number: *008601* Test Record Number: *1952*
Test Date: *06/23/2026* Test Time: *5:52pm EDT*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	5:52pm
FLO	Pass	5:52pm
FC	Pass	5:52pm

Temperature Tests

Test	Status	Time
FC1	Pass	5:53pm
SRC	Pass	5:53pm
DET	Pass	5:53pm
BAR	Pass	5:53pm
BT	Pass	5:53pm

Blank Tests

Test	Status	Time
AIR	Pass	5:53pm


Printer Tests

Test	Status	Time
PRNT	Pass	5:53pm

CRC Tests

Test	Status	Time
COMP	Pass	5:53pm
CAL	Pass	5:53pm

Preventive Maintenance
Status: Pass



Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Dare Instrument Location BAT Mobile Unit 12

Instrument Serial No. 008698

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

(1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;

(2) Verify instrument displays time and date;

(3) Initiate breath test sequence;

(4) Enter information as prompted;

(5) Verify instrument accuracy;

(6) When "PLEASE BLOW" appears, collect breath sample;

(7) When "PLEASE BLOW" appears, collect breath sample;

(8) Print test record;

(9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and

(10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 23rd day of June, 20 26 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.

Signature of Certifying Official

83034
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

DARE COUNTY BAT MOBILE UNIT 12 270

Serial Number: *008698*
Test Date: *06/23/2026*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name:
Crutchfield Jr., Marshall B
Permit Number: *0008-3034*
Effective:
03/01/2026-03/01/2028

Officer's Name: *NONE, NONE*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG431002
Exp Date: 11/05/2026

Test	g/210L	Time
DIAG	Pass	5:45pm
AIR BLK	.00	5:46pm
ACCY CHK	.08	5:47pm
AIR BLK	.00	5:48pm
SUB TEST	**.00**	**5:48pm**
AIR BLK	.00	5:49pm
SUB TEST	**.00**	**5:51pm**
AIR BLK	.00	5:52pm

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

DARE COUNTY BAT MOBILE UNIT 12 270

Serial Number: *008698* Test Record Number: *2784*
Test Date: *06/23/2026* Test Time: *5:53pm EDT*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	5:53pm
FLO	Pass	5:53pm
FC	Pass	5:53pm

Temperature Tests

Test	Status	Time
FC1	Pass	5:53pm
SRC	Pass	5:53pm
DET	Pass	5:53pm
BAR	Pass	5:53pm
BT	Pass	5:53pm

Blank Tests

Test	Status	Time
AIR	Pass	5:54pm

Printer Tests

Test	Status	Time
PRNT	Pass	5:54pm

CRC Tests

Test	Status	Time
COMP	Pass	5:54pm
CAL	Pass	5:54pm

Preventive Maintenance
Status: Pass



Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County DARE Instrument Location BAT Mobile Unit 12

Instrument Serial No. 008788

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

(1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;

(2) Verify instrument displays time and date;

(3) Initiate breath test sequence;

(4) Enter information as prompted;

(5) Verify instrument accuracy;

(6) When "PLEASE BLOW" appears, collect breath sample;

(7) When "PLEASE BLOW" appears, collect breath sample;

(8) Print test record;

(9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and

(10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 23rd day of June, 20 26 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.

Signature of Certifying Official

83034
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

DARE COUNTY BAT MOBILE UNIT 12 270

Serial Number: *008788*
Test Date: *06/23/2026*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name:
Crutchfield Jr., Marshall B
Permit Number: *0008-3034*
Effective:
03/01/2026-03/01/2028

Officer's Name: *NONE, NONE*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG534301
Exp Date: 12/09/2027

Test	g/210L	Time
DIAG	Pass	6:08pm
AIR BLK	.00	6:09pm
ACCY CHK	.07	6:10pm
AIR BLK	.00	6:10pm
SUB TEST	**.00**	**6:11pm**
AIR BLK	.00	6:12pm
SUB TEST	**.00**	**6:14pm**
AIR BLK	.00	6:14pm

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

DARE COUNTY BAT MOBILE UNIT 12 270

Serial Number: *008788* Test Record Number: *2568*
Test Date: *06/23/2026* Test Time: *6:15pm EDT*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	6:15pm
FLO	Pass	6:15pm
FC	Pass	6:15pm

Temperature Tests

Test	Status	Time
FC1	Pass	6:15pm
SRC	Pass	6:15pm
DET	Pass	6:15pm
BAR	Pass	6:15pm
BT	Pass	6:15pm

Blank Tests

Test	Status	Time
AIR	Pass	6:16pm


Printer Tests

Test	Status	Time
PRNT	Pass	6:16pm

CRC Tests

Test	Status	Time
COMP	Pass	6:16pm
CAL	Pass	6:16pm

Preventive Maintenance
Status: Pass



Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Dare Instrument Location Kill Devil Hills P.D.

Instrument Serial No. 008844 102 Town Hall Dr., Kill Devil Hills, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

(1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;

(2) Verify instrument displays time and date;

(3) Initiate breath test sequence;

(4) Enter information as prompted;

(5) Verify instrument accuracy;

(6) When "PLEASE BLOW" appears, collect breath sample;

(7) When "PLEASE BLOW" appears, collect breath sample;

(8) Print test record;

(9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and

(10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 19th day of June, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.

Signature of Certifying Official

206272
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

DHHS 4080 (04/20)

Intox EC/IR-II: Subject Test

DARE COUNTY KILL DEVIL HILLS PD 270

Serial Number: *008844*
Test Date: *06/19/2026*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name: *Chappell, Mark A*
Permit Number: *0020-6272*
Effective:
02/01/2026-02/01/2028

Officer's Name: *NONE, NONE*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG516203
Exp Date: 06/11/2027

Test	g/210L	Time
DIAG	Pass	12:31pm
AIR BLK	.00	12:32pm
ACCY CHK	.08	12:32pm
AIR BLK	.00	12:33pm
SUB TEST	**.00**	**12:35pm**
AIR BLK	.00	12:36pm
SUB TEST	**.00**	**12:37pm**
AIR BLK	.00	12:38pm

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

DARE COUNTY KILL DEVIL HILLS PD 270

Serial Number: *008844* Test Record Number: *3434*
Test Date: *06/19/2026* Test Time: *12:39pm EDT*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	12:39pm
FLO	Pass	12:39pm
FC	Pass	12:40pm

Temperature Tests

Test	Status	Time
FC1	Pass	12:40pm
SRC	Pass	12:40pm
DET	Pass	12:40pm
BAR	Pass	12:40pm
BT	Pass	12:40pm

Blank Tests

Test	Status	Time
AIR	Pass	12:40pm


Printer Tests

Test	Status	Time
PRNT	Pass	12:40pm

CRC Tests

Test	Status	Time
COMP	Pass	12:40pm
CAL	Pass	12:40pm

Preventive Maintenance
Status: Pass

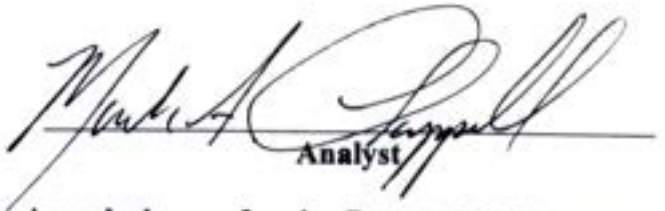

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Davidson Instrument Location BAT Mobile Unit 8

Instrument Serial No. 008615 –

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

(1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;

(2) Verify instrument displays time and date;

(3) Initiate breath test sequence;

(4) Enter information as prompted;

(5) Verify instrument accuracy;

(6) When "PLEASE BLOW" appears, collect breath sample;

(7) When "PLEASE BLOW" appears, collect breath sample;

(8) Print test record;

(9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and

(10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 13 day of June, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.

Signature of Certifying Official

2219283
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

DAVIDSON COUNTY BAT MOBILE UNIT 8 280

Serial Number: *008615*
Test Date: *06/13/2026*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name: *Glasscock, Jerry D*
Permit Number: *7180-9235*
Effective:
02/01/2026-02/01/2028

Officer's Name: *NONE, NONE*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG506303
Exp Date: 03/04/2027

Test	g/210L	Time
DIAG	Pass	12:27pm
AIR BLK	.00	12:28pm
ACCY CHK	.07	12:29pm
AIR BLK	.00	12:30pm
SUB TEST	**.00**	**12:30pm**
AIR BLK	.00	12:31pm
SUB TEST	**.00**	**12:33pm**
AIR BLK	.00	12:34pm

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

DAVIDSON COUNTY BAT MOBILE UNIT 8 280

Serial Number: *008615* Test Record Number: *6336*
Test Date: *06/13/2026* Test Time: *12:35pm EDT*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	12:36pm
FLO	Pass	12:36pm
FC	Pass	12:36pm

Temperature Tests

Test	Status	Time
FC1	Pass	12:36pm
SRC	Pass	12:36pm
DET	Pass	12:36pm
BAR	Pass	12:36pm
BT	Pass	12:36pm

Blank Tests

Test	Status	Time
AIR	Pass	12:37pm


Printer Tests

Test	Status	Time
PRNT	Pass	12:37pm

CRC Tests

Test	Status	Time
COMP	Pass	12:37pm
CAL	Pass	12:37pm

Preventive Maintenance
Status: Pass

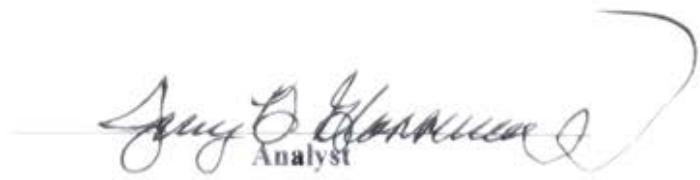

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Davidson Instrument Location BAT Mobile Unit 8

Instrument Serial No. 008736 —

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

(1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;

(2) Verify instrument displays time and date;

(3) Initiate breath test sequence;

(4) Enter information as prompted;

(5) Verify instrument accuracy;

(6) When "PLEASE BLOW" appears, collect breath sample;

(7) When "PLEASE BLOW" appears, collect breath sample;

(8) Print test record;

(9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and

(10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 13 day of June, 20 26 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.

Signature of Certifying Official

2219283
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

DHHS 4080 (04/20)

Intox EC/IR-II: Subject Test

DAVIDSON COUNTY BAT MOBILE UNIT 8 280

Serial Number: *008736*
Test Date: *06/13/2026*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name: *Glasscock, Jerry D*
Permit Number: *7180-9235*
Effective:
02/01/2026-02/01/2028

Officer's Name: *NONE, NONE*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG506303
Exp Date: 03/04/2027

Test	g/210L	Time
DIAG	Pass	12:26pm
AIR BLK	.00	12:28pm
ACCY CHK	.07	12:28pm
AIR BLK	.00	12:29pm
SUB TEST	**.00**	**12:30pm**
AIR BLK	.00	12:31pm
SUB TEST	**.00**	**12:32pm**
AIR BLK	.00	12:33pm

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

DAVIDSON COUNTY BAT MOBILE UNIT 8 280

Serial Number: *008736* Test Record Number: *1692*
Test Date: *06/13/2026* Test Time: *12:34pm EDT*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	12:34pm
FLO	Pass	12:34pm
FC	Pass	12:34pm

Temperature Tests

Test	Status	Time
FC1	Pass	12:35pm
SRC	Pass	12:35pm
DET	Pass	12:35pm
BAR	Pass	12:35pm
BT	Pass	12:35pm

Blank Tests

Test	Status	Time
AIR	Pass	12:35pm

Printer Tests

Test	Status	Time
PRNT	Pass	12:35pm

CRC Tests

Test	Status	Time
COMP	Pass	12:35pm
CAL	Pass	12:35pm

Preventive Maintenance
Status: Pass

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Davidson Instrument Location BAT Mobile Unit 8

Instrument Serial No. 008775

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

(1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;

(2) Verify instrument displays time and date;

(3) Initiate breath test sequence;

(4) Enter information as prompted;

(5) Verify instrument accuracy;

(6) When "PLEASE BLOW" appears, collect breath sample;

(7) When "PLEASE BLOW" appears, collect breath sample;

(8) Print test record;

(9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and

(10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 13 day of June, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.

Signature of Certifying Official

2219283
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

DAVIDSON COUNTY BAT MOBILE UNIT 8 280

Serial Number: *008775*
Test Date: *06/13/2026*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name: *Glasscock, Jerry D*
Permit Number: *7180-9235*
Effective:
02/01/2026-02/01/2028

Officer's Name: *NONE, NONE*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG506303
Exp Date: 03/04/2027

Test	g/210L	Time
DIAG	Pass	12:26pm
AIR BLK	.00	12:27pm
ACCY CHK	.08	12:28pm
AIR BLK	.00	12:29pm
SUB TEST	**.00**	**12:29pm**
AIR BLK	.00	12:30pm
SUB TEST	**.00**	**12:31pm**
AIR BLK	.00	12:32pm

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

DAVIDSON COUNTY BAT MOBILE UNIT 8 280

Serial Number: *008775* Test Record Number: *2543*
Test Date: *06/13/2026* Test Time: *12:33pm EDT*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	12:33pm
FLO	Pass	12:33pm
FC	Pass	12:33pm

Temperature Tests

Test	Status	Time
FC1	Pass	12:33pm
SRC	Pass	12:33pm
DET	Pass	12:33pm
BAR	Pass	12:33pm
BT	Pass	12:33pm

Blank Tests

Test	Status	Time
AIR	Pass	12:34pm

Printer Tests

Test	Status	Time
PRNT	Pass	12:34pm

CRC Tests

Test	Status	Time
COMP	Pass	12:34pm
CAL	Pass	12:34pm

Preventive Maintenance
Status: Pass



Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Davidson Instrument Location BAT Mobile Unit 8

Instrument Serial No. 008816 —

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

(1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;

(2) Verify instrument displays time and date;

(3) Initiate breath test sequence;

(4) Enter information as prompted;

(5) Verify instrument accuracy;

(6) When "PLEASE BLOW" appears, collect breath sample;

(7) When "PLEASE BLOW" appears, collect breath sample;

(8) Print test record;

(9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and

(10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 13 day of June, 20 26 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.

Signature of Certifying Official

2219283
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

DHHS 4080 (04/20)

Intox EC/IR-II: Subject Test

DAVIDSON COUNTY BAT MOBILE UNIT 8 280

Serial Number: *008816*
Test Date: *06/13/2026*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name: *Glasscock, Jerry D*
Permit Number: *7180-9235*
Effective:
02/01/2026-02/01/2028

Officer's Name: *NONE, NONE*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG431002
Exp Date: 11/05/2026

Test	g/210L	Time
DIAG	Pass	12:25pm
AIR BLK	.00	12:26pm
ACCY CHK	.07	12:27pm
AIR BLK	.00	12:28pm
SUB TEST	**.00**	**12:29pm**
AIR BLK	.00	12:30pm
SUB TEST	**.00**	**12:31pm**
AIR BLK	.00	12:32pm

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

DAVIDSON COUNTY BAT MOBILE UNIT 8 280

Serial Number: *008816* Test Record Number: *8121*
Test Date: *06/13/2026* Test Time: *12:33pm EDT*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	12:33pm
FLO	Pass	12:33pm
FC	Pass	12:33pm

Temperature Tests

Test	Status	Time
FC1	Pass	12:33pm
SRC	Pass	12:33pm
DET	Pass	12:33pm
BAR	Pass	12:33pm
BT	Pass	12:33pm

Blank Tests

Test	Status	Time
AIR	Pass	12:34pm

Printer Tests

Test	Status	Time
PRNT	Pass	12:34pm

CRC Tests

Test	Status	Time
COMP	Pass	12:34pm
CAL	Pass	12:34pm

Preventive Maintenance
Status: Pass



Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County DAVIDSON Instrument Location DAVIDSON COUNTY JAIL

Instrument Serial No. 008845 Lexington NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

(1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;

(2) Verify instrument displays time and date;

(3) Initiate breath test sequence;

(4) Enter information as prompted;

(5) Verify instrument accuracy;

(6) When "PLEASE BLOW" appears, collect breath sample;

(7) When "PLEASE BLOW" appears, collect breath sample;

(8) Print test record;

(9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and

(10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 29th day of June, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.

Signature of Certifying Official

509387
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

DHHS 4080 (04/20)

Intox EC/IR-II: Subject Test

DAVIDSON COUNTY DAVIDSON COUNTY JAIL
280

Serial Number: *008845*
Test Date: *06/29/2026*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name: *Long, Thomas A*
Permit Number: *0050-9387*
Effective:
02/01/2026-02/01/2028

Officer's Name: *NONE, NONE*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG503001
Exp Date: 01/30/2027

Test	g/210L	Time
DIAG	Pass	12:34pm
AIR BLK	.00	12:35pm
ACCY CHK	.07	12:35pm
AIR BLK	.00	12:37pm
SUB TEST	**.00**	**12:38pm**
AIR BLK	.00	12:39pm
SUB TEST	**.00**	**12:40pm**
AIR BLK	.00	12:41pm

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

DAVIDSON COUNTY DAVIDSON COUNTY JAIL 280

Serial Number: *008845* Test Record Number: *4724*
Test Date: *06/29/2026* Test Time: *12:41pm EDT*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	12:42pm
FLO	Pass	12:42pm
FC	Pass	12:42pm

Temperature Tests

Test	Status	Time
FC1	Pass	12:42pm
SRC	Pass	12:42pm
DET	Pass	12:42pm
BAR	Pass	12:42pm
BT	Pass	12:42pm

Blank Tests

Test	Status	Time
AIR	Pass	12:42pm


Printer Tests

Test	Status	Time
PRNT	Pass	12:42pm

CRC Tests

Test	Status	Time
COMP	Pass	12:43pm
CAL	Pass	12:43pm

Preventive Maintenance
Status: Pass



Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD INTOXIMETERS, MODEL INTOX EC/IR II and MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County DAVIDSON Instrument Location Thomasville Police

Instrument Serial No. 008872 Department

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

(1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;

(2) Verify instrument displays time and date;

(3) Initiate breath test sequence;

(4) Enter information as prompted;

(5) Verify instrument accuracy;

(6) When "PLEASE BLOW" appears, collect breath sample;

(7) When "PLEASE BLOW" appears, collect breath sample;

(8) Print test record;

(9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and

(10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 29th day of June, 20 26 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.

Signature of Certifying Official

509387
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

DHHS 4080 (04/20)

Intox EC/IR-II: Subject Test

DAVIDSON COUNTY THOMASVILLE PD 280

Serial Number: *008872*
Test Date: *06/29/2026*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name: *Long, Thomas A*
Permit Number: *0050-9387*
Effective:
02/01/2026-02/01/2028

Officer's Name: *NONE, NONE*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG503001
Exp Date: 01/30/2027

Test	g/210L	Time
DIAG	Pass	2:08pm
AIR BLK	.00	2:08pm
ACCY CHK	.08	2:09pm
AIR BLK	.00	2:10pm
SUB TEST	**.00**	**2:11pm**
AIR BLK	.00	2:12pm
SUB TEST	**.00**	**2:14pm**
AIR BLK	.00	2:15pm

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

DAVIDSON COUNTY THOMASVILLE PD 280

Serial Number: *008872* Test Record Number: *2035*
Test Date: *06/29/2026* Test Time: *2:15pm EDT*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	2:16pm
FLO	Pass	2:16pm
FC	Pass	2:16pm

Temperature Tests

Test	Status	Time
FC1	Pass	2:16pm
SRC	Pass	2:16pm
DET	Pass	2:16pm
BAR	Pass	2:16pm
BT	Pass	2:16pm

Blank Tests

Test	Status	Time
AIR	Pass	2:16pm


Printer Tests

Test	Status	Time
PRNT	Pass	2:17pm

CRC Tests

Test	Status	Time
COMP	Pass	2:17pm
CAL	Pass	2:17pm

Preventive Maintenance
Status: Pass

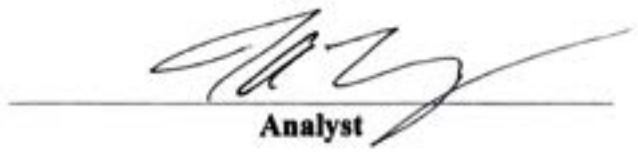

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County DAVIDSON Instrument Location LEXINGTON POLICE DEPARTMENT

Instrument Serial No. 008883

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

(1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;

(2) Verify instrument displays time and date;

(3) Initiate breath test sequence;

(4) Enter information as prompted;

(5) Verify instrument accuracy;

(6) When "PLEASE BLOW" appears, collect breath sample;

(7) When "PLEASE BLOW" appears, collect breath sample;

(8) Print test record;

(9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and

(10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 29th day of June, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.

Signature of Certifying Official

509387
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

DHHS 4080 (04/20)

Intox EC/IR-II: Subject Test

DAVIDSON COUNTY LEXINGTON PD 280

Serial Number: *008883*
Test Date: *06/29/2026*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name: *Long, Thomas A*
Permit Number: *0050-9387*
Effective:
02/01/2026-02/01/2028

Officer's Name: *NONE, NONE*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG501307
Exp Date: 01/13/2027

Test	g/210L	Time
DIAG	Pass	11:51am
AIR BLK	.00	11:52am
ACCY CHK	.07	11:52am
AIR BLK	.00	11:53am
SUB TEST	**.00**	**11:54am**
AIR BLK	.00	11:55am
SUB TEST	**.00**	**11:57am**
AIR BLK	.00	11:58am

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

DAVIDSON COUNTY LEXINGTON PD 280

Serial Number: *008883* Test Record Number: *3193*
Test Date: *06/29/2026* Test Time: *11:58am EDT*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	11:58am
FLO	Pass	11:58am
FC	Pass	11:58am

Temperature Tests

Test	Status	Time
FC1	Pass	11:59am
SRC	Pass	11:59am
DET	Pass	11:59am
BAR	Pass	11:59am
BT	Pass	11:59am

Blank Tests

Test	Status	Time
AIR	Pass	11:59am

Printer Tests

Test	Status	Time
PRNT	Pass	11:59am

CRC Tests

Test	Status	Time
COMP	Pass	11:59am
CAL	Pass	11:59am

Preventive Maintenance
Status: Pass

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Davidson Instrument Location BAT Mobile Unit 8

Instrument Serial No. 008929

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

(1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;

(2) Verify instrument displays time and date;

(3) Initiate breath test sequence;

(4) Enter information as prompted;

(5) Verify instrument accuracy;

(6) When "PLEASE BLOW" appears, collect breath sample;

(7) When "PLEASE BLOW" appears, collect breath sample;

(8) Print test record;

(9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and

(10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 13 day of June, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.

Signature of Certifying Official

2219283
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

DHHS 4080 (04/20)

Intox EC/IR-II: Subject Test

DAVIDSON COUNTY BAT MOBILE UNIT 8 280

Serial Number: *008929*
Test Date: *06/13/2026*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name: *Glasscock, Jerry D*
Permit Number: *7180-9235*
Effective:
02/01/2026-02/01/2028

Officer's Name: *NONE, NONE*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG506303
Exp Date: 03/04/2027

Test	g/210L	Time
DIAG	Pass	12:24pm
AIR BLK	.00	12:25pm
ACCY CHK	.07	12:26pm
AIR BLK	.00	12:27pm
SUB TEST	**.00**	**12:28pm**
AIR BLK	.00	12:29pm
SUB TEST	**.00**	**12:31pm**
AIR BLK	.00	12:32pm

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

DAVIDSON COUNTY BAT MOBILE UNIT 8 280

Serial Number: *008929* Test Record Number: *1828*
Test Date: *06/13/2026* Test Time: *12:32pm EDT*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	12:33pm
FLO	Pass	12:33pm
FC	Pass	12:33pm

Temperature Tests

Test	Status	Time
FC1	Pass	12:33pm
SRC	Pass	12:33pm
DET	Pass	12:33pm
BAR	Pass	12:33pm
BT	Pass	12:33pm

Blank Tests

Test	Status	Time
AIR	Pass	12:34pm

Printer Tests

Test	Status	Time
PRNT	Pass	12:34pm

CRC Tests

Test	Status	Time
COMP	Pass	12:34pm
CAL	Pass	12:34pm

Preventive Maintenance
Status: Pass



Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD INTOXIMETERS, MODEL INTOX EC/IR II and MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County DUPLIN Instrument Location DUPLIN COUNTY DETENTION CENTER

Instrument Serial No. 008864

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

(1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;

(2) Verify instrument displays time and date;

(3) Initiate breath test sequence;

(4) Enter information as prompted;

(5) Verify instrument accuracy;

(6) When "PLEASE BLOW" appears, collect breath sample;

(7) When "PLEASE BLOW" appears, collect breath sample;

(8) Print test record;

(9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and

(10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 1st day of JUNE, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.

Signature of Certifying Official

1H6279
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

DUPLIN COUNTY DETENTION CENTER 300

Serial Number: *008864*
Test Date: *06/01/2026*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name: *BARNES, ALVIN R*
Permit Number: *0014-6279*
Effective:
02/01/2026-02/01/2028

Officer's Name: *NONE, NONE*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG534301
Exp Date: 12/09/2027

Test	g/210L	Time
DIAG	Pass	11:57am
AIR BLK	.00	11:58am
ACCY CHK	.07	11:58am
AIR BLK	.00	11:59am
SUB TEST	**.00**	**12:00pm**
AIR BLK	.00	12:01pm
SUB TEST	**.00**	**12:03pm**
AIR BLK	.00	12:04pm

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

DUPLIN COUNTY DETENTION CENTER 300

Serial Number: *008864* Test Record Number: *5431*
Test Date: *06/01/2026* Test Time: *12:06pm EDT*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	12:06pm
FLO	Pass	12:06pm
FC	Pass	12:06pm

Temperature Tests

Test	Status	Time
FC1	Pass	12:06pm
SRC	Pass	12:06pm
DET	Pass	12:06pm
BAR	Pass	12:06pm
BT	Pass	12:06pm

Blank Tests

Test	Status	Time
AIR	Pass	12:07pm

Printer Tests

Test	Status	Time
PRNT	Pass	12:07pm

CRC Tests

Test	Status	Time
COMP	Pass	12:07pm
CAL	Pass	12:07pm

Preventive Maintenance
Status: Pass

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD INTOXIMETERS, MODEL INTOX EC/IR II and MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County DURHAM Instrument Location DURHAM Co. JAIL

Instrument Serial No. 008859 219 S. MANGUM St
DURHAM, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

(1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;

(2) Verify instrument displays time and date;

(3) Initiate breath test sequence;

(4) Enter information as prompted;

(5) Verify instrument accuracy;

(6) When "PLEASE BLOW" appears, collect breath sample;

(7) When "PLEASE BLOW" appears, collect breath sample;

(8) Print test record;

(9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and

(10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 24 day of JUNE, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.

THE GREAT SEAL OF THE STATE OF NORTH CAROLINA

E A Bryant
Signature of Certifying Official

179707
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

DURHAM COUNTY DURHAM COUNTY JAIL 310

Serial Number: *008859*
Test Date: *06/24/2026*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name: *Bryant, Earl A*
Permit Number: *0017-9707*
Effective:
02/01/2026-02/01/2028

Officer's Name: *NONE, NONE*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG534301
Exp Date: 12/09/2027

Test	g/210L	Time
DIAG	Pass	12:37pm
AIR BLK	.00	12:38pm
ACCY CHK	.08	12:39pm
AIR BLK	.00	12:40pm
SUB TEST	**.00**	**12:40pm**
AIR BLK	.00	12:41pm
SUB TEST	**.00**	**12:43pm**
AIR BLK	.00	12:44pm

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

DURHAM COUNTY DURHAM COUNTY JAIL 310

Serial Number: *008859* Test Record Number: *3535*
Test Date: *06/24/2026* Test Time: *12:47pm EDT*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	12:48pm
FLO	Pass	12:48pm
FC	Pass	12:48pm

Temperature Tests

Test	Status	Time
FC1	Pass	12:48pm
SRC	Pass	12:48pm
DET	Pass	12:48pm
BAR	Pass	12:48pm
BT	Pass	12:48pm

Blank Tests

Test	Status	Time
AIR	Pass	12:49pm

Printer Tests

Test	Status	Time
PRNT	Pass	12:49pm

CRC Tests

Test	Status	Time
COMP	Pass	12:49pm
CAL	Pass	12:49pm

Preventive Maintenance
Status: Pass

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County DURHAM Instrument Location DURHAM Co. JAIL

Instrument Serial No. 008878 219 S. MANGUM St DURHAM, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

(1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;

(2) Verify instrument displays time and date;

(3) Initiate breath test sequence;

(4) Enter information as prompted;

(5) Verify instrument accuracy;

(6) When "PLEASE BLOW" appears, collect breath sample;

(7) When "PLEASE BLOW" appears, collect breath sample;

(8) Print test record;

(9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and

(10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 24 day of JUNE, 20 26 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.

THE GREAT SEAL OF THE STATE OF NORTH CAROLINA

E A Bryant
Signature of Certifying Official

179707
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

DHHS 4080 (04/20)

Intox EC/IR-II: Subject Test

DURHAM COUNTY DURHAM COUNTY JAIL 310

Serial Number: *008878*
Test Date: *06/24/2026*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name: *Bryant, Earl A*
Permit Number: *0017-9707*
Effective:
02/01/2026-02/01/2028

Officer's Name: *NONE, NONE*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG534301
Exp Date: 12/09/2027

Test	g/210L	Time
DIAG	Pass	12:38pm
AIR BLK	.00	12:39pm
ACCY CHK	.08	12:40pm
AIR BLK	.00	12:41pm
SUB TEST	**.00**	**12:42pm**
AIR BLK	.00	12:43pm
SUB TEST	**.00**	**12:44pm**
AIR BLK	.00	12:45pm

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

DURHAM COUNTY DURHAM COUNTY JAIL 310

Serial Number: *008878* Test Record Number: *7149*
Test Date: *06/24/2026* Test Time: *12:49pm EDT*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	12:49pm
FLO	Pass	12:49pm
FC	Pass	12:49pm

Temperature Tests

Test	Status	Time
FC1	Pass	12:49pm
SRC	Pass	12:49pm
DET	Pass	12:49pm
BAR	Pass	12:49pm
BT	Pass	12:49pm

Blank Tests

Test	Status	Time
AIR	Pass	12:50pm

Printer Tests

Test	Status	Time
PRNT	Pass	12:50pm

CRC Tests

Test	Status	Time
COMP	Pass	12:50pm
CAL	Pass	12:50pm

Preventive Maintenance
Status: Pass

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County DURHAM Instrument Location DURHAM Co. JAIL

Instrument Serial No. 008891 219 S. MANGUM ST
DURHAM, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

(1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;

(2) Verify instrument displays time and date;

(3) Initiate breath test sequence;

(4) Enter information as prompted;

(5) Verify instrument accuracy;

(6) When "PLEASE BLOW" appears, collect breath sample;

(7) When "PLEASE BLOW" appears, collect breath sample;

(8) Print test record;

(9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and

(10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 24 day of JUNE, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.

E A Bryant
Signature of Certifying Official

179707
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

DHHS 4080 (04/20)

Intox EC/IR-II: Subject Test

DURHAM COUNTY DURHAM COUNTY JAIL 310

Serial Number: *008891*
Test Date: *06/24/2026*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name: *Bryant, Earl A*
Permit Number: *0017-9707*
Effective:
02/01/2026-02/01/2028

Officer's Name: *NONE, NONE*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG534301
Exp Date: 12/09/2027

Test	g/210L	Time
DIAG	Pass	12:45pm
AIR BLK	.00	12:46pm
ACCY CHK	.07	12:46pm
AIR BLK	.00	12:48pm
SUB TEST	**.00**	**12:48pm**
AIR BLK	.00	12:49pm
SUB TEST	**.00**	**12:51pm**
AIR BLK	.00	12:51pm

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

DURHAM COUNTY DURHAM COUNTY JAIL 310

Serial Number: *008891* Test Record Number: *5094*
Test Date: *06/24/2026* Test Time: *12:53pm EDT*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	12:54pm
FLO	Pass	12:54pm
FC	Pass	12:54pm

Temperature Tests

Test	Status	Time
FC1	Pass	12:54pm
SRC	Pass	12:54pm
DET	Pass	12:54pm
BAR	Pass	12:54pm
BT	Pass	12:54pm

Blank Tests

Test	Status	Time
AIR	Pass	12:55pm

Printer Tests

Test	Status	Time
PRNT	Pass	12:55pm

CRC Tests

Test	Status	Time
COMP	Pass	12:55pm
CAL	Pass	12:55pm

Preventive Maintenance
Status: Pass

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD INTOXIMETERS, MODEL INTOX EC/IR II and MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Edgecombe Instrument Location BAT Mobile Unit 12

Instrument Serial No. 008601

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

(1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;

(2) Verify instrument displays time and date;

(3) Initiate breath test sequence;

(4) Enter information as prompted;

(5) Verify instrument accuracy;

(6) When "PLEASE BLOW" appears, collect breath sample;

(7) When "PLEASE BLOW" appears, collect breath sample;

(8) Print test record;

(9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and

(10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 6th day of June, 20 26 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.

Signature of Certifying Official

83034
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

DHHS 4080 (04/20)

Intox EC/IR-II: Subject Test

EDGECOMBE COUNTY BAT MOBILE UNIT 12
320

Serial Number: *008601*
Test Date: *06/06/2026*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name:
Crutchfield Jr., Marshall B
Permit Number: *0008-3034*
Effective:
03/01/2026-03/01/2028

Officer's Name: *NONE, NONE*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG501307
Exp Date: 01/13/2027

Test	g/210L	Time
DIAG	Pass	10:36pm
AIR BLK	.00	10:37pm
ACCY CHK	.07	10:38pm
AIR BLK	.00	10:39pm
SUB TEST	**.00**	**10:39pm**
AIR BLK	.00	10:40pm
SUB TEST	**.00**	**10:42pm**
AIR BLK	.00	10:43pm

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

EDGECOMBE COUNTY BAT. MOBILE UNIT 12 320

Serial Number: *008601* Test Record Number: *1945*
Test Date: *06/06/2026* Test Time: *10:44pm EDT*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	10:45pm
FLO	Pass	10:45pm
FC	Pass	10:45pm

Temperature Tests

Test	Status	Time
FC1	Pass	10:45pm
SRC	Pass	10:45pm
DET	Pass	10:45pm
BAR	Pass	10:45pm
BT	Pass	10:45pm

Blank Tests

Test	Status	Time
AIR	Pass	10:45pm

Printer Tests

Test	Status	Time
PRNT	Pass	10:45pm

CRC Tests

Test	Status	Time
COMP	Pass	10:46pm
CAL	Pass	10:46pm

Preventive Maintenance
Status: Pass



Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Edgecombe Instrument Location BAT Mobile Unit 12

Instrument Serial No. 008618

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

(1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;

(2) Verify instrument displays time and date;

(3) Initiate breath test sequence;

(4) Enter information as prompted;

(5) Verify instrument accuracy;

(6) When "PLEASE BLOW" appears, collect breath sample;

(7) When "PLEASE BLOW" appears, collect breath sample;

(8) Print test record;

(9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and

(10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 6th day of June, 20 26 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.

Signature of Certifying Official

83034
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

DHHS 4080 (04/20)

Intox EC/IR-II: Subject Test

EDGECOMBE COUNTY BAT MOBILE UNIT 12
320

Serial Number: *008698*
Test Date: *06/06/2026*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name:
Crutchfield Jr., Marshall B
Permit Number: *0008-3034*
Effective:
03/01/2026-03/01/2028

Officer's Name: *NONE, NONE*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG431002
Exp Date: 11/05/2026

Test	g/210L	Time
DIAG	Pass	10:34pm
AIR BLK	.00	10:35pm
ACCY CHK	.08	10:35pm
AIR BLK	.00	10:36pm
SUB TEST	**.00**	**10:37pm**
AIR BLK	.00	10:38pm
SUB TEST	**.00**	**10:40pm**
AIR BLK	.00	10:41pm

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

EDGECOMBE COUNTY BAT MOBILE UNIT 12 320

Serial Number: *008698* Test Record Number: *2779*
Test Date: *06/06/2026* Test Time: *10:42pm EDT*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	10:42pm
FLO	Pass	10:42pm
FC	Pass	10:42pm

Temperature Tests

Test	Status	Time
FC1	Pass	10:42pm
SRC	Pass	10:42pm
DET	Pass	10:42pm
BAR	Pass	10:42pm
BT	Pass	10:42pm

Blank Tests

Test	Status	Time
AIR	Pass	10:43pm

Printer Tests

Test	Status	Time
PRNT	Pass	10:43pm

CRC Tests

Test	Status	Time
COMP	Pass	10:43pm
CAL	Pass	10:43pm

Preventive Maintenance
Status: Pass

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD INTOXIMETERS, MODEL INTOX EC/IR II and MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Edgecombe Instrument Location BAT Mobile Unit 12

Instrument Serial No. 008788

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

(1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;

(2) Verify instrument displays time and date;

(3) Initiate breath test sequence;

(4) Enter information as prompted;

(5) Verify instrument accuracy;

(6) When "PLEASE BLOW" appears, collect breath sample;

(7) When "PLEASE BLOW" appears, collect breath sample;

(8) Print test record;

(9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and

(10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 6th day of June, 20 26 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.

Signature of Certifying Official

83034
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

EDGECOMBE COUNTY BAT MOBILE UNIT 12
320

Serial Number: *008788*
Test Date: *06/06/2026*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name:
Crutchfield Jr., Marshall B
Permit Number: *0008-3034*
Effective:
03/01/2026-03/01/2028

Officer's Name: *NONE, NONE*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG417802
Exp Date: 06/26/2026

Test	g/210L	Time
DIAG	Pass	10:49pm
AIR BLK	.00	10:50pm
ACCY CHK	.08	10:50pm
AIR BLK	.00	10:51pm
SUB TEST	**.00**	**10:52pm**
AIR BLK	.00	10:52pm
SUB TEST	**.00**	**10:54pm**
AIR BLK	.00	10:55pm

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

EDGECOMBE COUNTY BAT MOBILE UNIT 12 320

Serial Number: *008788* Test Record Number: *2561*
Test Date: *06/06/2026* Test Time: *10:56pm EDT*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	10:56pm
FLO	Pass	10:56pm
FC	Pass	10:56pm

Temperature Tests

Test	Status	Time
FC1	Pass	10:56pm
SRC	Pass	10:56pm
DET	Pass	10:56pm
BAR	Pass	10:56pm
BT	Pass	10:56pm

Blank Tests

Test	Status	Time
AIR	Pass	10:57pm

Printer Tests

Test	Status	Time
PRNT	Pass	10:57pm

CRC Tests

Test	Status	Time
COMP	Pass	10:57pm
CAL	Pass	10:57pm

Preventive Maintenance
Status: Pass



Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Forsyth Instrument Location BAT Mobile Unit 8

Instrument Serial No. 008615 –

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

(1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;

(2) Verify instrument displays time and date;

(3) Initiate breath test sequence;

(4) Enter information as prompted;

(5) Verify instrument accuracy;

(6) When "PLEASE BLOW" appears, collect breath sample;

(7) When "PLEASE BLOW" appears, collect breath sample;

(8) Print test record;

(9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and

(10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 6 day of June, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.

Signature of Certifying Official

2219283
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

DHHS 4080 (04/20)

Intox EC/IR-II: Subject Test

FORSYTH COUNTY BAT MOBILE UNIT 8 330

Serial Number: *008615*
Test Date: *06/06/2026*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name: *Glasscock, Jerry D*
Permit Number: *7180-9235*
Effective:
02/01/2026-02/01/2028

Officer's Name: *NONE, NONE*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG506303
Exp Date: 03/04/2027

Test	g/210L	Time
DIAG	Pass	8:48pm
AIR BLK	.00	8:49pm
ACCY CHK	.07	8:49pm
AIR BLK	.00	8:50pm
SUB TEST	**.00**	**8:51pm**
AIR BLK	.00	8:52pm
SUB TEST	**.00**	**8:53pm**
AIR BLK	.00	8:54pm

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

FORSYTH COUNTY BAT MOBILE UNIT 8 330

Serial Number: *008615* Test Record Number: *6330*
Test Date: *06/06/2026* Test Time: *8:55pm EDT*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	8:55pm
FLO	Pass	8:55pm
FC	Pass	8:55pm

Temperature Tests

Test	Status	Time
FC1	Pass	8:56pm
SRC	Pass	8:56pm
DET	Pass	8:56pm
BAR	Pass	8:56pm
BT	Pass	8:56pm

Blank Tests

Test	Status	Time
AIR	Pass	8:56pm

Printer Tests

Test	Status	Time
PRNT	Pass	8:56pm

CRC Tests

Test	Status	Time
COMP	Pass	8:56pm
CAL	Pass	8:56pm

Preventive Maintenance
Status: Pass

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Forsyth Instrument Location BAT Mobile Unit 8

Instrument Serial No. 008736 —

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

(1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;

(2) Verify instrument displays time and date;

(3) Initiate breath test sequence;

(4) Enter information as prompted;

(5) Verify instrument accuracy;

(6) When "PLEASE BLOW" appears, collect breath sample;

(7) When "PLEASE BLOW" appears, collect breath sample;

(8) Print test record;

(9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and

(10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 6 day of June, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.

Signature of Certifying Official

2219283
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

DHHS 4080 (04/20)

Intox EC/IR-II: Subject Test

FORSYTH COUNTY BAT MOBILE UNIT 8 330

Serial Number: *008736*
Test Date: *06/06/2026*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name: *Glasscock, Jerry D*
Permit Number: *7180-9235*
Effective:
02/01/2026-02/01/2028

Officer's Name: *NONE, NONE*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG506303
Exp Date: 03/04/2027

Test	g/210L	Time
DIAG	Pass	8:48pm
AIR BLK	.00	8:49pm
ACCY CHK	.07	8:50pm
AIR BLK	.00	8:51pm
SUB TEST	**.00**	**8:51pm**
AIR BLK	.00	8:52pm
SUB TEST	**.00**	**8:53pm**
AIR BLK	.00	8:54pm

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

FORSYTH COUNTY BAT MOBILE UNIT 8 330

Serial Number: *008736* Test Record Number: *1686*
Test Date: *06/06/2026* Test Time: *8:55pm EDT*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	8:55pm
FLO	Pass	8:55pm
FC	Pass	8:55pm

Temperature Tests

Test	Status	Time
FC1	Pass	8:56pm
SRC	Pass	8:56pm
DET	Pass	8:56pm
BAR	Pass	8:56pm
BT	Pass	8:56pm

Blank Tests

Test	Status	Time
AIR	Pass	8:56pm

Printer Tests

Test	Status	Time
PRNT	Pass	8:56pm

CRC Tests

Test	Status	Time
COMP	Pass	8:56pm
CAL	Pass	8:56pm

Preventive Maintenance
Status: Pass



Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Forsyth Instrument Location BAT Mobile Unit 8

Instrument Serial No. 008775

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

(1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;

(2) Verify instrument displays time and date;

(3) Initiate breath test sequence;

(4) Enter information as prompted;

(5) Verify instrument accuracy;

(6) When "PLEASE BLOW" appears, collect breath sample;

(7) When "PLEASE BLOW" appears, collect breath sample;

(8) Print test record;

(9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and

(10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 6 day of June, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.

Signature of Certifying Official

2219283
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

DHHS 4080 (04/20)

FORSYTH COUNTY BAT MOBILE UNIT 8 330

Serial Number: *008775*
Test Date: *06/06/2026*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name: *Glasscock, Jerry D*
Permit Number: *7180-9235*
Effective:
02/01/2026-02/01/2028

Officer's Name: *NONE, NONE*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG506303
Exp Date: 03/04/2027

Test	g/210L	Time
DIAG	Pass	8:49pm
AIR BLK	.00	8:50pm
ACCY CHK	.08	8:50pm
AIR BLK	.00	8:51pm
SUB TEST	**.00**	**8:52pm**
AIR BLK	.00	8:53pm
SUB TEST	**.00**	**8:54pm**
AIR BLK	.00	8:55pm

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

FORSYTH COUNTY BAT MOBILE UNIT 8 330

Serial Number: *008775* Test Record Number: *2536*
Test Date: *06/06/2026* Test Time: *8:55pm EDT*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	8:56pm
FLO	Pass	8:56pm
FC	Pass	8:56pm

Temperature Tests

Test	Status	Time
FC1	Pass	8:56pm
SRC	Pass	8:56pm
DET	Pass	8:56pm
BAR	Pass	8:56pm
BT	Pass	8:56pm

Blank Tests

Test	Status	Time
AIR	Pass	8:56pm

Printer Tests

Test	Status	Time
PRNT	Pass	8:56pm

CRC Tests

Test	Status	Time
COMP	Pass	8:57pm
CAL	Pass	8:57pm

Preventive Maintenance
Status: Pass

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Forsyth Instrument Location BAT Mobile Unit 8

Instrument Serial No. 008816 –

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

(1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;

(2) Verify instrument displays time and date;

(3) Initiate breath test sequence;

(4) Enter information as prompted;

(5) Verify instrument accuracy;

(6) When "PLEASE BLOW" appears, collect breath sample;

(7) When "PLEASE BLOW" appears, collect breath sample;

(8) Print test record;

(9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and

(10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 6 day of JUNE, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.

THE GREAT SEAL OF THE STATE OF NORTH CAROLINA

Signature of Certifying Official

2219283
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

FORSYTH COUNTY BAT MOBILE UNIT 8 330

Serial Number: *008816*
Test Date: *06/06/2026*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name: *Glasscock, Jerry D*
Permit Number: *7180-9235*
Effective:
02/01/2026-02/01/2028

Officer's Name: *NONE, NONE*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG431002
Exp Date: 11/05/2026

Test	g/210L	Time
DIAG	Pass	8:50pm
AIR BLK	.00	8:51pm
ACCY CHK	.07	8:51pm
AIR BLK	.00	8:52pm
SUB TEST	**.00**	**8:53pm**
AIR BLK	.00	8:54pm
SUB TEST	**.00**	**8:55pm**
AIR BLK	.00	8:56pm

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

FORSYTH COUNTY BAT MOBILE UNIT 8 330

Serial Number: *008816* Test Record Number: *8115*
Test Date: *06/06/2026* Test Time: *8:56pm EDT*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	8:56pm
FLO	Pass	8:56pm
FC	Pass	8:57pm

Temperature Tests

Test	Status	Time
FC1	Pass	8:57pm
SRC	Pass	8:57pm
DET	Pass	8:57pm
BAR	Pass	8:57pm
BT	Pass	8:57pm

Blank Tests

Test	Status	Time
AIR	Pass	8:57pm

Printer Tests

Test	Status	Time
PRNT	Pass	8:57pm

CRC Tests

Test	Status	Time
COMP	Pass	8:58pm
CAL	Pass	8:58pm

Preventive Maintenance
Status: Pass

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Forsyth Instrument Location BAT Mobile Unit 8

Instrument Serial No. 008929 —

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

(1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;

(2) Verify instrument displays time and date;

(3) Initiate breath test sequence;

(4) Enter information as prompted;

(5) Verify instrument accuracy;

(6) When "PLEASE BLOW" appears, collect breath sample;

(7) When "PLEASE BLOW" appears, collect breath sample;

(8) Print test record;

(9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and

(10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 6 day of June, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.

Signature of Certifying Official

2219283
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

DHHS 4080 (04/20)

Intox EC/IR-II: Subject Test

FORSYTH COUNTY BAT MOBILE UNIT 8 330

Serial Number: *008929*
Test Date: *06/06/2026*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name: *Glasscock, Jerry D*
Permit Number: *7180-9235*
Effective:
02/01/2026-02/01/2028

Officer's Name: *NONE, NONE*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG506303
Exp Date: 03/04/2027

Test	g/210L	Time
DIAG	Pass	8:50pm
AIR BLK	.00	8:51pm
ACCY CHK	.07	8:52pm
AIR BLK	.00	8:53pm
SUB TEST	**.00**	**8:53pm**
AIR BLK	.00	8:54pm
SUB TEST	**.00**	**8:56pm**
AIR BLK	.00	8:57pm

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

FORSYTH COUNTY BAT MOBILE UNIT 8 330

Serial Number: *008929* Test Record Number: *1822*
Test Date: *06/06/2026* Test Time: *8:58pm EDT*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	8:58pm
FLO	Pass	8:58pm
FC	Pass	8:59pm

Temperature Tests

Test	Status	Time
FC1	Pass	8:59pm
SRC	Pass	8:59pm
DET	Pass	8:59pm
BAR	Pass	8:59pm
BT	Pass	8:59pm

Blank Tests

Test	Status	Time
AIR	Pass	8:59pm

Printer Tests

Test	Status	Time
PRNT	Pass	9:00pm

CRC Tests

Test	Status	Time
COMP	Pass	9:00pm
CAL	Pass	9:00pm

Preventive Maintenance
Status: Pass

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County FRANKLIN Instrument Location YOUNGSVILLE PD

Instrument Serial No. QQ 8781 134 Alt U.S. 1
YOUNGSVILLE, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

(1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;

(2) Verify instrument displays time and date;

(3) Initiate breath test sequence;

(4) Enter information as prompted;

(5) Verify instrument accuracy;

(6) When "PLEASE BLOW" appears, collect breath sample;

(7) When "PLEASE BLOW" appears, collect breath sample;

(8) Print test record;

(9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and

(10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 15 day of JUNE, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.

E A Bryant
Signature of Certifying Official

179707
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

DHHS 4080 (04/20)

Intox EC/IR-II: Subject Test

FRANKLIN COUNTY YOUNGSVILLE PD 340

Serial Number: *008781*
Test Date: *06/15/2026*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name: *Bryant, Earl A*
Permit Number: *0017-9707*
Effective:
02/01/2026-02/01/2028

Officer's Name: *NONE, NONE*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG534301
Exp Date: 12/09/2027

Test	g/210L	Time
DIAG	Pass	3:06pm
AIR BLK	.00	3:07pm
ACCY CHK	.07	3:07pm
AIR BLK	.00	3:08pm
SUB TEST	**.00**	**3:09pm**
AIR BLK	.00	3:10pm
SUB TEST	**.00**	**3:11pm**
AIR BLK	.00	3:12pm

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

FRANKLIN COUNTY YOUNGSVILLE PD 340

Serial Number: *008781* Test Record Number: *6366*
Test Date: *06/15/2026* Test Time: *3:14pm EDT*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	3:14pm
FLO	Pass	3:14pm
FC	Pass	3:15pm

Temperature Tests

Test	Status	Time
FC1	Pass	3:15pm
SRC	Pass	3:15pm
DET	Pass	3:15pm
BAR	Pass	3:15pm
BT	Pass	3:15pm

Blank Tests

Test	Status	Time
AIR	Pass	3:15pm

Printer Tests

Test	Status	Time
PRNT	Pass	3:15pm

CRC Tests

Test	Status	Time
COMP	Pass	3:16pm
CAL	Pass	3:16pm

Preventive Maintenance
Status: Pass

E A Bryant

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Gaston Instrument Location Gaston County Jail Gastonia, NC

Instrument Serial No. 008643

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

(1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;

(2) Verify instrument displays time and date;

(3) Initiate breath test sequence;

(4) Enter information as prompted;

(5) Verify instrument accuracy;

(6) When "PLEASE BLOW" appears, collect breath sample;

(7) When "PLEASE BLOW" appears, collect breath sample;

(8) Print test record;

(9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and

(10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 11th day of June, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.

Signature of Certifying Official

849845
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

DHHS 4080 (04/20)

Intox EC/IR-II: Subject Test

GASTON COUNTY GASTON COUNTY SO 350

Serial Number: *008643*
Test Date: *06/11/2026*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name: *Helms, Bryce A*
Permit Number: *0084-9845*
Effective:
02/01/2026-02/01/2028

Officer's Name: *NONE, NONE*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG506303
Exp Date: 03/04/2027

Test	g/210L	Time
DIAG	Pass	12:24pm
AIR BLK	.00	12:25pm
ACCY CHK	.07	12:26pm
AIR BLK	.00	12:27pm
SUB TEST	**.00**	**12:27pm**
AIR BLK	.00	12:28pm
SUB TEST	**.00**	**12:30pm**
AIR BLK	.00	12:31pm

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

GASTON COUNTY GASTON COUNTY SO 350

Serial Number: *008643* Test Record Number: *5464*
Test Date: *06/11/2026* Test Time: *12:31pm EDT*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	12:31pm
FLO	Pass	12:31pm
FC	Pass	12:32pm

Temperature Tests

Test	Status	Time
FC1	Pass	12:32pm
SRC	Pass	12:32pm
DET	Pass	12:32pm
BAR	Pass	12:32pm
BT	Pass	12:32pm

Blank Tests

Test	Status	Time
AIR	Pass	12:32pm

Printer Tests

Test	Status	Time
PRNT	Pass	12:32pm

CRC Tests

Test	Status	Time
COMP	Pass	12:33pm
CAL	Pass	12:33pm

Preventive Maintenance
Status: Pass

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Gaston Instrument Location Gaston County Jail Gastonia, NC

Instrument Serial No. 008084

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

(1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;

(2) Verify instrument displays time and date;

(3) Initiate breath test sequence;

(4) Enter information as prompted;

(5) Verify instrument accuracy;

(6) When "PLEASE BLOW" appears, collect breath sample;

(7) When "PLEASE BLOW" appears, collect breath sample;

(8) Print test record;

(9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and

(10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 10th day of June, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.

Signature of Certifying Official

849845
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

DHHS 4080 (04/20)

Intox EC/IR-II: Subject Test

GASTON COUNTY GASTON COUNTY SO 350

Serial Number: *008684*
Test Date: *06/11/2026*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name: *Helms, Bryce A*
Permit Number: *0084-9845*
Effective:
02/01/2026-02/01/2028

Officer's Name: *NONE, NONE*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG516203
Exp Date: 06/11/2027

Test	g/210L	Time
DIAG	Pass	12:21pm
AIR BLK	.00	12:22pm
ACCY CHK	.07	12:23pm
AIR BLK	.00	12:24pm
SUB TEST	**.00**	**12:25pm**
AIR BLK	.00	12:25pm
SUB TEST	**.00**	**12:27pm**
AIR BLK	.00	12:28pm

Reported AC: .00 g/210L

Bryce Helms
Signature of Chemical Analyst

Court CVR

Bryce Helms
Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

GASTON COUNTY GASTON COUNTY SO 350

Serial Number: *008684* Test Record Number: *7120*
Test Date: *06/11/2026* Test Time: *12:28pm EDT*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	12:29pm
FLO	Pass	12:29pm
FC	Pass	12:29pm

Temperature Tests

Test	Status	Time
FC1	Pass	12:29pm
SRC	Pass	12:29pm
DET	Pass	12:29pm
BAR	Pass	12:29pm
BT	Pass	12:29pm

Blank Tests

Test	Status	Time
AIR	Pass	12:29pm

Printer Tests

Test	Status	Time
PRNT	Pass	12:29pm

CRC Tests

Test	Status	Time
COMP	Pass	12:30pm
CAL	Pass	12:30pm

Preventive Maintenance
Status: Pass

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Gates Instrument Location BAT Mobile Unit 13

Instrument Serial No. 008865

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

(1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;

(2) Verify instrument displays time and date;

(3) Initiate breath test sequence;

(4) Enter information as prompted;

(5) Verify instrument accuracy;

(6) When "PLEASE BLOW" appears, collect breath sample;

(7) When "PLEASE BLOW" appears, collect breath sample;

(8) Print test record;

(9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and

(10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 6th day of June, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.

Signature of Certifying Official

307699
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

DHHS 4080 (04/20)

Intox EC/IR-II: Subject Test

GATES COUNTY BAT MOBILE UNIT 13 360

Serial Number: *008869*
Test Date: *06/06/2026*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name: *Whitehurst, Timothy B*
Permit Number: *0030-7699*
Effective:
03/01/2026-03/01/2028

Officer's Name: *NONE, NONE*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG506303
Exp Date: 03/04/2027

Test	g/210L	Time
DIAG	Pass	7:10pm
AIR BLK	.00	7:11pm
ACCY CHK	.08	7:11pm
AIR BLK	.00	7:12pm
SUB TEST	**.00**	**7:13pm**
AIR BLK	.00	7:14pm
SUB TEST	**.00**	**7:15pm**
AIR BLK	.00	7:16pm

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

GATES COUNTY BAT MOBILE UNIT 13 360

Serial Number: *008869* Test Record Number: *2217*
Test Date: *06/06/2026* Test Time: *7:17pm EDT*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	7:18pm
FLO	Pass	7:18pm
FC	Pass	7:18pm

Temperature Tests

Test	Status	Time
FC1	Pass	7:18pm
SRC	Pass	7:18pm
DET	Pass	7:18pm
BAR	Pass	7:18pm
BT	Pass	7:18pm

Blank Tests

Test	Status	Time
AIR	Pass	7:18pm

Printer Tests

Test	Status	Time
PRNT	Pass	7:18pm

CRC Tests

Test	Status	Time
COMP	Pass	7:19pm
CAL	Pass	7:19pm

Preventive Maintenance
Status: Pass

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Gates Instrument Location BAT Mobile Unit 13

Instrument Serial No. 008898

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

(1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;

(2) Verify instrument displays time and date;

(3) Initiate breath test sequence;

(4) Enter information as prompted;

(5) Verify instrument accuracy;

(6) When "PLEASE BLOW" appears, collect breath sample;

(7) When "PLEASE BLOW" appears, collect breath sample;

(8) Print test record;

(9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and

(10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 6th day of June, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.

Timothy B Nichols
Signature of Certifying Official

307699
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

DHHS 4080 (04/20)

Intox EC/IR-II: Subject Test

GATES COUNTY BAT MOBILE UNIT 13 360

Serial Number: *008898*
Test Date: *06/06/2026*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name: *Whitehurst, Timothy B*
Permit Number: *0030-7699*
Effective:
03/01/2026-03/01/2028

Officer's Name: *NONE, NONE*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG506302
Exp Date: 03/04/2027

Test	g/210L	Time
DIAG	Pass	6:55pm
AIR BLK	.00	6:56pm
ACCY CHK	.07	6:56pm
AIR BLK	.00	6:57pm
SUB TEST	**.00**	**6:58pm**
AIR BLK	.00	6:59pm
SUB TEST	**.00**	**7:00pm**
AIR BLK	.00	7:01pm

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

GATES COUNTY BAT MOBILE UNIT 13 360

Serial Number: *008898* Test Record Number: *2158*
Test Date: *06/06/2026* Test Time: *7:02pm EDT*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	7:02pm
FLO	Pass	7:02pm
FC	Pass	7:02pm

Temperature Tests

Test	Status	Time
FC1	Pass	7:02pm
SRC	Pass	7:02pm
DET	Pass	7:02pm
BAR	Pass	7:02pm
BT	Pass	7:02pm

Blank Tests

Test	Status	Time
AIR	Pass	7:03pm

Printer Tests

Test	Status	Time
PRNT	Pass	7:03pm

CRC Tests

Test	Status	Time
COMP	Pass	7:03pm
CAL	Pass	7:03pm

Preventive Maintenance
Status: Pass

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Gates Instrument Location BAT Mobile Unit 13

Instrument Serial No. 008939

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

(1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;

(2) Verify instrument displays time and date;

(3) Initiate breath test sequence;

(4) Enter information as prompted;

(5) Verify instrument accuracy;

(6) When "PLEASE BLOW" appears, collect breath sample;

(7) When "PLEASE BLOW" appears, collect breath sample;

(8) Print test record;

(9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and

(10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 6th day of June, 2024 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.

Timothy B White
Signature of Certifying Official

307699
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

DHHS 4080 (04/20)

Intox EC/IR-II: Subject Test

GATES COUNTY BAT MOBILE UNIT 13 360

Serial Number: *008939*
Test Date: *06/06/2026*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name: *Whitehurst, Timothy B*
Permit Number: *0030-7699*
Effective:
03/01/2026-03/01/2028

Officer's Name: *NONE, NONE*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG506302
Exp Date: 03/04/2027

Test	g/210L	Time
DIAG	Pass	6:41pm
AIR BLK	.00	6:42pm
ACCY CHK	.07	6:43pm
AIR BLK	.00	6:44pm
SUB TEST	**.00**	**6:45pm**
AIR BLK	.00	6:46pm
SUB TEST	**.00**	**6:47pm**
AIR BLK	.00	6:48pm

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

GATES COUNTY BAT MOBILE UNIT 13 360

Serial Number: *008939* Test Record Number: *2018*
Test Date: *06/06/2026* Test Time: *6:48pm EDT*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	6:49pm
FLO	Pass	6:49pm
FC	Pass	6:49pm

Temperature Tests

Test	Status	Time
FC1	Pass	6:49pm
SRC	Pass	6:49pm
DET	Pass	6:49pm
BAR	Pass	6:49pm
BT	Pass	6:49pm

Blank Tests

Test	Status	Time
AIR	Pass	6:50pm

Printer Tests

Test	Status	Time
PRNT	Pass	6:50pm

CRC Tests

Test	Status	Time
COMP	Pass	6:50pm
CAL	Pass	6:50pm

Preventive Maintenance
Status: Pass

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County GRANVILLE Instrument Location CREEDMOOR PD

Instrument Serial No. 008641 111 MASONIC ST
CREEDMOOR, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

(1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;

(2) Verify instrument displays time and date;

(3) Initiate breath test sequence;

(4) Enter information as prompted;

(5) Verify instrument accuracy;

(6) When "PLEASE BLOW" appears, collect breath sample;

(7) When "PLEASE BLOW" appears, collect breath sample;

(8) Print test record;

(9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and

(10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 24 day of JUNE, 20 26 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.

E H Bryant
Signature of Certifying Official

17707
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

DHHS 4080 (04/20)

Intox EC/IR-II: Subject Test

GRANVILLE COUNTY CREEDMOOR PD 380

Serial Number: *008641*
Test Date: *06/24/2026*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name: *Bryant, Earl A*
Permit Number: *0017-9707*
Effective:
02/01/2026-02/01/2028

Officer's Name: *NONE, NONE*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG431003
Exp Date: 11/05/2026

Test	g/210L	Time
DIAG	Pass	10:05am
AIR BLK	.00	10:05am
ACCY CHK	.07	10:06am
AIR BLK	.00	10:07am
SUB TEST	**.00**	**10:07am**
AIR BLK	.00	10:08am
SUB TEST	**.00**	**10:10am**
AIR BLK	.00	10:11am

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

GRANVILLE COUNTY CREEDMOOR PD 380

Serial Number: *008641* Test Record Number: *1717*
Test Date: *06/24/2026* Test Time: *10:11am EDT*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	10:12am
FLO	Pass	10:12am
FC	Pass	10:12am

Temperature Tests

Test	Status	Time
FC1	Pass	10:12am
SRC	Pass	10:12am
DET	Pass	10:12am
BAR	Pass	10:12am
BT	Pass	10:12am

Blank Tests

Test	Status	Time
AIR	Pass	10:13am

Printer Tests

Test	Status	Time
PRNT	Pass	10:13am

CRC Tests

Test	Status	Time
COMP	Pass	10:13am
CAL	Pass	10:13am

Preventive Maintenance
Status: Pass

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Greene Instrument Location Greene Co. S.O.

Instrument Serial No. 008588 301 N. Greene St, Snow Hill, N.C.

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

(1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;

(2) Verify instrument displays time and date;

(3) Initiate breath test sequence;

(4) Enter information as prompted;

(5) Verify instrument accuracy;

(6) When "PLEASE BLOW" appears, collect breath sample;

(7) When "PLEASE BLOW" appears, collect breath sample;

(8) Print test record;

(9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and

(10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 26th day of June, 20 26 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.

Signature of Certifying Official

377722
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

DHHS 4080 (04/20)

Intox EC/IR-II: Subject Test

GREENE COUNTY GREENE CO SO 390

Serial Number: *008588*
Test Date: *06/26/2026*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name: *Gray, Kelly D*
Permit Number: *0037-7722*
Effective:
02/01/2026-02/01/2028

Officer's Name: *NONE, NONE*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG431003
Exp Date: 11/05/2026

Test	g/210L	Time
DIAG	Pass	2:53pm
AIR BLK	.00	2:54pm
ACCY CHK	.08	2:54pm
AIR BLK	.00	2:55pm
SUB TEST	**.00**	**2:56pm**
AIR BLK	.00	2:56pm
SUB TEST	**.00**	**2:58pm**
AIR BLK	.00	2:59pm

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

GREENE COUNTY GREENE CO SO 390

Serial Number: *008588* Test Record Number: *1374*
Test Date: *06/26/2026* Test Time: *3:00pm EDT*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	3:01pm
FLO	Pass	3:01pm
FC	Pass	3:01pm

Temperature Tests

Test	Status	Time
FC1	Pass	3:01pm
SRC	Pass	3:01pm
DET	Pass	3:01pm
BAR	Pass	3:01pm
BT	Pass	3:01pm

Blank Tests

Test	Status	Time
AIR	Pass	3:02pm


Printer Tests

Test	Status	Time
PRNT	Pass	3:02pm

CRC Tests

Test	Status	Time
COMP	Pass	3:02pm
CAL	Pass	3:02pm

Preventive Maintenance
Status: Pass



Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD INTOXIMETERS, MODEL INTOX EC/IR II and MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Guilford Instrument Location Greensboro Jail

Instrument Serial No. 008638 Greensboro, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

(1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;

(2) Verify instrument displays time and date;

(3) Initiate breath test sequence;

(4) Enter information as prompted;

(5) Verify instrument accuracy;

(6) When "PLEASE BLOW" appears, collect breath sample;

(7) When "PLEASE BLOW" appears, collect breath sample;

(8) Print test record;

(9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and

(10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 11th day of June, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.

Signature of Certifying Official

509387
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

DHHS 4080 (04/20)

Intox EC/IR-II: Subject Test

GUILFORD COUNTY GREENSBORO JAIL 400

Serial Number: *008638*
Test Date: *06/11/2026*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name: *Long, Thomas A*
Permit Number: *0050-9387*
Effective:
02/01/2026-02/01/2028

Officer's Name: *NONE, NONE*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG602102
Exp Date: 01/21/2028

Test	g/210L	Time
DIAG	Pass	10:14am
AIR BLK	.00	10:15am
ACCY CHK	.07	10:15am
AIR BLK	.00	10:16am
SUB TEST	**.00**	**10:18am**
AIR BLK	.00	10:18am
SUB TEST	**.00**	**10:20am**
AIR BLK	.00	10:21am

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

GUILFORD COUNTY GREENSBORO JAIL 400

Serial Number: *008638* Test Record Number: *7561*
Test Date: *06/11/2026* Test Time: *10:33am EDT*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	10:33am
FLO	Pass	10:33am
FC	Pass	10:33am

Temperature Tests

Test	Status	Time
FC1	Pass	10:33am
SRC	Pass	10:33am
DET	Pass	10:33am
BAR	Pass	10:33am
BT	Pass	10:33am

Blank Tests

Test	Status	Time
AIR	Pass	10:34am

Printer Tests

Test	Status	Time
PRNT	Pass	10:34am

CRC Tests

Test	Status	Time
COMP	Pass	10:34am
CAL	Pass	10:34am

Preventive Maintenance
Status: Pass



Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Guilford Instrument Location Greensboro Police Department

Instrument Serial No. 008125

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

(1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;

(2) Verify instrument displays time and date;

(3) Initiate breath test sequence;

(4) Enter information as prompted;

(5) Verify instrument accuracy;

(6) When "PLEASE BLOW" appears, collect breath sample;

(7) When "PLEASE BLOW" appears, collect breath sample;

(8) Print test record;

(9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and

(10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 11th day of June, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.

Signature of Certifying Official

509387
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

DHHS 4080 (04/20)

Intox EC/IR-II: Subject Test

GUILFORD COUNTY GREENSBORO PD 400

Serial Number: *008725*
Test Date: *06/11/2026*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name: *Long, Thomas A*
Permit Number: *0050-9387*
Effective:
02/01/2026-02/01/2028

Officer's Name: *NONE, NONE*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG431003
Exp Date: 11/05/2026

Test	g/210L	Time
DIAG	Pass	11:54am
AIR BLK	.00	11:54am
ACCY CHK	.07	11:55am
AIR BLK	.00	11:56am
SUB TEST	**.00**	**11:57am**
AIR BLK	.00	11:58am
SUB TEST	**.00**	**12:00pm**
AIR BLK	.00	12:00pm

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

GUILFORD COUNTY GREENSBORO PD 400

Serial Number: *008725* Test Record Number: *4994*
Test Date: *06/11/2026* Test Time: *12:04pm EDT*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	12:04pm
FLO	Pass	12:04pm
FC	Pass	12:04pm

Temperature Tests

Test	Status	Time
FC1	Pass	12:04pm
SRC	Pass	12:04pm
DET	Pass	12:04pm
BAR	Pass	12:04pm
BT	Pass	12:04pm

Blank Tests

Test	Status	Time
AIR	Pass	12:05pm

Printer Tests

Test	Status	Time
PRNT	Pass	12:05pm

CRC Tests

Test	Status	Time
COMP	Pass	12:05pm
CAL	Pass	12:05pm

Preventive Maintenance
Status: Pass

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD INTOXIMETERS, MODEL INTOX EC/IR II and MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Guilford Instrument Location Greensboro Jail

Instrument Serial No. 008790 Greensboro, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

(1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;

(2) Verify instrument displays time and date;

(3) Initiate breath test sequence;

(4) Enter information as prompted;

(5) Verify instrument accuracy;

(6) When "PLEASE BLOW" appears, collect breath sample;

(7) When "PLEASE BLOW" appears, collect breath sample;

(8) Print test record;

(9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and

(10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 11th day of June, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.

Signature of Certifying Official

509387
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

DHHS 4080 (04/20)

Intox EC/IR-II: Subject Test

GUILFORD COUNTY GREENSBORO JAIL 400

Serial Number: *008790*
Test Date: *06/11/2026*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name: *Long, Thomas A*
Permit Number: *0050-9387*
Effective:
02/01/2026-02/01/2028

Officer's Name: *NONE, NONE*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG602102
Exp Date: 01/21/2028

Test	g/210L	Time
DIAG	Pass	10:17am
AIR BLK	.00	10:18am
ACCY CHK	.07	10:19am
AIR BLK	.00	10:20am
SUB TEST	**.00**	**10:21am**
AIR BLK	.00	10:22am
SUB TEST	**.00**	**10:23am**
AIR BLK	.00	10:24am

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

GUILFORD COUNTY GREENSBORO JAIL 400

Serial Number: *008790* Test Record Number: *8822*
Test Date: *06/11/2026* Test Time: *10:29am EDT*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	10:29am
FLO	Pass	10:29am
FC	Pass	10:29am

Temperature Tests

Test	Status	Time
FC1	Pass	10:29am
SRC	Pass	10:29am
DET	Pass	10:29am
BAR	Pass	10:29am
BT	Pass	10:29am

Blank Tests

Test	Status	Time
AIR	Pass	10:30am

Printer Tests

Test	Status	Time
PRNT	Pass	10:30am

CRC Tests

Test	Status	Time
COMP	Pass	10:30am
CAL	Pass	10:30am

Preventive Maintenance
Status: Pass

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD INTOXIMETERS, MODEL INTOX EC/IR II and MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Guilford Instrument Location Greensboro Jail

Instrument Serial No. 008794 Greensboro, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

(1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;

(2) Verify instrument displays time and date;

(3) Initiate breath test sequence;

(4) Enter information as prompted;

(5) Verify instrument accuracy;

(6) When "PLEASE BLOW" appears, collect breath sample;

(7) When "PLEASE BLOW" appears, collect breath sample;

(8) Print test record;

(9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and

(10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 11th day of June, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.

Signature of Certifying Official

509387
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

DHHS 4080 (04/20)

Intox EC/IR-II: Subject Test

GUILFORD COUNTY GREENSBORO JAIL 400

Serial Number: *008794*
Test Date: *06/11/2026*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name: *Long, Thomas A*
Permit Number: *0050-9387*
Effective:
02/01/2026-02/01/2028

Officer's Name: *NONE, NONE*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG602102
Exp Date: 01/21/2028

Test	g/210L	Time
DIAG	Pass	10:15am
AIR BLK	.00	10:16am
ACCY CHK	.07	10:17am
AIR BLK	.00	10:18am
SUB TEST	**.00**	**10:19am**
AIR BLK	.00	10:20am
SUB TEST	**.00**	**10:22am**
AIR BLK	.00	10:23am

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

GUILFORD COUNTY GREENSBORO JAIL 400

Serial Number: *008794* Test Record Number: *9380*
Test Date: *06/11/2026* Test Time: *10:28am EDT*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	10:28am
FLO	Pass	10:28am
FC	Pass	10:28am

Temperature Tests

Test	Status	Time
FC1	Pass	10:28am
SRC	Pass	10:28am
DET	Pass	10:28am
BAR	Pass	10:28am
BT	Pass	10:28am

Blank Tests

Test	Status	Time
AIR	Pass	10:29am

Printer Tests

Test	Status	Time
PRNT	Pass	10:29am

CRC Tests

Test	Status	Time
COMP	Pass	10:29am
CAL	Pass	10:29am

Preventive Maintenance
Status: Pass

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Guilford Instrument Location BAT Mobile Unit 13

Instrument Serial No. 008869

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

(1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;

(2) Verify instrument displays time and date;

(3) Initiate breath test sequence;

(4) Enter information as prompted;

(5) Verify instrument accuracy;

(6) When "PLEASE BLOW" appears, collect breath sample;

(7) When "PLEASE BLOW" appears, collect breath sample;

(8) Print test record;

(9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and

(10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 12th day of June, 20 26 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.

Signature of Certifying Official

307699
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

DHHS 4080 (04/20)

Intox EC/IR-II: Subject Test

GUILFORD COUNTY BAT MOBILE UNIT 13 400

Serial Number: *008869*
Test Date: *06/12/2026*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name: *Whitehurst, Timothy B*
Permit Number: *0030-7699*
Effective:
03/01/2026-03/01/2028

Officer's Name: *NONE, NONE*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG506303
Exp Date: 03/04/2027

Test	g/210L	Time
DIAG	Pass	8:34am
AIR BLK	.00	8:35am
ACCY CHK	.08	8:35am
AIR BLK	.00	8:36am
SUB TEST	**.00**	**8:37am**
AIR BLK	.00	8:38am
SUB TEST	**.00**	**8:39am**
AIR BLK	.00	8:40am

Reported AC: .00 g/210L

Timothy B Whitehurst
Signature of Chemical Analyst

Court CVR

Timothy B Whitehurst
Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

GUILFORD COUNTY BAT MOBILE UNIT 13 400

Serial Number: *008869* Test Record Number: *2219*
Test Date: *06/12/2026* Test Time: *8:42am EDT*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	8:42am
FLO	Pass	8:42am
FC	Pass	8:43am

Temperature Tests

Test	Status	Time
FC1	Pass	8:43am
SRC	Pass	8:43am
DET	Pass	8:43am
BAR	Pass	8:43am
BT	Pass	8:43am

Blank Tests

Test	Status	Time
AIR	Pass	8:43am

Printer Tests

Test	Status	Time
PRNT	Pass	8:43am

CRC Tests

Test	Status	Time
COMP	Pass	8:44am
CAL	Pass	8:44am

Preventive Maintenance
Status: Pass

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Guilford Instrument Location BAT Mobile Unit 13

Instrument Serial No. 008869

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

(1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;

(2) Verify instrument displays time and date;

(3) Initiate breath test sequence;

(4) Enter information as prompted;

(5) Verify instrument accuracy;

(6) When "PLEASE BLOW" appears, collect breath sample;

(7) When "PLEASE BLOW" appears, collect breath sample;

(8) Print test record;

(9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and

(10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 18th day of June, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.

THE GREAT SEAL OF THE STATE OF NORTH CAROLINA

John Lanier
Signature of Certifying Official

1604930
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

DHHS 4080 (04/20)

Intox EC/IR-II: Subject Test

GUILFORD COUNTY BAT MOBILE UNIT 13 400

Serial Number: *008869*
Test Date: *06/18/2026*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name: *Lanier Jr., John P*
Permit Number: *4582-9118*
Effective:
02/01/2026-02/01/2028

Officer's Name: *NONE, NONE*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG506303
Exp Date: 03/04/2027

Test	g/210L	Time
DIAG	Pass	9:04pm
AIR BLK	.00	9:05pm
ACCY CHK	.08	9:06pm
AIR BLK	.00	9:06pm
SUB TEST	**.00**	**9:07pm**
AIR BLK	.00	9:08pm
SUB TEST	**.00**	**9:10pm**
AIR BLK	.00	9:11pm

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

GUILFORD COUNTY BAT MOBILE UNIT 13 400

Serial Number: *008869* Test Record Number: *2222*
Test Date: *06/18/2026* Test Time: *9:12pm EDT*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	9:13pm
FLO	Pass	9:13pm
FC	Pass	9:13pm

Temperature Tests

Test	Status	Time
FC1	Pass	9:13pm
SRC	Pass	9:13pm
DET	Pass	9:13pm
BAR	Pass	9:13pm
BT	Pass	9:13pm

Blank Tests

Test	Status	Time
AIR	Pass	9:14pm


Printer Tests

Test	Status	Time
PRNT	Pass	9:14pm

CRC Tests

Test	Status	Time
COMP	Pass	9:14pm
CAL	Pass	9:14pm

Preventive Maintenance
Status: Pass

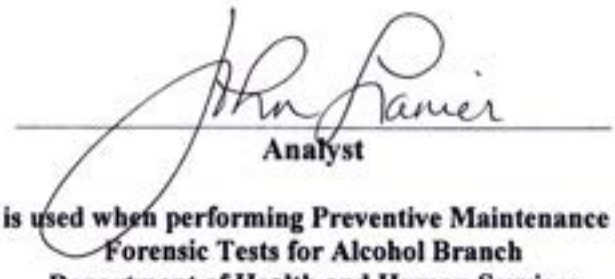

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Guilford Instrument Location BAT Mobile Unit 13

Instrument Serial No. D08898

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

(1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;

(2) Verify instrument displays time and date;

(3) Initiate breath test sequence;

(4) Enter information as prompted;

(5) Verify instrument accuracy;

(6) When "PLEASE BLOW" appears, collect breath sample;

(7) When "PLEASE BLOW" appears, collect breath sample;

(8) Print test record;

(9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and

(10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 12th day of June, 2024 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.

Timothy B White — Signature of Certifying Official

307699 — Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

DHHS 4080 (04/20)

Intox EC/IR-II: Subject Test

GUILFORD COUNTY BAT MOBILE UNIT 13 400

Serial Number: *008898*
Test Date: *06/12/2026*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name: *Whitehurst, Timothy B*
Permit Number: *0030-7699*
Effective:
03/01/2026-03/01/2028

Officer's Name: *NONE, NONE*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG506302
Exp Date: 03/04/2027

Test	g/210L	Time
DIAG	Pass	8:19am
AIR BLK	.00	8:20am
ACCY CHK	.07	8:20am
AIR BLK	.00	8:21am
SUB TEST	**.00**	**8:22am**
AIR BLK	.00	8:23am
SUB TEST	**.00**	**8:24am**
AIR BLK	.00	8:25am

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

GUILFORD COUNTY BAT MOBILE UNIT 13 400

Serial Number: *008898* Test Record Number: *2160*
Test Date: *06/12/2026* Test Time: *8:26am EDT*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	8:26am
FLO	Pass	8:26am
FC	Pass	8:26am

Temperature Tests

Test	Status	Time
FC1	Pass	8:26am
SRC	Pass	8:26am
DET	Pass	8:26am
BAR	Pass	8:26am
BT	Pass	8:26am

Blank Tests

Test	Status	Time
AIR	Pass	8:27am

Printer Tests

Test	Status	Time
PRNT	Pass	8:27am

CRC Tests

Test	Status	Time
COMP	Pass	8:27am
CAL	Pass	8:27am

Preventive Maintenance
Status: Pass

Tony B Watts
Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Guilford Instrument Location BAT Mobile Unit 13

Instrument Serial No. 008898

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

(1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;

(2) Verify instrument displays time and date;

(3) Initiate breath test sequence;

(4) Enter information as prompted;

(5) Verify instrument accuracy;

(6) When "PLEASE BLOW" appears, collect breath sample;

(7) When "PLEASE BLOW" appears, collect breath sample;

(8) Print test record;

(9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and

(10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 18th day of June, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.

Signature of Certifying Official

1604930
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

DHHS 4080 (04/20)

Intox EC/IR-II: Subject Test

GUILFORD COUNTY BAT MOBILE UNIT 13 400

Serial Number: *008898*
Test Date: *06/18/2026*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name: *Lanier Jr., John P*
Permit Number: *4582-9118*
Effective:
02/01/2026-02/01/2028

Officer's Name: *NONE, NONE*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG506302
Exp Date: 03/04/2027

Test	g/210L	Time
DIAG	Pass	9:03pm
AIR BLK	.00	9:04pm
ACCY CHK	.07	9:05pm
AIR BLK	.00	9:05pm
SUB TEST	**.00**	**9:07pm**
AIR BLK	.00	9:08pm
SUB TEST	**.00**	**9:09pm**
AIR BLK	.00	9:10pm

Reported AC: .00 g/210L

John Lanier
Signature of Chemical Analyst

Court CVR

John Lanier
Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

GUILFORD COUNTY BAT MOBILE UNIT 13 400

Serial Number: *008898* Test Record Number: *2162*
Test Date: *06/18/2026* Test Time: *9:12pm EDT*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	9:12pm
FLO	Pass	9:12pm
FC	Pass	9:12pm

Temperature Tests

Test	Status	Time
FC1	Pass	9:12pm
SRC	Pass	9:12pm
DET	Pass	9:12pm
BAR	Pass	9:12pm
BT	Pass	9:12pm

Blank Tests

Test	Status	Time
AIR	Pass	9:13pm


Printer Tests

Test	Status	Time
PRNT	Pass	9:13pm

CRC Tests

Test	Status	Time
COMP	Pass	9:13pm
CAL	Pass	9:13pm

Preventive Maintenance
Status: Pass

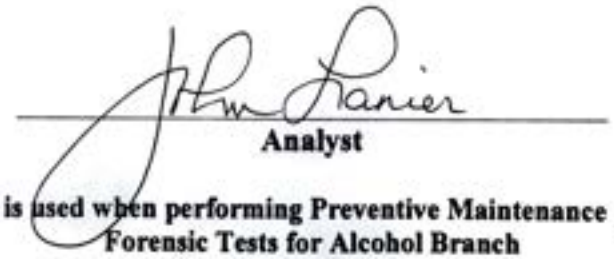

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Guilford Instrument Location BAT Mobile Unit 13

Instrument Serial No. 008939

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

(1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;

(2) Verify instrument displays time and date;

(3) Initiate breath test sequence;

(4) Enter information as prompted;

(5) Verify instrument accuracy;

(6) When "PLEASE BLOW" appears, collect breath sample;

(7) When "PLEASE BLOW" appears, collect breath sample;

(8) Print test record;

(9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and

(10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 12th day of June, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.

Signature of Certifying Official

307699
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

DHHS 4080 (04/20)

Intox EC/IR-II: Subject Test

GUILFORD COUNTY BAT MOBILE UNIT 13 400

Serial Number: *008939*
Test Date: *06/12/2026*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name: *Whitehurst, Timothy B*
Permit Number: *0030-7699*
Effective:
03/01/2026-03/01/2028

Officer's Name: *NONE, NONE*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG506302
Exp Date: 03/04/2027

Test	g/210L	Time
DIAG	Pass	7:56am
AIR BLK	.00	7:57am
ACCY CHK	.07	7:58am
AIR BLK	.00	7:59am
SUB TEST	**.00**	**7:59am**
AIR BLK	.00	8:00am
SUB TEST	**.00**	**8:02am**
AIR BLK	.00	8:03am

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

GUILFORD COUNTY BAT MOBILE UNIT 13 400

Serial Number: *008939* Test Record Number: *2020*
Test Date: *06/12/2026* Test Time: *8:07am EDT*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	8:08am
FLO	Pass	8:08am
FC	Pass	8:08am

Temperature Tests

Test	Status	Time
FC1	Pass	8:08am
SRC	Pass	8:08am
DET	Pass	8:08am
BAR	Pass	8:08am
BT	Pass	8:08am

Blank Tests

Test	Status	Time
AIR	Pass	8:09am

Printer Tests

Test	Status	Time
PRNT	Pass	8:09am

CRC Tests

Test	Status	Time
COMP	Pass	8:09am
CAL	Pass	8:09am

Preventive Maintenance
Status: Pass

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Guilford Instrument Location BFT Mobile Unit 13

Instrument Serial No. 008939

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

(1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;

(2) Verify instrument displays time and date;

(3) Initiate breath test sequence;

(4) Enter information as prompted;

(5) Verify instrument accuracy;

(6) When "PLEASE BLOW" appears, collect breath sample;

(7) When "PLEASE BLOW" appears, collect breath sample;

(8) Print test record;

(9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and

(10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 18th day of June, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.

Signature of Certifying Official

1604930
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

DHHS 4080 (04/20)

Intox EC/IR-II: Subject Test

GUILFORD COUNTY BAT MOBILE UNIT 13 400

Serial Number: *008939*
Test Date: *06/18/2026*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name: *Lanier Jr., John P*
Permit Number: *4582-9118*
Effective:
02/01/2026-02/01/2028

Officer's Name: *NONE, NONE*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG506302
Exp Date: 03/04/2027

Test	g/210L	Time
DIAG	Pass	9:06pm
AIR BLK	.00	9:07pm
ACCY CHK	.07	9:08pm
AIR BLK	.00	9:09pm
SUB TEST	**.00**	**9:09pm**
AIR BLK	.00	9:10pm
SUB TEST	**.00**	**9:12pm**
AIR BLK	.00	9:13pm

Reported AC: .00 g/210L

John Lanier

Signature of Chemical Analyst

Court CVR

John Lanier

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

GUILFORD COUNTY BAT MOBILE UNIT 13 400

Serial Number: *008939* Test Record Number: *2022*
Test Date: *06/18/2026* Test Time: *9:14pm EDT*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	9:15pm
FLO	Pass	9:15pm
FC	Pass	9:15pm

Temperature Tests

Test	Status	Time
FC1	Pass	9:15pm
SRC	Pass	9:15pm
DET	Pass	9:15pm
BAR	Pass	9:15pm
BT	Pass	9:15pm

Blank Tests

Test	Status	Time
AIR	Pass	9:16pm

Printer Tests

Test	Status	Time
PRNT	Pass	9:16pm

CRC Tests

Test	Status	Time
COMP	Pass	9:16pm
CAL	Pass	9:16pm

Preventive Maintenance
Status: Pass

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County HALIFAX Instrument Location ROANOKE RAPIDS POLICE DEPT.

Instrument Serial No. 008656 1040 ROANOKE AVE
ROANOKE RAPIDS, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

(1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;

(2) Verify instrument displays time and date;

(3) Initiate breath test sequence;

(4) Enter information as prompted;

(5) Verify instrument accuracy;

(6) When "PLEASE BLOW" appears, collect breath sample;

(7) When "PLEASE BLOW" appears, collect breath sample;

(8) Print test record;

(9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and

(10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 22 day of JUNE, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.

Signature of Certifying Official

179707
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

DHHS 4080 (04/20)

Intox EC/IR-II: Subject Test

HALIFAX CO. ROANOKE RAPIDS PD 410

Serial Number: *008656*
Test Date: *06/22/2026*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name: *Bryant, Earl A*
Permit Number: *0017-9707*
Effective:
02/01/2026-02/01/2028

Officer's Name: *NONE, NONE*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG534301
Exp Date: 12/09/2027

Test	g/210L	Time
DIAG	Pass	10:48am
AIR BLK	.00	10:49am
ACCY CHK	.07	10:49am
AIR BLK	.00	10:50am
SUB TEST	**.00**	**10:51am**
AIR BLK	.00	10:52am
SUB TEST	**.00**	**10:54am**
AIR BLK	.00	10:54am

Reported AC: .00 g/210L

E A Bryant

Signature of Chemical Analyst

Court CVR

E A Bryant

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

HALIFAX CO. ROANOKE RAPIDS PD 410

Serial Number: *008656* Test Record Number: *1243*
Test Date: *06/22/2026* Test Time: *10:56am EDT*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	10:56am
FLO	Pass	10:56am
FC	Pass	10:56am

Temperature Tests

Test	Status	Time
FC1	Pass	10:56am
SRC	Pass	10:56am
DET	Pass	10:56am
BAR	Pass	10:56am
BT	Pass	10:56am

Blank Tests

Test	Status	Time
AIR	Pass	10:57am

Printer Tests

Test	Status	Time
PRNT	Pass	10:57am

CRC Tests

Test	Status	Time
COMP	Pass	10:57am
CAL	Pass	10:57am

Preventive Maintenance
Status: Pass

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County HALIFAX Instrument Location HALIFAX CO. S.O.

Instrument Serial No. 008695 355 FERRELL LANE HALIFAX, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

(1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;

(2) Verify instrument displays time and date;

(3) Initiate breath test sequence;

(4) Enter information as prompted;

(5) Verify instrument accuracy;

(6) When "PLEASE BLOW" appears, collect breath sample;

(7) When "PLEASE BLOW" appears, collect breath sample;

(8) Print test record;

(9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and

(10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 17 day of JUNE, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.

Signature of Certifying Official

179707
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

DHHS 4080 (04/20)

Intox EC/IR-II: Subject Test

HALIFAX CO. HALIFAX CO SO 410

Serial Number: *008695*
Test Date: *06/17/2026*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name: *Bryant, Earl A*
Permit Number: *0017-9707*
Effective:
02/01/2026-02/01/2028

Officer's Name: *NONE, NONE*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG534301
Exp Date: 12/09/2027

Test	g/210L	Time
DIAG	Pass	5:03pm
AIR BLK	.00	5:03pm
ACCY CHK	.07	5:04pm
AIR BLK	.00	5:05pm
SUB TEST	**.00**	**5:06pm**
AIR BLK	.00	5:07pm
SUB TEST	**.00**	**5:08pm**
AIR BLK	.00	5:09pm

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

HALIFAX CO. HALIFAX CO SO 410

Serial Number: *008695* Test Record Number: *4105*
Test Date: *06/17/2026* Test Time: *5:10pm EDT*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	5:11pm
FLO	Pass	5:11pm
FC	Pass	5:11pm

Temperature Tests

Test	Status	Time
FC1	Pass	5:11pm
SRC	Pass	5:11pm
DET	Pass	5:11pm
BAR	Pass	5:11pm
BT	Pass	5:11pm

Blank Tests

Test	Status	Time
AIR	Pass	5:12pm

Printer Tests

Test	Status	Time
PRNT	Pass	5:12pm

CRC Tests

Test	Status	Time
COMP	Pass	5:12pm
CAL	Pass	5:12pm

Preventive Maintenance
Status: Pass

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Harnett Instrument Location Harnett County Detention Center

Instrument Serial No. 008728

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

(1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;

(2) Verify instrument displays time and date;

(3) Initiate breath test sequence;

(4) Enter information as prompted;

(5) Verify instrument accuracy;

(6) When "PLEASE BLOW" appears, collect breath sample;

(7) When "PLEASE BLOW" appears, collect breath sample;

(8) Print test record;

(9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and

(10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 4 day of June, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.

Signature of Certifying Official

365156
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

HARNETT COUNTY DETENTION CENTER 420

Serial Number: *008728*
Test Date: *06/04/2026*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name: *Garner, Joel K*
Permit Number: *0036-5156*
Effective:
02/01/2026-02/01/2028

Officer's Name: *NONE, NONE*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG534301
Exp Date: 12/09/2027

Test	g/210L	Time
DIAG	Pass	9:42am
AIR BLK	.00	9:42am
ACCY CHK	.08	9:43am
AIR BLK	.00	9:44am
SUB TEST	**.00**	**9:44am**
AIR BLK	.00	9:45am
SUB TEST	**.00**	**9:47am**
AIR BLK	.00	9:48am

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

HARNETT COUNTY DETENTION CENTER 420

Serial Number: *008728* Test Record Number: *592*
Test Date: *06/04/2026* Test Time: *9:48am EDT*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	9:49am
FLO	Pass	9:49am
FC	Pass	9:49am

Temperature Tests

Test	Status	Time
FC1	Pass	9:49am
SRC	Pass	9:49am
DET	Pass	9:49am
BAR	Pass	9:49am
BT	Pass	9:49am

Blank Tests

Test	Status	Time
AIR	Pass	9:49am


Printer Tests

Test	Status	Time
PRNT	Pass	9:49am

CRC Tests

Test	Status	Time
COMP	Pass	9:50am
CAL	Pass	9:50am

Preventive Maintenance
Status: Pass

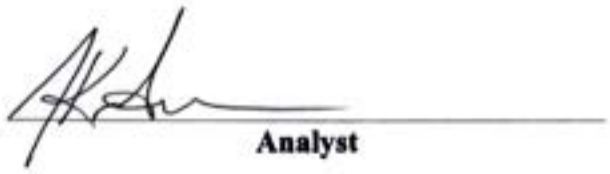

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Haywood Instrument Location Haywood Co. Jail

Instrument Serial No. 008712 Waynesville, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

(1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;

(2) Verify instrument displays time and date;

(3) Initiate breath test sequence;

(4) Enter information as prompted;

(5) Verify instrument accuracy;

(6) When "PLEASE BLOW" appears, collect breath sample;

(7) When "PLEASE BLOW" appears, collect breath sample;

(8) Print test record;

(9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and

(10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 4th day of June, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.

THE GREAT SEAL OF THE STATE OF NORTH CAROLINA

Signature of Certifying Official

843310
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

HAYWOOD COUNTY JAIL 430

Serial Number: *008712*
Test Date: *06/04/2026*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name: *Cutler, Daniel R*
Permit Number: *0084-3310*
Effective:
02/01/2026-02/01/2028

Officer's Name: *NONE, NONE*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG505001
Exp Date: 02/19/2027

Test	g/210L	Time
DIAG	Pass	11:55am
AIR BLK	.00	11:56am
ACCY CHK	.07	11:57am
AIR BLK	.00	11:58am
SUB TEST	**.00**	**11:59am**
AIR BLK	.00	12:00pm
SUB TEST	**.00**	**12:01pm**
AIR BLK	.00	12:02pm

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

HAYWOOD COUNTY JAIL 430

Serial Number: *008712* Test Record Number: *2572*
Test Date: *06/04/2026* Test Time: *12:02pm EDT*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	12:03pm
FLO	Pass	12:03pm
FC	Pass	12:03pm

Temperature Tests

Test	Status	Time
FC1	Pass	12:03pm
SRC	Pass	12:03pm
DET	Pass	12:03pm
BAR	Pass	12:03pm
BT	Pass	12:03pm

Blank Tests

Test	Status	Time
AIR	Pass	12:04pm


Printer Tests

Test	Status	Time
PRNT	Pass	12:04pm

CRC Tests

Test	Status	Time
COMP	Pass	12:04pm
CAL	Pass	12:04pm

Preventive Maintenance
Status: Pass

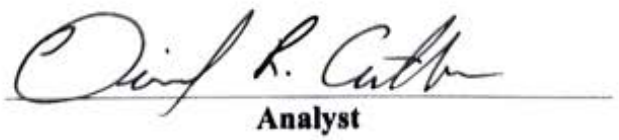

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Haywood Instrument Location Haywood Co. Jail

Instrument Serial No. 008714 Waynesville, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

(1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;

(2) Verify instrument displays time and date;

(3) Initiate breath test sequence;

(4) Enter information as prompted;

(5) Verify instrument accuracy;

(6) When "PLEASE BLOW" appears, collect breath sample;

(7) When "PLEASE BLOW" appears, collect breath sample;

(8) Print test record;

(9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and

(10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 4th day of June, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.

THE GREAT SEAL OF THE STATE OF NORTH CAROLINA

Chad R. Cuthbertson — Signature of Certifying Official

843310 — Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

HAYWOOD COUNTY HAYWOOD COUNTY JAIL 430

Serial Number: *008714*
Test Date: *06/04/2026*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name: *Cutler, Daniel R*
Permit Number: *0084-3310*
Effective:
02/01/2026-02/01/2028

Officer's Name: *NONE, NONE*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG534301
Exp Date: 12/09/2027

Test	g/210L	Time
DIAG	Pass	11:44am
AIR BLK	.00	11:44am
ACCY CHK	.08	11:45am
AIR BLK	.00	11:46am
SUB TEST	**.00**	**11:47am**
AIR BLK	.00	11:48am
SUB TEST	**.00**	**11:49am**
AIR BLK	.00	11:50am

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

HAYWOOD COUNTY HAYWOOD COUNTY JAIL 430

Serial Number: *008714* Test Record Number: *2624*
Test Date: *06/04/2026* Test Time: *11:51am EDT*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	11:52am
FLO	Pass	11:52am
FC	Pass	11:52am

Temperature Tests

Test	Status	Time
FC1	Pass	11:52am
SRC	Pass	11:52am
DET	Pass	11:52am
BAR	Pass	11:52am
BT	Pass	11:52am

Blank Tests

Test	Status	Time
AIR	Pass	11:53am


Printer Tests

Test	Status	Time
PRNT	Pass	11:53am

CRC Tests

Test	Status	Time
COMP	Pass	11:53am
CAL	Pass	11:53am

Preventive Maintenance
Status: Pass

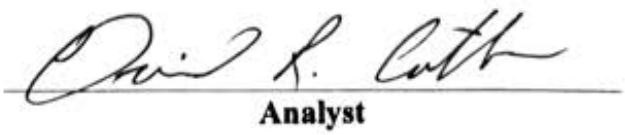

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Hyde Instrument Location Hyde Co. S.O. - Ocracoke

Instrument Serial No. 008797 NC 12, Ocracoke, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

(1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;

(2) Verify instrument displays time and date;

(3) Initiate breath test sequence;

(4) Enter information as prompted;

(5) Verify instrument accuracy;

(6) When "PLEASE BLOW" appears, collect breath sample;

(7) When "PLEASE BLOW" appears, collect breath sample;

(8) Print test record;

(9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and

(10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 16th day of June, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.

Signature of Certifying Official

206272
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

HYDE COUNTY HYDE CO SO OCRACOKE 470

Serial Number: *008797*
Test Date: *06/16/2026*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name: *Chappell, Mark A*
Permit Number: *0020-6272*
Effective:
02/01/2026-02/01/2028

Officer's Name: *NONE, NONE*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG516203
Exp Date: 06/11/2027

Test	g/210L	Time
DIAG	Pass	11:25am
AIR BLK	.00	11:26am
ACCY CHK	.07	11:27am
AIR BLK	.00	11:28am
SUB TEST	**.00**	**11:29am**
AIR BLK	.00	11:30am
SUB TEST	**.00**	**11:32am**
AIR BLK	.00	11:33am

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

HYDE COUNTY HYDE CO SO OCRACOKE 470

Serial Number: *008797* Test Record Number: *775*
Test Date: *06/16/2026* Test Time: *11:35am EDT*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	11:36am
FLO	Pass	11:36am
FC	Pass	11:36am

Temperature Tests

Test	Status	Time
FC1	Pass	11:36am
SRC	Pass	11:36am
DET	Pass	11:36am
BAR	Pass	11:36am
BT	Pass	11:36am

Blank Tests

Test	Status	Time
AIR	Pass	11:36am

Printer Tests

Test	Status	Time
PRNT	Pass	11:37am

CRC Tests

Test	Status	Time
COMP	Pass	11:37am
CAL	Pass	11:37am

Preventive Maintenance
Status: Pass

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Iredell Instrument Location BAT Mobile Unit 8

Instrument Serial No. 008615

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

(1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;

(2) Verify instrument displays time and date;

(3) Initiate breath test sequence;

(4) Enter information as prompted;

(5) Verify instrument accuracy;

(6) When "PLEASE BLOW" appears, collect breath sample;

(7) When "PLEASE BLOW" appears, collect breath sample;

(8) Print test record;

(9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and

(10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 12 day of June, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.

THE GREAT SEAL OF THE STATE OF NORTH CAROLINA

Signature of Certifying Official

2219283
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

IREDELL COUNTY BAT MOBILE UNIT 8 480

Serial Number: *008615*
Test Date: *06/12/2026*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name: *Glasscock, Jerry D*
Permit Number: *7180-9235*
Effective:
02/01/2026-02/01/2028

Officer's Name: *NONE, NONE*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG506303
Exp Date: 03/04/2027

Test	g/210L	Time
DIAG	Pass	9:47pm
AIR BLK	.00	9:48pm
ACCY CHK	.07	9:48pm
AIR BLK	.00	9:49pm
SUB TEST	**.00**	**9:50pm**
AIR BLK	.00	9:51pm
SUB TEST	**.00**	**9:52pm**
AIR BLK	.00	9:53pm

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

IREDELL COUNTY BAT MOBILE UNIT 8 480

Serial Number: *008615* Test Record Number: *6334*
Test Date: *06/12/2026* Test Time: *9:53pm EDT*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	9:54pm
FLO	Pass	9:54pm
FC	Pass	9:54pm

Temperature Tests

Test	Status	Time
FC1	Pass	9:54pm
SRC	Pass	9:54pm
DET	Pass	9:54pm
BAR	Pass	9:54pm
BT	Pass	9:54pm

Blank Tests

Test	Status	Time
AIR	Pass	9:55pm

Printer Tests

Test	Status	Time
PRNT	Pass	9:55pm

CRC Tests

Test	Status	Time
COMP	Pass	9:55pm
CAL	Pass	9:55pm

Preventive Maintenance
Status: Pass

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County IREDELL Instrument Location MOORESVILLE PD

Instrument Serial No. 008183 MOORESVILLE NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

(1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;

(2) Verify instrument displays time and date;

(3) Initiate breath test sequence;

(4) Enter information as prompted;

(5) Verify instrument accuracy;

(6) When "PLEASE BLOW" appears, collect breath sample;

(7) When "PLEASE BLOW" appears, collect breath sample;

(8) Print test record;

(9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and

(10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 10 day of June, 2020 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.

Signature of Certifying Official

274970
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

DHHS 4080 (04/20)

Intox EC/IR-II: Subject Test

IREDELL COUNTY MOORESVILLE PD 480

Serial Number: *008685*
Test Date: *06/10/2026*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name: *Fleming, Tina S*
Permit Number: *0027-4970*
Effective:
02/01/2025-02/01/2027

Officer's Name: *NONE, NONE*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG506302
Exp Date: 03/04/2027

Test	g/210L	Time
DIAG	Pass	12:01pm
AIR BLK	.00	12:02pm
ACCY CHK	.08	12:02pm
AIR BLK	.00	12:04pm
SUB TEST	**.00**	**12:05pm**
AIR BLK	.00	12:06pm
SUB TEST	**.00**	**12:08pm**
AIR BLK	.00	12:08pm

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

IREDELL COUNTY MOORESVILLE PD 480

Serial Number: *008685* Test Record Number: *5262*
Test Date: *06/10/2026* Test Time: *12:15pm EDT*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	12:16pm
FLO	Pass	12:16pm
FC	Pass	12:16pm

Temperature Tests

Test	Status	Time
FC1	Pass	12:16pm
SRC	Pass	12:16pm
DET	Pass	12:16pm
BAR	Pass	12:16pm
BT	Pass	12:16pm

Blank Tests

Test	Status	Time
AIR	Pass	12:17pm

Printer Tests

Test	Status	Time
PRNT	Pass	12:17pm

CRC Tests

Test	Status	Time
COMP	Pass	12:17pm
CAL	Pass	12:17pm

Preventive Maintenance
Status: Pass

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Iredell Instrument Location BAT Mobile Unit 8

Instrument Serial No. 008736

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

(1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;

(2) Verify instrument displays time and date;

(3) Initiate breath test sequence;

(4) Enter information as prompted;

(5) Verify instrument accuracy;

(6) When "PLEASE BLOW" appears, collect breath sample;

(7) When "PLEASE BLOW" appears, collect breath sample;

(8) Print test record;

(9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and

(10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 12 day of June, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.

Signature of Certifying Official

2219283
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

IREDELL COUNTY BAT MOBILE UNIT 8 480

Serial Number: *008736*
Test Date: *06/12/2026*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name: *Glasscock, Jerry D*
Permit Number: *7180-9235*
Effective:
02/01/2026-02/01/2028

Officer's Name: *NONE, NONE*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG506303
Exp Date: 03/04/2027

Test	g/210L	Time
DIAG	Pass	9:45pm
AIR BLK	.00	9:46pm
ACCY CHK	.07	9:47pm
AIR BLK	.00	9:48pm
SUB TEST	**.00**	**9:48pm**
AIR BLK	.00	9:49pm
SUB TEST	**.00**	**9:51pm**
AIR BLK	.00	9:52pm

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

IREDELL COUNTY BAT MOBILE UNIT 8 480

Serial Number: *008736* Test Record Number: *1690*
Test Date: *06/12/2026* Test Time: *9:52pm EDT*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	9:53pm
FLO	Pass	9:53pm
FC	Pass	9:53pm

Temperature Tests

Test	Status	Time
FC1	Pass	9:53pm
SRC	Pass	9:53pm
DET	Pass	9:53pm
BAR	Pass	9:53pm
BT	Pass	9:53pm

Blank Tests

Test	Status	Time
AIR	Pass	9:54pm

Printer Tests

Test	Status	Time
PRNT	Pass	9:54pm

CRC Tests

Test	Status	Time
COMP	Pass	9:54pm
CAL	Pass	9:54pm

Preventive Maintenance
Status: Pass

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Iredell Instrument Location BAT Mobile Unit 8

Instrument Serial No. 008775

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

(1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;

(2) Verify instrument displays time and date;

(3) Initiate breath test sequence;

(4) Enter information as prompted;

(5) Verify instrument accuracy;

(6) When "PLEASE BLOW" appears, collect breath sample;

(7) When "PLEASE BLOW" appears, collect breath sample;

(8) Print test record;

(9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and

(10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 12 day of June, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.

Signature of Certifying Official

2219283
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

IREDELL COUNTY BAT MOBILE UNIT 8 480

Serial Number: *008775*
Test Date: *06/12/2026*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name: *Glasscock, Jerry D*
Permit Number: *7180-9235*
Effective:
02/01/2026-02/01/2028

Officer's Name: *NONE, NONE*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG506303
Exp Date: 03/04/2027

Test	g/210L	Time
DIAG	Pass	9:44pm
AIR BLK	.00	9:45pm
ACCY CHK	.08	9:46pm
AIR BLK	.00	9:47pm
SUB TEST	**.00**	**9:47pm**
AIR BLK	.00	9:48pm
SUB TEST	**.00**	**9:50pm**
AIR BLK	.00	9:51pm

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

IREDELL COUNTY BAT MOBILE UNIT 8 480

Serial Number: *008775* Test Record Number: *2540*
Test Date: *06/12/2026* Test Time: *9:51pm EDT*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	9:51pm
FLO	Pass	9:51pm
FC	Pass	9:52pm

Temperature Tests

Test	Status	Time
FC1	Pass	9:52pm
SRC	Pass	9:52pm
DET	Pass	9:52pm
BAR	Pass	9:52pm
BT	Pass	9:52pm

Blank Tests

Test	Status	Time
AIR	Pass	9:52pm

Printer Tests

Test	Status	Time
PRNT	Pass	9:52pm

CRC Tests

Test	Status	Time
COMP	Pass	9:52pm
CAL	Pass	9:52pm

Preventive Maintenance
Status: Pass

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Iredell Instrument Location BAT Mobile Unit 8

Instrument Serial No. 008816

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

(1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;

(2) Verify instrument displays time and date;

(3) Initiate breath test sequence;

(4) Enter information as prompted;

(5) Verify instrument accuracy;

(6) When "PLEASE BLOW" appears, collect breath sample;

(7) When "PLEASE BLOW" appears, collect breath sample;

(8) Print test record;

(9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and

(10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 12 day of June, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.

Signature of Certifying Official

2219283
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

IREDELL COUNTY BAT MOBILE UNIT 8 480

Serial Number: *008816*
Test Date: *06/12/2026*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name: *Glasscock, Jerry D*
Permit Number: *7180-9235*
Effective:
02/01/2026-02/01/2028

Officer's Name: *NONE, NONE*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG431002
Exp Date: 11/05/2026

Test	g/210L	Time
DIAG	Pass	9:44pm
AIR BLK	.00	9:45pm
ACCY CHK	.07	9:46pm
AIR BLK	.00	9:47pm
SUB TEST	**.00**	**9:47pm**
AIR BLK	.00	9:48pm
SUB TEST	**.00**	**9:50pm**
AIR BLK	.00	9:50pm

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

IREDELL COUNTY BAT MOBILE UNIT 8 480

Serial Number: *008816* Test Record Number: *8119*
Test Date: *06/12/2026* Test Time: *9:51pm EDT*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	9:51pm
FLO	Pass	9:51pm
FC	Pass	9:52pm

Temperature Tests

Test	Status	Time
FC1	Pass	9:52pm
SRC	Pass	9:52pm
DET	Pass	9:52pm
BAR	Pass	9:52pm
BT	Pass	9:52pm

Blank Tests

Test	Status	Time
AIR	Pass	9:52pm

Printer Tests

Test	Status	Time
PRNT	Pass	9:52pm

CRC Tests

Test	Status	Time
COMP	Pass	9:53pm
CAL	Pass	9:53pm

Preventive Maintenance
Status: Pass

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County IREDELL Instrument Location MOORESVILLE PD

Instrument Serial No. 008823 MOORESVILLE NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

(1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;

(2) Verify instrument displays time and date;

(3) Initiate breath test sequence;

(4) Enter information as prompted;

(5) Verify instrument accuracy;

(6) When "PLEASE BLOW" appears, collect breath sample;

(7) When "PLEASE BLOW" appears, collect breath sample;

(8) Print test record;

(9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and

(10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 10 day of JUNE, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.

Signature of Certifying Official

274970
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

DHHS 4080 (04/20)

Intox EC/IR-II: Subject Test

IREDELL COUNTY MOORESVILLE PD 480

Serial Number: *008823*
Test Date: *06/10/2026*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name: *Fleming, Tina S*
Permit Number: *0027-4970*
Effective:
02/01/2025-02/01/2027

Officer's Name: *NONE, NONE*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG506302
Exp Date: 03/04/2027

Test	g/210L	Time
DIAG	Pass	10:15am
AIR BLK	.00	10:15am
ACCY CHK	.08	10:16am
AIR BLK	.00	10:17am
SUB TEST	**.00**	**10:18am**
AIR BLK	.00	10:19am
SUB TEST	**.00**	**10:20am**
AIR BLK	.00	10:21am

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

IREDELL COUNTY MOORESVILLE PD 480

Serial Number: *008823* Test Record Number: *2207*
Test Date: *06/10/2026* Test Time: *11:55am EDT*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	11:56am
FLO	Pass	11:56am
FC	Pass	11:56am

Temperature Tests

Test	Status	Time
FC1	Pass	11:56am
SRC	Pass	11:56am
DET	Pass	11:56am
BAR	Pass	11:56am
BT	Pass	11:56am

Blank Tests

Test	Status	Time
AIR	Pass	11:57am

Printer Tests

Test	Status	Time
PRNT	Pass	11:57am

CRC Tests

Test	Status	Time
COMP	Pass	11:57am
CAL	Pass	11:57am

Preventive Maintenance
Status: Pass

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Iredell Instrument Location BAT Mobile Unit 8

Instrument Serial No. 008929

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

(1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;

(2) Verify instrument displays time and date;

(3) Initiate breath test sequence;

(4) Enter information as prompted;

(5) Verify instrument accuracy;

(6) When "PLEASE BLOW" appears, collect breath sample;

(7) When "PLEASE BLOW" appears, collect breath sample;

(8) Print test record;

(9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and

(10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 12 day of June, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.

Signature of Certifying Official

2219283
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

DHHS 4080 (04/20)

Intox EC/IR-II: Subject Test

IREDELL COUNTY BAT MOBILE UNIT 8 480

Serial Number: *008929*
Test Date: *06/12/2026*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name: *Glasscock, Jerry D*
Permit Number: *7180-9235*
Effective:
02/01/2026-02/01/2028

Officer's Name: *NONE, NONE*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG506303
Exp Date: 03/04/2027

Test	g/210L	Time
DIAG	Pass	9:41pm
AIR BLK	.00	9:42pm
ACCY CHK	.07	9:43pm
AIR BLK	.00	9:44pm
SUB TEST	**.00**	**9:46pm**
AIR BLK	.00	9:47pm
SUB TEST	**.00**	**9:49pm**
AIR BLK	.00	9:50pm

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

IREDELL COUNTY BAT MOBILE UNIT 8 480

Serial Number: *008929* Test Record Number: *1826*
Test Date: *06/12/2026* Test Time: *9:50pm EDT*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	9:51pm
FLO	Pass	9:51pm
FC	Pass	9:51pm

Temperature Tests

Test	Status	Time
FC1	Pass	9:51pm
SRC	Pass	9:51pm
DET	Pass	9:51pm
BAR	Pass	9:51pm
BT	Pass	9:51pm

Blank Tests

Test	Status	Time
AIR	Pass	9:52pm

Printer Tests

Test	Status	Time
PRNT	Pass	9:52pm

CRC Tests

Test	Status	Time
COMP	Pass	9:52pm
CAL	Pass	9:52pm

Preventive Maintenance
Status: Pass

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Jackson Instrument Location Jackson Co. Jail

Instrument Serial No. 008722 Sylva, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

(1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;

(2) Verify instrument displays time and date;

(3) Initiate breath test sequence;

(4) Enter information as prompted;

(5) Verify instrument accuracy;

(6) When "PLEASE BLOW" appears, collect breath sample;

(7) When "PLEASE BLOW" appears, collect breath sample;

(8) Print test record;

(9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and

(10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 2nd day of June, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.

David R. Cutler
Signature of Certifying Official

843310
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

DHHS 4080 (04/20)

Intox EC/IR-II: Subject Test

JACKSON COUNTY JACKSON COUNTY JAIL 490

Serial Number: *008722*
Test Date: *06/02/2026*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name: *Cutler, Daniel R*
Permit Number: *0084-3310*
Effective:
02/01/2026-02/01/2028

Officer's Name: *NONE, NONE*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG431002
Exp Date: 11/05/2026

Test	g/210L	Time
DIAG	Pass	1:46pm
AIR BLK	.00	1:47pm
ACCY CHK	.07	1:47pm
AIR BLK	.00	1:49pm
SUB TEST	**.00**	**1:49pm**
AIR BLK	.00	1:50pm
SUB TEST	**.00**	**1:52pm**
AIR BLK	.00	1:52pm

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

JACKSON COUNTY JACKSON COUNTY JAIL 490

Serial Number: *008722* Test Record Number: *1736*
Test Date: *06/02/2026* Test Time: *1:53pm EDT*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	1:54pm
FLO	Pass	1:54pm
FC	Pass	1:54pm

Temperature Tests

Test	Status	Time
FC1	Pass	1:54pm
SRC	Pass	1:54pm
DET	Pass	1:54pm
BAR	Pass	1:54pm
BT	Pass	1:54pm

Blank Tests

Test	Status	Time
AIR	Pass	1:55pm


Printer Tests

Test	Status	Time
PRNT	Pass	1:55pm

CRC Tests

Test	Status	Time
COMP	Pass	1:55pm
CAL	Pass	1:55pm

Preventive Maintenance
Status: Pass



Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Johnston Instrument Location BAT Mobile unit 9

Instrument Serial No. 008575

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

(1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;

(2) Verify instrument displays time and date;

(3) Initiate breath test sequence;

(4) Enter information as prompted;

(5) Verify instrument accuracy;

(6) When "PLEASE BLOW" appears, collect breath sample;

(7) When "PLEASE BLOW" appears, collect breath sample;

(8) Print test record;

(9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and

(10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 4/ day of June, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.

Signature of Certifying Official

1937759
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

DHHS 4080 (04/20)

Intox EC/IR-II: Subject Test

JOHNSTON COUNTY BAT MOBILE UNIT 9 500

Serial Number: *008575*
Test Date: *06/04/2026*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name: *Carroll, Barry Jean D*
Permit Number: *0019-3759*
Effective:
04/01/2026-04/01/2028

Officer's Name: *NONE, NONE*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG516204
Exp Date: 06/11/2027

Test	g/210L	Time
DIAG	Pass	7:34pm
AIR BLK	.00	7:35pm
ACCY CHK	.07	7:36pm
AIR BLK	.00	7:37pm
SUB TEST	**.00**	**7:38pm**
AIR BLK	.00	7:39pm
SUB TEST	**.00**	**7:41pm**
AIR BLK	.00	7:42pm

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

JOHNSTON COUNTY BAT MOBILE UNIT 9 500

Serial Number: *008575* Test Record Number: *1600*
Test Date: *06/04/2026* Test Time: *7:43pm EDT*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	7:43pm
FLO	Pass	7:43pm
FC	Pass	7:43pm

Temperature Tests

Test	Status	Time
FC1	Pass	7:43pm
SRC	Pass	7:43pm
DET	Pass	7:43pm
BAR	Pass	7:43pm
BT	Pass	7:43pm

Blank Tests

Test	Status	Time
AIR	Pass	7:44pm

Printer Tests

Test	Status	Time
PRNT	Pass	7:44pm

CRC Tests

Test	Status	Time
COMP	Pass	7:44pm
CAL	Pass	7:44pm

Preventive Maintenance
Status: Pass

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Johnston Instrument Location BAT MOBILE UNIT 9

Instrument Serial No. 008575

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

(1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;

(2) Verify instrument displays time and date;

(3) Initiate breath test sequence;

(4) Enter information as prompted;

(5) Verify instrument accuracy;

(6) When "PLEASE BLOW" appears, collect breath sample;

(7) When "PLEASE BLOW" appears, collect breath sample;

(8) Print test record;

(9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and

(10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 5 day of June, 20 26 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.

Signature of Certifying Official

19375
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

DHHS 4080 (04/20)

Intox EC/IR-II: Subject Test

JOHNSTON COUNTY BAT MOBILE UNIT 9 500

Serial Number: *008575*
Test Date: *06/05/2026*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name: *Carroll, Barry Jean D*
Permit Number: *0019-3759*
Effective:
04/01/2026-04/01/2028

Officer's Name: *NONE, NONE*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG516204
Exp Date: 06/11/2027

Test	g/210L	Time
DIAG	Pass	7:43pm
AIR BLK	.00	7:44pm
ACCY CHK	.07	7:45pm
AIR BLK	.00	7:46pm
SUB TEST	**.00**	**7:49pm**
AIR BLK	.00	7:50pm
SUB TEST	**.00**	**7:51pm**
AIR BLK	.00	7:52pm

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

JOHNSTON COUNTY BAT MOBILE UNIT 9 500

Serial Number: *008575* Test Record Number: *1604*
Test Date: *06/05/2026* Test Time: *7:54pm EDT*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	7:54pm
FLO	Pass	7:54pm
FC	Pass	7:54pm

Temperature Tests

Test	Status	Time
FC1	Pass	7:54pm
SRC	Pass	7:54pm
DET	Pass	7:54pm
BAR	Pass	7:54pm
BT	Pass	7:54pm

Blank Tests

Test	Status	Time
AIR	Pass	7:55pm


Printer Tests

Test	Status	Time
PRNT	Pass	7:55pm

CRC Tests

Test	Status	Time
COMP	Pass	7:55pm
CAL	Pass	7:55pm

Preventive Maintenance
Status: Pass

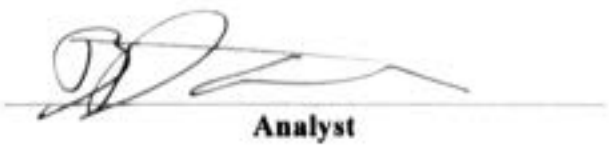

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Johnston Instrument Location BAT Mobile Unit 10

Instrument Serial No. 005584

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

(1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;

(2) Verify instrument displays time and date;

(3) Initiate breath test sequence;

(4) Enter information as prompted;

(5) Verify instrument accuracy;

(6) When "PLEASE BLOW" appears, collect breath sample;

(7) When "PLEASE BLOW" appears, collect breath sample;

(8) Print test record;

(9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and

(10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 19 day of June, 20 26 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.

Signature of Certifying Official

193759
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

DHHS 4080 (04/20)

Intox EC/IR-II: Subject Test

JOHNSTON COUNTY BAT MOBILE UNIT 10 500

Serial Number: *008584*
Test Date: *06/19/2026*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name: *Carroll, Barry Jean D*
Permit Number: *0019-3759*
Effective:
04/01/2026-04/01/2028

Officer's Name: *NONE, NONE*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG534301
Exp Date: 12/09/2027

Test	g/210L	Time
DIAG	Pass	7:17pm
AIR BLK	.00	7:18pm
ACCY CHK	.08	7:19pm
AIR BLK	.00	7:20pm
SUB TEST	**.00**	**7:20pm**
AIR BLK	.00	7:21pm
SUB TEST	**.00**	**7:23pm**
AIR BLK	.00	7:24pm

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

JOHNSTON COUNTY BAT MOBILE UNIT 10 500

Serial Number: *008584* Test Record Number: *2910*
Test Date: *06/19/2026* Test Time: *7:31pm EDT*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	7:31pm
FLO	Pass	7:31pm
FC	Pass	7:31pm

Temperature Tests

Test	Status	Time
FC1	Pass	7:32pm
SRC	Pass	7:32pm
DET	Pass	7:32pm
BAR	Pass	7:32pm
BT	Pass	7:32pm

Blank Tests

Test	Status	Time
AIR	Pass	7:32pm

Printer Tests

Test	Status	Time
PRNT	Pass	7:32pm

CRC Tests

Test	Status	Time
COMP	Pass	7:32pm
CAL	Pass	7:32pm

Preventive Maintenance
Status: Pass

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Johnston Instrument Location BAT Mobile Unit 9

Instrument Serial No. 008616

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

(1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;

(2) Verify instrument displays time and date;

(3) Initiate breath test sequence;

(4) Enter information as prompted;

(5) Verify instrument accuracy;

(6) When "PLEASE BLOW" appears, collect breath sample;

(7) When "PLEASE BLOW" appears, collect breath sample;

(8) Print test record;

(9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and

(10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 4 day of June, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.

Signature of Certifying Official

193759
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

DHHS 4080 (04/20)

Intox EC/IR-II: Subject Test

JOHNSTON COUNTY BAT MOBILE UNIT 9 500

Serial Number: *008616*
Test Date: *06/04/2026*

Citation Number: *M0000000-0*
Subject's Name:
PERVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name: *Carroll, Barry Jean D*
Permit Number: *0019-3759*
Effective:
04/01/2026-04/01/2028

Officer's Name: *NONE, NONE*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG506303
Exp Date: 03/04/2027

Test	g/210L	Time
DIAG	Pass	7:37pm
AIR BLK	.00	7:38pm
ACCY CHK	.07	7:38pm
AIR BLK	.00	7:40pm
SUB TEST	**.00**	**7:41pm**
AIR BLK	.00	7:42pm
SUB TEST	**.00**	**7:43pm**
AIR BLK	.00	7:45pm

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

JOHNSTON COUNTY BAT MOBILE UNIT 9 500

Serial Number: *008616* Test Record Number: *3015*
Test Date: *06/04/2026* Test Time: *7:45pm EDT*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	7:46pm
FLO	Pass	7:46pm
FC	Pass	7:46pm

Temperature Tests

Test	Status	Time
FC1	Pass	7:46pm
SRC	Pass	7:46pm
DET	Pass	7:46pm
BAR	Pass	7:46pm
BT	Pass	7:46pm

Blank Tests

Test	Status	Time
AIR	Pass	7:46pm

Printer Tests

Test	Status	Time
PRNT	Pass	7:46pm

CRC Tests

Test	Status	Time
COMP	Pass	7:47pm
CAL	Pass	7:47pm

Preventive Maintenance
Status: Pass

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Johnston Instrument Location BAT MOBILE UNIT 9

Instrument Serial No. 008616

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

(1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;

(2) Verify instrument displays time and date;

(3) Initiate breath test sequence;

(4) Enter information as prompted;

(5) Verify instrument accuracy;

(6) When "PLEASE BLOW" appears, collect breath sample;

(7) When "PLEASE BLOW" appears, collect breath sample;

(8) Print test record;

(9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and

(10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 5 day of June, 20 26 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.

Signature of Certifying Official

193759
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

DHHS 4080 (04/20)

Intox EC/IR-II: Subject Test

JOHNSTON COUNTY BAT MOBILE UNIT 9 500

Serial Number: *008616*
Test Date: *06/05/2026*

Citation Number: *M0000000-0*
Subject's Name:
PEVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name: *Carroll, Barry Jean D*
Permit Number: *0019-3759*
Effective:
04/01/2026-04/01/2028

Officer's Name: *NONE, NONE*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG506303
Exp Date: 03/04/2027

Test	g/210L	Time
DIAG	Pass	8:16pm
AIR BLK	.00	8:17pm
ACCY CHK	.07	8:17pm
AIR BLK	.00	8:18pm
SUB TEST	**.00**	**8:19pm**
AIR BLK	.00	8:20pm
SUB TEST	**.00**	**8:22pm**
AIR BLK	.00	8:23pm

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

JOHNSTON COUNTY BAT MOBILE UNIT 9 500

Serial Number: *008616* Test Record Number: *3022*
Test Date: *06/05/2026* Test Time: *8:28pm EDT*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	8:28pm
FLO	Pass	8:28pm
FC	Pass	8:28pm

Temperature Tests

Test	Status	Time
FC1	Pass	8:28pm
SRC	Pass	8:28pm
DET	Pass	8:28pm
BAR	Pass	8:28pm
BT	Pass	8:28pm

Blank Tests

Test	Status	Time
AIR	Pass	8:29pm


Printer Tests

Test	Status	Time
PRNT	Pass	8:29pm

CRC Tests

Test	Status	Time
COMP	Pass	8:29pm
CAL	Pass	8:29pm

Preventive Maintenance
Status: Pass



Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Johnston Instrument Location BAT Mobile Unit 9

Instrument Serial No. 008647

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

(1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;

(2) Verify instrument displays time and date;

(3) Initiate breath test sequence;

(4) Enter information as prompted;

(5) Verify instrument accuracy;

(6) When "PLEASE BLOW" appears, collect breath sample;

(7) When "PLEASE BLOW" appears, collect breath sample;

(8) Print test record;

(9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and

(10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 4 day of June, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.

Signature of Certifying Official

193759
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

DHHS 4080 (04/20)

Intox EC/IR-II: Subject Test

JOHNSTON COUNTY BAT MOBILE UNIT 9 500

Serial Number: *008647*
Test Date: *06/04/2026*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name: *Carroll, Barry Jean D*
Permit Number: *0019-3759*
Effective:
04/01/2026-04/01/2028

Officer's Name: *NONE, NONE*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG516203
Exp Date: 06/11/2027

Test	g/210L	Time
DIAG	Pass	7:39pm
AIR BLK	.00	7:40pm
ACCY CHK	.07	7:41pm
AIR BLK	.00	7:42pm
SUB TEST	**.00**	**7:42pm**
AIR BLK	.00	7:43pm
SUB TEST	**.00**	**7:45pm**
AIR BLK	.00	7:46pm

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

JOHNSTON COUNTY BAT MOBILE UNIT 9 500

Serial Number: *008647* Test Record Number: *2987*
Test Date: *06/04/2026* Test Time: *7:47pm EDT*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	7:47pm
FLO	Pass	7:47pm
FC	Pass	7:47pm

Temperature Tests

Test	Status	Time
FC1	Pass	7:47pm
SRC	Pass	7:47pm
DET	Pass	7:47pm
BAR	Pass	7:47pm
BT	Pass	7:47pm

Blank Tests

Test	Status	Time
AIR	Pass	7:48pm

Printer Tests

Test	Status	Time
PRNT	Pass	7:48pm

CRC Tests

Test	Status	Time
COMP	Pass	7:48pm
CAL	Pass	7:48pm

Preventive Maintenance
Status: Pass



Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Johnston Instrument Location BAT Mobile Unit 9

Instrument Serial No. 008647

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

(1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;

(2) Verify instrument displays time and date;

(3) Initiate breath test sequence;

(4) Enter information as prompted;

(5) Verify instrument accuracy;

(6) When "PLEASE BLOW" appears, collect breath sample;

(7) When "PLEASE BLOW" appears, collect breath sample;

(8) Print test record;

(9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and

(10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 5 day of June, 20 26 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.

Signature of Certifying Official

193759
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

DHHS 4080 (04/20)

Intox EC/IR-II: Subject Test

JOHNSTON COUNTY BAT MOBILE UNIT 9 500

Serial Number: *008647*
Test Date: *06/05/2026*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name: *Carroll, Barry Jean D*
Permit Number: *0019-3759*
Effective:
04/01/2026-04/01/2028

Officer's Name: *NONE, NONE*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG516203
Exp Date: 06/11/2027

Test	g/210L	Time
DIAG	Pass	7:49pm
AIR BLK	.00	7:50pm
ACCY CHK	.07	7:50pm
AIR BLK	.00	7:51pm
SUB TEST	**.00**	**7:52pm**
AIR BLK	.00	7:53pm
SUB TEST	**.00**	**7:54pm**
AIR BLK	.00	7:55pm

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

JOHNSTON COUNTY BAT MOBILE UNIT 9 500

Serial Number: *008647* Test Record Number: *2989*
Test Date: *06/05/2026* Test Time: *7:56pm EDT*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	7:56pm
FLO	Pass	7:56pm
FC	Pass	7:56pm

Temperature Tests

Test	Status	Time
FC1	Pass	7:56pm
SRC	Pass	7:56pm
DET	Pass	7:56pm
BAR	Pass	7:56pm
BT	Pass	7:56pm

Blank Tests

Test	Status	Time
AIR	Pass	7:57pm


Printer Tests

Test	Status	Time
PRNT	Pass	7:57pm

CRC Tests

Test	Status	Time
COMP	Pass	7:57pm
CAL	Pass	7:57pm

Preventive Maintenance
Status: Pass

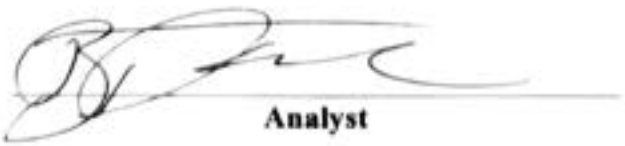

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Johnston Instrument Location BAT Mobile Unit 10

Instrument Serial No. 008686

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

(1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;

(2) Verify instrument displays time and date;

(3) Initiate breath test sequence;

(4) Enter information as prompted;

(5) Verify instrument accuracy;

(6) When "PLEASE BLOW" appears, collect breath sample;

(7) When "PLEASE BLOW" appears, collect breath sample;

(8) Print test record;

(9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and

(10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 19 day of June, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.

Signature of Certifying Official

193754
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

DHHS 4080 (04/20)

Intox EC/IR-II: Subject Test

JOHNSTON COUNTY BAT MOBILE UNIT 10 500

Serial Number: *008686*
Test Date: *06/19/2026*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name: *Carroll, Barry Jean D*
Permit Number: *0019-3759*
Effective:
04/01/2026-04/01/2028

Officer's Name: *NONE, NONE*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG506302
Exp Date: 03/04/2027

Test	g/210L	Time
DIAG	Pass	6:42pm
AIR BLK	.00	6:43pm
ACCY CHK	.08	6:43pm
AIR BLK	.00	6:44pm
SUB TEST	**.00**	**6:45pm**
AIR BLK	.00	6:46pm
SUB TEST	**.00**	**6:49pm**
AIR BLK	.00	6:50pm

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

JOHNSTON COUNTY BAT MOBILE UNIT 10 500

Serial Number: *008686* Test Record Number: *7257*
Test Date: *06/19/2026* Test Time: *6:52pm EDT*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	6:52pm
FLO	Pass	6:52pm
FC	Pass	6:52pm

Temperature Tests

Test	Status	Time
FC1	Pass	6:52pm
SRC	Pass	6:52pm
DET	Pass	6:52pm
BAR	Pass	6:52pm
BT	Pass	6:52pm

Blank Tests

Test	Status	Time
AIR	Pass	6:53pm

Printer Tests

Test	Status	Time
PRNT	Pass	6:53pm

CRC Tests

Test	Status	Time
COMP	Pass	6:53pm
CAL	Pass	6:53pm

Preventive Maintenance
Status: Pass



Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Johnston Instrument Location BAT Mobile Unit 9

Instrument Serial No. 0087041

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

(1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;

(2) Verify instrument displays time and date;

(3) Initiate breath test sequence;

(4) Enter information as prompted;

(5) Verify instrument accuracy;

(6) When "PLEASE BLOW" appears, collect breath sample;

(7) When "PLEASE BLOW" appears, collect breath sample;

(8) Print test record;

(9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and

(10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 4 day of June, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.

Signature of Certifying Official

193759
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

DHHS 4080 (04/20)

Intox EC/IR-II: Subject Test

JOHNSTON COUNTY BAT MOBILE UNIT 9 500

Serial Number: *008704*
Test Date: *06/04/2026*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name: *Carroll, Barry Jean D*
Permit Number: *0019-3759*
Effective:
04/01/2026-04/01/2028

Officer's Name: *NONE, NONE*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG506303
Exp Date: 03/04/2027

Test	g/210L	Time
DIAG	Pass	7:40pm
AIR BLK	.00	7:41pm
ACCY CHK	.07	7:42pm
AIR BLK	.00	7:43pm
SUB TEST	**.00**	**7:44pm**
AIR BLK	.00	7:44pm
SUB TEST	**.00**	**7:46pm**
AIR BLK	.00	7:47pm

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

JOHNSTON COUNTY BAT MOBILE UNIT 9 500

Serial Number: *008704* Test Record Number: *1037*
Test Date: *06/04/2026* Test Time: *7:49pm EDT*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	7:50pm
FLO	Pass	7:50pm
FC	Pass	7:50pm

Temperature Tests

Test	Status	Time
FC1	Pass	7:50pm
SRC	Pass	7:50pm
DET	Pass	7:50pm
BAR	Pass	7:50pm
BT	Pass	7:50pm

Blank Tests

Test	Status	Time
AIR	Pass	7:50pm

Printer Tests

Test	Status	Time
PRNT	Pass	7:51pm

CRC Tests

Test	Status	Time
COMP	Pass	7:51pm
CAL	Pass	7:51pm

Preventive Maintenance
Status: Pass



Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Johnston Instrument Location BAT MOBILE UNIT 9

Instrument Serial No. 008704

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

(1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;

(2) Verify instrument displays time and date;

(3) Initiate breath test sequence;

(4) Enter information as prompted;

(5) Verify instrument accuracy;

(6) When "PLEASE BLOW" appears, collect breath sample;

(7) When "PLEASE BLOW" appears, collect breath sample;

(8) Print test record;

(9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and

(10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 5 day of June, 20 26 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.

Signature of Certifying Official

193759
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

DHHS 4080 (04/20)

Intox EC/IR-II: Subject Test

JOHNSTON COUNTY BAT MOBILE UNIT 9 500

Serial Number: *008704*
Test Date: *06/05/2026*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name: *Carroll, Barry Jean D*
Permit Number: *0019-3759*
Effective:
04/01/2026-04/01/2028

Officer's Name: *NONE, NONE*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG506303
Exp Date: 03/04/2027

Test	g/210L	Time
DIAG	Pass	7:53pm
AIR BLK	.00	7:54pm
ACCY CHK	.07	7:55pm
AIR BLK	.00	7:56pm
SUB TEST	**.00**	**7:56pm**
AIR BLK	.00	7:57pm
SUB TEST	**.00**	**7:59pm**
AIR BLK	.00	8:00pm

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

JOHNSTON COUNTY BAT MOBILE UNIT 9 500

Serial Number: *008704* Test Record Number: *1040*
Test Date: *06/05/2026* Test Time: *8:05pm EDT*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	8:05pm
FLO	Pass	8:05pm
FC	Pass	8:05pm

Temperature Tests

Test	Status	Time
FC1	Pass	8:05pm
SRC	Pass	8:05pm
DET	Pass	8:05pm
BAR	Pass	8:05pm
BT	Pass	8:05pm

Blank Tests

Test	Status	Time
AIR	Pass	8:06pm

Printer Tests

Test	Status	Time
PRNT	Pass	8:06pm

CRC Tests

Test	Status	Time
COMP	Pass	8:06pm
CAL	Pass	8:06pm

Preventive Maintenance
Status: Pass



Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Johnston Instrument Location Johnston County Detention Center

Instrument Serial No. 008721

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

(1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;

(2) Verify instrument displays time and date;

(3) Initiate breath test sequence;

(4) Enter information as prompted;

(5) Verify instrument accuracy;

(6) When "PLEASE BLOW" appears, collect breath sample;

(7) When "PLEASE BLOW" appears, collect breath sample;

(8) Print test record;

(9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and

(10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 2 day of June, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.

Signature of Certifying Official

365156
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

DHHS 4080 (04/20)

Intox EC/IR-II: Subject Test

JOHNSTON COUNTY DETENTION CENTER 500

Serial Number: *008721*
Test Date: *06/02/2026*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name: *Garner, Joel K*
Permit Number: *0036-5156*
Effective:
02/01/2026-02/01/2028

Officer's Name: *NONE, NONE*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG602202
Exp Date: 01/22/2028

Test	g/210L	Time
DIAG	Pass	1:00pm
AIR BLK	.00	1:01pm
ACCY CHK	.08	1:01pm
AIR BLK	.00	1:02pm
SUB TEST	**.00**	**1:03pm**
AIR BLK	.00	1:04pm
SUB TEST	**.00**	**1:05pm**
AIR BLK	.00	1:06pm

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

JOHNSTON COUNTY DETENTION CENTER 500

Serial Number: *008721* Test Record Number: *2670*
Test Date: *06/02/2026* Test Time: *1:07pm EDT*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	1:07pm
FLO	Pass	1:07pm
FC	Pass	1:08pm

Temperature Tests

Test	Status	Time
FC1	Pass	1:08pm
SRC	Pass	1:08pm
DET	Pass	1:08pm
BAR	Pass	1:08pm
BT	Pass	1:08pm

Blank Tests

Test	Status	Time
AIR	Pass	1:08pm

Printer Tests

Test	Status	Time
PRNT	Pass	1:08pm

CRC Tests

Test	Status	Time
COMP	Pass	1:08pm
CAL	Pass	1:08pm

Preventive Maintenance
Status: Pass



Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Johnston Instrument Location BAT Mobile Unit 10

Instrument Serial No. 008776

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

(1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;

(2) Verify instrument displays time and date;

(3) Initiate breath test sequence;

(4) Enter information as prompted;

(5) Verify instrument accuracy;

(6) When "PLEASE BLOW" appears, collect breath sample;

(7) When "PLEASE BLOW" appears, collect breath sample;

(8) Print test record;

(9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and

(10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 19 day of June, 20 26 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.

Signature of Certifying Official

143754
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

DHHS 4080 (04/20)

Intox EC/IR-II: Subject Test

JOHNSTON COUNTY BAT MOBILE UNIT 10 500

Serial Number: *008776*
Test Date: *06/19/2026*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name: *Carroll, Barry Jean D*
Permit Number: *0019-3759*
Effective:
04/01/2026-04/01/2028

Officer's Name: *NONE, NONE*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG417803
Exp Date: 06/26/2026

Test	g/210L	Time
DIAG	Pass	6:45pm
AIR BLK	.00	6:46pm
ACCY CHK	.08	6:47pm
AIR BLK	.00	6:47pm
SUB TEST	**.00**	**6:49pm**
AIR BLK	.00	6:50pm
SUB TEST	**.00**	**6:52pm**
AIR BLK	.00	6:53pm

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

JOHNSTON COUNTY BAT MOBILE UNIT 10 500

Serial Number: *008776* Test Record Number: *4228*
Test Date: *06/19/2026* Test Time: *7:19pm EDT*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	7:19pm
FLO	Pass	7:19pm
FC	Pass	7:19pm

Temperature Tests

Test	Status	Time
FC1	Pass	7:19pm
SRC	Pass	7:19pm
DET	Pass	7:19pm
BAR	Pass	7:19pm
BT	Pass	7:19pm

Blank Tests

Test	Status	Time
AIR	Pass	7:20pm

Printer Tests

Test	Status	Time
PRNT	Pass	7:20pm

CRC Tests

Test	Status	Time
COMP	Pass	7:20pm
CAL	Pass	7:20pm

Preventive Maintenance
Status: Pass



Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Johnston Instrument Location BAT Mobile Unit 10

Instrument Serial No. 005779

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

(1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;

(2) Verify instrument displays time and date;

(3) Initiate breath test sequence;

(4) Enter information as prompted;

(5) Verify instrument accuracy;

(6) When "PLEASE BLOW" appears, collect breath sample;

(7) When "PLEASE BLOW" appears, collect breath sample;

(8) Print test record;

(9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and

(10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 19 day of June, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.

Signature of Certifying Official

193759
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

DHHS 4089 (04/26)

Intox EC/IR-II: Subject Test

JOHNSTON COUNTY BAT MOBILE UNIT 10 500

Serial Number: *008779*
Test Date: *06/19/2026*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name: *Carroll, Barry Jean D*
Permit Number: *0019-3759*
Effective:
04/01/2026-04/01/2028

Officer's Name: *NONE, NONE*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG431002
Exp Date: 11/05/2026

Test	g/210L	Time
DIAG	Pass	6:49pm
AIR BLK	.00	6:50pm
ACCY CHK	.08	6:50pm
AIR BLK	.00	6:51pm
SUB TEST	**.00**	**6:52pm**
AIR BLK	.00	6:53pm
SUB TEST	**.00**	**6:55pm**
AIR BLK	.00	6:56pm

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

JOHNSTON COUNTY BAT MOBILE UNIT 10 500

Serial Number: *008779* Test Record Number: *4152*
Test Date: *06/19/2026* Test Time: *6:57pm EDT*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	6:57pm
FLO	Pass	6:57pm
FC	Pass	6:57pm

Temperature Tests

Test	Status	Time
FC1	Pass	6:57pm
SRC	Pass	6:57pm
DET	Pass	6:57pm
BAR	Pass	6:57pm
BT	Pass	6:57pm

Blank Tests

Test	Status	Time
AIR	Pass	6:58pm


Printer Tests

Test	Status	Time
PRNT	Pass	6:58pm

CRC Tests

Test	Status	Time
COMP	Pass	6:58pm
CAL	Pass	6:58pm

Preventive Maintenance
Status: Pass

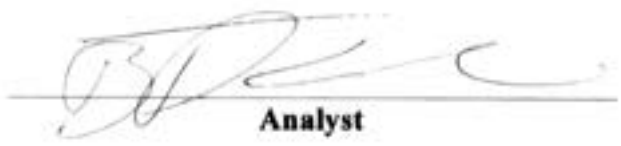

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Johnston Instrument Location Johnston County Detention Center

Instrument Serial No. 008810

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

(1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;

(2) Verify instrument displays time and date;

(3) Initiate breath test sequence;

(4) Enter information as prompted;

(5) Verify instrument accuracy;

(6) When "PLEASE BLOW" appears, collect breath sample;

(7) When "PLEASE BLOW" appears, collect breath sample;

(8) Print test record;

(9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and

(10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 2 day of June, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.

Signature of ~~Certifying~~ Official

365156
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

DHHS 4080 (04/20)

Intox EC/IR-II: Subject Test

JOHNSTON COUNTY DETENTION CENTER 500

Serial Number: *008810*
Test Date: *06/02/2026*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name: *Garner, Joel K*
Permit Number: *0036-5156*
Effective:
02/01/2026-02/01/2028

Officer's Name: *NONE, NONE*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG602202
Exp Date: 01/22/2028

Test	g/210L	Time
DIAG	Pass	12:59pm
AIR BLK	.00	1:00pm
ACCY CHK	.07	1:00pm
AIR BLK	.00	1:02pm
SUB TEST	**.00**	**1:02pm**
AIR BLK	.00	1:03pm
SUB TEST	**.00**	**1:04pm**
AIR BLK	.00	1:05pm

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

JOHNSTON COUNTY DETENTION CENTER 500

Serial Number: *008810* Test Record Number: *6759*
Test Date: *06/02/2026* Test Time: *1:11pm EDT*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	1:11pm
FLO	Pass	1:11pm
FC	Pass	1:12pm

Temperature Tests

Test	Status	Time
FC1	Pass	1:12pm
SRC	Pass	1:12pm
DET	Pass	1:12pm
BAR	Pass	1:12pm
BT	Pass	1:12pm

Blank Tests

Test	Status	Time
AIR	Pass	1:12pm

Printer Tests

Test	Status	Time
PRNT	Pass	1:12pm

CRC Tests

Test	Status	Time
COMP	Pass	1:12pm
CAL	Pass	1:12pm

Preventive Maintenance
Status: Pass



Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Johnston Instrument Location BAT Mobile Unit 9

Instrument Serial No. 008826

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

(1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;

(2) Verify instrument displays time and date;

(3) Initiate breath test sequence;

(4) Enter information as prompted;

(5) Verify instrument accuracy;

(6) When "PLEASE BLOW" appears, collect breath sample;

(7) When "PLEASE BLOW" appears, collect breath sample;

(8) Print test record;

(9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and

(10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 4 day of June, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.

Signature of Certifying Official

193759
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

DHHS 4080 (04/20)

Intox EC/IR-II: Subject Test

JOHNSTON COUNTY BAT MOBILE UNIT 9 500

Serial Number: *008826*
Test Date: *06/04/2026*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name: *Carroll, Barry Jean D*
Permit Number: *0019-3759*
Effective:
04/01/2026-04/01/2028

Officer's Name: *NONE, NONE*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG516204
Exp Date: 06/11/2027

Test	g/210L	Time
DIAG	Pass	7:32pm
AIR BLK	.00	7:33pm
ACCY CHK	.07	7:34pm
AIR BLK	.00	7:35pm
SUB TEST	**.00**	**7:36pm**
AIR BLK	.00	7:36pm
SUB TEST	**.00**	**7:38pm**
AIR BLK	.00	7:39pm

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

JOHNSTON COUNTY BAT MOBILE UNIT 9 500

Serial Number: *008826* Test Record Number: *8673*
Test Date: *06/04/2026* Test Time: *7:41pm EDT*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	7:41pm
FLO	Pass	7:41pm
FC	Pass	7:41pm

Temperature Tests

Test	Status	Time
FC1	Pass	7:42pm
SRC	Pass	7:42pm
DET	Pass	7:42pm
BAR	Pass	7:42pm
BT	Pass	7:42pm

Blank Tests

Test	Status	Time
AIR	Pass	7:42pm

Printer Tests

Test	Status	Time
PRNT	Pass	7:42pm

CRC Tests

Test	Status	Time
COMP	Pass	7:42pm
CAL	Pass	7:42pm

Preventive Maintenance
Status: Pass

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Johnston Instrument Location BAT MOBILE UNIT 9

Instrument Serial No. 008826

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

(1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;

(2) Verify instrument displays time and date;

(3) Initiate breath test sequence;

(4) Enter information as prompted;

(5) Verify instrument accuracy;

(6) When "PLEASE BLOW" appears, collect breath sample;

(7) When "PLEASE BLOW" appears, collect breath sample;

(8) Print test record;

(9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and

(10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 5 day of June, 20 26 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.

Signature of Certifying Official

193759
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

DHHS 4080 (04/20)

Intox EC/IR-II: Subject Test

JOHNSTON COUNTY BAT MOBILE UNIT 9 500

Serial Number: *008826*
Test Date: *06/05/2026*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name: *Carroll, Barry Jean D*
Permit Number: *0019-3759*
Effective:
04/01/2026-04/01/2028

Officer's Name: *NONE, NONE*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG516204
Exp Date: 06/11/2027

Test	g/210L	Time
DIAG	Pass	8:13pm
AIR BLK	.00	8:14pm
ACCY CHK	.07	8:15pm
AIR BLK	.00	8:16pm
SUB TEST	**.00**	**8:16pm**
AIR BLK	.00	8:17pm
SUB TEST	**.00**	**8:20pm**
AIR BLK	.00	8:21pm

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

JOHNSTON COUNTY BAT MOBILE UNIT 9 500

Serial Number: *008826* Test Record Number: *8676*
Test Date: *06/05/2026* Test Time: *8:27pm EDT*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	8:27pm
FLO	Pass	8:27pm
FC	Pass	8:27pm

Temperature Tests

Test	Status	Time
FC1	Pass	8:28pm
SRC	Pass	8:28pm
DET	Pass	8:28pm
BAR	Pass	8:28pm
BT	Pass	8:28pm

Blank Tests

Test	Status	Time
AIR	Pass	8:28pm


Printer Tests

Test	Status	Time
PRNT	Pass	8:28pm

CRC Tests

Test	Status	Time
COMP	Pass	8:28pm
CAL	Pass	8:28pm

Preventive Maintenance
Status: Pass



Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Lenoir Instrument Location BAT Mobile Unit 9

Instrument Serial No. 008575

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

(1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;

(2) Verify instrument displays time and date;

(3) Initiate breath test sequence;

(4) Enter information as prompted;

(5) Verify instrument accuracy;

(6) When "PLEASE BLOW" appears, collect breath sample;

(7) When "PLEASE BLOW" appears, collect breath sample;

(8) Print test record;

(9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and

(10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 27th day of June, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.

Signature of Certifying Official

226313
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

DHHS 4080 (04/20)

Intox EC/IR-II: Subject Test

LENOIR COUNTY BAT MOBILE UNIT 9 530

Serial Number: *008575*
Test Date: *06/27/2026*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name: *Sharpe Jr., Robert J*
Permit Number: *1820-8591*
Effective:
02/01/2026-02/01/2028

Officer's Name: *NONE, NONE*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG516204
Exp Date: 06/11/2027

Test	g/210L	Time
DIAG	Pass	7:05pm
AIR BLK	.00	7:06pm
ACCY CHK	.07	7:07pm
AIR BLK	.00	7:08pm
SUB TEST	**.00**	**7:08pm**
AIR BLK	.00	7:09pm
SUB TEST	**.00**	**7:11pm**
AIR BLK	.00	7:12pm

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

LENOIR COUNTY BAT MOBILE UNIT 9 530

Serial Number: *008575* Test Record Number: *1610*
Test Date: *06/27/2026* Test Time: *7:14pm EDT*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	7:15pm
FLO	Pass	7:15pm
FC	Pass	7:15pm

Temperature Tests

Test	Status	Time
FC1	Pass	7:15pm
SRC	Pass	7:15pm
DET	Pass	7:15pm
BAR	Pass	7:15pm
BT	Pass	7:15pm

Blank Tests

Test	Status	Time
AIR	Pass	7:16pm

Printer Tests

Test	Status	Time
PRNT	Pass	7:16pm

CRC Tests

Test	Status	Time
COMP	Pass	7:16pm
CAL	Pass	7:16pm

Preventive Maintenance
Status: Pass



Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Lenoir Instrument Location BAT Mobile Unit 9

Instrument Serial No. 008616

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

(1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;

(2) Verify instrument displays time and date;

(3) Initiate breath test sequence;

(4) Enter information as prompted;

(5) Verify instrument accuracy;

(6) When "PLEASE BLOW" appears, collect breath sample;

(7) When "PLEASE BLOW" appears, collect breath sample;

(8) Print test record;

(9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and

(10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 27th day of June, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.

Signature of Certifying Official

226313
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

DHHS 4080 (04/20)

Intox EC/IR-II: Subject Test

LENOIR COUNTY BAT MOBILE UNIT 9 530

Serial Number: *008616*
Test Date: *06/27/2026*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name: *Sharpe Jr., Robert J*
Permit Number: *1820-8591*
Effective:
02/01/2026-02/01/2028

Officer's Name: *NONE, NONE*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG506303
Exp Date: 03/04/2027

Test	g/210L	Time
DIAG	Pass	7:04pm
AIR BLK	.00	7:05pm
ACCY CHK	.07	7:06pm
AIR BLK	.00	7:07pm
SUB TEST	**.00**	**7:08pm**
AIR BLK	.00	7:09pm
SUB TEST	**.00**	**7:11pm**
AIR BLK	.00	7:12pm

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

LENOIR COUNTY BAT MOBILE UNIT 9 530

Serial Number: *008616* Test Record Number: *3035*
Test Date: *06/27/2026* Test Time: *7:12pm EDT*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	7:12pm
FLO	Pass	7:12pm
FC	Pass	7:13pm

Temperature Tests

Test	Status	Time
FC1	Pass	7:13pm
SRC	Pass	7:13pm
DET	Pass	7:13pm
BAR	Pass	7:13pm
BT	Pass	7:13pm

Blank Tests

Test	Status	Time
AIR	Pass	7:13pm

Printer Tests

Test	Status	Time
PRNT	Pass	7:13pm

CRC Tests

Test	Status	Time
COMP	Pass	7:14pm
CAL	Pass	7:14pm

Preventive Maintenance
Status: Pass



Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Lenoir Instrument Location Kinston P.D.

Instrument Serial No. 008624 205 E. King St., Kinston, NC.

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

(1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;

(2) Verify instrument displays time and date;

(3) Initiate breath test sequence;

(4) Enter information as prompted;

(5) Verify instrument accuracy;

(6) When "PLEASE BLOW" appears, collect breath sample;

(7) When "PLEASE BLOW" appears, collect breath sample;

(8) Print test record;

(9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and

(10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 4th day of June, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.

Signature of Certifying Official

377722
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

DHHS 4080 (04/20)

Intox EC/IR-II: Subject Test

LENOIR COUNTY KINSTON PD 530

Serial Number: *008624*
Test Date: *06/04/2026*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name: *Gray, Kelly D*
Permit Number: *0037-7722*
Effective:
02/01/2026-02/01/2028

Officer's Name: *NONE, NONE*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG534301
Exp Date: 12/09/2027

Test	g/210L	Time
DIAG	Pass	1:47pm
AIR BLK	.00	1:48pm
ACCY CHK	.08	1:49pm
AIR BLK	.00	1:50pm
SUB TEST	**.00**	**1:50pm**
AIR BLK	.00	1:51pm
SUB TEST	**.00**	**1:53pm**
AIR BLK	.00	1:54pm

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

LENOIR COUNTY KINSTON PD 530

Serial Number: *008624* Test Record Number: *2551*
Test Date: *06/04/2026* Test Time: *1:55pm EDT*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	1:55pm
FLO	Pass	1:55pm
FC	Pass	1:55pm

Temperature Tests

Test	Status	Time
FC1	Pass	1:55pm
SRC	Pass	1:55pm
DET	Pass	1:55pm
BAR	Pass	1:55pm
BT	Pass	1:55pm

Blank Tests

Test	Status	Time
AIR	Pass	1:56pm

Printer Tests

Test	Status	Time
PRNT	Pass	1:56pm

CRC Tests

Test	Status	Time
COMP	Pass	1:56pm
CAL	Pass	1:56pm

Preventive Maintenance
Status: Pass



Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Lenoir Instrument Location Lenoir Co. S.O.

Instrument Serial No. 008639 130 Queen St, Kinston, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

(1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;

(2) Verify instrument displays time and date;

(3) Initiate breath test sequence;

(4) Enter information as prompted;

(5) Verify instrument accuracy;

(6) When "PLEASE BLOW" appears, collect breath sample;

(7) When "PLEASE BLOW" appears, collect breath sample;

(8) Print test record;

(9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and

(10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 4th day of June, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.

Signature of Certifying Official

377722
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

DHHS 4080 (04/20)

Intox EC/IR-II: Subject Test

LENOIR COUNTY LENOIR CO SO 530

Serial Number: *008639*
Test Date: *06/04/2026*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name: *Gray, Kelly D*
Permit Number: *0037-7722*
Effective:
02/01/2026-02/01/2028

Officer's Name: *NONE, NONE*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG516203
Exp Date: 06/11/2027

Test	g/210L	Time
DIAG	Pass	12:55pm
AIR BLK	.00	12:56pm
ACCY CHK	.07	12:56pm
AIR BLK	.00	12:58pm
SUB TEST	**.00**	**12:58pm**
AIR BLK	.00	12:59pm
SUB TEST	**.00**	**1:01pm**
AIR BLK	.00	1:02pm

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

LENOIR COUNTY LENOIR CO SO 530

Serial Number: *008639* Test Record Number: *4462*
Test Date: *06/04/2026* Test Time: *1:02pm EDT*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	1:03pm
FLO	Pass	1:03pm
FC	Pass	1:03pm

Temperature Tests

Test	Status	Time
FC1	Pass	1:03pm
SRC	Pass	1:03pm
DET	Pass	1:03pm
BAR	Pass	1:03pm
BT	Pass	1:03pm

Blank Tests

Test	Status	Time
AIR	Pass	1:03pm

Printer Tests

Test	Status	Time
PRNT	Pass	1:04pm

CRC Tests

Test	Status	Time
COMP	Pass	1:04pm
CAL	Pass	1:04pm

Preventive Maintenance
Status: Pass

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Lenoir Instrument Location BAT Mobile Unit 9

Instrument Serial No. OO 8647

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

(1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;

(2) Verify instrument displays time and date;

(3) Initiate breath test sequence;

(4) Enter information as prompted;

(5) Verify instrument accuracy;

(6) When "PLEASE BLOW" appears, collect breath sample;

(7) When "PLEASE BLOW" appears, collect breath sample;

(8) Print test record;

(9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and

(10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 27th day of June, 20 26 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.

Signature of Certifying Official

226313
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

DHHS 4080 (04/20)

Intox EC/IR-II: Subject Test

LENOIR COUNTY BAT MOBILE UNIT 9 530

Serial Number: *008647*
Test Date: *06/27/2026*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name: *Sharpe Jr., Robert J*
Permit Number: *1820-8591*
Effective:
02/01/2026-02/01/2028

Officer's Name: *NONE, NONE*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG516203
Exp Date: 06/11/2027

Test	g/210L	Time
DIAG	Pass	7:08pm
AIR BLK	.00	7:09pm
ACCY CHK	.07	7:10pm
AIR BLK	.00	7:11pm
SUB TEST	**.00**	**7:11pm**
AIR BLK	.00	7:12pm
SUB TEST	**.00**	**7:13pm**
AIR BLK	.00	7:14pm

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

LENOIR COUNTY BAT MOBILE UNIT 9 530

Serial Number: *008647* Test Record Number: *2995*
Test Date: *06/27/2026* Test Time: *7:15pm EDT*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	7:15pm
FLO	Pass	7:15pm
FC	Pass	7:15pm

Temperature Tests

Test	Status	Time
FC1	Pass	7:16pm
SRC	Pass	7:16pm
DET	Pass	7:16pm
BAR	Pass	7:16pm
BT	Pass	7:16pm

Blank Tests

Test	Status	Time
AIR	Pass	7:16pm


Printer Tests

Test	Status	Time
PRNT	Pass	7:16pm

CRC Tests

Test	Status	Time
COMP	Pass	7:16pm
CAL	Pass	7:16pm

Preventive Maintenance
Status: Pass



Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Lenoir Instrument Location BAT Mobile Unit 9

Instrument Serial No. 008704

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

(1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;

(2) Verify instrument displays time and date;

(3) Initiate breath test sequence;

(4) Enter information as prompted;

(5) Verify instrument accuracy;

(6) When "PLEASE BLOW" appears, collect breath sample;

(7) When "PLEASE BLOW" appears, collect breath sample;

(8) Print test record;

(9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and

(10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 27th day of June, 20 24 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.

Signature of Certifying Official

2264313
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

DHHS 4080 (04/20)

Intox EC/IR-II: Subject Test

LENOIR COUNTY BAT MOBILE UNIT 9 530

Serial Number: *008704*
Test Date: *06/27/2026*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name: *Sharpe Jr., Robert J*
Permit Number: *1820-8591*
Effective:
02/01/2026-02/01/2028

Officer's Name: *NONE, NONE*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG506303
Exp Date: 03/04/2027

Test	g/210L	Time
DIAG	Pass	7:07pm
AIR BLK	.00	7:08pm
ACCY CHK	.07	7:08pm
AIR BLK	.00	7:09pm
SUB TEST	**.00**	**7:10pm**
AIR BLK	.00	7:11pm
SUB TEST	**.00**	**7:12pm**
AIR BLK	.00	7:13pm

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

LENOIR COUNTY BAT MOBILE UNIT 9 530

Serial Number: *008704* Test Record Number: *1045*
Test Date: *06/27/2026* Test Time: *7:14pm EDT*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	7:14pm
FLO	Pass	7:14pm
FC	Pass	7:14pm

Temperature Tests

Test	Status	Time
FC1	Pass	7:14pm
SRC	Pass	7:14pm
DET	Pass	7:14pm
BAR	Pass	7:14pm
BT	Pass	7:14pm

Blank Tests

Test	Status	Time
AIR	Pass	7:15pm

Printer Tests

Test	Status	Time
PRNT	Pass	7:15pm

CRC Tests

Test	Status	Time
COMP	Pass	7:15pm
CAL	Pass	7:15pm

Preventive Maintenance
Status: Pass

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Lenoir Instrument Location BAT Mobile Unit 9

Instrument Serial No. 008826

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

(1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;

(2) Verify instrument displays time and date;

(3) Initiate breath test sequence;

(4) Enter information as prompted;

(5) Verify instrument accuracy;

(6) When "PLEASE BLOW" appears, collect breath sample;

(7) When "PLEASE BLOW" appears, collect breath sample;

(8) Print test record;

(9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and

(10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 27th day of June, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.

Signature of Certifying Official

2266313
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

DHHS 4080 (04/20)

Intox EC/IR-II: Subject Test

LENOIR COUNTY BAT MOBILE UNIT 9 530

Serial Number: *008826*
Test Date: *06/27/2026*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name: *Sharpe Jr., Robert J*
Permit Number: *1820-8591*
Effective:
02/01/2026-02/01/2028

Officer's Name: *NONE, NONE*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG516204
Exp Date: 06/11/2027

Test	g/210L	Time
DIAG	Pass	7:06pm
AIR BLK	.00	7:07pm
ACCY CHK	.07	7:08pm
AIR BLK	.00	7:09pm
SUB TEST	**.00**	**7:09pm**
AIR BLK	.00	7:10pm
SUB TEST	**.00**	**7:12pm**
AIR BLK	.00	7:12pm

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

LENOIR COUNTY BAT MOBILE UNIT 9 530

Serial Number: *008826* Test Record Number: *8683*
Test Date: *06/27/2026* Test Time: *7:13pm EDT*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	7:13pm
FLO	Pass	7:13pm
FC	Pass	7:13pm

Temperature Tests

Test	Status	Time
FC1	Pass	7:13pm
SRC	Pass	7:13pm
DET	Pass	7:13pm
BAR	Pass	7:13pm
BT	Pass	7:13pm

Blank Tests

Test	Status	Time
AIR	Pass	7:14pm

Printer Tests

Test	Status	Time
PRNT	Pass	7:14pm

CRC Tests

Test	Status	Time
COMP	Pass	7:14pm
CAL	Pass	7:14pm

Preventive Maintenance
Status: Pass



Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Lincoln Instrument Location BAT Mobile Unit 8

Instrument Serial No. 008615 –

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

(1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;

(2) Verify instrument displays time and date;

(3) Initiate breath test sequence;

(4) Enter information as prompted;

(5) Verify instrument accuracy;

(6) When "PLEASE BLOW" appears, collect breath sample;

(7) When "PLEASE BLOW" appears, collect breath sample;

(8) Print test record;

(9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and

(10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 20 day of June, 20 26 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.

THE GREAT SEAL OF THE STATE OF NORTH CAROLINA

Signature of Certifying Official

2219283
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

LINCOLN COUNTY BAT MOBILE UNIT 8 540

Serial Number: *008615*
Test Date: *06/20/2026*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name: *Glasscock, Jerry D*
Permit Number: *7180-9235*
Effective:
02/01/2026-02/01/2028

Officer's Name: *NONE, NONE*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG506303
Exp Date: 03/04/2027

Test	g/210L	Time
DIAG	Pass	10:02am
AIR BLK	.00	10:03am
ACCY CHK	.07	10:04am
AIR BLK	.00	10:05am
SUB TEST	**.00**	**10:05am**
AIR BLK	.00	10:06am
SUB TEST	**.00**	**10:08am**
AIR BLK	.00	10:09am

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

LINCOLN COUNTY BAT MOBILE UNIT 8 540

Serial Number: *008615* Test Record Number: *6345*
Test Date: *06/20/2026* Test Time: *10:10am EDT*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	10:10am
FLO	Pass	10:10am
FC	Pass	10:10am

Temperature Tests

Test	Status	Time
FC1	Pass	10:10am
SRC	Pass	10:10am
DET	Pass	10:10am
BAR	Pass	10:10am
BT	Pass	10:10am

Blank Tests

Test	Status	Time
AIR	Pass	10:11am

Printer Tests

Test	Status	Time
PRNT	Pass	10:11am

CRC Tests

Test	Status	Time
COMP	Pass	10:11am
CAL	Pass	10:11am

Preventive Maintenance
Status: Pass

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Lincoln Instrument Location BAT Mobile Unit 8

Instrument Serial No. 008736 –

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

(1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;

(2) Verify instrument displays time and date;

(3) Initiate breath test sequence;

(4) Enter information as prompted;

(5) Verify instrument accuracy;

(6) When "PLEASE BLOW" appears, collect breath sample;

(7) When "PLEASE BLOW" appears, collect breath sample;

(8) Print test record;

(9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and

(10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 20 day of June, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.

Signature of Certifying Official

2219283
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

DHHS 4080 (04/20)

Intox EC/IR-II: Subject Test

LINCOLN COUNTY BAT MOBILE UNIT 8 540

Serial Number: *008736*
Test Date: *06/20/2026*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name: *Glasscock, Jerry D*
Permit Number: *7180-9235*
Effective:
02/01/2026-02/01/2028

Officer's Name: *NONE, NONE*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG506303
Exp Date: 03/04/2027

Test	g/210L	Time
DIAG	Pass	10:02am
AIR BLK	.00	10:03am
ACCY CHK	.07	10:04am
AIR BLK	.00	10:05am
SUB TEST	**.00**	**10:06am**
AIR BLK	.00	10:07am
SUB TEST	**.00**	**10:08am**
AIR BLK	.00	10:09am

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

LINCOLN COUNTY BAT MOBILE UNIT 8 540

Serial Number: *008736* Test Record Number: *1700*
Test Date: *06/20/2026* Test Time: *10:10am EDT*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	10:10am
FLO	Pass	10:10am
FC	Pass	10:10am

Temperature Tests

Test	Status	Time
FC1	Pass	10:10am
SRC	Pass	10:10am
DET	Pass	10:10am
BAR	Pass	10:10am
BT	Pass	10:10am

Blank Tests

Test	Status	Time
AIR	Pass	10:11am

Printer Tests

Test	Status	Time
PRNT	Pass	10:11am

CRC Tests

Test	Status	Time
COMP	Pass	10:11am
CAL	Pass	10:11am

Preventive Maintenance
Status: Pass

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Lincoln Instrument Location BAT Mobile Unit 8

Instrument Serial No. 008775

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

(1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;

(2) Verify instrument displays time and date;

(3) Initiate breath test sequence;

(4) Enter information as prompted;

(5) Verify instrument accuracy;

(6) When "PLEASE BLOW" appears, collect breath sample;

(7) When "PLEASE BLOW" appears, collect breath sample;

(8) Print test record;

(9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and

(10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 20 day of June, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.

Signature of Certifying Official

2219283
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

LINCOLN COUNTY BAT MOBILE UNIT 8 540

Serial Number: *008775*
Test Date: *06/20/2026*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name: *Glasscock, Jerry D*
Permit Number: *7180-9235*
Effective:
02/01/2026-02/01/2028

Officer's Name: *NONE, NONE*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG506303
Exp Date: 03/04/2027

Test	g/210L	Time
DIAG	Pass	10:03am
AIR BLK	.00	10:04am
ACCY CHK	.08	10:05am
AIR BLK	.00	10:05am
SUB TEST	**.00**	**10:06am**
AIR BLK	.00	10:07am
SUB TEST	**.00**	**10:08am**
AIR BLK	.00	10:09am

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

LINCOLN COUNTY BAT MOBILE UNIT 8 540

Serial Number: *008775* Test Record Number: *2555*
Test Date: *06/20/2026* Test Time: *10:10am EDT*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	10:10am
FLO	Pass	10:10am
FC	Pass	10:10am

Temperature Tests

Test	Status	Time
FC1	Pass	10:10am
SRC	Pass	10:10am
DET	Pass	10:10am
BAR	Pass	10:10am
BT	Pass	10:10am

Blank Tests

Test	Status	Time
AIR	Pass	10:11am

Printer Tests

Test	Status	Time
PRNT	Pass	10:11am

CRC Tests

Test	Status	Time
COMP	Pass	10:11am
CAL	Pass	10:11am

Preventive Maintenance
Status: Pass

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Lincoln Instrument Location BAT Mobile Unit 8

Instrument Serial No. 008816 —

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

(1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;

(2) Verify instrument displays time and date;

(3) Initiate breath test sequence;

(4) Enter information as prompted;

(5) Verify instrument accuracy;

(6) When "PLEASE BLOW" appears, collect breath sample;

(7) When "PLEASE BLOW" appears, collect breath sample;

(8) Print test record;

(9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and

(10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 20 day of June, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.

Signature of Certifying Official

2219283
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

DHHS 4080 (04/20)

Intox EC/IR-II: Subject Test

LINCOLN COUNTY BAT MOBILE UNIT 8 540

Serial Number: *008816*
Test Date: *06/20/2026*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name: *Glasscock, Jerry D*
Permit Number: *7180-9235*
Effective:
02/01/2026-02/01/2028

Officer's Name: *NONE, NONE*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG431002
Exp Date: 11/05/2026

Test	g/210L	Time
DIAG	Pass	10:04am
AIR BLK	.00	10:05am
ACCY CHK	.07	10:06am
AIR BLK	.00	10:07am
SUB TEST	**.00**	**10:07am**
AIR BLK	.00	10:08am
SUB TEST	**.00**	**10:10am**
AIR BLK	.00	10:10am

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

LINCOLN COUNTY BAT MOBILE UNIT 8 540

Serial Number: *008816* Test Record Number: *8129*
Test Date: *06/20/2026* Test Time: *10:11am EDT*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	10:11am
FLO	Pass	10:11am
FC	Pass	10:11am

Temperature Tests

Test	Status	Time
FC1	Pass	10:11am
SRC	Pass	10:11am
DET	Pass	10:11am
BAR	Pass	10:11am
BT	Pass	10:11am

Blank Tests

Test	Status	Time
AIR	Pass	10:12am

Printer Tests

Test	Status	Time
PRNT	Pass	10:12am

CRC Tests

Test	Status	Time
COMP	Pass	10:12am
CAL	Pass	10:12am

Preventive Maintenance
Status: Pass

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Lincoln Instrument Location BAT Mobile Unit 8

Instrument Serial No. 008929 —

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

(1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;

(2) Verify instrument displays time and date;

(3) Initiate breath test sequence;

(4) Enter information as prompted;

(5) Verify instrument accuracy;

(6) When "PLEASE BLOW" appears, collect breath sample;

(7) When "PLEASE BLOW" appears, collect breath sample;

(8) Print test record;

(9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and

(10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 20 day of June, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.

THE GREAT SEAL OF THE STATE OF NORTH CAROLINA

Signature of Certifying Official

2219283
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

DHHS 4080 (04-20)

Intox EC/IR-II: Subject Test

LINCOLN COUNTY BAT MOBILE UNIT 8 540

Serial Number: *008929*
Test Date: *06/20/2026*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name: *Glasscock, Jerry D*
Permit Number: *7180-9235*
Effective:
02/01/2026-02/01/2028

Officer's Name: *NONE, NONE*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG506303
Exp Date: 03/04/2027

Test	g/210L	Time
DIAG	Pass	10:04am
AIR BLK	.00	10:05am
ACCY CHK	.07	10:06am
AIR BLK	.00	10:07am
SUB TEST	**.00**	**10:08am**
AIR BLK	.00	10:09am
SUB TEST	**.00**	**10:10am**
AIR BLK	.00	10:11am

Reported AC: .00 g/210L

Signature Of Chemical Analyst

Court CVR

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

LINCOLN COUNTY BAT MOBILE UNIT 8 540

Serial Number: *008929* Test Record Number: *1838*
Test Date: *06/20/2026* Test Time: *10:12am EDT*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	10:13am
FLO	Pass	10:13am
FC	Pass	10:13am

Temperature Tests

Test	Status	Time
FC1	Pass	10:13am
SRC	Pass	10:13am
DET	Pass	10:13am
BAR	Pass	10:13am
BT	Pass	10:13am

Blank Tests

Test	Status	Time
AIR	Pass	10:14am

Printer Tests

Test	Status	Time
PRNT	Pass	10:14am

CRC Tests

Test	Status	Time
COMP	Pass	10:14am
CAL	Pass	10:14am

Preventive Maintenance
Status: Pass



Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Macon Instrument Location Macon Co. Magistrate

Instrument Serial No. 008795 Highlands, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

(1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;

(2) Verify instrument displays time and date;

(3) Initiate breath test sequence;

(4) Enter information as prompted;

(5) Verify instrument accuracy;

(6) When "PLEASE BLOW" appears, collect breath sample;

(7) When "PLEASE BLOW" appears, collect breath sample;

(8) Print test record;

(9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and

(10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 8th day of June, 20 26 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.

Owl R. Cuth
Signature of Certifying Official

843310
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

DHHS 4080 (04/20)

Intox EC/IR-II: Subject Test

MACON COUNTY MACON CO MAGISTRATE 550

Serial Number: *008795*
Test Date: *06/08/2026*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name: *Cutler, Daniel R*
Permit Number: *0084-3310*
Effective:
02/01/2026-02/01/2028

Officer's Name: *NONE, NONE*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG534301
Exp Date: 12/09/2027

Test	g/210L	Time
DIAG	Pass	4:03pm
AIR BLK	.00	4:03pm
ACCY CHK	.08	4:04pm
AIR BLK	.00	4:06pm
SUB TEST	**.00**	**4:06pm**
AIR BLK	.00	4:07pm
SUB TEST	**.00**	**4:09pm**
AIR BLK	.00	4:09pm

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

MACON COUNTY MACON CO MAGISTRATE 550

Serial Number: *008795* Test Record Number: *782*
Test Date: *06/08/2026* Test Time: *4:10pm EDT*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	4:10pm
FLO	Pass	4:10pm
FC	Pass	4:10pm

Temperature Tests

Test	Status	Time
FC1	Pass	4:10pm
SRC	Pass	4:10pm
DET	Pass	4:10pm
BAR	Pass	4:10pm
BT	Pass	4:10pm

Blank Tests

Test	Status	Time
AIR	Pass	4:11pm

Printer Tests

Test	Status	Time
PRNT	Pass	4:11pm

CRC Tests

Test	Status	Time
COMP	Pass	4:11pm
CAL	Pass	4:11pm

Preventive Maintenance
Status: Pass

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Madison Instrument Location Mars Hill PD

Instrument Serial No. 008582 Mars Hill, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

(1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;

(2) Verify instrument displays time and date;

(3) Initiate breath test sequence;

(4) Enter information as prompted;

(5) Verify instrument accuracy;

(6) When "PLEASE BLOW" appears, collect breath sample;

(7) When "PLEASE BLOW" appears, collect breath sample;

(8) Print test record;

(9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and

(10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 16 day of June, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.

Signature of Certifying Official

244987
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

DHHS 4080 (04/20)

Intox EC/IR-II: Subject Test

MADISON COUNTY MARS HILL PD 560

Serial Number: *008582*
Test Date: *06/16/2026*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name: *Loftis, Benjamin C*
Permit Number: *0024-4987*
Effective:
02/01/2026-02/01/2028

Officer's Name: *NONE, NONE*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG516204
Exp Date: 06/11/2027

Test	g/210L	Time
DIAG	Pass	1:05pm
AIR BLK	.00	1:05pm
ACCY CHK	.07	1:06pm
AIR BLK	.00	1:07pm
SUB TEST	**.00**	**1:08pm**
AIR BLK	.00	1:08pm
SUB TEST	**.00**	**1:10pm**
AIR BLK	.00	1:11pm

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

MADISON COUNTY MARS HILL PD 560

Serial Number: *008582* Test Record Number: *1385*
Test Date: *06/16/2026* Test Time: *1:11pm EDT*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	1:12pm
FLO	Pass	1:12pm
FC	Pass	1:12pm

Temperature Tests

Test	Status	Time
FC1	Pass	1:12pm
SRC	Pass	1:12pm
DET	Pass	1:12pm
BAR	Pass	1:12pm
BT	Pass	1:12pm

Blank Tests

Test	Status	Time
AIR	Pass	1:12pm

Printer Tests

Test	Status	Time
PRNT	Pass	1:12pm

CRC Tests

Test	Status	Time
COMP	Pass	1:13pm
CAL	Pass	1:13pm

Preventive Maintenance
Status: Pass

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Madison Instrument Location Madison County Jail

Instrument Serial No. 008599 Marshall, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

(1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;

(2) Verify instrument displays time and date;

(3) Initiate breath test sequence;

(4) Enter information as prompted;

(5) Verify instrument accuracy;

(6) When "PLEASE BLOW" appears, collect breath sample;

(7) When "PLEASE BLOW" appears, collect breath sample;

(8) Print test record;

(9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and

(10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 16 day of June, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.

Signature of Certifying Official

244987
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

DHHS 4080 (04/20)

Intox EC/IR-II: Subject Test

MADISON COUNTY MADISON COUNTY JAIL 560

Serial Number: *008599*
Test Date: *06/16/2026*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name: *Loftis, Benjamin C*
Permit Number: *0024-4987*
Effective:
02/01/2026-02/01/2028

Officer's Name: *NONE, NONE*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG503001
Exp Date: 01/30/2027

Test	g/210L	Time
DIAG	Pass	1:52pm
AIR BLK	.00	1:53pm
ACCY CHK	.07	1:53pm
AIR BLK	.00	1:55pm
SUB TEST	**.00**	**1:55pm**
AIR BLK	.00	1:56pm
SUB TEST	**.00**	**1:58pm**
AIR BLK	.00	1:58pm

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

MADISON COUNTY MADISON COUNTY JAIL 560

Serial Number: *008599* Test Record Number: *1619*
Test Date: *06/16/2026* Test Time: *2:00pm EDT*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	2:00pm
FLO	Pass	2:00pm
FC	Pass	2:00pm

Temperature Tests

Test	Status	Time
FC1	Pass	2:01pm
SRC	Pass	2:01pm
DET	Pass	2:01pm
BAR	Pass	2:01pm
BT	Pass	2:01pm

Blank Tests

Test	Status	Time
AIR	Pass	2:01pm

Printer Tests

Test	Status	Time
PRNT	Pass	2:01pm

CRC Tests

Test	Status	Time
COMP	Pass	2:01pm
CAL	Pass	2:01pm

Preventive Maintenance
Status: Pass



Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County MECKLENBURG Instrument Location HUNTERSVILLE PD

Instrument Serial No. CC-2573 HUNTERSVILLE NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

(1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;

(2) Verify instrument displays time and date;

(3) Initiate breath test sequence;

(4) Enter information as prompted;

(5) Verify instrument accuracy;

(6) When "PLEASE BLOW" appears, collect breath sample;

(7) When "PLEASE BLOW" appears, collect breath sample;

(8) Print test record;

(9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and

(10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 11e day of June, 2024 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.

Signature of Certifying Official

274970
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

DHHS 4080 (04/20)

Intox EC/IR-II: Subject Test

MECKLENBURG COUNTY HUNTERSVILLE PD 590

Serial Number: *008573*
Test Date: *06/16/2026*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name: *Fleming, Tina S*
Permit Number: *0027-4970*
Effective:
02/01/2025-02/01/2027

Officer's Name: *NONE, NONE*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG506302
Exp Date: 03/04/2027

Test	g/210L	Time
DIAG	Pass	10:03am
AIR BLK	.00	10:04am
ACCY CHK	.08	10:05am
AIR BLK	.00	10:06am
SUB TEST	**.00**	**10:06am**
AIR BLK	.00	10:07am
SUB TEST	**.00**	**10:09am**
AIR BLK	.00	10:10am

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

MECKLENBURG COUNTY HUNTERSVILLE PD 590

Serial Number: *008573* Test Record Number: *5769*
Test Date: *06/16/2026* Test Time: *10:11am EDT*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	10:12am
FLO	Pass	10:12am
FC	Pass	10:12am

Temperature Tests

Test	Status	Time
FC1	Pass	10:12am
SRC	Pass	10:12am
DET	Pass	10:12am
BAR	Pass	10:12am
BT	Pass	10:12am

Blank Tests

Test	Status	Time
AIR	Pass	10:12am

Printer Tests

Test	Status	Time
PRNT	Pass	10:12am

CRC Tests

Test	Status	Time
COMP	Pass	10:13am
CAL	Pass	10:13am

Preventive Maintenance
Status: Pass

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Mecklenburg Instrument Location CMPD LEC Charlotte, NC

Instrument Serial No 008594

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

(1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;

(2) Verify instrument displays time and date;

(3) Initiate breath test sequence;

(4) Enter information as prompted;

(5) Verify instrument accuracy;

(6) When "PLEASE BLOW" appears, collect breath sample;

(7) When "PLEASE BLOW" appears, collect breath sample;

(8) Print test record;

(9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and

(10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 23rd day of June, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.

Signature of Certifying Official

849845
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

DHHS 4080 (04/20)

Intox EC/IR-II: Subject Test

MECKLENBURG COUNTY CMPD LEC 590

Serial Number: *008594*
Test Date: *06/23/2026*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name: *Helms, Bryce A*
Permit Number: *0084-9845*
Effective:
02/01/2026-02/01/2028

Officer's Name: *NONE, NONE*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG602101
Exp Date: 01/21/2028

Test	g/210L	Time
DIAG	Pass	12:13pm
AIR BLK	.00	12:14pm
ACCY CHK	.08	12:14pm
AIR BLK	.00	12:16pm
SUB TEST	**.00**	**12:16pm**
AIR BLK	.00	12:17pm
SUB TEST	**.00**	**12:19pm**
AIR BLK	.00	12:19pm

Reported AC; .00 g/210L

Bryce Helms
Signature of Chemical Analyst

Court CVR

Bryce Helms
Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

MECKLENBURG COUNTY CMPD LEC 590

Serial Number: *008594* Test Record Number: *6942*
Test Date: *06/23/2026* Test Time: *12:20pm EDT*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	12:20pm
FLO	Pass	12:20pm
FC	Pass	12:21pm

Temperature Tests

Test	Status	Time
FC1	Pass	12:21pm
SRC	Pass	12:21pm
DET	Pass	12:21pm
BAR	Pass	12:21pm
BT	Pass	12:21pm

Blank Tests

Test	Status	Time
AIR	Pass	12:21pm

Printer Tests

Test	Status	Time
PRNT	Pass	12:21pm

CRC Tests

Test	Status	Time
COMP	Pass	12:21pm
CAL	Pass	12:21pm

Preventive Maintenance
Status: Pass

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Mecklenburg Instrument Location BAT Mobile Unit 8

Instrument Serial No. 008615

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

(1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;

(2) Verify instrument displays time and date;

(3) Initiate breath test sequence;

(4) Enter information as prompted;

(5) Verify instrument accuracy;

(6) When "PLEASE BLOW" appears, collect breath sample;

(7) When "PLEASE BLOW" appears, collect breath sample;

(8) Print test record;

(9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and

(10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 4 day of June, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.

Signature of Certifying Official

2219283
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

MECKLENBURG COUNTY BAT MOBILE UNIT 8
590

Serial Number: *008615*
Test Date: *06/04/2026*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name: *Glasscock, Jerry D*
Permit Number: *7180-9235*
Effective:
02/01/2026-02/01/2028

Officer's Name: *NONE, NONE*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG506303
Exp Date: 03/04/2027

Test	g/210L	Time
DIAG	Pass	9:05am
AIR BLK	.00	9:06am
ACCY CHK	.07	9:07am
AIR BLK	.00	9:07am
SUB TEST	**.00**	**9:09am**
AIR BLK	.00	9:10am
SUB TEST	**.00**	**9:12am**
AIR BLK	.00	9:13am

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

MECKLENBURG COUNTY BAT MOBILE UNIT 8 590

Serial Number: *008615* Test Record Number: *6326*
Test Date: *06/04/2026* Test Time: *9:13am EDT*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	9:14am
FLO	Pass	9:14am
FC	Pass	9:14am

Temperature Tests

Test	Status	Time
FC1	Pass	9:14am
SRC	Pass	9:14am
DET	Pass	9:14am
BAR	Pass	9:14am
BT	Pass	9:14am

Blank Tests

Test	Status	Time
AIR	Pass	9:14am

Printer Tests

Test	Status	Time
PRNT	Pass	9:14am

CRC Tests

Test	Status	Time
COMP	Pass	9:15am
CAL	Pass	9:15am

Preventive Maintenance
Status: Pass



Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Mecklenburg Instrument Location BAT Mobile Unit 8

Instrument Serial No. 008615

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

(1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;

(2) Verify instrument displays time and date;

(3) Initiate breath test sequence;

(4) Enter information as prompted;

(5) Verify instrument accuracy;

(6) When "PLEASE BLOW" appears, collect breath sample;

(7) When "PLEASE BLOW" appears, collect breath sample;

(8) Print test record;

(9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and

(10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 11 day of June, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.

THE GREAT SEAL OF THE STATE OF NORTH CAROLINA

Signature of Certifying Official

2219283
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

DHHS 4080 (04/20)

Intox EC/IR-II: Subject Test

MECKLENBURG COUNTY BAT MOBILE UNIT 8
590

Serial Number: *008615*
Test Date: *06/11/2026*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name: *Glasscock, Jerry D*
Permit Number: *7180-9235*
Effective:
02/01/2026-02/01/2028

Officer's Name: *NONE, NONE*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG506303
Exp Date: 03/04/2027

Test	g/210L	Time
DIAG	Pass	8:12pm
AIR BLK	.00	8:13pm
ACCY CHK	.07	8:14pm
AIR BLK	.00	8:15pm
SUB TEST	**.00**	**8:16pm**
AIR BLK	.00	8:17pm
SUB TEST	**.00**	**8:18pm**
AIR BLK	.00	8:19pm

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

MECKLENBURG COUNTY BAT MOBILE UNIT 8 590

Serial Number: *008615* Test Record Number: *6332*
Test Date: *06/11/2026* Test Time: *8:19pm EDT*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	8:20pm
FLO	Pass	8:20pm
FC	Pass	8:20pm

Temperature Tests

Test	Status	Time
FC1	Pass	8:20pm
SRC	Pass	8:20pm
DET	Pass	8:20pm
BAR	Pass	8:20pm
BT	Pass	8:20pm

Blank Tests

Test	Status	Time
AIR	Pass	8:21pm

Printer Tests

Test	Status	Time
PRNT	Pass	8:21pm

CRC Tests

Test	Status	Time
COMP	Pass	8:21pm
CAL	Pass	8:21pm

Preventive Maintenance
Status: Pass

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Mecklenburg Instrument Location BAT Mobile Unit 8

Instrument Serial No. 008615 –

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

(1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;

(2) Verify instrument displays time and date;

(3) Initiate breath test sequence;

(4) Enter information as prompted;

(5) Verify instrument accuracy;

(6) When "PLEASE BLOW" appears, collect breath sample;

(7) When "PLEASE BLOW" appears, collect breath sample;

(8) Print test record;

(9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and

(10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 18 day of June, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.

THE GREAT SEAL OF THE STATE OF NORTH CAROLINA

Signature of Certifying Official

2219283
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

MECKLENBURG COUNTY BAT MOBILE UNIT 8
590

Serial Number: *008615*
Test Date: *06/18/2026*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name: *Glasscock, Jerry D*
Permit Number: *7180-9235*
Effective:
02/01/2026-02/01/2028

Officer's Name: *NONE, NONE*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG506303
Exp Date: 03/04/2027

Test	g/210L	Time
DIAG	Pass	9:59pm
AIR BLK	.00	10:00pm
ACCY CHK	.07	10:00pm
AIR BLK	.00	10:02pm
SUB TEST	**.00**	**10:02pm**
AIR BLK	.00	10:03pm
SUB TEST	**.00**	**10:06pm**
AIR BLK	.00	10:07pm

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

MECKLENBURG COUNTY BAT MOBILE UNIT 8 590

Serial Number: *008615* Test Record Number: *6341*
Test Date: *06/18/2026* Test Time: *10:07pm EDT*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	10:07pm
FLO	Pass	10:07pm
FC	Pass	10:07pm

Temperature Tests

Test	Status	Time
FC1	Pass	10:07pm
SRC	Pass	10:07pm
DET	Pass	10:07pm
BAR	Pass	10:07pm
BT	Pass	10:07pm

Blank Tests

Test	Status	Time
AIR	Pass	10:08pm

Printer Tests

Test	Status	Time
PRNT	Pass	10:08pm

CRC Tests

Test	Status	Time
COMP	Pass	10:08pm
CAL	Pass	10:08pm

Preventive Maintenance
Status: Pass

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Mecklenburg Instrument Location BAT Mobile Unit 8

Instrument Serial No. 008615 —

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

(1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;

(2) Verify instrument displays time and date;

(3) Initiate breath test sequence;

(4) Enter information as prompted;

(5) Verify instrument accuracy;

(6) When "PLEASE BLOW" appears, collect breath sample;

(7) When "PLEASE BLOW" appears, collect breath sample;

(8) Print test record;

(9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and

(10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 19 day of June, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.

Signature of Certifying Official

2219283
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

DHHS 4080 (04/20)

Intox EC/IR-II: Subject Test

MECKLENBURG COUNTY BAT MOBILE UNIT 8
590

Serial Number: *008615*
Test Date: *06/19/2026*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name: *Glasscock, Jerry D*
Permit Number: *7180-9235*
Effective:
02/01/2026-02/01/2028

Officer's Name: *NONE, NONE*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG506303
Exp Date: 03/04/2027

Test	g/210L	Time
DIAG	Pass	8:34pm
AIR BLK	.00	8:35pm
ACCY CHK	.07	8:36pm
AIR BLK	.00	8:37pm
SUB TEST	**.00**	**8:37pm**
AIR BLK	.00	8:38pm
SUB TEST	**.00**	**8:40pm**
AIR BLK	.00	8:41pm

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

MECKLENBURG COUNTY BAT MOBILE UNIT 8 590

Serial Number: *008615* Test Record Number: *6343*
Test Date: *06/19/2026* Test Time: *8:41pm EDT*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	8:41pm
FLO	Pass	8:41pm
FC	Pass	8:41pm

Temperature Tests

Test	Status	Time
FC1	Pass	8:41pm
SRC	Pass	8:41pm
DET	Pass	8:41pm
BAR	Pass	8:41pm
BT	Pass	8:41pm

Blank Tests

Test	Status	Time
AIR	Pass	8:42pm

Printer Tests

Test	Status	Time
PRNT	Pass	8:42pm

CRC Tests

Test	Status	Time
COMP	Pass	8:42pm
CAL	Pass	8:42pm

Preventive Maintenance
Status: Pass



Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Mecklenburg Instrument Location BAT Mobile Unit 8

Instrument Serial No. 008615

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

(1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;

(2) Verify instrument displays time and date;

(3) Initiate breath test sequence;

(4) Enter information as prompted;

(5) Verify instrument accuracy;

(6) When "PLEASE BLOW" appears, collect breath sample;

(7) When "PLEASE BLOW" appears, collect breath sample;

(8) Print test record;

(9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and

(10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 20 day of June, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.

Signature of Certifying Official

2219283
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

DHHS 4080 (04/20)

Intox EC/IR-II: Subject Test

MECKLENBURG COUNTY BAT MOBILE UNIT 8
590

Serial Number: *008615*
Test Date: *06/20/2026*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name: *Glasscock, Jerry D*
Permit Number: *7180-9235*
Effective:
02/01/2026-02/01/2028

Officer's Name: *NONE, NONE*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG506303
Exp Date: 03/04/2027

Test	g/210L	Time
DIAG	Pass	9:26pm
AIR BLK	.00	9:27pm
ACCY CHK	.07	9:27pm
AIR BLK	.00	9:28pm
SUB TEST	**.00**	**9:29pm**
AIR BLK	.00	9:30pm
SUB TEST	**.00**	**9:32pm**
AIR BLK	.00	9:32pm

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev 12/2007

Intox EC/IR-II: Preventive Maintenance

MECKLENBURG COUNTY BAT MOBILE UNIT 8 590

Serial Number: *008615* Test Record Number: *6347*
Test Date: *06/20/2026* Test Time: *9:33pm EDT*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	9:33pm
FLO	Pass	9:33pm
FC	Pass	9:33pm

Temperature Tests

Test	Status	Time
FC1	Pass	9:33pm
SRC	Pass	9:33pm
DET	Pass	9:33pm
BAR	Pass	9:33pm
BT	Pass	9:33pm

Blank Tests

Test	Status	Time
AIR	Pass	9:34pm

Printer Tests

Test	Status	Time
PRNT	Pass	9:34pm

CRC Tests

Test	Status	Time
COMP	Pass	9:34pm
CAL	Pass	9:34pm

Preventive Maintenance
Status: Pass

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Mecklenburg Instrument Location Mecklenburg Co SO
Charlotte, NC

Instrument Serial No. 008665

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

(1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;

(2) Verify instrument displays time and date;

(3) Initiate breath test sequence;

(4) Enter information as prompted;

(5) Verify instrument accuracy;

(6) When "PLEASE BLOW" appears, collect breath sample;

(7) When "PLEASE BLOW" appears, collect breath sample;

(8) Print test record;

(9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and

(10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 23rd day of June, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.

Signature of Certifying Official

849845
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

DHHS 4080 (04/20)

Intox EC/IR-II: Subject Test

MECKLENBURG COUNTY SHERIFFS OFFICE 590

Serial Number: *008665*
Test Date: *06/23/2026*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name: *Helms, Bryce A*
Permit Number: *0084-9845*
Effective:
02/01/2026-02/01/2028

Officer's Name: *NONE, NONE*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG534301
Exp Date: 12/09/2027

Test	g/210L	Time
DIAG	Pass	11:34am
AIR BLK	.00	11:34am
ACCY CHK	.07	11:35am
AIR BLK	.00	11:36am
SUB TEST	**.00**	**11:37am**
AIR BLK	.00	11:38am
SUB TEST	**.00**	**11:39am**
AIR BLK	.00	11:40am

Reported AC: .00 g/210L

Bryce Helms
Signature of Chemical Analyst

Court CVR

Bryce Helms
Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

MECKLENBURG COUNTY SHERIFFS OFFICE 590

Serial Number: *008665* Test Record Number: *6039*
Test Date: *06/23/2026* Test Time: *11:41am EDT*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	11:41am
FLO	Pass	11:41am
FC	Pass	11:41am

Temperature Tests

Test	Status	Time
FC1	Pass	11:41am
SRC	Pass	11:41am
DET	Pass	11:41am
BAR	Pass	11:41am
BT	Pass	11:41am

Blank Tests

Test	Status	Time
AIR	Pass	11:42am


Printer Tests

Test	Status	Time
PRNT	Pass	11:42am

CRC Tests

Test	Status	Time
COMP	Pass	11:42am
CAL	Pass	11:42am

Preventive Maintenance
Status: Pass

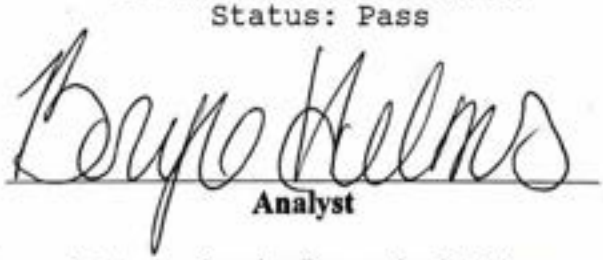

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Mecklenburg Instrument Location CMPD LEC

Instrument Serial No. 008091 Charlotte, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

(1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;

(2) Verify instrument displays time and date;

(3) Initiate breath test sequence;

(4) Enter information as prompted;

(5) Verify instrument accuracy;

(6) When "PLEASE BLOW" appears, collect breath sample;

(7) When "PLEASE BLOW" appears, collect breath sample;

(8) Print test record;

(9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and

(10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 23rd day of June, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.

Signature of Certifying Official

849845
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

DHHS 4080 (04/20)

Intox EC/IR-II: Subject Test

MECKLENBURG COUNTY CMPD LEC 590

Serial Number: *008691*
Test Date: *06/23/2026*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name: *Helms, Bryce A*
Permit Number: *0084-9845*
Effective:
02/01/2026-02/01/2028

Officer's Name: *NONE, NONE*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG534301
Exp Date: 12/09/2027

Test	g/210L	Time
DIAG	Pass	12:15pm
AIR BLK	.00	12:15pm
ACCY CHK	.07	12:16pm
AIR BLK	.00	12:17pm
SUB TEST	**.00**	**12:18pm**
AIR BLK	.00	12:19pm
SUB TEST	**.00**	**12:21pm**
AIR BLK	.00	12:22pm

Reported AC: .00 g/210L

Bryce Helms
Signature of Chemical Analyst

Court CVR

Bryce Helms
Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

MECKLENBURG COUNTY CMPD LEC 590

Serial Number: *008691* Test Record Number: *10204*
Test Date: *06/23/2026* Test Time: *12:24pm EDT*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	12:25pm
FLO	Pass	12:25pm
FC	Pass	12:25pm

Temperature Tests

Test	Status	Time
FC1	Pass	12:25pm
SRC	Pass	12:25pm
DET	Pass	12:25pm
BAR	Pass	12:25pm
BT	Pass	12:25pm

Blank Tests

Test	Status	Time
AIR	Pass	12:25pm


Printer Tests

Test	Status	Time
PRNT	Pass	12:25pm

CRC Tests

Test	Status	Time
COMP	Pass	12:26pm
CAL	Pass	12:26pm

Preventive Maintenance
Status: Pass

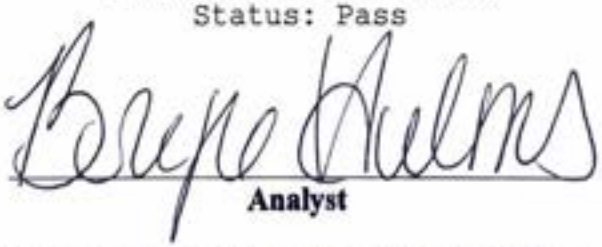

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Mecklenburg Instrument Location BAT Mobile Unit 8

Instrument Serial No. 008736

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

(1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;

(2) Verify instrument displays time and date;

(3) Initiate breath test sequence;

(4) Enter information as prompted;

(5) Verify instrument accuracy;

(6) When "PLEASE BLOW" appears, collect breath sample;

(7) When "PLEASE BLOW" appears, collect breath sample;

(8) Print test record;

(9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and

(10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 4 day of June, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.

Signature of Certifying Official

2219283
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

DHHS 4080 (04/20)

Intox EC/IR-II: Subject Test

MECKLENBURG COUNTY BAT MOBILE UNIT 8
590

Serial Number: *008736*
Test Date: *06/04/2026*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name: *Glasscock, Jerry D*
Permit Number: *7180-9235*
Effective:
02/01/2026-02/01/2028

Officer's Name: *NONE, NONE*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG506303
Exp Date: 03/04/2027

Test	g/210L	Time
DIAG	Pass	9:06am
AIR BLK	.00	9:07am
ACCY CHK	.07	9:07am
AIR BLK	.00	9:08am
SUB TEST	**.00**	**9:09am**
AIR BLK	.00	9:10am
SUB TEST	**.00**	**9:12am**
AIR BLK	.00	9:12am

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

MECKLENBURG COUNTY BAT MOBILE UNIT 8 590

Serial Number: *008736* Test Record Number: *1682*
Test Date: *06/04/2026* Test Time: *9:13am EDT*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	9:14am
FLO	Pass	9:14am
FC	Pass	9:14am

Temperature Tests

Test	Status	Time
FC1	Pass	9:14am
SRC	Pass	9:14am
DET	Pass	9:14am
BAR	Pass	9:14am
BT	Pass	9:14am

Blank Tests

Test	Status	Time
AIR	Pass	9:14am

Printer Tests

Test	Status	Time
PRNT	Pass	9:15am

CRC Tests

Test	Status	Time
COMP	Pass	9:15am
CAL	Pass	9:15am

Preventive Maintenance
Status: Pass



Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Mecklenburg Instrument Location BAT Mobile Unit 8

Instrument Serial No. 008736 —

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

(1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;

(2) Verify instrument displays time and date;

(3) Initiate breath test sequence;

(4) Enter information as prompted;

(5) Verify instrument accuracy;

(6) When "PLEASE BLOW" appears, collect breath sample;

(7) When "PLEASE BLOW" appears, collect breath sample;

(8) Print test record;

(9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and

(10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 11 day of June, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.

Signature of Certifying Official

2219283
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

DHHS 4080 (04/20)

Intox EC/IR-II: Subject Test

MECKLENBURG COUNTY BAT MOBILE UNIT 8
590

Serial Number: *008736*
Test Date: *06/11/2026*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name: *Glasscock, Jerry D*
Permit Number: *7180-9235*
Effective:
02/01/2026-02/01/2028

Officer's Name: *NONE, NONE*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG506303
Exp Date: 03/04/2027

Test	g/210L	Time
DIAG	Pass	8:13pm
AIR BLK	.00	8:14pm
ACCY CHK	.07	8:14pm
AIR BLK	.00	8:15pm
SUB TEST	**.00**	**8:16pm**
AIR BLK	.00	8:17pm
SUB TEST	**.00**	**8:18pm**
AIR BLK	.00	8:19pm

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

MECKLENBURG COUNTY BAT MOBILE UNIT 8 590

Serial Number: *008736* Test Record Number: *1688*
Test Date: *06/11/2026* Test Time: *8:19pm EDT*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	8:20pm
FLO	Pass	8:20pm
FC	Pass	8:20pm

Temperature Tests

Test	Status	Time
FC1	Pass	8:20pm
SRC	Pass	8:20pm
DET	Pass	8:20pm
BAR	Pass	8:20pm
BT	Pass	8:20pm

Blank Tests

Test	Status	Time
AIR	Pass	8:21pm

Printer Tests

Test	Status	Time
PRNT	Pass	8:21pm

CRC Tests

Test	Status	Time
COMP	Pass	8:21pm
CAL	Pass	8:21pm

Preventive Maintenance
Status: Pass



Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Mecklenburg Instrument Location BAT Mobile Unit 8

Instrument Serial No. 008736 —

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

(1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;

(2) Verify instrument displays time and date;

(3) Initiate breath test sequence;

(4) Enter information as prompted;

(5) Verify instrument accuracy;

(6) When "PLEASE BLOW" appears, collect breath sample;

(7) When "PLEASE BLOW" appears, collect breath sample;

(8) Print test record;

(9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and

(10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 18 day of June, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.

Signature of Certifying Official

2219283
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

DHHS 4080 (04/20)

Intox EC/IR-II: Subject Test

MECKLENBURG COUNTY BAT MOBILE UNIT 8
590

Serial Number: *008736*
Test Date: *06/18/2026*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name: *Glasscock, Jerry D*
Permit Number: *7180-9235*
Effective:
02/01/2026-02/01/2028

Officer's Name: *NONE, NONE*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG506303
Exp Date: 03/04/2027

Test	g/210L	Time
DIAG	Pass	10:00pm
AIR BLK	.00	10:01pm
ACCY CHK	.07	10:02pm
AIR BLK	.00	10:03pm
SUB TEST	**.00**	**10:03pm**
AIR BLK	.00	10:04pm
SUB TEST	**.00**	**10:06pm**
AIR BLK	.00	10:07pm

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

MECKLENBURG COUNTY BAT MOBILE UNIT 8 590

Serial Number: *008736* Test Record Number: *1696*
Test Date: *06/18/2026* Test Time: *10:07pm EDT*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	10:07pm
FLO	Pass	10:07pm
FC	Pass	10:07pm

Temperature Tests

Test	Status	Time
FC1	Pass	10:08pm
SRC	Pass	10:08pm
DET	Pass	10:08pm
BAR	Pass	10:08pm
BT	Pass	10:08pm

Blank Tests

Test	Status	Time
AIR	Pass	10:08pm

Printer Tests

Test	Status	Time
PRNT	Pass	10:08pm

CRC Tests

Test	Status	Time
COMP	Pass	10:08pm
CAL	Pass	10:08pm

Preventive Maintenance
Status: Pass

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Mecklenburg Instrument Location BAT Mobile Unit 8

Instrument Serial No. 008736 –

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

(1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;

(2) Verify instrument displays time and date;

(3) Initiate breath test sequence;

(4) Enter information as prompted;

(5) Verify instrument accuracy;

(6) When "PLEASE BLOW" appears, collect breath sample;

(7) When "PLEASE BLOW" appears, collect breath sample;

(8) Print test record;

(9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and

(10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 19 day of June, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.

Signature of Certifying Official

2219283
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

MECKLENBURG COUNTY BAT MOBILE UNIT 8
590

Serial Number: *008736*
Test Date: *06/19/2026*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name: *Glasscock, Jerry D*
Permit Number: *7180-9235*
Effective:
02/01/2026-02/01/2028

Officer's Name: *NONE, NONE*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG506303
Exp Date: 03/04/2027

Test	g/210L	Time
DIAG	Pass	8:33pm
AIR BLK	.00	8:34pm
ACCY CHK	.07	8:35pm
AIR BLK	.00	8:36pm
SUB TEST	**.00**	**8:36pm**
AIR BLK	.00	8:37pm
SUB TEST	**.00**	**8:38pm**
AIR BLK	.00	8:39pm

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

MECKLENBURG COUNTY BAT MOBILE UNIT 8 590

Serial Number: *008736* Test Record Number: *1698*
Test Date: *06/19/2026* Test Time: *8:39pm EDT*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	8:40pm
FLO	Pass	8:40pm
FC	Pass	8:40pm

Temperature Tests

Test	Status	Time
FC1	Pass	8:40pm
SRC	Pass	8:40pm
DET	Pass	8:40pm
BAR	Pass	8:40pm
BT	Pass	8:40pm

Blank Tests

Test	Status	Time
AIR	Pass	8:41pm

Printer Tests

Test	Status	Time
PRNT	Pass	8:41pm

CRC Tests

Test	Status	Time
COMP	Pass	8:41pm
CAL	Pass	8:41pm

Preventive Maintenance
Status: Pass



Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Mecklenburg Instrument Location BAT Mobile Unit 8

Instrument Serial No. 008736

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

(1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;

(2) Verify instrument displays time and date;

(3) Initiate breath test sequence;

(4) Enter information as prompted;

(5) Verify instrument accuracy;

(6) When "PLEASE BLOW" appears, collect breath sample;

(7) When "PLEASE BLOW" appears, collect breath sample;

(8) Print test record;

(9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and

(10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 20 day of June, 20 26 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.

Signature of Certifying Official

2219283
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

DHHS 4080 (04-20)

Intox EC/IR-II: Subject Test

MECKLENBURG COUNTY BAT MOBILE UNIT 8
590

Serial Number: *008736*
Test Date: *06/20/2026*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name: *Glasscock, Jerry D*
Permit Number: *7180-9235*
Effective:
02/01/2026-02/01/2028

Officer's Name: *NONE, NONE*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG506303
Exp Date: 03/04/2027

Test	g/210L	Time
DIAG	Pass	9:26pm
AIR BLK	.00	9:27pm
ACCY CHK	.07	9:28pm
AIR BLK	.00	9:28pm
SUB TEST	**.00**	**9:29pm**
AIR BLK	.00	9:30pm
SUB TEST	**.00**	**9:32pm**
AIR BLK	.00	9:32pm

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

MECKLENBURG COUNTY BAT MOBILE UNIT 8 590

Serial Number: *008736* Test Record Number: *1702*
Test Date: *06/20/2026* Test Time: *9:33pm EDT*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	9:33pm
FLO	Pass	9:33pm
FC	Pass	9:33pm

Temperature Tests

Test	Status	Time
FC1	Pass	9:33pm
SRC	Pass	9:33pm
DET	Pass	9:33pm
BAR	Pass	9:33pm
BT	Pass	9:33pm

Blank Tests

Test	Status	Time
AIR	Pass	9:34pm

Printer Tests

Test	Status	Time
PRNT	Pass	9:34pm

CRC Tests

Test	Status	Time
COMP	Pass	9:34pm
CAL	Pass	9:34pm

Preventive Maintenance
Status: Pass

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Mecklenburg Instrument Location BAT Mobile Unit 8

Instrument Serial No. 008775 —

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

(1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;

(2) Verify instrument displays time and date;

(3) Initiate breath test sequence;

(4) Enter information as prompted;

(5) Verify instrument accuracy;

(6) When "PLEASE BLOW" appears, collect breath sample;

(7) When "PLEASE BLOW" appears, collect breath sample;

(8) Print test record;

(9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and

(10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 4 day of June, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.

Signature of Certifying Official

2219283
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

DHHS 4080 (04/20)

Intox EC/IR-II: Subject Test

MECKLENBURG COUNTY BAT MOBILE UNIT 8
590

Serial Number: *008775*
Test Date: *06/04/2026*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name: *Glasscock, Jerry D*
Permit Number: *7180-9235*
Effective:
02/01/2026-02/01/2028

Officer's Name: *NONE, NONE*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG506303
Exp Date: 03/04/2027

Test	g/210L	Time
DIAG	Pass	9:07am
AIR BLK	.00	9:08am
ACCY CHK	.08	9:09am
AIR BLK	.00	9:10am
SUB TEST	**.00**	**9:10am**
AIR BLK	.00	9:11am
SUB TEST	**.00**	**9:13am**
AIR BLK	.00	9:14am

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

MECKLENBURG COUNTY BAT MOBILE UNIT 8 590

Serial Number: *008775* Test Record Number: *2532*
Test Date: *06/04/2026* Test Time: *9:15am EDT*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	9:16am
FLO	Pass	9:16am
FC	Pass	9:16am

Temperature Tests

Test	Status	Time
FC1	Pass	9:16am
SRC	Pass	9:16am
DET	Pass	9:16am
BAR	Pass	9:16am
BT	Pass	9:16am

Blank Tests

Test	Status	Time
AIR	Pass	9:16am

Printer Tests

Test	Status	Time
PRNT	Pass	9:17am

CRC Tests

Test	Status	Time
COMP	Pass	9:17am
CAL	Pass	9:17am

Preventive Maintenance
Status: Pass



Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Mecklenburg Instrument Location BAT Mobile Unit 8

Instrument Serial No. 008775 —

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

(1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;

(2) Verify instrument displays time and date;

(3) Initiate breath test sequence;

(4) Enter information as prompted;

(5) Verify instrument accuracy;

(6) When "PLEASE BLOW" appears, collect breath sample;

(7) When "PLEASE BLOW" appears, collect breath sample;

(8) Print test record;

(9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and

(10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 11 day of June, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.

Signature of Certifying Official

2219283
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

MECKLENBURG COUNTY BAT MOBILE UNIT 8
590

Serial Number: *008775*
Test Date: *06/11/2026*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*


Analyst's Name: *Glasscock, Jerry D*
Permit Number: *7180-9235*
Effective:
02/01/2026-02/01/2028

Officer's Name: *NONE, NONE*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG506303
Exp Date: 03/04/2027


Test	g/210L	Time
DIAG	Pass	8:13pm
AIR BLK	.00	8:14pm
ACCY CHK	.08	8:15pm
AIR BLK	.00	8:16pm
SUB TEST	**.00**	**8:16pm**
AIR BLK	.00	8:17pm
SUB TEST	**.00**	**8:19pm**
AIR BLK	.00	8:20pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR

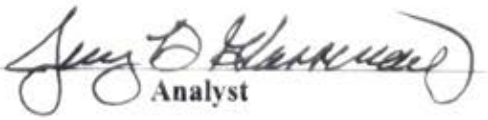

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

MECKLENBURG COUNTY BAT MOBILE UNIT 8 590

Serial Number: *008775* Test Record Number: *2538*
Test Date: *06/11/2026* Test Time: *8:20pm EDT*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	8:20pm
FLO	Pass	8:20pm
FC	Pass	8:20pm

Temperature Tests

Test	Status	Time
FC1	Pass	8:20pm
SRC	Pass	8:20pm
DET	Pass	8:20pm
BAR	Pass	8:20pm
BT	Pass	8:20pm

Blank Tests

Test	Status	Time
AIR	Pass	8:21pm

Printer Tests

Test	Status	Time
PRNT	Pass	8:21pm

CRC Tests

Test	Status	Time
COMP	Pass	8:21pm
CAL	Pass	8:21pm

Preventive Maintenance
Status: Pass



Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Mecklenburg Instrument Location BAT Mobile Unit 8

Instrument Serial No. 008775 –

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

(1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;

(2) Verify instrument displays time and date;

(3) Initiate breath test sequence;

(4) Enter information as prompted;

(5) Verify instrument accuracy;

(6) When "PLEASE BLOW" appears, collect breath sample;

(7) When "PLEASE BLOW" appears, collect breath sample;

(8) Print test record;

(9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and

(10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 18 day of June, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.

Gary D Hasselman
Signature of Certifying Official

2219283
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

MECKLENBURG COUNTY BAT MOBILE UNIT 8
590

Serial Number: *008775*
Test Date: *06/18/2026*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name: *Glasscock, Jerry D*
Permit Number: *7180-9235*
Effective:
02/01/2026-02/01/2028

Officer's Name: *NONE, NONE*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG506303
Exp Date: 03/04/2027

Test	g/210L	Time
DIAG	Pass	10:00pm
AIR BLK	.00	10:01pm
ACCY CHK	.08	10:01pm
AIR BLK	.00	10:02pm
SUB TEST	**.00**	**10:03pm**
AIR BLK	.00	10:03pm
SUB TEST	**.00**	**10:06pm**
AIR BLK	.00	10:06pm

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

MECKLENBURG COUNTY BAT MOBILE UNIT 8 590

Serial Number: *008775* Test Record Number: *2549*
Test Date: *06/18/2026* Test Time: *10:19pm EDT*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	10:19pm
FLO	Pass	10:19pm
FC	Pass	10:19pm

Temperature Tests

Test	Status	Time
FC1	Pass	10:20pm
SRC	Pass	10:20pm
DET	Pass	10:20pm
BAR	Pass	10:20pm
BT	Pass	10:20pm

Blank Tests

Test	Status	Time
AIR	Pass	10:20pm

Printer Tests

Test	Status	Time
PRNT	Pass	10:20pm

CRC Tests

Test	Status	Time
COMP	Pass	10:20pm
CAL	Pass	10:20pm

Preventive Maintenance
Status: Pass



Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Mecklenburg Instrument Location BAT Mobile Unit 8

Instrument Serial No. 008775

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

(1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;

(2) Verify instrument displays time and date;

(3) Initiate breath test sequence;

(4) Enter information as prompted;

(5) Verify instrument accuracy;

(6) When "PLEASE BLOW" appears, collect breath sample;

(7) When "PLEASE BLOW" appears, collect breath sample;

(8) Print test record;

(9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and

(10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 19 day of June, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.

Signature of Certifying Official

2219283
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

DHHS 4080 (04/20)

Intox EC/IR-II: Subject Test

MECKLENBURG COUNTY BAT MOBILE UNIT 8
590

Serial Number: *008775*
Test Date: *06/19/2026*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name: *Glasscock, Jerry D*
Permit Number: *7180-9235*
Effective:
02/01/2026-02/01/2028

Officer's Name: *NONE, NONE*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG506303
Exp Date: 03/04/2027

Test	g/210L	Time
DIAG	Pass	8:33pm
AIR BLK	.00	8:34pm
ACCY CHK	.08	8:34pm
AIR BLK	.00	8:35pm
SUB TEST	**.00**	**8:36pm**
AIR BLK	.00	8:37pm
SUB TEST	**.00**	**8:38pm**
AIR BLK	.00	8:39pm

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

MECKLENBURG COUNTY BAT MOBILE UNIT 8 590

Serial Number: *008775* Test Record Number: *2551*
Test Date: *06/19/2026* Test Time: *8:39pm EDT*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	8:39pm
FLO	Pass	8:39pm
FC	Pass	8:40pm

Temperature Tests

Test	Status	Time
FC1	Pass	8:40pm
SRC	Pass	8:40pm
DET	Pass	8:40pm
BAR	Pass	8:40pm
BT	Pass	8:40pm

Blank Tests

Test	Status	Time
AIR	Pass	8:40pm

Printer Tests

Test	Status	Time
PRNT	Pass	8:40pm

CRC Tests

Test	Status	Time
COMP	Pass	8:41pm
CAL	Pass	8:41pm

Preventive Maintenance
Status: Pass

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Mecklenburg Instrument Location BAT Mobile Unit 8

Instrument Serial No. 008775 —

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

(1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;

(2) Verify instrument displays time and date;

(3) Initiate breath test sequence;

(4) Enter information as prompted;

(5) Verify instrument accuracy;

(6) When "PLEASE BLOW" appears, collect breath sample;

(7) When "PLEASE BLOW" appears, collect breath sample;

(8) Print test record;

(9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and

(10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 20 day of June, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.

Signature of Certifying Official

2219283
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

DHHS 4080 (04-79)

Intox EC/IR-II: Subject Test

MECKLENBURG COUNTY BAT MOBILE UNIT 8
590

Serial Number: *008775*
Test Date: *06/20/2026*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name: *Glasscock, Jerry D*
Permit Number: *7180-9235*
Effective:
02/01/2026-02/01/2028

Officer's Name: *NONE, NONE*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG506303
Exp Date: 03/04/2027

Test	g/210L	Time
DIAG	Pass	9:27pm
AIR BLK	.00	9:28pm
ACCY CHK	.08	9:28pm
AIR BLK	.00	9:29pm
SUB TEST	**.00**	**9:30pm**
AIR BLK	.00	9:31pm
SUB TEST	**.00**	**9:32pm**
AIR BLK	.00	9:33pm

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

MECKLENBURG COUNTY BAT MOBILE UNIT 8 590

Serial Number: *008775* Test Record Number: *2560*
Test Date: *06/20/2026* Test Time: *9:34pm EDT*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	9:34pm
FLO	Pass	9:34pm
FC	Pass	9:34pm

Temperature Tests

Test	Status	Time
FC1	Pass	9:34pm
SRC	Pass	9:34pm
DET	Pass	9:34pm
BAR	Pass	9:34pm
BT	Pass	9:34pm

Blank Tests

Test	Status	Time
AIR	Pass	9:35pm

Printer Tests

Test	Status	Time
PRNT	Pass	9:35pm

CRC Tests

Test	Status	Time
COMP	Pass	9:35pm
CAL	Pass	9:35pm

Preventive Maintenance
Status: Pass

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Mecklenburg Instrument Location BAT Mobile Unit 8

Instrument Serial No. 008816 —

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

(1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;

(2) Verify instrument displays time and date;

(3) Initiate breath test sequence;

(4) Enter information as prompted;

(5) Verify instrument accuracy;

(6) When "PLEASE BLOW" appears, collect breath sample;

(7) When "PLEASE BLOW" appears, collect breath sample;

(8) Print test record;

(9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and

(10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 4 day of June, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.

Signature of Certifying Official

2219283
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

MECKLENBURG COUNTY BAT MOBILE UNIT 8
590

Serial Number: *008816*
Test Date: *06/04/2026*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name: *Glasscock, Jerry D*
Permit Number: *7180-9235*
Effective:
02/01/2026-02/01/2028

Officer's Name: *NONE, NONE*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG431002
Exp Date: 11/05/2026

Test	g/210L	Time
DIAG	Pass	9:18am
AIR BLK	.00	9:19am
ACCY CHK	.08	9:20am
AIR BLK	.00	9:21am
SUB TEST	**.00**	**9:21am**
AIR BLK	.00	9:22am
SUB TEST	**.00**	**9:24am**
AIR BLK	.00	9:25am

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

MECKLENBURG COUNTY BAT MOBILE UNIT 8 590

Serial Number: *008816* Test Record Number: *8111*
Test Date: *06/04/2026* Test Time: *9:26am EDT*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	9:27am
FLO	Pass	9:27am
FC	Pass	9:27am

Temperature Tests

Test	Status	Time
FC1	Pass	9:27am
SRC	Pass	9:27am
DET	Pass	9:27am
BAR	Pass	9:27am
BT	Pass	9:27am

Blank Tests

Test	Status	Time
AIR	Pass	9:28am

Printer Tests

Test	Status	Time
PRNT	Pass	9:28am

CRC Tests

Test	Status	Time
COMP	Pass	9:28am
CAL	Pass	9:28am

Preventive Maintenance
Status: Pass



Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Mecklenburg Instrument Location BAT Mobile Unit 8

Instrument Serial No. 008816

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

(1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;

(2) Verify instrument displays time and date;

(3) Initiate breath test sequence;

(4) Enter information as prompted;

(5) Verify instrument accuracy;

(6) When "PLEASE BLOW" appears, collect breath sample;

(7) When "PLEASE BLOW" appears, collect breath sample;

(8) Print test record;

(9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and

(10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 11 day of June, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.

THE GREAT SEAL OF THE STATE OF NORTH CAROLINA

Signature of Certifying Official

2219283
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

DHHS 4080 (04/20)

Intox EC/IR-II: Subject Test

MECKLENBURG COUNTY BAT MOBILE UNIT 8
590

Serial Number: *008816*
Test Date: *06/11/2026*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name: *Glasscock, Jerry D*
Permit Number: *7180-9235*
Effective:
02/01/2026-02/01/2028

Officer's Name: *NONE, NONE*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG431002
Exp Date: 11/05/2026

Test	g/210L	Time
DIAG	Pass	8:18pm
AIR BLK	.00	8:19pm
ACCY CHK	.07	8:19pm
AIR BLK	.00	8:20pm
SUB TEST	**.00**	**8:21pm**
AIR BLK	.00	8:22pm
SUB TEST	**.00**	**8:23pm**
AIR BLK	.00	8:24pm

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

MECKLENBURG COUNTY BAT MOBILE UNIT 8 590

Serial Number: *008816* Test Record Number: *8117*
Test Date: *06/11/2026* Test Time: *8:24pm EDT*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	8:25pm
FLO	Pass	8:25pm
FC	Pass	8:25pm

Temperature Tests

Test	Status	Time
FC1	Pass	8:25pm
SRC	Pass	8:25pm
DET	Pass	8:25pm
BAR	Pass	8:25pm
BT	Pass	8:25pm

Blank Tests

Test	Status	Time
AIR	Pass	8:26pm

Printer Tests

Test	Status	Time
PRNT	Pass	8:26pm

CRC Tests

Test	Status	Time
COMP	Pass	8:26pm
CAL	Pass	8:26pm

Preventive Maintenance
Status: Pass

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Mecklenburg Instrument Location BAT Mobile Unit 8

Instrument Serial No. 008816

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

(1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;

(2) Verify instrument displays time and date;

(3) Initiate breath test sequence;

(4) Enter information as prompted;

(5) Verify instrument accuracy;

(6) When "PLEASE BLOW" appears, collect breath sample;

(7) When "PLEASE BLOW" appears, collect breath sample;

(8) Print test record;

(9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and

(10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 18 day of June, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.

Signature of Certifying Official

2219283
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

DHHS 4080 (04/20)

Intox EC/IR-II: Subject Test

MECKLENBURG COUNTY BAT MOBILE UNIT 8
590

Serial Number: *008816*
Test Date: *06/18/2026*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name: *Glasscock, Jerry D*
Permit Number: *7180-9235*
Effective:
02/01/2026-02/01/2028

Officer's Name: *NONE, NONE*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG431002
Exp Date: 11/05/2026

Test	g/210L	Time
DIAG	Pass	9:58pm
AIR BLK	.00	9:59pm
ACCY CHK	.07	10:00pm
AIR BLK	.00	10:01pm
SUB TEST	**.00**	**10:02pm**
AIR BLK	.00	10:03pm
SUB TEST	**.00**	**10:04pm**
AIR BLK	.00	10:05pm

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

MECKLENBURG COUNTY BAT MOBILE UNIT 8 590

Serial Number: *008816* Test Record Number: *8125*
Test Date: *06/18/2026* Test Time: *10:07pm EDT*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	10:07pm
FLO	Pass	10:07pm
FC	Pass	10:07pm

Temperature Tests

Test	Status	Time
FC1	Pass	10:07pm
SRC	Pass	10:07pm
DET	Pass	10:07pm
BAR	Pass	10:07pm
BT	Pass	10:07pm

Blank Tests

Test	Status	Time
AIR	Pass	10:08pm

Printer Tests

Test	Status	Time
PRNT	Pass	10:08pm

CRC Tests

Test	Status	Time
COMP	Pass	10:08pm
CAL	Pass	10:08pm

Preventive Maintenance
Status: Pass

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Mecklenburg Instrument Location BAT Mobile Unit 8

Instrument Serial No. 008816

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

(1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;

(2) Verify instrument displays time and date;

(3) Initiate breath test sequence;

(4) Enter information as prompted;

(5) Verify instrument accuracy;

(6) When "PLEASE BLOW" appears, collect breath sample;

(7) When "PLEASE BLOW" appears, collect breath sample;

(8) Print test record;

(9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and

(10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 19 day of June, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.

Signature of Certifying Official

2219283
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

MECKLENBURG COUNTY BAT MOBILE UNIT 8
590

Serial Number: *008816*
Test Date: *06/19/2026*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name: *Glasscock, Jerry D*
Permit Number: *7180-9235*
Effective:
02/01/2026-02/01/2028

Officer's Name: *NONE, NONE*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG431002
Exp Date: 11/05/2026

Test	g/210L	Time
DIAG	Pass	8:32pm
AIR BLK	.00	8:33pm
ACCY CHK	.07	8:34pm
AIR BLK	.00	8:35pm
SUB TEST	**.00**	**8:36pm**
AIR BLK	.00	8:37pm
SUB TEST	**.00**	**8:38pm**
AIR BLK	.00	8:39pm

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

MECKLENBURG COUNTY BAT MOBILE UNIT 8 590

Serial Number: *008816* Test Record Number: *8127*
Test Date: *06/19/2026* Test Time: *8:39pm EDT*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	8:39pm
FLO	Pass	8:39pm
FC	Pass	8:40pm

Temperature Tests

Test	Status	Time
FC1	Pass	8:40pm
SRC	Pass	8:40pm
DET	Pass	8:40pm
BAR	Pass	8:40pm
BT	Pass	8:40pm

Blank Tests

Test	Status	Time
AIR	Pass	8:40pm

Printer Tests

Test	Status	Time
PRNT	Pass	8:40pm

CRC Tests

Test	Status	Time
COMP	Pass	8:41pm
CAL	Pass	8:41pm

Preventive Maintenance
Status: Pass



Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Mecklenburg Instrument Location BAT Mobile Unit 8

Instrument Serial No. 008816 —

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

(1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;

(2) Verify instrument displays time and date;

(3) Initiate breath test sequence;

(4) Enter information as prompted;

(5) Verify instrument accuracy;

(6) When "PLEASE BLOW" appears, collect breath sample;

(7) When "PLEASE BLOW" appears, collect breath sample;

(8) Print test record;

(9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and

(10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 20 day of June, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.

Signature of Certifying Official

2219283
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

DHHS 4080 (04-70)

Intox EC/IR-II: Subject Test

MECKLENBURG COUNTY BAT MOBILE UNIT 8
590

Serial Number: *008816*
Test Date: *06/20/2026*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name: *Glasscock, Jerry D*
Permit Number: *7180-9235*
Effective:
02/01/2026-02/01/2028

Officer's Name: *NONE, NONE*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG431002
Exp Date: 11/05/2026

Test	g/210L	Time
DIAG	Pass	9:28pm
AIR BLK	.00	9:29pm
ACCY CHK	.07	9:29pm
AIR BLK	.00	9:30pm
SUB TEST	**.00**	**9:31pm**
AIR BLK	.00	9:32pm
SUB TEST	**.00**	**9:33pm**
AIR BLK	.00	9:34pm

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

MECKLENBURG COUNTY BAT MOBILE UNIT 8 590

Serial Number: *008816* Test Record Number: *8132*
Test Date: *06/20/2026* Test Time: *9:35pm EDT*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	9:36pm
FLO	Pass	9:36pm
FC	Pass	9:36pm

Temperature Tests

Test	Status	Time
FC1	Pass	9:36pm
SRC	Pass	9:36pm
DET	Pass	9:36pm
BAR	Pass	9:36pm
BT	Pass	9:36pm

Blank Tests

Test	Status	Time
AIR	Pass	9:36pm

Printer Tests

Test	Status	Time
PRNT	Pass	9:36pm

CRC Tests

Test	Status	Time
COMP	Pass	9:37pm
CAL	Pass	9:37pm

Preventive Maintenance
Status: Pass

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Mecklenburg Instrument Location BAT Mobile Unit 8

Instrument Serial No. 008929 —

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

(1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;

(2) Verify instrument displays time and date;

(3) Initiate breath test sequence;

(4) Enter information as prompted;

(5) Verify instrument accuracy;

(6) When "PLEASE BLOW" appears, collect breath sample;

(7) When "PLEASE BLOW" appears, collect breath sample;

(8) Print test record;

(9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and

(10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 4 day of June, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.

Signature of Certifying Official

2219283
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

MECKLENBURG COUNTY BAT MOBILE UNIT 8
590

Serial Number: *008929*
Test Date: *06/04/2026*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name: *Glasscock, Jerry D*
Permit Number: *7180-9235*
Effective:
02/01/2026-02/01/2028

Officer's Name: *NONE, NONE*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG506303
Exp Date: 03/04/2027

Test	g/210L	Time
DIAG	Pass	9:09am
AIR BLK	.00	9:10am
ACCY CHK	.07	9:11am
AIR BLK	.00	9:12am
SUB TEST	**.00**	**9:12am**
AIR BLK	.00	9:14am
SUB TEST	**.00**	**9:15am**
AIR BLK	.00	9:16am

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

MECKLENBURG COUNTY BAT MOBILE UNIT 8 590

Serial Number: *008929* Test Record Number: *1818*
Test Date: *06/04/2026* Test Time: *9:17am EDT*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	9:17am
FLO	Pass	9:17am
FC	Pass	9:17am

Temperature Tests

Test	Status	Time
FC1	Pass	9:17am
SRC	Pass	9:17am
DET	Pass	9:17am
BAR	Pass	9:17am
BT	Pass	9:17am

Blank Tests

Test	Status	Time
AIR	Pass	9:18am

Printer Tests

Test	Status	Time
PRNT	Pass	9:18am

CRC Tests

Test	Status	Time
COMP	Pass	9:18am
CAL	Pass	9:18am

Preventive Maintenance
Status: Pass



Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Mecklenburg Instrument Location BAT Mobile Unit 8

Instrument Serial No. 008929 —

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

(1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;

(2) Verify instrument displays time and date;

(3) Initiate breath test sequence;

(4) Enter information as prompted;

(5) Verify instrument accuracy;

(6) When "PLEASE BLOW" appears, collect breath sample;

(7) When "PLEASE BLOW" appears, collect breath sample;

(8) Print test record;

(9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and

(10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 11 day of June, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.

Signature of Certifying Official

2219283
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

DHHS 4080 (04/20)

Intox EC/IR-II: Subject Test

MECKLENBURG COUNTY BAT MOBILE UNIT 8
590

Serial Number: *008929*
Test Date: *06/11/2026*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name: *Glasscock, Jerry D*
Permit Number: *7180-9235*
Effective:
02/01/2026-02/01/2028

Officer's Name: *NONE, NONE*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG506303
Exp Date: 03/04/2027

Test	g/210L	Time
DIAG	Pass	8:14pm
AIR BLK	.00	8:15pm
ACCY CHK	.08	8:16pm
AIR BLK	.00	8:17pm
SUB TEST	**.00**	**8:18pm**
AIR BLK	.00	8:19pm
SUB TEST	**.00**	**8:20pm**
AIR BLK	.00	8:21pm

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

MECKLENBURG COUNTY BAT MOBILE UNIT 8 590

Serial Number: *008929* Test Record Number: *1824*
Test Date: *06/11/2026* Test Time: *8:21pm EDT*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	8:22pm
FLO	Pass	8:22pm
FC	Pass	8:22pm

Temperature Tests

Test	Status	Time
FC1	Pass	8:22pm
SRC	Pass	8:22pm
DET	Pass	8:22pm
BAR	Pass	8:22pm
BT	Pass	8:22pm

Blank Tests

Test	Status	Time
AIR	Pass	8:24pm


Printer Tests

Test	Status	Time
PRNT	Pass	8:24pm

CRC Tests

Test	Status	Time
COMP	Pass	8:24pm
CAL	Pass	8:24pm

Preventive Maintenance
Status: Pass

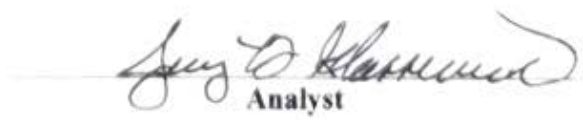

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Mecklenburg Instrument Location BAT Mobile Unit 8

Instrument Serial No. 008929

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

(1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;

(2) Verify instrument displays time and date;

(3) Initiate breath test sequence;

(4) Enter information as prompted;

(5) Verify instrument accuracy;

(6) When "PLEASE BLOW" appears, collect breath sample;

(7) When "PLEASE BLOW" appears, collect breath sample;

(8) Print test record;

(9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and

(10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 18 day of June, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.

Signature of Certifying Official

2219283
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

DHHS 4080 (04/20)

Intox EC/IR-II: Subject Test

MECKLENBURG COUNTY BAT MOBILE UNIT 8
590

Serial Number: *008929*
Test Date: *06/18/2026*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name: *Glasscock, Jerry D*
Permit Number: *7180-9235*
Effective:
02/01/2026-02/01/2028

Officer's Name: *NONE, NONE*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG506303
Exp Date: 03/04/2027

Test	g/210L	Time
DIAG	Pass	10:15pm
AIR BLK	.00	10:16pm
ACCY CHK	.07	10:16pm
AIR BLK	.00	10:18pm
SUB TEST	**.00**	**10:18pm**
AIR BLK	.00	10:19pm
SUB TEST	**.00**	**10:21pm**
AIR BLK	.00	10:22pm

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

MECKLENBURG COUNTY BAT MOBILE UNIT 8 590

Serial Number: *008929* Test Record Number: *1833*
Test Date: *06/18/2026* Test Time: *10:22pm EDT*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	10:22pm
FLO	Pass	10:22pm
FC	Pass	10:23pm

Temperature Tests

Test	Status	Time
FC1	Pass	10:23pm
SRC	Pass	10:23pm
DET	Pass	10:23pm
BAR	Pass	10:23pm
BT	Pass	10:23pm

Blank Tests

Test	Status	Time
AIR	Pass	10:23pm

Printer Tests

Test	Status	Time
PRNT	Pass	10:24pm

CRC Tests

Test	Status	Time
COMP	Pass	10:24pm
CAL	Pass	10:24pm

Preventive Maintenance
Status: Pass



Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Mecklenburg Instrument Location BAT Mobile Unit 8

Instrument Serial No. 008929 —

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

(1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;

(2) Verify instrument displays time and date;

(3) Initiate breath test sequence;

(4) Enter information as prompted;

(5) Verify instrument accuracy;

(6) When "PLEASE BLOW" appears, collect breath sample;

(7) When "PLEASE BLOW" appears, collect breath sample;

(8) Print test record;

(9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and

(10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 19 day of June, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.

Signature of Certifying Official

2219283
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

MECKLENBURG COUNTY BAT MOBILE UNIT 8
590

Serial Number: *008929*
Test Date: *06/19/2026*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name: *Glasscock, Jerry D*
Permit Number: *7180-9235*
Effective:
02/01/2026-02/01/2028

Officer's Name: *NONE, NONE*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG506303
Exp Date: 03/04/2027

Test	g/210L	Time
DIAG	Pass	8:31pm
AIR BLK	.00	8:32pm
ACCY CHK	.07	8:33pm
AIR BLK	.00	8:34pm
SUB TEST	**.00**	**8:35pm**
AIR BLK	.00	8:36pm
SUB TEST	**.00**	**8:37pm**
AIR BLK	.00	8:38pm

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

MECKLENBURG COUNTY BAT MOBILE UNIT 8 590

Serial Number: *008929* Test Record Number: *1835*
Test Date: *06/19/2026* Test Time: *8:39pm EDT*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	8:39pm
FLO	Pass	8:39pm
FC	Pass	8:39pm

Temperature Tests

Test	Status	Time
FC1	Pass	8:39pm
SRC	Pass	8:39pm
DET	Pass	8:39pm
BAR	Pass	8:39pm
BT	Pass	8:39pm

Blank Tests

Test	Status	Time
AIR	Pass	8:40pm

Printer Tests

Test	Status	Time
PRNT	Pass	8:40pm

CRC Tests

Test	Status	Time
COMP	Pass	8:40pm
CAL	Pass	8:40pm

Preventive Maintenance
Status: Pass



Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Mecklenburg Instrument Location BAT Mobile Unit 8

Instrument Serial No. 008929 —

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

(1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;

(2) Verify instrument displays time and date;

(3) Initiate breath test sequence;

(4) Enter information as prompted;

(5) Verify instrument accuracy;

(6) When "PLEASE BLOW" appears, collect breath sample;

(7) When "PLEASE BLOW" appears, collect breath sample;

(8) Print test record;

(9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and

(10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 20 day of June, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.

Signature of Certifying Official

2219283
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

MECKLENBURG COUNTY BAT MOBILE UNIT 8
590

Serial Number: *008929*
Test Date: *06/20/2026*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name: *Glasscock, Jerry D*
Permit Number: *7180-9235*
Effective:
02/01/2026-02/01/2028

Officer's Name: *NONE, NONE*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG506303
Exp Date: 03/04/2027

Test	g/210L	Time
DIAG	Pass	9:28pm
AIR BLK	.00	9:29pm
ACCY CHK	.07	9:30pm
AIR BLK	.00	9:31pm
SUB TEST	**.00**	**9:31pm**
AIR BLK	.00	9:32pm
SUB TEST	**.00**	**9:34pm**
AIR BLK	.00	9:35pm

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

MECKLENBURG COUNTY BAT MOBILE UNIT 8 590

Serial Number: *008929* Test Record Number: *1840*
Test Date: *06/20/2026* Test Time: *9:36pm EDT*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	9:36pm
FLO	Pass	9:36pm
FC	Pass	9:36pm

Temperature Tests

Test	Status	Time
FC1	Pass	9:36pm
SRC	Pass	9:36pm
DET	Pass	9:36pm
BAR	Pass	9:36pm
BT	Pass	9:36pm

Blank Tests

Test	Status	Time
AIR	Pass	9:37pm

Printer Tests

Test	Status	Time
PRNT	Pass	9:37pm

CRC Tests

Test	Status	Time
COMP	Pass	9:37pm
CAL	Pass	9:37pm

Preventive Maintenance
Status: Pass

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County MOORE Instrument Location PINEHURST POLICE DEPARTMENT

Instrument Serial No. 008710

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

(1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;

(2) Verify instrument displays time and date;

(3) Initiate breath test sequence;

(4) Enter information as prompted;

(5) Verify instrument accuracy;

(6) When "PLEASE BLOW" appears, collect breath sample;

(7) When "PLEASE BLOW" appears, collect breath sample;

(8) Print test record;

(9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and

(10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 24 day of JUNE, 20 26 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.

Signature of Certifying Official

239771
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

MOORE COUNTY PINEHURST PD 620

Serial Number: *008710*
Test Date: *06/24/2026*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name: *Galloway, Charles L*
Permit Number: *0023-9771*
Effective:
02/01/2026-02/01/2028

Officer's Name: *NONE, NONE*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG534301
Exp Date: 12/09/2027

Test	g/210L	Time
DIAG	Pass	5:29pm
AIR BLK	.00	5:30pm
ACCY CHK	.08	5:31pm
AIR BLK	.00	5:32pm
SUB TEST	**.00**	**5:32pm**
AIR BLK	.00	5:33pm
SUB TEST	**.00**	**5:35pm**
AIR BLK	.00	5:35pm

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

MOORE COUNTY PINEHURST PD 620

Serial Number: *008710* Test Record Number: *2347*
Test Date: *06/24/2026* Test Time: *5:36pm EDT*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	5:37pm
FLO	Pass	5:37pm
FC	Pass	5:37pm

Temperature Tests

Test	Status	Time
FC1	Pass	5:37pm
SRC	Pass	5:37pm
DET	Pass	5:37pm
BAR	Pass	5:37pm
BT	Pass	5:37pm

Blank Tests

Test	Status	Time
AIR	Pass	5:38pm

Printer Tests

Test	Status	Time
PRNT	Pass	5:38pm

CRC Tests

Test	Status	Time
COMP	Pass	5:38pm
CAL	Pass	5:38pm

Preventive Maintenance
Status: Pass



Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County MOORE Instrument Location MOORE COUNTY DETENTION CENTER

Instrument Serial No. 008735

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

(1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;

(2) Verify instrument displays time and date;

(3) Initiate breath test sequence;

(4) Enter information as prompted;

(5) Verify instrument accuracy;

(6) When "PLEASE BLOW" appears, collect breath sample;

(7) When "PLEASE BLOW" appears, collect breath sample;

(8) Print test record;

(9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and

(10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 24 day of JUNE, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.

Signature of Certifying Official

239771
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

MOORE COUNTY DETENTION CENTER 620

Serial Number: *008735*
Test Date: *06/24/2026*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name: *Galloway, Charles L*
Permit Number: *0023-9771*
Effective:
02/01/2026-02/01/2028

Officer's Name: *NONE, NONE*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG506301
Exp Date: 03/04/2027

Test	g/210L	Time
DIAG	Pass	1:09pm
AIR BLK	.00	1:10pm
ACCY CHK	.08	1:11pm
AIR BLK	.00	1:12pm
SUB TEST	**.00**	**1:12pm**
AIR BLK	.00	1:13pm
SUB TEST	**.00**	**1:15pm**
AIR BLK	.00	1:16pm

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

MOORE COUNTY DETENTION CENTER 620

Serial Number: *008735* Test Record Number: *3880*
Test Date: *06/24/2026* Test Time: *1:17pm EDT*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	1:17pm
FLO	Pass	1:17pm
FC	Pass	1:17pm

Temperature Tests

Test	Status	Time
FC1	Pass	1:17pm
SRC	Pass	1:17pm
DET	Pass	1:17pm
BAR	Pass	1:17pm
BT	Pass	1:17pm

Blank Tests

Test	Status	Time
AIR	Pass	1:18pm

Printer Tests

Test	Status	Time
PRNT	Pass	1:18pm

CRC Tests

Test	Status	Time
COMP	Pass	1:18pm
CAL	Pass	1:18pm

Preventive Maintenance
Status: Pass



Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County MOORE Instrument Location SOUTHERN PINES

Instrument Serial No. 008850 POLICE DEPARTMENT

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

(1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;

(2) Verify instrument displays time and date;

(3) Initiate breath test sequence;

(4) Enter information as prompted;

(5) Verify instrument accuracy;

(6) When "PLEASE BLOW" appears, collect breath sample;

(7) When "PLEASE BLOW" appears, collect breath sample;

(8) Print test record;

(9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and

(10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 24 day of JUNE, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.

Signature of ~~Certifying Official~~

239771
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

MOORE COUNTY SOUTHERN PINES PD 620

Serial Number: *008850*
Test Date: *06/24/2026*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name: *Galloway, Charles L*
Permit Number: *0023-9771*
Effective:
02/01/2026-02/01/2028

Officer's Name: *NONE, NONE*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG506301
Exp Date: 03/04/2027

Test	g/210L	Time
DIAG	Pass	3:14pm
AIR BLK	.00	3:15pm
ACCY CHK	.07	3:15pm
AIR BLK	.00	3:16pm
SUB TEST	**.00**	**3:17pm**
AIR BLK	.00	3:18pm
SUB TEST	**.00**	**3:20pm**
AIR BLK	.00	3:20pm

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

MOORE COUNTY SOUTHERN PINES PD 620

Serial Number: *008850* Test Record Number: *793*
Test Date: *06/24/2026* Test Time: *3:22pm EDT*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	3:23pm
FLO	Pass	3:23pm
FC	Pass	3:23pm

Temperature Tests

Test	Status	Time
FC1	Pass	3:23pm
SRC	Pass	3:23pm
DET	Pass	3:23pm
BAR	Pass	3:23pm
BT	Pass	3:23pm

Blank Tests

Test	Status	Time
AIR	Pass	3:23pm

Printer Tests

Test	Status	Time
PRNT	Pass	3:24pm

CRC Tests

Test	Status	Time
COMP	Pass	3:24pm
CAL	Pass	3:24pm

Preventive Maintenance
Status: Pass



Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County NASH Instrument Location NASH COUNTY DETENTION CENTER

Instrument Serial No. 008688 222 S. WASHINGTON ST
NASHVILLE, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

(1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;

(2) Verify instrument displays time and date;

(3) Initiate breath test sequence;

(4) Enter information as prompted;

(5) Verify instrument accuracy;

(6) When "PLEASE BLOW" appears, collect breath sample;

(7) When "PLEASE BLOW" appears, collect breath sample;

(8) Print test record;

(9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and

(10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 22 day of JUNE, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.

Signature of Certifying Official

179707
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

DHHS 4080 (04/20)

Intox EC/IR-II: Subject Test

NASH COUNTY NASH DETENTION CTR 630

Serial Number: *008688*
Test Date: *06/22/2026*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name: *Bryant, Earl A*
Permit Number: *0017-9707*
Effective:
02/01/2026-02/01/2028

Officer's Name: *NONE, NONE*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG501307
Exp Date: 01/13/2027

Test	g/210L	Time
DIAG	Pass	4:08pm
AIR BLK	.00	4:09pm
ACCY CHK	.07	4:10pm
AIR BLK	.00	4:11pm
SUB TEST	**.00**	**4:12pm**
AIR BLK	.00	4:12pm
SUB TEST	**.00**	**4:15pm**
AIR BLK	.00	4:15pm

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

NASH COUNTY NASH DETENTION CTR 630

Serial Number: *008688* Test Record Number: *1210*
Test Date: *06/22/2026* Test Time: *4:17pm EDT*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	4:17pm
FLO	Pass	4:17pm
FC	Pass	4:18pm

Temperature Tests

Test	Status	Time
FC1	Pass	4:18pm
SRC	Pass	4:18pm
DET	Pass	4:18pm
BAR	Pass	4:18pm
BT	Pass	4:18pm

Blank Tests

Test	Status	Time
AIR	Pass	4:18pm

Printer Tests

Test	Status	Time
PRNT	Pass	4:18pm

CRC Tests

Test	Status	Time
COMP	Pass	4:18pm
CAL	Pass	4:18pm

Preventive Maintenance
Status: Pass



Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County New Hanover Instrument Location Wilmington Police Department

Instrument Serial No. 008628

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

(1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;

(2) Verify instrument displays time and date;

(3) Initiate breath test sequence;

(4) Enter information as prompted;

(5) Verify instrument accuracy;

(6) When "PLEASE BLOW" appears, collect breath sample;

(7) When "PLEASE BLOW" appears, collect breath sample;

(8) Print test record;

(9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and

(10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 10th day of June, 20 26 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.

Signature of Certifying Official

845023
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

DHHS 4080 (04/20)

Intox EC/IR-II: Subject Test

NEW HANOVER COUNTY WILMINGTON PD 640

Serial Number: *008628*
Test Date: *06/10/2026*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name: *Ryan, Robert F*
Permit Number: *0084-5023*
Effective:
02/01/2026-02/01/2028

Officer's Name: *NONE, NONE*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG602102
Exp Date: 01/21/2028

Test	g/210L	Time
DIAG	Pass	11:27am
AIR BLK	.00	11:27am
ACCY CHK	.07	11:28am
AIR BLK	.00	11:29am
SUB TEST	**.00**	**11:30am**
AIR BLK	.00	11:31am
SUB TEST	**.00**	**11:32am**
AIR BLK	.00	11:33am

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

NEW HANOVER COUNTY WILMINGTON PD 640

Serial Number: *008628* Test Record Number: *7509*
Test Date: *06/10/2026* Test Time: *11:34am EDT*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	11:35am
FLO	Pass	11:35am
FC	Pass	11:35am

Temperature Tests

Test	Status	Time
FC1	Pass	11:35am
SRC	Pass	11:35am
DET	Pass	11:35am
BAR	Pass	11:35am
BT	Pass	11:35am

Blank Tests

Test	Status	Time
AIR	Pass	11:35am

Printer Tests

Test	Status	Time
PRNT	Pass	11:35am

CRC Tests

Test	Status	Time
COMP	Pass	11:36am
CAL	Pass	11:36am

Preventive Maintenance
Status: Pass

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County ONSLOW Instrument Location BAT Mobile Unit 12

Instrument Serial No. 008601

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

(1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;

(2) Verify instrument displays time and date;

(3) Initiate breath test sequence;

(4) Enter information as prompted;

(5) Verify instrument accuracy;

(6) When "PLEASE BLOW" appears, collect breath sample;

(7) When "PLEASE BLOW" appears, collect breath sample;

(8) Print test record;

(9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and

(10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 27th day of June, 20 26 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.

Signature of Certifying Official

83034
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

ONSLOW COUNTY BAT MOBILE UNIT 12 660

Serial Number: *008601*
Test Date: *06/27/2026*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name:
Crutchfield Jr., Marshall B
Permit Number: *0008-3034*
Effective:
03/01/2026-03/01/2028

Officer's Name: *NONE, NONE*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG501307
Exp Date: 01/13/2027

Test	g/210L	Time
DIAG	Pass	4:03pm
AIR BLK	.00	4:04pm
ACCY CHK	.07	4:04pm
AIR BLK	.00	4:05pm
SUB TEST	**.00**	**4:06pm**
AIR BLK	.00	4:07pm
SUB TEST	**.00**	**4:08pm**
AIR BLK	.00	4:09pm

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

ONSLOW COUNTY BAT MOBILE UNIT 12 660

Serial Number: *008601* Test Record Number: *1956*
Test Date: *06/27/2026* Test Time: *4:10pm EDT*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	4:11pm
FLO	Pass	4:11pm
FC	Pass	4:11pm

Temperature Tests

Test	Status	Time
FC1	Pass	4:11pm
SRC	Pass	4:11pm
DET	Pass	4:11pm
BAR	Pass	4:11pm
BT	Pass	4:11pm

Blank Tests

Test	Status	Time
AIR	Pass	4:11pm

Printer Tests

Test	Status	Time
PRNT	Pass	4:11pm

CRC Tests

Test	Status	Time
COMP	Pass	4:12pm
CAL	Pass	4:12pm

Preventive Maintenance
Status: Pass

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Onslow Instrument Location BAT Mobile Unit 12

Instrument Serial No. 008698

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

(1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;

(2) Verify instrument displays time and date;

(3) Initiate breath test sequence;

(4) Enter information as prompted;

(5) Verify instrument accuracy;

(6) When "PLEASE BLOW" appears, collect breath sample;

(7) When "PLEASE BLOW" appears, collect breath sample;

(8) Print test record;

(9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and

(10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 27th day of June, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.

Signature of Certifying Official

83034
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

ONSLOW COUNTY BAT MOBILE UNIT 12 660

Serial Number: *008698*
Test Date: *06/27/2026*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name:
Crutchfield Jr., Marshall B
Permit Number: *0008-3034*
Effective:
03/01/2026-03/01/2028

Officer's Name: *NONE, NONE*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG431002
Exp Date: 11/05/2026

Test	g/210L	Time
DIAG	Pass	4:03pm
AIR BLK	.00	4:04pm
ACCY CHK	.08	4:05pm
AIR BLK	.00	4:06pm
SUB TEST	**.00**	**4:06pm**
AIR BLK	.00	4:07pm
SUB TEST	**.00**	**4:09pm**
AIR BLK	.00	4:10pm

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

ONSLOW COUNTY BAT MOBILE UNIT 12 660

Serial Number: *008698* Test Record Number: *2788*
Test Date: *06/27/2026* Test Time: *4:10pm EDT*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	4:11pm
FLO	Pass	4:11pm
FC	Pass	4:11pm

Temperature Tests

Test	Status	Time
FC1	Pass	4:11pm
SRC	Pass	4:11pm
DET	Pass	4:11pm
BAR	Pass	4:11pm
BT	Pass	4:11pm

Blank Tests

Test	Status	Time
AIR	Pass	4:11pm

Printer Tests

Test	Status	Time
PRNT	Pass	4:12pm

CRC Tests

Test	Status	Time
COMP	Pass	4:12pm
CAL	Pass	4:12pm

Preventive Maintenance
Status: Pass

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Onslow Instrument Location BAT Mobile Unit 12

Instrument Serial No. 008788

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

(1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;

(2) Verify instrument displays time and date;

(3) Initiate breath test sequence;

(4) Enter information as prompted;

(5) Verify instrument accuracy;

(6) When "PLEASE BLOW" appears, collect breath sample;

(7) When "PLEASE BLOW" appears, collect breath sample;

(8) Print test record;

(9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and

(10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 27th day of June, 20 26 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.

Signature of Certifying Official

83034
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

DHHS 4080 (04/20)

Intox EC/IR-II: Subject Test

ONSLOW COUNTY BAT MOBILE UNIT 12 660

Serial Number: *008788*
Test Date: *06/27/2026*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name:
Crutchfield Jr., Marshall B
Permit Number: *0008-3034*
Effective:
03/01/2026-03/01/2028

Officer's Name: *NONE, NONE*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG534301
Exp Date: 12/09/2027

Test	g/210L	Time
DIAG	Pass	4:18pm
AIR BLK	.00	4:19pm
ACCY CHK	.07	4:20pm
AIR BLK	.00	4:21pm
SUB TEST	**.00**	**4:21pm**
AIR BLK	.00	4:22pm
SUB TEST	**.00**	**4:24pm**
AIR BLK	.00	4:24pm

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

ONSLOW COUNTY BAT MOBILE UNIT 12 660

Serial Number: *008788* Test Record Number: *2573*
Test Date: *06/27/2026* Test Time: *4:26pm EDT*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	4:26pm
FLO	Pass	4:26pm
FC	Pass	4:26pm

Temperature Tests

Test	Status	Time
FC1	Pass	4:26pm
SRC	Pass	4:26pm
DET	Pass	4:26pm
BAR	Pass	4:26pm
BT	Pass	4:26pm

Blank Tests

Test	Status	Time
AIR	Pass	4:27pm

Printer Tests

Test	Status	Time
PRNT	Pass	4:27pm

CRC Tests

Test	Status	Time
COMP	Pass	4:27pm
CAL	Pass	4:27pm

Preventive Maintenance
Status: Pass



Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Pasquotank Instrument Location Elizabeth City P.D.

Instrument Serial No. 008941 305 E. Main St.

Elizabeth City, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

(1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;

(2) Verify instrument displays time and date;

(3) Initiate breath test sequence;

(4) Enter information as prompted;

(5) Verify instrument accuracy;

(6) When "PLEASE BLOW" appears, collect breath sample;

(7) When "PLEASE BLOW" appears, collect breath sample;

(8) Print test record;

(9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and

(10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 26th day of June, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.

Mark A. Bryant
Signature of Certifying Official

206272
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

PASQUOTANK COUNTY ELIZABETH CITY PD
690

Serial Number: *008941*
Test Date: *06/26/2026*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name: *Chappell, Mark A*
Permit Number: *0020-6272*
Effective:
02/01/2026-02/01/2028

Officer's Name: *NONE, NONE*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG516203
Exp Date: 06/11/2027

Test	g/210L	Time
DIAG	Pass	2:37pm
AIR BLK	.00	2:38pm
ACCY CHK	.08	2:39pm
AIR BLK	.00	2:40pm
SUB TEST	**.00**	**2:41pm**
AIR BLK	.00	2:42pm
SUB TEST	**.00**	**2:43pm**
AIR BLK	.00	2:44pm

Reported AC: .00 g/210L

Mark A. Chappell
Signature of Chemical Analyst

Court CVR

Mark A. Chappell
Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

PASQUOTANK COUNTY ELIZABETH CITY PD 690

Serial Number: *008941* Test Record Number: *1793*
Test Date: *06/26/2026* Test Time: *2:45pm EDT*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	2:45pm
FLO	Pass	2:45pm
FC	Pass	2:45pm

Temperature Tests

Test	Status	Time
FC1	Pass	2:46pm
SRC	Pass	2:46pm
DET	Pass	2:46pm
BAR	Pass	2:46pm
BT	Pass	2:46pm

Blank Tests

Test	Status	Time
AIR	Pass	2:46pm

Printer Tests

Test	Status	Time
PRNT	Pass	2:46pm

CRC Tests

Test	Status	Time
COMP	Pass	2:46pm
CAL	Pass	2:46pm

Preventive Maintenance
Status: Pass



Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Pender Instrument Location BAT Mobile Unit 9

Instrument Serial No. 008575

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

(1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;

(2) Verify instrument displays time and date;

(3) Initiate breath test sequence;

(4) Enter information as prompted;

(5) Verify instrument accuracy;

(6) When "PLEASE BLOW" appears, collect breath sample;

(7) When "PLEASE BLOW" appears, collect breath sample;

(8) Print test record;

(9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and

(10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 26th day of June, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.

Signature of Certifying Official

226313
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

DHHS 4080 (04/20)

Intox EC/IR-II: Subject Test

PENDER COUNTY BAT MOBILE UNIT 9 700

Serial Number: *008575*
Test Date: *06/26/2026*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name: *Sharpe Jr., Robert J*
Permit Number: *1820-8591*
Effective:
02/01/2026-02/01/2028

Officer's Name: *NONE, NONE*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG516204
Exp Date: 06/11/2027

Test	g/210L	Time
DIAG	Pass	8:23pm
AIR BLK	.00	8:24pm
ACCY CHK	.08	8:24pm
AIR BLK	.00	8:25pm
SUB TEST	**.00**	**8:26pm**
AIR BLK	.00	8:27pm
SUB TEST	**.00**	**8:29pm**
AIR BLK	.00	8:30pm

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

PENDER COUNTY BAT MOBILE UNIT 9 700

Serial Number: *008575* Test Record Number: *1608*
Test Date: *06/26/2026* Test Time: *8:35pm EDT*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	8:36pm
FLO	Pass	8:36pm
FC	Pass	8:36pm

Temperature Tests

Test	Status	Time
FC1	Pass	8:36pm
SRC	Pass	8:36pm
DET	Pass	8:36pm
BAR	Pass	8:36pm
BT	Pass	8:36pm

Blank Tests

Test	Status	Time
AIR	Pass	8:37pm

Printer Tests

Test	Status	Time
PRNT	Pass	8:37pm

CRC Tests

Test	Status	Time
COMP	Pass	8:37pm
CAL	Pass	8:37pm

Preventive Maintenance
Status: Pass



Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Pender Instrument Location BAT Mobile Unit 9

Instrument Serial No. 008616

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

(1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;

(2) Verify instrument displays time and date;

(3) Initiate breath test sequence;

(4) Enter information as prompted;

(5) Verify instrument accuracy;

(6) When "PLEASE BLOW" appears, collect breath sample;

(7) When "PLEASE BLOW" appears, collect breath sample;

(8) Print test record;

(9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and

(10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 26th day of June, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.

Signature of Certifying Official

226310
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

DHHS 4080 (04/20)

Intox EC/IR-II: Subject Test

PENDER COUNTY BAT MOBILE UNIT 9 700

Serial Number: *008616*
Test Date: *06/26/2026*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name: *Sharpe Jr., Robert J*
Permit Number: *1820-8591*
Effective:
02/01/2026-02/01/2028

Officer's Name: *NONE, NONE*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG506303
Exp Date: 03/04/2027

Test	g/210L	Time
DIAG	Pass	8:22pm
AIR BLK	.00	8:23pm
ACCY CHK	.07	8:23pm
AIR BLK	.00	8:25pm
SUB TEST	**.00**	**8:25pm**
AIR BLK	.00	8:26pm
SUB TEST	**.00**	**8:28pm**
AIR BLK	.00	8:29pm

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

PENDER COUNTY BAT MOBILE UNIT 9 700

Serial Number: *008616* Test Record Number: *3033*
Test Date: *06/26/2026* Test Time: *8:35pm EDT*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	8:36pm
FLO	Pass	8:36pm
FC	Pass	8:36pm

Temperature Tests

Test	Status	Time
FC1	Pass	8:36pm
SRC	Pass	8:36pm
DET	Pass	8:36pm
BAR	Pass	8:36pm
BT	Pass	8:36pm

Blank Tests

Test	Status	Time
AIR	Pass	8:37pm

Printer Tests

Test	Status	Time
PRNT	Pass	8:37pm

CRC Tests

Test	Status	Time
COMP	Pass	8:37pm
CAL	Pass	8:37pm

Preventive Maintenance
Status: Pass



Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Pender Instrument Location BAT Mobile Unit 9

Instrument Serial No. 008647

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

(1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;

(2) Verify instrument displays time and date;

(3) Initiate breath test sequence;

(4) Enter information as prompted;

(5) Verify instrument accuracy;

(6) When "PLEASE BLOW" appears, collect breath sample;

(7) When "PLEASE BLOW" appears, collect breath sample;

(8) Print test record;

(9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and

(10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 26th day of June, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.

Signature of Certifying Official

226313
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

DHHS 4080 (04/20)

Intox EC/IR-II: Subject Test

PENDER COUNTY BAT MOBILE UNIT 9 700

Serial Number: *008647*
Test Date: *06/26/2026*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name: *Sharpe Jr., Robert J*
Permit Number: *1820-8591*
Effective:
02/01/2026-02/01/2028

Officer's Name: *NONE, NONE*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG516203
Exp Date: 06/11/2027

Test	g/210L	Time
DIAG	Pass	8:26pm
AIR BLK	.00	8:27pm
ACCY CHK	.07	8:28pm
AIR BLK	.00	8:29pm
SUB TEST	**.00**	**8:31pm**
AIR BLK	.00	8:32pm
SUB TEST	**.00**	**8:33pm**
AIR BLK	.00	8:34pm

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

PENDER COUNTY BAT MOBILE UNIT 9 700

Serial Number: *008647* Test Record Number: *2993*
Test Date: *06/26/2026* Test Time: *8:36pm EDT*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	8:37pm
FLO	Pass	8:37pm
FC	Pass	8:37pm

Temperature Tests

Test	Status	Time
FC1	Pass	8:37pm
SRC	Pass	8:37pm
DET	Pass	8:37pm
BAR	Pass	8:37pm
BT	Pass	8:37pm

Blank Tests

Test	Status	Time
AIR	Pass	8:37pm

Printer Tests

Test	Status	Time
PRNT	Pass	8:38pm

CRC Tests

Test	Status	Time
COMP	Pass	8:38pm
CAL	Pass	8:38pm

Preventive Maintenance
Status: Pass

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Pender Instrument Location BAT Mobile Unit 9

Instrument Serial No. 008704

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

(1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;

(2) Verify instrument displays time and date;

(3) Initiate breath test sequence;

(4) Enter information as prompted;

(5) Verify instrument accuracy;

(6) When "PLEASE BLOW" appears, collect breath sample;

(7) When "PLEASE BLOW" appears, collect breath sample;

(8) Print test record;

(9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and

(10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 26th day of June, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.

Signature of Certifying Official

226313
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

DHHS 4080 (04/20)

Intox EC/IR-II: Subject Test

PENDER COUNTY BAT MOBILE UNIT 9 700

Serial Number: *008704*
Test Date: *06/26/2026*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name: *Sharpe Jr., Robert J*
Permit Number: *1820-8591*
Effective:
02/01/2026-02/01/2028

Officer's Name: *Sharpe Jr., Robert J*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG506303
Exp Date: 03/04/2027

Test	g/210L	Time
DIAG	Pass	8:24pm
AIR BLK	.00	8:25pm
ACCY CHK	.07	8:26pm
AIR BLK	.00	8:27pm
SUB TEST	**.00**	**8:28pm**
AIR BLK	.00	8:29pm
SUB TEST	**.00**	**8:30pm**
AIR BLK	.00	8:31pm

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

PENDER COUNTY BAT MOBILE UNIT 9 700

Serial Number: *008704* Test Record Number: *1043*
Test Date: *06/26/2026* Test Time: *8:35pm EDT*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	8:36pm
FLO	Pass	8:36pm
FC	Pass	8:36pm

Temperature Tests

Test	Status	Time
FC1	Pass	8:36pm
SRC	Pass	8:36pm
DET	Pass	8:36pm
BAR	Pass	8:36pm
BT	Pass	8:36pm

Blank Tests

Test	Status	Time
AIR	Pass	8:37pm

Printer Tests

Test	Status	Time
PRNT	Pass	8:37pm

CRC Tests

Test	Status	Time
COMP	Pass	8:37pm
CAL	Pass	8:37pm

Preventive Maintenance
Status: Pass



Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Pender Instrument Location BAT Mobile Unit 9

Instrument Serial No. 00 8826

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

(1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;

(2) Verify instrument displays time and date;

(3) Initiate breath test sequence;

(4) Enter information as prompted;

(5) Verify instrument accuracy;

(6) When "PLEASE BLOW" appears, collect breath sample;

(7) When "PLEASE BLOW" appears, collect breath sample;

(8) Print test record;

(9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and

(10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 26th day of June, 20 26 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.

Signature of Certifying Official

226313
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

DHHS 4080 (04/20)

Intox EC/IR-II: Subject Test

PENDER COUNTY BAT MOBILE UNIT 9 700

Serial Number: *008826*
Test Date: *06/26/2026*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name: *Sharpe Jr., Robert J*
Permit Number: *1820-8591*
Effective:
02/01/2026-02/01/2028

Officer's Name: *NONE, NONE*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG516204
Exp Date: 06/11/2027

Test	g/210L	Time
DIAG	Pass	8:38pm
AIR BLK	.00	8:39pm
ACCY CHK	.07	8:39pm
AIR BLK	.00	8:40pm
SUB TEST	**.00**	**8:41pm**
AIR BLK	.00	8:42pm
SUB TEST	**.00**	**8:43pm**
AIR BLK	.00	8:44pm

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

PENDER COUNTY BAT MOBILE UNIT 9 700

Serial Number: *008826* Test Record Number: *8681*
Test Date: *06/26/2026* Test Time: *8:45pm EDT*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	8:45pm
FLO	Pass	8:45pm
FC	Pass	8:45pm

Temperature Tests

Test	Status	Time
FC1	Pass	8:45pm
SRC	Pass	8:45pm
DET	Pass	8:45pm
BAR	Pass	8:45pm
BT	Pass	8:45pm

Blank Tests

Test	Status	Time
AIR	Pass	8:46pm

Printer Tests

Test	Status	Time
PRNT	Pass	8:46pm

CRC Tests

Test	Status	Time
COMP	Pass	8:46pm
CAL	Pass	8:46pm

Preventive Maintenance
Status: Pass

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Person Instrument Location BAT Mobile Unit 10

Instrument Serial No. 005584

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

(1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;

(2) Verify instrument displays time and date;

(3) Initiate breath test sequence;

(4) Enter information as prompted;

(5) Verify instrument accuracy;

(6) When "PLEASE BLOW" appears, collect breath sample;

(7) When "PLEASE BLOW" appears, collect breath sample;

(8) Print test record;

(9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and

(10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 27 day of June, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.

Signature of Certifying Official

193759
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

DHHS 4080 (04/20)

Intox EC/IR-II: Subject Test

PERSON COUNTY BAT MOBILE UNIT 10 720

Serial Number: *008584*
Test Date: *06/27/2026*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name: *Carroll, Barry Jean D*
Permit Number: *0019-3759*
Effective:
04/01/2026-04/01/2028

Officer's Name: *NONE, NONE*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG534301
Exp Date: 12/09/2027

Test	g/210L	Time
DIAG	Pass	2:57pm
AIR BLK	.00	2:58pm
ACCY CHK	.08	2:59pm
AIR BLK	.00	3:00pm
SUB TEST	**.00**	**3:00pm**
AIR BLK	.00	3:01pm
SUB TEST	**.00**	**3:03pm**
AIR BLK	.00	3:04pm

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

PERSON COUNTY BAT MOBILE UNIT 10 720

Serial Number: *008584* Test Record Number: *2917*
Test Date: *06/27/2026* Test Time: *3:04pm EDT*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	3:05pm
FLO	Pass	3:05pm
FC	Pass	3:05pm

Temperature Tests

Test	Status	Time
FC1	Pass	3:05pm
SRC	Pass	3:05pm
DET	Pass	3:05pm
BAR	Pass	3:05pm
BT	Pass	3:05pm

Blank Tests

Test	Status	Time
AIR	Pass	3:05pm

Printer Tests

Test	Status	Time
PRNT	Pass	3:06pm

CRC Tests

Test	Status	Time
COMP	Pass	3:06pm
CAL	Pass	3:06pm

Preventive Maintenance
Status: Pass

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Person Instrument Location BAT Mobile unit 10

Instrument Serial No. 008686

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

(1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;

(2) Verify instrument displays time and date;

(3) Initiate breath test sequence;

(4) Enter information as prompted;

(5) Verify instrument accuracy;

(6) When "PLEASE BLOW" appears, collect breath sample;

(7) When "PLEASE BLOW" appears, collect breath sample;

(8) Print test record;

(9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and

(10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 27 day of June, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.

Signature of Certifying Official

193759
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

DHHS 4080 (04/20)

Intox EC/IR-II: Subject Test

PERSON COUNTY BAT MOBILE UNIT 10 720

Serial Number: *008686*
Test Date: *06/27/2026*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name: *Carroll, Barry Jean D*
Permit Number: *0019-3759*
Effective:
04/01/2026-04/01/2028

Officer's Name: *NONE, NONE*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG506302
Exp Date: 03/04/2027

Test	g/210L	Time
DIAG	Pass	3:02pm
AIR BLK	.00	3:03pm
ACCY CHK	.08	3:03pm
AIR BLK	.00	3:04pm
SUB TEST	**.00**	**3:05pm**
AIR BLK	.00	3:06pm
SUB TEST	**.00**	**3:07pm**
AIR BLK	.00	3:08pm

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

PERSON COUNTY BAT MOBILE UNIT 10 720

Serial Number: *008686* Test Record Number: *7262*
Test Date: *06/27/2026* Test Time: *3:26pm EDT*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	3:27pm
FLO	Pass	3:27pm
FC	Pass	3:27pm

Temperature Tests

Test	Status	Time
FC1	Pass	3:27pm
SRC	Pass	3:27pm
DET	Pass	3:27pm
BAR	Pass	3:27pm
BT	Pass	3:27pm

Blank Tests

Test	Status	Time
AIR	Pass	3:28pm

Printer Tests

Test	Status	Time
PRNT	Pass	3:28pm

CRC Tests

Test	Status	Time
COMP	Pass	3:28pm
CAL	Pass	3:28pm

Preventive Maintenance
Status: Pass

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County PERSON Instrument Location PERSON CO. LEC

Instrument Serial No. 008693 120 COURT ST
ROXBORO, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

(1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;

(2) Verify instrument displays time and date;

(3) Initiate breath test sequence;

(4) Enter information as prompted;

(5) Verify instrument accuracy;

(6) When "PLEASE BLOW" appears, collect breath sample;

(7) When "PLEASE BLOW" appears, collect breath sample;

(8) Print test record;

(9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and

(10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 24 day of JUNE, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.

E A Smith
Signature of Certifying Official

179207
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

DHHS 4080 (04/20)

Intox EC/IR-II: Subject Test

PERSON COUNTY LAW ENFORCEMENT CTR 720

Serial Number: *008693*
Test Date: *06/24/2026*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name: *Bryant, Earl A*
Permit Number: *0017-9707*
Effective:
02/01/2026-02/01/2028

Officer's Name: *NONE, NONE*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG501303
Exp Date: 01/13/2027

Test	g/210L	Time
DIAG	Pass	3:38pm
AIR BLK	.00	3:39pm
ACCY CHK	.07	3:39pm
AIR BLK	.00	3:40pm
SUB TEST	**.00**	**3:41pm**
AIR BLK	.00	3:42pm
SUB TEST	**.00**	**3:43pm**
AIR BLK	.00	3:44pm

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

PERSON COUNTY LAW ENFORCEMENT CTR 720

Serial Number: *008693* Test Record Number: *2238*
Test Date: *06/24/2026* Test Time: *3:46pm EDT*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	3:46pm
FLO	Pass	3:46pm
FC	Pass	3:46pm

Temperature Tests

Test	Status	Time
FC1	Pass	3:46pm
SRC	Pass	3:46pm
DET	Pass	3:46pm
BAR	Pass	3:46pm
BT	Pass	3:46pm

Blank Tests

Test	Status	Time
AIR	Pass	3:47pm

Printer Tests

Test	Status	Time
PRNT	Pass	3:47pm

CRC Tests

Test	Status	Time
COMP	Pass	3:47pm
CAL	Pass	3:47pm

Preventive Maintenance
Status: Pass



Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Person Instrument Location BAT Mobile Unit 10

Instrument Serial No. 008776

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

(1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;

(2) Verify instrument displays time and date;

(3) Initiate breath test sequence;

(4) Enter information as prompted;

(5) Verify instrument accuracy;

(6) When "PLEASE BLOW" appears, collect breath sample;

(7) When "PLEASE BLOW" appears, collect breath sample;

(8) Print test record;

(9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and

(10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 27 day of June, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.

Signature of Certifying Official

193759
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

DHHS 4080 (04/20)

Intox EC/IR-II: Subject Test

PERSON COUNTY BAT MOBILE UNIT 10 720

Serial Number: *008776*
Test Date: *06/27/2026*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name: *Carroll, Barry Jean D*
Permit Number: *0019-3759*
Effective:
04/01/2026-04/01/2028

Officer's Name: *NONE, NONE*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG534301
Exp Date: 12/09/2027

Test	g/210L	Time
DIAG	Pass	2:59pm
AIR BLK	.00	3:00pm
ACCY CHK	.08	3:01pm
AIR BLK	.00	3:02pm
SUB TEST	**.00**	**3:02pm**
AIR BLK	.00	3:03pm
SUB TEST	**.00**	**3:05pm**
AIR BLK	.00	3:06pm

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

PERSON COUNTY BAT MOBILE UNIT 10 720

Serial Number: *008776* Test Record Number: *4234*
Test Date: *06/27/2026* Test Time: *3:06pm EDT*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	3:07pm
FLO	Pass	3:07pm
FC	Pass	3:07pm

Temperature Tests

Test	Status	Time
FC1	Pass	3:07pm
SRC	Pass	3:07pm
DET	Pass	3:07pm
BAR	Pass	3:07pm
BT	Pass	3:07pm

Blank Tests

Test	Status	Time
AIR	Pass	3:08pm

Printer Tests

Test	Status	Time
PRNT	Pass	3:08pm

CRC Tests

Test	Status	Time
COMP	Pass	3:08pm
CAL	Pass	3:08pm

Preventive Maintenance
Status: Pass

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Person Instrument Location BAT Mobile unit 10

Instrument Serial No. 008779

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

(1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;

(2) Verify instrument displays time and date;

(3) Initiate breath test sequence;

(4) Enter information as prompted;

(5) Verify instrument accuracy;

(6) When "PLEASE BLOW" appears, collect breath sample;

(7) When "PLEASE BLOW" appears, collect breath sample;

(8) Print test record;

(9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and

(10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 27 day of June, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.

Signature of Certifying Official

193759
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

DHHS 4080 (04/20)

Intox EC/IR-II: Subject Test

PERSON COUNTY BAT MOBILE UNIT 10 720

Serial Number: *008779*
Test Date: *06/27/2026*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name: *Carroll, Barry Jean D*
Permit Number: *0019-3759*
Effective:
04/01/2026-04/01/2028

Officer's Name: *NONE, NONE*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG431002
Exp Date: 11/05/2026

Test	g/210L	Time
DIAG	Pass	2:59pm
AIR BLK	.00	3:00pm
ACCY CHK	.07	3:00pm
AIR BLK	.00	3:01pm
SUB TEST	**.00**	**3:02pm**
AIR BLK	.00	3:03pm
SUB TEST	**.00**	**3:05pm**
AIR BLK	.00	3:06pm

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

PERSON COUNTY BAT MOBILE UNIT 10 720

Serial Number: *008779* Test Record Number: *4158*
Test Date: *06/27/2026* Test Time: *3:06pm EDT*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	3:07pm
FLO	Pass	3:07pm
FC	Pass	3:07pm

Temperature Tests

Test	Status	Time
FC1	Pass	3:07pm
SRC	Pass	3:07pm
DET	Pass	3:07pm
BAR	Pass	3:07pm
BT	Pass	3:07pm

Blank Tests

Test	Status	Time
AIR	Pass	3:08pm

Printer Tests

Test	Status	Time
PRNT	Pass	3:08pm

CRC Tests

Test	Status	Time
COMP	Pass	3:08pm
CAL	Pass	3:08pm

Preventive Maintenance
Status: Pass



Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD INTOXIMETERS, MODEL INTOX EC/IR II and MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County PERSON Instrument Location ROXBORO PD

Instrument Serial No. 008880 109 N. LAMAR ST ROXBORO, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

(1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;

(2) Verify instrument displays time and date;

(3) Initiate breath test sequence;

(4) Enter information as prompted;

(5) Verify instrument accuracy;

(6) When "PLEASE BLOW" appears, collect breath sample;

(7) When "PLEASE BLOW" appears, collect breath sample;

(8) Print test record;

(9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and

(10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 16 day of JUNE, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.

E A Bryant
Signature of Certifying Official

179707
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

DHHS 4080 (04/20)

Intox EC/IR-II: Subject Test

PERSON COUNTY ROXBORO POLICE DEPT 720

Serial Number: *008880*
Test Date: *06/16/2026*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name: *Bryant, Earl A*
Permit Number: *0017-9707*
Effective:
02/01/2026-02/01/2028

Officer's Name: *NONE, NONE*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG516203
Exp Date: 06/11/2027

Test	g/210L	Time
DIAG	Pass	4:21pm
AIR BLK	.00	4:22pm
ACCY CHK	.08	4:23pm
AIR BLK	.00	4:24pm
SUB TEST	**.00**	**4:25pm**
AIR BLK	.00	4:25pm
SUB TEST	**.00**	**4:27pm**
AIR BLK	.00	4:28pm

Reported AC: .00 g/210L

E A Bryant

Signature of Chemical Analyst

Court CVR

E A Bryant

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

PERSON COUNTY ROXBORO POLICE DEPT 720

Serial Number: *008880* Test Record Number: *2651*
Test Date: *06/16/2026* Test Time: *4:28pm EDT*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	4:28pm
FLO	Pass	4:28pm
FC	Pass	4:29pm

Temperature Tests

Test	Status	Time
FC1	Pass	4:29pm
SRC	Pass	4:29pm
DET	Pass	4:29pm
BAR	Pass	4:29pm
BT	Pass	4:29pm

Blank Tests

Test	Status	Time
AIR	Pass	4:29pm

Printer Tests

Test	Status	Time
PRNT	Pass	4:29pm

CRC Tests

Test	Status	Time
COMP	Pass	4:30pm
CAL	Pass	4:30pm

Preventive Maintenance
Status: Pass

E A Bryant

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD INTOXIMETERS, MODEL INTOX EC/IR II and MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Pitt Instrument Location Pitt Co Detention Center

Instrument Serial No. 008668 124 New Hope Rd, Greenville, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

(1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;

(2) Verify instrument displays time and date;

(3) Initiate breath test sequence;

(4) Enter information as prompted;

(5) Verify instrument accuracy;

(6) When "PLEASE BLOW" appears, collect breath sample;

(7) When "PLEASE BLOW" appears, collect breath sample;

(8) Print test record;

(9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and

(10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 1st day of June, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.

Signature of Certifying Official

377722
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

DHHS 4080 (04/20)

Intox EC/IR-II: Subject Test

PITT COUNTY PITT CO DETENTION 730

Serial Number: *008668*
Test Date: *06/01/2026*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name: *Gray, Kelly D*
Permit Number: *0037-7722*
Effective:
02/01/2026-02/01/2028

Officer's Name: *NONE, NONE*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG506303
Exp Date: 03/04/2027

Test	g/210L	Time
DIAG	Pass	2:30pm
AIR BLK	.00	2:31pm
ACCY CHK	.07	2:32pm
AIR BLK	.00	2:33pm
SUB TEST	**.00**	**2:34pm**
AIR BLK	.00	2:34pm
SUB TEST	**.00**	**2:36pm**
AIR BLK	.00	2:37pm

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

PITT COUNTY PITT CO DETENTION 730

Serial Number: *008668* Test Record Number: *4933*
Test Date: *06/01/2026* Test Time: *2:38pm EDT*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	2:39pm
FLO	Pass	2:39pm
FC	Pass	2:39pm

Temperature Tests

Test	Status	Time
FC1	Pass	2:39pm
SRC	Pass	2:39pm
DET	Pass	2:39pm
BAR	Pass	2:39pm
BT	Pass	2:39pm

Blank Tests

Test	Status	Time
AIR	Pass	2:40pm

Printer Tests

Test	Status	Time
PRNT	Pass	2:40pm

CRC Tests

Test	Status	Time
COMP	Pass	2:40pm
CAL	Pass	2:40pm

Preventive Maintenance
Status: Pass

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD INTOXIMETERS, MODEL INTOX EC/IR II and MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Pitt Instrument Location Ayden P.D.

Instrument Serial No. 008851 414 West Ave., Ayden, NC.

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

(1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;

(2) Verify instrument displays time and date;

(3) Initiate breath test sequence;

(4) Enter information as prompted;

(5) Verify instrument accuracy;

(6) When "PLEASE BLOW" appears, collect breath sample;

(7) When "PLEASE BLOW" appears, collect breath sample;

(8) Print test record;

(9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and

(10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 30th day of June, 2024 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.

Signature of Certifying Official

377722
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

DHHS 4080 (04/20)

Intox EC/IR-II: Subject Test

PITT COUNTY AYDEN PD 730

Serial Number: *008851*
Test Date: *06/30/2026*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name: *Gray, Kelly D*
Permit Number: *0037-7722*
Effective:
02/01/2026-02/01/2028

Officer's Name: *NONE, NONE*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG602102
Exp Date: 01/21/2028

Test	g/210L	Time
DIAG	Pass	9:18am
AIR BLK	.00	9:18am
ACCY CHK	.08	9:19am
AIR BLK	.00	9:20am
SUB TEST	**.00**	**9:21am**
AIR BLK	.00	9:22am
SUB TEST	**.00**	**9:24am**
AIR BLK	.00	9:25am

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

PITT COUNTY AYDEN PD 730

Serial Number: *008851* Test Record Number: *1113*
Test Date: *06/30/2026* Test Time: *9:26am EDT*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	9:26am
FLO	Pass	9:26am
FC	Pass	9:26am

Temperature Tests

Test	Status	Time
FC1	Pass	9:27am
SRC	Pass	9:27am
DET	Pass	9:27am
BAR	Pass	9:27am
BT	Pass	9:27am

Blank Tests

Test	Status	Time
AIR	Pass	9:27am

Printer Tests

Test	Status	Time
PRNT	Pass	9:27am

CRC Tests

Test	Status	Time
COMP	Pass	9:27am
CAL	Pass	9:27am

Preventive Maintenance
Status: Pass

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Polk Instrument Location Polk County Jail

Instrument Serial No. 008832 Columbus, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

(1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;

(2) Verify instrument displays time and date;

(3) Initiate breath test sequence;

(4) Enter information as prompted;

(5) Verify instrument accuracy;

(6) When "PLEASE BLOW" appears, collect breath sample;

(7) When "PLEASE BLOW" appears, collect breath sample;

(8) Print test record;

(9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and

(10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 11 day of June, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.

Signature of Certifying Official

244987
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

DHHS 4080 (04/20)

Intox EC/IR-II: Subject Test

POLK COUNTY POLK COUNTY JAIL 740

Serial Number: *008832*
Test Date: *06/11/2026*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name: *Loftis, Benjamin C*
Permit Number: *0024-4987*
Effective:
02/01/2026-02/01/2028

Officer's Name: *NONE, NONE*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG431001
Exp Date: 11/05/2026

Test	g/210L	Time
DIAG	Pass	10:46am
AIR BLK	.00	10:46am
ACCY CHK	.07	10:47am
AIR BLK	.00	10:48am
SUB TEST	**.00**	**10:48am**
AIR BLK	.00	10:49am
SUB TEST	**.00**	**10:51am**
AIR BLK	.00	10:51am

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

POLK COUNTY POLK COUNTY JAIL 740

Serial Number: *008832* Test Record Number: *2068*
Test Date: *06/11/2026* Test Time: *10:52am EDT*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	10:52am
FLO	Pass	10:52am
FC	Pass	10:52am

Temperature Tests

Test	Status	Time
FC1	Pass	10:52am
SRC	Pass	10:52am
DET	Pass	10:52am
BAR	Pass	10:52am
BT	Pass	10:52am

Blank Tests

Test	Status	Time
AIR	Pass	10:53am

Printer Tests

Test	Status	Time
PRNT	Pass	10:53am

CRC Tests

Test	Status	Time
COMP	Pass	10:53am
CAL	Pass	10:53am

Preventive Maintenance
Status: Pass

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD INTOXIMETERS, MODEL INTOX EC/IR II and MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Polk Instrument Location Polk County Jail

Instrument Serial No. 008881 Columbus, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

(1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;

(2) Verify instrument displays time and date;

(3) Initiate breath test sequence;

(4) Enter information as prompted;

(5) Verify instrument accuracy;

(6) When "PLEASE BLOW" appears, collect breath sample;

(7) When "PLEASE BLOW" appears, collect breath sample;

(8) Print test record;

(9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and

(10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 11 day of June, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.

Signature of Certifying Official

244987
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

DHHS 4080 (04/20)

Intox EC/IR-II: Subject Test

POLK COUNTY POLK COUNTY JAIL 740

Serial Number: *008881*
Test Date: *06/11/2026*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: Male
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name: *Loftis, Benjamin C*
Permit Number: *0024-4987*
Effective:
02/01/2026-02/01/2028

Officer's Name: *NONE, NONE*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG506301
Exp Date: 03/04/2027

Test	g/210L	Time
DIAG	Pass	10:45am
AIR BLK	.00	10:45am
ACCY CHK	.08	10:46am
AIR BLK	.00	10:47am
SUB TEST	**.00**	**10:48am**
AIR BLK	.00	10:48am
SUB TEST	**.00**	**10:50am**
AIR BLK	.00	10:51am

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court/CVR

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

POLK COUNTY POLK COUNTY JAIL 740

Serial Number: *008881* Test Record Number: *1327*
Test Date: *06/11/2026* Test Time: *10:51am EDT*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	10:52am
FLO	Pass	10:52am
FC	Pass	10:52am

Temperature Tests

Test	Status	Time
FC1	Pass	10:52am
SRC	Pass	10:52am
DET	Pass	10:52am
BAR	Pass	10:52am
BT	Pass	10:52am

Blank Tests

Test	Status	Time
AIR	Pass	10:52am

Printer Tests

Test	Status	Time
PRNT	Pass	10:52am

CRC Tests

Test	Status	Time
COMP	Pass	10:52am
CAL	Pass	10:52am

Preventive Maintenance
Status: Pass

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County RANDOLPH Instrument Location RANDLEMAN POLICE DEPARTMENT

Instrument Serial No. 008737

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

(1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;

(2) Verify instrument displays time and date;

(3) Initiate breath test sequence;

(4) Enter information as prompted;

(5) Verify instrument accuracy;

(6) When "PLEASE BLOW" appears, collect breath sample;

(7) When "PLEASE BLOW" appears, collect breath sample;

(8) Print test record;

(9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and

(10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 22 day of JUNE, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.

Signature of Certifying Official

739771
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

RANDOLPH COUNTY RANDLEMAN PD 750

Serial Number: *008737*
Test Date: *06/22/2026*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name: *Galloway, Charles L*
Permit Number: *0023-9771*
Effective:
02/01/2026-02/01/2028

Officer's Name: *NONE, NONE*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG602202
Exp Date: 01/22/2028

Test	g/210L	Time
DIAG	Pass	5:35pm
AIR BLK	.00	5:36pm
ACCY CHK	.08	5:36pm
AIR BLK	.00	5:37pm
SUB TEST	**.00**	**5:38pm**
AIR BLK	.00	5:39pm
SUB TEST	**.00**	**5:40pm**
AIR BLK	.00	5:41pm

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

RANDOLPH COUNTY RANDLEMAN PD 750

Serial Number: *008737* Test Record Number: *1708*
Test Date: *06/22/2026* Test Time: *5:42pm EDT*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	5:42pm
FLO	Pass	5:42pm
FC	Pass	5:42pm

Temperature Tests

Test	Status	Time
FC1	Pass	5:42pm
SRC	Pass	5:42pm
DET	Pass	5:42pm
BAR	Pass	5:42pm
BT	Pass	5:42pm

Blank Tests

Test	Status	Time
AIR	Pass	5:43pm

Printer Tests

Test	Status	Time
PRNT	Pass	5:43pm

CRC Tests

Test	Status	Time
COMP	Pass	5:43pm
CAL	Pass	5:43pm

Preventive Maintenance
Status: Pass



Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County RANDOLPH Instrument Location ARCHDALE POLICE DEPARTMENT

Instrument Serial No. 008791

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

(1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;

(2) Verify instrument displays time and date;

(3) Initiate breath test sequence;

(4) Enter information as prompted;

(5) Verify instrument accuracy;

(6) When "PLEASE BLOW" appears, collect breath sample;

(7) When "PLEASE BLOW" appears, collect breath sample;

(8) Print test record;

(9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and

(10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 22 day of JUNE, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.

Signature of Certifying Official

239771
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

DHHS 4080 (04/20)

Intox EC/IR-II: Subject Test

RANDOLPH COUNTY ARCHDALE PD 750

Serial Number: *008791*
Test Date: *06/22/2026*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name: *Galloway, Charles L*
Permit Number: *0023-9771*
Effective:
02/01/2026-02/01/2028

Officer's Name: *NONE, NONE*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG602202
Exp Date: 01/22/2028

Test	g/210L	Time
DIAG	Pass	3:13pm
AIR BLK	.00	3:14pm
ACCY CHK	.08	3:15pm
AIR BLK	.00	3:16pm
SUB TEST	**.00**	**3:17pm**
AIR BLK	.00	3:18pm
SUB TEST	**.00**	**3:20pm**
AIR BLK	.00	3:21pm

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

RANDOLPH COUNTY ARCHDALE PD 750

Serial Number: *008791* Test Record Number: *1813*
Test Date: *06/22/2026* Test Time: *3:23pm EDT*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	3:24pm
FLO	Pass	3:24pm
FC	Pass	3:24pm

Temperature Tests

Test	Status	Time
FC1	Pass	3:24pm
SRC	Pass	3:24pm
DET	Pass	3:24pm
BAR	Pass	3:24pm
BT	Pass	3:24pm

Blank Tests

Test	Status	Time
AIR	Pass	3:25pm

Printer Tests

Test	Status	Time
PRNT	Pass	3:25pm

CRC Tests

Test	Status	Time
COMP	Pass	3:25pm
CAL	Pass	3:25pm

Preventive Maintenance
Status: Pass



Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County RANDOLPH Instrument Location LIBERTY POLICE DEPARTMENT

Instrument Serial No. 008846

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

(1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;

(2) Verify instrument displays time and date;

(3) Initiate breath test sequence;

(4) Enter information as prompted;

(5) Verify instrument accuracy;

(6) When "PLEASE BLOW" appears, collect breath sample;

(7) When "PLEASE BLOW" appears, collect breath sample;

(8) Print test record;

(9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and

(10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 22 day of JUNE, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.

Signature of Certifying Official

J39771
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

DHHS 4080 (04/20)

Intox EC/IR-II: Subject Test

RANDOLPH COUNTY LIBERTY PD 750

Serial Number: *008846*
Test Date: *06/22/2026*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name: *Galloway, Charles L*
Permit Number: *0023-9771*
Effective:
02/01/2026-02/01/2028

Officer's Name: *NONE, NONE*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG602202
Exp Date: 01/22/2028

Test	g/210L	Time
DIAG	Pass	7:07pm
AIR BLK	.00	7:08pm
ACCY CHK	.08	7:08pm
AIR BLK	.00	7:09pm
SUB TEST	**.00**	**7:10pm**
AIR BLK	.00	7:11pm
SUB TEST	**.00**	**7:13pm**
AIR BLK	.00	7:14pm

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

RANDOLPH COUNTY LIBERTY PD 750

Serial Number: *008846* Test Record Number: *6439*
Test Date: *06/22/2026* Test Time: *7:14pm EDT*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	7:15pm
FLO	Pass	7:15pm
FC	Pass	7:15pm

Temperature Tests

Test	Status	Time
FC1	Pass	7:15pm
SRC	Pass	7:15pm
DET	Pass	7:15pm
BAR	Pass	7:15pm
BT	Pass	7:15pm

Blank Tests

Test	Status	Time
AIR	Pass	7:15pm

Printer Tests

Test	Status	Time
PRNT	Pass	7:16pm

CRC Tests

Test	Status	Time
COMP	Pass	7:16pm
CAL	Pass	7:16pm

Preventive Maintenance
Status: Pass



Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County RANDOLPH Instrument Location RANDOLPH COUNTY DETENTION CENTER

Instrument Serial No. 008860

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

(1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;

(2) Verify instrument displays time and date;

(3) Initiate breath test sequence;

(4) Enter information as prompted;

(5) Verify instrument accuracy;

(6) When "PLEASE BLOW" appears, collect breath sample;

(7) When "PLEASE BLOW" appears, collect breath sample;

(8) Print test record;

(9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and

(10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 22 day of JUNE, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.

Signature of Certifying Officer

239771
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

RANDOLPH COUNTY DETENTION CENTER 750

Serial Number: *008860*
Test Date: *06/22/2026*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name: *Galloway, Charles L*
Permit Number: *0023-9771*
Effective:
02/01/2026-02/01/2028

Officer's Name: *NONE, NONE*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG506301
Exp Date: 03/04/2027

Test	g/210L	Time
DIAG	Pass	12:33pm
AIR BLK	.00	12:33pm
ACCY CHK	.07	12:34pm
AIR BLK	.00	12:35pm
SUB TEST	**.00**	**12:36pm**
AIR BLK	.00	12:36pm
SUB TEST	**.00**	**12:38pm**
AIR BLK	.00	12:39pm

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

RANDOLPH COUNTY DETENTION CENTER 750

Serial Number: *008860* Test Record Number: *3920*
Test Date: *06/22/2026* Test Time: *12:39pm EDT*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	12:40pm
FLO	Pass	12:40pm
FC	Pass	12:40pm

Temperature Tests

Test	Status	Time
FC1	Pass	12:40pm
SRC	Pass	12:40pm
DET	Pass	12:40pm
BAR	Pass	12:40pm
BT	Pass	12:40pm

Blank Tests

Test	Status	Time
AIR	Pass	12:41pm

Printer Tests

Test	Status	Time
PRNT	Pass	12:41pm

CRC Tests

Test	Status	Time
COMP	Pass	12:41pm
CAL	Pass	12:41pm

Preventive Maintenance
Status: Pass

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County RANDOLPH Instrument Location RANDOLPH COUNTY

Instrument Serial No. 008899 DETENTION CENTER

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

(1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;

(2) Verify instrument displays time and date;

(3) Initiate breath test sequence;

(4) Enter information as prompted;

(5) Verify instrument accuracy;

(6) When "PLEASE BLOW" appears, collect breath sample;

(7) When "PLEASE BLOW" appears, collect breath sample;

(8) Print test record;

(9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and

(10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 22 day of JUNE, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.

THE GREAT SEAL OF THE STATE OF NORTH CAROLINA

Signature of Certifying Official

23977I
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

RANDOLPH COUNTY DETENTION CENTER 750

Serial Number: *008899*
Test Date: *06/22/2026*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name: *Galloway, Charles L*
Permit Number: *0023-9771*
Effective:
02/01/2026-02/01/2028

Officer's Name: *NONE, NONE*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG506301
Exp Date: 03/04/2027

Test	g/210L	Time
DIAG	Pass	12:31pm
AIR BLK	.00	12:32pm
ACCY CHK	.07	12:33pm
AIR BLK	.00	12:34pm
SUB TEST	**.00**	**12:35pm**
AIR BLK	.00	12:36pm
SUB TEST	**.00**	**12:37pm**
AIR BLK	.00	12:38pm

Reported AC: .00 g/210L

Signature of ~~Chemical~~ Analyst

Court CVR

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

RANDOLPH COUNTY DETENTION CENTER 750

Serial Number: *008899* Test Record Number: *4524*
Test Date: *06/22/2026* Test Time: *12:39pm EDT*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	12:39pm
FLO	Pass	12:39pm
FC	Pass	12:39pm

Temperature Tests

Test	Status	Time
FC1	Pass	12:40pm
SRC	Pass	12:40pm
DET	Pass	12:40pm
BAR	Pass	12:40pm
BT	Pass	12:40pm

Blank Tests

Test	Status	Time
AIR	Pass	12:40pm

Printer Tests

Test	Status	Time
PRNT	Pass	12:40pm

CRC Tests

Test	Status	Time
COMP	Pass	12:40pm
CAL	Pass	12:40pm

Preventive Maintenance
Status: Pass



Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Randolph Instrument Location BAT Mobile Unit II

Instrument Serial No. 008970

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

(1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;

(2) Verify instrument displays time and date;

(3) Initiate breath test sequence;

(4) Enter information as prompted;

(5) Verify instrument accuracy;

(6) When "PLEASE BLOW" appears, collect breath sample;

(7) When "PLEASE BLOW" appears, collect breath sample;

(8) Print test record;

(9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and

(10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 19th day of June, 2024 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.

Signature of Certifying Official

062446
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

DHHS 4080 (04/20)

Intox EC/IR-II: Subject Test

RANDOLPH COUNTY BAT MOBILE UNIT 11 750

Serial Number: *008970*
Test Date: *06/19/2026*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name: *Gillstrap, Jeffrey L*
Permit Number: *0006-2446*
Effective:
03/01/2026-03/01/2028

Officer's Name: *NONE, NONE*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG602101
Exp Date: 01/21/2028

Test	g/210L	Time
DIAG	Pass	9:36pm
AIR BLK	.00	9:37pm
ACCY CHK	.07	9:38pm
AIR BLK	.00	9:39pm
SUB TEST	**.00**	**9:40pm**
AIR BLK	.00	9:41pm
SUB TEST	**.00**	**9:42pm**
AIR BLK	.00	9:43pm

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

RANDOLPH COUNTY BAT MOBILE UNIT 11 750

Serial Number: *008970* Test Record Number: *1469*
Test Date: *06/19/2026* Test Time: *9:48pm EDT*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	9:48pm
FLO	Pass	9:48pm
FC	Pass	9:48pm

Temperature Tests

Test	Status	Time
FC1	Pass	9:48pm
SRC	Pass	9:48pm
DET	Pass	9:48pm
BAR	Pass	9:48pm
BT	Pass	9:48pm

Blank Tests

Test	Status	Time
AIR	Pass	9:49pm

Printer Tests

Test	Status	Time
PRNT	Pass	9:49pm

CRC Tests

Test	Status	Time
COMP	Pass	9:49pm
CAL	Pass	9:49pm

Preventive Maintenance
Status: Pass



Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Randolph Instrument Location BAT Mobile Unit II

Instrument Serial No. 008973

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

(1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;

(2) Verify instrument displays time and date;

(3) Initiate breath test sequence;

(4) Enter information as prompted;

(5) Verify instrument accuracy;

(6) When "PLEASE BLOW" appears, collect breath sample;

(7) When "PLEASE BLOW" appears, collect breath sample;

(8) Print test record;

(9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and

(10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 19th day of June, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.

Signature of Certifying Official

062446
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

DHHS 4080 (04/20)

Intox EC/IR-II: Subject Test

RANDOLPH COUNTY BAT MOBILE UNIT 11 750

Serial Number: *008973*
Test Date: *06/19/2026*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name: *Gillstrap, Jeffrey L*
Permit Number: *0006-2446*
Effective:
03/01/2026-03/01/2028

Officer's Name: *NONE, NONE*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG431003
Exp Date: 11/05/2026

Test	g/210L	Time
DIAG	Pass	9:41pm
AIR BLK	.00	9:42pm
ACCY CHK	.07	9:42pm
AIR BLK	.00	9:43pm
SUB TEST	**.00**	**9:44pm**
AIR BLK	.00	9:45pm
SUB TEST	**.00**	**9:46pm**
AIR BLK	.00	9:47pm

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

RANDOLPH COUNTY BAT MOBILE UNIT 11 750

Serial Number: *008973* Test Record Number: *1508*
Test Date: *06/19/2026* Test Time: *9:50pm EDT*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	9:50pm
FLO	Pass	9:50pm
FC	Pass	9:50pm

Temperature Tests

Test	Status	Time
FC1	Pass	9:50pm
SRC	Pass	9:50pm
DET	Pass	9:50pm
BAR	Pass	9:50pm
BT	Pass	9:50pm

Blank Tests

Test	Status	Time
AIR	Pass	9:51pm


Printer Tests

Test	Status	Time
PRNT	Pass	9:51pm

CRC Tests

Test	Status	Time
COMP	Pass	9:51pm
CAL	Pass	9:51pm

Preventive Maintenance
Status: Pass

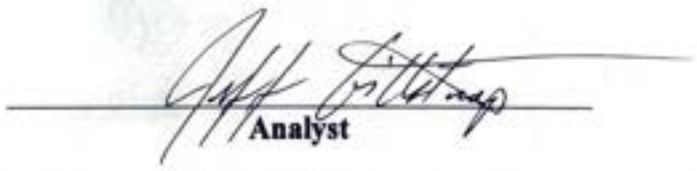

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Robeson Instrument Location BAT Mobile Unit 9

Instrument Serial No. 006575

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

(1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;

(2) Verify instrument displays time and date;

(3) Initiate breath test sequence;

(4) Enter information as prompted;

(5) Verify instrument accuracy;

(6) When "PLEASE BLOW" appears, collect breath sample;

(7) When "PLEASE BLOW" appears, collect breath sample;

(8) Print test record;

(9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and

(10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 30th day of June, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.

Signature of Certifying Official

2266313
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

DHHS 4080 (04/20)

Intox EC/IR-II: Subject Test

ROBESON COUNTY BAT MOBILE UNIT 9 770

Serial Number: *008575*
Test Date: *06/30/2026*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name: *Sharpe Jr., Robert J*
Permit Number: *1820-8591*
Effective:
02/01/2026-02/01/2028

Officer's Name: *NONE, NONE*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG516204
Exp Date: 06/11/2027

Test	g/210L	Time
DIAG	Pass	7:53pm
AIR BLK	.00	7:54pm
ACCY CHK	.07	7:54pm
AIR BLK	.00	7:55pm
SUB TEST	**.00**	**7:56pm**
AIR BLK	.00	7:57pm
SUB TEST	**.00**	**7:59pm**
AIR BLK	.00	8:00pm

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

ROBESON COUNTY BAT MOBILE UNIT 9 770

Serial Number: *008575* Test Record Number: *1612*
Test Date: *06/30/2026* Test Time: *8:00pm EDT*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	8:01pm
FLO	Pass	8:01pm
FC	Pass	8:01pm

Temperature Tests

Test	Status	Time
FC1	Pass	8:01pm
SRC	Pass	8:01pm
DET	Pass	8:01pm
BAR	Pass	8:01pm
BT	Pass	8:01pm

Blank Tests

Test	Status	Time
AIR	Pass	8:02pm


Printer Tests

Test	Status	Time
PRNT	Pass	8:02pm

CRC Tests

Test	Status	Time
COMP	Pass	8:02pm
CAL	Pass	8:02pm

Preventive Maintenance
Status: Pass

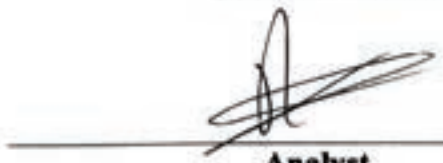

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Robeson Instrument Location BAT Mobile Unit 9

Instrument Serial No. 008616

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

(1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;

(2) Verify instrument displays time and date;

(3) Initiate breath test sequence;

(4) Enter information as prompted;

(5) Verify instrument accuracy;

(6) When "PLEASE BLOW" appears, collect breath sample;

(7) When "PLEASE BLOW" appears, collect breath sample;

(8) Print test record;

(9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and

(10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 30th day of June, 20 26 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.

Signature of Certifying Official

266313
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

DHHS 4080 (04/20)

Intox EC/IR-II: Subject Test

ROBESON COUNTY BAT MOBILE UNIT 9 770

Serial Number: *008616*
Test Date: *06/30/2026*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name: *Sharpe Jr., Robert J*
Permit Number: *1820-8591*
Effective:
02/01/2026-02/01/2028

Officer's Name: *NONE, NONE*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG506303
Exp Date: 03/04/2027

Test	g/210L	Time
DIAG	Pass	7:52pm
AIR BLK	.00	7:53pm
ACCY CHK	.07	7:54pm
AIR BLK	.00	7:55pm
SUB TEST	**.00**	**7:56pm**
AIR BLK	.00	7:57pm
SUB TEST	**.00**	**7:59pm**
AIR BLK	.00	8:00pm

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

ROBESON COUNTY BAT MOBILE UNIT 9 770

Serial Number: *008616* Test Record Number: *3037*
Test Date: *06/30/2026* Test Time: *8:00pm EDT*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	8:00pm
FLO	Pass	8:00pm
FC	Pass	8:01pm

Temperature Tests

Test	Status	Time
FC1	Pass	8:01pm
SRC	Pass	8:01pm
DET	Pass	8:01pm
BAR	Pass	8:01pm
BT	Pass	8:01pm

Blank Tests

Test	Status	Time
AIR	Pass	8:01pm

Printer Tests

Test	Status	Time
PRNT	Pass	8:01pm

CRC Tests

Test	Status	Time
COMP	Pass	8:02pm
CAL	Pass	8:02pm

Preventive Maintenance
Status: Pass



Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Robeson Instrument Location Lumberton Police Department

Instrument Serial No. 008629

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

(1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;

(2) Verify instrument displays time and date;

(3) Initiate breath test sequence;

(4) Enter information as prompted;

(5) Verify instrument accuracy;

(6) When "PLEASE BLOW" appears, collect breath sample;

(7) When "PLEASE BLOW" appears, collect breath sample;

(8) Print test record;

(9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and

(10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 9 day of June, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.

Signature of Certifying Official

365156
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

DHHS 4080 (04/20)

Intox EC/IR-II: Subject Test

ROBESON COUNTY LUMBERTON PD 770

Serial Number: *008629*
Test Date: *06/09/2026*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name: *Garner, Joel K*
Permit Number: *0036-5156*
Effective:
02/01/2026-02/01/2028

Officer's Name: *NONE, NONE*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG516204
Exp Date: 06/11/2027

Test	g/210L	Time
DIAG	Pass	12:58pm
AIR BLK	.00	12:58pm
ACCY CHK	.07	12:59pm
AIR BLK	.00	1:00pm
SUB TEST	**.00**	**1:00pm**
AIR BLK	.00	1:01pm
SUB TEST	**.00**	**1:03pm**
AIR BLK	.00	1:04pm

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

ROBESON COUNTY LUMBERTON PD 770

Serial Number: *008629* Test Record Number: *1573*
Test Date: *06/09/2026* Test Time: *1:05pm EDT*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	1:05pm
FLO	Pass	1:05pm
FC	Pass	1:05pm

Temperature Tests

Test	Status	Time
FC1	Pass	1:05pm
SRC	Pass	1:05pm
DET	Pass	1:05pm
BAR	Pass	1:05pm
BT	Pass	1:05pm

Blank Tests

Test	Status	Time
AIR	Pass	1:06pm

Printer Tests

Test	Status	Time
PRNT	Pass	1:06pm

CRC Tests

Test	Status	Time
COMP	Pass	1:06pm
CAL	Pass	1:06pm

Preventive Maintenance
Status: Pass

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Robeson Instrument Location BAT Mobile Unit 9

Instrument Serial No. 008647

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

(1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;

(2) Verify instrument displays time and date;

(3) Initiate breath test sequence;

(4) Enter information as prompted;

(5) Verify instrument accuracy;

(6) When "PLEASE BLOW" appears, collect breath sample;

(7) When "PLEASE BLOW" appears, collect breath sample;

(8) Print test record;

(9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and

(10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 30th day of June, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.

Signature of Certifying Official

226313
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

DHHS 4080 (04/20)

Intox EC/IR-II: Subject Test

ROBESON COUNTY BAT MOBILE UNIT 9 770

Serial Number: *008647*
Test Date: *06/30/2026*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name: *Sharpe Jr., Robert J*
Permit Number: *1820-8591*
Effective:
02/01/2026-02/01/2028

Officer's Name: *NONE, NONE*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG516203
Exp Date: 06/11/2027

Test	g/210L	Time
DIAG	Pass	7:56pm
AIR BLK	.00	7:57pm
ACCY CHK	.07	7:57pm
AIR BLK	.00	7:58pm
SUB TEST	**.00**	**7:59pm**
AIR BLK	.00	8:00pm
SUB TEST	**.00**	**8:01pm**
AIR BLK	.00	8:02pm

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

ROBESON COUNTY BAT MOBILE UNIT 9 770

Serial Number: *008647* Test Record Number: *2997*
Test Date: *06/30/2026* Test Time: *8:03pm EDT*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	8:03pm
FLO	Pass	8:03pm
FC	Pass	8:03pm

Temperature Tests

Test	Status	Time
FC1	Pass	8:03pm
SRC	Pass	8:03pm
DET	Pass	8:03pm
BAR	Pass	8:03pm
BT	Pass	8:03pm

Blank Tests

Test	Status	Time
AIR	Pass	8:04pm


Printer Tests

Test	Status	Time
PRNT	Pass	8:04pm

CRC Tests

Test	Status	Time
COMP	Pass	8:04pm
CAL	Pass	8:04pm

Preventive Maintenance
Status: Pass



Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD INTOXIMETERS, MODEL INTOX EC/IR II and MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Robeson Instrument Location BAT Mobile Unit 9

Instrument Serial No. 008704

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

(1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;

(2) Verify instrument displays time and date;

(3) Initiate breath test sequence;

(4) Enter information as prompted;

(5) Verify instrument accuracy;

(6) When "PLEASE BLOW" appears, collect breath sample;

(7) When "PLEASE BLOW" appears, collect breath sample;

(8) Print test record;

(9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and

(10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 30th day of June, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.

Signature of Certifying Official

266313
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

DHHS 4080 (04/20)

Intox EC/IR-II: Subject Test

ROBESON COUNTY BAT MOBILE UNIT 9 770

Serial Number: *008704*
Test Date: *06/30/2026*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name: *Sharpe Jr., Robert J*
Permit Number: *1820-8591*
Effective:
02/01/2026-02/01/2028

Officer's Name: *NONE, NONE*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG506303
Exp Date: 03/04/2027

Test	g/210L	Time
DIAG	Pass	7:54pm
AIR BLK	.00	7:55pm
ACCY CHK	.07	7:56pm
AIR BLK	.00	7:57pm
SUB TEST	**.00**	**7:57pm**
AIR BLK	.00	7:58pm
SUB TEST	**.00**	**8:00pm**
AIR BLK	.00	8:01pm

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

ROBESON COUNTY BAT MOBILE UNIT 9 770

Serial Number: *008704* Test Record Number: *1047*
Test Date: *06/30/2026* Test Time: *8:02pm EDT*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	8:02pm
FLO	Pass	8:02pm
FC	Pass	8:02pm

Temperature Tests

Test	Status	Time
FC1	Pass	8:02pm
SRC	Pass	8:02pm
DET	Pass	8:02pm
BAR	Pass	8:02pm
BT	Pass	8:02pm

Blank Tests

Test	Status	Time
AIR	Pass	8:03pm


Printer Tests

Test	Status	Time
PRNT	Pass	8:03pm

CRC Tests

Test	Status	Time
COMP	Pass	8:03pm
CAL	Pass	8:03pm

Preventive Maintenance
Status: Pass

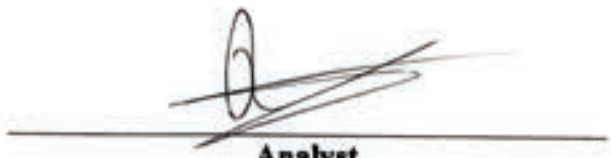

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Robeson Instrument Location Robeson County Detention Center

Instrument Serial No. 008805

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

(1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;

(2) Verify instrument displays time and date;

(3) Initiate breath test sequence;

(4) Enter information as prompted;

(5) Verify instrument accuracy;

(6) When "PLEASE BLOW" appears, collect breath sample;

(7) When "PLEASE BLOW" appears, collect breath sample;

(8) Print test record;

(9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and

(10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 9 day of June, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.

Signature of Certifying Official

365156
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

DHHS 4080 (04/20)

Intox EC/IR-II: Subject Test

ROBESON COUNTY DETENTION CENTER 770

Serial Number: *008805*
Test Date: *06/09/2026*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name: *Garner, Joel K*
Permit Number: *0036-5156*
Effective:
02/01/2026-02/01/2028

Officer's Name: *NONE, NONE*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG602203
Exp Date: 01/22/2028

Test	g/210L	Time
DIAG	Pass	11:38am
AIR BLK	.00	11:38am
ACCY CHK	.08	11:39am
AIR BLK	.00	11:40am
SUB TEST	**.00**	**11:40am**
AIR BLK	.00	11:41am
SUB TEST	**.00**	**11:43am**
AIR BLK	.00	11:43am

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

ROBESON COUNTY DETENTION CENTER 770

Serial Number: *008805* Test Record Number: *5954*
Test Date: *06/09/2026* Test Time: *11:45am EDT*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	11:45am
FLO	Pass	11:45am
FC	Pass	11:45am

Temperature Tests

Test	Status	Time
FC1	Pass	11:45am
SRC	Pass	11:45am
DET	Pass	11:45am
BAR	Pass	11:45am
BT	Pass	11:45am

Blank Tests

Test	Status	Time
AIR	Pass	11:46am

Printer Tests

Test	Status	Time
PRNT	Pass	11:46am

CRC Tests

Test	Status	Time
COMP	Pass	11:46am
CAL	Pass	11:46am

Preventive Maintenance
Status: Pass



Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Robeson Instrument Location St. Pauls

Instrument Serial No. 008814 Police Department

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

(1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;

(2) Verify instrument displays time and date;

(3) Initiate breath test sequence;

(4) Enter information as prompted;

(5) Verify instrument accuracy;

(6) When "PLEASE BLOW" appears, collect breath sample;

(7) When "PLEASE BLOW" appears, collect breath sample;

(8) Print test record;

(9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and

(10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 9 day of June, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.

Signature of Certifying Official

365156
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

DHHS 4080 (04/20)

Intox EC/IR-II: Subject Test

ROBESON COUNTY ST PAULS PD 770

Serial Number: *008814*
Test Date: *06/09/2026*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name: *Garner, Joel K*
Permit Number: *0036-5156*
Effective:
02/01/2026-02/01/2028

Officer's Name: *NONE, NONE*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG501308
Exp Date: 01/13/2027

Test	g/210L	Time
DIAG	Pass	1:54pm
AIR BLK	.00	1:55pm
ACCY CHK	.07	1:55pm
AIR BLK	.00	1:56pm
SUB TEST	**.00**	**1:57pm**
AIR BLK	.00	1:58pm
SUB TEST	**.00**	**1:59pm**
AIR BLK	.00	2:00pm

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

ROBESON COUNTY ST PAULS PD 770

Serial Number: *008814* Test Record Number: *1228*
Test Date: *06/09/2026* Test Time: *2:01pm EDT*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	2:01pm
FLO	Pass	2:01pm
FC	Pass	2:01pm

Temperature Tests

Test	Status	Time
FC1	Pass	2:01pm
SRC	Pass	2:01pm
DET	Pass	2:01pm
BAR	Pass	2:01pm
BT	Pass	2:01pm

Blank Tests

Test	Status	Time
AIR	Pass	2:02pm

Printer Tests

Test	Status	Time
PRNT	Pass	2:02pm

CRC Tests

Test	Status	Time
COMP	Pass	2:02pm
CAL	Pass	2:02pm

Preventive Maintenance
Status: Pass



Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Robeson Instrument Location BAT Mobile Unit 9

Instrument Serial No. 008826

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

(1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;

(2) Verify instrument displays time and date;

(3) Initiate breath test sequence;

(4) Enter information as prompted;

(5) Verify instrument accuracy;

(6) When "PLEASE BLOW" appears, collect breath sample;

(7) When "PLEASE BLOW" appears, collect breath sample;

(8) Print test record;

(9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and

(10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 30th day of June, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.

Signature of Certifying Official

226313
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

DHHS 4080 (04/20)

Intox EC/IR-II: Subject Test

ROBESON COUNTY BAT MOBILE UNIT 9 770

Serial Number: *008826*
Test Date: *06/30/2026*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name: *Sharpe Jr., Robert J*
Permit Number: *1820-8591*
Effective:
02/01/2026-02/01/2028

Officer's Name: *NONE, NONE*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG516204
Exp Date: 06/11/2027

Test	g/210L	Time
DIAG	Pass	8:05pm
AIR BLK	.00	8:06pm
ACCY CHK	.07	8:06pm
AIR BLK	.00	8:07pm
SUB TEST	**.00**	**8:08pm**
AIR BLK	.00	8:09pm
SUB TEST	**.00**	**8:11pm**
AIR BLK	.00	8:12pm

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

ROBESON COUNTY BAT MOBILE UNIT 9 770

Serial Number: *008826* Test Record Number: *8687*
Test Date: *06/30/2026* Test Time: *8:12pm EDT*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	8:13pm
FLO	Pass	8:13pm
FC	Pass	8:13pm

Temperature Tests

Test	Status	Time
FC1	Pass	8:13pm
SRC	Pass	8:13pm
DET	Pass	8:13pm
BAR	Pass	8:13pm
BT	Pass	8:13pm

Blank Tests

Test	Status	Time
AIR	Pass	8:13pm

Printer Tests

Test	Status	Time
PRNT	Pass	8:13pm

CRC Tests

Test	Status	Time
COMP	Pass	8:14pm
CAL	Pass	8:14pm

Preventive Maintenance
Status: Pass



Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Robeson Instrument Location Robeson County Detention Center

Instrument Serial No. 008836

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

(1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;

(2) Verify instrument displays time and date;

(3) Initiate breath test sequence;

(4) Enter information as prompted;

(5) Verify instrument accuracy;

(6) When "PLEASE BLOW" appears, collect breath sample;

(7) When "PLEASE BLOW" appears, collect breath sample;

(8) Print test record;

(9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and

(10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 9 day of June, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.

Signature of Certifying Official

365156
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

ROBESON COUNTY DETENTION CENTER 770

Serial Number: *008836*
Test Date: *06/09/2026*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name: *Garner, Joel K*
Permit Number: *0036-5156*
Effective:
02/01/2026-02/01/2028

Officer's Name: *NONE, NONE*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG602203
Exp Date: 01/22/2028

Test	g/210L	Time
DIAG	Pass	11:55am
AIR BLK	.00	11:56am
ACCY CHK	.08	11:57am
AIR BLK	.00	11:58am
SUB TEST	**.00**	**11:58am**
AIR BLK	.00	11:59am
SUB TEST	**.00**	**12:01pm**
AIR BLK	.00	12:02pm

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

ROBESON COUNTY DETENTION CENTER 770

Serial Number: *008836* Test Record Number: *8436*
Test Date: *06/09/2026* Test Time: *12:02pm EDT*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	12:03pm
FLO	Pass	12:03pm
FC	Pass	12:03pm

Temperature Tests

Test	Status	Time
FC1	Pass	12:03pm
SRC	Pass	12:03pm
DET	Pass	12:03pm
BAR	Pass	12:03pm
BT	Pass	12:03pm

Blank Tests

Test	Status	Time
AIR	Pass	12:04pm

Printer Tests

Test	Status	Time
PRNT	Pass	12:04pm

CRC Tests

Test	Status	Time
COMP	Pass	12:04pm
CAL	Pass	12:04pm

Preventive Maintenance
Status: Pass



Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Robeson Instrument Location Pembroke Police Department

Instrument Serial No. 008837

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

(1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;

(2) Verify instrument displays time and date;

(3) Initiate breath test sequence;

(4) Enter information as prompted;

(5) Verify instrument accuracy;

(6) When "PLEASE BLOW" appears, collect breath sample;

(7) When "PLEASE BLOW" appears, collect breath sample;

(8) Print test record;

(9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and

(10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 9 day of June, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.

Signature of Certifying Official

365156
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

DHHS 4080 (04/20)

Intox EC/IR-II: Subject Test

ROBESON COUNTY PEMBROKE POLICE DEPT
770

Serial Number: *008837*
Test Date: *06/09/2026*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name: *Garner, Joel K*
Permit Number: *0036-5156*
Effective:
02/01/2026-02/01/2028

Officer's Name: *NONE, NONE*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG501308
Exp Date: 01/13/2027

Test	g/210L	Time
DIAG	Pass	10:12am
AIR BLK	.00	10:13am
ACCY CHK	.08	10:13am
AIR BLK	.00	10:15am
SUB TEST	**.00**	**10:15am**
AIR BLK	.00	10:16am
SUB TEST	**.00**	**10:18am**
AIR BLK	.00	10:19am

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

ROBESON COUNTY PEMBROKE POLICE DEPT 770

Serial Number: *008837* Test Record Number: *1390*
Test Date: *06/09/2026* Test Time: *10:19am EDT*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	10:20am
FLO	Pass	10:20am
FC	Pass	10:20am

Temperature Tests

Test	Status	Time
FC1	Pass	10:20am
SRC	Pass	10:20am
DET	Pass	10:20am
BAR	Pass	10:20am
BT	Pass	10:20am

Blank Tests

Test	Status	Time
AIR	Pass	10:21am

Printer Tests

Test	Status	Time
PRNT	Pass	10:21am

CRC Tests

Test	Status	Time
COMP	Pass	10:21am
CAL	Pass	10:21am

Preventive Maintenance
Status: Pass



Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Robeson Instrument Location Red Springs Police Department

Instrument Serial No. 008857

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

(1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;

(2) Verify instrument displays time and date;

(3) Initiate breath test sequence;

(4) Enter information as prompted;

(5) Verify instrument accuracy;

(6) When "PLEASE BLOW" appears, collect breath sample;

(7) When "PLEASE BLOW" appears, collect breath sample;

(8) Print test record;

(9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and

(10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 9 day of June, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.

Signature of Certifying Official

365156
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

DHHS 4080 (04/20)

Intox EC/IR-II: Subject Test

ROBESON COUNTY RED SPRINGS PD 770

Serial Number: *008857*
Test Date: *06/09/2026*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name: *Garner, Joel K*
Permit Number: *0036-5156*
Effective:
02/01/2026-02/01/2028

Officer's Name: *NONE, NONE*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG431002
Exp Date: 11/05/2026

Test	g/210L	Time
DIAG	Pass	9:21am
AIR BLK	.00	9:21am
ACCY CHK	.07	9:22am
AIR BLK	.00	9:23am
SUB TEST	**.00**	**9:24am**
AIR BLK	.00	9:25am
SUB TEST	**.00**	**9:26am**
AIR BLK	.00	9:28am

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

ROBESON COUNTY RED SPRINGS PD 770

Serial Number: *008857* Test Record Number: *868*
Test Date: *06/09/2026* Test Time: *9:28am EDT*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	9:29am
FLO	Pass	9:29am
FC	Pass	9:29am

Temperature Tests

Test	Status	Time
FC1	Pass	9:29am
SRC	Pass	9:29am
DET	Pass	9:29am
BAR	Pass	9:29am
BT	Pass	9:29am

Blank Tests

Test	Status	Time
AIR	Pass	9:30am

Printer Tests

Test	Status	Time
PRNT	Pass	9:30am

CRC Tests

Test	Status	Time
COMP	Pass	9:30am
CAL	Pass	9:30am

Preventive Maintenance
Status: Pass



Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Rockingham Instrument Location BAT Mobile Unit II

Instrument Serial No. 008970

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

(1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;

(2) Verify instrument displays time and date;

(3) Initiate breath test sequence;

(4) Enter information as prompted;

(5) Verify instrument accuracy;

(6) When "PLEASE BLOW" appears, collect breath sample;

(7) When "PLEASE BLOW" appears, collect breath sample;

(8) Print test record;

(9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and

(10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 1st day of June, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.

Jeff Tilley
Signature of Certifying Official

062446
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

DHHS 4080 (04/20)

Intox EC/IR-II: Subject Test

ROCKINGHAM COUNTY BAT MOBILE UNIT 11
780

Serial Number: *008970*
Test Date: *06/06/2026*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name: *Gillstrap, Jeffrey L*
Permit Number: *0006-2446*
Effective:
03/01/2026-03/01/2028

Officer's Name: *NONE, NONE*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG417802
Exp Date: 06/26/2026

Test	g/210L	Time
DIAG	Pass	10:24pm
AIR BLK	.00	10:25pm
ACCY CHK	.07	10:25pm
AIR BLK	.00	10:26pm
SUB TEST	**.00**	**10:27pm**
AIR BLK	.00	10:28pm
SUB TEST	**.00**	**10:29pm**
AIR BLK	.00	10:30pm

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

ROCKINGHAM COUNTY BAT MOBILE UNIT 11 780

Serial Number: *008970* Test Record Number: *1456*
Test Date: *06/06/2026* Test Time: *10:31pm EDT*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	10:31pm
FLO	Pass	10:31pm
FC	Pass	10:31pm

Temperature Tests

Test	Status	Time
FC1	Pass	10:31pm
SRC	Pass	10:31pm
DET	Pass	10:31pm
BAR	Pass	10:31pm
BT	Pass	10:31pm

Blank Tests

Test	Status	Time
AIR	Pass	10:32pm

Printer Tests

Test	Status	Time
PRNT	Pass	10:32pm

CRC Tests

Test	Status	Time
COMP	Pass	10:32pm
CAL	Pass	10:32pm

Preventive Maintenance
Status: Pass



Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Rockingham Instrument Location BAT Mobile Unit 11

Instrument Serial No. 008970

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

(1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;

(2) Verify instrument displays time and date;

(3) Initiate breath test sequence;

(4) Enter information as prompted;

(5) Verify instrument accuracy;

(6) When "PLEASE BLOW" appears, collect breath sample;

(7) When "PLEASE BLOW" appears, collect breath sample;

(8) Print test record;

(9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and

(10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 13th day of June, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.

Signature of Certifying Official

062446
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

DHHS 4080 (04/20)

Intox EC/IR-II: Subject Test

ROCKINGHAM COUNTY BAT MOBILE UNIT 11
780

Serial Number: *008970*
Test Date: *06/13/2026*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name: *Gillstrap, Jeffrey L*
Permit Number: *0006-2446*
Effective:
03/01/2026-03/01/2028

Officer's Name: *NONE, NONE*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG417802
Exp Date: 06/26/2026

Test	g/210L	Time
DIAG	Pass	3:00pm
AIR BLK	.00	3:01pm
ACCY CHK	.07	3:01pm
AIR BLK	.00	3:02pm
SUB TEST	**.00**	**3:03pm**
AIR BLK	.00	3:04pm
SUB TEST	**.00**	**3:05pm**
AIR BLK	.00	3:06pm

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

ROCKINGHAM COUNTY BAT MOBILE UNIT 11 780

Serial Number: *008970* Test Record Number: *1462*
Test Date: *06/13/2026* Test Time: *3:08pm EDT*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	3:08pm
FLO	Pass	3:08pm
FC	Pass	3:08pm

Temperature Tests

Test	Status	Time
FC1	Pass	3:08pm
SRC	Pass	3:08pm
DET	Pass	3:08pm
BAR	Pass	3:08pm
BT	Pass	3:08pm

Blank Tests

Test	Status	Time
AIR	Pass	3:09pm


Printer Tests

Test	Status	Time
PRNT	Pass	3:09pm

CRC Tests

Test	Status	Time
COMP	Pass	3:09pm
CAL	Pass	3:09pm

Preventive Maintenance
Status: Pass

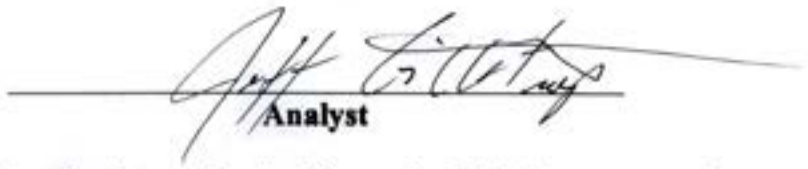

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD INTOXIMETERS, MODEL INTOX EC/IR II and MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Rockingham Instrument Location BAT Mobile Unit II

Instrument Serial No. 008973

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

(1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;

(2) Verify instrument displays time and date;

(3) Initiate breath test sequence;

(4) Enter information as prompted;

(5) Verify instrument accuracy;

(6) When "PLEASE BLOW" appears, collect breath sample;

(7) When "PLEASE BLOW" appears, collect breath sample;

(8) Print test record;

(9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and

(10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 6th day of June, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.

Signature of Certifying Official

062446
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

DHHS 4080 (04/20)

Intox EC/IR-II: Subject Test

ROCKINGHAM COUNTY BAT MOBILE UNIT 11
780

Serial Number: *008973*
Test Date: *06/06/2026*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name: *Gillstrap, Jeffrey L*
Permit Number: *0006-2446*
Effective:
03/01/2026-03/01/2028

Officer's Name: *NONE, NONE*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG431003
Exp Date: 11/05/2026

Test	g/210L	Time
DIAG	Pass	10:28pm
AIR BLK	.00	10:29pm
ACCY CHK	.07	10:30pm
AIR BLK	.00	10:31pm
SUB TEST	**.00**	**10:32pm**
AIR BLK	.00	10:33pm
SUB TEST	**.00**	**10:34pm**
AIR BLK	.00	10:35pm

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

ROCKINGHAM COUNTY BAT MOBILE UNIT 11 780

Serial Number: *008973* Test Record Number: *1496*
Test Date: *06/06/2026* Test Time: *10:35pm EDT*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	10:36pm
FLO	Pass	10:36pm
FC	Pass	10:36pm

Temperature Tests

Test	Status	Time
FC1	Pass	10:36pm
SRC	Pass	10:36pm
DET	Pass	10:36pm
BAR	Pass	10:36pm
BT	Pass	10:36pm

Blank Tests

Test	Status	Time
AIR	Pass	10:36pm

Printer Tests

Test	Status	Time
PRNT	Pass	10:36pm

CRC Tests

Test	Status	Time
COMP	Pass	10:37pm
CAL	Pass	10:37pm

Preventive Maintenance
Status: Pass



Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Rockingham Instrument Location BAT Mobile Unit II

Instrument Serial No. 008973

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

(1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;

(2) Verify instrument displays time and date;

(3) Initiate breath test sequence;

(4) Enter information as prompted;

(5) Verify instrument accuracy;

(6) When "PLEASE BLOW" appears, collect breath sample;

(7) When "PLEASE BLOW" appears, collect breath sample;

(8) Print test record;

(9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and

(10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 13th day of June, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.

Signature of Certifying Official

062446
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

DHHS 4080 (04/20)

Intox EC/IR-II: Subject Test

ROCKINGHAM COUNTY BAT MOBILE UNIT 11
780

Serial Number: *008973*
Test Date: *06/13/2026*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name: *Gillstrap, Jeffrey L*
Permit Number: *0006-2446*
Effective:
03/01/2026-03/01/2028

Officer's Name: *NONE, NONE*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG431003
Exp Date: 11/05/2026

Test	g/210L	Time
DIAG	Pass	2:56pm
AIR BLK	.00	2:57pm
ACCY CHK	.07	2:58pm
AIR BLK	.00	2:59pm
SUB TEST	**.00**	**2:59pm**
AIR BLK	.00	3:00pm
SUB TEST	**.00**	**3:02pm**
AIR BLK	.00	3:03pm

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

ROCKINGHAM COUNTY BAT MOBILE UNIT 11 780

Serial Number: *008973* Test Record Number: *1506*
Test Date: *06/13/2026* Test Time: *3:05pm EDT*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	3:06pm
FLO	Pass	3:06pm
FC	Pass	3:06pm

Temperature Tests

Test	Status	Time
FC1	Pass	3:06pm
SRC	Pass	3:06pm
DET	Pass	3:06pm
BAR	Pass	3:06pm
BT	Pass	3:06pm

Blank Tests

Test	Status	Time
AIR	Pass	3:06pm


Printer Tests

Test	Status	Time
PRNT	Pass	3:06pm

CRC Tests

Test	Status	Time
COMP	Pass	3:07pm
CAL	Pass	3:07pm

Preventive Maintenance
Status: Pass

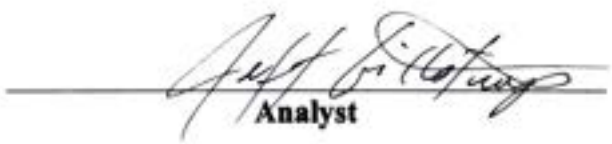

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Rutherford Instrument Location BAT Mobile Unit II

Instrument Serial No. 008970

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

(1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;

(2) Verify instrument displays time and date;

(3) Initiate breath test sequence;

(4) Enter information as prompted;

(5) Verify instrument accuracy;

(6) When "PLEASE BLOW" appears, collect breath sample;

(7) When "PLEASE BLOW" appears, collect breath sample;

(8) Print test record;

(9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and

(10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 5th day of June, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.

Jeff Gilbert
Signature of Certifying Official

062446
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

DHHS 4080 (04/20)

Intox EC/IR-II: Subject Test

RUTHERFORD COUNTY BAT MOBILE UNIT 11
800

Serial Number: *008970*
Test Date: *06/05/2026*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name: *Gillstrap, Jeffrey L*
Permit Number: *0006-2446*
Effective:
03/01/2026-03/01/2028

Officer's Name: *NONE, NONE*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG417802
Exp Date: 06/26/2026

Test	g/210L	Time
DIAG	Pass	8:15pm
AIR BLK	.00	8:16pm
ACCY CHK	.07	8:16pm
AIR BLK	.00	8:17pm
SUB TEST	**.00**	**8:18pm**
AIR BLK	.00	8:19pm
SUB TEST	**.00**	**8:20pm**
AIR BLK	.00	8:21pm

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

RUTHERFORD COUNTY BAT MOBILE UNIT 11 800

Serial Number: *008970* Test Record Number: *1451*
Test Date: *06/05/2026* Test Time: *8:22pm EDT*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	8:22pm
FLO	Pass	8:22pm
FC	Pass	8:22pm

Temperature Tests

Test	Status	Time
FC1	Pass	8:23pm
SRC	Pass	8:23pm
DET	Pass	8:23pm
BAR	Pass	8:23pm
BT	Pass	8:23pm

Blank Tests

Test	Status	Time
AIR	Pass	8:23pm


Printer Tests

Test	Status	Time
PRNT	Pass	8:23pm

CRC Tests

Test	Status	Time
COMP	Pass	8:23pm
CAL	Pass	8:23pm

Preventive Maintenance
Status: Pass

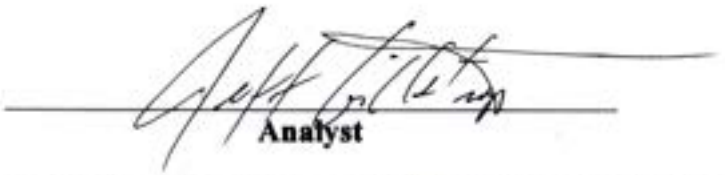

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Rutherford Instrument Location BAT Mobile Unit II

Instrument Serial No. 108973

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

(1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;

(2) Verify instrument displays time and date;

(3) Initiate breath test sequence;

(4) Enter information as prompted;

(5) Verify instrument accuracy;

(6) When "PLEASE BLOW" appears, collect breath sample;

(7) When "PLEASE BLOW" appears, collect breath sample;

(8) Print test record;

(9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and

(10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 5th day of June, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.

Signature of Certifying Official

062446
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

DHHS 4080 (04/20)

Intox EC/IR-II: Subject Test

RUTHERFORD COUNTY BAT MOBILE UNIT 11
800

Serial Number: *008973*
Test Date: *06/05/2026*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name: *Gillstrap, Jeffrey L*
Permit Number: *0006-2446*
Effective:
03/01/2026-03/01/2028

Officer's Name: *NONE, NONE*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG431003
Exp Date: 11/05/2026

Test	g/210L	Time
DIAG	Pass	8:40pm
AIR BLK	.00	8:40pm
ACCY CHK	.07	8:41pm
AIR BLK	.00	8:42pm
SUB TEST	**.00**	**8:43pm**
AIR BLK	.00	8:43pm
SUB TEST	**.00**	**8:45pm**
AIR BLK	.00	8:46pm

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

RUTHERFORD COUNTY BAT MOBILE UNIT 11 800

Serial Number: *008973* Test Record Number: *1492*
Test Date: *06/05/2026* Test Time: *8:47pm EDT*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	8:47pm
FLO	Pass	8:47pm
FC	Pass	8:47pm

Temperature Tests

Test	Status	Time
FC1	Pass	8:47pm
SRC	Pass	8:47pm
DET	Pass	8:47pm
BAR	Pass	8:47pm
BT	Pass	8:47pm

Blank Tests

Test	Status	Time
AIR	Pass	8:48pm

Printer Tests

Test	Status	Time
PRNT	Pass	8:48pm

CRC Tests

Test	Status	Time
COMP	Pass	8:48pm
CAL	Pass	8:48pm

Preventive Maintenance
Status: Pass



Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD INTOXIMETERS, MODEL INTOX EC/IR II and MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County: Stanly

Instrument Location: Locust PD
Locust, NC

Instrument Serial No. 088706

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

(1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;

(2) Verify instrument displays time and date;

(3) Initiate breath test sequence;

(4) Enter information as prompted;

(5) Verify instrument accuracy;

(6) When "PLEASE BLOW" appears, collect breath sample;

(7) When "PLEASE BLOW" appears, collect breath sample;

(8) Print test record;

(9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and

(10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 24th day of June, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.

Bryce Helms
Signature of Certifying Official

849845
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

STANLY COUNTY LOCUST PD 830

Serial Number: *008706*
Test Date: *06/24/2026*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name: *Helms, Bryce A*
Permit Number: *0084-9845*
Effective:
02/01/2026-02/01/2028

Officer's Name: *NONE, NONE*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG501303
Exp Date: 01/13/2027

Test	g/210L	Time
DIAG	Pass	1:00pm
AIR BLK	.00	1:00pm
ACCY CHK	.07	1:01pm
AIR BLK	.00	1:02pm
SUB TEST	**.00**	**1:03pm**
AIR BLK	.00	1:04pm
SUB TEST	**.00**	**1:05pm**
AIR BLK	.00	1:06pm

Reported AC: .00 g/210L

Bryce Helms
Signature of Chemical Analyst

Court CVR

Bryce Helms
Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

STANLY COUNTY LOCUST PD 830

Serial Number: *008706* Test Record Number: *3928*
Test Date: *06/24/2026* Test Time: *1:06pm EDT*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	1:07pm
FLO	Pass	1:07pm
FC	Pass	1:07pm

Temperature Tests

Test	Status	Time
FC1	Pass	1:07pm
SRC	Pass	1:07pm
DET	Pass	1:07pm
BAR	Pass	1:07pm
BT	Pass	1:07pm

Blank Tests

Test	Status	Time
AIR	Pass	1:08pm


Printer Tests

Test	Status	Time
PRNT	Pass	1:08pm

CRC Tests

Test	Status	Time
COMP	Pass	1:08pm
CAL	Pass	1:08pm

Preventive Maintenance
Status: Pass

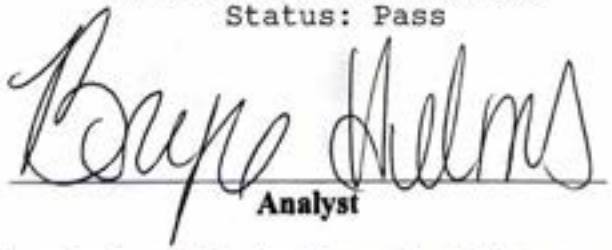

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Swain Instrument Location Cherokee Tribal Def.

Instrument Serial No. 008782 Cherokee, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

(1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;

(2) Verify instrument displays time and date;

(3) Initiate breath test sequence;

(4) Enter information as prompted;

(5) Verify instrument accuracy;

(6) When "PLEASE BLOW" appears, collect breath sample;

(7) When "PLEASE BLOW" appears, collect breath sample;

(8) Print test record;

(9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and

(10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 4th day of June, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.

David R. Cathey
Signature of Certifying Official

843310
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

DHHS 4080 (04/20)

Intox EC/IR-II: Subject Test

SWAIN COUNTY CHEROKEE DETENTION 860

Serial Number: *008782*
Test Date: *06/04/2026*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name: *Cutler, Daniel R*
Permit Number: *0084-3310*
Effective:
02/01/2026-02/01/2028

Officer's Name: *NONE, NONE*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG505001
Exp Date: 02/19/2027

Test	g/210L	Time
DIAG	Pass	10:03am
AIR BLK	.00	10:04am
ACCY CHK	.07	10:05am
AIR BLK	.00	10:06am
SUB TEST	**.00**	**10:07am**
AIR BLK	.00	10:07am
SUB TEST	**.00**	**10:09am**
AIR BLK	.00	10:10am

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

SWAIN COUNTY CHEROKEE DETENTION 860

Serial Number: *008782* Test Record Number: *1660*
Test Date: *06/04/2026* Test Time: *10:10am EDT*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	10:11am
FLO	Pass	10:11am
FC	Pass	10:11am

Temperature Tests

Test	Status	Time
FC1	Pass	10:11am
SRC	Pass	10:11am
DET	Pass	10:11am
BAR	Pass	10:11am
BT	Pass	10:11am

Blank Tests

Test	Status	Time
AIR	Pass	10:12am

Printer Tests

Test	Status	Time
PRNT	Pass	10:12am

CRC Tests

Test	Status	Time
COMP	Pass	10:12am
CAL	Pass	10:12am

Preventive Maintenance
Status: Pass

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD INTOXIMETERS, MODEL INTOX EC/IR II and MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Union Instrument Location Waxhaw PD

Instrument Serial No. 008598 Waxhaw, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

(1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;

(2) Verify instrument displays time and date;

(3) Initiate breath test sequence;

(4) Enter information as prompted;

(5) Verify instrument accuracy;

(6) When "PLEASE BLOW" appears, collect breath sample;

(7) When "PLEASE BLOW" appears, collect breath sample;

(8) Print test record;

(9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and

(10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 22nd day of June, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.

Signature of Certifying Official

849845
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

DHHS 4080 (04/20)

Intox EC/IR-II: Subject Test

UNION COUNTY WAXHAW PD 890

Serial Number: *008598*
Test Date: *06/22/2026*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name: *Helms, Bryce A*
Permit Number: *0084-9845*
Effective:
02/01/2026-02/01/2028

Officer's Name: *NONE, NONE*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG501303
Exp Date: 01/13/2027

Test	g/210L	Time
DIAG	Pass	12:42pm
AIR BLK	.00	12:42pm
ACCY CHK	.07	12:43pm
AIR BLK	.00	12:44pm
SUB TEST	**.00**	**12:45pm**
AIR BLK	.00	12:46pm
SUB TEST	**.00**	**12:48pm**
AIR BLK	.00	12:48pm

Reported AC: .00 g/210L

Bryce Helms
Signature of Chemical Analyst

Court CVR

Bryce Helms
Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

UNION COUNTY WAXHAW PD 890

Serial Number: *008598* Test Record Number: *1200*
Test Date: *06/22/2026* Test Time: *12:49pm EDT*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	12:49pm
FLO	Pass	12:49pm
FC	Pass	12:49pm

Temperature Tests

Test	Status	Time
FC1	Pass	12:49pm
SRC	Pass	12:49pm
DET	Pass	12:49pm
BAR	Pass	12:49pm
BT	Pass	12:49pm

Blank Tests

Test	Status	Time
AIR	Pass	12:50pm


Printer Tests

Test	Status	Time
PRNT	Pass	12:50pm

CRC Tests

Test	Status	Time
COMP	Pass	12:50pm
CAL	Pass	12:50pm

Preventive Maintenance
Status: Pass

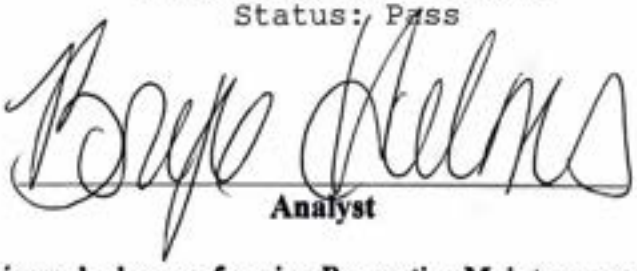

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Union Instrument Location BAT Mobile Unit 8

Instrument Serial No. 008615 —

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

(1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;

(2) Verify instrument displays time and date;

(3) Initiate breath test sequence;

(4) Enter information as prompted;

(5) Verify instrument accuracy;

(6) When "PLEASE BLOW" appears, collect breath sample;

(7) When "PLEASE BLOW" appears, collect breath sample;

(8) Print test record;

(9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and

(10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 25 day of June, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.

Signature of Certifying Official

2219283
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years

DHHS 4080 (04/20)

Intox EC/IR-II: Subject Test

UNION COUNTY BAT MOBILE UNIT 8 890

Serial Number: *008615*
Test Date: *06/25/2026*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name: *Glasscock, Jerry D*
Permit Number: *7180-9235*
Effective:
02/01/2026-02/01/2028

Officer's Name: *NONE, NONE*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG506303
Exp Date: 03/04/2027

Test	g/210L	Time
DIAG	Pass	9:51am
AIR BLK	.00	9:52am
ACCY CHK	.07	9:52am
AIR BLK	.00	9:53am
SUB TEST	**.00**	**9:54am**
AIR BLK	.00	9:55am
SUB TEST	**.00**	**9:56am**
AIR BLK	.00	9:57am

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

UNION COUNTY BAT MOBILE UNIT 8 890

Serial Number: *008615* Test Record Number: *6349*
Test Date: *06/25/2026* Test Time: *9:58am EDT*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	9:58am
FLO	Pass	9:58am
FC	Pass	9:58am

Temperature Tests

Test	Status	Time
FC1	Pass	9:58am
SRC	Pass	9:58am
DET	Pass	9:58am
BAR	Pass	9:58am
BT	Pass	9:58am

Blank Tests

Test	Status	Time
AIR	Pass	9:59am

Printer Tests

Test	Status	Time
PRNT	Pass	9:59am

CRC Tests

Test	Status	Time
COMP	Pass	9:59am
CAL	Pass	9:59am

Preventive Maintenance
Status: Pass

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Union Instrument Location BAT Mobile Unit 8

Instrument Serial No. 008736 —

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

(1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;

(2) Verify instrument displays time and date;

(3) Initiate breath test sequence;

(4) Enter information as prompted;

(5) Verify instrument accuracy;

(6) When "PLEASE BLOW" appears, collect breath sample;

(7) When "PLEASE BLOW" appears, collect breath sample;

(8) Print test record;

(9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and

(10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 25 day of June, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.

Signature of Certifying Official 2219283 Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

DHHS 4080 (04/20)

UNION COUNTY BAT MOBILE UNIT 8 890

Serial Number: *008736*
Test Date: *06/25/2026*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name: *Glasscock, Jerry D*
Permit Number: *7180-9235*
Effective:
02/01/2026-02/01/2028

Officer's Name: *NONE, NONE*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG506303
Exp Date: 03/04/2027

Test	g/210L	Time
DIAG	Pass	9:49am
AIR BLK	.00	9:50am
ACCY CHK	.07	9:51am
AIR BLK	.00	9:52am
SUB TEST	**.00**	**9:53am**
AIR BLK	.00	9:53am
SUB TEST	**.00**	**9:55am**
AIR BLK	.00	9:56am

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

UNION COUNTY BAT MOBILE UNIT 8 890

Serial Number: *008736* Test Record Number: *1704*
Test Date: *06/25/2026* Test Time: *9:58am EDT*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	9:58am
FLO	Pass	9:58am
FC	Pass	9:58am

Temperature Tests

Test	Status	Time
FC1	Pass	9:58am
SRC	Pass	9:58am
DET	Pass	9:58am
BAR	Pass	9:58am
BT	Pass	9:58am

Blank Tests

Test	Status	Time
AIR	Pass	9:59am

Printer Tests

Test	Status	Time
PRNT	Pass	9:59am

CRC Tests

Test	Status	Time
COMP	Pass	9:59am
CAL	Pass	9:59am

Preventive Maintenance
Status: Pass

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Union Instrument Location BAT Mobile Unit 8

Instrument Serial No. 008775 —

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

(1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;

(2) Verify instrument displays time and date;

(3) Initiate breath test sequence;

(4) Enter information as prompted;

(5) Verify instrument accuracy;

(6) When "PLEASE BLOW" appears, collect breath sample;

(7) When "PLEASE BLOW" appears, collect breath sample;

(8) Print test record;

(9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and

(10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 25 day of June, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.

Signature of Certifying Official

2219283
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

UNION COUNTY BAT MOBILE UNIT 8 890

Serial Number: *008775*
Test Date: *06/25/2026*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name: *Glasscock, Jerry D*
Permit Number: *7180-9235*
Effective:
02/01/2026-02/01/2028

Officer's Name: *NONE, NONE*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG506303
Exp Date: 03/04/2027

Test	g/210L	Time
DIAG	Pass	9:49am
AIR BLK	.00	9:50am
ACCY CHK	.08	9:51am
AIR BLK	.00	9:52am
SUB TEST	**.00**	**9:52am**
AIR BLK	.00	9:53am
SUB TEST	**.00**	**9:55am**
AIR BLK	.00	9:56am

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

UNION COUNTY BAT MOBILE UNIT 8 890

Serial Number: *008775* Test Record Number: *2562*
Test Date: *06/25/2026* Test Time: *9:57am EDT*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	9:57am
FLO	Pass	9:57am
FC	Pass	9:57am

Temperature Tests

Test	Status	Time
FC1	Pass	9:57am
SRC	Pass	9:57am
DET	Pass	9:57am
BAR	Pass	9:57am
BT	Pass	9:57am

Blank Tests

Test	Status	Time
AIR	Pass	9:58am

Printer Tests

Test	Status	Time
PRNT	Pass	9:58am

CRC Tests

Test	Status	Time
COMP	Pass	9:58am
CAL	Pass	9:58am

Preventive Maintenance
Status: Pass

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Union Instrument Location BAT Mobile Unit 8

Instrument Serial No. 008816 —

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

(1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;

(2) Verify instrument displays time and date;

(3) Initiate breath test sequence;

(4) Enter information as prompted;

(5) Verify instrument accuracy;

(6) When "PLEASE BLOW" appears, collect breath sample;

(7) When "PLEASE BLOW" appears, collect breath sample;

(8) Print test record;

(9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and

(10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 25 day of June, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.

THE GREAT SEAL OF THE STATE OF NORTH CAROLINA

Signature of Certifying Official

2219283
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years

DHHS 4080 (04/20)

Intox EC/IR-II: Subject Test

UNION COUNTY BAT MOBILE UNIT 8 890

Serial Number: *008816*
Test Date: *06/25/2026*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name: *Glasscock, Jerry D*
Permit Number: *7180-9235*
Effective:
02/01/2026-02/01/2028

Officer's Name: *NONE, NONE*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG431002
Exp Date: 11/05/2026

Test	g/210L	Time
DIAG	Pass	9:49am
AIR BLK	.00	9:50am
ACCY CHK	.07	9:50am
AIR BLK	.00	9:52am
SUB TEST	**.00**	**9:53am**
AIR BLK	.00	9:53am
SUB TEST	**.00**	**9:55am**
AIR BLK	.00	9:56am

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

UNION COUNTY BAT MOBILE UNIT 8 890

Serial Number: *008816* Test Record Number: *8134*
Test Date: *06/25/2026* Test Time: *9:57am EDT*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	9:57am
FLO	Pass	9:57am
FC	Pass	9:57am

Temperature Tests

Test	Status	Time
FC1	Pass	9:57am
SRC	Pass	9:57am
DET	Pass	9:57am
BAR	Pass	9:57am
BT	Pass	9:57am

Blank Tests

Test	Status	Time
AIR	Pass	9:58am

Printer Tests

Test	Status	Time
PRNT	Pass	9:58am

CRC Tests

Test	Status	Time
COMP	Pass	9:58am
CAL	Pass	9:58am

Preventive Maintenance
Status: Pass

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Union Instrument Location BAT Mobile Unit 8

Instrument Serial No. 008929 –

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

(1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;

(2) Verify instrument displays time and date;

(3) Initiate breath test sequence;

(4) Enter information as prompted;

(5) Verify instrument accuracy;

(6) When "PLEASE BLOW" appears, collect breath sample;

(7) When "PLEASE BLOW" appears, collect breath sample;

(8) Print test record;

(9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and

(10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 25 day of June, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.

Signature of Certifying Official 2219283 Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

DHHS 4080 (04/20)

Intox EC/IR-II: Subject Test

UNION COUNTY BAT MOBILE UNIT 8 890

Serial Number: *008929*
Test Date: *06/25/2026*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name: *Glasscock, Jerry D*
Permit Number: *7180-9235*
Effective:
02/01/2026-02/01/2028

Officer's Name: *NONE, NONE*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG506303
Exp Date: 03/04/2027

Test	g/210L	Time
DIAG	Pass	9:48am
AIR BLK	.00	9:49am
ACCY CHK	.08	9:50am
AIR BLK	.00	9:51am
SUB TEST	**.00**	**9:52am**
AIR BLK	.00	9:53am
SUB TEST	**.00**	**9:54am**
AIR BLK	.00	9:55am

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

UNION COUNTY BAT MOBILE UNIT 8 890

Serial Number: *008929* Test Record Number: *1843*
Test Date: *06/25/2026* Test Time: *9:56am EDT*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	9:56am
FLO	Pass	9:56am
FC	Pass	9:57am

Temperature Tests

Test	Status	Time
FC1	Pass	9:57am
SRC	Pass	9:57am
DET	Pass	9:57am
BAR	Pass	9:57am
BT	Pass	9:57am

Blank Tests

Test	Status	Time
AIR	Pass	9:58am

Printer Tests

Test	Status	Time
PRNT	Pass	9:58am

CRC Tests

Test	Status	Time
COMP	Pass	9:58am
CAL	Pass	9:58am

Preventive Maintenance
Status: Pass

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Wake Instrument Location BAT Mobile Unit 7

Instrument Serial No. 008002

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

(1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;

(2) Verify instrument displays time and date;

(3) Initiate breath test sequence;

(4) Enter information as prompted;

(5) Verify instrument accuracy;

(6) When "PLEASE BLOW" appears, collect breath sample;

(7) When "PLEASE BLOW" appears, collect breath sample;

(8) Print test record;

(9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and

(10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 12 day of June, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.

Signature of Certifying Official

193759
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

DHHS 4080 (04/20)

Intox EC/IR-II: Subject Test

WAKE COUNTY BAT MOBILE UNIT 7 910

Serial Number: *008002*
Test Date: *06/12/2026*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name: *Carroll, Barry Jean D*
Permit Number: *0019-3759*
Effective:
04/01/2026-04/01/2028

Officer's Name: *NONE, NONE*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG506303
Exp Date: 03/04/2027

Test	g/210L	Time
DIAG	Pass	9:03pm
AIR BLK	.00	9:04pm
ACCY CHK	.08	9:05pm
AIR BLK	.00	9:06pm
SUB TEST	**.00**	**9:06pm**
AIR BLK	.00	9:07pm
SUB TEST	**.00**	**9:09pm**
AIR BLK	.00	9:10pm

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

WAKE COUNTY BAT MOBILE UNIT 7 910

Serial Number: *008002* Test Record Number: *920*
Test Date: *06/12/2026* Test Time: *9:12pm EDT*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	9:12pm
FLO	Pass	9:12pm
FC	Pass	9:12pm

Temperature Tests

Test	Status	Time
FC1	Pass	9:12pm
SRC	Pass	9:12pm
DET	Pass	9:12pm
BAR	Pass	9:12pm
BT	Pass	9:12pm

Blank Tests

Test	Status	Time
AIR	Pass	9:13pm


Printer Tests

Test	Status	Time
PRNT	Pass	9:13pm

CRC Tests

Test	Status	Time
COMP	Pass	9:13pm
CAL	Pass	9:13pm

Preventive Maintenance
Status: Pass

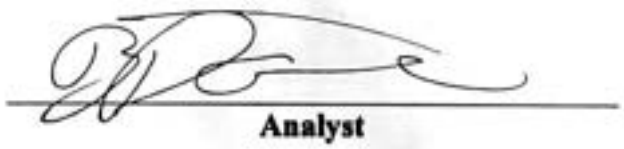

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Wake Instrument Location BAT Mobile Unit 7

Instrument Serial No. 008090

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

(1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;

(2) Verify instrument displays time and date;

(3) Initiate breath test sequence;

(4) Enter information as prompted;

(5) Verify instrument accuracy;

(6) When "PLEASE BLOW" appears, collect breath sample;

(7) When "PLEASE BLOW" appears, collect breath sample;

(8) Print test record;

(9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and

(10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 12 day of June, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.

Signature of Certifying Official

197759
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

DHHS 4080 (04/20)

Intox EC/IR-II: Subject Test

WAKE COUNTY BAT MOBILE UNIT 7 910

Serial Number: *008090*
Test Date: *06/12/2026*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name: *Carroll, Barry Jean D*
Permit Number: *0019-3759*
Effective:
04/01/2026-04/01/2028

Officer's Name: *NONE, NONE*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG602101
Exp Date: 01/21/2028

Test	g/210L	Time
DIAG	Pass	10:25pm
AIR BLK	.00	10:26pm
ACCY CHK	.07	10:27pm
AIR BLK	.00	10:28pm
SUB TEST	**.00**	**10:28pm**
AIR BLK	.00	10:29pm
SUB TEST	**.00**	**10:31pm**
AIR BLK	.00	10:31pm

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

WAKE COUNTY BAT MOBILE UNIT 7 910

Serial Number: *008090* Test Record Number: *280*
Test Date: *06/12/2026* Test Time: *10:32pm EDT*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	10:32pm
FLO	Pass	10:32pm
FC	Pass	10:32pm

Temperature Tests

Test	Status	Time
FC1	Pass	10:32pm
SRC	Pass	10:32pm
DET	Pass	10:32pm
BAR	Pass	10:32pm
BT	Pass	10:32pm

Blank Tests

Test	Status	Time
AIR	Pass	10:33pm

Printer Tests

Test	Status	Time
PRNT	Pass	10:33pm

CRC Tests

Test	Status	Time
COMP	Pass	10:33pm
CAL	Pass	10:33pm

Preventive Maintenance
Status: Pass



Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Wake Instrument Location BAT Mobile Unit 10

Instrument Serial No. 008584

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

(1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;

(2) Verify instrument displays time and date;

(3) Initiate breath test sequence;

(4) Enter information as prompted;

(5) Verify instrument accuracy;

(6) When "PLEASE BLOW" appears, collect breath sample;

(7) When "PLEASE BLOW" appears, collect breath sample;

(8) Print test record;

(9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and

(10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 26 day of June, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.

Signature of Certifying Official

193759
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

DHHS 4080 (04/20)

Intox EC/IR-II: Subject Test

WAKE COUNTY BAT MOBILE UNIT 10 910

Serial Number: *008584*
Test Date: *06/26/2026*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name: *Carroll, Barry Jean D*
Permit Number: *0019-3759*
Effective:
04/01/2026-04/01/2028

Officer's Name: *NONE, NONE*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG534301
Exp Date: 12/09/2027

Test	g/210L	Time
DIAG	Pass	8:49pm
AIR BLK	.00	8:50pm
ACCY CHK	.08	8:51pm
AIR BLK	.00	8:52pm
SUB TEST	**.00**	**8:53pm**
AIR BLK	.00	8:54pm
SUB TEST	**.00**	**8:55pm**
AIR BLK	.00	8:56pm

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

WAKE COUNTY BAT MOBILE UNIT 10 910

Serial Number: *008584* Test Record Number: *2912*
Test Date: *06/26/2026* Test Time: *8:57pm EDT*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	8:57pm
FLO	Pass	8:57pm
FC	Pass	8:57pm

Temperature Tests

Test	Status	Time
FC1	Pass	8:57pm
SRC	Pass	8:57pm
DET	Pass	8:57pm
BAR	Pass	8:57pm
BT	Pass	8:57pm

Blank Tests

Test	Status	Time
AIR	Pass	8:58pm

Printer Tests

Test	Status	Time
PRNT	Pass	8:58pm

CRC Tests

Test	Status	Time
COMP	Pass	8:58pm
CAL	Pass	8:58pm

Preventive Maintenance
Status: Pass



Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD INTOXIMETERS, MODEL INTOX EC/IR II and MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Wake Instrument Location Cary PD

Instrument Serial No. 008587 120 Wilkenson Ave.

Cary, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

(1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;

(2) Verify instrument displays time and date;

(3) Initiate breath test sequence;

(4) Enter information as prompted;

(5) Verify instrument accuracy;

(6) When "PLEASE BLOW" appears, collect breath sample;

(7) When "PLEASE BLOW" appears, collect breath sample;

(8) Print test record;

(9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and

(10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 23 day of June, 20 26 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.

Bryant L [illegible]
Signature of Certifying Official

169451
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

DHHS 4080 (04/20)

Intox EC/IR-II: Subject Test

WAKE COUNTY CARY PD 910

Serial Number: *008587*
Test Date: *06/23/2026*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name: *Brame, Bryant T*
Permit Number: *0016-9451*
Effective:
04/01/2026-04/01/2028

Officer's Name: *NONE, NONE*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG506303
Exp Date: 03/04/2027

Test	g/210L	Time
DIAG	Pass	1:57pm
AIR BLK	.00	1:57pm
ACCY CHK	.07	1:58pm
AIR BLK	.00	1:59pm
SUB TEST	**.00**	**2:00pm**
AIR BLK	.00	2:01pm
SUB TEST	**.00**	**2:02pm**
AIR BLK	.00	2:03pm

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

WAKE COUNTY CARY PD 910

Serial Number: *008587* Test Record Number: *5686*
Test Date: *06/23/2026* Test Time: *2:04pm EDT*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	2:04pm
FLO	Pass	2:04pm
FC	Pass	2:04pm

Temperature Tests

Test	Status	Time
FC1	Pass	2:04pm
SRC	Pass	2:04pm
DET	Pass	2:04pm
BAR	Pass	2:04pm
BT	Pass	2:04pm

Blank Tests

Test	Status	Time
AIR	Pass	2:05pm


Printer Tests

Test	Status	Time
PRNT	Pass	2:05pm

CRC Tests

Test	Status	Time
COMP	Pass	2:05pm
CAL	Pass	2:05pm

Preventive Maintenance
Status: Pass



Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD INTOXIMETERS, MODEL INTOX EC/IR II and MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County WAKE Instrument Location BAT Mobile Unit 12

Instrument Serial No. 008601

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

(1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;

(2) Verify instrument displays time and date;

(3) Initiate breath test sequence;

(4) Enter information as prompted;

(5) Verify instrument accuracy;

(6) When "PLEASE BLOW" appears, collect breath sample;

(7) When "PLEASE BLOW" appears, collect breath sample;

(8) Print test record;

(9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and

(10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 26 day of June, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.

Signature of Certifying Official

83034
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

DHHS 4080 (04/20)

Intox EC/IR-II: Subject Test

WAKE COUNTY BAT MOBILE UNIT 12 910

Serial Number: *008601*
Test Date: *06/26/2026*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name:
Crutchfield Jr., Marshall B
Permit Number: *0008-3034*
Effective:
03/01/2026-03/01/2028

Officer's Name: *NONE, NONE*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG501307
Exp Date: 01/13/2027

Test	g/210L	Time
DIAG	Pass	8:33pm
AIR BLK	.00	8:34pm
ACCY CHK	.07	8:35pm
AIR BLK	.00	8:36pm
SUB TEST	**.00**	**8:37pm**
AIR BLK	.00	8:38pm
SUB TEST	**.00**	**8:39pm**
AIR BLK	.00	8:40pm

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

WAKE COUNTY BAT MOBILE UNIT 12 910

Serial Number: *008601* Test Record Number: *1954*
Test Date: *06/26/2026* Test Time: *8:41pm EDT*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	8:42pm
FLO	Pass	8:42pm
FC	Pass	8:42pm

Temperature Tests

Test	Status	Time
FC1	Pass	8:42pm
SRC	Pass	8:42pm
DET	Pass	8:42pm
BAR	Pass	8:42pm
BT	Pass	8:42pm

Blank Tests

Test	Status	Time
AIR	Pass	8:43pm

Printer Tests

Test	Status	Time
PRNT	Pass	8:43pm

CRC Tests

Test	Status	Time
COMP	Pass	8:43pm
CAL	Pass	8:43pm

Preventive Maintenance
Status: Pass



Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD INTOXIMETERS, MODEL INTOX EC/IR II and MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Wake Instrument Location Raleigh PD Southwest Dist.

Instrument Serial No. 008612 601 Hutton St.

Raleigh, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

(1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;

(2) Verify instrument displays time and date;

(3) Initiate breath test sequence;

(4) Enter information as prompted;

(5) Verify instrument accuracy;

(6) When "PLEASE BLOW" appears, collect breath sample;

(7) When "PLEASE BLOW" appears, collect breath sample;

(8) Print test record;

(9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and

(10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 24 day of June, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.

Signature of Certifying Official

169451
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

DHHS 4080 (04/20)

Intox EC/IR-II: Subject Test

WAKE COUNTY SOUTH WEST DISTRICT 910

Serial Number: *008612*
Test Date: *06/24/2026*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name: *Brame, Bryant T*
Permit Number: *0016-9451*
Effective:
04/01/2026-04/01/2028

Officer's Name: *NONE, NONE*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG516203
Exp Date: 06/11/2027

Test	g/210L	Time
DIAG	Pass	11:32am
AIR BLK	.00	11:32am
ACCY CHK	.07	11:33am
AIR BLK	.00	11:34am
SUB TEST	**.00**	**11:35am**
AIR BLK	.00	11:36am
SUB TEST	**.00**	**11:37am**
AIR BLK	.00	11:38am

Reported **AC: .00 g/210L**

Signature of Chemical Analyst

Court CVR

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

WAKE COUNTY SOUTH WEST DISTRICT 910

Serial Number: *008612* Test Record Number: *5500*
Test Date: *06/24/2026* Test Time: *11:39am EDT*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	11:39am
FLO	Pass	11:39am
FC	Pass	11:39am

Temperature Tests

Test	Status	Time
FC1	Pass	11:39am
SRC	Pass	11:39am
DET	Pass	11:39am
BAR	Pass	11:39am
BT	Pass	11:39am

Blank Tests

Test	Status	Time
AIR	Pass	11:40am

Printer Tests

Test	Status	Time
PRNT	Pass	11:40am

CRC Tests

Test	Status	Time
COMP	Pass	11:40am
CAL	Pass	11:40am

Preventive Maintenance
Status: Pass

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County WAKE Instrument Location Apex PD Substation 4

Instrument Serial No. 008621 1615 E. Williams ST.

Apex, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

(1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;

(2) Verify instrument displays time and date;

(3) Initiate breath test sequence;

(4) Enter information as prompted;

(5) Verify instrument accuracy;

(6) When "PLEASE BLOW" appears, collect breath sample;

(7) When "PLEASE BLOW" appears, collect breath sample;

(8) Print test record;

(9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and

(10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 23 day of June, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.

Signature of Certifying Official

16945I
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

DHHS 4080 (04/20)

Intox EC/IR-II: Subject Test

WAKE COUNTY APEX PD 910

Serial Number: *008621*
Test Date: *06/23/2026*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name: *Brame, Bryant T*
Permit Number: *0016-9451*
Effective:
04/01/2026-04/01/2028

Officer's Name: *NONE, NONE*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG431003
Exp Date: 11/05/2026

Test	g/210L	Time
DIAG	Pass	11:16am
AIR BLK	.00	11:17am
ACCY CHK	.07	11:18am
AIR BLK	.00	11:19am
SUB TEST	**.00**	**11:19am**
AIR BLK	.00	11:20am
SUB TEST	**.00**	**11:22am**
AIR BLK	.00	11:22am

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

WAKE COUNTY APEX PD 910

Serial Number: *008621* Test Record Number: *3839*
Test Date: *06/23/2026* Test Time: *11:23am EDT*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	11:23am
FLO	Pass	11:23am
FC	Pass	11:23am

Temperature Tests

Test	Status	Time
FC1	Pass	11:24am
SRC	Pass	11:24am
DET	Pass	11:24am
BAR	Pass	11:24am
BT	Pass	11:24am

Blank Tests

Test	Status	Time
AIR	Pass	11:24am

Printer Tests

Test	Status	Time
PRNT	Pass	11:24am

CRC Tests

Test	Status	Time
COMP	Pass	11:24am
CAL	Pass	11:24am

Preventive Maintenance
Status: Pass

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Wake Instrument Location BAT Mobile Unit 10

Instrument Serial No. 008686

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

(1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;

(2) Verify instrument displays time and date;

(3) Initiate breath test sequence;

(4) Enter information as prompted;

(5) Verify instrument accuracy;

(6) When "PLEASE BLOW" appears, collect breath sample;

(7) When "PLEASE BLOW" appears, collect breath sample;

(8) Print test record;

(9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and

(10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 26 day of June, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.

Signature of Certifying Official

193759
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

DHHS 4080 (04/20)

Intox EC/IR-II: Subject Test

WAKE COUNTY BAT MOBILE UNIT 10 910

Serial Number: *008686*
Test Date: *06/26/2026*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name: *Carroll, Barry Jean D*
Permit Number: *0019-3759*
Effective:
04/01/2026-04/01/2028

Officer's Name: *NONE, NONE*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG506302
Exp Date: 03/04/2027

Test	g/210L	Time
DIAG	Pass	8:52pm
AIR BLK	.00	8:53pm
ACCY CHK	.08	8:54pm
AIR BLK	.00	8:55pm
SUB TEST	**.00**	**8:55pm**
AIR BLK	.00	8:56pm
SUB TEST	**.00**	**8:58pm**
AIR BLK	.00	8:59pm

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

WAKE COUNTY BAT MOBILE UNIT 10 910

Serial Number: *008686* Test Record Number: *7260*
Test Date: *06/26/2026* Test Time: *8:59pm EDT*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	9:00pm
FLO	Pass	9:00pm
FC	Pass	9:00pm

Temperature Tests

Test	Status	Time
FC1	Pass	9:00pm
SRC	Pass	9:00pm
DET	Pass	9:00pm
BAR	Pass	9:00pm
BT	Pass	9:00pm

Blank Tests

Test	Status	Time
AIR	Pass	9:00pm


Printer Tests

Test	Status	Time
PRNT	Pass	9:00pm

CRC Tests

Test	Status	Time
COMP	Pass	9:01pm
CAL	Pass	9:01pm

Preventive Maintenance
Status: Pass

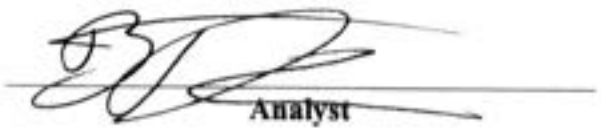

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County WAKE Instrument Location BAT Mobile Unit 12

Instrument Serial No. 008698

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

(1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;

(2) Verify instrument displays time and date;

(3) Initiate breath test sequence;

(4) Enter information as prompted;

(5) Verify instrument accuracy;

(6) When "PLEASE BLOW" appears, collect breath sample;

(7) When "PLEASE BLOW" appears, collect breath sample;

(8) Print test record;

(9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and

(10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 26th day of June, 20 26 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.

Signature of Certifying Official

83034
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

WAKE COUNTY BAT MOBILE UNIT 12 910

Serial Number: *008698*
Test Date: *06/26/2026*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name:
Crutchfield Jr., Marshall B
Permit Number: *0008-3034*
Effective:
03/01/2026-03/01/2028

Officer's Name: *NONE, NONE*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG431002
Exp Date: 11/05/2026

Test	g/210L	Time
DIAG	Pass	8:35pm
AIR BLK	.00	8:36pm
ACCY CHK	.08	8:36pm
AIR BLK	.00	8:37pm
SUB TEST	**.00**	**8:38pm**
AIR BLK	.00	8:39pm
SUB TEST	**.00**	**8:40pm**
AIR BLK	.00	8:41pm

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

WAKE COUNTY BAT MOBILE UNIT 12 910

Serial Number: *008698* Test Record Number: *2786*
Test Date: *06/26/2026* Test Time: *8:42pm EDT*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	8:42pm
FLO	Pass	8:42pm
FC	Pass	8:42pm

Temperature Tests

Test	Status	Time
FC1	Pass	8:42pm
SRC	Pass	8:42pm
DET	Pass	8:42pm
BAR	Pass	8:42pm
BT	Pass	8:42pm

Blank Tests

Test	Status	Time
AIR	Pass	8:43pm

Printer Tests

Test	Status	Time
PRNT	Pass	8:43pm

CRC Tests

Test	Status	Time
COMP	Pass	8:43pm
CAL	Pass	8:43pm

Preventive Maintenance
Status: Pass



Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Wake Instrument Location Holly Springs PD

Instrument Serial No. 008757 750 Holly Springs Rd

Holly Springs, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

(1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;

(2) Verify instrument displays time and date;

(3) Initiate breath test sequence;

(4) Enter information as prompted;

(5) Verify instrument accuracy;

(6) When "PLEASE BLOW" appears, collect breath sample;

(7) When "PLEASE BLOW" appears, collect breath sample;

(8) Print test record;

(9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and

(10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 23 day of June, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.

Signature of Certifying Official

16 9451
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

DHHS 4080 (04/20)

Intox EC/IR-II: Subject Test

WAKE COUNTY HOLLY SPRINGS PD 910

Serial Number: *008757*
Test Date: *06/23/2026*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name: *Brame, Bryant T*
Permit Number: *0016-9451*
Effective:
04/01/2026-04/01/2028

Officer's Name: *NONE, NONE*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG516203
Exp Date: 06/11/2027

Test	g/210L	Time
DIAG	Pass	10:02am
AIR BLK	.00	10:03am
ACCY CHK	.08	10:04am
AIR BLK	.00	10:05am
SUB TEST	**.00**	**10:05am**
AIR BLK	.00	10:06am
SUB TEST	**.00**	**10:08am**
AIR BLK	.00	10:08am

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

WAKE COUNTY HOLLY SPRINGS PD 910

Serial Number: *008757* Test Record Number: *3042*
Test Date: *06/23/2026* Test Time: *10:09am EDT*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	10:09am
FLO	Pass	10:09am
FC	Pass	10:09am

Temperature Tests

Test	Status	Time
FC1	Pass	10:10am
SRC	Pass	10:10am
DET	Pass	10:10am
BAR	Pass	10:10am
BT	Pass	10:10am

Blank Tests

Test	Status	Time
AIR	Pass	10:10am

Printer Tests

Test	Status	Time
PRNT	Pass	10:10am

CRC Tests

Test	Status	Time
COMP	Pass	10:10am
CAL	Pass	10:10am

Preventive Maintenance
Status: Pass



Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County WAKE Instrument Location BAT Mobile Unit 10

Instrument Serial No. 008776

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

(1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;

(2) Verify instrument displays time and date;

(3) Initiate breath test sequence;

(4) Enter information as prompted;

(5) Verify instrument accuracy;

(6) When "PLEASE BLOW" appears, collect breath sample;

(7) When "PLEASE BLOW" appears, collect breath sample;

(8) Print test record;

(9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and

(10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 26 day of June, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.

Signature of Certifying Official

193759
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

DHHS 4080 (04/20)

Intox EC/IR-II: Subject Test

WAKE COUNTY BAT MOBILE UNIT 10 910

Serial Number: *008776*
Test Date: *06/26/2026*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name: *Carroll, Barry Jean D*
Permit Number: *0019-3759*
Effective:
04/01/2026-04/01/2028

Officer's Name: *NONE, NONE*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG534301
Exp Date: 12/09/2027

Test	g/210L	Time
DIAG	Pass	9:16pm
AIR BLK	.00	9:16pm
ACCY CHK	.08	9:17pm
AIR BLK	.00	9:18pm
SUB TEST	**.00**	**9:18pm**
AIR BLK	.00	9:19pm
SUB TEST	**.00**	**9:21pm**
AIR BLK	.00	9:22pm

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

WAKE COUNTY BAT MOBILE UNIT 10 910

Serial Number: *008776* Test Record Number: *4231*
Test Date: *06/26/2026* Test Time: *9:22pm EDT*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	9:22pm
FLO	Pass	9:22pm
FC	Pass	9:22pm

Temperature Tests

Test	Status	Time
FC1	Pass	9:22pm
SRC	Pass	9:22pm
DET	Pass	9:22pm
BAR	Pass	9:22pm
BT	Pass	9:22pm

Blank Tests

Test	Status	Time
AIR	Pass	9:23pm

Printer Tests

Test	Status	Time
PRNT	Pass	9:23pm

CRC Tests

Test	Status	Time
COMP	Pass	9:23pm
CAL	Pass	9:23pm

Preventive Maintenance
Status: Pass

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Wake Instrument Location Wake County Detention Center

Instrument Serial No. DD 8778 3301 Hammond Rd.

Raleigh, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

(1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;

(2) Verify instrument displays time and date;

(3) Initiate breath test sequence;

(4) Enter information as prompted;

(5) Verify instrument accuracy;

(6) When "PLEASE BLOW" appears, collect breath sample;

(7) When "PLEASE BLOW" appears, collect breath sample;

(8) Print test record;

(9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and

(10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 1 day of June, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.

Signature of Certifying Official

169451
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

DHHS 4080 (04/20)

Intox EC/IR-II: Subject Test

WAKE COUNTY DETENTION CENTER 910

Serial Number: *008778*
Test Date: *06/01/2026*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name: *Brame, Bryant T*
Permit Number: *0016-9451*
Effective:
04/01/2026-04/01/2028

Officer's Name: *NONE, NONE*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG534301
Exp Date: 12/09/2027

Test	g/210L	Time
DIAG	Pass	9:28am
AIR BLK	.00	9:29am
ACCY CHK	.08	9:29am
AIR BLK	.00	9:30am
SUB TEST	**.00**	**9:31am**
AIR BLK	.00	9:32am
SUB TEST	**.00**	**9:33am**
AIR BLK	.00	9:34am

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

WAKE COUNTY DETENTION CENTER 910

Serial Number: *008778* Test Record Number: *9189*
Test Date: *06/01/2026* Test Time: *9:35am EDT*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	9:35am
FLO	Pass	9:35am
FC	Pass	9:35am

Temperature Tests

Test	Status	Time
FC1	Pass	9:36am
SRC	Pass	9:36am
DET	Pass	9:36am
BAR	Pass	9:36am
BT	Pass	9:36am

Blank Tests

Test	Status	Time
AIR	Pass	9:36am

Printer Tests

Test	Status	Time
PRNT	Pass	9:36am

CRC Tests

Test	Status	Time
COMP	Pass	9:36am
CAL	Pass	9:36am

Preventive Maintenance
Status: Pass

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Wake Instrument Location BAT Mobile Unit 10

Instrument Serial No. 008779

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

(1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;

(2) Verify instrument displays time and date;

(3) Initiate breath test sequence;

(4) Enter information as prompted;

(5) Verify instrument accuracy;

(6) When "PLEASE BLOW" appears, collect breath sample;

(7) When "PLEASE BLOW" appears, collect breath sample;

(8) Print test record;

(9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and

(10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 26 day of June, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.

Signature of Certifying Official

193759
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

DHHS 4080 (04/20)

Intox EC/IR-II: Subject Test

WAKE COUNTY BAT MOBILE UNIT 10 910

Serial Number: *008779*
Test Date: *06/26/2026*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name: *Carroll, Barry Jean D*
Permit Number: *0019-3759*
Effective:
04/01/2026-04/01/2028

Officer's Name: *NONE, NONE*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG431002
Exp Date: 11/05/2026

Test	g/210L	Time
DIAG	Pass	8:51pm
AIR BLK	.00	8:52pm
ACCY CHK	.08	8:52pm
AIR BLK	.00	8:53pm
SUB TEST	**.00**	**8:54pm**
AIR BLK	.00	8:55pm
SUB TEST	**.00**	**8:58pm**
AIR BLK	.00	8:59pm

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

WAKE COUNTY BAT MOBILE UNIT 10 910

Serial Number: *008779* Test Record Number: *4154*
Test Date: *06/26/2026* Test Time: *8:59pm EDT*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	9:00pm
FLO	Pass	9:00pm
FC	Pass	9:00pm

Temperature Tests

Test	Status	Time
FC1	Pass	9:00pm
SRC	Pass	9:00pm
DET	Pass	9:00pm
BAR	Pass	9:00pm
BT	Pass	9:00pm

Blank Tests

Test	Status	Time
AIR	Pass	9:01pm

Printer Tests

Test	Status	Time
PRNT	Pass	9:01pm

CRC Tests

Test	Status	Time
COMP	Pass	9:01pm
CAL	Pass	9:01pm

Preventive Maintenance
Status: Pass



Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County WAKE Instrument Location BAT Mobile Unit 12

Instrument Serial No. 008788

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

(1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;

(2) Verify instrument displays time and date;

(3) Initiate breath test sequence;

(4) Enter information as prompted;

(5) Verify instrument accuracy;

(6) When "PLEASE BLOW" appears, collect breath sample;

(7) When "PLEASE BLOW" appears, collect breath sample;

(8) Print test record;

(9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and

(10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 26th day of June, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.

Signature of Certifying Official

83034
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

DHHS 4080 (04/20)

Intox EC/IR-II: Subject Test

WAKE COUNTY BAT MOBILE UNIT 12 910

Serial Number: *008788*
Test Date: *06/26/2026*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name:
Crutchfield Jr., Marshall B
Permit Number: *0008-3034*
Effective:
03/01/2026-03/01/2028

Officer's Name: *NONE, NONE*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG534301
Exp Date: 12/09/2027

Test	g/210L	Time
DIAG	Pass	8:46pm
AIR BLK	.00	8:47pm
ACCY CHK	.07	8:47pm
AIR BLK	.00	8:48pm
SUB TEST	**.00**	**8:49pm**
AIR BLK	.00	8:50pm
SUB TEST	**.00**	**8:51pm**
AIR BLK	.00	8:52pm

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

WAKE COUNTY BAT MOBILE UNIT 12 910

Serial Number: *008788* Test Record Number: *2570*
Test Date: *06/26/2026* Test Time: *8:53pm EDT*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	8:53pm
FLO	Pass	8:53pm
FC	Pass	8:53pm

Temperature Tests

Test	Status	Time
FC1	Pass	8:53pm
SRC	Pass	8:53pm
DET	Pass	8:53pm
BAR	Pass	8:53pm
BT	Pass	8:53pm

Blank Tests

Test	Status	Time
AIR	Pass	8:54pm

Printer Tests

Test	Status	Time
PRNT	Pass	8:54pm

CRC Tests

Test	Status	Time
COMP	Pass	8:54pm
CAL	Pass	8:54pm

Preventive Maintenance
Status: Pass



Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Wake Instrument Location Knightdale PD

Instrument Serial No. 008838 979 Steeple Square Ct.
Knightdale, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

(1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;

(2) Verify instrument displays time and date;

(3) Initiate breath test sequence;

(4) Enter information as prompted;

(5) Verify instrument accuracy;

(6) When "PLEASE BLOW" appears, collect breath sample;

(7) When "PLEASE BLOW" appears, collect breath sample;

(8) Print test record;

(9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and

(10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 16 day of June, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.

Signature of Certifying Official

16951
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

DHHS 4080 (04/20)

Intox EC/IR-II: Subject Test

WAKE COUNTY KNIGHTDALE PD 910

Serial Number: *008838*
Test Date: *06/16/2026*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name: *Brame, Bryant T*
Permit Number: *0016-9451*
Effective:
04/01/2026-04/01/2028

Officer's Name: *NONE, NONE*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG534301
Exp Date: 12/09/2027

Test	g/210L	Time
DIAG	Pass	3:24pm
AIR BLK	.00	3:24pm
ACCY CHK	.07	3:25pm
AIR BLK	.00	3:26pm
SUB TEST	**.00**	**3:28pm**
AIR BLK	.00	3:28pm
SUB TEST	**.00**	**3:30pm**
AIR BLK	.00	3:31pm

Reported **AC:** .00 g/210L

Signature of Chemical Analyst

Court CVR

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

WAKE COUNTY KNIGHTDALE PD 910

Serial Number: *008838* Test Record Number: *3219*
Test Date: *06/16/2026* Test Time: *3:32pm EDT*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	3:32pm
FLO	Pass	3:32pm
FC	Pass	3:32pm

Temperature Tests

Test	Status	Time
FC1	Pass	3:32pm
SRC	Pass	3:32pm
DET	Pass	3:32pm
BAR	Pass	3:32pm
BT	Pass	3:32pm

Blank Tests

Test	Status	Time
AIR	Pass	3:33pm

Printer Tests

Test	Status	Time
PRNT	Pass	3:33pm

CRC Tests

Test	Status	Time
COMP	Pass	3:33pm
CAL	Pass	3:33pm

Preventive Maintenance
Status: Pass

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD INTOXIMETERS, MODEL INTOX EC/IR II and MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Wake Instrument Location BAT Mobile Unit 13

Instrument Serial No. 008869

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

(1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;

(2) Verify instrument displays time and date;

(3) Initiate breath test sequence;

(4) Enter information as prompted;

(5) Verify instrument accuracy;

(6) When "PLEASE BLOW" appears, collect breath sample;

(7) When "PLEASE BLOW" appears, collect breath sample;

(8) Print test record;

(9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and

(10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 5th day of June, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.

Tony B White — Signature of Certifying Official

307699 — Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

DHHS 4080 (04/20)

Intox EC/IR-II: Subject Test

WAKE COUNTY BAT MOBILE UNIT 13 910

Serial Number: *008869*
Test Date: *06/05/2026*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name: *Whitehurst, Timothy B*
Permit Number: *0030-7699*
Effective:
03/01/2026-03/01/2028

Officer's Name: *NONE, NONE*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG506303
Exp Date: 03/04/2027

Test	g/210L	Time
DIAG	Pass	9:29pm
AIR BLK	.00	9:31pm
ACCY CHK	.08	9:31pm
AIR BLK	.00	9:32pm
SUB TEST	**.00**	**9:33pm**
AIR BLK	.00	9:33pm
SUB TEST	**.00**	**9:35pm**
AIR BLK	.00	9:36pm

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

WAKE COUNTY BAT MOBILE UNIT 13 910

Serial Number: *008869* Test Record Number: *2213*
Test Date: *06/05/2026* Test Time: *9:41pm EDT*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	9:41pm
FLO	Pass	9:41pm
FC	Pass	9:41pm

Temperature Tests

Test	Status	Time
FC1	Pass	9:41pm
SRC	Pass	9:41pm
DET	Pass	9:41pm
BAR	Pass	9:41pm
BT	Pass	9:41pm

Blank Tests

Test	Status	Time
AIR	Pass	9:42pm

Printer Tests

Test	Status	Time
PRNT	Pass	9:42pm

CRC Tests

Test	Status	Time
COMP	Pass	9:42pm
CAL	Pass	9:42pm

Preventive Maintenance
Status: Pass

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Wake Instrument Location BAT Mobile Unit 13

Instrument Serial No. 008898

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

(1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;

(2) Verify instrument displays time and date;

(3) Initiate breath test sequence;

(4) Enter information as prompted;

(5) Verify instrument accuracy;

(6) When "PLEASE BLOW" appears, collect breath sample;

(7) When "PLEASE BLOW" appears, collect breath sample;

(8) Print test record;

(9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and

(10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 5th day of June, 2024 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.

Signature of Certifying Official

307699
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

DHHS 4080 (04/20)

Intox EC/IR-II: Subject Test

WAKE COUNTY BAT MOBILE UNIT 13 910

Serial Number: *008898*
Test Date: *06/05/2026*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name: *Whitehurst, Timothy B*
Permit Number: *0030-7699*
Effective:
03/01/2026-03/01/2028

Officer's Name: *NONE, NONE*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG506302
Exp Date: 03/04/2027

Test	g/210L	Time
DIAG	Pass	9:13pm
AIR BLK	.00	9:14pm
ACCY CHK	.07	9:15pm
AIR BLK	.00	9:16pm
SUB TEST	**.00**	**9:18pm**
AIR BLK	.00	9:19pm
SUB TEST	**.00**	**9:21pm**
AIR BLK	.00	9:22pm

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

WAKE COUNTY BAT MOBILE UNIT 13 910

Serial Number: *008898* Test Record Number: *2156*
Test Date: *06/05/2026* Test Time: *9:23pm EDT*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	9:23pm
FLO	Pass	9:23pm
FC	Pass	9:23pm

Temperature Tests

Test	Status	Time
FC1	Pass	9:23pm
SRC	Pass	9:23pm
DET	Pass	9:23pm
BAR	Pass	9:23pm
BT	Pass	9:23pm

Blank Tests

Test	Status	Time
AIR	Pass	9:24pm

Printer Tests

Test	Status	Time
PRNT	Pass	9:24pm

CRC Tests

Test	Status	Time
COMP	Pass	9:24pm
CAL	Pass	9:24pm

Preventive Maintenance
Status: Pass

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Wake Instrument Location Raleigh PD Downtown Dist.

Instrument Serial No. 008907 218 W Cabarrus St.

Raleigh, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

(1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;

(2) Verify instrument displays time and date;

(3) Initiate breath test sequence;

(4) Enter information as prompted;

(5) Verify instrument accuracy;

(6) When "PLEASE BLOW" appears, collect breath sample;

(7) When "PLEASE BLOW" appears, collect breath sample;

(8) Print test record;

(9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and

(10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 24 day of June, 20 26 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.

Signature of Certifying Official

169451
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

DHHS 4080 (04/20)

Intox EC/IR-II: Subject Test

WAKE COUNTY RALEIGH PD DOWNTOWN 910

Serial Number: *008907*
Test Date: *06/24/2026*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name: *Brame, Bryant T*
Permit Number: *0016-9451*
Effective:
04/01/2026-04/01/2028

Officer's Name: *NONE, NONE*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG516203
Exp Date: 06/11/2027

Test	g/210L	Time
DIAG	Pass	10:00am
AIR BLK	.00	10:01am
ACCY CHK	.08	10:02am
AIR BLK	.00	10:03am
SUB TEST	**.00**	**10:04am**
AIR BLK	.00	10:05am
SUB TEST	**.00**	**10:06am**
AIR BLK	.00	10:07am

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

WAKE COUNTY RALEIGH PD DOWNTOWN 910

Serial Number: *008907* Test Record Number: *1816*
Test Date: *06/24/2026* Test Time: *10:07am EDT*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	10:08am
FLO	Pass	10:08am
FC	Pass	10:08am

Temperature Tests

Test	Status	Time
FC1	Pass	10:08am
SRC	Pass	10:08am
DET	Pass	10:08am
BAR	Pass	10:08am
BT	Pass	10:08am

Blank Tests

Test	Status	Time
AIR	Pass	10:09am

Printer Tests

Test	Status	Time
PRNT	Pass	10:09am

CRC Tests

Test	Status	Time
COMP	Pass	10:09am
CAL	Pass	10:09am

Preventive Maintenance
Status: Pass

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Wake Instrument Location BAT Mobile Unit 13

Instrument Serial No. DD 8939

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

(1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;

(2) Verify instrument displays time and date;

(3) Initiate breath test sequence;

(4) Enter information as prompted;

(5) Verify instrument accuracy;

(6) When "PLEASE BLOW" appears, collect breath sample;

(7) When "PLEASE BLOW" appears, collect breath sample;

(8) Print test record;

(9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and

(10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 5th day of June, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.

Signature of Certifying Official

307699
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

DHHS 4080 (04/20)

Intox EC/IR-II: Subject Test

WAKE COUNTY BAT MOBILE UNIT 13 910

Serial Number: *008939*
Test Date: *06/05/2026*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name: *Whitehurst, Timothy B*
Permit Number: *0030-7699*
Effective:
03/01/2026-03/01/2028

Officer's Name: *NONE, NONE*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG506302
Exp Date: 03/04/2027

Test	g/210L	Time
DIAG	Pass	8:48pm
AIR BLK	.00	8:48pm
ACCY CHK	.07	8:49pm
AIR BLK	.00	8:50pm
SUB TEST	**.00**	**8:50pm**
AIR BLK	.00	8:51pm
SUB TEST	**.00**	**8:53pm**
AIR BLK	.00	8:54pm

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

WAKE COUNTY BAT MOBILE UNIT 13 910

Serial Number: *008939* Test Record Number: *2016*
Test Date: *06/05/2026* Test Time: *8:54pm EDT*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	8:54pm
FLO	Pass	8:54pm
FC	Pass	8:55pm

Temperature Tests

Test	Status	Time
FC1	Pass	8:55pm
SRC	Pass	8:55pm
DET	Pass	8:55pm
BAR	Pass	8:55pm
BT	Pass	8:55pm

Blank Tests

Test	Status	Time
AIR	Pass	8:55pm

Printer Tests

Test	Status	Time
PRNT	Pass	8:55pm

CRC Tests

Test	Status	Time
COMP	Pass	8:55pm
CAL	Pass	8:55pm

Preventive Maintenance
Status: Pass

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Wake Instrument Location BAT Mobile Unit 7

Instrument Serial No. 008968

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

(1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;

(2) Verify instrument displays time and date;

(3) Initiate breath test sequence;

(4) Enter information as prompted;

(5) Verify instrument accuracy;

(6) When "PLEASE BLOW" appears, collect breath sample;

(7) When "PLEASE BLOW" appears, collect breath sample;

(8) Print test record;

(9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and

(10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 12 day of June, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.

Signature of Certifying Official

193759
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

DHHS 4080 (04/20)

Intox EC/IR-II: Subject Test

WAKE COUNTY BAT MOBILE UNIT 7 910

Serial Number: *008968*
Test Date: *06/12/2026*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name: *Carroll, Barry Jean D*
Permit Number: *0019-3759*
Effective:
04/01/2026-04/01/2028

Officer's Name: *NONE, NONE*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG506303
Exp Date: 03/04/2027

Test	g/210L	Time
DIAG	Pass	9:04pm
AIR BLK	.00	9:05pm
ACCY CHK	.08	9:06pm
AIR BLK	.00	9:07pm
SUB TEST	**.00**	**9:08pm**
AIR BLK	.00	9:08pm
SUB TEST	**.00**	**9:10pm**
AIR BLK	.00	9:11pm

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

WAKE COUNTY BAT MOBILE UNIT 7 910

Serial Number: *008968* Test Record Number: *476*
Test Date: *06/12/2026* Test Time: *9:11pm EDT*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	9:12pm
FLO	Pass	9:12pm
FC	Pass	9:12pm

Temperature Tests

Test	Status	Time
FC1	Pass	9:12pm
SRC	Pass	9:12pm
DET	Pass	9:12pm
BAR	Pass	9:12pm
BT	Pass	9:12pm

Blank Tests

Test	Status	Time
AIR	Pass	9:12pm


Printer Tests

Test	Status	Time
PRNT	Pass	9:12pm

CRC Tests

Test	Status	Time
COMP	Pass	9:13pm
CAL	Pass	9:13pm

Preventive Maintenance
Status: Pass

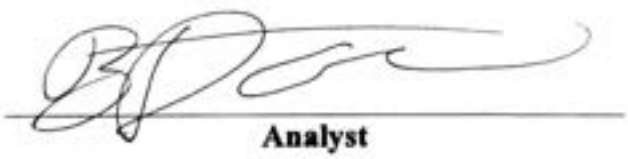

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Wake Instrument Location BAT Mobile unit 7

Instrument Serial No. 008971

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

(1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;

(2) Verify instrument displays time and date;

(3) Initiate breath test sequence;

(4) Enter information as prompted;

(5) Verify instrument accuracy;

(6) When "PLEASE BLOW" appears, collect breath sample;

(7) When "PLEASE BLOW" appears, collect breath sample;

(8) Print test record;

(9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and

(10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 12 day of June, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.

Signature of Certifying Official

193759
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

DHHS 4080 (04/20)

Intox EC/IR-II: Subject Test

WAKE COUNTY BAT MOBILE UNIT 7 910

Serial Number: *008971*
Test Date: *06/12/2026*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name: *Carroll, Barry Jean D*
Permit Number: *0019-3759*
Effective:
04/01/2026-04/01/2028

Officer's Name: *NONE, NONE*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG506302
Exp Date: 03/04/2027

Test	g/210L	Time
DIAG	Pass	9:13pm
AIR BLK	.00	9:14pm
ACCY CHK	.08	9:14pm
AIR BLK	.00	9:15pm
SUB TEST	**.00**	**9:16pm**
AIR BLK	.00	9:17pm
SUB TEST	**.00**	**9:18pm**
AIR BLK	.00	9:19pm

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

WAKE COUNTY BAT MOBILE UNIT 7 910

Serial Number: *008971* Test Record Number: *422*
Test Date: *06/12/2026* Test Time: *9:21pm EDT*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	9:22pm
FLO	Pass	9:22pm
FC	Pass	9:22pm

Temperature Tests

Test	Status	Time
FC1	Pass	9:22pm
SRC	Pass	9:22pm
DET	Pass	9:22pm
BAR	Pass	9:22pm
BT	Pass	9:22pm

Blank Tests

Test	Status	Time
AIR	Pass	9:22pm


Printer Tests

Test	Status	Time
PRNT	Pass	9:22pm

CRC Tests

Test	Status	Time
COMP	Pass	9:23pm
CAL	Pass	9:23pm

Preventive Maintenance
Status: Pass

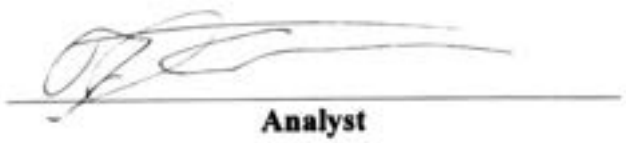

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Wake Instrument Location BAT Mobile Unit 7

Instrument Serial No. 008972

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

(1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;

(2) Verify instrument displays time and date;

(3) Initiate breath test sequence;

(4) Enter information as prompted;

(5) Verify instrument accuracy;

(6) When "PLEASE BLOW" appears, collect breath sample;

(7) When "PLEASE BLOW" appears, collect breath sample;

(8) Print test record;

(9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and

(10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 12 day of June, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.

Signature of Certifying Official

193759
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

DHHS 4080 (04/20)

Intox EC/IR-II: Subject Test

WAKE COUNTY BAT MOBILE UNIT 7 910

Serial Number: *008972*
Test Date: *06/12/2026*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name: *Carroll, Barry Jean D*
Permit Number: *0019-3759*
Effective:
04/01/2026-04/01/2028

Officer's Name: *NONE, NONE*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG506303
Exp Date: 03/04/2027

Test	g/210L	Time
DIAG	Pass	9:10pm
AIR BLK	.00	9:11pm
ACCY CHK	.08	9:12pm
AIR BLK	.00	9:13pm
SUB TEST	**.00**	**9:14pm**
AIR BLK	.00	9:15pm
SUB TEST	**.00**	**9:16pm**
AIR BLK	.00	9:17pm

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

WAKE COUNTY BAT MOBILE UNIT 7 910

Serial Number: *008972* Test Record Number: *490*
Test Date: *06/12/2026* Test Time: *9:18pm EDT*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	9:18pm
FLO	Pass	9:18pm
FC	Pass	9:18pm

Temperature Tests

Test	Status	Time
FC1	Pass	9:18pm
SRC	Pass	9:18pm
DET	Pass	9:18pm
BAR	Pass	9:18pm
BT	Pass	9:18pm

Blank Tests

Test	Status	Time
AIR	Pass	9:19pm

Printer Tests

Test	Status	Time
PRNT	Pass	9:19pm

CRC Tests

Test	Status	Time
COMP	Pass	9:19pm
CAL	Pass	9:19pm

Preventive Maintenance
Status: Pass

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County WATAUGA Instrument Location WATAUGA COUNTY DETENTION

Instrument Serial No. 008715 BOONE, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

(1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;

(2) Verify instrument displays time and date;

(3) Initiate breath test sequence;

(4) Enter information as prompted;

(5) Verify instrument accuracy;

(6) When "PLEASE BLOW" appears, collect breath sample;

(7) When "PLEASE BLOW" appears, collect breath sample;

(8) Print test record;

(9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and

(10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 15TH day of JUNE, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.

Signature of Certifying Official

353799
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

DHHS 4080 (04/20)

Intox EC/IR-II: Subject Test

WATAUGA COUNTY DETENTION CENTER 940

Serial Number: *008715*
Test Date: *06/15/2026*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name: *Oligmueller, Leo A*
Permit Number: *0035-3799*
Effective:
02/01/2025-02/01/2027

Officer's Name: *NONE, NONE*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG534301
Exp Date: 12/09/2027

Test	g/210L	Time
DIAG	Pass	1:54pm
AIR BLK	.00	1:54pm
ACCY CHK	.08	1:55pm
AIR BLK	.00	1:56pm
SUB TEST	**.00**	**1:57pm**
AIR BLK	.00	1:58pm
SUB TEST	**.00**	**1:59pm**
AIR BLK	.00	2:00pm

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

WATAUGA COUNTY DETENTION CENTER 940

Serial Number: *008715* Test Record Number: *3181*
Test Date: *06/15/2026* Test Time: *2:01pm EDT*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	2:01pm
FLO	Pass	2:01pm
FC	Pass	2:02pm

Temperature Tests

Test	Status	Time
FC1	Pass	2:02pm
SRC	Pass	2:02pm
DET	Pass	2:02pm
BAR	Pass	2:02pm
BT	Pass	2:02pm

Blank Tests

Test	Status	Time
AIR	Pass	2:02pm

Printer Tests

Test	Status	Time
PRNT	Pass	2:02pm

CRC Tests

Test	Status	Time
COMP	Pass	2:03pm
CAL	Pass	2:03pm

Preventive Maintenance
Status: Pass



Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Wayne Instrument Location Wayne Co. Detention Center

Instrument Serial No. 008649 200 Stronach Ave, Goldsboro, NC.

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

(1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;

(2) Verify instrument displays time and date;

(3) Initiate breath test sequence;

(4) Enter information as prompted;

(5) Verify instrument accuracy;

(6) When "PLEASE BLOW" appears, collect breath sample;

(7) When "PLEASE BLOW" appears, collect breath sample;

(8) Print test record;

(9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and

(10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 23rd day of June, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.

THE GREAT SEAL OF THE STATE OF NORTH CAROLINA

Signature of Certifying Official

377722
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

DHHS 4080 (04/20)

Intox EC/IR-II: Subject Test

WAYNE COUNTY DETENTION CENTER 950

Serial Number: *008649*
Test Date: *06/23/2026*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name: *Gray, Kelly D*
Permit Number: *0037-7722*
Effective:
02/01/2026-02/01/2028

Officer's Name: *NONE, NONE*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG516203
Exp Date: 06/11/2027

Test	g/210L	Time
DIAG	Pass	11:40am
AIR BLK	.00	11:41am
ACCY CHK	.08	11:42am
AIR BLK	.00	11:43am
SUB TEST	**.00**	**11:44am**
AIR BLK	.00	11:45am
SUB TEST	**.00**	**11:46am**
AIR BLK	.00	11:47am

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

WAYNE COUNTY DETENTION CENTER 950

Serial Number: *008649* Test Record Number: *6465*
Test Date: *06/23/2026* Test Time: *11:48am EDT*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	11:49am
FLO	Pass	11:49am
FC	Pass	11:49am

Temperature Tests

Test	Status	Time
FC1	Pass	11:49am
SRC	Pass	11:49am
DET	Pass	11:49am
BAR	Pass	11:49am
BT	Pass	11:49am

Blank Tests

Test	Status	Time
AIR	Pass	11:49am

Printer Tests

Test	Status	Time
PRNT	Pass	11:49am

CRC Tests

Test	Status	Time
COMP	Pass	11:50am
CAL	Pass	11:50am

Preventive Maintenance
Status: Pass

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Wayne Instrument Location Wayne Co. Detention Center

Instrument Serial No. 008879 200 Stronach Ave., Goldsboro, NC.

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

(1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;

(2) Verify instrument displays time and date;

(3) Initiate breath test sequence;

(4) Enter information as prompted;

(5) Verify instrument accuracy;

(6) When "PLEASE BLOW" appears, collect breath sample;

(7) When "PLEASE BLOW" appears, collect breath sample;

(8) Print test record;

(9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and

(10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 23rd day of June, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Signature of Certifying Official

377722
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

DHHS 4080 (04/20)

Intox EC/IR-II: Subject Test

WAYNE COUNTY DETENTION CENTER 950

Serial Number: *008879*
Test Date: *06/23/2026*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name: *Gray, Kelly D*
Permit Number: *0037-7722*
Effective:
02/01/2026-02/01/2028

Officer's Name: *NONE, NONE*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG516204
Exp Date: 06/11/2027

Test	g/210L	Time
DIAG	Pass	11:42am
AIR BLK	.00	11:42am
ACCY CHK	.08	11:43am
AIR BLK	.00	11:44am
SUB TEST	**.00**	**11:45am**
AIR BLK	.00	11:46am
SUB TEST	**.00**	**11:48am**
AIR BLK	.00	11:49am

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

WAYNE COUNTY DETENTION CENTER 950

Serial Number: *008879* Test Record Number: *3001*
Test Date: *06/23/2026* Test Time: *11:50am EDT*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	11:50am
FLO	Pass	11:50am
FC	Pass	11:50am

Temperature Tests

Test	Status	Time
FC1	Pass	11:51am
SRC	Pass	11:51am
DET	Pass	11:51am
BAR	Pass	11:51am
BT	Pass	11:51am

Blank Tests

Test	Status	Time
AIR	Pass	11:51am

Printer Tests

Test	Status	Time
PRNT	Pass	11:51am

CRC Tests

Test	Status	Time
COMP	Pass	11:51am
CAL	Pass	11:51am

Preventive Maintenance
Status: Pass

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD INTOXIMETERS, MODEL INTOX EC/IR II and MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Wilkes Instrument Location BAT Mobile Unit 7

Instrument Serial No. 008002

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

(1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;

(2) Verify instrument displays time and date;

(3) Initiate breath test sequence;

(4) Enter information as prompted;

(5) Verify instrument accuracy;

(6) When "PLEASE BLOW" appears, collect breath sample;

(7) When "PLEASE BLOW" appears, collect breath sample;

(8) Print test record;

(9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and

(10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 22nd day of June, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.

John Lanier
Signature of Certifying Official

1604930
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

DHHS 4080 (04/20)

Intox EC/IR-II: Subject Test

WILKES COUNTY BAT MOBILE UNIT 7 960

Serial Number: *008002*
Test Date: *06/22/2026*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name: *Lanier Jr., John P*
Permit Number: *4582-9118*
Effective:
02/01/2026-02/01/2028

Officer's Name: *NONE, NONE*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG506303
Exp Date: 03/04/2027

Test	g/210L	Time
DIAG	Pass	6:47pm
AIR BLK	.00	6:47pm
ACCY CHK	.07	6:48pm
AIR BLK	.00	6:49pm
SUB TEST	**.00**	**6:49pm**
AIR BLK	.00	6:50pm
SUB TEST	**.00**	**6:52pm**
AIR BLK	.00	6:53pm

Reported AC: .00 g/210L

John Lanier

Signature of Chemical Analyst

Court CVR

John Lanier

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

WILKES COUNTY BAT MOBILE UNIT 7 960

Serial Number: *008002* Test Record Number: *928*
Test Date: *06/22/2026* Test Time: *6:54pm EDT*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	6:54pm
FLO	Pass	6:54pm
FC	Pass	6:54pm

Temperature Tests

Test	Status	Time
FC1	Pass	6:54pm
SRC	Pass	6:54pm
DET	Pass	6:54pm
BAR	Pass	6:54pm
BT	Pass	6:54pm

Blank Tests

Test	Status	Time
AIR	Pass	6:55pm

Printer Tests

Test	Status	Time
PRNT	Pass	6:55pm

CRC Tests

Test	Status	Time
COMP	Pass	6:55pm
CAL	Pass	6:55pm

Preventive Maintenance
Status: Pass

John Ranier

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD INTOXIMETERS, MODEL INTOX EC/IR II and MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Wilkes Instrument Location BAT Mobile Unit 7

Instrument Serial No. 008090

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

(1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;

(2) Verify instrument displays time and date;

(3) Initiate breath test sequence;

(4) Enter information as prompted;

(5) Verify instrument accuracy;

(6) When "PLEASE BLOW" appears, collect breath sample;

(7) When "PLEASE BLOW" appears, collect breath sample;

(8) Print test record;

(9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and

(10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 22nd day of June, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.

John Lanier
Signature of Certifying Official

1604930
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

DHHS 4080 (04/20)

Intox EC/IR-II: Subject Test

WILKES COUNTY BAT MOBILE UNIT 7 960

Serial Number: *008090*
Test Date: *06/22/2026*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name: *Lanier Jr., John P*
Permit Number: *4582-9118*
Effective:
02/01/2026-02/01/2028

Officer's Name: *NONE, NONE*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG602101
Exp Date: 01/21/2028

Test	g/210L	Time
DIAG	Pass	6:36pm
AIR BLK	.00	6:37pm
ACCY CHK	.07	6:37pm
AIR BLK	.00	6:38pm
SUB TEST	**.00**	**6:39pm**
AIR BLK	.00	6:40pm
SUB TEST	**.00**	**6:42pm**
AIR BLK	.00	6:43pm

Reported AC: .00 g/210L

John Lanier
Signature of Chemical Analyst

Court CVR

John Lanier
Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

WILKES COUNTY BAT MOBILE UNIT 7 960

Serial Number: *008090* Test Record Number: *289*
Test Date: *06/22/2026* Test Time: *6:43pm EDT*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	6:43pm
FLO	Pass	6:43pm
FC	Pass	6:44pm

Temperature Tests

Test	Status	Time
FC1	Pass	6:44pm
SRC	Pass	6:44pm
DET	Pass	6:44pm
BAR	Pass	6:44pm
BT	Pass	6:44pm

Blank Tests

Test	Status	Time
AIR	Pass	6:44pm

Printer Tests

Test	Status	Time
PRNT	Pass	6:44pm

CRC Tests

Test	Status	Time
COMP	Pass	6:44pm
CAL	Pass	6:44pm

Preventive Maintenance
Status: Pass

John Ranier

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Wilkes Instrument Location BAT Mobile Unit 7

Instrument Serial No. 008968

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

(1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;

(2) Verify instrument displays time and date;

(3) Initiate breath test sequence;

(4) Enter information as prompted;

(5) Verify instrument accuracy;

(6) When "PLEASE BLOW" appears, collect breath sample;

(7) When "PLEASE BLOW" appears, collect breath sample;

(8) Print test record;

(9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and

(10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 22nd day of June, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.

John Lanier
Signature of Certifying Official

1604930
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

DHHS 4080 (04/20)

Intox EC/IR-II: Subject Test

WILKES COUNTY BAT MOBILE UNIT 7 960

Serial Number: *008968*
Test Date: *06/22/2026*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name: *Lanier Jr., John P*
Permit Number: *4582-9118*
Effective:
02/01/2026-02/01/2028

Officer's Name: *NONE, NONE*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG506303
Exp Date: 03/04/2027

Test	g/210L	Time
DIAG	Pass	4:51pm
AIR BLK	.00	4:52pm
ACCY CHK	.07	4:52pm
AIR BLK	.00	4:53pm
SUB TEST	**.00**	**4:54pm**
AIR BLK	.00	4:55pm
SUB TEST	**.00**	**4:56pm**
AIR BLK	.00	4:57pm

Reported AC: .00 g/210L

John Lanier

Signature of Chemical Analyst

Court CVR

John Lanier

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

WILKES COUNTY BAT MOBILE UNIT 7 960

Serial Number: *008968* Test Record Number: *483*
Test Date: *06/22/2026* Test Time: *5:00pm EDT*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	5:01pm
FLO	Pass	5:01pm
FC	Pass	5:01pm

Temperature Tests

Test	Status	Time
FC1	Pass	5:01pm
SRC	Pass	5:01pm
DET	Pass	5:01pm
BAR	Pass	5:01pm
BT	Pass	5:01pm

Blank Tests

Test	Status	Time
AIR	Pass	5:01pm

Printer Tests

Test	Status	Time
PRNT	Pass	5:02pm

CRC Tests

Test	Status	Time
COMP	Pass	5:02pm
CAL	Pass	5:02pm

Preventive Maintenance
Status: Pass

John Lanier

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Wilkes Instrument Location BAT Mobile Unit 7

Instrument Serial No. 008971

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

(1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;

(2) Verify instrument displays time and date;

(3) Initiate breath test sequence;

(4) Enter information as prompted;

(5) Verify instrument accuracy;

(6) When "PLEASE BLOW" appears, collect breath sample;

(7) When "PLEASE BLOW" appears, collect breath sample;

(8) Print test record;

(9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and

(10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 22nd day of June, 2020 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.

John Lanier
Signature of Certifying Official

1604930
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

DHHS 4080 (04/20)

Intox EC/IR-II: Subject Test

WILKES COUNTY BAT MOBILE UNIT 7 960

Serial Number: *008971*
Test Date: *06/22/2026*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name: *Lanier Jr., John P*
Permit Number: *4582-9118*
Effective:
02/01/2026-02/01/2028

Officer's Name: *NONE, NONE*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG506302
Exp Date: 03/04/2027

Test	g/210L	Time
DIAG	Pass	6:06pm
AIR BLK	.00	6:07pm
ACCY CHK	.08	6:08pm
AIR BLK	.00	6:08pm
SUB TEST	**.00**	**6:10pm**
AIR BLK	.00	6:11pm
SUB TEST	**.00**	**6:13pm**
AIR BLK	.00	6:13pm

Reported AC: .00 g/210L

John Lanier
Signature of Chemical Analyst

Court CVR

John Lanier
Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

WILKES COUNTY BAT MOBILE UNIT 7 960

Serial Number: *008971* Test Record Number: *429*
Test Date: *06/22/2026* Test Time: *6:15pm EDT*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	6:15pm
FLO	Pass	6:15pm
FC	Pass	6:15pm

Temperature Tests

Test	Status	Time
FC1	Pass	6:15pm
SRC	Pass	6:15pm
DET	Pass	6:15pm
BAR	Pass	6:15pm
BT	Pass	6:15pm

Blank Tests

Test	Status	Time
AIR	Pass	6:16pm

Printer Tests

Test	Status	Time
PRNT	Pass	6:16pm

CRC Tests

Test	Status	Time
COMP	Pass	6:16pm
CAL	Pass	6:16pm

Preventive Maintenance
Status: Pass

John Lanier

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Wilkes Instrument Location BAT Mobile Unit 7

Instrument Serial No. 008972

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

(1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;

(2) Verify instrument displays time and date;

(3) Initiate breath test sequence;

(4) Enter information as prompted;

(5) Verify instrument accuracy;

(6) When "PLEASE BLOW" appears, collect breath sample;

(7) When "PLEASE BLOW" appears, collect breath sample;

(8) Print test record;

(9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and

(10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 22nd day of June, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.

Signature of Certifying Official

1604930
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

DHHS 4080 (04/20)

Intox EC/IR-II: Subject Test

WILKES COUNTY BAT MOBILE UNIT 7 960

Serial Number: *008972*
Test Date: *06/22/2026*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name: *Lanier Jr., John P*
Permit Number: *4582-9118*
Effective:
02/01/2026-02/01/2028

Officer's Name: *NONE, NONE*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG506303
Exp Date: 03/04/2027

Test	g/210L	Time
DIAG	Pass	6:47pm
AIR BLK	.00	6:48pm
ACCY CHK	.07	6:48pm
AIR BLK	.00	6:49pm
SUB TEST	**.00**	**6:50pm**
AIR BLK	.00	6:51pm
SUB TEST	**.00**	**6:53pm**
AIR BLK	.00	6:53pm

Reported AC: .00 g/210L

John Lanier

Signature of Chemical Analyst

Court CVR

John Lanier

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

WILKES COUNTY BAT MOBILE UNIT 7 960

Serial Number: *008972* Test Record Number: *501*
Test Date: *06/22/2026* Test Time: *6:54pm EDT*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	6:55pm
FLO	Pass	6:55pm
FC	Pass	6:55pm

Temperature Tests

Test	Status	Time
FC1	Pass	6:55pm
SRC	Pass	6:55pm
DET	Pass	6:55pm
BAR	Pass	6:55pm
BT	Pass	6:55pm

Blank Tests

Test	Status	Time
AIR	Pass	6:55pm

Printer Tests

Test	Status	Time
PRNT	Pass	6:56pm

CRC Tests

Test	Status	Time
COMP	Pass	6:56pm
CAL	Pass	6:56pm

Preventive Maintenance
Status: Pass

John Lanier

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Yadkin Instrument Location BAT Mobile Unit 13

Instrument Serial No. 008869

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

(1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;

(2) Verify instrument displays time and date;

(3) Initiate breath test sequence;

(4) Enter information as prompted;

(5) Verify instrument accuracy;

(6) When "PLEASE BLOW" appears, collect breath sample;

(7) When "PLEASE BLOW" appears, collect breath sample;

(8) Print test record;

(9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and

(10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 19th day of June, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.

John Ranier
Signature of Certifying Official

16049-30
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

DHHS 4080 (04/20)

Intox EC/IR-II: Subject Test

YADKIN COUNTY BAT MOBILE UNIT 13 980

Serial Number: *008869*
Test Date: *06/19/2026*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name: *Lanier Jr., John P*
Permit Number: *4582-9118*
Effective:
02/01/2026-02/01/2028

Officer's Name: *NONE, NONE*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG506303
Exp Date: 03/04/2027

Test	g/210L	Time
DIAG	Pass	6:59pm
AIR BLK	.00	7:00pm
ACCY CHK	.08	7:00pm
AIR BLK	.00	7:01pm
SUB TEST	**.00**	**7:02pm**
AIR BLK	.00	7:03pm
SUB TEST	**.00**	**7:04pm**
AIR BLK	.00	7:05pm

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

YADKIN COUNTY BAT MOBILE UNIT 13 980

Serial Number: *008869* Test Record Number: *2226*
Test Date: *06/19/2026* Test Time: *7:07pm EDT*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	7:07pm
FLO	Pass	7:07pm
FC	Pass	7:07pm

Temperature Tests

Test	Status	Time
FC1	Pass	7:07pm
SRC	Pass	7:07pm
DET	Pass	7:07pm
BAR	Pass	7:07pm
BT	Pass	7:07pm

Blank Tests

Test	Status	Time
AIR	Pass	7:08pm

Printer Tests

Test	Status	Time
PRNT	Pass	7:08pm

CRC Tests

Test	Status	Time
COMP	Pass	7:08pm
CAL	Pass	7:08pm

Preventive Maintenance
Status: Pass

John Lanier
Analyst

is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
ment of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD INTOXIMETERS, MODEL INTOX EC/IR II and MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Yadkin Instrument Location BAT Mobile Unit 13

Instrument Serial No. 008898

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

(1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;

(2) Verify instrument displays time and date;

(3) Initiate breath test sequence;

(4) Enter information as prompted;

(5) Verify instrument accuracy;

(6) When "PLEASE BLOW" appears, collect breath sample;

(7) When "PLEASE BLOW" appears, collect breath sample;

(8) Print test record;

(9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and

(10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 19th day of June, 2026 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.

John Fanier
Signature of Certifying Official

1604930
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

DHHS 4080 (04/20)

Intox EC/IR-II: Subject Test

YADKIN COUNTY BAT MOBILE UNIT 13 980

Serial Number: *008898*
Test Date: *06/19/2026*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name: *Lanier Jr., John P*
Permit Number: *4582-9118*
Effective:
02/01/2026-02/01/2028

Officer's Name: *NONE, NONE*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG506302
Exp Date: 03/04/2027

Test	g/210L	Time
DIAG	Pass	7:03pm
AIR BLK	.00	7:04pm
ACCY CHK	.07	7:05pm
AIR BLK	.00	7:06pm
SUB TEST	**.00**	**7:06pm**
AIR BLK	.00	7:07pm
SUB TEST	**.00**	**7:09pm**
AIR BLK	.00	7:10pm

Reported AC: .00 g/210L

John Lanier

Signature of Chemical Analyst

Court CVR

John Lanier

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

YADKIN COUNTY BAT MOBILE UNIT 13 980

Serial Number: *008898* Test Record Number: *2164*
Test Date: *06/19/2026* Test Time: *7:11pm EDT*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	7:12pm
FLO	Pass	7:12pm
FC	Pass	7:12pm

Temperature Tests

Test	Status	Time
FC1	Pass	7:12pm
SRC	Pass	7:12pm
DET	Pass	7:12pm
BAR	Pass	7:12pm
BT	Pass	7:12pm

Blank Tests

Test	Status	Time
AIR	Pass	7:13pm

Printer Tests

Test	Status	Time
PRNT	Pass	7:13pm

CRC Tests

Test	Status	Time
COMP	Pass	7:13pm
CAL	Pass	7:13pm

Preventive Maintenance
Status: Pass

John Ranier

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Yadkin Instrument Location BAT Mobile Unit 13

Instrument Serial No. 008939

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

(1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;

(2) Verify instrument displays time and date;

(3) Initiate breath test sequence;

(4) Enter information as prompted;

(5) Verify instrument accuracy;

(6) When "PLEASE BLOW" appears, collect breath sample;

(7) When "PLEASE BLOW" appears, collect breath sample;

(8) Print test record;

(9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and

(10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 19th day of June, 2020 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.

John Lanier
Signature of Certifying Official

1604930
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

DHHS 4080 (04/20)

Intox EC/IR-II: Subject Test

YADKIN COUNTY BAT MOBILE UNIT 13 980

Serial Number: *008939*
Test Date: *06/19/2026*

Citation Number: *M0000000-0*
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: *11/11/1911*
Subject's Sex: *Male*
Driver's License State: *XX*
Driver's License Number: *NONE*

Analyst's Name: *Lanier Jr., John P*
Permit Number: *4582-9118*
Effective:
02/01/2026-02/01/2028

Officer's Name: *NONE, NONE*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG506302
Exp Date: 03/04/2027

Test	g/210L	Time
DIAG	Pass	7:04pm
AIR BLK	.00	7:05pm
ACCY CHK	.07	7:06pm
AIR BLK	.00	7:07pm
SUB TEST	**.00**	**7:07pm**
AIR BLK	.00	7:08pm
SUB TEST	**.00**	**7:10pm**
AIR BLK	.00	7:11pm

Reported AC: .00 g/210L

John Lanier

Signature of Chemical Analyst

Court CVR

John Lanier

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

YADKIN COUNTY BAT MOBILE UNIT 13 980

Serial Number: *008939* Test Record Number: *2024*
Test Date: *06/19/2026* Test Time: *7:17pm EDT*

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	7:18pm
FLO	Pass	7:18pm
FC	Pass	7:18pm

Temperature Tests

Test	Status	Time
FC1	Pass	7:18pm
SRC	Pass	7:18pm
DET	Pass	7:18pm
BAR	Pass	7:18pm
BT	Pass	7:18pm

Blank Tests

Test	Status	Time
AIR	Pass	7:19pm

Printer Tests

Test	Status	Time
PRNT	Pass	7:19pm

CRC Tests

Test	Status	Time
COMP	Pass	7:19pm
CAL	Pass	7:19pm

Preventive Maintenance
Status: Pass

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007