

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County ALAMANCE Instrument Location ALAMANCE CO JAIL
Instrument Serial No. 008853 1095 Maple ST GRAHAM, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 2 day of April, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Simon Thomas Brown
Signature of Certifying Official

146221
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

ALAMANCE COUNTY JAIL 000

Serial Number: 008853
Test Date: 04/02/2025

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Barnes, Simon S

Permit Number: 0014-6221

Effective:

02/01/2025-02/01/2027

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG501307

Exp Date: 01/13/2027

Test	g/210L	Time
DIAG	Pass	12:22pm
AIR BLK	.00	12:22pm
ACCY CHK	.07	12:23pm
AIR BLK	.00	12:24pm
SUB TEST	.00	12:25pm
AIR BLK	.00	12:26pm
SUB TEST	.00	12:27pm
AIR BLK	.00	12:28pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

ALAMANCE COUNTY JAIL 000

Serial Number: 008853 Test Record Number: 4961
Test Date: 04/02/2025 Test Time: 12:29pm EDT

System Check: Passed

Baseline Tests

Test	Status	Time
IR	Pass	12:29pm
FLO	Pass	12:29pm
FC	Pass	12:29pm

Temperature Tests

Test	Status	Time
FC1	Pass	12:29pm
SRC	Pass	12:29pm
DET	Pass	12:29pm
BAR	Pass	12:29pm
BT	Pass	12:29pm

Blank Tests

Test	Status	Time
AIR	Pass	12:30pm

Printer Tests

Test	Status	Time
PRNT	Pass	12:30pm

CRC Tests

Test	Status	Time
COMP	Pass	12:30pm
CAL	Pass	12:30pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Alamance Instrument Location BAT Mobile Unit 13
Instrument Serial No. 008869 Burlington PD

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 18 day of April, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



T. B. White
Signature of Certifying Official

307699
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

ALAMANCE COUNTY BAT MOBILE UNIT 13 000

Serial Number: 008869
Test Date: 04/18/2025

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Whitehurst, Timothy B

Permit Number: 0030-7699

Effective:

03/01/2025-03/01/2027

Officer's Name: NONE, NONE

Type of Agency: PTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG417803

Exp Date: 06/26/2026

Test	g/210L	Time
DIAG	Pass	9:16pm
AIR BLK	.00	9:17pm
ACCY CHK	.07	9:18pm
AIR BLK	.00	9:19pm
SUB TEST	.00	9:19pm
AIR BLK	.00	9:20pm
SUB TEST	.00	9:22pm
AIR BLK	.00	9:23pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

Intox EC/IR-II: Preventive Maintenance

ALAMANCE COUNTY BAT MOBILE UNIT 13 000

Serial Number: 008869 Test Record Number: 2008
Test Date: 04/18/2025 Test Time: 9:23pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	9:23pm
FLO	Pass	9:23pm
FC	Pass	9:24pm

Temperature Tests

Test	Status	Time
FCI	Pass	9:24pm
SRC	Pass	9:24pm
DET	Pass	9:24pm
BAR	Pass	9:24pm
BT	Pass	9:24pm

Blank Tests

Test	Status	Time
AIR	Pass	9:24pm

Printer Tests

Test	Status	Time
PRNT	Pass	9:24pm

CRC Tests

Test	Status	Time
COMP	Pass	9:25pm
CAL	Pass	9:25pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Alamance Instrument Location BAR Mobile Unit 13
Instrument Serial No. 008898 Burlington PD

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 18 day of April, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Tandy B. White
Signature of Certifying Official

307699
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

ALAMANCE COUNTY BAT MOBILE UNIT 13 000

Serial Number: 008898
Test Date: 04/18/2025

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Whitehurst, Timothy B

Permit Number: 0030-7699

Effective:

03/01/2025-03/01/2027

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG506302

Exp Date: 03/04/2027

Test	g/210L	Time
DIAG	Pass	9:03pm
AIR BLK	.00	9:04pm
ACCY CHK	.07	9:04pm
AIR BLK	.00	9:05pm
SUB TEST	.00	9:06pm
AIR BLK	.00	9:07pm
SUB TEST	.00	9:08pm
AIR BLK	.00	9:09pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

Intox EC/IR-II: Preventive Maintenance

ALAMANCE COUNTY BAT MOBILE UNIT 13 000

Serial Number: 008898 Test Record Number: 1980
Test Date: 04/18/2025 Test Time: 9:11pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	9:11pm
FLO	Pass	9:11pm
FC	Pass	9:11pm

Temperature Tests

Test	Status	Time
FC1	Pass	9:11pm
SRC	Pass	9:11pm
DET	Pass	9:11pm
BAR	Pass	9:11pm
BT	Pass	9:11pm

Blank Tests

Test	Status	Time
AIR	Pass	9:12pm

Printer Tests

Test	Status	Time
PRNT	Pass	9:12pm

CRC Tests

Test	Status	Time
COMP	Pass	9:12pm
CAL	Pass	9:12pm

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Alamance Instrument Location Alamance Co Jail
Instrument Serial No. 008913 105 S. Maple St Graham, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 2 day of April, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Simon Blake Brown
Signature of Certifying Official

146221
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

ALAMANCE COUNTY ALAMANCE CO. JAIL 000

Serial Number: 008913

Test Date: 04/02/2025

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Barnes, Simon S

Permit Number: 0014-6221

Effective:

02/01/2025-02/01/2027

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG501307

Exp Date: 01/13/2027

Test	g/210L	Time
DIAG	Pass	12:22pm
AIR BLK	.00	12:23pm
ACCY CHK	.07	12:24pm
AIR BLK	.00	12:25pm
SUB TEST	.00	12:26pm
AIR BLK	.00	12:26pm
SUB TEST	.00	12:28pm
AIR BLK	.00	12:29pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

ALAMANCE COUNTY ALAMANCE CO. JAIL 000

Serial Number: 008913 Test Record Number: 5667
Test Date: 04/02/2025 Test Time: 12:29pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	12:30pm
FLO	Pass	12:30pm
FC	Pass	12:30pm

Temperature Tests

Test	Status	Time
FC1	Pass	12:30pm
SRC	Pass	12:30pm
DET	Pass	12:30pm
BAR	Pass	12:30pm
BT	Pass	12:30pm

Blank Tests

Test	Status	Time
AIR	Pass	12:30pm

Printer Tests

Test	Status	Time
PRNT	Pass	12:30pm

CRC Tests

Test	Status	Time
COMP	Pass	12:31pm
CAL	Pass	12:31pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Alamance Instrument Location BAT Mobile Unit 13
Instrument Serial No. 008939 Burlington PD

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 18 day of April, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Timothy B. White
Signature of Certifying Official
307699
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

ALAMANCE COUNTY BAT MOBILE UNIT 13 000

Serial Number: 008939
Test Date: 04/18/2025

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Whitehurst, Timothy B

Permit Number: 0030-7699

Effective:

03/01/2025-03/01/2027

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG506302

Exp Date: 03/04/2027

Test	g/210L	Time
DIAG	Pass	9:00pm
AIR BLK	.00	9:01pm
ACCY CHK	.08	9:01pm
AIR BLK	.00	9:02pm
SUB TEST	.00	9:03pm
AIR BLK	.00	9:04pm
SUB TEST	.00	9:05pm
AIR BLK	.00	9:06pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

Intox EC/IR-II: Preventive Maintenance

ALAMANCE COUNTY BAT MOBILE UNIT 13 000

Serial Number: 008939 Test Record Number: 1848
Test Date: 04/18/2025 Test Time: 9:07pm EDT

System Check: Passed

Baseline Tests

Test	Status	Time
IR	Pass	9:07pm
FLO	Pass	9:07pm
FC	Pass	9:07pm

Temperature Tests

Test	Status	Time
FC1	Pass	9:08pm
SRC	Pass	9:08pm
DET	Pass	9:08pm
BAR	Pass	9:08pm
BT	Pass	9:08pm

Blank Tests

Test	Status	Time
AIR	Pass	9:08pm

Printer Tests

Test	Status	Time
PRNT	Pass	9:08pm

CRC Tests

Test	Status	Time
COMP	Pass	9:08pm
CAL	Pass	9:08pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)


County ALLEGHANY Instrument Location ALLEGHANY CO. JAIL
Instrument Serial No. 008890 SPARTA, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 28TH day of APRIL, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.




Signature of Certifying Official

353799
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

ALLEGHANY COUNTY ALLEGHANY CO JAIL 020

Serial Number: 008890

Test Date: 04/28/2025

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Oligmueller, Leo A

Permit Number: 0035-3799

Effective:

02/01/2025-02/01/2027

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG431002

Exp Date: 11/05/2026

Test	g/210L	Time
DIAG	Pass	11:46am
AIR BLK	.00	11:46am
ACCY CHK	.07	11:47am
AIR BLK	.00	11:48am
SUB TEST	.00	11:48am
AIR BLK	.00	11:49am
SUB TEST	.00	11:51am
AIR BLK	.00	11:52am

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

ALLEGHANY COUNTY ALLEGHANY CO JAIL 020

Serial Number: 008890 Test Record Number: 1047
Test Date: 04/28/2025 Test Time: 11:53am EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	11:54am
FLO	Pass	11:54am
FC	Pass	11:54am

Temperature Tests

Test	Status	Time
FC1	Pass	11:54am
SRC	Pass	11:54am
DET	Pass	11:54am
BAR	Pass	11:54am
BT	Pass	11:54am

Blank Tests

Test	Status	Time
AIR	Pass	11:55am

Printer Tests

Test	Status	Time
PRNT	Pass	11:55am

CRC Tests

Test	Status	Time
COMP	Pass	11:55am
CAL	Pass	11:55am

Preventive Maintenance
Status: Pass


Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County AVERT Instrument Location AVERT COUNTY JAIL

Instrument Serial No. 00844 NEWLAND NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 17 day of APRIL, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



James S. Stearns
Signature of Certifying Official

274970
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

AVERY COUNTY AVERY COUNTY JAIL 050

Serial Number: 008664
Test Date: 04/17/2025

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: Fleming, Tina S
Permit Number: 0027-4970
Effective:
10/01/2023-10/01/2025

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG431003
Exp Date: 11/05/2026


Test	g/210L	Time
DIAG	Pass	10:10am
AIR BLK	.00	10:11am
ACCY CHK	.08	10:12am
AIR BLK	.00	10:13am
SUB TEST	.00	10:14am
AIR BLK	.00	10:14am
SUB TEST	.00	10:16am
AIR BLK	.00	10:17am

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

AVERY COUNTY AVERY COUNTY JAIL 050

Serial Number: 008664 Test Record Number: 1290
Test Date: 04/17/2025 Test Time: 10:18am EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	10:18am
FLO	Pass	10:18am
FC	Pass	10:18am

Temperature Tests

Test	Status	Time
FC1	Pass	10:18am
SRC	Pass	10:18am
DET	Pass	10:18am
BAR	Pass	10:18am
BT	Pass	10:18am

Blank Tests

Test	Status	Time
AIR	Pass	10:19am

Printer Tests

Test	Status	Time
PRNT	Pass	10:19am

CRC Tests

Test	Status	Time
COMP	Pass	10:19am
CAL	Pass	10:19am

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Beaufort Instrument Location Beaufort Co. Courthouse
Instrument Serial No. 008586 112 W 2nd St, Washington,
NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 25th day of April, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Key D. M.
Signature of Certifying Official

377722
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

BEAUFORT COUNTY COURTHOUSE 060

Serial Number: 008586
Test Date: 04/25/2025

Citation Number: M0000000-0
Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Gray, Kelly D

Permit Number: 0037-7722

Effective:

02/01/2025-02/01/2027

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG400303

Exp Date: 01/03/2026

Test	g/210L	Time
DIAG	Pass	11:44am
AIR BLK	.00	11:44am
ACCY CHK	.07	11:45am
AIR BLK	.00	11:46am
SUB TEST	.00	11:47am
AIR BLK	.00	11:48am
SUB TEST	.00	11:49am
AIR BLK	.00	11:50am

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

BEAUFORT COUNTY COURTHOUSE 060

Serial Number: 008586 Test Record Number: 2320
Test Date: 04/25/2025 Test Time: 11:51am EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	11:51am
FLO	Pass	11:51am
FC	Pass	11:51am

Temperature Tests

Test	Status	Time
FC1	Pass	11:52am
SRC	Pass	11:52am
DET	Pass	11:52am
BAR	Pass	11:52am
BT	Pass	11:52am

Blank Tests

Test	Status	Time
AIR	Pass	11:52am


Printer Tests

Test	Status	Time
PRNT	Pass	11:52am

CRC Tests

Test	Status	Time
COMP	Pass	11:52am
CAL	Pass	11:52am

Preventive Maintenance
Status: *Pass*



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Beaufort Instrument Location Beaufort Co. Courthouse
112 W. 2nd St., Washington, NC
Instrument Serial No. 008909

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 25th day of April, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

377722
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

BEAUFORT COUNTY COURTHOUSE 060

Serial Number: 008909

Test Date: 04/25/2025

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Gray, Kelly D

Permit Number: 0037-7722

Effective:

02/01/2025-02/01/2027

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG400303

Exp Date: 01/03/2026

Test	g/210L	Time
DIAG	Pass	11:41am
AIR BLK	.00	11:41am
ACCY CHK	.07	11:42am
AIR BLK	.00	11:43am
SUB TEST	.00	11:44am
AIR BLK	.00	11:45am
SUB TEST	.00	11:47am
AIR BLK	.00	11:47am

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

BEAUFORT COUNTY COURTHOUSE 060

Serial Number: 008909 Test Record Number: 4277
Test Date: 04/25/2025 Test Time: 11:49am EDT

System Check: Passed

Baseline Tests

Test	Status	Time
IR	Pass	11:49am
FLO	Pass	11:49am
FC	Pass	11:49am

Temperature Tests

Test	Status	Time
FC1	Pass	11:49am
SRC	Pass	11:49am
DET	Pass	11:49am
BAR	Pass	11:49am
BT	Pass	11:49am

Blank Tests

Test	Status	Time
AIR	Pass	11:50am

Printer Tests

Test	Status	Time
PRNT	Pass	11:50am

CRC Tests

Test	Status	Time
COMP	Pass	11:50am
CAL	Pass	11:50am

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Bertie Instrument Location Bertie Co. S.O.
Instrument Serial No. 008897 222 County Farm Rd
Windsor, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 1st day of April, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

206272
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

BERTIE COUNTY BERTIE CO SO 070

Serial Number: 008897
Test Date: 04/01/2025

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE

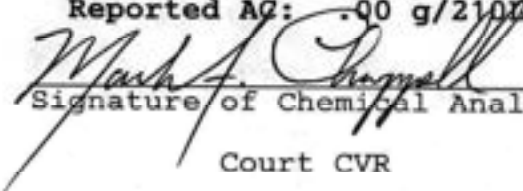
Analyst's Name: Chappell, Mark A
Permit Number: 0020-6272
Effective:
02/01/2025-02/01/2027

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG400303
Exp Date: 01/03/2026

Test	g/210L	Time
DIAG	Pass	10:04am
AIR BLK	.00	10:05am
ACCY CHK	.07	10:06am
AIR BLK	.00	10:07am
SUB TEST	.00	10:08am
AIR BLK	.00	10:09am
SUB TEST	.00	10:11am
AIR BLK	.00	10:11am

Reported AG: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

BERTIE COUNTY BERTIE CO SO 070

Serial Number: 008897 Test Record Number: 1664
Test Date: 04/01/2025 Test Time: 10:12am EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	10:13am
FLO	Pass	10:13am
FC	Pass	10:13am

Temperature Tests

Test	Status	Time
FC1	Pass	10:13am
SRC	Pass	10:13am
DET	Pass	10:13am
BAR	Pass	10:13am
BT	Pass	10:13am

Blank Tests

Test	Status	Time
AIR	Pass	10:14am

Printer Tests

Test	Status	Time
PRNT	Pass	10:14am

CRC Tests

Test	Status	Time
COMP	Pass	10:14am
CAL	Pass	10:14am

Preventive Maintenance
Status: Pass


Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Buncombe Instrument Location BAT Mobile Unit II
Instrument Serial No. 008970 Buncombe SD

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 12th day of April, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



John Lanier
Signature of Certifying Official

11604930
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

BUNCOMBE BAT MOBILE UNIT 11 100

Serial Number: 008970
Test Date: 04/12/2025

Citation Number: M0000000-0
Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Lanier Jr., John P

Permit Number: 4582-9118

Effective:

03/01/2025-03/01/2027

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

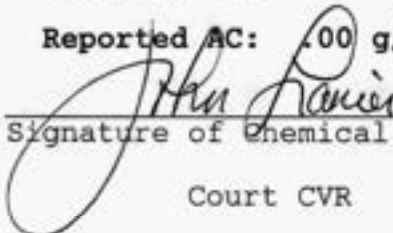
Test Type: Breath Test

Lot Number: AG417802

Exp Date: 06/26/2026

Test	g/210L	Time
DIAG	Pass	5:03pm
AIR BLK	.00	5:04pm
ACCY CHK	.08	5:05pm
AIR BLK	.00	5:05pm
SUB TEST	.00	5:06pm
AIR BLK	.00	5:07pm
SUB TEST	.00	5:08pm
AIR BLK	.00	5:09pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

BUNCOMBE BAT MOBILE UNIT 11 100

Serial Number: 008970 Test Record Number: 1190
Test Date: 04/12/2025 Test Time: 5:15pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	5:15pm
FLO	Pass	5:15pm
FC	Pass	5:15pm

Temperature Tests

Test	Status	Time
FC1	Pass	5:15pm
SRC	Pass	5:15pm
DET	Pass	5:15pm
BAR	Pass	5:15pm
BT	Pass	5:15pm

Blank Tests

Test	Status	Time
AIR	Pass	5:16pm

Printer Tests

Test	Status	Time
PRNT	Pass	5:16pm

CRC Tests

Test	Status	Time
COMP	Pass	5:16pm
CAL	Pass	5:16pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Buncombe Instrument Location BAT Mobile Unit II

Instrument Serial No. 008970 Buncombe SO

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 12th day of April, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



John Parier
Signature of Certifying Official

1104930
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

BUNCOMBE BAT MOBILE UNIT 11 100

Serial Number: 008970
Test Date: 04/12/2025

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE

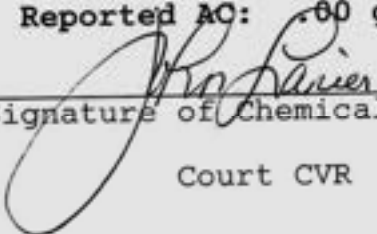
Analyst's Name: Lanier Jr., John P
Permit Number: 4582-9118
Effective:
03/01/2025-03/01/2027

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

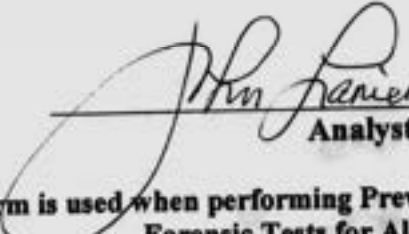
Lot Number: AG417802
Exp Date: 06/26/2026

Test	g/210L	Time
DIAG	Pass	6:47pm
AIR BLK	.00	6:48pm
ACCY CHK	.08	6:48pm
AIR BLK	.00	6:49pm
SUB TEST	.00	6:50pm
AIR BLK	.00	6:51pm
SUB TEST	.00	6:52pm
AIR BLK	.00	6:53pm

Reported AC: .60 g/210L



Signature of Chemical Analyst
Court CVR



Analyst

Intox EC/IR-II: Preventive Maintenance

BUNCOMBE BAT MOBILE UNIT 11 100

Serial Number: 008970 Test Record Number: 1192
Test Date: 04/12/2025 Test Time: 7:00pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	7:00pm
FLO	Pass	7:00pm
FC	Pass	7:00pm

Temperature Tests

Test	Status	Time
FC1	Pass	7:00pm
SRC	Pass	7:00pm
DET	Pass	7:00pm
BAR	Pass	7:00pm
BT	Pass	7:00pm

Blank Tests

Test	Status	Time
AIR	Pass	7:01pm

Printer Tests

Test	Status	Time
PRNT	Pass	7:01pm

CRC Tests

Test	Status	Time
COMP	Pass	7:01pm
CAL	Pass	7:01pm

Preventive Maintenance
Status: Pass



Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County Burcombe Instrument Location BAT Mobile Unit 11
Instrument Serial No. 008913 Burcombe SO

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 12th day of April, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Jeff G. [Signature]
Signature of Certifying Official

6-2446
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

BUNCOMBE BAT MOBILE UNIT 11 100

Serial Number: 008973

Test Date: 04/12/2025

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Gillstrap, Jeffrey L

Permit Number: 6-2446

Effective:

12/01/2023-12/01/2025

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG431003

Exp Date: 11/05/2026

Test	g/210L	Time
DIAG	Pass	5:17pm
AIR BLK	.00	5:18pm
ACCY CHK	.07	5:18pm
AIR BLK	.00	5:19pm
SUB TEST	.00	5:20pm
AIR BLK	.00	5:21pm
SUB TEST	.00	5:22pm
AIR BLK	.00	5:23pm

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR


Analyst

Intox EC/IR-II: Preventive Maintenance

BUNCOMBE BAT MOBILE UNIT 11 100

Serial Number: 008973

Test Record Number: 1241

Test Date: 04/12/2025

Test Time: 5:30pm EDT

System Check: Passed

Baseline Tests

Test	Status	Time
IR	Pass	5:30pm
FLO	Pass	5:30pm
FC	Pass	5:30pm

Temperature Tests

Test	Status	Time
FC1	Pass	5:30pm
SRC	Pass	5:30pm
DET	Pass	5:30pm
BAR	Pass	5:30pm
BT	Pass	5:30pm

Blank Tests

Test	Status	Time
AIR	Pass	5:31pm

Printer Tests

Test	Status	Time
PRNT	Pass	5:31pm

CRC Tests

Test	Status	Time
COMP	Pass	5:31pm
CAL	Pass	5:31pm

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Buncombe Instrument Location BAT Mobile Unit II
Instrument Serial No. 008973 Buncombe SD

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 12th day of April, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

6-2446
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

BUNCOMBE BAT MOBILE UNIT 11 100

Serial Number: 008973

Test Date: 04/12/2025

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Gillstrap, Jeffrey L

Permit Number: 6-2446

Effective:

12/01/2023-12/01/2025

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG431003

Exp Date: 11/05/2026

Test	g/210L	Time
DIAG	Pass	6:57pm
AIR BLK	.00	6:58pm
ACCY CHK	.07	6:59pm
AIR BLK	.00	7:00pm
SUB TEST	.00	7:00pm
AIR BLK	.00	7:01pm
SUB TEST	.00	7:03pm
AIR BLK	.00	7:03pm

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR


Analyst

Intox EC/IR-II: Preventive Maintenance

BUNCOMBE BAT MOBILE UNIT 11 100

Serial Number: 008973

Test Record Number: 1244

Test Date: 04/12/2025

Test Time: 7:10pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	7:11pm
FLO	Pass	7:11pm
FC	Pass	7:11pm

Temperature Tests

Test	Status	Time
FC1	Pass	7:11pm
SRC	Pass	7:11pm
DET	Pass	7:11pm
BAR	Pass	7:11pm
BT	Pass	7:11pm

Blank Tests

Test	Status	Time
AIR	Pass	7:11pm

Printer Tests

Test	Status	Time
PRNT	Pass	7:12pm

CRC Tests

Test	Status	Time
COMP	Pass	7:12pm
CAL	Pass	7:12pm

Preventive Maintenance
Status: *Pass*


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Cabarrus Instrument Location Cabarrus County 80
Instrument Serial No. 008590 Concord, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 4th day of April, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Boyp Helms
Signature of Certifying Official

849845
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

CABARRUS COUNTY CABARRUS COUNTY SO 120

Serial Number: 008590
Test Date: 04/04/2025

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE

Analyst's Name: Helms, Bryce A
Permit Number: 0084-9845
Effective:
02/01/2025-02/01/2027

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG417802
Exp Date: 06/26/2026

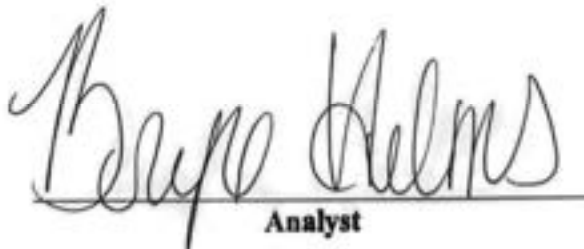
Test	g/210L	Time
DIAG	Pass	11:16am
AIR BLK	.00	11:17am
ACCY CHK	.08	11:17am
AIR BLK	.00	11:19am
SUB TEST	.00	11:20am
AIR BLK	.00	11:21am
SUB TEST	.00	11:22am
AIR BLK	.00	11:23am

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

Intox EC/IR-II: Preventive Maintenance

CABARRUS COUNTY CABARRUS COUNTY SO 120

Serial Number: 008590 Test Record Number: 5387
Test Date: 04/04/2025 Test Time: 11:43am EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	11:44am
FLO	Pass	11:44am
FC	Pass	11:44am

Temperature Tests

Test	Status	Time
FC1	Pass	11:44am
SRC	Pass	11:44am
DET	Pass	11:44am
BAR	Pass	11:44am
BT	Pass	11:44am

Blank Tests

Test	Status	Time
AIR	Pass	11:45am

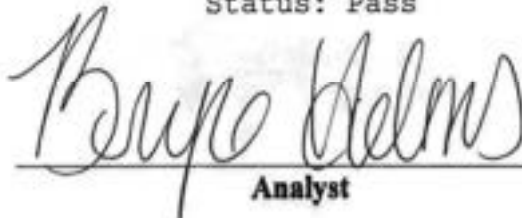
Printer Tests

Test	Status	Time
PRNT	Pass	11:45am

CRC Tests

Test	Status	Time
COMP	Pass	11:45am
CAL	Pass	11:45am

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County CABARRUS Instrument Location BAT MOBILE UNIT 8
Instrument Serial No. 008615 KANNAPOLIS PD

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 10 day of April, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

2219283
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

CABARRUS COUNTY BAT MOBILE UNIT 8 120

Serial Number: 008615
Test Date: 04/10/2025

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Glasscock, Jerry D

Permit Number: 7180-9235

Effective:

02/01/2025-02/01/2027

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG405102

Exp Date: 02/20/2026

Test	g/210L	Time
DIAG	Pass	7:16pm
AIR BLK	.00	7:17pm
ACCY CHK	.07	7:17pm
AIR BLK	.00	7:18pm
SUB TEST	.00	7:19pm
AIR BLK	.00	7:20pm
SUB TEST	.00	7:22pm
AIR BLK	.00	7:23pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

CABARRUS COUNTY BAT MOBILE UNIT 8 120

Serial Number: 008615 Test Record Number: 6058
Test Date: 04/10/2025 Test Time: 7:24pm EDT

System Check: Passed

Baseline Tests

Test	Status	Time
IR	Pass	7:24pm
FLO	Pass	7:24pm
FC	Pass	7:24pm

Temperature Tests

Test	Status	Time
FC1	Pass	7:24pm
SRC	Pass	7:24pm
DET	Pass	7:24pm
BAR	Pass	7:24pm
BT	Pass	7:24pm

Blank Tests

Test	Status	Time
AIR	Pass	7:25pm


Printer Tests

Test	Status	Time
PRNT	Pass	7:25pm

CRC Tests

Test	Status	Time
COMP	Pass	7:25pm
CAL	Pass	7:25pm

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Cabarrus Instrument Location Cabarrus County 80
Instrument Serial No. 008625 Concord, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 4th day of April, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Boyo Helms
Signature of Certifying Official

849845
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

CABARRUS COUNTY CABARRUS COUNTY SO 120

Serial Number: 008625
Test Date: 04/04/2025

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Helms, Bryce A

Permit Number: 0084-9845

Effective:

02/01/2025-02/01/2027

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG417802

Exp Date: 06/26/2026

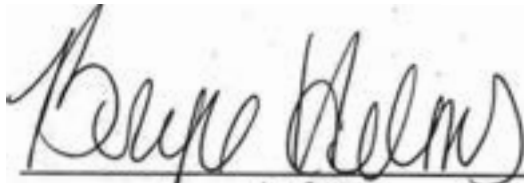
Test	g/210L	Time
DIAG	Pass	11:53am
AIR BLK	.00	11:54am
ACCY CHK	.07	11:55am
AIR BLK	.00	11:56am
SUB TEST	.00	11:57am
AIR BLK	.00	11:58am
SUB TEST	.00	11:59am
AIR BLK	.00	12:00pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

Intox EC/IR-II: Preventive Maintenance

CABARRUS COUNTY CABARRUS COUNTY SO '120

Serial Number: 008625 Test Record Number: 7094
Test Date: 04/04/2025 Test Time: 12:01pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	12:02pm
FLO	Pass	12:02pm
FC	Pass	12:02pm

Temperature Tests

Test	Status	Time
FC1	Pass	12:02pm
SRC	Pass	12:02pm
DET	Pass	12:02pm
BAR	Pass	12:02pm
BT	Pass	12:02pm

Blank Tests

Test	Status	Time
AIR	Pass	12:03pm

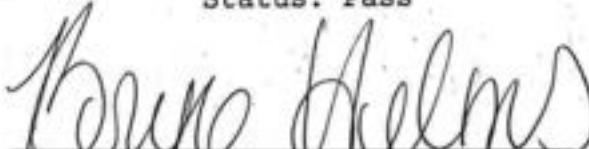
Printer Tests

Test	Status	Time
PRNT	Pass	12:03pm

CRC Tests

Test	Status	Time
COMP	Pass	12:03pm
CAL	Pass	12:03pm

Preventive Maintenance
Status: *Pass*



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County CABARRUS Instrument Location BAT MOBILE UNIT 8
Instrument Serial No. 008736 KANNAPOLIS PD

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 10 day of April, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

2219283
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

CABARRUS COUNTY BAT MOBILE UNIT 8 120

Serial Number: 008736
Test Date: 04/10/2025

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE

Analyst's Name: Glasscock, Jerry D
Permit Number: 7180-9235
Effective:
02/01/2025-02/01/2027

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG405102
Exp Date: 02/20/2026

Test	g/210L	Time
DIAG	Pass	7:16pm
AIR BLK	.00	7:17pm
ACCY CHK	.08	7:18pm
AIR BLK	.00	7:19pm
SUB TEST	.00	7:19pm
AIR BLK	.00	7:20pm
SUB TEST	.00	7:22pm
AIR BLK	.00	7:22pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

Intox EC/IR-II: Preventive Maintenance

CABARRUS COUNTY BAT MOBILE UNIT 8 120

Serial Number: 008736 Test Record Number: 1412
Test Date: 04/10/2025 Test Time: 7:37pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	7:38pm
FLO	Pass	7:38pm
FC	Pass	7:38pm

Temperature Tests

Test	Status	Time
FC1	Pass	7:38pm
SRC	Pass	7:38pm
DET	Pass	7:38pm
BAR	Pass	7:38pm
BT	Pass	7:38pm

Blank Tests

Test	Status	Time
AIR	Pass	7:38pm

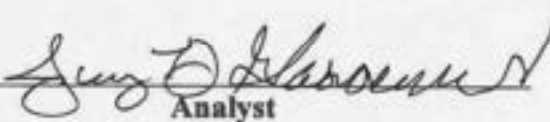
Printer Tests

Test	Status	Time
PRNT	Pass	7:39pm

CRC Tests

Test	Status	Time
COMP	Pass	7:39pm
CAL	Pass	7:39pm

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County Cabarrus Instrument Location BAT Mobile Unit 8
Instrument Serial No. 008775 KANNAPOLIS PD

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 10 day of April, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature] 2219283
Signature of Certifying Official Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

CABARRUS COUNTY BAT MOBILE UNIT 8 120

Serial Number: 008775
Test Date: 04/10/2025

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: Glasscock, Jerry D
Permit Number: 7180-9235
Effective:
02/01/2025-02/01/2027

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

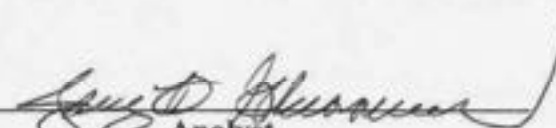
Lot Number: AG431002
Exp Date: 11/05/2026

Test	g/210L	Time
DIAG	Pass	7:14pm
AIR BLK	.00	7:15pm
ACCY CHK	.07	7:15pm
AIR BLK	.00	7:16pm
SUB TEST	.00	7:17pm
AIR BLK	.00	7:18pm
SUB TEST	.00	7:19pm
AIR BLK	.00	7:20pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

Intox EC/IR-II: Preventive Maintenance

CABARRUS COUNTY BAT MOBILE UNIT 8 120

Serial Number: 008775 Test Record Number: 2260
Test Date: 04/10/2025 Test Time: 7:21pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	7:21pm
FLO	Pass	7:21pm
FC	Pass	7:21pm

Temperature Tests

Test	Status	Time
FC1	Pass	7:22pm
SRC	Pass	7:22pm
DET	Pass	7:22pm
BAR	Pass	7:22pm
BT	Pass	7:22pm

Blank Tests

Test	Status	Time
AIR	Pass	7:23pm

Printer Tests

Test	Status	Time
PRNT	Pass	7:23pm

CRC Tests

Test	Status	Time
COMP	Pass	7:23pm
CAL	Pass	7:23pm

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Cabarrus Instrument Location Cabarrus County 80
Instrument Serial No. 008792 Concord, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 4th day of April, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

849845
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

CABARRUS COUNTY CABARRUS COUNTY SO 120

Serial Number: 008792
Test Date: 04/04/2025

Citation Number: M0000000-0
Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Helms, Bryce A

Permit Number: 0084-9845

Effective:

02/01/2025-02/01/2027

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG405103

Exp Date: 02/20/2026

Test	g/210L	Time
DIAG	Pass	11:14am
AIR BLK	.00	11:14am
ACCY CHK	.08	11:15am
AIR BLK	.00	11:17am
SUB TEST	.00	11:18am
AIR BLK	.00	11:18am
SUB TEST	.00	11:20am
AIR BLK	.00	11:21am

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR


Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

CABARRUS COUNTY CABARRUS COUNTY SO 120

Serial Number: 008792 Test Record Number: 4519
Test Date: 04/04/2025 Test Time: 11:22am EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	11:22am
FLO	Pass	11:22am
FC	Pass	11:23am

Temperature Tests

Test	Status	Time
FC1	Pass	11:23am
SRC	Pass	11:23am
DET	Pass	11:23am
BAR	Pass	11:23am
BT	Pass	11:23am

Blank Tests

Test	Status	Time
AIR	Pass	11:23am

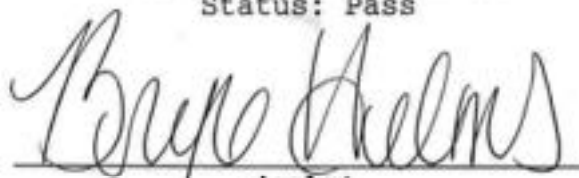
Printer Tests

Test	Status	Time
PRNT	Pass	11:23am

CRC Tests

Test	Status	Time
COMP	Pass	11:23am
CAL	Pass	11:23am

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County CABARRUS Instrument Location BAT MOBILE UNIT 8
Instrument Serial No. 008816 KANNAPOLIS PD

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 10 day of April, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature] 2219283
Signature of Certifying Official Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

CABARRUS COUNTY BAT MOBILE UNIT 8 120

Serial Number: 008816
Test Date: 04/10/2025

Citation Number: M0000000-0
Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Glasscock, Jerry D

Permit Number: 7180-9235

Effective:

02/01/2025-02/01/2027

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG431002

Exp Date: 11/05/2026

Test	g/210L	Time
DIAG	Pass	7:15pm
AIR BLK	.00	7:16pm
ACCY CHK	.08	7:16pm
AIR BLK	.00	7:17pm
SUB TEST	.00	7:18pm
AIR BLK	.00	7:19pm
SUB TEST	.00	7:20pm
AIR BLK	.00	7:21pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

Intox EC/IR-II: Preventive Maintenance

CABARRUS COUNTY BAT MOBILE UNIT 8 120

Serial Number: 008816 Test Record Number: 7849
Test Date: 04/10/2025 Test Time: 7:23pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	7:23pm
FLO	Pass	7:23pm
FC	Pass	7:24pm

Temperature Tests

Test	Status	Time
FC1	Pass	7:24pm
SRC	Pass	7:24pm
DET	Pass	7:24pm
BAR	Pass	7:24pm
BT	Pass	7:24pm

Blank Tests

Test	Status	Time
AIR	Pass	7:24pm

Printer Tests

Test	Status	Time
PRNT	Pass	7:24pm

CRC Tests

Test	Status	Time
COMP	Pass	7:24pm
CAL	Pass	7:24pm

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County CABARRUS Instrument Location BAT MOBILE UNIT 8
Instrument Serial No. 008929 KANNAPOLIS PD

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 10 day of April, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

2219283
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

CABARRUS COUNTY BAT MOBILE UNIT 8 120

Serial Number: 008929

Test Date: 04/10/2025

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Glasscock, Jerry D

Permit Number: 7180-9235

Effective:

02/01/2025-02/01/2027

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG506303


Exp Date: 03/04/2027

Test	g/210L	Time
DIAG	Pass	7:15pm
AIR BLK	.00	7:17pm
ACCY CHK	.07	7:17pm
AIR BLK	.00	7:19pm
SUB TEST	.00	7:19pm
AIR BLK	.00	7:20pm
SUB TEST	.00	7:22pm
AIR BLK	.00	7:23pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

CABARRUS COUNTY BAT MOBILE UNIT 8 120

Serial Number: 008929 Test Record Number: 1549
Test Date: 04/10/2025 Test Time: 7:25pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	7:25pm
FLO	Pass	7:25pm
FC	Pass	7:25pm

Temperature Tests

Test	Status	Time
FC1	Pass	7:25pm
SRC	Pass	7:25pm
DET	Pass	7:25pm
BAR	Pass	7:25pm
BT	Pass	7:25pm

Blank Tests

Test	Status	Time
AIR	Pass	7:26pm


Printer Tests

Test	Status	Time
PRNT	Pass	7:26pm

CRC Tests

Test	Status	Time
COMP	Pass	7:26pm
CAL	Pass	7:26pm

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County CALDWELL Instrument Location CALDWELL CO JAIL

Instrument Serial No. 008719 LE 1010 NR

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 01 day of APRIL, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

214970
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

CALDWELL COUNTY CALDWELL COUNTY JAIL
130

Serial Number: 008719
Test Date: 04/01/2025

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: Fleming, Tina S
Permit Number: 0027-4970
Effective:
10/01/2023-10/01/2025

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG431001
Exp Date: 11/05/2026

Test	g/210L	Time
DIAG	Pass	11:00am
AIR BLK	.00	11:00am
ACCY CHK	.08	11:01am
AIR BLK	.00	11:02am
SUB TEST	.00	11:03am
AIR BLK	.00	11:03am
SUB TEST	.00	11:05am
AIR BLK	.00	11:06am

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

Intox EC/IR-II: Preventive Maintenance

CALDWELL COUNTY CALDWELL COUNTY JAIL 130

Serial Number: 008719 Test Record Number: 3483
Test Date: 04/01/2025 Test Time: 11:07am EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	11:07am
FLO	Pass	11:07am
FC	Pass	11:07am

Temperature Tests

Test	Status	Time
FC1	Pass	11:07am
SRC	Pass	11:07am
DET	Pass	11:07am
BAR	Pass	11:07am
BT	Pass	11:07am

Blank Tests

Test	Status	Time
AIR	Pass	11:08am


Printer Tests

Test	Status	Time
PRNT	Pass	11:08am

CRC Tests

Test	Status	Time
COMP	Pass	11:08am
CAL	Pass	11:08am

Preventive Maintenance
Status: Pass



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Chowan Instrument Location Chowan Co Public Safety Center
Instrument Serial No. 008895 305 Freeman St. Edenton, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 21st day of April, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



M. J. Russell
Signature of Certifying Official

202272
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

CHOWAN COUNTY PUBLIC SAFETY CENTER 200

Serial Number: 008895
Test Date: 04/21/2025

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Chappell, Mark A

Permit Number: 0020-6272

Effective:

02/01/2025-02/01/2027

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG431001


Exp Date: 11/05/2026

Test	g/210L	Time
DIAG	Pass	9:51am
AIR BLK	.00	9:51am
ACCY CHK	.07	9:52am
AIR BLK	.00	9:53am
SUB TEST	.00	9:54am
AIR BLK	.00	9:55am
SUB TEST	.00	9:56am
AIR BLK	.00	9:57am

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

CHOWAN COUNTY PUBLIC SAFETY CENTER 200

Serial Number: 008895 Test Record Number: 1253
Test Date: 04/21/2025 Test Time: 9:58am EDT

System Check: Passed

Baseline Tests

Test	Status	Time
IR	Pass	9:58am
FLO	Pass	9:58am
FC	Pass	9:59am

Temperature Tests

Test	Status	Time
FC1	Pass	9:59am
SRC	Pass	9:59am
DET	Pass	9:59am
BAR	Pass	9:59am
BT	Pass	9:59am

Blank Tests

Test	Status	Time
AIR	Pass	9:59am

Printer Tests

Test	Status	Time
PRNT	Pass	9:59am

CRC Tests

Test	Status	Time
COMP	Pass	9:59am
CAL	Pass	9:59am

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Columbus Instrument Location BAT Mobile Unit 10

Instrument Serial No. 008584 Columbus County SO

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 11th day of Apr:1, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

2266313
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

COLUMBUS COUNTY BAT MOBILE UNIT 10 230

Serial Number: 008584

Test Date: 04/11/2025

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Sharpe Jr., Robert J

Permit Number: 1820-8591

Effective:

02/01/2025-02/01/2027

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG400303


Exp Date: 01/03/2026

Test	g/210L	Time
DIAG	Pass	8:26pm
AIR BLK	.00	8:27pm
ACCY CHK	.07	8:27pm
AIR BLK	.00	8:28pm
SUB TEST	.00	8:29pm
AIR BLK	.00	8:29pm
SUB TEST	.00	8:32pm
AIR BLK	.00	8:32pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

Intox EC/IR-II: Preventive Maintenance

COLUMBUS COUNTY BAT MOBILE UNIT 10 230

Serial Number: 008584 Test Record Number: 2778
Test Date: 04/11/2025 Test Time: 8:33pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	8:33pm
FLO	Pass	8:33pm
FC	Pass	8:33pm

Temperature Tests

Test	Status	Time
FC1	Pass	8:34pm
SRC	Pass	8:34pm
DET	Pass	8:34pm
BAR	Pass	8:34pm
BT	Pass	8:34pm

Blank Tests

Test	Status	Time
AIR	Pass	8:34pm

Printer Tests

Test	Status	Time
PRNT	Pass	8:34pm

CRC Tests

Test	Status	Time
COMP	Pass	8:34pm
CAL	Pass	8:34pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Columbus Instrument Location BAT Mobile Unit 10
Instrument Serial No. 008637 Columbus County SO

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 11th day of April, 20 25 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

2266313
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

COLUMBUS COUNTY BAT MOBILE UNIT 10 230

Serial Number: 008637

Test Date: 04/11/2025

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Sharpe Jr., Robert J

Permit Number: 1820-8591

Effective:

02/01/2025-02/01/2027

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG400303

Exp Date: 01/03/2026

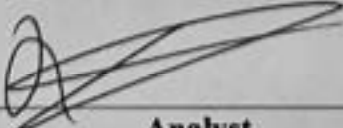
Test	g/210L	Time
DIAG	Pass	8:28pm
AIR BLK	.00	8:29pm
ACCY CHK	.08	8:30pm
AIR BLK	.00	8:31pm
SUB TEST	.00	8:32pm
AIR BLK	.00	8:33pm
SUB TEST	.00	8:34pm
AIR BLK	.00	8:35pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

This form is used when performing Preventive Maintenance procedures

Forensic Tests for Alcohol Branch

Department of Health and Human Services

Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

COLUMBUS COUNTY BAT MOBILE UNIT 10 230

Serial Number: 008637 Test Record Number: 3512
Test Date: 04/11/2025 Test Time: 8:36pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	8:36pm
FLO	Pass	8:36pm
FC	Pass	8:36pm

Temperature Tests

Test	Status	Time
FC1	Pass	8:36pm
SRC	Pass	8:36pm
DET	Pass	8:36pm
BAR	Pass	8:36pm
BT	Pass	8:36pm

Blank Tests

Test	Status	Time
AIR	Pass	8:37pm

Printer Tests

Test	Status	Time
PRNT	Pass	8:37pm

CRC Tests

Test	Status	Time
COMP	Pass	8:37pm
CAL	Pass	8:37pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Columbus Instrument Location BAT Mobile Unit 10

Instrument Serial No. 00 8686 Columbus County SO

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 11th day of April, 20 25 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.




Signature of Certifying Official

2266313
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

COLUMBUS COUNTY BAT MOBILE UNIT 10 230

Serial Number: 008686
Test Date: 04/11/2025

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Sharpe Jr., Robert J

Permit Number: 1820-8591

Effective:

02/01/2025-02/01/2027

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG506302

Exp Date: 03/04/2027


Test	g/210L	Time
DIAG	Pass	8:27pm
AIR BLK	.00	8:28pm
ACCY CHK	.08	8:28pm
AIR BLK	.00	8:29pm
SUB TEST	.00	8:31pm
AIR BLK	.00	8:32pm
SUB TEST	.00	8:33pm
AIR BLK	.00	8:34pm

Reported AC: 00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

Intox EC/IR-II: Preventive Maintenance

COLUMBUS COUNTY BAT MOBILE UNIT 10 230

Serial Number: 008686 Test Record Number: 7140
Test Date: 04/11/2025 Test Time: 8:34pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	8:35pm
FLO	Pass	8:35pm
FC	Pass	8:35pm

Temperature Tests

Test	Status	Time
FC1	Pass	8:35pm
SRC	Pass	8:35pm
DET	Pass	8:35pm
BAR	Pass	8:35pm
BT	Pass	8:35pm

Blank Tests

Test	Status	Time
AIR	Pass	8:35pm

Printer Tests

Test	Status	Time
PRNT	Pass	8:36pm

CRC Tests

Test	Status	Time
COMP	Pass	8:36pm
CAL	Pass	8:36pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Columbus Instrument Location BAT Mobile Unit 10
Instrument Serial No. 008776 Columbus County SO

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 11th day of April, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]

Signature of Certifying Official

2266313

Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

COLUMBUS COUNTY BAT MOBILE UNIT 10 230

Serial Number: 008776
Test Date: 04/11/2025

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Sharpe Jr., Robert J

Permit Number: 1820-8591

Effective:

02/01/2025-02/01/2027

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG417803


Exp Date: 06/26/2026

Test	g/210L	Time
DIAG	Pass	8:32pm
AIR BLK	.00	8:33pm
ACCY CHK	.08	8:33pm
AIR BLK	.00	8:34pm
SUB TEST	.00	8:35pm
AIR BLK	.00	8:36pm
SUB TEST	.00	8:37pm
AIR BLK	.00	8:38pm

Reported AC: ~~00~~ g/210L

Signature  of Chemical Analyst

Court CVR



Analyst

Intox EC/IR-II: Preventive Maintenance

COLUMBUS COUNTY BAT MOBILE UNIT 10 230

Serial Number: 008776 Test Record Number: 4098
Test Date: 04/11/2025 Test Time: 8:39pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	8:39pm
FLO	Pass	8:39pm
FC	Pass	8:39pm

Temperature Tests

Test	Status	Time
FC1	Pass	8:39pm
SRC	Pass	8:39pm
DET	Pass	8:39pm
BAR	Pass	8:39pm
BT	Pass	8:39pm

Blank Tests

Test	Status	Time
AIR	Pass	8:40pm


Printer Tests

Test	Status	Time
PRNT	Pass	8:40pm

CRC Tests

Test	Status	Time
COMP	Pass	8:40pm
CAL	Pass	8:40pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Columbus Instrument Location BAT Mobile Unit 10
Instrument Serial No. 008779 Columbus County SO

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 11th day of April, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

2266313
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

COLUMBUS COUNTY BAT MOBILE UNIT 10 230

Serial Number: 008779
Test Date: 04/11/2025

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Sharpe Jr., Robert J

Permit Number: 1820-8591

Effective:

02/01/2025-02/01/2027

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG431002

Exp Date: 11/05/2026

Test	g/210L	Time
DIAG	Pass	8:30pm
AIR BLK	.00	8:31pm
ACCY CHK	.07	8:32pm
AIR BLK	.00	8:33pm
SUB TEST	.00	8:33pm
AIR BLK	.00	8:34pm
SUB TEST	.00	8:35pm
AIR BLK	.00	8:36pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

Intox EC/IR-II: Preventive Maintenance

COLUMBUS COUNTY BAT MOBILE UNIT 10 230

Serial Number: 008779 Test Record Number: 4045

Test Date: 04/11/2025 Test Time: 8:40pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	8:40pm
FLO	Pass	8:40pm
FC	Pass	8:40pm

Temperature Tests

Test	Status	Time
FC1	Pass	8:40pm
SRC	Pass	8:40pm
DET	Pass	8:40pm
BAR	Pass	8:40pm
BT	Pass	8:40pm

Blank Tests

Test	Status	Time
AIR	Pass	8:41pm

Printer Tests

Test	Status	Time
PRNT	Pass	8:41pm

CRC Tests

Test	Status	Time
COMP	Pass	8:41pm
CAL	Pass	8:41pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Craven Instrument Location BAT Mobile Unit 10

Instrument Serial No. 008584 Craven County SO

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 12th day of April, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]

Signature of Certifying Official

2266313

Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

CRAVEN COUNTY BAT MOBILE UNIT 10 240

Serial Number: 008584
Test Date: 04/12/2025

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Sharpe Jr., Robert J

Permit Number: 1820-8591

Effective:

02/01/2025-02/01/2027

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG400303


Exp Date: 01/03/2026

Test	g/210L	Time
DIAG	Pass	10:24pm
AIR BLK	.00	10:25pm
ACCY CHK	.07	10:26pm
AIR BLK	.00	10:26pm
SUB TEST	.00	10:27pm
AIR BLK	.00	10:28pm
SUB TEST	.00	10:30pm
AIR BLK	.00	10:31pm

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR



Analyst

Intox EC/IR-II: Preventive Maintenance

CRAVEN COUNTY BAT MOBILE UNIT 10 240

Serial Number: 008584 Test Record Number: 2780
Test Date: 04/12/2025 Test Time: 10:31pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	10:32pm
FLO	Pass	10:32pm
FC	Pass	10:32pm

Temperature Tests

Test	Status	Time
FC1	Pass	10:32pm
SRC	Pass	10:32pm
DET	Pass	10:32pm
BAR	Pass	10:32pm
BT	Pass	10:32pm

Blank Tests

Test	Status	Time
AIR	Pass	10:32pm

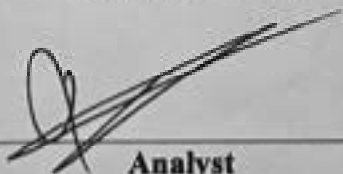
Printer Tests

Test	Status	Time
PRNT	Pass	10:32pm

CRC Tests

Test	Status	Time
COMP	Pass	10:33pm
CAL	Pass	10:33pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Craven Instrument Location BAT Mobile Unit 10
Instrument Serial No. 008637 Craven County SO

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 12th day of April, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

2266313
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

CRAVEN COUNTY BAT MOBILE UNIT 10 240

Serial Number: 008637

Test Date: 04/12/2025

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Sharpe Jr., Robert J

Permit Number: 1820-8591

Effective:

02/01/2025-02/01/2027

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG400303


Exp Date: 01/03/2026

Test	g/210L	Time
DIAG	Pass	10:26pm
AIR BLK	.00	10:27pm
ACCY CHK	.08	10:28pm
AIR BLK	.00	10:29pm
SUB TEST	.00	10:29pm
AIR BLK	.00	10:30pm
SUB TEST	.00	10:32pm
AIR BLK	.00	10:33pm

Reported AC: ~~00~~ g/210L

Signature of Chemical Analyst

Court CVR


Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

CRAVEN COUNTY BAT MOBILE UNIT 10 240

Serial Number: 008637 Test Record Number: 3514
Test Date: 04/12/2025 Test Time: 10:33pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	10:34pm
FLO	Pass	10:34pm
FC	Pass	10:34pm

Temperature Tests

Test	Status	Time
FC1	Pass	10:34pm
SRC	Pass	10:34pm
DET	Pass	10:34pm
BAR	Pass	10:34pm
BT	Pass	10:34pm

Blank Tests

Test	Status	Time
AIR	Pass	10:35pm

Printer Tests

Test	Status	Time
PRNT	Pass	10:35pm

CRC Tests

Test	Status	Time
COMP	Pass	10:35pm
CAL	Pass	10:35pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Craven Instrument Location BAT Mobile Unit 10
Instrument Serial No. 008686 Craven County SO

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 12th day of April, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

2266313
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

CRAVEN COUNTY BAT MOBILE UNIT 10 240

Serial Number: 008686
Test Date: 04/12/2025

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Sharpe Jr., Robert J

Permit Number: 1820-8591

Effective:

02/01/2025-02/01/2027

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG506302

Exp Date: 03/04/2027

Test	g/210L	Time
DIAG	Pass	10:25pm
AIR BLK	.00	10:26pm
ACCY CHK	.08	10:26pm
AIR BLK	.00	10:27pm
SUB TEST	.00	10:28pm
AIR BLK	.00	10:29pm
SUB TEST	.00	10:31pm
AIR BLK	.00	10:31pm

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR

Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

CRAVEN COUNTY BAT MOBILE UNIT 10 240

Serial Number: 008686 Test Record Number: 7142
Test Date: 04/12/2025 Test Time: 10:32pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	10:32pm
FLO	Pass	10:32pm
FC	Pass	10:33pm

Temperature Tests

Test	Status	Time
FC1	Pass	10:33pm
SRC	Pass	10:33pm
DET	Pass	10:33pm
BAR	Pass	10:33pm
BT	Pass	10:33pm

Blank Tests

Test	Status	Time
AIR	Pass	10:33pm

Printer Tests

Test	Status	Time
PRNT	Pass	10:33pm

CRC Tests

Test	Status	Time
COMP	Pass	10:33pm
CAL	Pass	10:33pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Craven Instrument Location BAT Mobile Unit 10
Instrument Serial No. 00 8776 Craven County SO

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 12th day of April, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

2266313
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

CRAVEN COUNTY BAT MOBILE UNIT 10 240

Serial Number: 008776

Test Date: 04/12/2025

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Sharpe Jr., Robert J

Permit Number: 1820-8591

Effective:

02/01/2025-02/01/2027

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG417803

Exp Date: 06/26/2026

Test	g/210L	Time
DIAG	Pass	10:28pm
AIR BLK	.00	10:29pm
ACCY CHK	.08	10:29pm
AIR BLK	.00	10:30pm
SUB TEST	.00	10:31pm
AIR BLK	.00	10:32pm
SUB TEST	.00	10:33pm
AIR BLK	.00	10:34pm

Reported AQ: .00 g/210L

Signature of Chemical Analyst

Court CVR


Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

CRAVEN COUNTY BAT MOBILE UNIT 10 240

Serial Number: 008776 Test Record Number: 4100
Test Date: 04/12/2025 Test Time: 10:35pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	10:35pm
FLO	Pass	10:35pm
FC	Pass	10:35pm

Temperature Tests

Test	Status	Time
FC1	Pass	10:35pm
SRC	Pass	10:35pm
DET	Pass	10:35pm
BAR	Pass	10:35pm
BT	Pass	10:35pm

Blank Tests

Test	Status	Time
AIR	Pass	10:36pm

Printer Tests

Test	Status	Time
PRNT	Pass	10:36pm

CRC Tests

Test	Status	Time
COMP	Pass	10:36pm
CAL	Pass	10:36pm

**Preventive Maintenance
Status: Pass**



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Craven Instrument Location BAT Mobile Unit 10
Instrument Serial No. 008779 Craven County SO

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 12th day of April, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

2266313
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

CRAVEN COUNTY BAT MOBILE UNIT 10 240

Serial Number: 008779

Test Date: 04/12/2025

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Sharpe Jr., Robert J

Permit Number: 1820-8591

Effective:

02/01/2025-02/01/2027

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG431002


Exp Date: 11/05/2026

Test	g/210L	Time
DIAG	Pass	10:28pm
AIR BLK	.00	10:29pm
ACCY CHK	.07	10:29pm
AIR BLK	.00	10:30pm
SUB TEST	.00	10:31pm
AIR BLK	.00	10:32pm
SUB TEST	.00	10:33pm
AIR BLK	.00	10:34pm

Reported AC: .00 g/210L

Signature  Chemical Analyst

Court CVR


Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

CRAVEN COUNTY BAT MOBILE UNIT 10 240

Serial Number: 008779 Test Record Number: 4047
Test Date: 04/12/2025 Test Time: 10:35pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	10:35pm
FLO	Pass	10:35pm
FC	Pass	10:35pm

Temperature Tests

Test	Status	Time
FC1	Pass	10:35pm
SRC	Pass	10:35pm
DET	Pass	10:35pm
BAR	Pass	10:35pm
BT	Pass	10:35pm

Blank Tests

Test	Status	Time
AIR	Pass	10:36pm

Printer Tests

Test	Status	Time
PRNT	Pass	10:36pm

CRC Tests

Test	Status	Time
COMP	Pass	10:36pm
CAL	Pass	10:36pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Cumberland Instrument Location Cumberland County
Instrument Serial No. 008632 Detention Center

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 1 day of April, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

365156
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

CUMBERLAND COUNTY DETENTION CENTER 250

Serial Number: 008632
Test Date: 04/01/2025

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: Garner, Joel K
Permit Number: 0036-5156
Effective:
02/01/2025-02/01/2027

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG417803
Exp Date: 06/26/2026


Test	g/210L	Time
DIAG	Pass	10:14am
AIR BLK	.00	10:15am
ACCY CHK	.07	10:16am
AIR BLK	.00	10:17am
SUB TEST	.00	10:17am
AIR BLK	.00	10:18am
SUB TEST	.00	10:21am
AIR BLK	.00	10:21am

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

Intox EC/IR-II: Preventive Maintenance

CUMBERLAND COUNTY DETENTION CENTER 250

Serial Number: 008632 Test Record Number: 4829
Test Date: 04/01/2025 Test Time: 10:22am EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	10:22am
FLO	Pass	10:22am
FC	Pass	10:22am

Temperature Tests

Test	Status	Time
FC1	Pass	10:23am
SRC	Pass	10:23am
DET	Pass	10:23am
BAR	Pass	10:23am
BT	Pass	10:23am

Blank Tests

Test	Status	Time
AIR	Pass	10:23am

Printer Tests

Test	Status	Time
PRNT	Pass	10:23am

CRC Tests

Test	Status	Time
COMP	Pass	10:23am
CAL	Pass	10:23am

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County Cumberland Instrument Location Cumberland County
Instrument Serial No. 008633 Detention Center

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 1 day of April, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

365156
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

CUMBERLAND COUNTY DETENTION CENTER 250

Serial Number: 008633
Test Date: 04/01/2025

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: Garner, Joel K
Permit Number: 0036-5156
Effective:
02/01/2025-02/01/2027

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG417803
Exp Date: 06/26/2026

Test	g/210L	Time
DIAG	Pass	10:15am
AIR BLK	.00	10:16am
ACCY CHK	.07	10:17am
AIR BLK	.00	10:18am
SUB TEST	.00	10:19am
AIR BLK	.00	10:20am
SUB TEST	.00	10:21am
AIR BLK	.00	10:22am

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

Intox EC/IR-II: Preventive Maintenance

CUMBERLAND COUNTY DETENTION CENTER 250

Serial Number: 008633 Test Record Number: 7202
Test Date: 04/01/2025 Test Time: 10:23am EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	10:23am
FLO	Pass	10:23am
FC	Pass	10:23am

Temperature Tests

Test	Status	Time
FC1	Pass	10:23am
SRC	Pass	10:23am
DET	Pass	10:23am
BAR	Pass	10:23am
BT	Pass	10:23am

Blank Tests

Test	Status	Time
AIR	Pass	10:24am

Printer Tests

Test	Status	Time
PRNT	Pass	10:24am

CRC Tests

Test	Status	Time
COMP	Pass	10:24am
CAL	Pass	10:24am

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County Cumberland Instrument Location Cumberland County
Instrument Serial No. 008672 Detention Center

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 1 day of April, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

365156
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

CUMBERLAND COUNTY DETENTION CENTER 250

Serial Number: 008672
Test Date: 04/01/2025

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: Garner, Joel K
Permit Number: 0036-5156
Effective:
02/01/2025-02/01/2027

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG417803
Exp Date: 06/26/2026


Test	g/210L	Time
DIAG	Pass	10:16am
AIR BLK	.00	10:17am
ACCY CHK	.07	10:17am
AIR BLK	.00	10:19am
SUB TEST	.00	10:19am
AIR BLK	.00	10:20am
SUB TEST	.00	10:21am
AIR BLK	.00	10:22am

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

Intox EC/IR-II: Preventive Maintenance

CUMBERLAND COUNTY DETENTION CENTER 250

Serial Number: 008672 Test Record Number: 8714
Test Date: 04/01/2025 Test Time: 10:24am EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	10:24am
FLO	Pass	10:24am
FC	Pass	10:24am

Temperature Tests

Test	Status	Time
FC1	Pass	10:24am
SRC	Pass	10:24am
DET	Pass	10:24am
BAR	Pass	10:24am
BT	Pass	10:24am

Blank Tests

Test	Status	Time
AIR	Pass	10:25am

Printer Tests

Test	Status	Time
PRNT	Pass	10:25am

CRC Tests

Test	Status	Time
COMP	Pass	10:25am
CAL	Pass	10:25am

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Dare Instrument Location Dare Co. Detention Center
Instrument Serial No. 008783 1044 Driftwood Dr Montecy,
NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 15th day of April, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

206272
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

DARE COUNTY DARE CO DETENTION CE 270

Serial Number: 008783
Test Date: 04/15/2025

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Chappell, Mark A

Permit Number: 0020-6272

Effective:

02/01/2025-02/01/2027

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

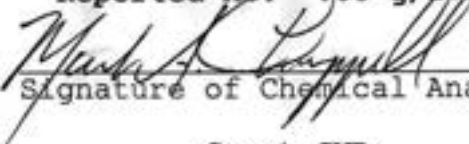
Test Type: Breath Test

Lot Number: AG400303

Exp Date: 01/03/2026

Test	g/210L	Time
DIAG	Pass	12:32pm
AIR BLK	.00	12:33pm
ACCY CHK	.07	12:33pm
AIR BLK	.00	12:34pm
SUB TEST	.00	12:35pm
AIR BLK	.00	12:36pm
SUB TEST	.00	12:37pm
AIR BLK	.00	12:38pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

DARE COUNTY DARE CO DETENTION CE 270

Serial Number: 008783 Test Record Number: 1708
Test Date: 04/15/2025 Test Time: 12:40pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	12:40pm
FLO	Pass	12:40pm
FC	Pass	12:40pm

Temperature Tests

Test	Status	Time
FC1	Pass	12:40pm
SRC	Pass	12:40pm
DET	Pass	12:40pm
BAR	Pass	12:40pm
BT	Pass	12:40pm

Blank Tests

Test	Status	Time
AIR	Pass	12:41pm

Printer Tests

Test	Status	Time
PRNT	Pass	12:41pm

CRC Tests

Test	Status	Time
COMP	Pass	12:41pm
CAL	Pass	12:41pm

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Dare Instrument Location Dare Co. Detention Center
Instrument Serial No. 008804 1044 Delfwood Dr. Montec, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 15th day of April, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

206272
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

DARE COUNTY DARE CO DETENTION CE 270

Serial Number: 008804
Test Date: 04/15/2025

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Chappell, Mark A

Permit Number: 0020-6272

Effective:

02/01/2025-02/01/2027

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

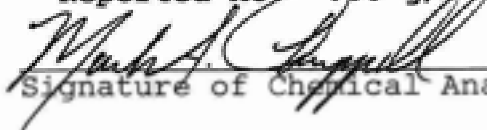
Test Type: Breath Test

Lot Number: AG431003

Exp Date: 11/05/2026

Test	g/210L	Time
DIAG	Pass	12:30pm
AIR BLK	.00	12:31pm
ACCY CHK	.07	12:32pm
AIR BLK	.00	12:33pm
SUB TEST	.00	12:34pm
AIR BLK	.00	12:35pm
SUB TEST	.00	12:36pm
AIR BLK	.00	12:37pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

DARE COUNTY DARE CO DETENTION CE 270

Serial Number: 008804 Test Record Number: 2900
Test Date: 04/15/2025 Test Time: 12:50pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	12:50pm
FLO	Pass	12:50pm
FC	Pass	12:51pm

Temperature Tests

Test	Status	Time
FC1	Pass	12:51pm
SRC	Pass	12:51pm
DET	Pass	12:51pm
BAR	Pass	12:51pm
BT	Pass	12:51pm

Blank Tests

Test	Status	Time
AIR	Pass	12:51pm

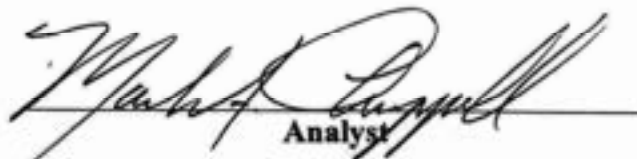
Printer Tests

Test	Status	Time
PRNT	Pass	12:51pm

CRC Tests

Test	Status	Time
COMP	Pass	12:51pm
CAL	Pass	12:51pm

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Davidson Instrument Location BAT Mobile Unit 8
Instrument Serial No. 008615 Davidson SO

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 15 day of April, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature] 2219283
Signature of Certifying Official Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

DAVIDSON COUNTY BAT MOBILE UNIT 8 280

Serial Number: 008615

Test Date: 04/15/2025

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Glasscock, Jerry D

Permit Number: 7180-9235

Effective: .

02/01/2025-02/01/2027

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG405102


Exp Date: 02/20/2026

Test	g/210L	Time
DIAG	Pass	8:57pm
AIR BLK	.00	8:58pm
ACCY CHK	.07	8:58pm
AIR BLK	.00	8:59pm
SUB TEST	.00	9:00pm
AIR BLK	.00	9:01pm
SUB TEST	.00	9:02pm
AIR BLK	.00	9:03pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

Intox EC/IR-II: Preventive Maintenance

DAVIDSON COUNTY BAT MOBILE UNIT 8 280

Serial Number: 008615 Test Record Number: 6068
Test Date: 04/15/2025 Test Time: 9:08pm EDT

System Check: Passed

Baseline Tests

Test	Status	Time
IR	Pass	9:09pm
FLO	Pass	9:09pm
FC	Pass	9:09pm

Temperature Tests

Test	Status	Time
FC1	Pass	9:09pm
SRC	Pass	9:09pm
DET	Pass	9:09pm
BAR	Pass	9:09pm
BT	Pass	9:09pm

Blank Tests

Test	Status	Time
AIR	Pass	9:09pm

Printer Tests

Test	Status	Time
PRNT	Pass	9:09pm

CRC Tests

Test	Status	Time
COMP	Pass	9:10pm
CAL	Pass	9:10pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Davidson Instrument Location BAT Mobile Unit 8
Instrument Serial No. 008736 Davidson 50

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 15 day of April, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

2219283
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

DAVIDSON COUNTY BAT MOBILE UNIT 8 280

Serial Number: 008736
Test Date: 04/15/2025

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE

Analyst's Name: Glasscock, Jerry D
Permit Number: 7180-9235
Effective:
02/01/2025-02/01/2027

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG405102
Exp Date: 02/20/2026

Test	g/210L	Time
DIAG	Pass	9:12pm
AIR BLK	.00	9:13pm
ACCY CHK	.07	9:13pm
AIR BLK	.00	9:14pm
SUB TEST	.00	9:15pm
AIR BLK	.00	9:16pm
SUB TEST	.00	9:17pm
AIR BLK	.00	9:18pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

Intox EC/IR-II: Preventive Maintenance

DAVIDSON COUNTY BAT MOBILE UNIT 8 280

Serial Number: 008736 Test Record Number: 1420
Test Date: 04/15/2025 Test Time: 9:19pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	9:19pm
FLO	Pass	9:19pm
FC	Pass	9:19pm

Temperature Tests

Test	Status	Time
FC1	Pass	9:19pm
SRC	Pass	9:19pm
DET	Pass	9:19pm
BAR	Pass	9:19pm
BT	Pass	9:19pm

Blank Tests

Test	Status	Time
AIR	Pass	9:20pm

Printer Tests

Test	Status	Time
PRNT	Pass	9:20pm

CRC Tests

Test	Status	Time
COMP	Pass	9:20pm
CAL	Pass	9:20pm

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Davidson Instrument Location BAT Mobile Unit 8
Instrument Serial No. 008775 Davidson 50

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 15 day of April, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

2219283
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

DAVIDSON COUNTY BAT MOBILE UNIT 8 280

Serial Number: 008775
Test Date: 04/15/2025

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: Glasscock, Jerry D
Permit Number: 7180-9235
Effective:
02/01/2025-02/01/2027

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG431002
Exp Date: 11/05/2026

Test	g/210L	Time
DIAG	Pass	8:55pm
AIR BLK	.00	8:56pm
ACCY CHK	.07	8:56pm
AIR BLK	.00	8:57pm
SUB TEST	.00	8:58pm
AIR BLK	.00	8:58pm
SUB TEST	.00	9:00pm
AIR BLK	.00	9:01pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

Intox EC/IR-II: Preventive Maintenance

DAVIDSON COUNTY BAT MOBILE UNIT 8 280

Serial Number: 008775 Test Record Number: 2272
Test Date: 04/15/2025 Test Time: 9:03pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	9:04pm
FLO	Pass	9:04pm
FC	Pass	9:04pm

Temperature Tests

Test	Status	Time
FC1	Pass	9:04pm
SRC	Pass	9:04pm
DET	Pass	9:04pm
BAR	Pass	9:04pm
BT	Pass	9:04pm

Blank Tests

Test	Status	Time
AIR	Pass	9:04pm

Printer Tests

Test	Status	Time
PRNT	Pass	9:04pm

CRC Tests

Test	Status	Time
COMP	Pass	9:05pm
CAL	Pass	9:05pm

Preventive Maintenance
Status: *Pass*


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Davidson Instrument Location BAT Mobile Unit 8
Instrument Serial No. 008816 Davidson SO

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 15 day of April, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

2219283
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

DAVIDSON COUNTY BAT MOBILE UNIT 8 280

Serial Number: 008816
Test Date: 04/15/2025

Citation Number: M0000000-0
Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Glasscock, Jerry D

Permit Number: 7180-9235

Effective:

02/01/2025-02/01/2027

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG431002

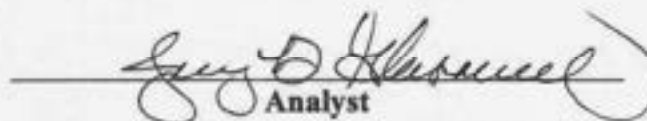
Exp Date: 11/05/2026

Test	g/210L	Time
DIAG	Pass	8:56pm
AIR BLK	.00	8:57pm
ACCY CHK	.08	8:57pm
AIR BLK	.00	8:58pm
SUB TEST	.00	8:59pm
AIR BLK	.00	9:00pm
SUB TEST	.00	9:01pm
AIR BLK	.00	9:02pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

Intox EC/IR-II: Preventive Maintenance

DAVIDSON COUNTY BAT MOBILE UNIT 8 280

Serial Number: 008816 Test Record Number: 7857
Test Date: 04/15/2025 Test Time: 9:04pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	9:04pm
FLO	Pass	9:04pm
FC	Pass	9:04pm

Temperature Tests

Test	Status	Time
FC1	Pass	9:04pm
SRC	Pass	9:04pm
DET	Pass	9:04pm
BAR	Pass	9:04pm
BT	Pass	9:04pm

Blank Tests

Test	Status	Time
AIR	Pass	9:05pm

Printer Tests

Test	Status	Time
PRNT	Pass	9:05pm

CRC Tests

Test	Status	Time
COMP	Pass	9:05pm
CAL	Pass	9:05pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Davidson Instrument Location BAT Mobile Unit 8
Instrument Serial No. 008929 Davidson SO

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 15 day of April, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

2219283
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

DAVIDSON COUNTY BAT MOBILE UNIT 8 280

Serial Number: 008929
Test Date: 04/15/2025

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: Glasscock, Jerry D
Permit Number: 7180-9235
Effective:
02/01/2025-02/01/2027

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG506303
Exp Date: 03/04/2027

Test	g/210L	Time
DIAG	Pass	8:56pm
AIR BLK	.00	8:58pm
ACCY CHK	.07	8:58pm
AIR BLK	.00	8:59pm
SUB TEST	.00	9:00pm
AIR BLK	.00	9:01pm
SUB TEST	.00	9:03pm
AIR BLK	.00	9:04pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

Intox EC/IR-II: Preventive Maintenance

DAVIDSON COUNTY BAT MOBILE UNIT 8 280

Serial Number: 008929 Test Record Number: 1558
Test Date: 04/15/2025 Test Time: 9:08pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	9:09pm
FLO	Pass	9:09pm
FC	Pass	9:09pm

Temperature Tests

Test	Status	Time
FC1	Pass	9:09pm
SRC	Pass	9:09pm
DET	Pass	9:09pm
BAR	Pass	9:09pm
BT	Pass	9:09pm

Blank Tests

Test	Status	Time
AIR	Pass	9:10pm


Printer Tests

Test	Status	Time
PRNT	Pass	9:10pm

CRC Tests

Test	Status	Time
COMP	Pass	9:10pm
CAL	Pass	9:10pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Durham Instrument Location Durham Co Jail
Instrument Serial No. 008859 219 S. Mangum St
Durham, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 3 day of April, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Saman Stokes Bruce
Signature of Certifying Official

146221
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

DURHAM COUNTY DURHAM COUNTY JAIL 310

Serial Number: 008859

Test Date: 04/03/2025

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Barnes, Simon S

Permit Number: 0014-6221

Effective:

02/01/2025-02/01/2027

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG431003

Exp Date: 11/05/2026

Test	g/210L	Time
DIAG	Pass	9:49am
AIR BLK	.00	9:50am
ACCY CHK	.08	9:50am
AIR BLK	.00	9:52am
SUB TEST	.00	9:52am
AIR BLK	.00	9:53am
SUB TEST	.00	9:55am
AIR BLK	.00	9:56am

Reported AC: .00 g/210L

Simon Stokes Barnes
Signature of Chemical Analyst

Court CVR

Simon Stokes Barnes
Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

DURHAM COUNTY DURHAM COUNTY JAIL 310

Serial Number: 008859 Test Record Number: 3255
Test Date: 04/03/2025 Test Time: 9:56am EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	9:57am
FLO	Pass	9:57am
FC	Pass	9:57am

Temperature Tests

Test	Status	Time
FC1	Pass	9:57am
SRC	Pass	9:57am
DET	Pass	9:57am
BAR	Pass	9:57am
BT	Pass	9:57am

Blank Tests

Test	Status	Time
AIR	Pass	9:57am

Printer Tests

Test	Status	Time
PRNT	Pass	9:57am

CRC Tests

Test	Status	Time
COMP	Pass	9:58am
CAL	Pass	9:58am

Preventive Maintenance
Status: *Pass*


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Durham Instrument Location Durham Co Jail
Instrument Serial No. 008878 219 S. Mangum St
Durham, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 3 day of April, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Simon Stokes Brown
Signature of Certifying Official

146221
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

DURHAM COUNTY DURHAM COUNTY JAIL 310

Serial Number: 008878
Test Date: 04/03/2025

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: Barnes, Simon S
Permit Number: 0014-6221
Effective:
02/01/2025-02/01/2027

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG431003
Exp Date: 11/05/2026

Test	g/210L	Time
DIAG	Pass	9:44am
AIR BLK	.00	9:45am
ACCY CHK	.08	9:46am
AIR BLK	.00	9:47am
SUB TEST	.00	9:47am
AIR BLK	.00	9:48am
SUB TEST	.00	9:50am
AIR BLK	.00	9:50am

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

Intox EC/IR-II: Preventive Maintenance

DURHAM COUNTY DURHAM COUNTY JAIL 310

Serial Number: 008878 Test Record Number: 6835
Test Date: 04/03/2025 Test Time: 9:51am EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	9:51am
FLO	Pass	9:51am
FC	Pass	9:51am

Temperature Tests

Test	Status	Time
FC1	Pass	9:52am
SRC	Pass	9:52am
DET	Pass	9:52am
BAR	Pass	9:52am
BT	Pass	9:52am

Blank Tests

Test	Status	Time
AIR	Pass	9:52am

Printer Tests

Test	Status	Time
PRNT	Pass	9:52am

CRC Tests

Test	Status	Time
COMP	Pass	9:52am
CAL	Pass	9:52am

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Durham Instrument Location Durham Co Jail
Instrument Serial No. 008891 219 S. Mangum ST
Durham, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 3 day of April, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Simon Stokes Brown
Signature of Certifying Official

146221
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

DURHAM COUNTY DURHAM COUNTY JAIL 310

Serial Number: 008891
Test Date: 04/03/2025

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Barnes, Simon S

Permit Number: 0014-6221

Effective:

02/01/2025-02/01/2027

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG431003

Exp Date: 11/05/2026

Test	g/210L	Time
DIAG	Pass	9:49am
AIR BLK	.00	9:50am
ACCY CHK	.07	9:51am
AIR BLK	.00	9:52am
SUB TEST	.00	9:52am
AIR BLK	.00	9:53am
SUB TEST	.00	9:55am
AIR BLK	.00	9:56am

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR



Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

DURHAM COUNTY DURHAM COUNTY JAIL 310

Serial Number: 008891 Test Record Number: 4839
Test Date: 04/03/2025 Test Time: 9:56am EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	9:56am
FLO	Pass	9:56am
FC	Pass	9:56am

Temperature Tests

Test	Status	Time
FC1	Pass	9:57am
SRC	Pass	9:57am
DET	Pass	9:57am
BAR	Pass	9:57am
BT	Pass	9:57am

Blank Tests

Test	Status	Time
AIR	Pass	9:57am

Printer Tests

Test	Status	Time
PRNT	Pass	9:57am

CRC Tests

Test	Status	Time
COMP	Pass	9:57am
CAL	Pass	9:57am

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Edgecombe Instrument Location BAT Mobile Unit 10
Instrument Serial No. 008584 Edgecombe County SO

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 10th day of April, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

2266313
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

EDGECOMBE COUNTY BAT MOBILE UNIT 10
320

Serial Number: 008584
Test Date: 04/10/2025

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Sharpe Jr., Robert J

Permit Number: 1820-8591

Effective:

02/01/2025-02/01/2027

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG400303

Exp Date: 01/03/2026

Test	g/210L	Time
DIAG	Pass	10:30pm
AIR BLK	.00	10:31pm
ACCY CHK	.07	10:32pm
AIR BLK	.00	10:32pm
SUB TEST	.00	10:33pm
AIR BLK	.00	10:34pm
SUB TEST	.00	10:36pm
AIR BLK	.00	10:37pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

EDGECOMBE COUNTY BAT MOBILE UNIT 10 320

Serial Number: 008584 Test Record Number: 2776
Test Date: 04/10/2025 Test Time: 10:38pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	10:38pm
FLO	Pass	10:38pm
FC	Pass	10:38pm

Temperature Tests

Test	Status	Time
FC1	Pass	10:38pm
SRC	Pass	10:38pm
DET	Pass	10:38pm
BAR	Pass	10:38pm
BT	Pass	10:38pm

Blank Tests

Test	Status	Time
AIR	Pass	10:39pm

Printer Tests

Test	Status	Time
PRNT	Pass	10:39pm

CRC Tests

Test	Status	Time
COMP	Pass	10:39pm
CAL	Pass	10:39pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County Edgecombe Instrument Location BAT Mobile Unit 10

Instrument Serial No. 008637 Edgecombe County SO

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 10th day of April, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

2266313
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

EDGECOMBE COUNTY BAT MOBILE UNIT 10
320

Serial Number: 008637
Test Date: 04/10/2025

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Sharpe Jr., Robert J

Permit Number: 1820-8591

Effective:

02/01/2025-02/01/2027

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG400303

Exp Date: 01/03/2026

Test	g/210L	Time
DIAG	Pass	10:32pm
AIR BLK	.00	10:33pm
ACCY CHK	.08	10:34pm
AIR BLK	.00	10:35pm
SUB TEST	.00	10:35pm
AIR BLK	.00	10:36pm
SUB TEST	.00	10:38pm
AIR BLK	.00	10:38pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

Intox EC/IR-II: Preventive Maintenance

EDGECOMBE COUNTY BAT MOBILE UNIT 10 320

Serial Number: 008637 Test Record Number: 3510
Test Date: 04/10/2025 Test Time: 10:39pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	10:39pm
FLO	Pass	10:39pm
FC	Pass	10:39pm

Temperature Tests

Test	Status	Time
FC1	Pass	10:39pm
SRC	Pass	10:39pm
DET	Pass	10:39pm
BAR	Pass	10:39pm
BT	Pass	10:39pm

Blank Tests

Test	Status	Time
AIR	Pass	10:40pm

Printer Tests

Test	Status	Time
PRNT	Pass	10:40pm

CRC Tests

Test	Status	Time
COMP	Pass	10:40pm
CAL	Pass	10:40pm

**Preventive Maintenance
Status: Pass**



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Edgecombe Instrument Location BAT Mobile Unit 10
Instrument Serial No. 008686 Edgecombe County SO

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 10th day of April, 20 25 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

2266313
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

EDGECOMBE COUNTY BAT MOBILE UNIT 10
320

Serial Number: 008686
Test Date: 04/10/2025

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Sharpe Jr., Robert J

Permit Number: 1820-8591

Effective:

02/01/2025-02/01/2027

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG506302

Exp Date: 03/04/2027

Test	g/210L	Time
DIAG	Pass	10:31pm
AIR BLK	.00	10:32pm
ACCY CHK	.08	10:32pm
AIR BLK	.00	10:33pm
SUB TEST	.00	10:34pm
AIR BLK	.00	10:35pm
SUB TEST	.00	10:36pm
AIR BLK	.00	10:37pm

Reported AC: .00 g/210L

Signature  Chemical Analyst

Court CVR


Analyst

Intox EC/IR-II: Preventive Maintenance

EDGECOMBE COUNTY BAT MOBILE UNIT 10 320

Serial Number: 008686 Test Record Number: 7138
Test Date: 04/10/2025 Test Time: 10:38pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	10:38pm
FLO	Pass	10:38pm
FC	Pass	10:38pm

Temperature Tests

Test	Status	Time
FC1	Pass	10:38pm
SRC	Pass	10:38pm
DET	Pass	10:38pm
BAR	Pass	10:38pm
BT	Pass	10:38pm

Blank Tests

Test	Status	Time
AIR	Pass	10:39pm

Printer Tests

Test	Status	Time
PRNT	Pass	10:39pm

CRC Tests

Test	Status	Time
COMP	Pass	10:39pm
CAL	Pass	10:39pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Edgecombe Instrument Location BAT Mobile Unit 10

Instrument Serial No. 008776 Edgecombe County SO

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 10th day of April, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

2266313
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

EDGECOMBE COUNTY BAT MOBILE UNIT 10
320

Serial Number: 008776
Test Date: 04/10/2025

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Sharpe Jr., Robert J

Permit Number: 1820-8591

Effective:

02/01/2025-02/01/2027

Officer's Name: NONE, NONE

Type of Agency: PTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG417803

Exp Date: 06/26/2026

Test	g/210L	Time
DIAG	Pass	10:33pm
AIR BLK	.00	10:34pm
ACCY CHK	.08	10:35pm
AIR BLK	.00	10:36pm
SUB TEST	.00	10:36pm
AIR BLK	.00	10:37pm
SUB TEST	.00	10:39pm
AIR BLK	.00	10:40pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

EDGECOMBE COUNTY BAT MOBILE UNIT 10 320

Serial Number: 008776 Test Record Number: 4096
Test Date: 04/10/2025 Test Time: 10:48pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	10:49pm
FLO	Pass	10:49pm
FC	Pass	10:49pm

Temperature Tests

Test	Status	Time
FC1	Pass	10:49pm
SRC	Pass	10:49pm
DET	Pass	10:49pm
BAR	Pass	10:49pm
BT	Pass	10:49pm

Blank Tests

Test	Status	Time
AIR	Pass	10:50pm

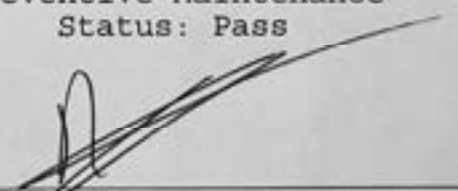
Printer Tests

Test	Status	Time
PRNT	Pass	10:50pm

CRC Tests

Test	Status	Time
COMP	Pass	10:50pm
CAL	Pass	10:50pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Edgecombe Instrument Location BAT Mobile Unit 10

Instrument Serial No. 008779 Edgecombe County SO

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 10th day of April, 20 25 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

2266313
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

EDGECOMBE COUNTY BAT MOBILE UNIT 10
320

Serial Number: 008779
Test Date: 04/10/2025

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE

Analyst's Name: Sharpe Jr., Robert J
Permit Number: 1820-8591
Effective:
02/01/2025-02/01/2027

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG431002
Exp Date: 11/05/2026


Test	g/210L	Time
DIAG	Pass	10:33pm
AIR BLK	.00	10:34pm
ACCY CHK	.07	10:35pm
AIR BLK	.00	10:35pm
SUB TEST	.00	10:36pm
AIR BLK	.00	10:37pm
SUB TEST	.00	10:38pm
AIR BLK	.00	10:39pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

Intox EC/IR-II: Preventive Maintenance

EDGECOMBE COUNTY BAT MOBILE UNIT 10 320

Serial Number: 008779 Test Record Number: 4043
Test Date: 04/10/2025 Test Time: 10:39pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	10:40pm
FLO	Pass	10:40pm
FC	Pass	10:40pm

Temperature Tests

Test	Status	Time
FC1	Pass	10:40pm
SRC	Pass	10:40pm
DET	Pass	10:40pm
BAR	Pass	10:40pm
BT	Pass	10:40pm

Blank Tests

Test	Status	Time
AIR	Pass	10:41pm

Printer Tests

Test	Status	Time
PRNT	Pass	10:41pm

CRC Tests

Test	Status	Time
COMP	Pass	10:41pm
CAL	Pass	10:41pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Forsyth Instrument Location BAT Mobile Unit 8
Instrument Serial No. 008615 Kernersville PD

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 11 day of April, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

2219283
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

FORSYTH COUNTY BAT MOBILE UNIT 8 330

Serial Number: 008615

Test Date: 04/11/2025

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Glasscock, Jerry D

Permit Number: 7180-9235

Effective:

02/01/2025-02/01/2027

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG405102

Exp Date: 02/20/2026

Test	g/210L	Time
DIAG	Pass	8:26pm
AIR BLK	.00	8:27pm
ACCY CHK	.08	8:28pm
AIR BLK	.00	8:29pm
SUB TEST	.00	8:30pm
AIR BLK	.00	8:30pm
SUB TEST	.00	8:32pm
AIR BLK	.00	8:33pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

Intox EC/IR-II: Preventive Maintenance

FORSYTH COUNTY BAT MOBILE UNIT 8 330

Serial Number: 008615 Test Record Number: 6062
Test Date: 04/11/2025 Test Time: 8:33pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	8:34pm
FLO	Pass	8:34pm
FC	Pass	8:34pm

Temperature Tests

Test	Status	Time
FC1	Pass	8:34pm
SRC	Pass	8:34pm
DET	Pass	8:34pm
BAR	Pass	8:34pm
BT	Pass	8:34pm

Blank Tests

Test	Status	Time
AIR	Pass	8:35pm


Printer Tests

Test	Status	Time
PRNT	Pass	8:35pm

CRC Tests

Test	Status	Time
COMP	Pass	8:35pm
CAL	Pass	8:35pm

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Forsyth Instrument Location BAT Mobile Unit 8
Instrument Serial No. 008736 Kernersville PD

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 11 day of April, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

2219283
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

FORSYTH COUNTY BAT MOBILE UNIT 8 330

Serial Number: 008736

Test Date: 04/11/2025

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Glasscock, Jerry D

Permit Number: 7180-9235

Effective:

02/01/2025-02/01/2027

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG405102

Exp Date: 02/20/2026

Test	g/210L	Time
DIAG	Pass	8:27pm
AIR BLK	.00	8:28pm
ACCY CHK	.08	8:28pm
AIR BLK	.00	8:29pm
SUB TEST	.00	8:30pm
AIR BLK	.00	8:31pm
SUB TEST	.00	8:32pm
AIR BLK	.00	8:33pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

This form is used when performing Preventive Maintenance procedures

Forensic Tests for Alcohol Branch

Department of Health and Human Services

Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

FORSYTH COUNTY BAT MOBILE UNIT 8 330

Serial Number: 008736 Test Record Number: 1416
Test Date: 04/11/2025 Test Time: 8:34pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	8:34pm
FLO	Pass	8:34pm
FC	Pass	8:34pm

Temperature Tests

Test	Status	Time
FC1	Pass	8:34pm
SRC	Pass	8:34pm
DET	Pass	8:34pm
BAR	Pass	8:34pm
BT	Pass	8:34pm

Blank Tests

Test	Status	Time
AIR	Pass	8:35pm

Printer Tests

Test	Status	Time
PRNT	Pass	8:35pm

CRC Tests

Test	Status	Time
COMP	Pass	8:35pm
CAL	Pass	8:35pm

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Forsyth Instrument Location BAT Mobile Unit 8
Instrument Serial No. 008775 Kernersville PD

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 11 day of April, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature] 2219283
Signature of Certifying Official Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

FORSYTH COUNTY BAT MOBILE UNIT 8 330

Serial Number: 008775
Test Date: 04/11/2025

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE

Analyst's Name: Glasscock, Jerry D
Permit Number: 7180-9235
Effective:
02/01/2025-02/01/2027

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG431002
Exp Date: 11/05/2026

Test	g/210L	Time
DIAG	Pass	8:28pm
AIR BLK	.00	8:29pm
ACCY CHK	.07	8:29pm
AIR BLK	.00	8:30pm
SUB TEST	.00	8:31pm
AIR BLK	.00	8:32pm
SUB TEST	.00	8:33pm
AIR BLK	.00	8:34pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

FORSYTH COUNTY BAT MOBILE UNIT 8 330

Serial Number: 008775 Test Record Number: 2265
Test Date: 04/11/2025 Test Time: 8:34pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	8:35pm
FLO	Pass	8:35pm
FC	Pass	8:35pm

Temperature Tests

Test	Status	Time
FC1	Pass	8:35pm
SRC	Pass	8:35pm
DET	Pass	8:35pm
BAR	Pass	8:35pm
BT	Pass	8:35pm

Blank Tests

Test	Status	Time
AIR	Pass	8:36pm

Printer Tests

Test	Status	Time
PRNT	Pass	8:36pm

CRC Tests

Test	Status	Time
COMP	Pass	8:36pm
CAL	Pass	8:36pm

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Forsyth Instrument Location BAT Mobile Unit 8
Instrument Serial No. 008816 Kernersville PD

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 11 day of April, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

2219283
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

FORSYTH COUNTY BAT MOBILE UNIT 8 330

Serial Number: 008816
Test Date: 04/11/2025

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Glasscock, Jerry D

Permit Number: 7180-9235

Effective:

02/01/2025-02/01/2027

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG431002

Exp Date: 11/05/2026

Test	g/210L	Time
DIAG	Pass	8:29pm
AIR BLK	.00	8:30pm
ACCY CHK	.08	8:30pm
AIR BLK	.00	8:31pm
SUB TEST	.00	8:32pm
AIR BLK	.00	8:33pm
SUB TEST	.00	8:34pm
AIR BLK	.00	8:35pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

Intox EC/IR-II: Preventive Maintenance

FORSYTH COUNTY BAT MOBILE UNIT 8 330

Serial Number: 008816 Test Record Number: 7853
Test Date: 04/11/2025 Test Time: 8:40pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	8:41pm
FLO	Pass	8:41pm
FC	Pass	8:41pm

Temperature Tests

Test	Status	Time
FC1	Pass	8:41pm
SRC	Pass	8:41pm
DET	Pass	8:41pm
BAR	Pass	8:41pm
BT	Pass	8:41pm

Blank Tests

Test	Status	Time
AIR	Pass	8:41pm

Printer Tests

Test	Status	Time
PRNT	Pass	8:41pm

CRC Tests

Test	Status	Time
COMP	Pass	8:42pm
CAL	Pass	8:42pm

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Forsyth Instrument Location BAT Mobile Unit 8
Instrument Serial No. 008929 Kernersville PD

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 11 day of April, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature] 2219283
Signature of Certifying Official Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

FORSYTH COUNTY BAT MOBILE UNIT 8 330

Serial Number: 008929
Test Date: 04/11/2025

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: Glasscock, Jerry D
Permit Number: 7180-9235
Effective:
02/01/2025-02/01/2027

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG506303
Exp Date: 03/04/2027

Test	g/210L	Time
DIAG	Pass	8:30pm
AIR BLK	.00	8:31pm
ACCY CHK	.07	8:31pm
AIR BLK	.00	8:33pm
SUB TEST	.00	8:33pm
AIR BLK	.00	8:34pm
SUB TEST	.00	8:36pm
AIR BLK	.00	8:37pm

Reported AC: 00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

Intox EC/IR-II: Preventive Maintenance

FORSYTH COUNTY BAT MOBILE UNIT 8 330

Serial Number: 008929 Test Record Number: 1554
Test Date: 04/11/2025 Test Time: 8:41pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	8:42pm
FLO	Pass	8:42pm
FC	Pass	8:42pm

Temperature Tests

Test	Status	Time
FC1	Pass	8:42pm
SRC	Pass	8:42pm
DET	Pass	8:42pm
BAR	Pass	8:42pm
BT	Pass	8:42pm

Blank Tests

Test	Status	Time
AIR	Pass	8:43pm

Printer Tests

Test	Status	Time
PRNT	Pass	8:43pm

CRC Tests

Test	Status	Time
COMP	Pass	8:43pm
CAL	Pass	8:43pm

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County GRANVILLE Instrument Location CREEDMOOR PD
Instrument Serial No. 008641 111 MASONIC ST
CREEDMOOR, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 25 day of April, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

179707
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

GRANVILLE COUNTY CREEDMOOR PD 380

Serial Number: 008641

Test Date: 04/25/2025

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Bryant, Earl A

Permit Number: 0017-9707

Effective:

02/01/2025-02/01/2027

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG431003

Exp Date: 11/05/2026

Test	g/210L	Time
DIAG	Pass	1:33pm
AIR BLK	.00	1:34pm
ACCY CHK	.07	1:34pm
AIR BLK	.00	1:35pm
SUB TEST	.00	1:36pm
AIR BLK	.00	1:36pm
SUB TEST	.00	1:38pm
AIR BLK	.00	1:39pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

GRANVILLE COUNTY CREEDMOOR PD 380

Serial Number: 008641 Test Record Number: 1664
Test Date: 04/25/2025 Test Time: 1:40pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	1:40pm
FLO	Pass	1:40pm
FC	Pass	1:40pm

Temperature Tests

Test	Status	Time
FC1	Pass	1:40pm
SRC	Pass	1:40pm
DET	Pass	1:40pm
BAR	Pass	1:40pm
BT	Pass	1:40pm

Blank Tests

Test	Status	Time
AIR	Pass	1:41pm

Printer Tests

Test	Status	Time
PRNT	Pass	1:41pm

CRC Tests

Test	Status	Time
COMP	Pass	1:41pm
CAL	Pass	1:41pm

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Guilford Instrument Location BAT Mobile Unit 8
Instrument Serial No. 008615 Guilford SO

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 10 day of April, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

2219283
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

GUILFORD COUNTY BAT MOBILE UNIT 8 400

Serial Number: 008615
Test Date: 04/10/2025

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Glasscock, Jerry D

Permit Number: 7180-9235

Effective:

02/01/2025-02/01/2027

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG405102

Exp Date: 02/20/2026

Test	g/210L	Time
DIAG	Pass	10:56pm
AIR BLK	.00	10:57pm
ACCY CHK	.07	10:57pm
AIR BLK	.00	10:58pm
SUB TEST	.00	10:59pm
AIR BLK	.00	11:00pm
SUB TEST	.00	11:01pm
AIR BLK	.00	11:02pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

GUILFORD COUNTY BAT MOBILE UNIT 8 400

Serial Number: 008615 Test Record Number: 6060
Test Date: 04/10/2025 Test Time: 11:03pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	11:03pm
FLO	Pass	11:03pm
FC	Pass	11:03pm

Temperature Tests

Test	Status	Time
FC1	Pass	11:03pm
SRC	Pass	11:03pm
DET	Pass	11:03pm
BAR	Pass	11:03pm
BT	Pass	11:03pm

Blank Tests

Test	Status	Time
AIR	Pass	11:04pm

Printer Tests

Test	Status	Time
PRNT	Pass	11:04pm

CRC Tests

Test	Status	Time
COMP	Pass	11:04pm
CAL	Pass	11:04pm

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County GUILFORD Instrument Location GREENSBORO JAIL
Instrument Serial No. 008638 GREENSBORO, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 29th day of APRIL, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Handwritten Signature]
Signature of Certifying Official

353799
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

GUILFORD GREENSBORO JAIL 400

Serial Number: 008638

Test Date: 04/29/2025

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Oligmueller, Leo A

Permit Number: 0035-3799

Effective:

02/01/2025-02/01/2027

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

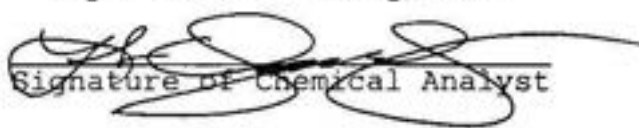
Test Type: Breath Test

Lot Number: AG431002

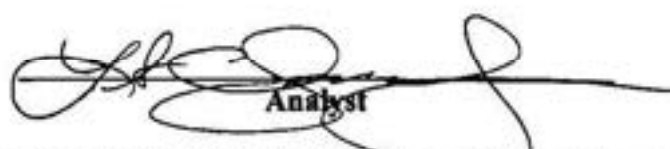
Exp Date: 11/05/2026

Test	g/210L	Time
DIAG	Pass	10:53am
AIR BLK	.00	10:54am
ACCY CHK	.08	10:54am
AIR BLK	.00	10:55am
SUB TEST	.00	10:56am
AIR BLK	.00	10:57am
SUB TEST	.00	10:59am
AIR BLK	.00	10:59am

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

GUILFORD GREENSBORO JAIL 400

Serial Number: 008638 Test Record Number: 6876
Test Date: 04/29/2025 Test Time: 11:01am EDT

System Check: Passed

Baseline Tests

Test	Status	Time
IR	Pass	11:01am
FLO	Pass	11:01am
FC	Pass	11:01am

Temperature Tests

Test	Status	Time
FC1	Pass	11:01am
SRC	Pass	11:01am
DET	Pass	11:01am
BAR	Pass	11:01am
BT	Pass	11:01am

Blank Tests

Test	Status	Time
AIR	Pass	11:02am

Printer Tests

Test	Status	Time
PRNT	Pass	11:02am

CRC Tests

Test	Status	Time
COMP	Pass	11:02am
CAL	Pass	11:02am

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Guilford Instrument Location BAT Mobile Unit 8
Instrument Serial No. 008736 Guilford SO

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 10 day of April, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

2219283
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

GUILFORD COUNTY BAT MOBILE UNIT 8 400

Serial Number: 008736
Test Date: 04/10/2025

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: Glasscock, Jerry D
Permit Number: 7180-9235
Effective:
02/01/2025-02/01/2027

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG405102
Exp Date: 02/20/2026

Test	g/210L	Time
DIAG	Pass	10:56pm
AIR BLK	.00	10:57pm
ACCY CHK	.08	10:58pm
AIR BLK	.00	10:59pm
SUB TEST	.00	10:59pm
AIR BLK	.00	11:00pm
SUB TEST	.00	11:01pm
AIR BLK	.00	11:02pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

Intox EC/IR-II: Preventive Maintenance

GUILFORD COUNTY BAT MOBILE UNIT 8 400

Serial Number: 008736 Test Record Number: 1414
Test Date: 04/10/2025 Test Time: 11:03pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	11:03pm
FLO	Pass	11:03pm
FC	Pass	11:03pm

Temperature Tests

Test	Status	Time
FC1	Pass	11:03pm
SRC	Pass	11:03pm
DET	Pass	11:03pm
BAR	Pass	11:03pm
BT	Pass	11:03pm

Blank Tests

Test	Status	Time
AIR	Pass	11:04pm


Printer Tests

Test	Status	Time
PRNT	Pass	11:04pm

CRC Tests

Test	Status	Time
COMP	Pass	11:04pm
CAL	Pass	11:04pm

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Guilford Instrument Location BAT Mobile Unit 8
Instrument Serial No. 008775 Guilford SO

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 10 day of April, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature] Signature of Certifying Official 2219283 Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

GUILFORD COUNTY BAT MOBILE UNIT 8 400

Serial Number: 008775
Test Date: 04/10/2025

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: Glasscock, Jerry D
Permit Number: 7180-9235
Effective:
02/01/2025-02/01/2027

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG431002
Exp Date: 11/05/2026

Test	g/210L	Time
DIAG	Pass	10:53pm
AIR BLK	.00	10:54pm
ACCY CHK	.07	10:55pm
AIR BLK	.00	10:56pm
SUB TEST	.00	10:57pm
AIR BLK	.00	10:57pm
SUB TEST	.00	10:59pm
AIR BLK	.00	11:00pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

Intox EC/IR-II: Preventive Maintenance

GUILFORD COUNTY BAT MOBILE UNIT 8 400

Serial Number: 008775 Test Record Number: 2262
Test Date: 04/10/2025 Test Time: 11:02pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	11:03pm
FLO	Pass	11:03pm
FC	Pass	11:03pm

Temperature Tests

Test	Status	Time
FC1	Pass	11:03pm
SRC	Pass	11:03pm
DET	Pass	11:03pm
BAR	Pass	11:03pm
BT	Pass	11:03pm

Blank Tests

Test	Status	Time
AIR	Pass	11:03pm

Printer Tests

Test	Status	Time
PRNT	Pass	11:03pm

CRC Tests

Test	Status	Time
COMP	Pass	11:04pm
CAL	Pass	11:04pm

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

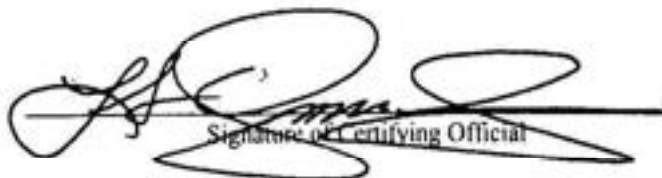
County GUILFORD Instrument Location GREENSBORO JAIL
Instrument Serial No. 008790 GREENSBORO, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 29TH day of APRIL, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.




Signature of Certifying Official

353799
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

GUILFORD COUNTY GREENSBORO JAIL 400

Serial Number: 008790
Test Date: 04/29/2025

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Oligmueller, Leo A

Permit Number: 0035-3799

Effective:

02/01/2025-02/01/2027

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG501307

Exp Date: 01/13/2027

Test	g/210L	Time
DIAG	Pass	10:21am
AIR BLK	.00	10:22am
ACCY CHK	.07	10:22am
AIR BLK	.00	10:23am
SUB TEST	.00	10:24am
AIR BLK	.00	10:25am
SUB TEST	.00	10:26am
AIR BLK	.00	10:27am

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

GUILFORD COUNTY GREENSBORO JAIL 400

Serial Number: 008790 Test Record Number: 8427
Test Date: 04/29/2025 Test Time: 10:31am EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	10:31am
FLO	Pass	10:31am
FC	Pass	10:31am

Temperature Tests

Test	Status	Time
FC1	Pass	10:31am
SRC	Pass	10:31am
DET	Pass	10:31am
BAR	Pass	10:31am
BT	Pass	10:31am

Blank Tests

Test	Status	Time
AIR	Pass	10:32am

Printer Tests

Test	Status	Time
PRNT	Pass	10:32am

CRC Tests

Test	Status	Time
COMP	Pass	10:32am
CAL	Pass	10:32am

Preventive Maintenance
Status: *Pass*


Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County GUILFORD Instrument Location GREENSBORO JAIL

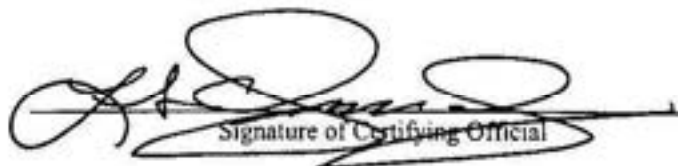
Instrument Serial No. 008794 GREENSBORO, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 29th day of APRIL, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.




Signature of Certifying Official

353799

Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

GUILFORD COUNTY GREENSBORO JAIL 400

Serial Number: 008794
Test Date: 04/29/2025

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Oligmueller, Leo A

Permit Number: 0035-3799

Effective:

02/01/2025-02/01/2027

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

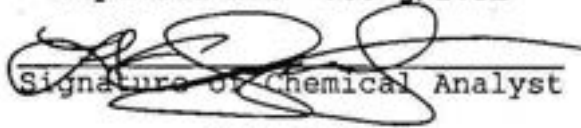
Test Type: Breath Test

Lot Number: AG431002

Exp Date: 11/05/2026

Test	g/210L	Time
DIAG	Pass	10:29am
AIR BLK	.00	10:30am
ACCY CHK	.07	10:30am
AIR BLK	.00	10:32am
SUB TEST	.00	10:33am
AIR BLK	.00	10:34am
SUB TEST	.00	10:36am
AIR BLK	.00	10:37am

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

GUILFORD COUNTY GREENSBORO JAIL 400

Serial Number: 008794 Test Record Number: 8866
Test Date: 04/29/2025 Test Time: 10:38am EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	10:39am
FLO	Pass	10:39am
FC	Pass	10:39am

Temperature Tests

Test	Status	Time
FC1	Pass	10:39am
SRC	Pass	10:39am
DET	Pass	10:39am
BAR	Pass	10:39am
BT	Pass	10:39am

Blank Tests

Test	Status	Time
AIR	Pass	10:40am

Printer Tests

Test	Status	Time
PRNT	Pass	10:40am

CRC Tests

Test	Status	Time
COMP	Pass	10:40am
CAL	Pass	10:40am

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Guilford Instrument Location BAT Mobile Unit 8
Instrument Serial No. 008816 Guilford SO

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 10 day of April, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

2219283
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

GUILFORD COUNTY BAT MOBILE UNIT 8 400

Serial Number: 008816

Test Date: 04/10/2025

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Glasscock, Jerry D

Permit Number: 7180-9235

Effective:

02/01/2025-02/01/2027

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG431002

Exp Date: 11/05/2026

Test	g/210L	Time
DIAG	Pass	10:55pm
AIR BLK	.00	10:56pm
ACCY CHK	.08	10:56pm
AIR BLK	.00	10:57pm
SUB TEST	.00	10:58pm
AIR BLK	.00	10:59pm
SUB TEST	.00	11:00pm
AIR BLK	.00	11:01pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

Intox EC/IR-II: Preventive Maintenance

GUILFORD COUNTY BAT MOBILE UNIT 8 400

Serial Number: 008816 Test Record Number: 7851
Test Date: 04/10/2025 Test Time: 11:02pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	11:02pm
FLO	Pass	11:02pm
FC	Pass	11:02pm

Temperature Tests

Test	Status	Time
FC1	Pass	11:02pm
SRC	Pass	11:02pm
DET	Pass	11:02pm
BAR	Pass	11:02pm
BT	Pass	11:02pm

Blank Tests

Test	Status	Time
AIR	Pass	11:03pm

Printer Tests

Test	Status	Time
PRNT	Pass	11:03pm

CRC Tests

Test	Status	Time
COMP	Pass	11:03pm
CAL	Pass	11:03pm

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Guilford Instrument Location BAT Mobile Unit 8
Instrument Serial No. 008929 Guilford 50

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 10 day of April, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature] 2219283
Signature of Certifying Official Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

GUILFORD COUNTY BAT MOBILE UNIT 8 400

Serial Number: 008929

Test Date: 04/10/2025

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Glasscock, Jerry D

Permit Number: 7180-9235

Effective:

02/01/2025-02/01/2027

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG506303

Exp Date: 03/04/2027

Test	g/210L	Time
DIAG	Pass	10:55pm
AIR BLK	.00	10:56pm
ACCY CHK	.07	10:57pm
AIR BLK	.00	10:58pm
SUB TEST	.00	10:59pm
AIR BLK	.00	11:00pm
SUB TEST	.00	11:01pm
AIR BLK	.00	11:02pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

This form is used when performing Preventive Maintenance procedures

Forensic Tests for Alcohol Branch

Department of Health and Human Services

Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

GUILFORD COUNTY BAT MOBILE UNIT 8 400

Serial Number: 008929 Test Record Number: 1551
Test Date: 04/10/2025 Test Time: 11:03pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	11:03pm
FLO	Pass	11:03pm
FC	Pass	11:03pm

Temperature Tests

Test	Status	Time
FC1	Pass	11:04pm
SRC	Pass	11:04pm
DET	Pass	11:04pm
BAR	Pass	11:04pm
BT	Pass	11:04pm

Blank Tests

Test	Status	Time
AIR	Pass	11:04pm

Printer Tests

Test	Status	Time
PRNT	Pass	11:04pm

CRC Tests

Test	Status	Time
COMP	Pass	11:05pm
CAL	Pass	11:05pm

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Holifax Instrument Location Holifax Co. S.O.
Instrument Serial No. 008695 355 FERRELL LANE
Holifax, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 23 day of April, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

179707
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

HALIFAX CO. HALIFAX CO SO 410

Serial Number: 008695

Test Date: 04/23/2025

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Bryant, Earl A

Permit Number: 0017-9707

Effective:

02/01/2025-02/01/2027

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG506303

Exp Date: 03/04/2027

Test	g/210L	Time
DIAG	Pass	6:41pm
AIR BLK	.00	6:42pm
ACCY CHK	.07	6:43pm
AIR BLK	.00	6:44pm
SUB TEST	.00	6:44pm
AIR BLK	.00	6:45pm
SUB TEST	.00	6:47pm
AIR BLK	.00	6:47pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

This form is used when performing Preventive Maintenance procedures

Forensic Tests for Alcohol Branch

Department of Health and Human Services

Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

HALIFAX CO. HALIFAX CO SO 410

Serial Number: 008695 Test Record Number: 3929
Test Date: 04/23/2025 Test Time: 6:48pm EDT

System Check: Passed

Baseline Tests

Test	Status	Time
IR	Pass	6:49pm
FLO	Pass	6:49pm
FC	Pass	6:49pm

Temperature Tests

Test	Status	Time
FC1	Pass	6:49pm
SRC	Pass	6:49pm
DET	Pass	6:49pm
BAR	Pass	6:49pm
BT	Pass	6:49pm

Blank Tests

Test	Status	Time
AIR	Pass	6:49pm

Printer Tests

Test	Status	Time
PRNT	Pass	6:49pm

CRC Tests

Test	Status	Time
COMP	Pass	6:50pm
CAL	Pass	6:50pm

Preventive Maintenance
Status: Pass


Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Henderson Instrument Location Henderson County Detention

Instrument Serial No. 008306 Hendersonville, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 15 day of April, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

244987
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

HENDERSON COUNTY HENDERSON COUNTY
DETENTION 440

Serial Number: 008806
Test Date: 04/15/2025

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE

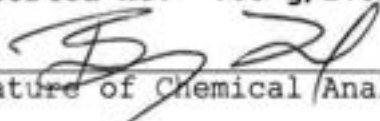
Analyst's Name: Loftis, Benjamin C
Permit Number: 0024-4987
Effective:
03/01/2025-03/01/2027

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG506301
Exp Date: 03/04/2027

Test	g/210L	Time
DIAG	Pass	11:11am
AIR BLK	.00	11:11am
ACCY CHK	.07	11:12am
AIR BLK	.00	11:13am
SUB TEST	.00	11:15am
AIR BLK	.00	11:16am
SUB TEST	.00	11:17am
AIR BLK	.00	11:18am

Reported AC: .00 g/210L



Signature of Chemical Analyst
Court CVR



Analyst

Intox EC/IR-II: Preventive Maintenance

HENDERSON COUNTY HENDERSON COUNTY DETENTION 440

Serial Number: 008806 Test Record Number: 3999
Test Date: 04/15/2025 Test Time: 11:18am EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	11:19am
FLO	Pass	11:19am
FC	Pass	11:19am

Temperature Tests

Test	Status	Time
FC1	Pass	11:19am
SRC	Pass	11:19am
DET	Pass	11:19am
BAR	Pass	11:19am
BT	Pass	11:19am

Blank Tests

Test	Status	Time
AIR	Pass	11:19am

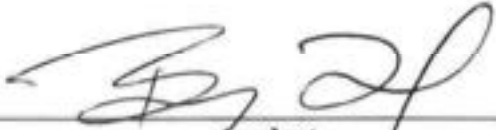
Printer Tests

Test	Status	Time
PRNT	Pass	11:19am

CRC Tests

Test	Status	Time
COMP	Pass	11:20am
CAL	Pass	11:20am

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County Henderson Instrument Location Henderson County Detention

Instrument Serial No. 009822 Hendersonville, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 15 day of April, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

244987
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

HENDERSON COUNTY HENDERSON COUNTY
DETENTION 440

Serial Number: 008822
Test Date: 04/15/2025

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE

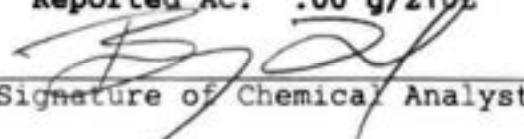
Analyst's Name: Loftis, Benjamin C
Permit Number: 0024-4987
Effective:
03/01/2025-03/01/2027

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test


Lot Number: AG405101
Exp Date: 02/20/2026

Test	g/210L	Time
DIAG	Pass	10:46am
AIR BLK	.00	10:47am
ACCY CHK	.07	10:47am
AIR BLK	.00	10:49am
SUB TEST	.00	10:49am
AIR BLK	.00	10:50am
SUB TEST	.00	10:52am
AIR BLK	.00	10:53am

Reported AC: .00 g/210L



Signature of Chemical Analyst
Court CVR



Analyst

Intox EC/IR-II: Preventive Maintenance

HENDERSON COUNTY HENDERSON COUNTY DETENTION 440

Serial Number: 008822 Test Record Number: 3494
Test Date: 04/15/2025 Test Time: 10:53am EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	10:53am
FLO	Pass	10:53am
FC	Pass	10:53am

Temperature Tests

Test	Status	Time
FC1	Pass	10:53am
SRC	Pass	10:53am
DET	Pass	10:53am
BAR	Pass	10:53am
BT	Pass	10:53am

Blank Tests

Test	Status	Time
AIR	Pass	10:54am

Printer Tests

Test	Status	Time
PRNT	Pass	10:54am

CRC Tests

Test	Status	Time
COMP	Pass	10:54am
CAL	Pass	10:54am

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Iredell Instrument Location BAT Mobile Unit 8
Instrument Serial No. 008615 Statesville PD

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 25 day of April, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

2219283
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

IREDELL COUNTY BAT MOBILE UNIT 8 480

Serial Number: 008615
Test Date: 04/25/2025

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE

Analyst's Name: Glasscock, Jerry D
Permit Number: 7180-9235
Effective:
02/01/2025-02/01/2027

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG405102
Exp Date: 02/20/2026

Test	g/210L	Time
DIAG	Pass	9:36pm
AIR BLK	.00	9:37pm
ACCY CHK	.07	9:38pm
AIR BLK	.00	9:39pm
SUB TEST	.00	9:40pm
AIR BLK	.00	9:41pm
SUB TEST	.00	9:42pm
AIR BLK	.00	9:43pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

Intox EC/IR-II: Preventive Maintenance

IREDELL COUNTY BAT MOBILE UNIT 8 480

Serial Number: 008615 Test Record Number: 6079
Test Date: 04/25/2025 Test Time: 9:47pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	9:47pm
FLO	Pass	9:47pm
FC	Pass	9:47pm

Temperature Tests

Test	Status	Time
FC1	Pass	9:47pm
SRC	Pass	9:47pm
DET	Pass	9:47pm
BAR	Pass	9:47pm
BT	Pass	9:47pm

Blank Tests

Test	Status	Time
AIR	Pass	9:48pm


Printer Tests

Test	Status	Time
PRNT	Pass	9:48pm

CRC Tests

Test	Status	Time
COMP	Pass	9:48pm
CAL	Pass	9:48pm

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County IRENELL Instrument Location STATESVILLE PD

Instrument Serial No. 008619 STATESVILLE NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 02 day of APRIL, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

274970
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

IREDELL COUNTY STATESVILLE PD 480

Serial Number: 008619
Test Date: 04/02/2025

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: Fleming, Tina S
Permit Number: 0027-4970
Effective:
10/01/2023-10/01/2025

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test


Lot Number: AG405102
Exp Date: 02/20/2026

Test	g/210L	Time
DIAG	Pass	1:59pm
AIR BLK	.00	1:59pm
ACCY CHK	.07	2:00pm
AIR BLK	.00	2:01pm
SUB TEST	.00	2:02pm
AIR BLK	.00	2:02pm
SUB TEST	.00	2:04pm
AIR BLK	.00	2:05pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

IREDELL COUNTY STATESVILLE PD 480

Serial Number: 008619 Test Record Number: 2256
Test Date: 04/02/2025 Test Time: 2:06pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	2:06pm
FLO	Pass	2:06pm
FC	Pass	2:07pm

Temperature Tests

Test	Status	Time
FC1	Pass	2:07pm
SRC	Pass	2:07pm
DET	Pass	2:07pm
BAR	Pass	2:07pm
BT	Pass	2:07pm

Blank Tests

Test	Status	Time
AIR	Pass	2:07pm

Printer Tests

Test	Status	Time
PRNT	Pass	2:07pm

CRC Tests

Test	Status	Time
COMP	Pass	2:07pm
CAL	Pass	2:07pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County IREDELL Instrument Location MOORESVILLE PD

Instrument Serial No. 008685 MOORESVILLE NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 02 day of APRIL, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

274970
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

IREDELL COUNTY MOORESVILLE PD 480

Serial Number: 008685
Test Date: 04/02/2025

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Fleming, Tina S

Permit Number: 0027-4970

Effective:

10/01/2023-10/01/2025

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

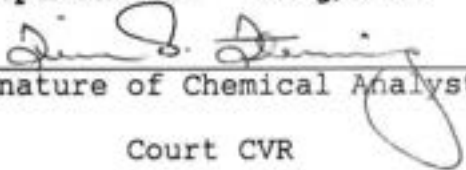
Test Type: Breath Test

Lot Number: AG431001

Exp Date: 11/05/2026

Test	g/210L	Time
DIAG	Pass	12:52pm
AIR BLK	.00	12:53pm
ACCY CHK	.08	12:54pm
AIR BLK	.00	12:55pm
SUB TEST	.00	12:56pm
AIR BLK	.00	12:57pm
SUB TEST	.00	12:59pm
AIR BLK	.00	1:00pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

IREDELL COUNTY MOORESVILLE PD 480

Serial Number: 008685 Test Record Number: 4991
Test Date: 04/02/2025 Test Time: 1:01pm EDT

System Check: Passed

Baseline Tests

Test	Status	Time
IR	Pass	1:01pm
FLO	Pass	1:01pm
FC	Pass	1:01pm

Temperature Tests

Test	Status	Time
FC1	Pass	1:01pm
SRC	Pass	1:01pm
DET	Pass	1:01pm
BAR	Pass	1:01pm
BT	Pass	1:01pm

Blank Tests

Test	Status	Time
AIR	Pass	1:02pm


Printer Tests

Test	Status	Time
PRNT	Pass	1:02pm

CRC Tests

Test	Status	Time
COMP	Pass	1:02pm
CAL	Pass	1:02pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Iredell Instrument Location BAT Mobile Unit 8
Instrument Serial No. 008736 Statesville PD

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 25 day of April, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

2219283
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

IREDELL COUNTY BAT MOBILE UNIT 8 480

Serial Number: 008736
Test Date: 04/25/2025

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: Glasscock, Jerry D
Permit Number: 7180-9235
Effective:
02/01/2025-02/01/2027

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test


Lot Number: AG405102
Exp Date: 02/20/2026

Test	g/210L	Time
DIAG	Pass	9:37pm
AIR BLK	.00	9:38pm
ACCY CHK	.07	9:39pm
AIR BLK	.00	9:40pm
SUB TEST	.00	9:40pm
AIR BLK	.00	9:41pm
SUB TEST	.00	9:43pm
AIR BLK	.00	9:44pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

Intox EC/IR-II: Preventive Maintenance

IREDELL COUNTY BAT MOBILE UNIT 8 480

Serial Number: 008736 Test Record Number: 1430
Test Date: 04/25/2025 Test Time: 9:46pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	9:47pm
FLO	Pass	9:47pm
FC	Pass	9:47pm

Temperature Tests

Test	Status	Time
FC1	Pass	9:47pm
SRC	Pass	9:47pm
DET	Pass	9:47pm
BAR	Pass	9:47pm
BT	Pass	9:47pm

Blank Tests

Test	Status	Time
AIR	Pass	9:48pm


Printer Tests

Test	Status	Time
PRNT	Pass	9:48pm

CRC Tests

Test	Status	Time
COMP	Pass	9:48pm
CAL	Pass	9:48pm

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Tredwell Instrument Location BAT Mobile Unit 8
Instrument Serial No. 008816 Statesville PD

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 25 day of April, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

2219283
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

IREDELL COUNTY BAT MOBILE UNIT 8 480

Serial Number: 008816
Test Date: 04/25/2025

Citation Number: M0000000-0
Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Glasscock, Jerry D

Permit Number: 7180-9235

Effective:

02/01/2025-02/01/2027

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG431002

Exp Date: 11/05/2026

Test	g/210L	Time
DIAG	Pass	9:38pm
AIR BLK	.00	9:39pm
ACCY CHK	.08	9:39pm
AIR BLK	.00	9:40pm
SUB TEST	.00	9:41pm
AIR BLK	.00	9:42pm
SUB TEST	.00	9:43pm
AIR BLK	.00	9:44pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

Intox EC/IR-II: Preventive Maintenance

IREDELL COUNTY BAT MOBILE UNIT 8 480

Serial Number: 008816 Test Record Number: 7867
Test Date: 04/25/2025 Test Time: 9:48pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	9:48pm
FLO	Pass	9:48pm
FC	Pass	9:48pm

Temperature Tests

Test	Status	Time
FC1	Pass	9:48pm
SRC	Pass	9:48pm
DET	Pass	9:48pm
BAR	Pass	9:48pm
BT	Pass	9:48pm

Blank Tests

Test	Status	Time
AIR	Pass	9:49pm

Printer Tests

Test	Status	Time
PRNT	Pass	9:49pm

CRC Tests

Test	Status	Time
COMP	Pass	9:49pm
CAL	Pass	9:49pm

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County IRENELL Instrument Location MOOREVILLE PD
Instrument Serial No. 008823 MOOREVILLE NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 02 day of APRIL, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

274970
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

IREDELL COUNTY MOORESVILLE PD 480

Serial Number: 008823
Test Date: 04/02/2025

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: Fleming, Tina S
Permit Number: 0027-4970
Effective:
10/01/2023-10/01/2025

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG405102
Exp Date: 02/20/2026

Test	g/210L	Time
DIAG	Pass	12:50pm
AIR BLK	.00	12:51pm
ACCY CHK	.08	12:51pm
AIR BLK	.00	12:52pm
SUB TEST	.00	12:53pm
AIR BLK	.00	12:54pm
SUB TEST	.00	12:56pm
AIR BLK	.00	12:56pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

IREDELL COUNTY MOORESVILLE PD 480

Serial Number: 008823 Test Record Number: 2108
Test Date: 04/02/2025 Test Time: 12:58pm EDT

System Check: Passed

Baseline Tests

Test	Status	Time
IR	Pass	12:58pm
FLO	Pass	12:58pm
FC	Pass	12:58pm

Temperature Tests

Test	Status	Time
FC1	Pass	12:58pm
SRC	Pass	12:58pm
DET	Pass	12:58pm
BAR	Pass	12:58pm
BT	Pass	12:58pm

Blank Tests

Test	Status	Time
AIR	Pass	12:59pm


Printer Tests

Test	Status	Time
PRNT	Pass	12:59pm

CRC Tests

Test	Status	Time
COMP	Pass	12:59pm
CAL	Pass	12:59pm

Preventive Maintenance
Status: Pass



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Iredell Instrument Location BAT Mobile Unit 8
Instrument Serial No. 008929 Statesville PD

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 25 day of April, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

2219283
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

IREDELL COUNTY BAT MOBILE UNIT 8 480

Serial Number: 008929

Test Date: 04/25/2025

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Glasscock, Jerry D

Permit Number: 7180-9235

Effective:

02/01/2025-02/01/2027

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG506303

Exp Date: 03/04/2027

Test	g/210L	Time
DIAG	Pass	9:48pm
AIR BLK	.00	9:49pm
ACCY CHK	.07	9:50pm
AIR BLK	.00	9:51pm
SUB TEST	.00	9:52pm
AIR BLK	.00	9:53pm
SUB TEST	.00	9:55pm
AIR BLK	.00	9:56pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

Intox EC/IR-II: Preventive Maintenance

IREDELL COUNTY BAT MOBILE UNIT 8 480

Serial Number: 008929 Test Record Number: 1569
Test Date: 04/25/2025 Test Time: 9:58pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	9:58pm
FLO	Pass	9:58pm
FC	Pass	9:58pm

Temperature Tests

Test	Status	Time
FC1	Pass	9:59pm
SRC	Pass	9:59pm
DET	Pass	9:59pm
BAR	Pass	9:59pm
BT	Pass	9:59pm

Blank Tests

Test	Status	Time
AIR	Pass	9:59pm


Printer Tests

Test	Status	Time
PRNT	Pass	9:59pm

CRC Tests

Test	Status	Time
COMP	Pass	10:00pm
CAL	Pass	10:00pm

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Jackson Instrument Location Jackson Co. Jail
Instrument Serial No. 008708 Sylva, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 1st day of April, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



David R. Luth

Signature of Certifying Official

843310

Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

JACKSON COUNTY JAIL 490

Serial Number: 008708
Test Date: 04/01/2025

Citation Number: M0000000-0
Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Cutler, Daniel R

Permit Number: 0084-3310

Effective:

02/01/2025-02/01/2027

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG431002

Exp Date: 11/05/2026

Test	g/210L	Time
DIAG	Pass	11:51am
AIR BLK	.00	11:51am
ACCY CHK	.07	11:52am
AIR BLK	.00	11:53am
SUB TEST	.00	11:54am
AIR BLK	.00	11:55am
SUB TEST	.00	11:56am
AIR BLK	.00	11:57am

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

Intox EC/IR-II: Preventive Maintenance

JACKSON COUNTY JAIL 490

Serial Number: 008708 Test Record Number: 2026
Test Date: 04/01/2025 Test Time: 11:57am EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	11:58am
FLO	Pass	11:58am
FC	Pass	11:58am

Temperature Tests

Test	Status	Time
FC1	Pass	11:58am
SRC	Pass	11:58am
DET	Pass	11:58am
BAR	Pass	11:58am
BT	Pass	11:58am

Blank Tests

Test	Status	Time
AIR	Pass	11:58am

Printer Tests

Test	Status	Time
PRNT	Pass	11:59am

CRC Tests

Test	Status	Time
COMP	Pass	11:59am
CAL	Pass	11:59am

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Jackson Instrument Location Jackson Co. Jail
Instrument Serial No. 008732 Sylva, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 1st day of April, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Chris R. Luth
Signature of Certifying Official

843310
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

JACKSON COUNTY JACKSON COUNTY JAIL 490

Serial Number: 008722
Test Date: 04/01/2025

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: Cutler, Daniel R
Permit Number: 0084-3310
Effective:
02/01/2025-02/01/2027

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG431002
Exp Date: 11/05/2026

Test	g/210L	Time
DIAG	Pass	11:52am
AIR BLK	.00	11:53am
ACCY CHK	.07	11:53am
AIR BLK	.00	11:55am
SUB TEST	.00	11:55am
AIR BLK	.00	11:56am
SUB TEST	.00	11:58am
AIR BLK	.00	11:59am

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

Intox EC/IR-II: Preventive Maintenance

JACKSON COUNTY JACKSON COUNTY JAIL 490

Serial Number: 008722 Test Record Number: 1635
Test Date: 04/01/2025 Test Time: 11:59am EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	11:59am
FLO	Pass	11:59am
FC	Pass	11:59am

Temperature Tests

Test	Status	Time
FC1	Pass	11:59am
SRC	Pass	11:59am
DET	Pass	11:59am
BAR	Pass	11:59am
BT	Pass	11:59am

Blank Tests

Test	Status	Time
AIR	Pass	12:00pm

Printer Tests

Test	Status	Time
PRNT	Pass	12:00pm

CRC Tests

Test	Status	Time
COMP	Pass	12:00pm
CAL	Pass	12:00pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Jackson Instrument Location BAT Mobile Unit II
Instrument Serial No. 008970 Jackson S.O.

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 18th day of April, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



John Parier
Signature of Certifying Official

1604930
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

JACKSON COUNTY BAT MOBILE UNIT 11 490

Serial Number: 008970
Test Date: 04/18/2025

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE

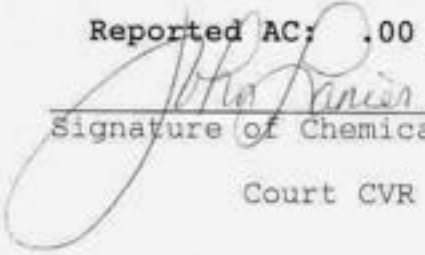
Analyst's Name: Lanier Jr., John P
Permit Number: 4582-9118
Effective:
03/01/2025-03/01/2027

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG417802
Exp Date: 06/26/2026

Test	g/210L	Time
DIAG	Pass	8:59pm
AIR BLK	.00	9:00pm
ACCY CHK	.07	9:01pm
AIR BLK	.00	9:02pm
SUB TEST	.00	9:03pm
AIR BLK	.00	9:03pm
SUB TEST	.00	9:05pm
AIR BLK	.00	9:06pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

JACKSON COUNTY BAT MOBILE UNIT 11 490

Serial Number: 008970 Test Record Number: 1196
Test Date: 04/18/2025 Test Time: 9:06pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	9:07pm
FLO	Pass	9:07pm
FC	Pass	9:07pm

Temperature Tests

Test	Status	Time
FC1	Pass	9:07pm
SRC	Pass	9:07pm
DET	Pass	9:07pm
BAR	Pass	9:07pm
BT	Pass	9:07pm

Blank Tests

Test	Status	Time
AIR	Pass	9:08pm

Printer Tests

Test	Status	Time
PRNT	Pass	9:08pm

CRC Tests

Test	Status	Time
COMP	Pass	9:08pm
CAL	Pass	9:08pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Jackson Instrument Location Bat Mobile Unit 11
Instrument Serial No. 008973 Jackson 50

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 18th day of April, 2023 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Jeff B. [Signature]
Signature of Certifying Official

6-2446
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

JACKSON COUNTY BAT MOBILE UNIT 11 490

Serial Number: 008973
Test Date: 04/18/2025

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Gillstrap, Jeffrey L

Permit Number: 6-2446

Effective:

12/01/2023-12/01/2025

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG431003

Exp Date: 11/05/2026


Test	g/210L	Time
DIAG	Pass	8:45pm
AIR BLK	.00	8:46pm
ACCY CHK	.07	8:46pm
AIR BLK	.00	8:47pm
SUB TEST	.00	8:48pm
AIR BLK	.00	8:48pm
SUB TEST	.00	8:50pm
AIR BLK	.00	8:51pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

JACKSON COUNTY BAT MOBILE UNIT 11 490

Serial Number: 008973 Test Record Number: 1246
Test Date: 04/18/2025 Test Time: 8:52pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	8:52pm
FLO	Pass	8:52pm
FC	Pass	8:53pm

Temperature Tests

Test	Status	Time
FC1	Pass	8:53pm
SRC	Pass	8:53pm
DET	Pass	8:53pm
BAR	Pass	8:53pm
BT	Pass	8:53pm

Blank Tests

Test	Status	Time
AIR	Pass	8:53pm

Printer Tests

Test	Status	Time
PRNT	Pass	8:53pm

CRC Tests

Test	Status	Time
COMP	Pass	8:53pm
CAL	Pass	8:53pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Johnston Instrument Location BAT Mobile Unit 8
Instrument Serial No. 008615 Clayton PD

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 12 day of April, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

2219283
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

JOHNSTON COUNTY BAT MOBILE UNIT 8 500

Serial Number: 008615
Test Date: 04/12/2025

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: Glasscock, Jerry D
Permit Number: 7180-9235
Effective:
02/01/2025-02/01/2027

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG405102
Exp Date: 02/20/2026

Test	g/210L	Time
DIAG	Pass	9:34pm
AIR BLK	.00	9:35pm
ACCY CHK	.08	9:36pm
AIR BLK	.00	9:37pm
SUB TEST	.00	9:38pm
AIR BLK	.00	9:39pm
SUB TEST	.00	9:40pm
AIR BLK	.00	9:41pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

Intox EC/IR-II: Preventive Maintenance

JOHNSTON COUNTY BAT MOBILE UNIT 8 500

Serial Number: 008615 Test Record Number: 6064
Test Date: 04/12/2025 Test Time: 9:42pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	9:42pm
FLO	Pass	9:42pm
FC	Pass	9:43pm

Temperature Tests

Test	Status	Time
FC1	Pass	9:43pm
SRC	Pass	9:43pm
DET	Pass	9:43pm
BAR	Pass	9:43pm
BT	Pass	9:43pm

Blank Tests

Test	Status	Time
AIR	Pass	9:43pm

Printer Tests

Test	Status	Time
PRNT	Pass	9:43pm

CRC Tests

Test	Status	Time
COMP	Pass	9:44pm
CAL	Pass	9:44pm

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Johnston Instrument Location BAT Mobile Unit 8

Instrument Serial No. 008736 Clayton PD

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 12 day of April, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

2219283
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

JOHNSTON COUNTY BAT MOBILE UNIT 8 500

Serial Number: 008736
Test Date: 04/12/2025

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE

Analyst's Name: Glasscock, Jerry D
Permit Number: 7180-9235
Effective:
02/01/2025-02/01/2027

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test


Lot Number: AG405102
Exp Date: 02/20/2026

Test	g/210L	Time
DIAG	Pass	9:35pm
AIR BLK	.00	9:36pm
ACCY CHK	.07	9:36pm
AIR BLK	.00	9:37pm
SUB TEST	.00	9:38pm
AIR BLK	.00	9:39pm
SUB TEST	.00	9:40pm
AIR BLK	.00	9:41pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

Intox EC/IR-II: Preventive Maintenance

JOHNSTON COUNTY BAT MOBILE UNIT 8 500

Serial Number: 008736 Test Record Number: 1418
Test Date: 04/12/2025 Test Time: 9:42pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	9:42pm
FLO	Pass	9:42pm
FC	Pass	9:43pm

Temperature Tests

Test	Status	Time
FC1	Pass	9:43pm
SRC	Pass	9:43pm
DET	Pass	9:43pm
BAR	Pass	9:43pm
BT	Pass	9:43pm

Blank Tests

Test	Status	Time
AIR	Pass	9:43pm


Printer Tests

Test	Status	Time
PRNT	Pass	9:43pm

CRC Tests

Test	Status	Time
COMP	Pass	9:44pm
CAL	Pass	9:44pm

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County Johnston Instrument Location BAT Mobile Unit 8
Instrument Serial No. 008775 Clayton PD

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 12 day of April, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Jerry D. [Signature] 2219283
Signature of Certifying Official Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

JOHNSTON COUNTY BAT MOBILE UNIT 8 500

Serial Number: 008775
Test Date: 04/12/2025

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: Glasscock, Jerry D
Permit Number: 7180-9235
Effective:
02/01/2025-02/01/2027

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test


Lot Number: AG431002
Exp Date: 11/05/2026

Test	g/210L	Time
DIAG	Pass	9:39pm
AIR BLK	.00	9:40pm
ACCY CHK	.07	9:40pm
AIR BLK	.00	9:41pm
SUB TEST	.00	9:42pm
AIR BLK	.00	9:43pm
SUB TEST	.00	9:44pm
AIR BLK	.00	9:45pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

Intox EC/IR-II: Preventive Maintenance

JOHNSTON COUNTY BAT MOBILE UNIT 8 500

Serial Number: 008775 Test Record Number: 2267
Test Date: 04/12/2025 Test Time: 9:46pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	9:46pm
FLO	Pass	9:46pm
FC	Pass	9:46pm

Temperature Tests

Test	Status	Time
FC1	Pass	9:46pm
SRC	Pass	9:46pm
DET	Pass	9:46pm
BAR	Pass	9:46pm
BT	Pass	9:46pm

Blank Tests

Test	Status	Time
AIR	Pass	9:47pm

Printer Tests

Test	Status	Time
PRNT	Pass	9:47pm

CRC Tests

Test	Status	Time
COMP	Pass	9:47pm
CAL	Pass	9:47pm

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Johnston Instrument Location BAT Mobile Unit 8
Instrument Serial No. 008816 Clayton PD

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 12 day of April, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature] 2219283
Signature of Certifying Official Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

JOHNSTON COUNTY BAT MOBILE UNIT 8 500

Serial Number: 008816
Test Date: 04/12/2025

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: Glasscock, Jerry D
Permit Number: 7180-9235
Effective:
02/01/2025-02/01/2027

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG431002
Exp Date: 11/05/2026

Test	g/210L	Time
DIAG	Pass	9:38pm
AIR BLK	.00	9:39pm
ACCY CHK	.08	9:40pm
AIR BLK	.00	9:41pm
SUB TEST	.00	9:42pm
AIR BLK	.00	9:43pm
SUB TEST	.00	9:45pm
AIR BLK	.00	9:46pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

Intox EC/IR-II: Preventive Maintenance

JOHNSTON COUNTY BAT MOBILE UNIT 8 500

Serial Number: 008816 Test Record Number: 7855
Test Date: 04/12/2025 Test Time: 9:49pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	9:49pm
FLO	Pass	9:49pm
FC	Pass	9:49pm

Temperature Tests

Test	Status	Time
FC1	Pass	9:50pm
SRC	Pass	9:50pm
DET	Pass	9:50pm
BAR	Pass	9:50pm
BT	Pass	9:50pm

Blank Tests

Test	Status	Time
AIR	Pass	9:50pm

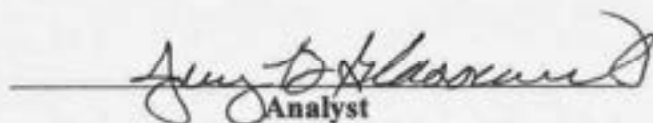
Printer Tests

Test	Status	Time
PRNT	Pass	9:50pm

CRC Tests

Test	Status	Time
COMP	Pass	9:50pm
CAL	Pass	9:50pm

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Johnston Instrument Location Johnston County
Instrument Serial No. 008846 Detention Center

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 9 day of April, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

365156
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

JOHNSTON COUNTY DETENTION CENTER 500

Serial Number: 008846
Test Date: 04/09/2025

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: Garner, Joel K
Permit Number: 0036-5156
Effective:
02/01/2025-02/01/2027

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG431003
Exp Date: 11/05/2026

Test	g/210L	Time
DIAG	Pass	9:09am
AIR BLK	.00	9:10am
ACCY CHK	.08	9:10am
AIR BLK	.00	9:12am
SUB TEST	.00	9:12am
AIR BLK	.00	9:13am
SUB TEST	.00	9:14am
AIR BLK	.00	9:15am

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

Intox EC/IR-II: Preventive Maintenance

JOHNSTON COUNTY DETENTION CENTER 500

Serial Number: 008846 Test Record Number: 6361
Test Date: 04/09/2025 Test Time: 9:16am EDT

System Check: Passed

Baseline Tests

Test	Status	Time
IR	Pass	9:16am
FLO	Pass	9:16am
FC	Pass	9:16am

Temperature Tests

Test	Status	Time
FC1	Pass	9:16am
SRC	Pass	9:16am
DET	Pass	9:16am
BAR	Pass	9:16am
BT	Pass	9:16am

Blank Tests

Test	Status	Time
AIR	Pass	9:17am


Printer Tests

Test	Status	Time
PRNT	Pass	9:17am

CRC Tests

Test	Status	Time
COMP	Pass	9:17am
CAL	Pass	9:17am

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Johnston Instrument Location BAT Mobile Unit 8

Instrument Serial No. 008929 Clayton PD

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 12 day of April, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

2219283
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

JOHNSTON COUNTY BAT MOBILE UNIT 8 500

Serial Number: 008929

Test Date: 04/12/2025

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Glasscock, Jerry D

Permit Number: 7180-9235

Effective:

02/01/2025-02/01/2027

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG506303

Exp Date: 03/04/2027

Test	g/210L	Time
DIAG	Pass	9:36pm
AIR BLK	.00	9:37pm
ACCY CHK	.08	9:38pm
AIR BLK	.00	9:39pm
SUB TEST	.00	9:40pm
AIR BLK	.00	9:41pm
SUB TEST	.00	9:42pm
AIR BLK	.00	9:43pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

Intox EC/IR-II: Preventive Maintenance

JOHNSTON COUNTY BAT MOBILE UNIT 8 500

Serial Number: 008929 Test Record Number: 1556
Test Date: 04/12/2025 Test Time: 9:45pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	9:45pm
FLO	Pass	9:45pm
FC	Pass	9:45pm

Temperature Tests

Test	Status	Time
FC1	Pass	9:45pm
SRC	Pass	9:45pm
DET	Pass	9:45pm
BAR	Pass	9:45pm
BT	Pass	9:45pm

Blank Tests

Test	Status	Time
AIR	Pass	9:46pm

Printer Tests

Test	Status	Time
PRNT	Pass	9:46pm

CRC Tests

Test	Status	Time
COMP	Pass	9:46pm
CAL	Pass	9:46pm

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Madison Instrument Location Mars Hill PD

Instrument Serial No. 008582 Mars Hill, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 1 day of April, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Handwritten Signature]
Signature of Certifying Official

244987
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

MADISON COUNTY MARS HILL PD 560

Serial Number: 008582

Test Date: 04/01/2025

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Loftis, Benjamin C

Permit Number: 0024-4987

Effective:

10/01/2023-10/01/2025

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG400303

Exp Date: 01/03/2026

Test	g/210L	Time
DIAG	Pass	11:03am
AIR BLK	.00	11:04am
ACCY CHK	.07	11:04am
AIR BLK	.00	11:06am
SUB TEST	.00	11:06am
AIR BLK	.00	11:07am
SUB TEST	.00	11:09am
AIR BLK	.00	11:09am

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

MADISON COUNTY MARS HILL PD 560

Serial Number: 008582 Test Record Number: 1307
Test Date: 04/01/2025 Test Time: 11:12am EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	11:13am
FLO	Pass	11:13am
FC	Pass	11:13am

Temperature Tests

Test	Status	Time
FC1	Pass	11:13am
SRC	Pass	11:13am
DET	Pass	11:13am
BAR	Pass	11:13am
BT	Pass	11:13am

Blank Tests

Test	Status	Time
AIR	Pass	11:14am


Printer Tests

Test	Status	Time
PRNT	Pass	11:14am

CRC Tests

Test	Status	Time
COMP	Pass	11:14am
CAL	Pass	11:14am

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Madison Instrument Location Madison County Jail

Instrument Serial No. 008599 Marshall, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 1 day of April, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

244987
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

MADISON COUNTY MADISON COUNTY JAIL 560

Serial Number: 008599
Test Date: 04/01/2025

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Loftis, Benjamin C

Permit Number: 0024-4987

Effective:

10/01/2023-10/01/2025

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG503001
Exp Date: 01/30/2027

Test	g/210L	Time
DIAG	Pass	12:19pm
AIR BLK	.00	12:20pm
ACCY CHK	.07	12:20pm
AIR BLK	.00	12:22pm
SUB TEST	.00	12:22pm
AIR BLK	.00	12:23pm
SUB TEST	.00	12:24pm
AIR BLK	.00	12:25pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

MADISON COUNTY MADISON COUNTY JAIL 560

Serial Number: 008599 Test Record Number: 1515
Test Date: 04/01/2025 Test Time: 12:26pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	12:26pm
FLO	Pass	12:26pm
FC	Pass	12:26pm

Temperature Tests

Test	Status	Time
FC1	Pass	12:26pm
SRC	Pass	12:26pm
DET	Pass	12:26pm
BAR	Pass	12:26pm
BT	Pass	12:26pm

Blank Tests

Test	Status	Time
AIR	Pass	12:27pm


Printer Tests

Test	Status	Time
PRNT	Pass	12:27pm

CRC Tests

Test	Status	Time
COMP	Pass	12:27pm
CAL	Pass	12:27pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Martin Instrument Location Martin Co. S.O.
Instrument Serial No. 008912 305 E. Main St.
Williamston, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 1st day of April, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Mary A. Puppell 206272
Signature of Certifying Official Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

MARTIN COUNTY SHERIFF'S OFFICE 570

Serial Number: 008912
Test Date: 04/01/2025

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE

Analyst's Name: Chappell, Mark A
Permit Number: 0020-6272
Effective:
02/01/2025-02/01/2027

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG431001
Exp Date: 11/05/2026

Test	g/210L	Time
DIAG	Pass	11:36am
AIR BLK	.00	11:37am
ACCY CHK	.08	11:37am
AIR BLK	.00	11:39am
SUB TEST	.00	11:40am
AIR BLK	.00	11:41am
SUB TEST	.00	11:42am
AIR BLK	.00	11:43am

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

MARTIN COUNTY SHERIFF'S OFFICE 570

Serial Number: 008912 Test Record Number: 2277
Test Date: 04/01/2025 Test Time: 11:45am EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	11:45am
FLO	Pass	11:45am
FC	Pass	11:45am

Temperature Tests

Test	Status	Time
FC1	Pass	11:45am
SRC	Pass	11:45am
DET	Pass	11:45am
BAR	Pass	11:45am
BT	Pass	11:45am

Blank Tests

Test	Status	Time
AIR	Pass	11:46am

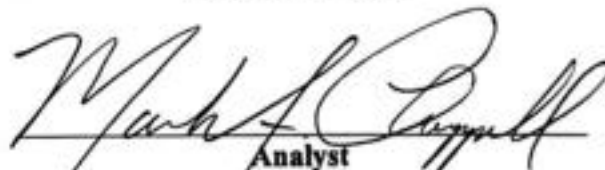
Printer Tests

Test	Status	Time
PRNT	Pass	11:46am

CRC Tests

Test	Status	Time
COMP	Pass	11:46am
CAL	Pass	11:46am

Preventive Maintenance
Status: Pass


Analyst

Intox EC/IR-II: Subject Test

MECKLENBURG COUNTY BAT MOBILE UNIT 8
590

Serial Number: 008615
Test Date: 04/16/2025

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE

Analyst's Name: Glasscock, Jerry D
Permit Number: 7180-9235
Effective:
02/01/2025-02/01/2027

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG405102
Exp Date: 02/20/2026

Test	g/210L	Time
DIAG	Pass	9:26pm
AIR BLK	.00	9:27pm
ACCY CHK	.07	9:27pm
AIR BLK	.00	9:28pm
SUB TEST	.00	9:29pm
AIR BLK	.00	9:30pm
SUB TEST	.00	9:31pm
AIR BLK	.00	9:32pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

MECKLENBURG COUNTY BAT MOBILE UNIT 8 590

Serial Number: 008615 Test Record Number: 6070
Test Date: 04/16/2025 Test Time: 9:32pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	9:33pm
FLO	Pass	9:33pm
FC	Pass	9:33pm

Temperature Tests

Test	Status	Time
FC1	Pass	9:33pm
SRC	Pass	9:33pm
DET	Pass	9:33pm
BAR	Pass	9:33pm
BT	Pass	9:33pm

Blank Tests

Test	Status	Time
AIR	Pass	9:34pm

Printer Tests

Test	Status	Time
PRNT	Pass	9:34pm

CRC Tests

Test	Status	Time
COMP	Pass	9:34pm
CAL	Pass	9:34pm

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Mecklenburg Instrument Location BAT Mobile Unit 8
Instrument Serial No. 008615 CMPO

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 17 day of April, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

2219283
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

MECKLENBURG COUNTY BAT MOBILE UNIT 8
590

Serial Number: 008615
Test Date: 04/17/2025

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Glasscock, Jerry D

Permit Number: 7180-9235

Effective:

02/01/2025-02/01/2027

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG405102


Exp Date: 02/20/2026

Test	g/210L	Time
DIAG	Pass	9:22pm
AIR BLK	.00	9:23pm
ACCY CHK	.07	9:24pm
AIR BLK	.00	9:24pm
SUB TEST	.00	9:25pm
AIR BLK	.00	9:26pm
SUB TEST	.00	9:27pm
AIR BLK	.00	9:28pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

MECKLENBURG COUNTY BAT MOBILE UNIT 8 590

Serial Number: 008615 Test Record Number: 6072
Test Date: 04/17/2025 Test Time: 9:30pm EDT

System Check: Passed

Baseline Tests

Test	Status	Time
IR	Pass	9:31pm
FLO	Pass	9:31pm
FC	Pass	9:31pm

Temperature Tests

Test	Status	Time
FC1	Pass	9:31pm
SRC	Pass	9:31pm
DET	Pass	9:31pm
BAR	Pass	9:31pm
BT	Pass	9:31pm

Blank Tests

Test	Status	Time
AIR	Pass	9:31pm

Printer Tests

Test	Status	Time
PRNT	Pass	9:32pm

CRC Tests

Test	Status	Time
COMP	Pass	9:32pm
CAL	Pass	9:32pm

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Mecklenburg Instrument Location BAT Mobile Unit 8
Instrument Serial No. 008615 Mint Hill PD

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 22 day of April, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

2219283
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

MECKLENBURG COUNTY BAT MOBILE UNIT 8
590

Serial Number: 008615
Test Date: 04/22/2025

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE

Analyst's Name: Glasscock, Jerry D
Permit Number: 7180-9235
Effective:
02/01/2025-02/01/2027

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG405102
Exp Date: 02/20/2026

Test	g/210L	Time
DIAG	Pass	8:45pm
AIR BLK	.00	8:46pm
ACCY CHK	.07	8:47pm
AIR BLK	.00	8:48pm
SUB TEST	.00	8:49pm
AIR BLK	.00	8:49pm
SUB TEST	.00	8:51pm
AIR BLK	.00	8:52pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

Intox EC/IR-II: Preventive Maintenance

MECKLENBURG COUNTY BAT MOBILE UNIT 8 590

Serial Number: 008615 Test Record Number: 6075
Test Date: 04/22/2025 Test Time: 8:53pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	8:53pm
FLO	Pass	8:53pm
FC	Pass	8:53pm

Temperature Tests

Test	Status	Time
FC1	Pass	8:53pm
SRC	Pass	8:53pm
DET	Pass	8:53pm
BAR	Pass	8:53pm
BT	Pass	8:53pm

Blank Tests

Test	Status	Time
AIR	Pass	8:54pm

Printer Tests

Test	Status	Time
PRNT	Pass	8:54pm

CRC Tests

Test	Status	Time
COMP	Pass	8:54pm
CAL	Pass	8:54pm

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Mecklenburg Instrument Location BAT Mobile Unit 8
Instrument Serial No. 008615 Matthews PD

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 24 day of April, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature] 2219283
Signature of Certifying Official Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

MECKLENBURG COUNTY BAT MOBILE UNIT 8
590

Serial Number: 008615
Test Date: 04/24/2025

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: Glasscock, Jerry D
Permit Number: 7180-9235
Effective:
02/01/2025-02/01/2027

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG405102
Exp Date: 02/20/2026

Test	g/210L	Time
DIAG	Pass	8:53pm
AIR BLK	.00	8:54pm
ACCY CHK	.07	8:55pm
AIR BLK	.00	8:56pm
SUB TEST	.00	8:57pm
AIR BLK	.00	8:57pm
SUB TEST	.00	8:59pm
AIR BLK	.00	9:00pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

Intox EC/IR-II: Preventive Maintenance

MECKLENBURG COUNTY BAT MOBILE UNIT 8 590

Serial Number: 008615 Test Record Number: 6077
Test Date: 04/24/2025 Test Time: 9:02pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	9:02pm
FLO	Pass	9:02pm
FC	Pass	9:03pm

Temperature Tests

Test	Status	Time
FC1	Pass	9:03pm
SRC	Pass	9:03pm
DET	Pass	9:03pm
BAR	Pass	9:03pm
BT	Pass	9:03pm

Blank Tests

Test	Status	Time
AIR	Pass	9:03pm


Printer Tests

Test	Status	Time
PRNT	Pass	9:03pm

CRC Tests

Test	Status	Time
COMP	Pass	9:03pm
CAL	Pass	9:03pm

Preventive Maintenance
Status: *Pass*


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County Mecklenburg Instrument Location CMPD LEC
Instrument Serial No. 008691 Charlotte, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 28th day of April, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Boye Helms
Signature of Certifying Official

849845
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

MECKLENBURG COUNTY CMPD LEC 590

Serial Number: 008691
Test Date: 04/28/2025

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: Helms, Bryce A
Permit Number: 0084-9845
Effective:
02/01/2025-02/01/2027

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG431001
Exp Date: 11/05/2026

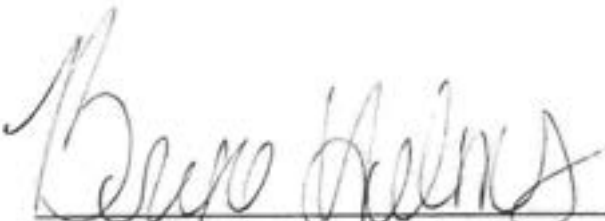
Test	g/210L	Time
DIAG	Pass	12:33pm
AIR BLK	.00	12:34pm
ACCY CHK	.07	12:35pm
AIR BLK	.00	12:36pm
SUB TEST	.00	12:37pm
AIR BLK	.00	12:38pm
SUB TEST	.00	12:39pm
AIR BLK	.00	12:40pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

Intox EC/IR-II: Preventive Maintenance

MECKLENBURG COUNTY CPD LEC 590

Serial Number: 008691 Test Record Number: 9756
Test Date: 04/28/2025 Test Time: 12:40pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	12:41pm
FLO	Pass	12:41pm
FC	Pass	12:41pm

Temperature Tests

Test	Status	Time
FC1	Pass	12:41pm
SRC	Pass	12:41pm
DET	Pass	12:41pm
BAR	Pass	12:41pm
BT	Pass	12:41pm

Blank Tests

Test	Status	Time
AIR	Pass	12:42pm

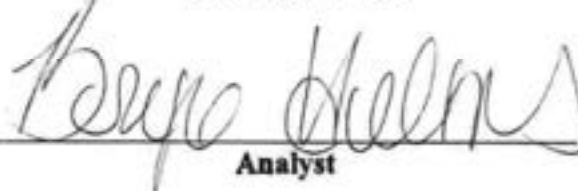
Printer Tests

Test	Status	Time
PRNT	Pass	12:42pm

CRC Tests

Test	Status	Time
COMP	Pass	12:42pm
CAL	Pass	12:42pm

Preventive Maintenance
Status: *Pass*


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County MECKLENBURG Instrument Location CORNELIUS PD

Instrument Serial No. 008692 CORNELIUS NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 02 day of APRIL, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



James S. Fleming
Signature of Certifying Official

274970
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

MECKLENBURG COUNTY CORNELIUS PD 590

Serial Number: 008692
Test Date: 04/02/2025

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Fleming, Tina S

Permit Number: 0027-4970

Effective:

10/01/2023-10/01/2025

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG431001

Exp Date: 11/05/2026

Test	g/210L	Time
DIAG	Pass	10:02am
AIR BLK	.00	10:03am
ACCY CHK	.08	10:03am
AIR BLK	.00	10:05am
SUB TEST	.00	10:05am
AIR BLK	.00	10:06am
SUB TEST	.00	10:08am
AIR BLK	.00	10:09am

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

MECKLENBURG COUNTY CORNELIUS PD 590

Serial Number: 008692 Test Record Number: 3828
Test Date: 04/02/2025 Test Time: 10:09am EDT

System Check: Passed

Baseline Tests

Test	Status	Time
IR	Pass	10:10am
FLO	Pass	10:10am
FC	Pass	10:10am

Temperature Tests

Test	Status	Time
FC1	Pass	10:10am
SRC	Pass	10:10am
DET	Pass	10:10am
BAR	Pass	10:10am
BT	Pass	10:10am

Blank Tests

Test	Status	Time
AIR	Pass	10:10am


Printer Tests

Test	Status	Time
PRNT	Pass	10:10am

CRC Tests

Test	Status	Time
COMP	Pass	10:11am
CAL	Pass	10:11am

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Mecklenburg Instrument Location BAT Mobile Unit 8
Instrument Serial No. 008736 CMPD

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 16 day of April, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

2219283
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

MECKLENBURG COUNTY BAT MOBILE UNIT 8
590

Serial Number: 008736
Test Date: 04/16/2025

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: Glasscock, Jerry D
Permit Number: 7180-9235
Effective:
02/01/2025-02/01/2027

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG405102
Exp Date: 02/20/2026

Test	g/210L	Time
DIAG	Pass	9:24pm
AIR BLK	.00	9:25pm
ACCY CHK	.07	9:25pm
AIR BLK	.00	9:26pm
SUB TEST	.00	9:27pm
AIR BLK	.00	9:28pm
SUB TEST	.00	9:29pm
AIR BLK	.00	9:30pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

MECKLENBURG COUNTY BAT MOBILE UNIT 8 590

Serial Number: 008736 Test Record Number: 1422
Test Date: 04/16/2025 Test Time: 9:31pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	9:32pm
FLO	Pass	9:32pm
FC	Pass	9:32pm

Temperature Tests

Test	Status	Time
FC1	Pass	9:32pm
SRC	Pass	9:32pm
DET	Pass	9:32pm
BAR	Pass	9:32pm
BT	Pass	9:32pm

Blank Tests

Test	Status	Time
AIR	Pass	9:33pm

Printer Tests

Test	Status	Time
PRNT	Pass	9:33pm

CRC Tests

Test	Status	Time
COMP	Pass	9:33pm
CAL	Pass	9:33pm

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County Mecklenburg Instrument Location BAT Mobile Unit 8
Instrument Serial No. 008736 CMPD

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 17 day of April, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

2219283
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

MECKLENBURG COUNTY BAT MOBILE UNIT 8
590

Serial Number: 008736
Test Date: 04/17/2025

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: Glasscock, Jerry D
Permit Number: 7180-9235
Effective:
02/01/2025-02/01/2027

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG405102
Exp Date: 02/20/2026

Test	g/210L	Time
DIAG	Pass	9:22pm
AIR BLK	.00	9:23pm
ACCY CHK	.07	9:24pm
AIR BLK	.00	9:25pm
SUB TEST	.00	9:25pm
AIR BLK	.00	9:26pm
SUB TEST	.00	9:28pm
AIR BLK	.00	9:29pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

Intox EC/IR-II: Preventive Maintenance

MECKLENBURG COUNTY BAT MOBILE UNIT 8 590

Serial Number: 008736 Test Record Number: 1424
Test Date: 04/17/2025 Test Time: 9:30pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	9:31pm
FLO	Pass	9:31pm
FC	Pass	9:31pm

Temperature Tests

Test	Status	Time
FC1	Pass	9:31pm
SRC	Pass	9:31pm
DET	Pass	9:31pm
BAR	Pass	9:31pm
BT	Pass	9:31pm

Blank Tests

Test	Status	Time
AIR	Pass	9:32pm

Printer Tests

Test	Status	Time
PRNT	Pass	9:32pm

CRC Tests

Test	Status	Time
COMP	Pass	9:32pm
CAL	Pass	9:32pm

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Mecklenburg Instrument Location BAT Mobile Unit 8
Instrument Serial No. 008736 Mint Hill PD

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 22 day of April, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

2219283
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

MECKLENBURG COUNTY BAT MOBILE UNIT 8
590

Serial Number: 008736
Test Date: 04/22/2025

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE

Analyst's Name: Glasscock, Jerry D
Permit Number: 7180-9235
Effective:
02/01/2025-02/01/2027

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

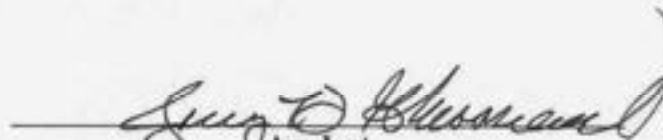
Lot Number: AG405102
Exp Date: 02/20/2026

Test	g/210L	Time
DIAG	Pass	8:46pm
AIR BLK	.00	8:47pm
ACCY CHK	.07	8:47pm
AIR BLK	.00	8:48pm
SUB TEST	.00	8:49pm
AIR BLK	.00	8:50pm
SUB TEST	.00	8:51pm
AIR BLK	.00	8:52pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

Intox EC/IR-II: Preventive Maintenance

MECKLENBURG COUNTY BAT MOBILE UNIT 8 590

Serial Number: 008736 Test Record Number: 1426
Test Date: 04/22/2025 Test Time: 8:53pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	8:53pm
FLO	Pass	8:53pm
FC	Pass	8:53pm

Temperature Tests

Test	Status	Time
FC1	Pass	8:53pm
SRC	Pass	8:53pm
DET	Pass	8:53pm
BAR	Pass	8:53pm
BT	Pass	8:53pm

Blank Tests

Test	Status	Time
AIR	Pass	8:54pm

Printer Tests

Test	Status	Time
PRNT	Pass	8:54pm

CRC Tests

Test	Status	Time
COMP	Pass	8:54pm
CAL	Pass	8:54pm

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Mecklenburg Instrument Location BAT Mobile Unit 8
Instrument Serial No. 008736 Matthews PD

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 24 day of April, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

2219283
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

MECKLENBURG COUNTY BAT MOBILE UNIT 8
590

Serial Number: 008736
Test Date: 04/24/2025

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: Glasscock, Jerry D
Permit Number: 7180-9235
Effective:
02/01/2025-02/01/2027

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test


Lot Number: AG405102
Exp Date: 02/20/2026

Test	g/210L	Time
DIAG	Pass	8:54pm
AIR BLK	.00	8:55pm
ACCY CHK	.07	8:56pm
AIR BLK	.00	8:57pm
SUB TEST	.00	8:57pm
AIR BLK	.00	8:58pm
SUB TEST	.00	9:00pm
AIR BLK	.00	9:00pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

Intox EC/IR-II: Preventive Maintenance

MECKLENBURG COUNTY BAT MOBILE UNIT 8 590

Serial Number: 008736 Test Record Number: 1428
Test Date: 04/24/2025 Test Time: 9:03pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	9:03pm
FLO	Pass	9:03pm
FC	Pass	9:03pm

Temperature Tests

Test	Status	Time
FC1	Pass	9:04pm
SRC	Pass	9:04pm
DET	Pass	9:04pm
BAR	Pass	9:04pm
BT	Pass	9:04pm

Blank Tests

Test	Status	Time
AIR	Pass	9:04pm

Printer Tests

Test	Status	Time
PRNT	Pass	9:04pm

CRC Tests

Test	Status	Time
COMP	Pass	9:04pm
CAL	Pass	9:04pm

Preventive Maintenance
Status: *Pass*


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County MECKLENBURG Instrument Location HUNTERSVILLE PD

Instrument Serial No. 008747 HUNTERSVILLE NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 02 day of APRIL, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Jim S. Steuning
Signature of Certifying Official

274970
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

MECKLENBURG COUNTY HUNTERSVILLE PD 590

Serial Number: 008747
Test Date: 04/02/2025

Citation Number: M0000000-0
Subject's Name:

PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: Fleming, Tina S
Permit Number: 0027-4970
Effective:
10/01/2023-10/01/2025

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG400301
Exp Date: 01/03/2026

Test	g/210L	Time
DIAG	Pass	8:55am
AIR BLK	.00	8:56am
ACCY CHK	.07	8:56am
AIR BLK	.00	8:57am
SUB TEST	.00	8:58am
AIR BLK	.00	8:58am
SUB TEST	.00	9:00am
AIR BLK	.00	9:01am

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

MECKLENBURG COUNTY HUNTERSVILLE PD 590

Serial Number: 008747 Test Record Number: 3371
Test Date: 04/02/2025 Test Time: 9:02am EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	9:02am
FLO	Pass	9:02am
FC	Pass	9:02am

Temperature Tests

Test	Status	Time
FC1	Pass	9:02am
SRC	Pass	9:02am
DET	Pass	9:02am
BAR	Pass	9:02am
BT	Pass	9:02am

Blank Tests

Test	Status	Time
AIR	Pass	9:03am

Printer Tests

Test	Status	Time
PRNT	Pass	9:03am

CRC Tests

Test	Status	Time
COMP	Pass	9:03am
CAL	Pass	9:03am

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Mecklenburg Instrument Location BAT Mobile Unit 8
Instrument Serial No. 008775 CMPO

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 16 day of April, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

2219283
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

MECKLENBURG COUNTY BAT MOBILE UNIT 8
590

Serial Number: 008775
Test Date: 04/16/2025

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE

Analyst's Name: Glasscock, Jerry D
Permit Number: 7180-9235
Effective:
02/01/2025-02/01/2027

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG431002
Exp Date: 11/05/2026

Test	g/210L	Time
DIAG	Pass	9:19pm
AIR BLK	.00	9:20pm
ACCY CHK	.07	9:21pm
AIR BLK	.00	9:22pm
SUB TEST	.00	9:22pm
AIR BLK	.00	9:23pm
SUB TEST	.00	9:25pm
AIR BLK	.00	9:26pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

Intox EC/IR-II: Preventive Maintenance

MECKLENBURG COUNTY BAT MOBILE UNIT 8 590

Serial Number: 008775 Test Record Number: 2274
Test Date: 04/16/2025 Test Time: 9:26pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	9:26pm
FLO	Pass	9:26pm
FC	Pass	9:26pm

Temperature Tests

Test	Status	Time
FC1	Pass	9:27pm
SRC	Pass	9:27pm
DET	Pass	9:27pm
BAR	Pass	9:27pm
BT	Pass	9:27pm

Blank Tests

Test	Status	Time
AIR	Pass	9:27pm


Printer Tests

Test	Status	Time
PRNT	Pass	9:27pm

CRC Tests

Test	Status	Time
COMP	Pass	9:27pm
CAL	Pass	9:27pm

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Mecklenburg Instrument Location BAT Mobile Unit 8
Instrument Serial No. 008775 CMPD

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 17 day of April, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

2219283
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

MECKLENBURG COUNTY BAT MOBILE UNIT 8
590

Serial Number: 008775
Test Date: 04/17/2025

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: Glasscock, Jerry D
Permit Number: 7180-9235
Effective:
02/01/2025-02/01/2027

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test


Lot Number: AG431002
Exp Date: 11/05/2026

Test	g/210L	Time
DIAG	Pass	9:20pm
AIR BLK	.00	9:21pm
ACCY CHK	.07	9:22pm
AIR BLK	.00	9:22pm
SUB TEST	.00	9:23pm
AIR BLK	.00	9:24pm
SUB TEST	.00	9:25pm
AIR BLK	.00	9:26pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

Intox EC/IR-II: Preventive Maintenance

MECKLENBURG COUNTY BAT MOBILE UNIT 8 590

Serial Number: 008775 Test Record Number: 2276
Test Date: 04/17/2025 Test Time: 9:27pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	9:27pm
FLO	Pass	9:27pm
FC	Pass	9:27pm

Temperature Tests

Test	Status	Time
FC1	Pass	9:27pm
SRC	Pass	9:27pm
DET	Pass	9:27pm
BAR	Pass	9:27pm
BT	Pass	9:27pm

Blank Tests

Test	Status	Time
AIR	Pass	9:28pm

Printer Tests

Test	Status	Time
PRNT	Pass	9:28pm

CRC Tests

Test	Status	Time
COMP	Pass	9:28pm
CAL	Pass	9:28pm

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Mecklenburg Instrument Location BAT Mobile Unit 8
Instrument Serial No. 008775 Mint Hill PD

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 22 day of April, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature] 2219283
Signature of Certifying Official Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

MECKLENBURG COUNTY BAT MOBILE UNIT 8
590

Serial Number: 008775
Test Date: 04/22/2025

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE

Analyst's Name: Glasscock, Jerry D
Permit Number: 7180-9235
Effective:
02/01/2025-02/01/2027

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG431002
Exp Date: 11/05/2026

Test	g/210L	Time
DIAG	Pass	8:43pm
AIR BLK	.00	8:44pm
ACCY CHK	.07	8:45pm
AIR BLK	.00	8:46pm
SUB TEST	.00	8:46pm
AIR BLK	.00	8:47pm
SUB TEST	.00	8:49pm
AIR BLK	.00	8:50pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

Intox EC/IR-II: Preventive Maintenance

MECKLENBURG COUNTY BAT MOBILE UNIT 8 590

Serial Number: 008775 Test Record Number: 2278
Test Date: 04/22/2025 Test Time: 8:53pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	8:53pm
FLO	Pass	8:53pm
FC	Pass	8:53pm

Temperature Tests

Test	Status	Time
FC1	Pass	8:53pm
SRC	Pass	8:53pm
DET	Pass	8:53pm
BAR	Pass	8:53pm
BT	Pass	8:53pm

Blank Tests

Test	Status	Time
AIR	Pass	8:54pm

Printer Tests

Test	Status	Time
PRNT	Pass	8:54pm

CRC Tests

Test	Status	Time
COMP	Pass	8:54pm
CAL	Pass	8:54pm

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Mecklenburg Instrument Location BAT Mobile Unit 8
Instrument Serial No. 008775 Matthews PD

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 24 day of April, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

2219283
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

MECKLENBURG COUNTY BAT MOBILE UNIT 8
590

Serial Number: 008775

Test Date: 04/24/2025

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Glasscock, Jerry D

Permit Number: 7180-9235

Effective:

02/01/2025-02/01/2027

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG431002

Exp Date: 11/05/2026

Test	g/210L	Time
DIAG	Pass	8:53pm
AIR BLK	.00	8:54pm
ACCY CHK	.07	8:54pm
AIR BLK	.00	8:55pm
SUB TEST	.00	8:56pm
AIR BLK	.00	8:56pm
SUB TEST	.00	8:58pm
AIR BLK	.00	8:59pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

MECKLENBURG COUNTY BAT MOBILE UNIT 8 590

Serial Number: 008775 Test Record Number: 2280
Test Date: 04/24/2025 Test Time: 9:04pm EDT

System Check: Passed

Baseline Tests

Test	Status	Time
IR	Pass	9:05pm
PLO	Pass	9:05pm
FC	Pass	9:05pm

Temperature Tests

Test	Status	Time
FC1	Pass	9:05pm
SRC	Pass	9:05pm
DET	Pass	9:05pm
BAR	Pass	9:05pm
BT	Pass	9:05pm

Blank Tests

Test	Status	Time
AIR	Pass	9:06pm

Printer Tests

Test	Status	Time
PRNT	Pass	9:06pm

CRC Tests

Test	Status	Time
COMP	Pass	9:06pm
CAL	Pass	9:06pm

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Mecklenburg Instrument Location BAT Mobile Unit 8
Instrument Serial No. 008816 CMPD

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 16 day of April, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature] 2219283
Signature of Certifying Official Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

MECKLENBURG COUNTY BAT MOBILE UNIT 8
590

Serial Number: 008816
Test Date: 04/16/2025

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE

Analyst's Name: Glasscock, Jerry D
Permit Number: 7180-9235
Effective:
02/01/2025-02/01/2027

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test


Lot Number: AG431002
Exp Date: 11/05/2026

Test	g/210L	Time
DIAG	Pass	9:20pm
AIR BLK	.00	9:21pm
ACCY CHK	.08	9:21pm
AIR BLK	.00	9:22pm
SUB TEST	.00	9:23pm
AIR BLK	.00	9:24pm
SUB TEST	.00	9:25pm
AIR BLK	.00	9:26pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

MECKLENBURG COUNTY BAT MOBILE UNIT 8 590

Serial Number: 008816 Test Record Number: 7859
Test Date: 04/16/2025 Test Time: 9:27pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	9:27pm
FLO	Pass	9:27pm
FC	Pass	9:27pm

Temperature Tests

Test	Status	Time
FC1	Pass	9:27pm
SRC	Pass	9:27pm
DET	Pass	9:27pm
BAR	Pass	9:27pm
BT	Pass	9:27pm

Blank Tests

Test	Status	Time
AIR	Pass	9:28pm


Printer Tests

Test	Status	Time
PRNT	Pass	9:28pm

CRC Tests

Test	Status	Time
COMP	Pass	9:28pm
CAL	Pass	9:28pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Mecklenburg Instrument Location BAT Mobile Unit 8
Instrument Serial No. 008816 CMPD

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 17 day of April, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

2219283
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

MECKLENBURG COUNTY BAT MOBILE UNIT 8
590

Serial Number: 008816
Test Date: 04/17/2025

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: Glasscock, Jerry D
Permit Number: 7180-9235
Effective:
02/01/2025-02/01/2027

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG431002
Exp Date: 11/05/2026

Test	g/210L	Time
DIAG	Pass	9:20pm
AIR BLK	.00	9:21pm
ACCY CHK	.08	9:22pm
AIR BLK	.00	9:23pm
SUB TEST	.00	9:24pm
AIR BLK	.00	9:24pm
SUB TEST	.00	9:26pm
AIR BLK	.00	9:27pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

Intox EC/IR-II: Preventive Maintenance

MECKLENBURG COUNTY BAT MOBILE UNIT 8 590

Serial Number: 008816 Test Record Number: 7861
Test Date: 04/17/2025 Test Time: 9:27pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	9:28pm
FLO	Pass	9:28pm
FC	Pass	9:28pm

Temperature Tests

Test	Status	Time
FC1	Pass	9:28pm
SRC	Pass	9:28pm
DET	Pass	9:28pm
BAR	Pass	9:28pm
BT	Pass	9:28pm

Blank Tests

Test	Status	Time
AIR	Pass	9:28pm


Printer Tests

Test	Status	Time
PRNT	Pass	9:29pm

CRC Tests

Test	Status	Time
COMP	Pass	9:29pm
CAL	Pass	9:29pm

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Mecklenburg Instrument Location BAT Mobile Unit 8
Instrument Serial No. 008816 Mint Hill PD

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 22 day of April, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

2219283
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

MECKLENBURG COUNTY BAT MOBILE UNIT 8
590

Serial Number: 008816
Test Date: 04/22/2025

Citation Number: M0000000-0
Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Glasscock, Jerry D

Permit Number: 7180-9235

Effective:

02/01/2025-02/01/2027

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG431002

Exp Date: 11/05/2026

Test	g/210L	Time
DIAG	Pass	8:44pm
AIR BLK	.00	8:45pm
ACCY CHK	.08	8:45pm
AIR BLK	.00	8:46pm
SUB TEST	.00	8:47pm
AIR BLK	.00	8:48pm
SUB TEST	.00	8:49pm
AIR BLK	.00	8:50pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

MECKLENBURG COUNTY BAT MOBILE UNIT 8 590

Serial Number: 008816 Test Record Number: 7863
Test Date: 04/22/2025 Test Time: 8:52pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	8:53pm
FLO	Pass	8:53pm
FC	Pass	8:53pm

Temperature Tests

Test	Status	Time
FC1	Pass	8:53pm
SRC	Pass	8:53pm
DET	Pass	8:53pm
BAR	Pass	8:53pm
BT	Pass	8:53pm

Blank Tests

Test	Status	Time
AIR	Pass	8:54pm

Printer Tests

Test	Status	Time
PRNT	Pass	8:54pm

CRC Tests

Test	Status	Time
COMP	Pass	8:54pm
CAL	Pass	8:54pm

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Mecklenburg Instrument Location BAT Mobile Unit 8
Instrument Serial No. 008816 Matthews PD

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 24 day of April, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature] 2219283
Signature of Certifying Official Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

MECKLENBURG COUNTY BAT MOBILE UNIT 8
590

Serial Number: 008816
Test Date: 04/24/2025

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Glasscock, Jerry D

Permit Number: 7180-9235

Effective:

02/01/2025-02/01/2027

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG431002

Exp Date: 11/05/2026

Test	g/210L	Time
DIAG	Pass	9:07pm
AIR BLK	.00	9:08pm
ACCY CHK	.08	9:09pm
AIR BLK	.00	9:10pm
SUB TEST	.00	9:11pm
AIR BLK	.00	9:12pm
SUB TEST	.00	9:13pm
AIR BLK	.00	9:14pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

Intox EC/IR-II: Preventive Maintenance

MECKLENBURG COUNTY BAT MOBILE UNIT 8 590

Serial Number: 008816 Test Record Number: 7865
Test Date: 04/24/2025 Test Time: 9:54pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	9:55pm
FLO	Pass	9:55pm
FC	Pass	9:55pm

Temperature Tests

Test	Status	Time
FC1	Pass	9:55pm
SRC	Pass	9:55pm
DET	Pass	9:55pm
BAR	Pass	9:55pm
BT	Pass	9:55pm

Blank Tests

Test	Status	Time
AIR	Pass	9:56pm

Printer Tests

Test	Status	Time
PRNT	Pass	9:56pm

CRC Tests

Test	Status	Time
COMP	Pass	9:56pm
CAL	Pass	9:56pm

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Mecklenburg Instrument Location BAT Mobile Unit 8
Instrument Serial No. 008929 CMPD

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 16 day of April, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

2219283
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

MECKLENBURG COUNTY BAT MOBILE UNIT 8
590

Serial Number: 008929
Test Date: 04/16/2025

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: Glasscock, Jerry D
Permit Number: 7180-9235
Effective:
02/01/2025-02/01/2027

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG506303
Exp Date: 03/04/2027

Test	g/210L	Time
DIAG	Pass	9:20pm
AIR BLK	.00	9:21pm
ACCY CHK	.07	9:22pm
AIR BLK	.00	9:23pm
SUB TEST	.00	9:24pm
AIR BLK	.00	9:25pm
SUB TEST	.00	9:26pm
AIR BLK	.00	9:27pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

Intox EC/IR-II: Preventive Maintenance

MECKLENBURG COUNTY BAT MOBILE UNIT 8 590

Serial Number: 008929 Test Record Number: 1560
Test Date: 04/16/2025 Test Time: 9:27pm EDT

System Check: Passed

Baseline Tests

Test	Status	Time
IR	Pass	9:28pm
FLO	Pass	9:28pm
FC	Pass	9:28pm

Temperature Tests

Test	Status	Time
FC1	Pass	9:28pm
SRC	Pass	9:28pm
DET	Pass	9:28pm
BAR	Pass	9:28pm
BT	Pass	9:28pm

Blank Tests

Test	Status	Time
AIR	Pass	9:29pm


Printer Tests

Test	Status	Time
PRNT	Pass	9:29pm

CRC Tests

Test	Status	Time
COMP	Pass	9:29pm
CAL	Pass	9:29pm

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Mecklenburg Instrument Location BAT Mobile Unit 8
Instrument Serial No. 008929 CPMD

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 17 day of April, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

2219283
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

MECKLENBURG COUNTY BAT MOBILE UNIT 8
590

Serial Number: 008929
Test Date: 04/17/2025

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE

Analyst's Name: Glasscock, Jerry D
Permit Number: 7180-9235
Effective:
02/01/2025-02/01/2027

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG506303
Exp Date: 03/04/2027

Test	g/210L	Time
DIAG	Pass	9:21pm
AIR BLK	.00	9:22pm
ACCY CHK	.07	9:23pm
AIR BLK	.00	9:24pm
SUB TEST	.00	9:24pm
AIR BLK	.00	9:25pm
SUB TEST	.00	9:27pm
AIR BLK	.00	9:28pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

Intox EC/IR-II: Preventive Maintenance

MECKLENBURG COUNTY BAT MOBILE UNIT 8 590

Serial Number: 008929 Test Record Number: 1562
Test Date: 04/17/2025 Test Time: 9:29pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	9:30pm
FLO	Pass	9:30pm
FC	Pass	9:30pm

Temperature Tests

Test	Status	Time
FC1	Pass	9:30pm
SRC	Pass	9:30pm
DET	Pass	9:30pm
BAR	Pass	9:30pm
BT	Pass	9:30pm

Blank Tests

Test	Status	Time
AIR	Pass	9:31pm


Printer Tests

Test	Status	Time
PRNT	Pass	9:31pm

CRC Tests

Test	Status	Time
COMP	Pass	9:31pm
CAL	Pass	9:31pm

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County Mecklenburg Instrument Location BAT Mobile Unit 8
Instrument Serial No. 008929 Mint Hill PD

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 22 day of April, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]) 2219283
Signature of Certifying Official Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

MECKLENBURG COUNTY BAT MOBILE UNIT 8
590

Serial Number: 008929
Test Date: 04/22/2025

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Glasscock, Jerry D

Permit Number: 7180-9235

Effective:

02/01/2025-02/01/2027

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG506303

Exp Date: 03/04/2027

Test	g/210L	Time
DIAG	Pass	8:56pm
AIR BLK	.00	8:57pm
ACCY CHK	.07	8:58pm
AIR BLK	.00	8:59pm
SUB TEST	.00	9:00pm
AIR BLK	.00	9:01pm
SUB TEST	.00	9:02pm
AIR BLK	.00	9:03pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

MECKLENBURG COUNTY BAT MOBILE UNIT 8 590

Serial Number: 008929 Test Record Number: 1565
Test Date: 04/22/2025 Test Time: 9:04pm EDT

System Check: Passed

Baseline Tests

Test	Status	Time
IR	Pass	9:04pm
FLO	Pass	9:04pm
FC	Pass	9:04pm

Temperature Tests

Test	Status	Time
FC1	Pass	9:04pm
SRC	Pass	9:04pm
DET	Pass	9:04pm
BAR	Pass	9:04pm
BT	Pass	9:04pm

Blank Tests

Test	Status	Time
AIR	Pass	9:05pm

Printer Tests

Test	Status	Time
PRNT	Pass	9:05pm

CRC Tests

Test	Status	Time
COMP	Pass	9:05pm
CAL	Pass	9:05pm

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Mecklenburg Instrument Location BAT Mobile Unit 8
Instrument Serial No. 008929 Matthews PD

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 24 day of April, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature] 2219283
Signature of Certifying Official Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

MECKLENBURG COUNTY BAT MOBILE UNIT 8
590

Serial Number: 008929
Test Date: 04/24/2025

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: Glasscock, Jerry D
Permit Number: 7180-9235
Effective:
02/01/2025-02/01/2027

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG506303
Exp Date: 03/04/2027

Test	g/210L	Time
DIAG	Pass	8:52pm
AIR BLK	.00	8:53pm
ACCY CHK	.07	8:54pm
AIR BLK	.00	8:55pm
SUB TEST	.00	8:56pm
AIR BLK	.00	8:57pm
SUB TEST	.00	8:58pm
AIR BLK	.00	8:59pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

Intox EC/IR-II: Preventive Maintenance

MECKLENBURG COUNTY BAT MOBILE UNIT 8 590

Serial Number: 008929 Test Record Number: 1567
Test Date: 04/24/2025 Test Time: 9:01pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	9:02pm
FLO	Pass	9:02pm
FC	Pass	9:02pm

Temperature Tests

Test	Status	Time
FC1	Pass	9:02pm
SRC	Pass	9:02pm
DET	Pass	9:02pm
BAR	Pass	9:02pm
BT	Pass	9:02pm

Blank Tests

Test	Status	Time
AIR	Pass	9:03pm

Printer Tests

Test	Status	Time
PRNT	Pass	9:03pm

CRC Tests

Test	Status	Time
COMP	Pass	9:03pm
CAL	Pass	9:03pm

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County MONTGOMERY Instrument Location MONTGOMERY COUNTY
Instrument Serial No. 008657 DETENTION CENTER

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 14 day of APRIL, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Handwritten Signature]
Signature of Certifying Official

239711
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

MONTGOMERY COUNTY DETENTION CENTER 610

Serial Number: 008657

Test Date: 04/14/2025

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Galloway, Charles L

Permit Number: 0023-9771

Effective:

02/01/2025-02/01/2027

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG417803

Exp Date: 06/26/2026

Test	g/210L	Time
DIAG	Pass	2:17pm
AIR BLK	.00	2:18pm
ACCY CHK	.08	2:19pm
AIR BLK	.00	2:20pm
SUB TEST	.00	2:20pm
AIR BLK	.00	2:21pm
SUB TEST	.00	2:23pm
AIR BLK	.00	2:24pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

MONTGOMERY COUNTY DETENTION CENTER 610

Serial Number: 008657 Test Record Number: 2218
Test Date: 04/14/2025 Test Time: 2:25pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	2:25pm
FLO	Pass	2:25pm
FC	Pass	2:26pm

Temperature Tests

Test	Status	Time
FC1	Pass	2:26pm
SRC	Pass	2:26pm
DET	Pass	2:26pm
BAR	Pass	2:26pm
BT	Pass	2:26pm

Blank Tests

Test	Status	Time
AIR	Pass	2:26pm

Printer Tests

Test	Status	Time
PRNT	Pass	2:26pm

CRC Tests

Test	Status	Time
COMP	Pass	2:26pm
CAL	Pass	2:26pm

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County MONTGOMERY Instrument Location MONTGOMERY COUNTY
Instrument Serial No. 008709 DETENTION CENTER

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 14 day of APRIL, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

239771
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

MONTGOMERY COUNTY DETENTION CENTER 610

Serial Number: 008709
Test Date: 04/14/2025

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE

Analyst's Name: Galloway, Charles L
Permit Number: 0023-9771
Effective:
02/01/2025-02/01/2027

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG417803
Exp Date: 06/26/2026

Test	g/210L	Time
DIAG	Pass	2:19pm
AIR BLK	.00	2:20pm
ACCY CHK	.07	2:21pm
AIR BLK	.00	2:22pm
SUB TEST	.00	2:23pm
AIR BLK	.00	2:24pm
SUB TEST	.00	2:26pm
AIR BLK	.00	2:27pm

Reported AC: .00 g/210L


Signature of Chemist/Analyst

Court CVR


Analyst

Intox EC/IR-II: Preventive Maintenance

MONTGOMERY COUNTY DETENTION CENTER 610

Serial Number: 008709 Test Record Number: 1543
Test Date: 04/14/2025 Test Time: 2:28pm EDT

System Check: Passed

Baseline Tests

Test	Status	Time
IR	Pass	2:28pm
FLO	Pass	2:28pm
FC	Pass	2:28pm

Temperature Tests

Test	Status	Time
FC1	Pass	2:28pm
SRC	Pass	2:28pm
DET	Pass	2:28pm
BAR	Pass	2:28pm
BT	Pass	2:28pm

Blank Tests

Test	Status	Time
AIR	Pass	2:29pm

Printer Tests

Test	Status	Time
PRNT	Pass	2:29pm

CRC Tests

Test	Status	Time
COMP	Pass	2:29pm
CAL	Pass	2:29pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Moore Instrument Location BAT Mobile Unit 10
Instrument Serial No. 009584 Vass PD

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 18th day of April, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.





Signature of Certifying Official

2266313

Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

MOORE COUNTY BAT MOBILE UNIT 10 620

Serial Number: 008584
Test Date: 04/18/2025

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Sharpe Jr., Robert J

Permit Number: 1820-8591

Effective:

02/01/2025-02/01/2027

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG400303

Exp Date: 01/03/2026


Test	g/210L	Time
DIAG	Pass	6:09pm
AIR BLK	.00	6:10pm
ACCY CHK	.07	6:11pm
AIR BLK	.00	6:11pm
SUB TEST	.00	6:12pm
AIR BLK	.00	6:13pm
SUB TEST	.00	6:14pm
AIR BLK	.00	6:15pm

Reported AC: ~~00~~ g/210L



Signature of Chemical Analyst

Court CVR



Analyst

Intox EC/IR-II: Preventive Maintenance

MOORE COUNTY BAT MOBILE UNIT 10 620

Serial Number: 008584 Test Record Number: 2786
Test Date: 04/18/2025 Test Time: 6:16pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	6:16pm
FLO	Pass	6:16pm
FC	Pass	6:16pm

Temperature Tests

Test	Status	Time
FC1	Pass	6:16pm
SRC	Pass	6:16pm
DET	Pass	6:16pm
BAR	Pass	6:16pm
BT	Pass	6:16pm

Blank Tests

Test	Status	Time
AIR	Pass	6:17pm

Printer Tests

Test	Status	Time
PRNT	Pass	6:17pm

CRC Tests

Test	Status	Time
COMP	Pass	6:17pm
CAL	Pass	6:17pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Moore Instrument Location BAT Mobile Unit 10
Instrument Serial No. 008637 Vass PD

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 18th day of April, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]

Signature of Certifying Official

2266313

Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

MOORE COUNTY BAT MOBILE UNIT 10 620

Serial Number: 008637
Test Date: 04/18/2025

Citation Number: M0000000-0
Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Sharpe Jr., Robert J

Permit Number: 1820-8591

Effective:

02/01/2025-02/01/2027

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG400303

Exp Date: 01/03/2026

Test	g/210L	Time
DIAG	Pass	6:04pm
AIR BLK	.00	6:05pm
ACCY CHK	.08	6:06pm
AIR BLK	.00	6:07pm
SUB TEST	.00	6:08pm
AIR BLK	.00	6:09pm
SUB TEST	.00	6:10pm
AIR BLK	.00	6:11pm

Reported AC: ~~0.00~~ g/210L



Signature of Chemical Analyst

Court CVR



Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

MOORE COUNTY BAT MOBILE UNIT 10 620

Serial Number: 008637 Test Record Number: 3522
Test Date: 04/18/2025 Test Time: 6:11pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	6:12pm
FLO	Pass	6:12pm
FC	Pass	6:12pm

Temperature Tests

Test	Status	Time
FC1	Pass	6:12pm
SRC	Pass	6:12pm
DET	Pass	6:12pm
BAR	Pass	6:12pm
BT	Pass	6:12pm

Blank Tests

Test	Status	Time
AIR	Pass	6:12pm

Printer Tests

Test	Status	Time
PRNT	Pass	6:13pm

CRC Tests

Test	Status	Time
COMP	Pass	6:13pm
CAL	Pass	6:13pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Moore Instrument Location BAT Mobile Unit 10
Instrument Serial No. 008686 Vass PD

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 18th day of April, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

2266313
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

MOORE COUNTY BAT MOBILE UNIT 10 620

Serial Number: 008686
Test Date: 04/18/2025

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Sharpe Jr., Robert J

Permit Number: 1820-8591

Effective:

02/01/2025-02/01/2027

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG506302

Exp Date: 03/04/2027

Test	g/210L	Time
DIAG	Pass	6:05pm
AIR BLK	.00	6:06pm
ACCY CHK	.08	6:06pm
AIR BLK	.00	6:07pm
SUB TEST	.00	6:09pm
AIR BLK	.00	6:09pm
SUB TEST	.00	6:11pm
AIR BLK	.00	6:12pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

MOORE COUNTY BAT MOBILE UNIT 10 620

Serial Number: 008686 Test Record Number: 7149
Test Date: 04/18/2025 Test Time: 6:16pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	6:16pm
FLO	Pass	6:16pm
FC	Pass	6:16pm

Temperature Tests

Test	Status	Time
FC1	Pass	6:16pm
SRC	Pass	6:16pm
DET	Pass	6:16pm
BAR	Pass	6:16pm
BT	Pass	6:16pm

Blank Tests

Test	Status	Time
AIR	Pass	6:17pm

Printer Tests

Test	Status	Time
PRNT	Pass	6:17pm

CRC Tests

Test	Status	Time
COMP	Pass	6:17pm
CAL	Pass	6:17pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Moore Instrument Location BAT Mobile Unit 10
Instrument Serial No. 008776 Vass PD

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 18th day of April, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

2266313
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

MOORE COUNTY BAT MOBILE UNIT 10 620

Serial Number: 008776
Test Date: 04/18/2025

Citation Number: M0000000-0
Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Sharpe Jr., Robert J

Permit Number: 1820-8591

Effective:

02/01/2025-02/01/2027

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG417803

Exp Date: 06/26/2026


Test	g/210L	Time
DIAG	Pass	6:06pm
AIR BLK	.00	6:07pm
ACCY CHK	.08	6:07pm
AIR BLK	.00	6:08pm
SUB TEST	.00	6:09pm
AIR BLK	.00	6:10pm
SUB TEST	.00	6:11pm
AIR BLK	.00	6:12pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

Intox EC/IR-II: Preventive Maintenance

MOORE COUNTY BAT MOBILE UNIT 10 620

Serial Number: 008776 Test Record Number: 4106
Test Date: 04/18/2025 Test Time: 6:13pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	6:13pm
FLO	Pass	6:13pm
FC	Pass	6:13pm

Temperature Tests

Test	Status	Time
FC1	Pass	6:13pm
SRC	Pass	6:13pm
DET	Pass	6:13pm
BAR	Pass	6:13pm
BT	Pass	6:13pm

Blank Tests

Test	Status	Time
AIR	Pass	6:14pm

Printer Tests

Test	Status	Time
PRNT	Pass	6:14pm

CRC Tests

Test	Status	Time
COMP	Pass	6:14pm
CAL	Pass	6:14pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Moore Instrument Location BAT Mobile Unit 10

Instrument Serial No. 008779 Vass PD

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 18th day of April, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]

Signature of Certifying Official

2266313

Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

MOORE COUNTY BAT MOBILE UNIT 10 620

Serial Number: 008779
Test Date: 04/18/2025

Citation Number: M0000000-0
Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911
Subject's Sex: Male

Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: Sharpe Jr., Robert J
Permit Number: 1820-8591
Effective:
02/01/2025-02/01/2027

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG431002
Exp Date: 11/05/2026

Test	g/210L	Time
DIAG	Pass	6:08pm
AIR BLK	.00	6:09pm
ACCY CHK	.07	6:09pm
AIR BLK	.00	6:10pm
SUB TEST	.00	6:11pm
AIR BLK	.00	6:12pm
SUB TEST	.00	6:13pm
AIR BLK	.00	6:14pm

Reported AC: ~~00~~ g/210L



Signature of Chemical Analyst

Court CVR



Analyst

Intox EC/IR-II: Preventive Maintenance

MOORE COUNTY BAT MOBILE UNIT 10 620

Serial Number: 008779 Test Record Number: 4053
Test Date: 04/18/2025 Test Time: 6:16pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	6:16pm
FLO	Pass	6:16pm
FC	Pass	6:16pm

Temperature Tests

Test	Status	Time
FC1	Pass	6:16pm
SRC	Pass	6:16pm
DET	Pass	6:16pm
BAR	Pass	6:16pm
BT	Pass	6:16pm

Blank Tests

Test	Status	Time
AIR	Pass	6:17pm

Printer Tests

Test	Status	Time
PRNT	Pass	6:17pm

CRC Tests

Test	Status	Time
COMP	Pass	6:17pm
CAL	Pass	6:17pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Nash Instrument Location BAT Mobile Unit 10
Instrument Serial No. 008584 Rocky Mount PD

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 17th day of April, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Handwritten Signature]

Signature of Certifying Official

2266313

Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

NASH COUNTY BAT MOBILE UNIT 10 630

Serial Number: 008584

Test Date: 04/17/2025

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Sharpe Jr., Robert J

Permit Number: 1820-8591

Effective:

02/01/2025-02/01/2027

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG400303

Exp Date: 01/03/2026

Test	g/210L	Time
DIAG	Pass	1:35pm
AIR BLK	.00	1:36pm
ACCY CHK	.07	1:36pm
AIR BLK	.00	1:37pm
SUB TEST	.00	1:38pm
AIR BLK	.00	1:39pm
SUB TEST	.00	1:41pm
AIR BLK	.00	1:42pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

Intox EC/IR-II: Preventive Maintenance

NASH COUNTY BAT MOBILE UNIT 10 630

Serial Number: 008584 Test Record Number: 2784
Test Date: 04/17/2025 Test Time: 1:42pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	1:42pm
FLO	Pass	1:42pm
FC	Pass	1:42pm

Temperature Tests

Test	Status	Time
FC1	Pass	1:43pm
SRC	Pass	1:43pm
DET	Pass	1:43pm
BAR	Pass	1:43pm
BT	Pass	1:43pm

Blank Tests

Test	Status	Time
AIR	Pass	1:43pm


Printer Tests

Test	Status	Time
PRNT	Pass	1:43pm

CRC Tests

Test	Status	Time
COMP	Pass	1:43pm
CAL	Pass	1:43pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Nash Instrument Location BAT Mobile Unit 10
Instrument Serial No. 008637 Rocky Mount PD

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 17th day of April, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

2266313
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

NASH COUNTY BAT MOBILE UNIT 10 630

Serial Number: 008637
Test Date: 04/17/2025

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Sharpe Jr., Robert J

Permit Number: 1820-8591

Effective:

02/01/2025-02/01/2027

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG400303

Exp Date: 01/03/2026

Test	g/210L	Time
DIAG	Pass	1:33pm
AIR BLK	.00	1:34pm
ACCY CHK	.08	1:35pm
AIR BLK	.00	1:36pm
SUB TEST	.00	1:37pm
AIR BLK	.00	1:38pm
SUB TEST	.00	1:39pm
AIR BLK	.00	1:40pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

Intox EC/IR-II: Preventive Maintenance

NASH COUNTY BAT MOBILE UNIT 10 630

Serial Number: 008637 Test Record Number: 3520
Test Date: 04/17/2025 Test Time: 1:40pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	1:41pm
FLO	Pass	1:41pm
FC	Pass	1:41pm

Temperature Tests

Test	Status	Time
FC1	Pass	1:41pm
SRC	Pass	1:41pm
DET	Pass	1:41pm
BAR	Pass	1:41pm
BT	Pass	1:41pm

Blank Tests

Test	Status	Time
AIR	Pass	1:42pm

Printer Tests

Test	Status	Time
PRNT	Pass	1:42pm

CRC Tests

Test	Status	Time
COMP	Pass	1:42pm
CAL	Pass	1:42pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Nash Instrument Location BAT Mobile Unit 10

Instrument Serial No. 008686 Rocky Mount PD

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 17th day of April, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.




Signature of Certifying Official

2266313
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

NASH COUNTY BAT MOBILE UNIT 10 630

Serial Number: 008686

Test Date: 04/17/2025

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Sharpe Jr., Robert J

Permit Number: 1820-8591

Effective:

02/01/2025-02/01/2027

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG506302

Exp Date: 03/04/2027


Test	g/210L	Time
DIAG	Pass	1:33pm
AIR BLK	.00	1:34pm
ACCY CHK	.08	1:35pm
AIR BLK	.00	1:36pm
SUB TEST	.00	1:38pm
AIR BLK	.00	1:38pm
SUB TEST	.00	1:40pm
AIR BLK	.00	1:41pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

Intox EC/IR-II: Preventive Maintenance

NASH COUNTY BAT MOBILE UNIT 10 630

Serial Number: 008686 Test Record Number: 7146
Test Date: 04/17/2025 Test Time: 1:41pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	1:41pm
FLO	Pass	1:41pm
FC	Pass	1:42pm

Temperature Tests

Test	Status	Time
FC1	Pass	1:42pm
SRC	Pass	1:42pm
DET	Pass	1:42pm
BAR	Pass	1:42pm
BT	Pass	1:42pm

Blank Tests

Test	Status	Time
AIR	Pass	1:42pm


Printer Tests

Test	Status	Time
PRNT	Pass	1:42pm

CRC Tests

Test	Status	Time
COMP	Pass	1:42pm
CAL	Pass	1:42pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Nash Instrument Location BAT Mobile Unit 10

Instrument Serial No. 008776 Rocky Mount PD

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 17th day of April, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

2266313
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

NASH COUNTY BAT MOBILE UNIT 10 630

Serial Number: 008776

Test Date: 04/17/2025

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Sharpe Jr., Robert J

Permit Number: 1820-8591

Effective:

02/01/2025-02/01/2027

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG417803

Exp Date: 06/26/2026

Test	g/210L	Time
DIAG	Pass	1:35pm
AIR BLK	.00	1:36pm
ACCY CHK	.08	1:37pm
AIR BLK	.00	1:38pm
SUB TEST	.00	1:38pm
AIR BLK	.00	1:39pm
SUB TEST	.00	1:40pm
AIR BLK	.00	1:41pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

Intox EC/IR-II: Preventive Maintenance

NASH COUNTY BAT MOBILE UNIT 10 630

Serial Number: 008776 Test Record Number: 4104
Test Date: 04/17/2025 Test Time: 1:42pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	1:42pm
FLO	Pass	1:42pm
FC	Pass	1:42pm

Temperature Tests

Test	Status	Time
FC1	Pass	1:42pm
SRC	Pass	1:42pm
DET	Pass	1:42pm
BAR	Pass	1:42pm
BT	Pass	1:42pm

Blank Tests

Test	Status	Time
AIR	Pass	1:43pm

Printer Tests

Test	Status	Time
PRNT	Pass	1:43pm

CRC Tests

Test	Status	Time
COMP	Pass	1:43pm
CAL	Pass	1:43pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Nash Instrument Location BAT Mobile Unit 10
Instrument Serial No. 008779 Rocky Mount PD

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 17th day of Apr. 1, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

2266313
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

NASH COUNTY BAT MOBILE UNIT 10 630

Serial Number: 008779
Test Date: 04/17/2025

Citation Number: M0000000-0
Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Sharpe Jr., Robert J

Permit Number: 1820-8591

Effective:

02/01/2025-02/01/2027

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG431002

Exp Date: 11/05/2026


Test	g/210L	Time
DIAG	Pass	1:38pm
AIR BLK	.00	1:39pm
ACCY CHK	.07	1:40pm
AIR BLK	.00	1:41pm
SUB TEST	.00	1:41pm
AIR BLK	.00	1:42pm
SUB TEST	.00	1:44pm
AIR BLK	.00	1:44pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

NASH COUNTY BAT MOBILE UNIT 10 630

Serial Number: 008779 Test Record Number: 4051
Test Date: 04/17/2025 Test Time: 1:45pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	1:45pm
FLO	Pass	1:45pm
FC	Pass	1:45pm

Temperature Tests

Test	Status	Time
FC1	Pass	1:45pm
SRC	Pass	1:45pm
DET	Pass	1:45pm
BAR	Pass	1:45pm
BT	Pass	1:45pm

Blank Tests

Test	Status	Time
AIR	Pass	1:46pm

Printer Tests

Test	Status	Time
PRNT	Pass	1:46pm

CRC Tests

Test	Status	Time
COMP	Pass	1:46pm
CAL	Pass	1:46pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Nash Instrument Location BAT Mobile Unit 13

Instrument Serial No. 008869 Nashville P.D.

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 26 day of April, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Timothy B. White
Signature of Certifying Official

307699
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

NASH COUNTY BAT MOBILE UNIT 13 630

Serial Number: 008869
Test Date: 04/26/2025

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE

Analyst's Name: Whitehurst, Timothy B
Permit Number: 0030-7699
Effective:
03/01/2025-03/01/2027

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG417803
Exp Date: 06/26/2026

Test	g/210L	Time
DIAG	Pass	9:08pm
AIR BLK	.00	9:09pm
ACCY CHK	.07	9:10pm
AIR BLK	.00	9:11pm
SUB TEST	.00	9:11pm
AIR BLK	.00	9:12pm
SUB TEST	.00	9:14pm
AIR BLK	.00	9:15pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

Intox EC/IR-II: Preventive Maintenance

NASH COUNTY BAT MOBILE UNIT 13 630

Serial Number: 008869 Test Record Number: 2011
Test Date: 04/26/2025 Test Time: 9:16pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	9:16pm
FLO	Pass	9:16pm
FC	Pass	9:17pm

Temperature Tests

Test	Status	Time
FC1	Pass	9:17pm
SRC	Pass	9:17pm
DET	Pass	9:17pm
BAR	Pass	9:17pm
BT	Pass	9:17pm

Blank Tests

Test	Status	Time
AIR	Pass	9:17pm

Printer Tests

Test	Status	Time
PRNT	Pass	9:17pm

CRC Tests

Test	Status	Time
COMP	Pass	9:18pm
CAL	Pass	9:18pm

Preventive Maintenance
Status: *Pass*



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Nash Instrument Location BAT Mobile Unit 13

Instrument Serial No. 008898 Nashville P.D.

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 26 day of April, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Tom B. White
Signature of Certifying Official

307699
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

NASH COUNTY BAT MOBILE UNIT 13 630

Serial Number: 008898
Test Date: 04/26/2025

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: Whitehurst, Timothy B
Permit Number: 0030-7699
Effective:
03/01/2025-03/01/2027

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG506302
Exp Date: 03/04/2027

Test	g/210L	Time
DIAG	Pass	9:18pm
AIR BLK	.00	9:19pm
ACCY CHK	.07	9:19pm
AIR BLK	.00	9:20pm
SUB TEST	.00	9:21pm
AIR BLK	.00	9:22pm
SUB TEST	.00	9:23pm
AIR BLK	.00	9:24pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

Intox EC/IR-II: Preventive Maintenance

NASH COUNTY BAT MOBILE UNIT 13 630

Serial Number: 008898 Test Record Number: 1985
Test Date: 04/26/2025 Test Time: 9:26pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	9:27pm
FLO	Pass	9:27pm
FC	Pass	9:27pm

Temperature Tests

Test	Status	Time
FC1	Pass	9:27pm
SRC	Pass	9:27pm
DET	Pass	9:27pm
BAR	Pass	9:27pm
BT	Pass	9:27pm

Blank Tests

Test	Status	Time
AIR	Pass	9:27pm

Printer Tests

Test	Status	Time
PRNT	Pass	9:27pm

CRC Tests

Test	Status	Time
COMP	Pass	9:28pm
CAL	Pass	9:28pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Nash Instrument Location BAT Mobile Unit 13

Instrument Serial No. 008939 Nashville PD

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 26 day of April, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Timothy B. White
Signature of Certifying Official

307699
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

NASH COUNTY BAT MOBILE UNIT 13 630

Serial Number: 008939
Test Date: 04/26/2025

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Whitehurst, Timothy B

Permit Number: 0030-7699

Effective:

03/01/2025-03/01/2027

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG506302

Exp Date: 03/04/2027

Test	g/210L	Time
DIAG	Pass	8:59pm
AIR BLK	.00	9:00pm
ACCY CHK	.08	9:00pm
AIR BLK	.00	9:01pm
SUB TEST	.00	9:02pm
AIR BLK	.00	9:03pm
SUB TEST	.00	9:04pm
AIR BLK	.00	9:05pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

Intox EC/IR-II: Preventive Maintenance

NASH COUNTY BAT MOBILE UNIT 13 630

Serial Number: 008939 Test Record Number: 1851
Test Date: 04/26/2025 Test Time: 9:10pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	9:11pm
FLO	Pass	9:11pm
FC	Pass	9:11pm

Temperature Tests

Test	Status	Time
FC1	Pass	9:11pm
SRC	Pass	9:11pm
DET	Pass	9:11pm
BAR	Pass	9:11pm
BT	Pass	9:11pm

Blank Tests

Test	Status	Time
AIR	Pass	9:12pm

Printer Tests

Test	Status	Time
PRNT	Pass	9:12pm

CRC Tests

Test	Status	Time
COMP	Pass	9:12pm
CAL	Pass	9:12pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Orange Instrument Location Chapel Hill PD
Instrument Serial No. 008856 828 Martin Luther King Jr Blvd
Chapel Hill, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 3 day of April, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Simon Stokes Barnes

Signature of Certifying Official

146221

Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

ORANGE COUNTY CHAPEL HILL PD 670

Serial Number: 008856
Test Date: 04/03/2025

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE

Analyst's Name: Barnes, Simon S
Permit Number: 0014-6221
Effective:
02/01/2025-02/01/2027

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG431003
Exp Date: 11/05/2026

Test	g/210L	Time
DIAG	Pass	11:19am
AIR BLK	.00	11:20am
ACCY CHK	.08	11:20am
AIR BLK	.00	11:22am
SUB TEST	.00	11:22am
AIR BLK	.00	11:23am
SUB TEST	.00	11:25am
AIR BLK	.00	11:25am

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

Intox EC/IR-II: Preventive Maintenance

ORANGE COUNTY CHAPEL HILL PD 670

Serial Number: 008856 Test Record Number: 3266
Test Date: 04/03/2025 Test Time: 11:26am EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	11:26am
FLO	Pass	11:26am
FC	Pass	11:26am

Temperature Tests

Test	Status	Time
FC1	Pass	11:26am
SRC	Pass	11:26am
DET	Pass	11:26am
BAR	Pass	11:26am
BT	Pass	11:26am

Blank Tests

Test	Status	Time
AIR	Pass	11:27am

Printer Tests

Test	Status	Time
PRNT	Pass	11:27am

CRC Tests

Test	Status	Time
COMP	Pass	11:27am
CAL	Pass	11:27am

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County ORANGE Instrument Location Orange Co Detention Ctr
Instrument Serial No. 008873 1200 US Hwy 70 West
Hillsborough, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 2 day of April, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Erin Stokes Brown

Signature of Certifying Official

146221

Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

ORANGE COUNTY DETENTION CENTER 670

Serial Number: 008873

Test Date: 04/02/2025

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Barnes, Simon S

Permit Number: 0014-6221

Effective:

02/01/2025-02/01/2027

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG400302

Exp Date: 01/03/2026

Test	g/210L	Time
DIAG	Pass	1:45pm
AIR BLK	.00	1:46pm
ACCY CHK	.07	1:46pm
AIR BLK	.00	1:47pm
SUB TEST	.00	1:48pm
AIR BLK	.00	1:49pm
SUB TEST	.00	1:50pm
AIR BLK	.00	1:51pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

Intox EC/IR-II: Preventive Maintenance

ORANGE COUNTY DETENTION CENTER 670

Serial Number: 008873 Test Record Number: 2276
Test Date: 04/02/2025 Test Time: 1:51pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	1:52pm
FLO	Pass	1:52pm
FC	Pass	1:52pm

Temperature Tests

Test	Status	Time
FC1	Pass	1:52pm
SRC	Pass	1:52pm
DET	Pass	1:52pm
BAR	Pass	1:52pm
BT	Pass	1:52pm

Blank Tests

Test	Status	Time
AIR	Pass	1:53pm

Printer Tests

Test	Status	Time
PRNT	Pass	1:53pm

CRC Tests

Test	Status	Time
COMP	Pass	1:53pm
CAL	Pass	1:53pm

Preventive Maintenance
Status: *Pass*



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Perquimans Instrument Location Perquimans C.S.O.
Instrument Serial No. 008971 110 N. Church St. Hertford, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 21st day of April, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

206272
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

PERQUIMANS COUNTY PERQUIMANS CO SO 710

Serial Number: 008921
Test Date: 04/21/2025

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE

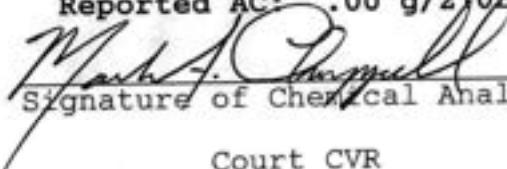
Analyst's Name: Chappell, Mark A
Permit Number: 0020-6272
Effective:
02/01/2025-02/01/2027

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG431001
Exp Date: 11/05/2026

Test	g/210L	Time
DIAG	Pass	12:52pm
AIR BLK	.00	12:52pm
ACCY CHK	.07	12:53pm
AIR BLK	.00	12:54pm
SUB TEST	.00	12:55pm
AIR BLK	.00	12:56pm
SUB TEST	.00	12:58pm
AIR BLK	.00	12:58pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

PERQUIMANS COUNTY PERQUIMANS CO SO 710

Serial Number: 008921 Test Record Number: 1359
Test Date: 04/21/2025 Test Time: 12:59pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	1:00pm
FLO	Pass	1:00pm
FC	Pass	1:00pm

Temperature Tests

Test	Status	Time
FC1	Pass	1:00pm
SRC	Pass	1:00pm
DET	Pass	1:00pm
BAR	Pass	1:00pm
BT	Pass	1:00pm

Blank Tests

Test	Status	Time
AIR	Pass	1:01pm

Printer Tests

Test	Status	Time
PRNT	Pass	1:01pm

CRC Tests

Test	Status	Time
COMP	Pass	1:01pm
CAL	Pass	1:01pm

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Pitt Instrument Location Pitt Co Detention Center
Instrument Serial No. 008646 124 New Hope Rd, Greenville,
NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 23rd day of April, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

377722
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

PITT COUNTY PITT CO DETENTION 730

Serial Number: 008646
Test Date: 04/23/2025

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: Gray, Kelly D
Permit Number: 0037-7722
Effective:
02/01/2025-02/01/2027

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG431003
Exp Date: 11/05/2026

Test	g/210L	Time
DIAG	Pass	3:20pm
AIR BLK	.00	3:20pm
ACCY CHK	.08	3:21pm
AIR BLK	.00	3:22pm
SUB TEST	.00	3:23pm
AIR BLK	.00	3:24pm
SUB TEST	.00	3:26pm
AIR BLK	.00	3:27pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

PITT COUNTY PITT CO DETENTION 730

Serial Number: 008646 Test Record Number: 5132
Test Date: 04/23/2025 Test Time: 3:28pm EDT

System Check: Passed

Baseline Tests

Test	Status	Time
IR	Pass	3:28pm
FLO	Pass	3:28pm
FC	Pass	3:28pm

Temperature Tests

Test	Status	Time
FC1	Pass	3:28pm
SRC	Pass	3:28pm
DET	Pass	3:28pm
BAR	Pass	3:28pm
BT	Pass	3:28pm

Blank Tests

Test	Status	Time
AIR	Pass	3:29pm


Printer Tests

Test	Status	Time
PRNT	Pass	3:29pm

CRC Tests

Test	Status	Time
COMP	Pass	3:29pm
CAL	Pass	3:29pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Polk Instrument Location Polk County Jail

Instrument Serial No. 009832 Columbus, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 4 day of April, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

244987
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

POLK COUNTY POLK COUNTY JAIL 740

Serial Number: 008832
Test Date: 04/04/2025

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE

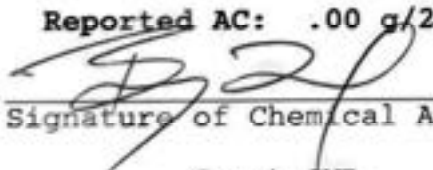
Analyst's Name: Loftis, Benjamin C
Permit Number: 0024-4987
Effective:
03/01/2025-03/01/2027

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG431001
Exp Date: 11/05/2026

Test	g/210L	Time
DIAG	Pass	11:19am
AIR BLK	.00	11:19am
ACCY CHK	.07	11:20am
AIR BLK	.00	11:21am
SUB TEST	.00	11:21am
AIR BLK	.00	11:22am
SUB TEST	.00	11:24am
AIR BLK	.00	11:25am

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

POLK COUNTY POLK COUNTY JAIL 740

Serial Number: 008832 Test Record Number: 1924
Test Date: 04/04/2025 Test Time: 11:25am EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	11:26am
FLO	Pass	11:26am
FC	Pass	11:26am

Temperature Tests

Test	Status	Time
FC1	Pass	11:26am
SRC	Pass	11:26am
DET	Pass	11:26am
BAR	Pass	11:26am
BT	Pass	11:26am

Blank Tests

Test	Status	Time
AIR	Pass	11:26am

Printer Tests

Test	Status	Time
PRNT	Pass	11:26am

CRC Tests

Test	Status	Time
COMP	Pass	11:27am
CAL	Pass	11:27am

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County Polk Instrument Location Polk County Jail
Instrument Serial No. 009981 Columbus, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 4 day of April, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

244987
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

POLK COUNTY POLK COUNTY JAIL 740

Serial Number: 008881

Test Date: 04/04/2025

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Loftis, Benjamin C

Permit Number: 0024-4987

Effective:

03/01/2025-03/01/2027

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

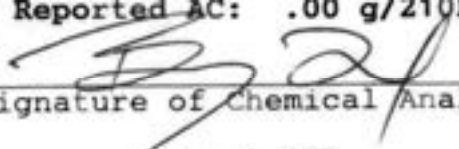
Test Type: Breath Test

Lot Number: AG506301

Exp Date: 03/04/2027

Test	g/210L	Time
DIAG	Pass	11:24am
AIR BLK	.00	11:25am
ACCY CHK	.08	11:25am
AIR BLK	.00	11:26am
SUB TEST	.00	11:27am
AIR BLK	.00	11:28am
SUB TEST	.00	11:29am
AIR BLK	.00	11:30am

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

POLK COUNTY POLK COUNTY JAIL 740

Serial Number: 008881 Test Record Number: 1268
Test Date: 04/04/2025 Test Time: 11:30am EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	11:31am
FLO	Pass	11:31am
FC	Pass	11:31am

Temperature Tests

Test	Status	Time
FC1	Pass	11:31am
SRC	Pass	11:31am
DET	Pass	11:31am
BAR	Pass	11:31am
BT	Pass	11:31am

Blank Tests

Test	Status	Time
AIR	Pass	11:31am

Printer Tests

Test	Status	Time
PRNT	Pass	11:31am

CRC Tests

Test	Status	Time
COMP	Pass	11:32am
CAL	Pass	11:32am

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Robeson Instrument Location BAT Mobile Unit 10
Instrument Serial No. 008584 Robeson County SO

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 2nd day of April, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]

Signature of Certifying Official

2266313

Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

ROBESON COUNTY BAT MOBILE UNIT 10 770

Serial Number: 008584
Test Date: 04/02/2025

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Sharpe Jr., Robert J

Permit Number: 1820-8591

Effective:

02/01/2025-02/01/2027

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG400303

Exp Date: 01/03/2026

Test	g/210L	Time
DIAG	Pass	3:26pm
AIR BLK	.00	3:27pm
ACCY CHK	.07	3:27pm
AIR BLK	.00	3:28pm
SUB TEST	.00	3:29pm
AIR BLK	.00	3:30pm
SUB TEST	.00	3:31pm
AIR BLK	.00	3:32pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

Intox EC/IR-II: Preventive Maintenance

ROBESON COUNTY BAT MOBILE UNIT 10 770

Serial Number: 008584 Test Record Number: 2772
Test Date: 04/02/2025 Test Time: 3:33pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	3:33pm
FLO	Pass	3:33pm
FC	Pass	3:33pm

Temperature Tests

Test	Status	Time
FC1	Pass	3:33pm
SRC	Pass	3:33pm
DET	Pass	3:33pm
BAR	Pass	3:33pm
BT	Pass	3:33pm

Blank Tests

Test	Status	Time
AIR	Pass	3:34pm

Printer Tests

Test	Status	Time
PRNT	Pass	3:34pm

CRC Tests

Test	Status	Time
COMP	Pass	3:34pm
CAL	Pass	3:34pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Robeson Instrument Location BAT Mobile Unit 10
Instrument Serial No. 008584 Lumberton PD

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 10th day of April, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

2266313
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

ROBESON COUNTY BAT MOBILE UNIT 10 770

Serial Number: 008584
Test Date: 04/10/2025

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Sharpe Jr., Robert J

Permit Number: 1820-8591

Effective:

02/01/2025-02/01/2027

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG400303

Exp Date: 01/03/2026

Test	g/210L	Time
DIAG	Pass	1:25pm
AIR BLK	.00	1:26pm
ACCY CHK	.07	1:26pm
AIR BLK	.00	1:27pm
SUB TEST	.00	1:28pm
AIR BLK	.00	1:29pm
SUB TEST	.00	1:31pm
AIR BLK	.00	1:32pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

ROBESON COUNTY BAT MOBILE UNIT 10 770

Serial Number: 008584 Test Record Number: 2774
Test Date: 04/10/2025 Test Time: 1:32pm EDT

System Check: Passed

Baseline Tests

Test	Status	Time
IR	Pass	1:33pm
FLO	Pass	1:33pm
FC	Pass	1:33pm

Temperature Tests

Test	Status	Time
FC1	Pass	1:33pm
SRC	Pass	1:33pm
DET	Pass	1:33pm
BAR	Pass	1:33pm
BT	Pass	1:33pm

Blank Tests

Test	Status	Time
AIR	Pass	1:34pm


Printer Tests

Test	Status	Time
PRNT	Pass	1:34pm

CRC Tests

Test	Status	Time
COMP	Pass	1:34pm
CAL	Pass	1:34pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Robeson Instrument Location BAT Mobile Unit 10
Instrument Serial No. 008584 Red Springs PD

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 15th day of April, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

2266313
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

ROBESON COUNTY BAT MOBILE UNIT 10 770

Serial Number: 008584
Test Date: 04/15/2025

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Sharpe Jr., Robert J

Permit Number: 1820-8591

Effective:

02/01/2025-02/01/2027

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG400303

Exp Date: 01/03/2026


Test	g/210L	Time
DIAG	Pass	2:14pm
AIR BLK	.00	2:15pm
ACCY CHK	.07	2:15pm
AIR BLK	.00	2:16pm
SUB TEST	.00	2:17pm
AIR BLK	.00	2:18pm
SUB TEST	.00	2:19pm
AIR BLK	.00	2:20pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

Intox EC/IR-II: Preventive Maintenance

ROBESON COUNTY BAT MOBILE UNIT 10 770

Serial Number: 008584 Test Record Number: 2782
Test Date: 04/15/2025 Test Time: 2:20pm EDT

System Check: Passed

Baseline Tests

Test	Status	Time
IR	Pass	2:21pm
FLO	Pass	2:21pm
FC	Pass	2:21pm

Temperature Tests

Test	Status	Time
FC1	Pass	2:21pm
SRC	Pass	2:21pm
DET	Pass	2:21pm
BAR	Pass	2:21pm
BT	Pass	2:21pm

Blank Tests

Test	Status	Time
AIR	Pass	2:22pm

Printer Tests

Test	Status	Time
PRNT	Pass	2:22pm

CRC Tests

Test	Status	Time
COMP	Pass	2:22pm
CAL	Pass	2:22pm

**Preventive Maintenance
Status: Pass**



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Robeson Instrument Location BAT Mobile Unit 10
Instrument Serial No. 008584 Robeson County SO

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 25th day of April, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

2266313
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

ROBESON COUNTY BAT MOBILE UNIT 10 770

Serial Number: 008584
Test Date: 04/25/2025

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Sharpe Jr., Robert J

Permit Number: 1820-8591

Effective:

02/01/2025-02/01/2027

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG400303

Exp Date: 01/03/2026

Test	g/210L	Time
DIAG	Pass	6:23pm
AIR BLK	.00	6:24pm
ACCY CHK	.07	6:25pm
AIR BLK	.00	6:26pm
SUB TEST	.00	6:26pm
AIR BLK	.00	6:27pm
SUB TEST	.00	6:29pm
AIR BLK	.00	6:30pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

ROBESON COUNTY BAT MOBILE UNIT 10 770

Serial Number: 008584 Test Record Number: 2790
Test Date: 04/25/2025 Test Time: 6:30pm EDT

System Check: Passed

Baseline Tests

Test	Status	Time
IR	Pass	6:31pm
FLO	Pass	6:31pm
FC	Pass	6:31pm

Temperature Tests

Test	Status	Time
FC1	Pass	6:31pm
SRC	Pass	6:31pm
DET	Pass	6:31pm
BAR	Pass	6:31pm
BT	Pass	6:31pm

Blank Tests

Test	Status	Time
AIR	Pass	6:31pm


Printer Tests

Test	Status	Time
PRNT	Pass	6:31pm

CRC Tests

Test	Status	Time
COMP	Pass	6:32pm
CAL	Pass	6:32pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Robeson Instrument Location BAT Mobile Unit 10
Instrument Serial No. 008637 Robeson County SO

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 20th day of April, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

2266313
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

ROBESON COUNTY BAT MOBILE UNIT 10 770

Serial Number: 008637

Test Date: 04/02/2025

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Sharpe Jr., Robert J

Permit Number: 1820-8591

Effective:

02/01/2025-02/01/2027

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG400303

Exp Date: 01/03/2026

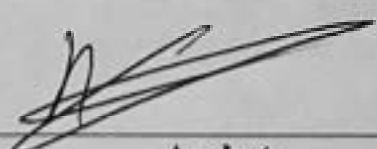
Test	g/210L	Time
DIAG	Pass	3:27pm
AIR BLK	.00	3:28pm
ACCY CHK	.08	3:28pm
AIR BLK	.00	3:29pm
SUB TEST	.00	3:30pm
AIR BLK	.00	3:31pm
SUB TEST	.00	3:33pm
AIR BLK	.00	3:33pm

Reported AC: 00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

This form is used when performing Preventive Maintenance procedures

Forensic Tests for Alcohol Branch

Department of Health and Human Services

Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

ROBESON COUNTY BAT MOBILE UNIT 10 770

Serial Number: 008637 Test Record Number: 3506
Test Date: 04/02/2025 Test Time: 3:35pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	3:35pm
FLO	Pass	3:35pm
FC	Pass	3:35pm

Temperature Tests

Test	Status	Time
FC1	Pass	3:35pm
SRC	Pass	3:35pm
DET	Pass	3:35pm
BAR	Pass	3:35pm
BT	Pass	3:35pm

Blank Tests

Test	Status	Time
AIR	Pass	3:36pm

Printer Tests

Test	Status	Time
PRNT	Pass	3:36pm

CRC Tests

Test	Status	Time
COMP	Pass	3:36pm
CAL	Pass	3:36pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Robeson Instrument Location BAT Mobile Unit 10
Instrument Serial No. 008637 Lumberton PD

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 10th day of April, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

2266313
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

ROBESON COUNTY BAT MOBILE UNIT 10 770

Serial Number: 008637

Test Date: 04/10/2025

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Sharpe Jr., Robert J

Permit Number: 1820-8591

Effective:

02/01/2025-02/01/2027

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG400303

Exp Date: 01/03/2026

Test	g/210L	Time
DIAG	Pass	1:27pm
AIR BLK	.00	1:28pm
ACCY CHK	.08	1:28pm
AIR BLK	.00	1:29pm
SUB TEST	.00	1:30pm
AIR BLK	.00	1:31pm
SUB TEST	.00	1:33pm
AIR BLK	.00	1:34pm

Reported AC: ~~.00~~ g/210L

Signature  Chemical Analyst

Court CVR


Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

ROBESON COUNTY BAT MOBILE UNIT 10 770

Serial Number: 008637 Test Record Number: 3508
Test Date: 04/10/2025 Test Time: 1:35pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	1:35pm
FLO	Pass	1:35pm
FC	Pass	1:35pm

Temperature Tests

Test	Status	Time
FC1	Pass	1:35pm
SRC	Pass	1:35pm
DET	Pass	1:35pm
BAR	Pass	1:35pm
BT	Pass	1:35pm

Blank Tests

Test	Status	Time
AIR	Pass	1:36pm

Printer Tests

Test	Status	Time
PRNT	Pass	1:36pm

CRC Tests

Test	Status	Time
COMP	Pass	1:36pm
CAL	Pass	1:36pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Robeson Instrument Location BAT Mobile Unit 10

Instrument Serial No. 008637 Red Springs PD

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 15th day of April, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Handwritten Signature]

Signature of Certifying Official

2266313

Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

ROBESON COUNTY BAT MOBILE UNIT 10 770

Serial Number: 008637

Test Date: 04/15/2025

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Sharpe Jr., Robert J

Permit Number: 1820-8591

Effective:

02/01/2025-02/01/2027

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG400303

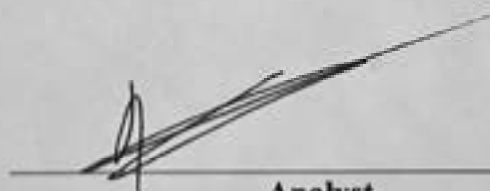
Exp Date: 01/03/2026

Test	g/210L	Time
DIAG	Pass	2:13pm
AIR BLK	.00	2:14pm
ACCY CHK	.08	2:14pm
AIR BLK	.00	2:15pm
SUB TEST	.00	2:16pm
AIR BLK	.00	2:17pm
SUB TEST	.00	2:19pm
AIR BLK	.00	2:20pm

Reported AC: ~~0.00~~ g/210L


Signature of Chemical Analyst

Court CVR


Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

ROBESON COUNTY BAT MOBILE UNIT 10 770

Serial Number: 008637 Test Record Number: 3516
Test Date: 04/15/2025 Test Time: 2:20pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	2:20pm
FLO	Pass	2:20pm
FC	Pass	2:20pm

Temperature Tests

Test	Status	Time
FC1	Pass	2:21pm
SRC	Pass	2:21pm
DET	Pass	2:21pm
BAR	Pass	2:21pm
BT	Pass	2:21pm

Blank Tests

Test	Status	Time
AIR	Pass	2:21pm

Printer Tests

Test	Status	Time
PRNT	Pass	2:21pm

CRC Tests

Test	Status	Time
COMP	Pass	2:21pm
CAL	Pass	2:21pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Robeson Instrument Location BAT Mobile Unit 10
Instrument Serial No. 008637 Robeson County SO

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 25th day of April, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

2266313
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

ROBESON COUNTY BAT MOBILE UNIT 10 770

Serial Number: 008637

Test Date: 04/25/2025

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Sharpe Jr., Robert J

Permit Number: 1820-8591

Effective:

02/01/2025-02/01/2027

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG400303

Exp Date: 01/03/2026

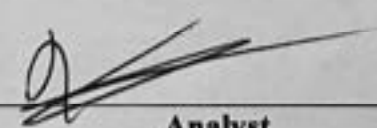
Test	g/210L	Time
DIAG	Pass	6:25pm
AIR BLK	.00	6:26pm
ACCY CHK	.08	6:27pm
AIR BLK	.00	6:28pm
SUB TEST	.00	6:29pm
AIR BLK	.00	6:30pm
SUB TEST	.00	6:32pm
AIR BLK	.00	6:32pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

ROBESON COUNTY BAT MOBILE UNIT 10 770

Serial Number: 008637 Test Record Number: 3526
Test Date: 04/25/2025 Test Time: 6:33pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	6:33pm
FLO	Pass	6:33pm
FC	Pass	6:33pm

Temperature Tests

Test	Status	Time
FC1	Pass	6:34pm
SRC	Pass	6:34pm
DET	Pass	6:34pm
BAR	Pass	6:34pm
BT	Pass	6:34pm

Blank Tests

Test	Status	Time
AIR	Pass	6:34pm

Printer Tests

Test	Status	Time
PRNT	Pass	6:34pm

CRC Tests

Test	Status	Time
COMP	Pass	6:34pm
CAL	Pass	6:34pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County Robeson Instrument Location BAT Mobile Unit 10
Instrument Serial No. 008686 Robeson County SC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 2nd day of April, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

2266313
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

ROBESON COUNTY BAT MOBILE UNIT 10 770

Serial Number: 008686
Test Date: 04/02/2025

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: Sharpe Jr., Robert J
Permit Number: 1820-8591
Effective:
02/01/2025-02/01/2027

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG506302
Exp Date: 03/04/2027


Test	g/210L	Time
DIAG	Pass	3:30pm
AIR BLK	.00	3:31pm
ACCY CHK	.08	3:32pm
AIR BLK	.00	3:33pm
SUB TEST	.00	3:34pm
AIR BLK	.00	3:34pm
SUB TEST	.00	3:36pm
AIR BLK	.00	3:37pm

Reported AC: 00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

Intox EC/IR-II: Preventive Maintenance

ROBESON COUNTY BAT MOBILE UNIT 10 770

Serial Number: 008686 Test Record Number: 7134
Test Date: 04/02/2025 Test Time: 3:38pm EDT

System Check: Passed

Baseline Tests

Test	Status	Time
IR	Pass	3:38pm
FLO	Pass	3:38pm
FC	Pass	3:38pm

Temperature Tests

Test	Status	Time
FC1	Pass	3:38pm
SRC	Pass	3:38pm
DET	Pass	3:38pm
BAR	Pass	3:38pm
BT	Pass	3:38pm

Blank Tests

Test	Status	Time
AIR	Pass	3:39pm

Printer Tests

Test	Status	Time
PRNT	Pass	3:39pm

CRC Tests

Test	Status	Time
COMP	Pass	3:39pm
CAL	Pass	3:39pm

**Preventive Maintenance
Status: Pass**



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Robeson Instrument Location BAT Mobile Unit 10
Instrument Serial No. 008686 Lumberton PD

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 10th day of April, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]

Signature of Certifying Official

2266313

Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

ROBESON COUNTY BAT MOBILE UNIT 10 770

Serial Number: 008686
Test Date: 04/10/2025

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Sharpe Jr., Robert J

Permit Number: 1820-8591

Effective:

02/01/2025-02/01/2027

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG506302

Exp Date: 03/04/2027

Test	g/210L	Time
DIAG	Pass	1:25pm
AIR BLK	.00	1:26pm
ACCY CHK	.08	1:27pm
AIR BLK	.00	1:28pm
SUB TEST	.00	1:29pm
AIR BLK	.00	1:30pm
SUB TEST	.00	1:32pm
AIR BLK	.00	1:33pm

Reported AC: .00 g/210L

Signature  Chemical Analyst

Court CVR


Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

ROBESON COUNTY BAT MOBILE UNIT 10 770

Serial Number: 008686 Test Record Number: 7136
Test Date: 04/10/2025 Test Time: 1:33pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	1:33pm
FLO	Pass	1:33pm
FC	Pass	1:33pm

Temperature Tests

Test	Status	Time
FC1	Pass	1:33pm
SRC	Pass	1:33pm
DET	Pass	1:33pm
BAR	Pass	1:33pm
BT	Pass	1:33pm

Blank Tests

Test	Status	Time
AIR	Pass	1:34pm

Printer Tests

Test	Status	Time
PRNT	Pass	1:34pm

CRC Tests

Test	Status	Time
COMP	Pass	1:34pm
CAL	Pass	1:34pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Robeson Instrument Location BAT Mobile Unit 10
Instrument Serial No. 00 8686 Red Springs PD

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 15th day of April, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

2266313
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

ROBESON COUNTY BAT MOBILE UNIT 10 770

Serial Number: 008686
Test Date: 04/15/2025

Citation Number: M0000000-0
Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Sharpe Jr., Robert J

Permit Number: 1820-8591

Effective:

02/01/2025-02/01/2027

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG506302
Exp Date: 03/04/2027

Test	g/210L	Time
DIAG	Pass	2:14pm
AIR BLK	.00	2:15pm
ACCY CHK	.08	2:16pm
AIR BLK	.00	2:17pm
SUB TEST	.00	2:18pm
AIR BLK	.00	2:19pm
SUB TEST	.00	2:20pm
AIR BLK	.00	2:21pm

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR

Analyst

Intox EC/IR-II: Preventive Maintenance

ROBESON COUNTY BAT MOBILE UNIT 10 770

Serial Number: 008686 Test Record Number: 7144
Test Date: 04/15/2025 Test Time: 2:22pm EDT

System Check: Passed

Baseline Tests

Test	Status	Time
IR	Pass	2:22pm
FLO	Pass	2:22pm
FC	Pass	2:22pm

Temperature Tests

Test	Status	Time
FC1	Pass	2:22pm
SRC	Pass	2:22pm
DET	Pass	2:22pm
BAR	Pass	2:22pm
BT	Pass	2:22pm

Blank Tests

Test	Status	Time
AIR	Pass	2:23pm

Printer Tests

Test	Status	Time
PRNT	Pass	2:23pm

CRC Tests

Test	Status	Time
COMP	Pass	2:23pm
CAL	Pass	2:23pm

**Preventive Maintenance
Status: Pass**



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Robeson Instrument Location BAT Mobile Unit 10
Instrument Serial No. 008686 Robeson County SU

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 25th day of April, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]

Signature of Certifying Official

2266313

Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

ROBESON COUNTY BAT MOBILE UNIT 10 770

Serial Number: 008686

Test Date: 04/25/2025

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Sharpe Jr., Robert J

Permit Number: 1820-8591

Effective:

02/01/2025-02/01/2027

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG506302

Exp Date: 03/04/2027

Test	g/210L	Time
DIAG	Pass	6:24pm
AIR BLK	.00	6:25pm
ACCY CHK	.07	6:25pm
AIR BLK	.00	6:26pm
SUB TEST	.00	6:27pm
AIR BLK	.00	6:28pm
SUB TEST	.00	6:29pm
AIR BLK	.00	6:30pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

ROBESON COUNTY BAT MOBILE UNIT 10 770

Serial Number: 008686 Test Record Number: 7153
Test Date: 04/25/2025 Test Time: 6:31pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	6:32pm
FLO	Pass	6:32pm
FC	Pass	6:32pm

Temperature Tests

Test	Status	Time
FC1	Pass	6:32pm
SRC	Pass	6:32pm
DET	Pass	6:32pm
BAR	Pass	6:32pm
BT	Pass	6:32pm

Blank Tests

Test	Status	Time
AIR	Pass	6:32pm

Printer Tests

Test	Status	Time
PRNT	Pass	6:32pm

CRC Tests

Test	Status	Time
COMP	Pass	6:33pm
CAL	Pass	6:33pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Robeson Instrument Location BAT Mobile Unit 10
Instrument Serial No. 00 8776 Robeson County SC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 2nd day of April, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

2266313
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

ROBESON COUNTY BAT MOBILE UNIT 10 770

Serial Number: 008776
Test Date: 04/02/2025

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Sharpe Jr., Robert J

Permit Number: 1820-8591

Effective:

02/01/2025-02/01/2027

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG417803


Exp Date: 06/26/2026

Test	g/210L	Time
DIAG	Pass	3:31pm
AIR BLK	.00	3:32pm
ACCY CHK	.08	3:33pm
AIR BLK	.00	3:34pm
SUB TEST	.00	3:35pm
AIR BLK	.00	3:35pm
SUB TEST	.00	3:37pm
AIR BLK	.00	3:38pm

Reported AC: .00 g/210L

Signature  Chemical Analyst

Court CVR


Analyst

Intox EC/IR-II: Preventive Maintenance

ROBESON COUNTY BAT MOBILE UNIT 10 770

Serial Number: 008776 Test Record Number: 4092
Test Date: 04/02/2025 Test Time: 3:39pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	3:39pm
FLO	Pass	3:39pm
FC	Pass	3:39pm

Temperature Tests

Test	Status	Time
FC1	Pass	3:39pm
SRC	Pass	3:39pm
DET	Pass	3:39pm
BAR	Pass	3:39pm
BT	Pass	3:39pm

Blank Tests

Test	Status	Time
AIR	Pass	3:40pm

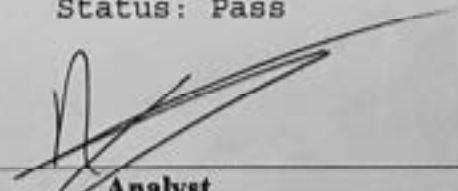
Printer Tests

Test	Status	Time
PRNT	Pass	3:40pm

CRC Tests

Test	Status	Time
COMP	Pass	3:40pm
CAL	Pass	3:40pm

Preventive Maintenance
Status: *Pass*



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Robeson Instrument Location BAT Mobile Unit 10
Instrument Serial No. 008776 Lumberton PD

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 10th day of April, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]

Signature of Certifying Official

2266313

Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

ROBESON COUNTY BAT MOBILE UNIT 10 770

Serial Number: 008776
Test Date: 04/10/2025

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: Sharpe Jr., Robert J
Permit Number: 1820-8591
Effective:
02/01/2025-02/01/2027

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG417803
Exp Date: 06/26/2026

Test	g/210L	Time
DIAG	Pass	1:28pm
AIR BLK	.00	1:29pm
ACCY CHK	.08	1:30pm
AIR BLK	.00	1:31pm
SUB TEST	.00	1:31pm
AIR BLK	.00	1:32pm
SUB TEST	.00	1:35pm
AIR BLK	.00	1:36pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

Intox EC/IR-II: Preventive Maintenance

ROBESON COUNTY BAT MOBILE UNIT 10 770

Serial Number: 008776 Test Record Number: 4094
Test Date: 04/10/2025 Test Time: 1:36pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	1:37pm
FLO	Pass	1:37pm
FC	Pass	1:37pm

Temperature Tests

Test	Status	Time
FC1	Pass	1:37pm
SRC	Pass	1:37pm
DET	Pass	1:37pm
BAR	Pass	1:37pm
BT	Pass	1:37pm

Blank Tests

Test	Status	Time
AIR	Pass	1:37pm


Printer Tests

Test	Status	Time
PRNT	Pass	1:37pm

CRC Tests

Test	Status	Time
COMP	Pass	1:38pm
CAL	Pass	1:38pm

Preventive Maintenance
Status: *Pass*



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Robeson Instrument Location BAT Mobile Unit 10
Instrument Serial No. 008776 Red Springs PD

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 15th day of April, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

2266313
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

ROBESON COUNTY BAT MOBILE UNIT 10 770

Serial Number: 008776
Test Date: 04/15/2025

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Sharpe Jr., Robert J

Permit Number: 1820-8591

Effective:

02/01/2025-02/01/2027

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG417803

Exp Date: 06/26/2026

Test	g/210L	Time
DIAG	Pass	2:18pm
AIR BLK	.00	2:19pm
ACCY CHK	.08	2:19pm
AIR BLK	.00	2:20pm
SUB TEST	.00	2:21pm
AIR BLK	.00	2:22pm
SUB TEST	.00	2:23pm
AIR BLK	.00	2:24pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

ROBESON COUNTY BAT MOBILE UNIT 10 770

Serial Number: 008776 Test Record Number: 4102
Test Date: 04/15/2025 Test Time: 2:24pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	2:25pm
FLO	Pass	2:25pm
FC	Pass	2:25pm

Temperature Tests

Test	Status	Time
FC1	Pass	2:25pm
SRC	Pass	2:25pm
DET	Pass	2:25pm
BAR	Pass	2:25pm
BT	Pass	2:25pm

Blank Tests

Test	Status	Time
AIR	Pass	2:25pm

Printer Tests

Test	Status	Time
PRNT	Pass	2:25pm

CRC Tests

Test	Status	Time
COMP	Pass	2:26pm
CAL	Pass	2:26pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Robeson Instrument Location BAT Mobile Unit 10
Instrument Serial No. 008776 Robeson County SO

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 25th day of April, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]

Signature of Certifying Official

2266313

Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

ROBESON COUNTY BAT MOBILE UNIT 10 770

Serial Number: 008776

Test Date: 04/25/2025

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Sharpe Jr., Robert J

Permit Number: 1820-8591

Effective:

02/01/2025-02/01/2027

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG417803

Exp Date: 06/26/2026

Test	g/210L	Time
DIAG	Pass	6:26pm
AIR BLK	.00	6:27pm
ACCY CHK	.08	6:28pm
AIR BLK	.00	6:29pm
SUB TEST	.00	6:29pm
AIR BLK	.00	6:30pm
SUB TEST	.00	6:32pm
AIR BLK	.00	6:33pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

ROBESON COUNTY BAT MOBILE UNIT 10 770

Serial Number: 008776 Test Record Number: 4110
Test Date: 04/25/2025 Test Time: 6:34pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	6:34pm
FLO	Pass	6:34pm
FC	Pass	6:34pm

Temperature Tests

Test	Status	Time
FC1	Pass	6:34pm
SRC	Pass	6:34pm
DET	Pass	6:34pm
BAR	Pass	6:34pm
BT	Pass	6:34pm

Blank Tests

Test	Status	Time
AIR	Pass	6:35pm

Printer Tests

Test	Status	Time
PRNT	Pass	6:35pm

CRC Tests

Test	Status	Time
COMP	Pass	6:35pm
CAL	Pass	6:35pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Robeson Instrument Location BAT Mobile Unit 10
Instrument Serial No. 00 8779 Robeson County SO

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 2nd day of April, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

2266313
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

ROBESON COUNTY BAT MOBILE UNIT 10 770

Serial Number: 008779
Test Date: 04/02/2025

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Sharpe Jr., Robert J

Permit Number: 1820-8591

Effective:

02/01/2025-02/01/2027

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG431002

Exp Date: 11/05/2026

Test	g/210L	Time
DIAG	Pass	3:28pm
AIR BLK	.00	3:29pm
ACCY CHK	.07	3:30pm
AIR BLK	.00	3:30pm
SUB TEST	.00	3:31pm
AIR BLK	.00	3:32pm
SUB TEST	.00	3:33pm
AIR BLK	.00	3:34pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

Intox EC/IR-II: Preventive Maintenance

ROBESON COUNTY BAT MOBILE UNIT 10 770

Serial Number: 008779 Test Record Number: 4039
Test Date: 04/02/2025 Test Time: 3:36pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	3:36pm
FLO	Pass	3:36pm
FC	Pass	3:36pm

Temperature Tests

Test	Status	Time
FC1	Pass	3:36pm
SRC	Pass	3:36pm
DET	Pass	3:36pm
BAR	Pass	3:36pm
BT	Pass	3:36pm

Blank Tests

Test	Status	Time
AIR	Pass	3:37pm

Printer Tests

Test	Status	Time
PRNT	Pass	3:37pm

CRC Tests

Test	Status	Time
COMP	Pass	3:37pm
CAL	Pass	3:37pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Robeson Instrument Location BAT Mobile Unit 10
Instrument Serial No. 008779 Lumberton PD

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 10th day of April, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

2266313
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

ROBESON COUNTY BAT MOBILE UNIT 10 770

Serial Number: 008779

Test Date: 04/10/2025

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Sharpe Jr., Robert J

Permit Number: 1820-8591

Effective:

02/01/2025-02/01/2027

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG431002

Exp Date: 11/05/2026

Test	g/210L	Time
DIAG	Pass	1:28pm
AIR BLK	.00	1:29pm
ACCY CHK	.07	1:29pm
AIR BLK	.00	1:30pm
SUB TEST	.00	1:31pm
AIR BLK	.00	1:32pm
SUB TEST	.00	1:33pm
AIR BLK	.00	1:34pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

ROBESON COUNTY BAT MOBILE UNIT 10 770

Serial Number: 008779 Test Record Number: 4041
Test Date: 04/10/2025 Test Time: 1:36pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	1:36pm
FLO	Pass	1:36pm
FC	Pass	1:36pm

Temperature Tests

Test	Status	Time
FC1	Pass	1:36pm
SRC	Pass	1:36pm
DET	Pass	1:36pm
BAR	Pass	1:36pm
BT	Pass	1:36pm

Blank Tests

Test	Status	Time
AIR	Pass	1:37pm


Printer Tests

Test	Status	Time
PRNT	Pass	1:37pm

CRC Tests

Test	Status	Time
COMP	Pass	1:37pm
CAL	Pass	1:37pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Robeson Instrument Location BAT Mobile Unit 10
Instrument Serial No. 00 8779 Red Springs PD

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 15th day of April, 20 25 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

2266313
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

ROBESON COUNTY BAT MOBILE UNIT 10 770

Serial Number: 008779

Test Date: 04/15/2025

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Sharpe Jr., Robert J

Permit Number: 1820-8591

Effective:

02/01/2025-02/01/2027

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG431002

Exp Date: 11/05/2026


Test	g/210L	Time
DIAG	Pass	2:16pm
AIR BLK	.00	2:17pm
ACCY CHK	.07	2:18pm
AIR BLK	.00	2:18pm
SUB TEST	.00	2:19pm
AIR BLK	.00	2:20pm
SUB TEST	.00	2:21pm
AIR BLK	.00	2:22pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

This form is used when performing Preventive Maintenance procedures

Forensic Tests for Alcohol Branch

Department of Health and Human Services

Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

ROBESON COUNTY BAT MOBILE UNIT 10 770

Serial Number: 008779 Test Record Number: 4049
Test Date: 04/15/2025 Test Time: 2:23pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	2:23pm
FLO	Pass	2:23pm
FC	Pass	2:23pm

Temperature Tests

Test	Status	Time
FC1	Pass	2:23pm
SRC	Pass	2:23pm
DET	Pass	2:23pm
BAR	Pass	2:23pm
BT	Pass	2:23pm

Blank Tests

Test	Status	Time
AIR	Pass	2:24pm

Printer Tests

Test	Status	Time
PRNT	Pass	2:24pm

CRC Tests

Test	Status	Time
COMP	Pass	2:24pm
CAL	Pass	2:24pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Robeson Instrument Location IBAT Mobile Unit 10
Instrument Serial No. 008779 Robeson County SO

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 25th day of April, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

2266313
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

ROBESON COUNTY BAT MOBILE UNIT 10 770

Serial Number: 008779
Test Date: 04/25/2025

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: Sharpe Jr., Robert J
Permit Number: 1820-8591
Effective:
02/01/2025-02/01/2027

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG431002
Exp Date: 11/05/2026

Test	g/210L	Time
DIAG	Pass	6:26pm
AIR BLK	.00	6:27pm
ACCY CHK	.07	6:28pm
AIR BLK	.00	6:29pm
SUB TEST	.00	6:29pm
AIR BLK	.00	6:30pm
SUB TEST	.00	6:32pm
AIR BLK	.00	6:33pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

Intox EC/IR-II: Preventive Maintenance

ROBESON COUNTY BAT MOBILE UNIT 10 770

Serial Number: 008779 Test Record Number: 4057
Test Date: 04/25/2025 Test Time: 6:33pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	6:34pm
FLO	Pass	6:34pm
FC	Pass	6:34pm

Temperature Tests

Test	Status	Time
FC1	Pass	6:34pm
SRC	Pass	6:34pm
DET	Pass	6:34pm
BAR	Pass	6:34pm
BT	Pass	6:34pm

Blank Tests

Test	Status	Time
AIR	Pass	6:35pm

Printer Tests

Test	Status	Time
PRNT	Pass	6:35pm

CRC Tests

Test	Status	Time
COMP	Pass	6:35pm
CAL	Pass	6:35pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County ROCKINGHAM Instrument Location EDEN POLICE
Instrument Serial No. 008636 DEPARTMENT

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 15TH day of APRIL, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.




Signature of Certifying Official

353799
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

ROCKINGHAM COUNTY EDEN PD 780

Serial Number: 008636
Test Date: 04/15/2025

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Oligmueller, Leo A

Permit Number: 0035-3799

Effective:

02/01/2025-02/01/2027

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG503001

Exp Date: 01/30/2027

Test	g/210L	Time
DIAG	Pass	2:44pm
AIR BLK	.00	2:45pm
ACCY CHK	.08	2:45pm
AIR BLK	.00	2:47pm
SUB TEST	.00	2:48pm
AIR BLK	.00	2:49pm
SUB TEST	.00	2:50pm
AIR BLK	.00	2:51pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

ROCKINGHAM COUNTY EDEN PD 780

Serial Number: 008636 Test Record Number: 2827
Test Date: 04/15/2025 Test Time: 2:52pm EDT

System Check: Passed

Baseline Tests

Test	Status	Time
IR	Pass	2:52pm
FLO	Pass	2:52pm
FC	Pass	2:53pm

Temperature Tests

Test	Status	Time
FC1	Pass	2:53pm
SRC	Pass	2:53pm
DET	Pass	2:53pm
BAR	Pass	2:53pm
BT	Pass	2:53pm

Blank Tests

Test	Status	Time
AIR	Pass	2:53pm

Printer Tests

Test	Status	Time
PRNT	Pass	2:53pm

CRC Tests

Test	Status	Time
COMP	Pass	2:54pm
CAL	Pass	2:54pm

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

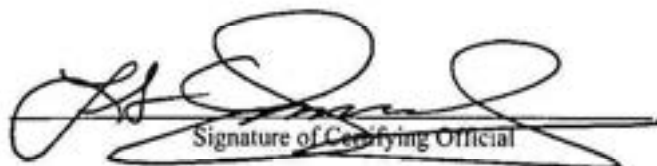
County ROCKINGHAM Instrument Location REIDSVILLE
Instrument Serial No. 008784 POLICE DEPARTMENT

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 15TH day of APRIL, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.




Signature of Certifying Official

353799
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

ROCKINGHAM COUNTY REIDSVILLE PD 780

Serial Number: 008784
Test Date: 04/15/2025

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Oligmueller, Leo A

Permit Number: 0035-3799

Effective:

02/01/2025-02/01/2027

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG417802

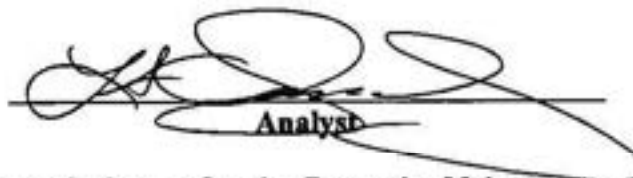
Exp Date: 06/26/2026

Test	g/210L	Time
DIAG	Pass	12:15pm
AIR BLK	.00	12:16pm
ACCY CHK	.08	12:16pm
AIR BLK	.00	12:18pm
SUB TEST	.00	12:18pm
AIR BLK	.00	12:19pm
SUB TEST	.00	12:21pm
AIR BLK	.00	12:22pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

ROCKINGHAM COUNTY REIDSVILLE PD 780

Serial Number: 008784 Test Record Number: 1591
Test Date: 04/15/2025 Test Time: 12:23pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	12:24pm
FLO	Pass	12:24pm
FC	Pass	12:24pm

Temperature Tests

Test	Status	Time
FC1	Pass	12:24pm
SRC	Pass	12:24pm
DET	Pass	12:24pm
BAR	Pass	12:24pm
BT	Pass	12:24pm

Blank Tests

Test	Status	Time
AIR	Pass	12:24pm

Printer Tests

Test	Status	Time
PRNT	Pass	12:24pm

CRC Tests

Test	Status	Time
COMP	Pass	12:25pm
CAL	Pass	12:25pm

Preventive Maintenance
Status: Pass


Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County ROCKINGHAM Instrument Location ROCKINGHAM COUNTY
Instrument Serial No. 008796 JAIL

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 15TH day of APRIL, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

669
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

ROCKINGHAM COUNTY ROCKINGHAM CO JAIL
780

Serial Number: 008796
Test Date: 04/15/2025

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Oligmueller, Leo A

Permit Number: 0035-3799

Effective:

02/01/2025-02/01/2027

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG431003

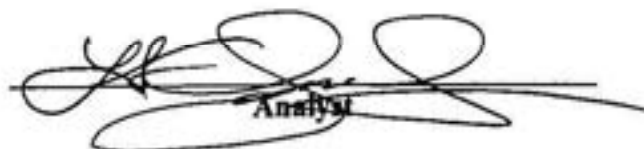
Exp Date: 11/05/2026

Test	g/210L	Time
DIAG	Pass	1:31pm
AIR BLK	.00	1:31pm
ACCY CHK	.08	1:32pm
AIR BLK	.00	1:33pm
SUB TEST	.00	1:34pm
AIR BLK	.00	1:35pm
SUB TEST	.00	1:36pm
AIR BLK	.00	1:37pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

ROCKINGHAM COUNTY ROCKINGHAM CO JAIL 780

Serial Number: 008796 Test Record Number: 3896
Test Date: 04/15/2025 Test Time: 1:40pm EDT

System Check: Passed

Baseline Tests

Test	Status	Time
IR	Pass	1:40pm
FLO	Pass	1:40pm
FC	Pass	1:40pm

Temperature Tests

Test	Status	Time
FC1	Pass	1:40pm
SRC	Pass	1:40pm
DET	Pass	1:40pm
BAR	Pass	1:40pm
BT	Pass	1:40pm

Blank Tests

Test	Status	Time
AIR	Pass	1:41pm

Printer Tests

Test	Status	Time
PRNT	Pass	1:41pm

CRC Tests

Test	Status	Time
COMP	Pass	1:41pm
CAL	Pass	1:41pm

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County ROCKINGHAM Instrument Location MADISON
Instrument Serial No. 008802 POLICE DEPARTMENT

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 15TH day of APRIL, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

353799
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

ROCKINGHAM COUNTY MADISON PD 780

Serial Number: 008802
Test Date: 04/15/2025

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Oligmueller, Leo A

Permit Number: 0035-3799

Effective:

02/01/2025-02/01/2027

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

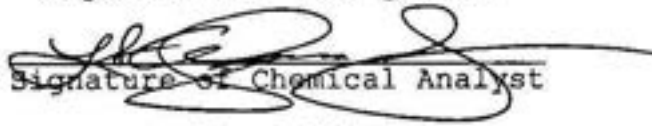
Test Type: Breath Test

Lot Number: AG400302

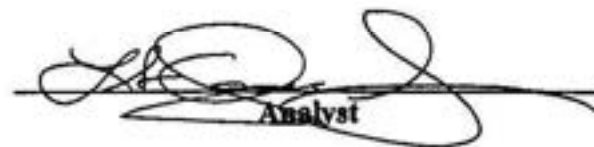
Exp Date: 01/03/2026

Test	g/210L	Time
DIAG	Pass	4:22pm
AIR BLK	.00	4:22pm
ACCY CHK	.08	4:23pm
AIR BLK	.00	4:24pm
SUB TEST	.00	4:25pm
AIR BLK	.00	4:26pm
SUB TEST	.00	4:29pm
AIR BLK	.00	4:30pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

ROCKINGHAM COUNTY MADISON PD 780

Serial Number: 008802 Test Record Number: 1107
Test Date: 04/15/2025 Test Time: 4:34pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	4:35pm
FLO	Pass	4:35pm
FC	Pass	4:35pm

Temperature Tests

Test	Status	Time
FC1	Pass	4:35pm
SRC	Pass	4:35pm
DET	Pass	4:35pm
BAR	Pass	4:35pm
BT	Pass	4:35pm

Blank Tests

Test	Status	Time
AIR	Pass	4:35pm

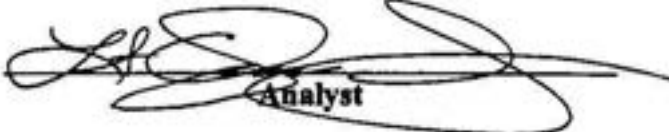
Printer Tests

Test	Status	Time
PRNT	Pass	4:35pm

CRC Tests

Test	Status	Time
COMP	Pass	4:36pm
CAL	Pass	4:36pm

Preventive Maintenance
Status: Pass


Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Sampson Instrument Location BAT Mobile Unit 10
Instrument Serial No. 008584 Sampson County SO

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 19th day of April, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]

Signature of Certifying Official

2266313

Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

SAMPSON COUNTY BAT MOBILE UNIT 10 810

Serial Number: 008584

Test Date: 04/19/2025

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Sharpe Jr., Robert J

Permit Number: 1820-8591

Effective:

02/01/2025-02/01/2027

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG400303

Exp Date: 01/03/2026

Test	g/210L	Time
DIAG	Pass	2:01pm
AIR BLK	.00	2:02pm
ACCY CHK	.07	2:02pm
AIR BLK	.00	2:03pm
SUB TEST	.00	2:04pm
AIR BLK	.00	2:05pm
SUB TEST	.00	2:06pm
AIR BLK	.00	2:07pm

Reported AC: ~~.00~~ g/210L

Signature of Chemical Analyst

Court CVR

Analyst

Intox EC/IR-II: Preventive Maintenance

SAMPSON COUNTY BAT MOBILE UNIT 10 810

Serial Number: 008584 Test Record Number: 2788
Test Date: 04/19/2025 Test Time: 2:07pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	2:07pm
FLO	Pass	2:07pm
FC	Pass	2:08pm

Temperature Tests

Test	Status	Time
FC1	Pass	2:08pm
SRC	Pass	2:08pm
DET	Pass	2:08pm
BAR	Pass	2:08pm
BT	Pass	2:08pm

Blank Tests

Test	Status	Time
AIR	Pass	2:08pm

Printer Tests

Test	Status	Time
PRNT	Pass	2:08pm

CRC Tests

Test	Status	Time
COMP	Pass	2:09pm
CAL	Pass	2:09pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Sampson Instrument Location BAT Mobile Unit 10
Instrument Serial No. 008637 Sampson County SO

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 19th day of April, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

2266313
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

SAMPSON COUNTY BAT MOBILE UNIT 10 810

Serial Number: 008637
Test Date: 04/19/2025

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Sharpe Jr., Robert J

Permit Number: 1820-8591

Effective:

02/01/2025-02/01/2027

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG400303

Exp Date: 01/03/2026


Test	g/210L	Time
DIAG	Pass	2:03pm
AIR BLK	.00	2:04pm
ACCY CHK	.08	2:04pm
AIR BLK	.00	2:05pm
SUB TEST	.00	2:06pm
AIR BLK	.00	2:07pm
SUB TEST	.00	2:08pm
AIR BLK	.00	2:09pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

SAMPSON COUNTY BAT MOBILE UNIT 10 810

Serial Number: 008637 Test Record Number: 3524

Test Date: 04/19/2025 Test Time: 2:10pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	2:10pm
FLO	Pass	2:10pm
FC	Pass	2:10pm

Temperature Tests

Test	Status	Time
FC1	Pass	2:10pm
SRC	Pass	2:10pm
DET	Pass	2:10pm
BAR	Pass	2:10pm
BT	Pass	2:10pm

Blank Tests

Test	Status	Time
AIR	Pass	2:11pm


Printer Tests

Test	Status	Time
PRNT	Pass	2:11pm

CRC Tests

Test	Status	Time
COMP	Pass	2:11pm
CAL	Pass	2:11pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Sampson Instrument Location BAT Mobile Unit 10

Instrument Serial No. 008686 Sampson County SO

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 19th day of April, 20 25 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]

Signature of Certifying Official

2266313

Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

SAMPSON COUNTY BAT MOBILE UNIT 10 810

Serial Number: 008686

Test Date: 04/19/2025

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Sharpe Jr., Robert J

Permit Number: 1820-8591

Effective:

02/01/2025-02/01/2027

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG506302

Exp Date: 03/04/2027

Test	g/210L	Time
DIAG	Pass	2:01pm
AIR BLK	.00	2:02pm
ACCY CHK	.08	2:03pm
AIR BLK	.00	2:03pm
SUB TEST	.00	2:04pm
AIR BLK	.00	2:05pm
SUB TEST	.00	2:07pm
AIR BLK	.00	2:08pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

Intox EC/IR-II: Preventive Maintenance

SAMPSON COUNTY BAT MOBILE UNIT 10 810

Serial Number: 008686 Test Record Number: 7151
Test Date: 04/19/2025 Test Time: 2:08pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	2:09pm
FLO	Pass	2:09pm
FC	Pass	2:09pm

Temperature Tests

Test	Status	Time
FC1	Pass	2:09pm
SRC	Pass	2:09pm
DET	Pass	2:09pm
BAR	Pass	2:09pm
BT	Pass	2:09pm

Blank Tests

Test	Status	Time
AIR	Pass	2:09pm

Printer Tests

Test	Status	Time
PRNT	Pass	2:09pm

CRC Tests

Test	Status	Time
COMP	Pass	2:10pm
CAL	Pass	2:10pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Sampson Instrument Location BAT Mobile Unit 10
Instrument Serial No. 008776 Sampson County SO

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 19th day of April, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]

Signature of Certifying Official

2266313
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

SAMPSON COUNTY BAT MOBILE UNIT 10 810

Serial Number: 008776
Test Date: 04/19/2025

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Sharpe Jr., Robert J

Permit Number: 1820-8591

Effective:

02/01/2025-02/01/2027

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG417803

Exp Date: 06/26/2026


Test	g/210L	Time
DIAG	Pass	2:04pm
AIR BLK	.00	2:05pm
ACCY CHK	.08	2:05pm
AIR BLK	.00	2:06pm
SUB TEST	.00	2:07pm
AIR BLK	.00	2:08pm
SUB TEST	.00	2:09pm
AIR BLK	.00	2:10pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

SAMPSON COUNTY BAT MOBILE UNIT 10 810

Serial Number: 008776 Test Record Number: 4108
Test Date: 04/19/2025 Test Time: 2:12pm EDT

System Check: Passed

Baseline Tests

Test	Status	Time
IR	Pass	2:12pm
FLO	Pass	2:12pm
FC	Pass	2:13pm

Temperature Tests

Test	Status	Time
FC1	Pass	2:13pm
SRC	Pass	2:13pm
DET	Pass	2:13pm
BAR	Pass	2:13pm
BT	Pass	2:13pm

Blank Tests

Test	Status	Time
AIR	Pass	2:13pm

Printer Tests

Test	Status	Time
PRNT	Pass	2:13pm

CRC Tests

Test	Status	Time
COMP	Pass	2:13pm
CAL	Pass	2:14pm

**Preventive Maintenance
Status: Pass**



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County Sampson Instrument Location BAT Mobile Unit 10
Instrument Serial No. 00 8779 Sampson County SO

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 19th day of April, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

2266313
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

SAMPSON COUNTY BAT MOBILE UNIT 10 810

Serial Number: 008779

Test Date: 04/19/2025

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Sharpe Jr., Robert J

Permit Number: 1820-8591

Effective:

02/01/2025-02/01/2027

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG431002

Exp Date: 11/05/2026


Test	g/210L	Time
DIAG	Pass	2:04pm
AIR BLK	.00	2:05pm
ACCY CHK	.07	2:05pm
AIR BLK	.00	2:06pm
SUB TEST	.00	2:06pm
AIR BLK	.00	2:07pm
SUB TEST	.00	2:09pm
AIR BLK	.00	2:10pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

SAMPSON COUNTY BAT MOBILE UNIT 10 810

Serial Number: 008779 Test Record Number: 4055
Test Date: 04/19/2025 Test Time: 2:10pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	2:11pm
FLO	Pass	2:11pm
FC	Pass	2:11pm

Temperature Tests

Test	Status	Time
FC1	Pass	2:11pm
SRC	Pass	2:11pm
DET	Pass	2:11pm
BAR	Pass	2:11pm
BT	Pass	2:11pm

Blank Tests

Test	Status	Time
AIR	Pass	2:11pm

Printer Tests

Test	Status	Time
PRNT	Pass	2:11pm

CRC Tests

Test	Status	Time
COMP	Pass	2:12pm
CAL	Pass	2:12pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Transylvania Instrument Location Transylvania County Jail
Instrument Serial No. 008609 Brevard, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 15 day of April, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

244987
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

TRANSYLVANIA COUNTY TRANSYLVANIA
COUNTY JAIL 870

Serial Number: 008609
Test Date: 04/15/2025

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: Loftis, Benjamin C
Permit Number: 0024-4987
Effective:
03/01/2025-03/01/2027

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG417803
Exp Date: 06/26/2026


Test	g/210L	Time
DIAG	Pass	12:22pm
AIR BLK	.00	12:22pm
ACCY CHK	.07	12:23pm
AIR BLK	.00	12:24pm
SUB TEST	.00	12:25pm
AIR BLK	.00	12:26pm
SUB TEST	.00	12:27pm
AIR BLK	.00	12:28pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

Intox EC/IR-II: Preventive Maintenance

TRANSYLVANIA COUNTY TRANSYLVANIA COUNTY JAIL 870

Serial Number: 008609 Test Record Number: 1317
Test Date: 04/15/2025 Test Time: 12:28pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	12:28pm
FLO	Pass	12:28pm
FC	Pass	12:29pm

Temperature Tests

Test	Status	Time
FC1	Pass	12:29pm
SRC	Pass	12:29pm
DET	Pass	12:29pm
BAR	Pass	12:29pm
BT	Pass	12:29pm

Blank Tests

Test	Status	Time
AIR	Pass	12:29pm


Printer Tests

Test	Status	Time
PRNT	Pass	12:29pm

CRC Tests

Test	Status	Time
COMP	Pass	12:30pm
CAL	Pass	12:30pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Transylvania Instrument Location Transylvania County Jail
Instrument Serial No. 008820 Brevard, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 15 day of April, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

244987
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

TRANSYLVANIA COUNTY TRANSYLVANIA
COUNTY JAIL 870

Serial Number: 008820
Test Date: 04/15/2025

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE

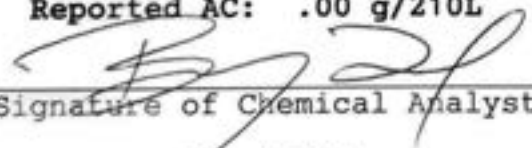
Analyst's Name: Loftis, Benjamin C
Permit Number: 0024-4987
Effective:
03/01/2025-03/01/2027

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG417803
Exp Date: 06/26/2026

Test	g/210L	Time
DIAG	Pass	12:22pm
AIR BLK	.00	12:23pm
ACCY CHK	.07	12:23pm
AIR BLK	.00	12:25pm
SUB TEST	.00	12:25pm
AIR BLK	.00	12:26pm
SUB TEST	.00	12:27pm
AIR BLK	.00	12:28pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

TRANSYLVANIA COUNTY TRANSYLVANIA COUNTY JAIL 870

Serial Number: 008820 Test Record Number: 1771
Test Date: 04/15/2025 Test Time: 12:29pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	12:29pm
FLO	Pass	12:29pm
FC	Pass	12:29pm

Temperature Tests

Test	Status	Time
FC1	Pass	12:29pm
SRC	Pass	12:29pm
DET	Pass	12:29pm
BAR	Pass	12:29pm
BT	Pass	12:29pm

Blank Tests

Test	Status	Time
AIR	Pass	12:30pm

Printer Tests

Test	Status	Time
PRNT	Pass	12:30pm

CRC Tests

Test	Status	Time
COMP	Pass	12:30pm
CAL	Pass	12:30pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Union Instrument Location Stallings PD
Instrument Serial No. 008927 Stallings, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 28th day of April, 2028 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Boyo Helms
Signature of Certifying Official

849845
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

UNION COUNTY STALLINGS PD 890

Serial Number: 008927
Test Date: 04/28/2025

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Helms, Bryce A

Permit Number: 0084-9845

Effective:

02/01/2025-02/01/2027

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG431001

Exp Date: 11/05/2026

Test	g/210L	Time
DIAG	Pass	1:53pm
AIR BLK	.00	1:54pm
ACCY CHK	.07	1:55pm
AIR BLK	.00	1:56pm
SUB TEST	.00	1:56pm
AIR BLK	.00	1:57pm
SUB TEST	.00	1:59pm
AIR BLK	.00	2:00pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

Intox EC/IR-II: Preventive Maintenance

UNION COUNTY STALLINGS PD 890

Serial Number: 008927 Test Record Number: 1266
Test Date: 04/28/2025 Test Time: 2:00pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	2:00pm
FLO	Pass	2:00pm
FC	Pass	2:01pm

Temperature Tests

Test	Status	Time
FC1	Pass	2:01pm
SRC	Pass	2:01pm
DET	Pass	2:01pm
BAR	Pass	2:01pm
BT	Pass	2:01pm

Blank Tests

Test	Status	Time
AIR	Pass	2:01pm

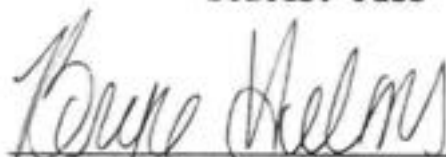
Printer Tests

Test	Status	Time
PRNT	Pass	2:01pm

CRC Tests

Test	Status	Time
COMP	Pass	2:02pm
CAL	Pass	2:02pm

Preventive Maintenance
Status: *Pass*



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County VANCE Instrument Location VANCE Co. S. D.
Instrument Serial No. 008870 156 Church St
HENDERSON, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 2 day of April, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

179707
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

VANCE COUNTY SHERIFF'S DEPARTMENT 900

Serial Number: 008870
Test Date: 04/02/2025

Citation Number: M0000000-0
Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Bryant, Earl A

Permit Number: 0017-9707

Effective:

02/01/2025-02/01/2027

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG501307

Exp Date: 01/13/2027

Test	g/210L	Time
DIAG	Pass	3:23pm
AIR BLK	.00	3:23pm
ACCY CHK	.08	3:24pm
AIR BLK	.00	3:26pm
SUB TEST	.00	3:26pm
AIR BLK	.00	3:27pm
SUB TEST	.00	3:29pm
AIR BLK	.00	3:30pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

This form is used when performing Preventive Maintenance procedures

Forensic Tests for Alcohol Branch

Department of Health and Human Services

Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

VANCE COUNTY SHERIFF'S DEPARTMENT 900

Serial Number: 008870 Test Record Number: 4004
Test Date: 04/02/2025 Test Time: 3:31pm EDT

System Check: Passed

Baseline Tests

Test	Status	Time
IR	Pass	3:32pm
FLO	Pass	3:32pm
FC	Pass	3:32pm

Temperature Tests

Test	Status	Time
FC1	Pass	3:32pm
SRC	Pass	3:32pm
DET	Pass	3:32pm
BAR	Pass	3:32pm
BT	Pass	3:32pm

Blank Tests

Test	Status	Time
AIR	Pass	3:32pm

Printer Tests

Test	Status	Time
PRNT	Pass	3:32pm

CRC Tests

Test	Status	Time
COMP	Pass	3:33pm
CAL	Pass	3:33pm

Preventive Maintenance
Status: Pass


Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County VANCE Instrument Location VANCE Co. S.D.
Instrument Serial No. 008937 156 Church St
HENDERSON, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 1 day of April, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

179707
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

VANCE COUNTY SHERIFF'S DEPARTMENT 900

Serial Number: 008937

Test Date: 04/01/2025

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Bryant, Earl A

Permit Number: 0017-9707

Effective:

02/01/2025-02/01/2027

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG501307

Exp Date: 01/13/2027

Test	g/210L	Time
DIAG	Pass	2:45pm
AIR BLK	.00	2:46pm
ACCY CHK	.08	2:47pm
AIR BLK	.00	2:48pm
SUB TEST	.00	2:49pm
AIR BLK	.00	2:50pm
SUB TEST	.00	2:51pm
AIR BLK	.00	2:52pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

This form is used when performing Preventive Maintenance procedures

Forensic Tests for Alcohol Branch

Department of Health and Human Services

Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

VANCE COUNTY SHERIFF'S DEPARTMENT 900

Serial Number: 008937 Test Record Number: 3565
Test Date: 04/01/2025 Test Time: 2:53pm EDT

System Check: Passed

Baseline Tests

Test	Status	Time
IR	Pass	2:54pm
FLO	Pass	2:54pm
FC	Pass	2:54pm

Temperature Tests

Test	Status	Time
FC1	Pass	2:54pm
SRC	Pass	2:54pm
DET	Pass	2:54pm
BAR	Pass	2:54pm
BT	Pass	2:54pm

Blank Tests

Test	Status	Time
AIR	Pass	2:55pm

Printer Tests

Test	Status	Time
PRNT	Pass	2:55pm

CRC Tests

Test	Status	Time
COMP	Pass	2:55pm
CAL	Pass	2:55pm

Preventive Maintenance
Status: Pass


Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Wake Instrument Location Wake County Detention Ctr
Instrument Serial No. 008577 3301 Hammond Rd
Raleigh, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 3 day of April, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Simon Stokes Brown

Signature of Certifying Official

146221

Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

WAKE COUNTY DETENTION CENTER 910

Serial Number: 008577
Test Date: 04/03/2025

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: Barnes, Simon S
Permit Number: 0014-6221
Effective:
02/01/2025-02/01/2027

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test


Lot Number: AG501307
Exp Date: 01/13/2027

Test	g/210L	Time
DIAG	Pass	1:10pm
AIR BLK	.00	1:11pm
ACCY CHK	.07	1:11pm
AIR BLK	.00	1:12pm
SUB TEST	.00	1:14pm
AIR BLK	.00	1:14pm
SUB TEST	.00	1:16pm
AIR BLK	.00	1:17pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

Intox EC/IR-II: Preventive Maintenance

WAKE COUNTY DETENTION CENTER 910

Serial Number: 008577 Test Record Number: 8579
Test Date: 04/03/2025 Test Time: 1:17pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	1:18pm
FLO	Pass	1:18pm
FC	Pass	1:18pm

Temperature Tests

Test	Status	Time
FC1	Pass	1:18pm
SRC	Pass	1:18pm
DET	Pass	1:18pm
BAR	Pass	1:18pm
BT	Pass	1:18pm

Blank Tests

Test	Status	Time
AIR	Pass	1:18pm


Printer Tests

Test	Status	Time
PRNT	Pass	1:18pm

CRC Tests

Test	Status	Time
COMP	Pass	1:18pm
CAL	Pass	1:18pm

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Wake Instrument Location RALEIGH PD Durham Dist
Instrument Serial No. 008651 218 W. CABARRUS ST
RALEIGH, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 11 day of April, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

179707
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

WAKE COUNTY RALEIGH PD DOWNTOWN 910

Serial Number: 008651

Test Date: 04/11/2025

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Bryant, Earl A

Permit Number: 0017-9707

Effective:

02/01/2025-02/01/2027

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG400301

Exp Date: 01/03/2026

Test	g/210L	Time
DIAG	Pass	10:11am
AIR BLK	.00	10:12am
ACCY CHK	.08	10:12am
AIR BLK	.00	10:13am
SUB TEST	.00	10:14am
AIR BLK	.00	10:15am
SUB TEST	.00	10:16am
AIR BLK	.00	10:17am

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

WAKE COUNTY RALEIGH PD DOWNTOWN 910

Serial Number: 008651 Test Record Number: 1839
Test Date: 04/11/2025 Test Time: 10:18am EDT

System Check: Passed

Baseline Tests

Test	Status	Time
IR	Pass	10:18am
FLO	Pass	10:18am
FC	Pass	10:18am

Temperature Tests

Test	Status	Time
FC1	Pass	10:18am
SRC	Pass	10:18am
DET	Pass	10:18am
BAR	Pass	10:18am
BT	Pass	10:18am

Blank Tests

Test	Status	Time
AIR	Pass	10:19am

Printer Tests

Test	Status	Time
PRNT	Pass	10:19am

CRC Tests

Test	Status	Time
COMP	Pass	10:19am
CAL	Pass	10:19am

Preventive Maintenance
Status: Pass



Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Wake Instrument Location Holly Springs PD
Instrument Serial No. 008757 750 Holly Springs PD
Holly Springs, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 4 day of April, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Erin Ashley Brown

Signature of Certifying Official

146221

Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

WAKE COUNTY HOLLY SPRINGS PD 910

Serial Number: 008757
Test Date: 04/04/2025

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE

Analyst's Name: Barnes, Simon S
Permit Number: 0014-6221
Effective:
02/01/2025-02/01/2027

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG400302
Exp Date: 01/03/2026

Test	g/210L	Time
DIAG	Pass	8:00am
AIR BLK	.00	8:01am
ACCY CHK	.08	8:02am
AIR BLK	.00	8:03am
SUB TEST	.00	8:03am
AIR BLK	.00	8:04am
SUB TEST	.00	8:05am
AIR BLK	.00	8:06am

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

WAKE COUNTY HOLLY SPRINGS PD 910

Serial Number: 008757 Test Record Number: 2901
Test Date: 04/04/2025 Test Time: 8:07am EDT

System Check: Passed

Baseline Tests

Test	Status	Time
IR	Pass	8:07am
FLO	Pass	8:07am
FC	Pass	8:07am

Temperature Tests

Test	Status	Time
FC1	Pass	8:07am
SRC	Pass	8:07am
DET	Pass	8:07am
BAR	Pass	8:07am
BT	Pass	8:07am

Blank Tests

Test	Status	Time
AIR	Pass	8:08am

Printer Tests

Test	Status	Time
PRNT	Pass	8:08am

CRC Tests

Test	Status	Time
COMP	Pass	8:08am
CAL	Pass	8:08am

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Wake Instrument Location Wake County Detention Ctr
Instrument Serial No. 008764 3301 Hammond Rd
Raleigh, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 3 day of April, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Simon Stokes Brewer
Signature of Certifying Official

146221
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

WAKE COUNTY DETENTION CENTER 910

Serial Number: 008760
Test Date: 04/03/2025

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: Barnes, Simon S
Permit Number: 0014-6221
Effective:
02/01/2025-02/01/2027

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG501307
Exp Date: 01/13/2027

Test	g/210L	Time
DIAG	Pass	1:10pm
AIR BLK	.00	1:11pm
ACCY CHK	.07	1:11pm
AIR BLK	.00	1:13pm
SUB TEST	.00	1:14pm
AIR BLK	.00	1:14pm
SUB TEST	.00	1:16pm
AIR BLK	.00	1:17pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

Intox EC/IR-II: Preventive Maintenance

WAKE COUNTY DETENTION CENTER 910

Serial Number: 008760 Test Record Number: 7234
Test Date: 04/03/2025 Test Time: 1:22pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	1:23pm
FLO	Pass	1:23pm
FC	Pass	1:23pm

Temperature Tests

Test	Status	Time
FC1	Pass	1:23pm
SRC	Pass	1:23pm
DET	Pass	1:23pm
BAR	Pass	1:23pm
BT	Pass	1:23pm

Blank Tests

Test	Status	Time
AIR	Pass	1:24pm

Printer Tests

Test	Status	Time
PRNT	Pass	1:24pm

CRC Tests

Test	Status	Time
COMP	Pass	1:24pm
CAL	Pass	1:24pm

Preventive Maintenance
Status: *Pass*



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County Wake Instrument Location Wake County Detention Ctr
Instrument Serial No. 008778 3301 Hammond Rd
Raleigh, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 3 day of April, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Simon Stokes Barnes

Signature of Certifying Official

146221

Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

WAKE COUNTY DETENTION CENTER 910

Serial Number: 008778

Test Date: 04/03/2025

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Barnes, Simon S

Permit Number: 0014-6221

Effective:

02/01/2025-02/01/2027

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG501307

Exp Date: 01/13/2027

Test	g/210L	Time
DIAG	Pass	1:07pm
AIR BLK	.00	1:08pm
ACCY CHK	.07	1:09pm
AIR BLK	.00	1:10pm
SUB TEST	.00	1:11pm
AIR BLK	.00	1:11pm
SUB TEST	.00	1:13pm
AIR BLK	.00	1:14pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

Intox EC/IR-II: Preventive Maintenance

WAKE COUNTY DETENTION CENTER 910

Serial Number: 008778 Test Record Number: 8615
Test Date: 04/03/2025 Test Time: 1:15pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	1:15pm
FLO	Pass	1:15pm
FC	Pass	1:15pm

Temperature Tests

Test	Status	Time
FC1	Pass	1:16pm
SRC	Pass	1:16pm
DET	Pass	1:16pm
BAR	Pass	1:16pm
BT	Pass	1:16pm

Blank Tests

Test	Status	Time
AIR	Pass	1:16pm

Printer Tests

Test	Status	Time
PRNT	Pass	1:16pm

CRC Tests

Test	Status	Time
COMP	Pass	1:16pm
CAL	Pass	1:16pm

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Wake Instrument Location BAT Mobile Unit 13
Instrument Serial No. 008869

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 17 day of April, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Timothy B. White
Signature of Certifying Official

307699
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

WAKE COUNTY BAT MOBILE UNIT 13 910

Serial Number: 008869
Test Date: 04/17/2025

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Whitehurst, Timothy B

Permit Number: 0030-7699

Effective:

03/01/2025-03/01/2027

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG417803


Exp Date: 06/26/2026

Test	g/210L	Time
DIAG	Pass	4:48pm
AIR BLK	.00	4:49pm
ACCY CHK	.07	4:49pm
AIR BLK	.00	4:50pm
SUB TEST	.00	4:51pm
AIR BLK	.00	4:52pm
SUB TEST	.00	4:54pm
AIR BLK	.00	4:55pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

WAKE COUNTY BAT MOBILE UNIT 13 910

Serial Number: 008869 Test Record Number: 2006
Test Date: 04/17/2025 Test Time: 4:55pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	4:56pm
FLO	Pass	4:56pm
FC	Pass	4:56pm

Temperature Tests

Test	Status	Time
FC1	Pass	4:56pm
SRC	Pass	4:56pm
DET	Pass	4:56pm
BAR	Pass	4:56pm
BT	Pass	4:56pm

Blank Tests

Test	Status	Time
AIR	Pass	4:57pm

Printer Tests

Test	Status	Time
PRNT	Pass	4:57pm

CRC Tests

Test	Status	Time
COMP	Pass	4:57pm
CAL	Pass	4:57pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Wake Instrument Location BAT Mobile Unit 13
Instrument Serial No. 005898

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 17 day of April, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Tommy B. White

Signature of Certifying Official

307699

Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

WAKE COUNTY BAT MOBILE UNIT 13 910

Serial Number: 008898

Test Date: 04/17/2025

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Whitehurst, Timothy B

Permit Number: 0030-7699

Effective:

03/01/2025-03/01/2027

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG506302

Exp Date: 03/04/2027

Test	g/210L	Time
DIAG	Pass	4:24pm
AIR BLK	.00	4:25pm
ACCY CHK	.07	4:26pm
AIR BLK	.00	4:27pm
SUB TEST	.00	4:27pm
AIR BLK	.00	4:28pm
SUB TEST	.00	4:30pm
AIR BLK	.00	4:31pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

WAKE COUNTY BAT MOBILE UNIT 13 910

Serial Number: 008898 Test Record Number: 1978
Test Date: 04/17/2025 Test Time: 4:34pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	4:34pm
FLO	Pass	4:34pm
FC	Pass	4:34pm

Temperature Tests

Test	Status	Time
FC1	Pass	4:34pm
SRC	Pass	4:34pm
DET	Pass	4:34pm
BAR	Pass	4:34pm
BT	Pass	4:34pm

Blank Tests

Test	Status	Time
AIR	Pass	4:35pm


Printer Tests

Test	Status	Time
PRNT	Pass	4:35pm

CRC Tests

Test	Status	Time
COMP	Pass	4:35pm
CAL	Pass	4:35pm

Preventive Maintenance
Status: Pass



Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Wake Instrument Location BAT Mobile Unit 13

Instrument Serial No. 008939

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 17 day of April, 2005 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Timothy B. White
Signature of Certifying Official

307699
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

WAKE COUNTY BAT MOBILE UNIT 13 910

Serial Number: 008939
Test Date: 04/17/2025

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE

Analyst's Name: Whitehurst, Timothy B
Permit Number: 0030-7699
Effective:
03/01/2025-03/01/2027

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test


Lot Number: AG506302
Exp Date: 03/04/2027

Test	g/210L	Time
DIAG	Pass	3:44pm
AIR BLK	.00	3:45pm
ACCY CHK	.07	3:46pm
AIR BLK	.00	3:47pm
SUB TEST	.00	3:47pm
AIR BLK	.00	3:48pm
SUB TEST	.00	3:50pm
AIR BLK	.00	3:51pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

WAKE COUNTY BAT MOBILE UNIT 13 910

Serial Number: 008939 Test Record Number: 1846
Test Date: 04/17/2025 Test Time: 3:51pm EDT

System Check: Passed

Baseline Tests

Test	Status	Time
IR	Pass	3:51pm
PLO	Pass	3:52pm
FC	Pass	3:52pm

Temperature Tests

Test	Status	Time
FC1	Pass	3:52pm
SRC	Pass	3:52pm
DET	Pass	3:52pm
BAR	Pass	3:52pm
BT	Pass	3:52pm

Blank Tests

Test	Status	Time
AIR	Pass	3:52pm

Printer Tests

Test	Status	Time
PRNT	Pass	3:52pm

CRC Tests

Test	Status	Time
COMP	Pass	3:53pm
CAL	Pass	3:53pm

Preventive Maintenance
Status: Pass



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County Washington Instrument Location Washington Co. S.O.
Instrument Serial No. 008829 120 Adams St., Plymouth, N.C.

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 28th day of April, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

377722
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

WASHINGTON COUNTY SHERIFF'S OFFICE 930

Serial Number: 008829

Test Date: 04/28/2025

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Gray, Kelly D

Permit Number: 0037-7722

Effective:

02/01/2025-02/01/2027

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG400303

Exp Date: 01/03/2026

Test	g/210L	Time
DIAG	Pass	11:13am
AIR BLK	.00	11:14am
ACCY CHK	.07	11:15am
AIR BLK	.00	11:16am
SUB TEST	.00	11:17am
AIR BLK	.00	11:18am
SUB TEST	.00	11:20am
AIR BLK	.00	11:20am

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

Intox EC/IR-II: Preventive Maintenance

WASHINGTON COUNTY SHERIFF'S OFFICE 930

Serial Number: 008829 Test Record Number: 1266
Test Date: 04/28/2025 Test Time: 11:22am EDT

System Check: Passed

Baseline Tests

Test	Status	Time
IR	Pass	11:22am
FLO	Pass	11:22am
FC	Pass	11:22am

Temperature Tests

Test	Status	Time
FC1	Pass	11:22am
SRC	Pass	11:22am
DET	Pass	11:22am
BAR	Pass	11:22am
BT	Pass	11:22am

Blank Tests

Test	Status	Time
AIR	Pass	11:23am


Printer Tests

Test	Status	Time
PRNT	Pass	11:23am

CRC Tests

Test	Status	Time
COMP	Pass	11:23am
CAL	Pass	11:23am

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County WATAUGA Instrument Location BOONE PD

Instrument Serial No. 008716 BOONE NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 17 day of APRIL, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

274970
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

WATAUGA COUNTY BOONE PD 940

Serial Number: 008716
Test Date: 04/17/2025

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: Fleming, Tina S
Permit Number: 0027-4970
Effective:
10/01/2023-10/01/2025

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG405102
Exp Date: 02/20/2026


Test	g/210L	Time
DIAG	Pass	12:17pm
AIR BLK	.00	12:17pm
ACCY CHK	.07	12:18pm
AIR BLK	.00	12:19pm
SUB TEST	.00	12:20pm
AIR BLK	.00	12:21pm
SUB TEST	.00	12:22pm
AIR BLK	.00	12:23pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

WATAUGA COUNTY BOONE PD 940

Serial Number: 008716 Test Record Number: 3300
Test Date: 04/17/2025 Test Time: 12:24pm EDT

System Check: Passed

Baseline Tests

Test	Status	Time
IR	Pass	12:24pm
FLO	Pass	12:24pm
FC	Pass	12:25pm

Temperature Tests

Test	Status	Time
FC1	Pass	12:25pm
SRC	Pass	12:25pm
DET	Pass	12:25pm
BAR	Pass	12:25pm
BT	Pass	12:25pm

Blank Tests

Test	Status	Time
AIR	Pass	12:25pm

Printer Tests

Test	Status	Time
PRNT	Pass	12:25pm

CRC Tests

Test	Status	Time
COMP	Pass	12:25pm
CAL	Pass	12:25pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Wayne Instrument Location Wayne (a Detention Center
207 E. Chestnut St., Goldsboro,
NC

Instrument Serial No. 008649

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 22nd day of April, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

377722
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

WAYNE COUNTY WAYNE CO DETENTION 950

Serial Number: 008649
Test Date: 04/22/2025

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE

Analyst's Name: Gray, Kelly D
Permit Number: 0037-7722
Effective:
02/01/2025-02/01/2027

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG400303
Exp Date: 01/03/2026

Test	g/210L	Time
DIAG	Pass	11:19am
AIR BLK	.00	11:19am
ACCY CHK	.08	11:20am
AIR BLK	.00	11:21am
SUB TEST	.00	11:22am
AIR BLK	.00	11:23am
SUB TEST	.00	11:24am
AIR BLK	.00	11:25am

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

WAYNE COUNTY WAYNE CO DETENTION 950

Serial Number: 008649 Test Record Number: 6190
Test Date: 04/22/2025 Test Time: 11:26am EDT

System Check: Passed

Baseline Tests

Test	Status	Time
IR	Pass	11:26am
FLO	Pass	11:26am
FC	Pass	11:26am

Temperature Tests

Test	Status	Time
FC1	Pass	11:27am
SRC	Pass	11:27am
DET	Pass	11:27am
BAR	Pass	11:27am
BT	Pass	11:27am

Blank Tests

Test	Status	Time
AIR	Pass	11:27am


Printer Tests

Test	Status	Time
PRNT	Pass	11:27am

CRC Tests

Test	Status	Time
COMP	Pass	11:27am
CAL	Pass	11:27am

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Wayne Instrument Location Wayne Co. Detention Center
Instrument Serial No. 008879 207 E. Chestnut St. Goldsboro,
NC.

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 2nd day of April, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

377722
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

WAYNE COUNTY WAYNE CO DETENTION 950

Serial Number: 008879
Test Date: 04/22/2025

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: Gray, Kelly D
Permit Number: 0037-7722
Effective:
02/01/2025-02/01/2027

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG405101
Exp Date: 02/20/2026

Test	g/210L	Time
DIAG	Pass	11:19am
AIR BLK	.00	11:20am
ACCY CHK	.08	11:21am
AIR BLK	.00	11:22am
SUB TEST	.00	11:23am
AIR BLK	.00	11:24am
SUB TEST	.00	11:25am
AIR BLK	.00	11:26am

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

Intox EC/IR-II: Preventive Maintenance

WAYNE COUNTY WAYNE CO DETENTION 950

Serial Number: 008879 Test Record Number: 2757
Test Date: 04/22/2025 Test Time: 11:27am EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	11:27am
FLO	Pass	11:27am
FC	Pass	11:27am

Temperature Tests

Test	Status	Time
FC1	Pass	11:27am
SRC	Pass	11:27am
DET	Pass	11:27am
BAR	Pass	11:27am
BT	Pass	11:27am

Blank Tests

Test	Status	Time
AIR	Pass	11:28am


Printer Tests

Test	Status	Time
PRNT	Pass	11:28am

CRC Tests

Test	Status	Time
COMP	Pass	11:28am
CAL	Pass	11:28am

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County Yancey Instrument Location Yancey County Jail
Instrument Serial No. 009655 Burnsville, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 17 day of April, 2025 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

244987
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

YANCEY COUNTY YANCEY COUNTY JAIL 990

Serial Number: 008653
Test Date: 04/17/2025

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE

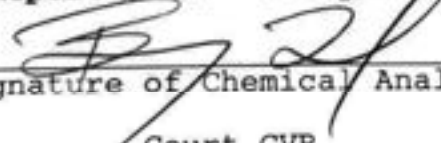
Analyst's Name: Loftis, Benjamin C
Permit Number: 0024-4987
Effective:
03/01/2025-03/01/2027

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test


Lot Number: AG503001
Exp Date: 01/30/2027

Test	g/210L	Time
DIAG	Pass	2:02pm
AIR BLK	.00	2:03pm
ACCY CHK	.08	2:03pm
AIR BLK	.00	2:04pm
SUB TEST	.00	2:05pm
AIR BLK	.00	2:06pm
SUB TEST	.00	2:07pm
AIR BLK	.00	2:08pm

Reported AC: .00 g/210D



Signature of Chemical Analyst
Court CVR



Analyst

Intox EC/IR-II: Preventive Maintenance

YANCEY COUNTY YANCEY COUNTY JAIL 990

Serial Number: 008653 Test Record Number: 1848
Test Date: 04/17/2025 Test Time: 2:10pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	2:10pm
FLO	Pass	2:10pm
FC	Pass	2:10pm

Temperature Tests

Test	Status	Time
FC1	Pass	2:11pm
SRC	Pass	2:11pm
DET	Pass	2:11pm
BAR	Pass	2:11pm
BT	Pass	2:11pm

Blank Tests

Test	Status	Time
AIR	Pass	2:11pm

Printer Tests

Test	Status	Time
PRNT	Pass	2:11pm

CRC Tests

Test	Status	Time
COMP	Pass	2:11pm
CAL	Pass	2:11pm

Preventive Maintenance
Status: Pass



Analyst