

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II**

County Pender Instrument Location BAT Mobile unit 6

Instrument Serial No. 008898 Wildlife

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 23 day of May, 2009 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



K. C. [Signature]
Signature of Certifying Official

601
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Preventive Maintenance

PENDER COUNTY BAT MOBILE UNIT 6 700

Serial Number: 008898 Test Record Number: 178
Test Date: 05/23/2009 Test Time: 2:00pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	2:01pm
FLO	Pass	2:01pm
FC	Pass	2:01pm

Temperature Tests

Test	Status	Time
FC1	Pass	2:01pm
SRC	Pass	2:01pm
DET	Pass	2:01pm
BAR	Pass	2:01pm
BT	Pass	2:01pm

Blank Tests

Test	Status	Time
AIR	Pass	2:02pm


Printer Tests

Test	Status	Time
PRNT	Pass	2:02pm

CRC Tests

Test	Status	Time
COMP	Pass	2:02pm
CAL	Pass	2:02pm

Preventive Maintenance
Status: Pass

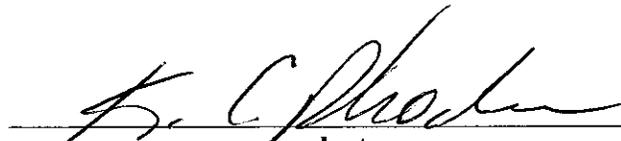

Analyst

Intox EC/IR-II: Subject Test

PENDER COUNTY BAT MOBILE UNIT 6 700

Serial Number: 008898
Test Date: 05/23/2009

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: RHODES, KENNETH C
Permit Number: 5329E
Effective:
02/01/2008-02/01/2010

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG814002
Exp Date: 05/19/2010

Test	g/210L	Time
DIAG	Pass	1:53pm
AIR BLK	.00	1:54pm
ACCY CHK	.07	1:54pm
AIR BLK	.00	1:55pm
SUB TEST	.00	1:56pm
AIR BLK	.00	1:56pm
SUB TEST	.00	1:58pm
AIR BLK	.00	1:59pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR.



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH


**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II**

County Stanly Instrument Location Stanly Co. S.D.
Instrument Serial No. 008824 201 S. Second St., Albemarle
704-986-3734

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 29 day of May, 2009 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Bobby E. Willis
Signature of Certifying Official

557
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

STANLY COUNTY STANLY COUNTY SD 830

Serial Number: 008824
Test Date: 05/29/2009

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE

Analyst's Name: WILLIS, BOBBY D
Permit Number: 08010E
Effective:
12/01/2007-12/01/2009

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG814101
Exp Date: 05/20/2010

Test	g/210L	Time
DIAG	Pass	9:58am
AIR BLK	.00	10:00am
ACCY CHK	.07	10:00am
AIR BLK	.00	10:01am
SUB TEST	.00	10:02am
AIR BLK	.00	10:02am
SUB TEST	.00	10:04am
AIR BLK	.00	10:05am

Reported AC: .00 g/210L

Bobby D. Willis
Signature of Chemical Analyst

Court CVR.

Bobby D. Willis
Analyst

Intox EC/IR-II: Preventive Maintenance

STANLY COUNTY STANLY COUNTY SD 830

Serial Number: 008824 Test Record Number: 242
Test Date: 05/29/2009 Test Time: 10:06am EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	10:07am
FLO	Pass	10:07am
FC	Pass	10:07am

Temperature Tests

Test	Status	Time
FC1	Pass	10:07am
SRC	Pass	10:07am
DET	Pass	10:07am
BAR	Pass	10:07am
BT	Pass	10:07am

Blank Tests

Test	Status	Time
AIR	Pass	10:08am


Printer Tests

Test	Status	Time
PRNT	Pass	10:08am

CRC Tests

Test	Status	Time
COMP	Pass	10:08am
CAL	Pass	10:08am

Preventive Maintenance
Status: Pass

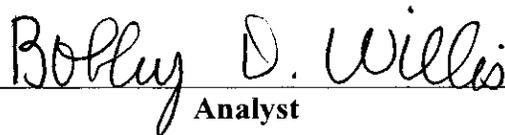
Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II**


County SCOTLAND Instrument Location LAURINBURG,

Instrument Serial No. 005834 Police Dept.

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 20 day of MAY, 2007 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Paul T. [Signature]
Signature of Certifying Official

578
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

SCOTLAND LAURINBURG PD 820

Serial Number: 008834
Test Date: 05/20/2009

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: SIMMONS, PAUL T
Permit Number: 08619E
Effective:
12/01/2007-12/01/2009

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test


Lot Number: AG814002
Exp Date: 05/19/2010

Test	g/210L	Time
DIAG	Pass	2:01pm
AIR BLK	.00	2:02pm
ACCY CHK	.07	2:03pm
AIR BLK	.00	2:04pm
SUB TEST	.00	2:04pm
AIR BLK	.00	2:05pm
SUB TEST	.00	2:07pm
AIR BLK	.00	2:07pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

Intox EC/IR-II: Preventive Maintenance

SCOTLAND LAURINBURG PD 820

Serial Number: 008834 Test Record Number: 152
Test Date: 05/20/2009 Test Time: 2:18pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	2:19pm
FLO	Pass	2:19pm
FC	Pass	2:19pm

Temperature Tests

Test	Status	Time
FC1	Pass	2:19pm
SRC	Pass	2:19pm
DET	Pass	2:19pm
BAR	Pass	2:19pm
BT	Pass	2:19pm

Blank Tests

Test	Status	Time
AIR	Pass	2:20pm

Printer Tests

Test	Status	Time
PRNT	Pass	2:20pm

CRC Tests

Test	Status	Time
COMP	Pass	2:20pm
CAL	Pass	2:20pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II**

County Robeson Instrument Location PEMBROKE
Instrument Serial No. 008837 Police Dept.

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 13 day of MAY, 2009 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Paul T. [Signature]

Signature of Certifying Official

578

Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

. Intox EC/IR-II: Subject Test

ROBESON PEMBROKE, PD. 770

Serial Number: 008837
Test Date: 05/13/2009

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: SIMMONS, PAUL T

Permit Number: 08619E

Effective:

12/01/2007-12/01/2009

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG814002

Exp Date: 05/19/2010

Test	g/210L	Time
DIAG	Pass	12:10pm
AIR BLK	.00	12:11pm
ACCY CHK	.07	12:12pm
AIR BLK	.00	12:12pm
SUB TEST	.00	12:13pm
AIR BLK	.00	12:14pm
SUB TEST	.00	12:15pm
AIR BLK	.00	12:16pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR.



Analyst

Intox EC/IR-II: Preventive Maintenance

ROBESON PEMBROKE, PD. 770

Serial Number: 008837 Test Record Number: 97
Test Date: 05/13/2009 Test Time: 12:18pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	12:19pm
FLO	Pass	12:19pm
FC	Pass	12:19pm

Temperature Tests

Test	Status	Time
FC1	Pass	12:19pm
SRC	Pass	12:19pm
DET	Pass	12:19pm
BAR	Pass	12:19pm
BT	Pass	12:19pm

Blank Tests

Test	Status	Time
AIR	Pass	12:19pm

Printer Tests

Test	Status	Time
PRNT	Pass	12:20pm

CRC Tests

Test	Status	Time
COMP	Pass	12:20pm
CAL	Pass	12:20pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II**


County Stanly Instrument Location Stanly Co. S.D.
Instrument Serial No. 008842 2015. Second St. Albemarle
704-986-3734

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

RECEIVED
JUN - 2 2009
FTA BRANCH

I certify that on the 29 day of May, 20 09 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Bobby C. Willey
Signature of Certifying Official

557
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

STANLY COUNTY STANLY COUNTY SD 830

Serial Number: 008842
Test Date: 05/29/2009

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE

Analyst's Name: WILLIS, BOBBY D
Permit Number: 08010E
Effective:
12/01/2007-12/01/2009

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG901901
Exp Date: 01/19/2011

Test	g/210L	Time
DIAG	Pass	10:33am
AIR BLK	.00	10:34am
ACCY CHK	.08	10:35am
AIR BLK	.00	10:36am
SUB TEST	.00	10:36am
AIR BLK	.00	10:37am
SUB TEST	.00	10:39am
AIR BLK	.00	10:39am

Reported AC: .00 g/210L

Bobby D. Willis
Signature of Chemical Analyst

Court CVR

Bobby D. Willis
Analyst

Intox EC/IR-II: Preventive Maintenance

STANLY COUNTY STANLY COUNTY SD 830

Serial Number: 008842 Test Record Number: 359
Test Date: 05/29/2009 Test Time: 10:41am EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	10:41am
FLO	Pass	10:41am
FC	Pass	10:41am

Temperature Tests

Test	Status	Time
FC1	Pass	10:41am
SRC	Pass	10:41am
DET	Pass	10:41am
BAR	Pass	10:41am
BT	Pass	10:41am

Blank Tests

Test	Status	Time
AIR	Pass	10:42am


Printer Tests

Test	Status	Time
PRNT	Pass	10:42am

CRC Tests

Test	Status	Time
COMP	Pass	10:42am
CAL	Pass	10:42am

Preventive Maintenance
Status: Pass

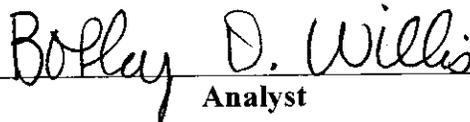
Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II**


County HOKE Instrument Location HOKE COUNTY

Instrument Serial No. 008852 DETENTION CENTER

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 21 day of MAY, 2009 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Paul T. Sumner
Signature of Certifying Official

578
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

HOKE COUNTY DETENTION CENTER 460

Serial Number: 008852
Test Date: 05/21/2009

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE

Analyst's Name: SIMMONS, PAUL T
Permit Number: 08619E
Effective:
12/01/2007-12/01/2009

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG814002
Exp Date: 05/19/2010

Test	g/210L	Time
DIAG	Pass	10:24am
AIR BLK	.00	10:25am
ACCY CHK	.07	10:26am
AIR BLK	.00	10:27am
SUB TEST	.00	10:27am
AIR BLK	.00	10:28am
SUB TEST	.00	10:30am
AIR BLK	.00	10:31am

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

Intox EC/IR-II: Preventive Maintenance

HOKE COUNTY DETENTION CENTER 460

Serial Number: 008852 Test Record Number: 110
Test Date: 05/21/2009 Test Time: 10:32am EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	10:32am
FLO	Pass	10:32am
FC	Pass	10:32am

Temperature Tests

Test	Status	Time
FC1	Pass	10:33am
SRC	Pass	10:33am
DET	Pass	10:33am
BAR	Pass	10:33am
BT	Pass	10:33am

Blank Tests

Test	Status	Time
AIR	Pass	10:33am


Printer Tests

Test	Status	Time
PRNT	Pass	10:33am

CRC Tests

Test	Status	Time
COMP	Pass	10:33am
CAL	Pass	10:33am

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II**


County Hoke Instrument Location Hoke County

Instrument Serial No. 008855 Detention Center

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 28 day of MAY, 2009 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Paul T. [Signature]

Signature of Certifying Official

578

Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

HOKE COUNTY DETENTION CENTER 460

Serial Number: 008855
Test Date: 05/28/2009

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: SIMMONS, PAUL T
Permit Number: 08619E
Effective:
12/01/2007-12/01/2009

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test


Lot Number: AG814101
Exp Date: 05/20/2010

Test	g/210L	Time
DIAG	Pass	10:33am
AIR BLK	.00	10:34am
ACCY CHK	.07	10:34am
AIR BLK	.00	10:35am
SUB TEST	.00	10:36am
AIR BLK	.00	10:37am
SUB TEST	.00	10:38am
AIR BLK	.00	10:39am

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

Intox EC/IR-II: Preventive Maintenance

HOKE COUNTY DETENTION CENTER 460

Serial Number: 008855 Test Record Number: 264
Test Date: 05/28/2009 Test Time: 10:40am EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	10:40am
FLO	Pass	10:40am
FC	Pass	10:40am

Temperature Tests

Test	Status	Time
FC1	Pass	10:41am
SRC	Pass	10:41am
DET	Pass	10:41am
BAR	Pass	10:41am
BT	Pass	10:41am

Blank Tests

Test	Status	Time
AIR	Pass	10:41am

Printer Tests

Test	Status	Time
PRNT	Pass	10:41am

CRC Tests

Test	Status	Time
COMP	Pass	10:41am
CAL	Pass	10:41am

Preventive Maintenance
Status: *Pass*



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II**


County Nash Instrument Location BAT Mobile Unit 6

Instrument Serial No. 008669

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 30 day of MAY, 2009 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

601
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Preventive Maintenance

NASH COUNTY BAT MOBILE UNIT 6 630

Serial Number: 008869 Test Record Number: 155
Test Date: 05/30/2009 Test Time: 8:57pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	8:57pm
FLO	Pass	8:57pm
FC	Pass	8:57pm

Temperature Tests

Test	Status	Time
FC1	Pass	8:57pm
SRC	Pass	8:57pm
DET	Pass	8:57pm
BAR	Pass	8:57pm
BT	Pass	8:57pm

Blank Tests

Test	Status	Time
AIR	Pass	8:58pm

Printer Tests

Test	Status	Time
PRNT	Pass	8:58pm

CRC Tests

Test	Status	Time
COMP	Pass	8:58pm
CAL	Pass	8:58pm

Preventive Maintenance
Status: Pass



Analyst

Intox EC/IR-II: Subject Test

NASH COUNTY BAT MOBILE UNIT 6 630

Serial Number: 008869
Test Date: 05/30/2009

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: RHODES, KENNETH C

Permit Number: 5329E

Effective:

02/01/2008-02/01/2010

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG814002


Exp Date: 05/19/2010

Test	g/210L	Time
DIAG	Pass	8:49pm
AIR BLK	.00	8:50pm
ACCY CHK	.07	8:51pm
AIR BLK	.00	8:52pm
SUB TEST	.00	8:52pm
AIR BLK	.00	8:53pm
SUB TEST	.00	8:55pm
AIR BLK	.00	8:56pm

Reported AC: .00 g/210L

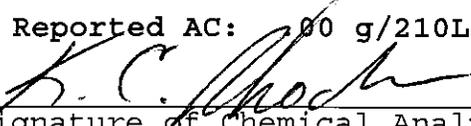
Signature of Chemical Analyst

Court CVR

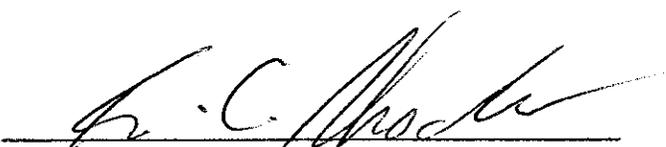
Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II**


County Nash Instrument Location Pat Mobile Unit 6

Instrument Serial No. 008898

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 30 day of MAY, 2009 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



A. C. Proctor
Signature of Certifying Official

601
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Preventive Maintenance

NASH COUNTY BAT MOBILE UNIT 6 630

Serial Number: 008898 Test Record Number: 187
Test Date: 05/30/2009 Test Time: 10:36pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	10:36pm
FLO	Pass	10:36pm
FC	Pass	10:36pm

Temperature Tests

Test	Status	Time
FC1	Pass	10:36pm
SRC	Pass	10:36pm
DET	Pass	10:36pm
BAR	Pass	10:36pm
BT	Pass	10:36pm

Blank Tests

Test	Status	Time
AIR	Pass	10:37pm

Printer Tests

Test	Status	Time
PRNT	Pass	10:37pm

CRC Tests

Test	Status	Time
COMP	Pass	10:37pm
CAL	Pass	10:37pm

Preventive Maintenance
Status: Pass



Analyst

Intox EC/IR-II: Subject Test

NASH COUNTY BAT MOBILE UNIT 6 630

Serial Number: 008898
Test Date: 05/30/2009

Citation Number: M0000000-0
Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: RHODES, KENNETH C

Permit Number: 5329E

Effective:

02/01/2008-02/01/2010

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG814002

Exp Date: 05/19/2010

Test	g/210L	Time
DIAG	Pass	10:28pm
AIR BLK	.00	10:29pm
ACCY CHK	.07	10:30pm
AIR BLK	.00	10:31pm
SUB TEST	.00	10:31pm
AIR BLK	.00	10:32pm
SUB TEST	.00	10:34pm
AIR BLK	.00	10:34pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II**

County CRAVEN Instrument Location BAT mobile Unit 6
Instrument Serial No. 008898 5HP

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 22 day of May, 2009 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature] Signature of Certifying Official 601 Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Preventive Maintenance

CRAVEN COUNTY BAT MOBILE UNIT 6 240

Serial Number: 008898 Test Record Number: 174
Test Date: 05/22/2009 Test Time: 11:36pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	11:37pm
FLO	Pass	11:37pm
FC	Pass	11:37pm

Temperature Tests

Test	Status	Time
FC1	Pass	11:37pm
SRC	Pass	11:37pm
DET	Pass	11:37pm
BAR	Pass	11:37pm
BT	Pass	11:37pm

Blank Tests

Test	Status	Time
AIR	Pass	11:38pm


Printer Tests

Test	Status	Time
PRNT	Pass	11:38pm

CRC Tests

Test	Status	Time
COMP	Pass	11:38pm
CAL	Pass	11:38pm

Preventive Maintenance
Status: Pass

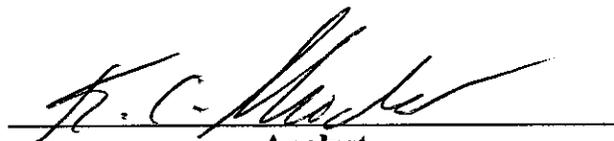

Analyst

***Intox EC/IR-II: Subject Test**

CRAVEN COUNTY BAT MOBILE UNIT 6 240

Serial Number: 008898
Test Date: 05/22/2009

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: RHODES, KENNETH C
Permit Number: 5329E
Effective:
02/01/2008-02/01/2010

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG814002
Exp Date: 05/19/2010

Test	g/210L	Time
DIAG	Pass	11:27pm
AIR BLK	.00	11:28pm
ACCY CHK	.07	11:28pm
AIR BLK	.00	11:29pm
SUB TEST	.00	11:30pm
AIR BLK	.00	11:31pm
SUB TEST	.00	11:34pm
AIR BLK	.00	11:35pm

Reported AC: .00 g/210L

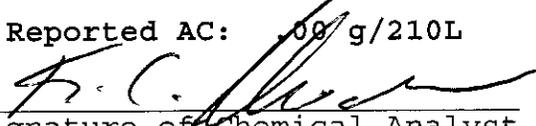

Signature of Chemical Analyst

Court CVR



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II**


County Rowan Instrument Location BAT mobile unit 6

Instrument Serial No. 000898

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 25 day of MAY, 2009 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

601
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Preventive Maintenance

ROWAN COUNTY BAT MOBILE UNIT 6 790

Serial Number: 008898 Test Record Number: 183
Test Date: 05/25/2009 Test Time: 11:50am EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	11:51am
FLO	Pass	11:51am
FC	Pass	11:51am

Temperature Tests

Test	Status	Time
FC1	Pass	11:51am
SRC	Pass	11:51am
DET	Pass	11:51am
BAR	Pass	11:51am
BT	Pass	11:51am

Blank Tests

Test	Status	Time
AIR	Pass	11:51am

Printer Tests

Test	Status	Time
PRNT	Pass	11:51am

CRC Tests

Test	Status	Time
COMP	Pass	11:52am
CAL	Pass	11:52am

Preventive Maintenance
Status: Pass



Analyst

Intox EC/IR-II: Subject Test

ROWAN COUNTY BAT MOBILE UNIT 6 790

Serial Number: 008898

Test Date: 05/25/2009

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: RHODES, KENNETH C

Permit Number: 5329E

Effective:

02/01/2008-02/01/2010

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG814002

Exp Date: 05/19/2010

Test	g/210L	Time
DIAG	Pass	11:42am
AIR BLK	.00	11:43am
ACCY CHK	.07	11:43am
AIR BLK	.00	11:44am
SUB TEST	.00	11:45am
AIR BLK	.00	11:46am
SUB TEST	.00	11:48am
AIR BLK	.00	11:49am

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II**


County McDowell Instrument Location McDowell Co. Jail

Instrument Serial No. 008892 Marion, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 4 day of May, 2009 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

649
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

MCDOWELL COUNTY JAIL 580

Serial Number: 008892
Test Date: 05/04/2009

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE

Analyst's Name: BURNETTE, ANTHONY J
Permit Number: 11304E
Effective:
12/01/2007-12/01/2009

Officer's Name: NONE,
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG816302
Exp Date: 06/11/2010

Test	g/210L	Time
DIAG	Pass	1:56pm
AIR BLK	.00	1:57pm
ACCY CHK	.07	1:58pm
AIR BLK	.00	1:58pm
SUB TEST	.00	1:59pm
AIR BLK	.00	2:00pm
SUB TEST	.00	2:01pm
AIR BLK	.00	2:02pm

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR


Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

MCDOWELL COUNTY JAIL 580

Serial Number: 008892 Test Record Number: 120
Test Date: 05/04/2009 Test Time: 2:03pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	2:03pm
FLO	Pass	2:03pm
FC	Pass	2:03pm

Temperature Tests

Test	Status	Time
FC1	Pass	2:03pm
SRC	Pass	2:03pm
DET	Pass	2:03pm
BAR	Pass	2:03pm
BT	Pass	2:03pm

Blank Tests

Test	Status	Time
AIR	Pass	2:04pm


Printer Tests

Test	Status	Time
PRNT	Pass	2:04pm

CRC Tests

Test	Status	Time
COMP	Pass	2:04pm
CAL	Pass	2:04pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II**


County McDowell Instrument Location McDowell Co. Jail

Instrument Serial No. 008888 Marion, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 4 day of May, 2009 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

649
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

MCDOWELL COUNTY JAIL 580

Serial Number: 008888
Test Date: 05/04/2009

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: BURNETTE, ANTHONY J

Permit Number: 11304E

Effective:

12/01/2007-12/01/2009

Officer's Name: NONE,

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG816302

Exp Date: 06/11/2010

Test	g/210L	Time
DIAG	Pass	1:51pm
AIR BLK	.00	1:52pm
ACCY CHK	.07	1:52pm
AIR BLK	.00	1:53pm
SUB TEST	.00	1:54pm
AIR BLK	.00	1:55pm
SUB TEST	.00	1:56pm
AIR BLK	.00	1:57pm

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR


Analyst

Intox EC/IR-II: Preventive Maintenance

MCDOWELL COUNTY JAIL 580

Serial Number: 008888 Test Record Number: 147
Test Date: 05/04/2009 Test Time: 1:59pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	2:00pm
FLO	Pass	2:00pm
FC	Pass	2:00pm

Temperature Tests

Test	Status	Time
FC1	Pass	2:00pm
SRC	Pass	2:00pm
DET	Pass	2:00pm
BAR	Pass	2:00pm
BT	Pass	2:00pm

Blank Tests

Test	Status	Time
AIR	Pass	2:01pm


Printer Tests

Test	Status	Time
PRNT	Pass	2:01pm

CRC Tests

Test	Status	Time
COMP	Pass	2:01pm
CAL	Pass	2:01pm

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH


**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II**

County Avery Instrument Location Banner Elk P.D.
Instrument Serial No. 008724 Banner Elk, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 22 day of May, 2009 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

649
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

AVERY COUNTY BANNER ELK PD 050

Serial Number: 008724
Test Date: 05/22/2009

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE

Analyst's Name: BURNETTE, ANTHONY J
Permit Number: 11304E
Effective:
12/01/2007-12/01/2009

Officer's Name: NONE,
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG816302
Exp Date: 06/11/2010

Test	g/210L	Time
DIAG	Pass	6:01pm
AIR BLK	.00	6:02pm
ACCY CHK	.08	6:03pm
AIR BLK	.00	6:03pm
SUB TEST	.00	6:04pm
AIR BLK	.00	6:05pm
SUB TEST	.00	6:06pm
AIR BLK	.00	6:07pm

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR


Analyst

Intox EC/IR-II: Preventive Maintenance

AVERY COUNTY BANNER ELK PD 050

Serial Number: 008724 Test Record Number: 113
Test Date: 05/22/2009 Test Time: 6:09pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	6:09pm
FLO	Pass	6:09pm
FC	Pass	6:09pm

Temperature Tests

Test	Status	Time
FC1	Pass	6:09pm
SRC	Pass	6:09pm
DET	Pass	6:09pm
BAR	Pass	6:09pm
BT	Pass	6:09pm

Blank Tests

Test	Status	Time
AIR	Pass	6:10pm

Printer Tests

Test	Status	Time
PRNT	Pass	6:10pm

CRC Tests

Test	Status	Time
COMP	Pass	6:10pm
CAL	Pass	6:10pm

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH


**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II**

County Mitchell Instrument Location Spruce Pine PD
Instrument Serial No. 008726 Spruce Pine, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 26 day of May, 2009 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

649
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

MITCHELL COUNTY SPRUCE PINE PD 600

Serial Number: 008726
Test Date: 05/26/2009

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE

Analyst's Name: BURNETTE, ANTHONY J
Permit Number: 11304E
Effective:
12/01/2007-12/01/2009

Officer's Name: NONE,
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test


Lot Number: AG722702
Exp Date: 08/14/2009

Test	g/210L	Time
DIAG	Pass	2:58pm
AIR BLK	.00	2:59pm
ACCY CHK	.07	2:59pm
AIR BLK	.00	3:00pm
SUB TEST	.00	3:01pm
AIR BLK	.00	3:01pm
SUB TEST	.00	3:03pm
AIR BLK	.00	3:04pm

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR



Analyst

Intox EC/IR-II: Preventive Maintenance

MITCHELL COUNTY SPRUCE PINE PD 600

Serial Number: 008726 Test Record Number: 179
Test Date: 05/26/2009 Test Time: 3:06pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	3:06pm
FLO	Pass	3:06pm
FC	Pass	3:06pm

Temperature Tests

Test	Status	Time
FC1	Pass	3:07pm
SRC	Pass	3:07pm
DET	Pass	3:07pm
BAR	Pass	3:07pm
BT	Pass	3:07pm

Blank Tests

Test	Status	Time
AIR	Pass	3:07pm


Printer Tests

Test	Status	Time
PRNT	Pass	3:07pm

CRC Tests

Test	Status	Time
COMP	Pass	3:07pm
CAL	Pass	3:07pm

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II**


County Burke Instrument Location Margaretton DPS

Instrument Serial No. 008904 Margaretton, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 21 day of May, 2009 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

649
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

BURKE COUNTY MORGANTON DPS 110

Serial Number: 008904
Test Date: 05/21/2009

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE

Analyst's Name: BURNETTE, ANTHONY J
Permit Number: 11304E
Effective:
12/01/2007-12/01/2009

Officer's Name: NONE,
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG723301
Exp Date: 08/20/2009

Test	g/210L	Time
DIAG	Pass	11:22am
AIR BLK	.00	11:23am
ACCY CHK	.07	11:24am
AIR BLK	.00	11:25am
SUB TEST	.00	11:25am
AIR BLK	.00	11:26am
SUB TEST	.00	11:27am
AIR BLK	.00	11:28am

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR


Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

BURKE COUNTY MORGANTON DPS 110

Serial Number: 008904 Test Record Number: 185
Test Date: 05/21/2009 Test Time: 11:29am EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	11:30am
FLO	Pass	11:30am
FC	Pass	11:30am

Temperature Tests

Test	Status	Time
FC1	Pass	11:30am
SRC	Pass	11:30am
DET	Pass	11:30am
BAR	Pass	11:30am
BT	Pass	11:30am

Blank Tests

Test	Status	Time
AIR	Pass	11:31am

Printer Tests

Test	Status	Time
PRNT	Pass	11:31am

CRC Tests

Test	Status	Time
COMP	Pass	11:31am
CAL	Pass	11:31am

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II**


County Burke Instrument Location Morganton DPS

Instrument Serial No. 009831 Morganton, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 21 day of May, 2009 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

649
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

BURKE COUNTY MORGANTON DPS 110

Serial Number: 008831

Test Date: 05/21/2009

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: BURNETTE, ANTHONY J

Permit Number: 11304E

Effective:

12/01/2007-12/01/2009

Officer's Name: NONE,

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG809301

Exp Date: 04/02/2010

Test	g/210L	Time
DIAG	Pass	11:22am
AIR BLK	.00	11:22am
ACCY CHK	.08	11:23am
AIR BLK	.00	11:24am
SUB TEST	.00	11:25am
AIR BLK	.00	11:26am
SUB TEST	.00	11:27am
AIR BLK	.00	11:28am

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR.



Analyst

Intox EC/IR-II: Preventive Maintenance

BURKE COUNTY MORGANTON DPS 110

Serial Number: 008831 Test Record Number: 484
Test Date: 05/21/2009 Test Time: 11:29am EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	11:30am
FLO	Pass	11:30am
FC	Pass	11:30am

Temperature Tests

Test	Status	Time
FC1	Pass	11:30am
SRC	Pass	11:30am
DET	Pass	11:30am
BAR	Pass	11:30am
BT	Pass	11:30am

Blank Tests

Test	Status	Time
AIR	Pass	11:30am

Printer Tests

Test	Status	Time
PRNT	Pass	11:30am

CRC Tests

Test	Status	Time
COMP	Pass	11:31am
CAL	Pass	11:31am

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II**

County Watauga

Instrument Location Watauga Co Jail

Instrument Serial No. 009716

Boone, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 20 day of May, 2009 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

649
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

WATAUGA COUNTY WATAUGA JAIL 940

Serial Number: 008716
Test Date: 05/20/2009

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE

Analyst's Name: BURNETTE, ANTHONY J
Permit Number: 11304E
Effective:
12/01/2007-12/01/2009

Officer's Name: NONE,
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG722802
Exp Date: 08/15/2009

Test	g/210L	Time
DIAG	Pass	11:20am
AIR BLK	.00	11:20am
ACCY CHK	.07	11:21am
AIR BLK	.00	11:22am
SUB TEST	.00	11:22am
AIR BLK	.00	11:23am
SUB TEST	.00	11:25am
AIR BLK	.00	11:26am

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR


Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

WATAUGA COUNTY WATAUGA JAIL 940

Serial Number: 008716 Test Record Number: 437
Test Date: 05/20/2009 Test Time: 11:27am EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	11:28am
FLO	Pass	11:28am
FC	Pass	11:28am

Temperature Tests

Test	Status	Time
FC1	Pass	11:28am
SRC	Pass	11:28am
DET	Pass	11:28am
BAR	Pass	11:28am
BT	Pass	11:28am

Blank Tests

Test	Status	Time
AIR	Pass	11:29am

Printer Tests

Test	Status	Time
PRNT	Pass	11:29am

CRC Tests

Test	Status	Time
COMP	Pass	11:29am
CAL	Pass	11:29am

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II**


County Watauga Instrument Location Watauga Co. Jail

Instrument Serial No. 008715 Boone, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 20 day of May, 2009 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

649
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

WATAUGA COUNTY WATAUGA JAIL 940

Serial Number: 008715

Test Date: 05/20/2009

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: BURNETTE, ANTHONY J

Permit Number: 11304E

Effective:

12/01/2007-12/01/2009

Officer's Name: NONE,

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG723302

Exp Date: 08/20/2009

Test	g/210L	Time
DIAG	Pass	11:20am
AIR BLK	.00	11:21am
ACCY CHK	.08	11:22am
AIR BLK	.00	11:23am
SUB TEST	.00	11:23am
AIR BLK	.00	11:24am
SUB TEST	.00	11:25am
AIR BLK	.00	11:26am

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR


Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

WATAUGA COUNTY WATAUGA JAIL 940

Serial Number: 008715 Test Record Number: 296
Test Date: 05/20/2009 Test Time: 11:28am EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	11:28am
FLO	Pass	11:28am
FC	Pass	11:28am

Temperature Tests

Test	Status	Time
FC1	Pass	11:28am
SRC	Pass	11:28am
DET	Pass	11:28am
BAR	Pass	11:28am
BT	Pass	11:28am

Blank Tests

Test	Status	Time
AIR	Pass	11:29am

Printer Tests

Test	Status	Time
PRNT	Pass	11:29am

CRC Tests

Test	Status	Time
COMP	Pass	11:29am
CAL	Pass	11:29am

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II**


County Avery Instrument Location Avery Co. Jail

Instrument Serial No. 008664 Newland, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 19 day of May, 2009 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature] Signature of Certifying Official 649 Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

AVERY COUNTY AVERY COUNTY JAIL 050

Serial Number: 008664
Test Date: 05/19/2009

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE

Analyst's Name: BURNETTE, ANTHONY J
Permit Number: 11304E
Effective:
12/01/2007-12/01/2009

Officer's Name: NONE,
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG722702
Exp Date: 08/14/2009

Test	g/210L	Time
DIAG	Pass	11:10am
AIR BLK	.00	11:11am
ACCY CHK	.07	11:11am
AIR BLK	.00	11:12am
SUB TEST	.00	11:13am
AIR BLK	.00	11:14am
SUB TEST	.00	11:16am
AIR BLK	.00	11:17am

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR.



Analyst

Intox EC/IR-II: Preventive Maintenance

AVERY COUNTY AVERY COUNTY JAIL 050

Serial Number: 008664 Test Record Number: 188
Test Date: 05/19/2009 Test Time: 11:18am EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	11:18am
FLO	Pass	11:18am
FC	Pass	11:18am

Temperature Tests

Test	Status	Time
FC1	Pass	11:18am
SRC	Pass	11:18am
DET	Pass	11:18am
BAR	Pass	11:18am
BT	Pass	11:18am

Blank Tests

Test	Status	Time
AIR	Pass	11:19am

Printer Tests

Test	Status	Time
PRNT	Pass	11:19am

CRC Tests

Test	Status	Time
COMP	Pass	11:19am
CAL	Pass	11:19am

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH


**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II**

County Lincoln Instrument Location Courthouse
Instrument Serial No. 008827 #1 Courthouse Sq, Lincolnton
704-732-9020

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 26 day of May, 2009 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Bobby L. Willis
Signature of Certifying Official

557
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

LINCOLN COUNTY COURTHOUSE 540

Serial Number: 008827
Test Date: 05/26/2009

Citation Number: M0000000-0
Subject's Name:

PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE

Analyst's Name: WILLIS, BOBBY D
Permit Number: 08010E
Effective:
12/01/2007-12/01/2009

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG723302
Exp Date: 08/20/2009

Test	g/210L	Time
DIAG	Pass	1:42pm
AIR BLK	.00	1:43pm
ACCY CHK	.07	1:44pm
AIR BLK	.00	1:45pm
SUB TEST	.00	1:45pm
AIR BLK	.00	1:46pm
SUB TEST	.00	1:48pm
AIR BLK	.00	1:48pm

Reported AC: .00 g/210L

Bobby D. Willis
Signature of Chemical Analyst

Court CVR

Bobby D. Willis
Analyst

Intox EC/IR-II: Preventive Maintenance

LINCOLN COUNTY COURTHOUSE 540

Serial Number: 008827 Test Record Number: 259

Test Date: 05/26/2009 Test Time: 1:51pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	1:51pm
FLO	Pass	1:51pm
FC	Pass	1:51pm

Temperature Tests

Test	Status	Time
FC1	Pass	1:51pm
SRC	Pass	1:51pm
DET	Pass	1:51pm
BAR	Pass	1:51pm
BT	Pass	1:51pm

Blank Tests

Test	Status	Time
AIR	Pass	1:52pm


Printer Tests

Test	Status	Time
PRNT	Pass	1:52pm

CRC Tests

Test	Status	Time
COMP	Pass	1:52pm
CAL	Pass	1:52pm

Preventive Maintenance
Status: Pass

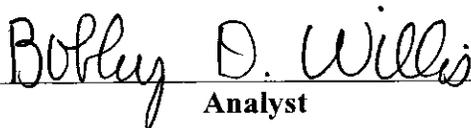
Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II**


County Lincoln Instrument Location Courthouse

Instrument Serial No. 008813 #1 Courthouse Sq., Lincolnton
704-732-9020

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 26 day of May, 20 09 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Bobby D. Willis
Signature of Certifying Official

557
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

LINCOLN COUNTY COURTHOUSE 540

Serial Number: 008823
Test Date: 05/26/2009

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE

Analyst's Name: WILLIS, BOBBY D
Permit Number: 08010E
Effective:
12/01/2007-12/01/2009

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG723302
Exp Date: 08/20/2009

Test	g/210L	Time
DIAG	Pass	1:18pm
AIR BLK	.00	1:19pm
ACCY CHK	.07	1:20pm
AIR BLK	.00	1:20pm
SUB TEST	.00	1:21pm
AIR BLK	.00	1:22pm
SUB TEST	.00	1:23pm
AIR BLK	.00	1:24pm

Reported AC: .00 g/210L

Bobby D. Willis
Signature of Chemical Analyst

Court CVR

Bobby D. Willis
Analyst

Intox EC/IR-II: Preventive Maintenance

LINCOLN COUNTY COURTHOUSE 540

Serial Number: 008823 Test Record Number: 414
Test Date: 05/26/2009 Test Time: 1:26pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	1:26pm
FLO	Pass	1:26pm
FC	Pass	1:26pm

Temperature Tests

Test	Status	Time
FC1	Pass	1:26pm
SRC	Pass	1:26pm
DET	Pass	1:26pm
BAR	Pass	1:26pm
BT	Pass	1:26pm

Blank Tests

Test	Status	Time
AIR	Pass	1:27pm


Printer Tests

Test	Status	Time
PRNT	Pass	1:27pm

CRC Tests

Test	Status	Time
COMP	Pass	1:27pm
CAL	Pass	1:27pm

Preventive Maintenance
Status: Pass

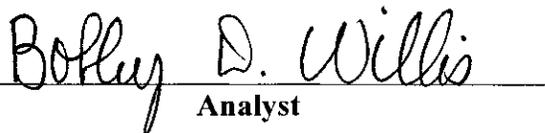
Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II**


County Randolph Instrument Location BAT Mobile Unit 4

Instrument Serial No. 008734

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 23rd day of May, 2009 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Daniel O. Trumble
Signature of Certifying Official

651
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Preventive Maintenance

RANDOLPH COUNTY BAT MOBILE UNIT 4 750

Serial Number: 008734 Test Record Number: 232
Test Date: 05/23/2009 Test Time: 9:14pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	9:15pm
FLO	Pass	9:15pm
FC	Pass	9:15pm

Temperature Tests

Test	Status	Time
FC1	Pass	9:15pm
SRC	Pass	9:15pm
DET	Pass	9:15pm
BAR	Pass	9:15pm
BT	Pass	9:15pm

Blank Tests

Test	Status	Time
AIR	Pass	9:15pm

Printer Tests

Test	Status	Time
PRNT	Pass	9:16pm

CRC Tests

Test	Status	Time
COMP	Pass	9:16pm
CAL	Pass	9:16pm

Preventive Maintenance
Status: Pass


Analyst

Intox EC/IR-II: Subject Test

RANDOLPH COUNTY BAT MOBILE UNIT 4 750

Serial Number: 008734
Test Date: 05/23/2009

Citation Number: M0000000-0
Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: TRUDELL, SR., DANIEL T

Permit Number: 21535E

Effective:

12/01/2007-12/01/2009

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG722501


Exp Date: 08/12/2009

Test	g/210L	Time
DIAG	Pass	9:05pm
AIR BLK	.00	9:06pm
ACCY CHK	.07	9:06pm
AIR BLK	.00	9:07pm
SUB TEST	.00	9:08pm
AIR BLK	.00	9:09pm
SUB TEST	.00	9:10pm
AIR BLK	.00	9:11pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II**


County Randolph Instrument Location BAT Mobile unit 4

Instrument Serial No. 008717

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 23rd day of May, 2009 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

651
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Preventive Maintenance

RANDOLPH COUNTY BAT MOBILE UNIT 4 750

Serial Number: 008717 Test Record Number: 159

Test Date: 05/23/2009 Test Time: 9:14pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	9:14pm
FLO	Pass	9:14pm
FC	Pass	9:14pm

Temperature Tests

Test	Status	Time
FC1	Pass	9:14pm
SRC	Pass	9:14pm
DET	Pass	9:14pm
BAR	Pass	9:14pm
BT	Pass	9:14pm

Blank Tests

Test	Status	Time
AIR	Pass	9:15pm


Printer Tests

Test	Status	Time
PRNT	Pass	9:15pm

CRC Tests

Test	Status	Time
COMP	Pass	9:15pm
CAL	Pass	9:15pm

Preventive Maintenance
Status: Pass


Analyst

Intox EC/IR-II: Subject Test

RANDOLPH COUNTY BAT MOBILE UNIT 4 750

Serial Number: 008717
Test Date: 05/23/2009

Citation Number: M0000000-0
Subject's Name:

PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: TRUDELL, SR., DANIEL T
Permit Number: 21535E
Effective:
12/01/2007-12/01/2009

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG723401
Exp Date: 08/21/2009

Test	g/210L	Time
DIAG	Pass	9:03pm
AIR BLK	.00	9:04pm
ACCY CHK	.07	9:05pm
AIR BLK	.00	9:06pm
SUB TEST	.00	9:06pm
AIR BLK	.00	9:07pm
SUB TEST	.00	9:09pm
AIR BLK	.00	9:10pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH


**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II**

County Wayne Instrument Location Wayne Co. Detention Center
Instrument Serial No. 008449 207 E. Chestnut St., Goldsboro, N.C.

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 13th day of May, 2009 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Jinda A. Rush
Signature of Certifying Official

447
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

WAYNE COUNTY WAYNE CO DETENTION 950

Serial Number: 008649
Test Date: 05/13/2009

Citation Number: M0000000-0
Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: KEESLER, LINDA A

Permit Number: 11646E

Effective:

12/01/2007-12/01/2009

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG722601

Exp Date: 08/13/2009


Test	g/210L	Time
DIAG	Pass	3:25pm
AIR BLK	.00	3:26pm
ACCY CHK	.07	3:27pm
AIR BLK	.00	3:28pm
SUB TEST	.00	3:29pm
AIR BLK	.00	3:29pm
SUB TEST	.00	3:31pm
AIR BLK	.00	3:32pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR

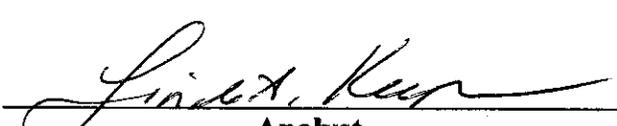

Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

WAYNE COUNTY WAYNE CO DETENTION 950

Serial Number: 008649 Test Record Number: 1033
Test Date: 05/13/2009 Test Time: 3:36pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	3:36pm
FLO	Pass	3:36pm
FC	Pass	3:36pm

Temperature Tests

Test	Status	Time
FC1	Pass	3:36pm
SRC	Pass	3:36pm
DET	Pass	3:36pm
BAR	Pass	3:36pm
BT	Pass	3:36pm

Blank Tests

Test	Status	Time
AIR	Pass	3:37pm

Printer Tests

Test	Status	Time
PRNT	Pass	3:37pm

CRC Tests

Test	Status	Time
COMP	Pass	3:37pm
CAL	Pass	3:37pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH


**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II**

County Wayne Instrument Location Wayne Co. Detention Center
Instrument Serial No. 004671 207E Chestnut St., Goldsboro, N.C.

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 13th day of May, 2009 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Jack A. Webb
Signature of Certifying Official

647
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

WAYNE COUNTY WAYNE CO DETENTION 950

Serial Number: 008671

Test Date: 05/13/2009

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: KEESLER, LINDA A

Permit Number: 11646E

Effective:

12/01/2007-12/01/2009

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG722801

Exp Date: 08/15/2009


Test	g/210L	Time
DIAG	Pass	3:27pm
AIR BLK	.00	3:28pm
ACCY CHK	.07	3:29pm
AIR BLK	.00	3:30pm
SUB TEST	.00	3:31pm
AIR BLK	.00	3:31pm
SUB TEST	.00	3:33pm
AIR BLK	.00	3:34pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

This form is used when performing Preventive Maintenance procedures

Forensic Tests for Alcohol Branch

Department of Health and Human Services

Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

WAYNE COUNTY WAYNE CO DETENTION 950

Serial Number: 008671 Test Record Number: 806
Test Date: 05/13/2009 Test Time: 3:36pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	3:36pm
FLO	Pass	3:36pm
FC	Pass	3:36pm

Temperature Tests

Test	Status	Time
FC1	Pass	3:36pm
SRC	Pass	3:36pm
DET	Pass	3:36pm
BAR	Pass	3:36pm
BT	Pass	3:36pm

Blank Tests

Test	Status	Time
AIR	Pass	3:37pm


Printer Tests

Test	Status	Time
PRNT	Pass	3:37pm

CRC Tests

Test	Status	Time
COMP	Pass	3:37pm
CAL	Pass	3:37pm

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II**

County Pitt Instrument Location Pitt Co. Detention Center
Instrument Serial No. 008662 124 Detention Ctr., Greenville, N.C.

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 13th day of May, 20 09 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Josh A. Kest
Signature of Certifying Official

447
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

PITT COUNTY PITT CO DETENTION 730

Serial Number: 008662
Test Date: 05/13/2009

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE

Analyst's Name: KEESLER, LINDA A
Permit Number: 11646E
Effective:
12/01/2007-12/01/2009

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG722602
Exp Date: 08/13/2009


Test	g/210L	Time
DIAG	Pass	11:25am
AIR BLK	.00	11:25am
ACCY CHK	.07	11:26am
AIR BLK	.00	11:27am
SUB TEST	.00	11:28am
AIR BLK	.00	11:29am
SUB TEST	.00	11:30am
AIR BLK	.00	11:31am

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR

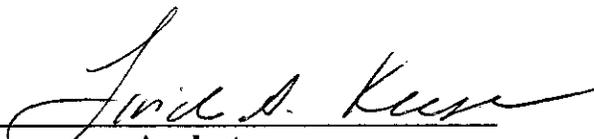

Analyst

Intox EC/IR-II: Preventive Maintenance

PITT COUNTY PITT CO DETENTION 730

Serial Number: 008662 Test Record Number: 309
Test Date: 05/13/2009 Test Time: 11:34am EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	11:34am
FLO	Pass	11:34am
FC	Pass	11:34am

Temperature Tests

Test	Status	Time
FC1	Pass	11:34am
SRC	Pass	11:34am
DET	Pass	11:34am
BAR	Pass	11:34am
BT	Pass	11:34am

Blank Tests

Test	Status	Time
AIR	Pass	11:35am


Printer Tests

Test	Status	Time
PRNT	Pass	11:35am

CRC Tests

Test	Status	Time
COMP	Pass	11:35am
CAL	Pass	11:35am

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH


**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II**

County Pike Instrument Location Pike Co. Detention Center
Instrument Serial No. 008644 124 Detention Dr., Greenville, N.C.

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 13th day of MAY, 20 09 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Frank A. West
Signature of Certifying Official

447
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

PITT COUNTY PITT CO DETENTION 730

Serial Number: 008646
Test Date: 05/13/2009

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE

Analyst's Name: KEESLER, LINDA A
Permit Number: 11646E
Effective:
12/01/2007-12/01/2009

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG825401
Exp Date: 09/10/2010


Test	g/210L	Time
DIAG	Pass	11:29am
AIR BLK	.00	11:30am
ACCY CHK	.08	11:31am
AIR BLK	.00	11:32am
SUB TEST	.00	11:33am
AIR BLK	.00	11:34am
SUB TEST	.00	11:36am
AIR BLK	.00	11:37am

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

Intox EC/IR-II: Preventive Maintenance

PITT COUNTY PITT CO DETENTION 730

Serial Number: 008646 Test Record Number: 509
Test Date: 05/13/2009 Test Time: 11:40am EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	11:40am
FLO	Pass	11:40am
FC	Pass	11:40am

Temperature Tests

Test	Status	Time
FC1	Pass	11:40am
SRC	Pass	11:40am
DET	Pass	11:40am
BAR	Pass	11:40am
BT	Pass	11:40am

Blank Tests

Test	Status	Time
AIR	Pass	11:41am

Printer Tests

Test	Status	Time
PRNT	Pass	11:41am

CRC Tests

Test	Status	Time
COMP	Pass	11:41am
CAL	Pass	11:41am

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH


**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II**

County Pitt Instrument Location Pitt Co. Detention Center
Instrument Serial No. 008264 124 Detention Pt., Greenville, N.C.

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 13th day of May, 20 09 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Jinda S. Kest
Signature of Certifying Official

447
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

PITT COUNTY PITT CO DETENTION 730

Serial Number: 008668
Test Date: 05/13/2009

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: KEESLER, LINDA A
Permit Number: 11646E
Effective:
12/01/2007-12/01/2009

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG816303
Exp Date: 06/11/2010

Test	g/210L	Time
DIAG	Pass	11:26am
AIR BLK	.00	11:27am
ACCY CHK	.07	11:27am
AIR BLK	.00	11:28am
SUB TEST	.00	11:29am
AIR BLK	.00	11:29am
SUB TEST	.00	11:31am
AIR BLK	.00	11:32am

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

Intox EC/IR-II: Preventive Maintenance

PITT COUNTY PITT CO DETENTION 730

Serial Number: 008668 Test Record Number: 935
Test Date: 05/13/2009 Test Time: 11:38am EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	11:38am
FLO	Pass	11:38am
FC	Pass	11:39am

Temperature Tests

Test	Status	Time
FC1	Pass	11:39am
SRC	Pass	11:39am
DET	Pass	11:39am
BAR	Pass	11:39am
BT	Pass	11:39am

Blank Tests

Test	Status	Time
AIR	Pass	11:39am


Printer Tests

Test	Status	Time
PRNT	Pass	11:39am

CRC Tests

Test	Status	Time
COMP	Pass	11:39am
CAL	Pass	11:39am

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II**


County Dare Instrument Location Dare Co SO. Hatteras

Instrument Serial No. 008807 503416 NC Hwy 12, Frisco, N.C.

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 12th day of May, 2009 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

643
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

DARE COUNTY DARE CO SO HATTERAS 270

Serial Number: 008807
Test Date: 05/12/2009

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE

Analyst's Name: GUARD, KELLY G
Permit Number: 12955E
Effective:
12/01/2007-12/01/2009

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG722802
Exp Date: 08/15/2009

Test	g/210L	Time
DIAG	Pass	1:26pm
AIR BLK	.00	1:27pm
ACCY CHK	.07	1:27pm
AIR BLK	.00	1:28pm
SUB TEST	.00	1:29pm
AIR BLK	.00	1:30pm
SUB TEST	.00	1:31pm
AIR BLK	.00	1:32pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

Intox EC/IR-II: Preventive Maintenance

DARE COUNTY DARE CO SO HATTERAS 270

Serial Number: 008807 Test Record Number: 131
Test Date: 05/12/2009 Test Time: 1:35pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	1:35pm
FLO	Pass	1:35pm
FC	Pass	1:35pm

Temperature Tests

Test	Status	Time
FC1	Pass	1:35pm
SRC	Pass	1:35pm
DET	Pass	1:35pm
BAR	Pass	1:35pm
BT	Pass	1:35pm

Blank Tests

Test	Status	Time
AIR	Pass	1:36pm


Printer Tests

Test	Status	Time
PRNT	Pass	1:36pm

CRC Tests

Test	Status	Time
COMP	Pass	1:36pm
CAL	Pass	1:36pm

Preventive Maintenance
Status: Pass

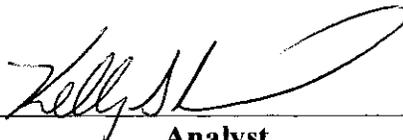

Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II**


County Hyde Instrument Location Hyde Co SD Orrardke

Instrument Serial No. 008797 NC 12, Ocotacoke, N.C.

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 12th day of May, 2009 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]

Signature of Certifying Official

643

Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

HYDE COUNTY HYDE CO SO OCRACOKE 470

Serial Number: 008797
Test Date: 05/12/2009

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: *GUARD, KELLY G*
Permit Number: 12955E
Effective:
12/01/2007-12/01/2009

Officer's Name: *NONE, NONE*
Type of Agency: *FTA*
Agency: *DHHS*
Test Type: *Breath Test*

Lot Number: AG722701
Exp Date: 08/14/2009

Test	g/210L	Time
DIAG	Pass	11:31am
AIR BLK	.00	11:32am
ACCY CHK	.07	11:33am
AIR BLK	.00	11:34am
SUB TEST	.00	11:34am
AIR BLK	.00	11:35am
SUB TEST	.00	11:37am
AIR BLK	.00	11:38am

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

Intox EC/IR-II: Preventive Maintenance

HYDE COUNTY HYDE CO SO OCRACOCKE 470

Serial Number: 008797 Test Record Number: 99
Test Date: 05/12/2009 Test Time: 11:40am EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	11:41am
FLO	Pass	11:41am
FC	Pass	11:41am

Temperature Tests

Test	Status	Time
FC1	Pass	11:41am
SRC	Pass	11:41am
DET	Pass	11:41am
BAR	Pass	11:41am
BT	Pass	11:41am

Blank Tests

Test	Status	Time
AIR	Pass	11:41am

Printer Tests

Test	Status	Time
PRNT	Pass	11:42am

CRC Tests

Test	Status	Time
COMP	Pass	11:42am
CAL	Pass	11:42am

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II**

County Greene Instrument Location Greene Co. S.O.

Instrument Serial No. 008670 301 N. Greene St., Snow Hill, N.C.

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 1st day of May, 2009 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Kelly M. D.
Signature of Certifying Official

643
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

GREENE COUNTY GREENE CO SO 390

Serial Number: 008670
Test Date: 05/01/2009

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE

Analyst's Name: GUARD, KELLY G
Permit Number: 12955E
Effective:
12/01/2007-12/01/2009

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG722601
Exp Date: 08/13/2009


Test	g/210L	Time
DIAG	Pass	10:15am
AIR BLK	.00	10:16am
ACCY CHK	.07	10:17am
AIR BLK	.00	10:17am
SUB TEST	.00	10:18am
AIR BLK	.00	10:19am
SUB TEST	.00	10:20am
AIR BLK	.00	10:21am

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

Intox EC/IR-II: Preventive Maintenance

GREENE COUNTY GREENE CO SO 390

Serial Number: 008670 Test Record Number: 714
Test Date: 05/01/2009 Test Time: 10:22am EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	10:23am
FLO	Pass	10:23am
FC	Pass	10:23am

Temperature Tests

Test	Status	Time
FC1	Pass	10:23am
SRC	Pass	10:23am
DET	Pass	10:23am
BAR	Pass	10:23am
BT	Pass	10:23am

Blank Tests

Test	Status	Time
AIR	Pass	10:23am

Printer Tests

Test	Status	Time
PRNT	Pass	10:23am

CRC Tests

Test	Status	Time
COMP	Pass	10:24am
CAL	Pass	10:24am

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II**

County Davie Instrument Location Davie Co. Jail

Instrument Serial No. 008828 Mocksville, N.C.

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 26 day of May, 2009 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



L. Kevin Dean
Signature of Certifying Official

642
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

DAVIE COUNTY DAVIE COUNTY JAIL 290

Serial Number: 008828

Test Date: 05/26/2009

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: DEAN, LARRY K

Permit Number: 11598E

Effective:

12/01/2007-12/01/2009

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG723401

Exp Date: 08/21/2009


Test	g/210L	Time
DIAG	Pass	3:40pm
AIR BLK	.00	3:40pm
ACCY CHK	.08	3:41pm
AIR BLK	.00	3:42pm
SUB TEST	.00	3:42pm
AIR BLK	.00	3:43pm
SUB TEST	.00	3:44pm
AIR BLK	.00	3:45pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

Intox EC/IR-II: Preventive Maintenance

DAVIE COUNTY DAVIE COUNTY JAIL 290

Serial Number: 008828 Test Record Number: 128
Test Date: 05/26/2009 Test Time: 3:36pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	3:37pm
FLO	Pass	3:37pm
FC	Pass	3:37pm

Temperature Tests

Test	Status	Time
FC1	Pass	3:37pm
SRC	Pass	3:37pm
DET	Pass	3:37pm
BAR	Pass	3:37pm
BT	Pass	3:37pm

Blank Tests

Test	Status	Time
AIR	Pass	3:37pm


Printer Tests

Test	Status	Time
PRNT	Pass	3:37pm

CRC Tests

Test	Status	Time
COMP	Pass	3:38pm
CAL	Pass	3:38pm

Preventive Maintenance
Status: Pass

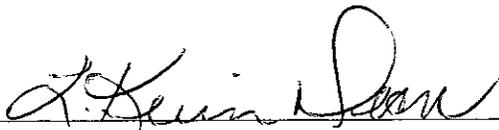

Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II**


County Cherokee Instrument Location Cherokee Co. Jail

Instrument Serial No. 008622 Murphy, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 6 day of May, 20 09 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



David R. Smith

Signature of Certifying Official

635

Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Preventive Maintenance

CHEROKEE COUNTY CHEOKEE COUNTY JAIL 190

Serial Number: 008622 Test Record Number: 493
Test Date: 05/06/2009 Test Time: 12:16pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	12:16pm
FLO	Pass	12:16pm
FC	Pass	12:16pm

Temperature Tests

Test	Status	Time
FC1	Pass	12:16pm
SRC	Pass	12:16pm
DET	Pass	12:16pm
BAR	Pass	12:16pm
BT	Pass	12:16pm

Blank Tests

Test	Status	Time
AIR	Pass	12:17pm


Printer Tests

Test	Status	Time
PRNT	Pass	12:17pm

CRC Tests

Test	Status	Time
COMP	Pass	12:17pm
CAL	Pass	12:17pm

Preventive Maintenance
Status: Pass



Analyst

Intox EC/IR-II: Subject Test

CHEROKEE COUNTY CHEOKEE COUNTY JAIL
190

Serial Number: 008622
Test Date: 05/06/2009

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE

Analyst's Name: CUTLER, DANIEL R
Permit Number: 08457E
Effective:
12/01/2007-12/01/2009

Officer's Name: NONE,
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG723301
Exp Date: 08/20/2009

Test	g/210L	Time
DIAG	Pass	12:08pm
AIR BLK	.00	12:09pm
ACCY CHK	.08	12:10pm
AIR BLK	.00	12:10pm
SUB TEST	.00	12:11pm
AIR BLK	.00	12:12pm
SUB TEST	.00	12:13pm
AIR BLK	.00	12:14pm

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II**


County Cherokee Instrument Location Cherokee Co. Jail

Instrument Serial No. 008711 Murphy, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 6 day of May, 2009 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Daniel R. Cathey
Signature of Certifying Official

635
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

CHEROKEE COUNTY CHEROKEE COUNTY JAIL
190

Serial Number: 008711
Test Date: 05/06/2009

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE

Analyst's Name: CUTLER, DANIEL R
Permit Number: 08457E
Effective:
12/01/2007-12/01/2009

Officer's Name: NONE,
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG723301
Exp Date: 08/20/2009

Test	g/210L	Time
DIAG	Pass	12:07pm
AIR BLK	.00	12:08pm
ACCY CHK	.07	12:08pm
AIR BLK	.00	12:09pm
SUB TEST	.00	12:10pm
AIR BLK	.00	12:10pm
SUB TEST	.00	12:12pm
AIR BLK	.00	12:13pm

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR



Analyst

Intox EC/IR-II: Preventive Maintenance

CHEROKEE COUNTY CHEROKEE COUNTY JAIL 190

Serial Number: 008711 Test Record Number: 113
Test Date: 05/06/2009 Test Time: 12:14pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	12:14pm
FLO	Pass	12:14pm
FC	Pass	12:15pm

Temperature Tests

Test	Status	Time
FC1	Pass	12:15pm
SRC	Pass	12:15pm
DET	Pass	12:15pm
BAR	Pass	12:15pm
BT	Pass	12:15pm

Blank Tests

Test	Status	Time
AIR	Pass	12:15pm


Printer Tests

Test	Status	Time
PRNT	Pass	12:15pm

CRC Tests

Test	Status	Time
COMP	Pass	12:15pm
CAL	Pass	12:15pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II**

County Swain Instrument Location Swain Co. Jail

Instrument Serial No. 008727 Bryson City, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 5 day of May, 2009 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



David R. Cuthbert

Signature of Certifying Official

635

Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

SWAIN COUNTY SWAIN COUNTY JAIL 860

Serial Number: 008727
Test Date: 05/05/2009

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE

Analyst's Name: CUTLER, DANIEL R
Permit Number: 08457E
Effective:
12/01/2007-12/01/2009

Officer's Name: NONE,
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG7220702
Exp Date: 08/14/2009

Test	g/210L	Time
DIAG	Pass	11:29am
AIR BLK	.00	11:29am
ACCY CHK	.07	11:30am
AIR BLK	.00	11:31am
SUB TEST	.00	11:31am
AIR BLK	.00	11:32am
SUB TEST	.00	11:34am
AIR BLK	.00	11:34am

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR



Analyst

Intox EC/IR-II: Preventive Maintenance

SWAIN COUNTY SWAIN COUNTY JAIL 860

Serial Number: 008727 Test Record Number: 261
Test Date: 05/05/2009 Test Time: 11:35am EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	11:35am
FLO	Pass	11:35am
FC	Pass	11:36am

Temperature Tests

Test	Status	Time
FC1	Pass	11:36am
SRC	Pass	11:36am
DET	Pass	11:36am
BAR	Pass	11:36am
BT	Pass	11:36am

Blank Tests

Test	Status	Time
AIR	Pass	11:36am

Printer Tests

Test	Status	Time
PRNT	Pass	11:36am

CRC Tests

Test	Status	Time
COMP	Pass	11:36am
CAL	Pass	11:36am

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II**

County Swain Instrument Location Swain Co. Jail

Instrument Serial No. 008723 Bryson City, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 5 day of May, 2009 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Ernie R. Galt
Signature of Certifying Official

635
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

SWAIN COUNTY SWAIN COUNTY JAIL 860

Serial Number: 008723
Test Date: 05/05/2009

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE

Analyst's Name: CUTLER, DANIEL R
Permit Number: 08457E
Effective:
12/01/2007-12/01/2009

Officer's Name: NONE,
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG722702
Exp Date: 08/14/2009

Test	g/210L	Time
DIAG	Pass	11:28am
AIR BLK	.00	11:28am
ACCY CHK	.07	11:29am
AIR BLK	.00	11:29am
SUB TEST	.00	11:30am
AIR BLK	.00	11:31am
SUB TEST	.00	11:32am
AIR BLK	.00	11:33am

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR.



Analyst

Intox EC/IR-II: Preventive Maintenance

SWAIN COUNTY SWAIN COUNTY JAIL 860

Serial Number: 008723 Test Record Number: 143
Test Date: 05/05/2009 Test Time: 11:34am EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	11:34am
FLO	Pass	11:34am
FC	Pass	11:35am

Temperature Tests

Test	Status	Time
FC1	Pass	11:35am
SRC	Pass	11:35am
DET	Pass	11:35am
BAR	Pass	11:35am
BT	Pass	11:35am

Blank Tests

Test	Status	Time
AIR	Pass	11:35am


Printer Tests

Test	Status	Time
PRNT	Pass	11:35am

CRC Tests

Test	Status	Time
COMP	Pass	11:35am
CAL	Pass	11:35am

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II**

County CHATHAM Instrument Location PITTSBORO POLICE DEPT.

Instrument Serial No. 008591 PITTSBORO NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 26 day of MAY, 20 09 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



R. H. Russell
Signature of Certifying Official

371
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

CHATHAM PITTSBORO PD 180

Serial Number: 008591
Test Date: 05/26/2009

Citation Number: M0000000-0
Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: NC

Driver's License Number: NONE

Analyst's Name: RUSSELL, LARRY H

Permit Number: 06108E

Effective:

12/01/2007-12/01/2009

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG904903

Exp Date: 02/18/2011


Test	g/210L	Time
DIAG	Pass	1:48pm
AIR BLK	.00	1:49pm
ACCY CHK	.08	1:50pm
AIR BLK	.00	1:51pm
SUB TEST	.00	1:52pm
AIR BLK	.00	1:52pm
SUB TEST	.00	1:54pm
AIR BLK	.00	1:55pm

Reported AC: .00 g/210L

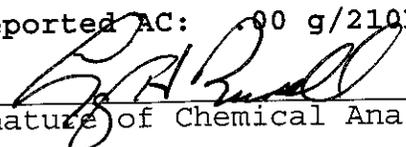

Signature of Chemical Analyst

Court CVR

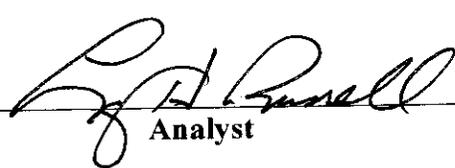

Analyst

Intox EC/IR-II: Preventive Maintenance

CHATHAM PITTSBORO PD 180

Serial Number: 008591 Test Record Number: 332
Test Date: 05/26/2009 Test Time: 1:59pm EDT

System Check: Passed

Baseline Tests

Test	Status	Time
IR	Pass	1:59pm
FLO	Pass	1:59pm
FC	Pass	1:59pm

Temperature Tests

Test	Status	Time
FC1	Pass	1:59pm
SRC	Pass	1:59pm
DET	Pass	1:59pm
BAR	Pass	1:59pm
BT	Pass	1:59pm

Blank Tests

Test	Status	Time
AIR	Pass	2:00pm


Printer Tests

Test	Status	Time
PRNT	Pass	2:00pm

CRC Tests

Test	Status	Time
COMP	Pass	2:00pm
CAL	Pass	2:00pm

Preventive Maintenance
Status: Pass

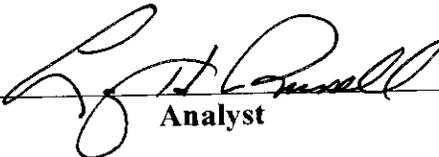

Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II**


County CRAVEN Instrument Location MCAS CHERRY POINT

Instrument Serial No. 010819

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 7 day of MAY, 2009 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Raney E. Hall

Signature of Certifying Official

354

Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

CRAVEN COUNTY MCAS CHERRY POINT 240

Serial Number: 010819
Test Date: 05/07/2009

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: HALL, RANDY E
Permit Number: 03462E
Effective:
12/01/2007-12/01/2009

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG902603
Exp Date: 01/26/2011


Test	g/210L	Time
DIAG	Pass	10:14am
AIR BLK	.00	10:15am
ACCY CHK	.08	10:16am
AIR BLK	.00	10:16am
SUB TEST	.00	10:17am
AIR BLK	.00	10:18am
SUB TEST	.00	10:19am
AIR BLK	.00	10:20am

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR

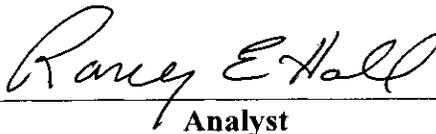

Analyst

Intox EC/IR-II: Preventive Maintenance

CRAVEN COUNTY MCAS CHERRY POINT 240

Serial Number: 010819 Test Record Number: 52
Test Date: 05/07/2009 Test Time: 10:22am EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	10:23am
FLO	Pass	10:23am
FC	Pass	10:23am

Temperature Tests

Test	Status	Time
FC1	Pass	10:23am
SRC	Pass	10:23am
DET	Pass	10:23am
BAR	Pass	10:23am
BT	Pass	10:23am

Blank Tests

Test	Status	Time
AIR	Pass	10:24am


Printer Tests

Test	Status	Time
PRNT	Pass	10:24am

CRC Tests

Test	Status	Time
COMP	Pass	10:24am
CAL	Pass	10:24am

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II**

County Onslow Instrument Location Camp Lejeune PMO

Instrument Serial No. 008919

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 12 day of MAY, 20 09 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Randy E. Hall

Signature of Certifying Official

354

Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

ONslow COUNTY CAMP LEJEUNE PMO 660

Serial Number: 008919
Test Date: 05/12/2009

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: HALL, RANDY E
Permit Number: 03462E
Effective:
12/01/2007-12/01/2009

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG722802
Exp Date: 08/15/2009


Test	g/210L	Time
DIAG	Pass	11:01am
AIR BLK	.00	11:02am
ACCY CHK	.07	11:03am
AIR BLK	.00	11:04am
SUB TEST	.00	11:04am
AIR BLK	.00	11:05am
SUB TEST	.00	11:07am
AIR BLK	.00	11:07am

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR

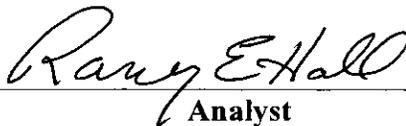

Analyst

Intox EC/IR-II: Preventive Maintenance

ONslow COUNTY CAMP LEJEUNE PMO 660

Serial Number: 008919 Test Record Number: 152
Test Date: 05/12/2009 Test Time: 11:08am EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	11:08am
FLO	Pass	11:08am
FC	Pass	11:09am

Temperature Tests

Test	Status	Time
FC1	Pass	11:09am
SRC	Pass	11:09am
DET	Pass	11:09am
BAR	Pass	11:09am
BT	Pass	11:09am

Blank Tests

Test	Status	Time
AIR	Pass	11:09am


Printer Tests

Test	Status	Time
PRNT	Pass	11:09am

CRC Tests

Test	Status	Time
COMP	Pass	11:10am
CAL	Pass	11:10am

Preventive Maintenance
Status: Pass

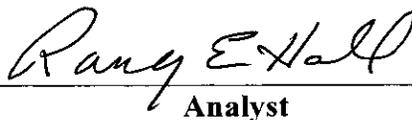

Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH


**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II**

County New Hanover Instrument Location Caroline Beach
Instrument Serial No. 8661 Police Dept.

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 21 day of May, 20 09 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Anthony K...
Signature of Certifying Official

634
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

NEW HANOVER COUNTY CAROLINA BEACH PD
640

Serial Number: 008661
Test Date: 05/21/2009

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: RIVERA, ANTHONY
Permit Number: 08259E
Effective:
12/01/2007-12/01/2009

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG901901
Exp Date: 01/19/2011


Test	g/210L	Time
DIAG	Pass	9:16pm
AIR BLK	.00	9:17pm
ACCY CHK	.08	9:18pm
AIR BLK	.00	9:19pm
SUB TEST	.00	9:19pm
AIR BLK	.00	9:20pm
SUB TEST	.00	9:21pm
AIR BLK	.00	9:22pm

Reported AC: 00 g/210L



Signature of Chemical Analyst

Court CVR

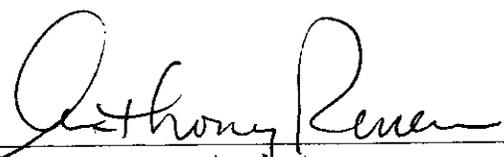

Analyst

Intox EC/IR-II: Preventive Maintenance

NEW HANOVER COUNTY CAROLINA BEACH PD 640

Serial Number: 008661 Test Record Number: 583
Test Date: 05/21/2009 Test Time: 9:24pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	9:24pm
FLO	Pass	9:24pm
FC	Pass	9:24pm

Temperature Tests

Test	Status	Time
FC1	Pass	9:24pm
SRC	Pass	9:24pm
DET	Pass	9:24pm
BAR	Pass	9:24pm
BT	Pass	9:24pm

Blank Tests

Test	Status	Time
AIR	Pass	9:25pm


Printer Tests

Test	Status	Time
PRNT	Pass	9:25pm

CRC Tests

Test	Status	Time
COMP	Pass	9:25pm
CAL	Pass	9:25pm

Preventive Maintenance
Status: Pass

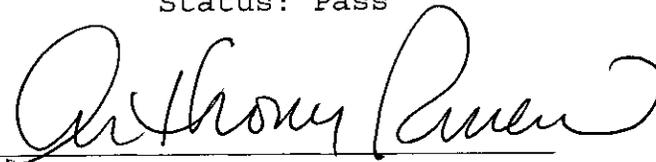

Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH


**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II**

County New Hanover Instrument Location Wrightsville Beach
Instrument Serial No. 8667 Police Dept.

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 21 day of May, 2009 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Anthony Rivera
Signature of Certifying Official

634
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

NEW HANOVER COUNTY WRIGHTSVILLE BCH PD
640

Serial Number: 008667
Test Date: 05/21/2009

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: RIVERA, ANTHONY
Permit Number: 08259E
Effective:
12/01/2007-12/01/2009

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG902901
Exp Date: 01/29/2011


Test	g/210L	Time
DIAG	Pass	8:26pm
AIR BLK	.00	8:27pm
ACCY CHK	.08	8:27pm
AIR BLK	.00	8:28pm
SUB TEST	.00	8:29pm
AIR BLK	.00	8:30pm
SUB TEST	.00	8:31pm
AIR BLK	.00	8:32pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR

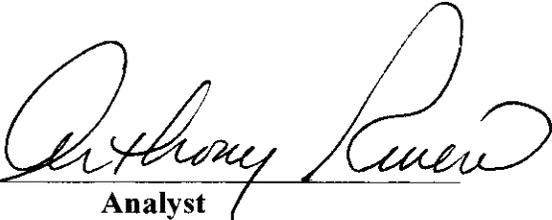

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

NEW HANOVER COUNTY WRIGHTSVILLE BCH PD 640

Serial Number: 008667 Test Record Number: 309
Test Date: 05/21/2009 Test Time: 8:33pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	8:33pm
FLO	Pass	8:33pm
FC	Pass	8:34pm

Temperature Tests

Test	Status	Time
FC1	Pass	8:34pm
SRC	Pass	8:34pm
DET	Pass	8:34pm
BAR	Pass	8:34pm
BT	Pass	8:34pm

Blank Tests

Test	Status	Time
AIR	Pass	8:34pm

Printer Tests

Test	Status	Time
PRNT	Pass	8:34pm

CRC Tests

Test	Status	Time
COMP	Pass	8:34pm
CAL	Pass	8:34pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II**

County New Hanover Instrument Location New Hanover County
Instrument Serial No. 8626 Sheriff's Dept.

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 21 day of May, 20 09 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Anthony Ruess
Signature of Certifying Official

634
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

NEW HANOVER COUNTY NEW HANOVER CO SD
640

Serial Number: 008626
Test Date: 05/21/2009

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: RIVERA, ANTHONY
Permit Number: 08259E
Effective:
12/01/2007-12/01/2009

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test


Lot Number: AG723301
Exp Date: 08/20/2009

Test	g/210L	Time
DIAG	Pass	7:29pm
AIR BLK	.00	7:30pm
ACCY CHK	.07	7:31pm
AIR BLK	.00	7:32pm
SUB TEST	.00	7:32pm
AIR BLK	.00	7:33pm
SUB TEST	.00	7:35pm
AIR BLK	.00	7:35pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR

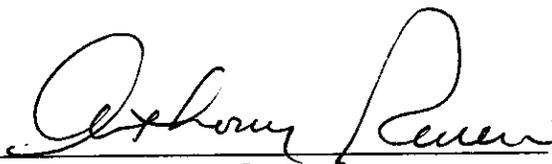
Analyst

Intox EC/IR-II: Preventive Maintenance

NEW HANOVER COUNTY NEW HANOVER CO SD 640

Serial Number: 008626 Test Record Number: 1383
Test Date: 05/21/2009 Test Time: 7:38pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	7:39pm
FLO	Pass	7:39pm
FC	Pass	7:39pm

Temperature Tests

Test	Status	Time
FC1	Pass	7:39pm
SRC	Pass	7:39pm
DET	Pass	7:39pm
BAR	Pass	7:39pm
BT	Pass	7:39pm

Blank Tests

Test	Status	Time
AIR	Pass	7:40pm


Printer Tests

Test	Status	Time
PRNT	Pass	7:40pm

CRC Tests

Test	Status	Time
COMP	Pass	7:40pm
CAL	Pass	7:40pm

Preventive Maintenance
Status: Pass

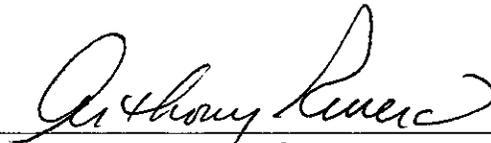

Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH


**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II**

County New Hanover Instrument Location New Hanover County
Instrument Serial No. 8617 Shirley Dept.

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 21 day of May, 2009 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Anthony Rivera
Signature of Certifying Official

634
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

NEW HANOVER COUNTY NEW HANOVER CO SD
640

Serial Number: 008617
Test Date: 05/21/2009

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: RIVERA, ANTHONY
Permit Number: 08259E
Effective:
12/01/2007-12/01/2009

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG723301
Exp Date: 08/20/2009

Test	g/210L	Time
DIAG	Pass	7:29pm
AIR BLK	.00	7:30pm
ACCY CHK	.08	7:30pm
AIR BLK	.00	7:31pm
SUB TEST	.00	7:32pm
AIR BLK	.00	7:33pm
SUB TEST	.00	7:34pm
AIR BLK	.00	7:35pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

Intox EC/IR-II: Preventive Maintenance

NEW HANOVER COUNTY NEW HANOVER CO SD 640

Serial Number: 008617 Test Record Number: 802
Test Date: 05/21/2009 Test Time: 7:37pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	7:37pm
FLO	Pass	7:37pm
FC	Pass	7:37pm

Temperature Tests

Test	Status	Time
FC1	Pass	7:37pm
SRC	Pass	7:37pm
DET	Pass	7:37pm
BAR	Pass	7:37pm
BT	Pass	7:37pm

Blank Tests

Test	Status	Time
AIR	Pass	7:38pm

Printer Tests

Test	Status	Time
PRNT	Pass	7:38pm

CRC Tests

Test	Status	Time
COMP	Pass	7:38pm
CAL	Pass	7:38pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH


**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II**

County Brunswick Instrument Location Brunswick County
Instrument Serial No. 8535 Sherrill Dept.

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 21 day of May, 20 09 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

634
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

BRUNSWICK COUNTY BRUNSWICK CO SD 090

Serial Number: 008585
Test Date: 05/21/2009

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: RIVERA, ANTHONY

Permit Number: 08259E

Effective:

12/01/2007-12/01/2009

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG901901

Exp Date: 01/19/2011


Test	g/210L	Time
DIAG	Pass	6:07pm
AIR BLK	.00	6:08pm
ACCY CHK	.08	6:08pm
AIR BLK	.00	6:09pm
SUB TEST	.00	6:10pm
AIR BLK	.00	6:11pm
SUB TEST	.00	6:14pm
AIR BLK	.00	6:15pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR

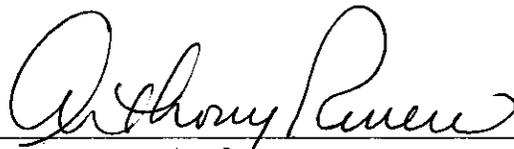

Analyst

Intox EC/IR-II: Preventive Maintenance

BRUNSWICK COUNTY BRUNSWICK CO SD 090

Serial Number: 008585 Test Record Number: 1074
Test Date: 05/21/2009 Test Time: 6:17pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	6:18pm
FLO	Pass	6:18pm
FC	Pass	6:18pm

Temperature Tests

Test	Status	Time
FC1	Pass	6:18pm
SRC	Pass	6:18pm
DET	Pass	6:18pm
BAR	Pass	6:18pm
BT	Pass	6:18pm

Blank Tests

Test	Status	Time
AIR	Pass	6:19pm


Printer Tests

Test	Status	Time
PRNT	Pass	6:19pm

CRC Tests

Test	Status	Time
COMP	Pass	6:19pm
CAL	Pass	6:19pm

Preventive Maintenance
Status: Pass

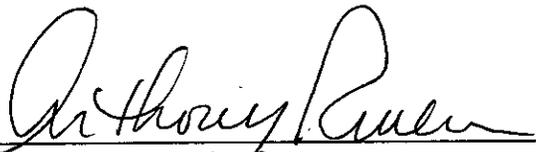

Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II**

County Brunswick Instrument Location Brunswick County
Instrument Serial No. 8602 Sherrill Dept.

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 21 day of May, 20 09 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Anthony Rivera 634
Signature of Certifying Official Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

BRUNSWICK COUNTY BRUNSWICK CO SD 090

Serial Number: 008602
Test Date: 05/21/2009

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: RIVERA, ANTHONY
Permit Number: 08259E
Effective:
12/01/2007-12/01/2009

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG902901
Exp Date: 01/29/2011


Test	g/210L	Time
DIAG	Pass	6:07pm
AIR BLK	.00	6:08pm
ACCY CHK	.08	6:08pm
AIR BLK	.00	6:09pm
SUB TEST	.00	6:10pm
AIR BLK	.00	6:10pm
SUB TEST	.00	6:14pm
AIR BLK	.00	6:15pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR

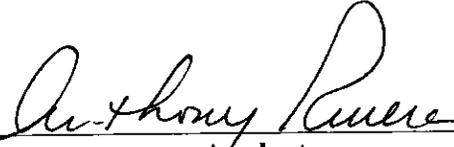

Analyst

Intox EC/IR-II: Preventive Maintenance

BRUNSWICK COUNTY BRUNSWICK CO SD 090

Serial Number: 008602 Test Record Number: 576
Test Date: 05/21/2009 Test Time: 6:17pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	6:17pm
FLO	Pass	6:17pm
FC	Pass	6:17pm

Temperature Tests

Test	Status	Time
FC1	Pass	6:17pm
SRC	Pass	6:17pm
DET	Pass	6:17pm
BAR	Pass	6:17pm
BT	Pass	6:17pm

Blank Tests

Test	Status	Time
AIR	Pass	6:18pm


Printer Tests

Test	Status	Time
PRNT	Pass	6:18pm

CRC Tests

Test	Status	Time
COMP	Pass	6:18pm
CAL	Pass	6:18pm

Preventive Maintenance
Status: Pass

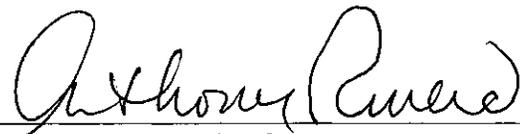

Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II**

County Brunswick Instrument Location Oak Island
Instrument Serial No. 8648 Police Dept.

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 21 day of May, 2009 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Anthony Rivera 634
Signature of Certifying Official Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

BRUNSWICK COUNTY OAK ISLAND PD 090

Serial Number: 008648
Test Date: 05/21/2009

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: RIVERA, ANTHONY
Permit Number: 08259E
Effective:
12/01/2007-12/01/2009

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG723301
Exp Date: 08/20/2009

Test	g/210L	Time
DIAG	Pass	4:16pm
AIR BLK	.00	4:17pm
ACCY CHK	.07	4:18pm
AIR BLK	.00	4:19pm
SUB TEST	.00	4:19pm
AIR BLK	.00	4:20pm
SUB TEST	.00	4:22pm
AIR BLK	.00	4:23pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

Intox EC/IR-II: Preventive Maintenance

BRUNSWICK COUNTY OAK ISLAND PD 090

Serial Number: 008648 Test Record Number: 488
Test Date: 05/21/2009 Test Time: 4:25pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	4:26pm
FLO	Pass	4:26pm
FC	Pass	4:26pm

Temperature Tests

Test	Status	Time
FC1	Pass	4:26pm
SRC	Pass	4:26pm
DET	Pass	4:26pm
BAR	Pass	4:26pm
BT	Pass	4:26pm

Blank Tests

Test	Status	Time
AIR	Pass	4:27pm


Printer Tests

Test	Status	Time
PRNT	Pass	4:27pm

CRC Tests

Test	Status	Time
COMP	Pass	4:27pm
CAL	Pass	4:27pm

Preventive Maintenance
Status: Pass

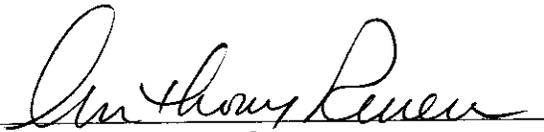

Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH


**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II**

County Rockingham Instrument Location Eden Police
Instrument Serial No. 008636 DEPARTMENT

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 21 day of MAY, 20 09 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



L. Kevin Dean
Signature of Certifying Official

642
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

ROCKINGHAM COUNTY EDEN PD 780

Serial Number: 008636
Test Date: 05/21/2009

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: DEAN, LARRY K
Permit Number: 11598E
Effective:
12/01/2007-12/01/2009

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG722701-07
Exp Date: 08/14/2009


Test	g/210L	Time
DIAG	Pass	2:10pm
AIR BLK	.00	2:11pm
ACCY CHK	.07	2:12pm
AIR BLK	.00	2:13pm
SUB TEST	.00	2:13pm
AIR BLK	.00	2:14pm
SUB TEST	.00	2:16pm
AIR BLK	.00	2:17pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

Intox EC/IR-II: Preventive Maintenance

ROCKINGHAM COUNTY EDEN PD 780

Serial Number: 008636 Test Record Number: 562
Test Date: 05/21/2009 Test Time: 2:17pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	2:17pm
FLO	Pass	2:17pm
FC	Pass	2:18pm

Temperature Tests

Test	Status	Time
FC1	Pass	2:18pm
SRC	Pass	2:18pm
DET	Pass	2:18pm
BAR	Pass	2:18pm
BT	Pass	2:18pm

Blank Tests

Test	Status	Time
AIR	Pass	2:18pm


Printer Tests

Test	Status	Time
PRNT	Pass	2:18pm

CRC Tests

Test	Status	Time
COMP	Pass	2:18pm
CAL	Pass	2:18pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II**


County Guilford Instrument Location High Point Jail

Instrument Serial No. 008655

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 12 day of May, 2009 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

642
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

GUILFORD COUNTY HIGH POINT JAIL 401

Serial Number: 008655
Test Date: 05/12/2009

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: DEAN, LARRY K
Permit Number: 11598E
Effective:
12/01/2007-12/01/2009

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test


Lot Number: AG902001
Exp Date: 01/20/2011

Test	g/210L	Time
DIAG	Pass	2:29pm
AIR BLK	.00	2:30pm
ACCY CHK	.08	2:31pm
AIR BLK	.00	2:32pm
SUB TEST	.00	2:32pm
AIR BLK	.00	2:33pm
SUB TEST	.00	2:35pm
AIR BLK	.00	2:35pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

Intox EC/IR-II: Preventive Maintenance

GUILFORD COUNTY HIGH POINT JAIL 401

Serial Number: 008655 Test Record Number: 773
Test Date: 05/12/2009 Test Time: 2:36pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	2:36pm
FLO	Pass	2:36pm
FC	Pass	2:36pm

Temperature Tests

Test	Status	Time
FC1	Pass	2:37pm
SRC	Pass	2:37pm
DET	Pass	2:37pm
BAR	Pass	2:37pm
BT	Pass	2:37pm

Blank Tests

Test	Status	Time
AIR	Pass	2:37pm


Printer Tests

Test	Status	Time
PRNT	Pass	2:37pm

CRC Tests

Test	Status	Time
COMP	Pass	2:37pm
CAL	Pass	2:37pm

Preventive Maintenance
Status: Pass

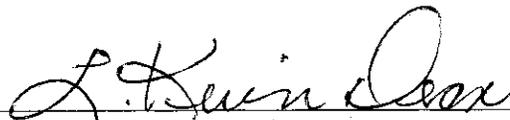

Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II**

County Guilford Instrument Location High Point Jail

Instrument Serial No. 008718

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 12 day of May, 20 09 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

642
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

GUILFORD COUNTY HIGH POINT JAIL 401

Serial Number: 008718
Test Date: 05/12/2009

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: *DEAN, LARRY K*
Permit Number: 11598E
Effective:
12/01/2007-12/01/2009

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG902001
Exp Date: 01/20/2011


Test	g/210L	Time
DIAG	Pass	2:10pm
AIR BLK	.00	2:11pm
ACCY CHK	.08	2:11pm
AIR BLK	.00	2:12pm
SUB TEST	.00	2:12pm
AIR BLK	.00	2:13pm
SUB TEST	.00	2:15pm
AIR BLK	.00	2:16pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

Intox EC/IR-II: Preventive Maintenance

GUILFORD COUNTY HIGH POINT JAIL 401

Serial Number: 008718 Test Record Number: 125
Test Date: 05/12/2009 Test Time: 2:17pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	2:18pm
FLO	Pass	2:18pm
FC	Pass	2:18pm

Temperature Tests

Test	Status	Time
FC1	Pass	2:18pm
SRC	Pass	2:18pm
DET	Pass	2:18pm
BAR	Pass	2:18pm
BT	Pass	2:18pm

Blank Tests

Test	Status	Time
AIR	Pass	2:18pm


Printer Tests

Test	Status	Time
PRNT	Pass	2:18pm

CRC Tests

Test	Status	Time
COMP	Pass	2:19pm
CAL	Pass	2:19pm

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH


**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II**

County Guilford Instrument Location Greensboro Police
Instrument Serial No. 008725 Department

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 11 day of May, 2009 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

642
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

GUILFORD COUNTY GREENSBORO PD 400

Serial Number: 008725
Test Date: 05/11/2009

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: DEAN, LARRY K
Permit Number: 11598E
Effective:
12/01/2007-12/01/2009

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test


Lot Number: AG816303
Exp Date: 06/11/2010

Test	g/210L	Time
DIAG	Pass	3:53pm
AIR BLK	.00	3:54pm
ACCY CHK	.07	3:55pm
AIR BLK	.00	3:56pm
SUB TEST	.00	3:56pm
AIR BLK	.00	3:57pm
SUB TEST	.00	3:59pm
AIR BLK	.00	4:00pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

GUILFORD COUNTY GREENSBORO PD 400

Serial Number: 008725 Test Record Number: 696
Test Date: 05/11/2009 Test Time: 4:00pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	4:01pm
FLO	Pass	4:01pm
FC	Pass	4:01pm

Temperature Tests

Test	Status	Time
FC1	Pass	4:01pm
SRC	Pass	4:01pm
DET	Pass	4:01pm
BAR	Pass	4:01pm
BT	Pass	4:01pm

Blank Tests

Test	Status	Time
AIR	Pass	4:02pm


Printer Tests

Test	Status	Time
PRNT	Pass	4:02pm

CRC Tests

Test	Status	Time
COMP	Pass	4:02pm
CAL	Pass	4:02pm

Preventive Maintenance
Status: Pass

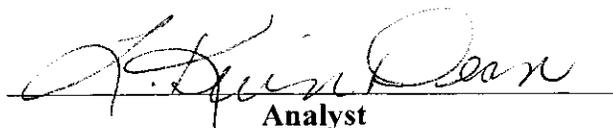
Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH


**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II**

County Rowan Instrument Location Salisbury Police
Instrument Serial No. 008835 Department

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 5 day of MAY, 2009 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

642
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

ROWAN COUNTY SALISBURY PD 790

Serial Number: 008835
Test Date: 05/05/2009

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: DEAN, LARRY K
Permit Number: 11598E
Effective:
12/01/2007-12/01/2009

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test


Lot Number: AG816303
Exp Date: 06/11/2010

Test	g/210L	Time
DIAG	Pass	4:42pm
AIR BLK	.00	4:43pm
ACCY CHK	.07	4:43pm
AIR BLK	.00	4:44pm
SUB TEST	.00	4:45pm
AIR BLK	.00	4:46pm
SUB TEST	.00	4:47pm
AIR BLK	.00	4:48pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR.


Analyst

Intox EC/IR-II: Preventive Maintenance

ROWAN COUNTY SALISBURY PD 790

Serial Number: 008835 Test Record Number: 245
Test Date: 05/05/2009 Test Time: 4:49pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	4:49pm
FLO	Pass	4:49pm
FC	Pass	4:49pm

Temperature Tests

Test	Status	Time
FC1	Pass	4:49pm
SRC	Pass	4:49pm
DET	Pass	4:49pm
BAR	Pass	4:49pm
BT	Pass	4:49pm

Blank Tests

Test	Status	Time
AIR	Pass	4:50pm


Printer Tests

Test	Status	Time
PRNT	Pass	4:50pm

CRC Tests

Test	Status	Time
COMP	Pass	4:50pm
CAL	Pass	4:50pm

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II**


County BOWAN Instrument Location Salisbury Police

Instrument Serial No. 0088168 DEPARTMENT

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 5 day of MAY, 2009 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

642
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

ROWAN COUNTY SALISBURY PD 790

Serial Number: 008868
Test Date: 05/05/2009

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE

Analyst's Name: DEAN, LARRY K
Permit Number: 11598E
Effective:
12/01/2007-12/01/2009

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test


Lot Number: AG816303
Exp Date: 06/11/2010

Test	g/210L	Time
DIAG	Pass	4:21pm
AIR BLK	.00	4:22pm
ACCY CHK	.07	4:22pm
AIR BLK	.00	4:23pm
SUB TEST	.00	4:24pm
AIR BLK	.00	4:24pm
SUB TEST	.00	4:26pm
AIR BLK	.00	4:27pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

Intox EC/IR-II: Preventive Maintenance

ROWAN COUNTY SALISBURY PD 790

Serial Number: 008868 Test Record Number: 435
Test Date: 05/05/2009 Test Time: 4:28pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	4:28pm
FLO	Pass	4:28pm
FC	Pass	4:28pm

Temperature Tests

Test	Status	Time
FC1	Pass	4:28pm
SRC	Pass	4:28pm
DET	Pass	4:28pm
BAR	Pass	4:28pm
BT	Pass	4:28pm

Blank Tests

Test	Status	Time
AIR	Pass	4:29pm


Printer Tests

Test	Status	Time
PRNT	Pass	4:29pm

CRC Tests

Test	Status	Time
COMP	Pass	4:29pm
CAL	Pass	4:29pm

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II**


County Wake Instrument Location But mobile unit

Instrument Serial No. 008600 Rabona

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 16th day of May, 2009 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

636
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Preventive Maintenance

WAKE COUNTY BAT MOBILE UNIT 5 910

Serial Number: 008600 Test Record Number: 471
Test Date: 05/16/2009 Test Time: 10:18pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	10:18pm
FLO	Pass	10:18pm
FC	Pass	10:18pm

Temperature Tests

Test	Status	Time
FC1	Pass	10:18pm
SRC	Pass	10:18pm
DET	Pass	10:18pm
BAR	Pass	10:18pm
BT	Pass	10:18pm

Blank Tests

Test	Status	Time
AIR	Pass	10:19pm


Printer Tests

Test	Status	Time
PRNT	Pass	10:19pm

CRC Tests

Test	Status	Time
COMP	Pass	10:19pm
CAL	Pass	10:19pm

Preventive Maintenance
Status: Pass

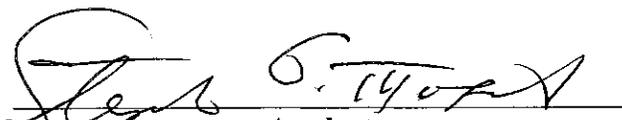
Analyst

Intox EC/IR-II: Subject Test

WAKE COUNTY BAT MOBILE UNIT 5 910

Serial Number: 008600
Test Date: 05/16/2009

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: MORGART, STEPHEN G
Permit Number: 09372E
Effective:
12/01/2007-12/01/2009

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test


Lot Number: AG723401
Exp Date: 08/21/2009

Test	g/210L	Time
DIAG	Pass	10:09pm
AIR BLK	.00	10:10pm
ACCY CHK	.07	10:10pm
AIR BLK	.00	10:11pm
SUB TEST	.00	10:12pm
AIR BLK	.00	10:13pm
SUB TEST	.00	10:15pm
AIR BLK	.00	10:15pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II**


County Wake Instrument Location BAT Insub. Lab #5

Instrument Serial No. 208758 Radiation

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 16th day of May, 2009 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

636
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Preventive Maintenance

WAKE COUNTY BAT MOBILE UNIT 5 910

Serial Number: 008788 Test Record Number: 188
Test Date: 05/16/2009 Test Time: 10:37pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	10:38pm
FLO	Pass	10:38pm
FC	Pass	10:38pm

Temperature Tests

Test	Status	Time
FC1	Pass	10:38pm
SRC	Pass	10:38pm
DET	Pass	10:38pm
BAR	Pass	10:38pm
BT	Pass	10:38pm

Blank Tests

Test	Status	Time
AIR	Pass	10:38pm


Printer Tests

Test	Status	Time
PRNT	Pass	10:38pm

CRC Tests

Test	Status	Time
COMP	Pass	10:39pm
CAL	Pass	10:39pm

Preventive Maintenance
Status: Pass


Analyst

Intox EC/IR-II: Subject Test . . .

WAKE COUNTY BAT MOBILE UNIT 5 910

Serial Number: 008788
Test Date: 05/16/2009

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: MORGART, STEPHEN G
Permit Number: 09372E
Effective:
12/01/2007-12/01/2009

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test


Lot Number: AG904903
Exp Date: 02/18/2011

Test	g/210L	Time
DIAG	Pass	10:28pm
AIR BLK	.00	10:28pm
ACCY CHK	.08	10:29pm
AIR BLK	.00	10:29pm
SUB TEST	.00	10:31pm
AIR BLK	.00	10:32pm
SUB TEST	.00	10:33pm
AIR BLK	.00	10:34pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH


**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II**

County Wake Instrument Location B&E mobile unit #5
Instrument Serial No. 008698 PA10144

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 16TH day of MAY, 2009 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]

Signature of Certifying Official

636

Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Preventive Maintenance

WAKE COUNTY BAT MOBILE UNIT 5 910

Serial Number: 008698 Test Record Number: 319
Test Date: 05/16/2009 Test Time: 10:17pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	10:17pm
FLO	Pass	10:17pm
FC	Pass	10:17pm

Temperature Tests

Test	Status	Time
FC1	Pass	10:18pm
SRC	Pass	10:18pm
DET	Pass	10:18pm
BAR	Pass	10:18pm
BT	Pass	10:18pm

Blank Tests

Test	Status	Time
AIR	Pass	10:18pm


Printer Tests

Test	Status	Time
PRNT	Pass	10:18pm

CRC Tests

Test	Status	Time
COMP	Pass	10:18pm
CAL	Pass	10:18pm

Preventive Maintenance
Status: Pass

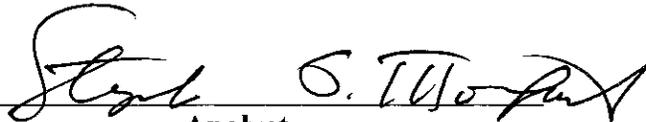

Analyst

Intox EC/IR-II: Subject Test

WAKE COUNTY BAT MOBILE UNIT 5 910

Serial Number: 008698
Test Date: 05/16/2009

Citation Number: M0000000-0
Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: MORGART, STEPHEN G

Permit Number: 09372E

Effective:

12/01/2007-12/01/2009

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG723401

Exp Date: 08/21/2009

Test	g/210L	Time
DIAG	Pass	10:05pm
AIR BLK	.00	10:06pm
ACCY CHK	.07	10:06pm
AIR BLK	.00	10:07pm
SUB TEST	.00	10:08pm
AIR BLK	.00	10:09pm
SUB TEST	.00	10:11pm
AIR BLK	.00	10:11pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II**


County CHATHAM Instrument Location BAT MOBILE UNIT #5

Instrument Serial No. 008698

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 15TH day of MAY, 2009 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Steph O. Thomas
Signature of Certifying Official

636
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Preventive Maintenance

CHATHAM COUNTY BAT MOBILE UNIT 5 180

Serial Number: 008698 Test Record Number: 316
Test Date: 05/15/2009 Test Time: 11:52pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	11:53pm
FLO	Pass	11:53pm
FC	Pass	11:53pm

Temperature Tests

Test	Status	Time
FC1	Pass	11:53pm
SRC	Pass	11:53pm
DET	Pass	11:53pm
BAR	Pass	11:53pm
BT	Pass	11:53pm

Blank Tests

Test	Status	Time
AIR	Pass	11:54pm


Printer Tests

Test	Status	Time
PRNT	Pass	11:54pm

CRC Tests

Test	Status	Time
COMP	Pass	11:54pm
CAL	Pass	11:54pm

Preventive Maintenance
Status: Pass



Analyst

Intox EC/IR-II: Subject Test

CHATHAM COUNTY BAT MOBILE UNIT 5 180

Serial Number: 008698
Test Date: 05/15/2009

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: MORGART, STEPHEN G

Permit Number: 09372E

Effective:

12/01/2007-12/01/2009

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG723401


Exp Date: 08/21/2009

Test	g/210L	Time
DIAG	Pass	11:43pm
AIR BLK	.00	11:44pm
ACCY CHK	.07	11:45pm
AIR BLK	.00	11:46pm
SUB TEST	.00	11:46pm
AIR BLK	.00	11:47pm
SUB TEST	.00	11:49pm
AIR BLK	.00	11:50pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH


**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II**

County ROBESON Instrument Location ST. PAULS
Instrument Serial No. 008814 Police Dept.

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 12 day of MAY, 2009 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Paul I. Cummings
Signature of Certifying Official

528
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

ROBESON ST. PAULS PD. 770

Serial Number: 008814
Test Date: 05/12/2009

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: SIMMONS, PAUL T

Permit Number: 08619E

Effective:

12/01/2007-12/01/2009

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG814101

Exp Date: 05/20/2010


Test	g/210L	Time
DIAG	Pass	1:19pm
AIR BLK	.00	1:19pm
ACCY CHK	.07	1:20pm
AIR BLK	.00	1:21pm
SUB TEST	.00	1:21pm
AIR BLK	.00	1:22pm
SUB TEST	.00	1:24pm
AIR BLK	.00	1:25pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

Intox EC/IR-II: Preventive Maintenance

ROBESON ST. PAULS PD. 770

Serial Number: 008814 Test Record Number: 104
Test Date: 05/12/2009 Test Time: 1:26pm EDT

System Check: Passed

Baseline Tests

Test	Status	Time
IR	Pass	1:26pm
FLO	Pass	1:26pm
FC	Pass	1:26pm

Temperature Tests

Test	Status	Time
FC1	Pass	1:27pm
SRC	Pass	1:27pm
DET	Pass	1:27pm
BAR	Pass	1:27pm
BT	Pass	1:27pm

Blank Tests

Test	Status	Time
AIR	Pass	1:27pm

Printer Tests

Test	Status	Time
PRNT	Pass	1:27pm

CRC Tests

Test	Status	Time
COMP	Pass	1:27pm
CAL	Pass	1:27pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH


**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II**

County ROBESON Instrument Location LUMBERTON
Instrument Serial No. 008805 LEC.

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 12 day of MAY, 2009 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Paul T. [Signature]
Signature of Certifying Official

578
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

ROBESON LUMBERTON, LEC 770

Serial Number: 008805

Test Date: 05/12/2009

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: SIMMONS, PAUL T

Permit Number: 08619E

Effective:

12/01/2007-12/01/2009

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG902603

Exp Date: 10/02/2011

Test	g/210L	Time
DIAG	Pass	2:47pm
AIR BLK	.00	2:47pm
ACCY CHK	.08	2:48pm
AIR BLK	.00	2:49pm
SUB TEST	.00	2:49pm
AIR BLK	.00	2:50pm
SUB TEST	.00	2:52pm
AIR BLK	.00	2:53pm

Reported AC: 00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

Intox EC/IR-II: Preventive Maintenance

ROBESON LUMBERTON, LEC 770

Serial Number: 008805 Test Record Number: 427
Test Date: 05/12/2009 Test Time: 2:54pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	2:55pm
FLO	Pass	2:55pm
FC	Pass	2:55pm

Temperature Tests

Test	Status	Time
FC1	Pass	2:55pm
SRC	Pass	2:55pm
DET	Pass	2:55pm
BAR	Pass	2:55pm
BT	Pass	2:55pm

Blank Tests

Test	Status	Time
AIR	Pass	2:56pm

Printer Tests

Test	Status	Time
PRNT	Pass	2:56pm

CRC Tests

Test	Status	Time
COMP	Pass	2:56pm
CAL	Pass	2:56pm

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH


**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II**

County ROBESON Instrument Location RED SPRINGS
Instrument Serial No. 008857 POLICE DEPT.

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 13 day of MAY, 2009 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Paul T. [Signature]
Signature of Certifying Official

578
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

ROBESON RED SPRINGS PD 770

Serial Number: 008857
Test Date: 05/13/2009

Citation Number: M0000000-0
Subject's Name:

PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE

Analyst's Name: SIMMONS, PAUL T
Permit Number: 08619E
Effective:
12/01/2007-12/01/2009

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG814101
Exp Date: 05/20/2010

Test	g/210L	Time
DIAG	Pass	10:49am
AIR BLK	.00	10:50am
ACCY CHK	.07	10:51am
AIR BLK	.00	10:52am
SUB TEST	.00	10:52am
AIR BLK	.00	10:53am
SUB TEST	.00	10:55am
AIR BLK	.00	10:56am

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

Intox EC/IR-II: Preventive Maintenance

ROBESON RED SPRINGS PD 770

Serial Number: 008857 Test Record Number: 67
Test Date: 05/13/2009 Test Time: 10:58am EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	10:58am
FLO	Pass	10:58am
FC	Pass	10:58am

Temperature Tests

Test	Status	Time
FC1	Pass	10:58am
SRC	Pass	10:58am
DET	Pass	10:58am
BAR	Pass	10:58am
BT	Pass	10:58am

Blank Tests

Test	Status	Time
AIR	Pass	10:59am

Printer Tests

Test	Status	Time
PRNT	Pass	10:59am

CRC Tests

Test	Status	Time
COMP	Pass	10:59am
CAL	Pass	10:59am

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH


**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II**

County Robeson Instrument Location Lumberton,
Instrument Serial No. 008836 LEC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 13 day of MAY, 2009 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Paul T. Simon
Signature of Certifying Official

578
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

ROBESON LUMBERTON, LEC 770

Serial Number: 008836
Test Date: 05/13/2009

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE

Analyst's Name: SIMMONS, PAUL T
Permit Number: 08619E
Effective:
12/01/2007-12/01/2009

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG902603
Exp Date: 01/26/2011

Test	g/210L	Time
DIAG	Pass	1:37pm
AIR BLK	.00	1:38pm
ACCY CHK	.08	1:38pm
AIR BLK	.00	1:39pm
SUB TEST	.00	1:40pm
AIR BLK	.00	1:40pm
SUB TEST	.00	1:42pm
AIR BLK	.00	1:43pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

Intox EC/IR-II: Preventive Maintenance

ROBESON LUMBERTON, LEC 770

Serial Number: 008836 Test Record Number: 393
Test Date: 05/13/2009 Test Time: 1:51pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	1:52pm
FLO	Pass	1:52pm
FC	Pass	1:52pm

Temperature Tests

Test	Status	Time
FC1	Pass	1:52pm
SRC	Pass	1:52pm
DET	Pass	1:52pm
BAR	Pass	1:52pm
BT	Pass	1:52pm

Blank Tests

Test	Status	Time
AIR	Pass	1:53pm

Printer Tests

Test	Status	Time
PRNT	Pass	1:53pm

CRC Tests

Test	Status	Time
COMP	Pass	1:53pm
CAL	Pass	1:53pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II**

County LEE Instrument Location SANFORD POLICE

Instrument Serial No. 008867 DEPT. SANFORD, NC.

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 14 day of MAY, 2009 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Paul J. [Signature] 578

Signature of Certifying Official

Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

LEE COUNTY SANFORD POLICE DEPT 520

Serial Number: 008867
Test Date: 05/14/2009

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: SIMMONS, PAUL T

Permit Number: 08619E

Effective:

12/01/2007-12/01/2009

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG825401


Exp Date: 10/02/2011

Test	g/210L	Time
DIAG	Pass	9:47am
AIR BLK	.00	9:48am
ACCY CHK	.07	9:48am
AIR BLK	.00	9:49am
SUB TEST	.00	9:50am
AIR BLK	.00	9:51am
SUB TEST	.00	9:52am
AIR BLK	.00	9:53am

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR.


Analyst

Intox EC/IR-II: Preventive Maintenance

LEE COUNTY SANFORD POLICE DEPT 520

Serial Number: 008867 Test Record Number: 54
Test Date: 05/14/2009 Test Time: 9:54am EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	9:55am
FLO	Pass	9:55am
FC	Pass	9:55am

Temperature Tests

Test	Status	Time
FC1	Pass	9:55am
SRC	Pass	9:55am
DET	Pass	9:55am
BAR	Pass	9:55am
BT	Pass	9:55am

Blank Tests

Test	Status	Time
AIR	Pass	9:55am

Printer Tests

Test	Status	Time
PRNT	Pass	9:55am

CRC Tests

Test	Status	Time
COMP	Pass	9:56am
CAL	Pass	9:56am

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH


**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II**

County Alexander Instrument Location Alexander County SD
Instrument Serial No. 008813 29 W. Main Avenue, Taylorsville
828-632-4658

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 7th day of May, 2009 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Joseph E. Hutchinson
Signature of Certifying Official

650
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

ALEXANDER COUNTY ALEXANDER COUNTY SD
010

Serial Number: 008813
Test Date: 05/07/2009

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: HUTCHINSON, JOSEPH E
Permit Number: 19951E
Effective:
12/01/2007-12/01/2009

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test


Lot Number: AG723301
Exp Date: 08/20/2009

Test	g/210L	Time
DIAG	Pass	4:24pm
AIR BLK	.00	4:24pm
ACCY CHK	.08	4:25pm
AIR BLK	.00	4:26pm
SUB TEST	.00	4:26pm
AIR BLK	.00	4:27pm
SUB TEST	.00	4:29pm
AIR BLK	.00	4:30pm

Reported AC: .00 g/210L

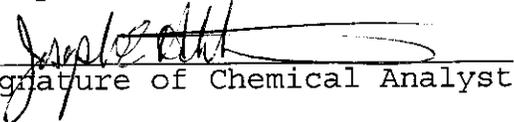
Signature of Chemical Analyst

Court CVR

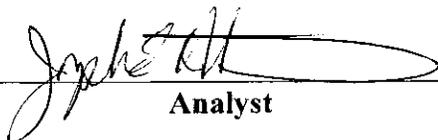
Analyst

Intox EC/IR-II: Preventive Maintenance

ALEXANDER COUNTY ALEXANDER COUNTY SD 010

Serial Number: 008813 Test Record Number: 289
Test Date: 05/07/2009 Test Time: 4:20pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	4:21pm
FLO	Pass	4:21pm
FC	Pass	4:21pm

Temperature Tests

Test	Status	Time
FC1	Pass	4:21pm
SRC	Pass	4:21pm
DET	Pass	4:21pm
BAR	Pass	4:21pm
BT	Pass	4:21pm

Blank Tests

Test	Status	Time
AIR	Pass	4:22pm


Printer Tests

Test	Status	Time
PRNT	Pass	4:22pm

CRC Tests

Test	Status	Time
COMP	Pass	4:22pm
CAL	Pass	4:22pm

Preventive Maintenance
Status: Pass

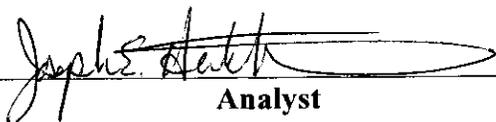
Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH


**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II**

County Duplin Instrument Location WALLACE
Instrument Serial No. 8858 Police Dept.

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 21 day of May, 20 09 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Anthony Rivera

Signature of Certifying Official

634

Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

DUPLIN COUNTY WALLACE PD 300

Serial Number: 008858
Test Date: 05/21/2009

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: *RIVERA, ANTHONY*
Permit Number: 08259E
Effective:
12/01/2007-12/01/2009

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG814101
Exp Date: 05/20/2010

Test	g/210L	Time
DIAG	Pass	12:47pm
AIR BLK	.00	12:48pm
ACCY CHK	.07	12:49pm
AIR BLK	.00	12:50pm
SUB TEST	.00	12:50pm
AIR BLK	.00	12:51pm
SUB TEST	.00	12:55pm
AIR BLK	.00	12:56pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

Intox EC/IR-II: Preventive Maintenance

DUPLIN COUNTY WALLACE PD 300

Serial Number: 008858 Test Record Number: 152
Test Date: 05/21/2009 Test Time: 12:58pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	12:58pm
FLO	Pass	12:58pm
FC	Pass	12:58pm

Temperature Tests

Test	Status	Time
FC1	Pass	12:58pm
SRC	Pass	12:58pm
DET	Pass	12:58pm
BAR	Pass	12:58pm
BT	Pass	12:58pm

Blank Tests

Test	Status	Time
AIR	Pass	12:59pm


Printer Tests

Test	Status	Time
PRNT	Pass	12:59pm

CRC Tests

Test	Status	Time
COMP	Pass	12:59pm
CAL	Pass	12:59pm

Preventive Maintenance
Status: Pass

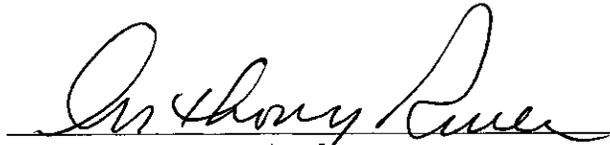
Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II**


County HALIFAX Instrument Location HALIFAX CO. SHERIFF DEPT

Instrument Serial No. 008695 FERRER LN HALIFAX, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 26 day of MAY, 2009 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

652
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

HALIFAX CO. HALIFAX CO. SD 410

Serial Number: 008695
Test Date: 05/26/2009

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name:
QUARANTELLA, NICHOLAS J
Permit Number: 21536E
Effective:
01/01/2008-01/01/2010

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG816302
Exp Date: 06/11/2010

Test	g/210L	Time
DIAG	Pass	1:25pm
AIR BLK	.00	1:26pm
ACCY CHK	.08	1:26pm
AIR BLK	.00	1:27pm
SUB TEST	.00	1:28pm
AIR BLK	.00	1:29pm
SUB TEST	.00	1:30pm
AIR BLK	.00	1:31pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

Intox EC/IR-II: Preventive Maintenance

HALIFAX CO. HALIFAX CO. SD 410

Serial Number: 008695 Test Record Number: 362
Test Date: 05/26/2009 Test Time: 1:32pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	1:33pm
FLO	Pass	1:33pm
FC	Pass	1:33pm

Temperature Tests

Test	Status	Time
FC1	Pass	1:33pm
SRC	Pass	1:33pm
DET	Pass	1:33pm
BAR	Pass	1:33pm
BT	Pass	1:33pm

Blank Tests

Test	Status	Time
AIR	Pass	1:33pm


Printer Tests

Test	Status	Time
PRNT	Pass	1:33pm

CRC Tests

Test	Status	Time
COMP	Pass	1:34pm
CAL	Pass	1:34pm

Preventive Maintenance
Status: Pass

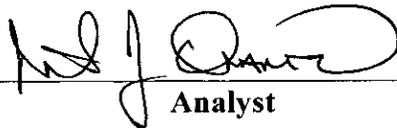

Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II**

County NORTHAMPTON

Instrument Location NORTHAMPTON CO. SHERIFFS DEPT

Instrument Serial No. 008688 105 W. JEFFERSON ST. JACKSON, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 26 day of MAY, 2009 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

652
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

NORTHAMPTON COUNTY SHERIFFS DEPARTMENT
650

Serial Number: 008688
Test Date: 05/26/2009

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name:
QUARANTELLA, NICHOLAS J
Permit Number: 21536E
Effective:
01/01/2008-01/01/2010

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test


Lot Number: AG723401
Exp Date: 08/21/2009

Test	g/210L	Time
DIAG	Pass	11:44am
AIR BLK	.00	11:45am
ACCY CHK	.07	11:46am
AIR BLK	.00	11:47am
SUB TEST	.00	11:47am
AIR BLK	.00	11:48am
SUB TEST	.00	11:49am
AIR BLK	.00	11:50am

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR

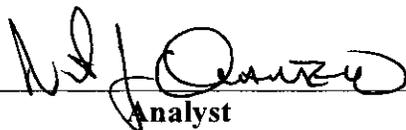
Analyst

Intox EC/IR-II: Preventive Maintenance

NORTHAMPTON COUNTY SHERIFFS DEPARTMENT 650

Serial Number: 008688 Test Record Number: 396
Test Date: 05/26/2009 Test Time: 11:54am EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	11:54am
FLO	Pass	11:54am
FC	Pass	11:54am

Temperature Tests

Test	Status	Time
FC1	Pass	11:55am
SRC	Pass	11:55am
DET	Pass	11:55am
BAR	Pass	11:55am
BT	Pass	11:55am

Blank Tests

Test	Status	Time
AIR	Pass	11:55am


Printer Tests

Test	Status	Time
PRNT	Pass	11:55am

CRC Tests

Test	Status	Time
COMP	Pass	11:55am
CAL	Pass	11:55am

Preventive Maintenance
Status: Pass

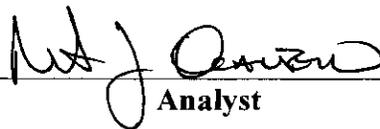

Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II**


County NORTHAMPTON Instrument Location NORTHAMPTON CO SHERIFFS DEPT

Instrument Serial No. 008607 105 W. JEFFERSON ST, JACKSON, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 26 day of MAY, 2009 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

652
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

NORTHAMPTON COUNTY SHERIFFS DEPARTMENT
650

Serial Number: 008607
Test Date: 05/26/2009

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE

Analyst's Name:
QUARANTELLA, NICHOLAS J
Permit Number: 21536E
Effective:
01/01/2008-01/01/2010

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG723401
Exp Date: 08/21/2009

Test	g/210L	Time
DIAG	Pass	11:43am
AIR BLK	.00	11:44am
ACCY CHK	.07	11:45am
AIR BLK	.00	11:46am
SUB TEST	.00	11:46am
AIR BLK	.00	11:47am
SUB TEST	.00	11:48am
AIR BLK	.00	11:49am

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

NORTHAMPTON COUNTY SHERIFFS DEPARTMENT 650

Serial Number: 008607 Test Record Number: 478
Test Date: 05/26/2009 Test Time: 11:51am EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	11:51am
FLO	Pass	11:51am
FC	Pass	11:51am

Temperature Tests

Test	Status	Time
FC1	Pass	11:51am
SRC	Pass	11:51am
DET	Pass	11:51am
BAR	Pass	11:51am
BT	Pass	11:51am

Blank Tests

Test	Status	Time
AIR	Pass	11:52am


Printer Tests

Test	Status	Time
PRNT	Pass	11:52am

CRC Tests

Test	Status	Time
COMP	Pass	11:52am
CAL	Pass	11:52am

Preventive Maintenance
Status: Pass

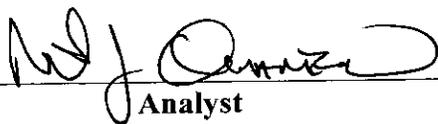

Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II**

County HALIFAX Instrument Location ROANOKE RAPIDS, PD

Instrument Serial No. 008635 1040 ROANOKE AVE. ROANOKE RAPIDS, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 26 day of MAY, 2009 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

650
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

HALIFAX CO ROANOKE RAPIDS PD 410

Serial Number: 008635
Test Date: 05/26/2009

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name:
QUARANTELLA, NICHOLAS J
Permit Number: 21536E
Effective:
01/01/2008-01/01/2010

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG722503
Exp Date: 08/12/2009


Test	g/210L	Time
DIAG	Pass	10:38am
AIR BLK	.00	10:39am
ACCY CHK	.07	10:40am
AIR BLK	.00	10:40am
SUB TEST	.00	10:41am
AIR BLK	.00	10:42am
SUB TEST	.00	10:44am
AIR BLK	.00	10:44am

Reported AC: .00 g/210L

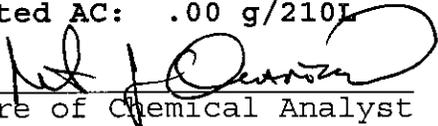

Signature of Chemical Analyst

Court CVR

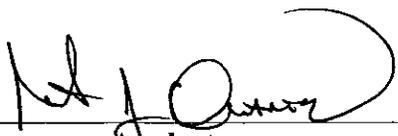

Analyst

Intox EC/IR-II: Preventive Maintenance

HALIFAX CO ROANOKE RAPIDS PD 410

Serial Number: 008635 Test Record Number: 414
Test Date: 05/26/2009 Test Time: 10:46am EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	10:46am
FLO	Pass	10:46am
FC	Pass	10:46am

Temperature Tests

Test	Status	Time
FC1	Pass	10:46am
SRC	Pass	10:46am
DET	Pass	10:46am
BAR	Pass	10:46am
BT	Pass	10:46am

Blank Tests

Test	Status	Time
AIR	Pass	10:47am


Printer Tests

Test	Status	Time
PRNT	Pass	10:47am

CRC Tests

Test	Status	Time
COMP	Pass	10:47am
CAL	Pass	10:47am

Preventive Maintenance
Status: Pass

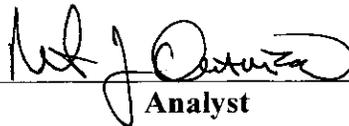

Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II**

County HALIFAX Instrument Location ROANOKE, RAPIDS PD
Instrument Serial No. 008656 1040 ROANOKE AVE, ROANOKE RAPIDS,
NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 26 day of MAY, 2009 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

652
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

HALIFAX CO. ROANOKE RAPIDS PD 410

Serial Number: 008656
Test Date: 05/26/2009

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name:
QUARANTELLA, NICHOLAS J
Permit Number: 21536E
Effective:
01/01/2008-01/01/2010

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG722702
Exp Date: 08/14/2009

Test	g/210L	Time
DIAG	Pass	10:39am
AIR BLK	.00	10:40am
ACCY CHK	.07	10:41am
AIR BLK	.00	10:42am
SUB TEST	.00	10:42am
AIR BLK	.00	10:43am
SUB TEST	.00	10:44am
AIR BLK	.00	10:45am

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

Intox EC/IR-II: Preventive Maintenance

HALIFAX CO. ROANOKE RAPIDS PD 410

Serial Number: 008656 Test Record Number: 255
Test Date: 05/26/2009 Test Time: 10:47am EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	10:47am
FLO	Pass	10:47am
FC	Pass	10:47am

Temperature Tests

Test	Status	Time
FC1	Pass	10:47am
SRC	Pass	10:47am
DET	Pass	10:47am
BAR	Pass	10:47am
BT	Pass	10:47am

Blank Tests

Test	Status	Time
AIR	Pass	10:48am

Printer Tests

Test	Status	Time
PRNT	Pass	10:48am

CRC Tests

Test	Status	Time
COMP	Pass	10:48am
CAL	Pass	10:48am

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II**

County WAKE Instrument Location CARY P.D.

Instrument Serial No. 008587 100 WILKINSON AVE. CARY, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 22 day of MAY, 2009 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

652
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

WAKE COUNTY CARY PD 910

Serial Number: 008587
Test Date: 05/22/2009

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name:

QUARANTELLA, NICHOLAS J

Permit Number: 21536E

Effective:

01/01/2008-01/01/2010

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG723401


Exp Date: 08/21/2009

Test	g/210L	Time
DIAG	Pass	11:25am
AIR BLK	.00	11:26am
ACCY CHK	.07	11:27am
AIR BLK	.00	11:28am
SUB TEST	.00	11:28am
AIR BLK	.00	11:29am
SUB TEST	.00	11:30am
AIR BLK	.00	11:31am

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR

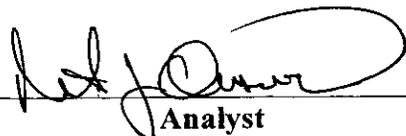
Analyst

Intox EC/IR-II: Preventive Maintenance

WAKE COUNTY CARY PD 910

Serial Number: 008587 Test Record Number: 753
Test Date: 05/22/2009 Test Time: 11:34am EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	11:34am
FLO	Pass	11:34am
FC	Pass	11:34am

Temperature Tests

Test	Status	Time
FC1	Pass	11:34am
SRC	Pass	11:34am
DET	Pass	11:34am
BAR	Pass	11:34am
BT	Pass	11:34am

Blank Tests

Test	Status	Time
AIR	Pass	11:35am

Printer Tests

Test	Status	Time
PRNT	Pass	11:35am

CRC Tests

Test	Status	Time
COMP	Pass	11:35am
CAL	Pass	11:35am

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II**


County WAKE Instrument Location KNIGHTDALE PS.

Instrument Serial No. 008838 979 SEEDIE SQUARE CT KNIGHTDALE NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 22 day of MAY, 2009 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



NW J. [Signature]
Signature of Certifying Official

652
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

WAKE COUNTY KNIGHTDALE PS 910

Serial Number: 008838
Test Date: 05/22/2009

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name:
QUARANTELLA, NICHOLAS J
Permit Number: 21536E
Effective:
01/01/2008-01/01/2010

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG814101
Exp Date: 05/20/2010

Test	g/210L	Time
DIAG	Pass	10:26am
AIR BLK	.00	10:27am
ACCY CHK	.07	10:28am
AIR BLK	.00	10:29am
SUB TEST	.00	10:30am
AIR BLK	.00	10:30am
SUB TEST	.00	10:32am
AIR BLK	.00	10:33am

Reported AC: .00 g/210L

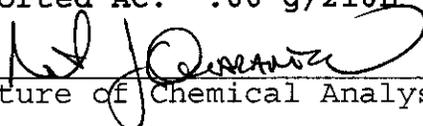

Signature of Chemical Analyst

Court CVR



Analyst

Intox EC/IR-II: Preventive Maintenance

WAKE COUNTY KNIGHTDALE PS 910

Serial Number: 008838 Test Record Number: 176
Test Date: 05/22/2009 Test Time: 10:34am EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	10:34am
FLO	Pass	10:34am
FC	Pass	10:34am

Temperature Tests

Test	Status	Time
FC1	Pass	10:34am
SRC	Pass	10:34am
DET	Pass	10:34am
BAR	Pass	10:34am
BT	Pass	10:34am

Blank Tests

Test	Status	Time
AIR	Pass	10:35am

Printer Tests

Test	Status	Time
PRNT	Pass	10:35am

CRC Tests

Test	Status	Time
COMP	Pass	10:35am
CAL	Pass	10:35am

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II**


County CASWELL Instrument Location SHP CASWELL OFFICE

Instrument Serial No. 008593 956 FIRETOWER RD, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 18 day of MAY, 2009 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

652
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

CASWELL COUNTY SHP YANCEYVILLE 160

Serial Number: 008593
Test Date: 05/18/2009

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name:
QUARANTELLA, NICHOLAS J
Permit Number: 21536E
Effective:
01/01/2008-01/01/2010

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG814002
Exp Date: 05/19/2010


Test	g/210L	Time
DIAG	Pass	10:52am
AIR BLK	.00	10:53am
ACCY CHK	.07	10:53am
AIR BLK	.00	10:54am
SUB TEST	.00	10:55am
AIR BLK	.00	10:56am
SUB TEST	.00	10:57am
AIR BLK	.00	10:58am

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

Intox EC/IR-II: Preventive Maintenance

CASWELL COUNTY SHP YANCEYVILLE 160

Serial Number: 008593 Test Record Number: 417
Test Date: 05/18/2009 Test Time: 10:59am EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	11:00am
FLO	Pass	11:00am
FC	Pass	11:00am

Temperature Tests

Test	Status	Time
FC1	Pass	11:00am
SRC	Pass	11:00am
DET	Pass	11:00am
BAR	Pass	11:00am
BT	Pass	11:00am

Blank Tests

Test	Status	Time
AIR	Pass	11:01am

Printer Tests

Test	Status	Time
PRNT	Pass	11:01am

CRC Tests

Test	Status	Time
COMP	Pass	11:01am
CAL	Pass	11:01am

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH


**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II**

County CABARRUS Instrument Location BAT MOBILE UNIT 3
Instrument Serial No. 008647 CONCORD, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 16 day of MAY, 2009 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Alan Ray Barnes
Signature of Certifying Official

648
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

CABARRUS COUNTY BAT MOBILE UNIT 3 120

Serial Number: 008647
Test Date: 05/16/2009

Citation Number: M0000000-0
Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: BARNES, ALVIN R

Permit Number: 15671E

Effective:

12/01/2007-12/01/2009

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG722602


Exp Date: 08/13/2009

Test	g/210L	Time
DIAG	Pass	11:10pm
AIR BLK	.00	11:11pm
ACCY CHK	.07	11:11pm
AIR BLK	.00	11:12pm
SUB TEST	.00	11:12pm
AIR BLK	.00	11:13pm
SUB TEST	.00	11:15pm
AIR BLK	.00	11:16pm

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR


Analyst

Intox EC/IR-II: Preventive Maintenance

CABARRUS COUNTY BAT MOBILE UNIT 3 120

Serial Number: 008647 Test Record Number: 491
Test Date: 05/16/2009 Test Time: 11:16pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	11:17pm
FLO	Pass	11:17pm
FC	Pass	11:17pm

Temperature Tests

Test	Status	Time
FC1	Pass	11:17pm
SRC	Pass	11:17pm
DET	Pass	11:17pm
BAR	Pass	11:17pm
BT	Pass	11:17pm

Blank Tests

Test	Status	Time
AIR	Pass	11:18pm


Printer Tests

Test	Status	Time
PRNT	Pass	11:18pm

CRC Tests

Test	Status	Time
COMP	Pass	11:18pm
CAL	Pass	11:18pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II**

County CABARRUS Instrument Location BAT MOBILE UNIT 3
Instrument Serial No. 008616 CONCORD, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 16 day of MAY, 2009 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Alvin Ray Bann
Signature of Certifying Official

648
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

CABARRUS COUNTY BAT MOBILE UNIT 3 120

Serial Number: 008616
Test Date: 05/16/2009

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE

Analyst's Name: BARNES, ALVIN R
Permit Number: 15671E
Effective:
12/01/2007-12/01/2009

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test


Lot Number: AG722601
Exp Date: 08/13/2009

Test	g/210L	Time
DIAG	Pass	3:13pm
AIR BLK	.00	3:14pm
ACCY CHK	.07	3:14pm
AIR BLK	.00	3:15pm
SUB TEST	.00	3:16pm
AIR BLK	.00	3:17pm
SUB TEST	.00	3:18pm
AIR BLK	.00	3:19pm

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR


Analyst

Intox EC/IR-II: Preventive Maintenance

CABARRUS COUNTY BAT MOBILE UNIT 3 120

Serial Number: 008616 Test Record Number: 491
Test Date: 05/16/2009 Test Time: 3:20pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	3:20pm
FLO	Pass	3:20pm
FC	Pass	3:20pm

Temperature Tests

Test	Status	Time
FC1	Pass	3:20pm
SRC	Pass	3:20pm
DET	Pass	3:20pm
BAR	Pass	3:20pm
BT	Pass	3:20pm

Blank Tests

Test	Status	Time
AIR	Pass	3:21pm


Printer Tests

Test	Status	Time
PRNT	Pass	3:21pm

CRC Tests

Test	Status	Time
COMP	Pass	3:21pm
CAL	Pass	3:21pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH


**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II**

County GUILFORD Instrument Location BAT MOBILE UNIT 3
Instrument Serial No. 008616 HIGH POINT, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 08 day of MAY, 2009 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Alan Ray Burnes
Signature of Certifying Official

648
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

GUILFORD COUNTY BAT MOBILE UNIT 3 401

Serial Number: 008616
Test Date: 05/08/2009

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE

Analyst's Name: BARNES, ALVIN R
Permit Number: 15671E
Effective:
12/01/2007-12/01/2009

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test


Lot Number: AG722601
Exp Date: 08/13/2009

Test	g/210L	Time
DIAG	Pass	10:07pm
AIR BLK	.00	10:08pm
ACCY CHK	.07	10:09pm
AIR BLK	.00	10:09pm
SUB TEST	.00	10:10pm
AIR BLK	.00	10:11pm
SUB TEST	.00	10:12pm
AIR BLK	.00	10:13pm

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR


Analyst

Intox EC/IR-II: Preventive Maintenance

GUILFORD COUNTY BAT MOBILE UNIT 3 401

Serial Number: 008616 Test Record Number: 485
Test Date: 05/08/2009 Test Time: 10:14pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	10:14pm
FLO	Pass	10:14pm
FC	Pass	10:14pm

Temperature Tests

Test	Status	Time
FC1	Pass	10:15pm
SRC	Pass	10:15pm
DET	Pass	10:15pm
BAR	Pass	10:15pm
BT	Pass	10:15pm

Blank Tests

Test	Status	Time
AIR	Pass	10:15pm


Printer Tests

Test	Status	Time
PRNT	Pass	10:15pm

CRC Tests

Test	Status	Time
COMP	Pass	10:15pm
CAL	Pass	10:15pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH


**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II**

County GUILFORD Instrument Location BATMOBILE UNIT 3
Instrument Serial No. 008647 HIGH POINT, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 08 day of MAY, 2009 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Alan Ray Barnes
Signature of Certifying Official

648
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

GUILFORD COUNTY BAT MOBILE UNIT 3 401

Serial Number: 008647
Test Date: 05/08/2009

Citation Number: M0000000-0
Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: BARNES, ALVIN R

Permit Number: 15671E

Effective:

12/01/2007-12/01/2009

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG722602


Exp Date: 08/13/2009

Test	g/210L	Time
DIAG	Pass	10:21pm
AIR BLK	.00	10:22pm
ACCY CHK	.07	10:23pm
AIR BLK	.00	10:23pm
SUB TEST	.00	10:24pm
AIR BLK	.00	10:25pm
SUB TEST	.00	10:26pm
AIR BLK	.00	10:27pm

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR


Analyst

Intox EC/IR-II: Preventive Maintenance

GUILFORD COUNTY BAT MOBILE UNIT 3 401

Serial Number: 008647 Test Record Number: 485
Test Date: 05/08/2009 Test Time: 10:28pm EDT

System Check: Passed

Baseline Tests

Test	Status	Time
IR	Pass	10:28pm
FLO	Pass	10:28pm
FC	Pass	10:28pm

Temperature Tests

Test	Status	Time
FC1	Pass	10:28pm
SRC	Pass	10:28pm
DET	Pass	10:28pm
BAR	Pass	10:28pm
BT	Pass	10:28pm

Blank Tests

Test	Status	Time
AIR	Pass	10:29pm


Printer Tests

Test	Status	Time
PRNT	Pass	10:29pm

CRC Tests

Test	Status	Time
COMP	Pass	10:29pm
CAL	Pass	10:29pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH


**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II**

County GUILFORD Instrument Location BAT MOBILE UNIT 3
Instrument Serial No. 008707 HIGH POINT, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 08 day of MAY, 2009 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Allen Ray Burns
Signature of Certifying Official

648
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

GUILFORD COUNTY BAT MOBILE UNIT 3 401

Serial Number: 008707
Test Date: 05/08/2009

Citation Number: M0000000-0
Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: BARNES, ALVIN R

Permit Number: 15671E

Effective:

12/01/2007-12/01/2009

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG902001


Exp Date: 01/20/2011

Test	g/210L	Time
DIAG	Pass	11:27pm
AIR BLK	.00	11:28pm
ACCY CHK	.08	11:29pm
AIR BLK	.00	11:30pm
SUB TEST	.00	11:30pm
AIR BLK	.00	11:31pm
SUB TEST	.00	11:33pm
AIR BLK	.00	11:33pm

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR


Analyst

Intox EC/IR-II: Preventive Maintenance

GUILFORD COUNTY BAT MOBILE UNIT 3 401

Serial Number: 008707 Test Record Number: 311
Test Date: 05/08/2009 Test Time: 11:39pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	11:39pm
FLO	Pass	11:39pm
FC	Pass	11:39pm

Temperature Tests

Test	Status	Time
FC1	Pass	11:40pm
SRC	Pass	11:40pm
DET	Pass	11:40pm
BAR	Pass	11:40pm
BT	Pass	11:40pm

Blank Tests

Test	Status	Time
AIR	Pass	11:40pm


Printer Tests

Test	Status	Time
PRNT	Pass	11:40pm

CRC Tests

Test	Status	Time
COMP	Pass	11:40pm
CAL	Pass	11:40pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II**


County MECKLENBURG Instrument Location BAT MOBILE UNIT 3

Instrument Serial No. 008707 CHARLOTTE, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 01 day of MAY, 2009 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Alan Ray Benson
Signature of Certifying Official

648
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

MECKLENBURG COUNTY BAT MOBILE UNIT 3
590

Serial Number: 008707
Test Date: 05/01/2009

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE

Analyst's Name: BARNES, ALVIN R
Permit Number: 15671E
Effective:
12/01/2007-12/01/2009

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test


Lot Number: AG816302
Exp Date: 06/11/2010

Test	g/210L	Time
DIAG	Pass	11:33pm
AIR BLK	.00	11:34pm
ACCY CHK	.08	11:35pm
AIR BLK	.00	11:36pm
SUB TEST	.00	11:36pm
AIR BLK	.00	11:37pm
SUB TEST	.00	11:39pm
AIR BLK	.00	11:40pm

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR



Analyst

Intox EC/IR-II: Preventive Maintenance

MECKLENBURG COUNTY BAT MOBILE UNIT 3 590

Serial Number: 008707 Test Record Number: 306
Test Date: 05/01/2009 Test Time: 11:41pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	11:41pm
FLO	Pass	11:41pm
FC	Pass	11:41pm

Temperature Tests

Test	Status	Time
FC1	Pass	11:41pm
SRC	Pass	11:41pm
DET	Pass	11:41pm
BAR	Pass	11:41pm
BT	Pass	11:41pm

Blank Tests

Test	Status	Time
AIR	Pass	11:42pm


Printer Tests

Test	Status	Time
PRNT	Pass	11:42pm

CRC Tests

Test	Status	Time
COMP	Pass	11:42pm
CAL	Pass	11:42pm

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH


**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II**

County MECKLENBURG Instrument Location BAT MOBILE UNIT 3
Instrument Serial No. 008616 CHARLOTTE, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 01 day of MAY, 2009 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Alan R. Bantz
Signature of Certifying Official

648
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

MECKLENBURG COUNTY BAT MOBILE UNIT 3
590

Serial Number: 008616
Test Date: 05/01/2009

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE

Analyst's Name: BARNES, ALVIN R
Permit Number: 15671E
Effective:
12/01/2007-12/01/2009

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG722601
Exp Date: 08/13/2009

Test	g/210L	Time
DIAG	Pass	11:15pm
AIR BLK	.00	11:16pm
ACCY CHK	.07	11:17pm
AIR BLK	.00	11:18pm
SUB TEST	.00	11:18pm
AIR BLK	.00	11:19pm
SUB TEST	.00	11:20pm
AIR BLK	.00	11:21pm

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR


Analyst

Intox EC/IR-II: Preventive Maintenance

MECKLENBURG COUNTY BAT MOBILE UNIT 3 590

Serial Number: 008616 Test Record Number: 472
Test Date: 05/01/2009 Test Time: 11:22pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	11:22pm
FLO	Pass	11:22pm
FC	Pass	11:22pm

Temperature Tests

Test	Status	Time
FC1	Pass	11:22pm
SRC	Pass	11:22pm
DET	Pass	11:22pm
BAR	Pass	11:22pm
BT	Pass	11:22pm

Blank Tests

Test	Status	Time
AIR	Pass	11:23pm


Printer Tests

Test	Status	Time
PRNT	Pass	11:23pm

CRC Tests

Test	Status	Time
COMP	Pass	11:23pm
CAL	Pass	11:23pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH


**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II**

County MECKLENBURG Instrument Location BAT MOBILE UNIT 3
Instrument Serial No. 008647 CHARLOTTE, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 01 day of MAY, 2009 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Alan R. Barnes
Signature of Certifying Official

648
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

MECKLENBURG COUNTY BAT MOBILE UNIT 3
590

Serial Number: 008647
Test Date: 05/01/2009

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: BARNES, ALVIN R

Permit Number: 15671E

Effective:

12/01/2007-12/01/2009

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG722602


Exp Date: 08/13/2009

Test	g/210L	Time
DIAG	Pass	11:17pm
AIR BLK	.00	11:18pm
ACCY CHK	.07	11:19pm
AIR BLK	.00	11:20pm
SUB TEST	.00	11:20pm
AIR BLK	.00	11:21pm
SUB TEST	.00	11:22pm
AIR BLK	.00	11:23pm

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR


Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

MECKLENBURG COUNTY BAT MOBILE UNIT 3 590

Serial Number: 008647 Test Record Number: 476
Test Date: 05/01/2009 Test Time: 11:24pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	11:24pm
FLO	Pass	11:24pm
FC	Pass	11:24pm

Temperature Tests

Test	Status	Time
FC1	Pass	11:25pm
SRC	Pass	11:25pm
DET	Pass	11:25pm
BAR	Pass	11:25pm
BT	Pass	11:25pm

Blank Tests

Test	Status	Time
AIR	Pass	11:25pm


Printer Tests

Test	Status	Time
PRNT	Pass	11:25pm

CRC Tests

Test	Status	Time
COMP	Pass	11:25pm
CAL	Pass	11:25pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II**

County Rockingham Instrument Location Rockingham Co. Jail
Instrument Serial No. 008796 Wentworth, N.C.

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 21 day of MAY, 2009 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



J. Kevin Dean
Signature of Certifying Official

642
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Preventive Maintenance

ROCKINGHAM COUNTY ROCKINGHAM CO JAIL 780

Serial Number: 008796 Test Record Number: 343
Test Date: 05/21/2009 Test Time: 3:11pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	3:11pm
FLO	Pass	3:11pm
FC	Pass	3:11pm

Temperature Tests

Test	Status	Time
FC1	Pass	3:11pm
SRC	Pass	3:11pm
DET	Pass	3:11pm
BAR	Pass	3:11pm
BT	Pass	3:11pm

Blank Tests

Test	Status	Time
AIR	Pass	3:12pm


Printer Tests

Test	Status	Time
PRNT	Pass	3:12pm

CRC Tests

Test	Status	Time
COMP	Pass	3:12pm
CAL	Pass	3:12pm

Preventive Maintenance
Status: Pass


Analyst

Intox EC/IR-II: Subject Test

ROCKINGHAM COUNTY ROCKINGHAM CO JAIL
780

Serial Number: 008796
Test Date: 05/21/2009

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: DEAN, LARRY K
Permit Number: 11598E
Effective:
12/01/2007-12/01/2009

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG902001
Exp Date: 01/20/2011

Test	g/210L	Time
DIAG	Pass	3:04pm
AIR BLK	.00	3:05pm
ACCY CHK	.08	3:06pm
AIR BLK	.00	3:07pm
SUB TEST	.00	3:07pm
AIR BLK	.00	3:08pm
SUB TEST	.00	3:09pm
AIR BLK	.00	3:10pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II**


County CUMBERLAND Instrument Location FORT BRAGG

Instrument Serial No. 008908 MILITARY POLICE

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 19 day of MAY, 2009 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]

Signature of Certifying Official

578

Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

CUMBERLAND FORT BRAGG, LEC. 250

Serial Number: 008908
Test Date: 05/19/2009

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: SIMMONS, PAUL T
Permit Number: 08619E
Effective:
12/01/2007-12/01/2009

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG901901
Exp Date: 01/19/2011

Test	g/210L	Time
DIAG	Pass	4:25pm
AIR BLK	.00	4:26pm
ACCY CHK	.08	4:27pm
AIR BLK	.00	4:27pm
SUB TEST	.00	4:28pm
AIR BLK	.00	4:29pm
SUB TEST	.00	4:31pm
AIR BLK	.00	4:32pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

Intox EC/IR-II: Preventive Maintenance

CUMBERLAND FORT BRAGG, LEC. 250

Serial Number: 008908 Test Record Number: 423
Test Date: 05/19/2009 Test Time: 4:34pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	4:34pm
FLO	Pass	4:34pm
FC	Pass	4:35pm

Temperature Tests

Test	Status	Time
FC1	Pass	4:35pm
SRC	Pass	4:35pm
DET	Pass	4:35pm
BAR	Pass	4:35pm
BT	Pass	4:35pm

Blank Tests

Test	Status	Time
AIR	Pass	4:35pm

Printer Tests

Test	Status	Time
PRNT	Pass	4:35pm

CRC Tests

Test	Status	Time
COMP	Pass	4:36pm
CAL	Pass	4:36pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH


**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II**

County CRAVEN Instrument Location BAT Mobile unit 6
Instrument Serial No. 008939 SAT

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 22 day of MAY, 2009 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

601
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Preventive Maintenance

CRAVEN COUNTY BAT MOBILE UNIT 6 240

Serial Number: 008939 Test Record Number: 171
Test Date: 05/22/2009 Test Time: 11:02pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	11:02pm
FLO	Pass	11:02pm
FC	Pass	11:02pm

Temperature Tests

Test	Status	Time
FC1	Pass	11:03pm
SRC	Pass	11:03pm
DET	Pass	11:03pm
BAR	Pass	11:03pm
BT	Pass	11:03pm

Blank Tests

Test	Status	Time
AIR	Pass	11:03pm

Printer Tests

Test	Status	Time
PRNT	Pass	11:03pm

CRC Tests

Test	Status	Time
COMP	Pass	11:03pm
CAL	Pass	11:03pm

Preventive Maintenance
Status: Pass



Analyst

Intox EC/IR-II: Subject Test

CRAVEN COUNTY BAT MOBILE UNIT 6 240

Serial Number: 008939
Test Date: 05/22/2009

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE

Analyst's Name: RHODES, KENNETH C
Permit Number: 5329E
Effective:
02/01/2008-02/01/2010

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG814101
Exp Date: 05/20/2010

Test	g/210L	Time
DIAG	Pass	10:55pm
AIR BLK	.00	10:56pm
ACCY CHK	.07	10:56pm
AIR BLK	.00	10:57pm
SUB TEST	.00	10:57pm
AIR BLK	.00	10:58pm
SUB TEST	.00	11:00pm
AIR BLK	.00	11:01pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II

County Nash Instrument Location BAT mobile unit 6

Instrument Serial No. 008939

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 30 day of May, 2009 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



T. C. [Signature]
Signature of Certifying Official

601
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Preventive Maintenance

NASH COUNTY BAT MOBILE UNIT 6 630

Serial Number: 008939 Test Record Number: 182
Test Date: 05/30/2009 Test Time: 10:21pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	10:22pm
FLO	Pass	10:22pm
FC	Pass	10:22pm

Temperature Tests

Test	Status	Time
FC1	Pass	10:22pm
SRC	Pass	10:22pm
DET	Pass	10:22pm
BAR	Pass	10:22pm
BT	Pass	10:22pm

Blank Tests

Test	Status	Time
AIR	Pass	10:23pm

Printer Tests

Test	Status	Time
PRNT	Pass	10:23pm

CRC Tests

Test	Status	Time
COMP	Pass	10:23pm
CAL	Pass	10:23pm

Preventive Maintenance
Status: Pass



Analyst

Intox EC/IR-II: Subject Test

NASH COUNTY BAT MOBILE UNIT 6 630

Serial Number: 008939
Test Date: 05/30/2009

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: RHODES, KENNETH C
Permit Number: 5329E
Effective:
02/01/2008-02/01/2010

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG814101
Exp Date: 05/20/2010


Test	g/210L	Time
DIAG	Pass	10:15pm
AIR BLK	.00	10:16pm
ACCY CHK	.07	10:16pm
AIR BLK	.00	10:17pm
SUB TEST	.00	10:18pm
AIR BLK	.00	10:18pm
SUB TEST	.00	10:20pm
AIR BLK	.00	10:21pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR

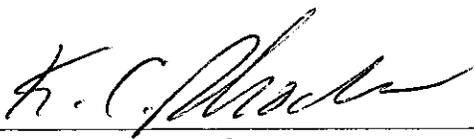

Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II**

County Wake

Instrument Location Pat Mobile Unit


Instrument Serial No. 102600

APV

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 30th day of May, 2009 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Steph G. Tipton

Signature of Certifying Official

636
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Preventive Maintenance

WAKE COUNTY BAT MOBILE UNIT 5 910

Serial Number: 008600 Test Record Number: 481
Test Date: 05/30/2009 Test Time: 11:30pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	11:30pm
FLO	Pass	11:30pm
FC	Pass	11:30pm

Temperature Tests

Test	Status	Time
FC1	Pass	11:30pm
SRC	Pass	11:30pm
DET	Pass	11:30pm
BAR	Pass	11:30pm
BT	Pass	11:30pm

Blank Tests

Test	Status	Time
AIR	Pass	11:31pm


Printer Tests

Test	Status	Time
PRNT	Pass	11:31pm

CRC Tests

Test	Status	Time
COMP	Pass	11:31pm
CAL	Pass	11:31pm

Preventive Maintenance
Status: Pass


Analyst

Intox EC/IR-II: Subject Test .

WAKE COUNTY BAT MOBILE UNIT 5 910

Serial Number: 008600
Test Date: 05/30/2009

Citation Number: M0000000-0
Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: MORGART, STEPHEN G

Permit Number: 09372E

Effective:

12/01/2007-12/01/2009

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG723401

Exp Date: 08/21/2009

Test	g/210L	Time
DIAG	Pass	11:20pm
AIR BLK	.00	11:21pm
ACCY CHK	.07	11:21pm
AIR BLK	.00	11:22pm
SUB TEST	.00	11:23pm
AIR BLK	.00	11:24pm
SUB TEST	.00	11:25pm
AIR BLK	.00	11:26pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II**


County Sampson Instrument Location 15AT Mobile Unit #5

Instrument Serial No. 008600

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 29th day of May, 2009 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

636
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Preventive Maintenance

SAMPSON COUNTY BAT MOBILE UNIT 5 810

Serial Number: 008600 Test Record Number: 478
Test Date: 05/29/2009 Test Time: 7:27pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	7:27pm
FLO	Pass	7:27pm
FC	Pass	7:27pm

Temperature Tests

Test	Status	Time
FC1	Pass	7:27pm
SRC	Pass	7:27pm
DET	Pass	7:27pm
BAR	Pass	7:27pm
BT	Pass	7:27pm

Blank Tests

Test	Status	Time
AIR	Pass	7:28pm


Printer Tests

Test	Status	Time
PRNT	Pass	7:28pm

CRC Tests

Test	Status	Time
COMP	Pass	7:28pm
CAL	Pass	7:28pm

Preventive Maintenance
Status: Pass



Analyst

Intox EC/IR-II: Subject Test

SAMPSON COUNTY BAT MOBILE UNIT 5 810

Serial Number: 008600
Test Date: 05/29/2009

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: MORGART, STEPHEN G

Permit Number: 09372E

Effective:

12/01/2007-12/01/2009

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG723401


Exp Date: 08/21/2009

Test	g/210L	Time
DIAG	Pass	7:18pm
AIR BLK	.00	7:19pm
ACCY CHK	.07	7:20pm
AIR BLK	.00	7:21pm
SUB TEST	.00	7:21pm
AIR BLK	.00	7:22pm
SUB TEST	.00	7:24pm
AIR BLK	.00	7:24pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH


**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II**

County CABARRUS Instrument Location BAT MOBILE UNIT 3
Instrument Serial No. 008616 CONCORD, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 23 day of MAY, 2009 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Alan Ray Barnes
Signature of Certifying Official

648
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

CABARRUS COUNTY BAT MOBILE UNIT 3 120

Serial Number: 008616
Test Date: 05/23/2009

Citation Number: M0000000-0
Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: BARNES, ALVIN R

Permit Number: 15671E

Effective:

12/01/2007-12/01/2009

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG722601


Exp Date: 08/13/2009

Test	g/210L	Time
DIAG	Pass	11:18pm
AIR BLK	.00	11:19pm
ACCY CHK	.07	11:20pm
AIR BLK	.00	11:21pm
SUB TEST	.00	11:22pm
AIR BLK	.00	11:23pm
SUB TEST	.00	11:24pm
AIR BLK	.00	11:25pm

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR



Analyst

Intox EC/IR-II: Preventive Maintenance

CABARRUS COUNTY BAT MOBILE UNIT 3 120

Serial Number: 008616 Test Record Number: 498
Test Date: 05/23/2009 Test Time: 11:26pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	11:27pm
FLO	Pass	11:27pm
FC	Pass	11:27pm

Temperature Tests

Test	Status	Time
FC1	Pass	11:27pm
SRC	Pass	11:27pm
DET	Pass	11:27pm
BAR	Pass	11:27pm
BT	Pass	11:27pm

Blank Tests

Test	Status	Time
AIR	Pass	11:28pm

Printer Tests


Test	Status	Time
PRNT	Pass	11:28pm

CRC Tests

Test	Status	Time
COMP	Pass	11:28pm
CAL	Pass	11:28pm

Preventive Maintenance

Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II**


County ALAMANCE Instrument Location Bar Mobile Unit-3

Instrument Serial No. 008616 BURLINGTON, N.C.

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 29 day of MAY, 2009 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



A. Keina Dean
Signature of Certifying Official

642
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

ALAMANCE COUNTY BAT MOBILE UNIT 3 000

Serial Number: 008616
Test Date: 05/29/2009

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: DEAN, LARRY K

Permit Number: 11598E

Effective:

12/01/2007-12/01/2009

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG722601


Exp Date: 08/13/2009

Test	g/210L	Time
DIAG	Pass	9:02pm
AIR BLK	.00	9:04pm
ACCY CHK	.07	9:04pm
AIR BLK	.00	9:05pm
SUB TEST	.00	9:05pm
AIR BLK	.00	9:06pm
SUB TEST	.00	9:08pm
AIR BLK	.00	9:09pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR



Analyst

This form is used when performing Preventive Maintenance procedures

Forensic Tests for Alcohol Branch

Department of Health and Human Services

Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

ALAMANCE COUNTY BAT MOBILE UNIT 3 000

Serial Number: 008616 Test Record Number: 502
Test Date: 05/29/2009 Test Time: 9:10pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	9:10pm
FLO	Pass	9:10pm
FC	Pass	9:10pm

Temperature Tests

Test	Status	Time
FC1	Pass	9:10pm
SRC	Pass	9:10pm
DET	Pass	9:10pm
BAR	Pass	9:10pm
BT	Pass	9:10pm

Blank Tests

Test	Status	Time
AIR	Pass	9:11pm


Printer Tests

Test	Status	Time
PRNT	Pass	9:11pm

CRC Tests

Test	Status	Time
COMP	Pass	9:11pm
CAL	Pass	9:11pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II**

County Forsyth Instrument Location Bat Mobile Unit-3
Instrument Serial No. 008616 Clemmons, N.C.

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 30 day of May, 2009 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

FORSYTH COUNTY BAT MOBILE UNIT 3 330

Serial Number: 008616
Test Date: 05/30/2009

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: DEAN, LARRY K
Permit Number: 11598E
Effective:
12/01/2007-12/01/2009

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG722601
Exp Date: 08/13/2009


Test	g/210L	Time
DIAG	Pass	11:31pm
AIR BLK	.00	11:32pm
ACCY CHK	.07	11:33pm
AIR BLK	.00	11:34pm
SUB TEST	.00	11:34pm
AIR BLK	.00	11:35pm
SUB TEST	.00	11:37pm
AIR BLK	.00	11:37pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

Intox EC/IR-II: Preventive Maintenance

FORSYTH COUNTY BAT MOBILE UNIT 3 330

Serial Number: 008616 Test Record Number: 509
Test Date: 05/30/2009 Test Time: 11:41pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	11:42pm
FLO	Pass	11:42pm
FC	Pass	11:42pm

Temperature Tests

Test	Status	Time
FC1	Pass	11:42pm
SRC	Pass	11:42pm
DET	Pass	11:42pm
BAR	Pass	11:42pm
BT	Pass	11:42pm

Blank Tests

Test	Status	Time
AIR	Pass	11:43pm


Printer Tests

Test	Status	Time
PRNT	Pass	11:43pm

CRC Tests

Test	Status	Time
COMP	Pass	11:43pm
CAL	Pass	11:43pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II**

County ALAMANCE Instrument Location Bar Mobile Unit-5

Instrument Serial No. 008647 BURLINGTON, N.C.

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 29 day of May, 2009 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

642
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

ALAMANCE COUNTY BAT MOBILE UNIT 3 000

Serial Number: 008647

Test Date: 05/29/2009

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: DEAN, LARRY K

Permit Number: 11598E

Effective:

12/01/2007-12/01/2009

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG722602

Exp Date: 08/13/2009


Test	g/210L	Time
DIAG	Pass	8:45pm
AIR BLK	.00	8:46pm
ACCY CHK	.07	8:47pm
AIR BLK	.00	8:48pm
SUB TEST	.00	8:48pm
AIR BLK	.00	8:49pm
SUB TEST	.00	8:51pm
AIR BLK	.00	8:52pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

Intox EC/IR-II: Preventive Maintenance

ALAMANCE COUNTY BAT MOBILE UNIT 3 000

Serial Number: 008647 Test Record Number: 502
Test Date: 05/29/2009 Test Time: 8:53pm EDT

System Check: Passed

Baseline Tests

Test	Status	Time
IR	Pass	8:53pm
FLO	Pass	8:53pm
FC	Pass	8:53pm

Temperature Tests

Test	Status	Time
FC1	Pass	8:53pm
SRC	Pass	8:53pm
DET	Pass	8:53pm
BAR	Pass	8:53pm
BT	Pass	8:53pm

Blank Tests

Test	Status	Time
AIR	Pass	8:54pm


Printer Tests

Test	Status	Time
PRNT	Pass	8:54pm

CRC Tests

Test	Status	Time
COMP	Pass	8:54pm
CAL	Pass	8:54pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH


**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II**

County Forsyth Instrument Location Bar Mobile Unit-3
Instrument Serial No. 008647 Clemmons, N.C.

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 30 day of May, 2009 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



L. Kevin Olson
Signature of Certifying Official

642
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

FORSYTH COUNTY BAT MOBILE UNIT 3 330

Serial Number: 008647
Test Date: 05/30/2009

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: DEAN, LARRY K
Permit Number: 11598E
Effective:
12/01/2007-12/01/2009

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG722602
Exp Date: 08/13/2009


Test	g/210L	Time
DIAG	Pass	11:30pm
AIR BLK	.00	11:32pm
ACCY CHK	.07	11:32pm
AIR BLK	.00	11:33pm
SUB TEST	.00	11:33pm
AIR BLK	.00	11:34pm
SUB TEST	.00	11:36pm
AIR BLK	.00	11:37pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

Intox EC/IR-II: Preventive Maintenance

FORSYTH COUNTY BAT MOBILE UNIT 3 330

Serial Number: 008647 Test Record Number: 507
Test Date: 05/30/2009 Test Time: 11:40pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	11:41pm
FLO	Pass	11:41pm
FC	Pass	11:41pm

Temperature Tests

Test	Status	Time
FC1	Pass	11:41pm
SRC	Pass	11:41pm
DET	Pass	11:41pm
BAR	Pass	11:41pm
BT	Pass	11:41pm

Blank Tests

Test	Status	Time
AIR	Pass	11:42pm


Printer Tests

Test	Status	Time
PRNT	Pass	11:42pm

CRC Tests

Test	Status	Time
COMP	Pass	11:42pm
CAL	Pass	11:42pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II**


County GUILFORD Instrument Location BAT MOBILE UNIT 3

Instrument Serial No. 008647 HIGH POINT, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 22 day of MAY, 20 09 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Alan Ray Bunn
Signature of Certifying Official

648
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

GUILFORD COUNTY BAT MOBILE UNIT 3 401

Serial Number: 008647
Test Date: 05/22/2009

Citation Number: M0000000-0
Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: BARNES, ALVIN R

Permit Number: 15671E

Effective:

12/01/2007-12/01/2009

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG722602


Exp Date: 08/13/2009

Test	g/210L	Time
DIAG	Pass	11:19pm
AIR BLK	.00	11:20pm
ACCY CHK	.07	11:21pm
AIR BLK	.00	11:21pm
SUB TEST	.00	11:22pm
AIR BLK	.00	11:23pm
SUB TEST	.00	11:24pm
AIR BLK	.00	11:25pm

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR


Analyst

Intox EC/IR-II: Preventive Maintenance

GUILFORD COUNTY BAT MOBILE UNIT 3 401

Serial Number: 008647 Test Record Number: 498
Test Date: 05/22/2009 Test Time: 11:26pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	11:26pm
FLO	Pass	11:26pm
FC	Pass	11:26pm

Temperature Tests

Test	Status	Time
FC1	Pass	11:26pm
SRC	Pass	11:26pm
DET	Pass	11:26pm
BAR	Pass	11:26pm
BT	Pass	11:26pm

Blank Tests

Test	Status	Time
AIR	Pass	11:27pm


Printer Tests

Test	Status	Time
PRNT	Pass	11:27pm

CRC Tests

Test	Status	Time
COMP	Pass	11:27pm
CAL	Pass	11:27pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II**

County Sampson Instrument Location BT Mobile Unit #5

Instrument Serial No. 008698

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 29th day of May, 2009 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Steph O. [Signature] 636
Signature of Certifying Official Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Preventive Maintenance

SAMPSON COUNTY BAT MOBILE UNIT 5 810

Serial Number: 008698 Test Record Number: 326
Test Date: 05/29/2009 Test Time: 7:26pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	7:26pm
FLO	Pass	7:26pm
FC	Pass	7:26pm

Temperature Tests

Test	Status	Time
FC1	Pass	7:26pm
SRC	Pass	7:26pm
DET	Pass	7:26pm
BAR	Pass	7:26pm
BT	Pass	7:26pm

Blank Tests

Test	Status	Time
AIR	Pass	7:27pm


Printer Tests

Test	Status	Time
PRNT	Pass	7:27pm

CRC Tests

Test	Status	Time
COMP	Pass	7:27pm
CAL	Pass	7:27pm

Preventive Maintenance
Status: Pass



Analyst

Intox EC/IR-II: Subject Test, . . .

SAMPSON COUNTY BAT MOBILE UNIT 5 810

Serial Number: 008698
Test Date: 05/29/2009

Citation Number: M0000000-0
Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: MORGART, STEPHEN G

Permit Number: 09372E

Effective:

12/01/2007-12/01/2009

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG723401

Exp Date: 08/21/2009

Test	g/210L	Time
DIAG	Pass	7:17pm
AIR BLK	.00	7:18pm
ACCY CHK	.07	7:18pm
AIR BLK	.00	7:19pm
SUB TEST	.00	7:20pm
AIR BLK	.00	7:21pm
SUB TEST	.00	7:22pm
AIR BLK	.00	7:23pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II**


County Wake Instrument Location BATMOBILE Unit #5

Instrument Serial No. 008698 APCV

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 30TH day of MAY, 2009 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

636
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Preventive Maintenance

WAKE COUNTY BAT MOBILE UNIT 5 910

Serial Number: 008698 Test Record Number: 328
Test Date: 05/30/2009 Test Time: 11:24pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	11:24pm
FLO	Pass	11:24pm
FC	Pass	11:24pm

Temperature Tests

Test	Status	Time
FC1	Pass	11:24pm
SRC	Pass	11:24pm
DET	Pass	11:24pm
BAR	Pass	11:24pm
BT	Pass	11:24pm

Blank Tests

Test	Status	Time
AIR	Pass	11:25pm

Printer Tests

Test	Status	Time
PRNT	Pass	11:25pm

CRC Tests

Test	Status	Time
COMP	Pass	11:25pm
CAL	Pass	11:25pm

Preventive Maintenance
Status: Pass



Analyst

Intox EC/IR-II: Subject Test

WAKE COUNTY BAT MOBILE UNIT 5 910

Serial Number: 008698
Test Date: 05/30/2009

Citation Number: M0000000-0
Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: MORGART, STEPHEN G

Permit Number: 09372E

Effective:

12/01/2007-12/01/2009

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG723401

Exp Date: 08/21/2009


Test	g/210L	Time
DIAG	Pass	11:11pm
AIR BLK	.00	11:12pm
ACCY CHK	.07	11:13pm
AIR BLK	.00	11:14pm
SUB TEST	.00	11:15pm
AIR BLK	.00	11:16pm
SUB TEST	.00	11:18pm
AIR BLK	.00	11:19pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH


**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II**

County Forsyth Instrument Location Bar Mobile Unit-3
Instrument Serial No. 008707 Clemmons, N.C.

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 30 day of May, 2009 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



L. Kevin Dean
Signature of Certifying Official

642
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

FORSYTH COUNTY BAT MOBILE UNIT 3 330

Serial Number: 008707

Test Date: 05/30/2009

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: DEAN, LARRY K

Permit Number: 11598E

Effective:

12/01/2007-12/01/2009

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG902001

Exp Date: 01/20/2011


Test	g/210L	Time
DIAG	Pass	11:30pm
AIR BLK	.00	11:31pm
ACCY CHK	.08	11:31pm
AIR BLK	.00	11:32pm
SUB TEST	.00	11:32pm
AIR BLK	.00	11:33pm
SUB TEST	.00	11:35pm
AIR BLK	.00	11:36pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

This form is used when performing Preventive Maintenance procedures

Forensic Tests for Alcohol Branch

Department of Health and Human Services

Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

FORSYTH COUNTY BAT MOBILE UNIT 3 330

Serial Number: 008707 Test Record Number: 319
Test Date: 05/30/2009 Test Time: 11:43pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	11:43pm
FLO	Pass	11:44pm
FC	Pass	11:44pm

Temperature Tests

Test	Status	Time
FC1	Pass	11:44pm
SRC	Pass	11:44pm
DET	Pass	11:44pm
BAR	Pass	11:44pm
BT	Pass	11:44pm

Blank Tests

Test	Status	Time
AIR	Pass	11:44pm

Printer Tests

Test	Status	Time
PRNT	Pass	11:44pm

CRC Tests

Test	Status	Time
COMP	Pass	11:45pm
CAL	Pass	11:45pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II


County GUILFORD Instrument Location BAT MOBILE UNIT 3

Instrument Serial No. 008707 HIGH POINT, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 22 day of MAY, 20 09 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Alvin Ray Bowers
Signature of Certifying Official

648
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

GUILFORD COUNTY BAT MOBILE UNIT 3 401

Serial Number: 008707

Test Date: 05/22/2009

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: BARNES, ALVIN R

Permit Number: 15671E

Effective:

12/01/2007-12/01/2009

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG902001


Exp Date: 01/20/2011

Test	g/210L	Time
DIAG	Pass	11:44pm
AIR BLK	.00	11:45pm
ACCY CHK	.08	11:46pm
AIR BLK	.00	11:46pm
SUB TEST	.00	11:47pm
AIR BLK	.00	11:48pm
SUB TEST	.00	11:49pm
AIR BLK	.00	11:50pm

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR



Analyst

Intox EC/IR-II: Preventive Maintenance

GUILFORD COUNTY BAT MOBILE UNIT 3 401

Serial Number: 008707 Test Record Number: 314
Test Date: 05/22/2009 Test Time: 11:51pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	11:51pm
FLO	Pass	11:51pm
FC	Pass	11:51pm

Temperature Tests

Test	Status	Time
FC1	Pass	11:52pm
SRC	Pass	11:52pm
DET	Pass	11:52pm
BAR	Pass	11:52pm
BT	Pass	11:52pm

Blank Tests

Test	Status	Time
AIR	Pass	11:52pm

Printer Tests

Test	Status	Time
PRNT	Pass	11:52pm

CRC Tests

Test	Status	Time
COMP	Pass	11:52pm
CAL	Pass	11:52pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II**


County Hoke Instrument Location BAT Mobile Unit 4

Instrument Serial No. 008717

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 30th day of May, 2009 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Dani O'Connell
Signature of Certifying Official

651
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Preventive Maintenance

HOKE COUNTY BAT MOBILE UNIT 4 460

Serial Number: 008717 Test Record Number: 162
Test Date: 05/30/2009 Test Time: 9:15pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	9:15pm
FLO	Pass	9:15pm
FC	Pass	9:15pm

Temperature Tests

Test	Status	Time
FC1	Pass	9:15pm
SRC	Pass	9:15pm
DET	Pass	9:15pm
BAR	Pass	9:15pm
BT	Pass	9:15pm

Blank Tests

Test	Status	Time
AIR	Pass	9:16pm


Printer Tests

Test	Status	Time
PRNT	Pass	9:16pm

CRC Tests

Test	Status	Time
COMP	Pass	9:16pm
CAL	Pass	9:16pm

Preventive Maintenance
Status: Pass


Analyst

Intox EC/IR-II: Subject Test

HOKE COUNTY BAT MOBILE UNIT 4 460

Serial Number: 008717
Test Date: 05/30/2009

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: TRUDELL, SR., DANIEL T

Permit Number: 21535E

Effective:

12/01/2007-12/01/2009

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG723401


Exp Date: 08/21/2009

Test	g/210L	Time
DIAG	Pass	9:07pm
AIR BLK	.00	9:08pm
ACCY CHK	.07	9:09pm
AIR BLK	.00	9:10pm
SUB TEST	.00	9:10pm
AIR BLK	.00	9:11pm
SUB TEST	.00	9:13pm
AIR BLK	.00	9:14pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II**

County Hoke


Instrument Location BAT Mobile Unit 4

Instrument Serial No. 008734

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 30th day of May, 2009 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Daniel T. [Signature]
Signature of Certifying Official

051
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Preventive Maintenance

HOKE COUNTY BAT MOBILE UNIT 4 460

Serial Number: 008734 Test Record Number: 238
Test Date: 05/30/2009 Test Time: 9:13pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	9:13pm
FLO	Pass	9:13pm
FC	Pass	9:13pm

Temperature Tests

Test	Status	Time
FC1	Pass	9:13pm
SRC	Pass	9:13pm
DET	Pass	9:13pm
BAR	Pass	9:13pm
BT	Pass	9:13pm

Blank Tests

Test	Status	Time
AIR	Pass	9:14pm


Printer Tests

Test	Status	Time
PRNT	Pass	9:14pm

CRC Tests

Test	Status	Time
COMP	Pass	9:14pm
CAL	Pass	9:14pm

Preventive Maintenance
Status: Pass


Analyst

Intox EC/IR-II: Subject Test

HOKE COUNTY BAT MOBILE UNIT 4 460

Serial Number: 008734
Test Date: 05/30/2009

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE

Analyst's Name: TRUDELL, SR., DANIEL T
Permit Number: 21535E
Effective:
12/01/2007-12/01/2009

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test


Lot Number: AG722501
Exp Date: 08/12/2009

Test	g/210L	Time
DIAG	Pass	9:05pm
AIR BLK	.00	9:06pm
ACCY CHK	.07	9:07pm
AIR BLK	.00	9:08pm
SUB TEST	.00	9:08pm
AIR BLK	.00	9:09pm
SUB TEST	.00	9:11pm
AIR BLK	.00	9:12pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH


**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II**

County CUMBERLAND Instrument Location SECURITY FORCES
Instrument Serial No. 008787 POPE AFB,

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 19 day of MAY, 2009 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Paul T. [Signature]
Signature of Certifying Official

578
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

CUMBERLAND SECURITY FORCES 250

Serial Number: 008787
Test Date: 05/19/2009

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: SIMMONS, PAUL T
Permit Number: 08619E
Effective:
12/01/2007-12/01/2009

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG722801
Exp Date: 08/15/2009

Test	g/210L	Time
DIAG	Pass	1:32pm
AIR BLK	.00	1:33pm
ACCY CHK	.07	1:33pm
AIR BLK	.00	1:34pm
SUB TEST	.00	1:35pm
AIR BLK	.00	1:36pm
SUB TEST	.00	1:37pm
AIR BLK	.00	1:38pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

Intox EC/IR-II: Preventive Maintenance

CUMBERLAND SECURITY FORCES 250

Serial Number: 008787 Test Record Number: 72
Test Date: 05/19/2009 Test Time: 1:39pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	1:40pm
FLO	Pass	1:40pm
FC	Pass	1:40pm

Temperature Tests

Test	Status	Time
FC1	Pass	1:40pm
SRC	Pass	1:40pm
DET	Pass	1:40pm
BAR	Pass	1:40pm
BT	Pass	1:40pm

Blank Tests

Test	Status	Time
AIR	Pass	1:41pm

Printer Tests

Test	Status	Time
PRNT	Pass	1:41pm

CRC Tests

Test	Status	Time
COMP	Pass	1:41pm
CAL	Pass	1:41pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II**

County WAKE Instrument Location Best Mobile Unit #15

Instrument Serial No. CC8788 Apex

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 30th day of May, 2009 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Preventive Maintenance

WAKE COUNTY BAT MOBILE UNIT 5 910

Serial Number: 008788 Test Record Number: 194
Test Date: 05/30/2009 Test Time: 11:53pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	11:53pm
FLO	Pass	11:53pm
FC	Pass	11:53pm

Temperature Tests

Test	Status	Time
FC1	Pass	11:53pm
SRC	Pass	11:53pm
DET	Pass	11:53pm
BAR	Pass	11:53pm
BT	Pass	11:53pm

Blank Tests

Test	Status	Time
AIR	Pass	11:54pm

Printer Tests

Test	Status	Time
PRNT	Pass	11:54pm

CRC Tests

Test	Status	Time
COMP	Pass	11:54pm
CAL	Pass	11:54pm

Preventive Maintenance
Status: Pass



Analyst

Intox EC/IR-II: Subject Test

WAKE COUNTY BAT MOBILE UNIT 5 910

Serial Number: 008788
Test Date: 05/30/2009

Citation Number: M0000000-0
Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: MORGART, STEPHEN G

Permit Number: 09372E

Effective:

12/01/2007-12/01/2009

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG904903


Exp Date: 02/18/2011

Test	g/210L	Time
DIAG	Pass	11:45pm
AIR BLK	.00	11:46pm
ACCY CHK	.08	11:46pm
AIR BLK	.00	11:47pm
SUB TEST	.00	11:48pm
AIR BLK	.00	11:49pm
SUB TEST	.00	11:51pm
AIR BLK	.00	11:52pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR

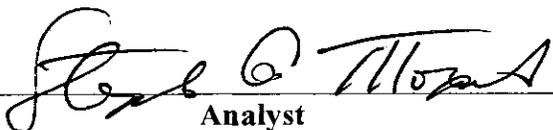
Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II**


County Iredell Instrument Location Statesville PD

Instrument Serial No. 008619 330 S. Tradd St. Statesville
704-878-3406

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 5th day of May, 2009 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Joseph E. Hutchins
Signature of Certifying Official

650
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

IREDELL COUNTY STATESVILLE PD 480

Serial Number: 008619
Test Date: 05/05/2009

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE

Analyst's Name: HUTCHINSON, JOSEPH E
Permit Number: 19951E
Effective:
12/01/2007-12/01/2009

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG723401
Exp Date: 08/21/2009

Test	g/210L	Time
DIAG	Pass	11:39am
AIR BLK	.00	11:40am
ACCY CHK	.07	11:41am
AIR BLK	.00	11:42am
SUB TEST	.00	11:42am
AIR BLK	.00	11:43am
SUB TEST	.00	11:45am
AIR BLK	.00	11:46am

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

Intox EC/IR-II: Preventive Maintenance

IREDELL COUNTY STATESVILLE PD 480

Serial Number: 008619 Test Record Number: 285
Test Date: 05/05/2009 Test Time: 11:47am EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	11:47am
FLO	Pass	11:47am
FC	Pass	11:47am

Temperature Tests

Test	Status	Time
FC1	Pass	11:47am
SRC	Pass	11:47am
DET	Pass	11:47am
BAR	Pass	11:47am
BT	Pass	11:47am

Blank Tests

Test	Status	Time
AIR	Pass	11:48am


Printer Tests

Test	Status	Time
PRNT	Pass	11:48am

CRC Tests

Test	Status	Time
COMP	Pass	11:48am
CAL	Pass	11:48am

Preventive Maintenance
Status: Pass

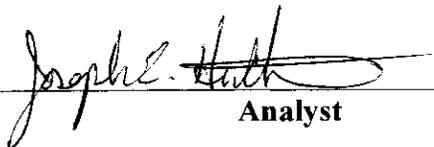

Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II**

County Iredell Instrument Location Iredell County SD
Instrument Serial No. 008809 221 East Water Street, Statesville
704-878-3131

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 5th day of May, 2009 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Joseph E. Hutchinson
Signature of Certifying Official

650
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

IREDELL COUNTY IREDELL COUNTY SD 480

Serial Number: 008809
Test Date: 05/05/2009

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: HUTCHINSON, JOSEPH E
Permit Number: 19951E
Effective:
12/01/2007-12/01/2009

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG722501
Exp Date: 08/12/2009


Test	g/210L	Time
DIAG	Pass	11:10am
AIR BLK	.00	11:11am
ACCY CHK	.07	11:12am
AIR BLK	.00	11:12am
SUB TEST	.00	11:13am
AIR BLK	.00	11:14am
SUB TEST	.00	11:15am
AIR BLK	.00	11:16am

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR

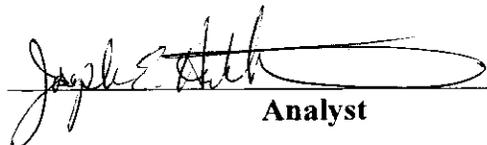

Analyst

Intox EC/IR-II: Preventive Maintenance

IREDELL COUNTY IREDELL COUNTY SD 480

Serial Number: 008809 Test Record Number: 578
Test Date: 05/05/2009 Test Time: 11:17am EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	11:17am
FLO	Pass	11:17am
FC	Pass	11:17am

Temperature Tests

Test	Status	Time
FC1	Pass	11:18am
SRC	Pass	11:18am
DET	Pass	11:18am
BAR	Pass	11:18am
BT	Pass	11:18am

Blank Tests

Test	Status	Time
AIR	Pass	11:18am


Printer Tests

Test	Status	Time
PRNT	Pass	11:18am

CRC Tests

Test	Status	Time
COMP	Pass	11:18am
CAL	Pass	11:18am

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II**


County Iredell Instrument Location Mooreville PD

Instrument Serial No. 008685 750 W. Iredell Ave, Mooreville
704-664-3311

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 5th day of May, 2009 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Joseph E. Hutchinson
Signature of Certifying Official

650
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

IREDELL COUNTY MOORESVILLE PD 480

Serial Number: 008685
Test Date: 05/05/2009

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: HUTCHINSON, JOSEPH E

Permit Number: 19951E

Effective:

12/01/2007-12/01/2009

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG902001

Exp Date: 01/20/2011

Test	g/210L	Time
DIAG	Pass	10:10am
AIR BLK	.00	10:11am
ACCY CHK	.08	10:12am
AIR BLK	.00	10:12am
SUB TEST	.00	10:13am
AIR BLK	.00	10:14am
SUB TEST	.00	10:15am
AIR BLK	.00	10:16am

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

Intox EC/IR-II: Preventive Maintenance

IREDELL COUNTY MOORESVILLE PD 480

Serial Number: 008685 Test Record Number: 490
Test Date: 05/05/2009 Test Time: 10:17am EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	10:18am
FLO	Pass	10:18am
FC	Pass	10:18am

Temperature Tests

Test	Status	Time
FC1	Pass	10:18am
SRC	Pass	10:18am
DET	Pass	10:18am
BAR	Pass	10:18am
BT	Pass	10:18am

Blank Tests

Test	Status	Time
AIR	Pass	10:19am


Printer Tests

Test	Status	Time
PRNT	Pass	10:19am

CRC Tests

Test	Status	Time
COMP	Pass	10:19am
CAL	Pass	10:19am

Preventive Maintenance
Status: Pass

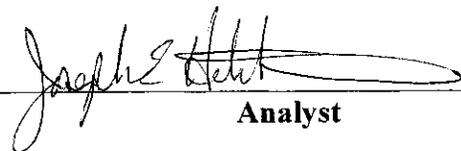
Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH


**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II**

County Mecklenburg Instrument Location Matthews PD
Instrument Serial No. 008699 1201 Crews Road, Matthews
704-847-4069

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 1st day of May, 20 09 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Joseph H. Hest
Signature of Certifying Official

650
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

MECKLENBURG COUNTY MATTHEWS PD 590

Serial Number: 008699
Test Date: 05/01/2009

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: HUTCHINSON, JOSEPH E

Permit Number: 19951E

Effective:

12/01/2007-12/01/2009

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG901901

Exp Date: 01/19/2011


Test	g/210L	Time
DIAG	Pass	1:16pm
AIR BLK	.00	1:17pm
ACCY CHK	.08	1:18pm
AIR BLK	.00	1:19pm
SUB TEST	.00	1:19pm
AIR BLK	.00	1:20pm
SUB TEST	.00	1:22pm
AIR BLK	.00	1:22pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR

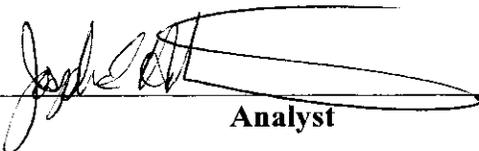

Analyst

Intox EC/IR-II: Preventive Maintenance

MECKLENBURG COUNTY MATTHEWS PD 590

Serial Number: 008699 Test Record Number: 649
Test Date: 05/01/2009 Test Time: 1:24pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	1:24pm
FLO	Pass	1:24pm
FC	Pass	1:24pm

Temperature Tests

Test	Status	Time
FC1	Pass	1:24pm
SRC	Pass	1:24pm
DET	Pass	1:24pm
BAR	Pass	1:24pm
BT	Pass	1:24pm

Blank Tests

Test	Status	Time
AIR	Pass	1:25pm


Printer Tests

Test	Status	Time
PRNT	Pass	1:25pm

CRC Tests

Test	Status	Time
COMP	Pass	1:25pm
CAL	Pass	1:25pm

Preventive Maintenance
Status: Pass

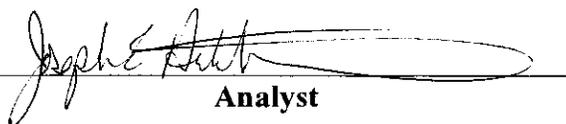
Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH


**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II**

County Mecklenburg Instrument Location Mecklenburg County SD
Instrument Serial No. 008665 801 East 4th Street, Charlotte
704-353-0180

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 1st day of May, 2009 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Joseph E. Hatcher
Signature of Certifying Official

650
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Preventive Maintenance

MECKLENBURG COUNTY SD

Serial Number: 008665 Test Record Number: 716
Test Date: 05/01/2009 Test Time: 12:09pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	12:10pm
FLO	Pass	12:10pm
FC	Pass	12:10pm

Temperature Tests

Test	Status	Time
FC1	Pass	12:10pm
SRC	Pass	12:10pm
DET	Pass	12:10pm
BAR	Pass	12:10pm
BT	Pass	12:10pm

Blank Tests

Test	Status	Time
AIR	Pass	12:11pm

Printer Tests

Test	Status	Time
PRNT	Pass	12:11pm

CRC Tests

Test	Status	Time
COMP	Pass	12:11pm
CAL	Pass	12:11pm

Preventive Maintenance
Status: Pass



Analyst

Intox EC/IR-II: Subject Test

MECKLENBURG COUNTY SD

Serial Number: 008665
Test Date: 05/01/2009

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: HUTCHINSON, JOSEPH E

Permit Number: 19951E

Effective:

12/01/2007-12/01/2009

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG816303

Exp Date: 06/11/2010


Test	g/210L	Time
DIAG	Pass	11:59am
AIR BLK	.00	11:59am
ACCY CHK	.08	12:00pm
AIR BLK	.00	12:01pm
SUB TEST	.00	12:02pm
AIR BLK	.00	12:03pm
SUB TEST	.00	12:06pm
AIR BLK	.00	12:07pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR

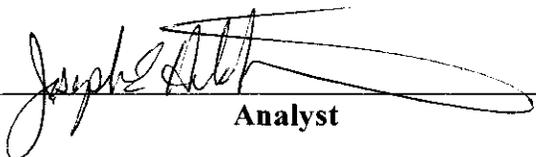

Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II**

County Mecklenburg Instrument Location Mecklenburg County SD
Instrument Serial No. 008690 801 E. 4th Street, Charlotte
704 - 353 - 0180

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 1st day of May, 2009 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Joseph E. Hutchinson
Signature of Certifying Official

650
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

MECKLENBURG COUNTY SD

Serial Number: 008690

Test Date: 05/01/2009

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: HUTCHINSON, JOSEPH E

Permit Number: 19951E

Effective:

12/01/2007-12/01/2009

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG816302


Exp Date: 06/11/2010

Test	g/210L	Time
DIAG	Pass	11:57am
AIR BLK	.00	11:58am
ACCY CHK	.08	11:58am
AIR BLK	.00	11:59am
SUB TEST	.00	11:59am
AIR BLK	.00	12:00pm
SUB TEST	.00	12:02pm
AIR BLK	.00	12:03pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR.

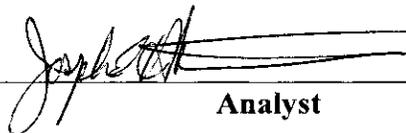
Analyst

Intox EC/IR-II: Preventive Maintenance

MECKLENBURG COUNTY SD

Serial Number: 008690 Test Record Number: 1243
Test Date: 05/01/2009 Test Time: 12:06pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	12:07pm
FLO	Pass	12:07pm
FC	Pass	12:07pm

Temperature Tests

Test	Status	Time
FC1	Pass	12:07pm
SRC	Pass	12:07pm
DET	Pass	12:07pm
BAR	Pass	12:07pm
BT	Pass	12:07pm

Blank Tests

Test	Status	Time
AIR	Pass	12:07pm


Printer Tests

Test	Status	Time
PRNT	Pass	12:07pm

CRC Tests

Test	Status	Time
COMP	Pass	12:07pm
CAL	Pass	12:07pm

Preventive Maintenance
Status: Pass

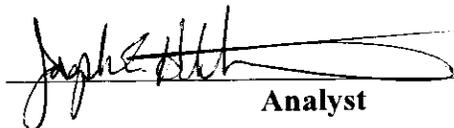
Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH


**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II**

County Mecklenburg Instrument Location Mecklenburg County SD
Instrument Serial No. 008691 801 East 4th Street, Charlotte
704-353-0180

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 1st day of May, 2009 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Joseph E. Hutchinson
Signature of Certifying Official

650
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

MECKLENBURG COUNTY SD 590

Serial Number: 008691

Test Date: 05/01/2009

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: HUTCHINSON, JOSEPH E

Permit Number: 19951E

Effective:

12/01/2007-12/01/2009

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG722802

Exp Date: 08/15/2009


Test	g/210L	Time
DIAG	Pass	11:55am
AIR BLK	.00	11:56am
ACCY CHK	.07	11:56am
AIR BLK	.00	11:57am
SUB TEST	.00	11:59am
AIR BLK	.00	12:00pm
SUB TEST	.00	12:02pm
AIR BLK	.00	12:03pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

Intox EC/IR-II: Preventive Maintenance

MECKLENBURG COUNTY SD 590

Serial Number: 008691 Test Record Number: 1341
Test Date: 05/01/2009 Test Time: 12:06pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	12:06pm
FLO	Pass	12:06pm
FC	Pass	12:06pm

Temperature Tests

Test	Status	Time
FC1	Pass	12:06pm
SRC	Pass	12:06pm
DET	Pass	12:06pm
BAR	Pass	12:06pm
BT	Pass	12:06pm

Blank Tests

Test	Status	Time
AIR	Pass	12:07pm


Printer Tests

Test	Status	Time
PRNT	Pass	12:07pm

CRC Tests

Test	Status	Time
COMP	Pass	12:07pm
CAL	Pass	12:07pm

Preventive Maintenance
Status: Pass

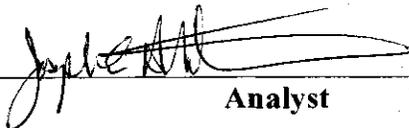

Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II**


County Mecklenburg Instrument Location Mecklenburg County SD

Instrument Serial No. 008703 801 E. 4th Street, Charlotte
704-353-0180

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 1st day of May, 2009 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Joseph E. Hutchinson
Signature of Certifying Official

650
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

MECKLENBURG COUNTY SD 590

Serial Number: 008703

Test Date: 05/01/2009

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: HUTCHINSON, JOSEPH E

Permit Number: 19951E

Effective:

12/01/2007-12/01/2009

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG722801

Exp Date: 08/15/2009


Test	g/210L	Time
DIAG	Pass	11:53am
AIR BLK	.00	11:54am
ACCY CHK	.08	11:55am
AIR BLK	.00	11:56am
SUB TEST	.00	11:59am
AIR BLK	.00	12:00pm
SUB TEST	.00	12:01pm
AIR BLK	.00	12:02pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR.



Analyst

Intox EC/IR-II: Preventive Maintenance

MECKLENBURG COUNTY SD 590

Serial Number: 008703 Test Record Number: 1398
Test Date: 05/01/2009 Test Time: 12:05pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	12:05pm
FLO	Pass	12:05pm
FC	Pass	12:05pm

Temperature Tests

Test	Status	Time
FC1	Pass	12:05pm
SRC	Pass	12:05pm
DET	Pass	12:05pm
BAR	Pass	12:05pm
BT	Pass	12:05pm

Blank Tests

Test	Status	Time
AIR	Pass	12:06pm


Printer Tests

Test	Status	Time
PRNT	Pass	12:06pm

CRC Tests

Test	Status	Time
COMP	Pass	12:06pm
CAL	Pass	12:06pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II**

County Daslow Instrument Location BAT Mobile Unit #6
Instrument Serial No. 00898 Swansboro

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 1 day of May, 2009 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



K. C. [Signature]
Signature of Certifying Official

6001
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Preventive Maintenance

ONslow COUNTY BAT MOBILE UNIT 6 660

Serial Number: 008898 Test Record Number: 159
Test Date: 05/01/2009 Test Time: 10:14pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	10:15pm
FLO	Pass	10:15pm
FC	Pass	10:15pm

Temperature Tests

Test	Status	Time
FC1	Pass	10:15pm
SRC	Pass	10:15pm
DET	Pass	10:15pm
BAR	Pass	10:15pm
BT	Pass	10:15pm

Blank Tests

Test	Status	Time
AIR	Pass	10:16pm

Printer Tests

Test	Status	Time
PRNT	Pass	10:16pm

CRC Tests

Test	Status	Time
COMP	Pass	10:16pm
CAL	Pass	10:16pm

Preventive Maintenance
Status: Pass



Analyst

Intox EC/IR-II: Subject Test

ONSLow COUNTY BAT MOBILE UNIT 6 660

Serial Number: 008898
Test Date: 05/01/2009

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: *RHODES, KENNETH C*
Permit Number: 5329E
Effective:
02/01/2008-02/01/2010

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG814002
Exp Date: 05/19/2010

Test	g/210L	Time
DIAG	Pass	10:04pm
AIR BLK	.00	10:05pm
ACCY CHK	.07	10:05pm
AIR BLK	.00	10:06pm
SUB TEST	.00	10:07pm
AIR BLK	.00	10:08pm
SUB TEST	.00	10:09pm
AIR BLK	.00	10:10pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH


**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II**

County Craven Instrument Location BAT Mobile Unit 6
Instrument Serial No. 008898 SHD

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 9 day of MAY, 2009 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



A. C. [Signature]
Signature of Certifying Official

601
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Preventive Maintenance

CRAVEN COUNTY BAT MOBILE UNIT 6 240

Serial Number: 008898 Test Record Number: 165
Test Date: 05/09/2009 Test Time: 10:36pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	10:36pm
FLO	Pass	10:36pm
FC	Pass	10:36pm

Temperature Tests

Test	Status	Time
FC1	Pass	10:37pm
SRC	Pass	10:37pm
DET	Pass	10:37pm
BAR	Pass	10:37pm
BT	Pass	10:37pm

Blank Tests

Test	Status	Time
AIR	Pass	10:37pm


Printer Tests

Test	Status	Time
PRNT	Pass	10:37pm

CRC Tests

Test	Status	Time
COMP	Pass	10:37pm
CAL	Pass	10:37pm

Preventive Maintenance
Status: Pass

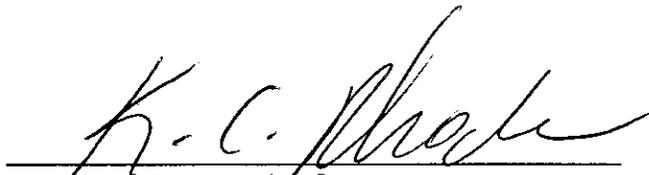

Analyst

Intox EC/IR-II: Subject Test

CRAVEN COUNTY BAT MOBILE UNIT 6 240

Serial Number: 008898
Test Date: 05/09/2009

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: RHODES, KENNETH C
Permit Number: 5329E
Effective:
02/01/2008-02/01/2010

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG814002
Exp Date: 05/19/2010


Test	g/210L	Time
DIAG	Pass	10:28pm
AIR BLK	.00	10:29pm
ACCY CHK	.07	10:30pm
AIR BLK	.00	10:31pm
SUB TEST	.00	10:31pm
AIR BLK	.00	10:32pm
SUB TEST	.00	10:33pm
AIR BLK	.00	10:34pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR

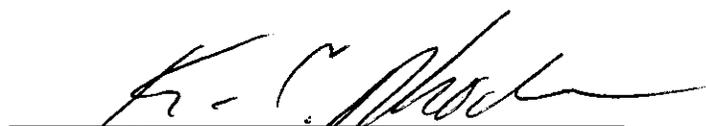

Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH


**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II**

County Onslow Instrument Location BAT Mobile Unit 6
Instrument Serial No. 008897 Lichlands

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 8 day of May, 2009 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



B. C. [Signature]
Signature of Certifying Official

601
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Preventive Maintenance

ONslow COUNTY BAT MOBILE UNIT 6 660

Serial Number: 008898 Test Record Number: 162
Test Date: 05/08/2009 Test Time: 11:57pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	11:57pm
FLO	Pass	11:57pm
FC	Pass	11:57pm

Temperature Tests

Test	Status	Time
FC1	Pass	11:57pm
SRC	Pass	11:57pm
DET	Pass	11:57pm
BAR	Pass	11:57pm
BT	Pass	11:57pm

Blank Tests

Test	Status	Time
AIR	Pass	11:58pm

Printer Tests

Test	Status	Time
PRNT	Pass	11:58pm

CRC Tests

Test	Status	Time
COMP	Pass	11:58pm
CAL	Pass	11:58pm

Preventive Maintenance
Status: Pass



Analyst

Intox•EC/IR-II: Subject Test

ONslow COUNTY BAT MOBILE UNIT 6 660

Serial Number: 008898
Test Date: 05/08/2009

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: RHODES, KENNETH C
Permit Number: 5329E
Effective:
02/01/2008-02/01/2010

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG814002
Exp Date: 05/19/2010


Test	g/210L	Time
DIAG	Pass	11:46pm
AIR BLK	.00	11:47pm
ACCY CHK	.07	11:47pm
AIR BLK	.00	11:48pm
SUB TEST	.00	11:49pm
AIR BLK	.00	11:50pm
SUB TEST	.00	11:51pm
AIR BLK	.00	11:52pm

Reported AC: 00 g/210L



Signature of Chemical Analyst

Court CVR

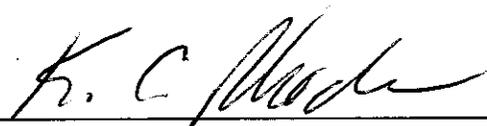

Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH


**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II**

County Oaslow Instrument Location DAT Mobile unit 6
Instrument Serial No. 008939 Swansboro

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 1 day of MAY, 2009 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

601
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Preventive Maintenance

ONslow COUNTY BAT MOBILE UNIT 6 660

Serial Number: 008939 Test Record Number: 159
Test Date: 05/01/2009 Test Time: 9:59pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	10:00pm
FLO	Pass	10:00pm
FC	Pass	10:00pm

Temperature Tests

Test	Status	Time
FC1	Pass	10:00pm
SRC	Pass	10:00pm
DET	Pass	10:00pm
BAR	Pass	10:00pm
BT	Pass	10:00pm

Blank Tests

Test	Status	Time
AIR	Pass	10:00pm


Printer Tests

Test	Status	Time
PRNT	Pass	10:01pm

CRC Tests

Test	Status	Time
COMP	Pass	10:01pm
CAL	Pass	10:01pm

Preventive Maintenance
Status: Pass

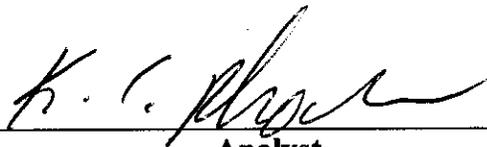

Analyst

Intox EC/IR-II: Subject Test

ONslow COUNTY BAT MOBILE UNIT 6 660

Serial Number: 008939
Test Date: 05/01/2009

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: RHODES, KENNETH C
Permit Number: 5329E
Effective:
02/01/2008-02/01/2010

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test


Lot Number: AG814101
Exp Date: 05/20/2010

Test	g/210L	Time
DIAG	Pass	9:49pm
AIR BLK	.00	9:50pm
ACCY CHK	.07	9:51pm
AIR BLK	.00	9:51pm
SUB TEST	.00	9:52pm
AIR BLK	.00	9:53pm
SUB TEST	.00	9:55pm
AIR BLK	.00	9:56pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II**

County Rutherford Instrument Location BAT Mobile Unit 4

Instrument Serial No. 008734

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 8th day of May, 2009 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

651
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Preventive Maintenance

BUNCOMBE COUNTY BAT MOBILE UNIT 4 100

Serial Number: 008734 Test Record Number: 227
Test Date: 05/08/2009 Test Time: 5:47pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	5:48pm
FLO	Pass	5:48pm
FC	Pass	5:48pm

Temperature Tests

Test	Status	Time
FC1	Pass	5:48pm
SRC	Pass	5:48pm
DET	Pass	5:48pm
BAR	Pass	5:48pm
BT	Pass	5:48pm

Blank Tests

Test	Status	Time
AIR	Pass	5:48pm


Printer Tests

Test	Status	Time
PRNT	Pass	5:48pm

CRC Tests

Test	Status	Time
COMP	Pass	5:49pm
CAL	Pass	5:49pm

Preventive Maintenance
Status: Pass


Analyst

Intox EC/IR-II: Subject Test

BUNCOMBE COUNTY BAT MOBILE UNIT 4 100

Serial Number: 008734
Test Date: 05/08/2009

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: *TRUDELL, SR., DANIEL T*
Permit Number: 21535E
Effective:
12/01/2007-12/01/2009

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: *Breath Test*

Lot Number: AG722501
Exp Date: 08/12/2009

Test	g/210L	Time
DIAG	Pass	5:39pm
AIR BLK	.00	5:40pm
ACCY CHK	.07	5:40pm
AIR BLK	.00	5:41pm
SUB TEST	.00	5:42pm
AIR BLK	.00	5:43pm
SUB TEST	.00	5:44pm
AIR BLK	.00	5:45pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II**


County NASH Instrument Location BAT MOBILE LOU.T #5

Instrument Serial No. 005698 SHIPS BUE

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 15 day of MAY, 2009 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

636
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Preventive Maintenance

NASH COUNTY BAT MOBILE UNIT 5 630

Serial Number: 008698 Test Record Number: 310
Test Date: 05/01/2009 Test Time: 11:01pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	11:01pm
FLO	Pass	11:01pm
FC	Pass	11:01pm

Temperature Tests

Test	Status	Time
FC1	Pass	11:01pm
SRC	Pass	11:01pm
DET	Pass	11:01pm
BAR	Pass	11:01pm
BT	Pass	11:01pm

Blank Tests

Test	Status	Time
AIR	Pass	11:02pm


Printer Tests

Test	Status	Time
PRNT	Pass	11:02pm

CRC Tests

Test	Status	Time
COMP	Pass	11:02pm
CAL	Pass	11:02pm

Preventive Maintenance
Status: Pass



Analyst

Intox EC/IR-II: Subject Test

NASH COUNTY BAT MOBILE UNIT 5 630

Serial Number: 008698

Test Date: 05/01/2009

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: MORGART, STEPHEN G

Permit Number: 09372E

Effective:

12/01/2007-12/01/2009

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG723401


Exp Date: 08/21/2009

Test	g/210L	Time
DIAG	Pass	10:52pm
AIR BLK	.00	10:53pm
ACCY CHK	.07	10:54pm
AIR BLK	.00	10:54pm
SUB TEST	.00	10:56pm
AIR BLK	.00	10:57pm
SUB TEST	.00	10:58pm
AIR BLK	.00	10:59pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II**

County NASH

Instrument Location BAT MOBILE UNIT #5


Instrument Serial No. 008600

STANBURY

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 15th day of MAY, 2009 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Steph G. Moad
Signature of Certifying Official

656
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Preventive Maintenance

NASH COUNTY BAT MOBILE UNIT 5 630

Serial Number: 008600 Test Record Number: 462
Test Date: 05/01/2009 Test Time: 10:54pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	10:54pm
FLO	Pass	10:54pm
FC	Pass	10:54pm

Temperature Tests

Test	Status	Time
FC1	Pass	10:54pm
SRC	Pass	10:54pm
DET	Pass	10:54pm
BAR	Pass	10:54pm
BT	Pass	10:54pm

Blank Tests

Test	Status	Time
AIR	Pass	10:55pm


Printer Tests

Test	Status	Time
PRNT	Pass	10:55pm

CRC Tests

Test	Status	Time
COMP	Pass	10:55pm
CAL	Pass	10:55pm

Preventive Maintenance
Status: Pass



Analyst

Intox EC/IR-II: Subject Test

NASH COUNTY BAT MOBILE UNIT 5 630

Serial Number: 008600

Test Date: 05/01/2009

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: MORGART, STEPHEN G

Permit Number: 09372E

Effective:

12/01/2007-12/01/2009

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG723401


Exp Date: 08/21/2009

Test	g/210L	Time
DIAG	Pass	10:45pm
AIR BLK	.00	10:46pm
ACCY CHK	.07	10:47pm
AIR BLK	.00	10:48pm
SUB TEST	.00	10:48pm
AIR BLK	.00	10:49pm
SUB TEST	.00	10:51pm
AIR BLK	.00	10:52pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH


**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II**

County NASH Instrument Location ISAT MOBILE UNIT #5
Instrument Serial No. 008788 SHARP 426

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 1st day of MAY, 2009 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Steph G. Tilton
Signature of Certifying Official

656
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Preventive Maintenance

NASH COUNTY BAT MOBILE UNIT 5 630

Serial Number: 008788 Test Record Number: 181
Test Date: 05/01/2009 Test Time: 10:57pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	10:57pm
FLO	Pass	10:57pm
FC	Pass	10:57pm

Temperature Tests

Test	Status	Time
FC1	Pass	10:57pm
SRC	Pass	10:57pm
DET	Pass	10:57pm
BAR	Pass	10:57pm
BT	Pass	10:57pm

Blank Tests

Test	Status	Time
AIR	Pass	10:58pm


Printer Tests

Test	Status	Time
PRNT	Pass	10:58pm

CRC Tests

Test	Status	Time
COMP	Pass	10:58pm
CAL	Pass	10:58pm

Preventive Maintenance
Status: Pass


Analyst

Intox EC/IR-II: Subject Test

NASH COUNTY BAT MOBILE UNIT 5 630

Serial Number: 008788
Test Date: 05/01/2009

Citation Number: M0000000-0
Subject's Name:

PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: MORGART, STEPHEN G
Permit Number: 09372E
Effective:
12/01/2007-12/01/2009

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test


Lot Number: AG722802
Exp Date: 08/15/2009

Test	g/210L	Time
DIAG	Pass	10:48pm
AIR BLK	.00	10:49pm
ACCY CHK	.08	10:50pm
AIR BLK	.00	10:50pm
SUB TEST	.00	10:51pm
AIR BLK	.00	10:52pm
SUB TEST	.00	10:53pm
AIR BLK	.00	10:54pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR

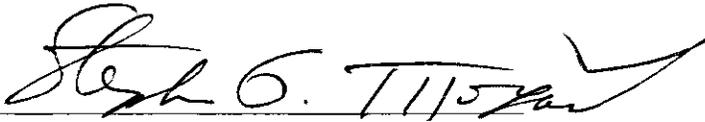
Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II**

County Gaston Instrument Location Belmont PD

Instrument Serial No. 008733 201 Chronicle Street, Belmont
704-825-3792

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 29th day of May, 2009 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Joseph E. Hutchins
Signature of Certifying Official

650
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

GASTON COUNTY BELMONT PD 350

Serial Number: 008733
Test Date: 05/29/2009

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: HUTCHINSON, JOSEPH E
Permit Number: 19951E
Effective:
12/01/2007-12/01/2009

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG722501
Exp Date: 08/12/2009


Test	g/210L	Time
DIAG	Pass	3:34pm
AIR BLK	.00	3:35pm
ACCY CHK	.07	3:36pm
AIR BLK	.00	3:37pm
SUB TEST	.00	3:37pm
AIR BLK	.00	3:38pm
SUB TEST	.00	3:39pm
AIR BLK	.00	3:40pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR

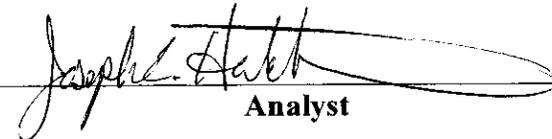

Analyst

Intox EC/IR-II: Preventive Maintenance

GASTON COUNTY BELMONT PD 350

Serial Number: 008733 Test Record Number: 230
Test Date: 05/29/2009 Test Time: 3:42pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	3:42pm
FLO	Pass	3:42pm
FC	Pass	3:42pm

Temperature Tests

Test	Status	Time
FC1	Pass	3:42pm
SRC	Pass	3:42pm
DET	Pass	3:42pm
BAR	Pass	3:42pm
BT	Pass	3:42pm

Blank Tests

Test	Status	Time
AIR	Pass	3:43pm


Printer Tests

Test	Status	Time
PRNT	Pass	3:43pm

CRC Tests

Test	Status	Time
COMP	Pass	3:43pm
CAL	Pass	3:43pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II**


County Gaston Instrument Location Gaston County SD

Instrument Serial No. 008706 425 N. Marietta Street, Gastonia
704-869-6800

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 29th day of May, 2009 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Joseph C. Hatt
Signature of Certifying Official

650
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

GASTON COUNTY GASTON COUNTY SD 350

Serial Number: 008706
Test Date: 05/29/2009

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: HUTCHINSON, JOSEPH E
Permit Number: 19951E
Effective:
12/01/2007-12/01/2009

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test


Lot Number: AG722602
Exp Date: 08/13/2009

Test	g/210L	Time
DIAG	Pass	1:47pm
AIR BLK	.00	1:48pm
ACCY CHK	.08	1:48pm
AIR BLK	.00	1:49pm
SUB TEST	.00	1:50pm
AIR BLK	.00	1:50pm
SUB TEST	.00	1:52pm
AIR BLK	.00	1:53pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR

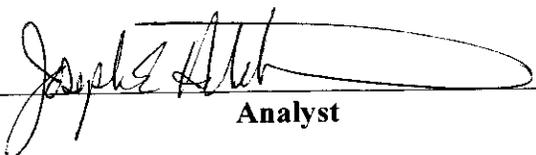
Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

GASTON COUNTY GASTON COUNTY SD 350

Serial Number: 008706 Test Record Number: 616
Test Date: 05/29/2009 Test Time: 1:54pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	1:55pm
FLO	Pass	1:55pm
FC	Pass	1:55pm

Temperature Tests

Test	Status	Time
FC1	Pass	1:55pm
SRC	Pass	1:55pm
DET	Pass	1:55pm
BAR	Pass	1:55pm
BT	Pass	1:55pm

Blank Tests

Test	Status	Time
AIR	Pass	1:56pm


Printer Tests

Test	Status	Time
PRNT	Pass	1:56pm

CRC Tests

Test	Status	Time
COMP	Pass	1:56pm
CAL	Pass	1:56pm

Preventive Maintenance
Status: Pass

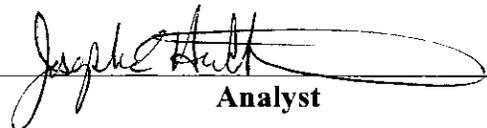
Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II**


County Gaston Instrument Location Gaston County SD

Instrument Serial No. 008643 425 N. Marietta Street, Gastonia
704-869-6800

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 29th day of May, 20 09 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Joseph E. Hatcher
Signature of Certifying Official

650
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

GASTON COUNTY GASTON COUNTY SD 350

Serial Number: 008643
Test Date: 05/29/2009

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: HUTCHINSON, JOSEPH E
Permit Number: 19951E
Effective:
12/01/2007-12/01/2009

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG722503
Exp Date: 08/12/2009


Test	g/210L	Time
DIAG	Pass	1:30pm
AIR BLK	.00	1:31pm
ACCY CHK	.07	1:32pm
AIR BLK	.00	1:33pm
SUB TEST	.00	1:34pm
AIR BLK	.00	1:35pm
SUB TEST	.00	1:36pm
AIR BLK	.00	1:37pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR

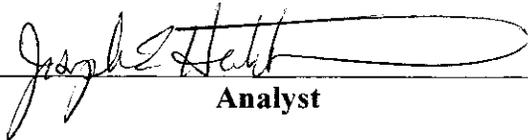

Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

GASTON COUNTY GASTON COUNTY SD 350

Serial Number: 008643 Test Record Number: 541
Test Date: 05/29/2009 Test Time: 1:38pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	1:39pm
FLO	Pass	1:39pm
FC	Pass	1:39pm

Temperature Tests

Test	Status	Time
FC1	Pass	1:39pm
SRC	Pass	1:39pm
DET	Pass	1:39pm
BAR	Pass	1:39pm
BT	Pass	1:39pm

Blank Tests

Test	Status	Time
AIR	Pass	1:40pm


Printer Tests

Test	Status	Time
PRNT	Pass	1:40pm

CRC Tests

Test	Status	Time
COMP	Pass	1:40pm
CAL	Pass	1:40pm

Preventive Maintenance
Status: Pass

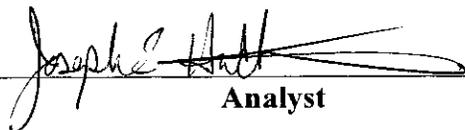
Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II**


County Gaston Instrument Location Gaston County SD

Instrument Serial No. 008684 425 N. Marietta Street, Gastonia
704 - 869 - 6800

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 29th day of May, 20 09 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Joseph E. Hatcher
Signature of Certifying Official

650
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

GASTON COUNTY GASTON COUNTY SD 350

Serial Number: 008684
Test Date: 05/29/2009

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: HUTCHINSON, JOSEPH E
Permit Number: 19951E
Effective:
12/01/2007-12/01/2009

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test


Lot Number: AG722503
Exp Date: 08/12/2009

Test	g/210L	Time
DIAG	Pass	1:28pm
AIR BLK	.00	1:29pm
ACCY CHK	.07	1:30pm
AIR BLK	.00	1:31pm
SUB TEST	.00	1:31pm
AIR BLK	.00	1:32pm
SUB TEST	.00	1:34pm
AIR BLK	.00	1:35pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR.

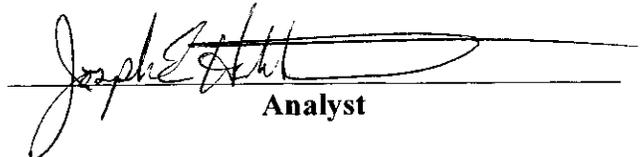
Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

GASTON COUNTY GASTON COUNTY SD 350

Serial Number: 008684 Test Record Number: 747
Test Date: 05/29/2009 Test Time: 1:36pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	1:36pm
FLO	Pass	1:36pm
FC	Pass	1:37pm

Temperature Tests

Test	Status	Time
FC1	Pass	1:37pm
SRC	Pass	1:37pm
DET	Pass	1:37pm
BAR	Pass	1:37pm
BT	Pass	1:37pm

Blank Tests

Test	Status	Time
AIR	Pass	1:37pm


Printer Tests

Test	Status	Time
PRNT	Pass	1:37pm

CRC Tests

Test	Status	Time
COMP	Pass	1:37pm
CAL	Pass	1:37pm

Preventive Maintenance
Status: Pass

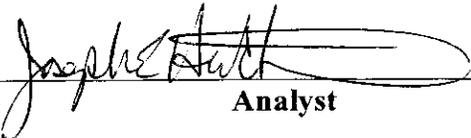
Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II**

County Cabarrus Instrument Location Kannapolis PD

Instrument Serial No. 008589 314 S Main Street, Kannapolis
704-920-4000

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 29th day of May, 20 09 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Joseph C. Stantman
Signature of Certifying Official

650
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

CABARRUS COUNTY KANNAPOLIS PD 120

Serial Number: 008589
Test Date: 05/29/2009

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: HUTCHINSON, JOSEPH E

Permit Number: 19951E

Effective:

12/01/2007-12/01/2009

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG816302

Exp Date: 06/11/2010


Test	g/210L	Time
DIAG	Pass	12:07pm
AIR BLK	.00	12:07pm
ACCY CHK	.08	12:08pm
AIR BLK	.00	12:09pm
SUB TEST	.00	12:09pm
AIR BLK	.00	12:10pm
SUB TEST	.00	12:12pm
AIR BLK	.00	12:13pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR.

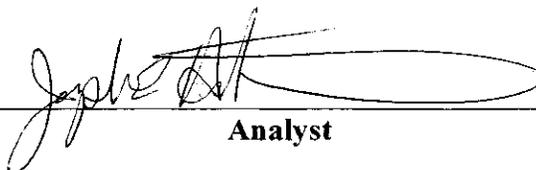

Analyst

Intox EC/IR-II: Preventive Maintenance

CABARRUS COUNTY KANNAPOLIS PD 120

Serial Number: 008589 Test Record Number: 665
Test Date: 05/29/2009 Test Time: 12:13pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	12:14pm
FLO	Pass	12:14pm
FC	Pass	12:14pm

Temperature Tests

Test	Status	Time
FC1	Pass	12:14pm
SRC	Pass	12:14pm
DET	Pass	12:14pm
BAR	Pass	12:14pm
BT	Pass	12:14pm

Blank Tests

Test	Status	Time
AIR	Pass	12:15pm

Printer Tests

Test	Status	Time
PRNT	Pass	12:15pm

CRC Tests

Test	Status	Time
COMP	Pass	12:15pm
CAL	Pass	12:15pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH


**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II**

County Union Instrument Location Union County SD
Instrument Serial No. 008876 3344 Presson Road, Monroe
704-283-3770

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 26th day of May, 2009 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Joseph S. Hutch
Signature of Certifying Official

650
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

UNION COUNTY UNION COUNTY SD 890

Serial Number: 008876
Test Date: 05/26/2009

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: HUTCHINSON, JOSEPH E

Permit Number: 19951E

Effective:

12/01/2007-12/01/2009

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG722501


Exp Date: 08/12/2009

Test	g/210L	Time
DIAG	Pass	3:35pm
AIR BLK	.00	3:36pm
ACCY CHK	.07	3:36pm
AIR BLK	.00	3:37pm
SUB TEST	.00	3:38pm
AIR BLK	.00	3:39pm
SUB TEST	.00	3:40pm
AIR BLK	.00	3:41pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR

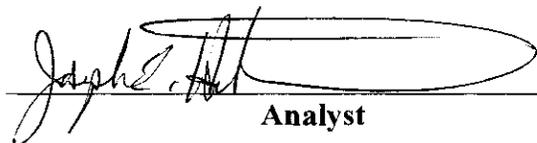
Analyst

Intox EC/IR-II: Preventive Maintenance

UNION COUNTY UNION COUNTY SD 890

Serial Number: 008876 Test Record Number: 587
Test Date: 05/26/2009 Test Time: 3:43pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	3:43pm
FLO	Pass	3:43pm
FC	Pass	3:43pm

Temperature Tests

Test	Status	Time
FC1	Pass	3:43pm
SRC	Pass	3:43pm
DET	Pass	3:43pm
BAR	Pass	3:43pm
BT	Pass	3:43pm

Blank Tests

Test	Status	Time
AIR	Pass	3:44pm


Printer Tests

Test	Status	Time
PRNT	Pass	3:44pm

CRC Tests

Test	Status	Time
COMP	Pass	3:44pm
CAL	Pass	3:44pm

Preventive Maintenance
Status: Pass

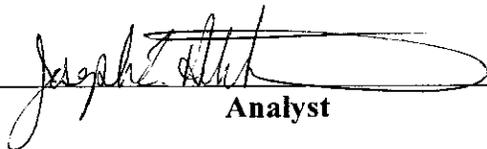
Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH


**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II**

County Union Instrument Location Union County SD
Instrument Serial No. 008866 3344 Presson Road, Monroe
704-283-3770

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 26th day of May, 2009 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Joseph S. Hutchins
Signature of Certifying Official

650
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

UNION COUNTY UNION COUNTY SD 890

Serial Number: 008866
Test Date: 05/26/2009

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: *HUTCHINSON, JOSEPH E*
Permit Number: 19951E
Effective:
12/01/2007-12/01/2009

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: *Breath Test*

Lot Number: AG814101
Exp Date: 05/20/2010

Test	g/210L	Time
DIAG	Pass	3:33pm
AIR BLK	.00	3:34pm
ACCY CHK	.08	3:35pm
AIR BLK	.00	3:36pm
SUB TEST	.00	3:36pm
AIR BLK	.00	3:37pm
SUB TEST	.00	3:39pm
AIR BLK	.00	3:40pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

Intox EC/IR-II: Preventive Maintenance

UNION COUNTY UNION COUNTY SD 890

Serial Number: 008866 Test Record Number: 377
Test Date: 05/26/2009 Test Time: 3:41pm EDT

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	3:41pm
FLO	Pass	3:41pm
FC	Pass	3:42pm

Temperature Tests

Test	Status	Time
FC1	Pass	3:42pm
SRC	Pass	3:42pm
DET	Pass	3:42pm
BAR	Pass	3:42pm
BT	Pass	3:42pm

Blank Tests

Test	Status	Time
AIR	Pass	3:42pm


Printer Tests

Test	Status	Time
PRNT	Pass	3:42pm

CRC Tests

Test	Status	Time
COMP	Pass	3:42pm
CAL	Pass	3:42pm

Preventive Maintenance
Status: Pass

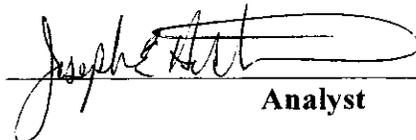

Analyst